

**Quick Card**

# 3D/4D for Gynecology

ACUSON Sequoia Ultrasound System  
3.5 (VB30)

[siemens-healthineers.com/sequoia](http://siemens-healthineers.com/sequoia)



# Getting Started

The 3D volume data set is a series of 2D images gathered over a timed acquisition.

- The 9VE4 and 7VC2 transducers perform an automated mechanical calibrated acquisition of the volume data set

---

## Step 1


- Press **3D/4D control**
- Select **3D** or **4D** from the touch screen



---

## Step 2

- Place the Volume of Interest (VOI) to include the anatomy desired. The VOI can be curved by selecting the Curve option on the trackball left set key
- The Volume of Interest box may be deactivated by selecting the VOI key on the touch screen. When disabled, the entire field of view will be acquired in the volume

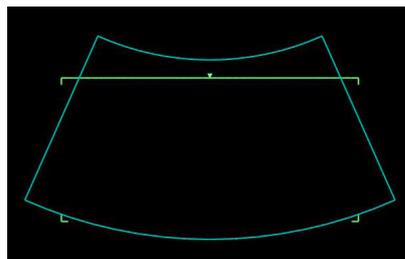

### 3D

- Press the **Update** key, and the system will automatically acquire a sweep and display the volume



### 4D

- Press the **Update** key to start the acquisition. The system will enter live 4D imaging; select Freeze to stop the acquisition

---

## Step 3

### 3D

- Press **Image** to store a volume

### 4D

- During live acquisition, press the **Clip** key to store a 4D clip
- Press the **Image** key to store a single volume on a frozen image




- Stored 3D volumes are marked with a cube graphic
- Stored 4D volume clips are marked with a cube containing a "play" icon



## Render Modes

There are four render modes available:

- **Surface:** Smooths the image contours, creating a soft sculptured appearance for highlighting surface features of soft tissue
- **Vascular (Minimum Intensity Projection/Min IP):**  
Best for visualizing hypo-echoic lesions and vascular structures
- **Skeletal (Maximum Intensity Projection/Max IP):**  
Best for intrauterine devices and bony structures
- **Light Source:** Helps increase depth perception, reveals surface details, provides an element of texture, and can provide a deeper understanding of relational anatomy. The adjustable light source direction is automatically activated in a 1:1 layout, but may be activated/deactivated in any layout by selecting the **Light** key on the touch screen.

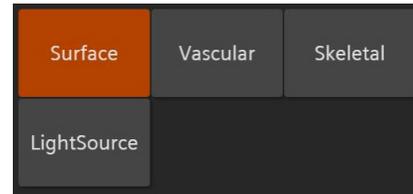

Use the trackball to adjust the direction of the light.

## FlexPlane





The FlexPlane tool allows the user to obtain and visualize anatomy of any shape along any plane. This is especially useful when imaging complex or irregularly shaped structures.

The user can choose from:

- **Line** – A straight line in any direction
- **Trace** – A freehand line traced in any direction
- **Spline** – An open spline controlled by selecting the set key along the path of the spline

Once the desired option is chosen:

- Press either **Set** control to begin the line
- Press either **Set** key again to end the Line/Trace tools or to change the direction of the Spline tool (double-click either **Set** control to end the Spline)
- To redraw the slice, press the **Update** control
- Use the rotary soft keys to adjust the volume thickness as well as line or slice orientation; to enable measurements on the rendered image, set the thickness to **Off**

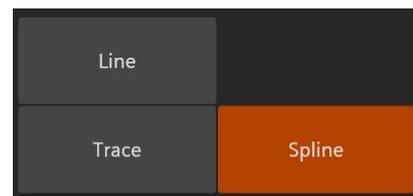


## MPR & VR Orientation

Adjust the Multiplanar Renderings (MPR) and the volume using the rotation tools on the control panel. These controls can be used during 4D live acquisition.

- Select the desired quadrant from the touch screen
- The MPR slicing function is manipulated using the 3D/4D control
- The X axis is manipulated using the M-mode control
- The Y axis is manipulated using the PW Doppler control
- The Z axis is manipulated using the Color Doppler control




Use the rotation tools on the touch screen to quickly rotate the volume rendering by set degrees.

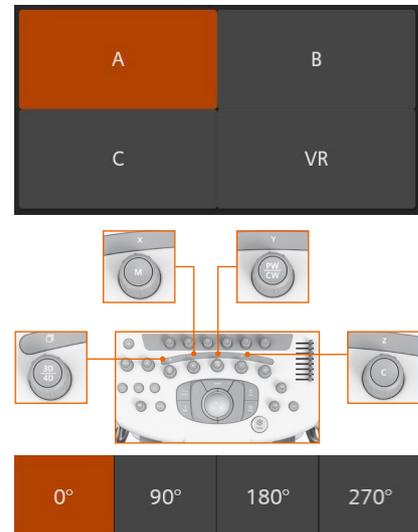

## Multislice

The Multislice tab contains options for viewing multiple slices of the selected MPR plane at the same time. It is often referred to as a CT or MRI view.



- Select the desired plane using the A, B, and C keys
- Select the desired layout from the touch screen
- Use the rotary soft keys to adjust the number of slices, distance between slices, and the position of the slices

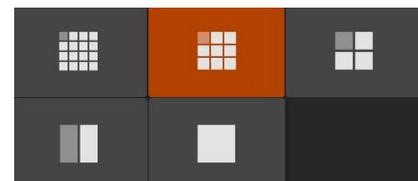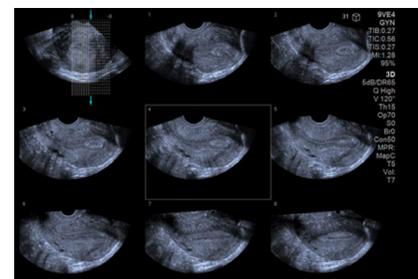

## Editing

The editing tab contains options for removing unnecessary structures.

- Select the desired tool from the touch screen
- Use the trackball and **Set** keys to delineate the area for removal
- Place the scissor icon in the area to be removed and press the **Set** key to finalize
- Edits may be reversed using the touch screen options



---

## Additional Optimization – Acquisition

### Angle

- Determines the angle of the volume sweep

### Quality

- Adjusts the resolution and sweep speed between Low, Mid, and High
- 

## Additional Optimization – VR

### Threshold

- Decreasing the threshold removes low-level echoes while increasing the threshold adds low-level echoes

### Opacity

- Adjusts the transparency of the voxel

### Smooth

- Averages the edges of the voxels with adjacent voxels to smooth the volume image appearance

### Brightness

- Changes the voxel saturation

### Contrast

- Raises or lowers the percentage of contrast to enhance differences in tissue

### Tint

- Applies assigned color shades to the gray scale
- 

## Additional Optimization – MPR

### Dynamic Range

- Decreasing the threshold removes low-level echoes while increasing the threshold adds low-level echoes

### Map

- Adjusts the transparency of the voxel


### Tint

- Applies assigned color shades to the gray scale
- 

## Review

- Select **Review** from the touch screen with the pointer, select the image for review

- Select the **3D/4D** tab on the touch screen to activate the volume manipulation tools if desired
- Any additional images stored while the volume is active in the **3D/4D** tab will be stored as volumes or volume clips. Additional images stored while in the **Review** tab will be stored as still images.

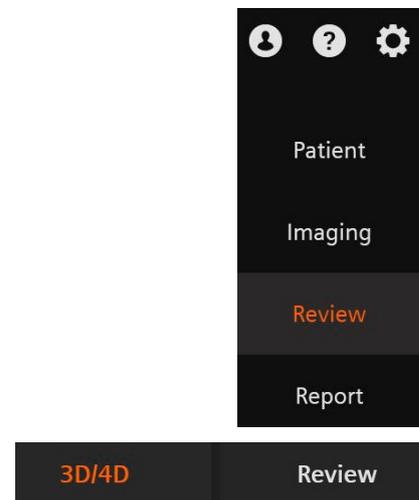

For the proper use of the software or hardware, please always use the Operator Manual or Instructions for Use (hereinafter collectively "Operator Manual") issued by Siemens Healthineers. This material is to be used as training material only and shall by no means substitute the Operator Manual. Any material used in this training will not be updated on a regular basis and does not necessarily reflect the latest version of the software and hardware available at the time of the training. The Operator Manual shall be used as your main reference, in particular for relevant safety information like warnings and cautions.

Note: Some functions shown in this material are optional and might not be part of your system.

Certain products, product related claims or functionalities described in the material (hereinafter collectively "Functionality") may not (yet) be commercially available in your country. Due to regulatory requirements, the future availability of said functionalities in any specific country is not guaranteed. Please contact your local Siemens Healthineers sales representative for the most current information. The reproduction, transmission or distribution of this training or its contents is not permitted without express written authority. Offenders will be liable for damages.

All names and data of patients, parameters and configuration dependent designations are fictional and examples only. All rights, including rights created by patent grant or registration of a utility model or design, are reserved.

ACUSON Sequoia is a trademark of Siemens Medical Solutions USA, Inc.

Siemens Healthineers Ultrasound owns the rights to all images.

At Siemens Healthineers, we pioneer breakthroughs in healthcare. For everyone. Everywhere. Sustainably. As a leader in medical technology, we want to advance a world in which breakthroughs in healthcare create new possibilities with a minimal impact on our planet. By consistently bringing innovations to the market, we enable healthcare professionals to innovate personalized care, achieve operational excellence, and transform the system of care.

Our portfolio, spanning in vitro and in vivo diagnostics to image-guided therapy and cancer care, is crucial for clinical decision-making and treatment pathways. With the unique combination of our strengths in patient twinning<sup>1</sup>, precision therapy, as well as digital, data, and artificial intelligence (AI), we are well positioned to take on the greatest challenges in healthcare. We will continue to build on these strengths to help overcome the world's most threatening diseases, enable efficient operations, and expand access to care.

We are a team of more than 71,000 Healthineers in over 70 countries passionately pushing the boundaries of what is possible in healthcare to help improve the lives of people around the world.

<sup>1</sup> *Personalization of diagnosis, therapy selection and monitoring, aftercare, and managing health.*

---

**Siemens Healthineers Headquarters**

Siemens Healthineers AG  
Siemensstr. 3  
91301 Forchheim, Germany  
Phone: +49 9191 18-0  
siemens-healthineers.com

**Manufacturer**

Siemens Medical Solutions USA, Inc.  
Ultrasound  
22010 S.E. 51st Street  
Issaquah, WA 98029, USA  
Phone: 1-888-826-9702  
siemens-healthineers.com/ultrasound