




VACUUM BLOOD COLLECTION SYSTEM

Lind-Vac[®]



InterVacTechnology OÜ
Estonia



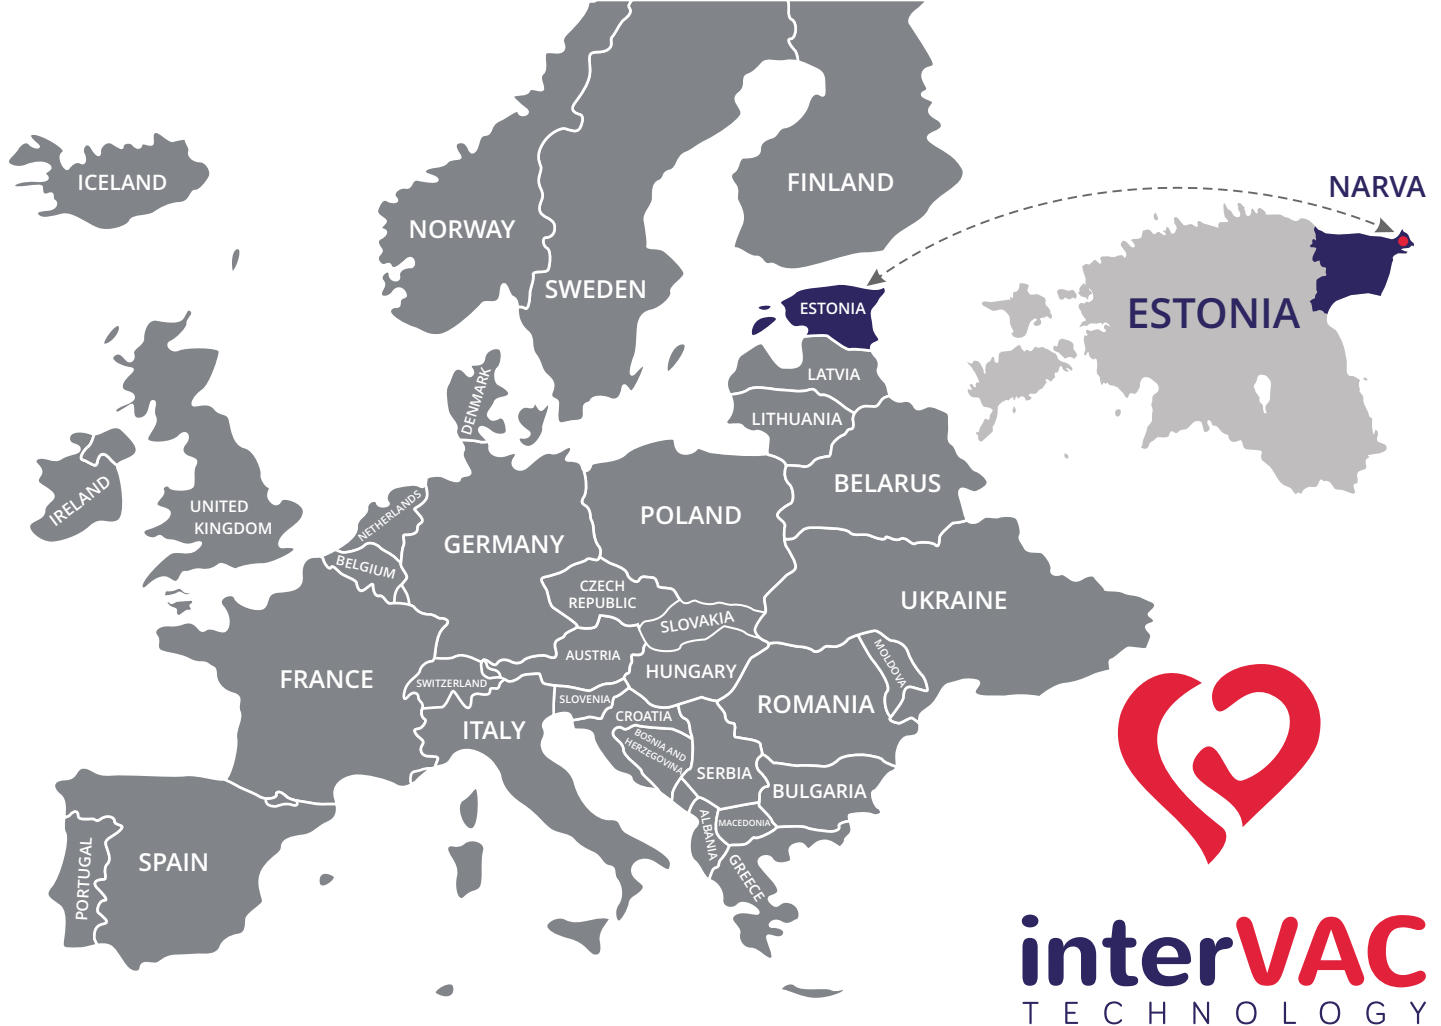

InterVacTechnology OÜ is the unique high-technology manufacturer of the vacuum blood collection system **Lind-Vac®** in the Baltic states. The **Lind-Vac®** vacuum blood collection system was introduced into market in 2011.

The system has been designed for quick, safe, correct and hygienic blood collection. We offer a complete range of blood collection tubes available in different sizes and with appropriate additives. Also we provide a wide range of **Lind-Vac®** needles and holders to perform a total safety of vacuum blood collection.

The **Lind-Vac®** vacuum blood collection systems are used in medical institutions and laboratories in more than 20 countries around the world and have had only positive feedbacks from medical personnel who have appreciated the quality, usability and safety of our products.



Certificates of InterVacTechnology OÜ



Certificate UNI CEI EN ISO 13485:2016



Free sales certificate (CE mark)



interVAC
TECHNOLOGY



Certificate ISO 9001:2015

Tubes	Color code	Additive	Tests
No additive		/	Clinical chemistry, serology, immunology
Clot activator		Clot activator	Clinical chemistry, serology, immunology, protein electrophoresis
Clot activator & Gel		Gel & Clot activator	Clinical chemistry, serology, immunology, protein electrophoresis
Thrombin		Thrombin	Clinical chemistry, express
Thrombin & Gel		Thrombin & Gel	Clinical chemistry, express
EDTA		EDTA K2 EDTA K3	Hematology
Sodium citrate 1 : 4		Sodium citrate 0,129 mol/l (3,8%)	Blood sedimentation
Sodium citrate 1 : 9		Sodium citrate 0,129 mol/l (3,8%) 0,109 mol/l (3,2%)	Coagulation
Heparin		Lithium heparin Sodium heparin	Study of plasma in biochemical studies
Glucose		Na fluoride / EDTA Na fluoride / Potassium oxalate	The level of glucose, lactate glycosylated hemoglobin
Glucose for the diagnosis of gestational diabetes		Na fluoride / EDTA K3 & Gel	The level of glucose for diagnosis of gestational diabetes (especially effective for pregnant women to detect latent diabetes).
Heparin & Gel		Lithium heparin & Gel Sodium heparin & Gel	Research of plasma in biochemical studies
EDTA & Gel		EDTA & Gel	Preparation of pure plasma for virus research and molecular diagnostics

ACD-A, ACD-B



ACD-A, ACD-B

Immunology, and are also intended for testing blood groups and blood storage



Description of base tubes

Lind-Vac®

Vacuum tube with no additive

Tubes are used to take samples of biological fluids (blood, urine, cerebrospinal fluid, exudates, etc.).

Usage: researches of biological fluids in clinical chemistry, serology, immunology.

Can be used as primary tubes for tests, storage and transportation of biomaterials.

Specimen: serum or other biological fluids.

Clotting time: 60 minutes.

Conditions of centrifugation: 1300 g for 10 minutes.
Before centrifuging the tubes with serum it is necessary to wait until blood clotting.

Color code: Red



No additive

REF	Size (mm)	Volume (ml)
NE1302	13*75	3
NE1402	13*75	4
NE2302	13*100	3
NE2402	13*100	4
NE2502	13*100	5
NE2602	13*100	6
NE2702	13*100	7
NE3902	16*100	9

Vacuum tube with clot activator

Serum Separation tubes are covered with clot activator powder to accelerate blood coagulation.

Silica (clot activator) is used as the activator.

Serum is a substance freed from the fibrinogen but containing fragments of thrombocyte and product of the metabolism.

Usage: to research serum in the clinical chemistry, immunology, serology, protein electrophoresis.

Specimen: serum.

Clotting time: from 10 to 30 minutes.

Conditions of centrifugation: 1500-1800 g for 10 minutes.

Before centrifuging the tubes with serum it is necessary to wait until blood clotting.

Color code: Red



Clot activator

REF	Size (mm)	Volume (ml)
AE1402	13*75	4
AE1502	13*75	5
AE2302	13*100	3
AE2402	13*100	4
AE2502	13*100	5
AE2602	13*100	6
AE2702	13*100	7
AE3802	16*100	8
AE3902	16*100	9
AE3102	16*100	10



Vacuum tube with clot activator & gel

As the activator it is used silica dioxide and biologically inert olefin gel.

Gel provides the separation of serum and clot up to 48 hours without re- centrifugation.

Gel is the special material intended for formation of barrier between cellular components of blood and serum during centrifugation.

The steady barrier is formed within 5 minutes after centrifugation is finished.

There is added gel silica dioxide in the test tube providing a complete clotting during the 30 min.

After capturing of blood sample into the vacuum tube with gel, it should be mixed 5-6 times.

Usage: to research serum in the clinical chemistry, immunology, serology, protein electrophoresis.

Specimen: serum.

Clotting time: from 5 to 30 minutes.

Conditions of centrifugation: 1800-2000 g for 10 minutes.

Test tubes with gel should be centrifuged no later than 2 hours after blood collection. The tubes can be frozen up to -20 ° C.

The Serum Separation Gel can not be re-centrifuged in order to avoid hemolysis of a specimen.

It is forbidden to use an angular rotor while the centrifuging gel tubes that to avoid getting a part of erythrocytes into the serum.

Color code: Yellow



Clot activator & gel		
REF	Size (mm)	Volume (ml)
AG1352	13*75	3.5
AG1402	13*75	4
AG2302	13*100	3
AG2402	13*100	4
AG2502	13*100	5
AG2602	13*100	6
AG3802	16*100	8
AG3852	16*100	8.5



Vacuum tube with thrombin

Thrombin is used for any laboratory tests, especially for rapid tests. A material is blood serum.

An inside surface of a tube is processed by a complex filler "thrombin with silica" that facilitates the rapid clots forming. After the process of centrifuging it allows to get a sample of serum for further researches much more rapidly. Using thrombin blood collection tubes it is possible to get more cleaned of fibrin threads and clots serum than using no additive tubes.

Usage: rapid tests of the serum in Clinic Chemistry, Immunology, Serology, protein electrophoresis.

Specimen: blood serum.

Clotting time: 3-5 minutes.

Centrifugation conditions: 1500-1800 g during 10 minutes.

Before centrifuging of tubes with the serum it is important to wait until full clotting.

Color code: Orange



REF	Size (mm)	Thrombin
		Volume (ml)
BE1202	13*75	2
BE1402	13*75	4
BE2502	13*100	5
BE3802	16*100	8
BE3902	16*100	9

Vacuum tube with thrombin & gel

Gel ensures dividing the serum and the clot during 48 hours without the additional centrifugation.

Into the thrombin & gel blood collection tube is added the filler "thrombin with silica" in an amount that facilitates the full clotting during 30 minutes.

Because of more accurate clotting a volume of the serum in the thrombin & gel blood collection tube is higher than in standard tubes.

Usage: rapid tests of the serum in Clinic Chemistry, Immunology, Serology, protein electrophoresis.

Specimen: blood serum.

Clotting time: 3-5 minutes.

Centrifugation conditions: 1500-2000 g during 10 minutes.

It is important to centrifuge gel tubes not later than in 2 hours after blood collection.

Is not recommended to centrifuge gel blood collection tubes twice in avoiding the hemolysis of a sample.

It is forbidden to use an angular rotor while the centrifuging gel tubes that to avoid getting a part of erythrocytes into the serum.

The collected sample should be mixed by turning the tube 5-6 times after the collection into gel tube.

Color code: Orange



REF	Size (mm)	Thrombin & gel
		Volume (ml)
BG1202	13*75	2
BG1402	13*75	4
BG2502	13*100	5
BG3802	16*100	8
BG3902	16*100	9

Vacuum tube for Hematology (potassium EDTA)

Additive: potassium salt of EDTA (ethylenediaminetetraacetate).

In accordance with international practice it is possible to use three options of EDTA:

- EDTA K3;
- EDTA K2;
- EDTA Na2

In vacuum tubes anticoagulant is added in powder EDTA K2 or EDTA K3 solution, concentration reaches 1.8 mg/ml in test tubes completely filled with blood.

After taking blood into the tube it should be mixed by turning 6-8 times. Lack of mixing can also cause platelet aggregation, coagulation or formation of micro clots.

Specimen: whole blood

Color code: Purple



EDTA K2		
REF	Size (mm)	Volume (ml)
EE1102	13*75	1
EE1202	13*75	2
EE1302	13*75	3
EE1402	13*75	4
EE1502	13*75	5
EE2402	13*100	4
EE2502	13*100	5
EE2602	13*100	6
EE3902	16*100	9
EE3952	16*100	9.5

EDTA K3		
REF	Size (mm)	Volume (ml)
TE1102	13*75	1
TE1202	13*75	2
TE1302	13*75	3
TE1402	13*75	4
TE1502	13*75	5
TE2402	13*100	4
TE2502	13*100	5
TE2602	13*100	6
TE3902	16*100	9
TE3952	16*100	9.5

EDTA K2 & Gel		
REF	Size (mm)	Volume (ml)
EG1202	13*75	2
EG1402	13*75	4
EG2402	13*100	4
EG2502	13*100	5
EG3902	16*100	9

EDTA K3 & Gel		
REF	Size (mm)	Volume (ml)
TG1202	13*75	2
TG1402	13*75	4
TG2402	13*100	4
TG2502	13*100	5
TG3902	16*100	9



Vacuum tube for coagulation (citrate)

Additive: to research the hemostatic system there is used trisodium citrate liquid concentration in vacuum tubes:

0.109mol/l - 3.20% (32.0g/l);

0.129mol/l - 3.80% (38.0g/l).

The volume ratio of blood and sodium citrate is 9:1.

Sodium citrate is an anticoagulant for collection of venous blood to research coagulation properties of blood.

Anti-coagulative properties of citrate are shown in complex formation with ions of Ca²⁺ and effective removal them from blood.

Usage: to research the hemostatic system.

Specimen: plasma.

Immediately after taking the blood into the tube with citrate it must be carefully mixed at least 5 times to prevent micro clots.

Requirements according to the NCCLS H21-A4 recommendations:

Samples of tests (e.g. thrombin time, Protein C, Factor V and Factor VII) can be stored at temperature 18-24 ° C and temperature 2-4 ° C, and should be centrifuged and analyzed no later than 4 hours after blood collection.

If it is not possible to make test for PV during 24 hours and for other analyses during 4 hours plasma must be separated from blood cells (transfused into another tube) and frozen after centrifuging.

Freezing samples may influence the results of the APTT.

Conditions of centrifugation: 2000-2500 g for 10-15 minutes.

Color code: Blue



Sodium citrate 3,8%

REF	Size (mm)	Volume (ml)
SE1272	13*75	2.7
SE1362	13*75	3.6
SE1452	13*75	4.5
SE2182	13*100	1.8
SE2272	13*100	2.7
SE2362	13*100	3.6
SE2452	13*100	4.5
SE3902	16*100	9

Sodium citrate 3,2%

REF	Size (mm)	Volume (ml)
KE1272	13*75	2.7
KE1352	13*75	3.5
KE1362	13*75	3.6
KE1452	13*75	4.5
KE2182	13*100	1.8
KE2272	13*100	2.7
KE2362	13*100	3.6
KE2452	13*100	4.5
KE3902	16*100	9

Vacuum tube for ESR

Additive: liquid trisodium citrate in a concentration of 0.129mol/l - 3.80% (38.0g/l).

Sodium citrate is an anticoagulant for collection of venous blood to research coagulation characteristics of blood.

It is used for the measurement of an erythrocyte sedimentation rate. Definition of indicators ESR occurs at an accelerated rate.

Specimen: whole blood

Color code: Black



ESR (sodium citrate)

REF	Size (mm)	Volume (ml)
RE1162	13*75	1.6
RE1242	13*75	2.4
RE1202	13*75	2.0
RE1302	13*75	3.0



Vacuum tube for plasma separation (lithium / sodium heparin)

Additive: Lithium or Sodium Heparin

Heparin is a natural anticoagulant which presents in any healthy body. Heparin is used to take the plasma and in chemical researches.

Plasma is freed from the cells by the centrifugation. Clotting of blood is prevented by the addition of an anticoagulant directly after the taking of blood.

For this purpose, the lithium or sodium heparin is added in this tube.

Advantages in comparison with serum:

The bigger volume of material in the same volume of blood. The results are independent on the condition of the coagulation system. The results are closer to in vivo.

Lower risk of hemolysis and thrombocytosis.

Specimen: heparin plasma.

The powder heparin is applied to the inner wall of the tube.

The tubes contain a reagent at 12 - 30 IU of heparin per 1 ml of blood.

Immediately after taking the blood into the tube with heparin it must be carefully mixed at least 8-10 time.

Conditions of centrifugation: 1300 g for 10 minutes.

Centrifugation should be made right after the drawing the blood into the tubes.

Color code: Green



Lithium heparin

REF	Size (mm)	Volume (ml)
LE1302	13*75	3
LE1402	13*75	4
LE2302	13*100	3
LE2402	13*100	4
LE2502	13*100	5
LE2602	13*100	6
LE3902	16*100	9

Sodium heparin

REF	Size (mm)	Volume (ml)
HE1302	13*75	3
HE1402	13*75	4
HE2302	13*100	3
HE2502	13*100	5
HE2602	13*100	6
HE3902	16*100	9

Sodium heparin & gel

REF	Size (mm)	Volume (ml)
HG1402	13*75	4
HG2302	13*100	3
HG2502	13*100	5
HG3802	16*100	8

Lithium heparin & gel

REF	Size (mm)	Volume (ml)
LG1402	13*75	4
LG2302	13*100	3
LG3802	16*100	8



Vacuum tube for glucose determination
(fluoride)

Additive: test tubes contain anticoagulant and the glucose stabilizer.

K3-EDTA, K2-EDTA, EDTA-Na, K oxalate, Li heparin, Na heparin can be used as an anticoagulant.

Na fluoride stabilizes blood sugar levels for up to 24 hours.

Additives:

Potassium oxalate / Na fluoride

K3-EDTA / Na fluoride

K2-EDTA / Na fluoride

EDTA-Na2 / Na fluoride

Li heparin / Na fluoride

Na heparin / Na fluoride

Addition of sodium fluoride and potassium EDTA into the test tube allows to prevent blood glucose destruction (a process called glycolysis) and keep its level in the taken sample of blood.

Sodium fluoride and potassium oxalate act as anticoagulants connecting ions of Ca2+. Moreover, sodium fluoride stabilizes the glucose level.

Specimen: plasma.

Vacuum test tubes for glucose should be filled completely to the specified mark on the label, the excess oxalate in it can cause hemolysis.

After drawing the blood into the tube it should be mixed by turning 6-8 times.

Because tubes with fluoride / oxalate are exposed to hemolysis much more than other they must be mixed with extreme caution.

Conditions of centrifugation: 1300 g for 10 minutes.

Centrifugation should be made right after taking the blood into the tubes.

Color code: Grey



Glucose tubes

REF	Size (mm)	Volume (ml)
FE1202	13*75	2
FE1402	13*75	4
FE2202	13*100	2
FE2302	13*100	3
FE2402	13*100	4
FE2502	13*100	5
FE2602	13*100	6
FE3902	16*100	9



* upon the request other specifications can be produced

Vacuum tube for analysis of free extracellular DNA

NEW

A vacuum tube is designed to collect venous blood for the subsequent analysis of free extracellular DNA. This kind of analysis is necessary for examination of DNA fragments. These can be, for example, fragments of fetal DNA in the blood of the mother. It's analysis lets determine the gender of the child at the early stages of development and identify some hereditary multations.

Also among free extracellular DNA there may be DNA fragments with somatic mutations resulting from carcinogenesis. Analysis of these fragments (liquid biopsy) allows you to diagnose the presence of malignant neoplasms at the early stages.

Another area of application of the test tube is hematological or genetic studies that require a long-term storag of blood. The use of additional preservatives ensures better preservation of blood cells and protects against hemolysis. Therefore, this tube shuold be used if long-term storage or shipment under temperature fluctuations is needed.

Extracellular DNA stabilization is possible for period of 7-14 days at a storage temperature of 4-30 C.

Specimen: whole blood.

Usage: examination of DNA fragments, hematological or genetic studies.

Conditions of centrifugation:

2000-6000 G during 10 minutes. The speed of centrifugation depends on a type of the DNA isolation kit used.

Color code: Ligt lilac

DNA

Size (mm)	Volume (ml)
WE1102 13*75	1
WE1302 13*75	3
WE2402 13*100	4
WE3802 16*100	8



Vacuum tube for determination of glucose level in blood plasma for diagnostics of gestational diabetes

The system is used for the precise determination of glucose level in blood plasma (for diagnostics of gestational diabetes) during 24 hours after venous blood drawing.

If to follow the rules for the venous blood collection and its storage (without freezing and the temperature of the storage must not be higher than +25°C) the glucose level will not be reduced during the prescribed time, the hemolysis of samples while the transport will be prevented, that is an advantage for using in centralized laboratories.

It is possible to determine the glucose level in a primary tube after the centrifugation without a risk of capturing erythrocytes by an analyzer.

The vacuum systems with fluoride and gel are the optimal decision for centralized laboratories where blood samples are transported between 2 and 24 hours after venous blood collection.

Specimen: plasma.

Additive: test tubes contain anticoagulant, glucose stabilizer and gel

Options of additives: Potassium oxalate / Na fluoride / Gel

K3-EDTA / Na fluoride / Gel

K2-EDTA / Na fluoride / Gel

Conditions of centrifugation:

1500-2000 g for 10 minutes.

Centrifugation should be made right after taking the blood into the tubes.

Color code: Olive

Glucose for the diagnosis of gestational diabetes. Potassium Oxalate/Na Fluoride/Gel Separator

Size (mm)	Volume (ml)
-----------	-------------

FG1102 13*75	1
FG2202 13*100	2
FG2402 13*100	4
FG3802 16*100	8

K3-EDTA/Na Fluoride/Gel Separator

IG1102 13*75	1
IG2202 13*100	2
IG3802 16*100	8

K2-EDTA/Na Fluoride/Gel Separator

JG1102 13*75	1
JG2202 13*100	2
JG3802 16*100	8



Vacuum tube with ACD-A, ACD-B

Immunohematology tubes are used for blood group analysis and blood storage.

Immunohematology tubes are available with an ACD solution (Acid Citrat Dextrose - citric acid, trisodium citrate, dextrose) in two versions of ACD-A or ACD-B.

Usage: test tubes can be used in immunology, and are also intended for testing blood groups and blood storage.

Specimen: stabilized whole blood.

Conditions of centrifugation: not required

The composition of the reagents additives allows to stabilize the energy metabolism of cells and store them at a temperature of +1 ... 6 ° C for 21 days.

Color code: lemon yellow.

ACD-A tubes			ACD-B tubes		
REF	Size (mm)	Volume (ml)	REF	Size (mm)	Volume (ml)
CE1202	13*75	2	DE1202	13*75	2
CE1402	13*75	4	DE1402	13*75	4
CE2502	13*100	5	DE2502	13*100	5
CE2602	13*100	6	DE2602	13*100	6
CE3802	16*100	8	DE3802	16*100	8
CE3902	16*100	9	DE3902	16*100	9
CE3102	16*100	10	DE3102	16*100	10

Sterile Safety-Lancets

Enable the safe, gentle collection of capillary blood. Since the needle point or blade is safely concealed before and after use, the risk of needle injuries and cross contamination is eliminated when the lancets are used according to the instructions. Our product range covers the most varied of skin types and the entire range of blood volumes to be extracted. The lancets cannot technically be reused once they have been triggered, and can be safely disposed of in our disposal boxes.



Blood collection set with a holder

REF	Needle size	Needle diameter	Catheter length	Color code
BH2012	20G x 3/4" x 12"	0,9 mm	300 mm	
BH2007	20G x 3/4" x 7"	0,9 mm	180 mm	
BH2112	21G x 3/4" x 12"	0,8 mm	300 mm	
BH2107	21G x 3/4" x 7"	0,8 mm	180 mm	
BH2212	22G x 3/4" x 12"	0,7 mm	300 mm	
BH2207	22G x 3/4" x 7"	0,7 mm	180 mm	
BH2312	23G x 3/4" x 12"	0,6 mm	300 mm	
BH2307	23G x 3/4" x 7"	0,6 mm	180 mm	
BH2412	24G x 3/4" x 12"	0,55 mm	300 mm	
BH2407	24G x 3/4" x 7"	0,55 mm	180 mm	
BH2512	25G x 3/4" x 12"	0,5 mm	300 mm	
BH2507	25G x 3/4" x 7"	0,5 mm	180 mm	



Safety blood collection set

REF	Needle size	Needle diameter	Catheter length	Color code
SS1912	19G x 3/4" x 12"	1,1 mm	300 mm	
SS1907	19G x 3/4" x 7"	1,1 mm	180 mm	
SS2112	21G x 3/4" x 12"	0,8 mm	300 mm	
SS2107	21G x 3/4" x 7"	0,8 mm	180 mm	
SS2212	22G x 3/4" x 12"	0,7 mm	300 mm	
SS2207	22G x 3/4" x 7"	0,7 mm	180 mm	
SS2312	23G x 3/4" x 12"	0,6 mm	300 mm	
SS2307	23G x 3/4" x 7"	0,6 mm	180 mm	
SS2512	25G x 3/4" x 12"	0,5 mm	300 mm	
SS2507	25G x 3/4" x 7"	0,5 mm	180 mm	



Safety blood collection set with a holder

REF	Needle size	Needle diameter	Catheter length	Color code
BS1912	19G x 3/4" x 12"	1,1 mm	300 mm	
BS1907	19G x 3/4" x 7"	1,1 mm	180 mm	
BS2112	21G x 3/4" x 12"	0,8 mm	300 mm	
BS2107	21G x 3/4" x 7"	0,8 mm	180 mm	
BS2212	22G x 3/4" x 12"	0,7 mm	300 mm	
BS2207	22G x 3/4" x 7"	0,7 mm	180 mm	
BS2312	23G x 3/4" x 12"	0,6 mm	300 mm	
BS2307	23G x 3/4" x 7"	0,6 mm	180 mm	
BS2512	25G x 3/4" x 12"	0,5 mm	300 mm	
BS2507	25G x 3/4" x 7"	0,5 mm	180 mm	



Holder

It is one of the components of vacuum blood collection systems. It is used to fix multi sample needles.

Safety holder

Safety holder with special needle protection is used to close the needle after venipuncture that makes blood collection procedure even more safety.

Luer adapter

Designed to connect intravenous catheters, perfusion devices and needles with Luer connectors with vacuum systems for blood collection. Luer adapter is provided with a thread for screwing into a holder and a safe rubber stopper.



HC01 Holder

SH01 Safety holder

LA2112 Luer adapter

Multi sample needle

REF	Needle size	Needle diameter	Needle length	Color code
MN1812	18G x 1 ½"	1,2 mm	38 mm	
MN1810	18G x 1"	1,2 mm	25 mm	
MN2012	20G x 1 ½"	0,9 mm	38 mm	
MN2010	20G x 1"	0,9 mm	25 mm	
MN2112	21G x 1 ½"	0,8 mm	38 mm	
MN2110	21G x 1"	0,8 mm	25 mm	
MN2212	22G x 1 ½"	0,7 mm	38 mm	
MN2210	22G x 1"	0,7 mm	25 mm	
MN2312	23G x 1 ½"	0,6 mm	38 mm	
MN2310	23G x 1"	0,6 mm	25 mm	



Multi sample needle with visual control (flash back)

REF	Needle size	Needle diameter	Needle length	Color code
VN2112	21G x 1 ½"	0,8 mm	38 mm	
VN2110	21G x 1"	0,8 mm	25 mm	
VN2212	22G x 1 ½"	0,7 mm	38 mm	
VN2210	22G x 1"	0,7 mm	25 mm	
VN2312	23G x 1 ½"	0,6 mm	38 mm	
VN2310	23G x 1"	0,6 mm	25 mm	




Safety needle set with a holder

REF	Needle size	Needle diameter	Needle length	Color code
HS2012	20G x 1-1 ½"	0,9 mm	38 mm	
HS2112	21G x 1-1 ½"	0,8 mm	38 mm	
HS2212	22G x 1-1 ½"	0,7 mm	38 mm	
HS2312	23G x 1-1 ½"	0,6 mm	38 mm	
HS2410	24G x 1"	0,55 mm	25 mm	
HS2510	25G x 1"	0,5 mm	25 mm	
HS2610	26G x 1"	0,45 mm	25 mm	
HS2710	27G x 1"	0,4 mm	25 mm	




Blood collection set

REF	Needle size	Needle diameter	Catheter length	Color code
SN2012	20G x 3/4" x 12"	0,9 mm	300 mm	
SN2007	20G x 3/4" x 7"	0,9 mm	180 mm	
SN2112	21G x 3/4" x 12"	0,8 mm	300 mm	
SN2107	21G x 3/4" x 7"	0,8 mm	180 mm	
SN2212	22G x 3/4" x 12"	0,7 mm	300 mm	
SN2207	22G x 3/4" x 7"	0,7 mm	180 mm	
SN2312	23G x 3/4" x 12"	0,6 mm	300 mm	
SN2307	23G x 3/4" x 7"	0,6 mm	180 mm	
SN2412	24G x 3/4" x 12"	0,55 mm	300 mm	
SN2407	24G x 3/4" x 7"	0,55 mm	180 mm	
SN2512	25G x 3/4" x 12"	0,5 mm	300 mm	
SN2507	25G x 3/4" x 7"	0,5 mm	180 mm	

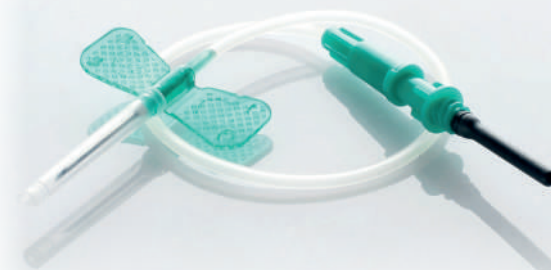


Venipuncture techniques by Multi Sample needles

1. Label the required tubes, specifying the name of the patient, department (in order to exclude errors when identifying the biomaterial sample).
2. Treat your hands hygienically, dry them.
3. Treat your hands with an antiseptic. Do not dry; wait until the antiseptic is completely dry.
4. Put gloves on hands.
5. Select tubes corresponding to required laboratory tests; prepare a needle, a holder, alcohol wipes, and a plaster.
6. Place a tourniquet on the arm 7-10 cm above the venipuncture place. Tourniquet must be applied no more than one minute. A longer vein squeeze time can influence the test results due to changes in the concentration of parameters in the blood.
7. Ask the patient to clench a hand into a fist. Do not give physical exertion to the arm, like "clenching and unclenching of a fist" because it can influence the test results due to changes in the concentration of parameters in the blood.
8. Select the venipuncture place. The ulnar and saphenous veins are the most common but smaller and fuller veins of the wrist and hand can be punctured too. Depending on the characteristics of the vein select the most convenient option for the venipuncture: a multisample needle or a blood collection set (a butterfly needle).
9. Take the needle and remove the protective cap.
10. Attach the needle into the holder.
11. Disinfect the venipuncture site with a gauze napkin or a pad moistened with an antiseptic solution, in a circular motion from the center to the periphery.
12. Wait until the antiseptic solution is completely dry.
13. Remove the cap on the other side of the needle. Position the needle along the line with the vein level up and puncture the vein at an angle of 15-30° to the skin.
14. Insert the prepared tube into the needle holder until it stops and hold it until the blood stops flowing into the tube. The tourniquet must be removed or released immediately after the blood flow has started leaking into the tube. Make sure the patient unclenches his fist. The blood passes into the tube until it completely compensates for the created vacuum. If the blood does not flow it means that the needle has gone through the vein. In this case there is need to pull out the needle slightly but not to remove it completely. Do it until the blood goes into the tube. The certainty of filling the tube is $\pm 10\%$ of the nominal volume.
15. Remove the tube from the holder. After filling the tube it must be immediately gently inverted to mix the sample with the filler: tubes without anticoagulants - 5-6 times; tubes with citrate - 3-4 times; tubes with heparin, EDTA and other additives - 8-10 times.
16. You can attach a number of other tubes to the holder to draw blood for various researches.
17. After all the required tubes are filled in put a dry sterile cloth on the venipuncture site and remove the needle. Make sure that the patient does not have external bleeding in the area of venipuncture. Apply a pressure bandage on the arm or a bactericidal plaster.

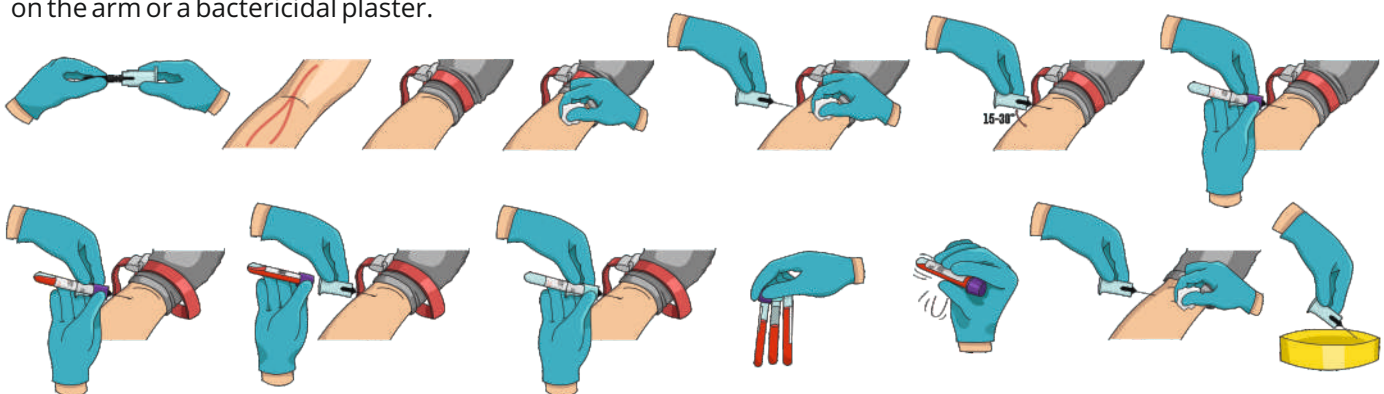

Recommended order of taking blood with tubes

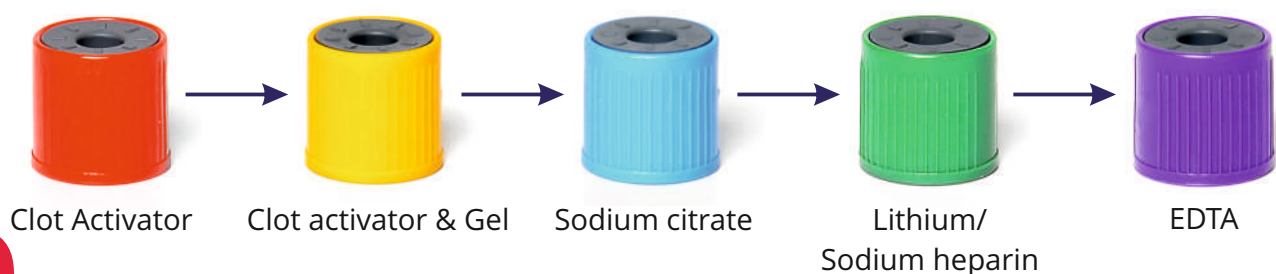

Symbol	Description
	Symbol for "Do Not Reuse"
	Symbol for "Use By"
	Symbol for "Batch Code"
	Symbol for "Catalogue Number"
	Symbol for "Date of Manufacture"
	Symbol for "Manufacturer"
	Symbol for "Sterilized Using Irradiation"
	CE Mark
	Symbol for "In Vitro Diagnostic Medical Device"
	Symbol for "Temperature Limitation"

Labels



VACUUM BLOOD
COLLECTION TUBES **Lind-Vac®**

Additive: **Clot activator & Gel**

Size: 13x75 mm

Volume: 3,5 ml

Q-ty: 100 psc

2018.08

2019.09

09343

REF

AG1352

STERILE

R


IVD

2

5°C

25°C

CE

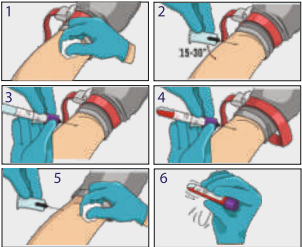



InterVacTechnology Ltd.,
Kadastiku 57, Narva, Estonia
+ (372) 35 71 007

info@intervactechnology.com

www.intervactechnology.com

Label on the rack

Lind-Vac®

Clot activator

REF

IVD

2

ml

CE

InterVacTechnology Ltd.

Estonia

08654

08654

Lind-Vac®

Clot activator

REF

IVD

CE

2

ml

InterVacTechnology Ltd.

Estonia

Standart label

Label with double code

Labels can be made under the order in any language and with the stated barcodes

* in this directory is an example of the label, the manufacturer can change the appearance of the labels

Packing

The tubes are packed in a foamed styrene rack and protective film.
 The tubes 13mm x 75mm and 13mm x 100mm are packed into the rack of 100 pieces.
 The tubes 16mm x 100mm are packed into the rack of 50 pieces.







OÜ InterVacTechnology

Kadastiku 57, 21004, Narva, Estonia

www.intervactechnology.com

e-mail: info@intervactechnology.com


Tel.: +372 35 71 007

Fax: +372 35 71 012



Date: November 2018


Blood Collection Tubes			
Brand name	Additive	Volume, ml / Size	Catalogue Number
Lind-Vac	No additive	0,5ml, 13*75	NE1052
Lind-Vac	No additive	1ml, 13*75	NE1102
Lind-Vac	No additive	2ml, 13*75	NE1202
Lind-Vac	No additive	3ml, 13*75	NE1302
Lind-Vac	No additive	4ml, 13*75	NE1402
Lind-Vac	No additive	5ml, 13*75	NE1502
Lind-Vac	No additive	3ml, 13*100	NE2302
Lind-Vac	No additive	4ml, 13*100	NE2402
Lind-Vac	No additive	5ml, 13*100	NE2502
Lind-Vac	No additive	6ml, 13*100	NE2602
Lind-Vac	No additive	7ml, 13*100	NE2702
Lind-Vac	No additive	8ml, 16*100	NE3802
Lind-Vac	No additive	9ml, 16*100	NE3902
Lind-Vac	No additive	10ml, 16*100	NE3102
Lind-Vac	ESR	0,5ml, 13*75	RE1052
Lind-Vac	ESR	1,6ml, 13*75	RE1162
Lind-Vac	ESR	2,0ml, 13*75	RE1202
Lind-Vac	ESR	2,4ml, 13*75	RE1242
Lind-Vac	ESR	3,0ml, 13*75	RE1302
Lind-Vac	ESR	1,6ml, 13*100	RE2162
Lind-Vac	ESR	2,4ml, 13*100	RE2242
Lind-Vac	Thrombin	0,5ml, 13*75	BE1052
Lind-Vac	Thrombin	1ml, 13*75	BE1102
Lind-Vac	Thrombin	2ml, 13*75	BE1202
Lind-Vac	Thrombin	3ml, 13*75	BE1302
Lind-Vac	Thrombin	4ml, 13*75	BE1402
Lind-Vac	Thrombin	5ml, 13*100	BE2502
Lind-Vac	Thrombin	6ml, 13*100	BE2602
Lind-Vac	Thrombin	8ml, 16*100	BE3802
Lind-Vac	Thrombin	9ml, 16*100	BE3902
Lind-Vac	Thrombin	10ml, 16*100	BE3102
Lind-Vac	Thrombin & Gel Separator	0,5ml, 13*75	BG1052
Lind-Vac	Thrombin & Gel Separator	1ml, 13*75	BG1102
Lind-Vac	Thrombin & Gel Separator	2ml, 13*75	BG1202
Lind-Vac	Thrombin & Gel Separator	3ml, 13*75	BG1302
Lind-Vac	Thrombin & Gel Separator	4ml, 13*75	BG1402
Lind-Vac	Thrombin & Gel Separator	5ml, 13*100	BG2502
Lind-Vac	Thrombin & Gel Separator	6ml, 13*100	BG2602
Lind-Vac	Thrombin & Gel Separator	8ml, 16*100	BG3802
Lind-Vac	Thrombin & Gel Separator	9ml, 16*100	BG3902
Lind-Vac	Clot Activator	0,5ml, 13*75	AE1052
Lind-Vac	Clot Activator	1ml, 13*75	AE1102
Lind-Vac	Clot Activator	2ml, 13*75	AE1202
Lind-Vac	Clot Activator	3ml, 13*75	AE1302
Lind-Vac	Clot Activator	4ml, 13*75	AE1402
Lind-Vac	Clot Activator	5ml, 13*75	AE1502
Lind-Vac	Clot Activator	3ml, 13*100	AE2302
Lind-Vac	Clot Activator	4ml, 13*100	AE2402
Lind-Vac	Clot Activator	5ml, 13*100	AE2502
Lind-Vac	Clot Activator	6ml, 13*100	AE2602
Lind-Vac	Clot Activator	7ml, 13*100	AE2702
Lind-Vac	Clot Activator	8ml, 16*100	AE3802
Lind-Vac	Clot Activator	9ml, 16*100	AE3902
Lind-Vac	Clot Activator	10ml, 16*100	AE3102
Lind-Vac	Clot Activator&Gel	0,5ml, 13*75	AG1052
Lind-Vac	Clot Activator&Gel	1ml, 13*75	AG1102
Lind-Vac	Clot Activator&Gel	3ml, 13*75	AG1302
Lind-Vac	Clot Activator&Gel	3,5ml, 13*75	AG1352



List of products

Lind-Vac®


Lind-Vac	Clot Activator&Gel	4ml, 13*75	AG1402
Lind-Vac	Clot Activator&Gel	3ml, 13*100	AG2302
Lind-Vac	Clot Activator&Gel	4ml, 13*100	AG2402
Lind-Vac	Clot Activator&Gel	5ml, 13*100	AG2502
Lind-Vac	Clot Activator&Gel	6ml, 13*100	AG2602
Lind-Vac	Clot Activator&Gel	8ml, 16*100	AG3802
Lind-Vac	Clot Activator&Gel	8,5ml, 16*100	AG3852
Lind-Vac	Clot Activator&Gel	9ml, 16*100	AG3902
Lind-Vac	Sodium Citrate 3,2 %	0,5ml, 13*75	KE1052
Lind-Vac	Sodium Citrate 3,2 %	0,9ml, 13*75	KE1092
Lind-Vac	Sodium Citrate 3,2 %	1,8ml, 13*75	KE1182
Lind-Vac	Sodium Citrate 3,2 %	2 ml, 13*75	KE1202
Lind-Vac	Sodium Citrate 3,2 %	2,7ml, 13*75	KE1272
Lind-Vac	Sodium Citrate 3,2 %	3,5ml, 13*75	KE1352
Lind-Vac	Sodium Citrate 3,2 %	3,6ml, 13*75	KE1362
Lind-Vac	Sodium Citrate 3,2 %	4,5ml, 13*75	KE1452
Lind-Vac	Sodium Citrate 3,2 %	1,8ml, 13*100	KE2182
Lind-Vac	Sodium Citrate 3,2 %	2,7ml, 13*100	KE2272
Lind-Vac	Sodium Citrate 3,2 %	3,6ml, 13*100	KE2362
Lind-Vac	Sodium Citrate 3,2 %	4,5ml, 13*100	KE2452
Lind-Vac	Sodium Citrate 3,2 %	5,4ml, 13*100	KE2542
Lind-Vac	Sodium Citrate 3,2 %	6,3ml, 13*100	KE2632
Lind-Vac	Sodium Citrate 3,2 %	8,1ml, 16*100	KE3812
Lind-Vac	Sodium Citrate 3,2 %	9ml, 16*100	KE3902
Lind-Vac	Sodium Citrate 3,2 %, double walled	0,5ml, 13*75	KE5052
Lind-Vac	Sodium Citrate 3,2 %, double walled	0,9ml, 13*75	KE5092
Lind-Vac	Sodium Citrate 3,2 %, double walled	1,8ml, 13*75	KE5182
Lind-Vac	Sodium Citrate 3,2 %, double walled	2,7ml, 13*75	KE5272
Lind-Vac	Sodium Citrate 3,2 %, double walled	3 ml, 13*75	KE5302
Lind-Vac	Sodium Citrate 3,2 %, double walled	3,5 ml, 13*75	KE5352
Lind-Vac	Sodium Citrate 3,2 % + Gel Separator	0,5ml, 13*75	KG1052
Lind-Vac	Sodium Citrate 3,2 % + Gel Separator	0,9ml, 13*75	KG1092
Lind-Vac	Sodium Citrate 3,2 % + Gel Separator	1,8ml, 13*75	KG1182
Lind-Vac	Sodium Citrate 3,2 % + Gel Separator	2,7ml, 13*75	KG1272
Lind-Vac	Sodium Citrate 3,2 % + Gel Separator	3,6ml, 13*75	KG1362
Lind-Vac	Sodium Citrate 3,2 % + Gel Separator	1,8ml, 13*100	KG2182
Lind-Vac	Sodium Citrate 3,2 % + Gel Separator	2,7ml, 13*100	KG2272
Lind-Vac	Sodium Citrate 3,2 % + Gel Separator	3,6ml, 13*100	KG2362
Lind-Vac	Sodium Citrate 3,2 % + Gel Separator	4,5ml, 13*100	KG2452
Lind-Vac	Sodium Citrate 3,2 % + Gel Separator	5,4ml, 13*100	KG2542
Lind-Vac	Sodium Citrate 3,2 % + Gel Separator	8,1ml, 16*100	KG3812
Lind-Vac	Sodium Citrate 3,2 % + Gel Separator	9ml, 16*100	KG3902
Lind-Vac	Sodium Citrate 3,8 %	0,5ml, 13*75	SE1052
Lind-Vac	Sodium Citrate 3,8 %	0,9ml, 13*75	SE1092
Lind-Vac	Sodium Citrate 3,8 %	1,8ml, 13*75	SE1182
Lind-Vac	Sodium Citrate 3,8 %	2ml, 13*75	SE1202
Lind-Vac	Sodium Citrate 3,8 %	2,7ml, 13*75	SE1272
Lind-Vac	Sodium Citrate 3,8 %	3,5ml, 13*75	SE1352
Lind-Vac	Sodium Citrate 3,8 %	3,6ml, 13*75	SE1362
Lind-Vac	Sodium Citrate 3,8 %	4,5ml, 13*75	SE1452
Lind-Vac	Sodium Citrate 3,8 %	1,8ml, 13*100	SE2182
Lind-Vac	Sodium Citrate 3,8 %	2,7ml, 13*100	SE2272
Lind-Vac	Sodium Citrate 3,8 %	3,6ml, 13*100	SE2362
Lind-Vac	Sodium Citrate 3,8 %	4,5ml, 13*100	SE2452
Lind-Vac	Sodium Citrate 3,8 %	5,4ml, 13*100	SE2542
Lind-Vac	Sodium Citrate 3,8 %	6,3ml, 13*100	SE2632
Lind-Vac	Sodium Citrate 3,8 %	8,1ml, 16*100	SE3812
Lind-Vac	Sodium Citrate 3,8 %	9ml, 16*100	SE3902
Lind-Vac	Sodium Citrate 3,8 %, double walled	0,5ml, 13*75	SE5052
Lind-Vac	Sodium Citrate 3,8 %, double walled	0,9ml, 13*75	SE5092



List of products

Lind-Vac®


Lind-Vac	Sodium Citrate 3,8 %, double walled	1,8ml, 13*75	SE5182
Lind-Vac	Sodium Citrate 3,8 %, double walled	2,7ml, 13*75	SE5272
Lind-Vac	Sodium Citrate 3,8 %, double walled	3 ml, 13*75	SE5302
Lind-Vac	Sodium Citrate 3,8 %, double walled	3,5 ml, 13*75	SE5352
Lind-Vac	Sodium Citrate 3,8 % + Gel Separator	0,5ml, 13*75	SG1052
Lind-Vac	Sodium Citrate 3,8 % + Gel Separator	0,9ml, 13*75	SG1092
Lind-Vac	Sodium Citrate 3,8 % + Gel Separator	1,8ml, 13*75	SG1182
Lind-Vac	Sodium Citrate 3,8 % + Gel Separator	2,7ml, 13*75	SG1272
Lind-Vac	Sodium Citrate 3,8 % + Gel Separator	3,6ml, 13*75	SG1362
Lind-Vac	Sodium Citrate 3,8 % + Gel Separator	1,8ml, 13*100	SG2182
Lind-Vac	Sodium Citrate 3,8 % + Gel Separator	2,7ml, 13*100	SG2272
Lind-Vac	Sodium Citrate 3,8 % + Gel Separator	3,6ml, 13*100	SG2362
Lind-Vac	Sodium Citrate 3,8 % + Gel Separator	4,5ml, 13*100	SG2452
Lind-Vac	Sodium Citrate 3,8 % + Gel Separator	5,4ml, 13*100	SG2542
Lind-Vac	Sodium Citrate 3,8 % + Gel Separator	8,1ml, 16*100	SG3812
Lind-Vac	Sodium Citrate 3,8 % + Gel Separator	9ml, 16*100	SG3902
Lind-Vac	Potassium Oxalate/Na Fluoride	0,5ml, 13*75	FE1052
Lind-Vac	Potassium Oxalate/Na Fluoride	1ml, 13*75	FE1102
Lind-Vac	Potassium Oxalate/Na Fluoride	2ml, 13*75	FE1202
Lind-Vac	Potassium Oxalate/Na Fluoride	3ml, 13*75	FE1302
Lind-Vac	Potassium Oxalate/Na Fluoride	4ml, 13*75	FE1402
Lind-Vac	Potassium Oxalate/Na Fluoride	2ml, 13*100	FE2202
Lind-Vac	Potassium Oxalate/Na Fluoride	3ml, 13*100	FE2302
Lind-Vac	Potassium Oxalate/Na Fluoride	4ml, 13*100	FE2402
Lind-Vac	Potassium Oxalate/Na Fluoride	5ml, 13*100	FE2502
Lind-Vac	Potassium Oxalate/Na Fluoride	6ml, 13*100	FE2602
Lind-Vac	Potassium Oxalate/Na Fluoride	8ml, 16*100	FE3802
Lind-Vac	Potassium Oxalate/Na Fluoride	9ml, 16*100	FE3902
Lind-Vac	Potassium Oxalate/Na Fluoride+ Gel Separator	0,5ml, 13*75	FG1052
Lind-Vac	Potassium Oxalate/Na Fluoride+ Gel Separator	1ml, 13*75	FG1102
Lind-Vac	Potassium Oxalate/Na Fluoride+ Gel Separator	2ml, 13*75	FG1202
Lind-Vac	Potassium Oxalate/Na Fluoride+ Gel Separator	3ml, 13*75	FG1302
Lind-Vac	Potassium Oxalate/Na Fluoride+ Gel Separator	2ml, 13*100	FG2202
Lind-Vac	Potassium Oxalate/Na Fluoride+ Gel Separator	3ml, 13*100	FG2302
Lind-Vac	Potassium Oxalate/Na Fluoride+ Gel Separator	4ml, 13*100	FG2402
Lind-Vac	Potassium Oxalate/Na Fluoride+ Gel Separator	5ml, 13*100	FG2502
Lind-Vac	Potassium Oxalate/Na Fluoride+ Gel Separator	8ml, 16*100	FG3802
Lind-Vac	Potassium Oxalate/Na Fluoride+ Gel Separator	9ml, 16*100	FG3902
Lind-Vac	K2 EDTA	0,5ml, 13*75	EE1052
Lind-Vac	K2 EDTA	1ml, 13*75	EE1102
Lind-Vac	K2 EDTA	2ml, 13*75	EE1202
Lind-Vac	K2 EDTA	3ml, 13*75	EE1302
Lind-Vac	K2 EDTA	4ml, 13*75	EE1402
Lind-Vac	K2 EDTA	5ml, 13*75	EE1502
Lind-Vac	K2 EDTA	4ml, 13*100	EE2402
Lind-Vac	K2 EDTA	5ml, 13*100	EE2502
Lind-Vac	K2 EDTA	6ml, 13*100	EE2602
Lind-Vac	K2 EDTA	8ml, 16*100	EE3802
Lind-Vac	K2 EDTA	9ml, 16*100	EE3902
Lind-Vac	K2 EDTA	9,5ml, 16*100	EE3952
Lind-Vac	K2 EDTA	10ml, 16*100	EE3102
Lind-Vac	K2 EDTA + Gel Separator	0,5ml, 13*75	EG1052
Lind-Vac	K2 EDTA + Gel Separator	1ml, 13*75	EG1102
Lind-Vac	K2 EDTA + Gel Separator	2ml, 13*75	EG1202
Lind-Vac	K2 EDTA + Gel Separator	3ml, 13*75	EG1302
Lind-Vac	K2 EDTA + Gel Separator	4ml, 13*75	EG1402
Lind-Vac	K2 EDTA + Gel Separator	4ml, 13*100	EG2402
Lind-Vac	K2 EDTA + Gel Separator	5ml, 13*100	EG2502
Lind-Vac	K2 EDTA + Gel Separator	6ml, 13*100	EG2602
Lind-Vac	K2 EDTA + Gel Separator	8ml, 16*100	EG3802



List of products

Lind-Vac®


Lind-Vac	K2 EDTA + Gel Separator	9ml, 16*100	EG3902
Lind-Vac	K2 EDTA/Na Fluoride	0,5ml, 13*75	JE1052
Lind-Vac	K2 EDTA/Na Fluoride	1ml, 13*75	JE1102
Lind-Vac	K2 EDTA/Na Fluoride	2ml, 13*75	JE1202
Lind-Vac	K2 EDTA/Na Fluoride	3ml, 13*75	JE1302
Lind-Vac	K2 EDTA/Na Fluoride	4ml, 13*75	JE1402
Lind-Vac	K2 EDTA/Na Fluoride	2ml, 13*100	JE2202
Lind-Vac	K2 EDTA/Na Fluoride	3ml, 13*100	JE2302
Lind-Vac	K2 EDTA/Na Fluoride	4ml, 13*100	JE2402
Lind-Vac	K2 EDTA/Na Fluoride	5ml, 13*100	JE2502
Lind-Vac	K2 EDTA/Na Fluoride	8ml, 16*100	JE3802
Lind-Vac	K2 EDTA/Na Fluoride	9ml, 16*100	JE3902
Lind-Vac	K2 EDTA/Na Fluoride+ Gel Separator, glucose level for pregnant women	0,5ml, 13*75	JG1052
Lind-Vac	K2 EDTA/Na Fluoride+ Gel Separator, glucose level for pregnant women	1ml, 13*75	JG1102
Lind-Vac	K2 EDTA/Na Fluoride+ Gel Separator, glucose level for pregnant women	2ml, 13*75	JG1202
Lind-Vac	K2 EDTA/Na Fluoride+ Gel Separator, glucose level for pregnant women	3ml, 13*75	JG1302
Lind-Vac	K2 EDTA/Na Fluoride+ Gel Separator, glucose level for pregnant women	2ml, 13*100	JG2202
Lind-Vac	K2 EDTA/Na Fluoride+ Gel Separator, glucose level for pregnant women	3ml, 13*100	JG2302
Lind-Vac	K2 EDTA/Na Fluoride+ Gel Separator, glucose level for pregnant women	4ml, 13*100	JG2402
Lind-Vac	K2 EDTA/Na Fluoride+ Gel Separator, glucose level for pregnant women	5ml, 13*100	JG2502
Lind-Vac	K2 EDTA/Na Fluoride+ Gel Separator, glucose level for pregnant women	8ml, 16*100	JG3802
Lind-Vac	K2 EDTA/Na Fluoride+ Gel Separator, glucose level for pregnant women	9ml, 16*100	JG3902
Lind-Vac	Na2 EDTA/Na Fluoride+ Gel Separator, glucose level for pregnant women	0,5ml, 13*75	VG1052
Lind-Vac	Na2 EDTA/Na Fluoride+ Gel Separator, glucose level for pregnant women	1ml, 13*75	VG1102
Lind-Vac	Na2 EDTA/Na Fluoride+ Gel Separator, glucose level for pregnant women	2ml, 13*75	VG1202
Lind-Vac	Na2 EDTA/Na Fluoride+ Gel Separator, glucose level for pregnant women	3ml, 13*75	VG1302
Lind-Vac	Na2 EDTA/Na Fluoride+ Gel Separator, glucose level for pregnant women	2ml, 13*100	VG2202
Lind-Vac	Na2 EDTA/Na Fluoride+ Gel Separator, glucose level for pregnant women	3ml, 13*100	VG2302
Lind-Vac	Na2 EDTA/Na Fluoride+ Gel Separator, glucose level for pregnant women	4ml, 13*100	VG2402
Lind-Vac	Na2 EDTA/Na Fluoride+ Gel Separator, glucose level for pregnant women	5ml, 13*100	VG2502
Lind-Vac	Na2 EDTA/Na Fluoride+ Gel Separator, glucose level for pregnant women	8ml, 16*100	VG3802
Lind-Vac	Na2 EDTA/Na Fluoride+ Gel Separator, glucose level for pregnant women	9ml, 16*100	VG3902
Lind-Vac	K3 EDTA	0,5ml, 13*75	TE1052
Lind-Vac	K3 EDTA	1ml, 13*75	TE1102
Lind-Vac	K3 EDTA	2ml, 13*75	TE1202
Lind-Vac	K3 EDTA	3ml, 13*75	TE1302
Lind-Vac	K3 EDTA	4ml, 13*75	TE1402
Lind-Vac	K3 EDTA	5ml, 13*75	TE1502
Lind-Vac	K3 EDTA	4ml, 13*100	TE2402



List of products

Lind-Vac®


Lind-Vac	K3 EDTA	5ml, 13*100	TE2502
Lind-Vac	K3 EDTA	6ml, 13*100	TE2602
Lind-Vac	K3 EDTA	8ml, 16*100	TE3802
Lind-Vac	K3 EDTA	9ml, 16*100	TE3902
Lind-Vac	K3 EDTA	10ml, 16*100	TE3102
Lind-Vac	K3 EDTA + Gel Separator	0,5ml, 13*75	TG1052
Lind-Vac	K3 EDTA + Gel Separator	1ml, 13*75	TG1102
Lind-Vac	K3 EDTA + Gel Separator	2ml, 13*75	TG1202
Lind-Vac	K3 EDTA + Gel Separator	3ml, 13*75	TG1302
Lind-Vac	K3 EDTA + Gel Separator	4ml, 13*75	TG1402
Lind-Vac	K3 EDTA + Gel Separator	4ml, 13*100	TG2402
Lind-Vac	K3 EDTA + Gel Separator	5ml, 13*100	TG2502
Lind-Vac	K3 EDTA + Gel Separator	6ml, 13*100	TG2602
Lind-Vac	K3 EDTA + Gel Separator	8ml, 16*100	TG3802
Lind-Vac	K3 EDTA + Gel Separator	9ml, 16*100	TG3902
Lind-Vac	K3 EDTA/Na Fluoride	0,5ml, 13*75	IE1052
Lind-Vac	K3 EDTA/Na Fluoride	1ml, 13*75	IE1102
Lind-Vac	K3 EDTA/Na Fluoride	2ml, 13*75	IE1202
Lind-Vac	K3 EDTA/Na Fluoride	3ml, 13*75	IE1302
Lind-Vac	K3 EDTA/Na Fluoride	4ml, 13*75	IE1402
Lind-Vac	K3 EDTA/Na Fluoride	2ml, 13*100	IE2202
Lind-Vac	K3 EDTA/Na Fluoride	3ml, 13*100	IE2302
Lind-Vac	K3 EDTA/Na Fluoride	4ml, 13*100	IE2402
Lind-Vac	K3 EDTA/Na Fluoride	5ml, 13*100	IE2502
Lind-Vac	K3 EDTA/Na Fluoride	8ml, 16*100	IE3802
Lind-Vac	K3 EDTA/Na Fluoride	9ml, 16*100	IE3902
Lind-Vac	K3 EDTA/Na Fluoride+ Gel Separator, glucose level for pregnant women	0,5ml, 13*75	IG1052
Lind-Vac	K3 EDTA/Na Fluoride+ Gel Separator, glucose level for pregnant women	1ml, 13*75	IG1102
Lind-Vac	K3 EDTA/Na Fluoride+ Gel Separator, glucose level for pregnant women	2ml, 13*75	IG1202
Lind-Vac	K3 EDTA/Na Fluoride+ Gel Separator, glucose level for pregnant women	3ml, 13*75	IG1302
Lind-Vac	K3 EDTA/Na Fluoride+ Gel Separator, glucose level for pregnant women	2ml, 13*100	IG2202
Lind-Vac	K3 EDTA/Na Fluoride+ Gel Separator, glucose level for pregnant women	3ml, 13*100	IG2302
Lind-Vac	K3 EDTA/Na Fluoride+ Gel Separator, glucose level for pregnant women	4ml, 13*100	IG2402
Lind-Vac	K3 EDTA/Na Fluoride+ Gel Separator, glucose level for pregnant women	5ml, 13*100	IG2502
Lind-Vac	K3 EDTA/Na Fluoride+ Gel Separator, glucose level for pregnant women	8ml, 16*100	IG3802
Lind-Vac	K3 EDTA/Na Fluoride+ Gel Separator, glucose level for pregnant women	9ml, 16*100	IG3902
Lind-Vac	Na2 EDTA/Na Fluoride	0,5ml, 13*75	VE1052
Lind-Vac	Na2 EDTA/Na Fluoride	1ml, 13*75	VE1102
Lind-Vac	Na2 EDTA/Na Fluoride	2ml, 13*75	VE1202
Lind-Vac	Na2 EDTA/Na Fluoride	3ml, 13*75	VE1302
Lind-Vac	Na2 EDTA/Na Fluoride	4ml, 13*75	VE1402
Lind-Vac	Na2 EDTA/Na Fluoride	2ml, 13*100	VE2202
Lind-Vac	Na2 EDTA/Na Fluoride	3ml, 13*100	VE2302
Lind-Vac	Na2 EDTA/Na Fluoride	4ml, 13*100	VE2402
Lind-Vac	Na2 EDTA/Na Fluoride	5ml, 13*100	VE2502
Lind-Vac	Na2 EDTA/Na Fluoride	8ml, 16*100	VE3802
Lind-Vac	Na2 EDTA/Na Fluoride	9ml, 16*100	VE3902
Lind-Vac	Li Heparin/Na Fluoride	0,5ml, 13*75	QE1052
Lind-Vac	Li Heparin/Na Fluoride	1ml, 13*75	QE1102
Lind-Vac	Li Heparin/Na Fluoride	2ml, 13*75	QE1202
Lind-Vac	Li Heparin/Na Fluoride	3ml, 13*75	QE1302




List of products

Lind-Vac®

Lind-Vac	Li Heparin/Na Fluoride	4ml, 13*75	QE1402
Lind-Vac	Li Heparin/Na Fluoride	2ml, 13*100	QE2202
Lind-Vac	Li Heparin/Na Fluoride	3ml, 13*100	QE2302
Lind-Vac	Li Heparin/Na Fluoride	4ml, 13*100	QE2402
Lind-Vac	Li Heparin/Na Fluoride	5ml, 13*100	QE2502
Lind-Vac	Li Heparin/Na Fluoride	8ml, 16*100	QE3802
Lind-Vac	Li Heparin/Na Fluoride	9ml, 16*100	QE3902
Lind-Vac	Li Heparin/Na Fluoride+ Gel Separator, glucose level for pregnant women	0,5ml, 13*75	QG1052
Lind-Vac	Li Heparin/Na Fluoride+ Gel Separator, glucose level for pregnant women	1ml, 13*75	QG1102
Lind-Vac	Li Heparin/Na Fluoride+ Gel Separator, glucose level for pregnant women	2ml, 13*75	QG1202
Lind-Vac	Li Heparin/Na Fluoride+ Gel Separator, glucose level for pregnant women	3ml, 13*75	QG1302
Lind-Vac	Li Heparin/Na Fluoride+ Gel Separator, glucose level for pregnant women	4ml, 13*75	QG1402
Lind-Vac	Li Heparin/Na Fluoride+ Gel Separator, glucose level for pregnant women	2ml, 13*100	QG2202
Lind-Vac	Li Heparin/Na Fluoride+ Gel Separator, glucose level for pregnant women	3ml, 13*100	QG2302
Lind-Vac	Li Heparin/Na Fluoride+ Gel Separator, glucose level for pregnant women	4ml, 13*100	QG2402
Lind-Vac	Li Heparin/Na Fluoride+ Gel Separator, glucose level for pregnant women	5ml, 13*100	QG2502
Lind-Vac	Li Heparin/Na Fluoride+ Gel Separator, glucose level for pregnant women	8ml, 16*100	QG3802
Lind-Vac	Li Heparin/Na Fluoride+ Gel Separator, glucose level for pregnant women	9ml, 16*100	QG3902
Lind-Vac	Na Heparin/Na Fluoride	0,5ml, 13*75	PE1052
Lind-Vac	Na Heparin/Na Fluoride	1ml, 13*75	PE1102
Lind-Vac	Na Heparin/Na Fluoride	2ml, 13*75	PE1202
Lind-Vac	Na Heparin/Na Fluoride	3ml, 13*75	PE1302
Lind-Vac	Na Heparin/Na Fluoride	4ml, 13*75	PE1402
Lind-Vac	Na Heparin/Na Fluoride	2ml, 13*100	PE2202
Lind-Vac	Na Heparin/Na Fluoride	3ml, 13*100	PE2302
Lind-Vac	Na Heparin/Na Fluoride	4ml, 13*100	PE2402
Lind-Vac	Na Heparin/Na Fluoride	5ml, 13*100	PE2502
Lind-Vac	Na Heparin/Na Fluoride	8ml, 16*100	PE3802
Lind-Vac	Na Heparin/Na Fluoride	9ml, 16*100	PE3902
Lind-Vac	Na Heparin/Na Fluoride+ Gel Separator, glucose level for pregnant women	0,5ml, 13*75	PG1052
Lind-Vac	Na Heparin/Na Fluoride+ Gel Separator, glucose level for pregnant women	1ml, 13*75	PG1102
Lind-Vac	Na Heparin/Na Fluoride+ Gel Separator, glucose level for pregnant women	2ml, 13*75	PG1202
Lind-Vac	Na Heparin/Na Fluoride+ Gel Separator, glucose level for pregnant women	3ml, 13*75	PG1302
Lind-Vac	Na Heparin/Na Fluoride+ Gel Separator, glucose level for pregnant women	4ml, 13*75	PG1402
Lind-Vac	Na Heparin/Na Fluoride+ Gel Separator, glucose level for pregnant women	2ml, 13*100	PG2202
Lind-Vac	Na Heparin/Na Fluoride+ Gel Separator, glucose level for pregnant women	3ml, 13*100	PG2302
Lind-Vac	Na Heparin/Na Fluoride+ Gel Separator, glucose level for pregnant women	4ml, 13*100	PG2402
Lind-Vac	Na Heparin/Na Fluoride+ Gel Separator, glucose level for pregnant women	5ml, 13*100	PG2502
Lind-Vac	Na Heparin/Na Fluoride+ Gel Separator, glucose level for pregnant women	8ml, 16*100	PG3802
Lind-Vac	Na Heparin/Na Fluoride+ Gel Separator, glucose level for pregnant women	9ml, 16*100	PG3902



	for pregnant women		
Lind-Vac	EDTA 2Na/2K, 6-Aminohexanoic acid, Glycine G.R., DNA	0,5ml, 13*75	WE1052
Lind-Vac	EDTA 2Na/2K, 6-Aminohexanoic acid, Glycine G.R., DNA	1ml, 13*75	WE1102
Lind-Vac	EDTA 2Na/2K, 6-Aminohexanoic acid, Glycine G.R., DNA	2ml, 13*75	WE1202
Lind-Vac	EDTA 2Na/2K, 6-Aminohexanoic acid, Glycine G.R., DNA	3ml, 13*75	WE1302
Lind-Vac	EDTA 2Na/2K, 6-Aminohexanoic acid, Glycine G.R., DNA	4ml, 13*75	WE1402
Lind-Vac	EDTA 2Na/2K, 6-Aminohexanoic acid, Glycine G.R., DNA	3ml, 13*100	WE2302
Lind-Vac	EDTA 2Na/2K, 6-Aminohexanoic acid, Glycine G.R., DNA	4ml, 13*100	WE2402
Lind-Vac	EDTA 2Na/2K, 6-Aminohexanoic acid, Glycine G.R., DNA	5ml, 13*100	WE2502
Lind-Vac	EDTA 2Na/2K, 6-Aminohexanoic acid, Glycine G.R., DNA	6ml, 13*100	WE2602
Lind-Vac	EDTA 2Na/2K, 6-Aminohexanoic acid, Glycine G.R., DNA	7ml, 16*100	WE3702
Lind-Vac	EDTA 2Na/2K, 6-Aminohexanoic acid, Glycine G.R., DNA	8ml, 16*100	WE3802
Lind-Vac	EDTA 2Na/2K, 6-Aminohexanoic acid, Glycine G.R., DNA	9ml, 16*100	WE3902
Lind-Vac	EDTA 2Na/2K, 6-Aminohexanoic acid, Glycine G.R., DNA	10ml, 16*100	WE3102
Lind-Vac	ACD-A	0,5ml, 13*75	CE1052
Lind-Vac	ACD-A	1ml, 13*75	CE1102
Lind-Vac	ACD-A	2ml, 13*75	CE1202
Lind-Vac	ACD-A	3ml, 13*75	CE1302
Lind-Vac	ACD-A	4ml, 13*75	CE1402
Lind-Vac	ACD-A	5ml, 13*100	CE2502
Lind-Vac	ACD-A	6ml, 13*100	CE2602
Lind-Vac	ACD-A	8ml, 16*100	CE3802
Lind-Vac	ACD-A	9ml, 16*100	CE3902
Lind-Vac	ACD-A	10ml, 16*100	CE3102
Lind-Vac	ACD-A & Gel Separator	0,5ml, 13*75	CG1052
Lind-Vac	ACD-A & Gel Separator	1ml, 13*75	CG1102
Lind-Vac	ACD-A & Gel Separator	2ml, 13*75	CG1202
Lind-Vac	ACD-A & Gel Separator	3ml, 13*75	CG1302
Lind-Vac	ACD-A & Gel Separator	5ml, 13*100	CG2502
Lind-Vac	ACD-A & Gel Separator	6ml, 13*100	CG2602
Lind-Vac	ACD-A & Gel Separator	8ml, 16*100	CG3802
Lind-Vac	ACD-A & Gel Separator	9ml, 16*100	CG3902
Lind-Vac	ACD-B	0,5ml, 13*75	DE1052
Lind-Vac	ACD-B	1ml, 13*75	DE1102
Lind-Vac	ACD-B	2ml, 13*75	DE1202
Lind-Vac	ACD-B	3ml, 13*75	DE1302
Lind-Vac	ACD-B	4ml, 13*75	DE1402
Lind-Vac	ACD-B	5ml, 13*100	DE2502
Lind-Vac	ACD-B	6ml, 13*100	DE2602
Lind-Vac	ACD-B	8ml, 16*100	DE3802
Lind-Vac	ACD-B	9ml, 16*100	DE3902
Lind-Vac	ACD-B	10ml, 16*100	DE3102
Lind-Vac	ACD-B & Gel Separator	0,5ml, 13*75	DG1052
Lind-Vac	ACD-B & Gel Separator	1ml, 13*75	DG1102
Lind-Vac	ACD-B & Gel Separator	2ml, 13*75	DG1202
Lind-Vac	ACD-B & Gel Separator	3ml, 13*75	DG1302
Lind-Vac	ACD-B & Gel Separator	5ml, 13*100	DG2502
Lind-Vac	ACD-B & Gel Separator	6ml, 13*100	DG2602
Lind-Vac	ACD-B & Gel Separator	8ml, 16*100	DG3802
Lind-Vac	ACD-B & Gel Separator	9ml, 16*100	DG3902
Lind-Vac	Lithium Heparin	0,5ml, 13*75	LE1052
Lind-Vac	Lithium Heparin	1ml, 13*75	LE1102
Lind-Vac	Lithium Heparin	2ml, 13*75	LE1202
Lind-Vac	Lithium Heparin	3ml, 13*75	LE1302
Lind-Vac	Lithium Heparin	4ml, 13*75	LE1402
Lind-Vac	Lithium Heparin	5ml, 13*75	LE1502
Lind-Vac	Lithium Heparin	3ml, 13*100	LE2302
Lind-Vac	Lithium Heparin	4ml, 13*100	LE2402
Lind-Vac	Lithium Heparin	5ml, 13*100	LE2502
Lind-Vac	Lithium Heparin	6ml, 13*100	LE2602



List of products

Lind-Vac®

Lind-Vac	Lithium Heparin	7ml, 13*100	LE2702
Lind-Vac	Lithium Heparin	8ml, 16*100	LE3802
Lind-Vac	Lithium Heparin	9ml, 16*100	LE3902
Lind-Vac	Lithium Heparin	10ml, 16*100	LE3102
Lind-Vac	Lithium Heparin + Gel Separator	0,5ml, 13*75	LG1052
Lind-Vac	Lithium Heparin + Gel Separator	1ml, 13*75	LG1102
Lind-Vac	Lithium Heparin + Gel Separator	2ml, 13*75	LG1202
Lind-Vac	Lithium Heparin + Gel Separator	3ml, 13*75	LG1302
Lind-Vac	Lithium Heparin + Gel Separator	4ml, 13*75	LG1402
Lind-Vac	Lithium Heparin + Gel Separator	3ml, 13*100	LG2302
Lind-Vac	Lithium Heparin + Gel Separator	4ml, 13*100	LG2402
Lind-Vac	Lithium Heparin + Gel Separator	5ml, 13*100	LG2502
Lind-Vac	Lithium Heparin + Gel Separator	6ml, 13*100	LG2602
Lind-Vac	Lithium Heparin + Gel Separator	8ml, 16*100	LG3802
Lind-Vac	Lithium Heparin + Gel Separator	9ml, 16*100	LG3902
Lind-Vac	Sodium Heparin	0,5ml, 13*75	HE1052
Lind-Vac	Sodium Heparin	1ml, 13*75	HE1102
Lind-Vac	Sodium Heparin	2ml, 13*75	HE1202
Lind-Vac	Sodium Heparin	3ml, 13*75	HE1302
Lind-Vac	Sodium Heparin	4ml, 13*75	HE1402
Lind-Vac	Sodium Heparin	5ml, 13*75	HE1502
Lind-Vac	Sodium Heparin	3ml, 13*100	HE2302
Lind-Vac	Sodium Heparin	4ml, 13*100	HE2402
Lind-Vac	Sodium Heparin	5ml, 13*100	HE2502
Lind-Vac	Sodium Heparin	6ml, 13*100	HE2602
Lind-Vac	Sodium Heparin	7ml, 13*100	HE2702
Lind-Vac	Sodium Heparin	8ml, 16*100	HE3802
Lind-Vac	Sodium Heparin	9ml, 16*100	HE3902
Lind-Vac	Sodium Heparin	10ml, 16*100	HE3102
Lind-Vac	Sodium Heparin + Gel Separator	0,5ml, 13*75	HG1052
Lind-Vac	Sodium Heparin + Gel Separator	1ml, 13*75	HG1102
Lind-Vac	Sodium Heparin + Gel Separator	2ml, 13*75	HG1202
Lind-Vac	Sodium Heparin + Gel Separator	3ml, 13*75	HG1302
Lind-Vac	Sodium Heparin + Gel Separator	4ml, 13*75	HG1402
Lind-Vac	Sodium Heparin + Gel Separator	3ml, 13*100	HG2302
Lind-Vac	Sodium Heparin + Gel Separator	4ml, 13*100	HG2402
Lind-Vac	Sodium Heparin + Gel Separator	5ml, 13*100	HG2502
Lind-Vac	Sodium Heparin + Gel Separator	6ml, 13*100	HG2602
Lind-Vac	Sodium Heparin + Gel Separator	8ml, 16*100	HG3802
Lind-Vac	Sodium Heparin + Gel Separator	9ml, 16*100	HG3902



Needles			
Brand name		Size/Dimensions	Catalogue Number
Lind-Vac	Safety Needle Set with a holder	20G x 1-1½" (0,9 x 38mm)	HS2012
Lind-Vac	Safety Needle Set with a holder	21G x 1-1½" (0,8 x 38mm)	HS2112
Lind-Vac	Safety Needle Set with a holder	22G x 1-1½" (0,7 x 38mm)	HS2212
Lind-Vac	Safety Needle Set with a holder	24G x 1" (0,55 x 25mm)	HS2410
Lind-Vac	Safety Needle Set with a holder	25G x 1" (0,5 x 25mm)	HS2510
Lind-Vac	Safety Needle Set with a holder	26G x 1" (0,45 x 25mm)	HS2610
Lind-Vac	Safety Needle Set with a holder	27G x 1" (0,4 x 25mm)	HS2710
Lind-Vac	Multi sample needle, with visual control	21G x 1½" (0,8 x 38mm)	VN2112
Lind-Vac	Multi sample needle, with visual control	21G x 1" (0,8 x 25mm)	VN2110
Lind-Vac	Multi sample needle, with visual control	22G x 1½" (0,7 x 38mm)	VN2212
Lind-Vac	Multi sample needle, with visual control	22G x 1" (0,7 x 25mm)	VN2210
Lind-Vac	Multi sample needle, with visual control	23G x 1½" (0,6 x 38mm)	VN2312
Lind-Vac	Multi sample needle, with visual control	23G x 1" (0,6 x 25mm)	VN2310
Lind-Vac	Multi sample needle, without visual control	18G x 1½" (1,2 x 38mm)	MN1812
Lind-Vac	Multi sample needle, without visual control	18G x 1" (1,2 x 25mm)	MN1810
Lind-Vac	Multi sample needle, without visual control	20G x 1½" (0,9 x 38mm)	MN2012
Lind-Vac	Multi sample needle, without visual control	20G x 1" (0,9 x 25mm)	MN2010
Lind-Vac	Multi sample needle, without visual control	21G x 1½" (0,8 x 38mm)	MN2112
Lind-Vac	Multi sample needle, without visual control	21G x 1" (0,8 x 25mm)	MN2110
Lind-Vac	Multi sample needle, without visual control	22G x 1½" (0,7 x 38mm)	MN2212
Lind-Vac	Multi sample needle, without visual control	22G x 1" (0,7 x 25mm)	MN2210
Lind-Vac	Multi sample needle, without visual control	23G x 1½" (0,6 x 38mm)	MN2312
Lind-Vac	Multi sample needle, without visual control	23G x 1" (0,6 x 25mm)	MN2310
Lind-Vac	Safety Multi-sample needle	22G x 1½" (0,7 x 38mm)	MS2212
Lind-Vac	Safety Multi-sample needle	23G x 1" (0,6 x 25mm)	MS2310
Lind-Vac	Safety Multi-sample needle	20G x 1½" (0,9 x 38mm)	MS2012
Lind-Vac	Safety Multi-sample needle	19G x 1½" (1,1 x 38mm)	MS1912
Lind-Vac	Safety Multi-sample needle	23G x 1½" (0,6 x 38mm)	MS2312
Lind-Vac	Safety Multi-sample needle	18G x 1¼" (1,2 x 32mm)	MS1814
Lind-Vac	Safety Multi-sample needle	20G x 1¼" (0,9 x 32mm)	MS2014
Lind-Vac	Safety Multi-sample needle	18G x 1½" (1,2 x 38mm)	MS1812
Lind-Vac	Safety Multi-sample needle	19G x 1¼" (1,1 x 32mm)	MS1914
Lind-Vac	Safety Multi-sample needle	21G x 1¼" (0,8 x 32mm)	MS2114
Lind-Vac	Safety Multi-sample needle	22G x 1" (0,7 x 25mm)	MS2210
Lind-Vac	Safety Multi-sample needle	22G x 1¼" (0,7 x 32mm)	MS2214
Lind-Vac	Safety Multi-sample needle	21G x 1" (0,8 x 25mm)	MS2110
Lind-Vac	Safety Multi-sample needle	21G x 1½" (0,8 x 38mm)	MS2112
Lind-Vac	Safety Multi-sample needle	23G x 1¼" (0,6 x 32mm)	MS2314
Lancets			
Brand name		Size/Dimensions	Catalogue Number
Lind-Vac	Contact-activated lancet (Safety lancet), blade	1.8mm	XL I-0118
Lind-Vac	Contact-activated lancet (Safety lancet), blade	1.5mmx1.6mm	XL II-1516
Lind-Vac	Contact-activated lancet (Safety lancet), blade	2.3mm	XL I-0223
Lind-Vac	Contact-activated lancet (Safety lancet), blade	1.5mmx2.0mm	XL II-1520
Lind-Vac	Contact-activated lancet (Safety lancet), needle	23G (0.6mmx1.8mm)	XL II-2318
Lind-Vac	Contact-activated lancet (Safety lancet), needle	21G (0.8 mmx2.2mm)	XL II-2122
Lind-Vac	Contact-activated lancet (Safety lancet), needle	28G (0.36mmx1.8mm)	XL II-2818
Lind-Vac	Contact-activated lancet (Safety lancet), needle	21G (0.8 mmx2.8mm)	XL II-2128
Lind-Vac	Contact-activated lancet (Safety lancet), needle	26G (0.45mmx1.8mm)	XL II-2618
Lind-Vac	Contact-activated lancet (Safety lancet), needle	21G (0.8 mmx1.8mm)	XL II-2118
Luer Adapter			
Lind-Vac	Luer-adapter		LA2112
Lind-Vac	Luer-adapter with Holder		LH2112



Blood Collection Sets			
Brand name		Size/Dimensions	Catalogue Number
Lind-Vac	Safety Blood Collection set, with holder	19G x 3/4" x 7" (1,1 x 190mm)	BS1907
Lind-Vac	Safety Blood Collection set, with holder	19G x 3/4" x 12" (1,1 x 300mm)	BS1912
Lind-Vac	Safety Blood Collection set, with holder	21G x 3/4" x 7" (0,8 x 190mm)	BS2107
Lind-Vac	Safety Blood Collection set, with holder	21G x 3/4" x 12" (0,8 x 300mm)	BS2112
Lind-Vac	Safety Blood Collection set, with holder	22G x 3/4" x 7" (0,7 x 190mm)	BS2207
Lind-Vac	Safety Blood Collection set, with holder	22G x 3/4" x 12" (0,7 x 300mm)	BS2212
Lind-Vac	Safety Blood Collection set, with holder	23G x 3/4" x 7" (0,6 x 190mm)	BS2307
Lind-Vac	Safety Blood Collection set, with holder	23G x 3/4" x 12" (0,6 x 300mm)	BS2312
Lind-Vac	Safety Blood Collection set, with holder	25G x 3/4" x 7" (0,8 x 190mm)	BS2507
Lind-Vac	Safety Blood Collection set, with holder	25G x 3/4" x 12" (0,5 x 300mm)	BS2512
Lind-Vac	Safety Blood Collection set, without holder	19G x 3/4" x 7" (1,1 x 190mm)	SS1907
Lind-Vac	Safety Blood Collection set, without holder	19G x 3/4" x 12" (1,1 x 300mm)	SS1912
Lind-Vac	Safety Blood Collection set, without holder	21G x 3/4" x 7" (0,8 x 190mm)	SS2107
Lind-Vac	Safety Blood Collection set, without holder	21G x 3/4" x 12" (0,8 x 300mm)	SS2112
Lind-Vac	Safety Blood Collection set, without holder	22G x 3/4" x 7" (0,7 x 190mm)	SS2207
Lind-Vac	Safety Blood Collection set, without holder	22G x 3/4" x 12" (0,7 x 300mm)	SS2212
Lind-Vac	Safety Blood Collection set, without holder	23G x 3/4" x 7" (0,6 x 190mm)	SS2307
Lind-Vac	Safety Blood Collection set, without holder	23G x 3/4" x 12" (0,6 x 300mm)	SS2312
Lind-Vac	Safety Blood Collection set, without holder	25G x 3/4" x 7" (0,8 x 190mm)	SS2507
Lind-Vac	Safety Blood Collection set, without holder	25G x 3/4" x 12" (0,5 x 300mm)	SS2512
Lind-Vac	Blood Collection set, with holder	22G x 3/4" x 7" (0,7 x 190mm)	BH2207
Lind-Vac	Blood Collection set, with holder	23G x 3/4" x 7" (0,6 x 190mm)	BH2307
Lind-Vac	Blood Collection set, with holder	24G x 3/4" x 7" (0,55 x 190mm)	BH2412
Lind-Vac	Blood Collection set, with holder	22G x 3/4" x 12" (0,7 x 300mm)	BH2212
Lind-Vac	Blood Collection set, with holder	21G x 3/4" x 12" (0,8 x 300mm)	BH2112
Lind-Vac	Blood Collection set, with holder	20G x 3/4" x 12" (0,9 x 300mm)	BH2012
Lind-Vac	Blood Collection set, with holder	25G x 3/4" x 7" (0,8 x 190mm)	BH2507
Lind-Vac	Blood Collection set, with holder	23G x 3/4" x 12" (0,6 x 300mm)	BH2312
Lind-Vac	Blood Collection set, with holder	24G x 3/4" x 7" (0,55 x 190mm)	BH2407
Lind-Vac	Blood Collection set, with holder	21G x 3/4" x 7" (0,8 x 190mm)	BH2107
Lind-Vac	Blood Collection set, with holder	25G x 3/4" x 12" (0,5 x 300mm)	BH2512
Lind-Vac	Blood Collection set, with holder	20G x 3/4" x 7" (0,9 x 190mm)	BH2007
Lind-Vac	Blood Collection set, without holder	22G x 3/4" x 12" (0,7 x 300mm)	SN2212
Lind-Vac	Blood Collection set, without holder	24G x 3/4" x 12" (0,55 x 300mm)	SN2412
Lind-Vac	Blood Collection set, without holder	23G x 3/4" x 12" (0,6 x 300mm)	SN2312
Lind-Vac	Blood Collection set, without holder	22G x 3/4" x 7" (0,7 x 190mm)	SN2207
Lind-Vac	Blood Collection set, without holder	23G x 3/4" x 7" (0,6 x 190mm)	SN2307
Lind-Vac	Blood Collection set, without holder	24G x 3/4" x 7" (0,55 x 190mm)	SN2407
Lind-Vac	Blood Collection set, without holder	20Gx3/4"x12" (0,9x300mm)	SN2012
Lind-Vac	Blood Collection set, without holder	25G x 3/4" x 7" (0,8 x 190mm)	SN2507
Lind-Vac	Blood Collection set, without holder	20G x 3/4" x 7" (0,9 x 190mm)	SN2007
Lind-Vac	Blood Collection set, without holder	21G x 3/4" x 12" (0,8 x 300mm)	SN2112
Lind-Vac	Blood Collection set, without holder	21G x 3/4" x 7" (0,8 x 190mm)	SN2107
Lind-Vac	Blood Collection set, without holder	25G x 3/4" x 12" (0,5 x 300mm)	SN2512
Holders			
Lind-Vac	Holder		HC01
Lind-Vac	Safety Needle Holder		SH01

