

Quality Control Report


AHD ELISA kit

(Cat No: KA00407H)

Lot No.: H250603D10

Date of Production: 2025-06-05

Expired: 2026-06-04

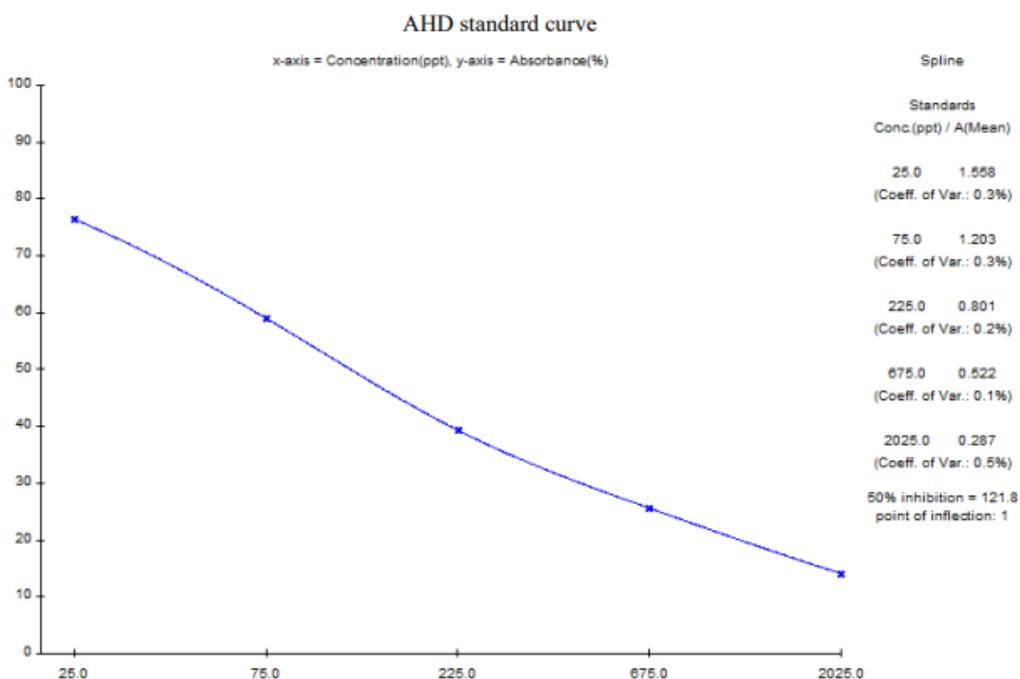

Standards						
Ser. No.	Concentration ppt	Absorbance (Mean)	(CV)	B/B0 (%)	calculated ppt	Deviation (%)
1	0.0	2.038	1.6	100.0		
2	25.0	1.558	0.3	76.4	25.0	0.0
3	75.0	1.203	0.3	59.0	75.0	0.0
4	225.0	0.801	0.2	39.3	225.3	0.1
5	675.0	0.522	0.1	25.6	674.3	0.1
6	2025.0	0.287	0.5	14.1	2025.7	0.0

Please notice: This QC report is only for reference, for the absorbance of the standard solutions may fluctuate in a certain range.

