


Adult Anesthesia Circuit Extendible PP Tube 200cm, 150cm limb, 2lt neoprene brathing bag

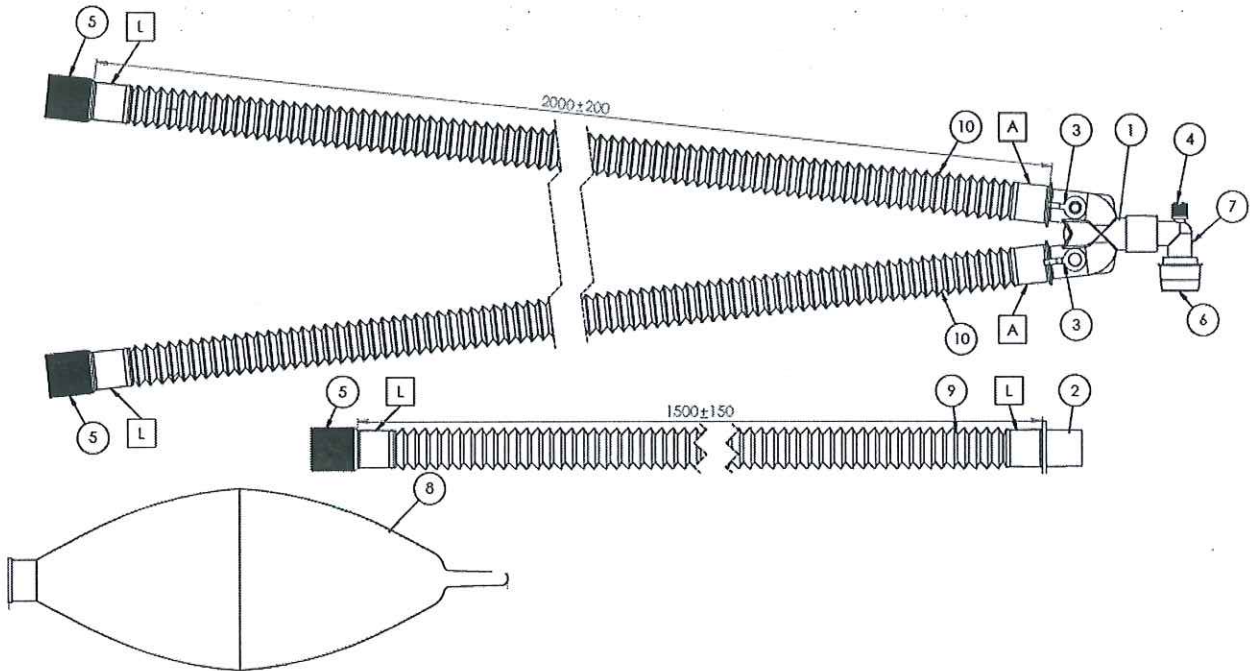

Meditera Tibbi Malzeme Sanayi ve Ticaret A.Ş.

Ethylene oxide sterilization. This product line is provided both as sterile and nonsterile.

Nylon packaging.

Disposable circuits used to conduct medical gases from the anaesthesia system to the patient. Anaesthetic gas exits the anaesthesia machine (via the common gas outlet) and then enters a breathing circuit. The function of the circuit is to deliver oxygen and anaesthetic gases to the patient and to eliminate CO₂. The CO₂ may be eliminated by gas inflow or by soda lime absorption.

5. Shelf life :

5 years from the date of production .

6. Product Description:

6.1. Classification: Class IIa Rule 2

6.2. This product does not contain any metallic parts

6.3. Spesification of the product :

UNIT NO.	PART NUMBER	DESCRIPTION	QUANTITY
1	151.03.225.01	ANGLED Y CONNECTOR FOR TIGHT FIT WIHT PORT PP	1
2	151.03.255	22-22 MM STRAIGHT CONNECTOR (NEW)	1
3	151.03.264	Y CONNECTOR CAP (NEW)	2
4	150.11.036	ELBOW CONNECTOR LUER CAP	1
5	151.03.261	22 MM STRAIGHT CONNECTOR EVA (NEW)	3
6	151.03.021.01	LONG CONNECTOR CAP RED	1
7	151.03.224.01	ELBOW CONNECTOR WITH PORT PP	1
8	150.07.040	2 LT NEOPRENE SINGLE FOLDED BREATHING BAG WITH STICKER(RIGID PP CONNECTOR)	1
9	151.05.02.203	22 MM EXTENDIBLE TUBING 150 CM CUT	1
10	151.05.02.218	22 MM EXTENDIBLE TUBING PP 200 CM CUT	2

7. Standarts:

EN ISO 13485:2016, 93/42/EEC Medical Device Directive, EN 556-1:2001, EN ISO 11607-1:2020, EN ISO 11607-2:2020, EN ISO 23328-1, EN ISO 23328-2

8. Waste Method:

After use product will be "contaminated medical waste" and package will be "packaging waste" so they should be handled according to relevant national and international standards and regulations.

MEDİTERA TİBBİ MALZEME
SAN. VE TİC. A.Ş.
 İbni Melek OSB Mh. TOSK. YOLU 455. No:29 35900 Tire-İZMİR
 Türe V.D: 060 020 8703 Tic. Sicil No: 2346
 Mersis No: 0804000029870300016
 Tel: 0 232 513 51 10 Faks: 0 232 513 51 14