



## STATEMENT

We, ACON Laboratories, Inc., having a registered office at *5850 Oberlin Drive #340, San Diego, CA 92121* authorize SRL Sanmedico having a registered office at *A. Corobceanu street 7A, apt. 9, Chisinău, MD-2012, Moldova*

to register, notify, renew or modify the registration of medical devices on the territory of the Republic of Moldova.

Date: March 18, 2024

Signature:

A handwritten signature in black ink, appearing to read "Xie", is written over a horizontal line.

Qiyi Xie, Md, MPH  
V.P. of Regulatory & Clinical Affairs  
ACON Laboratories, Inc.



Product Service

# Certificate

No. Q5 104507 0001 Rev. 03

**Holder of Certificate:** **ACON Laboratories, Inc.**  
 5850 Oberlin Drive, #340  
 San Diego CA 92121  
 USA

**Certification Mark:**



**Scope of Certificate:** **Design and Development, Manufacture and distribution of In Vitro Diagnostic Test Kits and Reagents for the Determination of Infectious Diseases, Clinical Chemistry, Drugs of Abuse, Tumor/Cardiac Marker, Fertility/Pregnancy and Blood Glucose Monitoring System, Lancing Devices and Lancets**

The Certification Body of TÜV SÜD Product Service GmbH certifies that the company mentioned above has established and is maintaining a quality management system, which meets the requirements of the listed standard(s). All applicable requirements of the testing and certification regulation of TÜV SÜD Group have to be complied with. For details and certificate validity see: [www.tuvsud.com/ps-cert?q=cert:Q5 104507 0001 Rev. 03](http://www.tuvsud.com/ps-cert?q=cert:Q5 104507 0001 Rev. 03)

**Report No.:** SH22743A01

**Valid from:** 2022-09-15  
**Valid until:** 2025-09-06

**Date,** 2022-09-15

Christoph Dicks  
 Head of Certification/Notified Body

# Certificate

No. Q5 104507 0001 Rev. 03

## Applied Standard(s):

EN ISO 13485:2016  
Medical devices - Quality management systems -  
Requirements for regulatory purposes  
(ISO 13485:2016)  
DIN EN ISO 13485:2016

## Facility(ies):

**ACON Laboratories, Inc.**  
**5850 Oberlin Drive, #340, San Diego CA 92121, USA**

Address holder for registration only

**ACON Laboratories, Inc.**  
**10125 Mesa Rim Road, San Diego CA 92121, USA**

Manufacture and distribution of  
In Vitro Diagnostic Test Kits and Reagents for the Determination of  
Infectious Diseases, Clinical Chemistry, Drugs of Abuse,  
Tumor/Cardiac Marker, Fertility/Pregnancy and Blood Glucose  
Monitoring System, Lancing Devices and Lancets

**ACON Laboratories, Inc.**  
**6865 Flanders Dr., Suite B, San Diego CA 92121, USA**

Storage of  
In Vitro Diagnostic Test Kits and Reagents for the Determination of  
Infectious Diseases, Clinical Chemistry, Drugs of Abuse,  
Tumor/Cardiac Marker, Fertility/Pregnancy and Blood Glucose  
Monitoring System, Lancing Devices and Lancets

**AZURE Institute, Inc.**  
**10125 Mesa Rim Road, San Diego CA 92121, USA**

Design and Development of  
In Vitro Diagnostic Test Kits and Reagents for the Determination of  
Infectious Diseases, Clinical Chemistry, Drugs of Abuse,  
Tumor/Cardiac Marker, Fertility/Pregnancy and Blood Glucose  
Monitoring System, Lancing Devices and Lancets

**Acon Laboratories Inc.**  
**Guerrero Negro 9942 Parque Industrial Pacifico IV, 22644**  
**Tijuana B.C. CP, MEXICO**

Manufacture of  
blood glucose test strips, antigen rapid test and IgG/IgM antibody  
rapid test for infectious disease.



# EC Certificate

Full Quality Assurance System

Directive 98/79/EC on In Vitro Diagnostic Medical Devices (IVDD), Annex IV excluding (4, 6)  
(List A and B and devices for self-testing)

**No. V1 104507 0003 Rev. 06**

**Manufacturer:** **ACON Laboratories, Inc.**  
5850 Oberlin Drive, #340  
San Diego CA 92121  
USA

**Product Category(ies):** **Blood glucose measuring systems for self testing  
and self-testing devices for clinical chemistry,  
hematology and pregnancy and ovulation**

The Certification Body of TÜV SÜD Product Service GmbH declares that the aforementioned manufacturer has implemented a quality assurance system for design, manufacture and final inspection of the respective devices / device families in accordance with IVDD Annex IV. This quality assurance system conforms to the requirements of this Directive and is subject to periodical surveillance. For marketing of List A devices an additional Annex IV (4) certificate is mandatory. All applicable requirements of the testing and certification regulation of TÜV SÜD Group have to be complied with. For details and certificate validity see: [www.tuvsud.com/ps-cert?q=cert:V1\\_104507\\_0003\\_Rev.06](http://www.tuvsud.com/ps-cert?q=cert:V1_104507_0003_Rev.06)

**Report no.:** SH22743EXT01

**Valid from:** 2022-05-04

**Valid until:** 2025-05-26

**Date,** 2022-05-04

Christoph Dicks  
Head of Certification/Notified Body



# EC Certificate

Full Quality Assurance System

Directive 98/79/EC on In Vitro Diagnostic Medical Devices (IVDD), Annex IV excluding (4, 6)  
(List A and B and devices for self-testing)

**No. V1 104507 0003 Rev. 06**

## Model(s):

On Call Plus Blood Glucose Monitoring System,  
On Call Plus Blood Glucose Test Strips,  
On Call EZ II Blood Glucose Monitoring System,  
On Call Advanced Blood Glucose Monitoring System,  
On Call Advanced Blood Glucose Test Strips,  
On Call Chosen Blood Glucose Test Strips,  
On Call Vivid Blood Glucose Monitoring System (OGM-101),  
On Call Vivid Blood Glucose Test Strips (OGS-101),  
On Call Sharp Blood Glucose Monitoring System (OGM-121),  
On Call Sharp Blood Glucose Test Strips (OGS-121)  
On Call Plus II Blood Glucose Monitoring System (OGM-171),  
On Call Plus II Blood Glucose Test Strips (OGS-171),  
On Call Extra Blood Glucose Monitoring System (OGM-191),  
On Call Extra Blood Glucose Test Strips (OGS-191),  
On Call GK Dual Blood Glucose & Ketone Monitoring System (OGM-161),  
On Call Blood Ketone Test Strips (OGS-161),  
Urinalysis Reagent Strips (Urine),  
UTI Urinary Tract Infection Test Strips,  
Cholesterol Monitoring System (CCM-111),  
CHOL Total Cholesterol Test Devices (CCS-111),  
TRIG Triglycerides Test Devices (CCS-112),  
HDL High Density Lipoprotein Test Devices (CCS-113),  
3-1 Lipid Panel Test Devices (CCS-114),  
Cholesterol CTRL Control Devices,  
Cholesterol Monitoring System (CCM-101),  
CHOL Total Cholesterol Test Strips (CCS-101),  
PT/INR Monitoring System (CCM-151),  
PT/INR Test Strips (CCS-151),  
Hemoglobin Testing System (CCM-141),  
Hemoglobin Test Strips (CCS-141),  
hCG Pregnancy Rapid Test Cassette (Urine),  
Pregnancy Rapid Test Midstream,  
On Call Extra Mobile Blood Glucose Monitoring System (OGM-281),  
On Call Sure Blood Glucose Monitoring System (OGM-211),  
On Call Sure Sync Blood Glucose Monitoring System (OGM-212),  
On Call Sure Blood Glucose Test Strips (OGS-211),  
GIMA Blood Glucose Monitoring System,  
GIMA Bluetooth Blood Glucose Monitoring System,  
GIMA Blood Glucose Test Strips,  
On Call GU Dual Blood Glucose & Uric Acid Monitoring



# EC Certificate

Full Quality Assurance System

Directive 98/79/EC on In Vitro Diagnostic Medical Devices (IVDD), Annex IV excluding (4, 6)  
(List A and B and devices for self-testing)

**No. V1 104507 0003 Rev. 06**

System (OGM-201),  
On Call Blood Uric Acid Test Strips (OGS-201),  
LH Ovulation Rapid Test Cassette (Urine),  
Ovulation Rapid Test Midstream,  
Ovulation & Pregnancy Test Combo Pack,  
On Call Extra Voice Blood Glucose Monitoring System  
(OGM-291),  
Early Detection Pregnancy Test,  
Digital Pregnancy Test,  
Go-Keto Blood Glucose & Ketone Monitoring System (OGM-  
161),  
Go-Keto Blood Ketone Test Strips (OGS-161),  
Go-Keto Blood Glucose Test Strips,  
On Call Extra GM Blood Glucose Monitoring System(OGM-  
191),  
On Call Extra GM Blood Glucose Test Strips (OGS-191),  
On Call Plus GM Blood Glucose Monitoring System,  
On Call Plus GM Blood Glucose Test Strips,  
Go-Keto Urinalysis Reagent Strips

## Facility(ies):

ACON Laboratories, Inc.  
5850 Oberlin Drive, #340, San Diego CA 92121, USA

ACON Laboratories, Inc.  
10125 Mesa Rim Road, San Diego CA 92121, USA

AZURE Institute, Inc.  
10125 Mesa Rim Road, San Diego CA 92121, USA

Acon Laboratories Inc.  
Guerrero Negro 9942 Parque Industrial Pacifico IV, 22644 Tijuana  
B.C. CP, MEXICO

# Declaration of Conformity

ACON Laboratories, Incorporated  
5850 Oberlin Drive #340  
San Diego, CA 92121 USA

**We, the manufacturer, declare under our sole responsibility that the  
in vitro diagnostic device:**

Device Name	REF Number
On Call® Plus Blood Glucose Monitoring System	G113-111
On Call® Plus Blood Glucose Meter	G113-211, G113-214
On Call® Plus Blood Glucose Test Strips	G133-111, G133-112, G133-114, G133-115, G133-117, G133-118, G133-119, G133-211
On Call® Plus Glucose Control Solution	G123-311

**classified for Annex II List B of the directive 98/79/EC,  
meets all the provisions of the directive 98/79/EC on *in vitro*  
diagnostic medical devices which apply to it**


**The declaration according to Annex IV of the Directive  
is based on approval by the notified body  
TÜV SÜD Product Service GmbH,  
Ridlerstraße 65,  
80339 MÜNCHEN, Germany,  
notified under No. 0123 to the EC Commission**

This declaration is valid until expiration of EC Certificate  
No. V1 104507 0003 Rev. 06  
Expiration Date: 2025-05-26

Authorized Representative:  
Medical Device Safety Service GmbH  
Schiffgraben 41  
30175 Hannover, Germany



Signed this 25 day of May, 2022  
in San Diego, CA USA



---

Qiyi Xie, MD, MPH  
Senior Staff, Regulatory Affairs & Clinical Affairs  
ACON Laboratories, Inc.





**Specification**



Feature	Specification
Technology	Biosensor/Electrochemical, Glucose oxidase (GOD)
Result Calibration	Plasma-equivalent
Test Time	10 seconds
Sample Size	0.5 µL
Sample Type	Fresh capillary whole blood
Hematocrit Range	25 - 60%
Glucose Test Range	20 - 600 mg/dL (1.1 - 33.3 mmol/L)
Memory Storage	300 results with date and time
Test Averaging	7, 14, 30-day averages
Data Transfer	USB
Control Solution	3 levels
Audio Feature	Optional beep for sample detection, error messages
Automatic Shutoff	2 minutes after last action
Battery	One (1) CR 2032 3.0V coin cell battery
Battery Life	1,000 measurements
Operating Conditions	41 - 113 °F (5 - 45°C) and 10 - 90% relative humidity
Strip Storage Temperature	2-35°C
Expiration Date	24 months (6 months after first opening)


**Catalog**

Product Name	Catalog No.	Contents			
On-Call <sup>®</sup> Plus Blood Glucose Monitoring System	G113-111 v †	1 Meter 1 Manual 10 Lancets	10 Test Strips 1 Carrying Case 1 Code Chip	1 Control Solution 1 1 Quick Reference Guide 1 Clear Cap (for testing on forearm and palm)	1 Lancing Device 1 Warranty Card
On-Call <sup>®</sup> Plus Blood Glucose Meter	G113-211 v †	1 Meter 1 Manual	1 Control Solution 1 1 Warranty Card	1 Carrying Case 1 Quick Reference Guide	
	G113-214 v	1 Meter 1 Manual 10 Lancets	1 Lancing Device 1 Carrying Case 1 Warranty Card	1 Control Solution 1 1 Quick Reference Guide 1 Clear Cap (for testing on forearm and palm)	
On-Call <sup>®</sup> Plus Blood Glucose Test Strips	G133-111 v †	50 Test Strips (25/vial)		1 Code Chip	1 Package Insert
		50 Test Strips (50/vial)		1 Code Chip	1 Package Insert
	G133-112 v	100 Test Strips (25/vial)		1 Code Chip	1 Package Insert
	G133-114 v	10 Test Strips (10/vial)		1 Code Chip	1 Package Insert
	G133-115 v	25 Test Strips (Individually Foil Wrapped)		1 Code Chip	1 Package Insert
	G133-117 v	50 Test Strips (Individually Foil Wrapped)		1 Code Chip	1 Package Insert
G133-118 v	25 Test Strips (25/vial)		1 Code Chip	1 Package Insert	
On-Call <sup>®</sup> Plus Blood Glucose Test Strips and Lancets	G133-211 v	50 Test Strips (25/vial)	50 Lancets (25/bag)	1 Code Chip	1 Package Insert
On-Call <sup>®</sup> Plus Blood Glucose Control Solution	G123-311 v †	1 Control Solution 0	1 Control Solution 1	1 Control Solution 2	1 Package Insert
On-Call <sup>®</sup> Lancets	G124-10A v †	100 Lancets (25/bag)			
On-Call <sup>®</sup> Lancing Device	G124-11AV	1 Lancing Device		1 Package Insert	
On-Call <sup>®</sup> Diabetes Management Software Kit	G124-13A †	1 USB Data Transfer Cable		1 Installation Disk	

v CE Marked for sale in the European Community 0123 † US 510(k) Cleared and CLIA Waived



**On-Call<sup>®</sup> Plus**  
Blood Glucose Monitoring System

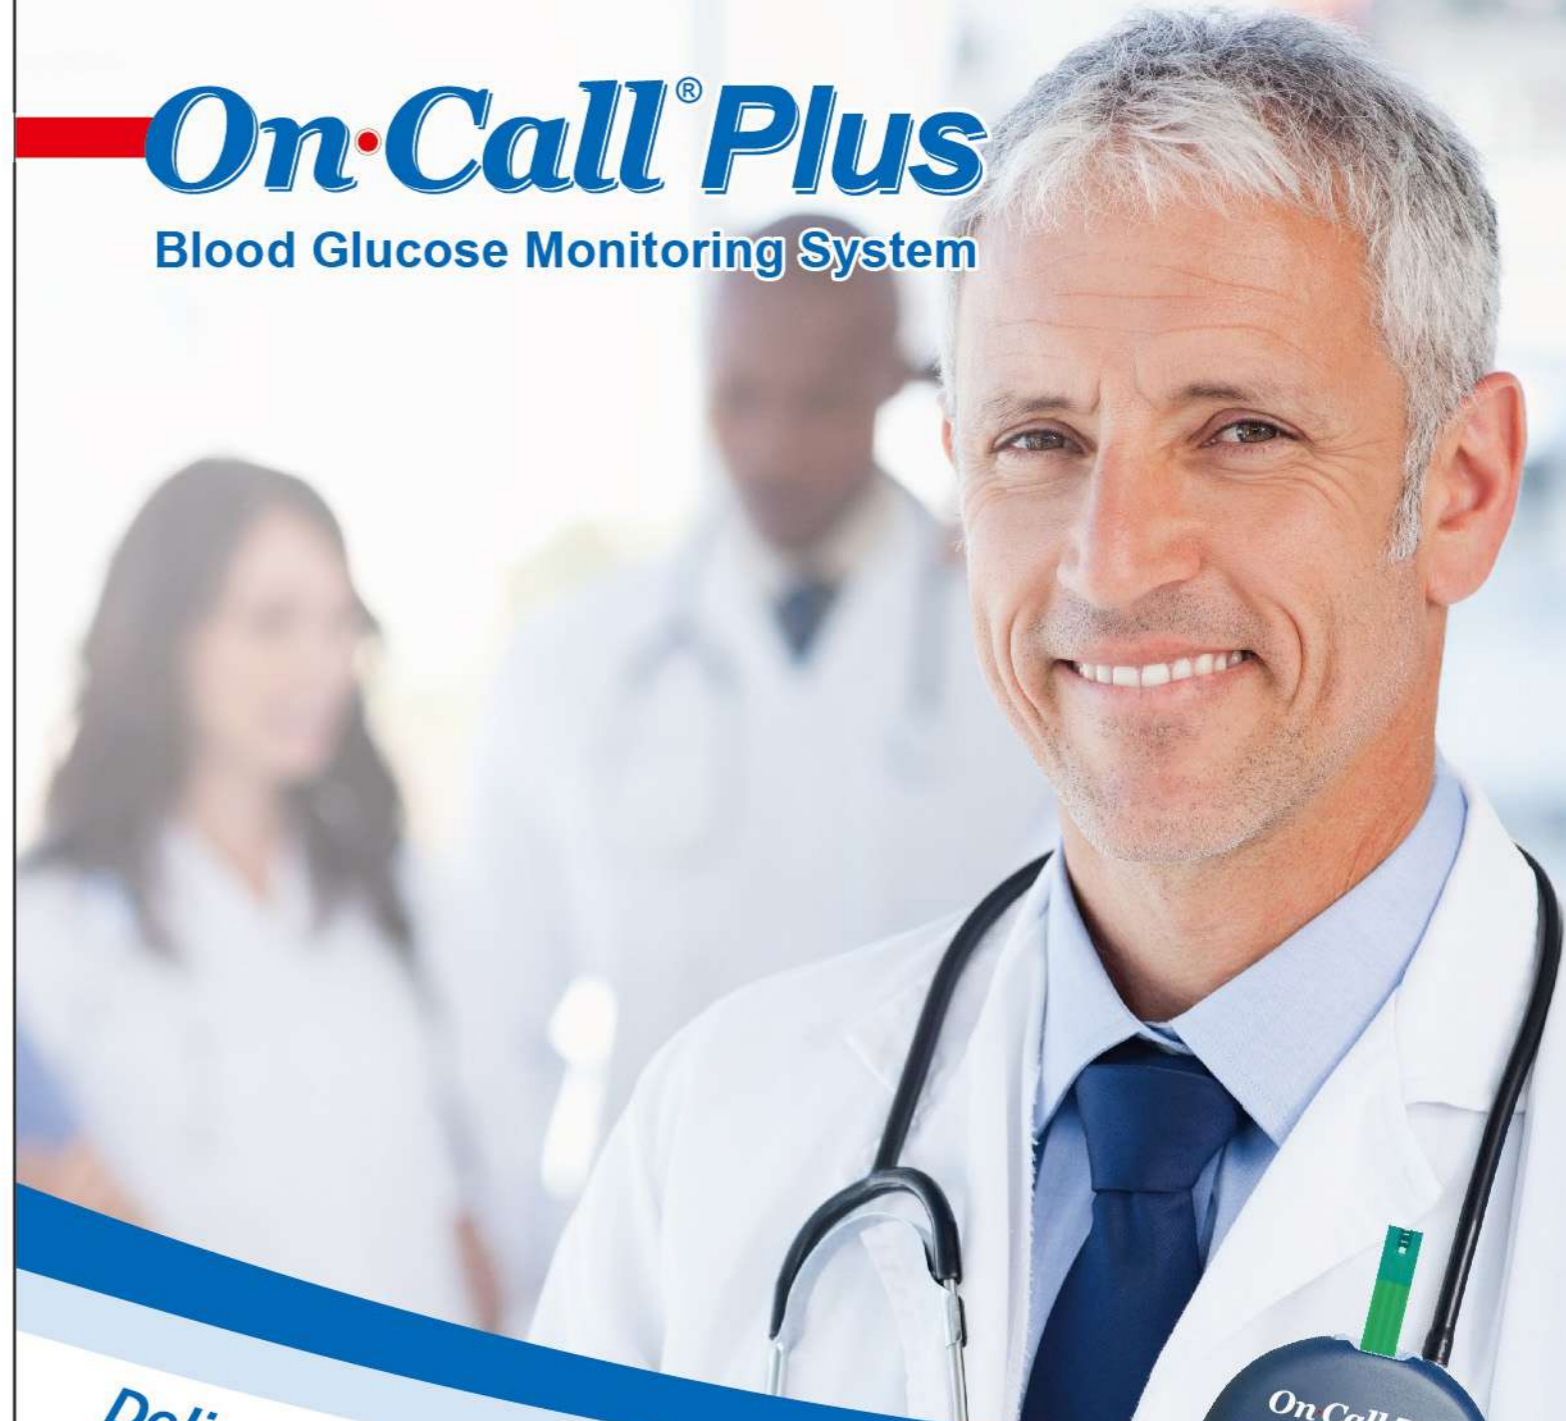


*Delivers Value and Quality*

- 0.5 µL Blood Sample
- Accurate & Reliable Results
- 25 - 60% HCT Range
- US 510(k) & CE




## Accurate and Reliable


Extensive clinical studies proved the accuracy of *On Call Plus* Blood Glucose Monitoring System with fresh capillary blood samples, which can comply with EN ISO 15197: 2015.

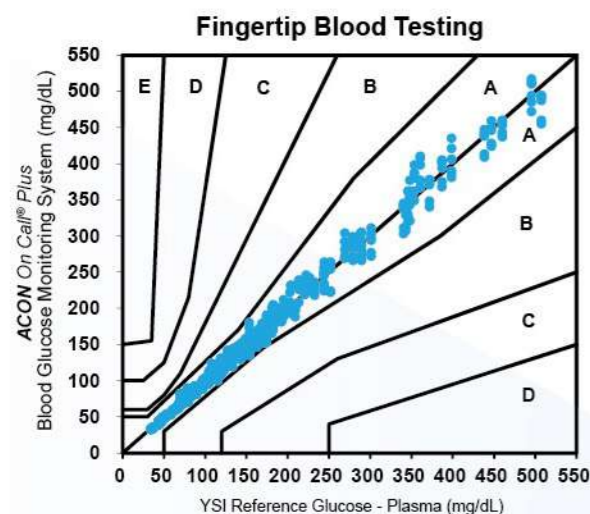

Consensus Error Grid Analysis Clinical Trial - Fingertip Capillary Blood, by Technican ACON On Call Plus Blood Glucose Monitoring System vs. YSI		
<b>System Accuracy Results for Glucose Concentration <math>\geq 100</math> mg/dL</b>		
Within $\pm 5\%$	Within $\pm 10\%$	Within $\pm 15\%$
290 / 462 (62.8%)	432 / 462 (93.5%)	462 / 462 (100.0%)
<b>System Accuracy Results for Glucose Concentration <math>&lt; 100</math> mg/dL</b>		
Within $\pm 5$ mg/dL	Within $\pm 10$ mg/dL	Within $\pm 15$ mg/dL
145 / 198 (73.2%)	193 / 198 (97.5%)	198 / 198 (100.0%)
<b>System Accuracy Results for both Glucose Concentration <math>\geq 100</math> mg/dL and <math>&lt; 100</math> mg/dL</b>		
Within $\pm 15\%$ or $\pm 15$ mg/dL		
658 / 660 (99.7%)		

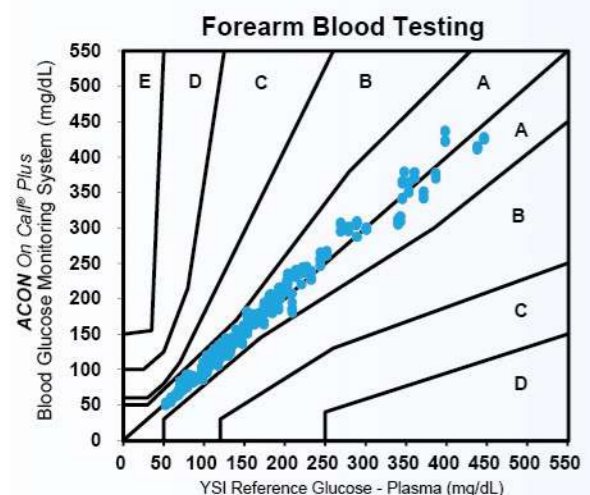

Consensus Error Grid Analysis Clinical Trial - Forearm Capillary Blood, by Technican ACON On Call Plus Blood Glucose Monitoring System vs. YSI		
<b>System Accuracy Results for Glucose Concentration <math>\geq 100</math> mg/dL</b>		
Within $\pm 5\%$	Within $\pm 10\%$	Within $\pm 15\%$
202 / 444 (45.5%)	375 / 444 (84.5%)	440 / 444 (99.1%)
<b>System Accuracy Results for Glucose Concentration <math>&lt; 100</math> mg/dL</b>		
Within $\pm 5$ mg/dL	Within $\pm 10$ mg/dL	Within $\pm 15$ mg/dL
110 / 168 (65.5%)	154 / 168 (91.7%)	168 / 168 (100.0%)
<b>System Accuracy Results for both Glucose Concentration <math>\geq 100</math> mg/dL and <math>&lt; 100</math> mg/dL</b>		
Within $\pm 15\%$ or $\pm 15$ mg/dL		
608 / 612 (99.3%)		

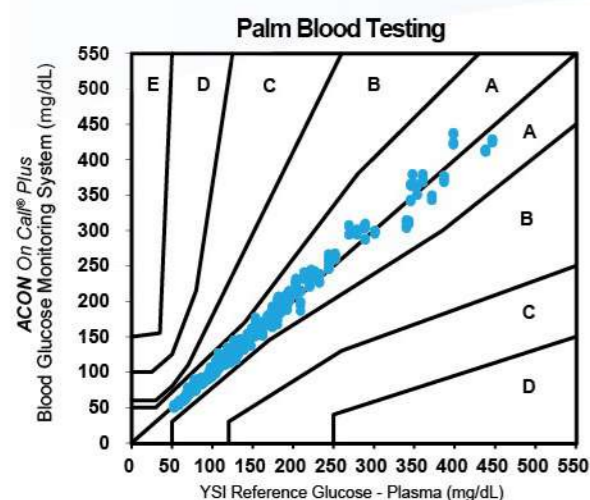

Consensus Error Grid Analysis Clinical Trial - Palm Capillary Blood, by Technican ACON On Call Plus Blood Glucose Monitoring System vs. YSI		
<b>System Accuracy Results for Glucose Concentration <math>\geq 100</math> mg/dL</b>		
Within $\pm 5\%$	Within $\pm 10\%$	Within $\pm 15\%$
219 / 444 (49.3%)	395 / 444 (89.0%)	441 / 444 (99.3%)
<b>System Accuracy Results for Glucose Concentration <math>&lt; 100</math> mg/dL</b>		
Within $\pm 5$ mg/dL	Within $\pm 10$ mg/dL	Within $\pm 15$ mg/dL
130 / 168 (77.4%)	166 / 168 (98.8%)	168 / 168 (100.0%)
<b>System Accuracy Results for both Glucose Concentration <math>\geq 100</math> mg/dL and <math>&lt; 100</math> mg/dL</b>		
Within $\pm 15\%$ or $\pm 15$ mg/dL		
609 / 612 (99.5%)		

## Key Features

The image shows the On-Call Plus glucose meter with a digital display showing a reading of 135 mg/dL. The meter is dark blue with a green test strip inserted into the top. The display also shows the time 2:07 PM and the date 6-20.

- 0.5  $\mu$ L blood sample
- HCT 25 - 60% HCT range
- 2 - 35°C strip storage temperature
- Optional individually packaged test strips available
- Alternative testing sites including fingertip, forearm and palm
- Automatic detection of insufficient sample
- 300 test memory with date and time
- 7, 14, 30 - day averages calculation
- Easy PC data transfer and smart App data analysis

## Authority Certificate



CE certificate

USFDA CFG certificate

Health Canada certificate

## Declaration of Conformity

ACON Laboratories, Incorporated  
5850 Oberlin Drive #340  
San Diego, CA 92121, USA

**We, the manufacturer, declare under our sole responsibility that the  
*in vitro* diagnostic device:**

*Mission*<sup>®</sup> Urinalysis Reagent Strips (U031-XX1)

**classified as Others in the directive 98/79/EC,**

**meets all the provisions of the directive 98/79/EC on *in vitro* diagnostic  
medical devices which apply to it**

**The self-declaration is according to Annex III  
(excluding Section 6) of the Directive.**

Authorized Representative:  
Medical Device Safety Service GmbH  
Schiffgraben 41  
30175 Hannover, Germany

Signed this 11 day of February, 2020  
in San Diego, CA USA



---

Qiyi Xie, MD, MPH  
Senior Staff, Regulatory Affairs & Clinical Affairs  
Acon Laboratories, Inc.



# Letter of Declaration

To whom it may concern:

We **Acon Laboratories, Inc.**, who is the legal manufacturer of Blood Glucose Monitoring System (Including Glucose Meter, Glucose test strip, Control Solution, Lancet and lancing device etc, to test the glucose level of human blood), have registered office at 10125 Mesa Rim Road, San Diego, CA 92121 USA, here to declare that:

- **On Call® Plus Strips** correspond with **On Call® Plus** Blood Glucose Monitoring System.
- We currently have in stock the tender required quantity of Meters, Strips and Lancets (1000/50000/50000).

This clarification letter will only be used for product registration, tender submission, sales and marketing of **On Call® Plus** Blood Glucose Monitoring System in **Moldova** it should not be used for any other business or non-business purposes.

Sincerely yours,

  
Eddie. Shi  
International Sales & Marketing Sales Manager  
Diabetes Care

**Acon Laboratories, Inc.**





**ACON Laboratories, Inc.**

10125 Mesa Rim Road. • San Diego, CA 92121 • USA  
Tel: (858) 875-8000 • Fax: (858) 875-8099 • E-mail: [info@aconlabs.com](mailto:info@aconlabs.com)

November 11<sup>th</sup> 2016

**CERTIFICATION LETTER**

This letter is to certify that, Vitalie Goreacii, employed by Sanmedico SRL located at: Republic of Moldova, city Chisinau, str. Petricani 88/1 of. 10, MD-2059, have received all required training and is enabled and authorized to provide services with installation, commissioning, and maintenance to the products listed below:

Mission® U120 Urine Analyzer  
Mission® U120 Ultra Urine Analyzer  
Mission® U500 Urine Analyzer  
Mission® PT/INR Coagulation Monitoring System  
Mission® Cholesterol Monitoring System  
Mission® Ultra Cholesterol Monitoring System  
Mission® HB Hemoglobin Testing System  
Mission® Plus HB Hemoglobin Testing System  
OnCall® Glucose Meter

For further questions or inquiries regarding this matter, please refer to the contact information below.

Sincerely

A handwritten signature in black ink, appearing to read "Jassy Alvarenga", is written over a red circular stamp.



Jassy Alvarenga  
International Account Manager  
ACON Laboratories, Inc. S.A.  
[jalvarenga@aconlabs.com](mailto:jalvarenga@aconlabs.com)  
+1 858 875 8085

# Mission® Urinalysis Reagent Strips and Urine Analyzers



Obtain reliable and cost-effective results with *Mission®* Urinalysis Reagent Strips and Urine Analyzers!

- *Accurate*
- *Reliable*
- *Convenient*



Global Diagnostics for Local Markets™

# Urinalysis Reagent Strips

## Simple and Accurate


- Analytical sensitivity better than or comparable to market leaders
- High quality color chart ensures accurate visual reading

## Flexible


- Compatible for visual and analyzer reading
- More than 30 different combinations available

## Multiple Packaging Options and Long Shelf Life


- Canister Packaging
  - Available in 25, 50, 100 and 150 strips per kit
  - 2 year shelf life for unopened canisters which offers cost savings and convenience for high volume testing
  - 3 month shelf life for strips in opened canisters
- Pouch Packaging *New!*
  - Single-strip Pouch
    - Individually packaged strips with 1, 3, 6 and 20 strips and 1 color chart per kit for OTC or low volume testing
    - Unique packaging maintains 2 year shelf life for all strips in the kit compared to 3 months for remaining strips in an opened canister
  - Multi-strip Pouch
    - Canister Refill Kits with 25 strips/pouch uniquely packaged to save cost for low volume testing and extended shelf life by using the canister for refills



Step 1: Immerse strip into urine



Step 2: Remove excess urine

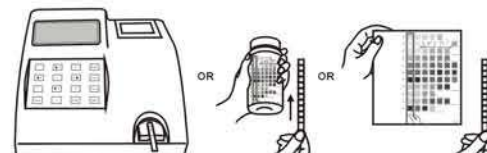

Step 3: Obtain results by analyzer or visual reading

Catalog No.	No. of Parameters	Type of Strip <sup>♦</sup>		Strips per Canister <sup>◇</sup>	Pouch Packaging <sup>▲</sup>	Reading Method			Analyzer-Read Strips: Standard (S) or Additional (A)	Parameters																	
		For Visual Reading	For Analyzer Reading (U120/U500)			Visual	U120	U500		ASC	GLU	BIL	KET	SG	BLO	pH	PRO	URO	NIT	LEU	ALB	CRE					
U031-131	13	13C	NA	100*	✓	✓	NA	NA	A	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*			
U031-111	11		11A	100	✓	✓	✓	✓	S	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*			
U031-101	10		10U	100	✓	✓	✓	✓	S	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*			
			10A			✓	✓	✓	A	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*		
			10C			✓	✓	✓	S	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	
U031-091	9		9U	100	✓	✓	✓	✓	S	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*			
U031-081	8		8U	100	✓	✓	✓	✓	A	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*		
			8N			✓	✓	✓	S	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*		
			8S			✓	✓	✓	A	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	
U031-071	7		7N	100	✓	✓	✓	✓	A	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*			
U031-061	6	6N	6NE	100	✓	✓	✓	✓	A	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*			
		6U	6UE			✓	✓	✓		*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*		
U031-051	5	5B	5BE	100	✓	✓	✓	✓	A	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*			
		5N	5NE			✓	✓	✓		*	*	*	*	*	*	*	*	*	*	*	*	*	*	*			
		5S	5SE			✓	✓	✓		*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	
		5U	5UE			✓	✓	✓		*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	
U031-041	4	4S	4SE	100	✓	✓	✓	✓	A	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*			
		4B	4BE			✓	✓	✓		*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*		
		4K	4KE			✓	✓	✓		*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	
		4G	4GE			✓	✓	✓		*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
		4N	4NE			✓	✓	✓		*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
		4P	4PE			✓	✓	✓		*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
U031-031	3	3P	3PE	100	✓	✓	✓	✓	A	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*			
		3K	3KE			✓	✓	✓		*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*		
		3G	3GE			✓	✓	✓		*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	
		3N	3NE			✓	✓	✓		*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
U031-021	2	2G	2GE	100	✓	✓	✓	✓	A	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*			
		2K	2KE			✓	✓	✓		*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*		
		2N	2NE			✓	✓	✓		*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	
		2B	2BE			✓	✓	✓		*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	
		2U	2UE			✓	✓	✓		*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
		2S	2SE			✓	✓	✓		*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
		2C	2CE			100*	✓	✓		✓	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
U031-011	1	1B	1BE	100	✓	✓	✓	✓	A	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*			
		1P	1PE			✓	✓	✓		*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*		
		1G	1GE			✓	✓	✓		*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	
		1K	1KE			✓	✓	✓		*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
		1R	1RE			✓	✓	✓		*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*

♦Type of Strip:  
Visual Strip Size  
1-6 Parameters: 5 mm x 80 mm; 7-11 Parameters: 5 mm x 108 mm;  
12-13 Parameters: 5 mm x 121 mm  
U120/U500 Strip Size  
1-11 Parameters: 5 mm x 108 mm;  
"E" means extended strip length for 1-6 Parameters

◇ Also available in canisters of 25, 50 and 150 strips.  
\* Not available in canisters of 150 strips  
▲ Single-strip Pouch available in 1, 3, 6 and 20 strip kit  
Canister Refill Kit, with 25 strips per pouch or canister, available in 3-pouch and 1- canister kit, or 4-pouch kit



# U120 Urine Analyzer



## Accurate

- Up to 120 tests/hour in Continuous Test Option
- Capable of reading 1 strip at a time in Single Test Option
- Test modes include Routine, STAT and QC
- Automatic calibration for accurate results and easy operation

## Reliable

- Can read up to 4 Strip combinations with 8, 9, 10, 11 parameters, additional strips with 1-11 parameters available upon request
- Minimal training required

## Convenient Operation

- Saves and recalls the last 2,000 results automatically
- Audible beep signals operator to dip strips in urine
- Can print up to 3 copies per test for convenient reviewing and easy record keeping
- Option to print results on sticker paper for quick and simple record management

## Easy Data Management

- Includes RS232C port for easy data transfer to an external computer or LIS
- Optional Barcode Reader to record patient ID

## Unique Lockout Functions *new!*

- Strip Lockout
  - Prevents using strips of another brand on the U120 Urine Analyzer
  - Requires barcode reader scan or manual entry of the canister code
- User Lockout
  - Eliminates unapproved users from testing
  - Up to 10 lab operators can perform testing, but only the lab administrator can change analyzer settings
- QC Lockout
  - Prevents testing without passing QC
  - QC tests can be performed once every 8 hours, day, week or month
  - Analyzer will alert when to run QC test
  - If QC tests fail, analyzer will switch to STAT mode and list "E" at the end of each test number

## Specifications

Feature	Specifications
Analyzer Type	Manual
Methodology	Reflectance Photometry
Detection	Photosensitive Diode
Throughput	Single Test Option: 60 tests/hour Continuous Test Option: 120 tests/hour
Test Modes	Routine, STAT and QC
Lockout Functions	Strip Lockout: Available Upon Request; User/QC Lockout: Included with option to turn ON/OFF
Memory	Last 2,000 results
Strip Incubation Time	1 Minute
Wavelength of Monochromatic LED	525 nm and 635 nm
Standard Strips	8, 9, 10, 11 Parameters (5 mm x 108 mm)
Additional Strips Available	1-11 Parameters (5 mm x 108 mm); see URS Parameters
Total Combinations Per Analyzer	4 Combinations
Analyzer Ports	Standard RS232C Port for Barcode Reader or Data Transfer USB Port for Data Transfer 25 Pin Parallel Port for External Printer
Capabilities	Internal Thermal Printer (included)      RS232C Barcode Reader (optional) Optional External Printer (not included)      USB or RS232C Data Transfer Cable (optional)
Major Readable Barcodes	Code 128, Code 39, Codabar (NW-7), Interleaved 25, UPC-A, UPC-E, EAN 8, EAN 13
Calibration	Automatic
Available Languages on the Screen	English and additional language(s)
Operating Conditions	0-40°C (32-104°F); ≤ 85% RH
Storage Conditions	-5-50°C (23-122°F); ≤ 90% RH
Power Source	100-240 VAC, 50-60 Hz
Dimensions (L x W x H)	27.2 cm x 26.9 cm x 14.6 cm (10.7" x 10.6" x 5.7")
Display Dimensions (L x W)	10.8 cm x 5.7 cm (4.2" x 2.2")
Weight	2.6 kg (5.7 lbs)

## Ordering Information

Product Name	Catalog No.	Components	Kit Box Dimensions (L x W x H) & Weight	Carton Dimensions (L x W x H) & Weight	Number of Kits/Carton
U120 Urine Analyzer	U111-101†	1 Urine Analyzer 1 Strip holder 2 Printer Paper Rolls	2 Fuses (2.0A) 1 Power Cord 1 Quick Start Guide 1 Instruction Manual	42.0 cm x 41.5 cm x 31 cm; 5.0 kg 16.4" x 16.2" x 12.1"; 176.4 oz	1
U120 Urine Analyzer with Barcode Reader	U111-111†	1 Urine Analyzer 1 Strip holder 2 Printer Paper Rolls 1 Barcode Reader (RS232C)	2 Fuses (2.0A) 1 Power Cord 1 Serial Splitter Cable (RS232C) 1 Quick Start Guide 1 Instruction Manual	44.5 cm x 44.5 cm x 40.0 cm; 5.5 kg 17.5" x 17.5" x 15.7"; 194 oz	1
Barcode Reader	U221-111†	1 Barcode Reader (RS232C)	1 Serial Splitter Cable (RS232C)	23.6 cm x 10.8 cm x 7.8 cm; 0.482 kg 9.3" x 4.3" x 3.1"; 17.0 oz 63.0 cm x 37.0 cm x 30.0 cm; 12.0 kg 24.8" x 14.6" x 11.8"; 423.3 oz	22
Printer Paper Rolls	U121-101	4 Printer Paper Rolls	Thermal Paper (0.06 m x 20 m): 200 results/roll Sticker Paper (0.06 m x 9 m): 100 results/roll	12.0 cm x 12.0 cm x 6.5 cm; 0.36 kg 4.7" x 4.7" x 2.6"; 12.7 oz 63.0 cm x 37.0 cm x 30.0 cm; 21.4 kg 24.8" x 14.6" x 11.8"; 684.3 oz 12.0 cm x 12.0 cm x 6.5 cm; 0.4 kg 4.7" x 4.7" x 2.6"; 14.1 oz 24.8" x 14.6" x 11.8"; 684.3 oz; 754.9 oz	50
U120 Data Transfer Kit	U221-131†	1 Data Transfer Cable (RS232C)	1 Package Insert	16.0 cm x 13.0 cm x 3.5 cm; 0.147 kg 6.3" x 5.1" x 1.4"; 5.2 oz 25.0 cm x 21.0 cm x 15.0 cm; 1.36 kg 9.8" x 8.3" x 5.9"; 48.0 oz	8

✓ CE Marked for sale in the European Community **CE**  
† Cleared for US 510(k)



# U500 Urine Analyzer



## Accurate and Efficient

- Up to 500 tests/hour for medium/large volume sample testing
- Professional accuracy equivalent to market leader
- Automatic strip detection and alignment for better efficiency
- Test modes include Routine, STAT and QC

## Easy to Operate

- Large touch screen LCD offers simple menu navigation
- Uniquely designed strip platform/waste tray unit for easy one-step cleaning

## Convenient

- Automatic calibration and waste disposal reduce hands-on time
- Can read strips with 8, 9, 10, 11 parameters, additional strips with 1-11 parameters available upon request
- Strip selection of up to 4 combinations for analyzer reading
- Stores up to 2,000 records and automatically flags abnormal results
- Capable of printing results on sticker paper for quick and easy record management

## Data Management Capability

- Includes RS232C port for easy data transfer to an external computer or LIS
- Optional Barcode Reader to record patient ID

## Unique Lockout Functions Coming Soon!

- Strip Lockout
  - Prevents using strips of another brand on the U500 Urine Analyzer
  - Requires barcode reader scan or manual entry of the canister code
- User Lockout
  - Eliminates unapproved users from testing
  - Up to 10 lab operators can perform testing, but only the lab administrator can change analyzer settings
- QC Lockout
  - Prevents testing without passing QC
  - QC tests can be performed once every 8 hours, day, week or month
  - Analyzer will alert when to run QC test
  - If QC tests fail, analyzer will switch to STAT mode and list "E" at the end of each test number

## Specifications

Feature	Specifications
Analyzer Type	Semi-Automatic
Methodology	Reflectance Photometry
Detection	Photosensitive Diode
Throughput	500 tests/hour (Measuring cycle: 7 seconds/test)
Test Modes	Routine, STAT and QC
Lockout Functions	Strip Lockout: Available Upon Request; User/QC Lockout: Included with option to turn ON/OFF
Memory	Last 2,000 Records
Strip Incubation Time	1 Minute
Wavelength	525 and 635 nm
Standard Strips	8, 9, 10, 11 Parameters (5 mm x 108 mm)
Additional Strips Available	1-11 Parameters (5 mm x 108 mm); see URS Parameters
Total Combinations Per Analyzer	4 Combinations
Waste Disposal Capacity	Up to 150 Strips
Analyzer Ports	Standard RS232C Port for Barcode Reader or Data Transfer 25 Pin Parallel Port for External Printer
Capabilities	Internal Thermal Printer (included)      RS232C Barcode Reader (optional) Optional External Printer (not included)      RS232C Data Transfer Cable (optional)
Major Readable Barcodes	Code 128, Code 39, Codabar (NW-7), Interleaved 25, UPC-A, UPC-E, EAN 8, EAN 13
Calibration	Automatic
Available Languages on the Screen	English and additional language(s)
Operating Conditions	0-40°C (32-104°F); ≤85% RH
Storage Conditions	-5-50°C (23-122°F); ≤90% RH
Power Source	100-240 VAC, 50-60 Hz
Dimensions (L x W x H)	36.6 cm x 28.3 cm x 19.5cm (14.4" x 11.1" x 7.7")
Display Dimensions (L x W)	11.5 cm x 9.0 cm (4.5" x 3.5")
Weight	4.0 kg (8.8 lbs)

## Ordering Information

Product Name	Catalog No.	Components	Kit Box Dimensions (L x W x H) & Weight	Carton Dimensions (L x W x H) & Weight	Number of Kits/Carton
U500 Urine Analyzer	U211-101 <sup>✓</sup>	1 Urine Analyzer 1 Strip Platform/Waste Tray 2 Printer Paper Rolls	2 Fuses (2.0A) 1 Power Cord 1 Instruction Manual	51.0 cm x 42.0 cm x 38.5 cm; 7 kg 20.1" x 16.5" x 15.2"; 246.9 oz	1
U500 Urine Analyzer with Barcode Reader	U211-111 <sup>✓</sup>	1 Urine Analyzer 1 Strip Platform/Waste Tray 2 Printer Paper Rolls 1 Barcode Reader (RS232C)	2 Fuses (2.0A) 1 Power Cord 1 Serial Splitter Cable (RS232C) 1 Instruction Manual	55.0 cm x 55.0 cm x 55.0cm; 9.2 kg 21.7" x 21.7" x 21.7"; 324.5 oz	1
Barcode Reader	U221-111 <sup>✓†</sup>	1 Barcode Reader (RS232C)	1 Serial Splitter Cable (RS232C)	23.6 cm x 10.8 cm x 7.8 cm; 0.482 kg 9.3" x 4.3" x 3.1"; 17.0 oz	22
Printer Paper Rolls	U121-101	4 Printer Paper Rolls	Thermal Paper (0.06 m x 20 m): 200 results/roll Sticker Paper (0.06 m x 9 m): 100 results/roll	12.0 cm x 12.0 cm x 6.5 cm; 0.360 kg 4.7" x 4.7" x 2.6"; 12.7oz 12.0 cm x 12.0 cm x 6.5 cm; 0.40 kg 4.7" x 4.7" x 2.6"; 14.1oz	50
U500 Data Transfer Kit	U221-131 <sup>✓</sup>	1 Data Transfer Cable (RS232C)	1 Package Insert	16.0 cm x 13.0 cm x 3.5 cm; 0.147kg 6.3" x 5.1" x 1.4"; 5.2 oz	8

**We also offer other rapid diagnostic and medical products:**

Blood Glucose Monitoring Systems, Immunoassay EIA/ELISA and more.

✓ CE Marked for sale in the European Community **CE**  
† Cleared for US 510(k)



# Mission® Urinalysis Reagent Strips (Urine)

## Package Insert

REF U031-011	REF U031-051	REF U031-091	English
REF U031-021	REF U031-061	REF U031-101	
REF U031-031	REF U031-071	REF U031-111	
REF U031-041	REF U031-081		

For rapid detection of multiple analytes in human urine.

For *in vitro* diagnostic use only.

### INTENDED USE

The Urinalysis Reagent Strips (Urine) are firm plastic strips onto which several separate reagent areas are affixed. The test is for the qualitative and semi-quantitative detection of one or more of the following analytes in urine: Ascorbic acid, Glucose, Bilirubin, Ketone (Acetoacetic acid), Specific Gravity, Blood, pH, Protein, Urobilinogen, Nitrite and Leukocytes.

### SUMMARY

Urine undergoes many changes during states of disease or body dysfunction before blood composition is altered to a significant extent. Urinalysis is a useful procedure as an indicator of health or disease, and as such, is a part of routine health screening. The Urinalysis Reagent Strips (Urine) can be used in general evaluation of health, and aids in the diagnosis and monitoring of metabolic or systemic diseases that affect kidney function, endocrine disorders and diseases or disorders of the urinary tract.<sup>1,2</sup>

### PRINCIPLE AND EXPECTED VALUES

**Ascorbic acid:** This test involves decolorization of Tillmann's reagent. The presence of ascorbic acid causes the color of the test field to change from blue-green to orange. Patients with adequate diet may excrete 2-10 mg/dL daily. After ingesting large amounts of ascorbic acid, levels can be around 200 mg/dL.

**Glucose:** This test is based on the enzymatic reaction that occurs between glucose oxidase, peroxidase and chromogen. Glucose is first oxidized to produce gluconic acid and hydrogen peroxide in the presence of glucose oxidase. The hydrogen peroxide reacts with potassium iodide chromogen in the presence of peroxidase. The extent to which the chromogen is oxidized determines the color which is produced, ranging from green to brown. Glucose should not be detected in normal urine. Small amounts of glucose may be excreted by the kidney.<sup>3</sup> Glucose concentrations as low as 100 mg/dL may be considered abnormal if results are consistent.

**Bilirubin:** This test is based on azo-coupling reaction of bilirubin with diazotized dichloroaniline in a strongly acidic medium. Varying bilirubin levels will produce a pinkish-tan color proportional to its concentration in urine. In normal urine, no bilirubin is detectable by even the most sensitive methods. Even trace amounts of bilirubin require further investigation. Atypical results (colors different from the negative or positive color blocks shown on the color chart) may indicate that bilirubin-derived bile pigments are present in the urine specimen, and are possibly masking the bilirubin reaction.

**Ketone:** This test is based on ketones reacting with nitroprusside and acetoacetic acid to produce a color change ranging from light pink for negative results to a darker pink or purple color for positive results. Ketones are normally not present in urine. Detectable ketone levels may occur in urine during physiological stress conditions such as fasting, pregnancy and frequent strenuous exercise.<sup>4-6</sup> In starvation diets, or in other abnormal carbohydrate metabolism situations, ketones appear in the urine in excessively high concentration before serum ketones are elevated.<sup>7</sup>

**Specific Gravity:** This test is based on the apparent pKa change of certain pretreated polyelectrolytes in relation to ionic concentration. In the presence of an indicator, colors range from deep blue-green in urine of low ionic concentration to green and yellow-green in urine of increasing ionic concentration. Randomly collected urine may vary in specific gravity from 1.003-1.035.<sup>8</sup> Twenty-four hour urine from healthy adults with normal diets and fluid intake will have a specific gravity of 1.016-1.022.<sup>3</sup> In cases of severe renal damage, the specific gravity is fixed at 1.010, the value of the glomerular filtrate.

**Blood:** This test is based on the peroxidase-like activity of hemoglobin which catalyzes the reaction of diisopropylbenzene dihydroperoxide and 3,3',5,5'-tetramethylbenzidine. The resulting color ranges from orange to green to dark blue. Any green spots or green color development on the reagent area within 60 seconds is significant and the urine specimen should be examined further. Blood is often, but not invariably, found in the urine of menstruating females. The significance of a trace reading varies among patients and clinical judgment is required in these specimens.

**pH:** This test is based on a double indicator system which gives a broad range of colors covering the entire urinary pH range. Colors range from orange to yellow and green to blue. The expected range for normal urine specimens from newborns is pH 5-7.<sup>9</sup> The expected range for other normal urine specimens is pH 4.5-8, with an average result of pH 6.<sup>9</sup>

**Protein:** This reaction is based on the phenomenon known as the "protein error" of pH indicators where an indicator that is highly buffered will change color in the presence of proteins (anions) as the indicator releases hydrogen ions to the protein. At a constant pH, the development of any green color is due to the presence of protein. Colors range from yellow to yellow-green for negative results and green to green-blue for positive results. 1-14 mg/dL of protein may be excreted by a normal kidney.<sup>10</sup> A color matching any block greater than trace indicates significant proteinuria. Clinical judgment is required to evaluate the significance of trace results.

**Urobilinogen:** This test is based on a modified Ehrlich reaction between p-diethylaminobenzaldehyde and urobilinogen in strongly acidic medium to produce a pink color. Urobilinogen is one of the major compounds produced in heme synthesis and is a normal substance in urine. The expected range for normal urine with this test is 0.2-1.0 mg/dL (3.5-17 μmol/L).<sup>8</sup> A result of 2.0 mg/dL (35 μmol/L) may be of clinical significance, and the patient specimen should be further evaluated.

**Nitrite:** This test depends upon the conversion of nitrate to nitrite by the action of Gram negative bacteria in the urine. In an acidic medium, nitrite in the urine reacts with p-arsanilic acid to form a diazonium compound. The diazonium compound in turn couples with 1 N-(1-naphthyl) ethylenediamine to produce a pink color. Nitrite is not detectable in normal urine.<sup>9</sup> The nitrite area will be positive in some cases of infection, depending on how long the urine specimens were retained in the bladder prior to collection. Retrieval of positive cases with the nitrite test ranges from as low as 40% in cases where little bladder incubation occurred, to as high as approximately 80% in cases where bladder incubation took place for at least 4 hours.

**Leukocytes:** This test reveals the presence of granulocyte esterases. The esterases cleave a derivatized pyrazole amino acid ester to liberate derivatized hydroxy pyrazole. This pyrazole then reacts with a diazonium salt to produce a beige-pink to purple color. Normal urine specimens generally yield negative results. Trace results may be of questionable clinical significance. When trace results occur, it is recommended to retest using a fresh specimen from the same patient. Repeated trace and positive results are of clinical significance.

### REAGENTS AND PERFORMANCE CHARACTERISTICS

Based on the dry weight at the time of impregnation, the concentrations given may vary within manufacturing tolerances. The following table below indicates read times and performance characteristics for each parameter.

Reagent	Read Time	Composition	Description
Ascorbic Acid (ASC)	30 seconds	2,6-dichlorophenolindophenol; buffer and non-reactive ingredients	Detects ascorbic acid as low as 5-10 mg/dL (0.28-0.56 mmol/L).
Glucose (GLU)	30 seconds	glucose oxidase; peroxidase; potassium iodide; buffer; non-reactive ingredients	Detects glucose as low as 50-100 mg/dL (2.5-5 mmol/L).
Bilirubin (BIL)	30 seconds	2,4-dichloroaniline diazonium salt; buffer and non-reactive ingredients	Detects bilirubin as low as 0.4-1.0 mg/dL (6.8-17 μmol/L).
Ketone (KET)	40 seconds	sodium nitroprusside; buffer	Detects acetoacetic acid as low as 2.5-5 mg/dL (0.25-0.5 mmol/L).
Specific Gravity (SG)	45 seconds	bromthymol blue indicator; buffer and non-reactive ingredients; poly (methyl vinyl ether/maleic anhydride); sodium hydroxide	Determines urine specific gravity between 1.000 and 1.030. Results correlate with values obtained by refractive index method within ± 0.005.
Blood (BLO)	60 seconds	3,3',5,5'-tetramethylbenzidine (TMB); diisopropylbenzene dihydroperoxide; buffer and non-reactive ingredients	Detects free hemoglobin as low as 0.018-0.060 mg/dL or 5-10 Ery/ $\mu$ L in urine specimens with ascorbic acid content of < 50 mg/dL.
pH	60 seconds	methyl red sodium salt; bromthymol blue; non-reactive ingredients	Permits the quantitative differentiation of pH values within the range of 5-9.
Protein (PRO)	60 seconds	tetrabromophenol blue; buffer and non-reactive ingredients	Detects albumin as low as 7.5-15 mg/dL (0.075-0.15 g/L).
Urobilinogen (URO)	60 seconds	p-diethylaminobenzaldehyde; buffer and non-reactive ingredients	Detects urobilinogen as low as 0.2-1.0 mg/dL (3.5-17 μmol/L).
Nitrite (NIT)	60 seconds	p-arsanilic acid; N-(1-naphthyl) ethylenediamine; non-reactive ingredients	Detects sodium nitrite as low as 0.05-0.1 mg/dL in urine with a low specific gravity and less than 30 mg/dL ascorbic acid.
Leukocytes (LEU)	120 seconds	derivatized pyrrole amino acid ester; diazonium salt; buffer; non-reactive ingredients	Detects leukocytes as low as 9-15 white blood cells Leu/ $\mu$ L in clinical urine.

The performance characteristics of the Urinalysis Reagent Strips (Urine) have been determined in both laboratory and clinical tests. Parameters of importance to the user are sensitivity, specificity, accuracy and precision. Generally, this test has been developed to be specific for the parameters to be measured with the exceptions of the interferences listed. Please refer to the Limitations section in this package insert.

Interpretation of visual results is dependent on several factors: the variability of color perception, the presence or absence of inhibitory factors, and the lighting conditions when the strip is read. Each color block on the chart corresponds to a range of analyte concentrations.

### PRECAUTIONS

- For *in vitro* diagnostic use only. Do not use after the expiration date.
- The strip should remain in the closed canister until use.
- Do not touch the reagent areas of the strip.
- Discard any discolored strips that may have deteriorated.
- All specimens should be considered potentially hazardous and handled in the same manner as an infectious agent.
- The used strip should be discarded according to local regulations after testing.

### STORAGE AND STABILITY

Store as packaged in the closed canister either at room temperature or refrigerated (2-30°C). Keep out of direct sunlight. The strip is stable through the expiration date printed on the canister label. Do not remove the desiccant. Remove only enough strips for immediate use. Replace cap immediately and tightly. **DO NOT FREEZE.** Do not use beyond the expiration date.

Note: Once the canister has been opened, the remaining strips are stable for up to 3 months. Stability may be reduced in high humidity conditions.

### SPECIMEN COLLECTION AND PREPARATION

A urine specimen must be collected in a clean and dry container and tested as soon as possible. Do not centrifuge. The use of urine preservatives is not recommended. If testing cannot be done within an hour after voiding, refrigerate the specimen immediately and let it return to room temperature before testing.

Prolonged storage of unpreserved urine at room temperature may result in microbial proliferation with resultant changes in pH. A shift to alkaline pH may cause false positive results with the protein test area. Urine containing glucose may decrease in pH as organisms metabolize the glucose.

Contamination of the urine specimen with skin cleansers containing chlorhexidine may affect protein (and to a lesser extent, specific gravity and bilirubin) test results.

### MATERIALS

#### Materials Provided

- Strips
- Package insert

#### Materials Required But Not Provided


- Specimen collection container
- Timer

### DIRECTIONS FOR USE

**Allow the strip, urine specimen, and/or controls to reach room temperature (15-30°C) prior to testing.**

- Remove the strip from the closed canister and use it as soon as possible. Immediately close the canister tightly after removing the required number of strip(s). Completely immerse the reagent areas of the strip in fresh, well-mixed urine and immediately remove the strip to avoid dissolving the reagents. See illustration 1 below.
- While removing the strip from the urine, run the edge of the strip against the rim of the urine container to remove excess urine. Hold the strip in a horizontal position and bring the edge of the strip into contact with an absorbent material (e.g. a paper towel) to avoid mixing chemicals from adjacent reagent areas and/or soiling hands with urine. See illustration 2 below.
- Compare the reagent areas to the corresponding color blocks on the canister label at the specified times. Hold the strip close to the color blocks and match carefully. See illustration 3 below.

Note: Results may be read up to 2 minutes after the specified times.

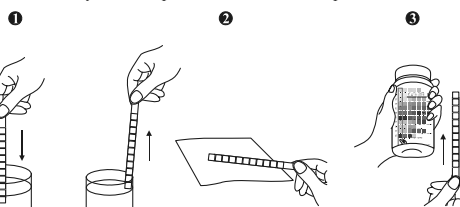

### INTERPRETATION OF RESULTS

Results are obtained by direct comparison of the color blocks printed on the canister label. The color blocks represent nominal values; actual values will vary close to the nominal values. In the event of unexpected or questionable results, the following steps are recommended: confirm that the strips have been tested within the expiration date printed on the canister label, compare results with known positive and negative controls and repeat the test using a new strip. If the problem persists, discontinue using the strip immediately and contact your local distributor.

### QUALITY CONTROL

For best results, performance of reagent strips should be confirmed by testing known positive and negative specimens/controls whenever a new test is performed, or whenever a new canister is first opened. Each laboratory should establish its own goals for adequate standards of performance.

### LIMITATIONS

**Note:** The Urinalysis Reagent Strips (Urine) may be affected by substances that cause abnormal urine color such as drugs containing azo dyes (e.g. Pyridium<sup>®</sup>, Azo Gantarin<sup>®</sup>, Azo Gantanol<sup>®</sup>), nitrofurantoin (Microdantin<sup>®</sup>, Furadantin<sup>®</sup>), and riboflavin.<sup>8</sup> The color development on the test pad may be masked or a color reaction may be produced that could be interpreted as false results.

**Ascorbic acid:** No interference is known.

**Glucose:** The reagent area does not react with lactose, galactose, fructose or other metabolic substances, nor with reducing metabolites of drugs (e.g. salicylates and nalidixic acid). Sensitivity may be decreased in specimens with high specific gravity (>1.025) and with ascorbic acid concentrations of  $\geq 25$  mg/dL. High ketone levels  $\geq 100$  mg/dL may cause false negative results for specimens containing a small amount of glucose (50-100 mg/dL).

**Bilirubin:** Bilirubin is absent in normal urine, so any positive result, including a trace positive, indicates an underlying pathological condition and requires further investigation. Reactions may occur with urine containing large doses of chlorpromazine or rifampin that might be mistaken for positive bilirubin.<sup>9</sup> The presence of bilirubin-derived bile pigments may mask the bilirubin reaction. This phenomenon is characterized by color development on the test patch that does not correlate with the colors on the color chart. Large concentrations of ascorbic acid may decrease sensitivity.

**Ketone:** The test does not react with acetone or  $\beta$ -hydroxybutyrate.<sup>8</sup> Urine specimens of high pigment, and other substances containing sulphydryl groups may occasionally give reactions up to and including trace ( $\pm$ ).

**Specific Gravity:** Ketoacidosis or protein higher than 300 mg/dL may cause elevated results. Results are not affected by non-ionic urine components such as glucose. If the urine has a pH of 7 or greater, add 0.005 to the specific gravity reading indicated on the color chart.

**Blood:** A uniform blue color indicates the presence of myoglobin, hemoglobin or hemolyzed erythrocytes.<sup>8</sup> Scattered or compacted blue spots indicate intact erythrocytes. To enhance accuracy, separate color scales are provided for hemoglobin and for erythrocytes. Positive results with this test are often seen with urine from menstruating females. It has been reported that urine of high pH reduces sensitivity, while moderate to

high concentration of ascorbic acid may inhibit color formation. Microbial peroxidase, associated with urinary tract infection, may cause a false positive reaction. The test is slightly more sensitive to free hemoglobin and myoglobin than to intact erythrocytes.

**pH:** If the procedure is not followed and excess urine remains on the strip, a phenomenon known as "runover" may occur, in which the acid buffer from the protein reagent will run onto the pH area, causing the pH result to appear artificially low. pH readings are not affected by variations in urinary buffer concentration.

**Protein:** Any green color indicates the presence of protein in the urine. This test is highly sensitive for albumin, and less sensitive to hemoglobin, globulin and mucoprotein.<sup>8</sup> A negative result does not rule out the presence of these other proteins. False positive results may be obtained with highly buffered or alkaline urine. Contamination of urine specimens with quaternary ammonium compounds or skin cleansers containing chlorhexidine may produce false positive results.<sup>8</sup> The urine specimens with high specific gravity may give false negative results.

**Urobilinogen:** All results lower than 1 mg/dL urobilinogen should be interpreted as normal. A negative result does not at any time preclude the absence of urobilinogen. The reagent area may react with interfering substances known to react with Ehrlich's reagent, such as p-aminosalicylic acid and sulfonamides.<sup>9</sup> False negative results may be obtained if formalin is present. The test cannot be used to detect porphobilinogen.

**Nitrite:** The test is specific for nitrite and will not react with any other substance normally excreted in urine. Any degree of uniform pink to red color should be interpreted as a positive result, suggesting the presence of nitrite. Color intensity is not proportional to the number of bacteria present in the urine specimen. Pink spots or pink edges should not be interpreted as a positive result. Comparing the reacted reagent area on a white background may aid in the detection of low nitrite levels, which might otherwise be missed. Ascorbic acid above 30 mg/dL may cause false negatives in urine containing less than 0.05 mg/dL nitrite ions. The sensitivity of this test is reduced for urine specimens with highly buffered alkaline urine or with high specific gravity. A negative result does not at any time preclude the possibility of bacteruria. Negative results may occur in urinary tract infections from organisms that do not contain reductase to convert nitrate to nitrite; when urine has not been retained in the bladder for a sufficient length of time (at least 4 hours) for reduction of nitrate to nitrite to occur; when receiving antibiotic therapy or when dietary nitrate is absent.

**Leukocytes:** The result should be read between 60-120 seconds to allow for complete color development. The intensity of the color that develops is proportional to the number of leukocytes present in the urine specimen. High specific gravity or elevated glucose concentrations ( $\geq 2,000$  mg/dL) may cause test results to be artificially low. The presence of cephalaxin, cephalothin, or high concentrations of oxalic acid may also cause test results to be artificially low. Tetracycline may cause decreased reactivity, and high levels of the drug may cause a false negative reaction. High urinary protein may diminish the intensity of the reaction color. This test will not react with erythrocytes or bacteria common in urine.<sup>8</sup>

### BIBLIOGRAPHY

- Free AH, Free HM. *Urinalysis, Critical Discipline of Clinical Science*. CRC Crit. Rev. Clin. Lab. Sci. 3(4): 481-531, 1972.
- Yoder J, Adams EC, Free, AH. *Simultaneous Screening for Urinary Occult Blood, Protein, Glucose, and pH*. Amer. J. Med Tech. 31:285, 1965.
- Shchersten B, Fritz H. *Subnormal Levels of Glucose in Urine*. JAMA 201:129-132, 1967.
- McGarry JD, Lilly. Lecture, 1978: New Perspectives in the Regulation of Ketogenesis. Diabetes 28: 517-523 May, 1978.
- Williamson DH. *Physiological Ketoses, or Why Ketone Bodies?* Postgrad. Med. J. (June Suppl.): 372-375, 1971.
- Paterson P, et al. *Maternal and Fetal Ketone Concentrations in Plasma and Urine*. Lancet: 862-865; April 22, 1967.
- Fraser J, et al. *Studies with a Simplified Nitroprusside Test for Ketone Bodies in Urine, Serum, Plasma and Milk*. Clin. Chem. Acta II: 372-378, 1965.
- Henry JB, et al. *Clinical Diagnosis and Management by Laboratory Methods*, 20<sup>th</sup> Ed. Philadelphia. Saunders. 371-372, 375, 379, 382, 385, 2001.
- Tietz NW. *Clinical Guide to Laboratory Tests*. W.B. Saunders Company. 1976.
- Burtis CA, Ashwood ER. *Tietz Textbook of Clinical Chemistry* 2<sup>nd</sup> Ed. 2205, 1994.

### Index of Symbols

	Consult instructions for use		Tests per kit		Manufacturer
	For <i>in vitro</i> diagnostic use only		Use by		Do not reuse
	Store between 2-30°C		Lot Number		REF Catalog #
	Authorized Representative				

**ACON Laboratories, Inc.**  
10125 Mesa Rim Road,  
San Diego, CA 92121, USA

**MDSS GmbH**  
Schiffgraben 41  
30175 Hannover, Germany

## TO WHOM IT MAY CONCERN

To any governmental departments,  
registration and/or trade offices in MOLDOVA

### Distribution Authorisation Letter

This letter confirms that **Sanmedico**  
**Mun. Chisinau**  
**Str. Petricani 88/1 of. 10**  
**Republica MOLDOVA**

is the **legal, exclusive and sole** representative of **TECO Medical Instruments Production + Trading GmbH, Dieselstr. 1, 84088 Neufahrn NB, Germany**, for the territory of **MOLDOVA** only for all TECO products listed below. **Sanmedico** may participate in public and private tenders, providing sales to all TECO customers in the territory. We as manufacturer certify that our warranty is duly passed to the purchaser through **Sanmedico** for the price, delivery schedules and the specifications of the published literature, catalogues and fully covering the commodities offered.

**Sanmedico** will provide the following information to TECO GmbH when so required in relation to its market surveillance activities:

Reporting of incidents to TECO must take place within 3 working days  
Serial number of the device, exact location of the device and the user.

Validity: January 1<sup>st</sup>, 2023 to December 31<sup>st</sup>, 2024

Termination: Confirmation ends automatically on Dec. 31<sup>st</sup> of 2024  
and must be then renewed.

#### Products:

- Coatron M1 Manual 1-channel Coagulometer (out of production)
- Coatron M2 Manual 2-channel Coagulometer (out of production)
- Coatron X Eco Manual 1-channel Coagulometer
- Coatron X Pro Manual 2-channel Coagulometer
- Coatron X Top Manual 4-channel Coagulometer
- Coatron A4 Fully automated Coagulometer, 4 optic channels
- Coatron A6 Fully automated Coagulometer, 6 optic channels
- Coatron A6 plus Fully automated Coagulometer, 6 optic channels
- Hemostasis Reagents all instruments with complete accessory, consumables and spare parts
- Complete product line

This document is signed in Neufahrn, Germany, on December 21<sup>st</sup>, 2022

TECO Medical Instruments Production+Trading GmbH

  
Christian Hoetzl



---

# Certificate of Approval

This is to certify that the Management System of:

## **TECO Medical Instruments, Production + Trading GmbH**

Dieselstr. 1, 84088 Neufahrn, Germany

has been approved by LRQA to the following standards:

**ISO 13485:2016**

Approval number(s): ISO 13485 – 00038268

**The scope of this approval is applicable to:**

Design, development, manufacturing, storage and sales of coagulation instruments and in-vitro-diagnostic reagents used in the hemostaseology and coagulation.



**Paul Graaf**

---

Area Operations Manager, Europe

Issued by: LRQA Limited



**KONFORMITÄTSERKLÄRUNG  
DECLARATION OF CONFORMITY**

Doc#200/08-2022

Hersteller / Manufacturer: **TECO Medical Instruments  
Production + Trading GmbH**  
 Adresse / Address: **Dieselstrasse 1, 84088 Neufahrn, Germany**  
 Marktakteur / Actor ID SRN: **DE-MF-000022642 <https://ec.europa.eu>**

Wir erklären hier für die im Anhang A ( Seite 2 – 23 IVD Produkte) spezifizierten Produkte dass sie gemäß der Richtlinie für In-vitro-Diagnostika Medizinprodukte 98/79/EC klassifiziert sind als allgemeine IVD.

Diese Konformitätserklärung wird unter der alleinigen Verantwortung des Herstellers i.V.m. Artikel 110 Abs.3 und Abs.4 der Verordnung (EU) 2017/746 und des § 8 Abs.1 des Medizinprodukte-Durchführungsgesetzes, in der jeweils geltenden Fassung, ausgestellt.

Im Falle eigenmächtiger Veränderungen am Produkt oder der nicht bestimmungsgemäßen Verwendung verliert diese Erklärung ihre Gültigkeit.

We declare herewith for the products specified in Annex A ( page 2 - 23 IVD products) that they are classified as general IVD according to the In Vitro Diagnostic Medical Devices Directive 98/79/EC.

This declaration of conformity is issued under the sole responsibility of the manufacturer in according to article 110 para.3 and para.4 of Regulation (EU) 217/746 and section 8 para.1 of the Medical Device Law Implementing Act.

In case of unauthorised modifications to the products or un-intended use, this declaration loses its validity.

Sie entsprechen den anwendbaren Anforderungen der Richtlinie:

They meet applicable requirements of:

Richtlinie 98/79/EG über In-vitro-Diagnostika  
klassifiziert gemäß Artikel 9 als "alle anderen Produkte"

Directive 98/79/EC on in-vitro-diagnostic medical devices  
classified according to article 9 as „all other products“

Die Qualitätssicherung entspricht den Anforderungen der  
Richtlinie 98/79/EG über In-vitro-Diagnostika  
für diese Art von Produkten.

The Quality Assurance is in accordance with the requirements  
of Directive 98/79/EC on in-vitro-diagnostic medical devices  
for those kind of products.

Der implementierte QM-Prozess entspricht der EN ISO 13485:2021

The implemented QM Process complies with EN ISO 13485:2021

Die vorstehende Konformitätserklärung ist gültig für alle Chargen  
dieser Produkte, die nach dem Datum der Unterzeichnung in Verkehr  
gebracht wurden.

The above mentioned declaration of conformity is valid for all lots  
of this product, which are distributed after the date of signature.

Das Konformitätsbewertungsverfahren entspricht Anhang III  
der Richtlinie 98/79/EG über In-vitro-Diagnostika  
für diese Art von Produkten.

The conformity assessment procedure complies with Annex III  
of Directive 98/79/EC on in-vitro-diagnostic medical devices  
for those kind of products.

Ort und Datum der Unterzeichnung: **Neufahrn, 2022-08-31**  
Place and date of issue:



Christian Hötzl  
Verantwortliche Person / PRRC

Doc#200/08-2022

## KONFORMITÄTSERKLÄRUNG – DECLARATION OF CONFORMITY

Directive 98/79/EC Annex A

Übrige Produkte – Reagenzien für In-vitro-Diagnostika

Other products – Reagents for in vitro diagnostic – general IVD

Pos.	Article No	Tradename	Unit	Generic Device Term	EMDN / GMDN Code EUDAMED DI
1	A0230-040	TEClot PT-S (Quick)	10x4ml PT-S	Prothrombin time ( quick test )	W0103020101 / 30539 B-PTS-A0230-040X7
2	A0230-100	TEClot PT-S (Quick)	10x10ml PT-S	Prothrombin time ( quick test )	W0103020101 / 30539 B-PTS-A0230-100WY
3	A0260-050	TEClot PT-B (Owren)	5x10ml PT-B	Prothrombin time ( quick test )	W0103020199 / 55986 B-PTB-A0260-050G2
4	A0320-050	TEClot APTT-S	10x5ml APTT-S	Activated partial thromboplastin time	W0103020102 / 55982 B-APTS-A0320-050AM
5	A0401-020	TEClot TT	10x2ml TT	Thrombin time / reptilase / batroxbin time	W0103020103 / 55988 B-TT-A0401-0207P
6	A0511-020	TEClot FIB	10x2ml FIB	Fibrinogen assays (factor i)	W0103020201 / 55997 B-FIB-A0511-020N2
7	A0511-050	TEClot FIB	10x5ml FIB	Fibrinogen assays (factor i)	W0103020201 / 55997 B-FIB-A0511-050NB
8	C1010-020	TEChrom AT	6x6ml reagent FXa 3x3 ml substrate	Antithrombin	W0103020602 / 56156 B-AT-C1010-020HL
9	D2010-012	Red D-Dimer	3x4ml latex 3x7ml reaction buffer	D-Dimer	W0103020503 / 47349 B-DD-D2010-0126W
10	D2020-005	Blue D-Dimer LC	1x5ml latex LC 1x7ml reaction buffer	D-Dimer	W0103020503 / 47349 B-DD-D2020-0057E
11	P8001-010	TECal N	10x1ml	Calibration plasma for haemostasis	W0103020701 / 45786 B-CAL-P8001-005X8
12	P8200-005	TECal DD	5x1ml	Calibration plasma for haemostasis	W0103020701 / 47348 B-CAL-P8200-005XX
13	P6001-010	TEControl N	10x1ml	Control plasma for haemostasis	W0103020702 / 30590 B-CTRL-P6001-010H7
14	P6101-010	TEControl A	10x1ml	Control plasma for haemostasis	W0103020702 / 30590 B-CTRL-P6101-010HQ
15	P6201-010	TEControl A Plus	10x1ml	Control plasma for haemostasis	W0103020702 / 30590 B-CTRL-P6201-010J9
16	P5001-010	TEClot Factor II	10x1ml	Coagulation factor ii ( prothrombin )	W0103020202 / 30542 B-FAC-II-P5001-010ML
17	P5101-010	TEClot Factor V	10x1ml	Coagulation factor v	W0103020204 / 30544 B-FAC-V-P5101-010AN
18	P5201-010	TEClot Factor VII	10x1ml	Coagulation factor vii	W0103020205 / 30545 B-FAC-VII-P5201-0107B
19	P5301-010	TEClot Factor VIII	10x1ml	Coagulation factor viii	W0103020207 / 30547 B-FAC-VIII-P5301-01097
20	P5401-010	TEClot Factor IX	10x1ml	Coagulation factor ix	W0103020208 / 30548 B-FAC-IX-P5401-0106C
21	P5501-010	TEClot Factor X	10x1ml	Coagulation factor x	W0103020209 / 30549 B-FAC-X-P5501-010EQ
22	P5601-010	TEClot Factor XI	10x1ml	Coagulation factor xi	W0103020210 / 30551 B-FAC-XI-P5601-010A8
23	P5701-010	TEClot Factor XII	10x1ml	Coagulation factor xii	W0103020211 / 30552 B-FAC-XII-P5701-010CJ

(Recital 23 of Directive 98/79/EC on In Vitro Diagnostics Medical Devices) - Annex A - general IVD



# KONFORMITÄTSERKLÄRUNG

## DECLARATION OF CONFORMITY

Doc#100/07-2021

Wir / We

### TECO Medical Instruments Production and Trading GmbH

Name des Herstellers / Manufacturer's name

**Dieselstrasse 1, 84088 Neufahrn, Germany**

Anschrift / Address

erklären in alleiniger Verantwortung, dass die unten gelisteten IVD Zubehör Produkte:  
*declare under our own responsibility, that the IVD accessories products, listed below:*

Doppelküvette / <i>Double cuvette</i>	Ref. 19 000 02
Einzelküvette / <i>Single cuvette</i>	Ref. 20 000 02, 24 100 00
4-fach Küvette / <i>Cuvette 4 pos/ea</i>	Ref. 80 521 10
6-fach Küvette / <i>Cuvette 6 pos/ea</i>	Ref. 80 560 00
6-fach Küvette (micro) / <i>Cuvette 6 pos/ea (micro)</i>	Ref. 80 570 00

allen anwendbaren Anforderungen folgender Richtlinien entsprechen: *meet all applicable requirements of:*

1. Richtlinie 98/79/EG über In-vitro Diagnostika und ihrem Zubehör, klassifiziert gemäß Artikel 9 als: "alle anderen Produkte"- im Sinne von Zubehör zu In vitro Diagnostika gemäß Artikel 1.

*1. Directive 98/79/EC on In-vitro diagnostic medical devices and their accessories, classified according to article 9 as: "all other products" – and in term of accessories for in vitro diagnostics according to article 1.*

2. Richtlinie 2011/65/EU (RoHS III)

*2. Directive 2011/65/EU (RoHS III)*

Das QM-System des Herstellers ist zertifiziert nach:

*The QM-system of the manufacturer is certified for:*

**EN ISO 13485:2016**

***EN ISO 13485:2016***

Konformitätsbewertungsverfahren gemäß:

*Conformity assessment procedure according to:*

Gemäß Anhang III der Richtlinie 98/79/EG

*According to Annex III of Directive 98/79/EC*

Ort und Datum der Unterzeichnung:  
Place and date of issue:

Neufahrn, 27.07.2021  
Neufahrn, July 27, 2021

Matthias Dieckmann  
General Manager



# TECO

MEDICAL INSTRUMENTS  
PRODUCTION+TRADING GMBH

Dieselstraße 1  
D-84088 Neufahrn N.B.  
fon: +49-8773/707 80-0  
fax: +49-8773/707 80-29

Neufahrn, 26/04/2018

## TO WHOM IT MAY CONCERN

We confirm that the instruments Coatron X Eco, Coatron X Pro and Coatron X Top have a closed cuvette system. Cuvettes have to be purchased with voucher identification code from TECO GmbH.



Christian Hoetzel  
General Manager  
TECO Germany





Quality Management  
We are certified  
Voluntary participation in regular  
monitoring according to ISO 9001:2008



# TECO

MEDICAL INSTRUMENTS  
PRODUCTION+TRADING GMBH

Dieselstraße 1  
D-84088 Neufahrn N.B.  
fon: +49-8773/707 80-0  
fax: +49-8773/707 80-29

# CERTIFICATE

for: **Mr. Vitalie Goreacii**

---

Company: **Sanmedico SRL**  
Str. Petricani 88/1, oficiul 10  
Chisinau - Rep. Moldava MD-2059  
MOLDOVA

have participated with success at the intensive training session:

**Application and technical training for following instruments:**

- **Coatron X series**
  - **Installation**
  - **Application**
  - **General use, also in combination with TECAM Software**
  - **Technical and After Sales Service**

Supervisors: **Mr. Chr. Hoetzi and Mrs. Wendy Guo**

---

Place of Training: **TECO – Germany**

Date: **November 18<sup>th</sup>, 2019**



Christian Hoetzi  
General Manager



TOP  
INNOVATION  
2017 - 2018

Clotting  
Chromogenic  
Immunturbidimetric

# Coatron

Semi-automated  
Coagulation Analyzer Series

With 1, 2 or 4 optical channels



# TECO

Innovation in Coagulation

# A new area of manual and semi-automated Coagulation Analyser rise up

The Coatron X instrument line is a consequent continuation in the development of the Coatron product line. Over 25 years in experience and innovation is the reference for our new Coatron X instrumentation line.

The unique detection principle in combination with the high-level analytical algorithm calculates exact, precise and reproducible results.

Easy in operation – self instructing user dialogue - reliable

## **Highest optical resolution, enlarged optic range, smallest sample and reagent volume**

0.1 mOD, 0 - 3800 mOD, just with 75 µL sample and reagent volume

## **Complete optical analysis**

No further parts required, like balls, stirrers etc.

## **Adaptation of the light level**

Automatic light level adjustment of the optic channels to each sample

## **Exclusion of disturbance**

Stray light reduction, exact temperature control, all parameter are preset

“Complete range of Coagulation Analysis with the highest standard and reliability. The new generation of Coagulation instruments with optical detection are here.”

Coatron X - product family



With 1, 2 or 4 optical channels.

[www.teco-medical.com](http://www.teco-medical.com)

## Prepared for the daily routine and the upcoming requirements


### One instrument – many possibilities

The Coatron X family is prepared to work with one, two or four channels. The built-up and functionality is specifically designed to each instrument version and requirements. The operation with the intuitive user dialogue and handling of the detection results are easy and effective. The possibility to connect the instrument to the **TECO Cloud** offers new perspective of instrument, reagent and consumables verification and handling. The precise and correct patient result is what we want to secure.




### Quality is our basic demand

TECO develop and produce with qualified and specialized companies, located in Germany. High reliability, nearly maintenance free instruments are our benefit. Our reference is 25 years, in worldwide laboratories, with satisfied users.

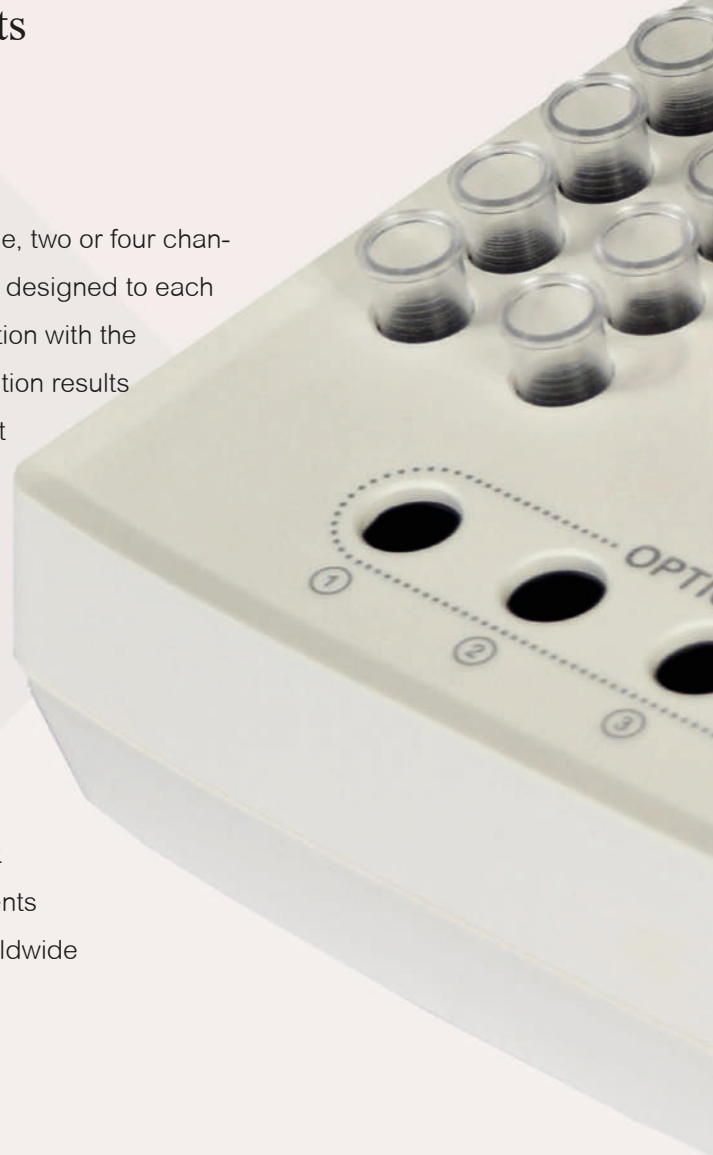

### TECO Cloud Services – A strong data bank and application service behind

All instrument versions of the Coatron X family are connectable via Bluetooth to Smart-devices, like mobile devices, tablets, etc. with a specific APP or direct access to the TECO Cloud Services.

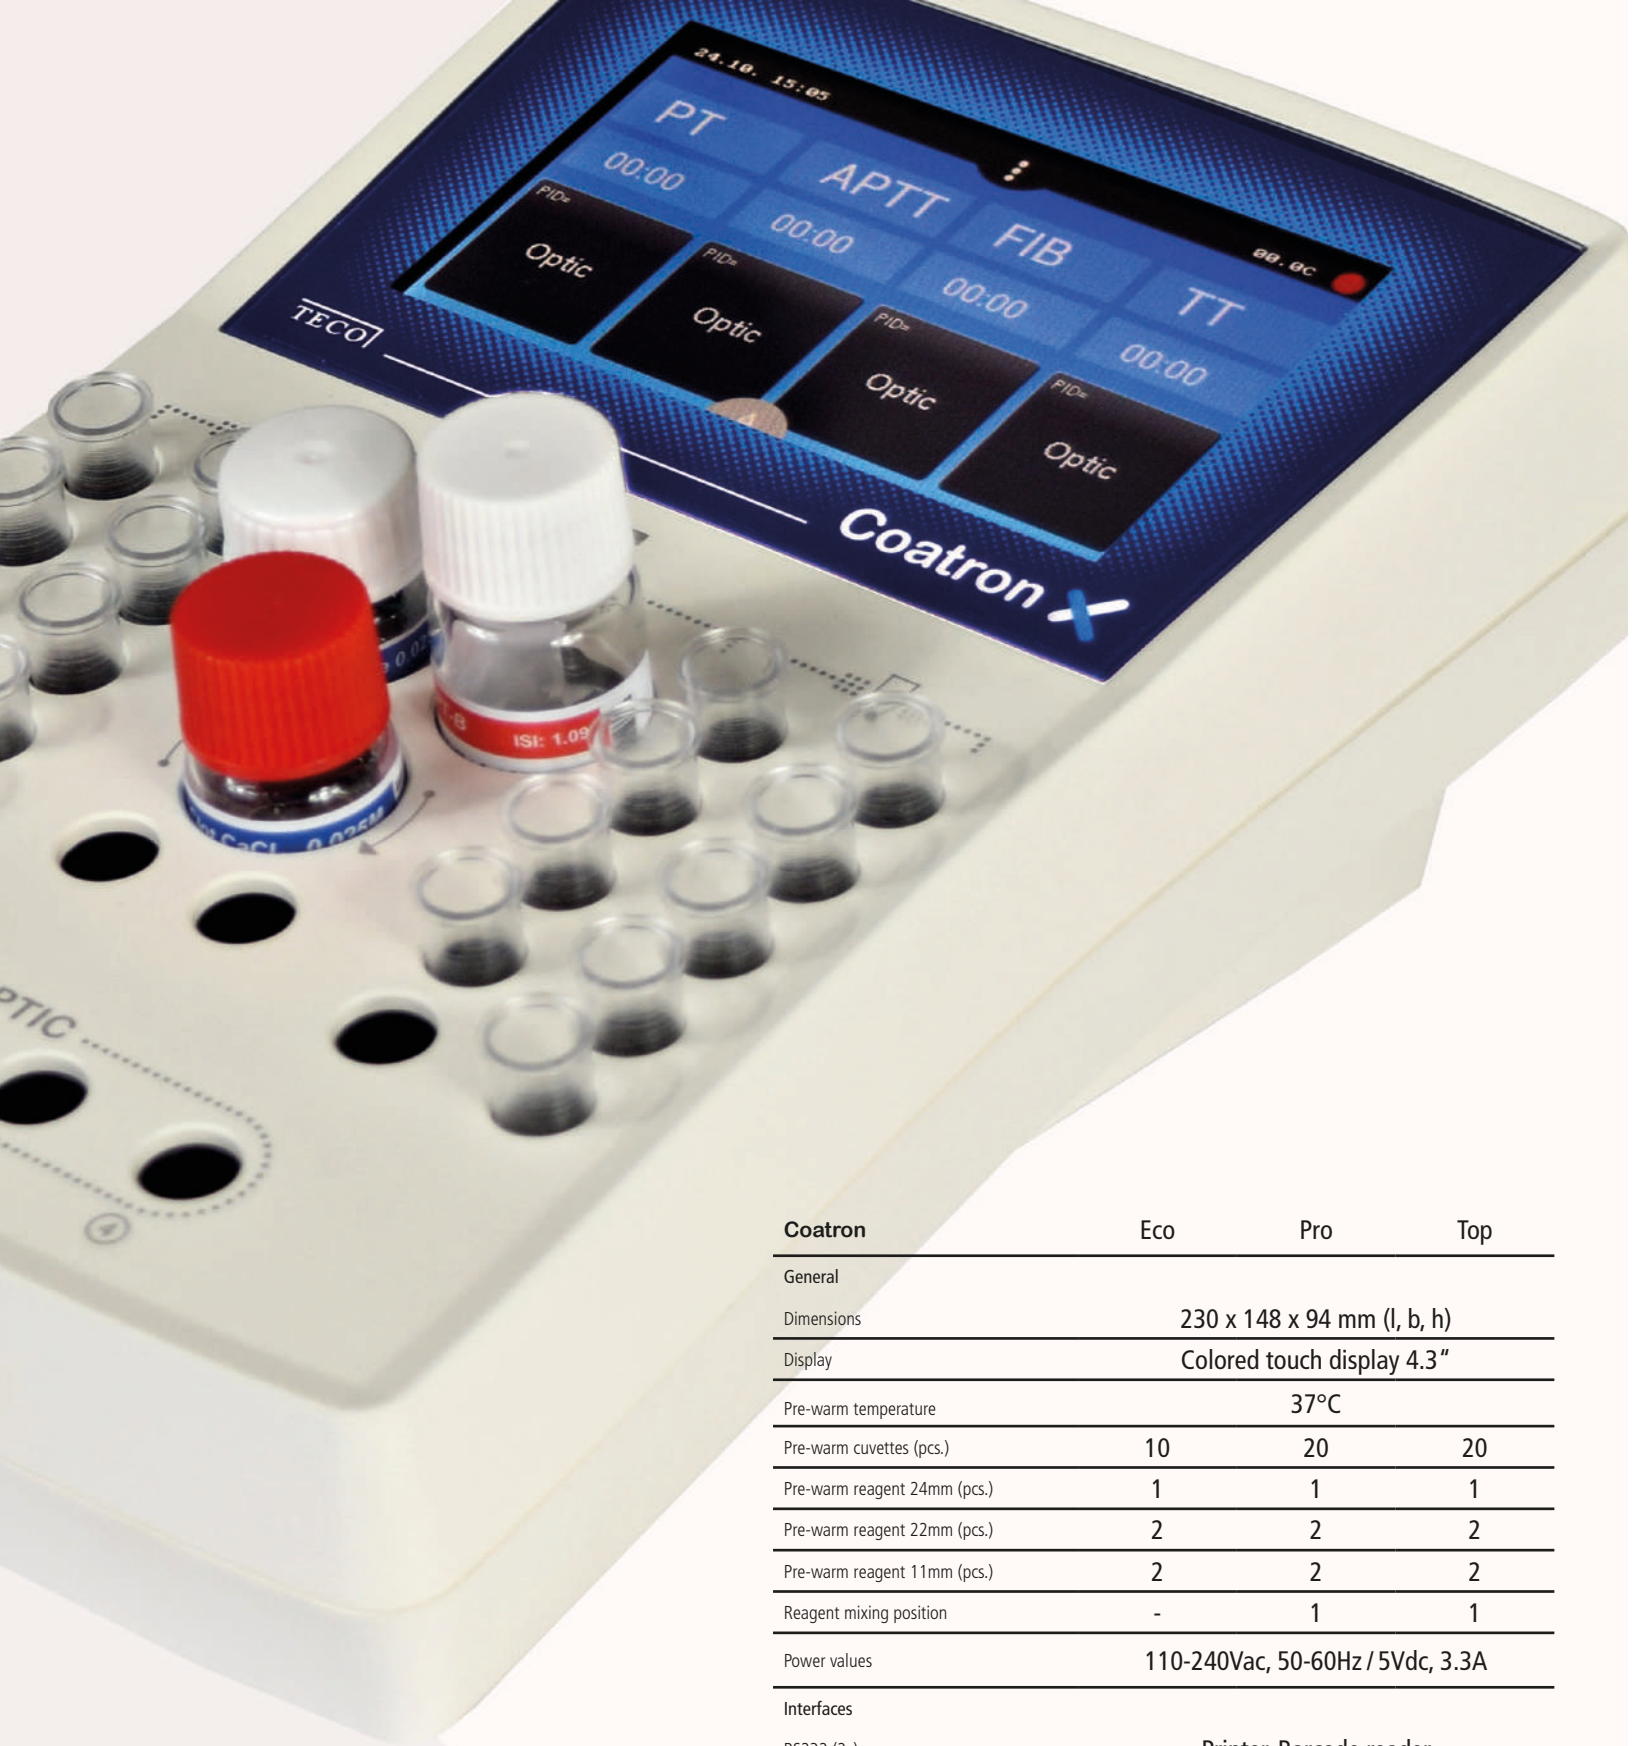

Coatron	Eco	Pro	Top
General			
Dimensions	230 x 148 x 94 mm (l, b, h)		
Display	Colored touch display 4.3"		
Pre-warm temperature	37°C		
Pre-warm cuvettes (pcs.)	10	20	20
Pre-warm reagent 24mm (pcs.)	1	1	1
Pre-warm reagent 22mm (pcs.)	2	2	2
Pre-warm reagent 11mm (pcs.)	2	2	2
Reagent mixing position	-	1	1
Power values	110-240Vac, 50-60Hz / 5Vdc, 3.3A		
Interfaces			
RS232 (2x)	Printer, Barcode reader		
USB (2x)	Network, Firmware update		
Bluetooth	TECO Cloud, App		
Optic / tests			
Optic channels	1	2	4
Wavelength (nm)	620 (red)	405 (UV)	405 (UV)
Global Coag. tests	PT, APTT, TT, FIB		
Specific Coag. tests	-	individual factors	
Chromogenic Coag. tests	-	AT, PC	
Latex based tests	D-Dimer		
Whole blood tests	PT-B	-	



## The details make the difference

### Coatron X


The remarkable details in every single component is achieved by selecting of premium suppliers.

The performance of a high level instrument is strongly depending on the concept in general and the perfect usability to reach the requirements of a modern laboratory analyser.

Priority No. 1 was to get a daily routine reliability and easy-to-use operation.

### Software and connection possibilities

With the Coatron X product family starts a new time line in analysis management and service maintenance. Operation via intuitive, colored touchscreen, as well patient result management are perfectly optimized.

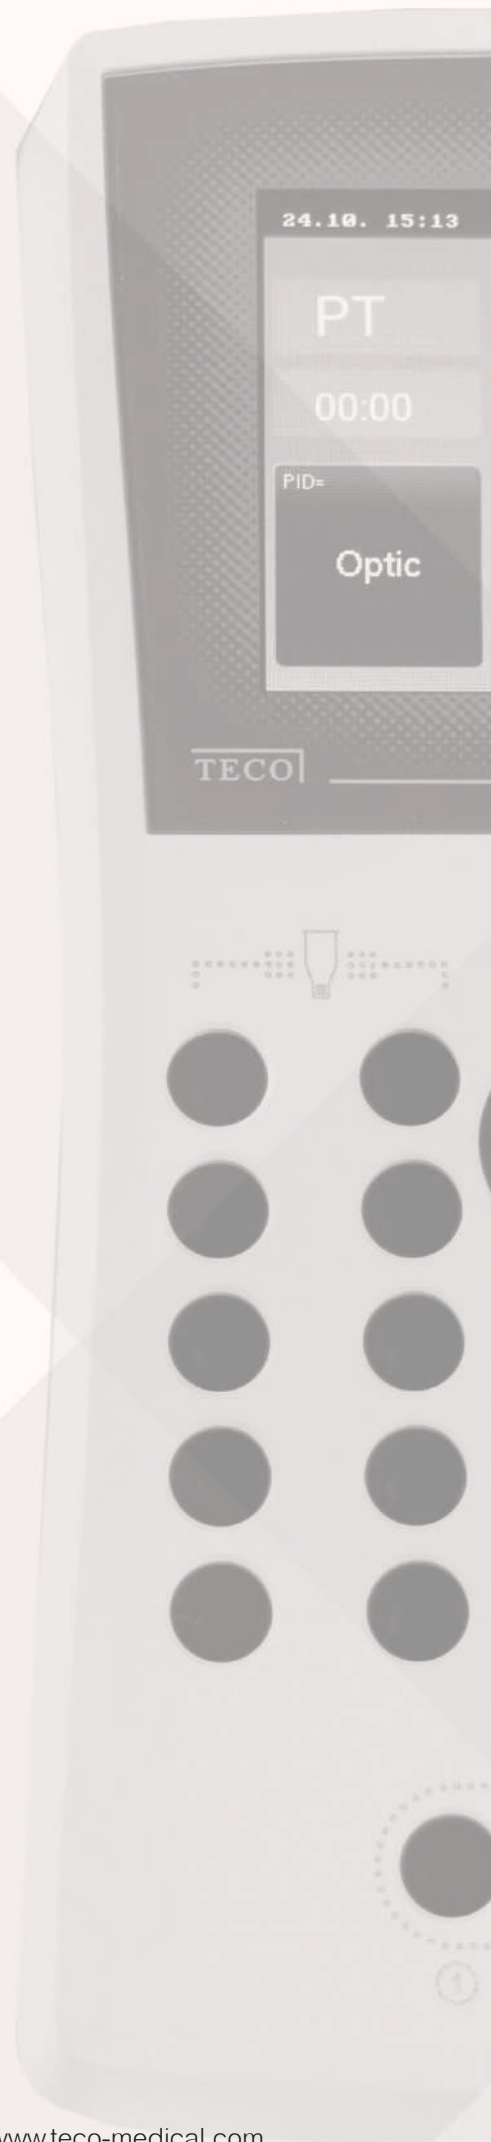

## Operation details

Coatron	Eco	Pro	Top
<b>Operation</b>			
Touchscreen 4.3"	✓	✓	✓
Real time clock	✓	✓	✓
Stopwatch	✓	✓	✓
Language selection	✓	✓	✓
<b>Interfaces</b>			
USB to LIS	✓	✓	✓
Network to LIS (TECAM software required)	✓	✓	✓
<b>Management</b>			
Test calibration	✓	✓	✓
Tracking to Pat.ID, Patient ID, Sample ID or Auto ID	✓	✓	✓
Automatic optic start (no Starterpipette required)	✓	✓	✓
Double determination	✗	✓	✓
Sample management (ID)	✗	✓	✓
Reagent management (ID) (lot und expiry)	✗	✓	✓
Internal result databank	✗	✓	✓
Patient identification with barcode		optional	



### Intuitive operation and control

Clear and easy to operate user dialogue with a high quality colored touchscreen

- Direct usable
- Short learning phase
- Logic, intuitive operation
- Reliable touchscreen surface
- Quick touch response



### For small and mediate laboratory requirements

Concept is suitable for daily routine work in Coagulation laboratories and hospitals

- Three different versions available, depending on number of samples per day
- In maximum up to 4 optic channels available

### Interfaces

#### RS232 (2x)

- For external serial printer and external barcodereader

#### LIS/USB

#### Bluetooth



Integrated barcode scan for reagents.







### **TECO Cloud Services**

#### **A strong data bank and application service behind**

All instrument versions of the Coatron X family are connectable via Bluetooth to Smart-devices, like mobile devices, tablets, etc. with a specific APP or direct access to the TECO Cloud Services.



For trading partners worldwide, please visit our web-page

**TECO Medical Instruments Production + Trading GmbH**  
Dieselstr. 1, 84088 Neufahrn, Germany  
Tel.: +49 (0) 8773 70780-0, Fax +49 (0) 8773 70780-29  
info@teco-gmbh.com, www.teco-medical.com

**TECO**  
Innovation in Coagulation



MEDICAL INSTRUMENTS  
PRODUCTION + TRADING GMBH  
Internet: www.teco-gmbh.com  
Email: info@teco-gmbh.com

DIESELSTRASSE 1  
D-84088 NEUFABRN NB.  
Tel: #49-8773-70780-0  
Fax: #49-8773-70780-29

## Certificate of Analysis TECLOT PT-S

( expected values for analysers of TECO Coatron series )

**REF** A0230-100

**LOT** 10233730

 Aug.2027

STD (%)	Coatron M4 C1.13d	Coatron A V1.07.05a	Coatron X 1.03.51	KC-4 Micro
100,0 %	13,5 s	12,3 s	12,7 s	13,7 s
50,0 %	19,3 s	17,4 s	17,6 s	19,6 s
25,0 %	30,1 s	27,4 s	25,9 s	31,8 s
12,5 %	57,2 s	53,3 s	53,2 s	59,0 s

<b>ISI value</b>	1,04			
<b>Normal time</b>	13,5 s	12,3 s	12,7 s	13,7 s

<b>Control Range</b>	see certificate of control			
----------------------	----------------------------	--	--	--

**En:** These values were determined by the laboratory of **TECO GmbH** according to standard operation procedure QMV-07-26. However, Lot-to-Lot variation of reagents, IBS buffer and other diluents, calibrators, controls as well as instruments or pipetting technique etc., may cause lab-to-lab different results. Therefore these assigned values must be seen as typical values. Each laboratory must establish its own calibration curve and follow local requirements and regulations for quality control.

**De:** Diese Werte wurden durch das Labor von **TECO GmbH** gemäß der Verfahrensanweisung QMV-07-26 ermittelt. Jedoch kann es je nach Charge der Reagenzien, IBS Puffer oder anderer Verdünnungslösungen, Kalibratoren, Kontrollen oder je nach Gerät, Pipettieretechnik usw. vorkommen dass die Werte von Labor zu Labor unterschiedlich ausfallen. Deshalb sind die angeführten Ergebnisse nur als Richtwerte zu bewerten. Jedes Labor muss die Eichkurve selbst bestimmen und die örtlichen Anforderungen für Qualitätskontrollen anwenden.

Table for conversion of the prothrombintime (PT) into % Quick resp. Int. Norm Ratio (INR)  
 Tabelle zur Umwandlung von Thromboplastinzeit (TPZ) in % Quick bzw. Int. Norm Ratio (INR)

KC4 micro			ISI = 1,04			Normal= 13,7s		
PT (s)	% Quick	INR	PT (s)	% Quick	INR	PT (s)	% Quick	INR
11,5	131,0	0,84	17,7	62,1	1,30	41,7	18,5	3,05
11,6	129,3	0,85	18,2	58,6	1,33	43,0	17,9	3,15
11,7	127,6	0,86	18,7	55,3	1,37	44,2	17,4	3,24
11,8	126,0	0,86	19,2	52,1	1,41	45,6	16,8	3,34
11,9	124,4	0,87	19,7	49,5	1,44	46,9	16,2	3,44
12,0	122,8	0,88	20,2	47,9	1,48	48,3	15,7	3,54
12,1	121,2	0,89	20,7	46,4	1,52	49,8	15,2	3,65
12,2	119,7	0,89	21,2	44,9	1,55	51,3	14,7	3,76
12,3	118,2	0,90	21,7	43,6	1,59	52,8	14,2	3,87
12,4	116,7	0,91	22,2	42,2	1,63	54,4	13,7	3,99
12,5	115,2	0,92	22,7	41,0	1,66	56,0	13,3	4,11
12,6	113,8	0,92	23,2	39,8	1,70	57,7	12,8	4,23
12,7	112,4	0,93	23,7	38,6	1,74	59,5	12,4	4,36
12,8	111,0	0,94	24,2	37,5	1,77	61,2	12,0	4,49
12,9	109,6	0,95	24,7	36,4	1,81	63,1	11,6	4,62
13,0	108,3	0,95	25,2	35,4	1,85	65,0	11,2	4,76
13,1	107,0	0,96	25,7	34,4	1,88	66,9	10,8	4,90
13,2	105,6	0,97	26,2	33,5	1,92	68,9	10,4	5,05
13,3	104,4	0,97	26,7	32,6	1,96	71,0	10,0	5,20
13,4	103,1	0,98	27,2	31,7	1,99	73,1	9,7	5,36
13,5	101,8	0,99	27,7	30,9	2,03	75,3	9,3	5,52
13,6	100,6	1,00	28,2	30,0	2,07	77,6	9,0	5,68
13,7	99,4	1,00	28,7	29,3	2,10	79,9	8,7	5,85
13,8	98,2	1,01	29,2	28,5	2,14	82,3	8,4	6,03
13,9	97,0	1,02	29,7	27,8	2,18	84,8	8,1	6,21
14,0	95,9	1,03	30,2	27,1	2,21	87,3	7,8	6,40
14,1	94,7	1,03	30,7	26,4	2,25	89,9	7,5	6,59
14,2	93,6	1,04	31,2	25,7	2,29	92,6	7,2	6,79
14,3	92,5	1,05	31,7	25,1	2,32	95,4	6,9	6,99
14,4	91,4	1,05	32,2	24,6	2,36	98,3	6,7	7,20
14,5	90,3	1,06	32,7	24,2	2,40	101,2	6,4	7,42
14,6	89,2	1,07	33,2	23,8	2,43	104,3	6,2	7,64
14,7	88,2	1,08	33,7	23,4	2,47	107,4	5,9	7,87
14,8	87,1	1,08	34,2	23,1	2,51	110,6	5,7	8,10
14,9	86,1	1,09	34,7	22,7	2,54	113,9	5,5	8,35
15,0	85,1	1,10	35,2	22,3	2,58	117,3	5,3	8,60
15,2	83,1	1,11	35,7	22,0	2,62	120,9	5,0	8,85
15,4	81,2	1,13	36,2	21,7	2,65	124,5	4,8	9,12
15,6	79,3	1,14	36,7	21,3	2,69	128,2	4,6	9,39
15,8	77,5	1,16	37,2	21,0	2,73	132,1	4,4	9,68
16,0	75,7	1,17	37,7	20,7	2,76	136,0	4,3	9,97
16,2	73,9	1,19	38,2	20,4	2,80	140,1	4,1	10,26
16,4	72,2	1,20	38,7	20,1	2,84	144,3	3,9	10,57
16,6	70,6	1,22	39,2	19,9	2,87	148,6	3,7	10,89
16,8	68,9	1,23	39,7	19,6	2,91	153,1	3,5	11,22
17,0	67,4	1,25	40,2	19,3	2,95	157,7	3,4	11,55
17,2	65,8	1,26	40,7	19,0	2,98	162,4	3,2	11,90




MEDICAL INSTRUMENTS  
PRODUCTION + TRADING GMBH  
Internet: www.teco-gmbh.com  
Email: info@teco-gmbh.com

DIESELSTRASSE 1  
D-84088 NEUFAHRN NB.  
Tel: #49-8773-70780-0  
Fax: #49-8773-70780-29

**Certificate of Analysis**  
**TEClot FIB**

**REF** A0511-020

**LOT** 10513715

 Jul. 2026

STD	mg/dL	Coatron M4	Coatron A4	Coatron X
1:5	574	7,7 s	7,7 s	9,0 s
1:10	287	16,3 s	12,2 s	14,1 s
1:20	144	29,7 s	21,1 s	26,2 s
1:30	96	42,4 s	28,5 s	34,9 s

(diluted with TEClot IBS LOT-10593315)

<b>Control Range</b>	see certificate of control
----------------------	----------------------------

**En:** These values were determined by the laboratory of **TECO GmbH** according to standard operation procedure QMV-07-26. However, Lot-to-Lot variation of reagents, IBS buffer and other diluents, calibrators, controls as well as instruments or pipetting technique etc., may cause lab-to-lab different results. Therefore these assigned values must be seen as typical values. Each laboratory must establish its own calibration curve and follow local requirements and regulations for quality control.

**De:** Diese Werte wurden durch das Labor von **TECO GmbH** gemäß der Verfahrensanweisung QMV-07-26 ermittelt. Jedoch kann es je nach Charge der Reagenzien, IBS Puffer oder anderer Verdünnungslösungen, Kalibratoren, Kontrollen oder je nach Gerät, Pipettiertechnik usw. vorkommen, dass die Werte von Labor zu Labor unterschiedlich ausfallen. Deshalb sind die angeführten Ergebnisse nur als Richtwerte zu bewerten. Jedes Labor muss die Eichkurve selbst bestimmen und die örtlichen Anforderungen für Qualitätskontrollen anwenden.



MEDICAL INSTRUMENTS  
PRODUCTION + TRADING GMBH  
Internet: www.teco-gmbh.com  
Email: info@teco-gmbh.com

DIESELSTRASSE 1  
D-84088 NEUFAHRN NB.  
Tel: #49-8773-70780-0  
Fax: #49-8773-70780-29

**Certificate of Analysis**  
**IBS Buffer**

**REF**

A0590-125

**LOT**

10593672



May.2026

Quality Control Specifications	Specification	Result
Appearance	Clear colorless solution free of particulates	Pass
pH	7,2 - 7,6	7,2



**Certificate of Analysis  
TEControl N**

REF P6001-010

LOT 96003697

⌚ Sep.2026

Prothrombin Time (PT)					
Reagent	Method	Unit	Target	Range	
TEClot PT-S	Coatron M	sec	14,2	11,6	- 16,7
		%	99	81	- 117
		INR	1,01	0,83	- 1,19
	Coatron A	sec	13,0	10,7	- 15,3
		%	104	85	- 122
		INR	0,98	0,80	- 1,15
	Coatron X	sec	13,0	10,7	- 15,3
		%	102	84	- 121
		INR	0,99	0,81	- 1,17
	KC4 micro	sec	14,2	11,6	- 16,8
		%	100	82	- 118
		INR	1,00	0,82	- 1,18
TEClot PT-B	Coatron X Eco + Dimex Jr.	sec	22,5	18,5	- 26,6
		%	104	85	- 123
		INR	0,97	0,80	- 1,15

Activated Partial Thromboplastin Time (aPTT)					
TEClot APTT-S	Coatron M	sec	33,0	27,0	- 38,9
	Coatron A	sec	31,6	25,9	- 37,2
	Coatron X	sec	31,2	25,5	- 36,8
	KC4 micro	sec	31,2	25,6	- 36,8

Fibrinogen (method Clauss, diluted 1:10)					
TEClot FIB	Coatron M	mg/dL	293	228	- 357
	Coatron X	mg/dL	272	212	- 332
	Coatron A	mg/dL	293	228	- 357

Thrombin Time (TT)					
TEClot TT	Coatron M + X	sec	19,4	16	- 23
	Coatron A	sec	20,5	17	- 24

Antithrombin					
Techrom AT	chromogen	%	106	83	- 129

D-Dimer (DD)					
Blue D-Dimer LC	latex immuno DDU	ng/mL	312	234	- 390
	latex immuno FEU	ng/mL	780	639	- 920
RED D-Dimer	latex immuno DDU	ng/mL	420	315	- 525
	latex immuno FEU	ng/mL	1051	788	- 1313

These values were determined by the laboratory of **TECO GmbH** according to standard operation procedure QMV-07-26. However, Lot-to-Lot variation of reagents, IBS buffer and other diluents, calibrators, controls as well as instruments or pipetting technique etc., may cause lab-to-lab different results. Therefore these assigned values must be seen as typical values. Each laboratory must establish its own calibration curve and follow local requirements and regulations for quality control.



**Certificate of Analysis**  
**TEControl A**

REF P6101-010

LOT 96103558

 Sep.2025

Prothrombin Time (PT)					
Reagent	Method	Unit	Target	Range	
TEClot PT-S	Coatron M	sec	31,2	24,6	- 37,8
		%	26	20	- 31
		INR	2,19	1,73	- 2,65
	Coatron A	sec	31,1	24,5	- 37,6
		%	26	21	- 32
		INR	2,33	1,84	- 2,82
	Coatron X	sec	28,2	22,3	- 34,1
		%	25	20	- 30
		INR	2,14	1,69	- 2,59
	KC4 micro	sec	29,0	22,9	- 35,1
		%	29	23	- 35
		INR	1,98	1,57	- 2,40
TEClot PT-B	Coatron X Eco + Dimex Jr.	sec	58,1	45,9	- 70,3
		%	29	23	- 35
		INR	2,62	2,07	- 3,17

Activated Partial Thromboplastin Time (aPTT)					
TEClot APTT-S	Coatron M	sec	62,5	49,4	- 75,6
	Coatron A	sec	63,5	50,1	- 76,8
	Coatron X	sec	56,3	44,5	- 68,1
	KC4 micro	sec	64,8	51,2	- 78,3

Fibrinogen (method Clauss, diluted 1:10)					
TEClot FIB	Coatron M	mg/dL	155	117	- 194
	Coatron X	mg/dL	139	105	- 174
	Coatron A	mg/dL	124	93	- 155

Thrombin Time (TT)					
TEClot TT	Coatron M + X	sec	n.a.	-	
	Coatron A	sec	n.a.	-	

Antithrombin					
Techrom AT	chromogen	%	52	39	- 65

D-Dimer (DD)					
Blue D-Dimer LC	latex immuno DDU	ng/mL	966	628	- 1305
	latex immuno FEU	ng/mL	2416	1909	- 2924
RED D-Dimer	latex immuno DDU	ng/mL	1005	653	- 1357
	latex immuno FEU	ng/mL	2513	1633	- 3392

Individual laboratory results must fall always within the corresponding ranges. Otherwise calibration data and material should be verified. Local regulation may require sharper control ranges ( e.g. Rilibaek ). However variations in analyzer, reagents (Lot to Lot), technique etc., may cause deviation from assigned target value. In this case the laboratory must establish its own target value according to local quality regulations.

# 24 100 00 Single Cuvettes - 500

# 24 200 00 Single Cuvettes - 5000



### Information of use

The Cuvette as general laboratory article is suitable to hold a reaction mixture for use in optical analyzers which are used in laboratories for in vitro diagnostic tests.

The cuvettes are ready for immediate use. They have unlimited shelf life if stored at 0 - 50°C.

### Content

Product	Single Cuvettes	Single Cuvettes
Cat.No.	24 100 00	24 200 00
Content	500 pcs (500 det.)	5000 pcs (5000 det.)

The Cuvettes can be used with Coatron X Analyzers.

For application with semi-automated Coagulation System Coatron X, each box contains a voucher label with a VIN and PIN code to generate a ticket on the web-based registration page ([www.teco-reg.com](http://www.teco-reg.com)).

The ticket information (VIN/PIN) must be entered for the respective device to release the number of tests for this device only. The (VIN/PIN) can only be used once per unit.

### Precautions and waste information

The Cuvette should only be used once in analyzers. To prevent contamination (sample/reagent), it is advised to avoid contact with skin and eyes. Suitable protective clothing and gloves are recommended.

Please also note the disposal of components in accordance with local regulations for infectious material.



Material: pure, clear Polystyrol (PS)  
 Maximum volume should be less than ~ 500µL  
 Minimum volume: 75 µL  
 Dimensions max.: Ø11,5 mm x 24 mm


### 24 100 00

Example Picture of the package – 500 Single Cuvettes



Packaging:

1. Log Bag, Dim.: (mm) 165 x 295 x 0,05, Mat.: LDPE;
2. Card Box, Dim.: (mm) 252 x 104 x 65
3. Paper Sleeve with Identification and Information

<b>Voucher</b>	Single Cuvettes
<b>VIN:</b> 71101 XXXXX	 500
<b>PIN:</b> 19823 78881	

Example of Voucher – 500 Single Cuvettes/Pack


### 24 200 00

Example Picture of the package – 5000 Single Cuvettes



Packaging:

1. Log Bag, Dim.: (mm) 600 x 400 x 0,05, Mat.: LDPE;
2. Card Box, Dim.: (mm) 400 x 250 x 150
3. Label with Identification and Information

<b>Voucher</b>	Single Cuvettes
<b>VIN:</b> 71200 XXXXX	 5000
<b>PIN:</b> 19823 78881	

Example of Voucher – 5000 Single Cuvettes/Pack



# 24 100 00 Single Cuvettes - 500

# 24 200 00 Single Cuvettes - 5000

# TECO

### Gebrauchsinformation

Die Küvette als allgemeiner Laborartikel eignet sich zur Aufnahme eines Reaktionsgemisches zur Verwendung in optischen Analysegeräten, welche in Laboren für in-vitro-diagnostische Tests verwendet werden.

Die Küvetten sind sofort einsatzbereit. Sie sind unbegrenzt haltbar, wenn sie bei 0 - 50°C gelagert werden.

### Inhalt

Produkt	Einzelküvette	Einzelküvette
Kat. Nr.	24 100 00	24 200 00
Inhalt (Stck.)	500 (500 Tests)	5000 (5000 Tests)

Die Küvetten können mit dem halb-automatischen Coagulations System Coatron X verwendet werden.

Dazu enthält jede Packung ein Voucher-Etikett mit einem VIN- und PIN-Code, um ein Ticket auf der webbasierten Registrierungsseite zu generieren ([www.teco-reg.com](http://www.teco-reg.com)).

Die Ticketinformationen (VIN/PIN) müssen für das jeweilige Gerät eingegeben werden, um die Anzahl der Tests für dieses Gerät freizugeben. Die (VIN/PIN) kann nur einmal pro Einheit verwendet werden.

### Vorsichtsmaßnahmen und Entsorgungshinweise

Die Küvette sollte nur einmal im Analysegerät verwendet werden. Um eine Kontamination (Probe/Reagenz) zu vermeiden, ist es ratsam, den Kontakt mit Haut und Augen zu vermeiden. Es werden geeignete Schutzkleidung und Handschuhe empfohlen.

Bitte beachten Sie auch die Entsorgung der Komponenten in Übereinstimmung mit den örtlichen Vorschriften für infektiöses Material.



Material: klares Polystyrol (PS)  
 maximales Volumen: nicht über ~ 500µL  
 minimales Volumen: : 75 µL  
 max. Abmessungen: Ø11,5 mm x 24 mm


### 24 100 00

Beispielbild – Packung mit 500 Einzelküvetten



Verpackung:

1. Beutel, Maße: (mm) 165 x 295 x 0,05, Mat.: LDPE;
2. Karton, Maße: (mm) 252 x 104 x 65
3. Papierhülle mit Beschreibung und Informationen

<b>Voucher</b>	Single Cuvettes
<b>VIN:</b> 71101 XXXXX	 500
<b>PIN:</b> 19823 78881	

Beispiel des Voucher – 500 Einzelküvetten/Pack


### 24 200 00

Beispielbild – Packung mit 5000 Einzelküvetten



Verpackung:

1. Beutel, Maße: (mm) 600 x 400 x 0,05, Mat.: LDPE;
2. Karton, Maße: (mm) 400 x 250 x 150
3. Label mit Artikelbeschreibung und Informationen

<b>Voucher</b>	Single Cuvettes
<b>VIN:</b> 71200 XXXXX	 5000
<b>PIN:</b> 19823 78881	

Beispiel des Voucher – 5000 Einzelküvetten/Pack



IVD

REF

A0230-010, A0230-040, A0230-100,

**Intended Use**

This product is used for the determination of prothrombin time (PT) in plasma according to Quick<sup>1,2</sup>. The test is sensitive to the extrinsic pathway coagulation factors II, V, VII, X and fibrinogen and therefore used for oral anticoagulant therapy with Vitamin-K inhibitors like Warfarin or Marcumar and also for the quantitative determination of extrinsic coagulation factors. The PT measures the extrinsic clotting time (factor VII activation) of test plasma after the addition PT reagent.

**Contents & Determinations**

Product	TECLOT PT-S	TECLOT PT-S	TECLOT PT-S
Cat.No.	A0230-010	A0230-040	A0230-100
PT-S Reagent*	5x2 mL	10x4 mL	10x10 mL

**Determinations**

Coatron M**	200 Det.	800 Det.	2000 Det.
Coatron A4	100 Det.	400 Det.	1000 Det.
Coatron A6	200 Det.	800 Det.	2000 Det.

\*contains an extract of Rabbit brain with buffer, stabilizers and Calcium chloride.

\*\*Micro method (75µL in total)

**Preparation**

Reconstitute with high purity water with the volume stated on the vial label.

A0230-010	A0230-040	A0230-100
2 mL	4 mL	10 mL

Let stand at room temperature with occasional swirling for at least 15 min. Then place reagent into instrument and let incubate for further 15 min. The reagent sediments and must be swirled before each testing. On Coatron instruments, you can use a mixing bar for this.

**Storage & Stability**

Unopened reagents are stable until the expiration date shown on the label stored at 2°-8°C. Opened reagent:

	2-8 °C	20-25 °C	37°C
PT Reagent	5 days	36 hours	8 hours

**Precautions**

Avoid contact with skin and eyes. Wear suitable protective clothing. Dispose components in compliance with local regulations for infectious material. All components are checked for HIV, HBV, HCV. However products from human blood should be considered as potentially infectious.

**Specimen collection and storage<sup>4</sup>**

- Obtain venous blood by clean vein puncture.
- Immediately mix 9 parts blood with 1 part 3.2% sodium citrate (0.105M) and mix well
- Centrifuge the specimen at 1500g for 10 min. (platelet < 10000/µL)
- Separate plasma after centrifugation and store in plastic or siliconised glass tube.
- Use plasma within 4 hours, otherwise store frozen and thaw just prior to use.

Stability of plasma: 4h at 18-26°C 8h at 2-8° 30d at -20°C 6m at -70°C

**Procedure****A. Automated Method: Coatron A**

Prothrombin Time		A4		A6				A4		A6	
PAT	Patient	50µl	CP1	25µl	CP1	Incubation	0s	SENS	2		
BUF	IBS Buffer	0µl	P39	0µl	P79	Maxtime	120s	POINTS	4		
CLR	-	0µl	-	0µl	-	Unit	251	MIX	No		
DP	-	0µl	P00	0µl	P00	Method	Coag	Clean	0	0	
R0	-	0µl	P00	0µl	P00	Math	log XY	Multi	1	3	
R1	-	0µl	P00	0µl	P00	CT-Mech	No	S-Corr	0%		
R2	PT Reagent	100µl	P25	50µl	P46	Deadtime	7s	T-Corr	30% - 4s		

**B. Manual Method: Coatron M system**

- Incubate PT reagent at 37°C for at least 10 minutes
- Pipette 25 µl of sample into a test cuvette. Incubate at 37°C for 1-2 minutes.
- Add 50 µl of PT reagent (37°C) and simultaneously start test.
- Record the clotting time in seconds.

For other instrument, please refer to your instrument manual for more detailed instrument specific instructions.

**Symbol keys**

	Expiry date		In Vitro Diagnostica		Biological hazard		Catalogue Number		Reconstitute with dest. water		Consult accompanying documents
	Store at 2-8°C		EU conformity		Manufacturer		Lot. Number		Ready to use		Authorized Representative

**Expected Results**

Typical seconds: 11 – 18 sec  
Normal range: 70 - 130% 0.85 – 1.15 INR

However results are influenced by instruments, technique, calibration etc. Each laboratory is recommended to establish its own range on the specific instrument used.

**Standardisation and Calibration**

The PT result is expressed as seconds or activity (% Quick) or INR (International Normalised Ratio).

**INR results:**

were calculated from normal time and ISI value (international sensitivity index). First is obtained by running fresh plasma from a pool of healthy individuals. The ISI value is stated in the LOT specific certificate of analysis.

$$INR = \left( \frac{Patient\ PT}{Normal\ PT} \right)^{ISI}$$

**Activity % (Quick) result:**

were calculated from a calibration curve, which is prepared from reference plasma (e.g. TECAL N) and dilutions in saline solution like 0.9% NaCl<sub>2</sub> or TECLOT IBS buffer. At least three or more calibration points are recommended. The calibration curve must be confirmed with control plasma in normal and abnormal range.

% of normal	100%*	50%	25%	12.5%**
diluted in saline	not dil.	1+1	1+3	1+7

\*The median of at least 21 healthy individuals is defined as 100%.<sup>5</sup>

\*\*12.5% dilution may cause "++++" results in some cases, because the level of fibrinogen is too high diluted for optical detection.

**Quality Control**

TEControl or other commercial control plasma should be used for reliable quality control of performance at a frequency in accordance with good laboratory practice (GLP). TEControl can be frozen one time after reconstitution. 120-150 µl stored in closed polypropylen tubes at -20°C is stable for 30 days

**Limitations**

Great care must be taken to minimize variations which may occur by seemingly insignificant factors.

**A. Specimen Collection. AVOID:**

- Use only plastic tubes or siliconised glass.
- Delayed mixing of blood with anticoagulant.
- Contamination with tissue thromboplastin.
- Improper ratio of anticoagulant with blood.
- Hemolyzed, icteric or lipemic samples may interfere optical systems

**B. Laboratory Techniques**

- Perform tests at 37°C.
- Use only high purity water.
- Optimum pH is 7.0-7.5.
- ISI value is not constant within the first 30 min after reconstitution.
- Reagent sediments and must be swirled before each testing.

**Performance Characteristics****Typical performance on instrument Coatron M4**

**Precision:** CV% (within run) CV% (inter-runs)  
Normal control < 3.0 < 5.0  
Abnormal control < 3.0 < 5.0

**Warranty**

This product is warranted to perform in accordance with its labelling and literature. TECO disclaims any implied warranty of merchantability or fitness for any other purpose, and in no event will TECO be liable for any consequential damages arising out of aforesaid express warranty.

**References**

- Quick, A.J., The Hemorrhagic Diseases and the Physiology of Hemostasis. Charles C. Thomas: Springfield, IL. 1942.
- Quick, A.J., Hemorrhagic Diseases. Lea and Febiger: Philadelphia. 1957.
- Miale, J.B., Laboratory Medicine-Hematology, 4th Edition. C.V. Mosby: St. Louis. 1972.
- National Committee for Clinical Laboratory Standards: Guidelines for the Standardized Collection, Transport and Preparation of Blood Specimens for Coagulation Testing and Performance of Coagulation Assays.
- Besselaar A M H P van den, Lewis SM, Mannucci P n Poller L. 1993. Status of present and candidate International Reference Preparations (IRP) of thromboplastin for prothrombin time. Thromb Hemostas 69; 85
- Besselaar A M H P van den. 1991. The significance of the International Normalized Ratio (INR) for oral anticoagulant therapy. H17CC 3; 146153.



IVD

REF

A0501-010, A0501-025, A0511-020, A0511-050

**Intended Use**

The TEClot FIB is intended for the quantitative determination of fibrinogen in human plasma according to method developed by Clauss.<sup>1</sup> Levels of fibrinogen can increase as a result of inflammation, pregnancy or oral contraceptive use<sup>2</sup>. Decreased levels can be found in certain states such as liver disease and DIC. Congenital deficiencies include afibrinogenemia (no detectable fibrinogen), hypofibrinogenemia (<1 mg/ml) and dysfibrinogenemia (abnormal fibrinogen molecule).

**Contents & Preparation**

Product	TEClot FIB Kit-10	TEClot FIB Kit-25	TEClot FIB	TEClot FIB
Cat.No.	A0501-010	A0501-025	A0511-020	A0511-050
Thrombin Reagent	5x2 mL	5x5 mL	10x2 mL	10x5 mL
IBS Buffer	1x125 mL	1x125 mL	-	-
TECal Normal	1x1 mL	1x1 mL	-	-
TEControl A	1x1 mL	1x1 mL	-	-

**Determinations**

Coatron M*	400 Det.	1000 Det.	800 Det.	2000 Det.
Coatron A4	200 Det.	500 Det.	400 Det.	1000 Det.
Coatron A6	200 Det.	500 Det.	400 Det.	1000 Det.

\*Micro method (75µl in total)

- Thrombin Reagent:  
Contains bovine thrombin (~80NIH) with stabilizers  
REF: A0501-010/A0511-020: Reconstitute with 2mL purified water  
REF: A0501-025/A0511-050: Reconstitute with 5mL purified water
- IBS Buffer: Ready to use. Contains Imdazole buffered saline
- TECal Normal: Reconstitute with 1 mL purified water.  
Contains citrated human plasma.
- TEControl A: Reconstitute with 1 mL purified water.  
Contains citrated human plasma.



Swirl gently after reconstitution and allow standing for 15 minutes at room temperature. Mix well before use. Do not shake.

**Storage & Stability**

Unopened reagents are stable until the expiration date shown on the label stored at 2°-8°C. Opened reagent:

Thrombin Reagent*	2-8 °C	15-25 °C	37 °C
	12 days	5 days	24 hours
TEControl or Plasma	2-8 °C	15-25 °C	-20 °C
	8 hours	4 hours	30 days

\* Reagent must be protected from UV-light and evaporation

**Precautions**

Avoid contact with skin and eyes. Wear suitable protective clothing. Dispose components in compliance with local regulations for infectious material. All components are checked for HIV, HBV, HCV. However products from human blood should be considered as potentially infectious.

**Specimen collection and storage<sup>3</sup>**

- Obtain venous blood by clean vein puncture.
- Immediately mix 9 parts blood with 1 part 3.2% sodium citrate (0.105M) and mix well
- Centrifuge the specimen at 1500g for 10 min. (platelet < 10000/µL)
- Separate plasma after centrifugation and store in plastic or siliconised glass tube.
- Use plasma within 4 hours, otherwise store frozen and thaw just prior to use.

**Procedure****A. Automated Method. Coatron A**

Fibrinogen		A4		A6				A4		A6	
PAT	Patient	10µl	CP1	10µl	CP1	Incubation	0s	SENS	0		
BUF	IBS Buffer	90µl	P39	90µl	P79	Maxtime	120s	POINTS	4		
CLR	-	0µl	-	0µl	-	Unit	769	MIX	No		
DP	-	0µl	P00	0µl	P00	Method	Coag	Clean	1	3	
RO	-	0µl	P00	0µl	P00	Math	log XY	Multi	1	1	
R1	-	0µl	P00	0µl	P00	CT-Mech	Yes	S-Corr	0%		
R2	Fibrinogen	50µl	P29	50µl	P49	Deadtime	3s	T-Corr	0%		

**B. Manual Method: Coatron M****1. Preparation of Standard, Control and Patient Dilutions**

Standard Dilution	Plasma	IBS Buffer
1:5	200µL Standard	800µL
1:10	500µL 1:5 STD	500µL
1:20	500µL 1:10 STD	500µL
1:40	500µL 1:20 STD	500µL
Patient or Control	100µL Plasma	900µL

2. Pipette **50 µl diluted standard or patient plasma** (1:10) into a test cuvette. Prewarm at 37°C for 1-2 minutes.

3. Add **25 µl Thrombin reagent** and simultaneously start test.

For other instrument, please refer to your instrument manual for more detailed instrument specific instructions.

**Calibration**

TECal Normal or other commercially prepared plasma standard in which Fibrinogen has been determined should be used as reference (200-300mg/dL). Plot the clotting time obtained with each of the FIB standard dilutions on the y-axis against the concentration of FIB (mg/dL) on the x-axis using log-log graph paper. The line of best fit should be determined by linear regression analysis. The fibrinogen in plasma samples can be determined by interpolation from the calibration curve.

**Expected Results**

Typical normal results are 180-450 mg/dL<sup>4,5</sup>. However results are influenced by the method of clot detection and can vary from laboratory to laboratory. Each laboratory is recommended to establish its own normal range on the specific instrument used.

**Quality Control**

TEControl or other commercial control plasma should be used for reliable quality control of performance at a frequency in accordance with good laboratory practice (GLP). TEControl can be frozen one time after reconstitution. 120-150 µl stored in closed polypropylen tubes at -20°C is stable for 30 days

**Limitations****A. Specimen Collection. AVOID:**

- Use only plastic tubes or siliconised glass.
- Delayed mixing of blood with anticoagulant.
- Contamination with tissue thromboplastin.
- Improper ratio of anticoagulant with blood.
- Hemolyzed, icteric or lipemic samples may interfere optical systems

**B. Laboratory Techniques**

- Perform tests at 37°C.
- Use only high purity water.
- Optimum pH is 7.0-7.5.

**Performance Characteristics**

<b>Precision:</b>	CV% (within run)	CV% (inter-runs)
Normal control	< 5.0	< 5.0
Abnormal control	< 5.0	< 10.0
(Typical performance on instrument Coatron M4)		

**Warranty**

This product is warranted to perform in accordance with its labelling and literature. TECO disclaims any implied warranty of merchantability or fitness for any other purpose, and in no event will TECO be liable for any consequential damages arising out of aforesaid express warranty.

**References**

- Clauss, A., Gerinnungsphysiologische Schnellmethode zur bestimmung des Fibrinogens. Acta Haematol., 1957, 17: 237-246.
- Shaw, T.S., Assays for Fibrinogen and its Derivatives, CRC Crit. Rev. Clin. Lab. Sci., 1977, 8: 145-192.
- National Committee for the National Laboratory (NCCLS) Standards: Collection transport and preparation of blood specimens for coagulation testing and performance of coagulation assays. Document H21-A2, vol. 11, No. 23, 1991.
- Scully, R.E. et al., Normal Reference Laboratory Values, N. Eng. J. Med., 1980, 302(37) : 37-48.
- Okuno, T. and Selenko, V., Amer. J. Med. Tech., 1972, 38(6) : 196-201.

Symbols key:

Expiry date	In Vitro Diagnostica	Biological hazard	Catalogue Number	Consult accompanying documents
Store at 2-8°C	EU conformity	Manufacturer	Lot. Number	Authorized Representative



IVD

REF

A0501-010, A0501-025, A0511-020, A0511-050

### Verwendungszweck

TEClot FIB wird zur quantitativen Bestimmung von Fibrinogen im menschlichen Plasma nach einer von Clauss<sup>1</sup> entwickelten Methode verwendet. Der Fibrinogenpegel kann auf Grund von Entzündungen, Schwangerschaft und dem Gebrauch von Ovulationshemmern ansteigen<sup>2</sup>. Geringere Konzentrationen können bei verschiedenen Krankheiten wie Leberversagen und DIC auftreten. Angeborene Defizite beinhalten Afibrinogenämie (kein auffindbares Fibrinogen), Hypofibrinogenämie (<1 mg/ml) und Dysfibrinogenämie (abnormale Fibrinogenmoleküle).

### Inhalte und Vorbereitungen

Produkt	TEClot FIB Kit-10	TEClot FIB Kit-25	TEClot FIB	TEClot FIB
Kat. Nr.	A0501-010	A0501-025	A0511-020	A0511-050
Thrombin Reagenz	5x2 mL	5x5 mL	10x2 mL	10x5 mL
IBS Puffer	1x125 mL	1x125 mL	-	-
TECal Normal	1x1 mL	1x1 mL	-	-
TEControl A	1x1 mL	1x1 mL	-	-

### Bestimmungen

	400 Def.	1000 Def.	800 Def.	2000 Def.
Coatron M*				
Coatron A4	200 Def.	500 Def.	400 Def.	1000 Def.
Coatron A6	200 Def.	500 Def.	400 Def.	1000 Def.

\*Mikromethode (75µL insgesamt)

- Thrombin Reagenz:  
Enthält Rinderthrombin (~80 NIH) mit Stabilisatoren.  
**REF: A0501-010/A0511-020:** mit 2ml hochreinem Wasser anlösen  
**REF: A0501-025/A0511-050:** mit 5ml hochreinem Wasser anlösen
- IBS Puffer: gebrauchsfertig, 125ml  
Enthält gepufferte Natriumchlorid Lösung, pH 7,3-7,4
- TECal Normal: Mit 1ml hochreinem Wasser anlösen  
Enthält mit Zitrat versetztes menschliches Plasma.
- TEControl A: Mit 1ml hochreinem Wasser anlösen  
Enthält mit Zitrat versetztes menschliches Plasma.

Nach der Anlösung vorsichtig leicht schwenken und bei Raumtemperatur 15 Minuten stehen lassen. Vor Gebrauch gut mischen. Nicht schütteln.

### Lagerung und Stabilität

Ungeöffnete Reagenzien sind bei Lagerung zwischen 2-8°C bis zum auf dem Etikett angegebenen Verfallsdatum haltbar. **Geöffnete Reagenzien:**

Thrombin Reagenz*	2-8 °C	15-25 °C	37 °C
	12 days	5 days	24 Std
TEControl oder Plasma	2-8 °C	15-25 °C	-20 °C
	8 Std	4 Std	30 Std

\* Reagenz muss vor UV-Licht und Verdunstung geschützt werden.

### Vorsichtsmaßnahme

Haut- & Augenkontakt vermeiden. Abfälle gemäß lokaler Richtlinien für infektiöse Materialien entsorgen. Alle Bestandteile wurden auf HIV, HBV und HCV getestet. Trotzdem müssen Produkte aus menschlichem Blut immer als potentiell infektiös behandelt werden.

### Probenentnahme und Lagerung<sup>3</sup>

- Venöses Blut mittels Venenpunktur unter sauberen Bedingungen entnehmen.
- Sofort 9 Teile Blut mit einem Teil 3,2% Natriumzitrat (0,105M) gut mischen.
- Probe bei 1500g 10 Minuten lang zentrifugieren (Thrombozyten <10000/µl)
- Plasma nach der Zentrifugierung entfernen und in einem Röhrchen aus Plastik oder silikonisiertes Glas aufbewahren.
- Plasma innerhalb von 4 Stunden verwenden, andernfalls gefroren lagern und kurz vor Gebrauch auftauen.

### Verfahren

#### A. Automatenmethode: Coatron A

Fibrinogen		A4		A6				A4		A6	
PAT	Patient	10µl	CP1	10µl	CP1	Incubation	0s	SENS	0		
BUF	IBS Buffer	90µl	P39	90µl	P79	Maxtime	120s	POINTS	4		
CLR	-	0µl	-	0µl	-	Unit	769	MIX	No		
DP	-	0µl	P00	0µl	P00	Method	Coag	Clean	1	3	
R0	-	0µl	P00	0µl	P00	Math	log XY	Multi	1	1	
R1	-	0µl	P00	0µl	P00	CT-Mech	Yes	S-Corr	0%		
R2	Fibrinogen	50µl	P29	50µl	P49	Deadtime	3s	T-Corr	0%		

Erklärung der Symbole:

Verfallsdatum	IVD	In-Vitro Diagnostik	Biologische Gefahr	REF	Katalog-Nummer	i	Begleitpapiere beachten	
Bei 2-8°C lagern	CE	EU Konformität	Hersteller	LOT	Lot.-Nummer	EC	REP	Bevollmächtigter

### B. Manuelle Methode: Coatron M

- Vorbereitung von Standard-, Kontroll- und Patientenlösungen

Standardlösung	Plasma	IBS Puffer
1:5	200µL Standard	800µL
1:10	500µL 1:5 STD	500µL
1:20	500µL 1:10 STD	500µL
1:40	500µL 1:20 STD	500µL
Patient oder Kontrolle	100µL Plasma	900µL

- 50µl verdünntes Standard- oder Patientenplasma (1:10) in eine Küvette pipettieren. Bei 37°C für 1-2 Minuten erwärmen
- 25µl Thrombinreagenz hinzufügen und gleichzeitig Test starten.
- Wenn Sie ein anderes Gerät verwenden, lesen Sie bitte für genauere Informationen die entsprechende Geräteanleitung.

### Kalibrierung

TECal Normal oder anderes kommerzielles Standardplasma, mit bekanntem Fibrinogengehalt, sollte als Referenz (200-300 mg/dl) verwendet werden. Geben Sie die Gerinnungszeit jeder FIB Standard Lösung auf der Y- Achse gegen die FIB Konzentration (mg/dl) auf der X- Achse an. Verwenden Sie Millimeterpapier. Die Reihe der besten Ergebnisse sollte durch lineare Regressionsanalyse bestimmt werden. Fibrinogen in den Plasmaproben kann durch Interpolation der Kalibrierungskurve bestimmt werden.

### Erwartete Ergebnisse

Typische normale Ergebnisse sind 180-450mg/dl<sup>4,5</sup>. Die Ergebnisse sind jedoch von der Methode, wie die Gerinnungszeit bestimmt wird, abhängig und können von Labor zu Labor variieren. Jedem Labor wird empfohlen, seinen eigenen normalen Ergebnisbereich auf dem verwendeten Instrument zu erstellen.

### Qualitätskontrolle

TEControl oder anderes kommerzielles Kontrollplasma sollte, um eine gute Qualität sicherzustellen, in regelmäßigen Abständen entsprechend Laborrichtlinien gemessen werden. In regelmäßigen Abständen entsprechend Laborrichtlinien gemessen werden. TEControl kann einmalig wieder eingefroren werden. Hierfür 120-150µl in einem verschließbaren polypropylen Gefäß bei -20°C aufbewahren und innerhalb der nächsten 30 Tage verwenden.

### Beschränkungen

A. Probenvorbereitung. Achten Sie auf:

- nur Plastikröhrchen oder silikonisiertes Glas verwenden
- verzögertes Mischen von Blut mit Antikoagulanzen vermeiden
- Kontamination mit Gewebethromboplastin vermeiden
- falsches Verhältnis von Antikoagulanzen und Blut vermeiden
- Hämolytische, lipämische oder ikterische Proben können optische Systeme stören

B. Labortechniken

- Tests bei 37°C durchführen
- nur hochreines Wasser verwenden
- der optimale pH Wert ist 7,0-7,5

### Leistungsdaten

<b>Präzision:</b>	VK% (Einzelauf)	VK% (Mehrfachlauf)
Normale Kontrolle	< 5,0	< 5,0
Abnormale Kontrolle	< 5,0	< 10,0

(Typische Leistung beim Gerät Coatron M4)

### Garantie

Es wird garantiert, dass die Wirkungsweise dieses Produktes den Angaben auf der Packung und in der Produktliteratur entspricht. TECO haftet weder für die Veräußerlichkeit oder Eignung dieses Produktes für irgendwelche andere Zwecke noch für irgendwelche Folgeschäden, die sich aus der vorstehenden, expliziten Garantie ergeben.

### Referenzen

- Clauss, A., Gerinnungsphysiologische Schnellmethode zur Bestimmung des Fibrinogens. Acta Haematol., 1957, 17: 237-246.
- Shaw, T.S., Assays for Fibrinogen and its Derivatives, CRC Crit. Rev. Clin. Lab. Sci., 1977, 8: 145-192.
- National Committee for the National Laboratory (NCCLS) Standards: Collection transport and preparation of blood specimens for coagulation testing and performance of coagulation assays. Document H21-A2, vol. 11, No. 23, 1991.
- Scully, R.E. et al., Normal Reference Laboratory Values, N. Eng. J. Med., 1980, 302(37) : 37-48.
- Okuno, T. and Selenko, V., Amer. J. Med. Tech., 1972, 38(6) : 196-201.



IVD

REF

A0501-010, A0501-025, A0511-020, A0511-050

**Revisions-Übersicht:**

Rev.	am	Änderung durch	Gültig für	Freigabe am	Freigabe durch
1	5.4.11	WG	Technoclone FIB		
	Beschreibung:	New box insert for Technoclone FIB.			
2	21.12.11	CB	Technoclone FIB	21.12.11	CH
	Beschreibung:	Neue Stabilitätsangaben. Die Vorgaben wurden dem Technoclone Stability Test Report „TC6E0C.01“ vom 5.5.2010 entnommen.			
3	11.11.13	CB	Technoclone FIB		
	Beschreibung:	<ul style="list-style-type: none"> <li>- Protokoll für A4+A6</li> <li>- Stabilitätsdaten neu</li> </ul>			
4	16.10.17	AR	Technoclone FIB	16.10.17	CH
	Beschreibung:	Technoclone Puffer (A0591-090) wird ersetzt durch IBS (A0590-125) (wegen deutlicher Messunterschiede bei Coatron A und X Serie) Wertermittlung für das CoA erfolgt ebenso mit IBS (A0590-125)			
5	23.01.18	VG	Technoclone FIB	23.01.18	VG
	Beschreibung:	Neue Stabilitätsangaben von Technoclone vom Thrombin Reagent.			





IVD

REF

A0590-125

### Intended Use

The IBS Buffer solution is optimally formulated for use on Coagulation Analyzers. Use in accordance with the recommended Operators Manuals for installing and replacing Owrens Veronal Buffer (OVB). The IBS can be used as the diluent for preparing plasma dilutions in the performance of Fibrinogen determinations and Coagulation Factor Assays with all manual, mechanical, or photo-optical means of clot detection. Follow Reagent manufacturer's recommended procedures for preparation of plasma dilutions using Imidazole Buffered Saline.

### Contents & Determinations

Product	IBS Buffer
Cat.No.	A0590-125
IBS Buffer	1x125 mL

### Preparation

IBS: pH 7.3 - 7.4, liquid  
Ready to use.

### Storage and Stability

Unopened reagents are stable until the expiration date shown on the label stored at 2-8°C.

### Precautions

Avoid contact with skin and eyes. Wear suitable protective clothing. Dispose components in compliance with local regulations for infectious material.

### Warranty

This product is warranted to perform in accordance with its labelling and literature. TECO disclaims any implied warranty of merchantability or fitness for any other purpose, and in no event will TECO be liable for any consequential damages arising out of aforesaid express warranty.

Symbols key:

Expiry date	In Vitro Diagnostica	Biological hazard	Catalogue Number	Consult accompanying documents
Store at 2-8°C	EU conformity	Manufacturer	Lot. Number	Authorized Representative



### Verwendungszweck

Die IBS Pufferlösung (Imidazole Buffered Saline) wird für die Verdünnung von Plasma verwendet werden, wie es z.B. bei der koagulometrischen Bestimmung von Fibrinogen, Einzelfaktoren oder auch Verdünnungsreihen für die Methoden Kalibrierung notwendig ist.

### Inhalte und Bestimmungen

Produkt	IBS Puffer
Kat.Nr.	A0590-125
IBS Buffer	1x125 mL

### Vorbereitung

IBS: pH 7.3 - 7.4, flüssig  
Gebrauchsfertig

### Lagerung und Stabilität

Ungeöffnete Reagenzien sind bei Lagerung zwischen 2-8°C bis zum auf dem Etikett angegebenen Verfallsdatum haltbar.











### Vorsichtsmaßnahmen

Haut- und Augenkontakt vermeiden. Angemessene Schutzkleidung tragen. Bestandteile gemäß lokaler Vorschriften für infektiöse Materialien entsorgen.

### Garantie

Es wird garantiert, dass die Wirkungsweise dieses Produktes den Angaben auf der Packung und in der Produktliteratur entspricht. TECO haftet weder für die Verkäuflichkeit oder Eignung dieses Produktes für irgendwelche andere Zwecke noch für irgendwelche Folgeschäden, die sich aus der vorstehenden, expliziten Garantie ergeben.

Erklärung der Symbole:

 Verfallsdatum	 In-Vitro Diagnostik	 Biologische Gefahr	 Katalog-Nummer	 Begleitpapiere beachten
 Bei 2-8°C lagern	 EU Konformität	 Hersteller	 Lot. - Nummer	 Bevollmächtigter



IVD

REF

P6001-010

**Intended Use**

Use as a normal control for following coagulation tests:

**PT, APTT, Thrombin time, Fibrinogen,  
Anti-thrombin and D-Dimer**

**Contents**

10 x 1mL freeze dried citrate-anticoagulated human plasma

**Preparation**

Reconstitute individual vials with **1,0 ml** distilled water. Allow to stand at room temperature, with occasional swirling, for 15 min before use. Be certain all particulate matter is well dissolved.

PT whole blood (TEClot PT-B): Reconstitute individual vials with **1,7 ml** distilled water.

**Storage & Stability**

Unopened vials are stable until the expiration date shown on the label stored at 2°-8°C.

Dissolved plasma change analytic levels below 10% if stored as following:

-20 °C	2-8 °C	20-25 °C
1 month	8 hours	4 hours

Dissolved plasma can be refrozen only one time in aliquots (120-150µL). Stored at -20°C in closed polypropylene tubes, the aliquots must be used within 30 days.

**Precautions**

This product contains substance from human origin!  
Avoid contact with skin and eyes. Wear suitable protective clothing. Dispose components in compliance with local regulations for infectious material. All components are checked for HIV, HBV and HCV. However products from human blood should be considered as potentially infectious.

**Expected Results**

Refer to "Certificate of Analysis".

**Warranty**

This product is warranted to perform in accordance with its labelling and literature. TECO disclaims any implied warranty of merchantability or fitness for any other purpose, and in no event will TECO be liable for any consequential damages arising out of aforesaid express warranty.

Symbols key:

Expiry date	In Vitro Diagnostica	Biological hazard	Catalogue Number	Consult accompanying documents
Store at 2-8°C	EU conformity	Manufacturer	Lot. Number	Authorized Representative







### Verwendungszweck

Als normale Kontrolle für folgende Gerinnungstests verwenden:

**PT, APTT, Thrombinzeit, Fibrinogen,  
Antiithrombin und D-Dimer**

### Inhalt

10 x 1mL gefriergetrocknetes mit Zitrat versetztes gerinnungshemmendes Humanplasma

### Vorbereitung

Die einzelnen Fläschchen mit 1,0ml destilliertem Wasser anlösen. Fläschchen bei Raumtemperatur bis zur Anwendung unter gelegentlichen Verwirbeln 15 Minuten lang stehen lassen. Stellen Sie sicher, dass alle Partikel gut aufgelöst sind.

Vollblut PT (TEClot PT-B): einzelne Fläschchen mit 1,7ml destilliertem Wasser anlösen.

### Lagerung und Stabilität

Ungeöffnete Fläschchen sind bei Lagerung zwischen 2-8°C zum bis auf dem Etikett angegebenen Verfallsdatum haltbar.

Gelöstes Plasma verändern die analytischen Levels unter 10% wenn wie folgt gelagert:

-20 °C	2-8 °C	20-25 °C
1 Monat	8 Stunden	4 Stunden

Gelöstes Plasma kann einmalig wiedereingefroren werden. Die Aliquots (120-150µL) sind 30 Tage haltbar, wenn sie in polypropylen Gefäßen bei -20°C aufbewahrt werden.

### Vorsichtsmaßnahmen

Dieses Produkt enthält Substanzen humanen Ursprungs! Haut- und Augenkontakt vermeiden. Angemessene Schutzkleidung tragen. Abfälle laut lokaler Regelungen für infektiöse Materialien entsorgen. Alle Bestandteile wurden auf HIV, HBV und HCV getestet. Trotzdem müssen Produkte aus menschlichem Blut immer als potentiell infektiös angesehen werden.

### Erwartete Ergebnisse

Lesen Sie das Analysenzertifikat

### Garantie

Es wird garantiert, dass die Wirkungsweise dieses Produkts den Angaben auf der Packung und in der Produktliteratur entspricht. TECO haftet weder für die Verkäuflichkeit oder Eignung dieses Produktes für irgendwelche andere Zwecke noch für irgendwelche Folgeschäden, die sich aus der vorstehenden, expliziten Garantie ergeben.

Erklärung der Symbole:

Verfallsdatum	In-Vitro Diagnostik	Biologische Gefahr	Katalog-Nummer	Begleitpapiere beachten
Bei 2-8°C lagern	EU Konformität	Hersteller	Lot. - Nummer	Bevollmächtigter



### Intended Use

Use as an abnormal control for following coagulation tests:

**PT, APTT, Thrombin time, Fibrinogen, Antithrombin and D-Dimer**

### Contents

10 x 1mL freeze dried citrate-anticoagulated human plasma

### Preparation

Reconstitute individual vials with **1,0 ml** distilled water. Allow to stand at room temperature, with occasional swirling, for 15 min before use. Be certain all particulate matter is well dissolved.

PT whole blood (TEClot PT-B): Reconstitute individual vials with **1,7 ml** distilled water.

### Storage & Stability

Unopened vials are stable until the expiration date shown on the label stored at 2°-8°C.

Dissolved plasma change analytic levels below 10% if stored as following:

-20 °C	2-8 °C	20-25 °C
1 month	8 hours	4 hours

Dissolved plasma can be refrozen only one time in aliquots (120-150µL). Stored at -20°C in closed polypropylene tubes, the aliquots must be used within 30 days.

### Precautions

This product contains substance from human origin! Avoid contact with skin and eyes. Wear suitable protective clothing. Dispose components in compliance with local regulations for infectious material. All components are checked for HIV, HBV and HCV. However products from human blood should be considered as potentially infectious.

### Expected Results

Refer to "Certificate of Analysis".

### Warranty

This product is warranted to perform in accordance with its labelling and literature. TECO disclaims any implied warranty of merchantability or fitness for any other purpose, and in no event will TECO be liable for any consequential damages arising out of aforesaid express warranty.

Symbols key:

Expiry date	In Vitro Diagnostica	Biological hazard	Catalogue Number	Consult accompanying documents
Store at 2-8°C	EU conformity	Manufacturer	Lot. Number	Authorized Representative

### Verwendungszweck

Als abnormale Kontrolle für folgende Gerinnungstests verwenden:

**PT, APTT, Thrombinzeit, Fibrinogen, Antithrombin und D-Dimer**

### Inhalt

10 x 1mL gefriergetrocknetes mit Zitrat versetztes gerinnungshemmendes Humanplasma

### Vorbereitung

Die einzelnen Fläschchen mit 1,0ml destilliertem Wasser anlösen. Fläschchen bei Raumtemperatur bis zur Anwendung unter gelegentlichen Verwirbeln 15 Minuten lang stehen lassen. Stellen Sie sicher, dass alle Partikel gut aufgelöst sind.

Vollblut PT (TEClot PT-B): einzelne Fläschchen mit 1,7ml destilliertem Wasser anlösen.

### Lagerung und Stabilität

Ungeöffnete Fläschchen sind bei Lagerung zwischen 2-8°C zum bis auf dem Etikett angegebenen Verfallsdatum haltbar.

Gelöstes Plasma verändern die analytischen Levels unter 10% wenn wie folgt gelagert:

-20 °C	2-8 °C	20-25 °C
1 Monat	8 Stunden	4 Stunden

Gelöstes Plasma kann einmalig wiedereingefroren werden. Die Aliquots (120-150µL) sind 30 Tage haltbar, wenn sie in polypropylen Gefäßen bei -20°C aufbewahrt werden.

### Vorsichtsmaßnahmen

Dieses Produkt enthält Substanzen humanen Ursprungs! Haut- und Augenkontakt vermeiden. Angemessene Schutzkleidung tragen. Abfälle laut lokaler Regelungen für infektiöse Materialien entsorgen. Alle Bestandteile wurden auf HIV, HBV und HCV getestet. Trotzdem müssen Produkte aus menschlichem Blut immer als potentiell infektiös angesehen werden.

### Erwartete Ergebnisse

Lesen Sie das Analysenzertifikat

### Garantie

Es wird garantiert, dass die Wirkungsweise dieses Produkts den Angaben auf der Packung und in der Produktliteratur entspricht. TECO haftet weder für die Verkäuflichkeit oder Eignung dieses Produktes für irgendwelche andere Zwecke noch für irgendwelche Folgeschäden, die sich aus der vorstehenden, expliziten Garantie ergeben.

Erklärung der Symbole:

Verfallsdatum	In-Vitro Diagnostik	Biologische Gefahr	Katalog-Nummer	Begleitpapiere beachten
Bei 2-8°C lagern	EU Konformität	Hersteller	Lot. - Nummer	Bevollmächtigter