

BZO Rapid Test Cassette (Whole Blood/Serum/Plasma)

Package Insert

A rapid test for the qualitative detection of Benzodiazepines in human whole blood or serum or plasma. For medical and other professional in vitro diagnostic use only.

INTENDED USE
The BZO Rapid Test Cassette (whole blood/serum/plasma) is a lateral flow chromatographic immunoassay for the detection of Benzodiazepines in whole blood or serum or plasma at a cut-off concentration of 100ng/ml. This test will detect other related compounds, please refer to the analytical Specificity table in this package insert.

This assay provides only a qualitative, preliminary analytical test result. A more specific alternate chemical method must be used in order to obtain a confirmed analytical result. Gas chromatography/mass spectrometry (GC/MS) is the preferred confirmatory method. Clinical consideration and professional judgment should be applied to any drug of abuse test result, particularly when preliminary positive results are used.

SUMMARY
Benzodiazepines are medications that are frequently prescribed for the symptomatic treatment of anxiety and sleep disorders. They produce their effects via specific receptors involving a neurochemical called gamma aminobutyric acid (GABA). Because they are safer and more effective, benzodiazepines have replaced barbiturates in the treatment of both anxiety and insomnia. Benzodiazepines are also used as sedatives before some surgical and medical procedures, and for the treatment of seizure disorders and alcohol withdrawal.

Risk of physical dependence increases if benzodiazepines are taken regularly (e.g., daily) for more than a few months, especially at higher than normal doses. Stopping abruptly can bring on such symptoms as trouble sleeping, gastrointestinal upset, feeling unwell, loss of appetite, sweating, trembling, weakness, anxiety and changes in perception.

Only trace amounts (less than 1%) of most benzodiazepines are excreted unaltered in the whole blood or serum or plasma; most of the concentration in whole blood or serum or plasma is conjugated drug.

The detection period for benzodiazepines in whole blood or serum or plasma is 3-7 days.

PRINCIPLE
The BZO Rapid Test Cassette (whole blood/serum/plasma) is an immunoassay based on the principle of competitive binding. Drugs that may be present in the whole blood/serum/plasma specimen compete against the drug conjugate for binding sites on the antibody.

During testing, a whole blood/serum/plasma specimen migrates upward by capillary action. Benzodiazepines, if present in the whole blood/serum/plasma specimen below the cut-off level, will not saturate the binding sites of the antibody in the test. The antibody coated particles will then be captured by immobilized Benzodiazepine-protein conjugate and a visible colored line will show up in the test line region. The colored line will not form in the test line region if the Benzodiazepine level exceeds the cut-off level because it will saturate all the binding sites of anti-Benzodiazepine antibodies.

A drug-positive whole blood/serum/plasma specimen will not generate a colored line in the test line region because of drug competition, while a drug-negative whole blood/serum/plasma specimen or a specimen containing a drug concentration less than the cut-off will generate a line in the test line region. To serve as a procedural control, a colored line will always appear at the control line region indicating that proper volume of specimen has been added and membrane wicking has occurred.

REAGENTS
The test contains mouse monoclonal anti- Benzodiazepines antibody coupled particles and Benzodiazepine -protein conjugate. A goat antibody is employed in the control line system.

PRECAUTIONS
• For professional in vitro diagnostic use only. Do not use after the expiration date.
• Do not eat, drink or smoke in the area where the specimens or kits are handled.
• Do not use test if pouch is damaged.
• Handle all specimens as if they contain infectious agents. Observe established precautions against microbiological hazards throughout testing and follow the standard procedures for proper disposal of specimens.
• Wear protective clothing such as laboratory coats, disposable gloves and eye protection when specimens are being tested.
• The used test should be discarded according to local regulations.
• Humidity and temperature can adversely affect results.

STORAGE AND STABILITY
Store as packaged in the sealed pouch at room temperature or refrigerated (2-30°C). The test is stable through the expiration date printed on the sealed pouch. The test must remain in the sealed pouch until use. **DO NOT FREEZE**. Do not use beyond the expiration date.

SPECIMEN COLLECTION AND PREPARATION

- The BZO Rapid Test Cassette can be performed using whole blood (from venipuncture or fingerstick) /serum/plasma.
- To collect **Fingerstick Whole Blood specimens**:
 - Wash the patient's hand with soap and warm water or clean with an alcohol swab. Allow to dry.
 - Massage the hand without touching the puncture site by rubbing down the hand towards the fingertip of the middle or ring finger.
 - Puncture the skin with a sterile lancet. Wipe away the first sign of blood.
 - Gently rub the hand from wrist to palm to form a rounded drop of blood over the puncture site.
- Add the Fingerstick Whole Blood specimen to the test by using a **capillary tube**:
 - Touch the end of the capillary tube to the blood until filled to approximately 40 μ l. Avoid air bubbles.
 - Place the bulb onto the top end of the capillary tube, then squeeze the bulb to dispense the whole blood to the specimen area of the test cassette.
- Testing should be performed immediately after the specimens have been collected. Do not leave the specimens at room temperature for prolonged periods. For long term storage, specimens should be kept below -20°C. Whole blood/serum/plasma collected by venipuncture should be stored at 2-8°C if the test is to be run within 2 days of collection. Do not freeze whole blood or serum or plasma specimens. Whole blood or serum or plasma collected by fingerstick should be tested immediately.
- Bring specimens to room temperature prior to testing. Frozen specimens must be completely thawed and mixed well prior to testing. Specimens should not be frozen and thawed repeatedly.
- If specimens are to be shipped, they should be packed in compliance with local regulations covering the transportation of etiologic agents.

MATERIALS

• Test cassettes	Materials Provided
• Specimen collection containers	• Droppers
• Lancets (for fingerstick whole blood only)	• Buffer
• Heparinized capillary tubes and dispensing bulb (for fingerstick whole blood only)	• Package insert
Materials Required But Not Provided	
• Centrifuge	• Timer

DIRECTIONS FOR USE


Allow the test, specimen, buffer and/or controls to reach room temperature (15-30°C) prior to testing.

For serum or plasma specimen:

1. Bring the pouch to room temperature (15-30°C) before opening it. Remove the cassette from the sealed pouch and use it within one hour.

2. Place the cassette on a clean and level surface. Hold the dropper vertically and transfer **1 full drop of serum or plasma** (approximately 40 μ l), then add **2 drops of buffer** (approximately 80 μ l) to the specimen well of the cassette, and then start the timer. Avoid trapping air bubbles in the specimen well. See illustration below.

3. Wait for the colored line(s) to appear. **Read the result at 5 minutes**. Do not interpret the result after 10 minutes.

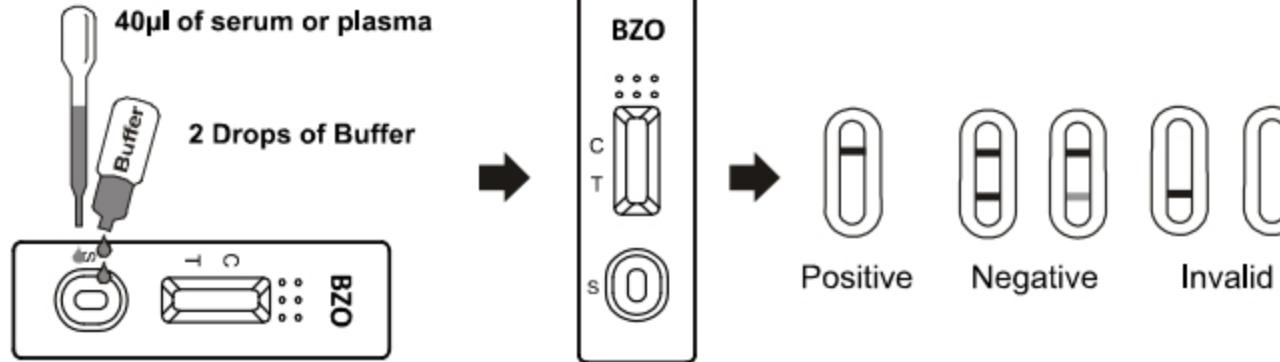

For whole blood specimen:

1. Bring the pouch to room temperature before opening it. Remove the test cassette from the sealed pouch and use it as soon as possible.
2. Place the cassette on a clean and level surface.


For **Venipuncture Whole Blood** specimen:

- Hold the dropper vertically and transfer **1 drop of whole blood** (approximately 40 μ l) to the specimen well, then add **2 drops of buffer** (approximately 80 μ l), and start the timer. See illustration below.

For **Fingerstick Whole Blood** specimen:

- To use a capillary tube: Fill the capillary tube and transfer **approximately 40 μ l of fingerstick whole blood specimen** to the specimen area of test cassette, then add **2 drops of buffer** (approximately 80 μ l) and start the timer. See illustration below.

3. Wait for the colored line(s) to appear. **Read results at 5 minutes**. Do not interpret the result after 10 minutes.

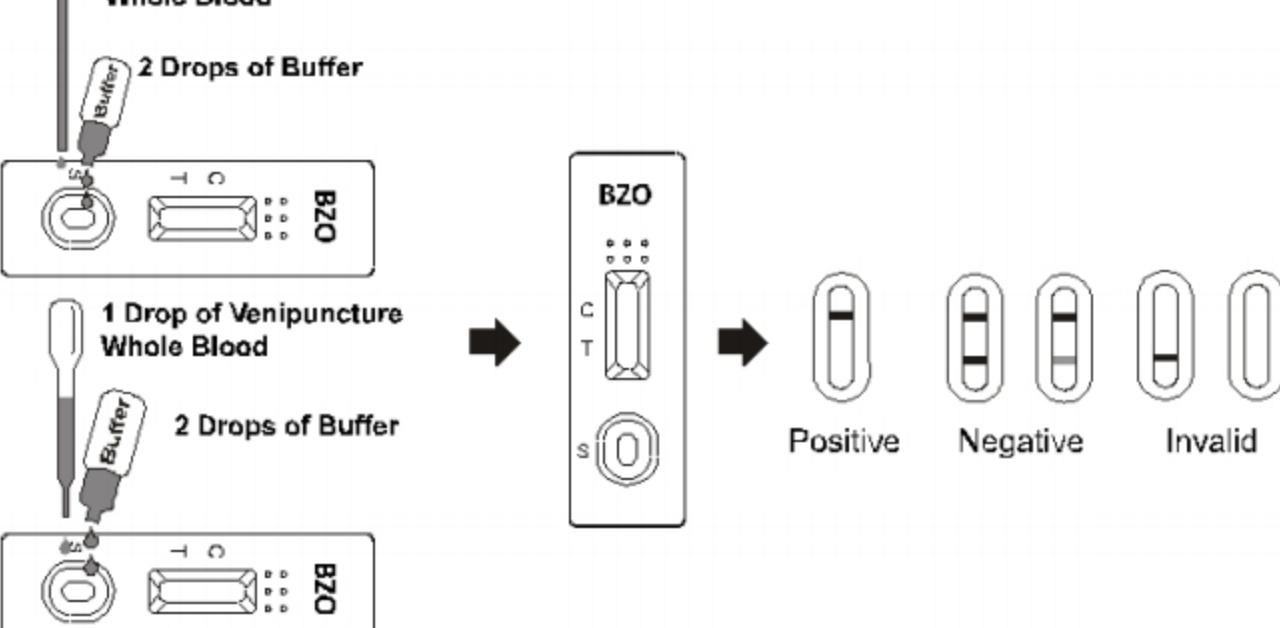

INTERPRETATION OF RESULTS

(Please refer to the illustration above)

NEGATIVE: Two lines appear. One colored line should be in the control line region (C), and another apparent colored line should be in the test line region (T). This negative result indicates that the Benzodiazepines concentration is below the detectable cut-off level.

NOTE: The shade of color in the test line region (T) may vary, but it should be considered negative whenever there is even a faint colored line.

POSITIVE: One colored line appears in the control line region (C). No line appears in the test line region (T). This positive result indicates that the Benzodiazepines concentration exceeds the detectable cut-off level.

INVALID: Control line fails to appear. Insufficient specimen volume or incorrect procedural techniques are the most likely reasons for control line failure. Review the procedure and repeat the test with a new test. If the problem persists, discontinue using the test kit immediately and contact your local distributor.

QUALITY CONTROL

A procedural control is included in the test. A colored line appearing in the control region (C) is the internal procedural control. It confirms sufficient specimen volume and correct procedural technique. Control standards are not supplied with this kit; however, it is recommended that positive and negative controls be tested as a good laboratory practice to confirm the test procedure and to verify proper test performance.

LIMITATIONS

1. The BZO Rapid Test Cassette (whole blood/serum/plasma) provides only a qualitative, preliminary analytical result. A secondary analytical method must be used to obtain a confirmed result. Gas chromatography/mass spectrometry (GC/MS) is the preferred confirmatory method.²
2. It is possible that technical or procedural errors, as well as other interfering substances in the Whole blood or serum or plasma specimen may cause erroneous results.
3. A positive result indicates presence of the drug or its metabolites but does not indicate level of intoxication, administration route or concentration in Whole blood or serum or plasma.
4. A negative result may not necessarily indicate drug-free Whole blood/serum/plasma. Negative results can be obtained when drug is present but below the cut-off level of the test.

5. Test does not distinguish between drugs of abuse and certain medications.

EXPECTED VALUES

This negative result indicates that the Benzodiazepines concentration is below the detectable level of 100ng/ml. Positive result means the concentration of Benzodiazepines is above the level of 100ng/ml.

The BZO Rapid Test Cassette has a sensitivity of 100ng/ml.

PERFORMANCE CHARACTERISTICS

Accuracy

A side-by-side comparison was conducted using The BZO Rapid Test Cassette and GC/MS at the cut-off of 100ng/ml. Testing was performed on 90 clinical specimens previously collected from subjects present for Drug Screen Testing. The following results were tabulated:

Clinic Result of Whole Blood

Method	GC/MS		Total Results
BZO Rapid Test Cassette	Results	Positive	Negative
	Positive	19	2

Negative	2	67	69
Total Results	21	69	90
% Agreement	90.5%	97.1%	95.6%

Clinic Result of Serum or Plasma

Method	GC/MS		Total Results
BZO Rapid Test Cassette	Results	Positive	Negative
Positive	19	2	21
Negative	2	67	69
Total Results	21	69	90
% Agreement	90.5%	97.1%	95.6%

Analytical Sensitivity

A drug-free whole blood/serum/plasma pool was spiked with Benzodiazepines at the following concentrations of $\pm 50\%$ cutoff and 3x cutoff. The data are summarized below:

For whole blood:

BZO Concentration (ng/ml)	Percent of Cut-off	n	Visual Result
0	0	30	Negative
50	-50%	30	0
100	Cut-off	30	15
150	+50%	30	30
300	3X	30	0

Analytical Specificity

The following table lists compounds that are positively detected in whole blood/serum/plasma by The BZO Rapid Test Cassette (whole blood/serum/plasma) at 5 minutes.

Compound

Concentration (ng/ml)

Compound	Concentration (ng/ml)
Alprazolam	40
a-hydroxyalprazolam	500
Clobazam	60
Clonazepam	150
Clorazepate/diethylamidine	150
Delorazepam	300
Desalkylflurazepam	60
Flunitrazepam	60
(\pm) lorazepam	1,000
RS-lorazepam glucuronide	600
Midazolam	2,000
Alprazolam	40
Bromazepam	300
Chlordiazepoxide	300
Nitrazepam	60
Nordiazepam	300
Oxazepam	100
Temazepam	40
Diazepam	100
Eszalox	2,000
Triazolam	1,000

The following table lists compounds that are positively detected in whole blood/serum/plasma by The BZO Rapid Test Cassette (whole blood/serum/plasma) at 5 minutes.

Compound

Concentration (ng/ml)

Compound	Concentration (ng/ml)	
Acetaminophen	Deoxycorticosterone MDE	β-Phenylethylamine
Acetylpromazine	Dextromethorphan	Phenylpropanolamine
N-Acetylprocainamide	Didofenac	Mepramate
Acetysalicylic acid	Diffenacul	Methadone
Aminopyrine	Digoxin	Prednisone
Amityptiline	Diphen	