

Digital Color Doppler Ultrasound System EBit 20/EBit 30/EBit 50/EBit 60

Operation Manual

V3.0

Oct. 21, 2022

57-00861-10

CHISON Medical Technologies Co., Ltd.

We reserve the right to make changes to this manual without prior notice.

Regulatory Requirement

C € 0197 This product conforms to the essential requirements of the Medical Device Directive 93/42/EEC. Accessories without the CE mark are not guaranteed to meet the Essential Requirements of the Medical Device Directive.

This manual is a reference for the EBit 20/EBit 30/EBit 50/EBit 60. Please verify that you are using the latest revision of this document. If you need the latest revision, contact your distributor.

Statement

- 1. No part of this manual may be reproduced, modified, copied or reprinted, in whole or in part, without written permission from CHISON.
- 2. The contents of this manual are subject to change without prior notice and without our legal obligation.
- 3. Before operating the system, please read and understand this manual. After reading, keep this manual in an easily accessible place. If you have any question or doubt, please contact CHISON's authorized service engineer.
- 4. CHISON's Warranty only cover material and parts costs for repair, but does not cover any labor cost or onsite service cost at end user's side.

Meaning of the signal words

In this manual, the warning words NOTE, CAUTION and WARNING are used for regarding safety and other important instructions. Please understand their meanings clearly before reading this manual. The words and their meanings are defined as follows:

Warning words	Meaning		
	Indicates information of interest to users of the equipment as to exceptional		
 ⚠ NOTE	conditions or operating procedures and make the system work in good		
	condition.		
A	Indicates an imminently hazardous situation which can not be avoided will		
<u>∠!</u> \warning	result in death, serious injury to the user or damage to the system.		
A	Indicates a potentially hazardous situation which can not be avoided, may		
∠!\CAUTION	result in death, serious injury to the user or make the system misoperation.		

Important information

<u>ACAUTION:</u>

- 1. It is prohibited to use the device for fetal sex examination, except for necessary medical needs.
 - 2. The device can only be sold to qualified medical institutions or doctors.
- 3. The users shall have got the qualification, and shall comply with the local laws and regulations, the local religion and customs, etc.
- 4. The users should read the operation manual carefully before operating the devices. Turning on the device means the users have read the operation manual and accept the listed cautions, warnings, and notes in the manuals. If the users disagree and cannot accept the cautions, the users can ask for returning the device.

- 1. It is the customer's responsibility to maintain and manage the system after delivery.
- 2. The warranty does not cover the following items, even during the warranty period:
- a. Damage or loss due to misuse or abuse with system and probes, for example, drop the probe, the liquid or the metal part fall into the system.
 - b. Damage or loss caused by Acts of God such as fires, earthquakes, floods, lightning, etc.
- c. Damage or loss caused by failure to meet the specified conditions for this system, such as inadequate power supply, improper installation or environmental conditions.
 - d. Damage or loss caused by non-approved transportation by CHISON.
- e. Damage or loss due to use the system outside the region where the system was originally sold.
- f. Damage or loss involving the system purchased from a source other than CHISON or its authorized agents.
- 3. Do not make changes or modifications to this system and probes. The System modified or repaired by people other than CHISON's qualified service engineers, CHISON shall not be liable for the system.
- 4. The system is to provide physicians with data for clinical diagnosis. It is the physician's responsibility for diagnostic procedures. CHISON shall not be liable for the results.
- 5. This manual contains warnings regarding foreseeable potential dangers, but user shall always be alert to dangers other than those indicated as well. CHISON shall not be liable for damage or loss that results from negligence or from ignoring the precautions and operating instructions described in this operation manual.
- 6. Important data must be backed up on external memory media. CHISON shall not be liable for loss of data stored in the memory of this system caused by operator error or accidents.
- 7. Please put this manual with the system to ensure operator and manager can reach it at any time. Due to negligence not following operation manual, CHISON shall not be liable for the results.
- 8. LED display screen may have some dark or light dots, it is normal for the LED. It does not mean that LED screen is defective.

Service Responsibility

If users install, use and maintain the system fully according to CHISON's installation manual, operation manual and service manual, then the main unit has a life time of 5 years and probes have life time of 5 years after ex-work.

The warranty of the system and probes after ex-work is as the time in the warranty card.

The system is a precise electronic system. Only the CHISON's authorized service engineer could replace the defective parts. Any assembly, disassembly, handling, repair, or replacement by any other people may have adverse impact on the safety and effectiveness of the systems and probes, and thus will reduce the life time of the system and probes, and such systems and probes will not be covered by CHISON warranty after the above improper handling. Standard maintenance must be performed by CHISON's authorized service engineer during the life time of the product.

<u> CAUTION:</u>

When the above life time is expired, the effectiveness and safety of system and probes maybe greatly affected, so it's NOT suggested to continue using the system and probes even the system and probes seem work properly. But if user still wants to continue using the system and probes, user should first contact CHISON service center at CHISON headquarter to arrange the necessary safety check and calibration by CHISON's authorized service engineer. If CHISON headquarter service center provides the calibration certificate for the related system or probe, then user could continue use the system or probes according to the calibration certificate. However, if CHISON headquarter service center concludes that the system or probe is no longer complied to the safety and effectiveness standard, then user should immediately stop using the system or probe. User understands that such check and calibration cost will be born by the user.

Systems and probes keep on using after the life time may also be difficult to repair and maintain, so it's suggested to renew the product after the life time.

Content

Digital Color Doppler Ultrasound System	1
Chapter 1 Introduction	1
1.1 System Overview	1
1.2 Contact Information	1
Chapter 2 System Safety	3
2.1 Safety Overview	3
2.2 Electrical Safety	4
2.3 Label	7
2.4 Patient Environmental Devices	10
2.5 Biological Safety	12
2.6 Scanning Patients and Education	14
2.7 Battery Handling Instructions	21
Chapter 3 System Introduction	23
3.1 Console View	23
3.2 Physical Specification	23
3.3 External Interface View	24
3.4 Key System Features	26
3.5 Installation Procedures	31
Chapter 4 Control Panel	39
4.1 Keyboard Appearance	39
4.2 Alphanumeric Keyboard	39
4.3 Function Keys/Knobs	40
4.4 Central Control	43
4.5 Information Area Indicating Machine Status	44
Chapter 5 Operation and Exam Mode	46
5.1 Preparing the System for Use	46
5.2 Choose Exam Mode	46
5.3 Patient Data Entry	47

	5.4 Image Interface Display	48
	5.5 Image Modes	49
	5.6 Parameters Adjustment on Control Panel	56
	5.7 B Image Menu & Parameters Adjustment	57
	5.8 M Image Menu & Parameters Adjustment	60
	5.9 CFM/CPA/DPD/TDI Image Menu & Parameters	61
	5.10 PW/CW Image Menu & Parameters	62
	5.11 Image and Cine Disposition	63
	5.12 Edit Comment	65
	5.13 Set Body Mark	67
	5.14 Set the Direction of Arrow	68
	5.15 Image Browse	68
	5.16 Archive Management	70
	5.17 Report	71
	5.18 DICOM	73
Ch	apter 6 Measurement and Calculation	75
	6.1 Keyboard for Measurement	75
	6.2 B Mode Measurement	77
	6.3 Measurement in M, B/M mode	92
	6.4 PW mode Measurement	96
Ch	apter 7 Preset	106
	7.1 General setting	106
	7.2 Measurement	109
	7.3 Comment	117
	7.4 Body marks	120
	7.5 Exam Mode	121
	7.6 Report	125
	7.7 DICOM	128
	7.8 Net	130

7.9 System	130
Chapter 8 System Maintenance	132
8.1 Machine Cleaning	132
8.2 Safety Check	132
8.3 Malfunction Check	133
Chapter 9 Probes	134
9.1 General Description	134
9.2 Care and Maintenance	134
9.3 Probe Operation Instructions	146
Appendix A: Acoustic Output Report Table	150
Appendix B: Guidance and Manufacturer's Declaration	291
Appendix C: Measurement Results Summary	295
Appendix D: Display Accuracy and Acoustic Measurement Uncertainties	296
Appendix E: Transducer Maximum Surface Temperature	297
Appendix F: Procedures of setting network sharing	299

Chapter 1 Introduction

This manual contains necessary information for safe system operation.

Read and understand all instructions in this manual before operating the system. Always keeping this manual with the equipment, and periodically review the procedures for operation and safety

precautions.

1.1 System Overview

Indications for Use

The device is a general-purpose ultrasonic imaging instrument intended for use by a qualified physician for evaluation of Fetal, Abdominal, Pediatric, Small Organ (breast, thyroid, testes), Neonatal Cephalic, Adult Cephalic, Cardiac (adult, pediatric), Musculo-skeletal (Conventional,

Superficial), Peripheral Vascular, Transesophageal, Transrectal, Transvaginal, Urology.

Contraindication

The system is NOT intended for ophthalmic use or any use that causes the acoustic beam to pass through the eye.

1.2 Contact Information

For additional information or assistance, please contact your local distributor or the appropriate support resource shown below:

CHISON website www.chison.com

Service Support CHISON Medical Technologies Co., Ltd.

Tel:0086-0510-85311707

Fax: 0086-0510-85310726

E-mail: service@chison.com.cn

Placing an Order CHISON Medical Technologies Co., Ltd.

Tel: 0086-0510-8531-0593/0937

Fax: 0086-0510-85310726

Email: export@chison.com.cn

Manufacturer CHISON Medical Technologies Co., Ltd.

No.3 Changjiang South Road, Xinwu District, Wuxi, 214028 Jiangsu, P.R.

China

US Agent Mr. Marco Mu, 2219 Rimland Drive, Suite 301, Bellingham, Barkley

Villiage Bellingham, Washington, 98226, UNITED STATES

Phone: 360-3257028, Fax: 360-9253199, Email: us.agent@mid-link.net

MID-LINK INTERNATIONAL CO., LTD

EC Representative Shanghai International Holding Corp.GmbH (Europe)

Address: Eiffestrasse 80, 20537 Hamburg, Germany

Tel: 0049-40-2513175

Fax: 0049-40-255726

E-mail: antonsissi@hotmail.com shholding@hotmail.com

Chapter 2 System Safety

2.1 Safety Overview

This section discusses the measures to ensure the safety of both the operator and patient. To ensure the safety of both operator and patient, please read the relevant details in this chapter carefully before operating this system. Disregarding the warnings or violation of relevant rules may result in personal injury for operator or patient, or even loss of life.

Users should observe the following precautions:

- 1. This system complies with Type BF general equipment, and the IEC standard.
- 2. Do not modify this system in any way. Necessary modifications must be made only by the manufacturer or its designated agents.
- 3. This system has been fully adjusted at the factory. Do not adjust any fixed adjustable parts.
- 4. In the event of a malfunction, turn off the system immediately and inform the manufacturer or its designated agents.
- 5. The power cable of the system should only be connected to a grounded power socket. Do not remove the ground cable for any reason.
- 6. Only connect this system, either electronically or mechanically, with devices that comply with the EN60601-1 standard. Recheck the leakage current and other safety performance indices of the entire system to avoid potential system damage caused by leakage from a current superposition.
- 7. The system does not incorporate any specialized protective measures in the event it is configured with high-frequency operation devices. The operator should use caution in these types of applications.
- 8. The system should be installed only by personnel authorized by the manufacturer. Do not attempt to install the system by yourself.
- 9. Only an authorized service engineer may perform maintenance.
- 10. Only a qualified operator, or someone under qualified supervision, should use the system.
- 11. Do not use this system in the presence of flammable substances, otherwise an explosion may

occur.

- 12. Do not continuously scan the same part of a patient or expose the patient to prolonged scanning; otherwise it may harm the patient.
- 13. When using the system for ultrasound testing, use only qualified ultrasound gel that complies with system standards.
- 14. Do not unplug probe when the system is in active operation. Always go to EXAM screen when need to remove the probe.
- 15. To prevent from arm or neck injury, the operator should not stay at the same position for too long during patient scanning without taking break.
- 16. Do not put liquid on top of the main unit. Except the printer all of the system could be used on 3000 meters above sea level. Please contact with the manufacture additionally, if you need the printer could be used on 2000-3000 meters above sea level.

\triangle NOTE:

- ✓ The system has built-in screen saver to avoid the tic mark on the display. It is not recommended to constantly turn on and off the unit.
- ✓ To dispose of this product properly, please call your local service department.

2.2 Electrical Safety

Type of protection against electric shock

Class I Equipment

CLASS I EQUIPMENT in which protection against electric shock does not rely on BASIC INSULATION only, but includes a protective earth ground. This additional safety precaution prevents exposed metal parts from becoming LIVE in the event of an insulation failure.

NOTE: The mains supply shall be cut off after disconnecting the power line and the net power.

Degree of protection against electric shock

Type BF Applied part (for Probes marked with BF symbol)

TYPE BF APPLIED PART providing a specified degree of protection against electric shock, with particular regard to allowable LEAKAGE CURRENT.

Level of protection against harmful ingress of water

Parts of probe likely to come into contact with operator or patient meet the requirements of drip-proof equipment (IPX1)

Parts of probe intended to be immersed in normal use meet the requirements of watertight equipment (IPX7).

• The IP Classification of System is Ordinary Equipment (IPX0)

Safety level when used in the presence of FLAMMABLE ANAESTHETIC MIXED WITH AIR (or WITH OXYGEN or WITH NITROUS OXIDE):

The Equipment is not suitable for use in the environment with FLAMMABLE ANAESTHETIC MIXED WITH AIR (or WITH OXYGEN or WITH NITROUS OXIDE).

Mode of operation

Continuous Operation

For maximum safety, always follow these guidelines:

Proper grounding of the system is critical to avoid electrical shock. For protection, ground the chassis with a three-wire cable and plug, and plug the system into a hospital-grade, three-hole outlet.

- Do not remove or circumvent the grounding wire.
- Do not remove the protective covers on the system. These covers protect users from hazardous voltages. Cabinet panels must remain in place while the system is in use. A qualified electronic technician must make all internal replacements.
- Do not operate this system in the presence of flammable gases or anesthetics.
- All peripheral devices (unless certified as medical grade) that are connected to the system must be powered through the electrical outlet through an optional isolation transformer.

Notice upon Installation of Product

Separation distance and effect from fixed radio communications equipment: field strengths from fixed transmitters, such as base stations for radio (cellular/cordless) telephones and land mobile radios, amateur radio, AM and FM radio broadcast, and TV broadcast transmitter cannot be predicted theoretically with accuracy. To assess the electromagnetic environment due to fixed RF transmitters, an electromagnetic site survey should be considered. If the measured field strength

in the location in which the ultrasound system is used exceeds the applicable RF compliance level as stated in the immunity declaration, the ultrasound system should be observed to verify normal operation. If abnormal operation is observed, additional measures may be necessary, such as re-orienting or relocating the ultrasound system or using an RF shielded examination room may be necessary.

- Use either power supply cords provided or designated by CHISON. Products equipped with a power source plug should be plugged into the fixed power socket which has the protective grounding conductor. Never use any adaptor or converter to connect with a power source plug (e.g. three-prong-to-two-prong converter).
- Locate the equipment as far away as possible from other electronic equipment.
- Be sure to use only the cables provided by or designated by CHISON. Connect these cables following the installation procedures (e.g. wire power cables separately from signal cables).
- Lay out the main equipment and other peripherals following the installation procedures described in this manual.

Notice against User Modification

The user should never modify this product.

User modifications may cause degradation in Electrical Safety. Modification of the product includes changes in:

- Cables (length, material, wiring, etc.)
- System configuration/components

User modifications may cause degradation in EMC performance. Modification of the product includes changes in:

- Cables (length, material, wiring, etc.)
- System installation/layout
- System configuration/components
- Securing system parts (cover open/close, cover screwing)

2.3 Label



Fig. 2-1 Rear panel label

2.3.1 Warning Symbols

This mark indicates that this product limited amount of hazardous substances in the Chinese Standard GB/T 26572-2011 "Limited Requirements for Restricted Substances in Electrical and Electronic Products". The numbers in the logo are the environmental protection use period of the product, indicating that under the normal use conditions, the harmful substances will not leak or be abrupt. The use of the product will not cause serious pollution to the environment or cause personal or property serious damage, the term unit is year.



ELECTRONIC EQUIPMENT (WEEE): This symbol is used for Environment Protection, it indicates that the waste of electrical and electronic equipment must not be disposed as unsorted waste and must be collected separately. Please contact your local Authority or distributor of the manufacturer for information concerning the decommissioning of your equipment.



Do not use the following devices near this equipment: cellular phone, radio receiver, and mobile radio transmitter, radio controlled toy, etc. Use of these devices near this equipment could cause this equipment to perform outside the published specifications. Keep power to these devices turned off when near this equipment.



Caution, consult accompanying documents.

This symbol advises the reader to consult the accompanying documents for important safety related information such as warnings and pre-cautions that cannot be presented on the device itself.



Refer to instruction manual/booklet.



The CE mark of Conformity indicates this equipment conforms with the Council Directive 93/42/EEC



AUTHORIZED REPRESENTATIVE IN THE EUROPEAN COMMUNITY: This symbol is accompanied by the name and the address of the authorized representative in the European Community.



Type-BF applied part

SN	
This symbol is followed by the serial number of	MANUFACTURER: This symbol is accompanied
the device.	by the name and the address of the
	manufacturer.
人	Rx only
Power On/off.	This symbol indicates that Federal law restricts
CAUTION: This Power Switch cannot isolate	
Mains Supply completely.	the device to sale by or on the order of a licensed
	practitioner or therapist in the united states.
YYYY-MM This symbol is followed by the manufacturing	CORRECT WRONG
date of the device in the form YYYY-MM.	CORRECT: The correct connection of the battery
	connector
	WRONG: The wrong connection of the battery
	connector
	₹
Direct current	Adapter Indicator: when the main unit connects to
To indicate on the rating plate that the equipment	the adapter with power supply, the indicator
is suitable for direct current only; to identify	lights, otherwise extinguishes.
relevant terminals.	
Battery Indicator: When the battery is charging,	Sleep Indicator: When the main unit is in sleep
the indicator lights yellow. Once the battery is	mode, the indicator lights, otherwise
charged, the indicator lights green. When the	extinguished.
battery volume is too low, the light flashes.	
Show the State of discharge and remaining	Show the State of charging and remaining
electric quantity and available time.	electric quantity
IPX7	IPX0
Protection against the effects of immersion	No protection against ingress of water (system)
(probes)	

2.4 Patient Environmental Devices

Left side:

- 1 LAN port
- 1 S-VIDEO port
- 2 USB ports
- 1 Footswitch port
- 1 Power in port

Rear panel:

- 2 Probe ports
- 2 USB ports
- 1 VIDEO OUT port
- 1 DVI port
- 1 VGA port
- 1 Remote port
- 1 ECG port

Acceptable Devices

The Patient Environmental devices shown above are specified to be suitable for use within the PATIENT ENVIRONMENT.

ACAUTION:

- ✓ DO NOT connect any probes or accessories without approval by CHISON within the PATIENT ENVIRONMENT.
- ✓ DO NOT touch patient and devices without IEC/EN 60601-1 approval to avoid the leakage current risk within the PATIENT ENVIRONMENT.

Unapproved Devices

ACAUTION:

- ✓ DO NOT use unapproved devices.
- ✓ If devices are connected without the approval of CHISON, the warranty will be INVALID.

✓ The system can't be used with HF surgical equipment; otherwise the burns to patient may occur.

Any device connected to this system must conform to one or more of the requirements listed below:

- ✓ IEC standard or equivalent standards appropriate to devices.
- ✓ The devices shall be connected to PROTECTIVE EARTH (GROUND).

ACAUTION:

Unsafe operation or malfunction may occur. Use only the accessories, options and supplies approved or recommended in these instructions for use.

Peripheral used in the patient environment

The system has been verified for overall safety, compatibility and compliance with the following on-board image recording devices:

B/W video printer: SONY UP-X898MD

The system may also be used safely while connected to devices other than those recommended above if the devices and their specifications, installation, and interconnection with the system conform to the requirements of IEC/EN 60601-1.

Adapter is considered as a part of ME equipment

The connection of equipment or transmission networks other than as specified in the user instructions can result in an electric shock hazard or equipment malfunction. Substitute or alternate equipment and connections require verification of compatibility and conformity to IEC/EN 60601-1 by the installer. Equipment modifications and possible resulting malfunctions and electromagnetic interference are the responsibilities of the owner.

General precautions for installing an alternate off-board, remote device or a network would include:

- The added device(s) must have appropriate safety standard conformance and CE Marking.
- There must be adequate mechanical mounting of the device and stability of the combination.
- Risk and leakage current of the combination must comply with IEC/EN 60601-1.

 Electromagnetic emissions and immunity of the combination must conform to IEC/EN 60601-1-2.

Peripheral used in the non-patient environment

The system has been verified for compatibility, and compliance for connection to a local area network (LAN) via a wire LAN, provided the LAN components are IEC/EN 60601-1 compliant.

General precautions for installing an alternate off-board, remote device or a network would include:

- The added device(s) must have appropriate safety standard conformance and CE Marking.
- The added device(s) must be used for their intended purpose having a compatible interface.

CAUTION: Make sure using ONLY the dedicated USB disk or removable media to save or back up data. Before connecting to the ultrasound system, make sure using the latest antivirus software on the USB disk or removable media to clean any virus. It is user's responsibility to ensure the USB disk or removable media is virus-free. Improper use of USB disk or removable media may cause the virus infections of system and eventually malfunction may occur. Such malfunction may impact the stability, effectiveness and safety of the system and probes, and users should immediately stop using the system and probes until CHISON authorized engineer has checked the system and confirm the effectiveness and safety of the system and probes.

CAUTION: Use only secure Local Area Network connection. Don't connect the ultrasound system to Internet. Make sure your hospital's firewall software is configured correctly, thus blocking incoming connection requests from Internet. Improper use of network connection may cause the virus infections of system and eventually malfunction may occur.

2.5 Biological Safety

This product, as with all diagnostic ultrasound equipment, should be used only for valid reasons and should be used both for the shortest period of time and at the lowest power settings necessary (ALARA - As Low As Reasonably Achievable) to produce diagnostically acceptable images. The AIUM offers the following guidelines:

Clinical Safety Quoted from AIUM

Approved March 26, 1997

Diagnostic ultrasound has been in use since the late 1950s. Given its known benefits and recognized efficacy for medical diagnosis, including use during human pregnancy, the American Institute of Ultrasound in Medicine herein addresses the clinical safety of such use:

There are no confirmed biological effects on patients or instrument operators caused by exposures from present diagnostic ultrasound instruments. Although the possibility exists that such biological effects may be identified in the future, current data indicate that the benefits to patients of the prudent use of diagnostic ultrasound outweigh the risks, if any that may be present.

Heating: Elevating tissue temperature during obstetrical examinations creates medical concerns. At the embryo development stage, the rise in temperature and the length of time exposed to heat combine to determine potential detrimental effects. Exercise caution particularly during Doppler/Color exams. The Thermal Index (TI) provides a statistical estimate of the potential temperature elevation (in centigrade) of tissue temperature. Three forms of TI are available: Soft Tissue Thermal Index (TIS), Bone Thermal Index (TIB) and Cranial Bone Thermal Index (TIC).

Soft Tissue Thermal Index (TIS). Used when imaging soft tissue only, it provides an estimate of potential temperature increase in soft tissue.

Bone Thermal Index (TIB). Used when bone is near the focus of the image as in the third trimester OB examination, it provides an estimate of potential temperature increase in the bone or adjacent soft tissue.

Cranial Bone Thermal Index (TIC). Used when bone is near the skin surface as in transcranial examination, it provides an estimate of potential temperature increase in the bone or adjacent soft tissue.

<u>Cavitations:</u> Cavitations may occur when sound passes through an area that contains a cavity, such as a gas bubble or air pocket (in the lung or intestine, for example). During the process of cavitations, the sound wave may cause the bubble to contract or resonate. This oscillation may cause the bubbles to explode and damage the tissue. The Mechanical Index (MI) has been created to help users accurately evaluate the likelihood of cavitations and the related adverse effects.

MI recognizes the importance of non-thermal processes, cavitations in particular, and the Index is an attempt to indicate the probability that they might occur within the tissue.

2.6 Scanning Patients and Education

The Track-3 or IEC60601-2-37 output display standard allows users to share the responsibility for the safe use of this ultrasound system. Follow these usage guidelines for safe operation:

- In order to maintain proper cleanliness of the probes, always clean them between patients.
- Always use a disinfected sheath on all EV/ER probes during every exam.
- Continuously move the probe, rather than staying in a single spot, to avoid elevated temperatures in one part of the patient's body.
- Move probe away from the patient when not actively scanning.
- Understand the meaning of the TI, TIS, TIB, TIC and MI output display, as well as the relationship between these parameters and the thermal/cavitation bio effect to the tissue.
- Expose the patient to only the very lowest practical transmit power levels for the shortest possible time to achieve a satisfactory diagnosis (ALARA As Low As Reasonably Achievable).

2.6.1 Safe Scanning Guidelines

- Ultrasound should only be used for medical diagnosis and only by trained medical personnel.
- Diagnostic ultrasound procedures should be done only by personnel fully trained in the use of the equipment, in the interpretation of the results and images, and in the safe use of ultrasound (including education as to potential hazards).
- Operators should understand the likely influence of the machine controls, the operating mode
 (e.g. B mode) and probe frequency on thermal and cavitation hazards.
- Select a low setting for each new patient. Output should only be increased during the examination if penetration is still required to achieve a satisfactory result, and after the Gain control has been moved to its maximum value.
- Maintain the shortest examination time necessary to produce a useful diagnostic result.
- Do not hold the probe in a fixed position for any longer than is necessary. The frozen frame and
 Cine loop capabilities allow images to be reviewed and discussed without exposing the patient to
 continuous scanning.

- Do not use endo-cavitary probes if there is noticeable self heating of the probe when operating in the air. Although applicable to any probe, take particular care during trans- vaginal exams during the first eight weeks of gestation.
- Take particular care to reduce output and minimize exposure time of an embryo or fetus when the temperature of the mother is already elevated.
- Take particular care to reduce the risk of thermal hazard during diagnostic ultrasound when exposing: an embryo less than eight weeks after gestation; or the head, brain or spine of any fetus or neonate.
- Operators should continually monitor the on-screen thermal index (TI) and mechanical index (MI) values and use control settings that keep these settings as low as possible while still achieving diagnostically useful results. In obstetric examinations, TIS (soft tissue thermal index) should be monitored during scans carried out in the first eight weeks after gestation, and TIB (bone thermal index) thereafter. In applications where the probe is very close to bone (e.g. trans-cranial applications), TIC (cranial bone thermal index) should be monitored.

MI> 0.3 there is a possibility of minor damage to neonatal lung or intestine. If such exposure is necessary, reduce the exposure time as much as possible.

MI> 0.7 there is a risk of cavitations if an ultrasound contrast agent containing gas micro-spheres is being used. There is a theoretical risk of cavitations without the presence of ultrasound contrast agents. The risk increases with MI values above this threshold.

TI> 0.7 the overall exposure time of an embryo or fetus should be restricted in accordance with **Table 2-2 below as a reference:**

TI	Maximum exposure time (minutes)
0.7	60
1.0	30
1.5	15
2.0	4
2.5	1

Maximum recommended exposure times for an embryo or fetus

• Non-diagnostic use of ultrasound equipment is not generally recommended. Examples of

non-diagnostic uses of ultrasound equipment include repeated scans for operator training, equipment demonstration using normal subjects, and the production of souvenir pictures or videos of a fetus. For equipment of which the safety indices are displayed over their full range of values, the TI should always be less than 0.5 and the MI should always be less than 0.3. Avoid frequent repeated exposure of any subject. Scans in the first trimester of pregnancy should not be carried out for the sole purpose of producing souvenir videos or photographs, nor should their production involve increasing the exposure levels or extending the scan times beyond those needed for clinical purposes.

Diagnostic ultrasound has the potential for both false positive and false negative results.
 Misdiagnosis is far more dangerous than any effect that might result from the ultrasound exposure.
 Therefore, diagnostic ultrasound system should be performed only by those with sufficient training and education.

2.6.2 Understanding the MI/TI Display

Track-3 follows the Output Display Standard for systems that include fetal Doppler applications. The acoustic output will not be evaluated on an application-specific basis, but the global maximum de-rated Ispta must be \leq 720 mW/cm² and either the global maximum MI must be \leq 1.9 or the global maximum de-rated Isppa must be \leq 190 W/cm². An exception is for ophthalmic use, in which case the TI=max (TIS_as, TIC) is not to exceed 1.0; Ispta.3 \leq 50mW/cm², and MI \leq 0.23. Track-3 gives the user the freedom to increase the output acoustic power for a specific exam, and still limit output acoustic power within the global maximum de-rated Ispta \leq 720 mW/cm² under an Output Display Standard.

For any diagnostic ultrasonic systems, Track-3 provides an Output Indices Display Standard. The diagnostic ultrasound systems and its operation manual contain the information regarding an ALARA (As Low As Reasonably Achievable) education program for the clinical end-user and the acoustic output indices, MI and TI. The MI describes the likelihood of cavitations, and the TI offers the predicted maximum temperature rise in tissue as a result of the diagnostic examination. In general, a temperature increase of 2.5°C must be present consistently at one spot for 2 hours to cause fetal abnormalities. Avoiding a local temperature rise above 1°C should ensure that no

thermally induced biologic effect occurs. When referring to the TI for potential thermal effect, a TI equal to 1 does not mean the temperature will rise 1 degree C. It only means an increased potential for thermal effects can be expected as the TI increases. A high index does not mean that bio effects are occurring, but only that the potential exists and there is no consideration in the TI for the scan duration, so minimizing the overall scan time will reduce the potential for effects. These operator control and display features shift the safety responsibility from the manufacturer to the user. So it is very important to have the Ultrasound systems display the acoustic output indices correctly and the education of the user to interpret the value appropriately.

RF: (De-rating factor)

In Situ intensity and pressure cannot currently be measured. Therefore, the acoustic power measurement is normally done in the water tank, and when soft tissue replaces water along the ultrasound path, a decrease in intensity is expected. The fractional reduction in intensity caused by attenuation is denoted by the de-rating factor (RF),

$$RF=10 (-0.1 a f z)$$

Where a is the attenuation coefficient in dB cm-1 MHz-1, f is the transducer center frequency, and z is the distance along the beam axis between the source and the point of interest.

De-rating factor RF for the various distances and frequencies with attenuation coefficient 0.3dB cm-1 MHz-1 in homogeneous soft tissue is listed in the following table. An example is if the user uses 7.5MHz frequency, the power will be attenuated by .0750 at 5cm, or 0.3x7.5x5=-11.25dB. The De- rated Intensity is also referred to as '.3' at the end (e.g. Ispta.3).

Distance	Frequency (MHz)			
(cm)	1	3	5	7.5
1	0.9332	0.8128	0.7080	0.5957
2	0.8710	0.6607	0.5012	0.3548
3	0.8128	0.5370	0.3548	0.2113
4	0.7586	0.4365	0.2512	0.1259
5	0.7080	0.3548	0.1778	0.0750

Distance	Frequency (MHz)			
(cm)	1	3	5	7.5
6	0.6607	0.2884	0.1259	0.0447
7	0.6166	0.2344	0.0891	0.0266
8	0.5754	0.1903	0.0631	0.0158

I'=I*RF Where I' is the intensity in soft tissue, I is the time-averaged intensity measured in water.

Tissue Model:

Tissue temperature elevation depends on power, tissue type, beam width, and scanning mode. Six models are developed to mimic possible clinical situations.

	Thermal Models	Composition	Mode	Specification	Application
1	TIS	Soft tissue	Unscanned	Large aperture (>1cm²)	Liver PW
2	TIS	Soft tissue	Unscanned	Small aperture (<1cm²)	Pencil Probe
3	TIS	Soft tissue	Scanned	Evaluated at surface	Breast color
4	TIB	Soft tissue and bone	Scanned	Soft tissue at surface	Muscle color
5	TIB	Soft tissue and bone	Unscanned	Bone at focus	Fetus head PW
6	TIC	Soft tissue and bone	Unscanned/scanned	Bone at surface	Transcranial

Soft tissue:

Describes low fat content tissue that does not contain calcifications or large gas-filled spaces.

Scanned: (auto-scan)

Refers to the steering of successive burst through the field of view, e.g. B and color mode.

Unscanned:

Emission of ultrasonic pulses occurs along a single line of sight and is unchanged until the transducer is moved to a new position. For instance, the PW, and M mode.

<u>TI:</u>

TI is defined as the ratio of the In Situ acoustic power (W.3) to the acoustic power required to raise tissue temperature by 1°C (Wdeg), TI=W.3/Wdeg.

Three TIs corresponding to soft tissue (TIS) for abdominal; bone (TIB) for fetal and neonatal cephalic; and cranial bone (TIC) for pediatric and adult cephalic, have been developed for applications in different exams.

An estimate of the acoustic power in milli-watts necessary to produce a 1°C temperature elevation in soft tissue is:

Wdeg=210/fc, for model 1 to 4, where fc is the center frequency in MHz.

Wdeg=40 K Dfor model 5 and 6, where K (beam shape factor) is 1.0, D is the aperture diameter in cm at the depth of interest.

MI:

Cavitation is more likely to occur at high pressures and low frequencies in pulse ultrasound wave in the tissue, which contains the bubble or air pocket (for instance, the lung, intestine, or scan with gas contrast agents). The threshold under optimum conditions of pulsed ultrasound is predicted by the ration of the peak pressure to the square root of the frequency.

MI=Pr'/sqrt(fc)

Pr' is the de-rated (0.3) peak rare-fractional pressure in Mpa at the point where PII is the maximum, and fc is the center frequency in MHz. PII is the Pulse Intensity Integral that the total energy per unit area carried by the wave during the time duration of the pulse. The peak rare- fractional pressure is measured in hydrophone maximum negative voltage normalized by the hydrophone calibration parameter.

Display Guideline:

For different operation modes, different indices must be displayed. However, only one index needs to be shown at a time. Display is not required if maximum MI is less than 1.0 for any setting of the operating mode, or if maximum TI is less than 1.0 for any setting of the operating mode. For TI, if the TIS and TIB are both greater than 1.0, the scanners need not be capable of displaying both

indices simultaneously. If the index falls below 0.4, no display is needed. The display increments are no greater than 0.2 for index value less than one and no greater than 1.0 for index values greater than one (e.g. 0.4, 0.6, 0.8, 1, 2, and 3).

Display and Report

Located on the upper middle section of the system display monitor, the acoustic output display provides the operator with real-time indication of acoustic levels being generated by the system.

For Scan

Only display and report MI, and start from 0.4 if maximum MI > 1.0, display in increments of 0.2.

Below is a simple guideline for the user when TI exceeds one limit exposure time to 4(6-TI) minutes based on the 'National Council on Radiation Protection. Exposure Criteria for Medical Diagnostic Ultrasound: I. Criteria Based on Thermal Mechanisms. Report No.113 1992'.

Operator Control Features:

The user should be aware that certain operator controls may affect the acoustic output. It is recommended to use the default (or lowest) output power setting and compensate using Gain control to acquire an image. Other than the output power setting in the soft-menu, which has the most direct impact on the power; the PRF, image sector size, frame rate, depth, and focal position also slightly affect the output power. The default setting is normally around 70% of the allowable power depending on the exam application mode.

Controls Affecting Acoustic Output:

The potential for producing mechanical bio effects (MI) or thermal bio effects (TI) can be influenced by certain controls.

Direct: The Acoustic Output control has the most significant effect on Acoustic Output.

Indirect: Indirect effects may occur when adjusting controls. Controls that can influence MI and TI are detailed under the bio effect portion of each control in the Optimizing the Image chapter.

Always observe the Acoustic Output display for possible effects.

Best practices while scanning

HINTS: Raise the Acoustic Output only after attempting image optimization with controls that have

no effect on Acoustic Output, such as Gain and STC.

WARNING: Be sure to have read and understood control explanations for each mode used before attempting to adjust the Acoustic Output control or any control that can affect Acoustic Output.

Use the minimum necessary acoustic output to get the best diagnostic image or measurement during an examination. Begin the exam with the probe that provides an optimum focal depth and penetration.

Acoustic Output Default Levels

In order to assure that an exam does not start at a high output level, the system initiates scanning at a reduced default output level. This reduced level is preset programmable and depends upon the exam icon and probe selected. It takes effect when the system is powered on or New Patient is selected. To modify acoustic output, adjust the Power Output level on the Soft Menu.

2.7 Battery Handling Instructions

CAUTION: Read and observe the following warnings and precautions to ensure correct and safe use of Li-ion batteries.

- Do not immerse the battery in water or allow it to get wet.
- Do not use or store the battery near sources of heat such as a fire or heater.
- Do not use any chargers other than those recommended.
- Do not reverse the positive (+) and negative (-) terminals.
- Do not connect the battery directly to wall outlets or car cigarette-lighter sockets.
- Do not put the battery into a fire or apply direct heat to it.
- Do not short-circuit the battery by connecting wires or other metal objects to the positive (+) and negative (-) terminals.
- Do not pierce the battery casing with a nail or other sharp object, break it open with a hammer, or step on it.
- Do not strike, throw or subject the battery to sever physical shock.
- Do not directly solder the battery terminals.

- Do not attempt to disassemble or modify the battery in any way.
- Do not place the battery in a microwave oven or pressurized container.
- Do not use the battery in combination with primary batteries (such as dry-cell batteries) or batteries of different capacity, type or brand.
- Do not use the battery if it gives off an odor, generates heat, becomes discolored or deformed, or appears abnormal in any way. If the battery is in use or being recharged, remove it from the device or charger immediately and discontinue use.
- Do not use or store the battery where is exposed to extremely hot, such as under window of a car in direct sunlight in a hot day. Otherwise, the battery may be overheated. This can also reduce battery performance and/or shorten service life.
- If the battery leaks and electrolyte gets in your eyes, do not rub them. Instead, rinse them with clean running water and immediately seek medical attention. If left as is, electrolyte can cause eye injury.

Chapter 3 System Introduction

3.1 Console View



Fig. 3-1 Console View

NOTE: The photograph above is EBit 60 for reference. The appearance of different modes please be subject to the actual product you have purchased.

3.2 Physical Specification

Dimensions of main unit (approx.): 358mm (Length) ×125mm (Width) ×399mm (Height)

Net weight of main unit (approx.): 7.8kg (no probe included)

3.3 External Interface View

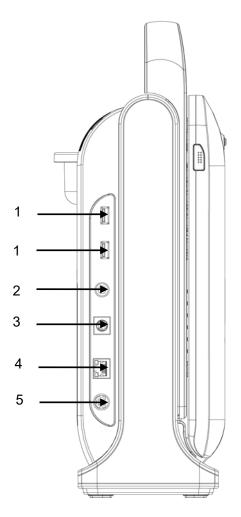


Fig. 2-2 System Left Side View

1. USB 2.0 2. FOOT SWITCH 3. S-VIDEO 4. Ethernet 5.Power in

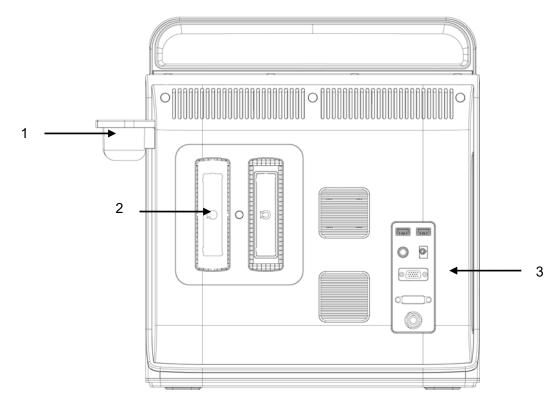


Fig. 3-3 Rear View

1.Probe Holder 2.Probe Ports 3.Rear External Interface

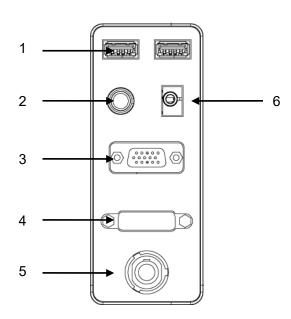


Fig. 3-4 Rear External Interface

1. USB 2.0 2.VIDEO OUT 3.VGA 4.DVI 5.ECG 6.REMOTE

3.4 Key System Features

No.	Key Features
1	Zoom and depth adjustment; Set the total gain, contrast, frequency band, 8
•	segments of STC, dynamic range, persistence.
2	256 gray-scale image display technology, Q-image technology, stable performance,
	high resolution.
	Image freezing and storage function; the stored images can be recalled for
3	analysis; Scanning direction can be changed and the image can be reversed in
	left/right, up/down direction.
	Distance, area, circumference, volume, fetal weight, heart rate etc. measurements
4	are available and automatic calculation of OB, cardiology are available. Direct
	display of gestation age and expected date of child delivery.
5	Elliptical method and tracing method are provided for area/circumference
	measurement.
6	Many kinds of body marks can be displayed together with corresponding probe
	position indication.
7	Display Patient ID, Time and Date according to the real-time clock.
0	Trackball available for operation and measurement. Characters can be input
8	directly by keyboard.
	Measure the percentage of stenosis, blood flow velocity, velocity ratio, blood flow
9	volume and pressure gradient. Automatically measure the values of maximum
	velocity, minimum velocity, time interval, pulsatility index and resistance index.
40	Possess multi-language interface display User interface change, shear plate,
10	printing, DICOM 3.0, biopsy guided functions.
	It has permanent storage for image and cine and HDD. It also can be connected to
11	removable storage via USB 2.0 port. To realize mass storage; can recall saved
	image for analysis.
12	Cine loop storage 256 frames real time image.

13	Screen rotation function make you adjust screen angle according to users' requirement; the adjustment range is 0~30°.		
14	Output standard PAL or NTSC video signal and VGA/DVI signal.		
15	Print or export graphic report.		

3.4.1 Image Modes

Mode	EBit 20	EBit 30	EBit 50	EBit 60
B Mode	Standard	Standard	Standard	Standard
2 B Mode	Standard	Standard	Standard	Standard
B/M Mode	Standard	Standard	Standard	Standard
M Mode	Standard	Standard	Standard	Standard
4B Mode	Standard	Standard	Standard	Standard
2D Steer	Option	Option	Option	Option
CFM Mode	Standard	Standard	Standard	Standard
CPA(PD) Mode	Standard	Standard	Standard	Standard
DPD Mode	Standard	Standard	Standard	Standard
PW Mode	Standard	Standard	Standard	Standard
Triplex Mode	Standard	Standard	Standard	Standard
CW Mode	Option	N/A	Option	Option
TDI	Option	N/A	Option	Option
Color M Mode	Option	N/A	Option	Option
Trapezoidal Mode	Standard	Standard	Standard	Standard
ECG	N/A	Option	Option	Option
B/BC Mode	Standard	Standard	Standard	Option
Super Needle	Option	Option	Option	Option
Elastography Mode	Option	Option	Option	Option
Free Steering M mode	Option	N/A	Option	Option
4D	N/A	Option	N/A	Option

Quadplex Mode	Option	Option	Option	Option
Curved Panoramic	Option	Option	Option	Option
Stress Echo	N/A	N/A	Option	Option

3.4.2 Accessories

Transducers:

Transducer	EBit 20	EBit 30	EBit 50	EBit 60
Convex transducer C3-E: 3.5MHz, 2.0-6.8MHz	Option	Option	Option	Option
Micro convex transducer V6-E: 6.0MHz, 4.0-12.0MHz	Option	Option	Option	Option
Linear transducer L12-E:12.0MHz,7.0-15. 0MHz	Option	Option	Option	Option
Micro convex transducer MC6-E: 6.0MHz,4.0-12.0MHz	Option	Option	Option	Option

Phased array transducer P3-E: 2.5MHz, 1.5-5.3MHz	Option	N/A	Option	Option
Linear transducer L7W-E: 7.5MHz,4.0-15.0MHz	Option	Option	Option	Option
Linear transducer L7-E: 7.5MHz, 4.0-15.0MHz	Option	Option	Option	Option
Micro convex transducer V7-E: 7.5MHz, 4.0-15.0MHz	Option	Option	Option	Option
Micro convex transducer MC3-E: 3.0MHz, 2.0-6.8MHZ	Option	Option	Option	Option

				T
Micro convex transducer MC5-E: 5.0MHz,4.0-10.7MHz	Option	Option	Option	Option
Phased array transducer P6-E: 6.0MHz, 2.0-8.0MHz	N/A	N/A	N/A	Option
Linear transducer L7R-E: 7.5MHz, 4.0-15.0MHz	Option	Option	Option	Option
Volume probe V4-EV: 4.5MHz, 2.0-6.8MHz	N/A	Option	N/A	Option

Peripherals

- S-VIDEO, VGA, DVI output for external monitor
- VIDEO output for B&W video printer
- LAN port output
- LAN for DICOM and image review station
- USB 2.0 for flash drive
- Foot Switch

AC/DC adapter: MENB1150A1949F03

Input: 100-240V~, 50-60Hz, 2.5A (2.5A-1.5A)

Output: +19V==7.8A

SL POWERTM and AULT®

Battery Pack: BT-2000 14.4V 9000Mah 130Wh, DONGGUAN YUNFAN ELECTRONICS

TECHNOLOGY CO., LTD

3.5 Installation Procedures

NOTE: Please do not turn on the power switch until finishing all the installation and necessary preparation.

3.5.1 Environment Condition

The system should be operated under the following environment.

3.5.1.1 Operation Environment Requirement

Ambient Temperature: 10 °C ~40 °C

Relative Humidity: 30%~75%RH

Atmospheric Pressure: 700hPa~1060hPa

Strong radiation sources or powerful electromagnetic waves (e.g. electro-magnetic waves from radio broadcasting) may result in image ghosting or noise. The system should be isolated from such radiation sources or electromagnetic waves.

To prevent damage to the system, do not use in the following locations:

- Exposed to direct sunlight
- Subject to sudden changes in temperature
- Dusty
- Subject to vibration
- Near heat generators
- High humidity

\triangle NOTE:

This equipment generates, uses and can radiate radio frequency energy. The equipment may cause radio frequency interference to other medical and non-medical devices and radio

communications. To provide reasonable protection against such interference, this product

complies with emissions limits for a Group 1, Class A Medical Devices Directive as stated in

IEC/EN 60601-1-2. However, there is no guarantee that interference will not occur in a particular

installation.

If this equipment is found to cause interference (which may be determined by turning the

equipment on and off), the user (or qualified service personnel) should attempt to correct the

problem by one or more of the following measure(s):

Reorient or relocate the affected device(s).

Increase the separation between the equipment and the affected device.

Power the equipment from a source different from that of the affected device.

Consult the point of purchase or service representative for further suggestions.

3.5.1.2 Transport and Storage Environmental Requirement

The following environmental transport and storage conditions are within system tolerances:

Temperature: -5° C ~ 40° C

Relative Humidity: ≤ 80% non-condensing

Atmosphere Pressure: 700hPa ~ 1060hPa

3.5.1.3 Electrical Requirements

Power Consumption: less than 150 VA

Voltage Fluctuation

riangleWARNING:

Maintain a fluctuation range of less than ±10% of voltage labeling on rear panel of the system,

otherwise the system may be damaged.

Grounding

Before connecting the power cable, connect the attached ground protection cable from

Equipotentiality terminal on system rear panel to a specialized grounding device.

NOTE:

✓ Please follow the outlined power requirements. Only use power cables that meet the system

Page 32

guidelines—failure to follow these procedures may produce system damage.

✓ Line power may vary in different geographic locations. Refer to the detailed ratings on the rear panel of the system for detailed information.

√ Battery

To avoid the battery bursting, igniting, or fumes from the battery; causing equipment damage, observe the following precautions: Do not immerse the battery in water or allow it to get wet. Do not put the battery into a microwave oven or pressurized container. If the battery leaks or emits an odor, remove it from all possible flammable sources. If the battery emits an odor or heat, is deformed or discolored, or in a way appears abnormal during use, recharging or storage, immediately remove it and stop using it. If you have any questions about the battery, short term (less than one month) storage of battery pack: Store the battery in a temperature range between 0 degrees C (32 degrees F) and 50 degrees C (122 degrees F).

Long term (3 months or more) storage of battery pack: Store the battery in a temperature range between-20 degrees C (-4 degrees F) and 45 degrees C (113 degrees F); Upon receipt of the EBit and before first time usage, it is highly recommended that the customer performs one full discharge/charge cycle. If the battery has not been used for >2 months, the customer is recommended to perform one full discharge/charge cycle. It is also recommended to store the battery in a shady and cool area with FCC (full current capacity). One Full Discharge/Charge Cycle Process:1. Full discharge of battery to let the EBit automatically shut down.2. Charge the EBit to 100% FCC (full current capacity).3. Discharge of Venue 40 for complete shutdown(takes one hour for discharge). When storing packs for more than 6 months, charge the pack at least once during the 6 month timeframe to prevent leakage and deterioration in performance.

3.5.1.4 Operation Space

Please leave enough free space from the back of the system to ensure well ventilation.

\triangle CAUTION:

Leave enough free space from the back of the system; otherwise, with the increasing of the temperature inside the unit, malfunction may occur.

3.5.1.5 System Positioning & Transporting

Moving the System

When moving or transporting the system, take the precautions described below to ensure maximum safety for personnel, the system and other equipment.

♦ Before Moving the System

- Press for 4 s, system will be forced to shut down and completely switch off the system.
- Disconnect all cables from off-board peripheral devices (external printer, etc.) from the console.

♠NOTE:

- ✓ To prevent damage to the power cord, DO NOT pull excessively on the cord or sharply bend the cord while wrapping it.
- ✓ Store all probes in their original cases or wrap them in soft cloth or foam to prevent damage.
- ✓ Replace gel and other essential accessories in the appropriate storage case.
- ✓ Ensure that no loose items are left on the console.

♦ When Moving the System

Carry the system with handle, or put the system on the cart to move it.

NOTE:

Walk slowly and carefully when moving the system.

Do not let the system strike walls or doorframe.

♦ Transporting the System

Use extra care when transporting the system in a vehicle. After preparing the system as described above, take the following additional precautions:

- Only use vehicles that are suitable for transport of the system.
- Before transporting, place the system in its original storage carton.
- Load and unload the system to a vehicle parked on a level surface.
- Load the unit abroad the vehicle carefully and over its center of gravity. Keep the unit still and upright.
- Ensure that the transporting vehicle can bear the weight of system plus the passengers.

- Secure the system firmly with straps or as directed within the vehicle to prevent movement during transport. Any movement, coupled with the weight of the system, could cause it to break loose.
- Drive carefully to prevent damage from vibration. Avoid unpaved roads, excessive speeds, and erratic stops or starts.

3.5.2 Powering the System

3.5.2.1 Acclimation Time

After being transported, the unit requires one hour for each 2.5 ° increment if its temperature is below 10 °C or above 40 °C.

\triangle NOTE:

Please keep at least 20 to 30 cm spare space away from the back of the system to ensure well ventilation. Otherwise, with the increasing of the temperature inside the unit, malfunction may occur.

3.5.2.2 Connecting the electric power

After making sure that the AC power supply in hospital is in normal status, and this AC voltage type matches to the power requirements indicated on the label of system, then please connect the plug of power cord to the POWER IN socket at the rear panel of the system, and connect the other end of power cord to the AC power supply socket in hospital.

Please use the power cable provided by the manufacturer, other type of power cable is not allowed.

Press , system boots up.

Press and system pops up dialog for shutting down. Click the enter key then system powers off.

Or press of for 4 s, system will be forced to shut down.

A CAUTION.

Connecting the system to the wrong AC power supply may cause damage to the system and

danger to the operators and animals.

3.5.3 Probe Installation

CAUTION: Please only use the probes provided by manufacturer for this model, other types of probes are not allowed to use with this system! Otherwise it may cause the damage to the system and the probe.

\triangle CAUTION:

Before connecting the probe, please carefully check the probe lens, probe cable and probe connector to see whether there is anything abnormal, such as cracks, falls off. Abnormal probe is not allowed to connect to the system; otherwise there is possibility of electricity shock.

- ✓ Hold the probe connector lock switch, and insert the connector socket vertically.
- ✓ Release the probe lock switch.
- ✓ Check the locked probe with one hand to make sure that it's not loose, and it's securely connected.

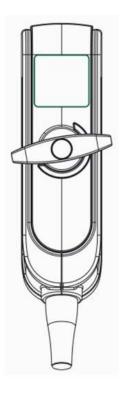


Fig. 3-5 Probe connector "Unlock" status

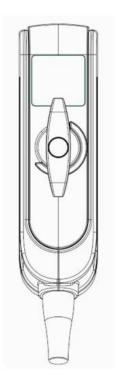


Fig. 3-6 Probe connector "Lock" status



✓ Only power supply at "turn off" state, can install/take-down the probe, otherwise it will damage the machine or the probe.

✓ When installing and disassembling probe, please put the probe head inside the probe holder, it can prevent the probe falling down to the ground.

3.5.3.1 Probe Disassembly

Turn the dead lock switch 90 degree in counterclockwise direction, extract probe connector plug vertically.

3.5.4 Accessories Installation

CAUTION: Please only use the optional parts provided or suggested by manufacturer! Using other types of optional devices may cause the damage to the system and the connected optional devices.

3.5.4.1 Video printer installation

- 1. Put video printer stably.
- 2. Connect cable of video printer to video port in the back of the device. And connect the other side to video signal output port in the rear side.
- 3. Connect the printer line to print control port in the printer rear side, and connect the other side to the print control port in the unit rear side.
- 4. Connect power cable of video printer to power system.
- 5. Adjust printer parameter preset according to the type of printing paper.

CAUTION: Do not use any other power cable to replace 3-wire power cable manufacturer provides, otherwise there is a danger of electric shock.

Video printer sign introduction

: Video signal input port
: Video signal output port
: Print control port
: Video printer switch

3.5.4.2 Graphic & PC printer installation

Put the printer stably; connect printer cable to USB port in the left side of the unit.

Connect the power cable of the printer to power system.

CAUTION: Please see packing list for fundamental configuration!

Chapter 4 Control Panel

4.1 Keyboard Appearance

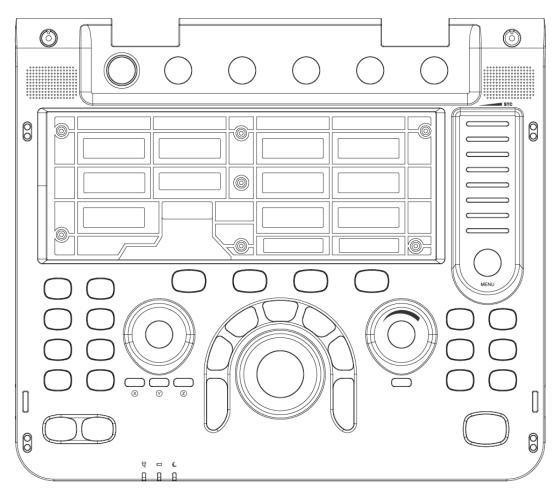


Fig. 4-1a keyboard appearance(Model: EBit Series)

4.2 Alphanumeric Keyboard

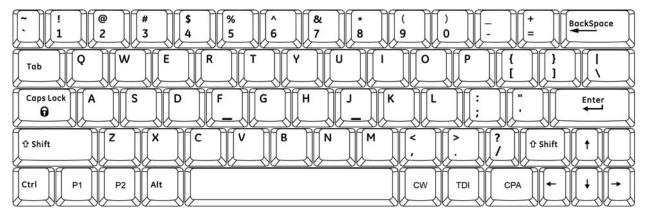


Fig. 4-2 Alphanumeric Keyboard

The alphanumeric keys are used for inputting patient number, name, character and figure etc.


4.3 Function Keys/Knobs

Key/knob Icon	Key/knob's name	Function description
	Switch	Turn on or off the device.
ŶŶ	Patient	Set up a new patient data, input name and other information.
A	Probe	Press this key for selecting probe. It can only select the connected probe.
	Review	File management of system, you can view and edit the patient's data.
5/2	Setup	Press this key to get in or out the system setting page.
	Report	Produce/Save/Recall an examination report.
EXIT	Exit	Press this key can exit measurement, dialog, and menu.
9	Zoom	Press this key to enter into image zoom.
4D/LIVE	4D/LIVE	Press this key to enter into 4D mode.
PRINT 1 PRINT 2	Print 1 & print 2	PRINT1: print the screen image by video printer connected to the system. PRINT2: print the report by printer connected to the system (Only report page works). Or print the image in the scanning page; Or print the image in the review page.
В	В	Display B mode.
C	С	Display CFM mode.
D	D	Display PW mode.
M	М	Display B/M mode. Press this key to change the mode between B/M and M.

Key/knob Icon	Key/knob's name	Function description
(X-CONTRAST)	X-CONTRAST	Press this key to activate the X-CONTRAST.
FHI	FHI	Press this key to open or close the FHI function.
ÎĻ	Up and Down Invert	Press this key to invert the image from up and down.
	Full screen	Press this key to enter into or quit full screen display mode.
	Cine	Press this key to save the current cine loop.
	Save	Press this key to save the current image.
***	Freeze	Press this key to freeze or unfreeze the current image.
MENU	Menu	Press the MENU knob for second time to select the item and adjust the parameters. Press this knob for third time to exit from current item. Rotate the MENU knob to select the item
GAIN	AIO_GAIN	Press the knob to activate AIO, automatic optimization image. Rotate the knob to adjust the gain of current mode.
DEPTH STEER ANGLE X Y Z	DEPTH_STEER_ANGLE	Press the knob to switch the knob function between depth, steer and angle. Rotate the knob to adjust the activated function. For 4D mode, rotate this knob to rotate image by X-axis, Y-axis and Z-axis.
ESC	ESC	This key's function is the same as key EXIT.
END	END	Press this key to finish the current exam.
	Bodymark	Press this key to enter into body mark working status, select the body mark and confirm the

Key/knob Icon	Key/knob's name	Function description
		probe scanning position on the screen.
ARROW	Arrow	Press this key to enter into arrow status. Add arrows icon to the image area.
	Comment	Press this key to enter into annotation status, and add annotations in the image area on the screen.
CLEAR	Clear	Press this key to clear all the measurement lines, body mark, and annotations.
	Biopsy	Press this key to activate biopsy.
	Single B	This key's function is the same as key B. Display B mode.
[AIA]	2B	Press this key to enter into 2B mode.
	4B	Press this key to enter into 4B mode.
	Volume	Press the volume key to adjust PW/CW volume.
SYS	SYS	The reserved key.
HELP	Help	The reserved key.
P1 P2	P1_P2	The reserved keys.
СРА	СРА	Press this key to enter into CPA mode.
TDI	TDI	Press this key to enter into TDI mode.
cw	CW	Press this key to enter into CW mode.

4.3.1 STC



STC can be used for adjusting gain compensation in different image depth.

4.3.2 Parameter Control Keys/Knobs












Increase/decrease the corresponding parameters of the screen, or open/close the function.

4.4 Central Control

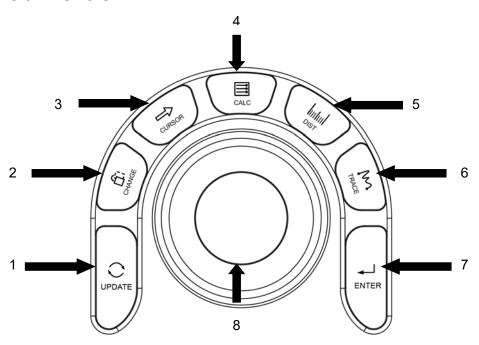

1. UPDATE 2.CHANGE 3.CURSOR 4.CALC 5. DIST 6.TRACE 7.ENTER 8.Trackball

Key/knob's name	Function description
-----------------	----------------------

	,
ENTER	This multifunction key is work with trackball. The function switches with the unit status. Such as, set the cursor position, body mark position, comment position, toggle trackball function, selected the menu, and confirm the input.
UPDATE	This multifunction key is work with trackball. The function switches with the unit status. Such as, call the annotation and back in measuring.
CURSOR	Press this key to show or hide the cursor.
CHANGE	Press this key to change the menu.
DIST	Press this key to enter into distance measurement.
TRACE	Press this key to enter into trace measurement.
CALC	Press this key to enter into measurement software package.
Trackball	Trackball is the main operation tool on screen. Position calipers in measurement, the function of the trackball is different under diverse working status.

4.5 Information Area Indicating Machine Status



Left-to-Right of the up row: hard disk, cable network, USB

- Hard disk: press this icon to show the capacity of disc to used save data or USB flash disk in current system
- Cable network: show the present situation of cable network; press this icon to show the IP address of current system.
- USB: show whether this system connects USB flash disk or not, press this icon to show USB safely remove interface.

Left-to-Right of the down row: input method, task queue, battery gauge

- Input method: press this icon to switch between uppercase and lowercase characters.
- Task queue: press this icon to show task and its situation. To terminate the task, delete, and so

on.

• Battery gauge: show the connecting situation of the battery, just press this icon to show the present State of charge and discharge, remaining electric quantity and available time.

Chapter 5 Operation and Exam Mode

This chapter mainly describes the process of the normal operation of the device, including the preparation before examination, how to get the image, optimize the image, add comments, body mark and so on.

5.1 Preparing the System for Use

The Device Inspection

- 1. The device is placed stability.
- 2. The grid voltage AC 100-240V, 50Hz-60Hz.
- 3. Cable is properly connected, firm and ground, the adapter is properly connected to the device.
- 4. Probe is connected and fixed.

Power On

Press to start the machine, wait for the system to enter the user interface, and then activate the probe into the B mode.

5.2 Choose Exam Mode

♦ The Probe Identification

The system default automatically identifies the current probe type, when the probe is inserted,

Press to switch the probe.

CAUTION: Please connect or disconnect the probe only after the system is freezing, in order to ensure stability and extend the service life of the probe.

♦ Mode Selection


In probe selection interface, probe and clinical application selection page is displayed, you can choose needed probe and inspection part, and press the default into the B mode, start scan detection.

NOTE: The system has been set clinical application preset before leaving factory, each probe has its own preset.

The detailed operation steps of the clinical application preset of the probe, please refer to the preset section.

5.3 Patient Data Entry

Press to display the Patient screen.

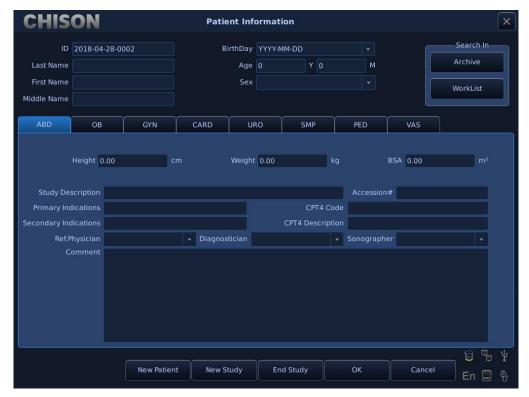

Function Buttons on Patient screen:

[Archive]: Operation on the patient information which has already existed.

[Worklist]: Recall patient information in worklist. And need to activate the DICOM function.

[New Patient]: Create a new patient information identity.

[New Study]: Choose exam applications (OB, GYN, CARD and so on) for the current patient.

[End Study]: End patient's exam item.

[OK]: Save patient's information.

[Cancel]: Cancel the operation of new patient's information.

Operation Methods:


- 1. Move the Trackball to the position of inputting character, and then input patient information by character keyboard.
- 2. Use the Trackball and the [ENTER] key to switch between different input options: ID, patient's

name, doctor's name, birthday (It can be automatically calculated when inputting age), age (It can be automatically calculated when inputting birthday), and gender.

- 3. Select the exam items, and input the regular inspection information.
- 4. After inputting the required information, click on the **[OK]** button to save the patient's information, the system will return to the B mode.
- 5. Recall information of the previous patient, you can use the Archive or Worklist to recall patient's information to exam.

CAUTION: Creating a diagnostic record, you should check the accuracy of the patient's information before saving measurement or image; otherwise, it will be stored in the wrong patient records. After checking the patient, press to save the patient's information in the system.

5.4 Image Interface Display

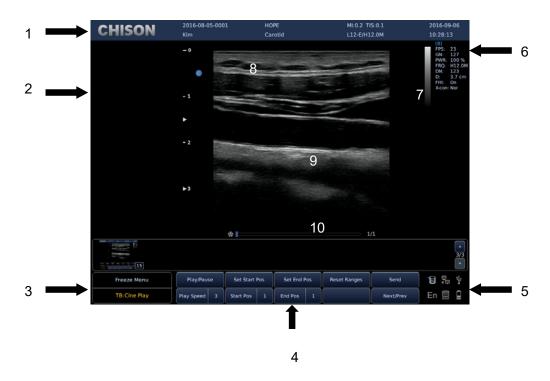

- 1, Logo 2, Control menu 3, Image status prompt 4, Image parameter area
 - 5, System state prompt 6, Image parameter area 7, Gray-scale strip
 - 8, Start point of scanning 9, Image Region 10, Cine loop

5.5 Image Modes

♦ B Mode

Press [B] key, and display the single B Mode image, B Mode is the basic mode for two-dimensional scanning and diagnosis.

2B Mode

Press [2B] key to display double B mode images side by side. One image is in real-time status; the other is in frozen status. The real-time image has start scan marker and ruler marker .Press [2B] key in 2B mode, the original active image is frozen while the original frozen image is activated.

In frozen status, Press [2B] to choose a B mode image to be activated when unfreezing the image.

◆ 4B Mode

Press **[4B]** key to enter into 4B mode, the screen will display four B mode images side by side, but only one image is in real-time status. Pressing it again can switch the real-time status among four images.

In frozen status, Press [4B] to choose a B mode image to be activated when unfreezing the image.

◆ B/M Mode

Press [M] key, a real time B mode image and a real-time M-mode image will be displayed at the same time. And a sample line will appear in the B mode image area, which indicates the active sample position for M image on the B image area. Move the sampling line by trackball.

M Mode

Press [M] key again, B mode image will disappear; M mode image is still active on the whole screen. M mode image stands for the tissue movement status at the sampling line. The M mode image varies with time, so it is mainly used for cardiac applications.

CFM Mode

CFM is a Doppler mode intended to add color-coded qualitative information concerning the relative velocity and direction of fluid motion within the B mode image.

CFM is useful to see flow in a broad area. It allows visualization of flow in the CROI, whereas Doppler mode provides spectral information in a smaller area. CFM is also used a stepping stone to Doppler mode. You can use CFM to locate flow and vessels prior to activating Doppler.

In CFM mode, move the trackball to change the position of sampling box. Activate the **[STEER]** knob and rotate the knob to adjust the angle of color sampling box (if current probe is linear probe). Press **[ENTER]** key to fix the position of color sampling box. At this time adjusts the size of color sampling box through moving trackball. Press **[ENTER]** key again and move trackball to change the color sampling position again.

Press [C] key to enter into CFM mode; after [C] key light is on, rotate the [GAIN] knob for adjusting the gain of CFM.

• CFM mode Exam Procedure:

- > Follow the same procedure as described under B mode to locate the anatomical area of interest.
- After optimizing the B mode image, add Color Flow.
- Move the color region of interest CROI as close to the center of the image as possible.
- > Optimize the color flow parameters so that a high frame rate can be achieved and appropriate flow velocity can be visualized.
- Press [FREEZE] key to hold the image in cine memory.
- Record color flow image as necessary.

CFM Scanning Hints:

- > PRF: increase/decrease the PRF on the color bar. Imaging of higher velocity flow requires increased velocity scale values to avoid aliasing
- ➤ Wall Filter: affect low flow sensitivity versus motion artifact
- ➤ Color Map: allow you to select a specific color map. It shows the direction of the flow and highlights the higher velocity flows.
- > Color Gain: amplify the overall strength of echoes processed in the CROI
- > Persistence: affect temporal smoothing and color Doppler 'robustness'.

◆ B/BC Mode

In active color mode, turn the **[B/BC]** item on to display a real B mode image at the right side of the screen and active Color mode image at the left side of the screen.

◆ CPA(PD) Mode

Power Doppler Imaging (PD) is a color flow mapping technique used to map the strength of the Doppler signal coming from the flow rather than the frequency shift of the signal. Using this technique, the ultrasound system plots color flow based on the number of reflectors that are moving, regardless of their velocity. PD does not map velocity; therefore it is not subject to aliasing.

Press [CPA] key to enter into the CPA mode.

Direction PD mode

In Power Doppler (CPA) mode, press **[MENU]** knob to pop up the PD Menu . Rotate **[MENU]** knob to select the DPD Mode and press **[MENU]** knob to enter into DPD mode.

If you need to go back to PD mode from DPD mode, you could press **[CPA]** key or select the PD mode item in the DPD mode.

PW Mode

Doppler is intended to provide measurement data concerning the velocity of moving tissues and fluids. PW Doppler lets you examine blood flow data selectively from a small region called the Sample Volume.

The X axis represents time while the Y axis represents velocity in either a forward or reverse direction.

PW Doppler is typically used for displaying the speed, direction, and spectral content of blood flow at selected anatomical sites.

PW Doppler can be combined with B mode for quick selection of the anatomical site for PW Doppler examination. The site where PW Doppler data is derived appears graphically on the B mode image (Sample Volume Gate). The Sample Volume Gate can be moved anywhere within B mode image.

PW mode Exam Procedure:

> Get a good B mode image. Press [C] key to help locate the vessel you wish to examine.

- Press [D] key to display the sample volume cursor and gate.
- ➤ Position the sample volume cursor by moving the Trackball left and right. Position or re-size the sample volume gate by moving the Trackball up and down, then press **[ENTER]** key.
- > Press [UPDATE] key to display PW Doppler spectrum and the system will run in combined B+Doppler mode. The Doppler signal can be heard through the speakers.
- > Optimize the PW Doppler spectrum as necessary.
- Ensure that the sample line is parallel to the blood flow.
- > Press to hold the trace in cine memory and stop imaging.
- > Perform measurements and calculations, as necessary.
- > Record results with your recording devices.
- > Press to resume imaging.
- > Repeat the above procedure until all relevant flow sites have been examined.
- Replace the probe in its respective holder.

When entering Duplex mode for the first time, the Doppler spectrum is not activated. The Doppler Sample Volume appears in the default position, and the B mode image or 2D (either B or Color) mode are active. Moving the Trackball will change the Sample Volume position. Press the **[ENTER]** key to toggle the Trackball function between Sample Volume Gate position and size. Press the **[UPDATE]** key after the Sample Volume Gate is defined to activate the Spectral Doppler mode. Press the **[UPDATE]** key for second time to toggle back to 2D (B or Color) update and deactivate the Spectral Doppler.

Doppler mode Scanning Hints:

The best Doppler data will be got when the scanning direction is parallel to the direction of the blood flow; when the scanning direction is perpendicular to the anatomic target, you can get the best B mode image, so you should keep the balance as you don't usually get both an ideal B mode image and ideal Doppler data simultaneously.

PRF: adjust the velocity scale to accommodate faster/slower blood flow velocity. Velocity scale determines pulse repetition frequency.

Wall Filter: remove the noise caused by vessel or heart wall motion at the expense of low flow

sensitivity.

Baseline: adjust the baseline to accommodate faster or slower blood flows to eliminate aliasing.

Angle: optimize the accuracy of the flow velocity. It estimates the flow velocity in a direction at an angle to the Doppler vector by computing the angle between the Doppler vector and the flow to be

measured. This is special useful in vascular applications where you need to measure velocity.

Doppler Gain: allow you to control the background information of spectral.

Sweep Speed: control speed of spectral update.

Doppler Sample Volume Gate Position and Size (Trackball and ENTER)

Move the sample volume on the B mode's Doppler cursor. The gate is positioned over a specific position within the vessel.

- To move Doppler cursor position, turn the trackball left or right until positioned over the vessel.
- To move sample volume gate position, move the trackball up or down until positioned inside the vessel.
- > To size sample volume gate, press [ENTER] key to toggle trackball function from sample volume gate positioning to sizing, then move the trackball to change sample volume gate size.

CW Mode

Continuous Wave Doppler allows examination of blood flow data all along the Doppler cursor rather than from any specific depth. Gather samples along the entire Doppler beam for rapid scanning of the heart. Range gated CW allows information to be gathered at higher velocities. It works with a phased array or pediatric probe.

If the velocity of the blood flow is even too high for the HPRF mode to detect, you have to try CW mode. Press [CW] key to enter CW mode when the probe supports CW mode.

◆ TDI Mode

TDI mode is tissue Doppler mode, which is intended to provide information of low-velocity tissue motion, specifically for cardiac movement. Only phased array probe is available for TDI function.

Color M Mode

Color M mode is used for fetal cardiac applications. Color flow overlays color on the M mode image using velocity and variance color maps. The color flow wedge overlays the B mode image and M mode timeline. The color flow maps available in M mode are the same as in CFM mode.

Color M mode is a Doppler mode intended to add color coded qualitative information concerning the relative velocity and direction of fluid motion within the M mode image.

If the system is in color mode and the probe supports Color M mode (e.g. phased array probe), press [M] key to enter Color M mode.

2D Steer

2D Steer is available for linear probes. It can steer the beam to obtain the left or right image and enlarge the area without to rotate the probes.

In B mode, press menu knob to pop up B Menu, adjust 2D Steer item to change 2D steer angle.

Trapezoidal Mode

Trapezoidal image is available for linear probes. In B mode, press menu knob to pop up B Menu, turn Trapezoidal Mode menu on to enter to Trapezoidal Mode.

◆ ECG

The ECG module is a device that provides the 3 lead ECG signal acquisition for cardiac application. It is not intent for the ECG diagnostic purpose as in the 12-lead module. In the cardiac application, the ECG trace is displayed on the bottom of the screen. For echo-stress, the R-wave triggering is used to gate or synchronize the image acquisition. The ECG has 3 leads: LL (left leg, RED), LA (left arm, BLACK), RA (right arm, WHITE). LA is for reference, which usually provides a bias voltage from the ECG module, and the LL, LA are the two signals from the body and going to the differential input of the ECG isolation amplifier.

◆ Biopsy and Super Needle

1. How to enter into Biopsy

Activate the [Biopsy] and press the [MENU] knob to show or hide biopsy line.

2. How to adjust the biopsy

After the biopsy line shows, press the **[ENTER]** key to activate the adjustment function of biopsy line, horizontal rolling the trackball can translate the biopsy line, vertical rolling the trackball can adjust the line angle, press the **[UPDATE]** key to set the default biopsy line position.

3. Super Needle

Super needle is used for enhance the needle image in the B mode image. After turning on the super needle, super needle and needle angle function will be active and user can adjust the needle angle to optimize the image for needle only (The angle is 5 degree per step.).

◆ Elastography Mode

Elastography shows the biological tissue elasticity properties with the ultrasound imaging system. It records the ultrasound signals before and after tissue distortion caused by applying external or internal forces. Based on the recorded signals, it analyzes, estimates and displays the strain of biological tissue.

In B mode, press **[MENU]** knob and turns elastography menu on to enter into elastography mode.

Curved Panoramic

Moving the probe to get a series of B mode images, Press and turn the menu on, select panoramic item, turn it on. The system will enter into Curved Panoramic mode.

Quadplex Mode

While in **B** mode, press **C**-knob and D-knob to access the **B+Doppler+Color** mode, turn Quadplex menu on to enter the Quadplex active mode.

4D Mode

4 D mode works with volume probe. When the 4D mode is available, press to enter the 4D mode. User can adjust the scanning range. Before entering the 4D interface, you can choose the 2D scanning range through ROI box. Assuming that the user's currently selected pitch direction scan angle is A, the system starts scanning from the -(A/2) angle and scans to the (A/2) angle. The range of each angle scan is determined by the ROI. ROI and pitch direction scanning angle together determine the scope of the three-dimensional scanning area.

Stress Echo

Stress Echo mode works with a phased array probe. Enter into menu and choose the Utility menu to select the Protocol item, press the menu knob to turn it on or off.

When the Protocol turns on, select the Default 4x4 template to start the study. User can also open the Timer1 for the study if needed. Save the cine for the study. After finishing the study,

enter into the Utility menu to select the Analyze to enter the Protocol Analyze interface. User can edit the Protocol Score for the study.

Free Steering M mode

Free steering M mode is only available on phased array probe. This mode can give you the ability to manipulate the cursor at different angle and position. The M-mode display changes as per the M cursor position.

At B/M mode status, press [MENU] knob and select [Free M] to turn on the Free Steering M mode.

Operation tips:

Angle

- Move trackball at horizontal direction to adjust the location of the angle line.
- Move trackball at vertical direction to adjust the point of steering angle. Select [Angle] and press [MENU] knob to activate the function. Then rotate [MENU] knob to adjust the direction of angle.

• Line Number

- > Select [Line Number], press and rotate [MENU] knob to add M line. User can add another 2 M lines at most.
- Press [UPDATE] knob to switch and activate between from different M lines.

5.6 Parameters Adjustment on Control Panel

Parameters' Name	Function description
Gain	In real status, rotate [GAIN] knob to adjust the Gain
STC	STC curves can be used for adjusting gain compensation in different image depth. Drag the slide of STC to adjust the value.
Depth	Press [DEPTH_STEER_ANGLE] selection knob until the indicator of [DEPTH] is lit, and then rotates the knob to change the depth of image.
Zoom	Press to appear the zoom box, press [UPDATE] key and move trackball to change the zoom ratio.

Parameters' Name	Function description
	B mode image and B/M mode image can be reversed horizontally and
Invert	vertically.
	Press (the displayed image is reversed in the up-down direction.
FHI	Press to turn on or off FHI function.
AIO	Press the [AIO] knob to activate the AIO function.
Full Screen Show	Full screen the image area. Press to activate the function; Press exit, or again to exit full screen show. When full screen shows, press [MENU] knob to show the menu of current mode (except bodymark, annotation, measurement).

5.7 B Image Menu & Parameters Adjustment

Menu & Parameters	Function description
Parameter control l	knobs
Freq	In real status, rotate the corresponding knob of [Freq] to adjust the frequency.
Dynamic	Dynamic range is used for adjusting the contrast resolution of B mode image and mode image, compressing or enlarging the display range of gray scale. At the real-time status, rotate the corresponding knob of [Dynamic] to adjust dynamic.
Focus Num	In B mode, 9 focus points can be selected simultaneously, and the number controlled by the depth, SRA and Compound. Rotate the corresponding knob of [Focus Num] to adjust.
Focus Pos.	Rotate the corresponding knob to change Focus Position.
Compound	In real status, rotate the corresponding knob of [Compound] to turn it on or off. The SRA can't be edited after opening the compound.
SRA	In real status, rotate the corresponding knob of [SRA] to turn it on or off.
Q-Image	In real status, rotate the corresponding knob of [Q-Image] to adjust.

Menu & Parameters	Function description
D	In real status, adjust the contrast and resolution.
Persistence	In real status, rotate the corresponding knob of [Persistence] to adjust.
	Scan Line Density function is only valid for the image in B mode, 2B mode,
	B/M mode or 4B mode image. The line density has two types: high density
Density	and low density. High density means better image quality while low density
	image has higher frame rate.
	Rotate the corresponding knob of [Density] adjust the line density.
	Adjust image gray scale inhibition parameters
B Rejection	Activate [B Rejection], and rotate [MENU] knob to adjust B Rejection
	parameters.
Menu	
Coop Width	Rotate the corresponding knob of [Scan Width] to adjust the scan width of
Scan Width	the corresponding size.
	Smoothness function is used for restraining the image noise and performing
Smooth	axial smooth processing to make the image smoother.
	Rotate the corresponding knob of [Smooth] to adjust.
Gamma	Adjust image gray value parameters. Choose [Gamma], and rotate [MENU]
Gamma	button to select the B Gamma parameters.
	Edge enhancement is used for enhancing the image outline. In this way the
Edge Enhance	user can view the tissue structure more clearly.
	Rotate the corresponding knob of [Edge Enhance] to adjust.
A Daway	Acoustic power means the acoustic power transmitting from the probe.
A Power	Rotate the corresponding knob of [A power] to adjust.
L/D Elia	Activate the [L/R Flip] and press the [MENU] knob to invert the image from
L/R Flip	left and right.
1 14:11:4.	This function includes post process, brightness and other items. Press
Utility	[MENU] knob, then choose Utility selection, it will appear Utility options.
Menus of Advance	
Zoom Coof	Adjust the size of the ruler.
Zoom Coef	Rotate the corresponding knob of [Zoom Coef] to adjust.
Tropozoidal Mada	Activate the [Trapezoidal Mode] and press the [MENU] knob to turn on or
Trapezoidal Mode	off the trapezoidal function.

Menu & Parameters	Function description
2D Steer	Activate the [2D Steer] and press the [MENU] knob to turn on or off the 2D
	Steer function.
ECG	Activate the [ECG] and press the [MENU] knob to turn on or off the ECG
ECG	function.
UD Invert	Activate the [UD Invert] and press the [MENU] knob to turn on/off the ECG
OD IIIvert	invert.
ECG Gain	Activate the [ECG GAIN] and rotate the [MENU] knob to increase or
LCG Gairi	decrease the ECG gain.
ECG Pos	Activate the [ECG POS] and rotate the [MENU] knob to set the ECG trace
LCG F0S	position.
ECG Velocity	Activate the [ECG Velocity] and rotate the [MENU] knob to set the ECG
LCG velocity	Velocity.
ECG Dyn	Activate the [ECG Dyn] and rotate the [MENU] knob to set the ECG
LCG Dyll	dynamic.
	Show or hide biopsy.
Biopsy	Activate the [Biopsy] and press the [MENU] knob to show or hide biopsy
	line.
Super Needle	Activate the [Super Needle] and press the [MENU] knob to turn on or off the
Super Needle	Super Needle function.
Needle Angle	Activate the [Needle Angle] and rotate the [MENU] knob to set the needle
	angle.
Center Line	Show or hide Center Line.
Octiver Lifte	Press the [MENU] knob to show or hide center line.
Elastography	Turn on or off the Elastography mode.

5.7.1 Utility Menu

This function includes post process, slide show and other items. Press **[MENU]** knob, then choose Utility selection, it will appear Utility options.

Menu & Parameters	Function description
Post Process	Chroma: Adjust the type of the chroma.
	Activate [Chroma], and rotate [MENU] knob to select the Chroma type.

Menu & Parameters	Function description
	2D Map: Select the type of the scale curve.
	Activate [2D Map], and rotate [MENU] knob to select the scale curve type.
	Gamma: Adjust image gray value parameters.
	Activate [Gamma], and rotate [MENU] knob to select the B Gamma
	parameters.
	B Rejection: Adjust image gray scale inhibition parameters
	Activate [B Rejection], and rotate [MENU] knob to adjust B Rejection
	parameters.
Brightness	Activate [Brightness], and rotate [MENU] knob to adjust the brightness of
	screen.
Slide show	Activate the [Slide show] to enter into slide show mode.
Keyboard Light	Activate the [Keyboard Light] to turn on/off the keyboard light.
Light Intensity	Activate [Light Intensity] and rotate [MENU] knob to select the light
	intensity.

5.8 M Image Menu & Parameters Adjustment

Menu & Parameters	Function description	
Parameter control knobs		
Speed	Rotate the corresponding knob of [Speed] to adjust M speed.	
M Chroma	Rotate the corresponding knob of [M Chroma] to select the Chroma type.	
Lavant	Rotate the corresponding knob of [Layout] to select the layout of B/M	
Layout	image.	
Menu		
M 2D Map	Rotate the corresponding knob of [M 2D Map] knob to select the scale	
	curve type.	
Utility	This function includes post process, brightness and other items. Press	
	[MENU] knob, then choose Utility selection, it will appear Utility options.	
Free M	Press [MENU] knob to turn on the Free M mode. Press [Exit] option to exit	
	from Free M mode.	
	Line Number: adjust the number of angle line.	
	Angle: adjust the direction of angle line.	

5.9 CFM/CPA/DPD/TDI Image Menu & Parameters

Menu & Parameters	Function description
Parameter control k	nobs
Freq	In real status, rotate the corresponding knob of [Freq] to adjust the
	frequency.
	Press [DEPTH_STEER_ANGLE] selection knob until the indicator of
Steer	[STEER] is lit, and then rotates the knob to change the steer of linear image
0.00.	ROI. Or rotate the corresponding knob of [Steer] to change the steer of
	linear image ROI.
Wall Filter	Rotate the corresponding knob of [Wall Filter] to adjust wall filter.
Color Map	Rotate the corresponding knob of [Color Map] knob to select the color type.
Coloi Map	(CFM mode only)
Q-flow	Press the corresponding knob of [Q-flow] to turn on or off the Q-flow
Q-110W	function.
PRF	Rotate the corresponding knob of [PRF] to Adjust PRF, adjustment range
110	depends on probe.
Color Invert	Press the corresponding knob of [Color Invert] to invert the color of flow.
Persistence	Rotate the corresponding knob of [Persistence] to adjust.
Q-beam	Press the corresponding knob of [Q-beam] to turn on or off the Q-beam
Q bouin	function.
Base Line	Adjust the position of baseline.
Badd Eirid	Rotate the corresponding knob of [Baseline] to change position of baseline.
Menu	
CF Mode	Activate [CF Mode], and rotate [MENU] knob to adjust CF mode, velocity or
	variance.
Wall Thre.	Activate [Wall Thre.], and rotate [MENU] knob to adjust wall thre
Blood Effection	Activate [Blood Effection], and rotate [MENU] knob to adjust blood
Blood Elicotion	effection, smooth or resolution.
Density	Rotate the corresponding knob of [Density] adjust the line density, high or
	low.
B/BC	Activate the [B/BC] and press the [MENU] knob to turn on or off the B/BC
	mode.

Menu & Parameters	Function description
Utility	This function includes post process, brightness and other items. Press
	[MENU] knob, then choose Utility selection, it will appear Utility options.

5.10 PW/CW Image Menu & Parameters

Function description		
Parameter control knobs		
In real status, rotate the corresponding knob of [Freq] to adjust the		
frequency.		
Rotate the corresponding knob of [Chroma] to select the Chroma type.		
Press parameter control key on [Wall Filter] to adjust wall filter.		
Adjust audio volume.		
Rotate the corresponding knob of [Audio] or press to adjust		
audio volume.		
Press the corresponding knob of [Triplex Mode] to turn on or off triplex		
mode.		
Rotate the corresponding knob of [PRF] to Adjust PRF, adjustment range		
depends on probe.		
Rotate the corresponding knob of [Speed] to adjust PW speed.		
Press parameter control key on Invert, or press key to invert spectrum.		
Adjust the position of baseline.		
Rotate the corresponding knob of [Baseline] to change position of baseline.		
Menu		
Rotate the corresponding knob of [2D Map] knob to select the 2D map.		
Activate [Spectrum Enhance] and rotate [MENU] knob to adjust spectrum		
enhance.		


Menu & Parameters	Function description
Dynamic Range	Activate [Dynamic Range] and rotate [MENU] knob to adjust dynamic
	range.
Utility	This function includes post process, brightness and other items. Press
	[MENU] knob, then choose Utility selection, it will appear Utility options.

5.11 Image and Cine Disposition

5.11.1 The Principle of Cine Storage

In real image status, the image can be stored in the movie memory in chronological order, maximum frames can be set. The maximum number of frames of the film storage can be set, please refer to preset chapter.

If the movie memory is full, the recent frame saved into memory, the previous frame removed from memory.



Cine loop indicate diagram

5.11.2 Manual Loop

Press to freeze image, pop cine playback bar, at this time, move trackball to play by hand.

5.11.3 Automatic Loop

After freezing image, press [Play/Pause] to play, press it again to stop.

Press **[ENTER]** key to choose the area of automatic playback area needed.

5.11.4 Loop Range Set

Rotate the corresponding knob of **[Start Pos]** and **[End Pos]** to set the loop start position and end position, the loop range settled.

Rotate the corresponding knob of [Reset Ranges] to reset the loop range to maximum.

5.11.5 Save and Recall Image

Press to save current image, the image will be displayed below the screen.

If you need to recall images that have been stored, move cursor to needed image, press **[ENTER]** key to recall it; or you can recall archived patient's information to recall image, please refer to archive chapter.

5.11.6 Save and Recall Cine


In freeze status, press to save cine, then it will be displayed below the screen, move cursor to needed cine, press **[ENTER]** key to recall cine.

5.11.7 Send image

After recalling the images, rotate the corresponding knob of **[Send]** to send images to USB flash disk, net storage, DICOM storage and print.

Hint1: Activate the DICOM before DICOM storage and print.

Hint2: Click the "Cine transform to AVI" to save the cines to AVI.

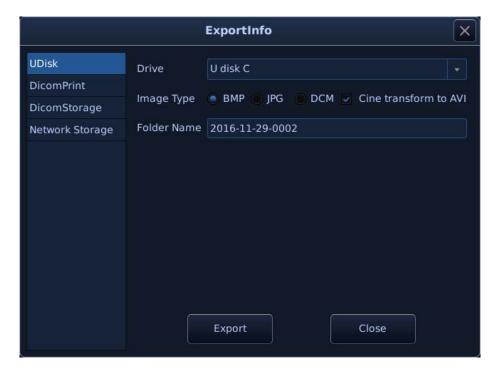

Sending Interface

5.12 Edit Comment

5.12.1 Overview

The comment is to enter text or symbols on the image.

- Enter COMMENT: Press enter into comments status; or input characters with alphanumeric keyboard, the system will enter into comments status too.
- Exit COMMENT: Press again or EXIT, ESC to exit.

Comment means input the words or symbols on images for making explanation. Add comments can through keyboard input directly or using the default comments.

The default comments are classified by examination mode as follows:

Classification	Function Description
Abdomen	Abdomen, general anatomy term
Obstetrics	Anatomy term of Obstetrics
Gynecology	Anatomy term of Gynecology
Heart	Anatomy term of Heart
Small Parts	Anatomy term of Small Parts
Pathological Change	Anatomy term of Pathological Change

NOTE: If you need to custom the default comments, refer to the preset section.

5.12.2 Input and Edit Comments

◆ Input characters

Operation:

- 1. Press, then system will go into the comment process; or input characters with alphanumeric keyboard, the system will enter into comments status too.
- 2. Move the cursor to the position where need to comment.
- 3. Input characters at cursor position by keyboard then press [ENTER] key to confirm.
- 4. Press again or EXIT, ESC to exit.

♦ Input Comment Library Characters

- 1. In comment status, move trackball to image area to edit.
- 2. Rotate the corresponding knob of **[Font size]** to adjust front size of comments, the range is 10~20.
- 3. Rotate [MENU] knob to select needed comments, then press [MENU] knob to exit.

♦ Input Quick Comments

- 1. Press **[Text]** to select needed quick comments.
- 2. Adjust front size of comments.
- 3. Press the corresponding knob of [Input] to place comments in the image area.

Edit Quick Comments

- 1. Rotate the corresponding knob of [Edit] to pop up quick comment edit box.
- 2. Input customized comments.
- 3. Press [Done] to finish edit, press [X] to cancel edit.

♦ Edit Comments

- 1. In comment status, move trackball to the comment, press [ENTER] key to activate it
- 2. Press [BACKSPACE] key to delete unnecessary characters.
- 3. Press **[ENTER]** key to confirm.

5.12.3 Move Comments

- 1. In comment status, move trackball to the comment, press [ENTER] key to activate it.
- 2. Move trackball to place the comment to target area.
- 3. Press [ENTER] key again to confirm the comment.

5.12.4 Delete Comments

Delete Characters

In comment status, activate the comment that need to be deleted, then press the **[ENTER]** key, it will display "|" on the screen, press **[BACKSPACE]** key to delete the character.

♦ Delete Single Comment

Activate the comment that needs to be deleted, press [Del] key to delete comment.

◆ Delete All Contents of the Comment

Don't activate the single comment; press to delete all characters that has inputted.

ACAUTION:

✓ Press [Clear] key, but it will delete the measurement and body mark at the same time.

5.12.5 Set the Position of Default Comment

Operation:

- 1. Press the corresponding knob of [Save Home Pos.] to move cursor to the initial position.
- 2. Press the corresponding knob of **[Load Home Pos.]** to set the initial position.

5.13 Set Body Mark

5.13.1 General Description


The body mark indicates patient's examination position and the direction of probe scan on the image.

Body marks are divided into: obstetric, abdomen, gynecology, heart and small parts, each has different body mark. Each type of body mark automatically is corresponding to current examination mode.

5.13.2 Body Mark Operation

Operation:

- 1. Press to enter into the body status.
- 2. Select the body mark that you need.
- 3. Move trackball after adding the body mark image and then adjust the position of probe. Rotate **[MENU]** or **[ANGLE]** knob can adjust the probe direction. Press **[ENTER]** key to confirm when adjustment was finished.

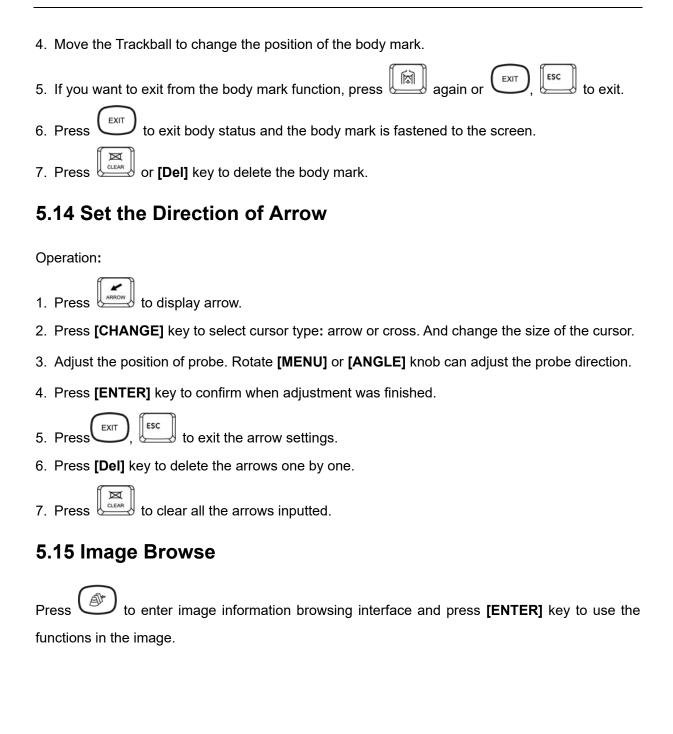




- ID: ID of Current patient.
- Name: Current patient's name.
- Information: Enter into current patient's information interface.
- Report: Enter into current patient's report interface.
- Send images: Send image to USB hard disk , DICOM storage and print.
- **Print images:** print the image which be chosen, it will be printed as the arrangement set.
- Delete images: Delete selected image.
- Row*Column: Select image's format.
- Pre page: Page up.
- Next page: Page back.
- Select All: Select all the images of this patient.
- Deselect All: Cancel to select all the images of this patient.
- New Exam: Exit current examination and open a new dialog box.
- Continue Exam: Exit image browsing interface and go on checking current patient.
- Archive: Open up archive management interface.
- Exit: Turn off image browsing interface.

5.16 Archive Management

Archive management can search for patient's information which has been stored in system. Press

and click [Archive] to archive management interface, all process can be opened up by moving cursor.

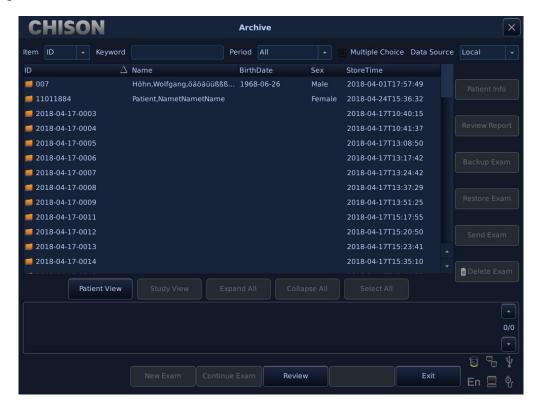

- Item: Type selection, select Patient's ID or Name.
- Keyword: Search for key words.
- **Period:** Time filter, select today, one week, one month, three months, six months, recent one year and all.
- Multiple Choice: Multiple choice.
- Data Source: Path choice, select hard disk or U disk.
- Patient info: Enter into patient's information interface.
- Review Report: Enter into report interface.
- Backup Exam: Select examination information to USB hard disk.
- Restore Exam: Recover examination information from USB hard disk.
- **Send Exam:** Send selected examination information remotely to USB hard disk or DICOM Storage/Print (Need to activate the DICOM).

- Delete Exam: Delete selected examination information.
- Patient View: Change display mode of information.
- Study View: Change different display mode of information.
- Expand All: Select Patient View, it will display sub-directory.
- Collapse All: Exit sub-directory.
- Select All: Select all examination information.
- New Exam: Exit current patient's examination.
- Continue Exam: Exit archive management interface and go on checking current patient.
- Edit Exam: Enter into the editing exam status of the selected examination.
- Review: Exit archive management interface and open up image browsing interface.
- Exit: Exit archive management interface and go on checking current patient.

5.17 Report

Move cursor to the images and press **[ENTER]** key to add the image into the report page. The report can be saved and printed. It is convenient for the doctor to view and edit the patient's information.

Reports contain normal report, abdominal report, cardiac report, small part report etc. Move the cursor to the required report page and press **[ENTER]** key to choose.

Press and the system pops up the report page of the current exam mode. Change the other exam mode report by the drop-down box.




- Report Title: Report options, different kinds of report can choose, such as General, OB/GYN etc.
- Hosp.: Display the hospital name.
- Cardiology Report: Display the kind of report.
- Patient Name: Display the patient name.
- Age: Display the patient age.
- Sex: Display the patient sex.
- Patient ID: Display the patient ID
- Diagnostic: Input the diagnostic instructions.
- **Description:** Input the description of symptom.
- Tips: Input note information.
- Clear All: Clear all the data including the selected status of the image, the result of the measurement etc.
- **Print:** Print the report with image.
- Export: Export the PDF report to the U disk.
- Save: Save the report in system.
- Exit: Press this key to exit the report function.

- The image on the right side: Press [ENTER] key on the image to add the image into the report.
- Select All: Press this key to add all the images on the right side into the report.
- Deselect All: Delete all the images added into the report.
- Input Template: Press this key to input report template.

5.18 DICOM

5.18.1 DICOM Worklist

Press [Worklist] button in Patient Interface, pop up the following dialog box

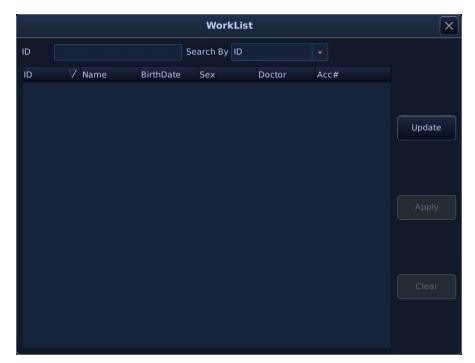


- ID: input ID or some characters, fuzzy query needs server.
- Search By: select term, ID or name.
- ID: display the ID of patients.
- Name: display the names of patients.
- BirthDate: display the birth date of patients.
- Sex: display sex of patients.
- Doctor: display names of doctors.
- Acc#: display the accession number of patients.
- **Update:** press this button to do search operation.

- **Apply:** select the searched patient and press this button , input all patient information into the new patient interface.
- Clear: clear all searched content.

5.18.2 DICOM Storage

Check the "Send while saving" in setting, then DICOM storage when saving cine and images.

Press send button in archive or freeze interface. DICOM Send interface as follows:

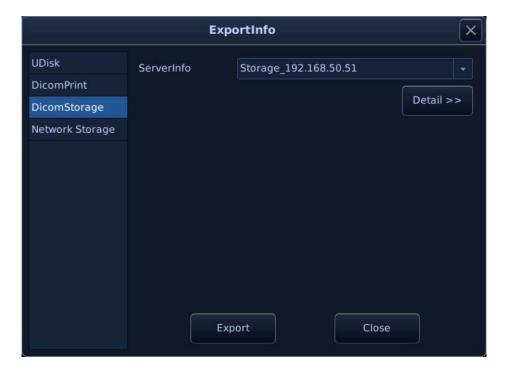

Select DICOM Storage in left, choose DICOM server and press Export button to DICOM storage.

Enter Task Queue and watch or edit DICOM process.

DICOM Print

DICOM Print operation is the same as DICOM storage.

5.18.3 DICOM SR

Press [Send DICOM SR] button in report interface, this task is added into Task Queue.

5.18.4 DICOM Print

DICOM Print operation is the same as DICOM storage.

Chapter 6 Measurement and Calculation

Main contents of this chapter:

Normal calculation and measurement on B mode image and M mode image, OB calculation and Urology measurement etc., system can enter into corresponding measurement mode depends on current exam mode, and enter into the corresponding report depends on the measurement mode. System has built-in the default measurement according to the exam mode, the change of measurement please refers to the chapter of preset settings.

ACAUTION:

Please select the most appropriate ultrasound images, measurement tools and measurement methods for measurements according to your diagnosis needs. The final measurement results must be determined and verified by a physician. Measurement accuracies are affected by many non-technical factors, for example operator's experience, patient's status. Please do not only use the ultrasound measurement results as the sole basis for diagnosis, please always use other clinical information to do integrated diagnostics.

6.1 Keyboard for Measurement

◆ Trackball

Trackball is used to move the cursor, main functions are as follows:

- 1. Before starting a measurement, use the trackball to choose the menu options.
- 2. After starting a measurement, move the trackball to move the cursor, during the measurement, the cursor should not be moved out image area.
- 3. During the Ellipse method measurement, use trackball to change the length of short axis.
- 4. Update the moving of the measurement result, move the trackball to change the position of the measurement result.

◆ [ENTER] key

During the measurement, the functions of [ENTER] key are as follows:

1. When cursor is on the menu, press the key to choose the options and start the measurement.

2. During the measurement, press the key to anchor the start point and end point.

♦ [UPDATE] key

- 1. Before the measurement, press **[UPDATE]** key to change the measurement method, such as ellipse, trace. The changeable measurement item has "< >".
- 2. During the measurement, **[UPDATE]** key is used to switch the start point and end point, long axis and short axis when the measurement is not finished.
- 3. During the distance measurement, press **[ENTER]** key to fix the start point, when the end point is not fixed, press **[UPDATE]** key to switch the start point and end point.
- 4. During the Ellipse measurement, when fix the long axis, but the short axis is not fixed, press **[UPDATE]** key to switch the long axis and short one.

♦ [CLEAR] key


Press to delete all the measurement results, comments and traces.

[Del] key


Press [Del] key to roll back the measurements step by step.

◆ [CHANGE] key

Press [CHANGE] to switch other menu.



♦ [Exit] key



♦ Parameters control key

Press the corresponding key to update the function and use the function.

6.2 B Mode Measurement

6.2.1 General Measurement Methods

The system B mode contains Distance, Ellipse, and Trace.

Distance

Measurement steps:

- 1. Press the **[CALC]** key to enter into measurement. Enter the **[distance]** item on the menu or press the quick measure key **[DIST]**, it will display a segment "+"icon.
- 2. Move the "+"icon by trackball to fit the one point of the line. Press **[ENTER]** key to fix the start point and the cursor can be moved to the next position.
- 3. Press [UPDATE] key can change the activated point, and fit the other point of the line.
- 4. Move the cursor to the end-point, press [ENTER] key again to complete the measurement.
- 5. After the measurement, the result will display in the measurement results area.
- 6. Repeat the steps from 1 ~ 4 to start next "distance" measurement.

NOTE:

✓ Each group of measurement is limited, if the measurement results beyond, it will begin a new group of measurement automatically.

♦ Ellipse

Measurement steps:

- 1. Press the **[CALC]** key to enter into measurement. Enter the **[Ellipse]** item on the menu; it will display a segment "+"icon.
- 2. Move the "+"icon by cursor, Press **[ENTER]** key to fix the point and the cursor can be moved to form a round.
- 3. Press [UPDATE] key can exchange the activated point and the fixed point.
- 4. Move the cursor to the end-point of the ellipse, press **[ENTER]** key to fix the axis, at the same time, the next axis be updated, and can change the size of the axis by the cursor.
- 5. Now press [UPDATE] key can exit to the step 4.

- 6. After fixing the next axis, can press [ENTER] key to complete the measurement.
- 7. After the measurement, the result will display in the measurement results area.
- 8. Repeat the steps from 1 ~ 6 to start next "ellipse" measurement.

<u>NOTE:</u>

✓ Each group of measurement is limited, if the measurement results beyond, it will begin a new group of measurement automatically.

◆ Trace

Measurement steps:

- 1. Press the **[CALC]** and **[CHANGE]** key to enter into General measurement. Update the **[Trace]** item in the menu or press the quick measure key **[TRACE]**, it will display a segment "+"icon.
- 2. Move the "+"icon by cursor, Press **[ENTER]** key to fix the point and the cursor can be moved to the next position.
- 3. Make the cursor tracing along the edge of required area, the traced line cannot be closed.
- 4. Now press [UPDATE] key to cancel the tracing.
- 5. Press **[ENTER]** key again in the endpoint, the start point and end point of trace line will be closed by a straight line.
- 6. After the measurement, the result will display in the measurement results area.
- 7. Repeat the steps from 1 ~ 5 to start next "trace" measurement.

MNOTE:

✓ Each group of measurement is limited, if the measurement results beyond, it will begin a new group of measurement automatically.

♦ Histogram

Histogram is used to calculate the gray distribution of the ultrasound echo signals within a specified area. Use the rectangle, ellipse or trace method to draw along the desired measurement area. The result is shown in the form of histogram.

Histogram can be measured only on the frozen image.

Measurement steps by rectangular method:

- $^{\prime\prime}$ to freeze the image.
- Press [CALC] and [CHANGE] to enter into the General measurement.
- Press [ENTER] key on [Histogram] menu to enter into measurement status.
- Press [ENTER] key to fix one apex of the rectangle.
- Move the trackball to change the cursor position and fix the diagonal point of the rectangle
- Move the trackball to change the cursor position, fix the diagonal point of the rectangle, and press [ENTER] key again to confirm the measurement area. The result will display on the measurement result area.
- Measure the histogram by ellipse or trace method: The method is the same as that to measure ellipse or trace method, press [UPDATE] key to change the measurement between ellipse and trace.

The horizontal axis represents the gray scale of the image ranging from 0 to 255.

The vertical axis represents the distribution ratio of each gray scale. The value shown on the top of vertical axis represents the percentage of the maximally distributed gray in the whole gray distribution.

Profile

Profile is used to measure the gray distribution of the ultrasound signals in the vertical or horizontal direction on a certain profile (section).

This measurement is only available in the frozen mode.

Measurement steps:

- to freeze the image.
- 2. Press [CALC] key, and choose [B General Meas.].
- 3. Draw a straight line at the measuring position. The method is the same as that to measure distance.
- 4. The calculated result of the profile will be displayed at the center of the screen.
- 1-The horizontal (or vertical) axis represents the projection of the profile line on the horizontal direction.
- 2-The vertical (or horizontal) axis represents the gray distribution of the corresponding points on

the profile line.

♦ Volume of A4CTrace method

A4CTrace tool is used to measure the cardiology item, Single Plane, Simpson BP etc. These measurements are used to calculate the volumes.

Measurement steps:

- 1. Press to freeze the image.
- 2. Press [CALC] key, and choose [Cardiology]. Activate an A4CTrace measurement such as Single Plane-EDV.
- 3. Move the cursor to a point and press [ENTER] key to set the start point, then move the cursor to next point and press [ENTER] key until the last point, and then set the straight line across the whole area.
- 4. The Volume of the chosen area will display on the measurement result area.

6.2.2 B Fast Measurement

Press **[DIST]** key to enter B Fast measurement in B mode. Press the corresponding parameter control key to switch the fast measurement item.

Meas. Menu	Submenu	Unit	Meas. Method/ Meas. Formula	Comment
	Distance	cm	Refer to Distance Meas.	
Distance	Ratio(Distance)		Refer to Distance Meas. Formula: R=D1/D2	D1: First Distance D2: Second Distance
	Angle	deg	Refer to Distance Meas.	Angle Range: 0°~ 180°
Area	Perimeter/Area	Area:c m² Perimet er: cm	Refer to Ellipse and trace meas.	Ellipse and trace.
	Ratio(Area)		Refer to ellipse Meas. Formula: R=A1/A2	A1: First Area A2: Second Area

Meas. Menu	Submenu	Unit	Meas. Method/ Meas. Formula	Comment
	Volume(1Distance)	ml	Refer to Distance Meas. Formula: V=(π/6)*D³	D means: Depth
	Volume(1Ellipse)	ml	Refer to ellipse meas. Formula: V=(π/6)*A*B ²	A: Long Axis B: Short Axis
Volume	Volume(2Distance)	ml	Refer to Distance Meas. Formula: V=(π/6)*D1*D2²	D1: the longer distance D2: the shorter distance
	Volume(3Distance)	ml	Refer to Distance Meas. Formula: V=(π/6)*D1*D2*D3	D1, D2, D3: Distance
	Volume(1Dis1Ellip)	ml	Refer to distance and ellipse Meas. Formula: V=(π/6)*A*B*M	A: Long Axis B: Short Axis M: Distance

6.2.3 B General Measurement

Press [B], [2B] or [4B] to enter into B, 2B or 4B mode, then click [CALC] key to enter into measurement status and press [CHANGE] to choose the General measurement.

Meas. Menu	Submenu	Unit	Meas. Method/ Meas. Formula	Comment
	Distance	cm	Refer to Distance	
	Distance	GIII	Meas.	
		Area:cm ²	Refer to Ellipse	Ellipse and trace.
	Perimeter/Area	Perimeter:	and trace meas.	Press [UPDATE] key to
		cm	and trace meas.	change.
General	Volume(1Distance)		Refer to Distance	
Measurement		ml	Meas.	D magna, Donth
Measurement		ml	Formula:	D means: Depth
			$V=(\pi/6)*D^3$	
			Refer to ellipse	
	\/olumo(1Ellings)	ml	meas.	A: Long Axis
	Volume(1Ellipse)	ml	Formula:	B: Short Axis
			V=(π/6)*A*B ²	

Meas. Menu	Submenu	Unit	Meas. Method/ Meas. Formula	Comment
	Volume(2Distance)	ml	Refer to Distance Meas. Formula: V=(π/6)*D1*D2 ²	D1: the longer distance D2: the shorter distance
	Volume(3Distance)	ml	Refer to Distance Meas. Formula: V=(π/6)*D1*D2*D3	D1, D2, D3: Distance
	Volume(1Dis1Ellip)	ml	Refer to distance and ellipse Meas. Formula: V=(π/6)*A*B*M	A: Long Axis B: Short Axis M: Distance
Ratio	Ratio(distance)		Refer to Distance Meas. Formula: R=D1/D2	D1: First Distance D2: Second Distance
Rallo	Ratio(area)		Refer to ellipse Meas. Formula: R=A1/A2	A1: First Area A2: Second Area
Angle		deg	Refer to Distance Meas.	Angle Range: 0°~ 180°
Histogram	_		Refer to Histogram	Press [UPDATE] key to change Rec, Ellips and Trace.
Profile			Refer to Profile	

6.2.4 B Abdomen Measurement

Choose Abdomen exam mode. Freeze the required image, then Press **[CALC]** key to enter into ABD measurement status. Or press **[CHANGE]** to choose the Abdomen measurement.

Meas. Menu	Submenu	Unit	Meas. Method/ Meas. Formula	Comment
Distance				
CBD			Refer to Distance Meas.	
GB wall		cm		
Liver Length				
Dray Aarta	Height	cm	Refer to Distance Meas.	
Prox Aorta	Width	cm	Refer to Distance Meas.	

Meas. Menu	Submenu	Unit	Meas. Method/ Meas. Formula	Comment
	StD%	%	Refer to Distance Meas. Formula: ((D1-D2)/D1)*100%	D1: Length of Normal D2: Length of Stenosis
	StA%	%	Refer to ellipse Meas. Formula: ((A1-A2)/A1)*100%	A1: Area of Normal A2: Area of Stenosis
	Vessel Area	cm ²	Refer to Ellipse and Trace Meas.	Ellipse and trace. Press [UPDATE] key to change.
	Vessel Distance	cm	Refer to Distance Meas.	
Mid Aorta	The same as above	The same as above	The same as above	The same as above
Distal Aorta	The same as above	The same as above	The same as above	The same as above
Spleen		cm	Refer to Distance Meas. Formula: V=(π/6)*L*H*W	L: Length H: Height W: Width
Renal Volume (Right/Left)		cm	Refer to Distance Meas. Formula: V=(π/6)*L*H*W	L: Length H: Height W: Width
	Height	cm	Refer to Distance Meas.	
	Width	cm	Refer to Distance Meas.	
	StD%	%	Refer to Distance Meas. Formula: ((D1-D2)/D1)*100%	D1: Length of Normal D2: Length of Stenosis
Lliac (Right/Left)	StA%	%	Refer to ellipse Meas. Formula:((A1-A2)/A1)*100%	A1: Area of Normal A2: Area of Stenosis
	Vessel Area	cm ²	Refer to Ellipse and Trace Meas.	Ellipse and trace. Press [UPDATE] key to change.
	Vessel Distance	cm	Refer to Distance Meas.	

6.2.5 B OB Measurement

Choose OB exam mode. Freeze the required image, then Press **[CALC]** key to enter into OB measurement status. Or press **[CHANGE]** to choose the OB measurement.

Meas. Menu	Submenu	Unit	Meas. Method	Comment
Distance				
GS				Formula to choose: CFEF, Campbell, Hadlock, Hansmann, Korean, Merz, Shinozuka
CRL		cm	Refer to Distance Meas.	Formula to choose: Hadlock, Hansmann, Korean, Nelson, Osaka, Rempen, Robinson, Shinozuka
BPD				Formula to choose: Bessis, CFEF, Campbell, Chitty, Hadlock, Hansmann, Jeanty, Johnsen, Korean, Kurtz, Merz, Osaka, Rempen, Sabbagha, Shinozuka
НС		cm	Refer to Ellipse and Trace Meas.	Formula to choose: CFEF, Campbell, Chitty, Hadlock, Hansmann, Johnsen, Korean, Merz
AC		cm	Refer to Ellipse and Trace Meas.	Formula to choose: CFEF, Campbell, Hadlock, Hansmann, Korean, Merz, Shinozuka
FL		cm	Refer to Distance Meas.	Formula to choose: Bessis, CFEF, Campbell, Chitty, Doubilet, Hadlock, Hansmann, Hohler, Jeanty, Johnsen, Korean, Merz, Osaka, Shinozuka
	YS			
	OFD			Formula to choose: Hansmann, Korean
	APD			Formula: Bessis
Fetal	TAD		Refer to Distance	Formula: CFEF
Biometry	FTA	cm	Meas.	Formula: Osaka
	SL			
	APTD			Formula: Hansmann
	TTD			Formula: Hansmann
	ThC			
Fetal Long	Humerus	om	Pofor to Diotor	Formula to choose: Jeanty, Korean, Merz, Osaka
Bones	ULNA	cm	Refer to Distance	Formula: Jeanty
	Tibia			Formula to choose: Jeanty, Merz

Meas. Menu	Submenu	Unit	Meas. Met	thod	Comment
	RAD				
	FIB				
	CLAV				Formula: Yarkoni
	CER				Formula to choose: Chitty, Hill
	СМ				
	NF				
	NT				
Fetal Cranium	OOD	cm	Refer to Distance Meas.	Distance	Formula: OOD
Cramum	IOD				
	NB				
	LVent				Formula: Tokyo
	HW				
	LtKid				
	RtKid				
00.00	LtRenalAP		Refer to	Distance	
OB Others	RtRenalAP	cm	Meas.		
	LVWrHEM				
	MAD				
AFI		cm	Refer to	Distance	AFI=AFI1+AFI2+AFI3+AFI4
\[\lambda_{\ \text{\color} \\ \		cm	Meas.		ALI-ALITAFIZTAFISTAFI4
CX_L		cm	Refer to	Distance	
O/L_E		5 /11	Meas.		

6.2.5.1 Twins and Multiple births Measurement

- 1.In the new patient OB page, choose the number of gestations from one to four.
- 2.In the measurement menu, press baby A, and then press **[ENTER]** key to switch babies, which could measure the babies separately.

6.2.5.2 EDD (estimated date of delivery) Estimation

- Calculating EDD by LMP (Last menstrual period)
- 1. In the new patient OB page, update the LMP input box.
- 2. Choose the LMP from the date dialog box or input the LMP date directly.
- 3. The calculated EDD value will appear in the result measurement area of OB page.
- Calculating EDD by BBT (Basal body temperature)

- 1. In the new patient OB page, update the Ovul.Date input box and input the bbt date.
- 2. The method is the same with the LMP method.

6.2.5.3 Growth curves

Function: Growth curves comparison is used to compare the measured data of the fetus with the normal growth curve in order to judge whether the fetus grows normally.

Measurement steps:

- 1. Finish the measurement of the OB item and get into the report page.
- 2. Choose the growth curve at the right list and press [ENTER] key to display the growth curve.
- 3. Choose the growth curve need to display, and check it to show the growth curve on report.
- 4. Click [*] icon on the dialog box to exit.

Tips: The abscissa of Growth curves is the gestational weeks calculated according to the LMP in patient information.

6.2.6 B Pediatrics Measurement

Select OB mode, press **[CALC]** to enter measurement, and then press **[CHANGE]** to switch to pediatrics measurement menu.

6.2.6.1 HIP Angle

HIP function is used for evaluating the fetal hip growth. In order to make calculation, three lines need to be added on the image, which is to conform to the fetal anatomic structure. The system will calculate and display two angles for doctor's reference.

Measurement steps:

- 1. Choose [HIP Angle] menu item, and click it to enter into measurement.
- 2. Click on the line image region, and appear one line with"+" .Move the line to the target measurement region.
- 3. Rotate [MENU] knob to adjust the line angle, press [ENTER] key to fix the line.
- 4. Then appear the second line, adjust the line according to the step 3, and fix the line.
- 5. Fix the 3 lines, the measurement result of the angle appears in the district.



- D 3 shows bias line between protruding of conjunction and acetabular bone
- D 2 shows direct line between osileum and acetabular bone
- D 1 shows base line between cotyle, joint purse, gristle periosteum and ilium.
- β is the angle between D1 and D2 (acute angle). α is the angle between D1 and D3 (acute angle).

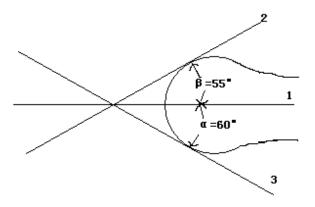


Fig. 6-1 HIP angle

6.2.7 B ORTH and Vascular Measurement

Refer to pediatrics measurement.

6.2.8 B GYN Measurement

GYN measurement includes measurement of UT-D (uterus diameter), ENDO (endometrium), CX-L (Uterine cervix length), LEFT OV and RIGHT OV (volume of left and right ovary) and LEFT FO and RIGHT FO (left and right follicle). The result will be calculated and displayed automatically on the screen by measuring relevant parameters.

Freeze the required image under GYN examination, then press [CALC] key to enter into GYN measurement status.

Meas. Menu	Submenu	Unit	Meas. Method/ Meas. Formula	Comment
Distance		cm	Refer to Distance Meas.	
	UT_L			
	CX_L		D () D' () M	
UT	UT_W	cm	Refer to Distance Meas.	
	UT_H			

Meas. Menu	Submenu	Unit	Meas. Method/ Meas. Formula	Comment
Cervix Vol.		ml	Refer to Distance Meas. Formula: V=(π/6)*L*H*W	L: Cervix_Length H: Cervix_Height W: Cervix_Width
ENDO		cm	Refer to Distance Meas.	
Ovary Volume (Left/Right)		ml	Refer to Distance Meas. Formula: V=(π/6)*L*H*W	L: Ovary_Length H: Ovary_Height W: Ovary_Width
	Follicle width Follicle height	cm cm	Refer to Distance Meas. Refer to Distance Meas.	
Follicle (Left/Right)	Follicle Volume	ml	Formula of 2 distance V= $(\pi/6)$ *A*B ² Formula of 3 distance V= $(\pi/6)$ *L*H*W	2distance A: the longer distance B: the shorter distance 3distance L: follicle length H: follicle height W: follicle width

6.2.9 B Small Parts Measurement

Freeze the required image under Small parts examination, then press **[CALC]** key to enter into small parts measurement status.

Meas. Menu	Submenu	Unit	Meas. Method/ Meas. Formula	Comment
Distance		Cm	Refer to Distance Meas.	
				L: Thyroid_
Thyroid		NAI	Refer to Distance Meas.	Length
Volume(Left/Right)		MI	Formula: V=(π/6)*L*H*W	H: Thyroid_Heigh
				W: Thyroid_Width
Angle		Dog	Defer to Distance Mass	Angle Range:
(Line1/Line2)		Deg	Refer to Distance Meas.	0°∼180°
Ratio			Defends Distance Mass	D1: First Distance
(Distance1/Distance2			Refer to Distance Meas.	D2: Second
)			Formula: R=D1/D2	Distance

6.2.10 B Urology Measurement

Normally urology measurements are performed in B and 2B mode.

Freeze the required image under Urology examination, then press **[CALC]** key to enter into Urology measurement status.

Meas. Menu	Submenu	Unit	Meas. Method/ Meas. Formula	Comment
Kidney			Refer to Distance Meas.	L: Kidney_L
Volume		MI	Formula:	H: Kidney_H
(Left/Right)			V=(π/6)*L*H*W	W: Kidney_w
	Vol.(L*W*H)		Refer to Distance Meas.	L: Bladder _L
Bladder	,	MI	Formula:	H: Bladder _H
	Vol.(Biplane)		V=0.497*L*H*W	W: Bladder _w
			Refer to Distance Meas.	L: Prostate _L
	Volume	MI	Formula:	H: Prostate _H
			V=(π/6)*L*H*W	W: Prostate _w
Prostate	PPSA	ng/ml	Formula:	
Prostate			PPSA=0.12*V	
				SPSA: input the SPSA
	PSAD	ng/ml	Formula: PSAD=SPSA/V	when create a new
				patient
			Refer to Distance Meas.	L: RVU_L
Residual	Volume	MI	Formula:	H: RVU_H
			V=0.7*L*H*W	W: RVU_w

6.2.11 B Cardiology Measurement

Normally cardiology measurements are performed in B and 2B mode.

Freeze the required image under Cardiac examination, then press [CALC] key to enter into Cardiac status.

NOTE: input the BSA when create a new patient.

Meas. Menu	Submenu	Meas. Method/ Meas. Formula	Comment
Teichholz	LVIDd LVIDs	Refer to Distance Meas. Formula: EDV=(7*LVIDd³)/(2.4+LVIDd) ESV=(7*LVIDs³)/(2.4+LVIDs) SV= EDV-ESV CO=SV*HR/1000 EF=SV/EDV*100 FS=(LVIDd-LVIDs)/LVIDd*100	
Single Plane	EDV(A2C/A4C) ESV(A2C/A4C)	SI=SV/BSA CI=CO/BSA Refer to Volume of A4CTrace method Formula:	
Simpson BP	EDV(A2C) ESV(A2C) EDV(A4C) ESV(A4C)	SV= EDV-ESV CO=SV*HR/1000 EF=SV/EDV*100 SI=SV/BSA CI=CO/BSA	
Modi Simpson	LVLd LVLs LVAMd LVAMs LVAPd LVAPs	Refer to Distance Meas. & Ellipse Mea. Formula: EDV= \[\frac{1 \text{VLYAMd}}{9} \times (4 \times \text{LVAMd} + 2 \times \text{LVAPd} + \sqrt{LVAMd} \times \text{LVAPd}) \] ESV= \[\frac{1 \text{LVLAMs}}{9} \times (4 \times \text{LVAMs} + 2 \times \text{LVAPs} + \sqrt{LVAMs} \times \text{LVAPs}) \] SV= EDV-ESV CO=SV*HR/1000 EF=SV/EDV*100 SI=SV/BSA CI=CO/BSA	
Cube	LVSd LVIDd LVPWd IVSs LVIDs LVPWs	Refer to Distance Meas. Formula: EDV=LVIDd³ ESV=LVIDs³ SV= EDV-ESV CO=SV*HR/1000 EF=SV/EDV*100 FS=(LVIDd-LVIDs)/LVIDd*100 SI=SV/BSA CI=CO/BSA	

Meas. Menu	Submenu	Meas. Method/	Comment
		Meas. Formula	
		Refer to Distance Meas.	
	LVLd	Formula:	
		EDV=(5/6.0)*LVLd*LVAMd	
Dullet Velume	LVLs	ESV=(5/6.0)*LVLs*LVAMs	
Bullet Volume	LVAMd	SV= EDV-ESV	
	LVAMs	CO=SV*HR/1000	
		EF=SV/EDV*100	
		SI=SV/BSA	
		CI=CO/BSA	
		Refer to Distance Meas.	
		Formula:	
		EDV=π/6*(0.98*LVIDd+5.9)*LVIDd*LVIDd	
		ESV=π/6*(0.98*LVIDs+5.9)*LVIDs*LVIDs	
Gibson	LVIDd	SV= EDV-ESV	
	LVIDs	CO=SV*HR/1000	
		EF=SV/EDV*100	
		FS=(LVIDd-LVIDs)/LVIDd*100	
		SI=SV/BSA	
		CI=CO/BSA	
	MV Diam	Refer to Distance Meas. & Ellipse Mea.	
Mitral Valve	MV Area	Formula:LA/AO=LAD/AOD	
	LA/AO		
Aortic Valve	AV Diam		
	AV Area		
Pulmonary	PV Diam		
Valve	PV Area		
Tricuspid	TV Diam	Refer to Distance Meas. & Ellipse Mea.	
Valve	TV Area	·	
LVOT	LVOT Diam		
	LVOT Area		
RVOT	RVOT Diam		
	RVOT Area		
RV/LV	RVIDd	Refer to Distance Meas.	
	LVIDd	Formula:RV/LV=RVIDd/LVIDd*100	
	PISA MR(Rad, Als Vel)		
PISA	PISA AR(Rad, Als Vel)	Refer to Distance Meas.	
1 10/1	PISA TR(Rad, Als Vel)	Formula:Flow Rate=2π*Rad*Rad*Als Vel	
	PISA PR(Rad, Als Vel)		

Meas. Menu	Submenu	Meas. Method/ Meas. Formula	Comment
LV Mass		Refer to Distance Meas. Formula: LV Mass=1.04*((LVSd+ LVIDd+ LVPWd)³- LVIDd³)-13.6 LV Mass Index=LV Mass/BSA Refer to Distance Meas. & Ellipse Mea. Formula: LVAd sax Epi × LVLd apical + LVAd sax Epi -	
	T-E(LVAd sax Epi, LVAd sax Endo, a, d)	Refer to Distance Meas. & Ellipse Mea. Formula: $1.05\pi \times \left\{ (b+t)^2 \left[\frac{2(a+t)}{3} + d - \frac{d^3}{3(a+t)^2} \right] - b^2 \left(\frac{2a}{3} + d - \frac{d^3}{3a^2} \right) \right\}$	
Qp/Qs	AV Diam PV Diam	Refer to Distance Meas.	

6.3 Measurement in M, B/M mode

- 1) At real-time status, press **[M]** key twice to enter M mode, press **[CALC]** key to enter into M mode measurement status.
- 2) At real-time status, click **[M]** key to enter B/M mode, press **[CALC]** key to enter into M mode measurement status.

6.3.1 Measurement Methods

◆ Distance

Measurement steps:

- 1. Select menu item [**Distance**] to enter into measurement.
- 2. Click on the M image area, it will display an orange dotted line with two horizontal short lines.

The orange dotted line represents the position need to be measured. The distance between the two short lines is the distance you want to measure. The yellow short line represents it's in active status. Click it and drag the short line to anywhere you want to put.

3. Press **[UPDATE]** key to activate the two short lines in turns and dragon them to change the distance between them. The measurement result will be displayed on the result area.

♦ Time

Measurement steps:

- 1. Select menu item **[Time]** to enter into measurement.
- 2. Click on the M image area, it will display two orange straight dotted line. The orange dotted line with one yellow short line on it represents it is in active status. The distance between the two straight lines stands for time you want to measure. You can drag the active straight line to anywhere you want to change the measured time.
- 3. Press **[UPDATE]** key to activate the two straight lines in turns and dragon them to change the distance between them. The measurement result will be displayed on the result area.

♦ Heart rate

Heart rate is used to calculate the number of heart beats per minute from cardiac image.

Measurement steps:

- 1. Choose [Heart Rate] menu item to enter into measurement.
- 2. The method is the same as Time.
- 3. After the above measurement, the calculated heart rate result is displayed in the measurement result area.
- 4. Repeat the steps form1 ~ 3 to start next measurement.

♦ <u>Velocity</u>

Measurement steps:

- 1. Click **[Velocity]** menu item to enter measurement condition.
- 2. Select the starting point and press **[ENTER]** key, the starting point and the removable cursor display, drag cursor to the end point.

- 3. Press **[ENTER]** key again, measurement completes, the result displays in the region of measurement
- 4. Repeat the steps from 1~3, and enter the next measurement of velocity.

NOTE: The maximum number of the measurement result on the image area is one. The second measurement result will cover the first one. The measurement result area will list all the measurement values.

6.3.2 General Measurement in M mode

At real time status, press [M] key twice to enter M mode, click [CALC] key to enter into M mode cardiology measurement status.

Meas. Menu	Submenu	Unit	Meas. Method/ Meas. Formula	Comment
Distance		Cm	Refer to M Distance Meas.	
Time		S	Refer to M Time Meas.	
Velocity		cm/s	Refer to M Velocity Meas.	
	One Cycle	Bpm	Refer to M Time Meas.	
Heart Rate	Double Cycles	Bpm	Refer to M Time Meas.	

6.3.3 M Cardiology Measurement

Freeze the required image under Cardiology examination, then press **[CALC]** key to enter into Cardiology measurement status. Or press **[CHANGE]** key to choose the cardiac measurement.

Meas. Menu	Submenu	Meas. Method/ Meas. Formula	Comment
Distance		Refer to M Distance Meas.	
Time		Refer to M Time Meas.	
Slope		Refer to M Velocity Meas.	

Meas.		Meas. Method/	
Menu	Submenu	Meas. Formula	Comment
Menu	Cube(LVSd, LVIDd, LVPWd, LVSs, LVIDs, LVPWs)	Refer to M Distance Meas. Formula: EDV=LVIDd³ ESV=LVIDS³ SV= EDV-ESV CO=SV*HR/1000 EF=SV/EDV*100 FS=(LVIDd-LVIDs)/LVIDd*100 SI=SV/BSA CI=CO/BSA Refer to M Distance Meas. Formula:	
Left Ventricle	Teichholz(LVIDd, LVIDs)	EDV=7*LVIDd³/(2.4+ LVIDd) ESV=7*LVIDs³/(2.4+ LVIDs) SV= EDV-ESV CO=SV*HR/1000 EF=SV/EDV*100 FS=(LVIDd-LVIDs)/LVIDd*100 SI=SV/BSA CI=CO/BSA	
	Gibson(LVIDd, LVIDs)	Refer to M Distance Meas. Formula: EDV=π/6*(.98*LVIDd+0.59)*LVIDd² ESV=π/6*(1.14*LVIDs+4.18)*LVIDs² SV=EDV-ESV CO=SV*HR/1000 EF=SV/EDV*100 FS=(LVIDd-LVIDs)/LVIDd*100 SI=SV/BSA CI=CO/BSA	
	IVSd/LVPWd		
	EPSS	Refer to M Distance Meas.	
	MV E Amp		
	MV A Amp		
Mitral	MV D-E Exc Dist		
Valve	MV E-F Slope	Refer to M Velocity Meas.	
	MV D-E Slope		
	A-C Int Slope	Defaute M Time M	
	E Duration	Refer to M Time Meas.	
	A Duration	Refer to M Time Meas.	

Meas. Menu	Submenu	Meas. Method/ Meas. Formula	Comment
	AOD		
	Ao Sinus Diam		
	Ao Asc Diam		
Aortio	Ao Arch Diam	Refer to M Distance Meas.	
Aortic Valve	Ao Desc Diam		
vaive	LVOT Diam		
	LAD		
	LVPEP/LVET	Refer to M Time Meas.	
	AA		
	RVOT Diam	Refer to M Distance Meas.	
Tuiscosial	RA Diam		
Tricuspid Valve	D-E Exc Dist		
vaive	E-F Slope	Refer to M Velocity Meas.	
	A-C Int Time		
	RVPEP	Refer to M Time Meas.	
Pulmonary	RVET	Refer to M Time Meas.	
Valve	A wave Amp	Refer to M Distance Meas.	
	B-C Slope	Refer to M Velocity Meas.	
D\//L\/	RVIDd	Pefer to M Dietanes Mass	
RV/LV	LVIDd	Refer to M Distance Meas.	

6.3.4 Other Measurement in M Mode

M Abdomen, OB, GYN, Urology, Small Parts, Pediatric and ORTH measurement refer to general measurement in M mode.

6.4 PW mode Measurement

Press [D] key to enter PW mode, and then press [CALC] key to enter PW mode measurement.

NOTE:

- ✓ In order to get accurate result, the PW image must be clear and high quality.
- ✓ Insure that you have fixed the cursor at the exact place of cardiac systole and diastole.

6.4.1 Measurement Methods

♦ Velocity

Measurement steps:

- 1. Select menu item [Velocity] to enter into measurement.
- 2. Click on the PW image area, the measurement result will be displayed on the result area.

◆ <u>Time</u>

Measurement steps:

- 1. Select menu item [Time] to enter into measurement.
- 2. Click on the PW image area, it will display two orange straight dotted lines. The orange dotted line with one yellow short line on it represents it is in active status. The distance between the two straight lines stands for time you want to measure. You can drag the active straight line to anywhere you want to change the measured time.
- 3. Press **[UPDATE]** key to activate the two straight lines in turns and drag them to change the distance between them. The measurement result will be displayed on the result area.

♦ Slope

Measurement steps:

- 1. Click [Slope] menu item to enter measurement condition.
- 2. Select the starting point and press **[ENTER]** key, the starting point and the removable cursor display, drag cursor to the end point.
- 3. Press **[ENTER]** key again, measurement completes, the result displays in the region of measurement
- 4. Repeat 1~3, and enter the next measurement of slope.

◆ Auto Trace

Measurement steps:

Move the trackball to select the start point of the one cycle and press [ENTER] key to fix it.

A second cursor "^" will appear, and move the trackball to the end point of the cycle, press **[ENTER]** key to fix it.

The measurement results will be displayed on the monitor and calculate other values of

parameters

♦ Manual Trace

Measurement steps:

- 1. Move the trackball to select the start point of the one cycle and press **[ENTER]** key to fix it.
- 2. Move the trackball along the spectrum and press **[ENTER]** key to complete.

The measurement results will be displayed on the monitor and calculate other values of parameters.

6.4.2 PW Fast Measurement

Press [**DIST**] key to enter PW Fast measurement in PW mode. Press the corresponding parameter control key to switch the fast measurement item.

Meas. Menu	Submenu	Unit	Meas. Method/ Meas. Formula	Comment
	Vs	cm/s	Refer to PW Slope Meas.	
	Pressure(s)	mmHg	Formula: Pressure=4*Vs*Vs/10000	
	Vd	cm/s	Refer to PW Slope Meas.	
Peak	Pressure(d)	mmHg	Formula: Pressure=4*Vd*Vd/10000	
	SD		Formula: SD=Vs/Vd	
	RI		Formula: SD=(Vs-Vd)/Vs	
	Time	s	Refer to PW Time Meas.	
HR	Single wave	bpm	Refer to PW Time Meas.	
	Vs	cm/s	Refer to PW Slope Meas.	
	Pressure(s)	mmHg	Formula: Pressure=4*Vs*Vs/10000	
	Vd	cm/s	Refer to PW Slope Meas.	
	Pressure(d)	mmHg	Formula: Pressure=4*Vd*Vd/10000	
At-	VMean	cm/s	Refer to PW Slope Meas.	
Auto Trace/Manual	Draggura () (Magn)	manal la	Formula:	
Trace/Manual	Pressure(VMean)	mmHg	Pressure=4*VMean*VMean/10000	
Trace	TVI	cm		
	SD		Formula: SD=Vs/Vd	
	RI		Formula: SD=(Vs-Vd)/Vs	
	PI		Formula: SD=(Vs-Vd)/VMean	
	HR(Single wave)	bpm		

6.4.3 PW General Measurement

Press [CALC] to enter PW measurement in PW mode. Press the corresponding parameter control key to switch the general measurement item.

Meas. Menu	Submenu	Unit	Meas. Method/ Meas. Formula	Comment
Velocity		cm/s	Refer to PW Slope Meas.	
Distance		cm	Refer to B Distance Meas.	
	Vs	cm/s	Refer to PW Slope Meas.	
	Pressure(s)	mmHg	Formula: Pressure=4*Vs*Vs/10000	
	Vd	cm/s	Refer to PW Slope Meas.	
Peak	Pressure(d)	mmHg	Formula: Pressure=4*Vd*Vd/10000	
	SD		Formula: SD=Vs/Vd	
	RI		Formula: SD=(Vs-Vd)/Vs	
	Time	s	Refer to PW Time Meas.	
	Vs	cm/s	Refer to PW Slope Meas.	
	Pressure(s)	mmHg	Formula: Pressure=4*Vs*Vs/10000	
	Vd	cm/s	Refer to PW Slope Meas.	
	Pressure(d)	mmHg	Formula: Pressure=4*Vd*Vd/10000	
	VMean	cm/s	Refer to PW Slope Meas.	
Trace <autotr ace=""></autotr>	Pressure(VMean)	mmHg	Formula: Pressure=4*VMean*VMean/10000	
	TVI	cm		
	SD		Formula: SD=Vs/Vd	
	RI		Formula: SD=(Vs-Vd)/Vs	
	PI		Formula: SD=(Vs-Vd)/VMean	
	HR(Single wave)	bpm		
	Distance1	cm	Refer to B Distance Meas.	
	Distance2	cm	Refer to B Distance Meas.	
StD%	StD%	%	Formula: StD%=((D1-D2)/D1)*100%	D1:Distance 1, D2:Distance 2
	Area1	cm ²	Refer to B Ellipse Meas.	
StA%	Area2	cm ²	Refer to B Ellipse Meas.	

Meas. Menu	Submenu	Unit	Meas. Method/ Meas. Formula	Comment
	0140/	%	Formula:	A1:Area1,A
	StA%	70	StA%=((A1-A2)/A1)*100%	2:Area2
	ICA	cm/s	Refer to PW Velocity Meas.	
	D (10 A)		Formula:	
	Pressure(ICA)	mmHg	Pressure=4*ICA*ICA/10000	
ICA/CCA	CCA	cm/s	Refer to PW Velocity Meas.	
	Pressure(CCA)	mmHg	Formula:	
			Pressure=4*CCA*CCA/10000	
	ICA/CCA		Formula: ICA/CCA	
	Diam	cm	Refer to B Distance Meas.	
	TVI	cm		
	Time	s	Refer to PW Time Meas.	
[] [] [] [] [] [] [] [] [] [] [] [] [] [HR(Single wave)	bpm		
Flow Volume	0)/		Formula:	
	SV	ml	SV=0.785*Diam*Diam* TVI	
		1/	Formula:	
	CO I/r	l/min	CO=SV*HR(Single wave)/1000	

6.4.4 PW OB Measurement

Press [CALC] key to enter PW measurement in PW OB mode. Or press the corresponding parameter control key to switch the OB measurement item.

Meas. Menu	Submenu	Unit	Meas. Method/ Meas. Formula	Comment
Umb A	Vs	cm/s	Refer to PW Trace Meas.	
Aorta,	Pressure(s)	mmHg	Formula: Pressure=4*Vs*Vs/10000	
Descending	Vd	cm/s	Refer to PW Trace Meas.	
Uterine	Pressure(d)	mmHg	Formula: Pressure=4*Vd*Vd/10000	
Artery(Lt),	VMean	cm/s	Refer to PW Trace Meas.	
Uterine	D		Formula:	
Artery(Rt),	Pressure(VMean)	mmHg	Pressure=4*VMean*VMean/10000	
Pulmonary	TVI	cm		
Artery,	SD		Formula: SD=Vs/Vd	
MCA	RI		Formula: SD=(Vs-Vd)/Vs	
Duct Veno	PI		Formula: SD=(Vs-Vd)/VMean	

Meas. Menu	Submenu	Unit	Meas. Method/ Meas. Formula	Comment
FHR	HR(Single wave)	bpm		

6.4.5 PW GYN Measurement

Press [CALC] to enter PW measurement in PW GYN mode. Or press the corresponding parameter control key to switch the GYN measurement item.

Meas. Menu	Submenu	Unit	Meas. Method/ Meas. Formula	Comment
	Vs	cm/s	Refer to PW Trace Meas.	
	Pressure(s)	mmHg	Formula: Pressure=4*Vs*Vs/10000	
	Vd	cm/s	Refer to PW Trace Meas.	
	Pressure(d)	mmHg	Formula: Pressure=4*Vd*Vd/10000	
Umb A,	VMean	cm/s	Refer to PW Trace Meas.	
MCA, Uterin A,	Pressure(VMean)	mmHg	Formula: Pressure=4*VMean*VMean/10000	
Fetal AO	TVI	cm		
1 Clai AO	SD		Formula: SD=Vs/Vd	
	RI		Formula: SD=(Vs-Vd)/Vs	
	PI		Formula: SD=(Vs-Vd)/VMean	
	HR(Single wave)	bpm		

6.4.6 PW Cardiology Measurement

Press [CALC] to enter PW measurement in PW cardiology mode. Or press the corresponding parameter control key to switch the cardiology measurement item.

Meas. Menu	Submenu	Unit	Meas. Method/ Meas. Formula
Velocity		cm/s	Refer to PW Velocity Meas.
Acceleration		cm/s ²	Refer to PW Slope Meas.
Time		s	Refer to PW Time Meas.
Slope		cm/s	Refer to PW Slope Meas.
HR(Single Wave)		bpm	Refer to PW Time Meas.
ED/PS	ED	cm/s	Refer to PW Velocity Meas.
	PS	011//3	Formular:RI=(ED-PS)/ED

	1	1	T
			Refer to PW Velocity Meas.
	MV E Vel	cm/s	Formular:MV E PG=4*MV E Vel*MV E Vel/10000 E/Ea=MV E Vel/Ea
			Refer to PW Velocity Meas.
			Formular:MV A PG=4*MV A Vel*MV A Vel/10000
	MV A Vel	cm/s	E/A=MV E Vel/MV A Vel
			A/E=MV A Vel/MV E Vel
			Refer to PW Trace Meas.
	NAN / N /TI		Formular:MV PGmax=4*MV Vmax*MV Vmax/10000
	MV VTI		MV PGmean=4*MV Vmean*MV Vmean/10000
			MV SV=0.785*MV Diam*MV Diam* MV VTI
			MR Fraction=MR Flow/MV SV*100
	MVA(PHT)		Formular:MV PHT=(-1)*0.3*VPeak/Slope
Mitral Valve			MVA PHT=220/MV PHT/1000
			Formular:
	MVA(VTI)		MV(VTI)=π* LVOT VTI*LVOT Diam*LVOT Diam /MV
			VTI/4
	MV E Dur	s	
	MV A Dur	s	Refer to PW Time Meas.
	MV DecT	s	
	MR Vmax	cm/s	Refer to PW Velocity Meas.
		CITI/S	Formula:MR PGmax=4*MR Vmax*MR Vmax/10000
	MR VTI		Refer to PW Trace Meas.
			Formula:MR PGmax=4*MR Vmax*MR Vmax/10000
			MR PGmean=4*MR PGmean*MR PGmean/10000
	dp/dt		Formula:dp/dt=32/Time
	IVRT	S	Refer to PW Time Meas.
	IVCT	s	relet to t w time mede.
	AV Vmax	cm/s	Refer to PW Velocity Meas.
	, tv viiiax	311.,0	Formular:AV PGmax=4*AV Vmax*AV Vmax/10000
			Refer to PW Trace Meas.
Aortic			Formular:AV PGmax=4*AV Vmax*AV Vmax/10000
	AV VTI		AV PGmax=4*AV Vmean*AV Vmean/10000
			AV SV=0.785*AV Diam*AV Diam* AV VTI
			AR Fraction=AR Flow/AV SV*100 Formular:
	AVA(VTI)		AVA(VTI)=π* LVOT VTI*LVOT Diam*LVOT
			Diam /AV VTI/4
			Diamp/W VII/T

			Defer to DW/\/alesity/Mage
	LVOT Verseur	/-	Refer to PW Velocity Meas.
	LVOT Vmax	cm/s	Formular:
			LVOT PGmax=4*LVOT Vmax*LVOT Vmax/10000 Refer to PW Trace Meas.
			Formular:
	LVOT VTI		LVOT PGmax=4*LVOT Vmax*LVOT Vmax/10000
			LVOT PGmax=4*LVOT Vmean*LVOT Vmean/10000
	LVPEP	s	
	LVET	S	Refer to PW Time Meas.
	AR Vmax	cm/s	Refer to PW Velocity Meas.
	7 11 7 7 7 7 7 7	511.,5	Formular:AR PGmax=4*AR Vmax*AR Vmax/10000
			Refer to PW Trace Meas.
	AR VTI		Formular:AR PGmax=4*AR Vmax*AR Vmax/10000
			AR PGmean=4*AR Vmean*AR Vmean/10000
	AR DecT	S	Refer to PW Time Meas.
	AR PHT		
	TV Vmax	cm/s	Refer to PW Velocity Meas.
	IV VIIIAX	CITI/S	Formular:TV PGmax=4*TV Vmax*TV Vmax/10000
	T./ E./ I	,	Refer to PW Velocity Meas.
	TV E Vel	cm/s	Formular:TV E PG=4*TV E Vel*TV E Vel/10000
			Refer to PW Velocity Meas.
		cm/s	Formular: TV A PG=4*TV A Vel*TV A Vel/10000
Tricuspid	TV A Vel		E/A=TV E Vel/TV A Vel
Valve			A/E=TV A Vel/TV E Vel
	T) (A () (T))		Formular:
	TVA(VTI)		TVA(VTI)= π * RVOT VTI*LVOT Diam*LVOT
			Diam /TV VTI/4
	RVSP		Formular: TR PGmax=4*TR Vmax*TR Vmax/10000
	TVOI		RVSP=RAP+4*TR Vmax*TR Vmax/10000
			Refer to PW Velocity Meas.
	RVOT Vmax		Formular:
			RVOT PGmax=4*RVOT Vmax*RVOT Vmax/10000
			Formular:
			RVOT PGmax=4*RVOT Vmax*RVOT Vmax/10000
Pulmonary	RVOT VTI		RVOT PGmax=4*RVOT Vmax*rvOT Vmax*rvOT
Valve			Vmean/10000
	PV Vmax	cm/s	Refer to PW Velocity Meas.
			Formular: PV PGmax=4*PV Vmax*PV Vmax/10000
			Formular:PV PGmax=4*PV Vmax*PV Vmax/10000
			PV PGmean=4*PV Vmean*PV Vmean/10000

ICI IIIUGA	ICT		1	
Tei Index	IRT		Refer to PW Time Meas.	
Qp/Qs	PV VTI		Refer to PW Trace Meas. Formular:PV SV=0.785*PV Diam*PV Diam/ PV VTI CO=PV SV*PV HR/1000 Qp/Qs Qp-Qs	
	AV VTI		Refer to PW Trace Meas. Formular:AV SV=0.785*AV Diam*AV Diam/ AV VTI CO=AV SV*AV HR/1000	
PISA	MR,AR,TR,PR		Refer to PW Trace Meas. Formular:EROA= Flow Rate/Vmax Flow=EROA/VTI Fraction=Flow/SV*100	
	PVein D VTI		Refer to PW Trace Meas.	
Velil	Pvein A Dur PVein S VTI		Refer to PW Time Meas.	
Vein	PVein A Vel PVein A Dur		Pofor to DW Time Mass	
Pulmonary	PVein D Vel		Refer to PW Velocity Meas.	
	PVein S Vel			
	PR PHT			
	PR VTI		Formular:PR PGmax=4*PR Vmax*PR Vmax/10000 PV PGmean=4*PR Vmean*PR Vmean/10000	
	FIX VIIIdX		Formular:PR PGmax=4*PR Vmax*PR Vmax/10000	
	PR Vmax		Refer to PW Velocity Meas.	
	RAEDP		RAEDP=RAP+4*PR Vmax*PR Vmax/10000	
			Formular:PR PGmax=4*PR Vmax*PR Vmax/10000	
	RVET	S	Refer to PW Time Meas.	
	RVPEP	6	LPA PGmax=4*LPA Vmax*LPA Vmax/10000	
	LPA Vmax	cm/s	Refer to PW Velocity Meas. Formular:	
	RPA Vmax	cm/s	Formular: RPA PGmax=4*RPA Vmax*RPA Vmax/10000	
			MPA PGmax=4*MPA Vmax*MPA Vmax/10000 Refer to PW Velocity Meas.	
	MPA Vmax	cm/s	Refer to PW Velocity Meas. Formular:	
			Diam /PV VTI/4	
	PVA(VTI)		PVA(VTI)=π* RVOT VTI*LVOT Diam*LVOT	
			Formular:	

	ET	Refer to PW Time Meas. Formular:Tei Index=(ICT+IRT)/ET
TDI	MV medial (Sa,Ea,Aa,ARa, DRa)	Refer to PW Velocity Meas. & Slope Meas.
	MV lateral (Sa,Ea,Aa,ARa)	

6.4.7 PW Vascular Measurement

Press [CALC] to enter PW measurement in PW vascular mode. Or press the corresponding parameter control key to switch the vascular measurement item.

Meas. Menu	Submenu	Unit	Meas. Method/ Meas. Formula
	Vs	cm/s	Refer to PW Slope Meas.
Subclavian A,	Pressure(s)	mmHg	Formula: Pressure=4*Vs*Vs/10000
Prox CCA,	Vd	cm/s	Refer to PW Slope Meas.
Mid CCA,	Pressure(d)	mmHg	Formula: Pressure=4*Vd*Vd/10000
Distal CCA,	VMean	cm/s	Refer to PW Slope Meas.
Bulb,	Pressure(VMean)	mmHg	Formula: Pressure=4*VMean*VMean/10000
Prox ICA,	TVI	cm	
Mid ICA, Distal ICA,	SD		Formula: SD=Vs/Vd
ECA,	RI		Formula: SD=(Vs-Vd)/Vs
Vertebral A	PI		Formula: SD=(Vs-Vd)/VMean
	HR(Single wave)	bpm	
	Diam	cm	Refer to PW Distance Meas.
	VTI	cm	
	Time	s	Refer to PW Time Meas.
Flow Volume	HR(Single wave)	bpm	
	SV	ml	Formula: SV=0.785*Diam*Diam* TVI
	СО	l/min	Formula: CO=SV*HR(Single wave)/1000

6.4.8 Other Measurement in PW Mode

PW Abdomen Urology, Small parts and Pediatric measurement refer to PW general measurement.

Chapter 7 Preset


This chapter introduces the operation to make settings of the system through preset menu at preset mode.

Preset function is used to set up working environment and status, parameters of each examination mode. The setting will be stored in the memory of system and not be lost even after the system is switched off. When the system is switched on, it will work automatically with the status which is required by the operator.

In preset interface, all operation relies on moving trackball to required Function key position. Press **[ENTER]** key to start the operation.

7.1 General setting

7.1.1 General Interface

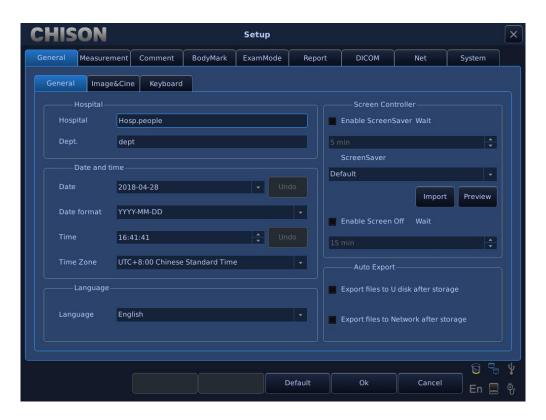


Press the [**SETUP**] to enter system setting interface. User can do user-defined setting.

Click [**X**] in the title bar or the exit key on the button can exit the system setting interface.

Function name	Setting method	Function description
Hospital, Department	Input freely	Set up the hospital name which is shown at top left corner of "General Setting" dialog box, 20 characters Max can be input.
Date and Time	Input freely	Set up the system date (calendar format), select current date directly. Date format can be changed by format setting.
Date Format	Set up freely	Set up date format: Year/Month/Date, Month/Date/Year, Date/Month/Year.
Time zone	Set up freely	Set up the working clock of the system.
Screen Controller	Select the function and set its start time	Enable screen saver, user can custom screen saver images, a custom picture named "screensaver", JPG, PNG, BMP format, size does not exceed 512 * 384 pixels.
Language	Select language	Select the language of operation interface(Simplified Chinese English and so on)
Auto Export	Select the need option	Select to export files to U disk or Network after storage.
Default	Press button	Recover all preset to factory setting.

7.1.2 Image & Cine setting

User can select Image&Cine option to set the screen type, parameters of image, cine or image area. See the following sheet 2 for detailed description.

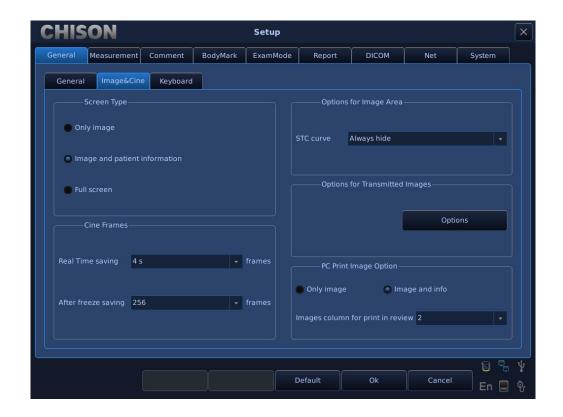

Function name	Setting method	Function description
Screen Type	Select the need type	Set the content which screen picture contain: only picture, image and patient information, full screen.
Cine Frames	Select the parameter	Set the default frame or time when saving the film.
Options for	Click the button to	Set the STC curve, including always shows, always hide
Image Area	open the setting box	and hide for 1 to 8 seconds.
Options for	Oliale that button to	Adjust the parameters of transmitted images:
Transmitted	Click the button to	brightness, contrast, and gamma and select the need
Images	open the setting box	image type.
PC Print Image	0-1	Including print area and arrangement condition in the
Option	Select the need option	image foresee interface.

7.1.3 Keyboard setting

Users can set the different functions for number keys and other optional buttons according to the using habits.




- **Key:** display the settable number keys and buttons and selected function.
- Output: including store images, store films, store images to U disk, store film to U disk, etc.
 function options.
- Image mode: including image full screen, biopsy, chroma, etc.
- Print: including video print, pc print etc.
- Measurement: including GS, CR, BPD, HC, AC, etc.
- Other: including arrow, archive.

7.2 Measurement

Measurement includes general measurement setting and measurement formula setting.


7.2.1 General measurement setting

General settings can only change the display of measurement unit.

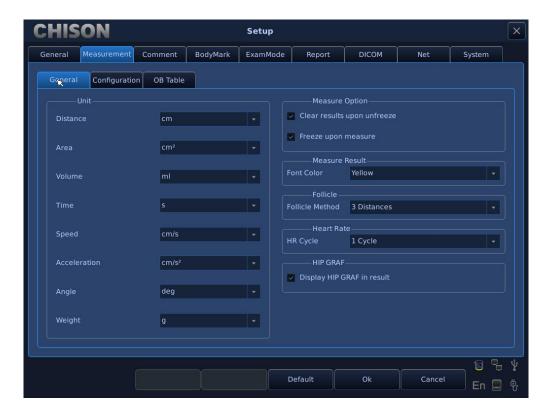

- Unit: display the unit of all measurement items.
- Measure Option: whether clear results upon unfreeze, and the automatic froze image.
- **Measure Result:** the color of the result font is alternative, including yellow/white/orange/green. Measurement formula setting.
- Follicle: ways to measure follicle, you can choose two distances and three distances.
- Heart Rate: cycle options for calculating the number of heart beats per minute of cardiac image.
- **HIP GRAF:** select to display HIP GRAF in result or not.

7.2.1.1 Interface Description-Measurement Menu

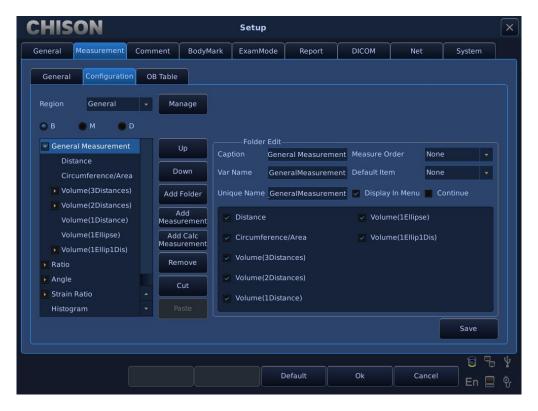


- Region: pull down and select needed measurement menu.
- Manage: pop up measurement software edition interface, add modify delete change marshalling sequence in measurement menu.
- B, M, D: display measurement of each Exam mode.
- Up: press this button to move selected measurement term up.
- **Down:** press this button to move selected measurement term down.
- Add Folder: add a measurement item. In the left column when the term is fold there is "+" otherwise "-".
- Add Measurement: add a measurement item for a term in the right column there is selected item and detailed parameter.
- Add Calc Measurement: add a calc item for a measurement term.
- Remove: remove selected measurement term or item.
- Default: restore all measurement term as factory setting.
- Save: save measurement item modification users did.

- Cut: select to cut the measurement option you want to paste.
- Paste: paste the measurement option you have cut.

Folder Edit content description

Caption	Display names of all items that is displayed name in		
	measurement menu.		
Var Name	The name of built-in selected measurement menu, user don't		
	need modify while display order according to the names.		
Unique Name	Built-in code, user doesn't need modify.		
Measurement Order	None: Disable rule, Repeat: Repeat this item, Next: measure		
	by sequence.		
Default item	After choosing the Repeat and Sequential, choose one		
	measurement or calculation to activate the measurement rule.		

7.2.1.2 Interface Description-Measurement Calculation

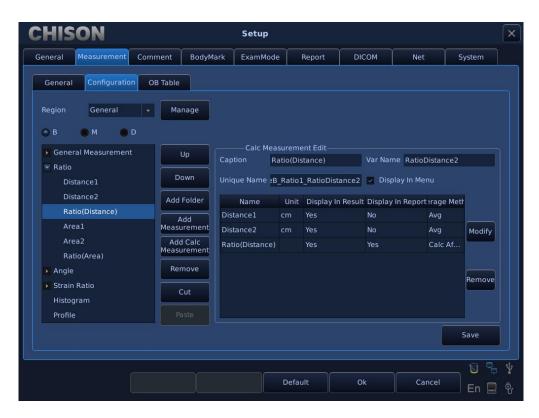


Calc Measurement Edit content description

Display the name of selected term that is display names in the		
measurement menu.		
The name of built-in selected measurement menu, user don't need		
modify while display order according to the names.		
Built-in code, users don't need to modify.		
Select available measurement tool type		
B distance (B line), area/circumference (ellipse, trace), M distance (M		
vertical line), time (M horizontal line), M slope (M slant).		
Check the required item and it will display on the measurement menu.		
The item without checking will not display on the measurement menu.		
Needed measurement operation of specific measurement and		
calculation.		
Data unit which measurement operation produces.		
Whether display in the result or not.		
Whether display in the report or not.		
Check the methods in measurement menu, press [update] key to		
switch the method; Otherwise, the measurement is not available.		
Press this button to move measurement operation up.		
Press this button to move measurement operation down.		
The average rule of data.		
Press this button to pop up interface to add measurement operation.		
Press this button to pop up interface to modify measurement		
operation.		
Press this button to delete selected measurement operation.		

7.2.1.3 Create Measurement Operation

Press [Add] button in measurement operation interface, pop up the following dialog box.

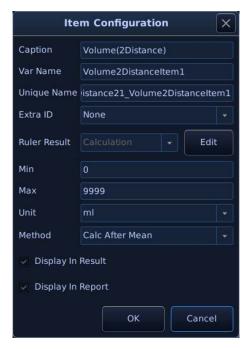


Operation content description of creating new measurement

Caption	Display the name of selected term that is display names in the measurement menu.		
Var Name	The name of built-in selected measurement menu, user don't need modify while display order according to the names.		
Unique Name	Built-in code, user doesn't need to modify.		
Ruler Result	Needed measurement operation of specific measurement and calculation.		
Edit	Enter into interface to edit formula when selecting calculation item.		
Max	The maximum value displays in result zone and report.		
Min	The minimum value displays in result zone and report.		
Unit	Data unit which measurement operation produces.		
Display In Result	Whether display in the result or not.		
Display In Report	Whether display in the report or not.		
Method	The average rule of data.		

7.2.1.4 Formula Edit-Normal

It is necessary to enter into the following interface when creating measurement operation except OB.

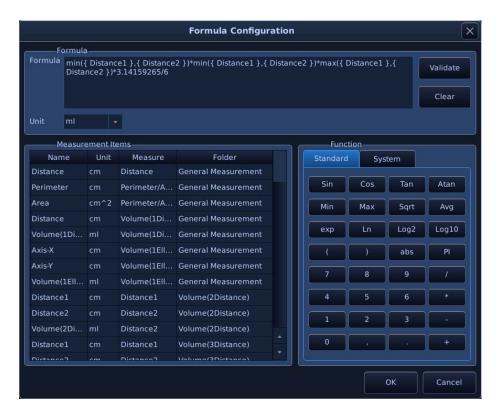

- Formula: edit formula in input box via keyboard and built-in formula.
- Validate: press this button to check whether the formula is right or not after editing formula.
- Clear: clear the content in the input box.
- Unit: select the unit of calculation consequence.
- Measurement Items: display all available measurement operation in the measurement menu.
- Function: built-in formula, number input and some parameters that system needs such as BSA,
 SPSA etc.
- Cancel: cancel editing formula and close the interface.
- **OK:** save edited operation and close the interface.

7.2.1.5 Formula Edit-OB


It is necessary to call built-in OB formula sheet when creating OB measurement operation the following function interface is required.

CAUTION: the results of GA and EDD don't require unit, the unit of this class has been built-in.



- Measurement Items: display created measurement term by now.
- **OB Tables:** built-in OB formula table.


OB List

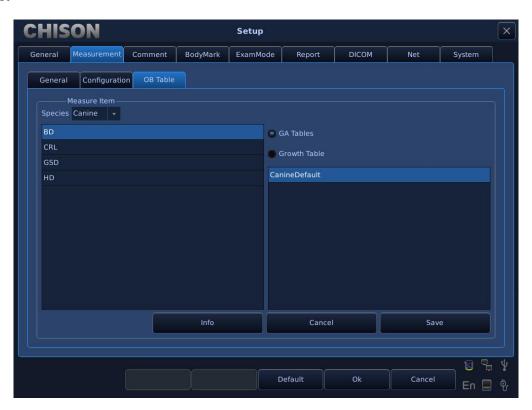

• Measure Item: OB Measurement Item.

- GA Tables: Gestational list for the current measuring project.
- Growth Table: Growth table for the current measuring.
- Fetal Weight: Fetal Weight calculation formula.
- EFW Equation: Fetal weight calculation for the current measuring.
- EFW Growth: Fetal weight growth curve for the current measuring.
- Info: Display the gestational age and fetal weight for the current measuring.
- Cancel: Cancel the operation of choosing the formula.
- Save: Save the users' choice of formulas.

7.3 Comment

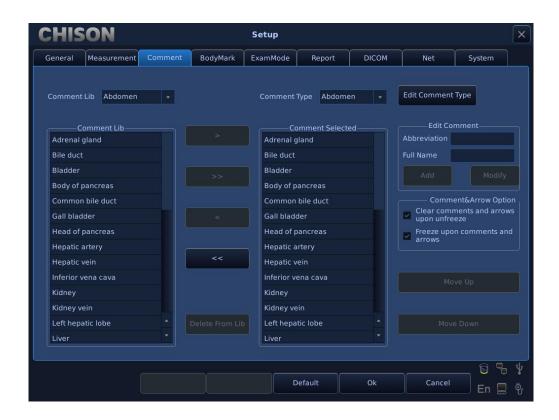

7.3.1 Comment Library

The annotation database of the system is classified as: abdomen, OB, GYN, Cardiac, small parts, Pathological change Annotation can be made by inputting characters from the soft keyboard or recalling the terms saved in annotation database.

Press [CommentLib] pull down button, pop up annotation name within system, through trackball and [ENTER] key to show required annotation status.

♦ Edit Comment Library

Operation:

- 1. At the annotation status, Move the cursor to the **[Edit Comment Type]** button then press **[ENTER]** key, the annotation will be updated, and can be edited.
- 2. Input name into the new created annotation status box, move the cursor to the **[Create]** button then press **[ENTER]** key, then create new annotation status and appear in selected annotation status list.
- 3. Move the cursor to the **[Delete]** button, press **[ENTER]** key, then delete current annotation status in the selected annotation list.
- 4. Alter name of current annotation status list in [Current Type Name] input box, press [ENTER] key on the [Rename] button, then rename the selected annotation status name.

⚠NOTE:

Factory Settings comments cannot be deleted or renamed.

♦ Edit Comment

Operator uses only current annotation instead of all content annotation status provides inlay common annotation. If necessary, user can import annotation or self-compiled annotation into common annotation.

Add comment from comment library

Operation:

- 1. Select needed source annotation status via Trackball and [ENTER] key.
- 2. Select needed annotation at **[CommentLib]** column then press the **[ENTER]** key to activate this annotation.
- 3. Press [ENTER] key on [>] button to import selected annotation into user-selected annotation status; press [ENTER] on [>] button to move selected annotation in [Comment Selected] column into source annotation.
- 4. Press [ENTER] on [>>] button to import all annotation in source into user-selected annotation status; Press [ENTER] on [>>] button to move all annotation in [Comment Selected] column into

source annotation.

Add comment manually

Operation:

1. Activate [Edit Comment] input box via Trackball and [ENTER] key, and then input needed

abbreviation and full name of annotation.

2. Press [ENTER] key on [Add] button, meanwhile this handout will be added into source and

user-selected annotation status.

Alter comment

Operation:

1. Alter annotation in user-selected status, the abbreviation and full name of annotation will be

displayed in [Edit Comment] box.

2. Activate needed abbreviation and full name via [ENTER] key and alter via keyboard.

3. Press [ENTER] key on [Modify] button, modify the annotation in both source and

user-selected status.

Delete comment in library

Operation:

Select needed annotation in source status, press [ENTER] key on [Delete from Lib] button, then


the annotation deleted.

7.3.2 Comment and Arrow Option

Optional: whether clear comments and arrows upon unfreeze.

Optional: whether freeze upon comments and arrows.

7.4 Body marks

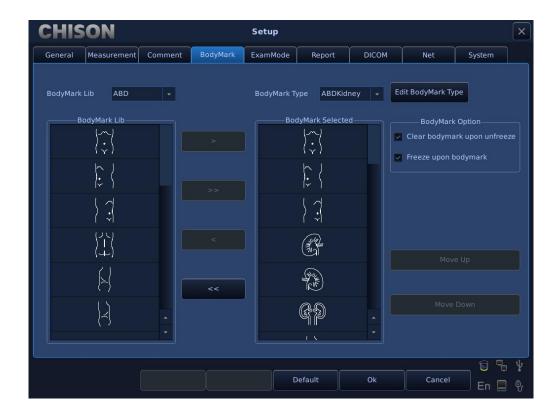

7.4.1 Body Marks Library

Built-in body marks: Abdomen OB, GYN, Cardiac, Small part, Urology, Vessel.

Press [BodyMarkLib] pull down button, pop up name of built-in body marks, show needed body marks via Trackball and [ENTER] key.

♦ Edit body marks library

Operation:

- 1. Press [ENTER] key on [Edit BodyMark Type], pop up edit box.
- 2. Input name into the new created body marks box, Move the cursor to the **[Create]** button then press **[ENTER]** key, then the new body marks will be created and appear in selected body marks list
- 3. Move the cursor to the **[Delete]** button then press **[ENTER]** key, then delete current body marks in the selected list.
- 4. Alter current annotation status list name in [Current Type Name] input box, press [ENTER] key on the [Rename] button, then rename the selected body marks.

7.4.2 Body mark edition

Operation:

1. Select needed source body marks via Trackball and [ENTER] key.

2. Select needed body marks at [BodyMarkLib] column then press the [ENTER] key to activate

it.

3. Press [ENTER] key on [>] button to import selected body marks into user-selected status.

Press [ENTER] key on [>] button to move selected body marks in [BodyMark Selected] column

into source body marks.

4. Press [ENTER] key on [>>] button to import all body marks in source into user-selected status.

Press [ENTER] key on [>>] button to move all body marks in [BodyMarks Selected] column into

source.

7.4.3 Bodymark Option

Optional: whether clear bodymark upon unfreeze.

Optional: whether freeze upon bodymark.

7.5 Exam Mode

7.5.1 Exam Mode Edit

Press Utility in the submenu of [MENU], the parameters control area shows as following. Press the corresponding control key to turn on or off the function.



• Preset: Display the current preset.

• Rename: Rename the current preset.


• Load Preset: Load the preset displayed.

• Save: Save the current preset.

• Save As: Save the current preset as others.

7.5.2 Exam Mode Selection


Choose Utility and press [MENU], the following interface pops up. Open the relate function by corresponding control area.

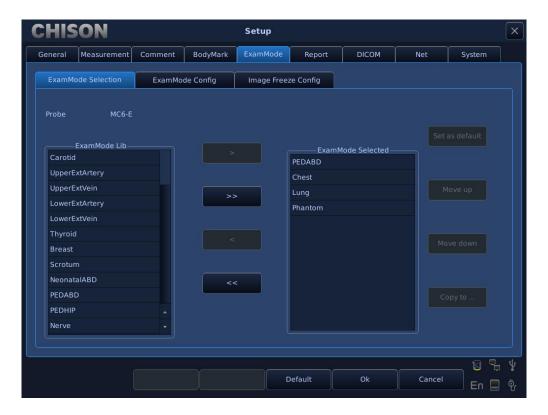

- Probe: select needed probe and ExamMode fit for it.
- ExamModeLib: show all existed Exam modes.
- ExamMode Selected: show Exam modes in probe column.
- >: import selected Exam modes from ExamModeLib column to ExamMode Selected column.
- >>: import all Exam modes from ExamModeLib column into ExamMode Selected column.
- <: delete selected Exam modes in ExamMode Selected column.
- <<: delete all Exam modes in ExamMode Selected column.
- Set as default: set selected Exam modes in ExamMode Selected column as default
- Move up: move selected Exam modes in ExamMode Selected column up.
- Move down: move selected Exam modes ExamMode Selected column down.
- Copy to: copy the exam mode selected in ExamMode to a specified preset.

7.5.3 Exam mode Config


Operator can define needed Exam mode in detail including annotation, body marks, measurement menu import and export etc.

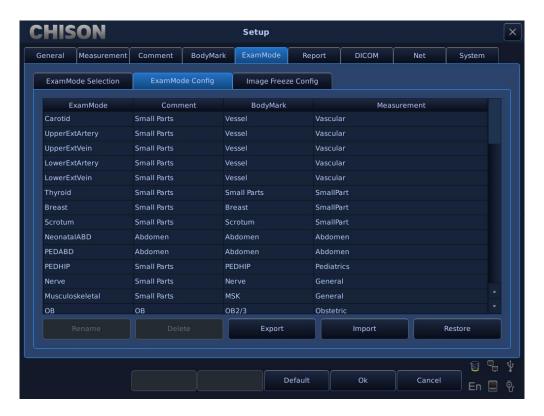

- ExamMode: show all existed Exam modes in system
- **Comment:** double press **[ENTER]** key to activate widget box, can choose existed annotation status name. After setting, the default of the Exam mode is user-selected.
- BodyMark: same as Comment, select user-needed default body marks.
- Measurement: same as Comment, select user-needed default measurement menu.
- Rename: rename selected Exam mode
- Delete: delete selected Exam mode
- Export: export all built-in Exam modes into USB flash disk.
- Import: import all built-in Exam modes into USB flash disk.
- **Restore:** restore all Exam mode as factory setting.

7.5.4 Image Freeze Config

Operator can define status after freezing image. The statuses list as below:

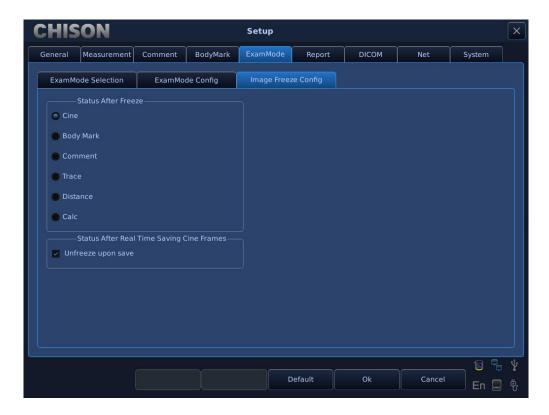


- Status After Freeze: options for status after freezing.
- Status After Real Time saving Cine Frames: whether unfreezing upon save or not.

7.6 Report

Users can set the layout and diagnostic template for report according to the requirement.


7.6.1 Layout Setting

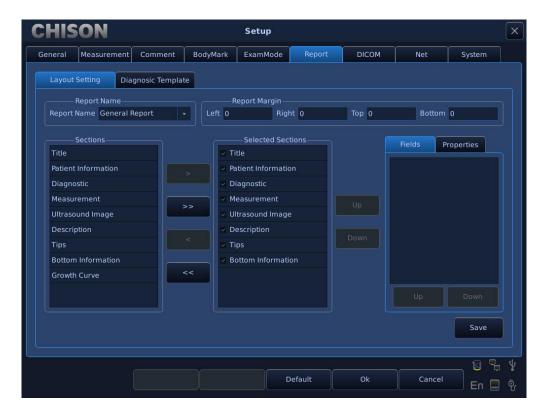

- Report Name: display the report type, select the report which you need to set.
- Report Margin: set the left, right, top and bottom space for the report margin.
- Section: all the optional contents you can select to display in the report.
- Selected Sections: show the selected contents displayed in the report.
- >: import the selected option from sections to the selected sections
- >>: import all the content from sections to the selected sections
- <: delete the selected content in the selected sections you does not want to display in the report.
- <<: delete all the content in the selected sections.
- UP/Down (right side of the selected sections): select [Up] or [Down] to set the displayed order of the selected contents in the report.
- Fields: display the corresponding content of options in the selected sections. For example,
 when you select title, it will display hospital name and title, you can select the content you
 want to display in the report or not.
- Properties: adjust the column or row layout in the vertical or horizontal direction for the selected content in selected sections.
- UP/Down (on the bottom of fields): adjust the displayed order in report for selected contents

in fields.

7.6.2 Diagnostic Template setting

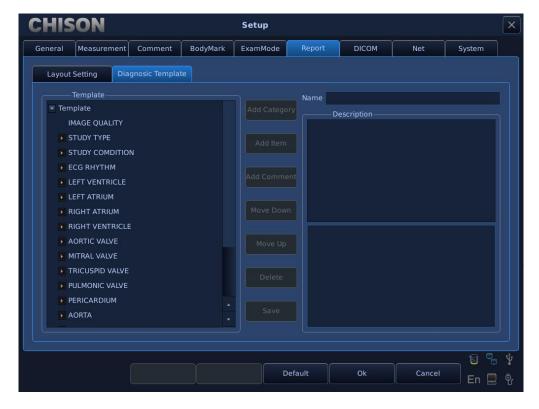

- Template: show the content of all the template.
- Name: show the name of the template you have selected.
- Description: the description display the detailed content of the submenu you have selected.
 when you select the option marked with "+", it will display the submenus and select an option you want to edit.
- Add Category: add a submenu for the option in the template you have selected. For example,
 when you select image quality, it will display a submenu named folder. Then you can select
 [Name] to modify the name for the folder.
- Add Item: add items for the submenus according to the user's requirement. After you add items,
 you can select [Name] to modify the items' name.
- Add Comment: add comment for the items under the submenu. After you add comment, it will
 display comment in the description area. Then you can select the bottom area in the
 description to modify the name for the comment.
- Move Up/Move Down: adjust the display order for the content in the template or in the


description you have selected.

- Delete: delete the content in the template or in the description you have selected.
- Save: after you complete the setting, select this option to save all the modification.

7.7 DICOM

DICOM includes DICOM Storage, DICOM Worklist, DICOM Print and DICOM SR. If DICOM is to be applied, please make sure DICOM has been activated. In the system page of setting interface, you can check whether DICOM is open or not. If you want to activate DICOM, please contact with CHISON.

There must be DICOM SCP server which has been installed with PACS or other relative DICOM server software.

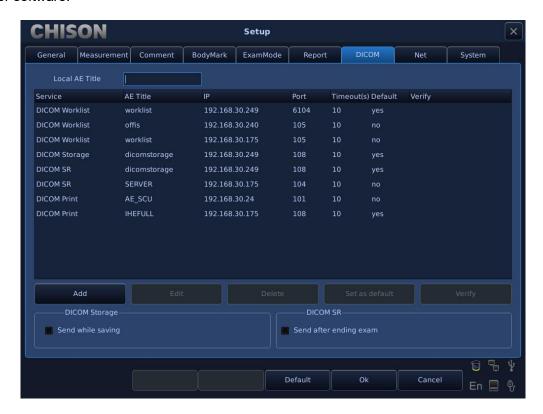

- Local AE Title: input local DICOM Title to separate the DICOM equipment in local network.
- Service: display the local DICOM function worklist,
- AE Title: display the name of local DICOM AE title,
- IP: display the IP of DICOM server,
- Port: display the port of DICOM server
- Timeout(s): display the delay time

- Default: display whether DICOM is default or not ,
- Verify: Press verify button and display whether DICOM setting is correct or not
- Add: add DICOM function and pop up setting dialog,
- Edit: edit information of DIOM function.
- Delete: delete the existed DICOM function
- Set as default: set one DICOM service as default,
- **DICOM Storage:** check this item and enable DICOM storage while saving image or cine, send clip or image according to activated function.
- **DICOM SR**: select this option the system will send DICOM SR after the operator ends the exam.

7.7.1 Add/Edit DICOM Function



Press [Add] button, then system pops up the DICOM Setting interface.

- Default: check this option, set DICOM function as default.
- Service: choose DICOM Storage, DICOM Worklist, DICOM Print or DICOM SR.
- Server AE Title: input DICOM server AE name.
- Server IP address: input DICOM IP address.
- SCP port: input DICOM server SCP port.
- Timeout: set the delay time of DICOM.
- Compression Mode: check this option, set Uncompressed or JPEG according to the

corresponding requirements.


- Compression Ratio: after selecting the JPEG as the compression mode, choose the appropriate compression ratio.
- Max Framerate: check this option, select proper feamerate according to the requirement.

Tip: choosing the DICOM Print type must be before relative print setting.

7.8 Net

Set the unit's and target unit's IP and do the connection testing. And network storage settings, details see the appendix G: Procedures of setting network sharing.

7.9 System

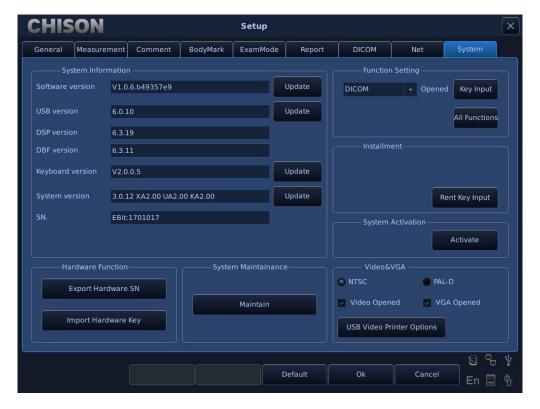

System information

Display the software version, hardware version, system version, etc.

Update

Software and Hardware can be updated by USB disk.

Software upgrades File Path: X:\update machine code\AAA.

Hardware upgrades File Path: X:\fpga_machine code\AAA.

Keyboard upgrades File Path: X:\keyboard update machine code\AAA.

X means USB disk. AAA means upgrades content .lt should restart manually after hardware update, and after software update, machine can be restarted automatically.

Function Setting

Show the status of current functions, and click the related button to turn on/off this function (need the key provided by CHISON).

Installment setting

Input relevant key to open trial function and the detail please contact CHISON Company.

System Activate

Select this item to activate the device if the user does not activate after powering on the system.

Video VGA

Choose the video data: NTSC and PAL-D.

Video opened: Choose the item to open this function.

VGA opened: Choose the item to open this function.

Hardware function

Export hardware SN and import hardware key, it only for engineer use.

System Maintenance

Only an authorized service engineer may perform maintenance.

USB Video Printer Option

Adjust the parameters of Video Printer Option: Dark, Light, Sharpness, and Gamma.

Select the parameters needed to adjust, press [Done] button on the slider of the parameter, and move the trackball to change the parameter.

Chapter 8 System Maintenance

8.1 Machine Cleaning

ACAUTION:

Do turn off the power before cleaning and pull out the cable from socket. There is possibility of electric shock if the device is on.

Cleaning methods:

Use the soft dry cloth to wrap the machine. If the device is quite dirty, use wet soft cloth. After wiping the blot, use soft dry cloth to wipe.

ACAUTION:

- ✓ Don't use organic solvent such as alcohol, otherwise surface may be ruined.
- ✓ When cleaning the machine, don't let the liquid inflow the machine, otherwise it may malfunction and there is a danger of electric shock.
- ✓ When it is necessary to clean the probe connector and peripheral instrument, please contact Sales office contact customer service or agent of CHISON. Any self-cleaning may result in malfunction or degrading the function of device.

8.2 Safety Check

To make sure this device works normally, a piece of maintenance plan is suggested to make to check the device regularly If any abnormal phenomena, immediately stop operation and contact with Sale Office, Customer Service department or Agents of manufacturer.


If no image or menu but image, please check following malfunction table. If the malfunction can't be solved, please contact with Sale Office, Customer Service department or Agents of manufacturer.

8.3 Malfunction Check

Serial number	Malfunction	Reason	Measures
1	Switch button lights but power LED not	Battery lose efficacy, Adapter works irregular	Check the connector between cable and power
2	Power Led lights but LED no image	The interval time is too short to restart	Restart after 1 minute
3	LED display character menu but no scan image	Launch power, gain or STC control errors Not connect to probe or the probe connection is not correct Device is in freezing condition	Control launch power, gain or STC control Make sure of right connection Exit from freezing condition
4	Abnormal image	Exam mode errors Image processing setting errors	Whether Exam mode is proper or not Adjust image processing setting or set it as default
5	Probe works improperly	1.The plug plugs loosely 2.Internal circuit protects	1.Extract the probe and reinsert 2.Restart
6	No OB calculation package menu	Do not select the OB application before scanning.	Select the OB application
7	PRINT-button doesn't work	1.The connected printer is approved 2.Printer power is not on 3.Printer is not connect well	1.Change the approved printer 2.Turn on the printer 3.Connect the printer again

Chapter 9 Probes

9.1 General Description

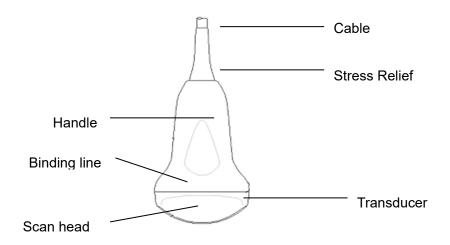

Convex Probe Overview

The probes provide high spatial and contrast ultrasound imaging of frequencies from 2.0MHz to 11.0MHz. These probes operate by pulsing sound waves into the body and listening to the returning echoes to produce high-resolution brightness mode, and a real time display.

9.2 Care and Maintenance

The probes that come with the system are designed to be durable and dependable. These precision instruments should be inspected daily and handled with care. Please observe the following precautions:

- 1. Do not drop the transducer on hard surface. This can damage the transducer elements and compromise the electrical safety of the transducer.
- 2. Avoid kinking or pinching the transducer cable.
- 3. Use only approved ultrasonic coupling gels.
- 4. Follow the instructions for cleaning and disinfecting that come with each probe.

CAUTION:

✓ Only person Received professional training can use the probes.

- ✓ Probes can't receive pressure sterilizer, when operation in sterile area, disposable sterile probe hood should be applied.
- ✓ Make sure not to drop the transducer on hard surface. This can damage the transducer elements and compromise the electrical safety of the transducer.
- ✓ Be careful when doing operation, make sure not to scratch the probe surface.
- ✓ Avoid kinking or pinching the transducer cable.
- ✓ Make sure not to connect the probe to plug or put adjacent cable into any kind of liquid.
- ✓ Keep the probe clean and dry. Power off or freeze when fixing or dismantling the probe.
- ✓ Make sure not to use or deposit the probe in the environment above 50 degree.
- ✓ If any abnormal phenomena of probe is found, immediately stop operation and contact with Sale Office, Customer Service department or Agents of manufacturer.

9.2.1 Inspecting Probes

Before and after each use, inspect carefully the probe's lens, cable, casing, and connector. Look for any damage that would allow liquid to enter the probe. If any damage is suspected, do not use the probe until it has been inspected and repaired/replaced by an authorized Service Representative.

⚠NOTE:

Keep a log of all probe maintenance, along with a picture of any probe malfunction.

∴WARNING:

The probes are designed to be used only with this ultrasound system. Use of these probes on any other system or a non-qualified probe may cause electrical shock or damage on the system/transducer.

9.2.2 Cleaning and Disinfecting

- Disconnect the probe from the ultrasound console and remove all coupling gel from the probe by wiping with a soft cloth and rinsing with flowing water.
- Wash the probe with mild soap in lukewarm water. Scrub the probe as needed using a soft sponge, gauze, or cloth to remove all visible residue from the probe surface. Scrub the probe as

needed using a soft sponge, gauze, or cloth to remove all visible residue from the probe surface.

- Rinse the probe with enough clean, potable water to remove all disinfectant residues.
- Use a soft cloth to clean the cable and the user section of the probe with the cleaning disinfectant liquid. Make sure that the surface of the probe and cable is wetted thoroughly with the cleaning-disinfectant.
- Allow probe to air dry completely.
- Reconnect the probe to the ultrasound console and place the probe into its holder.

♦ Cleaning

The cleaning procedure is fit for all probes. After operation every probe should do cleaning according to stated procedure of this passage. Inspection should be done for intracavity probe depends on condition of use

Cleaning procedure:

- 1. Wipe the remaining coupling gel and blot with flowing clear water. Avoid the joint part between cable and probe touching the water or others.
- 2. Use wet gauze or other soft cloth with a little liquid soap to clean the probe totally. Don't use cleaning agent and cleaner with abrasiveness.
- 3. Use flowing water to rinse fully. Use soft cloth which has been soaked by the concentration of 70% isopropyl alcohol to scrub. Then check the probe to make sure there is no blot.
- 4. Use clean cloth to dry the probe.

Cleaning Compatibility

Solution	Origin	Qualified Use	Active Ingredients
CIDEZYME	All	Soaking	Enzyme
Epizyme-Rapid(Rapid Multi-Enzyme cleaner)	All	Soaking	Enzyme
ANIOSYME DD1	FRA	Soaking	Enzyme
Neodisher mediclean	DEU	Soaking	Enzyme
MetriZyme	USA	Soaking	Enzyme
Endozime Xtreme Power	USA	Soaking	Enzyme
Sani-Cloth AF3	USA	Wiping	Quaternary ammonium chlorides

CAUTION: Don't put the body surface probe into liquid below acoustical lens. Intracavity probe can't exceed insertion region. Prohibit putting connector of probe into any liquid.

Disinfection

Disinfection procedure id fit for intracavity probe.

If it is necessary to use in surgery, please abide with instruction of professional disinfection person.

Disinfection procedure:

- 1. Obey the cleaning procedure to clean the probe totally.
- 2. Prepare and retreat the disinfection solution according to the instruction of manufacturer.
- 3. Put the insertion region of probe into disinfection solution, the inserting depth can't exceed insertion region. Don't let the probe connector touch any liquid.
- 4. Soak the probe for 3 h.
- 5. Pull out the probe, immediately rinse totally with sterile water and saline. To make sure of no any solution remaining. Please obey the rule to do right rinsing procedure including enough rinsing water and times.
- 6. When probe is used in sterile area, make sure to use disposable sterile probe hood.

Disinfectants Compatibility


Solution	Origin	Qualified Use	Active Ingredients
Aihujia Environmental Surface	All	Wining	Quatarnary ammanium ablaridas
Wipes	All	Wiping	Quaternary ammonium chlorides
WIP'ANIO	FRA	Wiping	Quaternary ammonium chlorides
Sani-Cloth Bleach Germicidal	1104	107	0 1 1 1 1
Wipes	USA	Wiping	Sodium hypochlorite
MetriCide OPA Plus	USA	Soaking	Orthophthalal-aldehyde
CIDEX OPA	All	Soaking	Orthophthalal-aldehyde

ACAUTION:

- ✓ Don't soak probe connector into any liquid.
- ✓ Don't let the soaking depth of intracavity probe exceed insertion region.

- ✓ Prohibit soaking the probe in the liquid for more than 12 h.
- ✓ Only use qualified disinfection solution.

◆ Probe Immersion Levels

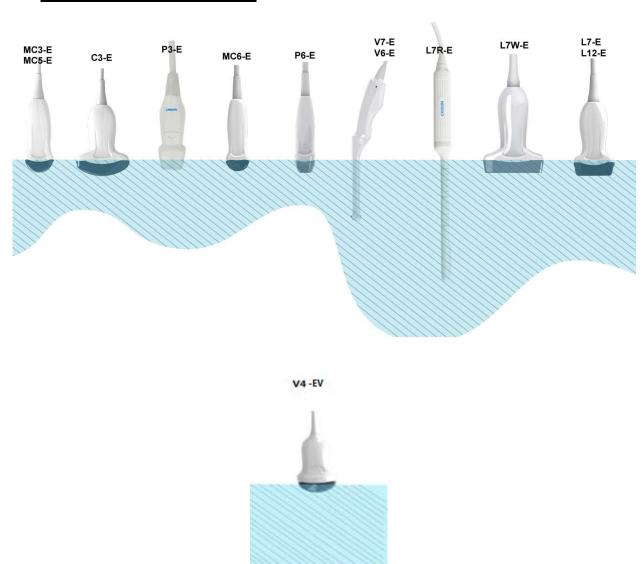

ACAUTION

These transducers are not designed to withstand heat sterilization methods. Exposure to temperatures in excess of 60 ° C will cause permanent damage. The transducers are not designed to be totally submerged in fluid, as permanent damage will result if the entire transducer is submerged.

9.2.3 Probe Safety

9.2.3.1 Handing Precaution

Ultrasound probes are highly sensitive medical instruments that can easily be damaged by improper handling. Use care when handling and protect from damage when not in use. DO NOT use a damaged or defective probe. Failure to follow these precautions can result in serious injury and equipment damage.

◆ Electrical shock hazard:

The probe is driven with electrical energy that can injure the patient or user if live internal parts are contacted by conductive solution:

- DO NOT immerse the probe into any liquid beyond the level indicated by the immersion level diagram. Never immerse the probe connector into any liquid.
- Prior to each use, visually inspect the probe lens and case area for cracks, cuts, tears, and other signs of physical damage. DO NOT use a probe that appears to be damaged until you verify functional and safe performance. You need to perform a more thorough inspection, including the cable, strain relief, and connector, each time you clean the probe.
- Before inserting the connector into the probe port, inspect the probe connector pins. If a pin is bent, DO NOT use the probe until it has been inspected and repaired/replaced by a CHISON Service Representative.
- Electrical leakage checks should be performed on a routine basis by CHISON Service or qualified hospital personnel.

Mechanical hazard:

A defective probe or excess force can cause patient injury or probe damage:

- Observe depth markings and do not apply excessive force when inserting or manipulating endo-cavitary probe.
- Inspect probes for sharp edges or rough surfaces that may injure sensitive tissue.
- DO NOT apply excessive force to the probe connector when inserting into the probe port. The pin of a probe connector may bend.

♦ Special handling instructions

Using protective sheaths

The use of market cleared probe sheaths is recommended for clinical applications. Reference FDA March 29, 1991 "Medical Alert on Latex Products".

Protective sheaths may be required to minimize disease transmission. Probe sheaths are available for use with all clinical situations where infection is a concern. Use of legally marketed, sterile probe sheaths is strongly recommended for endo-cavitary procedures.

DO NOT use pre-lubricated condoms as a sheath. In some cases, they can damage the probe. Lubricants in these condoms may not be compatible with probe construction.

Devices containing latex may cause severe allergic reaction in latex sensitive individuals. Refer to FDA's March 29, 1991 Medical Alert on latex products.

DO NOT use an expired probe sheath. Before using a sheath, verify if it has expired.

Endo-cavitary Probe Handling Precautions

If the sterilization solution comes out of the endo-cavitary probe, please follow the cautions below: Sterilant Exposure to Patient (e.g., Cidex): Contact with a sterilant to the patient's skin for mucous membrane may cause an inflammation. If this happens, refer to instruction manual of the sterilant.

Sterilant Exposure from Probe handle to Patient (e.g. Cidex): DO NOT allow the sterilant to contact the patient. Only immerse the probe to its specified level. Ensure that no solution has entered the probe's handle before scanning the patient. If sterilant comes into contact with the patient, refer to the sterilant's instruction manual.

Sterilant Exposure from Probe connector to Patient (e.g. Cidex): DO NOT allow the sterilant to contact the patient. Only immerse the probe to its specified level. Ensure that no solution has entered the probe's connector before scanning the patient. If sterilant comes into contact with the patient, refer to the sterilant's instruction manual.

Endo-cavitary Probe Point of Contact: Refer to the sterilant's instruction manual.

9.2.3.2 Probe Handing and Infection Control

This information is intended to increase user awareness of the risks of disease transmission

associated with using this equipment and provide guidance in making decisions directly affecting the safety of the patient as well as the equipment user.

Diagnostic ultrasound systems utilize ultrasound energy that must be coupled to the patient by direct physical contact.

Depending on the type of examination, this contact occurs with a variety of tissues ranging from intact skin in a routine exam to recirculating blood in a surgical procedure. The level of risk of infection varies greatly with the type of contact.

One of the most effective ways to prevent transmission between patients is with single use or disposable devices. However, ultrasound transducers are complex and expensive devices that must be reused between patients. It is very important, therefore, to minimize the risk of disease transmission by using barriers and through proper processing between patients.

Risk of Infection

ALWAYS clean and disinfect the probe between patients to the level appropriate for the type of examination and use FDA-cleared probe sheaths where appropriate.

Adequate cleaning and disinfection are necessary to prevent disease transmission. It is the responsibility of the equipment user to verify and maintain the effectiveness of the infection control procedures in use. Always use sterile, legally marketed probe sheaths for intra-cavitary procedures.

♦ Perform Cleaning probe after each use

- 1. Disconnect the probe from the ultrasound console and remove all coupling gel from the probe by wiping with a soft cloth and rinsing with flowing water.
- 2. Wash the probe with mild soap in lukewarm water. Scrub the probe as needed using a soft sponge, gauze, or cloth to remove all visible residue from the probe surface. Prolonged soaking or scrubbing with a soft bristle brush (such as a toothbrush) may be necessary if material has dried onto the probe surface.

riangleWARNING

To avoid electrical shock, always turn off the system and disconnect the probe before cleaning the

probe.

ACAUTION

- ✓ Take extra care when handling the lens face of the Ultrasound transducer. The lens face is especially sensitive and can easily be damaged by rough handling. NEVER use excessive force when cleaning the lens face.
- ✓ Rinse the probe with enough clean potable water to remove all visible soap residue.
- ✓ Air dry or dry with a soft cloth.

ACAUTION

To minimize the risk of infection from blood-borne pathogens, you must handle the probe and all disposables that have contacted blood, other potentially infectious materials, mucous membranes, and non-intact skin in accordance with infection control procedures. You must wear protective gloves when handling potentially infectious material. Use a face shield and gown if there is a risk of splashing or splatter.

♦ Coupling gels

DO NOT use unrecommended gels (lubricants). They may damage the probe and void the warranty. AQUASONIC Gel made by R. P. Kincheloe Company in USA is recommended.

In order to assure optimal transmission of energy between the patient and probe, a conductive gel must be applied liberally to the patient where scanning will be performed.

\triangle CAUTION

Please do not use any gel or other materials which are not provided by CHISON. Un-authorized gel, lubricants and other materials may corrode probes and other parts of the device, for example the keyboard. This may reduce the safety and effectiveness of the system and probes, and may also reduce the life time of the systems and probes. Damages caused by such reason will not be covered by the warranty.

DO NOT apply gel to the eyes. If there is gel contact to the eyes, flush eyes thoroughly with water.

Coupling gels should not contain the following ingredients as they are known to cause probe damage:

- Methanol, ethanol, isopropanol, or any other alcohol-based product.
- Mineral oil
- lodine
- Lotions
- Lanolin
- Aloe Vera
- Olive Oil
- Methyl or Ethyl Parabens (para hydroxybenzoic acid)
- Dimethyl silicone

9.2.3.3 Planned and Special Maintenance

Planned maintenance

The following maintenance plan is suggested for the system and probes to ensure optimum operation and safety.

Daily: inspect the probes.

After each use: clean the probes disinfect the probes.

As necessary: inspect the probes, clean the probes, and disinfect the probes.

Returning/Shipping Probes and Repair Parts

Transportation dept. and our policy require that equipment returned for service MUST be clean and free of blood and other infectious substances.

When you return a probe or part for service, you need to clean and disinfect the probe or part prior to packing and shipping the equipment.

Ensure that you follow probe cleaning and disinfection instructions provided in this Manual.

This ensures that employees in the transportation industry as well as the people who receive the package are protected from any risk.

♦Probe Covers

The transducer should be covered with a barrier. If the barriers used are condoms, these should be nonlubricated and nonmedicated. Practitioners should be aware that condoms have been shown to be less prone to leakage than commercial probe covers, and have a six-fold enhanced

AQL (acceptable quality level) when compared to standard examination gloves. They have an AQL equal to that of surgical gloves. Users should be aware of latex-sensitivity issues and have available nonlatex-containing barriers.

9.2.3.4 AIUM Outlines Cleaning the Endocavotary Transducer

Guidelines for Cleaning and Preparing Endocavitary Ultrasound Transducers between Patients from AIUM

Approved June 4, 2003

The purpose of this document is to provide guidance regarding the cleaning and disinfection of transvaginal and transrectal ultrasound probes.

All sterilization/disinfection represents a statistical reduction in the number of microbes present on a surface. Meticulous cleaning of the instrument is the essential icon to an initial reduction of the microbial/organic load by at least 99%. This cleaning is followed by a disinfecting procedure to ensure a high degree of protection from infectious disease transmission, even if a disposable barrier covers the instrument during use.

Medical instruments fall into different categories with respect to potential for infection transmission. The most critical level of instruments are those that are intended to penetrate skin or mucous membranes. These require sterilization. Less critical instruments (often called "semi-critical" instruments) that simply come into contact with mucous membranes such as fiber optic endoscopes require high-level disinfection rather than sterilization.

Although endocavitary ultrasound probes might be considered even less critical instruments because they are routinely protected by single use disposable probe covers, leakage rates of 0.9% - 2% for condoms and 8%-81% for commercial probe covers have been observed in recent studies. For maximum safety, one should therefore perform high-level disinfection of the probe between each use and use a probe cover or condom as an aid in keeping the probe clean.

There are four generally recognized categories of disinfection and sterilization. Sterilization is the complete elimination of all forms or microbial life including spores and viruses.

Disinfection, the selective removal of microbial life, is divided into three classes:

High-Level Disinfection - Destruction/removal of all microorganisms except bacterial spores.

Mid-Level Disinfection - Inactivation of Mycobacterium Tuberculosis, bacteria, most viruses, fungi, and some bacterial spores.

Low-Level Disinfection - Destruction of most bacteria, some viruses and some fungi. Low-level disinfection will not necessarily inactivate Mycobacterium Tuberculosis or bacterial spores.

The following specific recommendations are made for the use of Endocavitary ultrasound transducers. Users should also review the Centers for Disease Control and Prevention document on sterilization and disinfection of medical devices to be certain that their procedures conform to the CDC principles for disinfection of patient care equipment.

9.2.3.5 Aspetic Technique

For the protection of the patient and the health care worker, all endocavitary examinations should be performed with the operator properly gloved throughout the procedure. Gloves should be used to remove the condom or other barrier from the transducer and to wash the transducer as outlined above. As the barrier (condom) is removed, care should be taken not to contaminate the probe with secretions from the patient. At the completion of the procedure, hands should be thoroughly washed with soap and water.

NOTE: Obvious disruption in condom integrity does NOT require modification of this protocol. These guidelines take into account possible probe contamination due to a disruption in the barrier sheath.

In summary, routine high-level disinfection of the endocavitary probe between patients, plus the use of a probe cover or condom during each examination is required to properly protect patients from infection during endocavitary examinations. For all chemical disinfectants, precautions must be taken to protect workers and patients from the toxicity of the disinfectant.

Amis S, Ruddy M, Kibbler CC, Economides DL, MacLean AB. Assessment of condoms as probe covers for transvaginal sonography. J Clin Ultrasound 2000;28:295-8.

Rooks VJ, Yancey MK, Elg SA, Brueske L. Comparison of probe sheaths for endovaginal sonography. Obstet. Gynecol 1996;87:27-9.

Milki AA, Fisch JD. Vaginal ultrasound probe cover leakage: implications for patient care. Fertil Steril

1998;69:409-11.

Hignett M, Claman P. High rates of perforation are found in endovaginal ultrasound probe covers before and after oocyte retrieval for in vitro fertilization-embryo transfer. J Assist Reprod Genet 1995;12:606-9.

Sterilization and Disinfection of Medical Devices: General Principles. Centers for Disease Control, Division of Healthcare Quality Promotion. http://www.cdc.gov/ncidod/hip/sterile/sterilgp.htm (5-2003).

ODE Device Evaluation Information--FDA Cleared Sterilants and High Level Disinfectants with General Claims for Processing Reusable Medical and Dental Devices, March 2003. http://www.fda.gov/cdrh/ode/germlab.html (5-2003).

9.3 Probe Operation Instructions

Instruction for details on connecting, activating, deactivating, disconnecting, transporting and storing the probes.

9.3.1 Scanning the Patient

In order to assure optimal transmission of energy between the patient and probe, a conductive gel must be applied liberally to the patient where scanning will be performed.

After the examination is complete, follow the cleaning and disinfecting, or sterilizing procedures as appropriate.

9.3.2 Operating Transvaginal probe

The transvaginal probe is an endo-cavity probe, for the operation safety, please refer to "Care and Maintenance" for cleaning and disinfection.

The temperature at the tip of the probe displays on the screen for monitoring. No temperature above 43° C is allowed. It also depends on the patient's body temperature. When the temperature of probe tip exceeds 43° C, the probe will stop working immediately to protect the patient.

Transvaginal probe should be used with FDA approved condom or probe cover. See the following instructions to put the probe into the condom:

ACAUTION

- ✓ Some patients may be allergic to natural rubber or medical device with rubber contains. FDA suggests that the user to identify these patients and be prepared to treat allergic reactions promptly before scanning.
- ✓ Only water-solvable solutions or gel can be used. Petroleum or mineral oil-based materials may harm the cover.
- ✓ When the transvaginal probe is activated outside patient's body, its acoustic output level should be decreased to avoid any harmful interference with other equipment.

Operation Procedure:

- 1. Put on medical sterile glove
- 2. Get the condom for the package.
- 3. Unfold the condom.
- 4. Load some ultrasound gel into condom.
- 5. Take the condom with one hand, and put the probe head into the condom.
- 6. Fasten the condom on the end of the probe handle.
- 7 . Confirm the integrity of the condom, and repeat the above steps to the condom if any damage to the condom is found.

9.3.3 Cleaning and Disinfecting TV and TR Probes

We strongly recommend wearing gloves when cleaning and disinfecting any endocavitary probe.

- Every time before and after each exam, please clean the probe handle and disinfect the transvaginal and transrectal probes using liquid chemical germicides
- If the probe is contaminated with body fluids, you should disinfect the probe after cleaning.
- Regard any exam waste as potentially infectious and dispose of it accordingly.

ACAUTION

✓ Since the probe is not waterproof, you should disconnect it from the system before cleaning or

disinfecting.

Before and after each exam, please clean the probe handle and disinfect the transvaginal and transrectal probes using liquid chemical germicides.

Cleaning

You can clean the transvaginal and transrectal probes to remove all coupling gel by wiping with a soft cloth and rinsing with flowing water. Then wash the probe with mild soap in lukewarm water. Scrub the probe as needed and use a soft cloth to remove all visible residues from the transvaginal probe surface. Rinse the probe with enough clean potable water to remove all visible soap residues, and let the probe air dry.

\triangle CAUTION

- ✓ Please remove the cover (if any) before cleaning the probe.(The cover like condom is one time usable).
- ✓ When cleaning the TV and TR probes, it is important to be sure that all surfaces are thoroughly cleaned.

◆ Disinfecting

Cidex is the only germicide that has been evaluated for compatibility with the material used to construct the probes.

To keep the effectiveness of the disinfection solutions, a thoroughly cleaning must be done to the probe before the disinfecting, make sure no residues remain on the probe.

◆ Disinfecting Procedure:

- 1 . Following all precautions for storage, use and disposal, prepare the germicide solution according to the manufacturer's instructions.
- 2 . Place the cleaned and dried probe to contact with the germicide, being careful not to let the probe drop to the bottom of the container and thus damage the probe.
- 3 . After placing/immersing, rotate and shake the probe while it is below the surface of the germicide to eliminate air pockets. Allow the germicide to remain in contact with the fully immersed probe. For high level disinfection, follow the manufacturer's recommended time.

- 4 . Following all precautions for storage, use and disposal, prepare the germicide solution according to the manufacturer's instructions.
- 5 . After removing from the germicide, rinse the probe according to the germicide manufacturer's rinsing instructions.
- 6 . Flush all visible germicide residues from the probe and allow to air dry.

Appendix A: Acoustic Output Report Table

Transducer Model: <u>C3-E</u>

Operating Mode: B

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
	pobal Maximum Index Value $ \begin{array}{c ccccccccccccccccccccccccccccccccccc$			Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	i mum Index Value		0.7	1.0				
	p _{r.3}	(MPa)	1.32					
	Wo	(mW)		511.48				
		(mW)						
	Z 1	(cm)						
	Z _{bp}	(cm)						
	Z _{sp}	(cm)						
Parameter	z@PII.3max	(cm)	6.5					
	$d_{eq}(z_{sp})$	(cm)						
	fc	(MHz)	2.73	2.75				
	Dina of A	X (cm)		4.61				
	DIM Of A _{aprt}	Y (cm)		1.10				
	PD	(µsec)	0.55					
	PRF	(Hz)	9662					
	p _r @PII _{max}	(MPa)	2.35					
	d _{eq} @PII _{max}	(cm)						
Information		FL _x (cm)		0.21				
	Focal Length	FLy (cm)		0.33				
	I _{PA.3} @ MI _{max}	(W/cm ²)	75.41					
Operating	Mode	NA	В	В				
Control	Focus	(cm)	7	7				
Conditions	Power	(%)	100	100				

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: <u>C3-E</u>
Operating Mode: <u>THI-B</u>

					TIS		TIB	
	Index Label		МІ	0	non-	scan		TIC
	Maximum Index Value			Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value	_	0.7	0.7				
	p _{r.3}	(MPa)	1.24					
	Wo	(mW)		511.48				
		(mW)						
	Z 1	(cm)						
Associated	Z _{bp}	(cm)						
Acoustic Parameter	Z _{sp}	(cm)						
Parameter	z@PII.3max	(cm)	6.5					
	$d_{eq}(z_{sp})$	(cm)						
	fc	(MHz)	2.74	2.74				
	Dim of A	X (cm)		4.61				
	DIM Of Aaprt	Y (cm)		1.10				
	PD	(µsec)	0.54					
	PRF	(Hz)	9668					
011	p _r @PII _{max}	(MPa)	2.35					
Other Information	d _{eq} @PII _{max}	(cm)						
iniormation	Farall amouth	FL _x (cm)		0.24				
	Focal Length	FLy (cm)		0.31				
	I _{PA.3} @ MI _{max}	(W/cm ²)	75.39					
Operating	Mode	NA	THI-B	THI-B				
Control	Focus	(cm)	7	7				
Conditions	Power	(%)	100	100				

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: <u>C3-E</u>
Operating Mode: <u>B+C</u>

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.5	0.6				
	Pr.3	(MPa)	0.92					
	Wo	(mW)		345.59				
	min of [W _{.3} (z ₁), $I_{TA.3}(z_1)$]	(mW)						
	Z1	(cm)						
Associated	Z _{bp}	(cm)						
Acoustic Parameter	Z _{sp}	(cm)						
Farameter	z@PII.3max	(cm)	6.2					
	$d_{eq}(z_{sp})$	(cm)						
	fc	(MHz)	2.90	2.89				
	Dim of A	X (cm)		4.61				
	Dim of A _{aprt}	Y (cm)		1.10				
	PD	(µsec)	1.32					
	PRF	(Hz)	6012					
011	p _r @PII _{max}	(MPa)	1.65					
Other Information	d _{eq} @PII _{max}	(cm)						
Iniormation	Farall annih	FL _x (cm)		0.21				
	Focal Length	FLy (cm)		0.31				
	I _{PA.3} @ MI _{max}	(W/cm ²)	35.25					
Operating	Mode	NA	С	С				
Control	Focus	(cm)	6	6				
Conditions	Power	(%)	100	100				

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: <u>C3-E</u>
Operating Mode: <u>B+C+PW</u>

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
	$ \begin{array}{c ccccccccccccccccccccccccccccccccccc$			Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.5			1.8	1.0	
	Pr.3	(MPa)	0.84					
	Wo	(mW)					621.55	
		(mW)				276.05		
	Z1	(cm)				4.1		
	Z _{bp}	(cm)				3.8		
	Z _{sp}	(cm)					6.5	
Parameter	z@PII.3max	(cm)	4.4					
	$d_{eq}(z_{sp})$	(cm)					0.67	
	fc	(MHz)	2.88			2.85	2.82	
	Dim of A	X (cm)				4.61	4.61	
	DIM Of Aaprt	Y (cm)				1.10	1.10	
	PD	(µsec)	1.29					
	PRF	(Hz)	9659					
045	pr@PII _{max}	(MPa)	1.43					
	d _{eq} @PII _{max}	(cm)					0.63	
iniormation	Facal Lamenth	FL _x (cm)				0.31		
	Focal Length	FLy (cm)				0.41		
	I _{PA.3} @ MI _{max}	(W/cm ²)	129.62					
Operating	Mode	NA	PW			PW	PW	
Control	Focus	(cm)	6			7	10	
Conditions	Power	(%)	100			100	100	

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: <u>C3-E</u>

Operating Mode: M

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
	$ \begin{array}{c ccccccccccccccccccccccccccccccccccc$			Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		1.1			1.9	1.2	
	Pr.3	(MPa)	1.57					
	Wo	(mW)					511.21	
		(mW)				227.42		
	Z1	(cm)				4.2		
	Z _{bp}	(cm)				3.8		
	Z _{sp}	(cm)					5.1	
Parameter	z@PII.3max	(cm)	5.5					
	$d_{eq}(z_{sp})$	(cm)					0.81	
	fc	(MHz)	2.71			2.77	2.74	
	Dim of A	X (cm)				4.61	4.61	
	DITTI OI Aaprt	Y (cm)				1.10	1.10	
	PD	(µsec)	0.55					
	PRF	(Hz)	4756					
045	pr@PII _{max}	(MPa)	2.66					
	d _{eq} @PII _{max}	(cm)					0.8	
iniormation	Facal Lawath	FL _x (cm)				0.23		
	Focal Length	FLy (cm)				0.18		
	I _{PA.3} @ MI _{max}	(W/cm ²)	111.26					
Operating	Mode	NA	М			М	M	
Control	Focus	(cm)	7			6	6	
Conditions	Power	(%)	100			100	100	

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: <u>V4-EV</u>

Operating Mode: B

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	i mum Index Value		0.7	1.0				
	p _{r.3}	(MPa)	1.32					
	Wo	(mW)		511.48				
	min of [W.3(Z1), I _{TA.3} (Z1)]	(mW)						
^ : - t !	Z 1	(cm)						
Associated	Z _{bp}	(cm)						
Acoustic	Z _{sp}	(cm)						
Parameter	z@PII.3max	(cm)	6.5					
	$d_{eq}(z_{sp})$	(cm)						
	f _c	(MHz)	2.73	2.75				
	Dim of A	X (cm)		4.61				
	Dim of A _{aprt}	Y (cm)		1.10				
	PD	(µsec)	0.55					
	PRF	(Hz)	9662					
Other	pr@PII _{max}	(MPa)	2.35					
	d _{eq} @PII _{max}	(cm)						
Information	Canal Law with	FL _x (cm)		0.21				
	Focal Length	FLy (cm)		0.33				
	I _{PA.3} @ MI _{max}	(W/cm ²)	75.41					
Operating	Mode	NA	В	В				
Control	Focus	(cm)	7	7				
Conditions	Power	(%)	100	100				_

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: <u>V4-EV</u>

Operating Mode: THI-B

					TIS		TIB	
	$\begin{array}{c} W_{o} \\ \text{min of } [W_{.3}(z_{1}), \\ I_{TA.3}(z_{1})] \\ z_{1} \\ z_{bp} \\ z_{coustic} \\ z_{sp} \\ z@PII_{.3max} \\ d_{eq}(z_{sp}) \\ f_{c} \\ Dim of A_{aprt} \\ \hline \\ PD \\ PRF \\ p_{r}@PII_{max} \\ d_{eq}@PII_{max} \\ d_{eq}@PII_{max} \\ \end{array}$		МІ	Coon	non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value	T	0.7	0.7				
	p _{r.3}	(MPa)	1.24					
	Wo	(mW)		511.48				
		(mW)						
	Z1	(cm)						
	Z _{bp}	(cm)						
	Z _{sp}	(cm)						
Parameter	z@PII.3max	(cm)	6.5					
	$d_{eq}(z_{sp})$	(cm)						
	fc	(MHz)	2.74	2.74				
	Dim of A	X (cm)		4.61				
	DIM Of Aaprt	Y (cm)		1.10				
	PD	(µsec)	0.54					
	PRF	(Hz)	9668					
011	p _r @PII _{max}	(MPa)	2.35					
Information	d _{eq} @PII _{max}	(cm)						
iniormation	- II (I	FL _x (cm)		0.24				
	Focal Length	FLy (cm)		0.31				
	IPA.3@ MI _{max}	(W/cm ²)	75.39					
Operating	Mode	NA	THI-B	THI-B				
Control	Focus	(cm)	7	7				
Conditions	Power	(%)	100	100				

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: <u>V4-EV</u>
Operating Mode: <u>B+C</u>

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
	Acoustic Parameter P_{c} P			Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.5	0.6				
	pr.3	(MPa)	0.92					
	Wo	(mW)		345.59				
		(mW)						
	Z1	(cm)						
	Z _{bp}	(cm)						
	Z _{sp}	(cm)						
Parameter	z@PII.3max	(cm)	6.2					
	$d_{eq}(z_{sp})$	(cm)						
	fc	(MHz)	2.90	2.89				
	Dim of A	X (cm)		4.61				
	DITTI OI Aaprt	Y (cm)		1.10				
	PD	(µsec)	1.32					
	PRF	(Hz)	6012					
011	pr@PII _{max}	(MPa)	1.65					
	d _{eq} @PII _{max}	(cm)						
iniormation	F	FL _x (cm)		0.21				
	Focal Length	FLy (cm)		0.31				
	IPA.3@ MImax	(W/cm ²)	35.25					
Operating	Mode	NA	С	С				
Control	Focus	(cm)	6	6				
Conditions	Power	(%)	100	100				

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: V4-EV
Operating Mode: B+C+PW

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
	$ \begin{array}{c ccccccccccccccccccccccccccccccccccc$			Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.5			1.8	1.0	
	Pr.3	(MPa)	0.84					
	Wo	(mW)					621.55	
		(mW)				276.05		
	Z1	(cm)				4.1		
	Z _{bp}	(cm)				3.8		
	Z _{sp}	(cm)					6.5	
Parameter	z@PII.3max	(cm)	4.4					
	$d_{eq}(z_{sp})$	(cm)					0.67	
	fc	(MHz)	2.88			2.85	2.82	
	Dim of A	X (cm)				4.61	4.61	
	DIM Of Aaprt	Y (cm)				1.10	1.10	
	PD	(µsec)	1.29					
	PRF	(Hz)	9659					
045	pr@PII _{max}	(MPa)	1.43					
	d _{eq} @PII _{max}	(cm)					0.63	
iniormation	Facal Lamenth	FL _x (cm)				0.31		
	Focal Length	FLy (cm)				0.41		
	I _{PA.3} @ MI _{max}	(W/cm ²)	129.62					
Operating	Mode	NA	PW			PW	PW	
Control	Focus	(cm)	6			7	10	
Conditions	Power	(%)	100			100	100	

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: <u>V4-EV</u>

Operating Mode: M

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
	$ \begin{array}{c ccccccccccccccccccccccccccccccccccc$			Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		1.1			1.9	1.2	
	Pr.3	(MPa)	1.57					
	Wo	(mW)					511.21	
		(mW)				227.42		
	Z1	(cm)				4.2		
	Z _{bp}	(cm)				3.8		
	Z _{sp}	(cm)					5.1	
Parameter	z@PII.3max	(cm)	5.5					
	$d_{eq}(z_{sp})$	(cm)					0.81	
	fc	(MHz)	2.71			2.77	2.74	
	Dim of A	X (cm)				4.61	4.61	
	DITTI OI Aaprt	Y (cm)				1.10	1.10	
	PD	(µsec)	0.55					
	PRF	(Hz)	4756					
045	pr@PII _{max}	(MPa)	2.66					
	d _{eq} @PII _{max}	(cm)					0.8	
iniormation	Facal Lawath	FL _x (cm)				0.23		
	Focal Length	FLy (cm)				0.18		
	I _{PA.3} @ MI _{max}	(W/cm ²)	111.26					
Operating	Mode	NA	М			М	M	
Control	Focus	(cm)	7			6	6	
Conditions	Power	(%)	100			100	100	

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: <u>L7-E</u>

Operating Mode: B

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
		(MPa) 2.41 (mW) (mW) (mW) (mW) (mW) (mW) (mm) (mm)		Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.9	0.5				
	pr.3	(MPa)	2.41					
	Wo	(mW)		73.73				
	min of [W _{.3} (z_1), $I_{TA.3}(z_1)$]	(mW)						
	Z1	(cm)						
Associated	Z _{bp}	(cm)						
Acoustic Parameter	Z _{Sp}	(cm)						
Parameter	z@PII.3max	(cm)	2.2					
	$d_{eq}(z_{sp})$	(cm)						
	fc	(MHz)	6.23	6.25				
	Dim of A	X (cm)		2.05				
	Dim of A _{aprt}	Y (cm)		0.45				
	PD	(µsec)	0.23					
	PRF	(Hz)	2872					
045	p _r @PII _{max}	(MPa)	3.37					
Other Information	d _{eq} @PII _{max}	(cm)						
iniormation	Canal Lawreth	FL _x (cm)		0.26				
	Focal Length	FLy (cm)		0.36				
	IPA.3@ MImax	(W/cm ²)	43.96					
Operating	Mode	NA	В	В				
Control	Focus	(cm)	2	2				
Conditions	Power	(%)	100	100				

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: <u>L7-E</u>
Operating Mode: <u>THI-B</u>

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		1.0	0.4				
	Pr.3	(MPa)	2.32					
	Wo	(mW)		73.73				
	min of [W _{.3} (z ₁), $I_{TA.3}(z_1)$]	(mW)						
	Z1	(cm)						
Associated	Z _{bp}	(cm)						
Acoustic Parameter	Z _{sp}	(cm)						
Parameter	z@PII.3max	(cm)	2.1					
	$d_{eq}(z_{sp})$	(cm)						
	fc	(MHz)	6.21	6.22				
	Dim of A	X (cm)		2.05				
	Dim of A _{aprt}	Y (cm)		0.45				
	PD	(µsec)	0.23					
	PRF	(Hz)	2874					
011	p _r @PII _{max}	(MPa)	3.37					
Other Information	d _{eq} @PII _{max}	(cm)						
iniormation	Facal Law with	FL _x (cm)		0.26				
	Focal Length	FLy (cm)		0.34				
	I _{PA.3} @ MI _{max}	(W/cm ²)	43.89					
Operating	Mode	NA	THI-B	THI-B				
Control	Focus	(cm)	2	2				
Conditions	Power	(%)	100	100				

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: <u>L7-E</u>
Operating Mode: <u>B+C</u>

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.6	0.7				
	Pr.3	(MPa)	1.38					
	Wo	(mW)		106.50				
	min of [W _{.3} (z ₁), $I_{TA.3}(z_1)$]	(mW)						
	Z1	(cm)						
Associated	Z _{bp}	(cm)						
Acoustic Parameter	Z _{sp}	(cm)						
Parameter	z@PII.3max	(cm)	1.7					
	$d_{eq}(z_{sp})$	(cm)						
	fc	(MHz)	6.36	6.35				
	Dim of A	X (cm)		2.05				
	Dim of A _{aprt}	Y (cm)		0.45				
	PD	(µsec)	0.77					
	PRF	(Hz)	6944					
011	pr@PII _{max}	(MPa)	1.92					
Other Information	d _{eq} @PII _{max}	(cm)						
iniormation	Facal Lamenth	FL _x (cm)		0.23				
	Focal Length	FLy (cm)		0.35				
	IPA.3@ MI _{max}	(W/cm ²)	91.42					
Operating	Mode	NA	С	С				
Control	Focus	(cm)	2.5	1				
Conditions	Power	(%)	100	100				

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: <u>L7-E</u>
Operating Mode: <u>B+C+PW</u>

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.6		1.6		1.4	
	Pr.3	(MPa)	1.59					
	Wo	(mW)			221.18		73.73	
	min of [W _{.3} (z ₁), I _{TA.3} (z ₁)]	(mW)						
	Z1	(cm)						
Associated	Z _{bp}	(cm)						
Acoustic	Z _{sp}	(cm)					1.9	
Parameter	z@PII.3max	(cm)	1.7					
	$d_{eq}(z_{sp})$	(cm)					0.42	
	fc	(MHz)	6.34		6.22		6.31	
	Dim of A	X (cm)			2.05		2.05	
	Dim of A _{aprt}	Y (cm)			0.45		0.45	
	PD	(µsec)	0.58					
	PRF	(Hz)	2873					
011	p _r @PII _{max}	(MPa)	2.14					
Other Information	d _{eq} @PII _{max}	(cm)					0.44	
iniormation	Facal Lamenth	FL _x (cm)			0.24			
	Focal Length	FLy (cm)			0.33			
	I _{PA.3} @ MI _{max}	(W/cm ²)	118.84					
Operating	Mode	NA	PW		PW		PW	
Control	Focus	(cm)	4		2.5		2.5	
Conditions	Power	(%)	100		100		100	

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: <u>L7-E</u>

Operating Mode: M

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.7		1.2		1.6	
	Pr.3	(MPa)	1.89					
	Wo	(mW)			139.30		139.30	
	min of [W _{.3} (z ₁), I _{TA.3} (z ₁)]	(mW)						
	Z1	(cm)						
Associated	Z _{bp}	(cm)						
Acoustic	Z _{sp}	(cm)					1.8	
Parameter	z@PII.3max	(cm)	1.6					
	$d_{eq}(z_{sp})$	(cm)					0.89	
	fc	(MHz)	6.19		6.22		6.19	
	Dim of A	X (cm)			2.05		2.05	
	Dim of A _{aprt}	Y (cm)			0.45		0.45	
	PD	(µsec)	0.22					
	PRF	(Hz)	2866					
011	p _r @PII _{max}	(MPa)	2.60					
Other Information	d _{eq} @PII _{max}	(cm)					0.87	
iniormation	Facal Lamenth	FL _x (cm)			0.22			
	Focal Length	FLy (cm)			0.36			
	I _{PA.3} @ MI _{max}	(W/cm ²)	158.26					
Operating	Mode	NA	М		М		M	
Control	Focus	(cm)	2		1.5		2	
Conditions	Power	(%)	100		100		100	

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: V6-E

Operating Mode: B

					TIS non-scan Aaprt≤1 Aap		TIB	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.7	0.4				
	Pr.3	(MPa)	1.49					
	Wo	(mW)		43.78				
	min of [W _{.3} (z ₁), $I_{TA.3}(z_1)$]	(mW)						
	Z1	(cm)						
Associated	Z _{bp}	(cm)						
Acoustic Parameter	Z _{sp}	(cm)						
Parameter	z@PII.3max	(cm)	2.5					
	$d_{eq}(z_{sp})$	(cm)						
	fc	(MHz)	4.94	5.14				
	Dim of A	X (cm)		1.21				
	Dim of A _{aprt}	Y (cm)		0.90				
	PD	(µsec)	0.34					
	PRF	(Hz)	7286					
011	pr@PII _{max}	(MPa)	1.95					
Other Information	d _{eq} @PII _{max}	(cm)						
iniormation	Facal Lawath	FL _x (cm)		0.29				
	Focal Length	FLy (cm)		0.26				
	IPA.3@ MI _{max}	(W/cm ²)	62.76					
Operating	Mode	NA	В	В				
Control	Focus	(cm)	3	2				
Conditions	Power	(%)	100	100				

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: <u>V6-E</u>
Operating Mode: <u>THI-B</u>

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.6	0.3				
	Pr.3	(MPa)	1.42					
	Wo	(mW)		43.78				
	min of [W _{.3} (z ₁), I _{TA.3} (z ₁)]	(mW)						
	Z1	(cm)						
Associated	Z _{bp}	(cm)						
Acoustic Parameter	Z _{Sp}	(cm)						
Parameter	z@PII.3max	(cm)	2.5					
	$d_{eq}(z_{sp})$	(cm)						
	f _c	(MHz)	4.92	5.14				
	Dim of A	X (cm)		1.21				
	Dim of A _{aprt}	Y (cm)		0.90				
	PD	(µsec)	0.33					
	PRF	(Hz)	7279					
Othern	pr@PII _{max}	(MPa)	1.95					
Other Information	d _{eq} @PII _{max}	(cm)						
IIIIOIIIIalioii	Facal Lamenth	FL _x (cm)		0.29				
	Focal Length	FLy (cm)		0.26				
	IPA.3@ MI _{max}	(W/cm ²)	62.74					
Operating	Mode	NA	THI-B	THI-B				
Control	Focus	(cm)	3	2				
Conditions	Power	(%)	100	100				

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: V6-E
Operating Mode: B+C

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.4	0.7				
	pr.3	(MPa)	0.89					
	Wo	(mW)		77.82				
	min of [W _{.3} (z ₁), $I_{TA.3}(z_1)$]	(mW)						
	Z1	(cm)						
Associated	Z _{bp}	(cm)						
Acoustic Parameter	Z _{Sp}	(cm)						
Parameter	z@PII.3max	(cm)	3.4					
	$d_{eq}(z_{sp})$	(cm)						
	fc	(MHz)	4.03	5.25				
	Dim of A	X (cm)		1.21				
	Dim of A _{aprt}	Y (cm)		0.90				
	PD	(µsec)	1.19					
	PRF	(Hz)	5000.23					
Othern	pr@PII _{max}	(MPa)	1.29					
Other Information	d _{eq} @PII _{max}	(cm)						
IIIIOIIIIalioii	Facal Law with	FL _x (cm)		0.22				
	Focal Length	FLy (cm)		0.34				
	IPA.3@ MI _{max}	(W/cm ²)	34.32					
Operating	Mode	NA	С	С				
Control	Focus	(cm)	4	2.5				
Conditions	Power	(%)	100	100				

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: V6-E
Operating Mode: B+C+PW

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.5			1.1	1.8	
	Pr.3	(MPa)	1.17					
	Wo	(mW)					72.88	
	min of [W _{.3} (z ₁), I _{TA.3} (z ₁)]	(mW)				38.11		
	Z1	(cm)				1.8		
Associated	Z _{bp}	(cm)				1.8		
Acoustic	Z _{sp}	(cm)					2.0	
Parameter	z@PII.3max	(cm)	2.4					
	$d_{eq}(z_{sp})$	(cm)					0.44	
	fc	(MHz)	5.21			5.22	5.17	
	Dina of A	X (cm)				1.21	1.21	
	Dim of A _{aprt}	Y (cm)				0.90	0.90	
	PD	(µsec)	0.70					
	PRF	(Hz)	7279					
011	pr@PII _{max}	(MPa)	1.54					
Other	d _{eq} @PII _{max}	(cm)					0.42	
Information	F 11 (1	FL _x (cm)				0.24		
	Focal Length	FLy (cm)				0.22		
	I _{PA.3} @ MI _{max}	(W/cm ²)	142.89					
Operating	Mode	NA	PW			PW	PW	
Control	Focus	(cm)	3			3.5	3.5	
Conditions	Power	(%)	100			100	100	

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: V6-E

Operating Mode: M

				Scan non-scan non-scan Aaprt≤1 Aaprt>1 0.4 1.1 1.7 24.3 13.24 1.8 1.8 2.1 3.3 0.23 4.87 4.85 1.21 1.24 0.90 0.90 1 0.90 0.23 0.23 0.35 0.27	TIB			
	Index Label		МІ	_	non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.7			0.4	1.1	
	pr.3	(MPa)	1.77					
	Wo	(mW)					24.32	
	min of [W _{.3} (z_1), $I_{TA.3}(z_1)$]	(mW)				13.24		
	Z1	(cm)				1.8		
Associated	Zbp	(cm)				1.8		
Acoustic Parameter	Z _{Sp}	(cm)					2.1	
	z@PII.3max	(cm)	2.3					
	$d_{eq}(z_{sp})$	(cm)					0.23	
	f _c	(MHz)	4.87			4.87	4.85	
	Dim of A	X (cm)				1.21	1.21	
	Dim of A _{aprt}	Y (cm)				0.90	0.90	
	PD	(µsec)	0.31					
	PRF	(Hz)	7273					
011	pr@PII _{max}	(MPa)	2.29					
Other	d _{eq} @PII _{max}	(cm)					0.23	
Information	- II #	FL _x (cm)				0.35		
	Focal Length	FLy (cm)				0.27		
	IPA.3@ MImax	(W/cm ²)	120.55					
Operating	Mode	NA	М			М	М	
Control	Focus	(cm)	3			3	3	
Conditions	Power	(%)	100			100	100	

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: P3-E

Operating Mode: B

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		1.2	1.7				
	pr.3	(MPa)	1.84					
	Wo	(mW)		269.95				
	min of [W _{.3} (z_1), $I_{TA.3}(z_1)$]	(mW)						
	Z1	(cm)						
Associated	Z _{bp}	(cm)						
Acoustic Parameter	Z _{sp}	(cm)						
Parameter	z@PII.3max	(cm)	4.5					
	$d_{eq}(z_{sp})$	(cm)						
	f _c	(MHz)	2.28	2.38				
	Dim of A	X (cm)		1.92				
	Dim of A _{aprt}	Y (cm)		1.58				
	PD	(µsec)	0.97					
	PRF	(Hz)	3337.5					
045	p _r @PII _{max}	(MPa)	3.83					
Other Information	d _{eq} @PII _{max}	(cm)						
iniormation	F	FL _x (cm)		0.32				
	Focal Length	FLy (cm)		0.24				
	IPA.3@ MImax	(W/cm ²)	98.54					
Operating	Mode	NA	В	В				
Control	Focus	(cm)	4	1				
Conditions	Power	(%)	100	100				

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: P3-E
Operating Mode: THI-B

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		1.2	1.5				
	Pr.3	(MPa)	1.76					
	Wo	(mW)		269.95				
	min of [W _{.3} (z ₁), $I_{TA.3}(z_1)$]	(mW)						
	Z1	(cm)						
Associated	Z _{bp}	(cm)						
Acoustic Parameter	Z _{sp}	(cm)						
Parameter	z@PII.3max	(cm)	4.5					
	$d_{eq}(z_{sp})$	(cm)						
	fc	(MHz)	2.25	2.44				
	Dim of A	X (cm)		1.92				
	Dim of A _{aprt}	Y (cm)		1.58				
	PD	(µsec)	0.97					
	PRF	(Hz)	3336					
011	p _r @PII _{max}	(MPa)	3.83					
Other Information	d _{eq} @PII _{max}	(cm)						
iniormation	Facal Law with	FL _x (cm)		0.36				
	Focal Length	FLy (cm)		0.22				
	I _{PA.3} @ MI _{max}	(W/cm ²)	98.50					
Operating	Mode	NA	THI-B	THI-B				
Control	Focus	(cm)	4	1				
Conditions	Power	(%)	100	100				

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: P3-E
Operating Mode: B+C

					TIS		TIB non-scan	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.9	0.5				
	pr.3	(MPa)	1.35					
	Wo	(mW)		92.18				
	min of [W _{.3} (z_1), $I_{TA.3}(z_1)$]	(mW)						
	Z1	(cm)						
Associated	Z _{bp}	(cm)						
Acoustic Parameter	Z _{sp}	(cm)						
Parameter	z@PII.3max	(cm)	3.6					
	$d_{eq}(z_{sp})$	(cm)						
	fc	(MHz)	2.25	2.29				
	Dim of A	X (cm)		1.92				
	Dim of A _{aprt}	Y (cm)		1.58				
	PD	(µsec)	1.69					
	PRF	(Hz)	5948					
045	p _r @PII _{max}	(MPa)	1.76					
Other Information	d _{eq} @PII _{max}	(cm)						
iniormation	Canal Lawreth	FL _x (cm)		0.27				
	Focal Length	FLy (cm)		0.32				
	IPA.3@ MImax	(W/cm ²)	57.36					
Operating	Mode	NA	С	С				
Control	Focus	(cm)	4	1				
Conditions	Power	(%)	100	100				

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: <u>P3-E</u> Operating Mode: <u>B+C+PW</u>

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.8			0.5	1.2	
	Pr.3	(MPa)	1.25					
	Wo	(mW)					122.88	
	min of [W _{.3} (z ₁), I _{TA.3} (z ₁)]	(mW)				80.74		
	Z1	(cm)				3.1		
Associated	Z _{bp}	(cm)				2.9		
Acoustic Parameter	Z _{sp}	(cm)					5.4	
Parameter	z@PII.3max	(cm)	6.0					
	$d_{eq}(z_{sp})$	(cm)					0.40	
	fc	(MHz)	1.99			1.98	1.99	
	Dim of A	X (cm)				1.92	1.92	
	Dim of A _{aprt}	Y (cm)				1.58	1.58	
	PD	(µsec)	1.83					
	PRF	(Hz)	5049					
011	pr@PII _{max}	(MPa)	1.81					
Other Information	d _{eq} @PII _{max}	(cm)					0.40	
iniormation	Facal Lawath	FL _x (cm)				0.32		
	Focal Length	FLy (cm)				0.39		
	I _{PA.3} @ MI _{max}	(W/cm ²)	150.40					
Operating	Mode	NA	PW			PW	PW	
Control	Focus	(cm)	1			1	1	
Conditions	Power	(%)	100			100	100	

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: P3-E

Operating Mode: M

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		1.2			0.8	1.4	
	Pr.3	(MPa)	1.64					
	Wo	(mW)					89.20	
	min of [W _{.3} (z ₁), $I_{TA.3}(z_1)$]	(mW)				30.72		
	Z1	(cm)				2.9		
Associated	Z _{bp}	(cm)				2.9		
Acoustic Parameter	Z _{sp}	(cm)					2.9	
Parameter	z@PII.3max	(cm)	2.6					
	$d_{eq}(z_{sp})$	(cm)					0.44	
	fc	(MHz)	1.88			1.89	1.88	
	Dim of A	X (cm)				1.92	1.92	
	Dim of A _{aprt}	Y (cm)				1.58	1.58	
	PD	(µsec)	0.45					
	PRF	(Hz)	5543					
011	pr@PII _{max}	(MPa)	1.59					
Other Information	d _{eq} @PII _{max}	(cm)					0.33	
iniormation	Facal Lawath	FL _x (cm)				0.28		
	Focal Length	FLy (cm)				0.34		
	IPA.3@ MI _{max}	(W/cm ²)	189.20					
Operating	Mode	NA	М			М	М	
Control	Focus	(cm)	5			5	6	
Conditions	Power	(%)	100			100	100	

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: <u>P3-E</u> Operating Mode: <u>B+C+CW</u>

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		1.2	0.3			0.7	1.7
	p _{r.3}	(MPa)	0.42					
	Wo	(mW)					178.00	172.00
	min of [W _{.3} (z ₁), $I_{TA.3}(z_1)$]	(mW)				79.00		
	Z1	(cm)				5.4		
Associated	Z _{bp}	(cm)				2.0		
Acoustic Parameter	Z _{sp}	(cm)					6.7	
Parameter	z@PII.3max	(cm)	6.8					
	d _{eq} (z _{sp})	(cm)					0.80	
	f _c	(MHz)	2.65			2.75	2.70	2.75
	Dim of A	X (cm)				1.92	1.92	1.92
	Dim of A _{aprt}	Y (cm)				1.58	1.58	1.58
	PD	(µsec)	26.00					
	PRF	(Hz)	0					
011	pr@PII _{max}	(MPa)	0.12					
Other Information	d _{eq} @PII _{max}	(cm)					0.81	
IIIIOIIIIalioii	Facal Law with	FL _x (cm)				0.42		0.43
	Focal Length	FLy (cm)				0.32		0.30
	IPA.3@ MI _{max}	(W/cm ²)	38.96					
Operating	Mode	NA	CW			CW	CW	CW
Control	Focus	(cm)	3			5	6	6
Conditions	Power	(%)	100			100	100	100

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: <u>P3-E</u>
Operating Mode: <u>CFM-M</u>

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		1.1			0.1	0.8	
	p _{r.3}	(MPa)	1.51					
	Wo	(mW)					254.00	
	min of [W _{.3} (z ₁), $I_{TA.3}(z_1)$]	(mW)				12.49		
	Z1	(cm)				6.1		
Associated	Z _{bp}	(cm)				2.8		
Acoustic Parameter	Z _{sp}	(cm)					6.2	
Parameter	z@PII.3max	(cm)	6.1					
	$d_{eq}(z_{sp})$	(cm)					3.08	
	f _c	(MHz)	2.36			2.36	2.35	
	Dim of A	X (cm)				1.92	1.92	
	Dim of A _{aprt}	Y (cm)				1.58	1.58	
	PD	(µsec)	0.71					
	PRF	(Hz)	200					
011	pr@PII _{max}	(MPa)	2.61					
Other Information	d _{eq} @PII _{max}	(cm)					3.01	
IIIIOIIIIalioii	Facal Law with	FL _x (cm)				0.42		
	Focal Length	FLy (cm)				0.54		
	IPA.3@ MI _{max}	(W/cm ²)	82.33					
Operating	Mode	NA	CFM-M			CFM-M	CFM-M	
Control	Focus	(cm)	4			5	6	
Conditions	Power	(%)	100			100	100	

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: <u>L12-E</u>

Operating Mode: B

					TIS		TIB	
	Index Label		MI		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.6	0.1				
	Pr.3	(MPa)	1.39					
	Wo	(mW)		8.19				
	min of [W _{.3} (z_1), $I_{TA.3}(z_1)$]	(mW)						
	Z1	(cm)						
Associated	Z _{bp}	(cm)						
Acoustic Parameter	Z _{sp}	(cm)						
Parameter	z@PII.3max	(cm)	1.8					
	$d_{eq}(z_{sp})$	(cm)						
	fc	(MHz)	5.91	5.91				
	Dina of A	X (cm)		2.05				
	Dim of A _{aprt}	Y (cm)		0.45				
	PD	(µsec)	0.23					
	PRF	(Hz)	5319					
011	pr@PII _{max}	(MPa)	2.03					
Other Information	d _{eq} @PII _{max}	(cm)						
inionnation	Facal Law with	FL _x (cm)		0.33				
	Focal Length	FLy (cm)		0.24				
	IPA.3@ MI _{max}	(W/cm ²)	84.56					
Operating	Mode	NA	В	В				
Control	Focus	(cm)	2.5	2.5				
Conditions	Power	(%)	100	100				

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: <u>L12-E</u>
Operating Mode: <u>THI-B</u>

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.6	0.1				
	Pr.3	(MPa)	1.39					
	Wo	(mW)		8.19				
	min of [W _{.3} (z_1), $I_{TA.3}(z_1)$]	(mW)						
	Z1	(cm)						
Associated	Z _{bp}	(cm)						
Acoustic Parameter	Z _{sp}	(cm)						
Parameter	z@PII.3max	(cm)	1.8					
	$d_{eq}(z_{sp})$	(cm)						
	fc	(MHz)	5.89	5.90				
	D: (A	X (cm)		2.05				
	Dim of A _{aprt}	Y (cm)		0.45				
	PD	(µsec)	0.23					
	PRF	(Hz)	5319					
011	pr@PII _{max}	(MPa)	2.03					
Other Information	d _{eq} @PII _{max}	(cm)						
imormation	F	FL _x (cm)		0.33				
	Focal Length	FLy (cm)		0.22				
	IPA.3@ MImax	(W/cm ²)	84.49					
Operating	Mode	NA	THI-B	THI-B				
Control	Focus	(cm)	2.5	2.5				
Conditions	Power	(%)	100	100				

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: <u>L12-E</u>
Operating Mode: <u>B+C</u>

					TIS		TIB	
	Index Label		MI		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.5	0.4				
	Pr.3	(MPa)	1.18					
	Wo	(mW)		57.34				
	min of [$W_{.3}(z_1)$, $I_{TA.3}(z_1)$]	(mW)						
	Z1	(cm)						
Associated	Z _{bp}	(cm)						
Acoustic Parameter	Z _{sp}	(cm)						
Parameter	z@PII.3max	(cm)	1.8					
	$d_{eq}(z_{sp})$	(cm)						
	fc	(MHz)	5.12	5.40				
	D: (A	X (cm)		2.05				
	Dim of A _{aprt}	Y (cm)		0.45				
	PD	(µsec)	0.86					
	PRF	(Hz)	7887					
011	pr@PII _{max}	(MPa)	1.51					
Other Information	d _{eq} @PII _{max}	(cm)						
Iniormation	F	FL _x (cm)		0.27				
	Focal Length	FLy (cm)		0.32				
	IPA.3@ MImax	(W/cm ²)	72.65					
Operating	Mode	NA	С	С				
Control	Focus	(cm)	2.5	2.5				
Conditions	Power	(%)	100	100				

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: <u>L12-E</u>
Operating Mode: <u>B+C+PW</u>

					TIS		TIB	
	Index Label		МІ	Scan	non-	scan		TIC
				Scari	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.2			1.4	1.8	
	p _{r.3}	(MPa)	0.54					
	Wo	(mW)					106.50	
	min of [W _{.3} (z_1), $I_{TA.3}(z_1)$]	(mW)				54.21		
	Z 1	(cm)				1.8		
Associated	Z _{bp}	(cm)				1.8		
Acoustic Parameter	Z _{sp}	(cm)					1.8	
Parameter	z@PII.3max	(cm)	3.0					
	$d_{eq}(z_{sp})$	(cm)					0.86	
	fc	(MHz)	5.43			5.43	5.43	
	Dim of A	X (cm)				2.05	2.05	
	Dim of A _{aprt}	Y (cm)				0.45	0.45	
	PD	(µsec)	0.83					
	PRF	(Hz)	8051					
Other	pr@PII _{max}	(MPa)	0.75					
Information	d _{eq} @PII _{max}	(cm)					0.86	
Iniormation	F	FL _x (cm)				0,26		
	Focal Length	FLy (cm)				0.21		
	IPA.3@ MI _{max}	(W/cm ²)	103.77					
Operating	Mode	NA	PW			PW	PW	
Control	Focus	(cm)	2.5			2.5	2.5	
Conditions	Power	(%)	100			100	100	

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: <u>L12-E</u>

Operating Mode: M

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.5			0.6	1.0	
	Pr.3	(MPa)	1.21					
	Wo	(mW)					40.98	
	min of [W _{.3} (z ₁), $I_{TA.3}(z_1)$]	(mW)				19.75		
	Z1	(cm)				1.8		
Associated	Z _{bp}	(cm)				1.8		
Acoustic Parameter	Z _{sp}	(cm)					1.8	
Parameter	z@PII.3max	(cm)	1.8					
	$d_{eq}(z_{sp})$	(cm)					0.67	
	fc	(MHz)	5.85			5.87	5.82	
	Dim of A	X (cm)				2.05	2.05	
	Dim of A _{aprt}	Y (cm)				0.45	0.45	
	PD	(µsec)	0.23					
	PRF	(Hz)	5319					
011	pr@PII _{max}	(MPa)	1.74					
Other Information	d _{eq} @PII _{max}	(cm)					0.67	
IIIIOIIIIalioii	Facal Law with	FL _x (cm)				0.25		
	Focal Length	FLy (cm)				0.18		
	IPA.3@ MI _{max}	(W/cm ²)	170.00					
Operating	Mode	NA	М			М	М	
Control	Focus	(cm)	2.5			2.5	2	
Conditions	Power	(%)	100			100	100	

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: P6-E

Operating Mode: B

					TIS		TIB	
	Index Label		MI		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.9	1.5				
	Pr.3	(MPa)	1.80					
	Wo	(mW)		1.34				
	min of [W _{.3} (z_1), $I_{TA.3}(z_1)$]	(mW)						
	Z1	(cm)						
Associated	Z _{bp}	(cm)						
Acoustic Parameter	Z _{sp}	(cm)						
Parameter	z@PII.3max	(cm)	2.2					
	$d_{eq}(z_{sp})$	(cm)						
	fc	(MHz)	3.82	3.90				
	Dina of A	X (cm)		0.83				
	Dim of A _{aprt}	Y (cm)		0.90				
	PD	(µsec)	0.46					
	PRF	(Hz)	4201					
011	pr@PII _{max}	(MPa)	2.20					
Other Information	d _{eq} @PII _{max}	(cm)						
inionnation	Facal Law with	FL _x (cm)		0.26				
	Focal Length	FLy (cm)		0.32				
	IPA.3@ MI _{max}	(W/cm ²)	98.14					
Operating	Mode	NA	В	В				
Control	Focus	(cm)	5	8				
Conditions	Power	(%)	100	100				

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: <u>P6-E</u> Operating Mode: <u>THI-B</u>

					TIS		TIB	
	Index Label		MI		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.9	1.4				
	Pr.3	(MPa)	1.72					
	Wo	(mW)		1.34				
	min of [W _{.3} (z_1), $I_{TA.3}(z_1)$]	(mW)						
	Z1	(cm)						
Associated	Z _{bp}	(cm)						
Acoustic Parameter	Z _{sp}	(cm)						
Parameter	z@PII.3max	(cm)	2.2					
	$d_{eq}(z_{sp})$	(cm)						
	fc	(MHz)	3.80	3.88				
	Dim of A	X (cm)		0.83				
	Dim of A _{aprt}	Y (cm)		0.90				
	PD	(µsec)	0.46					
	PRF	(Hz)	4201					
045	pr@PII _{max}	(MPa)	2.20					
Other Information	d _{eq} @PII _{max}	(cm)						
inionnation	Facal Lawsith	FL _x (cm)		0.26				
	Focal Length	FLy (cm)		0.32				
	IPA.3@ MI _{max}	(W/cm ²)	98.11					
Operating	Mode	NA	THI-B	THI-B				
Control	Focus	(cm)	5	8				
Conditions	Power	(%)	100	100				

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: P6-E
Operating Mode: B+C

					TIS		TIB	
	Index Label		MI	_	non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.6	0.9				
	Pr.3	(MPa)	1.24					
	Wo	(mW)		1.00				
	min of [W _{.3} (z_1), $I_{TA.3}(z_1)$]	(mW)						
	Z1	(cm)						
Associated	Z _{bp}	(cm)						
Acoustic Parameter	Z _{sp}	(cm)						
Farameter	z@PII.3max	(cm)	2.3					
	$d_{eq}(z_{sp})$	(cm)						
	fc	(MHz)	4.05	4.06				
	Dim of A	X (cm)		0.83				
	Dim of A _{aprt}	Y (cm)		0.90				
	PD	(µsec)	0.97					
	PRF	(Hz)	6993					
O41	pr@PII _{max}	(MPa)	1.58					
Other Information	d _{eq} @PII _{max}	(cm)						
iniormation	Facal Law with	FL _x (cm)		0.33				
	Focal Length	FLy (cm)		0.22				
	IPA.3@ MI _{max}	(W/cm ²)	65.50					
Operating	Mode	NA	С	С				
Control	Focus	(cm)	6	7				
Conditions	Power	(%)	100	100				

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: P6-E
Operating Mode: B+C+PW

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.4		0.9		1.1	
	p _{r.3}	(MPa)	0.95					
	Wo	(mW)			24.96		24.96	
	min of [W _{.3} (z ₁), $I_{TA.3}(z_1)$]	(mW)						
	Z 1	(cm)						
Associated	Z _{bp}	(cm)						
Acoustic Parameter	Z _{sp}	(cm)					1.8	
Parameter	z@PII.3max	(cm)	2.0					
	d _{eq} (z _{sp})	(cm)					0.20	
	fc	(MHz)	7.35		7.36		7.35	
	Dim of A	X (cm)			0.83		0.83	
	Dim of A _{aprt}	Y (cm)			0.90		0.90	
	PD	(µsec)	2.03					
	PRF	(Hz)	6983					
011	pr@PII _{max}	(MPa)	1.42					
Other Information	d _{eq} @PII _{max}	(cm)					0.20	
iniormation	F	FL _x (cm)			0.22			
	Focal Length	FLy (cm)			0.34			
	I _{PA.3} @ MI _{max}	(W/cm ²)	119.18					
Operating	Mode	NA	PW		PW		PW	
Control	Focus	(cm)	7		5		5	
Conditions	Power	(%)	100		100		100	

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: P6-E

Operating Mode: M

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		1.0		1.2		1.3	
	Pr.3	(MPa)	1.87					
	Wo	(mW)			66.56		66.56	
	min of [W _{.3} (z ₁), $I_{TA.3}(z_1)$]	(mW)						
	Z 1	(cm)						
Associated	Z _{bp}	(cm)						
Acoustic Parameter	Z _{sp}	(cm)					2.0	
Parameter	z@PII.3max	(cm)	2.1					
	d _{eq} (z _{sp})	(cm)					0.33	
	f _c	(MHz)	3.84		3.84		3.80	
	Dim of A	X (cm)			0.83		0.83	
	Dim of A _{aprt}	Y (cm)			0.90		0.90	
	PD	(µsec)	0.45					
	PRF	(Hz)	5814					
011	pr@PII _{max}	(MPa)	2.33					
Other Information	d _{eq} @PII _{max}	(cm)					0.33	
IIIIOIIIIalioii	Facal Law with	FL _x (cm)			0.23			
	Focal Length	FLy (cm)			0.36			
	IPA.3@ MI _{max}	(W/cm ²)	147.25					
Operating	Mode	NA	М		М		M	
Control	Focus	(cm)	5		5		6	
Conditions	Power	(%)	100		100		100	

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: <u>P6-E</u> Operating Mode: <u>B+C+CW</u>

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.3		0.9		1.0	0.9
	Pr.3	(MPa)	0.47					
	Wo	(mW)			70.00		68.00	75.00
	min of [W _{.3} (z_1), $I_{TA.3}(z_1)$]	(mW)						
	Z1	(cm)						
Associated	Z _{bp}	(cm)						
Acoustic Parameter	Z _{sp}	(cm)					4.1	
Parameter	z@PII.3max	(cm)	4.0					
	d _{eq} (z _{sp})	(cm)					0.57	
	f _c	(MHz)	3.25		3.50		3.61	3.54
	Dim of A	X (cm)			0.83		0.83	0.83
	Dim of A _{aprt}	Y (cm)			0.70		0.70	0.70
	PD	(µsec)	18.94					
	PRF	(Hz)	0					
011	pr@PII _{max}	(MPa)	0.09					
Other Information	d _{eq} @PII _{max}	(cm)					0.62	
IIIIOIIIIalioii	Facal Law with	FL _x (cm)			0.30			0.21
	Focal Length	FLy (cm)			0.25			0.24
	IPA.3@ MI _{max}	(W/cm ²)	26.80					
Operating	Mode	NA	CW		CW		CW	CW
Control	Focus	(cm)	5		5		6	6
Conditions	Power	(%)	100		100		100	100

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: P6-E
Operating Mode: CFM-M

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.7		0.2		0.3	
	Pr.3	(MPa)	1.22					
	Wo	(mW)			14.00		16.00	
	min of [W _{.3} (z_1), $I_{TA.3}(z_1)$]	(mW)						
	Z1	(cm)						
Associated	Z _{bp}	(cm)						
Acoustic Parameter	Z _{sp}	(cm)					3.0	
Parameter	z@PII.3max	(cm)	3.2					
	$d_{eq}(z_{sp})$	(cm)					0.90	
	fc	(MHz)	3.48		3.53		3.63	
	Dim of A	X (cm)			0.83		0.83	
	Dim of A _{aprt}	Y (cm)			0.70		0.70	
	PD	(µsec)	0.93					
	PRF	(Hz)	200					
Othern	pr@PII _{max}	(MPa)	2.39					
Other Information	d _{eq} @PII _{max}	(cm)					0.58	
IIIIOIIIIalioii	Facal Law with	FL _x (cm)			0.39			
	Focal Length	FLy (cm)			0.60			
	I _{PA.3} @ MI _{max}	(W/cm ²)	55.88					
Operating	Mode	NA	CFM-M		CFM-M		CFM-M	
Control	Focus	(cm)	5		5		6	
Conditions	Power	(%)	100		100		100	

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: <u>L7R-E</u>

Operating Mode: B

					TIS		TIB	
	Index Label		MI		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.8	0.5				
	Pr.3	(MPa)	2.08					
	Wo	(mW)		73.28				
	min of [W _{.3} (z ₁), I _{TA.3} (z ₁)]	(mW)						
	Z1	(cm)						
Associated	Z _{bp}	(cm)						
Acoustic Parameter	Z _{sp}	(cm)						
Farameter	z@PII.3max	(cm)	1.9					
	$d_{eq}(z_{sp})$	(cm)						
	fc	(MHz)	6.14	6.14				
	Dina of A	X (cm)		2.05				
	Dim of A _{aprt}	Y (cm)		0.45				
	PD	(µsec)	0.22					
	PRF	(Hz)	2865.3					
011	pr@PII _{max}	(MPa)	3.07					
Other Information	d _{eq} @PII _{max}	(cm)						
iniormation	F	FL _x (cm)		2.32				
	Focal Length	FLy (cm)		2.18				
	IPA.3@ MImax	(W/cm ²)	178.21					
Operating	Mode	NA	В	В				
Control	Focus	(cm)	3	3				
Conditions	Power	(%)	100	100				

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: <u>L7R-E</u>
Operating Mode: <u>THI-B</u>

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.7	0.4				
	Pr.3	(MPa)	2.04					
	Wo	(mW)		73.17				
	min of [W _{.3} (z_1), $I_{TA.3}(z_1)$]	(mW)						
	Z1	(cm)						
Associated	Z _{bp}	(cm)						
Acoustic Parameter	Z _{sp}	(cm)						
Parameter	z@PII.3max	(cm)	1.9					
	$d_{eq}(z_{sp})$	(cm)						
	fc	(MHz)	6.11	6.12				
	Dina of A	X (cm)		2.05				
	Dim of A _{aprt}	Y (cm)		0.45				
	PD	(µsec)	0.21					
	PRF	(Hz)	2855.4					
0.11	pr@PII _{max}	(MPa)	3.04					
Other Information	d _{eq} @PII _{max}	(cm)						
iniormation	Farall amounts	FL _x (cm)		2.31				
	Focal Length	FLy (cm)		2.24				
	I _{PA.3} @ MI _{max}	(W/cm ²)	169.56					
Operating	Mode	NA	THI-B	THI-B				
Control	Focus	(cm)	3	3				
Conditions	Power	(%)	100	100				

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: <u>L7R-E</u>

Operating Mode: B+C

					TIS		TIB	
	Index Label		MI		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.5	0.8				
	Pr.3	(MPa)	1.25					
	Wo	(mW)		105.62				
	min of [W _{.3} (z_1), $I_{TA.3}(z_1)$]	(mW)						
	Z1	(cm)						
Associated	Z _{bp}	(cm)						
Acoustic Parameter	Z _{sp}	(cm)						
Parameter	z@PII.3max	(cm)	1.6					
	$d_{eq}(z_{sp})$	(cm)						
	fc	(MHz)	6.36	6.35				
	Dina of A	X (cm)		2.05				
	Dim of A _{aprt}	Y (cm)		0.45				
	PD	(µsec)	0.75					
	PRF	(Hz)	6855.2					
O41	pr@PII _{max}	(MPa)	1.85					
Other Information	d _{eq} @PII _{max}	(cm)						
imormation	F	FL _x (cm)		1.46				
	Focal Length	FLy (cm)		1.52				
	I _{PA.3} @ MI _{max}	(W/cm ²)	88.5					
Operating	Mode	NA	С	С				
Control	Focus	(cm)	2	2.5				
Conditions	Power	(%)	100	100				

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: <u>L7R-E</u>
Operating Mode: <u>B+C+PW</u>

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.6		2.2		1.8	
	p _{r.3}	(MPa)	1.39					
	Wo	(mW)			73.72		73.72	
	min of [W _{.3} (z ₁), $I_{TA.3}(z_1)$]	(mW)						
	Z 1	(cm)						
Associated	Z _{bp}	(cm)						
Acoustic Parameter	Z _{sp}	(cm)					1.6	
Parameter	z@PII.3max	(cm)	1.6					
	d _{eq} (z _{sp})	(cm)					0.45	
	fc	(MHz)	6.32		6.32		6.33	
	Dim of A	X (cm)			2.05		2.05	
	Dim of A _{aprt}	Y (cm)			0.45		0.45	
	PD	(µsec)	0.62					
	PRF	(Hz)	2798.5					
011	pr@PII _{max}	(MPa)	1.86					
Other Information	d _{eq} @PII _{max}	(cm)					0.45	
IIIIOIIIIalioii	Facal Law with	FL _x (cm)			1.25			
	Focal Length	FLy (cm)			1.32			
	IPA.3@ MI _{max}	(W/cm ²)	100.41					
Operating	Mode	NA	PW		PW		PW	
Control	Focus	(cm)	2		2		3	
Conditions	Power	(%)	100		100		100	

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: <u>L7R-E</u>

Operating Mode: M

					TIS		TIB	
	Index Label		МІ	_	non-s	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.7		4.1		1.5	
	Pr.3	(MPa)	1.71					
	Wo	(mW)			136.51		139.30	
	min of [$W_{.3}(z_1)$, $I_{TA.3}(z_1)$]	(mW)						
	Z1	(cm)						
Associated	Z _{bp}	(cm)						
Acoustic	Z _{sp}	(cm)					1.8	
Parameter	z@PII.3max	(cm)	2.6					
	$d_{eq}(z_{sp})$	(cm)					0.95	
	fc	(MHz)	6.05		6.18		6.05	
	Dim of A	X (cm)			2.05		2.05	
	Dim of A _{aprt}	Y (cm)			0.45		0.45	
	PD	(µsec)	0.22					
	PRF	(Hz)	2655.3					
045	pr@PII _{max}	(MPa)	2.52					
Other Information	d _{eq} @PII _{max}	(cm)					0.89	
iniormation	Facal Law with	FL _x (cm)			1.25			
	Focal Length	FLy (cm)			1.31			
	IPA.3@ MI _{max}	(W/cm ²)	134.51					
Operating	Mode	NA	М		М		М	
Control	Focus	(cm)	2		2		2	
Conditions	Power	(%)	100		100		100	

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: V7-E

Operating Mode: B

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.5	0.2				
	Pr.3	(MPa)	0.98					
	Wo	(mW)		29.70				
	min of [W _{.3} (z_1), $I_{TA.3}(z_1)$]	(mW)						
	Z1	(cm)						
Associated	Z _{bp}	(cm)						
Acoustic Parameter	Z _{sp}	(cm)						
Farameter	z@PII.3max	(cm)	2.4					
	$d_{eq}(z_{sp})$	(cm)						
	fc	(MHz)	4.15	4.17				
	Dina of A	X (cm)		1.48				
	Dim of A _{aprt}	Y (cm)		0.70				
	PD	(µsec)	0.67					
	PRF	(Hz)	4342					
O41	pr@PII _{max}	(MPa)	1.30					
Other Information	d _{eq} @PII _{max}	(cm)						
IIIIOIIIIalioii	Facel Langth	FL _x (cm)		0.22				
	Focal Length	FLy (cm)		0.36				
	I _{PA.3} @ MI _{max}	(W/cm ²)	41.35					
Operating	Mode	NA	В	В				
Control	Focus	(cm)	2.5	1.5				
Conditions	Power	(%)	100	100				

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: <u>V7-E</u>
Operating Mode: <u>THI-B</u>

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.4	0.2				
	Pr.3	(MPa)	0.87					
	Wo	(mW)		29.70				
	min of [W _{.3} (z ₁), I _{TA.3} (z ₁)]	(mW)						
	Z1	(cm)						
Associated	Z _{bp}	(cm)						
Acoustic Parameter	Z _{sp}	(cm)						
Parameter	z@PII.3max	(cm)	2.3					
	$d_{eq}(z_{sp})$	(cm)						
	fc	(MHz)	4.13	4.16				
	Dim of A	X (cm)		1.48				
	Dim of A _{aprt}	Y (cm)		0.70				
	PD	(µsec)	0.67					
	PRF	(Hz)	4347					
O41	pr@PII _{max}	(MPa)	1.30					
Other Information	d _{eq} @PII _{max}	(cm)						
iniormation	Facal Law with	FL _x (cm)		0.22				
	Focal Length	FLy (cm)		0.31				
	IPA.3@ MI _{max}	(W/cm ²)	41.35					
Operating	Mode	NA	THI-B	THI-B				
Control	Focus	(cm)	2.5	1.5				
Conditions	Power	(%)	100	100				

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: <u>V7-E</u>
Operating Mode: <u>B+C</u>

					TIS		TIB	
	Index Label		MI		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.4	0.7				
	p _{r.3}	(MPa)	0.95					
	Wo	(mW)		77.20				
	min of [W _{.3} (z ₁), $I_{TA.3}(z_1)$]	(mW)						
	Z1	(cm)						
Associated	Z _{bp}	(cm)						
Acoustic Parameter	Z _{sp}	(cm)						
Parameter	z@PII.3max	(cm)	2.5					
	$d_{eq}(z_{sp})$	(cm)						
	f _c	(MHz)	5.27	5.29				
	Dim of A	X (cm)		1.48				
	Dim of A _{aprt}	Y (cm)		0.70				
	PD	(µsec)	0.70					
	PRF	(Hz)	6024					
O41	pr@PII _{max}	(MPa)	1.38					
Other Information	d _{eq} @PII _{max}	(cm)						
IIIIOIIIIalioii	Facal Law with	FL _x (cm)		0.21				
	Focal Length	FLy (cm)		0.29				
	IPA.3@ MI _{max}	(W/cm ²)	30.21					
Operating	Mode	NA	С	С				
Control	Focus	(cm)	2.5	2				
Conditions	Power	(%)	100	100				

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: <u>V7-E</u>
Operating Mode: <u>B+C+PW</u>

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.5			1.3	2.2	
	p _{r.3}	(MPa)	1.07					
	Wo	(mW)					100.97	
	min of [W _{.3} (z ₁), $I_{TA.3}(z_1)$]	(mW)				53.19		
	Z1	(cm)				1.8		
Associated	Z _{bp}	(cm)				1.7		
Acoustic Parameter	Z _{sp}	(cm)					2.0	
Parameter	z@PII.3max	(cm)	2.6					
	$d_{eq}(z_{sp})$	(cm)					0.51	
	f _c	(MHz)	5.30			5.30	5.28	
	Dim of A	X (cm)				1.48	1.48	
	Dim of A _{aprt}	Y (cm)				0.70	0.70	
	PD	(µsec)	0.87					
	PRF	(Hz)	5551					
011	pr@PII _{max}	(MPa)	1.52					
Other Information	d _{eq} @PII _{max}	(cm)					0.51	
iniormation	Facal Law with	FL _x (cm)				0.26		
	Focal Length	FLy (cm)				0.22		
	IPA.3@ MI _{max}	(W/cm ²)	143.32					
Operating	Mode	NA	PW			PW	PW	
Control	Focus	(cm)	3			2.5	2	
Conditions	Power	(%)	100			100	100	

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: <u>V7-E</u>

Operating Mode: M

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.5			0.6	1.2	
	Pr.3	(MPa)	0.98					
	Wo	(mW)					47.51	
	min of [W _{.3} (z ₁), $I_{TA.3}(z_1)$]	(mW)				28.70		
	Z1	(cm)				1.8		
Associated	Z _{bp}	(cm)				1.7		
Acoustic Parameter	Z _{sp}	(cm)					2.3	
Parameter	z@PII.3max	(cm)	2.4					
	$d_{eq}(z_{sp})$	(cm)					0.46	
	f _c	(MHz)	4.13			4.16	4.13	
	Dim of A	X (cm)				1.48	1.48	
	Dim of A _{aprt}	Y (cm)				0.70	0.70	
	PD	(µsec)	0.67					
	PRF	(Hz)	5546					
011	pr@PII _{max}	(MPa)	1.30					
Other Information	d _{eq} @PII _{max}	(cm)					0.45	
inionnation	F	FL _x (cm)				0.25		
	Focal Length	FLy (cm)				0.21		
	IPA.3@ MI _{max}	(W/cm ²)	140.31					
Operating	Mode	NA	М			М	М	
Control	Focus	(cm)	3			2	3	
Conditions	Power	(%)	100			100	100	

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: MC5-E

Operating Mode: B

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.9	1.7				
	Pr.3	(MPa)	1.96					
	Wo	(mW)		350.19				
	min of [$W_{.3}(z_1)$, $I_{TA.3}(z_1)$]	(mW)						
	Z1	(cm)						
Associated	Z _{bp}	(cm)						
Acoustic Parameter	Z _{sp}	(cm)						
Parameter	z@PII.3max	(cm)	2.4					
	$d_{eq}(z_{sp})$	(cm)						
	fc	(MHz)	4.82	5.01				
	Dina of A	X (cm)		1.46				
	Dim of A _{aprt}	Y (cm)		1.00				
	PD	(µsec)	0.43					
	PRF	(Hz)	14701					
011	pr@PII _{max}	(MPa)	2.69					
Other Information	d _{eq} @PII _{max}	(cm)						
Iniormation	F	FL _x (cm)		0.27				
	Focal Length	FLy (cm)		0.22				
	I _{PA.3} @ MI _{max}	(W/cm ²)	80.61					
Operating	Mode	NA	В	В				
Control	Focus	(cm)	4	1.5				
Conditions	Power	(%)	100	100				

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: MC5-E
Operating Mode: THI-B

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.8	1.9				
	Pr.3	(MPa)	1.81					
	Wo	(mW)		350.21				
	min of [W _{.3} (z_1), $I_{TA.3}(z_1)$]	(mW)						
	Z 1	(cm)						
Associated	Z _{bp}	(cm)						
Acoustic Parameter	Z _{sp}	(cm)						
Parameter	z@PII.3max	(cm)	2.5					
	d _{eq} (z _{sp})	(cm)						
	f _c	(MHz)	4.80	4.72				
	Dim of A	X (cm)		1.46				
	Dim of A _{aprt}	Y (cm)		1.00				
	PD	(µsec)	0.43					
	PRF	(Hz)	14701					
045	pr@PII _{max}	(MPa)	2.65					
Other Information	d _{eq} @PII _{max}	(cm)						
iniormation	Facal Law with	FL _x (cm)		0.27				
	Focal Length	FLy (cm)		0.21				
	IPA.3@ MI _{max}	(W/cm ²)	80.53					
Operating	Mode	NA	THI-B	THI-B				
Control	Focus	(cm)	4	1.5				
Conditions	Power	(%)	100	100				

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: MC5-E

Operating Mode: B+C

					TIS		TIB	
	Index Label		MI		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.6	2.2				
	Pr.3	(MPa)	1.39					
	Wo	(mW)		321.02				
	min of [W _{.3} (z ₁), I _{TA.3} (z ₁)]	(mW)						
	Z1	(cm)						
Associated	Z _{bp}	(cm)						
Acoustic Parameter	Z _{sp}	(cm)						
Farameter	z@PII.3max	(cm)	2.9					
	$d_{eq}(z_{sp})$	(cm)						
	fc	(MHz)	3.98	4.02				
	Dina of A	X (cm)		1.46				
	Dim of A _{aprt}	Y (cm)		1.00				
	PD	(µsec)	0.96					
	PRF	(Hz)	5949					
011	pr@PII _{max}	(MPa)	1.70					
Other	d _{eq} @PII _{max}	(cm)						
Information	- II II	FL _x (cm)		0.18				
	Focal Length	FLy (cm)		0.23				
	IPA.3@ MImax	(W/cm ²)	58.35					
Operating	Mode	NA	С	С				
Control	Focus	(cm)	3.5	3.5				
Conditions	Power	(%)	100	100				

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: MC5-E
Operating Mode: B+C+PW

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.7			1.7	1.5	
	Pr.3	(MPa)	1.60					
	Wo	(mW)					449.43	
	min of [W _{.3} (z_1), $I_{TA.3}(z_1)$]	(mW)				256.69		
	Z1	(cm)				2.1		
Associated	Z _{bp}	(cm)				2.0		
Acoustic Parameter	Z _{sp}	(cm)					2.2	
Farameter	z@PII.3max	(cm)	2.3					
	d _{eq} (z _{sp})	(cm)					0.72	
	f _c	(MHz)	3.93			3.94	3.95	
	Dim of A	X (cm)				1.46	1.46	
	Dim of A _{aprt}	Y (cm)				1.00	1.00	
	PD	(µsec)	0.95					
	PRF	(Hz)	6022					
045	pr@PII _{max}	(MPa)	2.10					
Other Information	d _{eq} @PII _{max}	(cm)					0.69	
iniormation	Facal Law with	FL _x (cm)				0.16		
	Focal Length	FLy (cm)				0.21		
	IPA.3@ MI _{max}	(W/cm ²)	101.25					
Operating	Mode	NA	PW			PW	PW	
Control	Focus	(cm)	2			3	3	
Conditions	Power	(%)	100			100	100	

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: MC5-E

Operating Mode: M

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.8			2.1	2.0	
	p _{r.3}	(MPa)	2.02					
	Wo	(mW)					356.04	
	min of [W _{.3} (z ₁), $I_{TA.3}(z_1)$]	(mW)				177.51		
	Z1	(cm)				2.1		
Associated	Z _{bp}	(cm)				2.0		
Acoustic Parameter	Z _{sp}	(cm)					2.1	
Parameter	z@PII.3max	(cm)	2.2					
	$d_{eq}(z_{sp})$	(cm)					0.74	
	f _c	(MHz)	4.75			4.92	4.83	
	Dim of A	X (cm)				1.46	1.46	
	Dim of A _{aprt}	Y (cm)				1.00	1.00	
	PD	(µsec)	0.42					
	PRF	(Hz)	14725					
011	pr@PII _{max}	(MPa)	2.83					
Other Information	d _{eq} @PII _{max}	(cm)					0.74	
iniormation	Facal Law with	FL _x (cm)				0.31		
	Focal Length	FLy (cm)				0.26		
	IPA.3@ MI _{max}	(W/cm ²)	111.30					
Operating	Mode	NA	М			М	М	
Control	Focus	(cm)	3.5			2.5	2	
Conditions	Power	(%)	100			100	100	

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: MC3-E

Operating Mode: B

					TIS		TIB	
	Index Label		MI		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.7	1.6				
	p _{r.3}	(MPa)	1.30					
	Wo	(mW)		365.52				
	min of [W _{.3} (z ₁), $I_{TA.3}(z_1)$]	(mW)						
	Z 1	(cm)						
Associated	Z _{bp}	(cm)						
Acoustic Parameter	Z _{sp}	(cm)						
Parameter	z@PII.3max	(cm)	5.0					
	$d_{eq}(z_{sp})$	(cm)						
	fc	(MHz)	3.27	3.42				
	Dim of A	X (cm)		2.05				
	Dim of A _{aprt}	Y (cm)		1.30				
	PD	(µsec)	0.60					
	PRF	(Hz)	3846					
011	pr@PII _{max}	(MPa)	2.22					
Other Information	d _{eq} @PII _{max}	(cm)						
IIIIOIIIIalioii	Facal Law with	FL _x (cm)		0.23				
	Focal Length	FLy (cm)		0.25				
	IPA.3@ MI _{max}	(W/cm ²)	55.70					
Operating	Mode	NA	В	В				
Control	Focus	(cm)	5	7				
Conditions	Power	(%)	100	100				

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: MC3-E
Operating Mode: THI-B

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.7	1.7				
	Pr.3	(MPa)	1.24					
	Wo	(mW)		365.57				
	min of [W _{.3} (z_1), $I_{TA.3}(z_1)$]	(mW)						
	Z 1	(cm)						
Associated	Z _{bp}	(cm)						
Acoustic Parameter	Z _{sp}	(cm)						
Parameter	z@PII.3max	(cm)	4.9					
	$d_{eq}(z_{sp})$	(cm)						
	f _c	(MHz)	3.25	3.36				
	Dim of A	X (cm)		2.05				
	Dim of A _{aprt}	Y (cm)		1.30				
	PD	(µsec)	0.60					
	PRF	(Hz)	3841					
011	pr@PII _{max}	(MPa)	2.22					
Other Information	d _{eq} @PII _{max}	(cm)						
IIIIOIIIIalioii	Facal Law with	FL _x (cm)		0.25				
	Focal Length	FLy (cm)		0.25				
	IPA.3@ MI _{max}	(W/cm ²)	55.74					
Operating	Mode	NA	THI-B	THI-B				
Control	Focus	(cm)	5	7				
Conditions	Power	(%)	100	100				

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: MC3-E

Operating Mode: B+C

					TIS		TIB	
	Index Label		MI		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.4	0.3				
	Pr.3	(MPa)	0.49					
	Wo	(mW)		136.19				
	min of [$W_{.3}(z_1)$, $I_{TA.3}(z_1)$]	(mW)						
	Z1	(cm)						
Associated	Z _{bp}	(cm)						
Acoustic Parameter	Z _{sp}	(cm)						
Parameter	z@PII.3max	(cm)	3.8					
	$d_{eq}(z_{sp})$	(cm)						
	fc	(MHz)	2.84	2.84				
	Dina of A	X (cm)		2.05				
	Dim of A _{aprt}	Y (cm)		1.30				
	PD	(µsec)	0.91					
	PRF	(Hz)	5948					
011	pr@PII _{max}	(MPa)	0.79					
Other Information	d _{eq} @PII _{max}	(cm)						
Iniormation	F	FL _x (cm)		0.21				
	Focal Length	FLy (cm)		0.21				
	I _{PA.3} @ MI _{max}	(W/cm ²)	10.35					
Operating	Mode	NA	С	С				
Control	Focus	(cm)	5	5				
Conditions	Power	(%)	100	100				

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: MC3-E
Operating Mode: B+C+PW

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.3			0.4	0.7	
	p _{r.3}	(MPa)	0.54					
	Wo	(mW)					78.80	
	min of [W _{.3} (z ₁), $I_{TA.3}(z_1)$]	(mW)				36.09		
	Z1	(cm)				3.8		
Associated	Z _{bp}	(cm)				2.8		
Acoustic Parameter	Z _{sp}	(cm)					3.4	
Parameter	z@PII.3max	(cm)	5.5					
	$d_{eq}(z_{sp})$	(cm)					1.13	
	fc	(MHz)	2.90			2.90	2.89	
	Dim of A	X (cm)				2.05	2.05	
	Dim of A _{aprt}	Y (cm)				1.30	1.30	
	PD	(µsec)	0.90					
	PRF	(Hz)	3835					
011	pr@PII _{max}	(MPa)	0.74					
Other Information	d _{eq} @PII _{max}	(cm)					1.07	
IIIIOIIIIalioii	Facal Law with	FL _x (cm)				0.25		
	Focal Length	FLy (cm)				0.31		
	IPA.3@ MI _{max}	(W/cm ²)	170.36					
Operating	Mode	NA	PW			PW	PW	
Control	Focus	(cm)	5			5	5	
Conditions	Power	(%)	100			100	100	

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: MC3-E

Operating Mode: M

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.8			1.7	1.5	
	Pr.3	(MPa)	1.27					
	Wo	(mW)					487.42	
	min of [W _{.3} (z_1), $I_{TA.3}(z_1)$]	(mW)				219.13		
	Z1	(cm)				3.6		
Associated	Z _{bp}	(cm)				2.8		
Acoustic Parameter	Z _{sp}	(cm)					4.3	
Parameter	z@PII.3max	(cm)	4.6					
	$d_{eq}(z_{sp})$	(cm)					0.92	
	fc	(MHz)	3.26			3.26	3.25	
	Dim of A	X (cm)				2.05	2.05	
	Dim of A _{aprt}	Y (cm)				1.30	1.30	
	PD	(µsec)	0.50					
	PRF	(Hz)	7573					
Othern	pr@PII _{max}	(MPa)	1.92					
Other Information	d _{eq} @PII _{max}	(cm)					0.89	
IIIIOIIIIalioii	Facel Langth	FL _x (cm)				0.34		
	Focal Length	FLy (cm)				0.26		
	I _{PA.3} @ MI _{max}	(W/cm ²)	162.39					
Operating	Mode	NA	М			М	М	
Control	Focus	(cm)	5			5	5	
Conditions	Power	(%)	100			100	100	

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: MC6-E

Operating Mode: B

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.8	1.1				
	Pr.3	(MPa)	1.92					
	Wo	(mW)		409.60				
	min of [W _{.3} (z ₁), I _{TA.3} (z ₁)]	(mW)						
	Z1	(cm)						
Associated	Z _{bp}	(cm)						
Acoustic	Z _{sp}	(cm)						
Parameter	z@PII.3max	(cm)	2.7					
	$d_{eq}(z_{sp})$	(cm)						
	fc	(MHz)	5.66	5.85				
	Dina of A	X (cm)		1.22				
	Dim of A _{aprt}	Y (cm)		0.90				
	PD	(µsec)	0.26					
	PRF	(Hz)	5923					
011	pr@PII _{max}	(MPa)	2.75					
Other Information	d _{eq} @PII _{max}	(cm)						
IIIIOIIIIalioii	Facal Law with	FL _x (cm)		0.32				
	Focal Length	FLy (cm)		0.33				
	I _{PA.3} @ MI _{max}	(W/cm ²)	83.76					
Operating	Mode	NA	В	В				
Control	Focus	(cm)	2.5	2				
Conditions	Power	(%)	100	100				

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: MC6-E
Operating Mode: THI-B

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.8	1.2				
	Pr.3	(MPa)	1.85					
	Wo	(mW)		409.60				
	min of [$W_{.3}(z_1)$, $I_{TA.3}(z_1)$]	(mW)						
	Z1	(cm)						
Associated	Z _{bp}	(cm)						
Acoustic	Z _{sp}	(cm)						
Parameter	z@PII.3max	(cm)	2.7					
	$d_{eq}(z_{sp})$	(cm)						
	fc	(MHz)	5.63	5.78				
	Dina of A	X (cm)		1.22				
	Dim of A _{aprt}	Y (cm)		0.90				TIC
	PD	(µsec)	0.26					
	PRF	(Hz)	5924					
0.11	pr@PII _{max}	(MPa)	2.77					
Other Information	d _{eq} @PII _{max}	(cm)						
iniormation	Farall amounts	FL _x (cm)		0.31				
	Focal Length	FLy (cm)		0.34				
	I _{PA.3} @ MI _{max}	(W/cm ²)	83.73					
Operating	Mode	NA	THI-B	THI-B				
Control	Focus	(cm)	2.5	2				
Conditions	Power	(%)	100	100				

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: MC6-E

Operating Mode: B+C

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.7	1.2				
	p _{r.3}	(MPa)	1.72					
	Wo	(mW)		296.70				
	min of [W _{.3} (z ₁), $I_{TA.3}(z_1)$]	(mW)						
	Z1	(cm)						
Associated	Z _{bp}	(cm)						
	Acoustic Z _{sp}	(cm)						
Parameter	z@PII.3max	(cm)	1.8					
	$d_{eq}(z_{sp})$	(cm)						
	f _c	(MHz)	5.26	5.34				
	Dina of A	X (cm)		1.22				
	Dim of A _{aprt}	Y (cm)		0.90				
	PD	(µsec)	0.72					
	PRF	(Hz)	6024					
011	pr@PII _{max}	(MPa)	2.39					
Other Information	d _{eq} @PII _{max}	(cm)						
iniormation	F	FL _x (cm)		0.21				
	Focal Length	FLy (cm)		0.34				
	IPA.3@ MImax	(W/cm ²)	94.75					
Operating	Mode	NA	С	С				
Control	Focus	(cm)	2.5	1				
Conditions	Power	(%)	100	100				

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: MC6-E
Operating Mode: B+C+PW

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.6			1.4	1.3	
	Pr.3	(MPa)	1.58					
	Wo	(mW)					204.29	
	min of [W _{.3} (z ₁), $I_{TA.3}(z_1)$]	(mW)				104.65		
	Z1	(cm)				1.8		
Associated	Z _{bp}	(cm)				1.6		
Acoustic Parameter	Z _{sp}	(cm)					1.8	
	z@PII.3max	(cm)	2.9					
	$d_{eq}(z_{sp})$	(cm)					0.70	
	fc	(MHz)	5.21			5.34	5.36	
	Dim of A	X (cm)				1.22	1.22	
	Dim of A _{aprt}	Y (cm)				0.90	0.90	
	PD	(µsec)	0.50					
	PRF	(Hz)	5924					
011	pr@PII _{max}	(MPa)	2.40					
Other Information	d _{eq} @PII _{max}	(cm)					0.70	
iniormation	Facal Law with	FL _x (cm)				0.30		
	Focal Length	FLy (cm)				0.28		
	IPA.3@ MI _{max}	(W/cm ²)	188.48					
Operating	Mode	NA	PW			PW	PW	
Control	Focus	(cm)	2.5			3.5	3.5	
Conditions	Power	(%)	100			100	100	

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: MC6-E

Operating Mode: M

					TIS		TIB	
	Index Label		MI		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.6			1.2	1.8	
	Pr.3	(MPa)	1.79					
	Wo	(mW)					272.38	
	min of [W _{.3} (z ₁), I _{TA.3} (z ₁)]	(mW)				128.38		
	Z1	(cm)				2.0		
Associated	Z _{bp}	(cm)				1.8		
Acoustic Parameter	Z _{sp}	(cm)					2.0	
	z@PII.3max	(cm)	3.6					
	$d_{eq}(z_{sp})$	(cm)					0.78	
	fc	(MHz)	4.91			5.42	4.96	
	Dim of A	X (cm)				1.22	1.22	
	Dim of A _{aprt}	Y (cm)				0.90	0.90	
	PD	(µsec)	0.28					
	PRF	(Hz)	11236					
Other	pr@PII _{max}	(MPa)	2.44					
Information	d _{eq} @PII _{max}	(cm)					0.65	
inionnation	Facal Law with	FL _x (cm)				0.26		
	Focal Length	FLy (cm)				0.31		
	I _{PA.3} @ MI _{max}	(W/cm ²)	180.80					
Operating	Mode	NA	М			М	М	
Control	Focus	(cm)	4			2	3.5	
Conditions	Power	(%)	100			100	100	

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: <u>L7W-E</u>

Operating Mode: B

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.6	0.5				
	p _{r.3}	(MPa)	1.34					
	Wo	(mW)		98.3				
	min of [W _{.3} (z ₁), $I_{TA.3}(z_1)$]	(mW)						
	Z 1	(cm)						
Associated	Z _{bp}	(cm)						
	Acoustic Z _{sp}	(cm)						
Parameter	z@PII.3max	(cm)	2.7					
	$d_{eq}(z_{sp})$	(cm)						
	fc	(MHz)	5.99	6.09				
	Dim of A	X (cm)		3.07				
	Dim of A _{aprt}	Y (cm)		0.65				
	PD	(µsec)	0.39					
	PRF	(Hz)	6408					
011	pr@PII _{max}	(MPa)	2.1					
Other Information	d _{eq} @PII _{max}	(cm)						
IIIIOIIIIalioii	Facal Law with	FL _x (cm)		0.13				
	Focal Length	FLy (cm)		0.24				
	IPA.3@ MI _{max}	(W/cm ²)	66.88					
Operating	Mode	NA	В	В				
Control	Focus	(cm)	3	2.5				
Conditions	Power	(%)	100	100				

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: <u>L7W-E</u>
Operating Mode: <u>THI-B</u>

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.5	0.4				
	p _{r.3}	(MPa)	1.32					
	Wo	(mW)		98.3				
	min of [W _{.3} (z ₁), $I_{TA.3}(z_1)$]	(mW)						
	Z 1	(cm)						
Associated	Z _{bp}	(cm)						
	Acoustic Z _{sp}	(cm)						
Parameter	z@PII.3max	(cm)	2.7					
	$d_{eq}(z_{sp})$	(cm)						
	fc	(MHz)	5.95	6.11				
	Dim of A	X (cm)		3.07				
	Dim of A _{aprt}	Y (cm)		0.65				
	PD	(µsec)	0.39					
	PRF	(Hz)	6414					
011	pr@PII _{max}	(MPa)	2.1					
Other Information	d _{eq} @PII _{max}	(cm)						
IIIIOIIIIalioii	Facal Law with	FL _x (cm)		0.13				
	Focal Length	FLy (cm)		0.23				
	IPA.3@ MI _{max}	(W/cm ²)	66.91					
Operating	Mode	NA	THI-B	THI-B				
Control	Focus	(cm)	3	2.5				
Conditions	Power	(%)	100	100				

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: <u>L7W-E</u>

Operating Mode: B+C

					TIS		TIB	
	Index Label		MI		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.4	1.3				
	Pr.3	(MPa)	1					
	Wo	(mW)		307.2				
	min of [$W_{.3}(z_1)$, $I_{TA.3}(z_1)$]	(mW)						
	Z1	(cm)						
Associated	Z _{bp}	(cm)						
	Acoustic Z _{sp}	(cm)						
Farameter	z@PII.3max	(cm)	3					
	$d_{eq}(z_{sp})$	(cm)						
	fc	(MHz)	5.39	5.41				
	Dim of A	X (cm)		3.07				
	Dim of A _{aprt}	Y (cm)		0.65				
	PD	(µsec)	0.88					
	PRF	(Hz)	8988					
O41	pr@PII _{max}	(MPa)	1.59					
Other Information	d _{eq} @PII _{max}	(cm)						
IIIIOIIIIalioii	Facal Law with	FL _x (cm)		0.26				
	Focal Length	FLy (cm)		0.29				
	I _{PA.3} @ MI _{max}	(W/cm ²)	46.59					
Operating	Mode	NA	С	С				
Control	Focus	(cm)	3	2				
Conditions	Power	(%)	100	100				

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: <u>L7W-E</u>
Operating Mode: <u>B+C+PW</u>

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.5			1.2	0.7	
	p _{r.3}	(MPa)	1.1					
	Wo	(mW)					208.9	
	min of [W _{.3} (z ₁), $I_{TA.3}(z_1)$]	(mW)				85.11		
	Z1	(cm)				2.4		
Associated	Z _{bp}	(cm)				2.4		
Acoustic Parameter	Z _{sp}	(cm)					2.4	
	z@PII.3max	(cm)	3.2					
	$d_{eq}(z_{sp})$	(cm)					1.19	
	f _c	(MHz)	5.42			5.42	5.41	
	Dim of A	X (cm)				3.07	3.07	
	Dim of A _{aprt}	Y (cm)				0.65	0.65	
	PD	(µsec)	0.7					
	PRF	(Hz)	6411					
011	pr@PII _{max}	(MPa)	1.65					
Other Information	d _{eq} @PII _{max}	(cm)					1.19	
IIIIOIIIIalioii	Facal Law with	FL _x (cm)				0.25		
	Focal Length	FLy (cm)				0.16		
	IPA.3@ MI _{max}	(W/cm ²)	163.49					
Operating	Mode	NA	PW			PW	PW	
Control	Focus	(cm)	2.5			3.5	2.5	
Conditions	Power	(%)	100			100	100	

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: <u>L7W-E</u>

Operating Mode: M

					TIS		TIB	
	Index Label		МІ		non-	scan		TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	non-scan	
Global Max	imum Index Value		0.5			1.8	2.1	
	Pr.3	(MPa)	1.24					
	Wo	(mW)					172.00	
	min of [W _{.3} (z_1), $I_{TA.3}(z_1)$]	(mW)				63.39		
	Z1	(cm)				2.4		
Associated	Z _{bp}	(cm)				2.3		
Acoustic	Z _{sp}	(cm)					2.4	
Parameter	z@PII.3max	(cm)	2.7					
	d _{eq} (z _{sp})	(cm)					0.96	
	fc	(MHz)	6.02			6.04	6.08	
	Dim of A	X (cm)				3.07	3.07	
	Dim of A _{aprt}	Y (cm)				0.65	0.65	
	PD	(µsec)	0.39					
	PRF	(Hz)	7042					
Other	pr@PII _{max}	(MPa)	1.89					
Information	d _{eq} @PII _{max}	(cm)					0.96	
IIIIOIIIIalioii	Facel Langth	FL _x (cm)				0.23		
	Focal Length	FLy (cm)				0.26		
	I _{PA.3} @ MI _{max}	(W/cm ²)	157.33					
Operating	Mode	NA	М			М	М	
Control	Focus	(cm)	3			3	2	
Conditions	Power	(%)	100			100	100	

- (a) This index is not required for this operating mode. See section 4.1.3.1. of the Output Display Standard (NEMA UD-3).
- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed.

Transducer Model: V4-E

Operating Mode: B

Operating					TIS		TIB	
	Index Label		МІ	Saan	non-s	scan	non-sca	TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	n	
Global Max	imum Index Value	•	0.7	1.3				
	P _{r.3}	(MPa)	1.40					
	Wo	(mW)		123.40				
	min of [W.3(z ₁), I _{TA.3} (z ₁)]	(mW)						
Associated	Z ₁	(cm)						
	Z _{bp}	(cm)						
Acoustic	Z _{sp}	(cm)						
Parameter	z@PII.3max	(cm)	3.20					
	$d_{eq}(z_{sp})$	(cm)						
	f _c	(MHz)	4.25	4.33				
	Dim of A _{aprt}	X (cm)		2.56				
	DITT Of Aaprt	Y (cm)		1.20				
	PD	(µsec)	0.43					
	PRF	(Hz)	9260					
Other	p _r @PII _{max}	(MPa)	2.23					
	d _{eq} @PII _{max}	(cm)						
Information	Focal Length	FL _x (cm)		0.28				
	Focal Length	FLy (cm)		0.30				
	I _{PA.3} @ MI _{max}	(W/cm ²)	56.88					
	Mode	NA	В	В				
Operating	Focus	(cm)	4.0	2.0				
, ,	Depth	(cm)	6.61	5.40				
Control	Scanning width	%	100	100				
Conditions	Freq	MHz	4.0	4.0				
	Power	(%)	100	100				

- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed..

Transducer Model: <u>V4-E</u>
Operating Mode: B +C

					TIS		TIB	
	Index Label		МІ	Caara.	non-s	scan	non-sca	TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	n	
Global Max	imum Index Value	,	0.5	0.5				
	P _{r.3}	(MPa)	0.94					
	Wo	(mW)		46.52				
	min of [W.3(z ₁), I _{TA.3} (z ₁)]	(mW)						
Associated	Z1	(cm)						
Acoustic	Z _{bp}	(cm)						
Parameter	Zsp	(cm)						
Parameter	z@PII.3max	(cm)	5.27					
	d _{eq} (z _{sp})	(cm)						
	fc	(MHz)	3.85	3.76				
	Dim of A	X (cm)		2.56				
	Dim of A _{aprt}	Y (cm)		1.20				
	PD	(µsec)	1.20					
	PRF	(Hz)	6000					
	pr@PII _{max}	(MPa)	1.25					
Other	d _{eq} @PII _{max}	(cm)						
Information	Focal Length	FL _x (cm)		0.25				
	1 ocal Ecrigii	FLy (cm)		0.34				
	I _{PA.3} @ MI _{max}	(W/cm ²)	36.21					
	Mode	NA	С	С				
Operating	Focus	(cm)	6.0	6.0				
Control	Depth	(cm)	10.59	11.82				
	Scanning width	%	100	100				
Conditions	Freq	MHz	5.0/5.0	5.0/5.0				
	Power	(%)	100	100				

- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed..

Transducer Model: <u>V4-E</u>
Operating Mode: PW

					TIS		TIB	
	Index Label		МІ	Scan	non-s	scan	non-sca	TIC
				Scall	A _{aprt} ≤1	A _{aprt} >1	n	
Global Max	imum Index Value	•	0.4			1.0	1.0	
	P _{r.3}	(MPa)	0.78					
	Wo	(mW)					86.92	
	min of [W.3(z ₁), I _{TA.3} (z ₁)]	(mW)				53.03		
Associated	Z 1	(cm)				4.02		
Acoustic	Z _{bp}	(cm)				2.98		
Danamatan	Zsp	(cm)					3.98	
Parameter	z@PII.3max	(cm)	3.20					
	$d_{eq}(z_{sp})$	(cm)					1.09	
	fc	(MHz)	3.85			3.96	4.02	
	Dim of A	X (cm)				5.12	5.12	
	Dim of A _{aprt}	Y (cm)				1.20	1.20	
	PD	(µsec)	1.26					
	PRF	(Hz)	6000					
	pr@PII _{max}	(MPa)	1.20					
Other	d _{eq} @PII _{max}	(cm)					1.09	
Information	Focal Length	FL _x (cm)				0.24		
	1 ocal Length	FLy (cm)				0.35		
	I _{PA.3} @ MI _{max}	(W/cm ²)	121.20					
	Mode	NA	PW			PW	PW	
Operating	Focus	(cm)	6.0			7.0	6.0	
Control	Depth	(cm)	8.13			8.13	8.13	
	Scanning width	%	100			100	100	
Conditions	Freq	MHz	5.0/5.0			5.0/5.0	5.0/5.0	
	Power	(%)	100			100	100	

- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed..

Transducer Model: <u>V4-E</u>
Operating Mode: B+M

					TIS		TIB	
	Index Label		МІ	Scan	non-s	scan	non-sca	TIC
				Scan	A _{aprt} ≤1	A _{aprt} >1	n	
Global Max	imum Index Value		0.7			0.9	1.0	
	P _{r.3}	(MPa)	1.29					
	Wo	(mW)					72.13	
	min of [W.3(Z ₁), I _{TA.3} (Z ₁)]	(mW)				47.85		
Associated	Z1	(cm)				3.78		
Acoustic	Z _{bp}	(cm)				2.89		
	Zsp	(cm)					5.03	
Parameter	z@PII.3max	(cm)	4.10					
	$d_{eq}(z_{sp})$	(cm)					0.84	
	fc	(MHz)	3.93			3.95	4.02	
	Direct A	X (cm)				5.12	5.12	
	Dim of A _{aprt}	Y (cm)				1.20	1.20	
	PD	(µsec)	0.54					
	PRF	(Hz)	4642					
	pr@PII _{max}	(MPa)	2.36					
Other	d _{eq} @PII _{max}	(cm)					0.68	
Information	Focal Length	FL _x (cm)				0.33		
	1 ocal Length	FLy (cm)				0.30		
	I _{PA.3} @ MI _{max}	(W/cm ²)	198.00					
	Mode	NA	М			М	М	
Operating	Focus	(cm)	7.0			4.0	5.0	
Control	Depth	(cm)	8.13			5.40	6.61	
	Scanning width	%	100			100	100	
Conditions	Freq	MHz	5.0			5.0	5.0	
	Power	(%)	100			100	100	

- (b) This probe is not intended for transcranial or neonatal cephalic uses.
- (c) This formulation for TIS is less than that for an alternate formulation in this mode.
- # No data are reported for this operating condition since the global maximum index value is not reported for the reason listed..

Transducer Model: <u>V4-E</u>
Operating Mode: B

			MI	TI	IS	Т	IB	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	ex value		0.7	1.	.3	1	.6	-
Index compoi	nent value			1.3	1.3	1.6	1.3	
	$p_{r,\alpha}$ at Z_{MI}	Мра	1.40					
	Р	mW		123	3.40	123	3.40	_
	P _{1x1}	mW		63.	.05	63	.05	
Acoustic	Z_s	cm			-			
Parameters	Z_{b}	cm					-	
	Z _{MI}	cm	3.20					
	Zpii,α	cm	ı					
	fawf	MHz	4.25	4.5	33	4.33		-
	prr	Hz	9260					
	srr	Hz	72.34					
	n _{pps}		_					
Other	I _{pa,α} at z _{pii,α}	W/cm ²	1					
Information	I _{spta,α} at z _{pii,α} or z _{sii,α}	mW/cm ²	15.36					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	39.30					
	p _r at z _{pii}	Мра	-					
	Focus	cm	4.0	2.	.0	2	.0	-
Operating	Depth	cm	6.61	5.4	40	5.4	40	-
control	Scanning width	%	100	10	00	10	00	-
conditions	Freq	MHz	4.0	4.	.0	4	.0	_
	Power	%	100	10	00	10	00	-

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

NOTE 6 The depths z_{pii} and z_{pii,α} apply to NON-SCANNING MODES, while the depths z_{sii} and z_{sii,α} apply to SCANNING MODES. Transducer Model: V4-E

Operating Mode: B+C

			MI	Т	IS	Т	IB	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum in	dex value		0.5	0	.5	0.	.6	_
Index compo	onent value			0.5	0.5	0.6	0.5	
	$p_{r,\alpha}$ at Z_{Ml}	Мра	0.94					
	Р	mW		46	.52	46	.52	-
	P _{1x1}	mW		27	.93	27	.93	
Acoustic	Zs	cm			-			
Parameters	Z_b	cm					-	
	Z _{MI}	cm	5.27					
	Z _{pii,α}	cm	-					
	f _{awf}	MHz	3.85	3.	76	3.	76	1
	prr	Hz	6000					
	srr	Hz	46.88					
	n _{pps}		_					
Other	I _{pa,α} at z _{pii,α}	W/cm ²	-					
Information	I _{spta,α} at z _{pii,α} or z _{sii,α}	mW/cm ²	15.84					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	64.33					
	p _r at z _{pii}	Мра	ı					
	Focus	cm	6.0	6	.0	6.	.0	-
Operating	Depth	cm	10.59	11.	.82	11.82		_
control	Scanning width	%	100	10	00	100		-
conditions	Freq	MHz	5.0/5.0	5.0	/5.0	5.0/5.0		_
	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI. NOTE 6 The depths z_{pii} and z_{pii,α} apply to NON-SCANNING MODES, while the depths z_{sii} and z_{sii,α} apply to SCANNING MODES. Transducer Model: <u>V4-E</u>
Operating Mode: PW

			MI	Т	IS	Т	IB	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum in	dex value		0.4	1.	.0	1	.1	_
Index compo	onent value			0.9	1.0	1.1	1.0	
	$p_{r,\alpha}$ at Z_{Ml}	Мра	0.78					
	Р	mW		85.	.28	86	.92	-
	P _{1x1}	mW		47.	.73	48	.55	
Acoustic	Zs	cm			4.02			
Parameters	Z _b	cm					3.98	
	Z _М і	cm	3.20					
- - 1	Z _{pii,α}	cm	3.20					
	f _{awf}	MHz	3.85	3.9	96	4.02		-
	prr	Hz	6000					
	srr	Hz	_					
	n _{pps}		-					
Other	I _{pa,α} at z _{pii,α}	W/cm ²	121.20					
Information	I _{spta,α} at z _{pii,α} or z _{sii,α}	mW/cm ²	126.34					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	295.90					
	p _r at z _{pii}	Мра	1.20					
	Focus	cm	6.0	7.	.0	6	.0	-
Operating	Depth	cm	8.13	8.	13	8.	13	-
control	Scanning width	%	100		00	100		_
conditions	Freq	MHz	5.0/5.0		/5.0	5.0/5.0		_
	Power	%	100	10	00	10	00	-

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI. NOTE 6 The depths z_{pii} and z_{pii,α} apply to NON-SCANNING MODES, while the depths z_{sii} and z_{sii,α} apply to SCANNING MODES. Transducer Model: <u>V4-E</u>
Operating Mode: B+M

			MI	T	IS	T	IB	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum in	dex value		0.7	1.	.5	1.	.6	_
Index compo	onent value			1.3	1.5	1.3	1.6	
	$p_{r,\alpha}$ at Z_{Ml}	Мра	1.29					
	Р	mW		124	.55	126	3.91	-
	P _{1x1}	mW		69	.12	69.	.46	
Acoustic	Zs	cm			3.78			
Parameters	Z _b	cm					5.03	
	Z _{MI}	cm	4.10					
-	Z _{pii,α}	cm	4.10					
	f _{awf}	MHz	3.93	3.9	95	4.0	02	_
	prr	Hz	4642					
	srr	Hz	-					
	n _{pps}		-					
Other	$I_{pa,\alpha}$ at $z_{pii,\alpha}$	W/cm ²	198.00					
Information	I _{spta,α} at z _{pii,α} or z _{sii,α}	mW/cm ²	132.42					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	403.04					
	p _r at z _{pii}	Мра	2.36					
	Focus	cm	7.0	4	.0	5	.0	_
Operating	Depth	cm	8.13	5.4	40	6.61		_
control	Scanning width	%	100	10	00	10	00	_
conditions	Freq	MHz	5.0	5	.0	5.0		-
	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI. NOTE 6 The depths z_{pii} and z_{pii,α} apply to NON-SCANNING MODES, while the depths z_{sii} and z_{sii,α} apply to SCANNING MODES. Transducer Model: <u>C3-E</u>

Operating Mode: B

			MI	T	IS	T	IB	TIC
	Index label			At	Below	At	Below	
				surface	surface	surface	surface	
Maximum ind	dex value		0.70	1.0	00	1.	00	-
Index compo	nent value			1.00	1.00	0.91	1.00	
	$p_{r,\alpha}$ at Z_{MI}	Мра	1.32					
	Р	mW		511.48		511	1.48	-
	P _{1x1}	mW		74	.00	74	.00	
Acoustic	Zs	cm			-			
Parameters	Zb	cm					_	
	Z _M I	cm	6.30					
	Zpii,α	cm	_					
	f _{awf}	MHz	2.73	2.	75	2.	75	_
	prr	Hz	_					
	srr	Hz	75.48					
	n _{pps}		1					
Other	I _{pa,α} at z _{pii,α}	W/cm ²	_					
Information	I _{spta,α} at z _{pii,α} or z _{sii,α}	mW/cm ²	72.32					
	I _{spta} at z _{pii} or Z _{sii}	mW/cm ²	95.55					
	p _r at z _{pii}	Мра	-					
Operating	Focus	cm	7.00	7.	00	7.00		
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: <u>C3-E</u> Operating Mode: <u>THI-B</u>

			MI	Т	IS	T	IB	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	dex value		0.70	0.	70	0.	70	_
Index compo	nent value			0.70	0.70	0.65	0.70	
	$p_{r,\alpha}$ at Z_{MI}	Мра	1.24					
	Р	mW		511	.48	511	.48	_
	P _{1x1}	mW		74	.00	74	.00	
Acoustic	Zs	cm			ı			
Parameters	Zb	cm					_	
	Zмı	cm	6.44					
ļ	Zpii,α	cm	1					
	f _{awf}	MHz	2.74	2.	74	2.	74	-
	prr	Hz	1					
	srr	Hz	75.53					
	n _{pps}		1					
Other	I _{pa,α} at z _{pii,α}	W/cm ²	_					
Information	I _{spta,α} at z _{pii,α} or z _{sii,α}	mW/cm ²	74.45					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	95.55					
	p _r at z _{pii}	Мра	_					
Operating	Focus	cm	7.00	7.	00	7.00		_
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: <u>C3-E</u>
Operating Mode: <u>B+C</u>

			MI	Т	IS	T	IB	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	dex value		0.50	0.	60	0.60		-
Index compo	nent value			0.60	0.60	0.54	0.60	
	p _{r,α} at Z _{MI} Mpa		0.92					
	Р	mW		345.59		345	5.59	_
	P _{1x1}	mW		50	.00	50	.00	
Acoustic	Zs	cm			_			
Parameters	Zb	cm					_	
	Z _M I	cm	6.11					
	Zpii,α	cm	-					
	f _{awf}	MHz	2.90	2.	89	2.	89	_
	prr	Hz	-					
	srr	Hz	46.97					
	n _{pps}		1					
Other	I _{pa,α} at z _{pii,α}	W/cm ²	_					
Information	I _{spta,α} at z _{pii,α} or z _{sii,α}	mW/cm ²	33.32					
	I _{spta} at z _{pii} or Z _{sii}	mW/cm ²	56.25					
	p _r at z _{pii}	Мра	_					
Operating	Focus	cm	6.00	6.	00	6.	00	_
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: <u>C3-E</u> Operating Mode: B+C+PW

			MI	T	IS	TI	IB	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	dex value		0.50	1.	80	1.0	00	-
Index compo	nent value			1.50	1.80	0.94	1.00	
	$p_{r,\alpha}$ at Z_{MI}	Мра	0.84					
	Р	mW		621	.55	621	.55	_
	P _{1x1} mW			89	.92	89.	.92	
Acoustic	Zs	cm			4.10			
Parameters	Zb	cm					6.50	
	Z _M I	cm	4.32					
	Zpii,α	cm	4.40					
	f _{awf}	MHz	2.88	2.	85	2.8	82	_
	prr	Hz	9659.00					
	srr	Hz	75.46					
	n _{pps}		1					
Other	$I_{pa,\alpha}$ at $z_{pii,\alpha}$	W/cm ²	129.62					
Information	$I_{spta,\alpha} \text{ at } z_{pii,\alpha}$ or $z_{sii,\alpha}$	mW/cm ²	130.23					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	153.22					
	p _r at z _{pii}	Мра	1.43					
Operating	Focus	cm	6.00	7.0	00	10.	.00	_
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: <u>C3-E</u>

Operating Mode: M

			МІ	Т	IS	TI	В	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	dex value		1.10	1.9	90	1.20		-
Index compo	nent value			1.84	1.90	1.15	1.20	
	$p_{r,\alpha}$ at Z_{MI}	Мра	1.57					
	Р	mW		511	.21	511	.21	_
	P _{1x1}	mW		73	.96	73.	.96	
Acoustic	Zs	cm			4.20			
Parameters	Zb	cm					5.10	
	Z _M I	cm	5.44					
ļ	Zpii,α	cm	5.50					
	f _{awf}	MHz	2.71	2.	77	2.	74	-
	prr	Hz	4756.00					
	srr	Hz	37.16					
	n _{pps}		1					
Other	I _{pa,α} at z _{pii,α}	W/cm ²	111.26					
Information	$I_{spta,\alpha} \text{ at } z_{pii,\alpha}$ or $z_{sii,\alpha}$	mW/cm ²	110.23					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	133.32					
	p _r at z _{pii}	Мра	2.66					
Operating	Focus	cm	7.00	6.	00	6.0	00	_
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: <u>L7-E</u>

Operating Mode: B

			МІ	Т	IS	TI	IB	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	dex value		0.90	0.	50	0.50		-
Index compo	nent value			0.50	0.50	0.44	0.50	
	p _{r,α} at Z _{MI} Mpa		2.41					
	Р	mW		73	.73	73	.73	_
	P _{1x1}	mW		18	.00	18	.00	
Acoustic	Zs	cm			-			
Parameters	Z _b	cm					_	
	Zмı	cm	2.11					
ļ	Zpii,α	cm	_					
	f _{awf}	MHz	6.23	6.	25	6.:	25	1
	prr	Hz	1					
	srr	Hz	22.44					
	N _{pps}		1					
Other	I _{pa,α} at z _{pii,α}	W/cm ²	_					
Information	I _{spta,α} at z _{pii,α} or z _{sii,α}	mW/cm ²	40.23					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	62.21					
	p _r at z _{pii}	Мра	_					
Operating	Focus	cm	2.00	2.	00	2.	00	_
control conditions	Power	%	100	10	00	100		_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: <u>L7-E</u>
Operating Mode: <u>THI-B</u>

			MI	T	IS	TI	В	TIC
	Index label			At	Below	At	Below	
				surface	surface	surface	surface	
Maximum ind	dex value		1.00	0.4	40	0.40		ı
Index compo	nent value			0.40	0.40	0.33	0.33 0.40	
	$p_{r,\alpha}$ at Z_{MI}	Мра	2.32					
	Р	mW		73	.73	73.	.73	_
	P _{1x1}	mW		18	.00	18.	.00	
Acoustic	Zs	cm			_			
Parameters	Z _b	cm					_	
	Z _M I	cm	2.02					
	Zpii,α	cm	_					
	f _{awf}	MHz	6.21	6.:	22	6.:	22	_
	prr	Hz	_					
	srr	Hz	22.45					
	n _{pps}		1					
Other	$I_{pa,\alpha}$ at $z_{pii,\alpha}$	W/cm ²	_					
Information	I _{spta,α} at z _{pii,α} or z _{sii,α}	mW/cm ²	40.99					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	62.25					
	p _r at z _{pii}	Мра	_					
Operating	Focus	cm	2.00	2.	00	2.0	2.00	
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: <u>L7-E</u>
Operating Mode: <u>B+C</u>

			MI	T	IS	TI	IB	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	dex value		0.60	0.	70	0.	70	-
Index compo	nent value			0.70	0.70 0.70 0.66 0.70			
	$p_{r,\alpha}$ at Z_{MI}	Мра	1.38					
	Р	mW		106	5.50	106	3.50	_
	P _{1x1}	mW	At surface Below surface At surface Below surface 0.60 0.70 0.70 0.66 0.70 Mpa 1.38 106.50 106.50 - mW 26.00 26.00 - - - cm -<					
Acoustic	Zs	cm			_		9 surface 0.70 0.70 06.50 6.00	
Parameters	Z _b	cm					_	
	Zмı	cm	1.66					
	Zpii,α	cm	-					
	f _{awf}	At surface Below surface At surface Below surface 0.60 0.70 0.70 0.70 Mpa 1.38 106.50 106.50 mW 26.00 26.00 26.00 cm - - - cm 1.66 - - MHz 6.36 6.35 6.35 Hz - - mW/cm² - - mW/cm² 90.23 - mW/cm² 114.45 - cm 2.50 1.00 1.00	_					
	prr	Hz	-				35	
	srr	Hz	54.25					
	N _{pps}		1					
Other	I _{pa,α} at z _{pii,α}	W/cm ²	-					
Information	I _{spta,α} at z _{pii,α} or z _{sii,α}	mW/cm ²	90.23					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	114.45					
	p _r at z _{pii}	Мра	_					
Operating	Focus	cm	2.50	1.0	00	1.0	00	_
control conditions	Power		100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: <u>L7-E</u>
Operating Mode: <u>B+C+PW</u>

			MI	T	IS	TI	IB	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	dex value		0.60	1.0	60	1.4	40	-
Index compo	nent value	e 1.55		1.55	1.60	1.33	1.40	
	$p_{r,\alpha}$ at Z_{MI}	Мра	1.59					
	Р	mW		221	221.18 73.73		_	
	P _{1x1}	mW		54.	.00	18.	.00	
Acoustic	Zs	cm			1.84			
Parameters	Zb	cm					1.90	
	Z _M I	cm	1.66					
	Zpii,α	cm	1.70					
	f _{awf}	MHz	6.34	6.3	22	6.3	31	_
	prr	Hz	2873.00					
	srr	Hz	22.45					
	n _{pps}		1					
Other	$I_{pa,\alpha}$ at $z_{pii,\alpha}$	W/cm ²	118.84					
Information	$I_{spta,\alpha}$ at $z_{pii,\alpha}$ or $z_{sii,\alpha}$	mW/cm ²	115.52					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	133.23					
	p _r at z _{pii}	Мра	2.14					
Operating	Focus	cm	4.00	2.	50	2.	50	_
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: <u>L7-E</u>

Operating Mode: M

			МІ	Т	IS	TI	IB	TIC
	Index label			At	Below	At	Below	
				surface	surface	surface	surface	
Maximum ind	dex value		0.70	1.:	20	1.60		-
Index compo	nent value			1.11	1.20	1.20	1.20 1.60	
	$p_{r,\alpha}$ at Z_{MI}	Мра	1.89					
	Р	mW		139	0.30	139	9.30	_
	P _{1x1}	mW		34	.01	34.	.01	
Acoustic	Zs	cm			1.77			
Parameters	Zb	cm					1.80	
	Z _M I	cm	1.54					
	Zpii,α	cm	1.60					
	f _{awf}	MHz	6.19	6.:	22	6.	19	_
	prr	Hz	2866.00					
	srr	Hz	22.39					
	n _{pps}		1					
Other	$I_{pa,\alpha}$ at $z_{pii,\alpha}$	W/cm ²	158.26					
Information	$I_{spta,\alpha}$ at $z_{pii,\alpha}$ or $z_{sii,\alpha}$	mW/cm ²	155.25					
	I _{spta} at Z _{pii} or Z _{sii}	mW/cm ²	177.48					
	p _r at z _{pii}	Мра	2.60					
Operating	Focus	cm	2.00	1.	50	2.0	00	_
control conditions	Power	%	100	10	00	10	00	-

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: V6-E

Operating Mode: B

			MI	Т	IS	Ţ	IB	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	dex value		0.70	0.	40	0.4	40	_
Index compo	nent value			0.40	0.40	0.33	0.40	
	$p_{r,\alpha}$ at Z_{MI}	Мра	1.49					
	Р	mW		43	.78	43	.78	_
	P _{1x1}	mW		18	.00	18	.00	
Acoustic	Zs	cm			1			
Parameters	Z _b	cm					_	
	Z _M I	cm	2.44					
	Zpii,α	cm	ı					
	f _{awf}	MHz	4.94	5.	14	5.	14	-
	prr	Hz	ı					
	srr	Hz	56.92					
	n _{pps}		1					
Other	I _{pa,α} at z _{pii,α}	W/cm ²	ı					
Information	I _{spta,α} at z _{pii,α} or z _{sii,α}	mW/cm ²	60.23					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	84.45					
	p _r at z _{pii}	Мра	-					
Operating	Focus	cm	3.00	2.	00	2.	00	_
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: <u>V6-E</u>
Operating Mode: <u>THI-B</u>

			МІ	Т	IS	T	IB	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	dex value		0.60	0.	30	0.3	30	-
Index compo	nent value			0.30	0.30	0.22	0.30	
	$p_{r,\alpha}$ at Z_{MI}	Мра	1.42					
	Р	mW		43	.78	43	.78	-
	P _{1x1}	mW		18	.00	18	.00	
Acoustic	Zs	cm			_			
Parameters	Z _b	cm					_	
	Z _M I	cm	2.41					
	Zpii,α	cm	_					
	f _{awf}	MHz	4.92	5.	14	5.	14	_
	prr	Hz	-					
	srr	Hz	56.87					
	n _{pps}		1					
Other	I _{pa,α} at z _{pii,α}	W/cm ²	-					
Information	I _{spta,α} at Z _{pii,α} or Z _{sii,α}	mW/cm ²	63.32					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	85.55					
	p _r at z _{pii}	Мра	ı					
Operating	Focus	cm	3.00	2.00 2.00		00	_	
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: V6-E
Operating Mode: B+C

			MI	Т	IS	T	IB	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	dex value		0.40	0.	70	0.	70	-
Index compo	nent value			0.70	0.70	0.65	0.70	
	$p_{r,\alpha}$ at Z_{MI}	Мра	0.89					
	Р	mW		77	.82	77.82		_
	P _{1x1}	mW		32	.00	32	.00	
Acoustic	Zs	cm			_			
Parameters	Zb	cm					_	
	Z _M I	cm	3.33					
	Zpii,α	cm	1					
	f _{awf}	MHz	4.03	5.	25	5.	25	_
	prr	Hz	1					
	srr	Hz	39.06					
	n _{pps}		1					
Other	I _{pa,α} at z _{pii,α}	W/cm ²	-					
Information	I _{spta,α} at z _{pii,α} or z _{sii,α}	mW/cm ²	33.22					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	55.25					
	p _r at z _{pii}	Мра	ı					
Operating	Focus	cm	4.00	2.	50	2.	50	_
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: <u>V6-E</u>
Operating Mode: <u>B+C+PW</u>

			MI	T	IS	TI	IB	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	dex value		0.50	1.	10	1.8	80	-
Index compo	nent value			1.05	1.10	1.64	1.80	
	p _{r,α} at Z _{MI} Mpa		1.17					
	Р	mW		72	.88	72.	.88	_
	P _{1x1}	mW		29	.97	29.	.97	
Acoustic	Zs	cm			1.8			
Parameters	Zb	cm					2.00	
	Z _M I	cm	2.33					
	Zpii,α	cm	2.40					
	f _{awf}	MHz	5.21	5.:	22	5.	17	ı
	prr	Hz	7279.00					
	srr	Hz	56.87					
	n _{pps}		1					
Other	$I_{pa,\alpha}$ at $z_{pii,\alpha}$	W/cm ²	142.89					
Information	$I_{spta,\alpha}$ at $z_{pii,\alpha}$ or $z_{sii,\alpha}$	mW/cm ²	140.23					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	163.32					
	p _r at z _{pii}	Мра	1.54					
Operating	Focus	cm	3.00	3.	50	3.	50	_
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: V6-E

Operating Mode: M

			MI	Т	IS	TI	IB	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	dex value		0.70	0.4	40	1.	10	-
Index compo	nent value			0.22	0.40	1.00	1.10	
	p _{r,α} at Z _{MI}	Мра	1.77					
	Р	mW		24	.32	24.	.32	_
	P _{1x1}	mW		10	.00	10.	.00	
Acoustic	Zs	cm			1.80			
Parameters	Z _b	cm					2.10	
	Z _M I	cm	2.22					
Z _{MI} Z _{pii,α} f _{awf} prr srr	Zpii,α	cm	2.30					
	f _{awf}	MHz	4.87	4.	87	4.8	85	-
	prr	Hz	7273.00					
	srr	Hz	56.82					
	n _{pps}		1					
Other	I _{pa,α} at z _{pii,α}	W/cm ²	120.55					
Information	$I_{spta,\alpha}$ at $z_{pii,\alpha}$ or $z_{sii,\alpha}$	mW/cm ²	118.85					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	139.65					
	p _r at z _{pii}	Мра	2.29					
Operating	Focus	cm	3.00	3.0	00	3.0	00	_
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: <u>L12-E</u>

Operating Mode: B

			MI	Т	IS	T	IB	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	dex value		0.60	0.	10	0.	10	-
Index compo	nent value			0.10	0.10	0.09	0.10	
	$p_{r,\alpha}$ at Z_{MI}	Мра	1.39					
	Р	mW		8.	19	8.	19	-
	P _{1x1}	mW		2.	00	2.	00	
Acoustic	Zs	cm			_			
Parameters	Zb	cm					1	
	Z _M I	cm	1.74					
	Zpii,α	cm	ı					
	f _{awf}	MHz	5.91	5.	91	5.9	91	ı
	prr	Hz	1					
	srr	Hz	41.55					
	N _{pps}		1					
Other	$I_{pa,\alpha}$ at $z_{pii,\alpha}$	W/cm ²	-					
Information	I _{spta,α} at z _{pii,α} or z _{sii,α}	mW/cm ²	85.25					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	110.23					
	p _r at z _{pii}	Мра	1					
Operating	Focus	cm	2.50	2.	50	2.	50	_
control conditions	Power	%	100	100		100		_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: <u>L12-E</u>
Operating Mode: <u>THI-B</u>

			МІ	Т	IS	TI	IB	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	dex value		0.60	0.	10	0.	10	-
Index compo	nent value			0.10	0.10	0.08	0.10	
	$p_{r,\alpha}$ at Z_{MI}	Мра	1.39					
	Р	mW		8.	19	8.	19	-
	P _{1x1}	mW		2.	00	2.0	surface surface	
Acoustic	Zs	cm			_			
Parameters	Zb	cm					_	
	Z _M I	cm	1.74					
	Zpii,α	cm	ı					
	f _{awf}	MHz	5.89	5.	90	5.9	90	-
	prr	Hz	1					
	srr	Hz	41.55					
	n _{pps}		1					
Other	I _{pa,α} at z _{pii,α}	W/cm ²	-					
Information	I _{spta,α} at z _{pii,α} or z _{sii,α}	mW/cm ²	83.32					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	105.02					
	p _r at z _{pii}	Мра	1					
Operating	Focus	cm	2.50	2.	50	2.50		_
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: <u>L12-E</u>
Operating Mode: B+C

			MI	Т	IS	T	IB	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	dex value		0.50	0.4	40	0.4	40	ı
Index compo	nent value			0.40	0.40	0.33	0.40	
	p _{r,α} at Z _{MI}	Мра	1.18					
	Р	mW		57	.34	57	.34	_
	P _{1x1}	mW		14	.00	14	.00	
Acoustic	Zs	cm			1			
Parameters	Z _b	cm					-	
	Z _M I	cm	1.74					
	Zpii,α	cm	ı					
	f _{awf}	MHz	5.12	5.4	40	5.4	40	ı
	prr	Hz	ı					
	srr	Hz	61.62					
	n _{pps}		1					
Other	$I_{pa,\alpha}$ at $z_{pii,\alpha}$	W/cm ²	1					
Information	I _{spta,α} at z _{pii,α} or z _{sii,α}	mW/cm ²	70.32					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	93.65					
	p _r at z _{pii}	Мра	1					
Operating	Focus	cm	2.50	2.	50	2.	50	_
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: <u>L12-E</u>
Operating Mode: <u>B+C+PW</u>

			MI	T	IS	T	IB	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	dex value		0.20	1.4	40	1.	80	-
Index compo	nent value			1.32	1.40	1.74	1.80	
	$p_{r,\alpha}$ at Z_{MI}	Мра	0.54					
	Р	mW		106	3.50	106	3.50	_
	proponent value $\begin{array}{c ccccccccccccccccccccccccccccccccccc$	mW		26	.00	26	.00	
Acoustic	Zs	cm			1.80			
Parameters	Zb	cm					1.80	
	Z _M I	cm	2.88					
	Zpii,α	cm	3.00					
	f _{awf}	MHz	5.43	5.4	43	5.	43	_
	prr	Hz	8051.00					
	srr	Hz	62.90					
	n _{pps}		1					
Other	I _{pa,α} at z _{pii,α}	W/cm ²	103.77					
Information		mW/cm ²	105.32					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	123.32					
	p _r at z _{pii}	Мра	0.75					
Operating	Focus	cm	2.50	2.	50	2.	50	_
control conditions	Power	%	100	10	00	10	00	-

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: <u>L12-E</u>

Operating Mode: M

			MI	T	IS	T	IB	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	dex value		0.50	0.0	60	1.0	00	-
Index compo	nent value			0.54	0.60	0.88	1.00	
	p _{r,α} at Z _{MI}	Мра	1.21					
	Р	mW		40	.98	40	.98	-
	P _{1x1}	mW		10	.00	10	.00	
Acoustic	Zs	cm			1.80			
Parameters	Zb	cm					1.80	
	Z _{MI}	cm	1.74					
	Zpii,α	cm	1.80					
	f _{awf}	MHz	5.85	5.	87	5.	82	-
	prr	Hz	5319.00					
	srr	Hz	41.55					
	n _{pps}		1					
Other	$I_{pa,\alpha}$ at $z_{pii,\alpha}$	W/cm ²	170.00					
Information	$I_{spta,\alpha}$ at $z_{pii,\alpha}$ or $z_{sii,\alpha}$	mW/cm ²	168.56					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	191.22					
	p _r at z _{pii}	Мра	1.74					
Operating	Focus	cm	2.50	2.	50	2.	00	_
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: <u>V7-E</u>

Operating Mode: B

			MI	Т	IS	T	IB	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	dex value		0.50	0	20	0.20		-
Index compo	nent value			0.20	0.20	0.11	0.20	
	$p_{r,\alpha}$ at Z_{MI}	Мра	0.98					
	Р	mW		29	.70	29	.70	_
	P _{1x1}	mW		10	.00	10	.00	
Acoustic	Zs	cm			1			
Parameters	Zb	cm					_	
	Z _{MI}	cm	2.33					
	Zpii,α	cm	ı					
	f _{awf}	MHz	4.15	4.	17	4.	17	-
	prr	Hz	ı					
	srr	Hz	33.92					
	n _{pps}		1					
Other	I _{pa,α} at z _{pii,α}	W/cm ²	ı					
Information	I _{spta,α} at Z _{pii,α} or Z _{sii,α}	mW/cm ²	40.22					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	62.32					
	p _r at z _{pii}	Мра	-					
Operating	Focus	cm	2.50	1.	50	1.	50	
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: <u>V7-E</u>
Operating Mode: <u>THI-B</u>

			MI	Т	IS	T	IB	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	dex value		0.40	0.	20	0	20	-
Index compo	nent value			0.20	0.20	0.15	0.20	
	$p_{r,\alpha}$ at Z_{MI}	Мра	0.87					
	Р	mW		29	.70	29	.70	-
	P _{1x1}	mW		10	.00	10	.00	
Acoustic	Zs	cm			-			
Parameters	Zb	cm					_	
	Z _M I	cm	2.22					
	Zpii,α	cm	1					
	f _{awf}	MHz	4.13	4.	16	4.	16	_
	prr	Hz	1					
	srr	Hz	33.96					
	n _{pps}		1					
Other	I _{pa,α} at z _{pii,α}	W/cm ²	-					
Information	I _{spta,α} at z _{pii,α} or z _{sii,α}	mW/cm ²	38.66					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	62.32					
	p _r at z _{pii}	Мра	ı					
Operating	Focus	cm	2.50	1.	50	1.5	50	_
control conditions	Power	%	100	10	00	100		_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: <u>V7-E</u>
Operating Mode: <u>B+C</u>

			MI	Т	IS	T	IB	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	dex value		0.40	0.	70	0.	70	-
Index compo	nent value			0.70	0.70	0.66	0.70	
	$p_{r,\alpha}$ at Z_{MI}	Мра	0.95					
	Р	mW		77	.20	77	.20	-
	P _{1x1}	mW		26	.00	26	.00	
Acoustic	Zs	cm			-			
Parameters	Zb	cm					_	
	Z _M I	cm	2.33					
	Zpii,α	cm	1					
	f _{awf}	MHz	5.27	5.	29	5	29	_
	prr	Hz	1					
	srr	Hz	47.06					
	n _{pps}		1					
Other	I _{pa,α} at z _{pii,α}	W/cm ²	-					
Information	I _{spta,α} at z _{pii,α} or z _{sii,α}	mW/cm ²	28.56					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	50.23					
	p _r at z _{pii}	Мра	ı					
Operating	Focus	cm	2.50	2.	00	2.	00	_
control conditions	Power	%	100	10	00	100		_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: <u>V7-E</u>
Operating Mode: <u>B+C+PW</u>

			MI	Т	IS	T	В	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	dex value		0.50	1.	30	2.:	20	ı
Index compo	nent value			1.15	1.30	2.06	2.20	
	$p_{r,\alpha}$ at Z_{MI}	Мра	1.07					
	Р	mW		100).97	100).97	_
	P _{1x1}	mW		34	.00	34	.00	
Acoustic	Zs	cm			1.80			
Parameters	Zb	cm					2.00	
	Z _M I	cm	2.51					
	Zpii,α	cm	2.60					
	f _{awf}	MHz	5.30	5.	30	5	28	ı
	prr	Hz	5551.00					
	srr	Hz	43.37					
	n _{pps}		1					
Other	$I_{pa,\alpha}$ at $z_{pii,\alpha}$	W/cm ²	143.32					
Information	$I_{spta,\alpha}$ at $z_{pii,\alpha}$ or $z_{sii,\alpha}$	mW/cm ²	140.23					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	165.55					
	p _r at z _{pii}	Мра	1.52					
Operating	Focus	cm	3.00	2.	50	2.	00	
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: V7-E

Operating Mode: M

			МІ	Т	IS	Т	IB	TIC
	Index label			At	Below	At	Below	
	$\begin{array}{c ccccccccccccccccccccccccccccccccccc$			surface	surface	surface	surface	
Maximum ind	dex value		0.50	0.0	60	1.3	20	-
Index compo	nent value			0.55	0.60	1.00	1.20	
	$p_{r,\alpha}$ at Z_{MI}	Мра	0.98					
	Р	mW		47.	.51	47	.51	_
	P _{1x1}	mW		16.	.00	16	.00	
Acoustic	Zs	cm			1.80			
Parameters	Zb	cm					2.30	
	Z _M I	cm	2.33					
	Z _{pii,α}	cm	2.40					
	f _{awf}	MHz	4.13	4.	16	4.	13	_
	prr	Hz	5546.00					
	srr	Hz	43.33					
	n _{pps}		1					
Other	I _{pa,α} at z _{pii,α}	W/cm ²	140.31					
Information		mW/cm ²	135.26					
		mW/cm ²	162.32					
	p _r at z _{pii}	Мра	1.30					
Operating	Focus	cm	3.00	2.0	00	3.	00	_
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: MC5-E

Operating Mode: B

			MI	T	IS	Т	IB	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	dex value		0.90	1.	70	1.	70	ı
Index compo	nent value			1.70	1.70	1.65	1.70	
	p _{r,α} at Z _{MI}	Мра	1.96					
	Р	mW		350.19		350).19	-
	P _{1x1}	mW		121	1.59	121	surface	
Acoustic	Zs	cm			_			
Parameters	Zb	cm					_	
	Z _M I	cm	2.33					
	Zpii,α	cm	-					
	f _{awf}	MHz	4.82	5.	01	5.	01	-
	prr	Hz	-					
	srr	Hz	114.85					
	n _{pps}		1					
Other	I _{pa,α} at z _{pii,α}	W/cm ²	-					
Information	I _{spta,α} at z _{pii,α} or z _{sii,α}	mW/cm ²	78.89					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	100.23					
	p _r at z _{pii}	Мра	_					
Operating	Focus	cm	4.00	1.	50	1.	50	_
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: MC5-E
Operating Mode: THI-B

			MI	T	IS	T	IB	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	dex value		0.80	1.9	90	1.9	90	-
Index compo	nent value			1.90	1.90	1.84	1.90	
	$p_{r,\alpha}$ at Z_{MI}	Мра	1.81					
	Р	mW		350).21	350).21	_
	P _{1x1}	mW		121	.60	121	.60	
Acoustic	Zs	cm			_			
Parameters	Zb	cm					_	
	Zмі	cm	2.44					
	Z _{pii,α}	cm	1					
	f _{awf}	MHz	4.80	4.	72	4.	72	_
	prr	Hz	1					
	srr	Hz	114.85					
	n _{pps}		1					
Other	$I_{pa,\alpha}$ at $z_{pii,\alpha}$	W/cm ²	1					
Information	I _{spta,α} at z _{pii,α} or z _{sii,α}	mW/cm ²	77.89					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	99.56					
	p _r at z _{pii}	Мра	-					
Operating	Focus	cm	4.00	1.	50	1.	50	_
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: MC5-E

Operating Mode: B+C

			MI	Т	IS	T	IB	TIC
	$\begin{array}{c ccccccccccccccccccccccccccccccccccc$			At surface	Below surface	At surface	Below surface	
Maximum ind	dex value		0.60	2.:	20	2.20		-
Index compo	nent value			2.20	2.20	2.11	2.11 2.20	
	$p_{r,\alpha}$ at Z_{MI}	Мра	1.39					
	Р	mW		321.02		321	1.02	_
	P _{1x1}	mW		111	.47	111	.47	
Acoustic	Zs	cm			_			
Parameters	Zb	cm					_	
	Z _{MI}	cm	2.77					
	Zpii,α	cm	ı					
	f _{awf}	MHz	3.98	4.	02	4.	02	1
	prr	Hz	ı					
	srr	Hz	46.48					
	n _{pps}		1					
Other	$I_{pa,\alpha}$ at $z_{pii,\alpha}$	W/cm ²	ı					
Information		mW/cm ²	55.65					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	75.55					
	p _r at z _{pii}	Мра	_					
Operating	Focus	cm	3.50	3.	50	3.	50	_
control conditions	Power	%	100	100		100		-

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: MC5-E
Operating Mode: B+C+PW

			MI	Т	IS	T	IB	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	dex value		0.70	1.	70	1.	50	_
Index compo	nent value			1.66	1.70	1.32	1.50	
	$p_{r,\alpha}$ at Z_{MI}	Мра	1.60					
	Р	mW		449	0.43	449	0.43	_
	P _{1x1}	mW		156	3.05	156	3.05	
Acoustic	Zs	cm			2.10			
Parameters	Zb	cm					2.20	
	Zмı	cm	2.11					
	Zpii,α	cm	2.30					
	f _{awf}	MHz	3.93	3.9	94	3.9	95	_
	prr	Hz	6022.00					
	srr	Hz	47.05					
	n _{pps}		1					
Other	$I_{pa,\alpha}$ at $z_{pii,\alpha}$	W/cm ²	101.25					
Information	I _{spta,α} at z _{pii,α} or z _{sii,α}	mW/cm ²	100.14					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	126.32					
	p _r at z _{pii}	Мра	2.10					
Operating	Focus	cm	2.00	3.	00	3.	00	_
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: MC5-E

Operating Mode: M

	<u></u>		MI	Т	IS	TI	В	TIC
	Index label			At	Below	At	Below	
	$\begin{array}{c ccccccccccccccccccccccccccccccccccc$			surface	surface	surface	surface	
Maximum ind	dex value		0.80	2.	10	2.0	00	ı
Index compo	nent value			1.99	2.10	1.85	2.00	
	$p_{r,\alpha}$ at Z_{MI}	Мра	2.02					
	Р	mW		356	6.04	356	5.04	-
	P _{1x1}	mW		123	3.63	123	3.63	
Acoustic	Zs	cm			2.10			
Parameters	Z _b	cm					2.10	
	Z _{MI}	cm	2.14					
	Z _{pii,α}	cm	2.20					
	f _{awf}	MHz	4.75	4.9	92	4.8	83	-
	prr	Hz	14725.00					
	srr	Hz	115.04					
	n _{pps}		1					
Other	$I_{pa,\alpha}$ at $z_{pii,\alpha}$	W/cm ²	111.30					
Information	•	mW/cm ²	100.62					
	I _{spta} at z _{pii} or Z _{sii}	mW/cm ²	122.65					
	p _r at z _{pii}	Мра	2.83					
Operating	Focus	cm	3.50	2.	50	2.0	00	_
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: MC3-E

Operating Mode: B

			MI	Т	IS	Т	IB	TIC
	Index label			At	Below	At	Below	
				surface	surface	surface	surface	
Maximum ind	dex value		0.70	1.0	60	1.0	60	ı
Index compo	nent value			1.60	1.60	1.55	1.60	
	p _{r,α} at Z _{MI}	Мра	1.30					
	Р	mW		365.52		365	5.52	_
	P _{1x1}	mW		95	.19	95	.19	
Acoustic	Zs	cm			_			
Parameters	Zb	cm					_	
	Zмı	cm	4.89					
	Zpii,α	cm	_					
	f _{awf}	MHz	3.27	3.	42	3.	42	_
	prr	Hz	_					
	srr	Hz	30.05					
	n _{pps}		1					
Other	I _{pa,α} at z _{pii,α}	W/cm ²	_					
Information	I _{spta,α} at z _{pii,α} or z _{sii,α}	mW/cm ²	53.60					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	75.64					
	p _r at z _{pii}	Мра	_					
Operating	Focus	cm	5.00	7.	00	7.	00	_
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: MC3-E
Operating Mode: THI-B

			MI	Т	IS	Т	IB	TIC
	Index label			At	Below	At	Below	
				surface	surface	surface	surface	
Maximum ind	dex value		0.70	1.	70	1.70		ı
Index compo	nent value			1.70	1.70	1.62	1.70	
	$p_{r,\alpha}$ at Z_{MI}	Мра	1.24					
	Р			365	5.57	365	5.57	_
	P _{1x1}	mW		95	.20	95	.20	
Acoustic	Zs	cm			_			
Parameters	Zb	cm					_	
	Z _M I	cm	4.81					
	Z pii,α	cm	_					
	f _{awf}	MHz	3.25	3.	36	3.	36	-
	prr	Hz	_					
	srr	Hz	30.01					
	n _{pps}	_	1					
Other	$I_{pa,\alpha}$ at $z_{pii,\alpha}$	W/cm ²	_					
Information	I _{spta,α} at Z _{pii,α} or Z _{sii,α}	mW/cm ²	53.21					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	75.56					
	p _r at z _{pii}	Мра	_					
Operating	Focus	cm	5.00	7.	00	7.	00	_
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: MC3-E

Operating Mode: B+C

Operating			MI	Т	IS	Т	IB	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	dex value		0.40	0.	30	0.3	30	ı
Index compo	nent value			0.30	0.30	0.22	0.30	
	$p_{r,\alpha}$ at Z_{MI}	Мра	0.49					
	Р	mW		136.19		136	6.19	-
	P _{1x1}	mW		35	.47	35	.47	
Acoustic	Zs	cm			_			
Parameters	Zb	cm					_	
	Z _M I	cm	3.77					
	Zpii,α	cm	ı					
	f _{awf}	MHz	2.84	2.	84	2.	84	1
	prr	Hz	ı					
	srr	Hz	46.67					
	n _{pps}		1					
Other	$I_{pa,\alpha}$ at $z_{pii,\alpha}$	W/cm ²	_					
Information	$I_{spta,\alpha}$ at $z_{pii,\alpha}$ or $z_{sii,\alpha}$	mW/cm ²	11.33					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	20.25					
	p _r at z _{pii}	Мра	_					
Operating	Focus	cm	5.00	5.	5.00 5.00		00	
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: MC3-E
Operating Mode: B+C+PW

			МІ	Т	IS	TI	IB	TIC
	Index label			At	Below	At	Below	
				surface	surface	surface	surface	
Maximum ind	dex value		0.30	0.4	40	0.70		_
Index compo	nent value			0.33	0.40	0.64	0.70	
	$p_{r,\alpha}$ at Z_{MI}	Мра	0.54					
	Р	mW		78.80		78.	.80	_
	P _{1x1}	mW		20	.52	20	.52	
Acoustic	Zs	cm			3.80			
Parameters	Zb	cm					3.40	
	Z _M I	cm	5.33					
	Zpii,α	cm	5.50					
	f _{awf}	MHz	2.90	2.9	90	2.8	89	_
	prr	Hz	3835.00					
	srr	Hz	29.96					
	n _{pps}		1					
Other	$I_{pa,\alpha}$ at $z_{pii,\alpha}$	W/cm ²	170.36					
Information	I _{spta,α} at z _{pii,α} or z _{sii,α}	mW/cm ²	166.23					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	190.32					
	p _r at z _{pii}	Мра	0.74					
Operating	Focus	cm	5.00	5.	00	5.0	00	_
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: MC3-E

Operating Mode: M

			MI	Т	IS	T	IB	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	dex value		0.80	1.	70	1.	50	-
Index compo	nent value			1.65	1.70	1.44	1.50	
	$p_{r,\alpha}$ at Z_{MI}	Мра	1.27					
	Р	mW		487.42		487	' .42	_
	P _{1x1}	mW		126	.93	126	1.50	
Acoustic	Zs	cm			3.60			
Parameters	Zb	cm					4.30	
	Z _M I	cm	4.46					
ļ	Zpii,α	cm	4.60					
	f _{awf}	MHz	3.26	3.:	26	3.:	25	_
	prr	Hz	7573.00					
	srr	Hz	59.16					
	n _{pps}		1					
Other	$I_{pa,\alpha}$ at $z_{pii,\alpha}$	W/cm ²	162.39					
Information	$I_{spta,\alpha}$ at $z_{pii,\alpha}$ or $z_{sii,\alpha}$	mW/cm ²	160.52					
	I _{spta} at z _{pii} or Z _{sii}	mW/cm ²	184.56					
	p _r at z _{pii}	Мра	1.92					
Operating	Focus	cm	5.00	5.	00	5.	00	_
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: MC6-E

Operating Mode: B

			MI	T	IS	TI	В	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	dex value		0.80	1.	10	1.	10	-
Index compo	nent value			1.10	1.10	1.02	1.10	
	$p_{r,\alpha}$ at Z_{MI}	Мра	1.92					
	Р	mW		409	0.60	409	0.60	_
	P _{1x1}	mW		168	3.42	168	3.42	
Acoustic	Zs	cm			-			
Parameters	Zb	cm					1	
	Z _M I	cm	2.62					
	Zpii,α	cm	1					
	f _{awf}	MHz	5.66	5.	85	5.8	85	-
	prr	Hz	1					
	srr	Hz	46.27					
	n _{pps}		1					
Other	I _{pa,α} at z _{pii,α}	W/cm ²	_					
Information	I _{spta,α} at Z _{pii,α} or Z _{sii,α}	mW/cm ²	85.64					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	110.25					
	p _r at z _{pii}	Мра	1					
Operating	Focus	cm	2.50	2.0	00	2.0	00	_
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: MC6-E
Operating Mode: THI-B

			MI	T	S	T	IB	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	dex value		0.80	1	20	1	20	-
Index compo	nent value			1.20	1.20	1.11	1.20	
	$p_{r,\alpha}$ at Z_{MI}	Мра	1.85					
	Р	mW		409	.60	409	9.60	_
	P _{1x1}	mW		168	3.42	168	3.42	
Acoustic	Zs	cm			-			
Parameters	Zb	cm					1	
	Z _M I	cm	2.65					
	Zpii,α	cm	ı					
	f _{awf}	MHz	5.63	5.	78	5.	78	-
	prr	Hz	1					
	srr	Hz	46.28					
	n _{pps}		1					
Other	I _{pa,α} at z _{pii,α}	W/cm ²	1					
Information	I _{spta,α} at z _{pii,α} or z _{sii,α}	mW/cm ²	85.22					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	110.64					
	p _r at z _{pii}	Мра	1					
Operating	Focus	cm	2.50	2.0	00	2.	00	
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: MC6-E

Operating Mode: B+C

			MI	T	IS	T	IB	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	dex value		0.70	1	20	1	20	ı
Index compo	nent value			1.20	1.20	1.09	1.20	
	$p_{r,\alpha}$ at Z_{MI}	Мра	1.72					
	Р	mW		296.70		296	3.70	_
	P _{1x1}	mW		1.20 1.20 1.20 1.20 1.20 1.20				
Acoustic	Zs	cm			_			
Parameters	Zb	cm					_	
	Zмı	cm	1.74					
	Zpii,α	cm	1					
	f _{awf}	MHz	5.26	5.3	34	5.3	34	-
	prr	Hz	_					
	srr	Hz	47.06					
	n _{pps}		1					
Other	$I_{pa,\alpha}$ at $z_{pii,\alpha}$	W/cm ²	_					
Information	I _{spta,α} at Z _{pii,α} or Z _{sii,α}	mW/cm ²	92.21					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	115.22					
	p _r at z _{pii}	Мра	_					
Operating	Focus	cm	2.50	1.0	00	1.0	00	_
Other Information	Power	%	100	100		100		_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: MC6-E
Operating Mode: B+C+PW

			MI	T	IS	TI	IB	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	dex value		0.60	1.4	40	1.30		-
Index compo	nent value			1.30	1.40	1.22	1.30	
	$p_{r,\alpha}$ at Z_{MI}	Мра	1.58					
	Р	mW		204	1.29	204	1.29	-
	P _{1x1}	mW		84	.00	84.00		
Acoustic	Zs	cm			1.80			
Parameters	Z _b	cm					1.80	
	Z _M I	cm	2.84					
	Zpii,α	cm	2.90					
	f _{awf}	MHz	5.21	5.3	34	5.3	36	-
	prr	Hz	5924.00					
	srr	Hz	46.28					
	n _{pps}		1					
Other	$I_{pa,\alpha}$ at $z_{pii,\alpha}$	W/cm ²	188.48					
Information	$I_{spta,\alpha} \text{ at } z_{pii,\alpha}$ or $z_{sii,\alpha}$	mW/cm ²	185.52					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	210.33					
	p _r at z _{pii}	Мра	2.40					
Operating	Focus	cm	2.50	3.5	50	3.5	50	_
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: MC6-E

Operating Mode: M

			MI	Т	IS	TI	В	TIC
I	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	dex value		0.60	1.	20	1.8	30	-
Index compo	nent value			1.11	1.20	1.66	1.80	
	$p_{r,\alpha}$ at Z_{MI}	Мра	1.79					
	Р	mW		272	2.38	272	2.38	_
	P _{1x1}	mW		112	2.00	112	1.80 1.80 272.38 12.00 2.00 4.96	
Acoustic	Zs	cm			2.00			
Parameters	Zb	cm					2.00	
	Z _M I	cm	3.35					
	Zpii,α	cm	3.60					
	f _{awf}	MHz	4.91	5.	42	4.9	96	-
	prr	Hz	11236.00					
	srr	Hz	87.78					
	n _{pps}		1					
Other	$I_{pa,\alpha}$ at $z_{pii,\alpha}$	W/cm ²	180.80					
Information	I _{spta,α} at z _{pii,α} or z _{sii,α}	mW/cm ²	174.65					
	I_{spta} at z_{pii} or z_{sii}	mW/cm ²	201.22					
	p _r at z _{pii}	Мра	2.44					
Operating	Focus	cm	4.00	2.	00	3.9	50	_
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: <u>L7R-E</u>

Operating Mode: B

			MI	T	IS	T	IB	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	dex value		0.80	0.8	50	0.8	50	ı
Index compo	nent value			0.50	0.50	0.44	0.50	
	$p_{r,\alpha}$ at Z_{MI}	Мра	2.08					
	Р	mW		73.28		73	.28	_
	P _{1x1}	mW		17	.89	17	.89	
Acoustic	Zs	cm			_			
Parameters	Zb	cm					_	
	Zмı	cm	1.84					
	Zpii,α	cm	-					
	f _{awf}	MHz	6.14	6.	14	6.	14	1
	prr	Hz	-					
	srr	Hz	22.39					
	n _{pps}		1					
Other	$I_{pa,\alpha}$ at $z_{pii,\alpha}$	W/cm ²	-					
Information	I _{spta,α} at z _{pii,α} or z _{sii,α}	mW/cm ²	180.32					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	220.32					
	p _r at z _{pii}	Мра	_					
Operating	Focus	cm	3.00	3.0	00	3.	00	_
Acoustic Parameters Other Information	Power	%	100	10	00	100		-

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: <u>L7R-E</u>
Operating Mode: <u>THI-B</u>

			MI	T	S	TI	В	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	dex value		0.70	0.4	40	0.4	40	-
Index compo	nent value			0.40	0.40	0.32	0.40	
	$p_{r,\alpha}$ at Z_{MI}	Мра	2.04					
	Р	mW		73	.17	73.	.17	_
	P _{1x1}	mW		17	.86	17.86		
Acoustic	Zs	cm			1			
Parameters	Z _b	cm					-	
	Z _M I	cm	1.84					
	Zpii,α	cm	_					
	f _{awf}	MHz	6.11	6.	12	6.	12	-
	prr	Hz	_					
	srr	Hz	22.31					
	n _{pps}		1					
Other	$I_{pa,\alpha}$ at $z_{pii,\alpha}$	W/cm ²	_					
Information	I _{spta,α} at z _{pii,α} or z _{sii,α}	mW/cm ²	165.26					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	200.23					
	p _r at z _{pii}	Мра	_					
Operating	Focus	cm	3.00	3.0	00	3.0	00	_
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: <u>L7R-E</u>

Operating Mode: B+C

			MI	Т	IS	TI	IB	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	dex value		0.50	0.	80	0.80		-
Index compo	nent value			0.80	0.80	0.65	0.80	
	$p_{r,\alpha}$ at Z_{MI}	Мра	1.25					
	Р	mW		105	5.62	105	5.62	-
	P _{1x1}	mW		25	.79	25.	.79	
Acoustic	Zs	cm			-			
Parameters	Z _b	cm					-	
	Z _{MI}	cm	1.55					
	Zpii,α	cm	_					
	f _{awf}	MHz	6.36	6.	35	6.3	35	ı
	prr	Hz	ı					
	srr	Hz	53.56					
	n _{pps}		1					
Other	I _{pa,α} at z _{pii,α}	W/cm ²	ı					
Information	I _{spta,α} at z _{pii,α} or z _{sii,α}	mW/cm ²	85.23					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	110.32					
	p _r at z _{pii}	Мра	_					
Operating	Focus	cm	2.00	2.	50	2.	50	_
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: <u>L7R-E</u>
Operating Mode: <u>B+C+PW</u>

	-		MI	T	IS	TI	В	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	dex value		0.60	2.:	20	1.8	30	ı
Index compo	nent value			2.05	2.20	1.74	1.80	
	$p_{r,\alpha}$ at Z_{MI}	Мра	1.39					
	Р	mW		73	.72	73.	.72	_
	P _{1x1}	mW		18	.00	18.	.00	
Acoustic	Zs	cm			1.52			
Parameters	Zb	cm					1.60	
	Z _M I	cm	1.52					
	Zpii,α	cm	1.60					
	f _{awf}	MHz	6.32	6.3	32	6.3	33	
	prr	Hz	2798.50					
	srr	Hz	21.86					
	n _{pps}		1					
Other	I _{pa,α} at z _{pii,α}	W/cm ²	100.41					
Information	$I_{spta,\alpha} \text{ at } z_{pii,\alpha}$ or $z_{sii,\alpha}$	mW/cm ²	98.55					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	125.65					
	p _r at z _{pii}	Мра	1.86					
Operating	Focus	cm	2.00	2.00 3.00				
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: <u>L7R-E</u>

Operating Mode: M

			MI	Т	IS	T	IB	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	dex value		0.70	4.	10	1.	50	-
Index compo	nent value			3.30	4.10	1.32	1.50	
	$p_{r,\alpha}$ at Z_{MI}	Мра	1.71					
	Р	mW		136	3.51	139	0.30	_
	P _{1x1}	mW		33	.33	34	.01	
Acoustic	Zs	cm			1.77			
Parameters	Z _b	cm					1.80	
	Z _M I	cm	2.55					
	Zpii,α	cm	2.60					
	f _{awf}	MHz	6.05	6.	18	6.	05	ı
	prr	Hz	2655.30					
	srr	Hz	20.74					
	n _{pps}		1					
Other	I _{pa,α} at z _{pii,α}	W/cm ²	134.51					
Information	$I_{spta,\alpha} \text{ at } z_{pii,\alpha}$ or $z_{sii,\alpha}$	mW/cm ²	135.22					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	160.23					
	p _r at z _{pii}	Мра	2.52					
Operating	Focus	cm	2.00	2.	00	2.	00	
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: <u>L7W-E</u>

Operating Mode: B

			MI	Т	IS	T	IB	TIC
	Index label			At	Below	At	Below	
				surface	surface	surface	surface	
Maximum ind	dex value		0.60	0.	50	0.50		-
Index compo	nent value			0.50	0.50	0.44	0.50	
	p _{r,α} at Z _{MI} <i>Mpa</i>		1.34					
	Р	mW		98	.30	98	.30	_
	P _{1x1}	mW		19	.39	19	.39	
Acoustic	Zs	cm			_			
Parameters	Zb	cm					_	
	Z _M I	cm	2.66					
	Zpii,α	cm	_					
	f _{awf}	MHz	5.99	6.	09	6.	09	_
	prr	Hz	_					
	srr	Hz	50.06					
	n _{pps}	_	1					
Other	I _{pa,α} at z _{pii,α}	W/cm ²	_					
Information	$I_{spta,\alpha}$ at $z_{pii,\alpha}$ or $z_{sii,\alpha}$	mW/cm ²	65.52					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	90.56					
	p _r at z _{pii}	Мра	ı					
Operating	Focus	cm	3.00	2.	50	2.	50	_
control conditions	Power	%	100	10	00	10	00	-

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: <u>L7W-E</u>
Operating Mode: <u>THI-B</u>

			MI	Т	IS	Т	IB	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	dex value		0.50	0.4	40	0.4	40	-
Index compo	nent value			0.40	0.40	0.33	0.40	
	$p_{r,\alpha}$ at Z_{MI}	Мра	1.32					
	Р	mW		98	.30	98	.30	-
	P _{1x1}	mW		19	.39	19	.39	
Acoustic	Zs	cm			_			
Parameters	Zb	cm					_	
	Zмı	cm	2.66					
	Z pii,α	cm	ı					
	f _{awf}	MHz	5.95	6.	11	6.	11	_
	prr	Hz	ı					
	srr	Hz	50.11					
	N _{pps}		1					
Other	I _{pa,α} at z _{pii,α}	W/cm ²	ı					
Information	$I_{spta,\alpha}$ at $z_{pii,\alpha}$ or $z_{sii,\alpha}$	mW/cm ²	65.52					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	88.88					
	p _r at z _{pii}	Мра	-					
Operating	Focus	cm	3.00	2.	50	2.	50	_
control conditions	Power	%	100	10	00	100		_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: <u>L7W-E</u>

Operating Mode: B+C

			MI	T	IS	T	IB	TIC
	Index label			At	Below	At	Below	
				surface	surface	surface	surface	
Maximum ind	dex value		0.40	1.3	30	1.30		-
Index compo	nent value			1.30	1.30	1.22	1.30	
	p _{r,α} at Z _{MI} Mpa		1.00					
	Р	mW		307.20		307	' .20	-
	P _{1x1}	mW		60	.61	60.61		
Acoustic	Zs	cm			_			
Parameters	Zb	cm					_	
	Z _M I	cm	2.88					
	Zpii,α	cm	_					
	f _{awf}	MHz	5.39	5.	41	5.	41	-
	prr	Hz	_					
	srr	Hz	70.22					
	n _{pps}		1					
Other	I _{pa,α} at z _{pii,α}	W/cm ²	_					
Information	I _{spta,α} at z _{pii,α} or z _{sii,α}	mW/cm ²	45.55					
	I _{spta} at z _{pii} or Z _{sii}	mW/cm ²	68.49					
	p _r at z _{pii}	Мра	_					
Operating	Focus	cm	3.00	2.	00	2.	00	_
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: <u>L7W-E</u>
Operating Mode: <u>B+C+PW</u>

			МІ	T	IS	T	IB	TIC
	Index label			At	Below	At	Below	
				surface	surface	surface	surface	
Maximum ind	dex value		0.50	1.:	20	0.	70	-
Index compo	nent value			1.09	1.20	0.66	0.70	
	$p_{r,\alpha}$ at Z_{MI} Mpa		1.10					
	Р	mW		208.90		208	3.90	_
	P _{1x1}	mW		41	.21	41.21		
Acoustic	Zs	cm			2.40			
Parameters	Zb	cm					2.40	
	Z _M I	cm	3.11					
Ī	Zpii,α	cm	3.20					
	f _{awf}	MHz	5.42	5.4	42	5.	41	_
	prr	Hz	6411.00					
	srr	Hz	50.09					
	n _{pps}		1					
Other	$I_{pa,\alpha}$ at $z_{pii,\alpha}$	W/cm ²	163.49					
Information	$I_{spta,\alpha}$ at $z_{pii,\alpha}$ or $z_{sii,\alpha}$	mW/cm ²	165.22					
	I _{spta} at Z _{pii} or Z _{sii}	mW/cm ²	190.52					
	p _r at z _{pii}	Мра	1.65					
Operating	Focus	cm	2.50	3.	50	2.	50	_
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: <u>L7W-E</u>

Operating Mode: M

			MI	T	IS	T	IB	TIC
	Index label			At	Below	At	Below	
				surface	surface	surface	surface	
Maximum ind	dex value		0.50	1.8	80	2.10		-
Index compo	nent value			1.65	1.80	2.03	2.10	
	$p_{r,\alpha}$ at Z_{MI} Mpa		1.24					
	Р	mW		172	2.00	172.00		_
	P _{1x1}	mW		33	.93	33	.93	
Acoustic	Zs	cm			2.40			
Parameters	Zb	cm					2.40	
	Z _M I	cm	2.65					
	Zpii,α	cm	2.70					
	f _{awf}	MHz	6.02	6.	04	6.	08	_
	prr	Hz	7042.00					
	srr	Hz	55.02					
	n _{pps}		1					
Other	$I_{pa,\alpha}$ at $z_{pii,\alpha}$	W/cm ²	157.33					
Information	$I_{spta,\alpha}$ at $z_{pii,\alpha}$ or $z_{sii,\alpha}$	mW/cm ²	155.24					
	I _{spta} at Z _{pii} or Z _{sii}	mW/cm ²	178.54					
	p _r at z _{pii}	Мра	1.89					
Operating	Focus	cm	3.00	3.	00	2.	00	_
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: P3-E

Operating Mode: B

			MI	Т	IS	TI	В	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	dex value		1.20	1.	70	1.3	70	-
Index compo	nent value			1.70	1.70	1.55	1.70	
	$p_{r,\alpha}$ at Z_{MI}	Мра	1.84					
	Р	mW		269.95		269	0.95	_
	P _{1x1}	mW		140	0.60	140	0.60	
Acoustic	Zs	cm			-			
Parameters	Zb	cm					_	
	Z _{MI}	cm	4.44					
	Zpii,α	cm	_					
	f _{awf}	MHz	2.28	2.	38	2.3	38	ı
	prr	Hz	_					
	srr	Hz	26.07					
	n _{pps}		1					
Other	I _{pa,α} at z _{pii,α}	W/cm ²	_					
Information	I _{spta,α} at z _{pii,α} or z _{sii,α}	mW/cm ²	100.23					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	121.21					
	p _r at z _{pii}	Мра	_					
Operating	Focus	cm	4.00	1.	00	1.0	00	_
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: P3-E
Operating Mode: THI-B

			MI	T	IS	TI	IB	TIC
	Index label			At	Below	At	Below	
				surface	surface	surface	surface	
Maximum ind	dex value		1.20	1.9	50	1.	50	ı
Index compo	nent value			1.50	1.50	1.32	1.50	
	$p_{r,\alpha}$ at Z_{MI} Mpa		1.76					
	Р	mW		269	.95	269	9.95	-
	P _{1x1}	mW		140	.60	140).60	
Acoustic	Zs	cm			_			
Parameters	Zb	cm					_	
	Z _M I	cm	4.43					
	Zpii,α	cm	_					
	f _{awf}	MHz	2.25	2.4	44	2.4	44	-
	prr	Hz	_					
	srr	Hz	26.06					
	n _{pps}		1					
Other	I _{pa,α} at z _{pii,α}	W/cm ²	_					
Information	I _{spta,α} at z _{pii,α} or z _{sii,α}	mW/cm ²	99.50					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	118.55					
	p _r at z _{pii}	Мра	_					
Operating	Focus	cm	4.00	1.0	00	1.0	00	_
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: P3-E
Operating Mode: B+C

			MI	Т	IS	T	IB	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	dex value		0.90	0.	50	0.	50	ı
Index compo	nent value			0.50	0.50	0.44	0.50	
	$p_{r,\alpha}$ at Z_{MI}	Мра	1.35					
	Р	mW		92	.18	92	.18	_
	P _{1x1}	mW		48	.01	48	.01	
Acoustic	Zs	cm			-			
Parameters	Zb	cm					_	
	Zмı	cm	3.54					
	Zpii,α	cm	_					
	f _{awf}	MHz	2.25	2.	29	2.	29	ı
	prr	Hz	1					
	srr	Hz	46.67					
	n _{pps}		1					
Other	I _{pa,α} at z _{pii,α}	W/cm ²	_					
Information	I _{spta,α} at z _{pii,α} or z _{sii,α}	mW/cm ²	55.65					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	78.58					
	p _r at z _{pii}	Мра	ı					
Operating	Focus	cm	4.00	1.	00	1.	00	_
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: <u>P3-E</u>
Operating Mode: B+C+PW

			MI	Т	IS	TI	В	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	dex value		0.80	0.	50	1.3	20	-
Index compo	nent value			0.39	0.50	1.11	1.20	
	p _{r,α} at Z _{MI}	Мра	1.25					
	Р	mW		122	2.88	122	2.88	-
	P _{1x1}	mW		64	.00	64.	.00	
Acoustic	Zs	cm			3.10			
Parameters	Z _b	cm					5.40	
	Z _M I	cm	5.59					
	Zpii,α	cm	6.00					
	f _{awf}	MHz	1.99	1.9	98	1.9	99	ı
	prr	Hz	5049.00					
	srr	Hz	39.45					
	n _{pps}		1					
Other	I _{pa,α} at z _{pii,α}	W/cm ²	150.40					
Information	$I_{spta,\alpha}$ at $z_{pii,\alpha}$ or $z_{sii,\alpha}$	mW/cm ²	144.62					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	165.25					
	p _r at z _{pii}	Мра	1.81					
Operating	Focus	cm	1.00	1.0	00	1.0	00	
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: P3-E

Operating Mode: M

			МІ	T	IS	T	IB	TIC
	Index label			At	Below	At	Below	
				surface	surface	surface	surface	
Maximum ind	Maximum index value		1.20	0.8	80	1.4	40	-
Index compo	nent value			0.66	0.80	1.25	1.40	
	$p_{r,\alpha}$ at Z_{MI}	Мра	1.64					
	Р	mW		89	.20	89	.20	_
	P _{1x1}	mW		46	.46	46	.46	
Acoustic	Zs	cm			2.90			
Parameters	Zb	cm					2.90	
	Z _M I	cm	2.55					
	Zpii,α	cm	2.60					
	f _{awf}	MHz	1.88	1.8	89	1.5	88	_
	prr	Hz	5543.00					
	srr	Hz	43.30					
	n _{pps}		1					
Other	$I_{pa,\alpha}$ at $z_{pii,\alpha}$	W/cm ²	189.20					
Information	$I_{spta,\alpha}$ at $z_{pii,\alpha}$ or $z_{sii,\alpha}$	mW/cm ²	185.23					
	I _{spta} at Z _{pii} or Z _{sii}	mW/cm ²	210.23					
	p _r at z _{pii}	Мра	1.59					
Operating	Focus	cm	5.00	5.	00	6.	00	_
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: <u>P3-E</u>
Operating Mode: B+C+CW

			MI	Т	IS	TI	В	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	Maximum index value		0.30	0.	70	1.	70	1.00
Index compo	nent value			0.65	0.70	1.66	1.70	
	$p_{r,\alpha}$ at Z_{MI}	Мра	0.42					
	Р	mW		178	3.00	178	3.00	172.00
	P _{1x1}	mW		92	.71	92	.71	
Acoustic	Zs	cm			5.40			
Parameters	Zb	cm					6.70	
	Z _{MI}	cm	6.55					
	Zpii,α	cm	6.80					
	f _{awf}	MHz	2.65	2.	75	2.	70	2.75
	prr	Hz	0.00					
	srr	Hz	0.00					
	n _{pps}		1					
Other	$I_{pa,\alpha}$ at $z_{pii,\alpha}$	W/cm ²	38.96					
Information	I _{spta,α} at z _{pii,α} or z _{sii,α}	mW/cm ²	40.23					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	62.22					
	p _r at z _{pii}	Мра	0.12					
Operating	Focus	cm	3.00	5.	00	6.0	00	6.00
control conditions	Power	%	100	10	00	10	00	100

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: P3-E
Operating Mode: CFM-M

			MI	T	IS	T	IB	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	Maximum index value		1.10	0.	10	0.	80	ı
Index compo	nent value			0.05	0.10	0.56	0.80	
	p _{r,α} at Z _{MI}	Мра	1.51					
	Р	mW		254	.00	254	1.00	ı
	P _{1x1}	mW		132	2.29	132	2.29	
Acoustic	Zs	cm			6.10			
Parameters	Zb	cm					6.20	
	Z _M I	cm	5.88					
	Zpii,α	cm	6.10					
	f _{awf}	MHz	2.36	2.3	36	2.	35	ı
	prr	Hz	200.00					
	srr	Hz	1.56					
	n _{pps}		1					
Other	I _{pa,α} at z _{pii,α}	W/cm ²	82.33					
Information	I _{spta,α} at z _{pii,α} or z _{sii,α}	mW/cm ²	80.55					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	102.25					
	p _r at z _{pii}	Мра	2.61					
Operating	Focus	cm	4.00	5.0	00	6.	00	
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: P6-E

Operating Mode: B

			MI	T	IS	TI	В	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	dex value		0.90	1.	50	1.9	50	-
Index compo	nent value			1.50	1.50	1.30	1.50	
	$p_{r,\alpha}$ at Z_{MI}	Мра	1.80					
	Р	mW		1.3	34	1.3	34	_
	P _{1x1}	mW		1.0	61	1.0	61	
Acoustic	Zs	cm			-			
Parameters	Zb	cm					1	
	Z _M I	cm	2.19					
	Zpii,α	cm	1					
	f _{awf}	MHz	3.82	3.9	90	3.9	90	ı
	prr	Hz	1					
	srr	Hz	32.82					
	n _{pps}		1					
Other	I _{pa,α} at z _{pii,α}	W/cm ²	_					
Information	I _{spta,α} at Z _{pii,α} or Z _{sii,α}	mW/cm ²	95.56					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	118.58					
	p _r at z _{pii}	Мра	1					
Operating	Focus	cm	5.00	8.0	00	8.0	00	_
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: P6-E
Operating Mode: THI-B

			MI	T	IS	Т	IB	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	Maximum index value		0.90	1.4	40	1.	40	1
Index compo	Index component value			1.40	1.40	1.32	1.40	
	$p_{r,\alpha}$ at Z_{MI}	Мра	1.72					
	Р	mW		1.3	34	1.	34	1
	P _{1x1}	mW		1.0	61	1.	61	
Acoustic	Zs	cm			_			
Parameters	Zb	cm					_	
	Z _M I	cm	2.18					
	Zpii,α	cm	_					
	f _{awf}	MHz	3.80	3.8	88	3.	88	_
	prr	Hz	_					
	srr	Hz	32.82					
	n _{pps}		1					
Other	I _{pa,α} at z _{pii,α}	W/cm ²	_					
Information	I _{spta,α} at z _{pii,α} or z _{sii,α}	mW/cm ²	95.54					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	118.85					
	p _r at z _{pii}	Мра	_					
Operating	Focus	cm	5.00	8.0	00	8.	00	_
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: P6-E
Operating Mode: B+C

			MI	Т	IS	TI	В	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	dex value		0.60	0.9	90	0.9	90	_
Index compo	nent value			0.90	0.90	0.84	0.90	
	p _{r,α} at Z _{MI}	Мра	1.24					
	Р	mW		1.	00	1.0	00	-
	P _{1x1}	mW		1.:	20	1.:	20	
Acoustic	Zs	cm			_			
Parameters	Zb	cm					_	
	Z _M I	cm	2.22					
	Zpii,α	cm	_					
	f _{awf}	MHz	4.05	4.	06	4.0	06	_
	prr	Hz	_					
	srr	Hz	54.63					
	n _{pps}		1					
Other	I _{pa,α} at z _{pii,α}	W/cm ²	_					
Information	I _{spta,α} at z _{pii,α} or z _{sii,α}	mW/cm ²	60.32					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	84.45					
	p _r at z _{pii}	Мра	_					
Operating	Focus	cm	6.00	7.	00	7.0	00	_
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: P6-E
Operating Mode: B+C+PW

			МІ	T	IS	TI	В	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum index value		0.40	0.9	90	1.	10	-	
Index compo	nent value			0.84	0.90	1.02	1.10	
	$p_{r,\alpha}$ at Z_{MI}	Мра	0.95					
	Р	mW		24	.96	24	.96	_
	P _{1x1}	mW		30	.00	30	.00	
Acoustic	Zs	cm			1.54			
Parameters	Zb	cm					1.80	
	Z _M I	cm	1.88					
	Zpii,α	cm	2.00					
	f _{awf}	MHz	7.35	7.3	36	7.3	35	_
	prr	Hz	6983.00					
	srr	Hz	54.55					
	n _{pps}		1					
Other	$I_{pa,\alpha}$ at $z_{pii,\alpha}$	W/cm ²	119.18					
Information	$I_{spta,\alpha}$ at $z_{pii,\alpha}$ or $z_{sii,\alpha}$	mW/cm ²	120.23					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	145.52					
	p _r at z _{pii}	Мра	1.42					
Operating	Focus	cm	7.00	5.0	00	5.0	00	_
control conditions	Power	%	100	10	00	10	00	-

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: P6-E

Operating Mode: M

			MI	Т	IS	TI	IB	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum index value		1.00	1	20	1.3	30	-	
Index compo	nent value			1.15	1.20	1.22	1.30	
	p _{r,α} at Z _{MI}	Мра	1.87					
	Р	mW		66	.56	66	.56	_
	P _{1x1}	mW		80	.00	80	.00	
Acoustic	Zs	cm			1.88			
Parameters	Zb	cm					2.00	
	Z _M I	cm	2.01					
	Zpii,α	cm	2.10					
	f _{awf}	MHz	3.84	3.	84	3.	80	_
	prr	Hz	5814.00					
	srr	Hz	45.42					
	n _{pps}		1					
Other	I _{pa,α} at z _{pii,α}	W/cm ²	147.25					
Information	$I_{spta,\alpha} \text{ at } z_{pii,\alpha}$ or $z_{sii,\alpha}$	mW/cm ²	145.52					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	170.25					
	p _r at z _{pii}	Мра	2.33					
Operating	Focus	cm	5.00	5.	00	6.0	00	_
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: <u>P6-E</u> Operating Mode: B+C+CW

			MI	Т	IS	T	В	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	Maximum index value		0.30	0.	90	1.0	00	0.90
Index compo	nent value			0.88	0.90	0.94	1.00	
	$p_{r,\alpha}$ at Z_{MI}	Мра	0.47					
	Р	mW		70	.00	68	.00	75.00
	P _{1x1}	mW		84	.13	81	.73	
Acoustic	Zs	cm			3.94			
Parameters	Zb	cm					4.10	
	Z _{MI}	cm	3.84					
	Zpii,α	cm	4.00					
	f _{awf}	MHz	3.25	3.	50	3.0	61	3.54
	prr	Hz	0.00					
	srr	Hz	0.00					
	n _{pps}		1					
Other	I _{pa,α} at z _{pii,α}	W/cm ²	26.80					
Information	I _{spta,α} at Z _{pii,α} or Z _{sii,α}	mW/cm ²	25.53					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	43.32					
	p _r at z _{pii}	Мра	0.09					
Operating	Focus	cm	5.00	5.	00	6.0	00	6.00
control conditions	Power	%	100	10	00	10	00	100

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Transducer Model: P6-E
Operating Mode: CFM-M

			МІ	T	IS	T	В	TIC
	Index label			At surface	Below surface	At surface	Below surface	
Maximum ind	Maximum index value		0.70	0.:	20	0.3	30	_
Index compo	nent value			0.14	0.20	0.22	0.30	
	$p_{r,\alpha}$ at Z_{MI}	Мра	1.22					
	Р	mW		14	.00	16	.00	1
	P _{1x1}	mW		16	.83	19	.23	
Acoustic	Zs	cm			2.64			
Parameters	Zb	cm					3.00	
	Z _M I	cm	3.15					
	Zpii,α	cm	3.20					
	f _{awf}	MHz	3.48	3.	53	3.	63	ı
	prr	Hz	200.00					
	srr	Hz	1.56					
	n _{pps}		1					
Other	I _{pa,α} at z _{pii,α}	W/cm ²	55.88					
Information	I _{spta,α} at Z _{pii,α} or Z _{sii,α}	mW/cm ²	56.32					
	I _{spta} at z _{pii} or z _{sii}	mW/cm ²	64.55					
	p _r at z _{pii}	Мра	2.39					
Operating	Focus	cm	5.00	5.0	00	6.	00	_
control conditions	Power	%	100	10	00	10	00	_

NOTE 1 Only one operating condition per index.

NOTE 2 Data should be entered for "at surface" and "below surface" both in the columns related to TIS or TIB.

NOTE 3 Information need not be provided regarding TIC for any TRANSDUCER ASSEMBLY not intended for transcranial or neonatal cephalic uses.

NOTE 4 If the requirements of 201.12.4.2a) are met, it is not required to enter any data in the columns related to TIS, TIB or TIC.

NOTE 5 If the requirements of 201.12.4.2b) are met, it is not required to enter any data in the column related to MI.

Appendix B: Guidance and Manufacturer's Declaration

1. Guidance and manufacturer's declaration – electromagnetic emissions

The EBit Series is intended for use in the electromagnetic environment specified below. The customer or the user of the EBit Series should assure that it is used in such an environment.

Emissions test	Compliance	Electromagnetic environment –
		guidance
RF emissions	Group 1	The EBit Series uses RF energy
CISPR 11		only for its internal function.
		Therefore, its RF emissions are
		very low and are not likely to
		cause any interference in nearby
		electronic equipment.
RF emissions	Class A	The EBit Series is suitable for use
CISPR 11		in medical establishments
Harmonic emissions	Class A	including domestic
IEC 61000-3-2		establishments and those directly
Voltage fluctuations/	Complies	connected to the public
flicker emissions		high-voltage power supply
IEC 61000-3-3		network that used for
		non-domestic purposes.

2. Guidance and manufacturer's declaration – electromagnetic immunity

The EBit Series is intended for use in the electromagnetic environment the EBit Series should assure that it is used in such an environment.

assure that it is used if	i such an environment.		
Immunity test	IEC 60601	Compliance level	Electromagnetic
	test level		environment –
			guidance
Electrostatic	±6 kV contact	±6 kV contact	Floors should be wood,
discharge	±8 kV air	±8 kV air	concrete or ceramic tile. If
(ESD)			floors are covered with
IEC 61000-4-2			synthetic material, the
			relative humidity should
			be at least 30 %.

Electrical fast	±2 kV for power	±2 kV for power	Mains power quality
transient/burst	supply lines	supply lines	should be that of a typical
IEC 61000-4-4	±1 kV for input/output	±1 kV for input/output	commercial or hospital
	lines	lines	environment.
Surge	±1 kV line(s) to line(s)	±1 kV line(s) to line(s)	Mains power quality
IEC 61000-4-5	±2 kV line(s) to earth	±2 kV line(s) to earth	should be that of a typical
			commercial or hospital
			environment.
interruptions	<5 % UT	<5 % UT	Mains power quality
and	(>95 % dip in UT)	(>95 % dip in UT)	should be that of a typical
voltage	for 0,5 cycle	for 0,5 cycle	commercial or hospital
variations	40 % UT	40 % UT	environment. If the user
on power	(60 % dip in UT)	(60 % dip in UT)	of the EBit Series
supply	for 5 cycles	for 5 cycles	requires continued
input lines	70 % UT	70 % UT	operation during power
IEC	(30 % dip in UT)	(30 % dip in UT)	mains interruptions, it is
61000-4-11	for 25 cycles	for 25 cycles	recommended that the
	<5 % UT	<5 % UT	EBit Series be powered
	(>95 % dip in UT)	(>95 % dip in UT)	from an uninterruptible
	for 5 sec	for 5 sec	power supply or a battery.
Power	3 A/m	3 A/m	Power frequency
frequency			magnetic fields should be
frequency			at levels characteristic of
(50-60 Hz)			a typical location in a
magnetic field			typical commercial or
IEC 61000-4-8			hospital environment.
NOTE LIT: (I		F C 60 1 11 1	

NOTE UT is the a.c. mains voltage prior to application of the test level.

3 Guidance and manufacturer's declaration – electromagnetic immunity			
The EBit Series is intended for use in the electromagnetic environment specified below. The			
customer or the user of the EBit Series should assure that it is used in such an environment.			
3.1. Immunity	IEC 60601 test	IEC 60601 test	Electromagnetic environment – guidance
test	level	level	

Conducted RF	3 Vrms	3 Vrms	Portable and mobile RF communications
IEC 61000-4-6	150 kHz to 80	3 V/m	equipment should be used no closer to
Radiated RF	MHz		any part of the EBit Series, including
IEC 61000-4-3	3 V/m		cables, than the recommended separation
	80 MHz to 2,5		distance calculated from the equation
	GHz		applicable to the frequency of the
			transmitter.
			Recommended separation distance
			$d = 1,2 \sqrt{P}$
			$d = 1,2 \sqrt{P} $ 80 MHz to 800 MHz
			1,2 V1 60 MH2 to 600 MH2
			$d=2,3 \ \sqrt{P}$ 800 MHz to 2,5 GHz
			where P is the maximum output power rating o
			the transmitter in watts (W) according to the
			transmitter manufacturer and d is the
			recommended separation distance in metres (
			Field strengths from fixed RF transmitters, as
			determined by an electromagnetic site survey,
			should be less than the compliance level in ea
			frequency range.ь
			Interference may occur in the vicinity of
			equipment marked with the following symbol:
			(((()))
NOTE 4 At 00 MU	000 MH		- 1

NOTE 1 At 80 MHz and 800 MHz, the higher frequency range applies.

NOTE 2 These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.

a Field strengths from fixed transmitters, such as base stations for radio (cellular/cordless) telephones and land mobile radios, amateur radio, AM and FM radio broadcast and TV broadcast cannot be predicted theoretically with accuracy. To assess the electromagnetic environment due to fixed RF transmitters, an electromagnetic site survey should be considered. If the measured field strength in the location in which the EBit Series is used exceeds the applicable RF compliance level above, the EBit Series should be observed to verify normal operation. If abnormal performance is observed, additional measures may be necessary, such as reorienting or relocating the EBit Series.

b Over the frequency range 150 kHz to 80 MHz, field strengths should be less than 3 V/m.

Recommended separation distances between

portable and mobile RF communications equipment and the EBit Series

The EBit Series is intended for use in an electromagnetic environment in which radiated RF disturbances are controlled. The customer or the user of the EBit Series can help prevent electromagnetic interference by maintaining a minimum distance between portable and mobile RF communications equipment (transmitters) and the EBit Series as recommended below, according to the maximum output power of the communications equipment.

Rated	maxim	ium	Separation distance according to frequency of transmitter m		
output	power	of	150 kHz to 80 MHz	80 MHz to 800 MHz	800 MHz to 2,5 GHz
transmit	tter W		$d = 1,2 \sqrt{P}$	d = 1,2 √P	$d = 2,3 \sqrt{P}$
0,01			0,12	0,12	0,23
0,1			0,38	0,38	0,73
1			1,2	1,2	2,3
10			3,8	3,8	7,3
100			12	12	23

For transmitters rated at a maximum output power not listed above, the recommended separation distance d in meters (m) can be estimated using the equation applicable to the frequency of the transmitter, where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer.

NOTE 1 At 80 MHz and 800 MHz, the separation distance for the higher frequency range applies.

NOTE 2 These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.

Appendix C: Measurement Results Summary

Measurement	Useful Range	Accuracy
Distance	Full Screen	<±5%
Circumference:	Full Screen	<±5%
trace method, ellipse method		
Area:	Full Screen	<±10%
trace method, ellipse method		
Volume	Full screen	<±10%
Angle	Full screen	<±5%
Time	Full Screen	<±5%
Heart rate	Full Screen	<±5%
Velocity	Full Screen	<±10%

Appendix D: Display Accuracy and Acoustic Measurement Uncertainties

According to IEC60601-2-37 and NEMA UD-3 2004, the display accuracy and acoustic measurement uncertainties are summarized in the table below.

Display accuracy of MI is ±20%, and TI is ±40% or <0.1, if MI, TI below 0.5.

Item	Measurement Uncertainty (Percentage, 95% Confidence Value
Center Frequency	±15%
Acoustic Power	±30%
Acoustic Intensity	±30%
Peak Rarefactional Pressure	±15%

Appendix E: Transducer Maximum Surface Temperature

According section 201.11 standard to the requirements of the in the IEC60601-2-37:2007/AMD1:2015, the transducer surface temperature has been tested in two kinds of conditions: the transducer suspended in still air or transducer contacting human-tissue mimicking material. The calculation of the expanded uncertainty is based on the ISO Guide tout ye Expression of uncertainty in measurement. Three transducer samples have been tested and the confidence coefficient is at 95%, the value of t.975 is 4.30.

The measurement data were obtained under the test conditions employed at CHISON.

Transducer model	Maximum surface temperature(℃) Contacting human-tissue mimicking material	Maximum surface temperature(℃) Suspending in air
С3-Е	41±1	48±1
L7-E	40±1	47±1
V6-E	41±1	43±1
P3-E	41±2	48±1
L12-E	39±2	47±2
P6-E	40±1	48±1
L7R-E	38±2	47±2
V7-E	41±1	43±2
МС5-Е	41±1	46±1
мсз-Е	38±2	47±2
MC6-E	41±1	46±1
L7W-E	38±1	48±1
V4-EV	41±1	43±1


NOTE: Values following the "±"mark indicate the expanded uncertainty with a

confidence lever of 95%, t.975=4.30.


Appendix F: Procedures of setting network sharing

For Windows set up, set up a shared document


1. Choose the file you want to share, as the "test" file




2. Right click this file, choose "properties", and click "share".

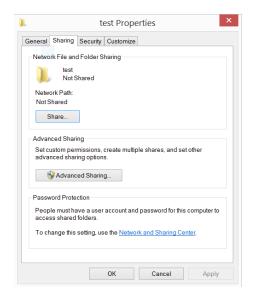


3. Then you can see the sharing setting interface, as you can see in the picture, choose "everyone", and click "add".

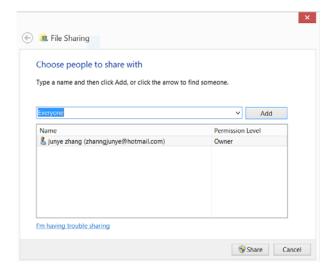

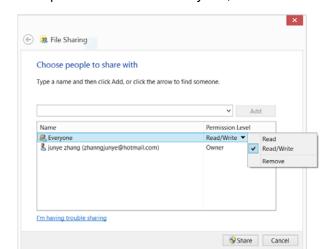


4. Choose "read/write" in the permission level in everyone, then click "share", after that, confirm.

- 5. If the windows have not set the code, then turn off the password protected sharing is necessary. Instructions as the image shows.
 - a) Click "network and sharing center" in the sharing properties.

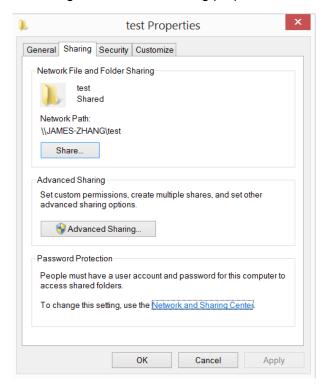

b) In the network and sharing center interface, choose "public", in the password protected sharing; choose turn off password protected sharing.

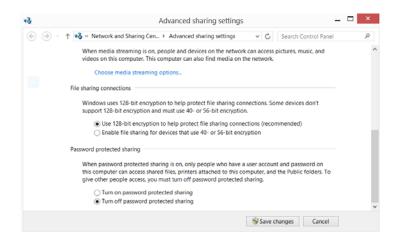

Set up in system

IP set up


1. First confirm the service address of shared files, you can get the IP address in windows interface.

In windows "start"-"run" type in "cmd" and enter, then type in "ipconfig" and enter, you can see the IP address of local service.


```
Connection-specific DNS Suffix :
Link-local IPu6 Address : : fe80::d91e:e058:f895:336d%3
IPu4 Address : : 192.168.1.131
Subnet Mask : : 255.255.255.0
Default Gateway : : 192.168.1.1
```


2. Enter into set up interface, choose net. Choose "DHCP" (automatically get the IP address) or "static" (type in IP address manually).

TIP: if you want to type in IP address manually, make sure the IP address is in the same internet section with the service, and won't confused with other IP in the LAN.

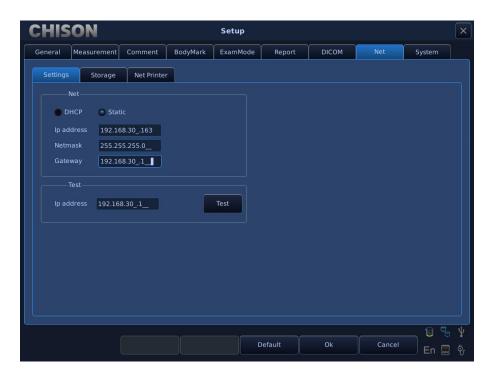

3. Choose net "storage" interface, type in service name, IP address, user name, password and the name of shared files, click "add" to add a network storage, you can choose the export route. As shown in the picture.

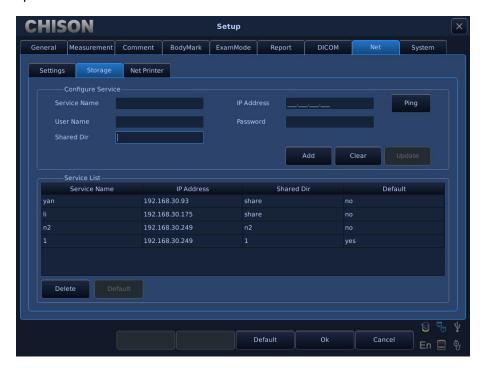

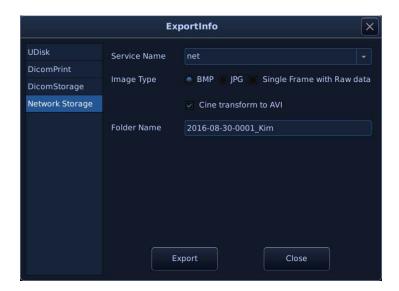

Ping: test if the IP is connected or not.

Clear: clear all the IP address, user name, password and names of shared file

Update: update the content to the chosen item.

Delete: delete the chosen service item.


Default: set the chosen item as the default net route.

NOTE: you can add multi-numbers of network storage service to realize the transmission among multi systems.

NOTE: If windows turn off password protected sharing, then in EBit set up, you can type in user name and password arbitrarily.

Net Printer Setup

1. Press key to enter into the Setup interface, then click Net and Net Printer. See picture as follow:

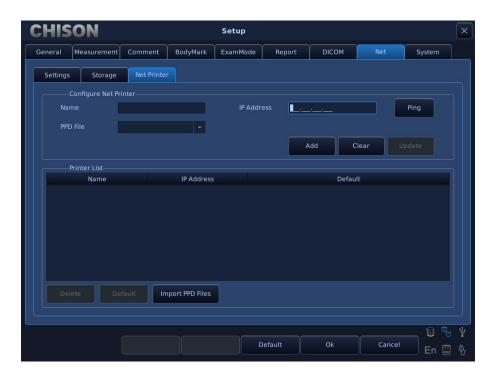

2. Configure Net Printer

Operation:

- a) Input name and IP Address which has installed printer equipment.
- b) Click [Ping] to confirm whether the net connect normally.
- c) Select PPD File and click **[Add]**, the net connecting information can be saved on the Printer List.
- 3. Choose the information on the Printer List to finish the printing according to the requirement.



CHISON



CHISON Medical Technologies Co., Ltd.