

Quality Control Report

Nitroimidazole ELISA kit


(Cat No: HA05904H)

Lot No.: YT210923A10

Date of Production: 2021-09-28

Expired: 2022-09-27

Nitroimidazole Standard Curve

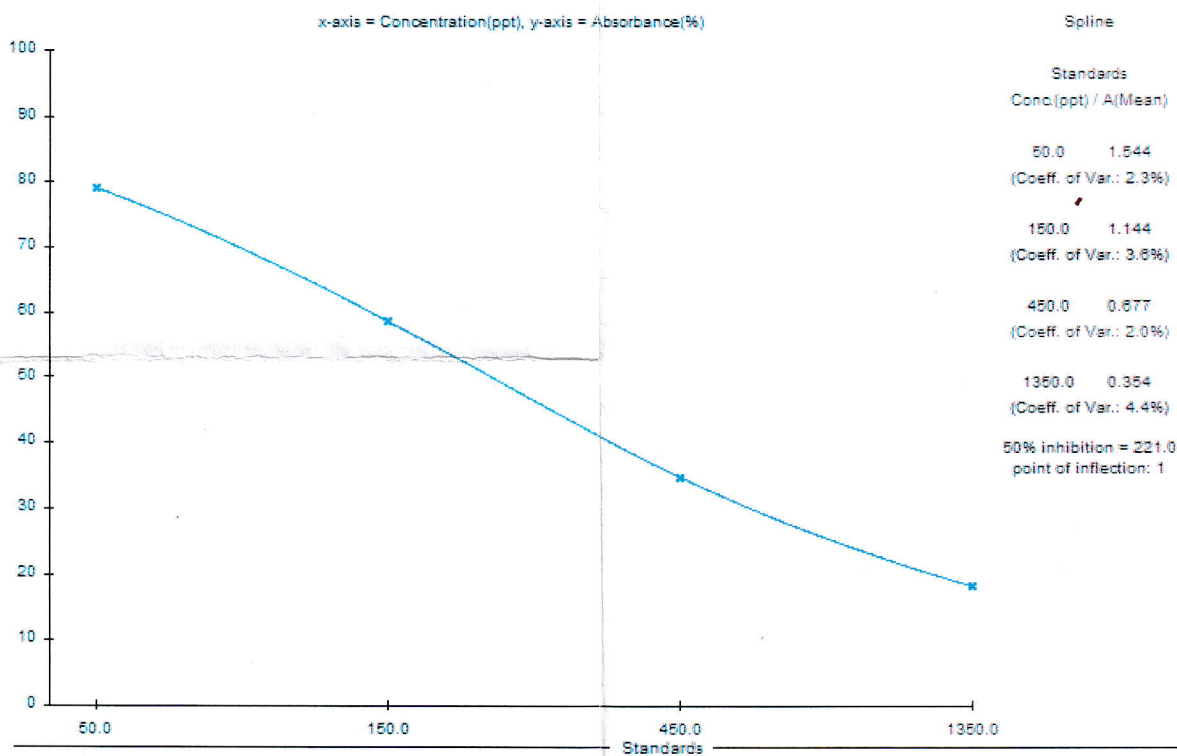

| Ser. No. | Concentration ppt | Absorbance (Mean) | (CV) | B/B0 (%) | calculated ppt | Deviation (%) |
|----------|-------------------|-------------------|------|----------|----------------|---------------|
| 1 | 0.0 | 1.950 | 0.2 | 100.0 | | |
| 2 | 50.0 | 1.544 | 2.3 | 78.2 | 50.0 | 0.0 |
| 3 | 150.0 | 1.144 | 3.6 | 58.7 | 149.9 | 0.1 |
| 4 | 450.0 | 0.677 | 2.0 | 34.7 | 450.5 | 0.1 |
| 5 | 1350.0 | 0.354 | 4.4 | 18.2 | 1349.6 | 0.0 |

Please notice: This QC report is only for reference, for the absorbance of the standard solutions may fluctuate in a certain range.

QC Department
2021-09-28
QC Code: ★
质检专用章