


MAQUET

O2 CELL WITH SEAL

Servo/Servos


REF 66 40 044

LOT 2023-01

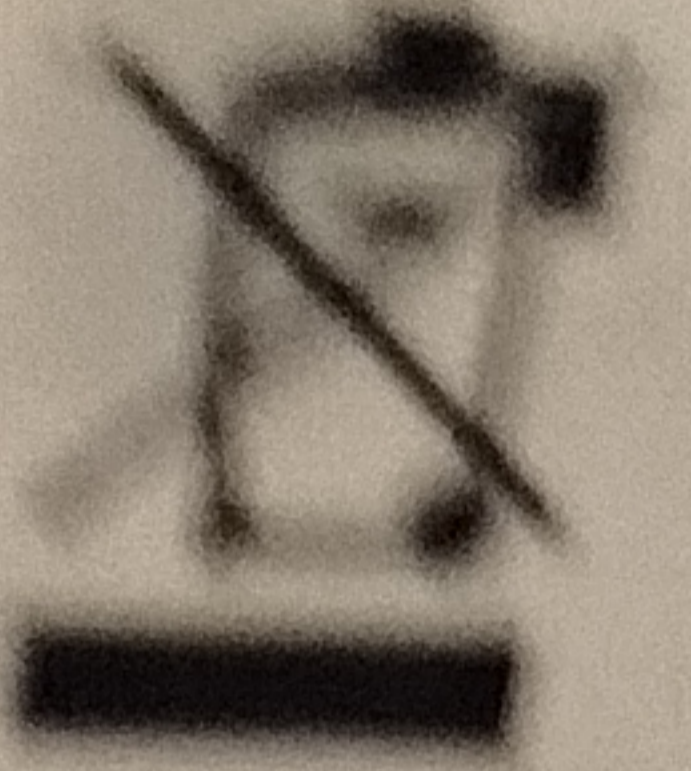

SN AA450442

Shelf life
exp. date 2023-10-01

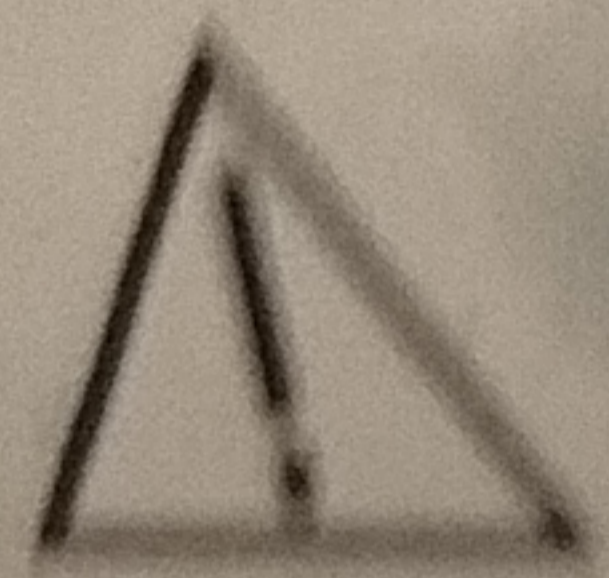

**DO NOT OPEN THIS SEALED PACKAGING
UNTIL READY TO PLACE CELL IN SERVICE.**

After installing cell, allow the instrument to equilibrate in room air
(approx. 15 min) prior to adjusting the calibration to 20.9 percent.



Maquet Critical Care AB
Röntgenvägen 2
SE-17154 Soina, Sweden

Made in Germany

Sauerstoffsensoren Sensor de oxigeno
Capteur d'oxygène Кислородный датчик Sauerstoff
Sensor de oxigeno Oxygen Sensor

