

**Intersurgical Ltd.**

Crane House, Molly Millars Lane, Wokingham, Berkshire, RG41 2RZ, UK

**Scope**

**Sterile and Non-Sterile medical devices for respiratory care, in the areas of airway management, anaesthesia, critical care, oxygen and aerosol therapy:**

**Sterile and Non-Sterile Anaesthetic Breathing Systems**

**Aerosol and Oxygen Face Masks**

**Anaesthetic Face Masks**

**Sterile Endotracheal Tube Introducer and Sterile Airway Stylets**

**Sterile and Non-Sterile Breathing Systems**

**Non-Heated Respiratory Bubble Humidifier**

**Sterile and Non-Sterile Catheter Mounts**

**Sterile and Non-Sterile Breathing System Connectors**

**Sterile and Non-Sterile Respiratory Filters**

**Breathing System Flexible Tubing**

**High Concentration Oxygen Face Masks**

**Sterile and Non-Sterile Heat and Moisture Exchangers**

**Sterile and Non-Sterile HME Filters**

**Sterile and Non-Sterile Inspiratory Line Humidification Chambers**

**Sterile I-gel Supraglottic Airways**

**Sterile Laryngeal Airways**

**Gas Sampling/Monitoring Respiratory Tubing**

**Sterile and Non-Sterile Heated Wire Breathing Systems,  
Heated Wires and attachments (electrical adaptor leads)**

Authorised by



Global Medical Devices Certification Manager

**SGS Belgium NV, Notified Body 1639**

SGS House Noorderlaan 87 2030 Antwerp Belgium  
t +32 (0)3 545 48 48 f +32 (0)3 545 48 49 www.sgs.com

LPMD5105 – Corrigendum to Certificate

Page 1 of 2

SGS Belgium NV

Certification and Business Enhancement Maatschappelijke Zetel/Siège Social:

Noorderlaan 87 B-2030 Antwerpen/Anvers

t +32 (0)3 545 48 48 f +32 (0)3 545 48 49

[www.be.sgs.com](http://www.be.sgs.com)

Member of the SGS Group

RPR Antwerp VAT – BE 0404.882.750 Citibank BE87 5701 3412 5594

**Electrically Powered Moisture Condenser, Nasal Cannulae  
 Nebulising System Delivery Sets  
 Suction and Irrigation Oral Care Toothbrush  
 Oxygen Administration Tubing  
 Repeated Use Breathing Systems  
 Breathing Systems Reservoir Bags  
 Manual Pulmonary Resuscitation Systems  
 Carbon Dioxide Absorbents  
 Sterile and Non-Sterile Tracheal Suction Systems  
 Sterile Endotracheal Tubes  
 Venturi Valves and Venturi Valve Face Mask Kits  
 Wall Humidifier Nebuliser  
 Breathing System Water Traps  
 CPAP Bi-level Nasal Masks and NIV Face Masks  
 Pressure Limiting Valves  
 Peep Valves One Way Directional Valves  
 Infant Nasal CPAP Breathing System  
 Oxygen Recovery Kits  
 Endoscopy Molar Bite Block  
 Carbon Dioxide Cuvette  
 Class I sterile: Sterility aspects only - Restricted to the aspects of  
 manufacture  
 concerned with securing and maintaining sterile conditions:  
 Sterile Guedel Airways**

This corrigendum is only valid together with accompanying 93/42/EEC certificate  
 issue 8

<b>Correction Date</b>	<b>Correction</b>
Change approved by SGS on 11 January 2022	The client is removing one of their additional sites Unit 3 Mollay Millars Bridge, RG41 2WY
Change approved by SGS on 08 November 2022	This client is removing one of their additional facilities: Circuit House, Pitronnerie Road, Industrial Estate, St Peter Port, Guernsey, GY1 2RL, UK

The management system of

# Intersurgical Ltd.

Crane House, Molly Millars Lane, Wokingham, Berkshire, RG41 2RZ, UK

has been assessed and certified as meeting the requirements of

## Directive 93/42/EEC

on medical devices, Annex II (excluding Section 4)

For the following products

The scope of registration appears on page 2 of this certificate.

This certificate is valid from 24 May 2021 until 26 November 2023  
and remains valid subject to satisfactory surveillance audits.

Issue 8. Certified since 11 January 1995

Certification is based on reports numbered GB/PC 04303

This is a multi-site certification.

Additional site details are listed on the subsequent page.

Authorised by



Global Medical Devices Head of Notified Body

SGS Belgium NV, Notified Body 1639


SGS House Noorderlaan 87 2030 Antwerp Belgium  
t +32 (0)3 545 48 48 f +32 (0)3 545 48 49 [www.sgs.com](http://www.sgs.com)

LPMD5007 - Certificate CE1639 Annex I-4 EN rev. 02

Page 1 of 3



SGS SGS SGS

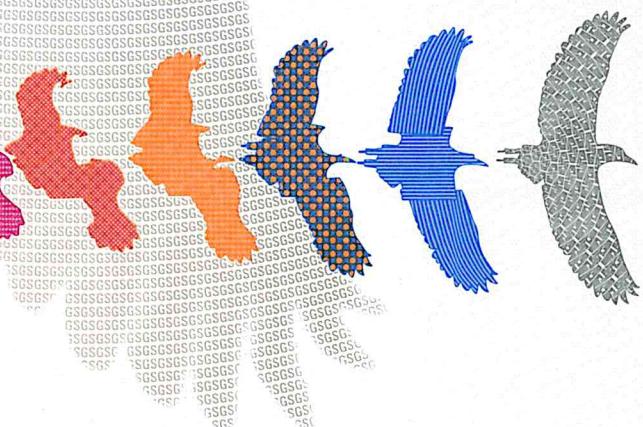

# Intersurgical Ltd.

## Directive 93/42/EEC

on medical devices, Annex II (excluding Section 4)

Issue 8

Detailed scope

**Sterile and Non-Sterile medical devices for respiratory care, in the areas of airway management, anaesthesia, critical care, oxygen and aerosol therapy:**

**Sterile and Non-Sterile Anaesthetic Breathing Systems**

**Aerosol and Oxygen Face Masks**

**Anaesthetic Face Masks**

**Sterile Endotracheal Tube Introducer and Sterile Airway Stylets**

**Sterile and Non-Sterile Breathing Systems**

**Non-Heated Respiratory Bubble Humidifier**

**Sterile and Non-Sterile Catheter Mounts**

**Sterile and Non-Sterile Breathing System Connectors**

**Sterile and Non-Sterile Respiratory Filters**

**Breathing System Flexible Tubing**

**High Concentration Oxygen Face Masks**

**Sterile and Non-Sterile Heat and Moisture Exchangers**

**Sterile and Non-Sterile HME Filters**

**Sterile and Non-Sterile Inspiratory Line Humidification Chambers**

**Sterile I-gel Supraglottic Airways**

**Sterile Laryngeal Airways**

**Gas Sampling/Monitoring Respiratory Tubing**

**Sterile and Non-Sterile Heated Wire Breathing Systems,**

**Heated Wires and attachments (electrical adaptor leads)**

**Electrically Powered Moisture Condenser, Nasal Cannulae**

**Nebulising System Delivery Sets**

**Suction and Irrigation Oral Care Toothbrush**

**Oxygen Administration Tubing**

**Repeated Use Breathing Systems**

**Breathing Systems Reservoir Bags**

**Manual Pulmonary Resuscitation Systems**

**Carbon Dioxide Absorbents**

**Sterile and Non-Sterile Tracheal Suction Systems**

**Sterile Endotracheal Tubes**

**Venturi Valves and Venturi Valve Face Mask Kits**

**Wall Humidifier Nebuliser**

**Breathing System Water Traps**

**CPAP Bi-level Nasal Masks and NIV Face Masks**

**Pressure Limiting Valves**

**Peep Valves One Way Directional Valves**

**Infant Nasal CPAP Breathing System**

**Oxygen Recovery Kits**

**Endoscopy Molar Bite Block**

**Carbon Dioxide Cuvette**

**Class I sterile: Sterility aspects only - Restricted to the aspects of manufacture concerned with securing and maintaining sterile conditions**

**Sterile Guedel Airways**

Certificate GB19/964232 continued

# Intersurgical Ltd.

## Directive 93/42/EEC

on medical devices, Annex II (excluding Section 4)

Issue 8

Detailed scope

Additional facilities

**Crane House, Molly Millars Lane, Wokingham, Berkshire, RG41 2RZ, UK**

**Unit 3, Molly Millars Bridge, RG41 2WY, UK**

**Dray House, Molly Millars Lane, RG41 2PX, UK**

**Brook House, Molly Millars Bridge, RG41 2WY, UK**

**Unit 1, Molly Millars Lane, RG41 2QZ, UK**

**Circuit House, Pitronnerie Road, Industrial Estate, St Peter Port, Guernsey, GY1 2RL, UK**

**UAB Intersurgical Arnionių g.60, LT-18170 Pabradė, Lithuania**

**Arnionių g. 60A, Pabradė, LT-18170, Lithuania**

**Arnionių g. 45, Pabradė, LT-18170, Lithuania**

**Duksto kelias 84A, Visaginas, LT-31146, Lithuania**



**Intersurgical Ltd**  
Crane House, Molly Millars Lane  
Wokingham, Berkshire  
RG41 2RZ  
UK

04/09/2023

**Confirmation Letter Reference: CLNB1639 GBPC04303**

To whom it may concern,

**Confirmation of receipt of a formal application and conclusion of written agreement in the framework of Regulation EU 2023/607 amending Regulations (EU) 2017/745 and (EU) 2017/746 as regards the transitional provisions for certain medical devices and in vitro diagnostic medical devices**

This letter confirms that, SGS Belgium NV, a Notified Body (NB) designated against Regulation (EU) 2017/745 (MDR) and identified by the number 1639 on NANDO, has received a formal application in accordance with Section 4.3, first subparagraph of Annex VII of MDR and has signed a written agreement in accordance with Section 4.3, second subparagraph of Annex VII of MDR with the following manufacturer:

**Intersurgical Ltd**  
Crane House, Molly Millars Lane  
Wokingham, Berkshire  
RG41 2RZ  
UK  
SRN number: GB-MF-000004798

**Authorised Representative**  
**UAB Intersurgical**  
Arnionių g. 60  
LT-18170 Pabradė,  
Lithuania  
SRN number: LT-AR-000003907

The devices covered by the formal application and the written agreement mentioned above are shown at the end of this letter.

In the case of devices covered by certificates issued under Directive 90/385/EEC (AIMDD) or Directive 93/42/EEC (MDD) that expired prior to the publication of the Regulation EU 2023/607 on 15 March 2023, this letter also confirms that:

- the manufacturer submitted the MDR application and signed the written agreement by the date of MDD/AMDD certificate expiry;

- the certificates expired after 26 May 2021 by course of time and were valid at the date of their expiry neither having been suspended nor withdrawn.

The transition timelines that apply to the devices covered by this letter, subject to the manufacturer's continued compliance to the other conditions specified in Article 120.3 of MDR (as amended by EU 2023/607), are shown below:

- 26 May 2026 for Class III custom-made implantable devices
- 31 December 2027 for Class III devices and Class IIb implantable devices excluding Well-established technologies (WET - sutures, staples, dental fillings, dental braces, tooth crowns, screws, wedges, plates, wires, pins, clips and connectors)
- 31 December 2028 for other Class IIb devices, Class IIa, Class I devices placed on the market in sterile condition or have a measuring function
- 31 December 2028 for devices not requiring the involvement of a notified body under MDD but requiring it under MDR (e.g., class I devices that qualify as re-usable surgical instruments)

On behalf of the Notified Body SGS Belgium NV 1639,



Virginie SILORET  
 Global Medical Device Certification Manager  
 Email: [Virginie.siloret@sgs.com](mailto:Virginie.siloret@sgs.com)  
 Phone : +41 22 739 98 58

**Devices covered by this letter:**

Device name / Basic UDI-DI (under MDR application)	MDR Device classification (as proposed by the manufacturer and verified at the pre-application stage)	If the MDR device is a substitute device, identification of the corresponding MDD/AIMDD device	MDD/AIMDD Certificate Reference(s) of the devices under MDR application, and the NB Identification
Sterile and Non-Sterile medical devices for respiratory care, in the areas of airway management, anaesthesia, critical care, oxygen and aerosol therapy:  -Sterile and Non-Sterile Anaesthetic Breathing Systems	IIa	N/A	GB19/964232; NB1639



Device name / Basic UDI-DI (under MDR application)	MDR Device classification (as proposed by the manufacturer and verified at the pre-application stage)	If the MDR device is a substitute device, identification of the corresponding MDD/AIMDD device	MDD/AIMDD Certificate Reference(s) of the devices under MDR application, and the NB Identification
05030267ABSL6  -Aerosol and Oxygen Face Masks 05030267AEROXY65  Anaesthetic Face Masks 05030267AMSKBX  Sterile Endotracheal Tube Introducer and Sterile Airway Stylets 05030267BOUGCE  Sterile and Non-Sterile Breathing Systems 05030267BS2M  Non-Heated Respiratory Bubble Humidifier 05030267BUBHUM6E  Sterile and Non-Sterile Catheter Mounts 05030267CATHMT3K  Sterile and Non-Sterile Breathing System Connectors 05030267CONNRR8V  Sterile and Non-Sterile Respiratory Filters 05030267FILTER6S  Breathing System Flexible Tubing 05030267FLEXTU8H  High Concentration Oxygen Face Masks			



Device name / Basic UDI-DI (under MDR application)	MDR Device classification (as proposed by the manufacturer and verified at the pre-application stage)	If the MDR device is a substitute device, identification of the corresponding MDD/AIMDD device	MDD/AIMDD Certificate Reference(s) of the devices under MDR application, and the NB Identification
05030267HICON7E  Sterile and Non-Sterile Heat and Moisture Exchangers 05030267HMEME  Sterile and Non-Sterile HME Filters 05030267HMEFBU  Sterile and Non-Sterile Inspiratory Line Humidification Chambers 05030267HUMCHA4  Sterile I-gel Supraglottic Airways 05030267IGELBH  Sterile Laryngeal Airways 05030267LMAMS  Gas Sampling / Monitoring Respiratory Tubing 05030267MONTUBCM  Sterile and Non-Sterile Heated Wire Breathing Systems, Heated Wires and attachments (electrical adaptor leads) 05030267HW3F  Electrically Powered Moisture Condenser, 05030267INTCOOLDZ  Nasal Cannulae 05030267NACAN6E			CONFIRMATION LETTER REGULATION (EU) 2023/601



Device name / Basic UDI-DI (under MDR application)	MDR Device classification (as proposed by the manufacturer and verified at the pre-application stage)	If the MDR device is a substitute device, identification of the corresponding MDD/AIMDD device	MDD/AIMDD Certificate Reference(s) of the devices under MDR application, and the NB Identification
Nebulising System Delivery Sets 05030267NEBME			
Suction and Irrigation Oral Care Toothbrush 05030267ORANGE9K			
Oxygen Administration Tubing 05030267OXYTUBJX			
Repeated Use Breathing Systems 05030267REPSYSCX			
Breathing Systems Reservoir Bags 05030267RESBAG7X			
Manual Pulmonary Resuscitation Systems 05030267RESUSDC			
Carbon Dioxide Absorbents 05030267SODAE6			
Sterile and Non-Sterile Tracheal Suction Systems 05030267SUCSYSFZ			
Sterile Endotracheal Tubes 05030267TRACTUBFN			
Venturi Valves and Venturi Valve Face Mask Kits 05030267VNTURIHK			
Wall Humidifier Nebuliser 05030267WALNEB8Z			

Device name / Basic UDI-DI (under MDR application)	MDR Device classification (as proposed by the manufacturer and verified at the pre-application stage)	If the MDR device is a substitute device, identification of the corresponding MDD/AIMDD device	MDD/AIMDD Certificate Reference(s) of the devices under MDR application, and the NB Identification
Breathing System Water Traps 05030267WT4N			
CPAP Bi-level Nasal Masks and NIV Face Masks 05030267CPNVMASKN6			
Pressure Limiting Valves 05030267PLVALVEGW			
Peep Valves 05030267PVALVECF			
One Way Directional Valves 05030267OWVALVELU			
Infant Nasal CPAP Breathing System 05030267NFLOWAS			
Oxygen Recovery Kits 05030267OXYRECH7			
Endoscopy Molar Bite Block 05030267BITEBLOCKR9			
Carbon Dioxide Cuvette 05030267STREAMMONBW			
Sterile Guedel Airways 05030267GUEDEL6W	Is	N/A	GB19/964232; NB1639

#### Confirmation Letter Revision History

Date	NB internal reference traceable to each version of the letter	Action
2023/09/04	Version 1	Initial issue

**Intersurgical Ltd.**

Crane House, Molly Millars Lane, Wokingham, Berkshire, RG41 2RZ, UK

**Scope**

**Sterile and Non-Sterile medical devices for respiratory care, in the areas of airway management, anaesthesia, critical care, oxygen and aerosol therapy:**

**Sterile and Non-Sterile Anaesthetic Breathing Systems**

**Aerosol and Oxygen Face Masks**

**Anaesthetic Face Masks**

**Sterile Endotracheal Tube Introducer and Sterile Airway Stylets**

**Sterile and Non-Sterile Breathing Systems**

**Non-Heated Respiratory Bubble Humidifier**

**Sterile and Non-Sterile Catheter Mounts**

**Sterile and Non-Sterile Breathing System Connectors**

**Sterile and Non-Sterile Respiratory Filters**

**Breathing System Flexible Tubing**

**High Concentration Oxygen Face Masks**

**Sterile and Non-Sterile Heat and Moisture Exchangers**

**Sterile and Non-Sterile HME Filters**

**Sterile and Non-Sterile Inspiratory Line Humidification Chambers**

**Sterile I-gel Supraglottic Airways**

**Sterile Laryngeal Airways**

**Gas Sampling/Monitoring Respiratory Tubing**

**Sterile and Non-Sterile Heated Wire Breathing Systems,  
Heated Wires and attachments (electrical adaptor leads)**

Authorised by



Global Medical Devices Certification Manager

**SGS Belgium NV, Notified Body 1639**

SGS House Noorderlaan 87 2030 Antwerp Belgium  
t +32 (0)3 545 48 48 f +32 (0)3 545 48 49 www.sgs.com

LPMD5105 – Corrigendum to Certificate

Page 1 of 2

SGS Belgium NV

Certification and Business Enhancement Maatschappelijke Zetel/Siège Social:

Noorderlaan 87 B-2030 Antwerpen/Anvers

t +32 (0)3 545 48 48 f +32 (0)3 545 48 49

[www.be.sgs.com](http://www.be.sgs.com)

Member of the SGS Group

RPR Antwerp VAT – BE 0404.882.750 Citibank BE87 5701 3412 5594

**Electrically Powered Moisture Condenser, Nasal Cannulae  
 Nebulising System Delivery Sets  
 Suction and Irrigation Oral Care Toothbrush  
 Oxygen Administration Tubing  
 Repeated Use Breathing Systems  
 Breathing Systems Reservoir Bags  
 Manual Pulmonary Resuscitation Systems  
 Carbon Dioxide Absorbents  
 Sterile and Non-Sterile Tracheal Suction Systems  
 Sterile Endotracheal Tubes  
 Venturi Valves and Venturi Valve Face Mask Kits  
 Wall Humidifier Nebuliser  
 Breathing System Water Traps  
 CPAP Bi-level Nasal Masks and NIV Face Masks  
 Pressure Limiting Valves  
 Peep Valves One Way Directional Valves  
 Infant Nasal CPAP Breathing System  
 Oxygen Recovery Kits  
 Endoscopy Molar Bite Block  
 Carbon Dioxide Cuvette  
 Class I sterile: Sterility aspects only - Restricted to the aspects of  
 manufacture  
 concerned with securing and maintaining sterile conditions:  
 Sterile Guedel Airways**

This corrigendum is only valid together with accompanying 93/42/EEC certificate  
 issue 8

<b>Correction Date</b>	<b>Correction</b>
Change approved by SGS on 11 January 2022	The client is removing one of their additional sites Unit 3 Mollay Millars Bridge, RG41 2WY
Change approved by SGS on 08 November 2022	This client is removing one of their additional facilities: Circuit House, Pitronnerie Road, Industrial Estate, St Peter Port, Guernsey, GY1 2RL, UK

The management system of

# Intersurgical Ltd.

Crane House, Molly Millars Lane, Wokingham, Berkshire, RG41 2RZ, UK

has been assessed and certified as meeting the requirements of

## Directive 93/42/EEC

on medical devices, Annex II (excluding Section 4)

For the following products

The scope of registration appears on page 2 of this certificate.

This certificate is valid from 24 May 2021 until 26 November 2023  
and remains valid subject to satisfactory surveillance audits.

Issue 8. Certified since 11 January 1995

Certification is based on reports numbered GB/PC 04303

This is a multi-site certification.

Additional site details are listed on the subsequent page.

Authorised by



Global Medical Devices Head of Notified Body

SGS Belgium NV, Notified Body 1639


SGS House Noorderlaan 87 2030 Antwerp Belgium  
t +32 (0)3 545 48 48 f +32 (0)3 545 48 49 [www.sgs.com](http://www.sgs.com)

LPMD5007 - Certificate CE1639 Annex I-4 EN rev. 02

Page 1 of 3



SGS SGS SGS

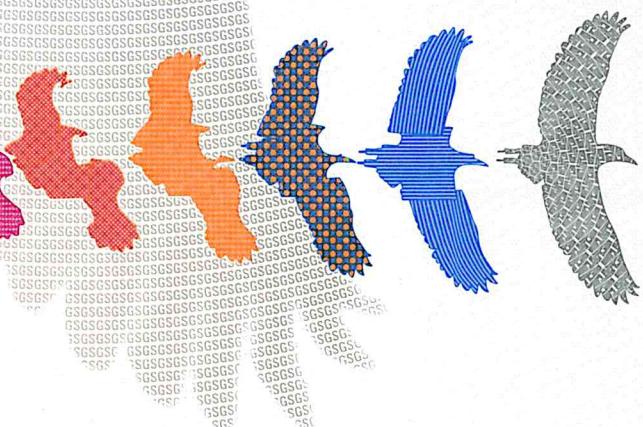

# Intersurgical Ltd.

## Directive 93/42/EEC

on medical devices, Annex II (excluding Section 4)

Issue 8

Detailed scope

**Sterile and Non-Sterile medical devices for respiratory care, in the areas of airway management, anaesthesia, critical care, oxygen and aerosol therapy:**

**Sterile and Non-Sterile Anaesthetic Breathing Systems**

**Aerosol and Oxygen Face Masks**

**Anaesthetic Face Masks**

**Sterile Endotracheal Tube Introducer and Sterile Airway Stylets**

**Sterile and Non-Sterile Breathing Systems**

**Non-Heated Respiratory Bubble Humidifier**

**Sterile and Non-Sterile Catheter Mounts**

**Sterile and Non-Sterile Breathing System Connectors**

**Sterile and Non-Sterile Respiratory Filters**

**Breathing System Flexible Tubing**

**High Concentration Oxygen Face Masks**

**Sterile and Non-Sterile Heat and Moisture Exchangers**

**Sterile and Non-Sterile HME Filters**

**Sterile and Non-Sterile Inspiratory Line Humidification Chambers**

**Sterile I-gel Supraglottic Airways**

**Sterile Laryngeal Airways**

**Gas Sampling/Monitoring Respiratory Tubing**

**Sterile and Non-Sterile Heated Wire Breathing Systems,**

**Heated Wires and attachments (electrical adaptor leads)**

**Electrically Powered Moisture Condenser, Nasal Cannulae**

**Nebulising System Delivery Sets**

**Suction and Irrigation Oral Care Toothbrush**

**Oxygen Administration Tubing**

**Repeated Use Breathing Systems**

**Breathing Systems Reservoir Bags**

**Manual Pulmonary Resuscitation Systems**

**Carbon Dioxide Absorbents**

**Sterile and Non-Sterile Tracheal Suction Systems**

**Sterile Endotracheal Tubes**

**Venturi Valves and Venturi Valve Face Mask Kits**

**Wall Humidifier Nebuliser**

**Breathing System Water Traps**

**CPAP Bi-level Nasal Masks and NIV Face Masks**

**Pressure Limiting Valves**

**Peep Valves One Way Directional Valves**

**Infant Nasal CPAP Breathing System**

**Oxygen Recovery Kits**

**Endoscopy Molar Bite Block**

**Carbon Dioxide Cuvette**

**Class I sterile: Sterility aspects only - Restricted to the aspects of manufacture concerned with securing and maintaining sterile conditions**

**Sterile Guedel Airways**

Certificate GB19/964232 continued

# Intersurgical Ltd.

## Directive 93/42/EEC

on medical devices, Annex II (excluding Section 4)

Issue 8

Detailed scope

Additional facilities

**Crane House, Molly Millars Lane, Wokingham, Berkshire, RG41 2RZ, UK**

**Unit 3, Molly Millars Bridge, RG41 2WY, UK**

**Dray House, Molly Millars Lane, RG41 2PX, UK**

**Brook House, Molly Millars Bridge, RG41 2WY, UK**

**Unit 1, Molly Millars Lane, RG41 2QZ, UK**

**Circuit House, Pitronnerie Road, Industrial Estate, St Peter Port, Guernsey, GY1 2RL, UK**

**UAB Intersurgical Arnionių g.60, LT-18170 Pabradė, Lithuania**

**Arnionių g. 60A, Pabradė, LT-18170, Lithuania**

**Arnionių g. 45, Pabradė, LT-18170, Lithuania**

**Duksto kelias 84A, Visaginas, LT-31146, Lithuania**