

ORGENTEC Diagnostika GmbH


Carl-Zeiss-Straße 49-51

55129 Mainz - Germany

Phone: +49 (0) 61 31 / 92 58-0

Fax: +49 (0) 61 31 / 92 58-58

Internet: www.orgentec.com



ORG 600 ANA Detect

INTENDED PURPOSE

ANA Detect is an ELISA test system for the qualitative measurement of IgG class autoantibodies against SS-A-52 (Ro-52), SS-A-60 (Ro-60), SS-B (La), RNP/Sm, RNP-70, RNP-A, RNP-C, Sm-BB, Sm-D, Sm-E, Sm-F, Sm-G, Scl-70, Jo-1, dsDNA, ssDNA, polynucleosomes, mononucleosomes, histone complex, histone H1, histone H2A, histone H2B, histone 3, histone H4, Pm-Scl-100 and centromere B in human serum or plasma samples. This product is intended for professional in vitro diagnostic use only.

The test is used for screening of patients with suspected autoimmune connective tissue diseases, e.g. systemic lupus erythematosus, mixed connective tissue disease, Sjogren's syndrome, scleroderma, and polymyositis/dermatomyositis. Evaluation of a test result should always take into account all clinical and laboratory diagnostic findings.

SYMBOLS USED ON LABELS



In vitro diagnostic medical device



Manufacturer



Catalogue number



Sufficient for 96 determinations



Batch code



Use by



Temperature limitation



Keep away from sunlight



Do not reuse



Date of manufacture



CE marked according to 98/79/EC



Consult instructions for use



Electronic Instruction For Use: version



Microplate



Control



Control



Control



Sample Buffer P



Enzyme Conjugate



TMB Substrate



Stop solution



Wash Buffer



Ready to use

PRINCIPLE OF THE TEST

A mixture of purified antigens SS-A-52 (Ro-52), SS-A-60 (Ro-60), SS-B (La), RNP/Sm, RNP-70, RNP-A, RNP-C, Sm-BB, Sm-D, Sm-E, Sm-F, Sm-G, Scl-70, Jo-1, dsDNA, ssDNA, polynucleosomes, mononucleosomes, histone complex, histone H1, histone H2A, histone H2B, histone 3, histone H4, Pm-Scl-100 and centromere B is coated on to microwells.

The determination is based on an indirect enzyme linked immune reaction with the following steps:

Specific antibodies in the patient sample bind to the antigen coated on the surface of the reaction wells. After incubation, a washing step removes unbound and unspecifically bound serum or plasma components. Subsequently added enzyme conjugate binds to the immobilized antibody-antigen-complexes. After incubation, a second washing step removes unbound enzyme conjugate. After addition of substrate solution the bound enzyme conjugate hydrolyses the substrate forming a blue coloured product. Addition of an acid stops the reaction generating a yellow end-product. The intensity of the yellow color correlates with the concentration of the antibody-antigen-complex and can be measured photometrically at 450 nm.

WARNINGS AND PRECAUTIONS

- All reagents of this kit are intended for professional in vitro diagnostic use only.
- Components containing human serum were tested and found negative for HBsAg, HCV, HIV1 and HIV2 by FDA approved methods. No test can guarantee the absence of HBsAg, HCV, HIV1 or HIV2, and so all human serum based reagents in this kit must be handled as though capable of transmitting infection.
- Bovine serum albumin (BSA) used in components has been tested for BSE and found negative.
- Avoid contact with the substrate TMB (3,3',5,5'-Tetramethyl-benzidine).
- Stop solution contains acid, classification is non-hazardous. Avoid contact with skin.
- Control, sample buffer and wash buffer contain sodium azide 0.09% as preservative. This concentration is classified as non-hazardous.
- Enzyme conjugate contains ProClin 300 0.05% as preservative. This concentration is classified as non-hazardous.

During handling of all reagents, controls and serum samples observe the existing regulations for laboratory safety regulations and good laboratory practice:

- First aid measures: In case of skin contact, immediately wash thoroughly with water and soap. Remove contaminated clothing and shoes and wash before reuse. If system fluid comes into contact with skin, wash thoroughly with water. After contact with the eyes carefully rinse the opened eye with running water for at least 10 minutes. Get medical attention if necessary.
 - Personal precautions, protective equipment and emergency procedures:
Observe laboratory safety regulations. Avoid contact with skin and eyes. Do not swallow. Do not pipette by mouth. Do not eat, drink, smoke or apply makeup in areas where specimens or kit reagents are handled. When spilled, absorb with an inert material and put the spilled material in an appropriate waste disposal.
 - Exposure controls / personal protection: Wear protective gloves of nitril rubber or natural latex. Wear protective glasses. Used according to intended use no dangerous reactions known.
 - Conditions to avoid: Since substrate solution is light-sensitive. Store in the dark.
 - For disposal of laboratory waste the national or regional legislation has to be observed.
- Observe the guidelines for performing quality control in medical laboratories by assaying control sera.

CONTENTS OF THE KIT

ORG 600	▽ 96	Sufficient for 96 determinations
MICROPLATE	1	One divisible microplate consisting of 12 modules of 8 wells each. Ready to use. Product code on module: ANA
CONTROL A	1x 1.5 ml	Control A (negative), containing ANA antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN ₃ 0.09%), yellow. Ready to use.
CONTROL B	1x 1.5 ml	Control B (cut-off), containing ANA antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN ₃ 0.09%), yellow. Ready to use.
CONTROL C	1x 1.5 ml	Control C (positive), containing ANA antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN ₃ 0.09%), yellow. Ready to use.
DILUENT	20 ml	Sample Buffer P, containing PBS, BSA, detergent, preservative sodium azide 0.09%, yellow, concentrate (5 x).
CONJUGATE	15 ml	Enzyme Conjugate containing anti-human IgG antibodies, HRP labelled; PBS, BSA, detergent, preservative PROCLIN 0.05%, light red. Ready to use.
TMB	15 ml	TMB Substrate; containing 3,3', 5,5'- Tetramethylbenzidin, colorless. Ready to use.
STOP	15 ml	Stop solution; contains acid. Ready to use.
WASH	20 ml	Wash Buffer, containing Tris, detergent, preservative sodium azide 0.09%; 50 x conc.
i	1	Certificate of Analysis

MATERIALS REQUIRED

- Microplate reader capable of endpoint measurements at 450 nm; optional: reference filter at 620 nm
- Data reduction software
- Multi-channel dispenser or repeatable pipette for 100 µl
- Vortex mixer
- Pipettes for 10 µl, 100 µl and 1000 µl
- Laboratory timing device
- Distilled or deionised water
- Measuring cylinder for 1000 ml and 100 ml
- Plastic container for storage of the wash solution

This ELISA assay is suitable for use on open automated ELISA processors. Each assay has to be validated on the respective automated system. Detailed information is provided upon request.

SPECIMEN COLLECTION, STORAGE AND HANDLING

- Collect whole blood specimens using acceptable medical techniques to avoid hemolysis.
- Allow blood to clot and separate the serum or plasma by centrifugation.
- Test serum should be clear and non-hemolyzed. Contamination by hemolysis or lipemia should be avoided, but does not interfere with this assay.
- Specimens may be refrigerated at 2-8°C for up to five days or stored at -20°C up to six months.
- Avoid repetitive freezing and thawing of serum or plasma samples. This may result in variable loss of antibody activity.
- Testing of heat-inactivated sera is not recommended.

STORAGE AND STABILITY

- Store test kit at 2-8°C in the dark.
- Do not expose reagents to heat, sun, or strong light during storage and usage.
- Store microplate sealed and desiccated in the clip bag provided.
- Shelf life of the unopened test kit is 18 months from day of production.
Unopened reagents are stable until expiration of the kit. See labels for individual batch.
- Diluted Wash Buffer and Sample Buffer are stable for at least 30 days when stored at 2-8°C.
We recommend consumption on the same day.

PROCEDURAL NOTES

- Do not use kit components beyond their expiration dates.
- Do not interchange kit components from different lots and products.

- All materials must be at room temperature (20-28°C) prior to use.
- Prepare all reagents and samples. Once started, perform the test without interruption.
- Double determinations may be done. By this means pipetting errors may become obvious.
- Perform the assay steps only in the order indicated.
- Always use fresh sample dilutions.
- Pipette all reagents and samples into the bottom of the wells.
- To avoid carryover or contamination, change the pipette tip between samples and different kit controls.
- Wash microwells thoroughly and remove the last droplets of wash buffer.
- All incubation steps must be accurately timed.
- Do not re-use microplate wells.

PREPARATION OF REAGENTS

WASH

Dilute the contents of one vial of the buffered wash solution concentrate (50x) with distilled or deionised water to a final volume of 1000 ml prior to use.

DILUENT

Sample Buffer P: Prior to use dilute the contents (20 ml) of one vial of sample buffer 5x concentrate with distilled or deionised water to a final volume of 100 ml.

Preparation of samples

Dilute patient samples 1:100 before the assay: Put 990 µl of prediluted sample buffer in a polystyrene tube and add 10 µl of sample. Mix well. Note: Calibrators / Controls are ready to use and need not be diluted.

TEST PROCEDURE

Prepare enough microplate modules for all calibrators / controls and patient samples.

- Pipette **100 µl** of calibrators, controls and prediluted patient samples into the wells.
Incubate for **30 minutes** at room temperature (20-28 °C).
Discard the contents of the microwells and **wash 3 times** with **300 µl** of wash solution.
- Dispense **100 µl** of enzyme conjugate into each well.
Incubate for **15 minutes** at room temperature.
Discard the contents of the microwells and **wash 3 times** with **300 µl** of wash solution.
- Dispense **100 µl** of TMB substrate solution into each well.
Incubate for **15 minutes** at room temperature
- Add 100 µl** of stop solution to each well of the modules
Incubate for **5 minutes** at room temperature.
Read the optical density at 450 nm (reference 600-690nm) and calculate the results.
The developed colour is stable for at least 30 minutes. Read during this time.

Example for a pipetting scheme:

	1	2	3	4	5	6	7	8	9	10	11	12
A	A											
B	B											
C	C											
D	P1											
E	P2											
F	P3											
G												
H												

P1, ... patient sample A-C controls

VALIDATION

Test results are valid if the optical densities at 450 nm for calibrators / controls and the results for controls comply with the reference ranges indicated on the Certificate of Analysis enclosed in each test kit.

If these quality control criteria are not met the assay run is invalid and should be repeated.

CALCULATION OF RESULTS

For qualitative results the optical density (OD) of a sample is compared to the optical density of Control B:

Negative: OD sample < OD Control B

Positive: OD sample ≥ OD Control B

For detailed results the optical density of a sample is expressed as Index value:

Index = OD sample / OD Control B

PERFORMANCE CHARACTERISTICS

Calibration

The assay system is calibrated against the internationally recognised reference sera from CDC, Atlanta, USA and furthermore against the reference preparation WHO Wo/80 for human anti-dsDNA.

Measuring range

not applicable

Expected values

In a normal range study with samples from healthy blood donors the following ranges have been established with this ELISA assay: Cut-off Index 1.0

Interpretation of results

Negative: Index < 1.0
Borderline: Index 1.0 - 1.2
Positive: Index > 1.2

Linearity

Patient samples containing high levels of specific antibody were serially diluted in sample buffer. Activity for each dilution step was calculated as Index-Value.

Sample	Dilution	Observed Index	Expected Index	O/E [%]
1	1:100	4.8	4.8	100
	1:200	2.2	2.4	92
	1:400	1.3	1.2	108
2	1:800	0.6	0.6	100
	1:100	2.8	2.8	100
	1:200	1.5	1.4	107
3	1:400	0.8	0.7	114
	1:800	0.4	0.4	111
	1:100	3.5	3.5	100
	1:200	1.7	1.8	94
	1:400	0.8	0.9	89
	1:800	0.5	0.5	96

Limit of detection (not applicable)

n.a.

Reproducibility

Intra-assay precision: Coefficient of variation (CV) was calculated for each of three samples from the results of 24 determinations in a single run. Results for precision-within-assay are shown in the table below.

Inter-assay precision: Coefficient of variation (CV) was calculated for each of three samples from the results of 6 determinations in 5 different runs. Results for run-to-run precision are shown in the table below.

Intra-Assay		
Sample	Mean Index	CV %
1	1.8	6.9
2	2.4	9.1
3	2.8	10.4

Inter-Assay		
Sample	Mean Index	CV %
1	1.6	9.9
2	3.7	10.4
3	4.1	11.2

Interfering substances

No interference has been observed with haemolytic (up to 1000 mg/dl) or lipemic (up to 3 g/dl triglycerides) sera or plasma, or bilirubin (up to 40 mg/dl) containing sera or plasma. Nor have any interfering effects been observed with the use of anticoagulants (Citrate, EDTA, Heparine). However for practical reasons it is recommended that grossly hemolyzed or lipemic samples should be avoided.

Study results

Study population	n	n Pos	%
SLE	63	62	98.4
Sjogren's syndrome	2	2	100.0
MCTD	9	9	100.0
Poly-/dermatomyositis	8	8	100.0
Scleroderma	3	3	100.0
CREST syndrome	9	9	100.0
Normal human sera	148	3	2.0

		Clinical Diagnosis		
		POS	NEG	
ORG 600	POS	93	3	242
	NEG	1	145	
		94	148	
Sensitivity:		98.9 %		
Specificity:		98.0 %		
Overall agreement:		98.3 %		

LIMITATIONS OF THE PROCEDURE

This assay is a diagnostic aid. A definite clinical diagnosis should not be based on the results of a single test, but should be made by the physician after all clinical and laboratory findings have been evaluated concerning the entire clinical picture of the patient. Also every decision for therapy should be taken individually.

The above pathological and normal reference ranges for antibodies in patient samples should be regarded as recommendations only. Each laboratory should establish its own ranges according to ISO 15189 or other applicable laboratory guidelines.

REFERENCES

- Alba P, Bento L, Cuadrado MJ, Karim Y, Tungekar MF, Abbs I et al. Anti-dsDNA, anti-Sm antibodies, and the lupus anticoagulant: significant factors associated with lupus nephritis. *Ann Rheum Dis* 2003; 62(6):556-560.
- Antico A, Platzgummer S, Bassetti D, Bizzaro N, Tozzoli R, Villalta D. Diagnosing systemic lupus erythematosus: new-generation immunoassays for measurement of anti-dsDNA antibodies are an effective alternative to the Farr technique and the Crithidia luciliae immunofluorescence test. *Lupus* 2010; 19(8):906-912.
- Brouwer R, Hengstman GJ, Vree EW, Ehrfeld H, Bozic B, Ghirardello A et al. Autoantibody profiles in the sera of European patients with myositis. *Ann Rheum Dis* 2001; 60(2):116-123.
- Castro C, Gourley M. Diagnostic testing and interpretation of tests for autoimmunity. *J Allergy Clin Immunol* 2010; 125(2 Suppl 2):S238-S247.
- Defendenti C, Atzeni F, Spina MF, Grosso S, Cereda A, Guercilena G et al. Clinical and laboratory aspects of Ro/SSA-52 autoantibodies. *Autoimmun Rev* 2011; 10(3):150-154.
- Eriksson C, Kokkonen H, Johansson M, Hallmans G, Wadell G, Rantapaa-Dahlqvist S. Autoantibodies predate the onset of Systemic Lupus Erythematosus in northern Sweden. *Arthritis Research & Therapy* 2011; 13(1):R30.
- Haugbro K, Nossent JC, Winkler T, Figenschau Y, Rekvig OP. Anti-dsDNA antibodies and disease classification in antinuclear antibody positive patients: the role of analytical diversity. *Ann Rheum Dis JID* - 0372355 2004; 63(4):386-394.
- Ippolito A, Wallace DJ, Gladman D, Fortin PR, Urowitz M, Werth V et al. Autoantibodies in systemic lupus erythematosus: comparison of historical and current assessment of seropositivity. *Lupus* 2011; 20(3):250-255.
- Isenberg DA, Manson JJ, Ehrenstein MR, Rahman A. Fifty years of anti-ds DNA antibodies: are we approaching journey's end? *Rheumatology (Oxford)* 2007; 46(7):1052-1056.
- Kattah NH, Kattah MG, Utz PJ. The U1-snRNP complex: structural properties relating to autoimmune pathogenesis in rheumatic diseases. *Immunol Rev* 2010; 233(1):126-145.
- Kumar Y, Bhatia A, Minz RW. Antinuclear antibodies and their detection methods in diagnosis of connective tissue diseases: a journey revisited. *Diagn Pathol* 2009; 4:1.
- Meroni PL, Schur PH. ANA screening: an old test with new recommendations. *Ann Rheum Dis* 2010; 69:1420-1422.
- Petri M, Magder L. Classification criteria for systemic lupus erythematosus: a review. *Lupus* 2004; 13(11):829-837.
- Poole BD, Schneider RI, Guthridge JM, Velte CA, Reichlin M, Harley JB et al. Early targets of nuclear RNP humoral autoimmunity in human systemic lupus erythematosus. *Arthritis Rheum* 2009; 60(3):848-859.
- Putova I, Dostal C, Becvar R. Prevalence of antinucleosome antibodies by enzyme-linked immunosorbent assays in patients with systemic lupus erythematosus and other autoimmune systemic diseases. *Ann N Y Acad Sci* 2007; 1109:275-286.
- Reveille JD. Predictive value of autoantibodies for activity of systemic lupus erythematosus. *Lupus JID* - 9204265 2004; 13(5):290-297.
- Simon JA, Cabiedes J, Ortiz E, Alcocer-Varela J, Sanchez-Guerrero J. Anti-nucleosome antibodies in patients with systemic lupus erythematosus of recent onset. Potential utility as a diagnostic tool and disease activity marker. *Rheumatology (Oxford)* 2004; 43(2):220-224.
- Sinclair D, Saas M, Williams D, Hart M, Goswami R. Can an ELISA replace immunofluorescence for the detection of anti-nuclear antibodies?--The routine use of anti-nuclear antibody screening ELISAs. *Clin Lab*

2007; 53(3-4):183-191.

- Tozzoli R, Bizzaro N, Tonutti E, Villalta D, Bassetti D, Manoni F et al. Guidelines for the laboratory use of autoantibody tests in the diagnosis and monitoring of autoimmune rheumatic diseases. *Am J Clin Pathol* 2002; 117(2):316-324.
- Maidhof W., Hilius O. Lupus: an overview of the disease and management options. *P T* 2012; 37(4):240-9.
- Hahn BH, McMahon MA, Wilkinson A, Wallace WD, Daikh DI, Fitzgerald JD et al. American College of Rheumatology guidelines for screening, treatment, and management of lupus nephritis. *Arthritis Care Res (Hoboken)* 2012; 64(6):797-808.

Notice to the user (European Union):

Any serious incident that has occurred in relation to the device shall be reported to the manufacturer and the competent authority of the EU Member State in which the user and/or the patient is established .

Change Control

Former version: *ORG 600_IFU_EN_QM113200_2013-12-16_1.2* Reason for revision: *Introduction electronic IFU on homepage*

- 1** Pipet **100 µl** calibrator, control or patient sample
→ Incubate for **30 minutes** at room temperature
→ Discard the contents of the wells and wash 3 times with **300 µl** wash solution
- 2** Pipet **100 µl** enzyme conjugate
→ Incubate for **15 minutes** at room temperature
→ Discard the contents of the wells and wash 3 times with **300 µl** wash solution
- 3** Pipet **100 µl** substrate solution
→ Incubate for **15 minutes** at room temperature
- 4** Add **100 µl** stop solution
→ Leave untouched for **5 minutes**
→ Read at **450 nm**

ORGENTEC Diagnostika GmbH

Carl-Zeiss-Straße 49-51


55129 Mainz - Germany

Phone: +49 (0) 61 31 / 92 58-0

Fax: +49 (0) 61 31 / 92 58-58

Internet: www.orgentec.com



 **601_3**





























ORG 601 Anti-CCP hs® (high sensitive)

INTENDED PURPOSE

Anti-CCP hs® (high sensitive) is an ELISA test system for the quantitative measurement of IgG class autoantibodies against cyclic citrullinated peptides (CCP) in human serum or plasma. This product is intended for professional in vitro diagnostic use only.

Measurement of anti-CCP antibodies may aid in the diagnosis of rheumatoid arthritis (RA), where anti-CCP antibody levels represent one parameter of a multi-criterion diagnostic process, encompassing both clinical and laboratory-based assessments.

SYMBOLS USED ON LABELS

	In vitro diagnostic medical device		Microplate
	Manufacturer		Calibrator
	Catalogue number		Calibrator
	Sufficient for 96 determinations		Calibrator
	Batch code		Calibrator
	Use by		Calibrator
	Temperature limitation		Calibrator
	Keep away from sunlight		Control positive
	Do not reuse		Control negative
	Date of manufacture		Sample Buffer P
	CE marked according to 98/79/EC		Enzyme Conjugate
	Consult instructions for use		TMB Substrate
	Electronic Instruction For Use: version		Stop solution
			Wash Buffer
			Ready to use

PRINCIPLE OF THE TEST

Highly purified cyclic citrullinated vimentin peptides (CCP) is bound to microwells.

The determination is based on an indirect enzyme linked immune reaction with the following steps:

Specific antibodies in the patient sample bind to the antigen coated on the surface of the reaction wells. After incubation, a washing step removes unbound and unspecifically bound serum or plasma components. Subsequently added enzyme conjugate binds to the immobilized antibody-antigen-complexes. After incubation, a second washing step removes unbound enzyme conjugate. After addition of substrate solution the bound enzyme conjugate hydrolyses the substrate forming a blue coloured product. Addition of an acid stops the reaction generating a yellow end-product. The intensity of the yellow color correlates with the concentration of the antibody-antigen-complex and can be measured photometrically at 450 nm.

WARNINGS AND PRECAUTIONS

- All reagents of this kit are intended for professional in vitro diagnostic use only.
- Components containing human serum were tested and found negative for HBsAg, HCV, HIV1 and HIV2 by FDA approved methods. No test can guarantee the absence of HBsAg, HCV, HIV1 or HIV2, and so all human serum based reagents in this kit must be handled as though capable of transmitting infection.
- Bovine serum albumin (BSA) used in components has been tested for BSE and found negative.
- Avoid contact with the substrate TMB (3,3',5,5'-Tetramethyl-benzidine).
- Stop solution contains acid, classification is non-hazardous. Avoid contact with skin.
- Control, sample buffer and wash buffer contain sodium azide 0.09% as preservative. This concentration is classified as non-hazardous.
- Enzyme conjugate contains ProClin 300 0.05% as preservative. This concentration is classified as non-hazardous.

During handling of all reagents, controls and serum samples observe the existing regulations for laboratory safety regulations and good laboratory practice:

- First aid measures: In case of skin contact, immediately wash thoroughly with water and soap. Remove contaminated clothing and shoes and wash before reuse. If system fluid comes into contact with skin, wash thoroughly with water. After contact with the eyes carefully rinse the opened eye with running water for at least 10 minutes. Get medical attention if necessary.
- Personal precautions, protective equipment and emergency procedures:
Observe laboratory safety regulations. Avoid contact with skin and eyes. Do not swallow. Do not pipette by mouth. Do not eat, drink, smoke or apply makeup in areas where specimens or kit reagents are handled. When spilled, absorb with an inert material and put the spilled material in an appropriate waste disposal.
- Exposure controls / personal protection: Wear protective gloves of nitril rubber or natural latex. Wear protective glasses. Used according to intended use no dangerous reactions known.
- Conditions to avoid: Since substrate solution is light-sensitive. Store in the dark.
- For disposal of laboratory waste the national or regional legislation has to be observed.

Observe the guidelines for performing quality control in medical laboratories by assaying control sera.

CONTENTS OF THE KIT

ORG 601	▽ 96	Sufficient for 96 determinations
MICROPLATE	1	One divisible microplate consisting of 12 modules of 8 wells each. Ready to use. Product code on module: CCP
CALIBRATOR A	1x 1.5 ml	Calibrator A 0 U/ml, containing serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
CALIBRATOR B	1x 1.5 ml	Calibrator B 20 U/ml, containing CCP antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
CALIBRATOR C	1x 1.5 ml	Calibrator C 40 U/ml, containing CCP antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
CALIBRATOR D	1x 1.5 ml	Calibrator D 100 U/ml, containing CCP antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
CALIBRATOR E	1x 1.5 ml	Calibrator E 300 U/ml, containing CCP antibodies in a serum/buffer matrix (PBS, BSA, NaN3 0.09%), yellow. Ready to use.
CALIBRATOR F	1x 1.5 ml	Calibrator F 1000 U/ml, containing CCP antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
CONTROL +	1x 1.5 ml	Control positive, containing CCP antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use. The concentration is specified on the certificate of analysis.
CONTROL -	1x 1.5 ml	Control negative, containing CCP antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use. The concentration is specified on the certificate of analysis.
DILUENT	20 ml	Sample Buffer P, containing PBS, BSA, detergent, preservative sodium azide 0.09%, yellow, concentrate (5 x).
CONJUGATE	15 ml	Enzyme Conjugate containing anti-human IgG antibodies, HRP labelled; PBS, BSA, detergent, preservative PROCLIN 0.05%, light red. Ready to use.
TMB	15 ml	TMB Substrate; containing 3,3', 5,5'- Tetramethylbenzidin, colorless. Ready to use.
STOP	15 ml	Stop solution; contains acid. Ready to use.
WASH	20 ml	Wash Buffer, containing Tris, detergent, preservative sodium azide 0.09%; 50 x conc.
i	1	Certificate of Analysis

MATERIALS REQUIRED

- Microplate reader capable of endpoint measurements at 450 nm; optional: reference filter at 620 nm
- Data reduction software
- Multi-channel dispenser or repeatable pipette for 100 µl
- Vortex mixer
- Pipettes for 10 µl, 100 µl and 1000 µl
- Laboratory timing device
- Distilled or deionised water
- Measuring cylinder for 1000 ml and 100 ml
- Plastic container for storage of the wash solution

This ELISA assay is suitable for use on open automated ELISA processors. Each assay has to be validated on the respective automated system. Detailed information is provided upon request.

SPECIMEN COLLECTION, STORAGE AND HANDLING

- Collect whole blood specimens using acceptable medical techniques to avoid hemolysis.
- Allow blood to clot and separate the serum or plasma by centrifugation.
- Test serum should be clear and non-hemolyzed. Contamination by hemolysis or lipemia should be avoided, but does not interfere with this assay.
- Specimens may be refrigerated at 2-8°C for up to five days or stored at -20°C up to six months.
- Avoid repetitive freezing and thawing of serum or plasma samples. This may result in variable loss of antibody activity.
- Testing of heat-inactivated sera is not recommended.

STORAGE AND STABILITY

- Store test kit at 2-8°C in the dark.
- Do not expose reagents to heat, sun, or strong light during storage and usage.
- Store microplate sealed and desiccated in the clip bag provided.
- Shelf life of the unopened test kit is 18 months from day of production.
Unopened reagents are stable until expiration of the kit. See labels for individual batch.
- Diluted Wash Buffer and Sample Buffer are stable for at least 30 days when stored at 2-8°C.
We recommend consumption on the same day.

PROCEDURAL NOTES

- Do not use kit components beyond their expiration dates.
- Do not interchange kit components from different lots and products.
- All materials must be at room temperature (20-28°C) prior to use.
- Prepare all reagents and samples. Once started, perform the test without interruption.
- Double determinations may be done. By this means pipetting errors may become obvious.
- Perform the assay steps only in the order indicated.
- Always use fresh sample dilutions.
- Pipette all reagents and samples into the bottom of the wells.
- To avoid carryover or contamination, change the pipette tip between samples and different kit controls.
- Wash microwells thoroughly and remove the last droplets of wash buffer.
- All incubation steps must be accurately timed.
- Do not re-use microplate wells.

PREPARATION OF REAGENTS

WASH

Dilute the contents of one vial of the buffered wash solution concentrate (50x) with distilled or deionised water to a final volume of 1000 ml prior to use.

DILUENT

Sample Buffer P: Prior to use dilute the contents (20 ml) of one vial of sample buffer 5x concentrate with distilled or deionised water to a final volume of 100 ml.

Preparation of samples

Dilute patient samples 1:100 before the assay: Put 990 µl of prediluted sample buffer in a polystyrene tube and add 10 µl of sample. Mix well. Note: Calibrators / Controls are ready to use and need not be diluted.

TEST PROCEDURE

Prepare enough microplate modules for all calibrators / controls and patient samples.

- Pipette **100 µl** of calibrators, controls and prediluted patient samples into the wells.
Incubate for **30 minutes** at room temperature (20-28 °C).
Discard the contents of the microwells and **wash 3 times** with **300 µl** of wash solution.
- Dispense **100 µl** of enzyme conjugate into each well.
Incubate for **15 minutes** at room temperature.
Discard the contents of the microwells and **wash 3 times** with **300 µl** of wash solution.
- Dispense **100 µl** of TMB substrate solution into each well.
Incubate for **15 minutes** at room temperature.
- Add 100 µl** of stop solution to each well of the modules
Incubate for **5 minutes** at room temperature.
Read the optical density at 450 nm (reference 600-690nm) and calculate the results.
The developed colour is stable for at least 30 minutes. Read during this time.

Example for a pipetting scheme:

	1	2	3	4	5	6	7	8	9	10	11	12
A	A	P1										
B	B	P2										
C	C	P3										
D	D											
E	E											
F	F											
G	C+											
H	C-											

P1, ... patient sample A-F calibrators C+, C- controls

VALIDATION

Test results are valid if the optical densities at 450 nm for calibrators / controls and the results for controls comply with the reference ranges indicated on the Certificate of Analysis enclosed in each test kit.

If these quality control criteria are not met the assay run is invalid and should be repeated.

CALCULATION OF RESULTS

For quantitative results plot the optical density of each calibrator versus the calibrator concentration to create a calibration curve. The concentration of patient samples may then be estimated from the calibration curve by interpolation.

Using data reduction software a 4-Parameter-Fit with lin-log coordinates for optical density and concentration is the data reduction method of choice.

PERFORMANCE CHARACTERISTICS

Calibration

This assay system is calibrated in relative arbitrary units. It is calibrated against an external anti-CCP Assay, since no international reference sera for RA diagnostic are available so far.

Measuring range

The calculation range of this ELISA assay is 0 - 1000 U/ml

Expected values

In a normal range study with samples from healthy blood donors the following ranges have been established with this ELISA assay: Cut-off 20 U/ml

Interpretation of results

Negative: < 20 U/ml
Positive: ≥ 20 U/ml

Linearity

Patient samples containing high levels of specific antibody were serially diluted in sample buffer to demonstrate the dynamic range of the assay and the upper / lower end of linearity. Activity for each dilution was calculated from the calibration curve using a 4-Parameter-Fit with lin-log coordinates.

Sample	Dilution	Observed U/ml	Expected U/ml	O/E [%]
1	1:100	950.2	950.2	100
	1:200	467.3	475.1	98
	1:400	245.4	237.6	103
	1:800	115.6	118.8	97
2	1:100	120.0	120.0	100
	1:200	60.5	60.0	101
	1:400	31.4	30.0	105
	1:800	14.2	15.0	95
3	1:1600	7.3	7.5	97
	1:100	321.3	321.3	100
	1:200	157.9	160.7	98
	1:400	96.4	80.3	120
	1:800	48.2	40.2	120

Limit of detection

Functional sensitivity was determined to be: 1 U/ml

Reproducibility

Intra-assay precision: Coefficient of variation (CV) was calculated for each of three samples from the results of 24 determinations in a single run. Results for precision-within-assay are shown in the table below.

Inter-assay precision: Coefficient of variation (CV) was calculated for each of three samples from the results of 6 determinations in 5 different runs. Results for run-to-run precision are shown in the table below.

Intra-Assay		
Sample	Mean U/ml	CV %
1	13.0	7.8
2	144.5	9.9
3	250.6	13.6

Inter-Assay		
Sample	Mean U/ml	CV %
1	12.3	6.1
2	134.9	7.1
3	262.2	9.3

Interfering substances

No interference has been observed with haemolytic (up to 1000 mg/dl) or lipemic (up to 3 g/dl triglycerides) sera or plasma, or bilirubin (up to 40 mg/dl) containing sera or plasma. Nor have any interfering effects been observed with the use of anticoagulants (Citrate, EDTA, Heparine). However for practical reasons it is recommended that grossly hemolyzed or lipemic samples should be avoided.

Study results

Study population	n	n Pos	%
Rheumatoid arthritis	259	237	91.5
Other arthritis	22	6	27.3
Other rheumatic disease	37	1	2.7
Healthy controls	118	1	0.8

		Clinical Diagnosis		
		POS	NEG	
ORG 601	POS	237	8	
	NEG	22	169	
		259	177	436
Sensitivity:		91.5 %		
Specificity:		95.5 %		
Overall agreement:		93.1 %		

LIMITATIONS OF THE PROCEDURE

This assay is a diagnostic aid. A definite clinical diagnosis should not be based on the results of a single test, but should be made by the physician after all clinical and laboratory findings have been evaluated concerning the entire clinical picture of the patient. Also every decision for therapy should be taken individually.

The above pathological and normal reference ranges for antibodies in patient samples should be regarded as recommendations only. Each laboratory should establish its own ranges according to ISO 15189 or other applicable laboratory guidelines.

REFERENCES

- Bang H, Egerer K, Gaudiard A, et al. Mutation and citrullination modifies vimentin to a novel autoantigen for rheumatoid arthritis. *Arthritis Rheum.* 56(8):2503, 2007.
- Aletaha D, et al. Rheumatoid arthritis classification criteria: An American College of Rheumatology/European League Against Rheumatism collaborative initiative. *Arthritis & Rheumatism* 62 (9):2569-2581, 2010.
- Prujin GJ, Wiik A, van Venrooij WJ. The use of citrullinated peptides and proteins for the diagnosis of rheumatoid arthritis. *Arthritis Res Ther* 12 (1):203, 2010.
- Snir O, Widhe M, Hermansson M, von Spee C, Lindberg J, Hensen S, Lundberg K, Engstrom A, Venables PJ, Toes RE, Holmdahl R, Klareskog L, Malmstrom V. Antibodies to several citrullinated antigens are enriched in the joints of rheumatoid arthritis patients. *Arthritis Rheum* 62 (1):44-52, 2009.
- Van Steendam K, Tillemans K, Deforce D. The relevance of citrullinated vimentin in the production of antibodies against citrullinated proteins and the pathogenesis of rheumatoid arthritis. *Rheumatology (Oxford)*, 2011.
- Van Steendam K, Tillemans K, De Ceuleneer M, De Keyser F, Elewaut D, Deforce D. Citrullinated vimentin as an important antigen in immune complexes from synovial fluid of rheumatoid arthritis patients with antibodies against citrullinated proteins. *Arthritis Res Ther* 12 (4):R132, 2010.
- Syversen SW, Goll GL, van der Heijde D, Landewe R, Lie BA, Odegard S, Uhlig T, Gaarder PI, Kvien TK. Prediction of radiographic progression in rheumatoid arthritis and the role of antibodies against mutated citrullinated vimentin: results from a ten-year prospective study. *Ann.Rheum.Dis.* 69 (2):345-351, 2009.
- Innala L, Kokkonen H, Eriksson C, Jidell E, Berglin E, Dahlqvist SR. Antibodies against mutated citrullinated vimentin are a better predictor of disease activity at 24 months in early rheumatoid arthritis than antibodies against cyclic citrullinated peptides. *J Rheumatol.* 35(6):1002, 2008.
- Mathsson L, Mullazehi M, Wick MC, et al. Antibodies against citrullinated vimentin in rheumatoid arthritis: higher sensitivity and extended prognostic value concerning future radiographic progression as compared with antibodies against cyclic citrullinated peptides. *Arthritis Rheum.* 58(1):36, 2008.
- Soós L, Szekanez Z, Szabó Z, et al. Clinical evaluation of anti-mutated citrullinated vimentin by ELISA in rheumatoid arthritis. *J Rheumatol.* 34(8):1658, 2007.
- Bizzaro N, Tonutti E, Tozzoli R, Villalta D. Analytical and diagnostic characteristics of 11 2nd- and 3rd-generation immunoenzymatic methods for the detection of antibodies to citrullinated proteins. *Clin Chem.* 53 (8):1527, 2007.
- Coenen D, Verschuere P, Westhovens R, Bossuyt X. Technical and diagnostic performance of 6 assays for the measurement of citrullinated protein/peptide antibodies in the diagnosis of rheumatoid arthritis. *Clin Chem.* 53(3):498, 2007.
- Dejaco C, Klotz W, Larcher H, Duftner C, Schirmer M, Herold M. Diagnostic value of antibodies against a modified citrullinated vimentin in rheumatoid arthritis. *Arthritis Res Ther.* 8(4):R119, 2006.
- Keskin G, Inal A, Keskin D, et al. Diagnostic utility of anti-cyclic citrullinated peptide and anti-modified citrullinated vimentin antibodies in rheumatoid arthritis. *Protein Pept Lett.* 15(3):314 2008.
- Poulsom H, Charles PJ. Antibodies to citrullinated vimentin are a specific and sensitive marker for the diagnosis of rheumatoid arthritis. *Clin Rev Allergy Immunol.* 34(1):4 2008.
- Song JS, Park GB, Park AJ. Comparison of anti-mutated citrullinated vimentin with anti-cyclic citrullinated peptide and rheumatoid factors for the diagnostic value of rheumatoid arthritis [in Korean]. *J Korean Rheum Assoc.* 14(3):235 2007.

- Ursum J, Nielsen MM, van Schaardenburg D, et al. Antibodies to mutated citrullinated vimentin and disease activity score in early arthritis: a cohort study. *Arthritis Res Ther.* 10(1):R12, 2008.
- Besada E, Nikolaisen C, Nossent H. Diagnostic value of antibodies against mutated citrullinated vimentin for rheumatoid arthritis. *Clin Exp Rheumatol.* 29(1):85 2011.

Notice to the user (European Union):

Any serious incident that has occurred in relation to the device shall be reported to the manufacturer and the competent authority of the EU Member State in which the user and/or the patient is established .

Change Control

Former version: *ORG 601_IFU_EN_QM113201_2016-04-18_2*

Reason for revision: *Introduction electronic IFU on homepage*

- 1 Pipet **100 µl** calibrator, control or patient sample
 - Incubate for **30 minutes** at room temperature
 - Discard the contents of the wells and wash 3 times with **300 µl** wash solution
- 2 Pipet **100 µl** enzyme conjugate
 - Incubate for **15 minutes** at room temperature
 - Discard the contents of the wells and wash 3 times with **300 µl** wash solution
- 3 Pipet **100 µl** substrate solution
 - Incubate for **15 minutes** at room temperature
- 4 Add **100 µl** stop solution
 - Leave untouched for **5 minutes**
 - Read at **450 nm**

Anti-LKM-1 ELISA (IgG) Test instruction

ORDER NO.	ANTIBODIES AGAINST	IG CLASS	SUBSTRATE	FORMAT
EA 1321-9601 G	LKM-1	IgG	Ag-coated microplate wells	96 x 01 (96)

Indications: The ELISA test kit provides a semiquantitative or quantitative in vitro assay for human antibodies of the IgG class against liver-kidney microsomes (LKM) in serum or plasma for the diagnosis of inexplainable increase in transaminases, suspected autoimmune hepatitis.

Application: According to the simplified diagnostic criteria by EM Hennes and colleagues (*International Autoimmune Hepatitis Group*) published in 2008, the detection of autoantibodies against LKM belongs to the routine investigations performed to diagnose autoimmune hepatitis. Antibodies against LKM-1 are mostly observed in children, but may be also present in adult patients with AIH. For delimitation from a virus hepatitis, the parallel determination of the other autoantibodies associated with AIH, such as ANA, pANCA, ASMA or antibodies against LC-1 and SLA/LP is recommended.

Principles of the test: The test kit contains microtiter strips each with 8 break-off reagent wells coated with LKM-1. In the first reaction step, diluted patient samples are incubated in the wells. In the case of positive samples, specific IgG antibodies (also IgA and IgM) will bind to the antigens. To detect the bound antibodies, a second incubation is carried out using an enzyme-labelled anti-human IgG (enzyme conjugate) catalysing a colour reaction.

Contents of the test kit:

Component	Colour	Format	Symbol
1. Microplate wells coated with antigens 12 microplate strips each containing 8 individual break-off wells in a frame, ready for use	---	12 x 8	STRIPS
2. Calibrator 1 200 RU/ml (IgG, human), ready for use	dark red	1 x 2.0 ml	CAL 1
3. Calibrator 2 20 RU/ml (IgG, human), ready for use	red	1 x 2.0 ml	CAL 2
4. Calibrator 3 2 RU/ml (IgG, human), ready for use	light red	1 x 2.0 ml	CAL 3
5. Positive control (IgG, human), ready for use	blue	1 x 2.0 ml	POS CONTROL
6. Negative control (IgG, human), ready for use	green	1 x 2.0 ml	NEG CONTROL
7. Enzyme conjugate peroxidase-labelled anti-human IgG (rabbit), ready for use	green	1 x 12 ml	CONJUGATE
8. Sample buffer ready for use	light blue	1 x 100 ml	SAMPLE BUFFER
9. Wash buffer 10x concentrate	colourless	1 x 100 ml	WASH BUFFER 10x
10. Chromogen/substrate solution TMB/H ₂ O ₂ , ready for use	colourless	1 x 12 ml	SUBSTRATE
11. Stop solution 0.5 M sulphuric acid, ready for use	colourless	1 x 12 ml	STOP SOLUTION
12. Test instruction	---	1 booklet	
13. Quality control certificate	---	1 protocol	

LOT Lot description

IVD In vitro diagnostic medical device




Storage temperature

Unopened usable until



Preparation and stability of the reagents

Note: All reagents must be brought to room temperature (+18°C to +25°C) approx. 30 minutes before use. After first use, the reagents are stable until the indicated expiry date if stored at +2°C to +8°C and protected from contamination, unless stated otherwise below.

- **Coated wells:** Ready for use. Tear open the resealable protective wrapping of the microplate at the recesses above the grip seam. Do not open until the microplate has reached room temperature to prevent the individual strips from moistening. Immediately replace the remaining wells of a partly used microplate in the protective wrapping and tightly seal with the integrated grip seam (Do not remove the desiccant bag).
Once the protective wrapping has been opened for the first time, the wells coated with antigens can be stored in a dry place and at a temperature between +2°C and +8°C for 4 months.
- **Calibrators and controls:** Ready for use. The reagents must be mixed thoroughly before use.
- **Enzyme conjugate:** Ready for use. The enzyme conjugate must be mixed thoroughly before use.
- **Sample buffer:** Ready for use.
- **Wash buffer:** The wash buffer is a 10x concentrate. If crystallisation occurs in the concentrated buffer, warm it to 37°C and mix well before diluting. The quantity required should be removed from the bottle using a clean pipette and diluted with deionised or distilled water (1 part reagent plus 9 parts distilled water).
For example: For 1 microplate strip, 5 ml concentrate plus 45 ml water.
The working strength wash buffer is stable for 4 weeks when stored at +2°C to +8°C and handled properly.
- **Chromogen/substrate solution:** Ready for use. Close the bottle immediately after use, as the contents are sensitive to light . The chromogen/substrate solution must be clear on use. Do not use the solution if it is blue coloured.
- **Stop solution:** Ready for use.

Storage and stability: The test kit has to be stored at a temperature between +2°C to +8°C. Do not freeze. Unopened, all test kit components are stable until the indicated expiry date.

Waste disposal: Patient samples, calibrators, controls and incubated microplate strips should be handled as infectious waste. All reagents must be disposed of in accordance with local disposal regulations.

Warning: The calibrators and controls of human origin have tested negative for HBsAg, anti-HCV, anti-HIV-1 and anti-HIV-2. Nonetheless, all materials should be treated as being a potential infection hazard and should be handled with care. Some of the reagents contain the agent sodium azide in a non-declarable concentration. Avoid skin contact.

Preparation and stability of the patient samples

Samples: Human serum or EDTA, heparin or citrate plasma.

Stability: Patient samples to be investigated can generally be stored at +2°C to +8°C for up to 14 days. Diluted samples should be incubated within one working day.

Sample dilution: Patient samples are diluted **1:101** in sample buffer. For example: dilute 10 µl of sample in 1.0 ml sample buffer and mix well by vortexing (sample pipettes are not suitable for mixing).

NOTE: Calibrators and controls are prediluted and ready for use, do not dilute them.



Incubation

For **semiquantitative analysis** incubate **calibrator 2** along with the positive and negative controls and patient samples. For **quantitative analysis** incubate **calibrators 1, 2 and 3** along with the positive and negative controls and patient samples.

(Partly) manual test performance

Sample incubation: (1st step) Transfer 100 µl of the calibrators, positive and negative controls or diluted patient samples into the individual microplate wells according to the pipetting protocol. Incubate for **30 minutes** at room temperature (+18°C to +25°C).

Washing: Manual: Empty the wells and subsequently wash 3 times using 300 µl of working strength wash buffer for each wash.
Automatic: Wash reagent wells 3 times with 450 µl of working strength wash buffer (program setting: e.g. TECAN Columbus Washer "Overflow Modus").

Leave the wash buffer in each well for 30 to 60 seconds per washing cycle, then empty the wells. After washing (manual and automated tests), thoroughly dispose of all liquid from the microplate by tapping it on absorbent paper with the openings facing downwards to remove all residual wash buffer.

Note: Residual liquid (> 10 µl) remaining in the reagent wells after washing can interfere with the substrate and lead to false low extinction values. Insufficient washing (e.g., less than 3 wash cycles, too small wash buffer volumes, or too short residence times) can lead to false high extinction values.

Free positions on the microplate strip should be filled with blank wells of the same plate format as that of the parameter to be investigated.

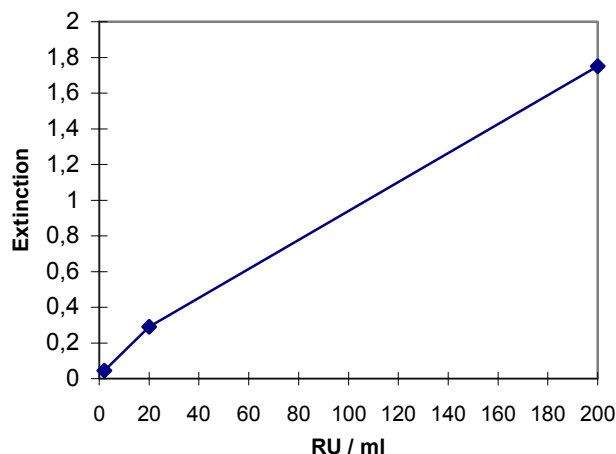
Conjugate incubation: (2nd step) Pipette 100 µl of enzyme conjugate (peroxidase-labelled anti-human IgG) into each of the microplate wells. Incubate for **30 minutes** at room temperature (+18°C to +25°C).

Washing: Empty the wells. Wash as described above.

Substrate incubation: (3rd step) Pipette 100 µl of chromogen/substrate solution into each of the microplate wells. Incubate for **15 minutes** at room temperature (+18°C to +25°C), protect from direct sunlight.

Stopping the reaction: Pipette 100 µl of stop solution into each of the microplate wells in the same order and at the same speed as the chromogen/substrate solution was introduced.

Measurement: **Photometric measurement** of the colour intensity should be made at a **wavelength of 450 nm** and a reference wavelength between 620 nm and 650 nm **within 30 minutes of adding the stop solution**. Prior to measuring, slightly shake the microplate to ensure a homogeneous distribution of the solution.



If the extinction for a patient sample lies above the value of calibrator 1 (200 RU/ml), the result should be reported as ">200 RU/ml". It is recommended that the sample be re-tested at a dilution of e.g. 1:400. The result in RU/ml read from the calibration curve for this sample must then be multiplied by a factor of 4.

The upper limit of the normal range (**cut-off**) recommended by EUROIMMUN is 20 relative units (RU)/ml. EUROIMMUN recommends interpreting results as follows:

<20 RU/ml:	negative
≥20 RU/ml:	positive

For duplicate determinations the mean of the two values should be taken. If the two values deviate substantially from one another, EUROIMMUN recommends to retest the samples.

For diagnosis, the clinical picture of the patient always needs to be taken into account along with the serological findings.

Test characteristics

Calibration: As no international reference serum exists for antibodies against LKM-1, the calibration is performed in relative units (RU).

For every group of tests performed, the extinction values of the calibrators and the relative units and/or ratio determined for the positive and negative controls must lie within the limits stated for the relevant test kit lot. A quality control certificate containing these reference values is included. If the values specified for the controls are not achieved, the test results may be inaccurate and the test should be repeated.

The binding activity of the antibodies and the activity of the enzyme used are temperature-dependent. It is therefore recommended using a thermostat in all three incubation steps. The higher the room temperature during the incubation steps, the greater will be the extinction values. Corresponding variations apply also to the incubation times. However, the calibrators are subject to the same influences, with the result that such variations will be largely compensated in the calculation of the result.

Antigen: The reagent wells are coated with recombinant cytochrome P450 IID6 which constitutes the specific target antigen for antibodies against LKM1.

Linearity: The linearity of the Anti-LKM-1 ELISA (IgG) was determined by assaying 4 serial dilutions of different patient samples. The coefficient of determination R^2 for all sera was > 0.95. The Anti-LKM-1 ELISA (IgG) is linear at least in the tested concentration range (2 RU/ml to 194 RU/ml).



Detection limit: The lower detection limit is defined as the mean value of an analyte-free sample plus three times the standard deviation and is the smallest detectable antibody titer. The lower detection limit of the Anti-LKM-1 ELISA (IgG) is 1.4 RU/ml.

Cross reactivity: This ELISA showed no cross reactivity.

Interference: Haemolytic, lipaemic and icteric samples showed no influences on the result up to a concentration of 10 mg/ml for haemoglobin, 20 mg/ml for triglycerides and 0.4 mg/ml for bilirubin in this ELISA.

Reproducibility: The reproducibility of the test was investigated by determining the intra- and inter-assay coefficients of variation (CV) using 3 sera. The intra-assay CVs are based on 20 determinations and the inter-assay CVs on 4 determinations performed in 6 different test runs.

<i>Intra-Assay Variation, n = 20</i>		
Serum	Mean value (RU/ml)	CV (%)
1	55	3.0
2	96	2.7
3	158	2.3

<i>Inter-Assay Variation, n = 4 x 6</i>		
Serum	Mean value (RU/ml)	CV (%)
1	58	3.2
2	96	3.7
3	160	2.5

Specificity and sensitivity: 18 patient samples suffering from autoimmune hepatitis and 489 patient samples from a reference laboratory were investigated with the EUROIMMUN Anti-LKM-1 ELISA (IgG). The EUROIMMUN-IIFT (IgG) was used as a reference method. The ELISA has a specificity of 99.4% and a sensitivity of 100% with reference to the EUROIMMUN IIFT.

Serum panel (n = 507)		IIFT (rat liver/rat kidney)	
		positive	negative
Anti-LKM-1 ELISA	positive	27	3
	negative	0	477

A patient sample which reacted positive in ELISA and negative in IIFT belongs to a patient with characterised AIH.

Reference range: The levels of the anti-LKM-1 antibodies (IgG) were analysed with this EUROIMMUN ELISA in a panel of 200 healthy blood donors. With a cut-off of 20 RU/ml, 0.5% of the blood donors were anti-LKM-1 positive.

Clinical significance

In Western Europe the incidence of AIH is 1.9 cases per 100,000 inhabitants per year. Untreated, AIH soon develops into liver cirrhosis. However, if low-dose immunosuppressive therapy is started early enough and continued lifelong, patients have a normal life expectancy.

Circulating autoantibodies have come to play a significant role in the diagnosis of AIH. Antibodies against the following antigens are associated with AIH: soluble liver antigen/liver-pancreas antigen (SLA/LP), cell nuclei (ANA), nDNA, smooth muscles (SMA, the most important target antigen being F actin), liver-kidney microsomes (LKM-1, target antigen: cytochrome P450 IID6), liver cytosolic antigen type 1 (LC-1, target antigen: formiminotransferase cyclo-deaminase) and granulocytes (pANCA). Anti-mitochondrial antibodies (AMA) are also investigated in this context to exclude the possibility of primary biliary cirrhosis (PBC). AIH is sometimes classified according to the antibody status, i.e., subtype I (ANA, SMA), subtype II (antibodies against LKM-1 and LC-1), or subtype III (antibodies against SLA/LP). However, this classification is probably neither clinically nor therapeutically or prognostically relevant, since 10 to 20% of patients with PBC develop secondary AIH (overlap). In these cases the same autoantibodies as in AIH are frequently detected.



Autoantibodies against LKM-1 (LKM-1, antigen: cytochrome P450 IID6) are present in 1% of adults with AIH. In children they are more common. Antibodies against LKM-1 are also found in 1 to 2% of patients with hepatitis C-positive serology.

The highest diagnostic accuracy currently available for AIH is probably provided by the various EUROIMMUN enzyme immunoassays that detect autoantibodies against SLA/LP. Although SLA/LP autoantibodies have a prevalence of only 10 to 30% in AIH patients, the predictive value is nearly 100%. Every positive anti-SLA/LP result essentially indicates AIH (provided the relevant clinical symptoms are also present).

Literature references

1. Berg PA, Stechemesser E, Strienz J. **Hypergammaglobulinämische chronisch aktive Hepatitis mit Nachweis von Leber-Pankreas-spezifischen komplementbindenden Autoantikörpern.** Verhandlungen Deutsche Gesellschaft für Innere Medizin 87: 921-927 (1981).
2. Boberg KM, Aadland E, Jahnsen J, Raknerud N, Stiris M, Bell H. **Incidence and prevalence of primary biliary cirrhosis, primary sclerosing cholangitis, and autoimmune hepatitis in a Norwegian population.** Scandinavian Journal of Gastroenterology 33: 99-103 (1998).
3. Czaja AJ, Manns MP, Homburger HA. **Frequency and significance of antibodies to liver/kidney microsome type 1 in adults with chronic active hepatitis.** Gastroenterology 103: 1290-1295 (1992).
4. Kanzler S, Weidemann C, Gerken G, Löhr HF, Galle PR, Meyer zum Büschenfelde K-H, Lohse AW. **Clinical significance of autoantibodies to soluble liver antigen in autoimmune hepatitis.** Journal of Hepatology 31: 635-640 (1999).
5. Kanzler S, Löhr HF, Gerken G, Galle PR, Lohse AW. **Long-term management and prognosis of autoimmune hepatitis (AIH): A single center experience.** Zeitschrift für Gastroenterologie 39: 339-348 (2001).
6. Krawitt EL. **Autoimmune hepatitis.** New England Journal of Medicine 334: 897-903 (1996).
7. Lohse AW, Gerken G, Mohr H, Löhr HF, Treichel U, Dienes HP, et al. **Relation between autoimmune liver diseases and viral hepatitis: Clinical and serological characteristics in 859 patients.** Zeitschrift für Gastroenterologie 33: 571-578 (1995).
8. Lohse AW. **Autoimmune liver disease.** In: Gastroenterology and Hepatology (Hrsg: G. Bianchi Porro), Maidenhead, England: 499-509 (1999).
9. Ma Y, Peakman M, Lobo-Yeo A, Wen L, Lenzi M, Gaken J, Farzaneh F, Mieli-Vergani G, Bianchi FB, Vergani D. **Differences in immune recognition of cytochrome P450 IID6 by liver kidney microsomal (LKM) antibody in autoimmune hepatitis and chronic hepatitis C virus infection.** Clinical and Experimental Immunology 97: 94-99 (1994).
10. Manns MP, Johnson EF, Griffin KJ, Tan EM, Sullivan KF. **Major antigen of liver kidney microsomal autoantibodies in idiopathic autoimmune hepatitis is cytochrome P450 db1.** Journal of Clinical Investigation 83: 1066-1072 (1989).
11. Manns MP, Gerken G, Kyriatsoulis A, Staritz M, Meyer zum Büschenfelde K-H. **Characterisation of a new subgroup of autoimmune chronic active hepatitis by autoantibodies against a soluble liver antigen.** Lancet i: 292-294 (1987).
12. McFarlane IG. **The relationship between autoimmune markers and different clinical syndromes in autoimmune hepatitis.** Gut 42: 599-602 (1998).
13. Meyer zum Büschenfelde KH, Lohse AW. **Autoimmune hepatitis.** New England Journal of Medicine 333: 1004-1005 (1995).
14. Obermayer-Straub P, Strassburg CP, Manns MP. **Autoimmune hepatitis.** Journal of Hepatology 32 (1 Suppl.): 181-197 (2000).

15. Schramm C, Kanzler S, Meyer zum Büschenfelde K-H, Galle PR, Lohse AW. **Autoimmune hepatitis in the elderly**. American Journal of Gastroenterology 96: 99-103 (1998)
16. Seelig R, Renz M, Bünger G, Schröter H, Seelig HP. **Anti-LKM-1 antibodies determined by use of recombinant P450 IID6 in ELISA and western blot and their association with anti-HCV and HCV-RNA**. Clinical and Experimental Immunology 92: 373-380 (1993).
17. Stechemesser E, Strienz J, Berg PA. **Serological definition of new subgroup of patients with autoimmune chronic active hepatitis (letter)**. Lancet i: 683 (1987).
18. Vergani D, Mieli-Vergani G. **Type II autoimmune hepatitis: the conundrum of cytochrome P450 IID6**. Clinical and Experimental Immunology 92: 367-368 (1993).
19. Wies I, Denzer U, Brunner S, Meyer zum Büschenfelde K-H, Manns MP, Arand M, et al. **Neither cytokeratins nor glutathione-S-transferase is major target antigen of autoantibodies to soluble liver antigen (SLA) in autoimmune hepatitis (abstract)**. Hepatology 548A (1998).
20. Wies I, Brunner S, Henninger J, Herkel J, Kanzler S, Meyer zum Büschenfelde K-H, Lohse AW. **Identification of target antigen for SLA/LP autoantibodies K-H, in autoimmune hepatitis**. Lancet 355: 1510-1515 (2000).

ORGENTEC Diagnostika GmbH

Carl-Zeiss-Straße 49-51


55129 Mainz - Germany

Phone: +49 (0) 61 31 / 92 58-0

Fax: +49 (0) 61 31 / 92 58-58

Internet: www.orgentec.com



 **518_3**





























ORG 518 Anti-PR3 (cANCA)

INTENDED PURPOSE

Anti-PR3 is an ELISA test system for the quantitative measurement of IgG class autoantibodies against proteinase 3 (PR3) in human serum or plasma. This product is intended for professional in vitro diagnostic use only.

Anti-neutrophil cytoplasmic antibodies (ANCA) are diagnostic markers for ANCA-associated vasculitides. Anti-PR3 characterises granulomatosis with polyangiitis (GPA, formerly: Wegener's granulomatosis). The test supports the differential diagnosis of vasculitis when used in combination with other laboratory and clinical findings.

SYMBOLS USED ON LABELS

	In vitro diagnostic medical device		Microplate
	Manufacturer		Calibrator
	Catalogue number		Calibrator
	Sufficient for 96 determinations		Calibrator
	Batch code		Calibrator
	Use by		Calibrator
	Temperature limitation		Calibrator
	Keep away from sunlight		Control positive
	Do not reuse		Control negative
	Date of manufacture		Sample Buffer P
	CE marked according to 98/79/EC		Enzyme Conjugate
	Consult instructions for use		TMB Substrate
	Electronic Instruction For Use: version		Stop solution
			Wash Buffer
			Ready to use

PRINCIPLE OF THE TEST

Highly purified Proteinase 3 (PR3) is bound to microwells.

The determination is based on an indirect enzyme linked immune reaction with the following steps:
Specific antibodies in the patient sample bind to the antigen coated on the surface of the reaction wells. After incubation, a washing step removes unbound and unspecifically bound serum or plasma components. Subsequently added enzyme conjugate binds to the immobilized antibody-antigen-complexes. After incubation, a second washing step removes unbound enzyme conjugate. After addition of substrate solution the bound enzyme conjugate hydrolyses the substrate forming a blue coloured product. Addition of an acid stops the reaction generating a yellow end-product. The intensity of the yellow color correlates with the concentration of the antibody-antigen-complex and can be measured photometrically at 450 nm.

WARNINGS AND PRECAUTIONS



- All reagents of this kit are intended for professional in vitro diagnostic use only.
- Components containing human serum were tested and found negative for HBsAg, HCV, HIV1 and HIV2 by FDA approved methods. No test can guarantee the absence of HBsAg, HCV, HIV1 or HIV2, and so all human serum based reagents in this kit must be handled as though capable of transmitting infection.
- Bovine serum albumin (BSA) used in components has been tested for BSE and found negative.
- Avoid contact with the substrate TMB (3,3',5,5'-Tetramethyl-benzidine).
- Stop solution contains acid, classification is non-hazardous. Avoid contact with skin.
- Control, sample buffer and wash buffer contain sodium azide 0.09% as preservative. This concentration is classified as non-hazardous.
- Enzyme conjugate contains ProClin 300 0.05% as preservative. This concentration is classified as non-hazardous.

During handling of all reagents, controls and serum samples observe the existing regulations for laboratory safety regulations and good laboratory practice:

- First aid measures: In case of skin contact, immediately wash thoroughly with water and soap. Remove contaminated clothing and shoes and wash before reuse. If system fluid comes into contact with skin, wash thoroughly with water. After contact with the eyes carefully rinse the opened eye with running water for at least 10 minutes. Get medical attention if necessary.
- Personal precautions, protective equipment and emergency procedures:
Observe laboratory safety regulations. Avoid contact with skin and eyes. Do not swallow. Do not pipette by mouth. Do not eat, drink, smoke or apply makeup in areas where specimens or kit reagents are handled. When spilled, absorb with an inert material and put the spilled material in an appropriate waste disposal.
- Exposure controls / personal protection: Wear protective gloves of nitril rubber or natural latex. Wear protective glasses. Used according to intended use no dangerous reactions known.
- Conditions to avoid: Since substrate solution is light-sensitive. Store in the dark.
- For disposal of laboratory waste the national or regional legislation has to be observed.

Observe the guidelines for performing quality control in medical laboratories by assaying control sera.

CONTENTS OF THE KIT

ORG 518		Sufficient for 96 determinations
MICROPLATE	1	One divisible microplate consisting of 12 modules of 8 wells each. Ready to use. Product code on module: PR3
CALIBRATOR A	1x 1.5 ml	Calibrator A 0 U/ml, containing serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
CALIBRATOR B	1x 1.5 ml	Calibrator B 5 U/ml, containing PR3 antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
CALIBRATOR C	1x 1.5 ml	Calibrator C 10 U/ml, containing PR3 antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
CALIBRATOR D	1x 1.5 ml	Calibrator D 20 U/ml, containing PR3 antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
CALIBRATOR E	1x 1.5 ml	Calibrator E 40 U/ml, containing PR3 antibodies in a serum/buffer matrix (PBS, BSA, NaN3 0.09%), yellow. Ready to use.
CALIBRATOR F	1x 1.5 ml	Calibrator F 100 U/ml, containing PR3 antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
CONTROL +	1x 1.5 ml	Control positive, containing PR3 antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use. The concentration is specified on the certificate of analysis.
CONTROL -	1x 1.5 ml	Control negative, containing PR3 antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use. The concentration is specified on the certificate of analysis.
DILUENT	20 ml	Sample Buffer P, containing PBS, BSA, detergent, preservative sodium azide 0.09%, yellow, concentrate (5 x).
CONJUGATE	15 ml	Enzyme Conjugate containing anti-human IgG antibodies, HRP labelled; PBS, BSA, detergent, preservative PROCLIN 0.05%, light red. Ready to use.
TMB	15 ml	TMB Substrate; containing 3,3', 5,5'- Tetramethylbenzidin, colorless. Ready to use.
STOP	15 ml	Stop solution; contains acid. Ready to use.
WASH	20 ml	Wash Buffer, containing Tris, detergent, preservative sodium azide 0.09%; 50 x conc.
	1	Certificate of Analysis

MATERIALS REQUIRED

- Microplate reader capable of endpoint measurements at 450 nm; optional: reference filter at 620 nm
- Data reduction software
- Multi-channel dispenser or repeatable pipette for 100 µl
- Vortex mixer
- Pipettes for 10 µl, 100 µl and 1000 µl
- Laboratory timing device
- Distilled or deionised water
- Measuring cylinder for 1000 ml and 100 ml
- Plastic container for storage of the wash solution

This ELISA assay is suitable for use on open automated ELISA processors. Each assay has to be validated on the respective automated system. Detailed information is provided upon request.

SPECIMEN COLLECTION, STORAGE AND HANDLING

- Collect whole blood specimens using acceptable medical techniques to avoid hemolysis.
- Allow blood to clot and separate the serum or plasma by centrifugation.
- Test serum should be clear and non-hemolyzed. Contamination by hemolysis or lipemia should be avoided, but does not interfere with this assay.
- Specimens may be refrigerated at 2-8°C for up to five days or stored at -20°C up to six months.
- Avoid repetitive freezing and thawing of serum or plasma samples. This may result in variable loss of antibody activity.
- Testing of heat-inactivated sera is not recommended.

STORAGE AND STABILITY

- Store test kit at 2-8°C in the dark.
- Do not expose reagents to heat, sun, or strong light during storage and usage.
- Store microplate sealed and desiccated in the clip bag provided.
- Shelf life of the unopened test kit is 18 months from day of production.
Unopened reagents are stable until expiration of the kit. See labels for individual batch.
- Diluted Wash Buffer and Sample Buffer are stable for at least 30 days when stored at 2-8°C.
We recommend consumption on the same day.

PROCEDURAL NOTES

- Do not use kit components beyond their expiration dates.
- Do not interchange kit components from different lots and products.
- All materials must be at room temperature (20-28°C) prior to use.
- Prepare all reagents and samples. Once started, perform the test without interruption.
- Double determinations may be done. By this means pipetting errors may become obvious.
- Perform the assay steps only in the order indicated.
- Always use fresh sample dilutions.
- Pipette all reagents and samples into the bottom of the wells.
- To avoid carryover or contamination, change the pipette tip between samples and different kit controls.
- Wash microwells thoroughly and remove the last droplets of wash buffer.
- All incubation steps must be accurately timed.
- Do not re-use microplate wells.

PREPARATION OF REAGENTS

WASH
Dilute the contents of one vial of the buffered wash solution concentrate (50x) with distilled or deionised water to a final volume of 1000 ml prior to use.

DILUENT
Sample Buffer P: Prior to use dilute the contents (20 ml) of one vial of sample buffer 5x concentrate with distilled or deionised water to a final volume of 100 ml.

Preparation of samples

Dilute patient samples 1:100 before the assay: Put 990 µl of prediluted sample buffer in a polystyrene tube and add 10 µl of sample. Mix well. Note: Calibrators / Controls are ready to use and need not be diluted.

TEST PROCEDURE

Prepare enough microplate modules for all calibrators / controls and patient samples.

- Pipette **100 µl** of calibrators, controls and prediluted patient samples into the wells.
Incubate for **30 minutes** at room temperature (20-28 °C).
Discard the contents of the microwells and **wash 3 times** with **300 µl** of wash solution.
- Dispense **100 µl** of enzyme conjugate into each well.
Incubate for **15 minutes** at room temperature.
Discard the contents of the microwells and **wash 3 times** with **300 µl** of wash solution.
- Dispense **100 µl** of TMB substrate solution into each well.
Incubate for **15 minutes** at room temperature.
- Add 100 µl** of stop solution to each well of the modules
Incubate for **5 minutes** at room temperature.
Read the optical density at 450 nm (reference 600-690nm) and calculate the results.
The developed colour is stable for at least 30 minutes. Read during this time.

Example for a pipetting scheme:

	1	2	3	4	5	6	7	8	9	10	11	12
A	A	P1										
B	B	P2										
C	C	P3										
D	D											
E	E											
F	F											
G	C+											
H	C-											

P1, ... patient sample A-F calibrators C+, C- controls

VALIDATION

Test results are valid if the optical densities at 450 nm for calibrators / controls and the results for controls comply with the reference ranges indicated on the Certificate of Analysis enclosed in each test kit.
If these quality control criteria are not met the assay run is invalid and should be repeated.

CALCULATION OF RESULTS

For quantitative results plot the optical density of each calibrator versus the calibrator concentration to create a calibration curve. The concentration of patient samples may then be estimated from the calibration curve by interpolation.

Using data reduction software a 4-Parameter-Fit with lin-log coordinates for optical density and concentration is the data reduction method of choice.

PERFORMANCE CHARACTERISTICS

Calibration

This assay system is calibrated in relative arbitrary units, since no international reference preparation is available for this assay.

Measuring range

The calculation range of this ELISA assay is 0 - 100 U/ml

Expected values

In a normal range study with samples from healthy blood donors the following ranges have been established with this ELISA assay: Cut-off 5 U/ml

Interpretation of results

Negative: < 5 U/ml
Positive: ≥ 5 U/ml

Linearity

Patient samples containing high levels of specific antibody were serially diluted in sample buffer to demonstrate the dynamic range of the assay and the upper / lower end of linearity. Activity for each dilution was calculated from the calibration curve using a 4-Parameter-Fit with lin-log coordinates.

Sample	Dilution	Observed U/ml	Expected U/ml	O/E [%]
1	1:100	78.9	78.9	100
.	1:200	39.8	39.5	101
.	1:400	20.6	19.7	105
.	1:800	10.6	9.9	107
.	1:1600	5.3	4.9	108
2	1:100	77.5	77.5	100
.	1:200	37.4	38.8	96
.	1:400	19.1	19.4	98
.	1:800	9.7	9.7	100
.	1:1600	5.0	4.8	104

Limit of detection

Functional sensitivity was determined to be: 0.5 U/ml

Reproducibility

Intra-assay precision: Coefficient of variation (CV) was calculated for each of three samples from the results of 24 determinations in a single run. Results for precision-within-assay are shown in the table below.

Inter-assay precision: Coefficient of variation (CV) was calculated for each of three samples from the results of 6 determinations in 5 different runs. Results for run-to-run precision are shown in the table below.

Intra-Assay		
Sample	Mean U/ml	CV %
1	10.9	4.7
2	24.6	2.8
3	58.5	2.8

Inter-Assay		
Sample	Mean U/ml	CV %
1	10.4	6.2
2	23.4	8.8
3	60.7	3.9

Interfering substances

No interference has been observed with haemolytic (up to 1000 mg/dl) or lipemic (up to 3 g/dl triglycerides) sera or plasma, or bilirubin (up to 40 mg/dl) containing sera or plasma. Nor have any interfering effects been observed with the use of anticoagulants (Citrate, EDTA, Heparine). However for practical reasons it is recommended that grossly hemolyzed or lipemic samples should be avoided.

Study results

Study population	n	n Pos	%
Morbus Wegener (c-ANCA pos, vasculitis (pANCA-positive)	61	52	85.2
infammatory/Non-inflammatory	20	0	0.0
Normal human sera	150	3	2.0
	80	0	0.0

		Immunological Diagnosis		
		POS	NEG	
ORG 518	POS	52	3	
	NEG	9	247	
		61	250	311

Sensitivity: 85.2 %

Specificity: 98.8 %

Overall agreement: 96.1 %

LIMITATIONS OF THE PROCEDURE

This assay is a diagnostic aid. A definite clinical diagnosis should not be based on the results of a single test, but should be made by the physician after all clinical and laboratory findings have been evaluated concerning the entire clinical picture of the patient. Also every decision for therapy should be taken individually.

The above pathological and normal reference ranges for antibodies in patient samples should be regarded as recommendations only. Each laboratory should establish its own ranges according to ISO 15189 or other applicable laboratory guidelines.

REFERENCES

1. Jennette, J. C. and Falk, R.J . Antineutrophil Cytoplasmic Autoantibodies and Associated Diseases: a Review. Am. J. Kidney Dis. 1990, Vol. XV, No. 6: 517 - 529.
2. Gross, W. L. et al. Antineutrophil Cytoplasmic Autoantibody-Associated Diseases: A Rheumatologist's Perspective. Am. J. Kidney Dis. 1991, Vol. XVIII, No. 2: 175 - 179.
3. Wieslander, J. How are Antineutrophil Cytoplasmic Autoantibodies Detected ? Am. J. Kidney Dis. 1991, Vol. XVIII, No. 2: 154 - 158.
4. Lesavre, P. Antineutrophil cytoplasmic antibodies antigen specificity. Am. J. Kidney Dis. 1991,Vol. XVIII,No. 2: 159 - 163.
5. Hagen, E. C. et al. Antineutrophil cytoplasmic autoantibodies: a review of the antigens involved, the assays, and the clinical and possible pathogenic consequences. Blood 1993, Vol.81: 1996 - 2000.
6. Gross, W .L. et al. Immunodiagnostische und immunopathogenetische Bedeutung von Anti-Neutrophilen-Cytoplasma-Antikörpern. Deutsche Medizinische Wochenschrift 1993, Vol. 118: 191 - 199.

Notice to the user (European Union):

Any serious incident that has occurred in relation to the device shall be reported to the manufacturer and the competent authority of the EU Member State in which the user and/or the patient is established .

Change Control

Former version: *ORG 518_IFU_EN_QM113147_2013-12-16_1.2* Reason for revision: *Introduction electronic IFU on homepage*

- 1** Pipet **100 µl** calibrator, control or patient sample
→ Incubate for **30 minutes** at room temperature
→ Discard the contents of the wells and wash 3 times with **300 µl** wash solution
- 2** Pipet **100 µl** enzyme conjugate
→ Incubate for **15 minutes** at room temperature
→ Discard the contents of the wells and wash 3 times with **300 µl** wash solution
- 3** Pipet **100 µl** substrate solution
→ Incubate for **15 minutes** at room temperature
- 4** Add **100 µl** stop solution
→ Leave untouched for **5 minutes**
→ Read at **450 nm**

ORGENTEC Diagnostika GmbH


Carl-Zeiss-Straße 49-51

55129 Mainz - Germany

Phone: +49 (0) 61 31 / 92 58-0

Fax: +49 (0) 61 31 / 92 58-58

Internet: www.orgentec.com



ORG 519 Anti-MPO (pANCA)

INTENDED PURPOSE

Anti-MPO is an ELISA test system for the quantitative measurement of IgG class autoantibodies against myeloperoxidase (MPO) in human serum or plasma. This product is intended for professional in vitro diagnostic use only.

Anti-neutrophil cytoplasmic antibodies (ANCA) are diagnostic markers for ANCA-associated vasculitides. Anti-MPO differentiates microscopic polyangiitis (MPA) and eosinophilic granulomatosis with polyangiitis (EGPA) The test supports differential diagnosis of vasculitis, when used in conjunction with other clinical and laboratory findings.

SYMBOLS USED ON LABELS

	In vitro diagnostic medical device		Microplate
	Manufacturer		Calibrator
	Catalogue number		Calibrator
	Sufficient for 96 determinations		Calibrator
	Batch code		Calibrator
	Use by		Calibrator
	Temperature limitation		Calibrator
	Keep away from sunlight		Control positive
	Do not reuse		Control negative
	Date of manufacture		Sample Buffer P
	CE marked according to 98/79/EC		Enzyme Conjugate
	Consult instructions for use		TMB Substrate
	Electronic Instruction For Use: version		Stop solution
			Wash Buffer
			Ready to use

PRINCIPLE OF THE TEST

Highly purified myeloperoxidase (MPO) is bound to microwells.

The determination is based on an indirect enzyme linked immune reaction with the following steps: Specific antibodies in the patient sample bind to the antigen coated on the surface of the reaction wells. After incubation, a washing step removes unbound and unspecifically bound serum or plasma components. Subsequently added enzyme conjugate binds to the immobilized antibody-antigen-complexes. After incubation, a second washing step removes unbound enzyme conjugate. After addition of substrate solution the bound enzyme conjugate hydrolyses the substrate forming a blue coloured product. Addition of an acid stops the reaction generating a yellow end-product. The intensity of the yellow color correlates with the concentration of the antibody-antigen-complex and can be measured photometrically at 450 nm.



WARNINGS AND PRECAUTIONS

- All reagents of this kit are intended for professional in vitro diagnostic use only.
- Components containing human serum were tested and found negative for HBsAg, HCV, HIV1 and HIV2 by FDA approved methods. No test can guarantee the absence of HBsAg, HCV, HIV1 or HIV2, and so all human serum based reagents in this kit must be handled as though capable of transmitting infection.
- Bovine serum albumin (BSA) used in components has been tested for BSE and found negative.
- Avoid contact with the substrate TMB (3,3',5,5'-Tetramethyl-benzidine).
- Stop solution contains acid, classification is non-hazardous. Avoid contact with skin.
- Control, sample buffer and wash buffer contain sodium azide 0.09% as preservative. This concentration is classified as non-hazardous.
- Enzyme conjugate contains ProClin 300 0.05% as preservative. This concentration is classified as non-hazardous.

During handling of all reagents, controls and serum samples observe the existing regulations for laboratory safety regulations and good laboratory practice:

- First aid measures: In case of skin contact, immediately wash thoroughly with water and soap. Remove contaminated clothing and shoes and wash before reuse. If system fluid comes into contact with skin, wash thoroughly with water. After contact with the eyes carefully rinse the opened eye with running water for at least 10 minutes. Get medical attention if necessary.
 - Personal precautions, protective equipment and emergency procedures:
Observe laboratory safety regulations. Avoid contact with skin and eyes. Do not swallow. Do not pipette by mouth. Do not eat, drink, smoke or apply makeup in areas where specimens or kit reagents are handled. When spilled, absorb with an inert material and put the spilled material in an appropriate waste disposal.
 - Exposure controls / personal protection: Wear protective gloves of nitril rubber or natural latex. Wear protective glasses. Used according to intended use no dangerous reactions known.
 - Conditions to avoid: Since substrate solution is light-sensitive. Store in the dark.
 - For disposal of laboratory waste the national or regional legislation has to be observed.
- Observe the guidelines for performing quality control in medical laboratories by assaying control sera.

CONTENTS OF THE KIT

ORG 519		Sufficient for 96 determinations
MICROPLATE	1	One divisible microplate consisting of 12 modules of 8 wells each. Ready to use. Product code on module: MPO
CALIBRATOR A	1x 1.5 ml	Calibrator A 0 U/ml, containing serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
CALIBRATOR B	1x 1.5 ml	Calibrator B 5 U/ml, containing MPO antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
CALIBRATOR C	1x 1.5 ml	Calibrator C 10 U/ml, containing MPO antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
CALIBRATOR D	1x 1.5 ml	Calibrator D 20 U/ml, containing MPO antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
CALIBRATOR E	1x 1.5 ml	Calibrator E 40 U/ml, containing MPO antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
CALIBRATOR F	1x 1.5 ml	Calibrator F 100 U/ml, containing MPO antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
CONTROL +	1x 1.5 ml	Control positive, containing MPO antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use. The concentration is specified on the certificate of analysis.
CONTROL -	1x 1.5 ml	Control negative, containing MPO antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use. The concentration is specified on the certificate of analysis.
DILUENT	20 ml	Sample Buffer P, containing PBS, BSA, detergent, preservative sodium azide 0.09%, yellow, concentrate (5 x).
CONJUGATE	15 ml	Enzyme Conjugate containing anti-human IgG antibodies, HRP labelled; PBS, BSA, detergent, preservative PROCLIN 0.05%, light red. Ready to use.
TMB	15 ml	TMB Substrate; containing 3,3', 5,5'- Tetramethylbenzidin, colorless. Ready to use.
STOP	15 ml	Stop solution; contains acid. Ready to use.
WASH	20 ml	Wash Buffer, containing Tris, detergent, preservative sodium azide 0.09%; 50 x conc.
	1	Certificate of Analysis

MATERIALS REQUIRED

- Microplate reader capable of endpoint measurements at 450 nm; optional: reference filter at 620 nm
- Data reduction software
- Multi-channel dispenser or repeatable pipette for 100 µl
- Vortex mixer
- Pipettes for 10 µl, 100 µl and 1000 µl
- Laboratory timing device
- Distilled or deionised water
- Measuring cylinder for 1000 ml and 100 ml
- Plastic container for storage of the wash solution

This ELISA assay is suitable for use on open automated ELISA processors. Each assay has to be validated on the respective automated system. Detailed information is provided upon request.

SPECIMEN COLLECTION, STORAGE AND HANDLING

- Collect whole blood specimens using acceptable medical techniques to avoid hemolysis.
- Allow blood to clot and separate the serum or plasma by centrifugation.
- Test serum should be clear and non-hemolyzed. Contamination by hemolysis or lipemia should be avoided, but does not interfere with this assay.
- Specimens may be refrigerated at 2-8°C for up to five days or stored at -20°C up to six months.
- Avoid repetitive freezing and thawing of serum or plasma samples. This may result in variable loss of antibody activity.
- Testing of heat-inactivated sera is not recommended.

STORAGE AND STABILITY

- Store test kit at 2-8°C in the dark.
- Do not expose reagents to heat, sun, or strong light during storage and usage.
- Store microplate sealed and desiccated in the clip bag provided.
- Shelf life of the unopened test kit is 18 months from day of production.
Unopened reagents are stable until expiration of the kit. See labels for individual batch.
- Diluted Wash Buffer and Sample Buffer are stable for at least 30 days when stored at 2-8°C.
We recommend consumption on the same day.

PROCEDURAL NOTES

- Do not use kit components beyond their expiration dates.
- Do not interchange kit components from different lots and products.
- All materials must be at room temperature (20-28°C) prior to use.
- Prepare all reagents and samples. Once started, perform the test without interruption.
- Double determinations may be done. By this means pipetting errors may become obvious.
- Perform the assay steps only in the order indicated.
- Always use fresh sample dilutions.
- Pipette all reagents and samples into the bottom of the wells.
- To avoid carryover or contamination, change the pipette tip between samples and different kit controls.
- Wash microwells thoroughly and remove the last droplets of wash buffer.
- All incubation steps must be accurately timed.
- Do not re-use microplate wells.

PREPARATION OF REAGENTS

WASH

Dilute the contents of one vial of the buffered wash solution concentrate (50x) with distilled or deionised water to a final volume of 1000 ml prior to use.

DILUENT

Sample Buffer P: Prior to use dilute the contents (20 ml) of one vial of sample buffer 5x concentrate with distilled or deionised water to a final volume of 100 ml.

Preparation of samples

Dilute patient samples 1:100 before the assay: Put 990 µl of prediluted sample buffer in a polystyrene tube and add 10 µl of sample. Mix well. Note: Calibrators / Controls are ready to use and need not be diluted.

TEST PROCEDURE

Prepare enough microplate modules for all calibrators / controls and patient samples.

- Pipette **100 µl** of calibrators, controls and prediluted patient samples into the wells.
Incubate for **30 minutes** at room temperature (20-28 °C).
Discard the contents of the microwells and **wash 3 times** with **300 µl** of wash solution.
- Dispense **100 µl** of enzyme conjugate into each well.
Incubate for **15 minutes** at room temperature.
Discard the contents of the microwells and **wash 3 times** with **300 µl** of wash solution.
- Dispense **100 µl** of TMB substrate solution into each well.
Incubate for **15 minutes** at room temperature.
- Add 100 µl** of stop solution to each well of the modules
Incubate for **5 minutes** at room temperature.
Read the optical density at 450 nm (reference 600-690nm) and calculate the results.
The developed colour is stable for at least 30 minutes. Read during this time.

Example for a pipetting scheme:

	1	2	3	4	5	6	7	8	9	10	11	12
A	A	P1										
B	B	P2										
C	C	P3										
D	D											
E	E											
F	F											
G	C+											
H	C-											

P1, ... patient sample A-F calibrators C+, C- controls

VALIDATION

Test results are valid if the optical densities at 450 nm for calibrators / controls and the results for controls comply with the reference ranges indicated on the Certificate of Analysis enclosed in each test kit.
If these quality control criteria are not met the assay run is invalid and should be repeated.

CALCULATION OF RESULTS

For quantitative results plot the optical density of each calibrator versus the calibrator concentration to create a calibration curve. The concentration of patient samples may then be estimated from the calibration curve by interpolation.

Using data reduction software a 4-Parameter-Fit with lin-log coordinates for optical density and concentration is the data reduction method of choice.

PERFORMANCE CHARACTERISTICS

Calibration

This assay system is calibrated in relative arbitrary units, since no international reference preparation is available for this assay.

Measuring range

The calculation range of this ELISA assay is 0 - 100 U/ml

Expected values

In a normal range study with samples from healthy blood donors the following ranges have been established with this ELISA assay: Cut-off 5 U/ml

Interpretation of results

Negative: < 5 U/ml
Positive: ≥ 5 U/ml

Linearity

Patient samples containing high levels of specific antibody were serially diluted in sample buffer to demonstrate the dynamic range of the assay and the upper / lower end of linearity. Activity for each dilution was calculated from the calibration curve using a 4-Parameter-Fit with lin-log coordinates.

Sample	Dilution	Observed U/ml	Expected U/ml	O/E [%]
1	1:100	87.3	87.3	100
.	1:200	44.1	43.7	101
.	1:400	21.5	21.8	99
.	1:800	9.7	10.9	89
.	1:1600	5.0	5.5	91
2	1:100	79.9	79.9	100
.	1:200	39.3	40.0	98
.	1:400	19.0	20.0	95
.	1:800	8.5	10.0	85
.	1:1600	4.3	5.0	86

Limit of detection

Functional sensitivity was determined to be: 0.5 U/ml

Reproducibility

Intra-assay precision: Coefficient of variation (CV) was calculated for each of three samples from the results of 24 determinations in a single run. Results for precision-within-assay are shown in the table below.

Inter-assay precision: Coefficient of variation (CV) was calculated for each of three samples from the results of 6 determinations in 5 different runs. Results for run-to-run precision are shown in the table below.

Intra-Assay		
Sample	Mean U/ml	CV %
1	7.5	6.4
2	30.2	4.1
3	59.9	3.1

Inter-Assay		
Sample	Mean U/ml	CV %
1	7.0	5.0
2	33.8	4.9
3	78.3	6.3

Interfering substances

No interference has been observed with haemolytic (up to 1000 mg/dl) or lipemic (up to 3 g/dl triglycerides) sera or plasma, or bilirubin (up to 40 mg/dl) containing sera or plasma. Nor have any interfering effects been observed with the use of anticoagulants (Citrate, EDTA, Heparine). However for practical reasons it is recommended that grossly hemolyzed or lipemic samples should be avoided.

Study results

Study population	n	n Pos	%
Crescendic glomerulonephritis	55	53	96.4
Morbus Wegener (cANCA pos)	20	1	5.0
Non-ANCA kidney disease	10	1	10.0
Normal human sera	120	3	2.5

		Immunological Diagnosis		
		POS	NEG	
ORG 519	POS	54	5	205
	NEG	1	145	
		55	150	

Sensitivity: 98.2 %

Specificity: 96.7 %

Overall agreement: 97.1 %

LIMITATIONS OF THE PROCEDURE

This assay is a diagnostic aid. A definite clinical diagnosis should not be based on the results of a single test, but should be made by the physician after all clinical and laboratory findings have been evaluated concerning the entire clinical picture of the patient. Also every decision for therapy should be taken individually.

The above pathological and normal reference ranges for antibodies in patient samples should be regarded as recommendations only. Each laboratory should establish its own ranges according to ISO 15189 or other applicable laboratory guidelines.

REFERENCES

1. Jennette, J. C. and Falk, R.J . Antineutrophil Cytoplasmic Autoantibodies and Associated Diseases: a Review. Am. J. Kidney Dis. 1990, Vol. XV, No. 6: 517 - 529.
2. Gross, W. L. et al. Antineutrophil Cytoplasmic Autoantibody-Associated Diseases: A Rheumatologist's Perspective. Am. J. Kidney Dis. 1991, Vol. XVIII, No. 2: 175 - 179.
3. Wieslander, J. How are Antineutrophil Cytoplasmic Autoantibodies Detected ? Am. J. Kidney Dis. 1991, Vol. XVIII, No. 2: 154 - 158.
4. Lesavre, P. Antineutrophil cytoplasmic antibodies antigen specificity. Am. J. Kidney Dis. 1991, Vol. XVIII, No. 2: 159 - 163.
5. Hagen, E. C. et al. Antineutrophil cytoplasmic autoantibodies: a review of the antigens involved, the assays, and the clinical and possible pathogenic consequences. Blood 1993, Vol.81: 1996 - 2000.
6. Gross, W .L. et al. Immunodiagnostische und immunopathogenetische Bedeutung von Anti-Neutrophilen-Cytoplasma-Antikörpern. Deutsche Medizinische Wochenschrift 1993, Vol. 118: 191 - 199.

Notice to the user (European Union):

Any serious incident that has occurred in relation to the device shall be reported to the manufacturer and the competent authority of the EU Member State in which the user and/or the patient is established .

Change Control

Former version: *ORG 519_IFU_EN_QM113148_2016-05-03_1.3* Reason for revision: *Introduction electronic IFU on homepage*

- 1** Pipet **100 µl** calibrator, control or patient sample
→ Incubate for **30 minutes** at room temperature
→ Discard the contents of the wells and wash 3 times with **300 µl** wash solution
- 2** Pipet **100 µl** enzyme conjugate
→ Incubate for **15 minutes** at room temperature
→ Discard the contents of the wells and wash 3 times with **300 µl** wash solution
- 3** Pipet **100 µl** substrate solution
→ Incubate for **15 minutes** at room temperature
- 4** Add **100 µl** stop solution
→ Leave untouched for **5 minutes**
→ Read at **450 nm**

ORGENTEC Diagnostika GmbH


Carl-Zeiss-Straße 49-51

55129 Mainz - Germany

Phone: +49 (0) 61 31 / 92 58-0

Fax: +49 (0) 61 31 / 92 58-58

Internet: www.orgentec.com



ORG 548 Anti-MCV

INTENDED PURPOSE

Anti-MCV is an ELISA test system for the quantitative measurement of IgG class autoantibodies against mutated citrullinated vimentin (MCV) in human serum or plasma. This product is intended for professional in vitro diagnostic use only.

Measurement of anti-MCV antibodies contributes to early diagnosis of rheumatoid arthritis (RA), where anti-MCV antibody levels represent one parameter of a multi-criterion diagnostic process, encompassing both clinical and laboratory-based assessments.

SYMBOLS USED ON LABELS

	In vitro diagnostic medical device		Microplate
	Manufacturer		Calibrator
	Catalogue number		Calibrator
	Sufficient for 96 determinations		Calibrator
	Batch code		Calibrator
	Use by		Calibrator
	Temperature limitation		Calibrator
	Keep away from sunlight		Control positive
	Do not reuse		Control negative
	Date of manufacture		Sample Buffer P
	CE marked according to 98/79/EC		Enzyme Conjugate
	Consult instructions for use		TMB Substrate
	Electronic Instruction For Use: version		Stop solution
			Wash Buffer
			Ready to use

PRINCIPLE OF THE TEST

Mutated citrullinated vimentin (MCV) is bound to microwells.

The determination is based on an indirect enzyme linked immune reaction with the following steps:

Specific antibodies in the patient sample bind to the antigen coated on the surface of the reaction wells. After incubation, a washing step removes unbound and unspecifically bound serum or plasma components. Subsequently added enzyme conjugate binds to the immobilized antibody-antigen-complexes. After incubation, a second washing step removes unbound enzyme conjugate. After addition of substrate solution the bound enzyme conjugate hydrolyses the substrate forming a blue coloured product. Addition of an acid stops the reaction generating a yellow end-product. The intensity of the yellow color correlates with the concentration of the antibody-antigen-complex and can be measured photometrically at 450 nm.

WARNINGS AND PRECAUTIONS

- All reagents of this kit are intended for professional in vitro diagnostic use only.
- Components containing human serum were tested and found negative for HBsAg, HCV, HIV1 and HIV2 by FDA approved methods. No test can guarantee the absence of HBsAg, HCV, HIV1 or HIV2, and so all human serum based reagents in this kit must be handled as though capable of transmitting infection.
- Bovine serum albumin (BSA) used in components has been tested for BSE and found negative.
- Avoid contact with the substrate TMB (3,3',5,5'-Tetramethyl-benzidine).
- Stop solution contains acid, classification is non-hazardous. Avoid contact with skin.
- Control, sample buffer and wash buffer contain sodium azide 0.09% as preservative. This concentration is classified as non-hazardous.
- Enzyme conjugate contains ProClin 300 0.05% as preservative. This concentration is classified as non-hazardous.

During handling of all reagents, controls and serum samples observe the existing regulations for laboratory safety regulations and good laboratory practice:

- First aid measures: In case of skin contact, immediately wash thoroughly with water and soap. Remove contaminated clothing and shoes and wash before reuse. If system fluid comes into contact with skin, wash thoroughly with water. After contact with the eyes carefully rinse the opened eye with running water for at least 10 minutes. Get medical attention if necessary.
 - Personal precautions, protective equipment and emergency procedures:
Observe laboratory safety regulations. Avoid contact with skin and eyes. Do not swallow. Do not pipette by mouth. Do not eat, drink, smoke or apply makeup in areas where specimens or kit reagents are handled. When spilled, absorb with an inert material and put the spilled material in an appropriate waste disposal.
 - Exposure controls / personal protection: Wear protective gloves of nitril rubber or natural latex. Wear protective glasses. Used according to intended use no dangerous reactions known.
 - Conditions to avoid: Since substrate solution is light-sensitive. Store in the dark.
 - For disposal of laboratory waste the national or regional legislation has to be observed.
- Observe the guidelines for performing quality control in medical laboratories by assaying control sera.

CONTENTS OF THE KIT

ORG 548	▽ 96	Sufficient for 96 determinations
MICROPLATE	1	One divisible microplate consisting of 12 modules of 8 wells each. Ready to use. Product code on module: MCV
CALIBRATOR A	1x 1.5 ml	Calibrator A 0 U/ml, containing serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
CALIBRATOR B	1x 1.5 ml	Calibrator B 20 U/ml, containing MCV antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
CALIBRATOR C	1x 1.5 ml	Calibrator C 40 U/ml, containing MCV antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
CALIBRATOR D	1x 1.5 ml	Calibrator D 100 U/ml, containing MCV antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
CALIBRATOR E	1x 1.5 ml	Calibrator E 300 U/ml, containing MCV antibodies in a serum/buffer matrix (PBS, BSA, NaN3 0.09%), yellow. Ready to use.
CALIBRATOR F	1x 1.5 ml	Calibrator F 1000 U/ml, containing MCV antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
CONTROL +	1x 1.5 ml	Control positive, containing MCV antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use. The concentration is specified on the certificate of analysis.
CONTROL -	1x 1.5 ml	Control negative, containing MCV antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use. The concentration is specified on the certificate of analysis.
DILUENT	20 ml	Sample Buffer P, containing PBS, BSA, detergent, preservative sodium azide 0.09%, yellow, concentrate (5 x).
CONJUGATE	15 ml	Enzyme Conjugate containing anti-human IgG antibodies, HRP labelled; PBS, BSA, detergent, preservative PROCLIN 0.05%, light red. Ready to use.
TMB	15 ml	TMB Substrate; containing 3,3', 5,5'- Tetramethylbenzidin, colorless. Ready to use.
STOP	15 ml	Stop solution; contains acid. Ready to use.
WASH	20 ml	Wash Buffer, containing Tris, detergent, preservative sodium azide 0.09%; 50 x conc.
i	1	Certificate of Analysis

MATERIALS REQUIRED

- Microplate reader capable of endpoint measurements at 450 nm; optional: reference filter at 620 nm
- Data reduction software
- Multi-channel dispenser or repeatable pipette for 100 µl
- Vortex mixer
- Pipettes for 10 µl, 100 µl and 1000 µl
- Laboratory timing device
- Distilled or deionised water
- Measuring cylinder for 1000 ml and 100 ml
- Plastic container for storage of the wash solution

This ELISA assay is suitable for use on open automated ELISA processors. Each assay has to be validated on the respective automated system. Detailed information is provided upon request.

SPECIMEN COLLECTION, STORAGE AND HANDLING

- Collect whole blood specimens using acceptable medical techniques to avoid hemolysis.
- Allow blood to clot and separate the serum or plasma by centrifugation.
- Test serum should be clear and non-hemolyzed. Contamination by hemolysis or lipemia should be avoided, but does not interfere with this assay.
- Specimens may be refrigerated at 2-8°C for up to five days or stored at -20°C up to six months.
- Avoid repetitive freezing and thawing of serum or plasma samples. This may result in variable loss of antibody activity.
- Testing of heat-inactivated sera is not recommended.

STORAGE AND STABILITY

- Store test kit at 2-8°C in the dark.
- Do not expose reagents to heat, sun, or strong light during storage and usage.
- Store microplate sealed and dessicated in the clip bag provided.
- Shelf life of the unopened test kit is 18 months from day of production.
Unopened reagents are stable until expiration of the kit. See labels for individual batch.
- Diluted Wash Buffer and Sample Buffer are stable for at least 30 days when stored at 2-8°C.
We recommend consumption on the same day.

PROCEDURAL NOTES

- Do not use kit components beyond their expiration dates.
- Do not interchange kit components from different lots and products.
- All materials must be at room temperature (20-28°C) prior to use.
- Prepare all reagents and samples. Once started, perform the test without interruption.
- Double determinations may be done. By this means pipetting errors may become obvious.
- Perform the assay steps only in the order indicated.
- Always use fresh sample dilutions.
- Pipette all reagents and samples into the bottom of the wells.
- To avoid carryover or contamination, change the pipette tip between samples and different kit controls.
- Wash microwells thoroughly and remove the last droplets of wash buffer.
- All incubation steps must be accurately timed.
- Do not re-use microplate wells.

PREPARATION OF REAGENTS

WASH

Dilute the contents of one vial of the buffered wash solution concentrate (50x) with distilled or deionised water to a final volume of 1000 ml prior to use.

DILUENT

Sample Buffer P: Prior to use dilute the contents (20 ml) of one vial of sample buffer 5x concentrate with distilled or deionised water to a final volume of 100 ml.

Preparation of samples

Dilute patient samples 1:100 before the assay: Put 990 µl of prediluted sample buffer in a polystyrene tube and add 10 µl of sample. Mix well. Note: Calibrators / Controls are ready to use and need not be diluted.

TEST PROCEDURE

Prepare enough microplate modules for all calibrators / controls and patient samples.

- Pipette **100 µl** of calibrators, controls and prediluted patient samples into the wells.
Incubate for **30 minutes** at room temperature (20-28 °C).
Discard the contents of the microwells and **wash 3 times** with **300 µl** of wash solution.
- Dispense **100 µl** of enzyme conjugate into each well.
Incubate for **15 minutes** at room temperature.
Discard the contents of the microwells and **wash 3 times** with **300 µl** of wash solution.
- Dispense **100 µl** of TMB substrate solution into each well.
Incubate for **15 minutes** at room temperature
- Add 100 µl** of stop solution to each well of the modules
Incubate for **5 minutes** at room temperature.
Read the optical density at 450 nm (reference 600-690nm) and calculate the results.
The developed colour is stable for at least 30 minutes. Read during this time.

Example for a pipetting scheme:

	1	2	3	4	5	6	7	8	9	10	11	12
A	A	P1										
B	B	P2										
C	C	P3										
D	D											
E	E											
F	F											
G	C+											
H	C-											

P1, ... patient sample A-F calibrators C+, C- controls

VALIDATION

Test results are valid if the optical densities at 450 nm for calibrators / controls and the results for controls comply with the reference ranges indicated on the Certificate of Analysis enclosed in each test kit.
If these quality control criteria are not met the assay run is invalid and should be repeated.

CALCULATION OF RESULTS

For quantitative results plot the optical density of each calibrator versus the calibrator concentration to create a calibration curve. The concentration of patient samples may then be estimated from the calibration curve by interpolation.

Using data reduction software a 4-Parameter-Fit with lin-log coordinates for optical density and concentration is the data reduction method of choice.

PERFORMANCE CHARACTERISTICS

CALIBRATION

This assay system is calibrated in relative arbitrary units, since no international reference preparation is available for this assay.

Measuring range

The calculation range of this ELISA assay is 0 - 1000 U/ml

Expected values

In a normal range study with samples from healthy blood donors the following ranges have been established with this ELISA assay: Cut-off 20 U/ml

Interpretation of results

Negative: < 20 U/ml
Positive: ≥ 20 U/ml

Linearity

Patient samples containing high levels of specific antibody were serially diluted in sample buffer to demonstrate the dynamic range of the assay and the upper / lower end of linearity. Activity for each dilution was calculated from the calibration curve using a 4-Parameter-Fit with lin-log coordinates.

Sample	Dilution	Observed U/ml	Expected U/ml	O/E [%]
1	1:100	882.8	882.8	100
.	1:200	386.0	441.4	87
.	1:400	205.2	220.7	93
.	1:800	110.7	110.4	100
.	1:1600	52.2	55.2	95
.	1:3200	23.4	27.6	85
2	1:100	932.1	932.1	100
.	1:200	486.0	466.1	104
.	1:400	250.1	233.0	107
.	1:800	126.6	116.5	109
.	1:1600	61.7	58.3	106
.	1:3200	28.2	29.1	97
3	1:100	727.9	727.9	100
.	1:200	362.4	364.0	100
.	1:400	178.2	182.0	98
.	1:800	85.7	91.0	94
.	1:1600	47.1	45.5	104
.	1:3200	19.2	22.7	85

Limit of detection

Functional sensitivity was determined to be: 1 U/ml

Reproducibility

Intra-assay precision: Coefficient of variation (CV) was calculated for each of three samples from the results of 24 determinations in a single run. Results for precision-within-assay are shown in the table below.

Inter-assay precision: Coefficient of variation (CV) was calculated for each of three samples from the results of 6 determinations in 5 different runs. Results for run-to-run precision are shown in the table below.

Intra-Assay		
Sample	Mean U/ml	CV %
1	22.7	6.2
2	118.8	6.4
3	548.1	4.6

Inter-Assay		
Sample	Mean U/ml	CV %
1	20.2	5.3
2	111.0	9.2
3	451.6	7.7

Interfering substances

No interference has been observed with haemolytic (up to 1000 mg/dl) or lipemic (up to 3 g/dl triglycerides) sera or plasma, or bilirubin (up to 40 mg/dl) containing sera or plasma. Nor have any interfering effects been observed with the use of anticoagulants (Citrate, EDTA, Heparine). However for practical reasons it is recommended that grossly hemolyzed or lipemic samples should be avoided.

Study results

Study population	n	n Pos	%
Rheumatoid arthritis	490	398	81.2
Other diseases	522	14	2.7
Normal human sera	234	1	0.4

		Clinical Diagnosis		
		POS	NEG	
ORG 548	POS	398	15	1246
	NEG	92	741	
		490	756	

Sensitivity: 81.2 %
Specificity: 98.0 %
Overall agreement: 91.4 %

LIMITATIONS OF THE PROCEDURE

This assay is a diagnostic aid. A definite clinical diagnosis should not be based on the results of a single test, but should be made by the physician after all clinical and laboratory findings have been evaluated concerning the entire clinical picture of the patient. Also every decision for therapy should be taken individually.

The above pathological and normal reference ranges for antibodies in patient samples should be regarded as recommendations only. Each laboratory should establish its own ranges according to ISO 15189 or other applicable laboratory guidelines.

REFERENCES

1. F.Bobbio-Pallavicini, C.Alpini, R.Caporali, S.Avale, S.Bugatti, C.Montecuccio. Autoantibody profile in rheumatoid arthritis during long-term infliximab treatment. *Arthritis Res Ther* 2004; 6:R264-R272 (DOI 10.1186/ar1173)
2. E.R.Vossenaar, N.Deprés, E.Lapointe, A. van der Heijden, M.Lora, T.Senshu, W.J. van Venrooij, H.A.Ménard. Rheumatoid arthritis specific anti Sa antibodies target citrullinated vimentin. *Arthritis Research & Therapie* Vol.6 No.2
3. O.Vittecoq, S.Poplin, K.Krzyszowska, F.Jouen-Beades, J.F.Ménard, A.Daragon, F.Tron, X.Loet. Rheumatoid Factor is the strongest predictor of radiological progression of rheumatoid arthritis in a three-year prospective study in community-recruited patients. *Rheumatology* 2003; 42:939-946
4. W.J. van Venrooij, J.M.Hazes, H.Visser. Anticitrullinated protein/peptide antibody and its role in the diagnosis and prognosis of early rheumatoid arthritis. *The Netherland Journal of Medicine*.
5. M.Escalon, F.J.Lópees-Longo, C.M. González, I.Monteagudo, M.Rodríguez-Mahou, R.Grau, L.Carreno. Anti-Sa Sera from patients with Rheumatoid Arthritis contain at least 2 different subpopulations of Anti-Sa antibodies. *The Journal of Rheumatology* 2002; 29:10 2053-60
6. Ch.Vincent, L.Nogueira, M.Sebba, S.Chapuy-Regaud, M.Arnaud, O.Letourneur, D.Rolland, B.Rounie, A. Cantagrel, M.Jolivet, G.Serre. Detecion of antibodies to determined recombinant tat flaggrin by Enzyme-Linked Immunosorbent Assay. *Arthritis & Rheumatism* Vo. 46, No.8, August 2002, pp. 2051 -58
7. G.Steiner, J.Smolen. Antibodies in rheumatoid arthritis and their clinical significance. *Arthritis Res* 2002,4 (suppl 2);S1-S5
8. R.Goldbach-Mansky, J.Lee, A.McCoy, J.Hoxworth, C.Yarboro, J.S.Smolen, G.Steiner, A.Rosen, C.Zhang, H.A. Ménard, Z.J.Zhou, T.Palosuo, W.J. Van Venrooij, R.L.Wilder, J.H.Klippel, H.R.Schumacher Jr., H.S.El-Gabalawy. Rheumatoid arthritis associated antibodies in patients with synovitis of recent onset. *Arthritis Res* 2000,2:236-243
9. H.Ménard, E.Lapointe, M.D.Rochdi, Z.J.Zhou. Insights into rheumatoid arthritis derived from the Sa immune system. *Arthritis Research* 2000,2:429-432
10. G.Hayem, P.Chazerain, B.Combe, A.Elias, T.Haim, P.Nicaise, K.Benali, J-F Eliau, M-F Kahn, J.Sany, O.Meyer. Anti-Sa antibody is an accurate diagnostic and prognostic Marker in adult Rheumatoid Arthritis. *The Journal of Rheumatology* 1999;26:7-13
11. N. Deprés, G.Boire, F.J. Lopez-Longo, H.A. Ménard. The Sa System : A novel antigen antibody system specific for rheumatoid arthritis. *The Journal of Rheumatology* 1994; 21 :1 027- 33
12. E.R.Vossenaar, T.R.D. Radstake, A. van der Heijden, M.A.M. van Mansum, C. Dieteren, D.-J. de Rooij, P. Barrera, A.J.W. Zendman, W.J. van Venrooij. Expression and activity of citrullinase peptidylarginine deiminase enzymes in monocytes and macrophages. *Ann Rheum Dis* 2004; 63:373-381
13. H. Burkhardt, B. Sehnert, R. Bockermann, A. Engström, J.R. Kalden, R. Holmdahl. Humoral immune response to citrullinated collagen type II determinants in early rheumatoid arthritis. *Eur. J. Immunol.* 2005.35: 1643-1652
14. Ch.Vincent, L. Nogueira, C. Clavel, M. Sebbag, G. Serre. Autoantibodies to citrullinated pro-teins: ACPA. *Autoimmunity*, February 2005; 38 (1): 17-24
15. M. Sebbag, S. Chapuy-Regaud, I. Auger, E. Petit-Teixeira, C. Clavel, L. Nogueira, Ch.Vincent, F. Cornélis, J. Roudier, G. Serre. Clinical and pathophysiological significance of the autoimmune response to citrullinated proteins in rheumatoid arthritis. *Joint bone Spine* 71 (2004) 493-502

References Concerning Classification of RA

16. Liao KP, Batra KL, Chibnik L, Schur PH, Costenbader KH. Anti-CCP revised criteria for the classification of rheumatoid arthritis. *Ann Rheum Dis* 2008.
17. Arnett FC, Edworthy SM, Bloch DA, McShane DJ, Fries JF, Cooper NS et al. The American Rheumatism Association 1987 revised criteria for the classification of rheumatoid arthritis. *Arthritis Rheum* 1988; 31(3):315-24. Further Reading on Diagnostic Performance of Anti-MCV vs. Predicate Assay:
18. Gyetvai A, Szekanecz Z, Soos L, Szabo Z, Fekete A, Kapitany A et al. New classification of the shared epitope in rheumatoid arthritis: impact on the production of various anti-citrullinated protein antibodies. *Rheumatology (Oxford)* 2010; 49(1):25-33.
19. Pruijn G, Wiik A, van Venrooij W. The use of citrullinated peptides and proteins for the diagnosis of rheumatoid arthritis. *Arthritis Research & Therapy* 2010; 12(1):203.
20. Aggarwal R, Liao K, Nair R, Ringold S, Costenbader KH. Anti-citrullinated peptide antibody assays and their role in the diagnosis of rheumatoid arthritis. *Arthritis Rheum* 2009; 61(11):1472-83.
21. Feitsma AL, van der Voort EI, Franken KL, El BH, Elferink BG, Drijfhout JW et al. Identification of citrullinated vimentin peptides as T cell epitopes in HLA-DR4-positive patients with rheumatoid arthritis. *Arthritis Rheum* 2009; 62(1):117-25.
22. Klareskog L, Catrina AI, Paget S. Rheumatoid arthritis. *Lancet* 2009; 373(9664):659-72.
23. Liu X, Jia R, Zhao J, Li Z. The Role of Anti-Mutated Citrullinated Vimentin Antibodies in the Diagnosis of Early Rheumatoid Arthritis. *J Rheumatol* 2009.
24. Luime JJ, Colin EM, Hazes JM, Lubberts E. Does anti-MCV has additional value as serological marker in the diagnostic and prognostic work-up of patients with rheumatoid arthritis? A systematic review. *Ann Rheum Dis* 2009.
25. Mjaavatten MD, Uhlig T, Haugen AJ, Nygaard H, Sidenvall G, Helgetveit K et al. Positive anti-citrullinated protein antibody status and small joint arthritis are consistent predictors of chronic disease in patients with very early arthritis: results from the NOR-VEAC cohort. *Arthritis Res Ther* 2009; 11(5):R146.
26. Engelmann R, Brandt J, Eggert M, Karberg K, Krause A, Neeck G et al. The Anti-mutated Citrullinated Vimentin Response Classifies Patients with Rheumatoid Arthritis into Broad and Narrow Responders. *J Rheumatol* 2009.
27. Raza K, Mathsson L, Buckley CD, Filer A, Ronnelid J. Anti-modified citrullinated vimentin (MCV) antibodies in patients with very early synovitis. *Ann Rheum Dis* 2009.
28. Snir O, Widhe M, Hermansson M, von SC, Lindberg J, Hensen S et al. Antibodies to several citrullinated antigens are enriched in the joints of rheumatoid arthritis patients. *Arthritis Rheum* 2009; 62(1):44-52.
29. Syversen SW, Goll GL, van der Heijde D, Landewe R, Lie BA, Odegard S et al. Prediction of radiographic progression in rheumatoid arthritis and the role of antibodies against mutated citrullinated vimentin: results from a ten-year prospective study. *Ann Rheum Dis* 2009.
30. van der Linden MP, van der Woude D, Ioan-Facsinay A, Levarht EW, Stoeken-Rijsbergen G, Huizinga TW et al. Value of anti-modified citrullinated vimentin and third-generation anti-cyclic citrullinated peptide compared with second-generation anti-cyclic citrullinated peptide and rheumatoid factor in predicting disease outcome in undifferentiated arthritis and rheumatoid arthritis. *Arthritis Rheum* 2009; 60(8):2232-41.
31. Wagner E, Skoumal M, Bayer PM, Klaushofer K. Antibody against mutated citrullinated vimentin: a new sensitive marker in the diagnosis of rheumatoid arthritis. *Rheumatol Int* 2009.
32. Keskin G, Inal A, Keskin D, Pekel A, Baysal O, Dizer U et al. Diagnostic Utility of Anti-Cyclic Citrullinated Peptide and Anti-Modified Citrullinated Vimentin Antibodies in Rheumatoid Arthritis. *Protein Pept Lett* 2008; 15 (3):314-7.
33. Szekanecz Z, Lakos G. Rheumatoid arthritis diagnosis with antimitated citrullinated vimentin ELISA by Orgentec Diagnostika. *Exp Opin Med Diagnostics* 2008; 2(9):1083-90.
34. Szekanecz Z, Soos L, Szabo Z, Fekete A, Kapitany A, Vegvari A et al. Anti-Citrullinated Protein Antibodies in Rheumatoid Arthritis: As Good as it Gets? *Clin Rev Allergy Immunol* 2008; 34(1):26-31.

Notice to the user (European Union):

Any serious incident that has occurred in relation to the device shall be reported to the manufacturer and the competent authority of the EU Member State in which the user and/or the patient is established .

Change Control

Former version: *ORG 548_IFU_EN_QM113183_2013-12-16_1.2* Reason for revision: *Introduction electronic IFU on homepage*

- 1 Pipet **100 µl** calibrator, control or patient sample
 - Incubate for **30 minutes** at room temperature
 - Discard the contents of the wells and wash 3 times with **300 µl** wash solution
- 2 Pipet **100 µl** enzyme conjugate
 - Incubate for **15 minutes** at room temperature
 - Discard the contents of the wells and wash 3 times with **300 µl** wash solution
- 3 Pipet **100 µl** substrate solution
 - Incubate for **15 minutes** at room temperature
- 4 Add **100 µl** stop solution
 - Leave untouched for **5 minutes**
 - Read at **450 nm**

ORGENTEC Diagnostika GmbH


Carl-Zeiss-Straße 49-51

55129 Mainz - Germany

Phone: +49 (0) 61 31 / 92 58-0

Fax: +49 (0) 61 31 / 92 58-58

Internet: www.orgentec.com



ORG 549 Anti-C1q

INTENDED PURPOSE

Anti-C1q is an ELISA test system for the quantitative measurement of IgG class autoantibodies against C1q in human serum or plasma. This product is intended for professional in vitro diagnostic use only.

The test is used as an aid in the differential diagnosis of systemic autoimmune diseases with renal involvement, e.g. systemic lupus erythematosus, lupus nephritis. Evaluation of a test result should always take into account all clinical and laboratory diagnostic findings.

SYMBOLS USED ON LABELS

	In vitro diagnostic medical device		Microplate
	Manufacturer		Calibrator
	Catalogue number		Calibrator
	Sufficient for 96 determinations		Calibrator
	Batch code		Calibrator
	Use by		Calibrator
	Temperature limitation		Calibrator
	Keep away from sunlight		Control positive
	Do not reuse		Control negative
	Date of manufacture		Sample Buffer P
	CE marked according to 98/79/EC		Enzyme Conjugate
	Consult instructions for use		TMB Substrate
	Electronic Instruction For Use: version		Stop solution
			Wash Buffer
			Ready to use

PRINCIPLE OF THE TEST

Highly purified human C1q is bound to microwells.

The determination is based on an indirect enzyme linked immune reaction with the following steps: Specific antibodies in the patient sample bind to the antigen coated on the surface of the reaction wells. After incubation, a washing step removes unbound and unspecifically bound serum or plasma components. Subsequently added enzyme conjugate binds to the immobilized antibody-antigen-complexes. After incubation, a second washing step removes unbound enzyme conjugate. After addition of substrate solution the bound enzyme conjugate hydrolyses the substrate forming a blue coloured product. Addition of an acid stops the reaction generating a yellow end-product. The intensity of the yellow color correlates with the concentration of the antibody-antigen-complex and can be measured photometrically at 450 nm.

WARNINGS AND PRECAUTIONS

- All reagents of this kit are intended for professional in vitro diagnostic use only.
- Components containing human serum were tested and found negative for HBsAg, HCV, HIV1 and HIV2 by FDA approved methods. No test can guarantee the absence of HBsAg, HCV, HIV1 or HIV2, and so all human serum based reagents in this kit must be handled as though capable of transmitting infection.
- Bovine serum albumin (BSA) used in components has been tested for BSE and found negative.
- Avoid contact with the substrate TMB (3,3',5,5'-Tetramethyl-benzidine).
- Stop solution contains acid, classification is non-hazardous. Avoid contact with skin.
- Control, sample buffer and wash buffer contain sodium azide 0.09% as preservative. This concentration is classified as non-hazardous.
- Enzyme conjugate contains ProClin 300 0.05% as preservative. This concentration is classified as non-hazardous.

During handling of all reagents, controls and serum samples observe the existing regulations for laboratory safety regulations and good laboratory practice:

- First aid measures: In case of skin contact, immediately wash thoroughly with water and soap. Remove contaminated clothing and shoes and wash before reuse. If system fluid comes into contact with skin, wash thoroughly with water. After contact with the eyes carefully rinse the opened eye with running water for at least 10 minutes. Get medical attention if necessary.
- Personal precautions, protective equipment and emergency procedures:
Observe laboratory safety regulations. Avoid contact with skin and eyes. Do not swallow. Do not pipette by mouth. Do not eat, drink, smoke or apply makeup in areas where specimens or kit reagents are handled. When spilled, absorb with an inert material and put the spilled material in an appropriate waste disposal.
- Exposure controls / personal protection: Wear protective gloves of nitril rubber or natural latex. Wear protective glasses. Used according to intended use no dangerous reactions known.
- Conditions to avoid: Since substrate solution is light-sensitive. Store in the dark.
- For disposal of laboratory waste the national or regional legislation has to be observed.

Observe the guidelines for performing quality control in medical laboratories by assaying control sera.

CONTENTS OF THE KIT

ORG 549	▽ 96	Sufficient for 96 determinations
MICROPLATE	1	One divisible microplate consisting of 12 modules of 8 wells each. Ready to use. Product code on module: C1Q
CALIBRATOR A	1x 1.5 ml	Calibrator A 0 U/ml, containing serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
CALIBRATOR B	1x 1.5 ml	Calibrator B 6.3 U/ml, containing C1q antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
CALIBRATOR C	1x 1.5 ml	Calibrator C 12.5 U/ml, containing C1q antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
CALIBRATOR D	1x 1.5 ml	Calibrator D 25 U/ml, containing C1q antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
CALIBRATOR E	1x 1.5 ml	Calibrator E 50 U/ml, containing C1q antibodies in a serum/buffer matrix (PBS, BSA, NaN3 0.09%), yellow. Ready to use.
CALIBRATOR F	1x 1.5 ml	Calibrator F 100 U/ml, containing C1q antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
CONTROL +	1x 1.5 ml	Control positive, containing C1q antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use. The concentration is specified on the certificate of analysis.
CONTROL -	1x 1.5 ml	Control negative, containing C1q antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use. The concentration is specified on the certificate of analysis.
DILUENT	20 ml	Sample Buffer P, containing PBS, BSA, detergent, preservative sodium azide 0.09%, yellow, concentrate (5 x).
CONJUGATE	15 ml	Enzyme Conjugate containing anti-human IgG antibodies, HRP labelled; PBS, BSA, detergent, preservative PROCLIN 0.05%, light red. Ready to use.
TMB	15 ml	TMB Substrate; containing 3,3', 5,5'- Tetramethylbenzidin, colorless. Ready to use.
STOP	15 ml	Stop solution; contains acid. Ready to use.
WASH	20 ml	Wash Buffer, containing Tris, detergent, preservative sodium azide 0.09%; 50 x conc.
i	1	Certificate of Analysis

MATERIALS REQUIRED

- Microplate reader capable of endpoint measurements at 450 nm; optional: reference filter at 620 nm
- Data reduction software
- Multi-channel dispenser or repeatable pipette for 100 µl
- Vortex mixer
- Pipettes for 10 µl, 100 µl and 1000 µl
- Laboratory timing device
- Distilled or deionised water
- Measuring cylinder for 1000 ml and 100 ml
- Plastic container for storage of the wash solution

This ELISA assay is suitable for use on open automated ELISA processors. Each assay has to be validated on the respective automated system. Detailed information is provided upon request.

SPECIMEN COLLECTION, STORAGE AND HANDLING

- Collect whole blood specimens using acceptable medical techniques to avoid hemolysis.
- Allow blood to clot and separate the serum or plasma by centrifugation.
- Test serum should be clear and non-hemolyzed. Contamination by hemolysis or lipemia should be avoided, but does not interfere with this assay.
- Specimens may be refrigerated at 2-8°C for up to five days or stored at -20°C up to six months.
- Avoid repetitive freezing and thawing of serum or plasma samples. This may result in variable loss of antibody activity.
- Testing of heat-inactivated sera is not recommended.

STORAGE AND STABILITY

- Store test kit at 2-8°C in the dark.
- Do not expose reagents to heat, sun, or strong light during storage and usage.
- Store microplate sealed and dessicated in the clip bag provided.
- Shelf life of the unopened test kit is 18 months from day of production.
Unopened reagents are stable until expiration of the kit. See labels for individual batch.
- Diluted Wash Buffer and Sample Buffer are stable for at least 30 days when stored at 2-8°C.
We recommend consumption on the same day.

PROCEDURAL NOTES

- Do not use kit components beyond their expiration dates.
- Do not interchange kit components from different lots and products.
- All materials must be at room temperature (20-28°C) prior to use.
- Prepare all reagents and samples. Once started, perform the test without interruption.
- Double determinations may be done. By this means pipetting errors may become obvious.
- Perform the assay steps only in the order indicated.
- Always use fresh sample dilutions.
- Pipette all reagents and samples into the bottom of the wells.
- To avoid carryover or contamination, change the pipette tip between samples and different kit controls.
- Wash microwells thoroughly and remove the last droplets of wash buffer.
- All incubation steps must be accurately timed.
- Do not re-use microplate wells.

PREPARATION OF REAGENTS

WASH

Dilute the contents of one vial of the buffered wash solution concentrate (50x) with distilled or deionised water to a final volume of 1000 ml prior to use.

DILUENT

Sample Buffer P: Prior to use dilute the contents (20 ml) of one vial of sample buffer 5x concentrate with distilled or deionised water to a final volume of 100 ml.

Preparation of samples

Dilute patient samples 1:100 before the assay: Put 990 µl of prediluted sample buffer in a polystyrene tube and add 10 µl of sample. Mix well. Note: Calibrators / Controls are ready to use and need not be diluted.

TEST PROCEDURE

Prepare enough microplate modules for all calibrators / controls and patient samples.

- Pipette **100 µl** of calibrators, controls and prediluted patient samples into the wells.
Incubate for **30 minutes** at room temperature (20-28 °C).
Discard the contents of the microwells and **wash 3 times** with **300 µl** of wash solution.
- Dispense **100 µl** of enzyme conjugate into each well.
Incubate for **15 minutes** at room temperature.
Discard the contents of the microwells and **wash 3 times** with **300 µl** of wash solution.
- Dispense **100 µl** of TMB substrate solution into each well.
Incubate for **15 minutes** at room temperature
- Add 100 µl** of stop solution to each well of the modules
Incubate for **5 minutes** at room temperature.
Read the optical density at 450 nm (reference 600-690nm) and calculate the results.
The developed colour is stable for at least 30 minutes. Read during this time.

Example for a pipetting scheme:

	1	2	3	4	5	6	7	8	9	10	11	12
A	A	P1										
B	B	P2										
C	C	P3										
D	D											
E	E											
F	F											
G	C+											
H	C-											

P1, ... patient sample A-F calibrators C+, C- controls

VALIDATION

Test results are valid if the optical densities at 450 nm for calibrators / controls and the results for controls comply with the reference ranges indicated on the Certificate of Analysis enclosed in each test kit.
If these quality control criteria are not met the assay run is invalid and should be repeated.

CALCULATION OF RESULTS

For quantitative results plot the optical density of each calibrator versus the calibrator concentration to create a calibration curve. The concentration of patient samples may then be estimated from the calibration curve by interpolation. Using data reduction software a 4-Parameter-Fit with lin-log coordinates for optical density and concentration is the data reduction method of choice.

PERFORMANCE CHARACTERISTICS

Calibration

This assay system is calibrated in relative arbitrary units, since no international reference preparation is available for this assay.

Measuring range

The calculation range of this ELISA assay is 0 - 100 U/ml

Expected values

In a normal range study with samples from healthy blood donors the following ranges have been established with this ELISA assay: Cut-off 10 U/ml

Interpretation of results

Negative: < 10 U/ml
Positive: ≥ 10 U/ml

Linearity

Patient samples containing high levels of specific antibody were serially diluted in sample buffer to demonstrate the dynamic range of the assay and the upper / lower end of linearity. Activity for each dilution was calculated from the calibration curve using a 4-Parameter-Fit with lin-log coordinates.

Sample	Dilution	Observed U/ml	Expected U/ml	O/E [%]
1	1:100	88.4	88.4	100
	1:200	43.8	44.2	99
	1:400	22.7	22.1	103
	1:800	11.5	11.1	104
2	1:1600	5.4	5.5	98
	1:100	65.2	65.2	100
	1:200	32.1	32.6	98
	1:400	16.1	16.3	99
	1:800	7.9	8.2	97
	1:1600	3.7	4.1	91

Limit of detection

Functional sensitivity was determined to be: 0.5 U/ml

Reproducibility

Intra-assay precision: Coefficient of variation (CV) was calculated for each of three samples from the results of 24 determinations in a single run. Results for precision-within-assay are shown in the table below.

Inter-assay precision: Coefficient of variation (CV) was calculated for each of three samples from the results of 6 determinations in 5 different runs. Results for run-to-run precision are shown in the table below.

Intra-Assay		
Sample	Mean U/ml	CV %
1	25.2	3.7
2	58.6	3.0
3	75.4	2.9

Inter-Assay		
Sample	Mean U/ml	CV %
1	22.0	4.8
2	33.2	2.5
3	53.3	1.9

Interfering substances

No interference has been observed with haemolytic (up to 1000 mg/dl) or lipemic (up to 3 g/dl triglycerides) sera or plasma, or bilirubin (up to 40 mg/dl) containing sera or plasma. Nor have any interfering effects been observed with the use of anticoagulants (Citrate, EDTA, Heparine). However for practical reasons it is recommended that grossly hemolyzed or lipemic samples should be avoided.

Study results

Study population	n	n Pos	%
Lupus nephritis	34	29	85.3
Systemic lupus erythematosus	70	40	57.1
Other diseases	91	13	14.3
Normal human sera	74	4	5.4

		Clinical Diagnosis		
		POS	NEG	
ORG 549	POS	69	17	104
	NEG	35	148	
				269

Sensitivity: 66.3 %

Specificity: 89.7 %

Overall agreement: 80.7 %

LIMITATIONS OF THE PROCEDURE

This assay is a diagnostic aid. A definite clinical diagnosis should not be based on the results of a single test, but should be made by the physician after all clinical and laboratory findings have been evaluated concerning the entire clinical picture of the patient. Also every decision for therapy should be taken individually.

The above pathological and normal reference ranges for antibodies in patient samples should be regarded as recommendations only. Each laboratory should establish its own ranges according to ISO 15189 or other applicable laboratory guidelines.

REFERENCES

1. Siegert, C. E. H., and M. R. Daha. C1q as Antigen in Humoral Autoimmune Re-sponses. *Immunobiologie*, 1998, 199 (2): 295-302.
2. Kumar, A., R. Gupta, T. Varghese, R. M. Pande, V. K. Singal, and O. P. Garg. Anti-C1q antibody as a marker of disease activity in systemic lupus erythematosus. *Indian J Med Res*, 1999, 110:190-193
3. Walport, M. J. Complement and systemic lupus erythematosus. *Arthritis Res.*, 2002, 4 (suppl 3): 279-293.
4. Botto, M., Ch. Dell'Agnola, A. E. Bygrave, E. M. Thompson, H. T. Cook, F. Petry, M. Loos, P. P. Pandolfi, and M. J. Walport. Homozygous C1q deficiency causes glomerulonephritis associated with multiple apoptotic bodies. *Nat. Genetics*, 1998, 19(1): 56-59
5. Walport, M. J., K. A. Davies, M. Botto. C1q and Systemic Lupus Erythematosus. *Immunobiologie*, 1998, 199 (2): 265-285.
6. Trendelenburg, M., and J. A. Schifferli. Apoptose und C1q: Erklärungsansätze für die Pathogenese des SLE. *Z Rheumatol.*, 2000, 59: 172-175.
7. Conrad, K., W. Schößler, and F. Hiepe. Autoantikörper bei systemischen Autoimmunerkrankungen. Pabst Science Publishers, 2001, p. 38.

Notice to the user (European Union):

Any serious incident that has occurred in relation to the device shall be reported to the manufacturer and the competent authority of the EU Member State in which the user and/or the patient is established .

Change Control

Former version: *ORG 549_IFU_EN_QM113184_2013-12-16_1.2* Reason for revision: *Introduction electronic IFU on homepage*

- 1** Pipet **100 µl** calibrator, control or patient sample
→ Incubate for **30 minutes** at room temperature
→ Discard the contents of the wells and wash 3 times with **300 µl** wash solution
- 2** Pipet **100 µl** enzyme conjugate
→ Incubate for **15 minutes** at room temperature
→ Discard the contents of the wells and wash 3 times with **300 µl** wash solution
- 3** Pipet **100 µl** substrate solution
→ Incubate for **15 minutes** at room temperature
- 4** Add **100 µl** stop solution
→ Leave untouched for **5 minutes**
→ Read at **450 nm**

ORGENTEC Diagnostika GmbH


Carl-Zeiss-Straße 49-51

55129 Mainz - Germany

Phone: +49 (0) 61 31 / 92 58-0

Fax: +49 (0) 61 31 / 92 58-58

Internet: www.orgentec.com



ORG 512 Anti-Sci-70

INTENDED PURPOSE

Anti-Sci-70 is an ELISA test system for the quantitative measurement of IgG class autoantibodies against Sci-70 in human serum or plasma. This product is intended for professional in vitro diagnostic use only.

Antibodies against Sci-70 (DNA topoisomerase I) are an accepted marker for progressive systemic scleroderma. They contribute to the differential diagnosis of scleroderma. Evaluation of a test result should always take into account all clinical and laboratory diagnostic findings.

SYMBOLS USED ON LABELS

	In vitro diagnostic medical device		Microplate
	Manufacturer		Calibrator
	Catalogue number		Calibrator
	Sufficient for 96 determinations		Calibrator
	Batch code		Calibrator
	Use by		Calibrator
	Temperature limitation		Calibrator
	Keep away from sunlight		Control positive
	Do not reuse		Control negative
	Date of manufacture		Sample Buffer P
	CE marked according to 98/79/EC		Enzyme Conjugate
	Consult instructions for use		TMB Substrate
	Electronic Instruction For Use: version		Stop solution
			Wash Buffer
			Ready to use

PRINCIPLE OF THE TEST

Highly purified Sci-70 is bound to microwells.

The determination is based on an indirect enzyme linked immune reaction with the following steps:
Specific antibodies in the patient sample bind to the antigen coated on the surface of the reaction wells. After incubation, a washing step removes unbound and unspecifically bound serum or plasma components. Subsequently added enzyme conjugate binds to the immobilized antibody-antigen-complexes. After incubation, a second washing step removes unbound enzyme conjugate. After addition of substrate solution the bound enzyme conjugate hydrolyses the substrate forming a blue coloured product. Addition of an acid stops the reaction generating a yellow end-product. The intensity of the yellow color correlates with the concentration of the antibody-antigen-complex and can be measured photometrically at 450 nm.

WARNINGS AND PRECAUTIONS



- All reagents of this kit are intended for professional in vitro diagnostic use only.
- Components containing human serum were tested and found negative for HBsAg, HCV, HIV1 and HIV2 by FDA approved methods. No test can guarantee the absence of HBsAg, HCV, HIV1 or HIV2, and so all human serum based reagents in this kit must be handled as though capable of transmitting infection.
- Bovine serum albumin (BSA) used in components has been tested for BSE and found negative.
- Avoid contact with the substrate TMB (3,3',5,5'-Tetramethyl-benzidine).
- Stop solution contains acid, classification is non-hazardous. Avoid contact with skin.
- Control, sample buffer and wash buffer contain sodium azide 0.09% as preservative. This concentration is classified as non-hazardous.
- Enzyme conjugate contains ProClin 300 0.05% as preservative. This concentration is classified as non-hazardous.

During handling of all reagents, controls and serum samples observe the existing regulations for laboratory safety regulations and good laboratory practice:

- First aid measures: In case of skin contact, immediately wash thoroughly with water and soap. Remove contaminated clothing and shoes and wash before reuse. If system fluid comes into contact with skin, wash thoroughly with water. After contact with the eyes carefully rinse the opened eye with running water for at least 10 minutes. Get medical attention if necessary.
- Personal precautions, protective equipment and emergency procedures:
Observe laboratory safety regulations. Avoid contact with skin and eyes. Do not swallow. Do not pipette by mouth. Do not eat, drink, smoke or apply makeup in areas where specimens or kit reagents are handled. When spilled, absorb with an inert material and put the spilled material in an appropriate waste disposal.
- Exposure controls / personal protection: Wear protective gloves of nitril rubber or natural latex. Wear protective glasses. Used according to intended use no dangerous reactions known.
- Conditions to avoid: Since substrate solution is light-sensitive. Store in the dark.
- For disposal of laboratory waste the national or regional legislation has to be observed.

Observe the guidelines for performing quality control in medical laboratories by assaying control sera.

CONTENTS OF THE KIT

ORG 512		Sufficient for 96 determinations
MICROPLATE	1	One divisible microplate consisting of 12 modules of 8 wells each. Ready to use. Color code on module
CALIBRATOR A	1x 1.5 ml	Calibrator A 0 U/ml, containing serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
CALIBRATOR B	1x 1.5 ml	Calibrator B 12.5 U/ml, containing Scl-70 antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
CALIBRATOR C	1x 1.5 ml	Calibrator C 25 U/ml, containing Scl-70 antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
CALIBRATOR D	1x 1.5 ml	Calibrator D 50 U/ml, containing Scl-70 antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
CALIBRATOR E	1x 1.5 ml	Calibrator E 100 U/ml, containing Scl-70 antibodies in a serum/buffer matrix (PBS, BSA, NaN3 0.09%), yellow. Ready to use.
CALIBRATOR F	1x 1.5 ml	Calibrator F 200 U/ml, containing Scl-70 antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
CONTROL +	1x 1.5 ml	Control positive, containing Scl-70 antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use. The concentration is specified on the certificate of analysis.
CONTROL -	1x 1.5 ml	Control negative, containing Scl-70 antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use. The concentration is specified on the certificate of analysis.
DILUENT	20 ml	Sample Buffer P, containing PBS, BSA, detergent, preservative sodium azide 0.09%, yellow, concentrate (5 x).
CONJUGATE	15 ml	Enzyme Conjugate containing anti-human IgG antibodies, HRP labelled; PBS, BSA, detergent, preservative PROCLIN 0.05%, light red. Ready to use.
TMB	15 ml	TMB Substrate; containing 3,3', 5,5'- Tetramethylbenzidin, colorless. Ready to use.
STOP	15 ml	Stop solution; contains acid. Ready to use.
WASH	20 ml	Wash Buffer, containing Tris, detergent, preservative sodium azide 0.09%; 50 x conc.
	1	Certificate of Analysis

MATERIALS REQUIRED

- Microplate reader capable of endpoint measurements at 450 nm; optional: reference filter at 620 nm
- Data reduction software
- Multi-channel dispenser or repeatable pipette for 100 µl
- Vortex mixer
- Pipettes for 10 µl, 100 µl and 1000 µl
- Laboratory timing device
- Distilled or deionised water
- Measuring cylinder for 1000 ml and 100 ml
- Plastic container for storage of the wash solution

This ELISA assay is suitable for use on open automated ELISA processors. Each assay has to be validated on the respective automated system. Detailed information is provided upon request.

SPECIMEN COLLECTION, STORAGE AND HANDLING

- Collect whole blood specimens using acceptable medical techniques to avoid hemolysis.
- Allow blood to clot and separate the serum or plasma by centrifugation.
- Test serum should be clear and non-hemolyzed. Contamination by hemolysis or lipemia should be avoided, but does not interfere with this assay.
- Specimens may be refrigerated at 2-8°C for up to five days or stored at -20°C up to six months.
- Avoid repetitive freezing and thawing of serum or plasma samples. This may result in variable loss of antibody activity.
- Testing of heat-inactivated sera is not recommended.

STORAGE AND STABILITY

- Store test kit at 2-8°C in the dark.
- Do not expose reagents to heat, sun, or strong light during storage and usage.
- Store microplate sealed and desiccated in the clip bag provided.
- Shelf life of the unopened test kit is 18 months from day of production. Unopened reagents are stable until expiration of the kit. See labels for individual batch.
- Diluted Wash Buffer and Sample Buffer are stable for at least 30 days when stored at 2-8°C. We recommend consumption on the same day.

PROCEDURAL NOTES

- Do not use kit components beyond their expiration dates.
- Do not interchange kit components from different lots and products.
- All materials must be at room temperature (20-28°C) prior to use.
- Prepare all reagents and samples. Once started, perform the test without interruption.
- Double determinations may be done. By this means pipetting errors may become obvious.
- Perform the assay steps only in the order indicated.
- Always use fresh sample dilutions.
- Pipette all reagents and samples into the bottom of the wells.
- To avoid carryover or contamination, change the pipette tip between samples and different kit controls.
- Wash microwells thoroughly and remove the last droplets of wash buffer.
- All incubation steps must be accurately timed.
- Do not re-use microplate wells.

PREPARATION OF REAGENTS

WASH
Dilute the contents of one vial of the buffered wash solution concentrate (50x) with distilled or deionised water to a final volume of 1000 ml prior to use.

DILUENT
Sample Buffer P: Prior to use dilute the contents (20 ml) of one vial of sample buffer 5x concentrate with distilled or deionised water to a final volume of 100 ml.

Preparation of samples

Dilute patient samples 1:100 before the assay: Put 990 µl of prediluted sample buffer in a polystyrene tube and add 10 µl of sample. Mix well. Note: Calibrators / Controls are ready to use and need not be diluted.

TEST PROCEDURE

Prepare enough microplate modules for all calibrators / controls and patient samples.

- Pipette **100 µl** of calibrators, controls and prediluted patient samples into the wells.
Incubate for **30 minutes** at room temperature (20-28 °C).
Discard the contents of the microwells and **wash 3 times** with **300 µl** of wash solution.
- Dispense **100 µl** of enzyme conjugate into each well.
Incubate for **15 minutes** at room temperature.
Discard the contents of the microwells and **wash 3 times** with **300 µl** of wash solution.
- Dispense **100 µl** of TMB substrate solution into each well.
Incubate for **15 minutes** at room temperature
- Add 100 µl** of stop solution to each well of the modules
Incubate for **5 minutes** at room temperature.
Read the optical density at 450 nm (reference 600-690nm) and calculate the results.
The developed colour is stable for at least 30 minutes. Read during this time.

Example for a pipetting scheme:

	1	2	3	4	5	6	7	8	9	10	11	12
A	A	P1										
B	B	P2										
C	C	P3										
D	D											
E	E											
F	F											
G	C+											
H	C-											

P1, ... patient sample A-F calibrators C+, C- controls

VALIDATION

Test results are valid if the optical densities at 450 nm for calibrators / controls and the results for controls comply with the reference ranges indicated on the Certificate of Analysis enclosed in each test kit.
If these quality control criteria are not met the assay run is invalid and should be repeated.

CALCULATION OF RESULTS

For quantitative results plot the optical density of each calibrator versus the calibrator concentration to create a calibration curve. The concentration of patient samples may then be estimated from the calibration curve by interpolation.

Using data reduction software a 4-Parameter-Fit with lin-log coordinates for optical density and concentration is the data reduction method of choice.

PERFORMANCE CHARACTERISTICS

Calibration

The assay system is calibrated against the internationally recognized reference sera from CDC, Atlanta USA.

Measuring range

The calculation range of this ELISA assay is 0 - 200 U/ml

Expected values

In a normal range study with samples from healthy blood donors the following ranges have been established with this ELISA assay: Cut-off 25 U/ml

Interpretation of results

Negative:	< 15 U/ml
Borderline:	15 - 25 U/ml
Positive:	> 25 U/ml

Linearity

Patient samples containing high levels of specific antibody were serially diluted in sample buffer to demonstrate the dynamic range of the assay and the upper / lower end of linearity. Activity for each dilution was calculated from the calibration curve using a 4-Parameter-Fit with lin-log coordinates.

Sample	Dilution	Observed U/ml	Expected U/ml	O/E [%]
1	1:100	146.9	146.9	100
	1:200	76.3	73.5	104
	1:400	38.1	36.7	104
2	1:800	18.8	18.4	102
	1:100	122.3	122.3	100
	1:200	60.4	61.2	99
	1:400	29.6	30.6	97
	1:800	14.8	15.3	97

Limit of detection

Functional sensitivity was determined to be: 1 U/ml

Reproducibility

Intra-assay precision: Coefficient of variation (CV) was calculated for each of three samples from the results of 24 determinations in a single run. Results for precision-within-assay are shown in the table below.

Inter-assay precision: Coefficient of variation (CV) was calculated for each of three samples from the results of 6 determinations in 5 different runs. Results for run-to-run precision are shown in the table below.

Intra-Assay		
Sample	Mean U/ml	CV %
1	45.7	4.0
2	90.4	3.2
3	184.1	3.4

Inter-Assay		
Sample	Mean U/ml	CV %
1	41.1	2.8
2	89.9	2.8
3	157.4	2.3

Interfering substances

No interference has been observed with haemolytic (up to 1000 mg/dl) or lipemic (up to 3 g/dl triglycerides) sera or plasma, or bilirubin (up to 40 mg/dl) containing sera or plasma. Nor have any interfering effects been observed with the use of anticoagulants (Citrate, EDTA, Heparine). However for practical reasons it is recommended that grossly hemolyzed or lipemic samples should be avoided.

Study results

Study population	n	n Pos	%
Scleroderma	25	19	76.0
Rheumatoid arthritis	20	0	0.0
Normal human sera	80	1	1.3

		Clinical Diagnosis		
		POS	NEG	
ORG 512	POS	19	1	25
	NEG	6	99	
		25	100	125

Sensitivity: 76.0 %

Specificity: 99.0 %

Overall agreement: 94.4 %

LIMITATIONS OF THE PROCEDURE

This assay is a diagnostic aid. A definite clinical diagnosis should not be based on the results of a single test, but

should be made by the physician after all clinical and laboratory findings have been evaluated concerning the entire clinical picture of the patient. Also every decision for therapy should be taken individually.

The above pathological and normal reference ranges for antibodies in patient samples should be regarded as recommendations only. Each laboratory should establish its own ranges according to ISO 15189 or other applicable laboratory guidelines.

REFERENCES

1. Alba P, Bento L, Cuadrado MJ, Karim Y, Tungekar MF, Abbs I et al. Anti-dsDNA, anti-Sm antibodies, and the lupus anticoagulant: significant factors associated with lupus nephritis. *Ann Rheum Dis* 2003; 62(6):556-560.
2. Antico A, Platzgummer S, Bassetti D, Bizzaro N, Tozzoli R, Villalta D. Diagnosing systemic lupus erythematosus: new-generation immunoassays for measurement of anti-dsDNA antibodies are an effective alternative to the Farr technique and the Crithidia luciliae immunofluorescence test. *Lupus* 2010; 19(8):906-912.
3. Brouwer R, Hengstman GJ, Vree EW, Ehrfeld H, Bozic B, Ghirardello A et al. Autoantibody profiles in the sera of European patients with myositis. *Ann Rheum Dis* 2001; 60(2):116-123.
4. Castro C, Gourley M. Diagnostic testing and interpretation of tests for autoimmunity. *J Allergy Clin Immunol* 2010; 125(2 Suppl 2):S238-S247.
5. Defendenti C, Atzeni F, Spina MF, Grosso S, Cereda A, Guercilena G et al. Clinical and laboratory aspects of Ro/SSA-52 autoantibodies. *Autoimmun Rev* 2011; 10(3):150-154.
6. Eriksson C, Kokkonen H, Johansson M, Hallmans G, Wadell G, Rantapaa-Dahlqvist S. Autoantibodies predate the onset of Systemic Lupus Erythematosus in northern Sweden. *Arthritis Research & Therapy* 2011; 13(1):R30.
7. Haugbro K, Nossent JC, Winkler T, Figenschau Y, Rekvig OP. Anti-dsDNA antibodies and disease classification in antinuclear antibody positive patients: the role of analytical diversity. *Ann Rheum Dis JID* - 0372355 2004; 63(4):386-394.
8. Ippolito A, Wallace DJ, Gladman D, Fortin PR, Urowitz M, Werth V et al. Autoantibodies in systemic lupus erythematosus: comparison of historical and current assessment of seropositivity. *Lupus* 2011; 20(3):250-255.
9. Isenberg DA, Manson JJ, Ehrenstein MR, Rahman A. Fifty years of anti-ds DNA antibodies: are we approaching journey's end? *Rheumatology (Oxford)* 2007; 46(7):1052-1056.
10. Kattah NH, Kattah MG, Utz PJ. The U1-snRNP complex: structural properties relating to autoimmune pathogenesis in rheumatic diseases. *Immunol Rev* 2010; 233(1):126-145.
11. Kumar Y, Bhatia A, Minz RW. Antinuclear antibodies and their detection methods in diagnosis of connective tissue diseases: a journey revisited. *Diagn Pathol* 2009; 4:1.
12. Meroni PL, Schur PH. ANA screening: an old test with new recommendations. *Ann Rheum Dis* 2010; 69:1420-1422.
13. Petri M, Magder L. Classification criteria for systemic lupus erythematosus: a review. *Lupus* 2004; 13(11):829-837.
14. Poole BD, Schneider RI, Guthridge JM, Vette CA, Reichlin M, Harley JB et al. Early targets of nuclear RNP humoral autoimmunity in human systemic lupus erythematosus. *Arthritis Rheum* 2009; 60(3):848-859.
15. Putova I, Dostal C, Becvar R. Prevalence of antinucleosome antibodies by enzyme-linked immunosorbent assays in patients with systemic lupus erythematosus and other autoimmune systemic diseases. *Ann N Y Acad Sci* 2007; 1109:275-286.
16. Reveille JD. Predictive value of autoantibodies for activity of systemic lupus erythematosus. *Lupus JID* - 9204265 2004; 13(5):290-297.
17. Simon JA, Cabiedes J, Ortiz E, Alcocer-Varela J, Sanchez-Guerrero J. Anti-nucleosome antibodies in patients with systemic lupus erythematosus of recent onset. Potential utility as a diagnostic tool and disease activity marker. *Rheumatology (Oxford)* 2004; 43(2):220-224.
18. Sinclair D, Saas M, Williams D, Hart M, Goswami R. Can an ELISA replace immunofluorescence for the detection of anti-nuclear antibodies?--The routine use of anti-nuclear antibody screening ELISAs. *Clin Lab* 2007; 53(3-4):183-191.
19. Tozzoli R, Bizzaro N, Tonutti E, Villalta D, Bassetti D, Manoni F et al. Guidelines for the laboratory use of autoantibody tests in the diagnosis and monitoring of autoimmune rheumatic diseases. *Am J Clin Pathol* 2002; 117(2):316-324.
20. Moidhof W., Hiliak O. Lupus: an overview of the disease and management options. *P T* 2012; 37(4):240-9.
21. Hahn BH, McMahon MA, Wilkinson A, Wallace WD, Daikh DI, Fitzgerald JD et al. American College of Rheumatology guidelines for screening, treatment, and management of lupus nephritis. *Arthritis Care Res (Hoboken)* 2012; 64(6):797-808.

Notice to the user (European Union):

Any serious incident that has occurred in relation to the device shall be reported to the manufacturer and the

competent authority of the EU Member State in which the user and/or the patient is established .

Change Control

Former version: *ORG 512_IFU_EN_QM113139_2013-12-16_1.2* Reason for revision: *Introduction electronic IFU on homepage*

- 1 Pipet **100 µl** calibrator, control or patient sample
 - Incubate for **30 minutes** at room temperature
 - Discard the contents of the wells and wash 3 times with **300 µl** wash solution
- 2 Pipet **100 µl** enzyme conjugate
 - Incubate for **15 minutes** at room temperature
 - Discard the contents of the wells and wash 3 times with **300 µl** wash solution
- 3 Pipet **100 µl** substrate solution
 - Incubate for **15 minutes** at room temperature
- 4 Add **100 µl** stop solution
 - Leave untouched for **5 minutes**
 - Read at **450 nm**

ORGENTEC Diagnostika GmbH


Carl-Zeiss-Straße 49-51

55129 Mainz - Germany

Phone: +49 (0) 61 31 / 92 58-0

Fax: +49 (0) 61 31 / 92 58-58

Internet: www.orgentec.com



ORG 515 Anti-Cardiolipin IgG/IgM

INTENDED PURPOSE

Anti-Cardiolipin IgG/IgM is an ELISA test system for the quantitative measurement of IgG and IgM class autoantibodies against cardiolipin in human serum or plasma. This product is intended for professional in vitro diagnostic use only.

Antiphospholipid syndrome (APS, Hughes Syndrome) is a systemic autoimmune disease that causes thromboses, recurrent miscarriage or stillbirths, and stroke. Clinical symptoms are accompanied by specific autoantibodies in the blood, which bind to phospholipids like cardiolipin, or phospholipid-binding proteins like beta-2-glycoprotein I. Autoantibodies against proteins of the coagulation cascade, e.g. prothrombin or annexin V may also be found in patients with APS with otherwise negative phospholipid antibody results. In primary APS autoantibodies against phospholipids appear independently, while in secondary APS phospholipid antibodies are detected in conjunction with other autoimmune diseases, such as lupus erythematosus, rheumatoid arthritis, or Sjögren's syndrome.

SYMBOLS USED ON LABELS

In vitro diagnostic medical device

Manufacturer

Catalogue number

Sufficient for 96 determinations

Batch code

Use by

Temperature limitation

Keep away from sunlight

Do not reuse

Date of manufacture

CE marked according to 98/79/EC

Consult instructions for use

Electronic Instruction For Use: version

Microplate

Calibrator

Calibrator

Calibrator

Calibrator

Calibrator

Calibrator

Control positive

Control negative

Sample Buffer P

Enzyme Conjugate

Enzyme Conjugate

TMB Substrate

Stop solution

Wash Buffer

Ready to use

PRINCIPLE OF THE TEST

Highly purified cardiolipin is coated on microwells saturated with beta-2-glycoprotein I.

The determination is based on an indirect enzyme linked immune reaction with the following steps:

Specific antibodies in the patient sample bind to the antigen coated on the surface of the reaction wells. After incubation, a washing step removes unbound and unspecifically bound serum or plasma components. Subsequently added enzyme conjugate binds to the immobilized antibody-antigen-complexes. After incubation, a second washing step removes unbound enzyme conjugate. After addition of substrate solution the bound enzyme conjugate hydrolyses the substrate forming a blue coloured product. Addition of an acid stops the reaction generating a yellow end-product. The intensity of the yellow color correlates with the concentration of the antibody-antigen-complex and can be measured photometrically at 450 nm.

WARNINGS AND PRECAUTIONS


















- All reagents of this kit are intended for professional in vitro diagnostic use only.
- Components containing human serum were tested and found negative for HBsAg, HCV, HIV1 and HIV2 by FDA approved methods. No test can guarantee the absence of HBsAg, HCV, HIV1 or HIV2, and so all human serum based reagents in this kit must be handled as though capable of transmitting infection.
- Bovine serum albumin (BSA) used in components has been tested for BSE and found negative.
- Avoid contact with the substrate TMB (3,3',5,5'-Tetramethyl-benzidine).
- Stop solution contains acid, classification is non-hazardous. Avoid contact with skin.
- Control, sample buffer and wash buffer contain sodium azide 0.09% as preservative. This concentration is classified as non-hazardous.
- Enzyme conjugate contains ProClin 300 0.05% as preservative. This concentration is classified as non-hazardous.

During handling of all reagents, controls and serum samples observe the existing regulations for laboratory safety regulations and good laboratory practice:

- First aid measures: In case of skin contact, immediately wash thoroughly with water and soap. Remove contaminated clothing and shoes and wash before reuse. If system fluid comes into contact with skin, wash thoroughly with water. After contact with the eyes carefully rinse the opened eye with running water for at least 10 minutes. Get medical attention if necessary.
- Personal precautions, protective equipment and emergency procedures:
Observe laboratory safety regulations. Avoid contact with skin and eyes. Do not swallow. Do not pipette by mouth. Do not eat, drink, smoke or apply makeup in areas where specimens or kit reagents are handled. When spilled, absorb with an inert material and put the spilled material in an appropriate waste disposal.
- Exposure controls / personal protection: Wear protective gloves of nitril rubber or natural latex. Wear protective glasses. Used according to intended use no dangerous reactions known.
- Conditions to avoid: Since substrate solution is light-sensitive. Store in the dark.
- For disposal of laboratory waste the national or regional legislation has to be observed.

Observe the guidelines for performing quality control in medical laboratories by assaying control sera.

CONTENTS OF THE KIT

ORG 515		96	Sufficient for 96 determinations
	1		One divisible microplate consisting of 12 modules of 8 wells each. Ready to use. Product code on module: CLP
	1x 1.5 ml		Calibrator A 0 GPL-U/ml / 0 MPL-U/ml, containing serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
	1x 1.5 ml		Calibrator B 7.5 GPL-U/ml / 5 MPL-U/ml, containing Cardioliipin antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
	1x 1.5 ml		Calibrator C 15 GPL-U/ml / 10 MPL-U/ml, containing Cardioliipin antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
	1x 1.5 ml		Calibrator D 30 GPL-U/ml / 20 MPL-U/ml, containing Cardioliipin antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
	1x 1.5 ml		Calibrator E 60 GPL-U/ml / 40 MPL-U/ml, containing Cardioliipin antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
	1x 1.5 ml		Calibrator F 120 GPL-U/ml / 80 MPL-U/ml, containing Cardioliipin antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
	1x 1.5 ml		Control positive, containing cardioliipin antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use. The concentration is specified on the certificate of analysis.
	1x 1.5 ml		Control negative, containing cardioliipin antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use. The concentration is specified on the certificate of analysis.
	20 ml		Sample Buffer P; containing PBS, BSA, detergent, preservative sodium azide 0.09%, yellow, concentrate 5x.
	15 ml		Enzyme Conjugate IgG; containing anti-human IgG antibodies, HRP labelled; PBS, BSA, detergent, preservative PROCLIN 0.05%, light red. Ready to use.
	15 ml		Enzyme Conjugate IgM; containing anti-human IgM antibodies, HRP labelled; PBS, BSA, detergent, preservative PROCLIN 0.05%, light red. Ready to use.
	15 ml		TMB Substrate, containing 3,3', 5,5'- Tetramethylbenzidin. Ready to use.
	15 ml		Stop solution; contains acid. Ready to use.
	20 ml		Wash Buffer, containing Tris, detergent, preservative sodium azide 0.09%; 50 x conc.
	1		Certificate of Analysis

MATERIALS REQUIRED

- Microplate reader capable of endpoint measurements at 450 nm; optional: reference filter at 620 nm
- Data reduction software
- Multi-channel dispenser or repeatable pipette for 100 µl
- Vortex mixer
- Pipettes for 10 µl, 100 µl and 1000 µl
- Laboratory timing device
- Distilled or deionised water
- Measuring cylinder for 1000 ml and 100 ml
- Plastic container for storage of the wash solution

This ELISA assay is suitable for use on open automated ELISA processors. Each assay has to be validated on the respective automated system. Detailed information is provided upon request.

SPECIMEN COLLECTION, STORAGE AND HANDLING

- Collect whole blood specimens using acceptable medical techniques to avoid hemolysis.
- Allow blood to clot and separate the serum or plasma by centrifugation.
- Test serum should be clear and non-hemolyzed. Contamination by hemolysis or lipemia should be avoided, but does not interfere with this assay.
- Specimens may be refrigerated at 2-8°C for up to five days or stored at -20°C up to six months.
- Avoid repetitive freezing and thawing of serum or plasma samples. This may result in variable loss of antibody activity.
- Testing of heat-inactivated sera is not recommended.

STORAGE AND STABILITY

- Store test kit at 2-8°C in the dark.
- Do not expose reagents to heat, sun, or strong light during storage and usage.
- Store microplate sealed and desiccated in the clip bag provided.
- Shelf life of the unopened test kit is 18 months from day of production.
Unopened reagents are stable until expiration of the kit. See labels for individual batch.
- Diluted Wash Buffer and Sample Buffer are stable for at least 30 days when stored at 2-8°C.
We recommend consumption on the same day.

PROCEDURAL NOTES

- Do not use kit components beyond their expiration dates.
- Do not interchange kit components from different lots and products.
- All materials must be at room temperature (20-28°C) prior to use.
- Prepare all reagents and samples. Once started, perform the test without interruption.
- Double determinations may be done. By this means pipetting errors may become obvious.
- Perform the assay steps only in the order indicated.
- Always use fresh sample dilutions.
- Pipette all reagents and samples into the bottom of the wells.
- To avoid carryover or contamination, change the pipette tip between samples and different kit controls.
- Wash microwells thoroughly and remove the last droplets of wash buffer.
- All incubation steps must be accurately timed.
- Do not re-use microplate wells.

PREPARATION OF REAGENTS

WASH

Dilute the contents of one vial of the buffered wash solution concentrate (50x) with distilled or deionised water to a final volume of 1000 ml prior to use.

DILUENT

Sample Buffer P: Prior to use dilute the contents (20 ml) of one vial of sample buffer 5x concentrate with distilled or deionised water to a final volume of 100 ml.

Preparation of samples

Dilute patient samples 1:100 before the assay: Put 990 µl of prediluted sample buffer in a polystyrene tube and add 10 µl of sample. Mix well. Note: Calibrators / Controls are ready to use and need not be diluted.

TEST PROCEDURE

Prepare enough microplate modules for all calibrators / controls and patient samples.

- Pipette **100 µl** of calibrators, controls and prediluted patient samples into the wells.
Incubate for **30 minutes** at room temperature (20-28 °C).
Discard the contents of the microwells and **wash 3 times** with **300 µl** of wash solution.
- Dispense **100 µl** of enzyme conjugate into each well.
Incubate for **15 minutes** at room temperature.
Discard the contents of the microwells and **wash 3 times** with **300 µl** of wash solution.
- Dispense **100 µl** of TMB substrate solution into each well.
Incubate for **15 minutes** at room temperature
- Add 100 µl** of stop solution to each well of the modules
Incubate for **5 minutes** at room temperature.
Read the optical density at 450 nm (reference 600-690nm) and calculate the results.
The developed colour is stable for at least 30 minutes. Read during this time.

Example for a pipetting scheme:

	1	2	3	4	5	6	7	8	9	10	11	12
A	A	P1	A	P1								
B	B	P2	B	P2								
C	C	P3	C	P3								
D	D	P4	D	P4								
E	E	P5	E	P5								
F	F	P6	F	P6								
G	C+	P7	C+	P7								
H	C-	P8	C-	P8								

IgG IgG IgM IgM

P1, ... patient sample A-F calibrators C+, C- controls

VALIDATION

Test results are valid if the optical densities at 450 nm for calibrators / controls and the results for controls comply with the reference ranges indicated on the Certificate of Analysis enclosed in each test kit.

If these quality control criteria are not met the assay run is invalid and should be repeated.

CALCULATION OF RESULTS

For quantitative results plot the optical density of each calibrator versus the calibrator concentration to create a calibration curve. The concentration of patient samples may then be estimated from the calibration curve by interpolation.

Using data reduction software a 4-Parameter-Fit with lin-log coordinates for optical density and concentration is the data reduction method of choice.

PERFORMANCE CHARACTERISTICS

Calibration

The assay system is calibrated against the internationally recognised reference sera from E.N. Harris, Louisville and the specific reference material IRP 97/656 (IgG) and HCAL (IgG) / EY2C9 (IgM).

Measuring range

The calculation range of this ELISA assay is IgG: 0 - 120 GPL-U/ml IgM: 0 - 80 MPL-U/ml

Expected values

In a normal range study with samples from healthy blood donors the following ranges have been established with this ELISA assay: Cut-off IgG: 10 GPL-U/ml IgM: 7 MPL-U/ml

Interpretation of results

Negative: IgG < 10 GPL-U/ml IgM < 7 MPL-U/ml
Positive: ≥ 10 GPL-U/ml ≥ 7 MPL-U/ml

Linearity

Patient samples containing high levels of specific antibody were serially diluted in sample buffer to demonstrate the dynamic range of the assay and the upper / lower end of linearity. Activity for each dilution was calculated from the calibration curve using a 4-Parameter-Fit with lin-log coordinates.

Sample	Dilution Factor	Observed	Expected	O/E [%]
		GPL/MPL-U/ml	GPL/MPL-U/ml	
IgG 1	1	73.0	73.0	100
	2	37.1	36.5	102
	4	19.6	18.3	107
	8	10.9	9.1	120
IgG 2	1	80.5	80.5	100
	2	42.0	40.3	104
	4	22.2	20.1	111
	8	12.1	10.1	120
IgG 3	1	66.2	64.4	103
	2	34.5	32.2	107
	4	16.2	16.1	101
	8	8.1	8.1	101
IgM 1	1	70.9	70.9	100
	2	34.1	35.5	96
	4	18.2	17.7	103
	8	10.1	8.9	114
IgM 2	1	114.0	114.0	100
	2	50.6	57.0	89
	4	27.3	28.5	96
	8	14.8	14.3	104
IgM 3	1	48.2	48.2	100
	2	24.7	24.1	102
	4	12.7	12.1	105
	8	7.1	6.0	118

Limit of detection

Functional sensitivity was determined to be: IgG: 1 GPL-U/ml IgM: 0.5 MPL-U/ml

Reproducibility

Intra-assay precision: Coefficient of variation (CV) was calculated for each of three samples from the results of 24 determinations in a single run. Results for precision-within-assay are shown in the table below.

Inter-assay precision: Coefficient of variation (CV) was calculated for each of three samples from the results of 6 determinations in 5 different runs. Results for run-to-run precision are shown in the table below.

Intra-Assay IgG		
Sample	Mean GPL-U/ml	CV %
1	10.9	5.5
2	20.5	5.4
3	73.0	5.4

Inter-Assay IgG		
Sample	Mean GPL-U/ml	CV %
1	11.8	5.3
2	21.1	3.7
3	70.5	6.3

Intra-Assay IgM		
Sample	Mean MPL-U/ml	CV %
1	12.8	3.7
2	30.7	4.1
3	65.2	3.8

Inter-Assay IgM		
Sample	Mean MPL-U/ml	CV %
1	12.2	3.5
2	31.4	3.5
3	64.9	4.2

Interfering substances

No interference has been observed with haemolytic (up to 1000 mg/dl) or lipemic (up to 3 g/dl triglycerides) sera or plasma, or bilirubin (up to 40 mg/dl) containing sera or plasma. Nor have any interfering effects been observed with the use of anticoagulants (Citrate, EDTA, Heparine). However for practical reasons it is recommended that grossly hemolyzed or lipemic samples should be avoided.

Study results

Study population	n	Pos IgG	%	Pos IgM	%
Primary APS	8	6	75.0	4	50.0
Secondary APS	65	57	87.7	26	40.0
Normal human serum	150	6	4.0	3	2.0

		Clinical Diagnosis		
		POS	NEG	
ORG 515	POS	63	6	223
IgG	NEG	10	144	
		73	150	
Sensitivity:		86.3 %		
Specificity:		96.0 %		
Overall agreement:		92.8 %		

		Clinical Diagnosis		
		Pos	Neg	
ORG 515	Pos	30	3	223
IgM	Neg	43	147	
		73	150	
Sensitivity:		41.1 %		
Specificity:		98.0 %		
Overall agreement:		79.4 %		

LIMITATIONS OF THE PROCEDURE

This assay is a diagnostic aid. A definite clinical diagnosis should not be based on the results of a single test, but should be made by the physician after all clinical and laboratory findings have been evaluated concerning the entire clinical picture of the patient. Also every decision for therapy should be taken individually.

The above pathological and normal reference ranges for antibodies in patient samples should be regarded as recommendations only. Each laboratory should establish its own ranges according to ISO 15189 or other applicable laboratory guidelines.

REFERENCES

- Banzato A, Pozzi N, Frasson R, De F, V, Ruffatti A, Bison E et al. Antibodies to Domain I of beta(2)Glycoprotein I are in close relation to patients risk categories in Antiphospholipid Syndrome (APS). *Thromb Res* 2011; 128 (6):583-6.
- Bertolaccini ML, Amengual O, Atsumi T, Binder WL, de LB, Forastiero R et al. 'Non-criteria' aPL tests: report of a task force and preconference workshop at the 13th International Congress on Antiphospholipid Antibodies, Galveston, TX, USA, April 2010. *Lupus* 2011; 20(2):191-205.
- de Laat B, de Groot PG. Autoantibodies directed against domain I of beta2-glycoprotein I. *Curr Rheumatol Rep* 2011; 13(1):70-6.
- de Laat B, Mertens K, de Groot PG. Mechanisms of disease: antiphospholipid antibodies-from clinical association to pathologic mechanism. *Nat Clin Pract Rheumatol* 2008; 4(4):192-9.
- de Laat B, Pengo V, Pabinger I, Musial J, Voskuyl AE, Bultink IE et al. The association between circulating antibodies against domain I of beta2-glycoprotein I and thrombosis: an international multicenter study. *J Thromb Haemost* 2009; 7(11):1767-73.
- Espinosa G, Cervera R. Antiphospholipid syndrome. *Arthritis Res Ther* 2008; 10(6):230.
- Favaloro EJ, Wong RC. Laboratory testing for the antiphospholipid syndrome: making sense of antiphospholipid antibody assays. *Clin Chem Lab Med* 2011; 49(3):447-61.
- Fischer MJ, Rauch J, Levine JS. The antiphospholipid syndrome. *Arthritis Rheum* 2007; 27(1):35-46.
- Giannakopoulos B, Passam F, Ioannou Y, Krilis SA. How we diagnose the antiphospholipid syndrome. *Blood* 2009; 113(5):985-94.
- Greaves M, Cohen H, Machin SJ, Mackie I. Guidelines on the investigation and management of the antiphospholipid syndrome. *Br J Haematol* 2000; 109(4):704-15.
- Hughes GR. Hughes syndrome: antiphospholipid syndrome. *J R Coll Physicians Lond* 1998; 32(3):260-4.
- Hughes GR. Hughes Syndrome (the antiphospholipid syndrome): ten clinical lessons. *Autoimmun Rev* 2008; 7(3):262-6.
- Hughes GR. Antiphospholipid syndrome, migraine and stroke. *Lupus* 2010; 19(5):555-6.
- Hughes GR, Harris NN, Gharavi AE. The anticardiolipin syndrome. *J Rheumatol* 1986; 13(3):486-9.

- Koike T, Bohgaki M, Amengual O, Atsumi T. Antiphospholipid antibodies: lessons from the bench. *J Autoimmun* 2007; 28(2-3):129-33.
- Lakos G, Favaloro EJ, Harris EN, Meroni PL, Tincani A, Wong RC et al. International consensus guidelines on anticardiolipin and anti-beta2-glycoprotein I testing: report from the 13th International Congress on Antiphospholipid Antibodies. *Arthritis Rheum* 2012; 64(1):1-10.
- Mackworth-Young C. Primary antiphospholipid syndrome: a distinct entity? *Autoimmun Rev* 2006; 5(1):70-5.
- Miyakis S, Lockshin MD, Atsumi T, Branch DW, Brey RL, Cervera R et al. International consensus statement on an update of the classification criteria for definite antiphospholipid syndrome (APS). *J Thromb Haemost* 2006; 4(2):295-306.
- Molina JF, Gutierrez-Urena S, Molina J, Uribe O, Richards S, De CC et al. Variability of anticardiolipin antibody isotype distribution in 3 geographic populations of patients with systemic lupus erythematosus. *J Rheumatol* 1997; 24(2):291-6.
- Oku K, Atsumi T, Amengual O, Koike T. Antiprothrombin antibody testing: detection and clinical utility. *Semin Thromb Hemost* 2008; 34(4):335-9.
- Pengo V, Biasiolo A, Bison E, Chantarangkul V, Tripodi A. Antiphospholipid antibody ELISAs: survey on the performance of clinical laboratories assessed by using lyophilized affinity-purified IgG with anticardiolipin and anti-beta2-Glycoprotein I activity. *Thromb Res* 2007; 120(1):127-33.
- Pierangeli SS, de Groot PG, Dlott J, Favaloro E, Harris EN, Lakos G et al. 'Criteria' aPL tests: report of a task force and preconference workshop at the 13th International Congress on Antiphospholipid Antibodies, Galveston, Texas, April 2010. *Lupus* 2011; 20(2):182-90.
- Pierangeli SS, Favaloro EJ, Lakos G, Meroni PL, Tincani A, Wong RC et al. Standards and reference materials for the anticardiolipin and anti-beta-2-glycoprotein I assays: a report of recommendations from the APL Task Force at the 13th International Congress on Antiphospholipid Antibodies. *Clin Chim Acta* 2012; 413(1-2):358-60.
- Sinico RA, Bollini B, Sabadini E, Di Toma L, Radice A. The use of laboratory tests in diagnosis and monitoring of systemic lupus erythematosus. *J Nephrol JID - 9012268* 2002; 15 Suppl 6:S20-S27.
- Tincani A, Andreoli L, Casu C, Cattaneo R, Meroni P. Antiphospholipid antibody profile: implications for the evaluation and management of patients. *Lupus* 2010; 19(4):432-5.
- Tincani A, Morozzi G, Afeltra A, Alessandri C, Allegri F, Bistoni O et al. Antiprothrombin antibodies: a comparative analysis of homemade and commercial methods. A collaborative study by the Forum Interdisciplinare per la Ricerca nelle Malattie Autoimmuni (FIRMA). *Clin Exp Rheumatol* 2007; 25(2):268-74.
- Wilson WA, Gharavi AE, Koike T, Lockshin MD, Branch DW, Piette JC et al. International consensus statement on preliminary classification criteria for definite antiphospholipid syndrome: report of an international workshop. *Arthritis Rheum* 1999; 42(7):1309-11.
- Wong RC, Favaloro EJ, Adelstein S, Baumgart K, Bird R, Brighton TA et al. Consensus guidelines on anti-beta 2 glycoprotein I testing and reporting. *Pathology* 2008; 40(1):58-63.
- Wong RC, Gillis D, Adelstein S, Baumgart K, Favaloro EJ, Hendle MJ et al. Consensus guidelines on anticardiolipin antibody testing and reporting. *Pathology* 2004; 36(1):63-8.

Notice to the user (European Union):

Any serious incident that has occurred in relation to the device shall be reported to the manufacturer and the competent authority of the EU Member State in which the user and/or the patient is established .

Change Control

Former version: *ORG 515_IFU_EN_QM113142_2016-04-18_2*

Reason for revision: *Introduction electronic IFU on homepage*

- 1 Pipet **100 µl** calibrator, control or patient sample
 - Incubate for **30 minutes** at room temperature
 - Discard the contents of the wells and wash 3 times with **300 µl** wash solution
- 2 Pipet **100 µl** enzyme conjugate
 - Incubate for **15 minutes** at room temperature
 - Discard the contents of the wells and wash 3 times with **300 µl** wash solution
- 3 Pipet **100 µl** substrate solution
 - Incubate for **15 minutes** at room temperature
- 4 Add **100 µl** stop solution
 - Leave untouched for **5 minutes**
 - Read at **450 nm**

ORGENTEC Diagnostika GmbH


Carl-Zeiss-Straße 49-51

55129 Mainz - Germany

Phone: +49 (0) 61 31 / 92 58-0

Fax: +49 (0) 61 31 / 92 58-58

Internet: www.orgentec.com



ORG 529 Anti-Phospholipid Screen IgG/IgM

INTENDED PURPOSE

Anti-Phospholipid Screen IgG/IgM is an ELISA test system to screen for the presence of IgG and IgM class autoantibodies against cardiolipin, phosphatidyl serine, phosphatidyl inositol, phosphatidic acid and beta-2-glycoprotein I in human serum or plasma. This product is intended for professional in vitro diagnostic use only.

Antiphospholipid syndrome (APS, Hughes Syndrome) is a systemic autoimmune disease that causes thromboses, recurrent miscarriage or stillbirths, and stroke. Clinical symptoms are accompanied by specific autoantibodies in the blood, which bind to phospholipids like cardiolipin, or phospholipid-binding proteins like beta-2-glycoprotein I. Autoantibodies against proteins of the coagulation cascade, e.g. prothrombin or annexin V may also be found in patients with APS with otherwise negative phospholipid antibody results. In primary APS autoantibodies against phospholipids appear independently, while in secondary APS phospholipid antibodies are detected in conjunction with other autoimmune diseases, such as lupus erythematosus, rheumatoid arthritis, or Sjögren's syndrome.

SYMBOLS USED ON LABELS

In vitro diagnostic medical device

Manufacturer

Catalogue number

Sufficient for 96 determinations

Batch code

Use by

Temperature limitation

Keep away from sunlight

Do not reuse

Date of manufacture

CE marked according to 98/79/EC

Consult instructions for use

Electronic Instruction For Use: version

Microplate

Calibrator

Calibrator

Calibrator

Calibrator

Calibrator

Calibrator

Control positive

Control negative

Sample Buffer P

Enzyme Conjugate

Enzyme Conjugate

TMB Substrate

Stop solution

Wash Buffer

Ready to use

PRINCIPLE OF THE TEST

A mixture of highly purified cardiolipin, phosphatidyl serine, phosphatidyl inositol, phosphatidic acid and human beta-2-Glycoprotein I is bound to microwells.

The determination is based on an indirect enzyme linked immune reaction with the following steps:

Specific antibodies in the patient sample bind to the antigen coated on the surface of the reaction wells. After incubation, a washing step removes unbound and unspecifically bound serum or plasma components. Subsequently added enzyme conjugate binds to the immobilized antibody-antigen-complexes. After incubation, a second washing step removes unbound enzyme conjugate. After addition of substrate solution the bound enzyme conjugate hydrolyses the substrate forming a blue coloured product. Addition of an acid stops the reaction generating a yellow end-product. The intensity of the yellow color correlates with the concentration of the antibody-antigen-complex and can be measured photometrically at 450 nm.

WARNINGS AND PRECAUTIONS

- All reagents of this kit are intended for professional in vitro diagnostic use only.
- Components containing human serum were tested and found negative for HBsAg, HCV, HIV1 and HIV2 by FDA approved methods. No test can guarantee the absence of HBsAg, HCV, HIV1 or HIV2, and so all human serum based reagents in this kit must be handled as though capable of transmitting infection.
- Bovine serum albumin (BSA) used in components has been tested for BSE and found negative.
- Avoid contact with the substrate TMB (3,3',5,5'-Tetramethyl-benzidine).
- Stop solution contains acid, classification is non-hazardous. Avoid contact with skin.
- Control, sample buffer and wash buffer contain sodium azide 0.09% as preservative. This concentration is classified as non-hazardous.
- Enzyme conjugate contains ProClin 300 0.05% as preservative. This concentration is classified as non-hazardous.

During handling of all reagents, controls and serum samples observe the existing regulations for laboratory safety regulations and good laboratory practice:

- First aid measures: In case of skin contact, immediately wash thoroughly with water and soap. Remove contaminated clothing and shoes and wash before reuse. If system fluid comes into contact with skin, wash thoroughly with water. After contact with the eyes carefully rinse the opened eye with running water for at least 10 minutes. Get medical attention if necessary.
- Personal precautions, protective equipment and emergency procedures: Observe laboratory safety regulations. Avoid contact with skin and eyes. Do not swallow. Do not pipette by mouth. Do not eat, drink, smoke or apply makeup in areas where specimens or kit reagents are handled. When spilled, absorb with an inert material and put the spilled material in an appropriate waste disposal.
- Exposure controls / personal protection: Wear protective gloves of nitril rubber or natural latex. Wear protective glasses. Used according to intended use no dangerous reactions known.
- Conditions to avoid: Since substrate solution is light-sensitive. Store in the dark.
- For disposal of laboratory waste the national or regional legislation has to be observed.

Observe the guidelines for performing quality control in medical laboratories by assaying control sera.

CONTENTS OF THE KIT

ORG 529	▽ 96	Sufficient for 96 determinations
MICROPLATE	1	One divisible microplate consisting of 12 modules of 8 wells each. Ready to use. Product code on module: PSC
CALIBRATOR A	1x 1.5 ml	Calibrator A 0 GPL-U/ml / 0 MPL-U/ml, containing serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
CALIBRATOR B	1x 1.5 ml	Calibrator B 6.3 GPL-U/ml / 6.3 MPL-U/ml, containing phospholipid antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
CALIBRATOR C	1x 1.5 ml	Calibrator C 12.5 GPL-U/ml / 12.5 MPL-U/ml, containing phospholipid antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
CALIBRATOR D	1x 1.5 ml	Calibrator D 25 GPL-U/ml / 25 MPL-U/ml, containing phospholipid antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
CALIBRATOR E	1x 1.5 ml	Calibrator E 50 GPL-U/ml / 50 MPL-U/ml, containing phospholipid antibodies in a serum/buffer matrix (PBS, BSA, NaN3 0.09%), yellow. Ready to use.
CALIBRATOR F	1x 1.5 ml	Calibrator F 100 GPL-U/ml / 100 MPL-U/ml, containing phospholipid antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
CONTROL +	1x 1.5 ml	Control positive, containing phospholipid antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use. The concentration is specified on the certificate of analysis.
CONTROL -	1x 1.5 ml	Control negative, containing phospholipid antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use. The concentration is specified on the certificate of analysis.
DILUENT	20 ml	Sample Buffer P, containing PBS, BSA, detergent, preservative sodium azide 0.09%, yellow, concentrate (5 x).
CONJUGATE G	15 ml	Enzyme Conjugate; containing anti-human IgG antibodies, HRP labelled; PBS, BSA, detergent, preservative PROCLIN 0.05%, light red. Ready to use.
CONJUGATE M	15 ml	Enzyme Conjugate; containing anti-human IgM antibodies, HRP labelled; PBS, BSA, detergent, preservative PROCLIN 0.05%, light red. Ready to use.
TMB	15 ml	TMB Substrate; containing 3,3', 5,5'- Tetramethylbenzidin, colorless. Ready to use.
STOP	15 ml	Stop solution; contains acid. Ready to use.
WASH	20 ml	Wash Buffer, containing Tris, detergent, preservative sodium azide 0.09%; 50 x concn.
i	1	Certificate of Analysis

MATERIALS REQUIRED

- Microplate reader capable of endpoint measurements at 450 nm; optional: reference filter at 620 nm
- Data reduction software
- Multi-channel dispenser or repeatable pipette for 100 µl
- Vortex mixer
- Pipettes for 10 µl, 100 µl and 1000 µl
- Laboratory timing device
- Distilled or deionised water
- Measuring cylinder for 1000 ml and 100 ml
- Plastic container for storage of the wash solution

This ELISA assay is suitable for use on open automated ELISA processors. Each assay has to be validated on the respective automated system. Detailed information is provided upon request.

SPECIMEN COLLECTION, STORAGE AND HANDLING

- Collect whole blood specimens using acceptable medical techniques to avoid hemolysis.
- Allow blood to clot and separate the serum or plasma by centrifugation.
- Test serum should be clear and non-hemolyzed. Contamination by hemolysis or lipemia should be avoided, but does not interfere with this assay.
- Specimens may be refrigerated at 2-8°C for up to five days or stored at -20°C up to six months.
- Avoid repetitive freezing and thawing of serum or plasma samples. This may result in variable loss of antibody activity.
- Testing of heat-inactivated sera is not recommended.

STORAGE AND STABILITY

- Store test kit at 2-8°C in the dark.
- Do not expose reagents to heat, sun, or strong light during storage and usage.
- Store microplate sealed and desiccated in the clip bag provided.
- Shelf life of the unopened test kit is 18 months from day of production.
Unopened reagents are stable until expiration of the kit. See labels for individual batch.
- Diluted Wash Buffer and Sample Buffer are stable for at least 30 days when stored at 2-8°C.
We recommend consumption on the same day.

PROCEDURAL NOTES

- Do not use kit components beyond their expiration dates.
- Do not interchange kit components from different lots and products.
- All materials must be at room temperature (20-28°C) prior to use.
- Prepare all reagents and samples. Once started, perform the test without interruption.
- Double determinations may be done. By this means pipetting errors may become obvious.
- Perform the assay steps only in the order indicated.
- Always use fresh sample dilutions.
- Pipette all reagents and samples into the bottom of the wells.
- To avoid carryover or contamination, change the pipette tip between samples and different kit controls.
- Wash microwells thoroughly and remove the last droplets of wash buffer.
- All incubation steps must be accurately timed.
- Do not re-use microplate wells.

PREPARATION OF REAGENTS

WASH

Dilute the contents of one vial of the buffered wash solution concentrate (50x) with distilled or deionised water to a final volume of 1000 ml prior to use.

DILUENT

Sample Buffer P: Prior to use dilute the contents (20 ml) of one vial of sample buffer 5x concentrate with distilled or deionised water to a final volume of 100 ml.

Preparation of samples

Dilute patient samples 1:100 before the assay: Put 990 µl of prediluted sample buffer in a polystyrene tube and add 10 µl of sample. Mix well. Note: Calibrators / Controls are ready to use and need not be diluted.

TEST PROCEDURE

Prepare enough microplate modules for all calibrators / controls and patient samples.

- Pipette **100 µl** of calibrators, controls and prediluted patient samples into the wells.
Incubate for **30 minutes** at room temperature (20-28 °C).
Discard the contents of the microwells and **wash 3 times** with **300 µl** of wash solution.
- Dispense **100 µl** of enzyme conjugate into each well.
Incubate for **15 minutes** at room temperature.
Discard the contents of the microwells and **wash 3 times** with **300 µl** of wash solution.
- Dispense **100 µl** of TMB substrate solution into each well.
Incubate for **15 minutes** at room temperature
- Add 100 µl** of stop solution to each well of the modules
Incubate for **5 minutes** at room temperature.
Read the optical density at 450 nm (reference 600-690nm) and calculate the results.
The developed colour is stable for at least 30 minutes. Read during this time.

Example for a pipetting scheme:

	1	2	3	4	5	6	7	8	9	10	11	12
A	A	P1	A	P1								
B	B	P2	B	P2								
C	C	P3	C	P3								
D	D	P4	D	P4								
E	E	P5	E	P5								
F	F	P6	F	P6								
G	C+	P7	C+	P7								
H	C-	P8	C-	P8								
	IgG	IgG	IgM	IgM								

P1, ... patient sample A-F calibrators C+, C- controls

VALIDATION

Test results are valid if the optical densities at 450 nm for calibrators / controls and the results for controls comply with the reference ranges indicated on the Certificate of Analysis enclosed in each test kit.

If these quality control criteria are not met the assay run is invalid and should be repeated.

CALCULATION OF RESULTS

For quantitative results plot the optical density of each calibrator versus the calibrator concentration to create a calibration curve. The concentration of patient samples may then be estimated from the calibration curve by interpolation.

Using data reduction software a 4-Parameter-Fit with lin-log coordinates for optical density and concentration is the data reduction method of choice.

PERFORMANCE CHARACTERISTICS

Calibration

Calibration is related to the internationally recognised reference sera from E.N. Harris, Louisville and to IRP 97/656 (IgG) and HCAL (IgG) / EY2C9 (IgM).

Measuring range

The calculation range of this ELISA assay is IgG: 0 - 100 GPL-U/ml IgM: 0 - 100 MPL-U/ml

Expected values

In a normal range study with samples from healthy blood donors the following ranges have been established with this ELISA assay: Cut-off IgG: 10 GPL-U/ml IgM: 10 MPL-U/ml

Interpretation of results

Negative: IgG < 10 GPL-U/ml IgM < 10 MPL-U/ml
Positive: ≥ 10 GPL-U/ml ≥ 10 MPL-U/ml

Linearity

Patient samples containing high levels of specific antibody were serially diluted in sample buffer to demonstrate the dynamic range of the assay and the upper / lower end of linearity. Activity for each dilution was calculated from the calibration curve using a 4-Parameter-Fit with lin-log coordinates.

Sample	Dilution	Observed GPL/MPL-U/ml	Expected GPL/MPL-U/ml	O/E [%]
IgG 1	1:100	98.0	98.4	100
	1:200	49.6	49.2	101
	1:400	24.3	24.6	99
	1:800	12.0	12.3	98
IgG 2	1:1600	5.8	6.2	94
	1:100	92.4	92.4	100
	1:200	45.9	46.2	99
	1:400	22.7	23.1	98
IgM 1	1:800	11.4	11.6	99
	1:1600	5.4	5.8	94
	1:100	92.7	92.7	100
	1:200	45.7	46.4	99
IgM 2	1:400	22.8	23.2	98
	1:800	11.2	11.6	97
	1:1600	5.4	5.8	93
	1:100	72.4	74.2	100
IgM 2	1:200	36.5	37.1	98
	1:400	18.7	18.6	101
	1:800	8.9	9.3	96
	1:1600	4.4	4.6	95

Limit of detection

Functional sensitivity was determined to be: IgG: 0.5 GPL-U/ml IgM: 0.5 MPL-U/ml

Reproducibility

Intra-assay precision: Coefficient of variation (CV) was calculated for each of three samples from the results of 24 determinations in a single run. Results for precision-within-assay are shown in the table below.

Inter-assay precision: Coefficient of variation (CV) was calculated for each of three samples from the results of 6 determinations in 5 different runs. Results for run-to-run precision are shown in the table below.

Intra-Assay IgG		
Sample	Mean GPL-U/ml	CV %
1	10.4	5.1
2	18.7	3.4
3	59.9	5.2

Inter-Assay IgG		
Sample	Mean GPL-U/ml	CV %
1	10.0	3.6
2	17.7	5.4
3	57.9	4.9

Intra-Assay IgM		
Sample	Mean MPL-U/ml	CV %
1	12.8	4.1
2	30.8	3.5
3	63.8	3.7

Inter-Assay IgM		
Sample	Mean MPL-U/ml	CV %
1	12.6	5.3
2	31.9	4.1
3	62.1	4.2

Interfering substances

No interference has been observed with haemolytic (up to 1000 mg/dl) or lipemic (up to 3 g/dl triglycerides) sera or plasma, or bilirubin (up to 40 mg/dl) containing sera or plasma. Nor have any interfering effects been observed with the use of anticoagulants (Citrate, EDTA, Heparine). However for practical reasons it is recommended that grossly hemolyzed or lipemic samples should be avoided.

Study results

Study population	n	Pos IgG	%	Pos IgM	%
Primary APS	8	7	87.5	6	75.0
Secondary APS	65	60	92.3	33	50.8
Normal human sera	150	4	2.7	5	3.3

		Clinical Diagnosis		
		POS	NEG	
ORG 529	POS	67	4	223
IgG	NEG	6	146	
		73	150	
Sensitivity:		91.8 %		
Specificity:		97.3 %		
Overall agreement:		95.5 %		

		Clinical Diagnosis		
		Pos	Neg	
ORG 529	Pos	39	5	223
IgM	Neg	34	145	
		73	150	
Sensitivity:		53.4 %		
Specificity:		96.7 %		
Overall agreement:		82.5 %		

LIMITATIONS OF THE PROCEDURE

This assay is a diagnostic aid. A definite clinical diagnosis should not be based on the results of a single test, but should be made by the physician after all clinical and laboratory findings have been evaluated concerning the entire clinical picture of the patient. Also every decision for therapy should be taken individually.

The above pathological and normal reference ranges for antibodies in patient samples should be regarded as recommendations only. Each laboratory should establish its own ranges according to ISO 15189 or other applicable laboratory guidelines.

REFERENCES

- Banzato A, Pozzi N, Frasson R, De F, V, Ruffatti A, Bison E et al. Antibodies to Domain I of beta(2)Glycoprotein I are in close relation to patients risk categories in Antiphospholipid Syndrome (APS). *Thromb Res* 2011; 128 (6):583-6.
- Bertolaccini ML, Amengual O, Atsumi T, Binder WL, de LB, Forastiero R et al. 'Non-criteria' aPL tests: report of a task force and preconference workshop at the 13th International Congress on Antiphospholipid Antibodies, Galveston, TX, USA, April 2010. *Lupus* 2011; 20(2):191-205.
- de Laat B, de Groot PG. Autoantibodies directed against domain I of beta2-glycoprotein I. *Curr Rheumatol Rep* 2011; 13(1):70-6.
- de Laat B, Mertens K, de Groot PG. Mechanisms of disease: antiphospholipid antibodies-from clinical association to pathologic mechanism. *Nat Clin Pract Rheumatol* 2008; 4(4):192-9.
- de Laat B, Pengo V, Pabinger I, Musial J, Voskuyl AE, Bultink IE et al. The association between circulating antibodies against domain I of beta2-glycoprotein I and thrombosis: an international multicenter study. *J Thromb Haemost* 2009; 7(11):1767-73.
- Espinosa G, Cervera R. Antiphospholipid syndrome. *Arthritis Res Ther* 2008; 10(6):230.
- Favaloro EJ, Wong RC. Laboratory testing for the antiphospholipid syndrome: making sense of antiphospholipid antibody assays. *Clin Chem Lab Med* 2011; 49(3):447-61.
- Fischer MJ, Rauch J, Levine JS. The antiphospholipid syndrome. *Arthritis Rheum* 2007; 27(1):35-46.
- Giannakopoulos B, Passam F, Ioannou Y, Krilis SA. How we diagnose the antiphospholipid syndrome. *Blood* 2009; 113(5):985-94.
- Greaves M, Cohen H, Machin SJ, Mackie I. Guidelines on the investigation and management of the antiphospholipid syndrome. *Br J Haematol* 2000; 109(4):704-15.
- Hughes GR. Hughes syndrome: antiphospholipid syndrome. *J R Coll Physicians Lond* 1998; 32(3):260-4.
- Hughes GR. Hughes Syndrome (the antiphospholipid syndrome): ten clinical lessons. *Autoimmun Rev* 2008; 7(3):262-6.
- Hughes GR. Antiphospholipid syndrome, migraine and stroke. *Lupus* 2010; 19(5):555-6.
- Hughes GR, Harris NN, Gharavi AE. The anticardiolipin syndrome. *J Rheumatol* 1986; 13(3):486-9.
- Koike T, Bohgaki M, Amengual O, Atsumi T. Antiphospholipid antibodies: lessons from the bench. *J Autoimmun* 2007; 28(2-3):129-33.
- Lakos G, Favaloro EJ, Harris EN, Meroni PL, Tincani A, Wong RC et al. International consensus guidelines on anticardiolipin and anti-beta2-glycoprotein I testing: report from the 13th International Congress on Antiphospholipid Antibodies. *Arthritis Rheum* 2012; 64(1):1-10.
- Mackworth-Young C. Primary antiphospholipid syndrome: a distinct entity? *Autoimmun Rev* 2006; 5(1):70-5.

- Miyakis S, Lockshin MD, Atsumi T, Branch DW, Brey RL, Cervera R et al. International consensus statement on an update of the classification criteria for definite antiphospholipid syndrome (APS). *J Thromb Haemost* 2006; 4(2):295-306.
- Molina JF, Gutierrez-Urena S, Molina J, Uribe O, Richards S, De CC et al. Variability of anticardiolipin antibody isotype distribution in 3 geographic populations of patients with systemic lupus erythematosus. *J Rheumatol* 1997; 24(2):291-6.
- Oku K, Atsumi T, Amengual O, Koike T. Antiprothrombin antibody testing: detection and clinical utility. *Semin Thromb Hemost* 2008; 34(4):335-9.
- Pengo V, Biasiolo A, Bison E, Chantarangkul V, Tripodi A. Antiphospholipid antibody ELISAs: survey on the performance of clinical laboratories assessed by using lyophilized affinity-purified IgG with anticardiolipin and anti-beta2-Glycoprotein I activity. *Thromb Res* 2007; 120(1):127-33.
- Pierangeli SS, de Groot PG, Dlott J, Favaloro E, Harris EN, Lakos G et al. 'Criteria' aPL tests: report of a task force and preconference workshop at the 13th International Congress on Antiphospholipid Antibodies, Galveston, Texas, April 2010. *Lupus* 2011; 20(2):182-90.
- Pierangeli SS, Favaloro EJ, Lakos G, Meroni PL, Tincani A, Wong RC et al. Standards and reference materials for the anticardiolipin and anti-beta-2-glycoprotein I assays: a report of recommendations from the APL Task Force at the 13th International Congress on Antiphospholipid Antibodies. *Clin Chim Acta* 2012; 413(1-2):358-60.
- Sinico RA, Bollini B, Sabadini E, Di Toma L, Radice A. The use of laboratory tests in diagnosis and monitoring of systemic lupus erythematosus. *J Nephrol JID* - 9012268 2002; 15 Suppl 6:S20-S27.
- Tincani A, Andreoli L, Casu C, Cattaneo R, Meroni P. Antiphospholipid antibody profile: implications for the evaluation and management of patients. *Lupus* 2010; 19(4):432-5.
- Tincani A, Morozzi G, Afeltra A, Alessandri C, Allegri F, Bistoni O et al. Antiprothrombin antibodies: a comparative analysis of homemade and commercial methods. A collaborative study by the Forum Interdisciplinare per la Ricerca nelle Malattie Autoimmuni (FIRMA). *Clin Exp Rheumatol* 2007; 25(2):268-74.
- Wilson WA, Gharavi AE, Koike T, Lockshin MD, Branch DW, Piette JC et al. International consensus statement on preliminary classification criteria for definite antiphospholipid syndrome: report of an international workshop. *Arthritis Rheum* 1999; 42(7):1309-11.
- Wong RC, Favaloro EJ, Adelstein S, Baumgart K, Bird R, Brighton TA et al. Consensus guidelines on anti-beta 2 glycoprotein I testing and reporting. *Pathology* 2008; 40(1):58-63.
- Wong RC, Gillis D, Adelstein S, Baumgart K, Favaloro EJ, Hendle MJ et al. Consensus guidelines on anticardiolipin antibody testing and reporting. *Pathology* 2004; 36(1):63-8.

Notice to the user (European Union):

Any serious incident that has occurred in relation to the device shall be reported to the manufacturer and the competent authority of the EU Member State in which the user and/or the patient is established .

Change Control

Former version: ORG 529_IFU_EN_QM113163_2016-04-18_3

Reason for revision: Introduction electronic IFU on homepage

- 1** Pipet **100 µl** calibrator, control or patient sample
→ Incubate for **30 minutes** at room temperature
→ Discard the contents of the wells and wash 3 times with **300 µl** wash solution
- 2** Pipet **100 µl** enzyme conjugate
→ Incubate for **15 minutes** at room temperature
→ Discard the contents of the wells and wash 3 times with **300 µl** wash solution
- 3** Pipet **100 µl** substrate solution
→ Incubate for **15 minutes** at room temperature
- 4** Add **100 µl** stop solution
→ Leave untouched for **5 minutes**
→ Read at **450 nm**

ORGENTEC Diagnostika GmbH


Carl-Zeiss-Straße 49-51

55129 Mainz - Germany

Phone: +49 (0) 61 31 / 92 58-0

Fax: +49 (0) 61 31 / 92 58-58

Internet: www.orgentec.com



ORG 516 AMA-M2

INTENDED PURPOSE

AMA-M2 is an ELISA test system for the quantitative measurement of IgG class autoantibodies against mitochondrial M2 subtype antigen in human serum or plasma. This product is intended for professional in vitro diagnostic use only.

The test is used as an aid in the differential diagnosis of primary biliary cirrhosis (PBC). In patients with other autoimmune diseases occurrence of AMA antibodies may be related to the development or association of PBC. Evaluation of a test result should always take into account all clinical and laboratory diagnostic findings.

SYMBOLS USED ON LABELS

	In vitro diagnostic medical device		Microplate
	Manufacturer		Calibrator
	Catalogue number		Calibrator
	Sufficient for 96 determinations		Calibrator
	Batch code		Calibrator
	Use by		Calibrator
	Temperature limitation		Calibrator
	Keep away from sunlight		Control positive
	Do not reuse		Control negative
	Date of manufacture		Sample Buffer P
	CE marked according to 98/79/EC		Enzyme Conjugate
	Consult instructions for use		TMB Substrate
	Electronic Instruction For Use: version		Stop solution
			Wash Buffer
			Ready to use



PRINCIPLE OF THE TEST

Highly purified mitochondrial M2 subtype (PDC-E2, BCOADC-E2, OGDC-E2) antigen is bound to microwells. The determination is based on an indirect enzyme linked immune reaction with the following steps: Specific antibodies in the patient sample bind to the antigen coated on the surface of the reaction wells. After incubation, a washing step removes unbound and unspecifically bound serum or plasma components. Subsequently added enzyme conjugate binds to the immobilized antibody-antigen-complexes. After incubation, a second washing step removes unbound enzyme conjugate. After addition of substrate solution the bound enzyme conjugate hydrolyses the substrate forming a blue coloured product. Addition of an acid stops the reaction generating a yellow end-product. The intensity of the yellow color correlates with the concentration of the antibody-antigen-complex and can be measured photometrically at 450 nm.

WARNINGS AND PRECAUTIONS

- All reagents of this kit are intended for professional in vitro diagnostic use only.
 - Components containing human serum were tested and found negative for HBsAg, HCV, HIV1 and HIV2 by FDA approved methods. No test can guarantee the absence of HBsAg, HCV, HIV1 or HIV2, and so all human serum based reagents in this kit must be handled as though capable of transmitting infection.
 - Bovine serum albumin (BSA) used in components has been tested for BSE and found negative.
 - Avoid contact with the substrate TMB (3,3',5,5'-Tetramethyl-benzidine).
 - Stop solution contains acid, classification is non-hazardous. Avoid contact with skin.
 - Control, sample buffer and wash buffer contain sodium azide 0.09% as preservative. This concentration is classified as non-hazardous.
 - Enzyme conjugate contains ProClin 300 0.05% as preservative. This concentration is classified as non-hazardous.
- During handling of all reagents, controls and serum samples observe the existing regulations for laboratory safety regulations and good laboratory practice:
- First aid measures: In case of skin contact, immediately wash thoroughly with water and soap. Remove contaminated clothing and shoes and wash before reuse. If system fluid comes into contact with skin, wash thoroughly with water. After contact with the eyes carefully rinse the opened eye with running water for at least 10 minutes. Get medical attention if necessary.
 - Personal precautions, protective equipment and emergency procedures:
Observe laboratory safety regulations. Avoid contact with skin and eyes. Do not swallow. Do not pipette by mouth. Do not eat, drink, smoke or apply makeup in areas where specimens or kit reagents are handled. When spilled, absorb with an inert material and put the spilled material in an appropriate waste disposal.
 - Exposure controls / personal protection: Wear protective gloves of nitril rubber or natural latex. Wear protective glasses. Used according to intended use no dangerous reactions known.
 - Conditions to avoid: Since substrate solution is light-sensitive. Store in the dark.
 - For disposal of laboratory waste the national or regional legislation has to be observed.
- Observe the guidelines for performing quality control in medical laboratories by assaying control sera.

CONTENTS OF THE KIT

ORG 516		Sufficient for 96 determinations
MICROPLATE	1	One divisible microplate consisting of 12 modules of 8 wells each. Ready to use. Product code on module: AMA
CALIBRATOR A	1x 1.5 ml	Calibrator A 0 IU/ml, containing serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
CALIBRATOR B	1x 1.5 ml	Calibrator B 12.5 IU/ml, containing AMA-M2 antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
CALIBRATOR C	1x 1.5 ml	Calibrator C 25 IU/ml, containing AMA-M2 antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
CALIBRATOR D	1x 1.5 ml	Calibrator D 50 IU/ml, containing AMA-M2 antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
CALIBRATOR E	1x 1.5 ml	Calibrator E 100 IU/ml, containing AMA-M2 antibodies in a serum/buffer matrix (PBS, BSA, NaN3 0.09%), yellow. Ready to use.
CALIBRATOR F	1x 1.5 ml	Calibrator F 200 IU/ml, containing AMA-M2 antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
CONTROL +	1x 1.5 ml	Control positive, containing AMA-M2 antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use. The concentration is specified on the certificate of analysis.
CONTROL -	1x 1.5 ml	Control negative, containing AMA-M2 antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use. The concentration is specified on the certificate of analysis.
DILUENT	20 ml	Sample Buffer P, containing PBS, BSA, detergent, preservative sodium azide 0.09%, yellow, concentrate (5 x).
CONJUGATE	15 ml	Enzyme Conjugate containing anti-human IgG antibodies, HRP labelled; PBS, BSA, detergent, preservative PROCLIN 0.05%, light red. Ready to use.
TMB	15 ml	TMB Substrate; containing 3,3', 5,5'- Tetramethylbenzidin, colorless. Ready to use.
STOP	15 ml	Stop solution; contains acid. Ready to use.
WASH	20 ml	Wash Buffer, containing Tris, detergent, preservative sodium azide 0.09%; 50 x conc.
	1	Certificate of Analysis

MATERIALS REQUIRED

- Microplate reader capable of endpoint measurements at 450 nm; optional: reference filter at 620 nm
 - Data reduction software
 - Multi-channel dispenser or repeatable pipette for 100 µl
 - Vortex mixer
 - Pipettes for 10 µl, 100 µl and 1000 µl
 - Laboratory timing device
 - Distilled or deionised water
 - Measuring cylinder for 1000 ml and 100 ml
 - Plastic container for storage of the wash solution
- This ELISA assay is suitable for use on open automated ELISA processors. Each assay has to be validated on the respective automated system. Detailed information is provided upon request.

SPECIMEN COLLECTION, STORAGE AND HANDLING

- Collect whole blood specimens using acceptable medical techniques to avoid hemolysis.
- Allow blood to clot and separate the serum or plasma by centrifugation.
- Test serum should be clear and non-hemolyzed. Contamination by hemolysis or lipemia should be avoided, but does not interfere with this assay.
- Specimens may be refrigerated at 2-8°C for up to five days or stored at -20°C up to six months.
- Avoid repetitive freezing and thawing of serum or plasma samples. This may result in variable loss of antibody activity.
- Testing of heat-inactivated sera is not recommended.

STORAGE AND STABILITY

- Store test kit at 2-8°C in the dark.
- Do not expose reagents to heat, sun, or strong light during storage and usage.
- Store microplate sealed and desiccated in the clip bag provided.
- Shelf life of the unopened test kit is 18 months from day of production.
Unopened reagents are stable until expiration of the kit. See labels for individual batch.
- Diluted Wash Buffer and Sample Buffer are stable for at least 30 days when stored at 2-8°C.
We recommend consumption on the same day.

PROCEDURAL NOTES

- Do not use kit components beyond their expiration dates.
- Do not interchange kit components from different lots and products.
- All materials must be at room temperature (20-28°C) prior to use.
- Prepare all reagents and samples. Once started, perform the test without interruption.
- Double determinations may be done. By this means pipetting errors may become obvious.
- Perform the assay steps only in the order indicated.
- Always use fresh sample dilutions.
- Pipette all reagents and samples into the bottom of the wells.
- To avoid carryover or contamination, change the pipette tip between samples and different kit controls.
- Wash microwells thoroughly and remove the last droplets of wash buffer.
- All incubation steps must be accurately timed.
- Do not re-use microplate wells.

PREPARATION OF REAGENTS

WASH
Dilute the contents of one vial of the buffered wash solution concentrate (50x) with distilled or deionised water to a final volume of 1000 ml prior to use.

DILUENT
Sample Buffer P: Prior to use dilute the contents (20 ml) of one vial of sample buffer 5x concentrate with distilled or deionised water to a final volume of 100 ml.

Preparation of samples

Dilute patient samples 1:100 before the assay: Put 990 µl of prediluted sample buffer in a polystyrene tube and add 10 µl of sample. Mix well. Note: Calibrators / Controls are ready to use and need not be diluted.

TEST PROCEDURE

Prepare enough microplate modules for all calibrators / controls and patient samples.

- Pipette **100 µl** of calibrators, controls and prediluted patient samples into the wells.
Incubate for **30 minutes** at room temperature (20-28 °C).
Discard the contents of the microwells and **wash 3 times** with **300 µl** of wash solution.
- Dispense **100 µl** of enzyme conjugate into each well.
Incubate for **15 minutes** at room temperature.
Discard the contents of the microwells and **wash 3 times** with **300 µl** of wash solution.
- Dispense **100 µl** of TMB substrate solution into each well.
Incubate for **15 minutes** at room temperature
- Add 100 µl** of stop solution to each well of the modules
Incubate for **5 minutes** at room temperature.
Read the optical density at 450 nm (reference 600-690nm) and calculate the results.
The developed colour is stable for at least 30 minutes. Read during this time.

Example for a pipetting scheme:

	1	2	3	4	5	6	7	8	9	10	11	12
A	A	P1										
B	B	P2										
C	C	P3										
D	D											
E	E											
F	F											
G	C+											
H	C-											

P1, ... patient sample A-F calibrators C+, C- controls

VALIDATION

Test results are valid if the optical densities at 450 nm for calibrators / controls and the results for controls comply with the reference ranges indicated on the Certificate of Analysis enclosed in each test kit.
If these quality control criteria are not met the assay run is invalid and should be repeated.

CALCULATION OF RESULTS

For quantitative results plot the optical density of each calibrator versus the calibrator concentration to create a calibration curve. The concentration of patient samples may then be estimated from the calibration curve by interpolation.

Using data reduction software a 4-Parameter-Fit with lin-log coordinates for optical density and concentration is the data reduction method of choice.

PERFORMANCE CHARACTERISTICS

Calibration

The assay system is calibrated against the international reference preparation WHO 67/183 for AMA-M2 as 100 IU/ml.

Measuring range

The calculation range of this ELISA assay is 0 - 200 IU/ml

Expected values

In a normal range study with samples from healthy blood donors the following ranges have been established with this ELISA assay: Cut-off 10 IU/ml

Interpretation of results

Negative: < 10 IU/ml
Positive: ≥ 10 IU/ml

Linearity

Samples containing high levels of specific antibody were serially diluted in sample buffer to demonstrate the dynamic range of the assay and the upper / lower end of linearity. Activity for each dilution was calculated from the calibration curve using a 4-Parameter-Fit with lin-log coordinates.

Sample	Dilution	Observed IU/ml	Expected IU/ml	O/E [%]
WHO	1:100	108.5	100.0	109
.	1:200	51.2	50.0	102
.	1:400	25.2	25.0	101
.	1:800	12.8	12.5	102
.	1:1600	6.1	6.3	98
.	1:3200	3.1	3.1	99
1	1:100	49.5	49.5	100
.	1:200	25.0	24.8	101
.	1:400	12.2	12.4	99
.	1:800	5.9	6.2	95

Limit of detection

Functional sensitivity was determined to be: 1 IU/ml

Reproducibility

Intra-assay precision: Coefficient of variation (CV) was calculated for each of three samples from the results of 24 determinations in a single run. Results for precision-within-assay are shown in the table below.

Inter-assay precision: Coefficient of variation (CV) was calculated for each of three samples from the results of 6 determinations in 5 different runs. Results for run-to-run precision are shown in the table below.

Intra-Assay		
Sample	Mean IU/ml	CV %
1	39.8	7.0
2	81.3	3.8
3	177.3	3.6

Inter-Assay		
Sample	Mean IU/ml	CV %
1	40.1	6.2
2	84.6	11.8
3	180.4	3.8

Interfering substances

No interference has been observed with haemolytic (up to 1000 mg/dl) or lipemic (up to 3 g/dl triglycerides) sera or plasma, or bilirubin (up to 40 mg/dl) containing sera or plasma. Nor have any interfering effects been observed with the use of anticoagulants (Citrate, EDTA, Heparine). However for practical reasons it is recommended that grossly hemolyzed or lipemic samples should be avoided.

Study results

Study population	n	n Pos	%
Primary biliary cirrhosis (PBC)	143	139	97.2
Rheumatoid Arthritis	60	1	1.7
Normal human sera	267	18	6.7

		Clinical Diagnosis		
		POS	NEG	
ORG 516	POS	139	19	470
	NEG	4	308	
		143	327	

Sensitivity: 97.2 %

Specificity: 94.2 %

Overall agreement: 95.1 %

LIMITATIONS OF THE PROCEDURE

This assay is a diagnostic aid. A definite clinical diagnosis should not be based on the results of a single test, but should be made by the physician after all clinical and laboratory findings have been evaluated concerning the entire clinical picture of the patient. Also every decision for therapy should be taken individually.

The above pathological and normal reference ranges for antibodies in patient samples should be regarded as recommendations only. Each laboratory should establish its own ranges according to ISO 15189 or other applicable laboratory guidelines.

REFERENCES

1. Berg, P.A. and Klein, R. Diagnose der primär-biliären Zirrhose. IVD Nachrichten 1990; 1/1: 6 -7.
2. Berg, P.A. and Klein, R. Heterogeneity of anti-mitochondrial antibodies. Sem. Liver Dis. 1989; 9: 103 - 116.
3. Berg, P.A. and Klein, R. Immunology of primary biliary cirrhosis. Ballière's Clin.Gastroenterol. 1987; 1: 675 - 706.
4. Baum, H. and Palmer, C. The PBC specific antigen. Mol. Aspects Med. 1985; 8: 201 - 234.
5. Fussey, S.P.M., Guest, J.R., James, O.F W. et al. Identification and analysis of the major M2 autoantigens in primary biliary cirrhosis. PNAS, USA 1988; 85: 8654 - 8658.

Notice to the user (European Union):

Any serious incident that has occurred in relation to the device shall be reported to the manufacturer and the competent authority of the EU Member State in which the user and/or the patient is established .

Change Control

Former version: *ORG 516_IFU_EN_QM113145_2013-12-16_2.1* Reason for revision: *Introduction electronic IFU on homepage*

- 1 Pipet **100 µl** calibrator, control or patient sample
 - Incubate for **30 minutes** at room temperature
 - Discard the contents of the wells and wash 3 times with **300 µl** wash solution
- 2 Pipet **100 µl** enzyme conjugate
 - Incubate for **15 minutes** at room temperature
 - Discard the contents of the wells and wash 3 times with **300 µl** wash solution
- 3 Pipet **100 µl** substrate solution
 - Incubate for **15 minutes** at room temperature
- 4 Add **100 µl** stop solution
 - Leave untouched for **5 minutes**
 - Read at **450 nm**

ORGENTEC Diagnostika GmbH

Carl-Zeiss-Straße 49-51


55129 Mainz - Germany

Phone: +49 (0) 61 31 / 92 58-0

Fax: +49 (0) 61 31 / 92 58-58

Internet: www.orgentec.com



 521_3






























ORG 521 Anti-beta-2-Glycoprotein I IgG/IgM

INTENDED PURPOSE

Anti-beta-2-Glycoprotein I IgG/IgM is an ELISA test system for the quantitative measurement of I IgG and IgM class autoantibodies against beta-2-Glycoprotein I in human serum or plasma. This product is intended for professional in vitro diagnostic use only.

Antiphospholipid syndrome (APS, Hughes Syndrome) is a systemic autoimmune disease that causes thromboses, recurrent miscarriage or stillbirths, and stroke. Clinical symptoms are accompanied by specific autoantibodies in the blood, which bind to phospholipids like cardiolipin, or phospholipid-binding proteins like beta-2-glycoprotein I. Autoantibodies against proteins of the coagulation cascade, e.g. prothrombin or annexin V may also be found in patients with APS with otherwise negative phospholipid antibody results. In primary APS autoantibodies against phospholipids appear independently, while in secondary APS phospholipid antibodies are detected in conjunction with other autoimmune diseases, such as lupus erythematosus, rheumatoid arthritis, or Sjögren's syndrome.

SYMBOLS USED ON LABELS

	In vitro diagnostic medical device		Microplate
	Manufacturer		Calibrator
	Catalogue number		Calibrator
	Sufficient for 96 determinations		Calibrator
	Batch code		Calibrator
	Use by		Calibrator
	Temperature limitation		Calibrator
	Keep away from sunlight		Control positive
	Do not reuse		Control negative
	Date of manufacture		Sample Buffer P
	CE marked according to 98/79/EC		Enzyme Conjugate
	Consult instructions for use		Enzyme Conjugate
	Electronic Instruction For Use: version		TMB Substrate
			Stop solution
			Wash Buffer
			Ready to use

PRINCIPLE OF THE TEST

Highly purified beta-2-glycoprotein I is bound to microwells.

The determination is based on an indirect enzyme linked immune reaction with the following steps: Specific antibodies in the patient sample bind to the antigen coated on the surface of the reaction wells. After incubation, a washing step removes unbound and unspecifically bound serum or plasma components. Subsequently added enzyme conjugate binds to the immobilized antibody-antigen-complexes. After incubation, a second washing step removes unbound enzyme conjugate. After addition of substrate solution the bound enzyme conjugate hydrolyses the substrate forming a blue coloured product. Addition of an acid stops the reaction generating a yellow end-product. The intensity of the yellow color correlates with the concentration of the antibody-antigen-complex and can be measured photometrically at 450 nm.

WARNINGS AND PRECAUTIONS


















- All reagents of this kit are intended for professional in vitro diagnostic use only.
- Components containing human serum were tested and found negative for HBsAg, HCV, HIV1 and HIV2 by FDA approved methods. No test can guarantee the absence of HBsAg, HCV, HIV1 or HIV2, and so all human serum based reagents in this kit must be handled as though capable of transmitting infection.
- Bovine serum albumin (BSA) used in components has been tested for BSE and found negative.
- Avoid contact with the substrate TMB (3,3',5,5'-Tetramethyl-benzidine).
- Stop solution contains acid, classification is non-hazardous. Avoid contact with skin.
- Control, sample buffer and wash buffer contain sodium azide 0.09% as preservative. This concentration is classified as non-hazardous.
- Enzyme conjugate contains ProClin 300 0.05% as preservative. This concentration is classified as non-hazardous.

During handling of all reagents, controls and serum samples observe the existing regulations for laboratory safety regulations and good laboratory practice:

- First aid measures: In case of skin contact, immediately wash thoroughly with water and soap. Remove contaminated clothing and shoes and wash before reuse. If system fluid comes into contact with skin, wash thoroughly with water. After contact with the eyes carefully rinse the opened eye with running water for at least 10 minutes. Get medical attention if necessary.
- Personal precautions, protective equipment and emergency procedures:
Observe laboratory safety regulations. Avoid contact with skin and eyes. Do not swallow. Do not pipette by mouth. Do not eat, drink, smoke or apply makeup in areas where specimens or kit reagents are handled. When spilled, absorb with an inert material and put the spilled material in an appropriate waste disposal.
- Exposure controls / personal protection: Wear protective gloves of nitril rubber or natural latex. Wear protective glasses. Used according to intended use no dangerous reactions known.
- Conditions to avoid: Since substrate solution is light-sensitive. Store in the dark.
- For disposal of laboratory waste the national or regional legislation has to be observed.

Observe the guidelines for performing quality control in medical laboratories by assaying control sera.

CONTENTS OF THE KIT

ORG 521		96	Sufficient for 96 determinations
	1		One divisible microplate consisting of 12 modules of 8 wells each. Ready to use. Product code on module: B2G
	1x 1.5 ml	Calibrator A	0 U/ml, containing serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
	1x 1.5 ml	Calibrator B	6.3 U/ml, containing beta-2-glycoprotein I antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
	1x 1.5 ml	Calibrator C	12.5 U/ml, containing beta-2-glycoprotein I antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
	1x 1.5 ml	Calibrator D	25 U/ml, containing beta-2-glycoprotein I antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
	1x 1.5 ml	Calibrator E	50 U/ml, containing beta-2-glycoprotein I antibodies in a serum/buffer matrix (PBS, BSA, NaN3 0.09%), yellow. Ready to use.
	1x 1.5 ml	Calibrator F	100 U/ml, containing beta-2-glycoprotein I antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use.
	1x 1.5 ml	Control positive	, containing beta-2-glycoprotein I antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use. The concentration is specified on the certificate of analysis.
	1x 1.5 ml	Control negative	, containing beta-2-glycoprotein I antibodies in a serum/buffer matrix (PBS, BSA, detergent, NaN3 0.09%), yellow. Ready to use. The concentration is specified on the certificate of analysis.
	20 ml	Sample Buffer P	, containing PBS, BSA, detergent, preservative sodium azide 0.09%, yellow, concentrate (5 x).
	15 ml	Enzyme Conjugate	; containing anti-human IgG antibodies, HRP labelled; PBS, BSA, detergent, preservative PROCLIN 0.05%, light red. Ready to use.
	15 ml	Enzyme Conjugate	; containing anti-human IgM antibodies, HRP labelled; PBS, BSA, detergent, preservative PROCLIN 0.05%, light red. Ready to use.
	15 ml	TMB Substrate	; containing 3,3', 5,5'- Tetramethylbenzidin, colorless. Ready to use.
	15 ml	Stop solution	; contains acid. Ready to use.
	20 ml	Wash Buffer	, containing Tris, detergent, preservative sodium azide 0.09%; 50 x conc.
	1	Certificate of Analysis	

MATERIALS REQUIRED

- Microplate reader capable of endpoint measurements at 450 nm; optional: reference filter at 620 nm
- Data reduction software
- Multi-channel dispenser or repeatable pipette for 100 µl
- Vortex mixer
- Pipettes for 10 µl, 100 µl and 1000 µl
- Laboratory timing device
- Distilled or deionised water
- Measuring cylinder for 1000 ml and 100 ml
- Plastic container for storage of the wash solution

This ELISA assay is suitable for use on open automated ELISA processors. Each assay has to be validated on the respective automated system. Detailed information is provided upon request.

SPECIMEN COLLECTION, STORAGE AND HANDLING

- Collect whole blood specimens using acceptable medical techniques to avoid hemolysis.
- Allow blood to clot and separate the serum or plasma by centrifugation.
- Test serum should be clear and non-hemolyzed. Contamination by hemolysis or lipemia should be avoided, but does not interfere with this assay.
- Specimens may be refrigerated at 2-8°C for up to five days or stored at -20°C up to six months.
- Avoid repetitive freezing and thawing of serum or plasma samples. This may result in variable loss of antibody activity.
- Testing of heat-inactivated sera is not recommended.

STORAGE AND STABILITY

- Store test kit at 2-8°C in the dark.
- Do not expose reagents to heat, sun, or strong light during storage and usage.
- Store microplate sealed and desiccated in the clip bag provided.
- Shelf life of the unopened test kit is 18 months from day of production.
Unopened reagents are stable until expiration of the kit. See labels for individual batch.
- Diluted Wash Buffer and Sample Buffer are stable for at least 30 days when stored at 2-8°C.
We recommend consumption on the same day.

PROCEDURAL NOTES

- Do not use kit components beyond their expiration dates.
- Do not interchange kit components from different lots and products.
- All materials must be at room temperature (20-28°C) prior to use.
- Prepare all reagents and samples. Once started, perform the test without interruption.
- Double determinations may be done. By this means pipetting errors may become obvious.
- Perform the assay steps only in the order indicated.
- Always use fresh sample dilutions.
- Pipette all reagents and samples into the bottom of the wells.
- To avoid carryover or contamination, change the pipette tip between samples and different kit controls.
- Wash microwells thoroughly and remove the last droplets of wash buffer.
- All incubation steps must be accurately timed.
- Do not re-use microplate wells.

PREPARATION OF REAGENTS

WASH

Dilute the contents of one vial of the buffered wash solution concentrate (50x) with distilled or deionised water to a final volume of 1000 ml prior to use.

DILUENT

Sample Buffer P: Prior to use dilute the contents (20 ml) of one vial of sample buffer 5x concentrate with distilled or deionised water to a final volume of 100 ml.

Preparation of samples

Dilute patient samples 1:100 before the assay: Put 990 µl of prediluted sample buffer in a polystyrene tube and add 10 µl of sample. Mix well. Note: Calibrators / Controls are ready to use and need not be diluted.

TEST PROCEDURE

Prepare enough microplate modules for all calibrators / controls and patient samples.

- Pipette **100 µl** of calibrators, controls and prediluted patient samples into the wells.
Incubate for **30 minutes** at room temperature (20-28 °C).
Discard the contents of the microwells and **wash 3 times** with **300 µl** of wash solution.
- Dispense **100 µl** of enzyme conjugate into each well.
Incubate for **15 minutes** at room temperature.
Discard the contents of the microwells and **wash 3 times** with **300 µl** of wash solution.
- Dispense **100 µl** of TMB substrate solution into each well.
Incubate for **15 minutes** at room temperature
- Add 100 µl** of stop solution to each well of the modules
Incubate for **5 minutes** at room temperature.
Read the optical density at 450 nm (reference 600-690nm) and calculate the results.
The developed colour is stable for at least 30 minutes. Read during this time.

Example for a pipetting scheme:

	1	2	3	4	5	6	7	8	9	10	11	12
A	A	P1	A	P1								
B	B	P2	B	P2								
C	C	P3	C	P3								
D	D	P4	D	P4								
E	E	P5	E	P5								
F	F	P6	F	P6								
G	C+	P7	C+	P7								
H	C-	P8	C-	P8								
	IgG	IgG	IgM	IgM								

P1, ... patient sample A-F calibrators C+, C- controls

VALIDATION

Test results are valid if the optical densities at 450 nm for calibrators / controls and the results for controls comply with the reference ranges indicated on the Certificate of Analysis enclosed in each test kit.

If these quality control criteria are not met the assay run is invalid and should be repeated.

CALCULATION OF RESULTS

For quantitative results plot the optical density of each calibrator versus the calibrator concentration to create a calibration curve. The concentration of patient samples may then be estimated from the calibration curve by interpolation. Using data reduction software a 4-Parameter-Fit with lin-log coordinates for optical density and concentration is the data reduction method of choice.

PERFORMANCE CHARACTERISTICS

Calibration

This assay system is calibrated in relative arbitrary units. Calibration is related to the internationally recognised reference sera from E.N. Harris, Louisville and to IRP 97/656 (IgG) and HCAL (IgG) / EY2C9 (IgM).

Measuring range

The calculation range of this ELISA assay is IgG: 0 - 100 U/ml IgM: 0 - 100 U/ml

Expected values

In a normal range study with samples from healthy blood donors the following ranges have been established with this ELISA assay: Cut-off IgG: 8 U/ml IgM: 8 U/ml

Interpretation of results

Negative:	IgG < 5 U/ml	IgM < 5 U/ml
Borderline:	5 - 8 U/ml	5 - 8 U/ml
Positive:	> 8 U/ml	> 8 U/ml

Linearity

Patient samples containing high levels of specific antibody were serially diluted in sample buffer to demonstrate the dynamic range of the assay and the upper / lower end of linearity. Activity for each dilution was calculated from the calibration curve using a 4-Parameter-Fit with lin-log coordinates.

Sample	Dilution	Observed U/ml	Expected U/ml	O/E [%]
IgG 1	1:100	100.0	100.0	100
	1:200	49.8	50.0	100
	1:400	25.5	25.0	102
	1:800	13.1	12.5	105
IgG 2	1:1600	6.9	6.3	110
	1:100	80.9	80.9	100
	1:200	42.0	40.5	104
	1:400	21.1	20.2	104
IgM 1	1:800	10.7	10.1	106
	1:1600	5.6	5.1	110
	1:100	97.6	97.6	100
	1:200	49.0	48.8	100
IgM 2	1:400	23.2	24.4	95
	1:800	13.4	12.2	110
	1:1600	6.4	6.1	105
	1:100	70.3	70.3	100
	1:200	33.5	35.2	95
	1:400	18.6	17.6	106
	1:800	10.1	8.8	115
	1:1600	4.9	4.4	111

Limit of detection

Functional sensitivity was determined to be: IgG: 0.5 U/ml IgM: 0.5 U/ml

Reproducibility

Intra-assay precision: Coefficient of variation (CV) was calculated for each of three samples from the results of 24 determinations in a single run. Results for precision-within-assay are shown in the table below.

Inter-assay precision: Coefficient of variation (CV) was calculated for each of three samples from the results of 6 determinations in 5 different runs. Results for run-to-run precision are shown in the table below.

Intra-Assay IgG		
Sample	Mean U/ml	CV %
1	8.1	3.3
2	17.8	3.1
3	40.2	3.7

Inter-Assay IgG		
Sample	Mean U/ml	CV %
1	8.3	6.0
2	17.7	3.4
3	40.1	4.0

Intra-Assay IgM		
Sample	Mean U/ml	CV %
1	11.5	1.8
2	30.8	2.3
3	66.3	3.1

Inter-Assay IgM		
Sample	Mean U/ml	CV %
1	11.4	3.0
2	30.7	4.4
3	66.9	2.5

Interfering substances

No interference has been observed with haemolytic (up to 1000 mg/dl) or lipemic (up to 3 g/dl triglycerides) sera or plasma, or bilirubin (up to 40 mg/dl) containing sera or plasma. Nor have any interfering effects been observed with the use of anticoagulants (Citrate, EDTA, Heparine). However for practical reasons it is recommended that grossly hemolyzed or lipemic samples should be avoided.

Study results

Study population	n	Pos IgG	%	Pos IgM	%
Primary APS	8	6	75.0	4	50.0
Secondary APS	65	56	86.2	27	41.5
Normal human sera	150	2	1.3	3	2.0

		Clinical Diagnosis		
		POS	NEG	
ORG 521	POS	62	2	223
IgG	NEG	11	148	
		73	150	
Sensitivity:				84.9 %
Specificity:				98.7 %
Overall agreement:				94.2 %

		Clinical Diagnosis		
		Pos	Neg	
ORG 521	Pos	31	3	223
IgM	Neg	42	147	
		73	150	
Sensitivity:				42.5 %
Specificity:				98.0 %
Overall agreement:				79.8 %

LIMITATIONS OF THE PROCEDURE

This assay is a diagnostic aid. A definite clinical diagnosis should not be based on the results of a single test, but should be made by the physician after all clinical and laboratory findings have been evaluated concerning the entire clinical picture of the patient. Also every decision for therapy should be taken individually.

The above pathological and normal reference ranges for antibodies in patient samples should be regarded as recommendations only. Each laboratory should establish its own ranges according to ISO 15189 or other applicable laboratory guidelines.

REFERENCES

- Banzato A, Pozzi N, Frasson R, De F, V, Ruffatti A, Bison E et al. Antibodies to Domain I of beta(2)Glycoprotein I are in close relation to patients risk categories in Antiphospholipid Syndrome (APS). *Thromb Res* 2011; 128 (6):583-6.
- Bertolaccini ML, Amengual O, Atsumi T, Binder WL, de LB, Forastiero R et al. 'Non-criteria' aPL tests: report of a task force and preconference workshop at the 13th International Congress on Antiphospholipid Antibodies, Galveston, TX, USA, April 2010. *Lupus* 2011; 20(2):191-205.
- de Laat B, de Groot PG. Autoantibodies directed against domain I of beta2-glycoprotein I. *Curr Rheumatol Rep* 2011; 13(1):70-6.
- de Laat B, Mertens K, de Groot PG. Mechanisms of disease: antiphospholipid antibodies-from clinical association to pathologic mechanism. *Nat Clin Pract Rheumatol* 2008; 4(4):192-9.
- de Laat B, Pengo V, Pabinger I, Musial J, Voskuyl AE, Bultink IE et al. The association between circulating antibodies against domain I of beta2-glycoprotein I and thrombosis: an international multicenter study. *J Thromb Haemost* 2009; 7(11):1767-73.
- Espinosa G, Cervera R. Antiphospholipid syndrome. *Arthritis Res Ther* 2008; 10(6):230.
- Favaloro EJ, Wong RC. Laboratory testing for the antiphospholipid syndrome: making sense of antiphospholipid antibody assays. *Clin Chem Lab Med* 2011; 49(3):447-61.
- Fischer MJ, Rauch J, Levine JS. The antiphospholipid syndrome. *Arthritis Rheum* 2007; 27(1):35-46.
- Giannakopoulos B, Passam F, Ioannou Y, Krilis SA. How we diagnose the antiphospholipid syndrome. *Blood* 2009; 113(5):985-94.
- Greaves M, Cohen H, Machin SJ, Mackie I. Guidelines on the investigation and management of the antiphospholipid syndrome. *Br J Haematol* 2000; 109(4):704-15.
- Hughes GR. Hughes syndrome: antiphospholipid syndrome. *J R Coll Physicians Lond* 1998; 32(3):260-4.
- Hughes GR. Hughes Syndrome (the antiphospholipid syndrome): ten clinical lessons. *Autoimmun Rev* 2008; 7(3):262-6.
- Hughes GR. Antiphospholipid syndrome, migraine and stroke. *Lupus* 2010; 19(5):555-6.
- Hughes GR, Harris NN, Gharavi AE. The anticardiolipin syndrome. *J Rheumatol* 1986; 13(3):486-9.
- Koike T, Bohgaki M, Amengual O, Atsumi T. Antiphospholipid antibodies: lessons from the bench. *J Autoimmun* 2007; 28(2-3):129-33.
- Lakos G, Favaloro EJ, Harris EN, Meroni PL, Tincani A, Wong RC et al. International consensus guidelines on anticardiolipin and anti-beta2-glycoprotein I testing: report from the 13th International Congress on Antiphospholipid Antibodies. *Arthritis Rheum* 2012; 64(1):1-10.
- Mackworth-Young C. Primary antiphospholipid syndrome: a distinct entity? *Autoimmun Rev* 2006; 5(1):70-5.

- Miyakis S, Lockshin MD, Atsumi T, Branch DW, Brey RL, Cervera R et al. International consensus statement on an update of the classification criteria for definite antiphospholipid syndrome (APS). *J Thromb Haemost* 2006; 4(2):295-306.
- Molina JF, Gutierrez-Urena S, Molina J, Uribe O, Richards S, De CC et al. Variability of anticardiolipin antibody isotype distribution in 3 geographic populations of patients with systemic lupus erythematosus. *J Rheumatol* 1997; 24(2):291-6.
- Oku K, Atsumi T, Amengual O, Koike T. Antiprothrombin antibody testing: detection and clinical utility. *Semin Thromb Hemost* 2008; 34(4):335-9.
- Pengo V, Biasiolo A, Bison E, Chantarangkul V, Tripodi A. Antiphospholipid antibody ELISAs: survey on the performance of clinical laboratories assessed by using lyophilized affinity-purified IgG with anticardiolipin and anti-beta2-Glycoprotein I activity. *Thromb Res* 2007; 120(1):127-33.
- Pierangeli SS, de Groot PG, Dlott J, Favaloro E, Harris EN, Lakos G et al. 'Criteria' aPL tests: report of a task force and preconference workshop at the 13th International Congress on Antiphospholipid Antibodies, Galveston, Texas, April 2010. *Lupus* 2011; 20(2):182-90.
- Pierangeli SS, Favaloro EJ, Lakos G, Meroni PL, Tincani A, Wong RC et al. Standards and reference materials for the anticardiolipin and anti-beta-2-glycoprotein I assays: a report of recommendations from the APL Task Force at the 13th International Congress on Antiphospholipid Antibodies. *Clin Chim Acta* 2012; 413(1-2):358-60.
- Sinico RA, Bollini B, Sabadini E, Di Toma L, Radice A. The use of laboratory tests in diagnosis and monitoring of systemic lupus erythematosus. *J Nephrol JID - 9012268* 2002; 15 Suppl 6:S20-S27.
- Tincani A, Andreoli L, Casu C, Cattaneo R, Meroni P. Antiphospholipid antibody profile: implications for the evaluation and management of patients. *Lupus* 2010; 19(4):432-5.
- Tincani A, Morozzi G, Afeltra A, Alessandri C, Allegri F, Bistoni O et al. Antiprothrombin antibodies: a comparative analysis of homemade and commercial methods. A collaborative study by the Forum Interdisciplinare per la Ricerca nelle Malattie Autoimmuni (FIRMA). *Clin Exp Rheumatol* 2007; 25(2):268-74.
- Wilson WA, Gharavi AE, Koike T, Lockshin MD, Branch DW, Piette JC et al. International consensus statement on preliminary classification criteria for definite antiphospholipid syndrome: report of an international workshop. *Arthritis Rheum* 1999; 42(7):1309-11.
- Wong RC, Favaloro EJ, Adelstein S, Baumgart K, Bird R, Brighton TA et al. Consensus guidelines on anti-beta 2 glycoprotein I testing and reporting. *Pathology* 2008; 40(1):58-63.
- Wong RC, Gillis D, Adelstein S, Baumgart K, Favaloro EJ, Hendle MJ et al. Consensus guidelines on anticardiolipin antibody testing and reporting. *Pathology* 2004; 36(1):63-8.

Notice to the user (European Union):

Any serious incident that has occurred in relation to the device shall be reported to the manufacturer and the competent authority of the EU Member State in which the user and/or the patient is established .

Change Control

Former version: ORG 521_IFU_EN_QM113150_2016-04-18_2

Reason for revision: Introduction electronic IFU on homepage

- 1** Pipet **100 µl** calibrator, control or patient sample
 - Incubate for **30 minutes** at room temperature
 - Discard the contents of the wells and wash 3 times with **300 µl** wash solution
- 2** Pipet **100 µl** enzyme conjugate
 - Incubate for **15 minutes** at room temperature
 - Discard the contents of the wells and wash 3 times with **300 µl** wash solution
- 3** Pipet **100 µl** substrate solution
 - Incubate for **15 minutes** at room temperature
- 4** Add **100 µl** stop solution
 - Leave untouched for **5 minutes**
 - Read at **450 nm**