
OTICON | Jet Technical data sheet

BTF / BTF PP

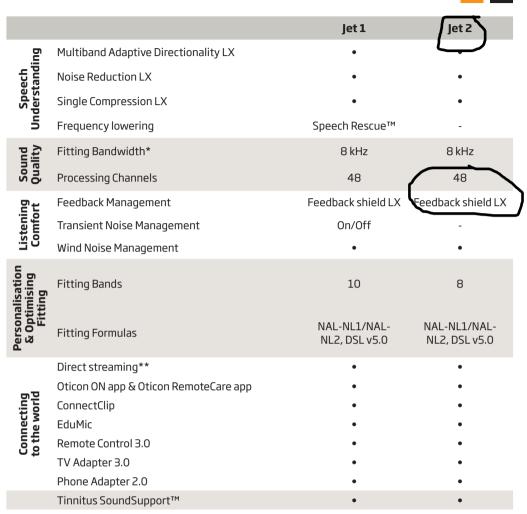

^{*}Bandwidth accessible for gain adjustments during fitting

Operating Conditions

Temperature: +1°C to +40°C (34°F to 104°F) Humidity: 5% to 93% relative humidity,

non-condensing Atmospheric pressure: 700 hPa to 1060 hPa

Storage and transportation conditions

Temperature and humidity should not exceed the below limits for extended periods during transportation and storage.

Storage

Transportation

Temperature: -25°C to +60°C (-13°F to 140°F) Humidity: 5% to 93% relative humidity, non-condensina Atmospheric pressure: 700 hPa to 1060 hPa

Temperature: -25°C to +60°C (-13°F to 140°F) Humidity: 5% to 93% relative humidity, non-condensina Atmospheric pressure: 700 hPa to 1060 hPa

Apple, the Apple logo, iPhone, iPad, and iPod touch are trademarks of Apple Inc., registered in the U.S. and other countries.



85

105

Oticon let BTE and BTE PP features a tactile double push-button for easy operation of volume and programs. They are both powered by disposable batteries and features Bluetooth® Low Energy technology, which makes them Made for iPhone® hearing aids that can stream directly from iPhone, iPad®, and iPod touch®.

Multiband Adaptive Directionality LX provides fast and responsive adaptation of directional modes in 15 independent frequency bands to put speech in front in more focus when the environment becomes noisier.

Noise Reduction LX removes unwanted noise to provide a comfortable listening experience. The feature is adapting fast enough to remove noise even in between words.

The Velox™ platform is a powerful and fast processor providing the power and memory needed for the adaptive processing in Oticon let.










^{**}From iPhone, iPad, and iPod touch

Oticon Jet 1 & 2 **BTE 85**

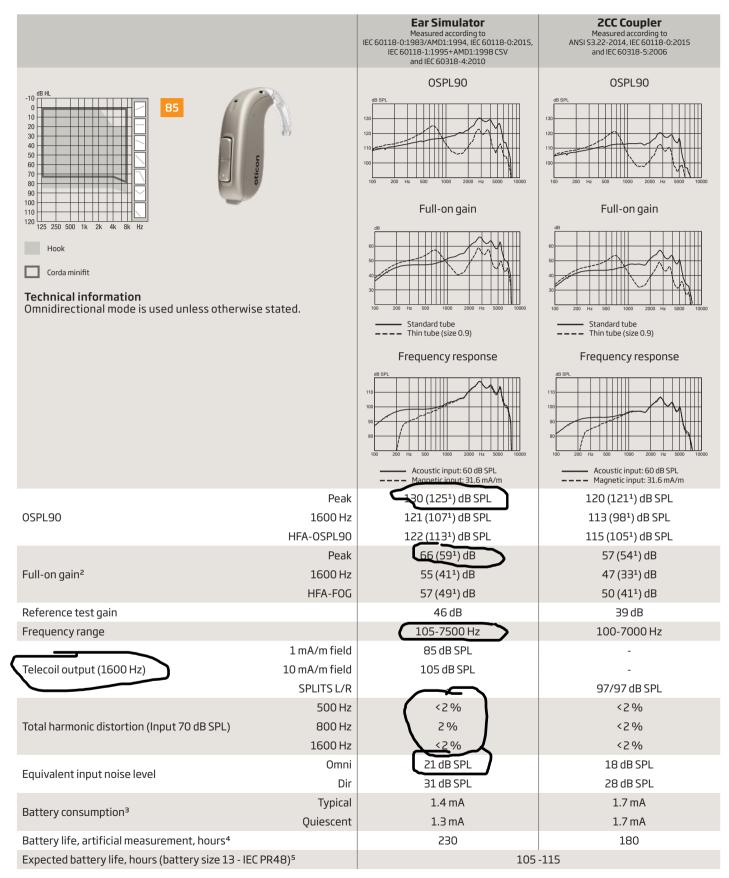

¹⁾ For instruments fitted with Corda miniFit


²⁾ Measured with the gain control of the hearing aids set to their full-on position minus 20 dB and with an input SPL of 70 dB. This is to obtain a gain response equal to the full-on gain response from e.g. IEC 60118-0:1983+A1:1994 but without influence of feedback.

3) Battery current is measured according to IEC 60118-0:1983/AMD1:1994 §7.11, IEC 60118-0:2015 §7.7 and ANSI S3.22:2014 §6.13 after a settling time of minimum 3 minutes.

⁴⁾ Based on the standardised battery consumption measurement (e.g. IEC 60118-0:1983/AMD1:1994). The actual battery life depends on battery quality, use pattern, active feature set, hearing loss and sound environment.

⁵⁾ Real usage battery life is shown as an estimated interval based on mixed use cases with variable amplification settings and variable input levels, incl. direct stereo streaming from a TV (25% of the time) and streaming from a mobile phone (6% of the time).

Oticon Jet 1 & 2 BTE PP 105

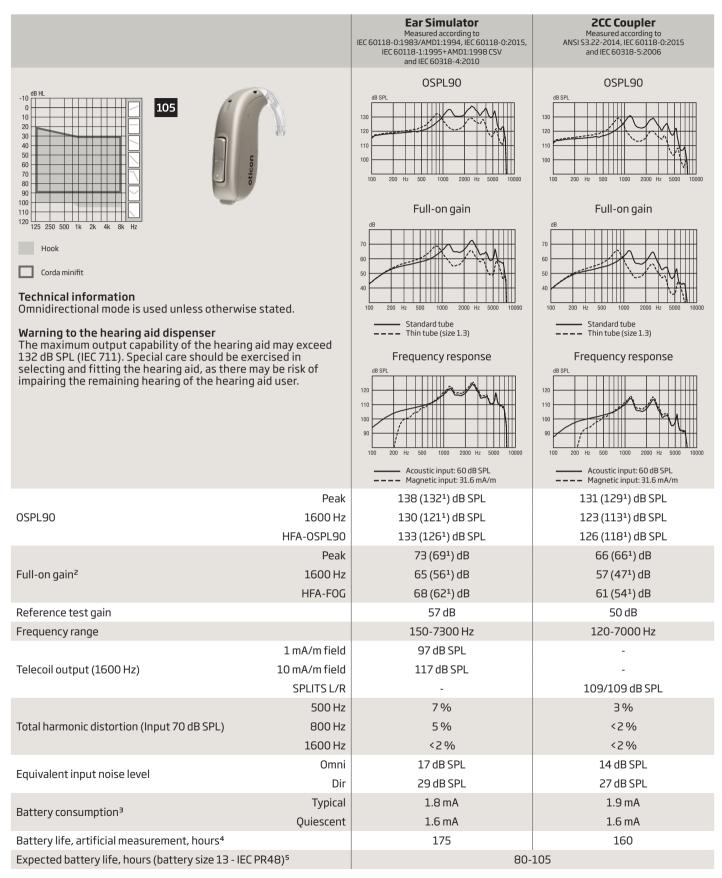

¹⁾ For instruments fitted with Corda miniFit Power

²⁾ Measured with the gain control of the hearing aids set to their full-on position minus 20 dB and with an input SPL of 70 dB. This is to

obtain a gain response equal to the full-on gain response from e.g. IEC 60118-0:1983+A1:1994 but without influence of feedback.

3) Battery current is measured according to IEC 60118-0:1983/AMD1:1994 §7.11, IEC 60118-0:2015 §7.7 and ANSI S3.22:2014 §6.13 after a settling time of minimum 3 minutes.

⁴⁾ Based on the standardised battery consumption measurement (e.g. IEC 60118-0:1983/AMD1:1994). The actual battery life depends on battery quality, use pattern, active feature set, hearing loss and sound environment.

⁵⁾ Real usage battery life is shown as an estimated interval based on mixed use cases with variable amplification settings and variable input levels, incl. direct stereo streaming from a TV (25% of the time) and streaming from a mobile phone (6% of the time).

Headquarters Oticon A/S Kongebakken 9 DK-2765 Smørum Denmark



