

## HiSep™ LSM 1077

Density: 1.077+ 0.0010 g/ml

Product Code: LS001

### Intended use:

Isolation of mononuclear cells (lymphocytes and monocytes) from peripheral human blood.

### Principle:

The first step in studying lymphocytes is to isolate them so that their behavior can be analyzed *in vitro*. Lymphocytes are present in blood, peritoneal exudates or lymphoid organs mixed with other cells. Human lymphocytes can be isolated most readily from peripheral blood. A pure population of lymphocytes can be obtained by various separation procedures.

HiSep™ LSM 1077 is based on the adapted method of isolating human mononuclear cells using centrifugation techniques by Bøyum in which defibrinated blood is layered on a solution of sodium diatrizoate and polysucrose and centrifuged at low speeds for 30 minutes. Differential migration following centrifugation results in the formation of several cell layers. Mononuclear cells (lymphocytes and monocytes) and platelets are contained in the banded plasma-LSM interphase due to their density, and the pellet that is formed contains mostly erythrocytes and granulocytes, which have migrated through the gradient to the bottom of the tube.

### Product Description:

HiMedia's HiSep™ LSM 1077 is an iso-osmotic, low viscosity medium containing polysucrose and diatrizoic acid dihydrate, adjusted to a density of  $1.0770 \pm 0.0010$  g/ml. This medium offers a quick and reliable method for the simple isolation of human mononuclear cells and lymphocytes from defibrinated EDTA or heparin treated human blood. It is certified for in vitro Diagnostic (IVD) use.

Separation of human peripheral blood by the recommended protocol typically yields a mononuclear cell preparation with:

- $95 \pm 5\%$  mononuclear cells present in the separated fraction
- $>90\%$  viability of the separated cells as determined by trypan blue exclusion staining
- $5 \pm 2\%$  red blood cells
- $3 \pm 2\%$  granulocytes

### Application:

- The method is applicable for studying cell-mediated lympholysis and for human lymphocyte antigen (HLA) typing. It may be employed as the initial step prior to enumeration of T-, B- and "null" lymphocytes.
- Human mononuclear cells are used in clinical research and cell therapy applications.

- It may be used in the preparation of pure lymphocyte suspensions for cell culture and cytotoxicity assays.

### Composition:

Ingredients	g/dl
Polysucrose	5.700
Diatrizoic acid dihydrate	9.000

### Type of specimen:

Human Blood

### Specimen Collection and Handling:

For clinical samples follow appropriate techniques for handling as per established guidelines <sup>4,5</sup>.

1. Disinfect the vacutainer by applying 70% isopropyl alcohol to the rubber stopper.
2. If using blood collection tube containing suitable anticoagulant (EDTA, sodium citrate etc.), disinfect the tube by applying 70% isopropyl alcohol.
3. Wait for 1 minute.
4. Palpate vein before disinfection of venipuncture site.
5. Cleanse the site with 70% isopropyl alcohol.
6. Starting at the center, swab the site concentrically with tincture iodine or chlorhexidine.
7. Allow the disinfectant to dry.
8. Collect the required volume of blood by venipuncture.
9. Mix gently by inverting tube 2 – 3times to avoid coagulation.
10. After venipuncture, remove iodine from the skin with alcohol.
11. Sterilize the needle, syringe and other materials used for blood collection by autoclaving before discarding.

### Note:

- *The blood should be kept at room temperature (15-25°C) prior to use and during centrifugation, and should be collected aseptically in the presence of EDTA or heparin.*
- *Blood should be processed within two hours of collection for maximum separation and functionality. However, acceptable separation can be obtained for up to six hours.*

- *As there is no known method available for complete assurance that blood samples or tissue will not transmit infection, therefore it is suggested to consider all blood derivatives or tissue specimens to be potentially infectious.*
- *Do not palpate the vein without sterile gloves. Only fresh blood should be used to ensure good separation and high viability of isolated cells.*

### Precautions:

- Dilution or adulteration of this reagent may result in inadequate mononuclear cells separation.
- Do not use reagent beyond expiry date.
- The solution may cause sensitization by inhalation and skin contact. Wear suitable protective clothing and gloves.
- Never pipette by mouth and avoid contact with skin and mucous membranes.
- Avoid microbial contamination of reagents, which may lead to incorrect results.
- Use of high binding plastics such as polystyrene may bind cells to the walls of centrifuge tube.

### Materials required but not provided:

Reagents/Consumables/Equipment	Product Code
Phosphate buffered saline solution	TL1006
Centrifuge Tubes, 15ml	TCP103 TCP105
Centrifuge Tubes, 50ml	TCP104 TCP106
Disposable Serological Pipettes, 5ml	PW1193
Disposable Serological Pipettes, 10ml	PW1194
Disposable Serological Pipettes, 25ml	PW1195
Clean glass Pasteur pipette	
Centrifuge machine	

## Directions:

1. Make a 1:1 dilution of whole blood (sometimes 1:2 dilution of the blood may be needed depending upon the absolute cell numbers). Dilutions should be made in physiological saline or isotonic phosphate buffered saline.
2. Aseptically transfer 2.5 ml of HiSep™ LSM 1077 to a 15ml clean centrifuge tube and overlay with 7.5ml diluted blood. The ratio of LS001 to diluted blood should be 1:3. DO NOT MIX. The quality of the separation is dependent upon a sharp interphase between lymphocytes and the solution.

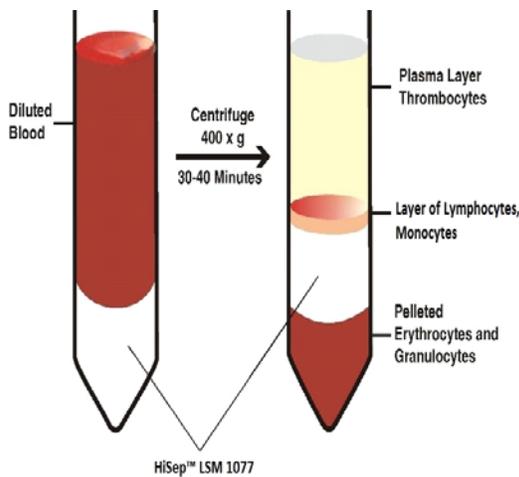


Figure 1. Performance of LS001

Centrifuge at 1000x g, at room temperature (15-25°C) without brake for 30 minutes. Centrifugation will sediment erythrocytes and polynuclear leukocytes and band mononuclear lymphocytes above HiSep™ LSM 1077 as show in Fig. 1.

3. Discard by aspirating most of the plasma and platelet containing supernatant above the interface band (granulocytes and erythrocytes will be in the red pellet).
4. Using pipette carefully aspirate the mononuclear cells and transfer it to a clean centrifuge tube.
5. Add 10ml of isotonic phosphate buffered saline to mononuclear cells layer in the centrifuge tube and mix by gentle aspiration. Centrifuge at 300-400x g at room temperature (15-25°C) for 10 minutes. This washing with isotonic phosphate buffered saline removes HiSep™ LSM and reduces the number of platelets.

6. Wash the cells again with isotonic phosphate buffered saline and resuspend in an appropriate medium for your applications.

**NOTE:** Count the cells and determine the number of viable cells by trypan blue exclusion staining. In case of low cell viability, phosphate buffered saline may be replaced with appropriate tissue culture medium.

## Quality Control:

### Appearance

Clear, colorless solution

### pH

6.5 – 8.5

### Osmolality (mOsm/kg H<sub>2</sub>O)

240 – 350

### Density (g/cm<sup>3</sup>)

1.0760 – 1.0780

### Sterility

No bacterial or fungal growth is observed after 14 days of incubation as per USP specification.

### Viability of mononuclear cells

NLT 90%

### Visual inspection test

Buffy coat present at the plasma and medium interphase

### Percentage of Mononuclear Cells (Flow cytometry CD45 analysis)

NLT 90%

### Percentage of granulocytes (Flow cytometry CD15 analysis)

NMT 5 %

### Endotoxin Level

NMT 1 EU/mL

### Storage and Shelf Life:

HiSep™ LSM 1077 is shipped at ambient temperature.

Upon receipt, store the product tightly closed at 2-8°C.

Shelf life is 36 months.

Do not use, if the material is cloudy, has a distinct yellow color, or shows any sign of contamination. For best results, bring the solution to room temperature (15-25°C) before use.

### Disposal:

User must ensure proper cleaning of equipment. Other surplus and non-recyclable solutions to a licensed disposal company.

### Safety Information:

Take appropriate laboratory safety measures and wear gloves when handling. Not compatible with disinfecting agents containing bleach. Please refer the Safety Data Sheet (SDS) for information regarding hazards and safe handling practices.


### References:

1. Bøyum, A. "Isolation of mononuclear cells and granulocytes from human blood." Scand. J. Clin. Lab.
2. EC Guide to GMP (Good Manufacturing Practice), annex 1 "Manufacture of Sterile Medicinal Products".
3. Bøyum, A. "Isolation of mononuclear cells and granulocytes from human blood." Scand. J. Clin. Lab. Invest. 21, Suppl. 97 (Paper IV), 77-89 (1968).
4. Isenberg, H.D. Clinical Microbiology Procedures Handbook. 2nd Edition.
5. Jorgensen, J. H., Pfaller, M.A., Carroll, K.C., Funke, G. Landry, M.L., Richter, S.S and Warnock., D.W.

(2015), Manual of Clinical Microbiology, 11th Edition. Vol. 1.

### Nomogram for determining relative centrifuge forces

How to establish the rpm required to obtain 400 x g for the lymphocyte separation procedure.

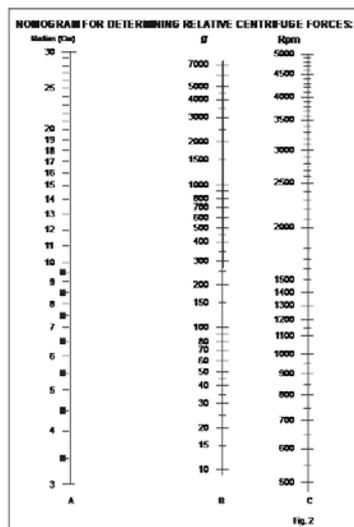

A nomogram can be used to derive the rpm setting for your centrifuge.

- Measure the radius (cm) from the center of the centrifuge spindle to the end of the test tube carrier. Mark this value on scale A.
- Mark the relative centrifugal force (e.g., 400) on scale B.
- With a ruler, draw a straight line between points on columns A and B, extending it to intersect column C. The reading on column C is the rpm setting for the centrifuge.

## Troubleshooting:

HiSep™ LSM products if used as per the recommended procedure, are said to give trouble-free isolation of mononuclear cells. In case of any deviations in certain experimental procedures or parameters, may lead to poor results. However, this troubleshooting table will assist in the rapid identification and rectification of the problem hindering the performance.

Problem	Possible Reason	Solution
Contamination of lymphocytes with red blood cells.	A. Low temperature	The densities of HiSep™ LSM are greater at low temperature. As a result, they are agitated less well. Raise the temperature to 18°C to 20°C.
	B. Low centrifugation speed	Use adequate g-force and if required increase the centrifugation speed.
	C. Stale blood	Process the blood as soon as possible.
Mononuclear cells with low yield and viability.	Must be due to high temperature	HiSep™ LSM products are less dense at high temperatures, therefore some lymphocytes may penetrate into the interface layer. Try and reduce the temperature to 18°C to 20°C. This might improve the cell viability too.
Mononuclear cells with low yield and normal viability.	The blood must not have been diluted 1:1 with balanced salt solution. High hematocrit.	Dilute the blood samples even further.
Mononuclear cells with low yield and increased granulocyte contamination.	Centrifugation rotor vibration that leads to the stirring of the gradient.	Check to see if the rotor is well balanced. Preferably choose the rotor speed to avoid natural resonant frequencies.
Mononuclear cells with low yield, low viability and contamination by other cell types.	Blood used might be non-human.	Use freshly collected human blood. Strictly do not use pathological blood, non-human blood samples, old blood samples or blood from sources other than peripheral blood.

### Disclaimer:

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ Publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal diagnostic or therapeutic use but for laboratory, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.

Revision:01/2022



THE INTERNATIONAL CERTIFICATION NETWORK

# CERTIFICATE

Quality Austria

has issued an IQNet recognized certificate that the organization:

**HiMedia Laboratories Pvt. Ltd.**

**Plot NO. C40, ROAD - 21Y, WAGLE INDUSTRIAL ESTATE,  
THANE (WEST) - 400604 MAHARASHTRA, INDIA**

for the following scope:

**Design, Development & Testing of Microbiology, Animal Cell Culture,  
Plant Tissue Culture & Molecular Biology products**

EAC: 34

has implemented and maintains a

## QUALITY MANAGEMENT SYSTEM

which fulfils the requirements of the following standard

### ISO 9001:2015

This attestation is directly linked to the IQNet Partner's original certificate and shall not be used as a stand-alone document

Issued on:	2022-02-28
Validity date:	2025-02-27
Quality Austria certified since:	2022-02-28

**Registration Number: AT-27302/0**

**Alex Stoichitoiu**  
*President of IQNet*

**Mag. Friedrich Khuen-Belasi**  
*Authorised Representative  
of Quality Austria*



**IQNet Partners\*:**

AENOR Spain AFNOR Certification France APCER Portugal CCC Cyprus CISQ Italy  
CQC China CQM China CQS Czech Republic Cro Cert Croatia DQS Holding GmbH Germany EAGLE Certification Group USA  
FCAV Brazil FONDONORMA Venezuela ICONTEC Colombia Inspecta Sertifointi Oy Finland INTECO Costa Rica  
IRAM Argentina JQA Japan KFQ Korea MIRTEC Greece MSZT Hungary Nemko AS Norway NSAI Ireland  
NYCE-SIGE México PCBC Poland Quality Austria Austria RR Russia SII Israel SIQ Slovenia  
SIRIM QAS International Malaysia SQS Switzerland SRAC Romania TEST St Petersburg Russia TSE Turkey YUQS Serbia

\* The list of IQNet partners is valid at the time of issue of this certificate. Updated information is available under [www.iqnet-certification.com](http://www.iqnet-certification.com)

# CERTIFICATE

Quality Austria - Trainings, Zertifizierungs und Begutachtungs GmbH awards this **qualityaustria** certificate to the following organisation:

This **qualityaustria** certificate confirms the application and further development of an effective

**HIMEDIA**<sup>®</sup>

**HiMedia Laboratories Pvt. Ltd.**

Plot NO. C40, Road - 21Y, Wagle Industrial Estate,  
Thane (West) - 400604 Maharashtra, INDIA

**QUALITY MANAGEMENT SYSTEM**

complying with the requirements of standard  
**ISO 9001:2015**

Quality Austria - Trainings, Zertifizierungs und Begutachtungs GmbH is accredited according to the Austrian Accreditation Act by the BMWFV (Federal Ministry of Science, Research and Economy).

Quality Austria is accredited as an organisation for environmental verification by the BMLFUW (Federal Ministry of Agriculture, Forestry, Environment and Water Management).

Quality Austria is authorized by the VDA (Association of the Automotive Industry).

For accreditation registration details please refer to the applicable decisions or recognition documents.

Quality Austria is the Austrian member of IQNet (International Certification Network).

Dok. Nr. FO\_24\_028

1702280c-6c19-4683-8f36-3ea2e4167c18

The current validity of the certificate is documented exclusively on the Internet under <http://www.qualityaustria.com/en/cert> EAC: 34

Design, Development & Testing of Microbiology, Animal Cell Culture, Plant Tissue Culture & Molecular Biology products

Registration No.: 27302/0

Date of initial issue: 28 February 2022

Valid until: 27 February 2025

Vienna, 28 February 2022

Quality Austria - Trainings, Zertifizierungs und Begutachtungs GmbH,  
AT-1010 Vienna, Zelinkagasse 10/3



 **qualityaustria**

PARTNER OF  




Mag. Christoph Mondl  
General Manager



Mag. Dr. Werner Paar  
General Manager



Mag. Dr. Anni Koubek  
Specialist representative

# CERTIFICATE

Quality Austria - Trainings, Zertifizierungs und Begutachtungs GmbH awards this **qualityaustria** certificate to the following organisation:

This **qualityaustria** certificate confirms the application and further development of an effective

**HIMEDIA**

## HiMedia Laboratories Pvt. Ltd.

Plot NO. C40, Road - 21Y, Wagle Industrial Estate,  
Thane (West) - 400604 Maharashtra, INDIA

## QUALITY MANAGEMENT SYSTEM

complying with the requirements of standard

### ISO 13485:2016

Medical devices - Quality management systems -  
Requirements for regulatory purposes

Quality Austria - Trainings, Zertifizierungs und Begutachtungs GmbH is accredited according to the Austrian Accreditation Act by the BMWFV (Federal Ministry of Science, Research and Economy).

Quality Austria is accredited as an organisation for environmental verification by the BMLFUW (Federal Ministry of Agriculture, Forestry, Environment and Water Management).

Quality Austria is authorized by the VDA (Association of the Automotive Industry).

For accreditation registration details please refer to the applicable decisions or recognition documents.

Quality Austria is the Austrian member of IQNet (International Certification Network).

Dok. Nr. FO\_24\_028

c74e1d5d-8d70-4bfe-a660-b5ea89bf3600

The current validity of the certificate is documented exclusively on the Internet under <http://www.qualityaustria.com/en/cert> EAC: 34

Design, Development & Testing of Biosciences Products for application in Microbiology, Animal Cell Culture & Molecular Biology products

Registration No.: 00391/0

Date of initial issue: 28 February 2022

Valid until: 27 February 2025

Vienna, 28 February 2022

Quality Austria - Trainings, Zertifizierungs und Begutachtungs GmbH,  
AT-1010 Vienna, Zelinkagasse 10/3



 **qualityaustria**

PARTNER OF  




Mag. Christoph Mondl  
General Manager



Mag. Dr. Werner Paar  
General Manager



Mag. Dr. Anni Koubek  
Specialist representative



THE INTERNATIONAL CERTIFICATION NETWORK

# CERTIFICATE

Quality Austria

has issued an IQNet recognized certificate that the organization:

**HiMedia Laboratories Pvt. Ltd.**

**Plot NO. C40, ROAD - 21Y, WAGLE INDUSTRIAL ESTATE,  
THANE (WEST) - 400604 MAHARASHTRA, INDIA**

for the following scope:

**Design, Development & Testing of Biosciences Products for application in Microbiology,  
Animal Cell Culture & Molecular Biology products**

EAC: 34

has implemented and maintains a

## QUALITY MANAGEMENT SYSTEM

which fulfils the requirements of the following standard

### ISO 13485:2016

This attestation is directly linked to the IQNet Partner's original certificate and shall not be used as a stand-alone document

Issued on:	2022-02-28
Validity date:	2025-02-27
Quality Austria certified since:	2022-02-28

**Registration Number: AT-00391/0**

**Alex Stoichitoiu**  
President of IQNet

**Mag. Friedrich Khuen-Belasi**  
Authorised Representative  
of Quality Austria



**IQNet Partners\*:**

AENOR Spain AFNOR Certification France APCER Portugal CCC Cyprus CISQ Italy  
CQC China CQM China CQS Czech Republic Cro Cert Croatia DQS Holding GmbH Germany EAGLE Certification Group USA  
FCAV Brazil FONDONORMA Venezuela ICONTEC Colombia Inspecta Sertifointi Oy Finland INTECO Costa Rica  
IRAM Argentina JQA Japan KFQ Korea MIRTEC Greece MSZT Hungary Nemko AS Norway NSAI Ireland  
NYCE-SIGE México PCBC Poland Quality Austria Austria RR Russia SII Israel SIQ Slovenia  
SIRIM QAS International Malaysia SQS Switzerland SRAC Romania TEST St Petersburg Russia TSE Turkey YUQS Serbia

\* The list of IQNet partners is valid at the time of issue of this certificate. Updated information is available under [www.iqnet-certification.com](http://www.iqnet-certification.com)