


Ordering information

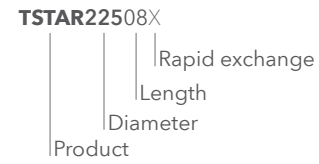

Stent diameter (mm)	Stent length (mm)									
	8	12	15	18	22	26	30	34	38	
2.00	TSTAR20008X	TSTAR20012X	TSTAR20015X	TSTAR20018X	TSTAR20022X	TSTAR20026X	TSTAR20030X	---	---	
2.25	TSTAR22508X	TSTAR22512X	TSTAR22515X	TSTAR22518X	TSTAR22522X	TSTAR22526X	TSTAR22530X	TSTAR22534X	TSTAR22538X	
2.50	TSTAR25008X	TSTAR25012X	TSTAR25015X	TSTAR25018X	TSTAR25022X	TSTAR25026X	TSTAR25030X	TSTAR25034X	TSTAR25038X	
2.75	TSTAR27508X	TSTAR27512X	TSTAR27515X	TSTAR27518X	TSTAR27522X	TSTAR27526X	TSTAR27530X	TSTAR27534X	TSTAR27538X	
3.00	TSTAR30008X	TSTAR30012X	TSTAR30015X	TSTAR30018X	TSTAR30022X	TSTAR30026X	TSTAR30030X	TSTAR30034X	TSTAR30038X	
3.50	TSTAR35008X	TSTAR35012X	TSTAR35015X	TSTAR35018X	TSTAR35022X	TSTAR35026X	TSTAR35030X	TSTAR35034X	TSTAR35038X	
4.00	TSTAR40008X	TSTAR40012X	TSTAR40015X	TSTAR40018X	TSTAR40022X	TSTAR40026X	TSTAR40030X	TSTAR40034X	TSTAR40038X	
4.50	---	TSTAR45012X	TSTAR45015X	TSTAR45018X	TSTAR45022X	TSTAR45026X	TSTAR45030X	---	---	
5.00	---	TSTAR50012X	TSTAR50015X	TSTAR50018X	TSTAR50022X	TSTAR50026X	TSTAR50030X	---	---	

5 F min. guide catheter I.D.: 1.4 mm (0.056 in)

¹Third-party brands are trademarks of their respective owners.
²Stent delivery system updates were implemented on the 2.0-4.0 mm Onyx TruStar DES diameter.
³Compared to Resolute Onyx 3.0 mm balloon design.
⁴Stents should not be expanded to a diameter beyond the maximum labeled diameter listed per the IFU. Post-dilation required for overexpansion.
⁵Compared to 2.0-4.0 mm sizes.
⁶Based on bench test data on file at Medtronic, D00624519, Rev A. Compared to Resolute Onyx DES. May not be indicative of clinical performance.
⁷Based on bench test data on file at Medtronic, D00339634, Rev C. May not be indicative of clinical performance. N = 7 DES of each tested: Onyx TruStar DES, Resolute Onyx DES, Orsiro[®] DES, XIENCE Sierra[™] DES, SYNERGY[™] DES.
⁸Based on bench test data on file at Medtronic, 44RD21031-040047, Version 1.0. Compared to Resolute Onyx DES. May not be indicative of clinical performance.
⁹Resolute Onyx DES IFU M989444A002 C 2021-12-03 and Onyx TruStar DES IFU M031943C002 A 2022-04-28.
¹⁰Third-party modeling and analysis. Mottier MDT-ON14-report-curved-v10-20150229_Onyx_Synergy.pdf. May not be indicative of clinical performance. Evaluated the following stent platforms: Resolute Onyx DES, SYNERGY[™] DES, and XIENCE Alpine[™] DES (Multi-Link B platform).
¹¹Based on bench test data on file at Medtronic, CO10276086 University of Budapest Visibility Testing, v1. May not be indicative of clinical performance.
¹²Rolleder T, Kedhi E, Berta B, et al. Short-term stent coverage of second-generation zotarolimus-eluting durable polymer stents: Onyx one-month optical coherence tomography study. *Adv Interv Cardiol.* 2019;15(2):143-150.
¹³Yeh RW, Silber S, Chen L, et al. 5-Year Safety and Efficacy of Resolute Zotarolimus-Eluting Stent: The RESOLUTE Global Clinical Trial Program. *JACC Cardiovasc Interv.* February 13, 2017;10(3):247-254.
¹⁴Based on bench test data on file at Medtronic, Concept Select Tip Catch Frequency for S10 MV_Jason_xls, V1.0. May not be indicative of clinical performance.
¹⁵Based on bench test data on file at Medtronic, D00339634, Rev C. May not be indicative of clinical performance. N=5 of each DES tested.
¹⁶Cuellas C, et al. Use of a Zotarolimus-eluting stent for small vessel disease (DISCO 9 Study). Presented at PCR 2021.
¹⁷Bench test data on file at Medtronic, D00333762, Rev A. May not be indicative of clinical performance.
¹⁸Taranini G, Fovino LN, Varbella F, et al. A large, prospective, multicentre study of left main PCI using a latest-generation zotarolimus-eluting stent: the ROLEX study. *EuroIntervention.* Published online August 31, 2022.
¹⁹Windecker S, Latib A, Kedhi E, et al. Polymer-based or Polymer-free Stents in Patients at High Bleeding Risk. *N Engl J Med.* March 26, 2020;382(13):1208-1218.

See the device manual for detailed information regarding the instructions for use, the implant procedure, indications, contraindications, warnings, precautions, and potential adverse events. For further information, contact your local Medtronic representative and/or consult the Medtronic website at www.medtronic.eu. For applicable products, consult instructions for use on manuals.medtronic.com. Manuals can be viewed using a current version of any major internet browser. For best results, use Adobe Acrobat[®] Reader with the browser.

Medtronic

Europe
 Medtronic International Trading Sàrl.
 Route du Molliau 31
 Case postale
 CH-1131 Tolochenaz
 Tel: +41 (0)21 802 70 00
 Fax: +41 (0)21 802 79 00

UC202306018EE-onyx-trustar-des-brochure-en-we-8109333 ©2022 Medtronic. All rights reserved. Medtronic and the Medtronic logo are trademarks of Medtronic. All other brands are trademarks of a Medtronic company. For distribution only in markets where the Onyx TruStar coronary stent system has been approved. Not for distribution in the USA, Japan, France, or Canada.

medtronic.eu

Medtronic



Onyx TruStar[™] DES

Designed to lead the way



Designed to deliver



Designed differently



Designed for complex PCI

1-mo DAPT

Onyx TruStar DES is indicated for 1-month DAPT in high bleeding risk (HBR) patients, including those unable to tolerate long-term DAPT

Onyx ONE Global Trial¹⁴
 1,003 Resolute Onyx DES patients studied

COMPLEX PATIENTS

33% AF patients
53% ACS patients
39% diabetic patients

COMPLEX LESIONS


46% moderate to severe calcified lesions
80% B2/C lesions
38 mm average stented length

- Indication is based on the results from the Onyx ONE Global Trial, which evaluated real-world, complex, HBR patients on 1-month DAPT treated with a Resolute Onyx DES or a BioFreedom[™] DCS
- The data is intended to better inform short-DAPT decisions in these patients, including those at high risk of thrombotic events¹⁴
- Results showed that Resolute Onyx DES was safe and effective¹⁴

Designed to deliver

Onyx TruStar DES introduces an enhanced delivery system[#] designed to take the acute performance of Resolute Onyx™ DES even further.

Enhanced delivery system[#] features:

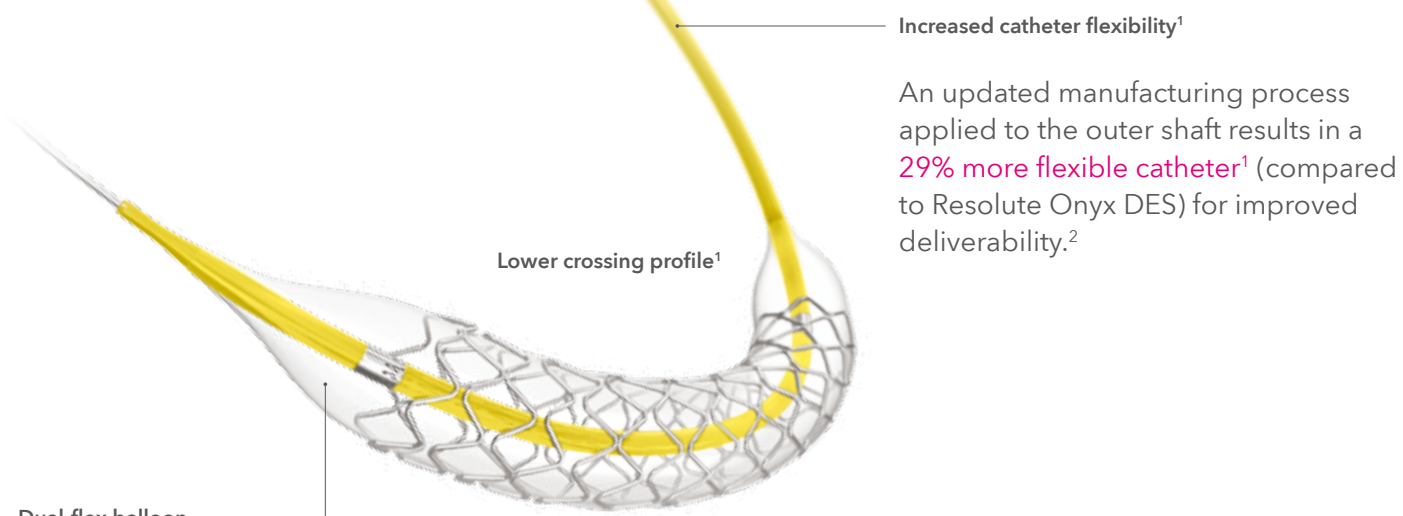


Provides increased flexibility and is comprised of a unique blend of two layers:

- Inner layer enhances flexibility³
- Outer layer maintains strength⁴

This results in a **thinner balloon[#]** with the same rated burst pressure (RBP)⁴ and a 7.5% lower crossing profile compared to Resolute Onyx DES.¹



Deliverability comparison 3.0 mm DES

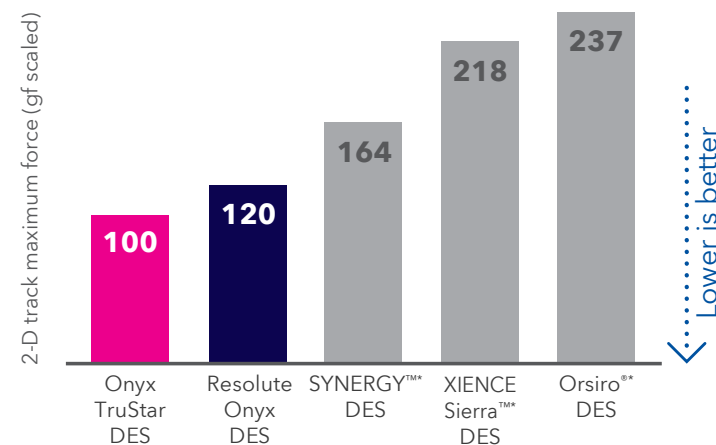


At least
39%
more deliverable than competitive DES^{#2}

[#]Stent delivery system updates were implemented on the 2.0-4.0 mm Onyx TruStar DES diameters.

Designed differently

Onyx TruStar DES builds off the legacy of Resolute Onyx DES, featuring the same stent design differentiators that provide the conformability,⁵ visibility,⁶ fast healing,⁷ and size matrix you've come to rely on.

In comparison to laser-cut drug-eluting stents, only Medtronic DES are made from a single wire to enable a fluid range of motion and the conformability needed for **superior strut apposition.**⁵

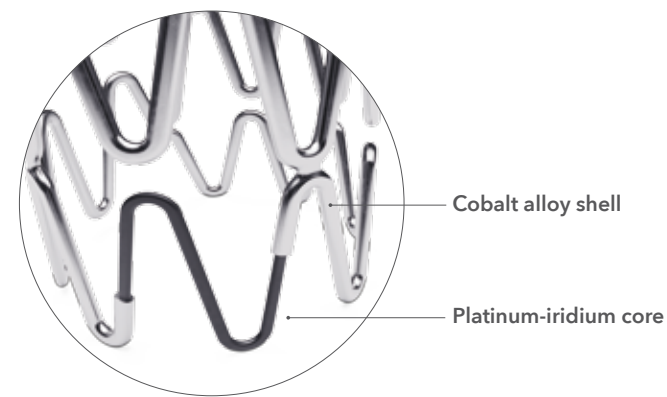

The platinum-iridium core within Onyx TruStar DES is **more visible⁶** than competitive DES, while enabling greater radial strength⁶ with thin struts.

The zotarolimus drug inhibits neointimal growth,⁸ while the BioLin[™] biocompatible polymer – the only polymer specifically designed for a DES – **promotes faster healing.**⁷


Only Medtronic offers DES in **2.0 mm to 5.0 mm** sizes, with overexpansion capabilities up to 6.0 mm,⁵ to treat the broadest range of coronary vessel diameters.

Platform	Diameter (mm)	Stent length (mm)										MSID ⁹ (mm)
		8	12	15	18	22	26	30	34	38	4.00	
Small vessels	2.00	8	12	15	18	22	26	30	—	—	3.50	
	2.25	8	12	15	18	22	26	30	34	38	3.50	
Medium vessels	2.50	8	12	15	18	22	26	30	34	38	3.50	
	2.75	8	12	15	18	22	26	30	34	38	4.00	
Large vessels	3.00	8	12	15	18	22	26	30	34	38	4.00	
	3.50	8	12	15	18	22	26	30	34	38	5.00	
Extra-large vessels	4.00	8	12	15	18	22	26	30	34	38	5.00	
	4.50	—	12	15	18	22	26	30	—	—	6.00	
	5.00	—	12	15	18	22	26	30	—	—	6.00	

Four platforms specifically designed to meet the unique needs of each vessel size.


Designed for complex PCI

An exclusive set of design features and meaningful clinical data inherited from Resolute Onyx DES provide support for your most challenging cases.

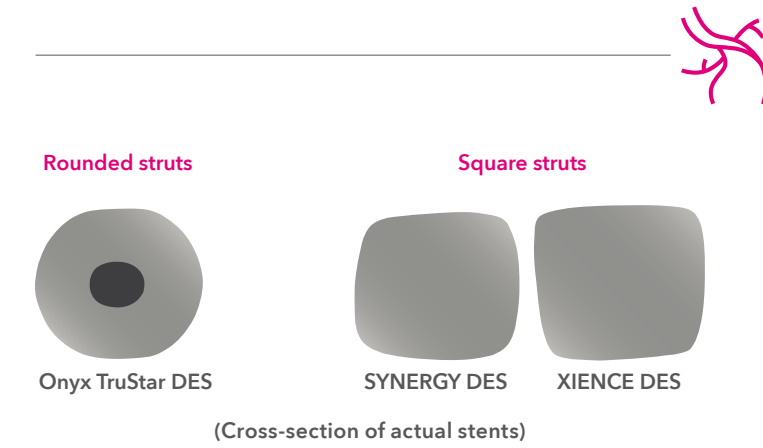


Extra-small vessels (2.00-2.50 mm)

- 2.0 mm offers the lowest crossing profile of any DES¹⁰
- Demonstrated 2% target lesion revascularisation and 0% stent thrombosis at one year in a complex, small-vessel population¹¹

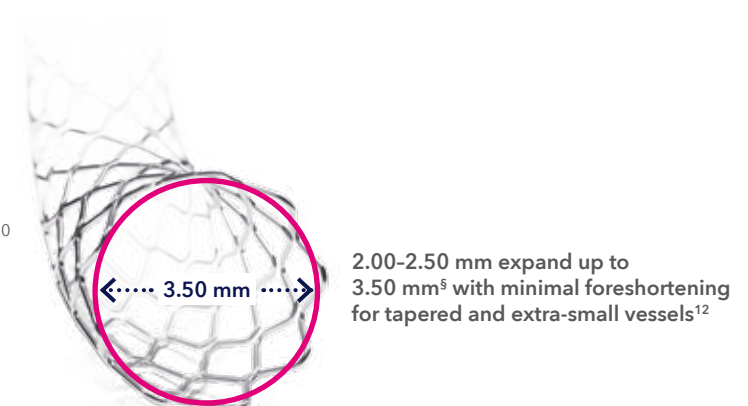


2.00-2.50 mm expand up to 3.50 mm⁵ with minimal foreshortening for tapered and extra-small vessels¹²

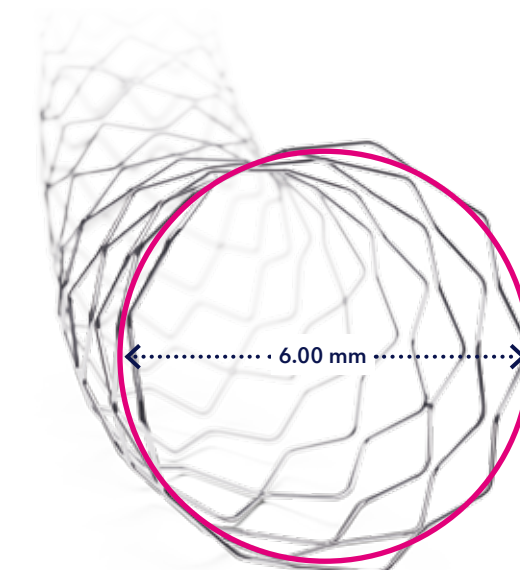

4.50-5.00 mm expand up to 6.00 mm⁵ while maintaining structural integrity¹²

ROLEX Registry

Low 5.1% TLF, 2.0% TLR, and 1.1% ST at one year¹³

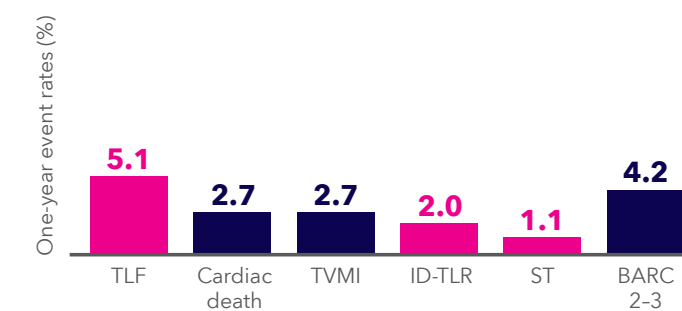

Left main and other extra-large vessel PCI (4.50-5.00 mm)

- Specifically designed with additional crowns and thicker struts⁹ to provide the radial strength needed for the left main and extra-large vessels¹²
- ROLEX Registry showed Resolute Onyx DES was safe and effective in left main PCI in a complex patient population¹³

59% multivessel disease
53% acute coronary syndrome
30% diabetic