





Telescopes

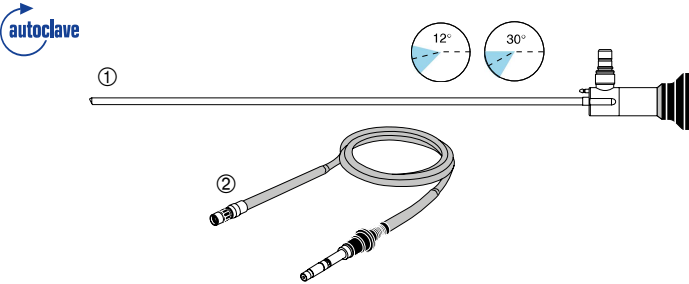

- ① **WA2T412A** Telescope "OES ELITE", 4 mm, HD, autoclavable, 12°
- WA2T430A** Telescope "OES ELITE", 4 mm, HD, autoclavable, 30°
- ② **WA03300A** Light-guide cable, 2.8 mm, 3 m, CF type


For details on "OES ELITE" Telescopes, see page 61.

Resection Sheaths

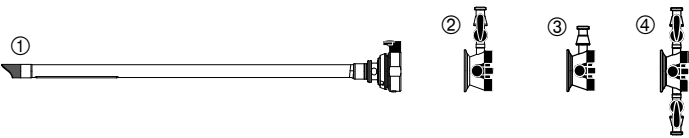


	24 Fr.	26 Fr.	28 Fr.	
①	A22041A	A22042A	-	Resection sheath, without irrigation port, incl. standard obturator
	A22041T	A22042T	-	Resection sheath, without irrigation port, incl. obturator with deflecting tip
②	A22051A	A22051A	A22051A	Irrigation port, for resection sheaths, 1 stopcock, rotatable
	A22054A	A22054A	A22054A	Irrigation port, for resection sheaths, 1 vertical stopcock, fixed
③	A22052A	A22052A	A22052A	Irrigation port, for resection sheaths, 1 Luer-lock connector, rotatable
④	A22053A	A22053A	A22053A	Irrigation port, for resection sheaths, 2 stopcocks, rotatable

Obturator

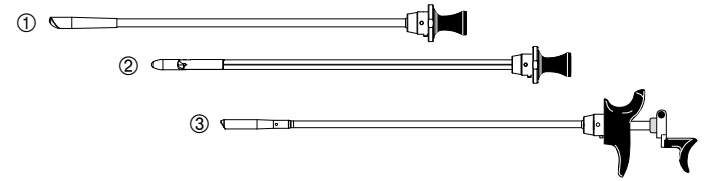

	26 Fr.	27 Fr.	
①	A22081A	A22082A	Obturator, standard
②	A22085A	A22086A	Obturator, deflecting tip
③	A22071A	A22072A	Obturator, optical


PLASMA

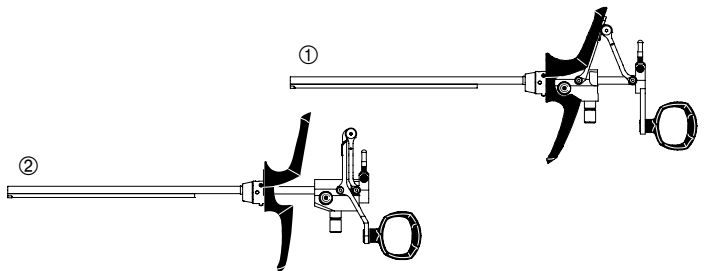

- ① **WA22366A** Working element, active, for resection in saline
- ② **WA22367A** Working element, passive, for resection in saline

For PLASMA resection electrodes and HF cable, see page 69 and 70.
 For PK Technology PLASMA resection electrodes with cables, see page 77.

Monopolar

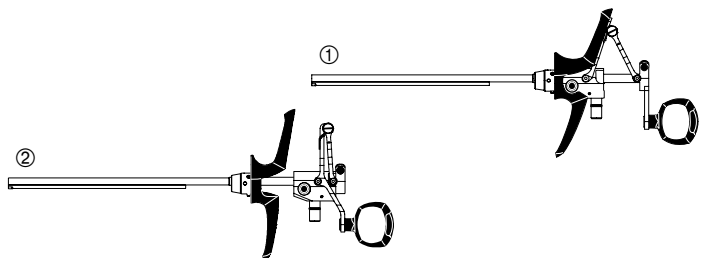


- ① **WA22066A** Working element, active
- ② **WA22067A** Working element, passive

For monopolar HF resection electrodes and HF cables, see page 81 and 82.

ESG PLASMA Electrodes

**24 Fr. Sterile, Single-Use
26 Fr. HF-Resection Electrodes
27 Fr.**

STERILE

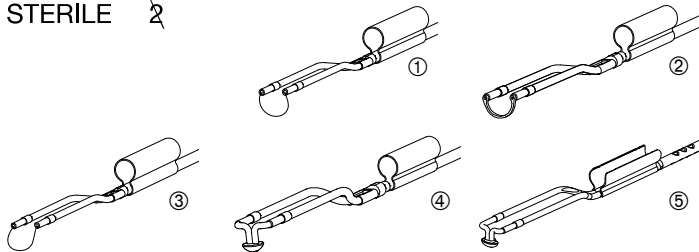


- ① **WA22301S** HF-resection electrode "PlasmaLoop", small loop, 24 Fr., 12°/16°, in saline
- WA22302D** HF-resection electrode, loop, 24 Fr., 0.2 wire, medium, 12°, sterile, single use, 12 pcs., for TURis
- WA22503D** HF-resection electrode, loop, 24 Fr., 0.2 wire, large, 12°, sterile, single use, 12 pcs., for TURis
- WA22305S** HF-resection electrode "PlasmaLoop", small loop, 24 Fr., 12°-30°, in saline
- WA22306D** HF-resection electrode, loop, 24 Fr., 0.2 wire, medium, 30°, sterile, single use, 12 pcs., for TURis
- WA22507D** HF-resection electrode, loop, 24 Fr., 0.2 wire, large, 30°, sterile, single use, 12 pcs., for TURis
- ② **WA22521C** HF-resection electrode, band, 24 Fr., medium, 12°, sterile, single use, 12 pcs., for TURis
- WA22523C** HF-resection electrode, band, 24 Fr., medium, 30°, sterile, single use, 12 pcs., for TURis
- ③ **WA22331D** HF-resection electrode, loop, 24-28 Fr., 0.2 wire, small, 45° angled, 12° and 30°, sterile, single use, 12 pcs., for TURis
- WA22332D** HF-resection electrode, loop, 24-28 Fr., 0.2 wire, medium, 45° angled, 12° and 30°, sterile, single use, 12 pcs., for TURis
- ④ **WA22557C** HF-resection electrode, button, 24-28 Fr., 12° and 30°, sterile, single use, 12 pcs., for TURis
- ⑤ **WA22566S** HF-resection electrode "Plasma-OvalButton", oval button, 24 Fr., 12°-30°, in saline

S = 5 pcs.
C/D = 12 pcs.

**24 Fr. Sterile, Single-Use
26 Fr. HF-Resection Electrodes
27 Fr. (cont.)**

STERILE

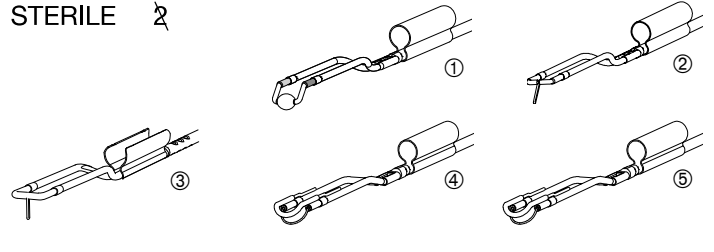

- ① **WA22351C** HF-resection electrode, roller, 24-28 Fr., 12° and 30°, sterile, single use, 12 pcs., for TURis
 - For coagulation only
- ② **WA22355C** HF-resection electrode, 45° needle, 24-28 Fr., 12° and 30°, sterile, single use, 12 pcs., for TURis
- ③ **WA22540S** HF-resection electrode "PlasmaNeedle", right-angled needle, 24 Fr., 12°-30°, in saline
- ④ **WA22558C** HF-resection electrode, loop, 24-28 Fr., 45° angled, 12° and 30°, sterile, single use, 12 pcs., for TURis enucleation
- ⑤ **WA22559S** HF-resection electrode "Plasma-TUEBLoop", loop, TUEB, 24 Fr., 12°-30°, in saline

S = 5 pcs.
C = 12 pcs.