

### Specificație tehnică completată

**Model: Logiq Fortis; Producator: GE Ultrasound Korea, GE Medical Systems SCS;  
Tara: Korea si Franta**

Specificarea tehnică deplină solicitată de către autoritatea contractantă	Specificarea tehnică deplină propusă de către autoritatea ofertantă
<p>Ultrasonograf General, Cardiac performanță înaltă Cod 300100 APLICAȚII CLINICE General, cardiac</p> <p>PROBE PORTURI <math>\geq 5</math> active</p> <p>PROBE TIP, MHz Linear 4 – 14 MHz</p> <p>numar de elemente <math>\geq 250</math></p> <p>Convex 1.5 -6,0 MHz</p> <p>"numar de elemente <math>\geq 192</math> Tehnologie Syngle Crystal (mono-cristal)"</p> <p>Phased/Vector 1,5-4,5 MHz</p> <p>numar de elemente <math>\geq 80</math>, Tehnologie Syngle Crystal (mono-cristal) NIVELE DE GRI <math>\geq 256</math></p> <p>GAMA DINAMICA <math>\geq 260</math>dB</p> <p>Adâncimea scanării <math>\geq 40</math> cm</p> <p>PREPROCESARE, canale digitale <math>\geq 8.000.000</math></p> <p>POSTPROCESARE da IMAGINE MODURI</p> <p>M-mod da</p>	<p>Ultrasonograf General, Cardiac, performanță înaltă Cod 300100 APLICAȚII CLINICE General, cardiac, <b>DA Vezi pagina 2 din LOGIQ Fortis R3.x HDU Product Specification Sheet "Applications "</b></p> <p>PROBE PORTURI <math>\geq 5</math>, cel puțin 4 active + <b>1 inactiv DA Vezi pagina 2 din LOGIQ Fortis R3.x HDU Product Specification Sheet " Console Design "</b></p> <p>PROBE TIP, MHz <b>DA</b> Linear <b>4 - 16 MHz - MODEL: ML6-15-D Vezi pagina 19 din LOGIQ Fortis R3.x HDU Product Specification Sheet</b></p> <p>numar de elemente - <b>1008 DA</b> <b>Tehnologie Matriciala sau sigle cristal inclusă</b> Convex <b>1.0 -6,0 MHz - MODEL: C1-6-D Vezi pagina 16 din LOGIQ Fortis R3.x HDU Product Specification Sheet</b></p> <p>numar de elemente - <b>192 DA</b> Tehnologie Syngle Crystal (mono-cristal) – <b>XDclear inclusă</b> Phased/Vector <b>1-5 MHz – MODELUL: M5Sc-D Vezi pagina 19 din LOGIQ Fortis R3.x HDU Product Specification Sheet</b></p> <p>numar de elemente – <b>288 DA</b> Tehnologie Syngle Crystal (mono-cristal)- <b>XDclear</b> NIVELE DE GRI - <b>256 DA Vezi pagina 7 din LOGIQ Fortis R3.x HDU Product Specification Sheet</b></p> <p>GAMA DINAMICA <math>\geq 260</math>dB <b>DA Vezi pagina 7 din LOGIQ Fortis R3.x HDU Product Specification Sheet " Adjustable dynamic range, infinite upper level"</b></p> <p>Adâncimea scanării - <b>100 cm DA Vezi pagina 7 din LOGIQ Fortis R3.x HDU Product Specification Sheet</b></p> <p>PREPROCESARE, canale digitale <math>\geq 8.000.000</math> <b>DA</b> <b>DA Vezi pagina 7 din LOGIQ Fortis R3.x HDU Product Specification Sheet " cSound™ Imageformer: Infinite number of effective channels"</b></p> <p>POSTPROCESARE <b>DA</b> <b>IMAGINE MODURI - Vezi pagina 2 din LOGIQ Fortis R3.x HDU Product Specification Sheet " Operation Modes "</b></p> <p>M-mod <b>DA</b></p>



Anexa 9

M-mod și 2-D da	M-mod și 2-D/ <b>B-Mode DA</b>
Mod Anatomic si Anatomic Curbat da	Mod Anatomic si Anatomic Curbat <b>DA Vezi pagina 11 din LOGIQ Fortis R3.x HDU Product Specification Sheet ” TVI (Option)”</b>
Harmonic imaging da	Harmonic imaging <b>DA Vezi pagina 9 din LOGIQ Fortis R3.x HDU Product Specification Sheet ” Coded Harmonic Imaging”</b>
Imagine prin Compunere Spatiala da	Imagine prin Compunere Spatiala <b>DA Vezi pagina 9 din LOGIQ Fortis R3.x HDU Product Specification Sheet ” CrossXBeam”</b>
DOPPLER Tip CW, PW, CFM	DOPPLER Tip CW, PW, CFM <b>DA Vezi pagina 2 din LOGIQ Fortis R3.x HDU Product Specification Sheet ” Operation Modes ”</b>
Afișare frecvență da	Afișare frecvență <b>DA Vezi pagina 4 din LOGIQ Fortis R3.x HDU Product Specification Sheet ” Display Annotaion ”</b>
Afișare viteză da	Afișare viteză <b>DA Vezi pagina 4 din LOGIQ Fortis R3.x HDU Product Specification Sheet ” Digital B-Mode/ Digital M-Mode”</b>
Power Doppler da	Power Doppler <b>DA Vezi pagina 4 din LOGIQ Fortis R3.x HDU Product Specification Sheet ”Digital Power Doppler Imaging”</b>
Duplex da	Duplex <b>DA Vezi pagina 3 din LOGIQ Fortis R3.x HDU Product Specification Sheet ”Simultaneous capability –Ex B/M”</b>
Triplex da	Triplex <b>DA Vezi pagina 3-4 din LOGIQ Fortis R3.x HDU Product Specification Sheet ”Simultaneous capability –Ex B/CFM/PW”</b>
<b>FUNCȚIONALITĂȚI</b>	<b>FUNCȚIONALITĂȚI</b>
Măsurători digitale da	Măsurători digitale <b>DA Vezi pagina 9din LOGIQ Fortis R3.x HDU Product Specification Sheet ”Measurment/Calculations”</b>
Optimizarea automata a imaginii prin apăsarea unui buton da	Optimizarea automata a imaginii prin apăsarea unui buton <b>DA Vezi pagina 9din LOGIQ Fortis R3.x HDU Product Specification Sheet ”Auto Optimization”</b>
Diapazon dinamic selectabil da	Diapazon dinamic selectabil <b>DA Vezi pagina 7 din LOGIQ Fortis R3.x HDU Product Specification Sheet ”Scanning Parameters”</b>
Focalizare de transmisie ajustabilă da	Focalizare de transmisie ajustabilă <b>DA</b>
Focalizare de recepție dinamică da	Focalizare de recepție dinamică <b>DA</b>
Măsurători pe reluarea video da	Măsurători pe reluarea video <b>DA</b>
Măsurarea automată a intimei-media da	Măsurarea automată a intimei-media <b>DA Inclus Vezi pagina 7 din LOGIQ Fortis R3.x HDU Product Specification Sheet ”Auto Ejection Fraction”</b>
Măsurarea automată a fracției de ejeecție da	Măsurarea automată a fracției de ejeecție <b>DA Inclus Vezi pagina 7 din LOGIQ Fortis R3.x HDU Product Specification Sheet ”System Options”</b>
Vizualizare în rezoluție înaltă a fluxului sangvin da	Vizualizare în rezoluție înaltă a fluxului sangvin <b>DA Vezi pagina 5, 6, 8, 12, 14, 18, 19,20, 22,23, 35 din LOGIQ Fortis™ Powerful   Streamlined   Multi-purpose Always ready. Always by your side</b>



Anexa 9

Vizualizare în regim 3D a fluxului sangvin 2D color da	Vizualizarea 3D a fluxului în regim 2D <b>DA Vezi pagina 5, 6, 8, 12, 14, 18, 19,20, 22,23, 35 din LOGIQ Fortis™ Powerful   Streamlined   Multi-purpose Always ready. Always by your side.</b>
StressEcho da	StressEcho <b>DA Vezi pagina 11 din LOGIQ Fortis R3.x HDU Product Specification Sheet "Stress echo"</b>
Soft de îmbunătățire a imaginii în regim cardiac da	Soft de îmbunătățire a imaginii în regim cardiac <b>DA</b>
Analiza cantitativa TDI da	Analiza cantitativa TDI ( <b>Doppler Tisular</b> ) <b>DA</b>
Urmărirea mișcării țesuturilor (Tissue Tracking) da	<b>prescurtarea folosita de GE Healthcare este TVI si este valabil acest lucru, pentru regimul vascular este Quantitative flow analysis</b> Urmărirea mișcării țesuturilor (Tissue Tracking) <b>DA</b>
Vizualizare a imaginii de contrast da, optional	<b>DA Prescurtarea folosita de GE Cardiac Strain/Cardiac AFI</b> Vizualizare a imaginii de contrast da, optional <b>DA</b>
PAN/ZOOM imagine în timp real da	<b>Vezi pagina 5, 6, 8, 12, 14, 18, 19,20, 22,23, 35 din LOGIQ Fortis™ Powerful   Streamlined   Multi-purpose Always ready. Always by your side</b>
imagine înghețată da	PAN/ZOOM imagine în timp real <b>DA</b>
STOCARE IMAGINI Capacitate ≥ 512GB SSD sau Hybrid (SSD+HDD)	imagine înghețată <b>DA</b>
Cine da	STOCARE IMAGINI Capacitate - 1Tb SSD <b>DA Vezi pagina 1 din LOGIQ Fortis R3.x HDU Product Specification Sheet " Console Design"</b>
DICOM 3.0 COMPLIANT da	Cine <b>DA Vezi pagina 6 din LOGIQ Fortis R3.x HDU Product Specification Sheet "CINE Memory/Image Memory"</b>
PACHETE DE ANALIZĂ	DICOM 3.0 COMPLIANT <b>DA Vezi pagina 6 din LOGIQ Fortis R3.x HDU Product Specification Sheet " Connectivity"</b>
General da	<b>PACHETE DE ANALIZĂ</b>
Cardiac	General <b>DA</b>
Regim panoramic avansat da	Cardiac <b>DA H43332CA Include: The Cardiac Package includes the following advanced tools: ECG Kit (incl.AutoEF &amp; TVI ) , IEC ECG cable, Cardiac AFI, Stress Echo, AutoIMT , Flow QA, Comapre Ass., Scan Ass.</b>
Elastografie strain (de compresie manuală) da	Regim panoramic avansat <b>DA</b>
Elastografie sharewave (compresie acustică) pentru sondele convexe, liniare, endocavitare da	Elastografie de tip compresiv (de compresie manuală) <b>pe sondele convexe, liniare și endocavitare DA Vezi pagina 11 din LOGIQ Fortis R3.x HDU Product Specification Sheet " Strain elastography" – PN H43332LC + H43332LD</b>
Soft inteligent de analiză a țesutului glandei mamare da	Elastografie sharewave (compresie acustică) pentru sondele convexe, liniare, endocavitare <b>DA Vezi pagina 11 din LOGIQ Fortis R3.x HDU Product Specification Sheet "Shear wave elastography" –PN H46622LE</b>
	Soft inteligent de analiză a țesutului glandei mamare <b>DA</b>



## Anexa 9

<p>Soft inteligent de analiză a țesutului glandei tiroide da  Soft dedicat pentru analiza planseului pelvin da  Altele Să se indice  Modul ECG cu accesorii da  Timp de încărcare a sistemului nu mai mare de 45 sec da</p> <p><b>MONITOR</b>  rezoluție înaltă, <math>\geq 1920 \times 1080 \text{px}</math> <math>\geq 23''</math></p> <p>Unghi de vizualizare <math>\geq 175^\circ</math></p> <p>Monitor integrat de control touch-screen, rezoluție FullHD <math>\geq 12''</math></p> <p>reglarea unghiului de înclinare da</p> <p>Panou de control reglabil pe înălțime, cel puțin <math>\pm 14 \text{cm}</math> da, manual</p> <p>rotire, cel puțin <math>\pm 70^\circ</math> da</p> <p>butoane configurabile, cel puțin 6 da</p> <p>Baterie integrată timp de lucru de la baterie, cel puțin 40 min da, optional</p> <p>Încălzitor gel da</p> <p>Port USB <math>\geq 5</math> da  DIVIZARE MONITOR da</p>	<p>Soft inteligent de analiză a țesutului glandei tiroide <b>DA</b>  Soft dedicat pentru analiza planseului pelvin <b>DA</b>  Altele Să se indice  Modul ECG cu accesorii <b>DA Inclus in PN H43332CA</b>  Timp de încărcare a sistemului nu mai mare de 45 sec da</p> <p><b>MONITOR</b>  rezoluție înaltă, <math>- 1920 \times 1080 \text{px}</math> , <b>23,8'' DA Vezi pagina 1 din LOGIQ Fortis R3.x HDU Product Specification Sheet "Monitor"</b>  Unghi de vizualizare - <b>89/89/89/89° DA Vezi pagina 1 din LOGIQ Fortis R3.x HDU Product Specification Sheet "Monitor"</b>  Monitor integrat de control touch-screen rezoluție FullHD <b>12,1'' DA Vezi pagina 1 din LOGIQ Fortis R3.x HDU Product Specification Sheet "Touch Screen"</b>  reglarea unghiului de înclinare <b>DA pentru monitorul central</b></p> <p>Panou de control reglabil electronic pe înălțime <b>50 cm DA vezi pagina 3-51 din LOGIQ Fortis – Basic User Manual , Vezi pagina 1 din LOGIQ Fortis R3.x HDU Product Specification Sheet "Dimensions and Weight "</b>  rotire, cel puțin <math>\pm 70^\circ</math> <b>DA vezi pagina 3-52 din LOGIQ Fortis – Basic User Manual , Vezi pagina 1 din LOGIQ Fortis R3.x HDU Product Specification Sheet "Dimensions and Weight "</b>  Butoane configurabile Cel puțin 6 <b>DA vezi pagina 13-14 din LOGIQ Fortis – Basic User Manual</b>  Baterie integrată timp de lucru de la baterie, cel puțin 20 min da, <b>optional vezi pagina 13-537 din LOGIQ Fortis – Basic User Manual</b>  Încălzitor gel <b>DA Vezi pagina 1 din LOGIQ Fortis R3.x HDU Product Specification Sheet "Operator Keyboard "</b>  Port USB - 5 <b>DA</b>  DIVIZARE MONITOR <b>DA</b></p>
--	---



REGISTRUL DE STAT AL DISPOZITIVELOR MEDICALE

Tip	Denumire
I.3. Certificatul CE	Certificat CE
I.2. Declarația de conformitate CE	Declaratie de conformitate CE

Nr	Denumire	Den.comerc.	Model	Nr. catalog	Tara	Producatorul	Reprezentant	Ordin	Data	Cod vamal
<input type="text"/>	<input type="text"/>	<input type="text" value="fortis"/>	<input type="text" value="hdu"/>	<input type="text"/>	<input type="text"/>	<input type="text"/>	<input type="text"/>	<input type="text"/>	<input type="text"/>	<input type="text"/>
DM000349915	ULTRASONOGRAF	LOGIQ FORTIS™	ULTRASOUND CONSOLE HDU	H43302LA	Coreea Sud	GE ULTRASOUND KOREA, LTD.	INTERMED S.R.L.	Rg04-000115	12-05-2022	

☒  Содержит([Model], 'hdu') И Содержит([NameMake], 'fortis'). [Очистить](#)





## EC DECLARATION OF CONFORMITY

Following the provisions of the medical devices regulation 2017/745

Following the directive 2011/65/EU, directive 2014/53/EU

We

Manufacturer and manufacturing site	EU Authorized Representative
<b>GE Ultrasound Korea, Ltd.</b> 9, Sunhwan-ro 214beon-gil, Jungwon-gu, Seongnam-si Gyeonggi-do 13204, Republic of Korea SRN: KR-MF-000001860	<b>GE Medical Systems SCS</b> 283 rue de la Minière 78530 BUC, France SRN: FR-AR-000000344

Declare under our sole responsibility that the device:

### LOGIQ Fortis

Basic UDI-DI: **8406821BUG00214GZ**

Identification number:

REF Catalog	H-Catalog Number	UDI-DI
<b>LOGIQ Fortis HDU</b>	<b>H43302LA</b>	<b>00195278405326</b>
<b>LOGIQ Fortis LCD</b>	<b>H43302LB</b>	<b>00195278405333</b>

Intended Purpose: The LOGIQ Fortis is a general-purpose diagnostic ultrasound system intended for use by qualified and trained healthcare professionals for ultrasound imaging, measurement, display and analysis of the human body and fluid.

EMDN Code: **Z110401**

EMDN Description: Ultrasound Scanners

GMDN Code: **40761**

GMDN Description: General-purpose ultrasound imaging system

UMDNS Code: **15-976**

Classification: **IIa**

Classification rule (Annex VIII): **Rule 10, Class: IIa**

To which this declaration relates is in conformity with the requirements of the medical devices regulation 2017/745 that apply to it and with the requirements of the directive 2011/65/EU on the restriction of the use of certain hazardous substances in electrical and electronic equipment (RoHS) and the directive 2014/53/EU on the radio equipment (RED).





This conformity is based on the following elements:

- Technical Documentation reference: DOC2379389, of the product to which this declaration relates.
- EC certificate No. HZ 2004702-01:
  - Conformity assessment procedure followed: Annex IX of the medical device regulation 2017/745
  - Delivered by TUV Rheinland LGA Products GmbH (Notified Body n° 0197)

This EC declaration of conformity is the initial release.

**SIGNATURE:**

Date of issue: 13-12-2021  
Place of issue: China  
Name: Qingmeng Chen  
Function: Regulatory Affairs Program Manager  
Signature:

*Qingmeng Chen*





**ADDENDUM TO THE EC DECLARATION OF CONFORMITY**  
**LOGIQ Fortis including accessories and components**  
**dated 13-12-2021**

Product Description	H-Catalog Number <sup>1</sup>
<b>Ultrasound Console</b>	
LOGIQ Fortis HDU Console	H43302LA / 6602000
LOGIQ Fortis LCD Console	H43302LB / 6601000
<b>Probe Options<sup>2</sup></b>	
IC5-9-D	H40442LK
ML6-15-D	H40452LG
L8-18i-D	H40452LL
C2-9-D (XDClear)	H40462LN
C1-6-D (XDClear)	H40472LT
C1-6VN-D (XDClear)	H40472LW
C2-9VN-D (XDClear)	H40472LY
C3-10-D (XDClear)	H40482LB
M5Sc-D (XDClear)	H44901AE
L2-9-D	H44901AI
L2-9VN-D	H44901AJ
6Tc-RS	H45551ZE
C2-7-D	H46422LM
C2-7VN-D	H46422LN
P2D	H4830JE
RIC5-9-D	H48651MS
RAB6-D	H48681MG
P6D	H4830JG
BE9CS-D	H40482LE
L3-12-D	H48062AA
6S-D	H45021RR
L6-24-D Probe	H4920HF
<b>TEE Probe Accessories<sup>2</sup></b>	
TEE RS-DLP Adapter	H46352LK
Adult TEE Clip-on Bite Guard	H45511EE
Adult TEE Clip-on Bite Guard Opr.	H45521CB
Adult TEE Scanhead Protection Cover	H45521CK
Adult TEE Conventional Bite Guard	H45521JH
BITE HOLE INDICATOR	H45531HS
TEE STORAGE RACK	H45551NM
<b>Software Options</b>	
Advanced Security	H46622LL
Coded Contrast	H43332LA
Parametric Imaging	H43332LB
Cardiac AFI	H46622LN
LOGIQ Exx DVR	H4918DR
Report Writer	H46622LR
Stress Echo	H46622LS
Tricefy	H46622LT
LOGIQ Apps	H46622LW
KOIOS SW	H46622LY
LOGIQ Exx KOIOS Thyroid	H4920KT
LOGIQ E10 KOIOS INSTALL	H4919KI





Product Description	H-Catalog Number <sup>1</sup>
KOIOS 3.x INSTALL	H4921KY
Scan Assistant	H46622LZ
Advanced Probes	H46612LS
AUTO IMT	H46612LT
B Steer+	H46612LW
B-FLOW	H46612LY
Compare Assistant	H46612LZ
DICOM	H46622LA
FLOW QA	H46622LB
Measure Assist Breast	H46622LC
Measure Assist OB	H46622LD
Elastography	H43332LC
Elasto QA	H43332LD
Shear Wave Elastgraphy	H46622LE
LOGIQ Exx SRI HD Type2	H4920SR
UGAP	H46622LH
SonoNT SonoIT	H46622LJ
LOGIQ Exx VNAV Image	H4920VR
Hepatic Assistant - SWE-UGAP	H43332LE
Omni View	H43332LF
STIC	H43332LG
TUI	H43332LH
VCI-Static	H43332LJ
VOCAL_II	H43332LK
Thyroid Productivity	H43332LL
Breast Productivity	H43332LM
Vita on Demand	H43332LN
<b>Hardware Options<sup>2</sup></b>	
CW Doppler	H43342LA
Realtime 4D	H43342LB
ECG Option	H43342LC
Scan on battery option kit	H43342LD
Power Assistant	H43342LE
Volume Navigation	H43342LF
Volume Navigation for V-Nav Inside T1	H43372LK
Wireless Option	H43342LG
S-Video Option	H43342LH
Pencil CW	H43342LJ
<b>Peripheral Options<sup>2</sup></b>	
USB FOOTSWITCH 3 BUTTON	H46732LF
SONY UPD25MD COLOR PRINTR	H4911JT
BW Printer Installation Kit T1	H43342LK
LOGIQ Exx Protective Cover	H4918DC
LOGIQ Exx Inkjet Printer	H4918RP
LOGIQ Fortis High Cabinet	H43342LL
LOGIQ Fortis Low Cabinet	H43342LM
LOGIQ Fortis Side Cabinet	H43342LN
Sinch bay Option	H43342LP
<b>An Keyboard Assembly</b>	
AN Keyboard ENGLISH	H43342LR
AN Keyboard GERMAN	H43342LS
AN Keyboard FRENCH	H43342LT
AN Keyboard GREEK	H43342LW
AN keyboard NORWEGIAN	H43342LY





Product Description	H-Catalog Number <sup>1</sup>
AN Keyboard SWEDISH	H43352LA
<b>Accessories<sup>2</sup></b>	
Ethernet protection Cable	H43272LJ
FC389,ECG CABLE SET	H45521AL
VNav Stand (Offboard)	H4908NS
ECG CABLE - AHA STYLE	H4910EC
VNav NEEDLE TRACKING	H4910NT
VNav VirtuTRAX Starter Kit	H4910NY
ECG Cables IEC Style	H4911JC
VNav Virtual Tracker	H4911NG
VNav Active Tracker kit	H4913AT
VNav Needle Tracking storage insert	H4913NS
VNav Needle Tracking Kit - 18/20g or less	H4913NT
VNav ETRAX 12 14G ST KT	H4913NU
VNav ETRAX 14 16G ST KT	H4913NV
VNav Probe sensors	H4913PS
VNav MR Active Tracker	H4915MT
Small Probe Holder	H43352LC
VERTICAL TV PROBE HOLDER	H43352LD
TVTR Probe Holder	H43352LE
PROBE CABLE HANGER	H44412LA
OPTION TRAY BOX	H43372LF
OPTION TRAY Bracket	H43372LG
<b>Power Cords Destination Sets</b>	
Power Cord 220V for EU	H46342LZ
Power Cord DK STD C13 GRY	H46692LK
DESTINATION SET UK	H46712LM
DESTINATION SET SWISS	H46712LS
DESTINATION SET DENMARK	H46712LT
DESTINATION SET ITALY	H46722LD
<b>V-nav Options<sup>2</sup></b>	
ML6-15 M_BPSY_TRU3D_SKIT	H40432LK
C3-10 VNav Holder Starter Kit	H40482LF
IC5-9 V NAV BRACKET	H4908NF
L8-18I V NAV BRACKET	H4908NH
M5S V NAV BRACKET	H4908NM
<b>Biopsy Kits<sup>2</sup></b>	
E721 STARTER KIT	E8385MJ
IC5-9-D Reusable Biopsy Guide	H40412LN
ML6-15 M_BIOPSY_SKIT	H40432LJ
C2-7 Biopsy Kit	H40482LK
C2-7 Biopsy Kit Stainless	H40482LL
L2-9 Needle Guide Starter Kit	H44901AM
M5Sc-D Biopsy Bracket	H45561FC
RAB BIOPSY STARTER KIT	H46701AE
RIC5-9-D Biopsy Guide	H46721R
C2-9 Biopsy Starter Kit	H4913BA
C1-6-D Verza Biopsy Starter Kit	H4917VB
C1-6-D Biopsy Starter Kit	H4913BB
L3-12-D Biopsy Kit	H48302AA
RAB6-D BIOPSY STARTER KIT	H48681ML
BE9CS Biopsy Kit 742-401	H42742LJ





Notes:

[1] *H-Catalog number identifies the device(s) in the manufacturer's catalog and is usually included on commercial documents like sales contract, order processing documents and shipping documents.*

[2] *Probes and accessories may carry the CE-mark and when applicable, the Notified Body number corresponding to the EC Declaration under which the products are CE-marked by their manufacturer. GE Ultrasound Korea Ltd. has verified the mutual compatibility of the devices in combination with LOGIQ Fortis and included relevant information to users with the LOGIQ Fortis instructions for use.*

---

End of Document



## **ATTESTATION CE / EC CERTIFICATE**

**Approbation du Système Complet d'assurance Qualité / Approval of full Quality Assurance System**

**ANNEXE II excluant le point 4 Directive 93/42/CEE relative aux dispositifs médicaux**

**ANNEX II excluding section 4 Directive 93/42/EEC concerning medical devices**

**Pour les dispositifs de classe III, un certificat CE de conception est requis**

**For class III devices, a EC design certificate is required**

**Fabricant / Manufacturer**

**GE ULTRASOUND KOREA, Ltd.**

**9, Sunhwan-ro 214beon-gil, Jungwon-gu,**

**SEONGNAM-SI, GYEONGGI-DO, REPUBLIC OF KOREA**

**Catégorie du(des) dispositif(s) / Device(s) category**

**Dispositif ou système de diagnostic par ultrasons**

*Ultrasound diagnostic device or system*

**Voir document complémentaire GMED / See GMED additional document**

**n° 36988**

**GMED atteste qu'à l'examen des résultats figurant dans le rapport référencé P183396, P601203, le système d'assurance qualité - pour la conception, la production et le contrôle final - des dispositifs médicaux énumérés ci-dessus est conforme aux exigences de l'annexe II excluant le point 4 de la Directive 93/42/CEE.**


*GMED certifies that, on the basis of the results contained in the file referenced P183396, P601203, the quality system - for design, manufacturing, and final inspection - of medical devices listed here above complies with the requirements of the Directive 93/42/EEC, annex II excluding section 4.*

**La validité du présent certificat est soumise à une vérification périodique ou imprévue**

**The validity of the certificate is subject to periodic or unexpected verification**

**Début de validité / Effective date : September 14th, 2020 (included)**

**Valable jusqu'au / Expiry date : May 26th, 2024 (included)**



**Lionel DREUX**  
**Certification Director**



Ce document complémentaire GMED n° 36988 rev. 0 atteste de la validité du certificat CE n° 7697 rev. 18 au regard des informations listées ci-dessous.


*This GMED additional document N° 36988 rev. 0 attests to the validity of CE certificate n° 7697 rev. 18 with regard to the information listed below.*

Fabricant / Manufacturer:

**GE ULTRASOUND KOREA, Ltd.**  
9, Sunhwan-ro 214beon-gil, Jungwon-gu,  
SEONGNAM-SI, GYEONGGI-DO, REPUBLIC OF KOREA

### Identification des dispositifs / Identification of devices

Désignation du dispositif / Accessoires marqués CE <i>Device designation / CE marked accessories</i>	Réf commerciale du dispositif ou code article <i>Device commercial reference or article code</i>	Classe du DM MD class
Dispositif ou système de diagnostic par ultrasons <i>Ultrasound diagnostic device or system</i>	LOGIQ P7	Ila
Dispositif ou système de diagnostic par ultrasons <i>Ultrasound diagnostic device or system</i>	LOGIQ P8	Ila
Dispositif ou système de diagnostic par ultrasons <i>Ultrasound diagnostic device or system</i>	LOGIQ P9	Ila
Dispositif ou système de diagnostic par ultrasons <i>Ultrasound diagnostic device or system</i>	LOGIQ P10	Ila
Dispositif ou système de diagnostic par ultrasons <i>Ultrasound diagnostic device or system</i>	VOLUSON S6	Ila
Dispositif ou système de diagnostic par ultrasons <i>Ultrasound diagnostic device or system</i>	VOLUSON S8	Ila
Dispositif ou système de diagnostic par ultrasons <i>Ultrasound diagnostic device or system</i>	VOLUSON S8t	Ila
Dispositif ou système de diagnostic par ultrasons <i>Ultrasound diagnostic device or system</i>	VOLUSON S10	Ila



**Lionel DREUX**  
Certification Director



Désignation du dispositif / Accessoires marqués CE <i>Device designation / CE marked accessories</i>	Réf commerciale du dispositif ou code article <i>Device commercial reference or article code</i>	Classe du DM MD class
Dispositif ou système de diagnostic par ultrasons <i>Ultrasound diagnostic device or system</i>	VOLUSON S10 Expert	Ila
Dispositif ou système de diagnostic par ultrasons <i>Ultrasound diagnostic device or system</i>	VOLUSON P6	Ila
Dispositif ou système de diagnostic par ultrasons <i>Ultrasound diagnostic device or system</i>	VOLUSON P8	Ila
Dispositif ou système de diagnostic par ultrasons <i>Ultrasound diagnostic device or system</i>	VOLUSON SWIFT	Ila
Dispositif ou système de diagnostic par ultrasons <i>Ultrasound diagnostic device or system</i>	VOLUSON SWIFT+	Ila
Dispositif ou système de diagnostic par ultrasons <i>Ultrasound diagnostic device or system</i>	LOGIQ S8	Ila
Dispositif ou système de diagnostic par ultrasons <i>Ultrasound diagnostic device or system</i>	LOGIQ S7 Expert	Ila
Dispositif ou système de diagnostic par ultrasons <i>Ultrasound diagnostic device or system</i>	LOGIQ S7 Pro	Ila
Dispositif ou système de diagnostic par ultrasons <i>Ultrasound diagnostic device or system</i>	LOGIQ S7 XDclear2.0	Ila
Dispositif ou système de diagnostic par ultrasons <i>Ultrasound diagnostic device or system</i>	LOGIQ E10s	Ila

### Site couvert et Activités / Locations and Activities

Site / Location	Activités / Activities
GE ULTRASOUND KOREA, Ltd. 9, Sunhwan-ro 214beon-gil, Jungwon-gu, Seongnam-si, Gyeonggi-do, REPUBLIC OF KOREA équivalent à equivalent to GE ULTRASOUND KOREA, Ltd. 65-1, Sangdaewon-dong, Jungwon-gu, Seongnam-si, Gyeonggi-do - 462-120 REPUBLIC OF KOREA	Conception, fabrication et contrôle final Design, manufacture and final control



Lionel DREUX

Certification Director

GMED - 36988 rev. 0

GMED • Société par Actions Simplifiée au capital de 300 000 € • RCS Paris 839 022 522 • Organisme notifié n° 0459  
Siège social : 1, rue Gaston Boissier - 75015 Paris • Tél. : 01 40 43 37 00 • gmed.fr

720 GMED 0901-4 rev 0 du 31/08/2020





# Certificate

No. Q5 075707 0058 Rev. 02

**Holder of Certificate:** **GE Healthcare Austria GmbH & Co OG**  
Tiefenbach 15  
4871 Zipf  
AUSTRIA

**Facility(ies):** GE Healthcare Austria GmbH & Co OG  
Tiefenbach 15, 4871 Zipf, AUSTRIA  
  
Design and Development, Production  
and Distribution of Diagnostic Ultrasound  
Systems, Probes and Standalone Software  
for Ultrasound-Image Processing

**Certification Mark:**



**Scope of Certificate:** **Design and Development, Production  
and Distribution of Diagnostic Ultrasound  
Systems, Probes and Standalone Software  
for Ultrasound-Image Processing**

**Applied Standard(s):** EN ISO 13485:2016  
Medical devices - Quality management systems -  
Requirements for regulatory purposes  
(ISO 13485:2016)  
DIN EN ISO 13485:2016

The Certification Body of TÜV SÜD Product Service GmbH certifies that the company mentioned above has established and is maintaining a quality management system, which meets the requirements of the listed standard(s). All applicable requirements of the testing and certification regulation of TÜV SÜD Group have to be complied with. For details and certificate validity see: [www.tuvsud.com/ps-cert?q=cert:Q5 075707 0058 Rev. 02](http://www.tuvsud.com/ps-cert?q=cert:Q5 075707 0058 Rev. 02)

**Report No.:** 713202497

**Valid from:** 2021-11-20

**Valid until:** 2024-04-23

**Date,** 2021-11-11

Christoph Dicks  
Head of Certification/Notified Body





# LOGIQ Fortis R3.x HDU

## Product Specification Sheet

Last updated on: Thursday, January 13, 2022

1	<b>General Specifications</b>	
2	<b>Dimensions and Weight</b> (Dimensions given with floating keyboard stowed and display tilted for transport)	
3	Depth	885 mm, 34.8"
4	Height	1250 – 1800 mm, 49 – 71"
5	Weight	85 kg (187.4 lb)
6	Width	530 mm, 20.9" (Caster), 565 mm, 22.2" (Monitor)
7	<b>Electrical Power</b>	
8	Voltage: 100 – 240 Vac	
9	Frequency: 50/60 Hz	
10	Power consumption maximum of 0.9 kVA with peripherals	
11	<b>Console Design</b>	
12	4 active probe ports	
13	1 inactive probe storage port	
14	Integrated SSD (1 TB)	
15	Integrated DVD-R Multi Drive	
16	On-board storage of thermal printer	
17	Integrated speaker	
18	Integrated locking mechanism that provides rolling lock and caster swivel lock	
19	Integrated cable management	
20	Front and rear handles	
21	Easily removable air filters	
22	Windows 10 64-bit	
23	<b>User Interface</b>	
24	<b>Operator Keyboard</b>	
25	Operating keyboard adjustable in height and rotation	
26	Ergonomic hard key layout	
27	Interactive back-lighting	
28	Integrated recording keys for remote control of up to 4 peripheral devices or DICOM® devices	
29	Integrated gel warmer	
30	<b>Touch Screen</b>	
31	12.1" High-resolution, color, touch, display screen	
32	Interactive dynamic software menu	
33	Brightness adjustment	
34	User-configurable layout	
35	<b>Monitor</b>	
36	23.8" Wide screen high-resolution HDU display	
37	Display translation (independent of console)	
38	350 mm, (13.7 in) horizontal (both directions)	
39	150 mm, (5.9 in) vertical	
40	90° swivel (both directions)	
41	Fold-down and lock mechanism for transportation	
42	Resolution: 1920 X 1080	
43	Anti-glare	
44	Viewing angle 89/89/89/89°	
45	Contrast Ratio: >20,000:1	
46	<b>System Overview</b>	
47	<b>Applications</b>	
48	Abdominal	
49	Obstetrical	
50	Gynecological	
51	Breast	



52	Small Parts
53	Peripheral Vascular
54	Transcranial (adult and neonatal)
55	Pediatric and neonatal
56	Musculoskeletal (general and superficial)
57	Urological
58	Cardiac (adult and pediatric)
59	Interventional
60	Pleural
61	<b>Operating Modes</b>
62	B-Mode
63	M-Mode
64	Color Flow Mode (CFM)
65	B-Flow (Option)
66	Extended Field of View (LOGIQView)
67	Power Doppler Imaging (PDI)
68	PW Doppler
69	CW Doppler (Option)
70	Volume Modes (3D/4D) (Option)
71	Anatomical M-Mode
72	Coded Contrast Imaging (Option)
73	Strain elastography (Option)
74	B Steer+ (Option)
75	Shear wave elastography (Option)
76	UGAP (Option) - Ultrasound Guided Attenuation Parameter Imaging
77	<b>Scanning Methods</b>
78	Electronic sector
79	Electronic convex
80	Electronic linear
81	Mechanical volume sweep
82	<b>Probe Types</b>
83	Sector phased array
84	Convex array
85	Microconvex array
86	Linear array
87	Matrix array
88	Volume probes (4D)
89	Split crystal
90	<b>System Standard Features</b>
91	Advanced user interface with high-resolution 12.1" display touch panel
92	Automatic optimization
93	CrossXBeam™ compounding
94	Speckle Reduction Imaging (SRI-HD, Advanced SRI Type 1)
95	Fine angle steer
96	Coded harmonic imaging
97	Virtual convex
98	Patient information database
99	Image archive on integrated CD/DVD and hard drive
100	Advanced 3D
101	Raw data analysis
102	Real-time automatic Doppler calculations
103	OB calculations
104	Fetal trending
105	Multi gestational calculations
106	Hip dysplasia calculations
107	Gynecological calculations
108	Vascular calculations
109	Urological calculations
110	Renal calculations
111	Cardiac calculations
112	InSite™ capability
113	On-board electronic documentation
114	Auto Doppler Assist



115	Privacy and security, including user and rights management	
116	LOGIQView	
117	External USB printer connection	
118	Network printer support	
119	HDMI output (available for compatible devices)	
120	<b>System Options</b>	
121	Tricefy®	
122	DICOM	
123	B-Flow	
124	Compare Assistant	
125	Auto IMT	
126	Scan Assistant	
127	Breast productivity package	
128	Thyroid productivity package	
129	OB measure assistant	
130	Quantitative Flow Analysis available with Color Flow/PDI	
131	Breast Measure Assistant	
132	B Steer+	
133	Strain elastography	
134	Elastography Quantification	
135	Advanced privacy and security (vulnerability scan)	
136	Power assistant and scan on battery	
137	Storage bins	
138	Shear wave Elastography	
139	Volume Navigation	
140	UGAP	
141	Hepatic Assistant	
142	Coded Contrast Imaging	
143	Stress echo	
144	Cardiac Strain (Automatic Function Imaging)	
145	On-board reporting	
146	TVI	
147	Wireless LAN	
148	CW	
149	DVR	
150	Table tools	
151	Advanced probes	
152	Breast Assistant, Powered by Koios DS™	
153	SonoNT SonoIT	
154	Advanced SRI Type 2	
155	<b>Peripheral Options</b>	
156	Integrated Option for Digital Color thermal Printer	
157	Digital A6 color thermal printer	
158	Foot switch, with programmable functionality	
159	CRF-200U card reader support (Japan Only)	
160	Console protective cover	
161	LOGIQ smart device apps	<ul style="list-style-type: none"> <li>• Photo Assistant</li> <li>• Remote Control</li> </ul>
162	<b>Display Modes</b>	
163	Live and stored display format	<ul style="list-style-type: none"> <li>• Full size and split screen – both w/ thumbnails. For still and CINE</li> </ul>
164	Review image format	<ul style="list-style-type: none"> <li>• 4x4, and thumbnails. For still and CINE</li> </ul>
165	Time line display	<ul style="list-style-type: none"> <li>• Independent Dual B or CrossXBeam/PW Display</li> <li>• CW</li> <li>• Display formats top/bottom selectable format</li> <li>• Side/side selectable format</li> </ul>
166	Virtual convex	
167	<b>Simultaneous capability</b>	
168	B or CrossXBeam/PW	
169	B or CrossXBeam/CW (Option)	
170	B or CrossXBeam/CFM or PDI	
171	B/M	
172	B/CrossXBeam	
173	B-Flow/PW	



174	Real-time Triplex Mode - B or CrossXBeam + CFM or PDI/PW	
175	<b>Selectable alternating modes</b>	
176	B or CrossXBeam/PW	
177	B or CrossXBeam + CFM (PDI)/PW	
178	B/CW (Option)	
179	<b>Multi-image (split/quad screen)</b>	
180	Live and/or frozen	
181	B or CrossXBeam + B or CrossXBeam/CFM or PDI or B-Flow (Option)	
182	PW/M	
183	Independent Cine playback	
184	<b>Display Annotation</b>	
185	Patient name: first, last and middle	
186	Patient ID	
187	Alternate patient ID	
188	Age, sex and date of birth	
189	Hospital name	
190	Date format: three types selectable	<ul style="list-style-type: none"> <li>• MM/DD/YY</li> <li>• DD/MM/YY</li> <li>• YY/MM/DD</li> </ul>
191	Time format: 2 types selectable	<ul style="list-style-type: none"> <li>• 24 hours</li> <li>• 12 hours</li> </ul>
192	Gestational age from	<ul style="list-style-type: none"> <li>• LMP</li> <li>• GA</li> <li>• EDD</li> <li>• BBT</li> </ul>
193	Probe name	
194	Map names	
195	Probe orientation	
196	Depth scale marker	
197	Lateral scale marker	
198	Focal zone markers	
199	Image depth	
200	Zoom depth	
201	B-Mode	<ul style="list-style-type: none"> <li>• Gain</li> <li>• Dynamic range</li> <li>• Imaging frequency</li> <li>• Frame averaging</li> <li>• Gray map</li> <li>• SRI</li> </ul>
202	M-Mode	<ul style="list-style-type: none"> <li>• Gain</li> <li>• Dynamic range</li> <li>• Time scale</li> </ul>
203	Doppler Mode	<ul style="list-style-type: none"> <li>• Gain</li> <li>• Angle</li> <li>• Sample volume depth and width</li> <li>• Wall filter</li> <li>• Velocity and/or frequency scale</li> <li>• Spectrum inversion</li> <li>• Time scale</li> <li>• PRF</li> <li>• Doppler frequency</li> </ul>
204	Color Flow Doppler Mode	<ul style="list-style-type: none"> <li>• Line density</li> <li>• Frame averaging</li> <li>• Color scale, 3 types: Power, directional PDI and symmetrical velocity imaging</li> <li>• Color velocity range and baseline</li> <li>• Color threshold marker</li> <li>• Color gain</li> <li>• PDI</li> <li>• Spectrum inversion</li> <li>• Doppler frequency</li> </ul>
205	Digital TGC with 8 independent controls	
206	Acoustic frame rate	



207	CINE gage, image number/frame number	
208	Body pattern: multiple human and animal types	
209	Application name	
210	Measurement results	
211	Operator message	
212	Displayed acoustic output	<ul style="list-style-type: none"> <li>• TIS: Thermal Index Soft Tissue</li> <li>• TIC: Thermal Index Cranial (Bone)</li> <li>• TIB: Thermal Index Bone</li> <li>• MI: Mechanical Index</li> </ul>
213	% of maximum power output	
214	Biopsy guide line and zone	
215	Heart rate	



216	<b>General System Parameters</b>	
217	<b>System Setup</b>	
218	Pre-programmable categories	
219	User programmable preset capability	
220	Factory default preset data	
221	Languages: English, French, German, Spanish, Italian, Brazilian, Portuguese, Russian, Greek, Swedish, Danish, Dutch, Finnish, Norwegian	
222	OB Report Formats including Tokyo Univ., Osaka Univ., USA, Europe and ASUM and WHO	
223	User defined annotations	
224	Body patterns	
225	Customized comment home position	
226	EZ Imaging: Simplified user interface for high volume workflow	
227	<b>Complete user manual available on board through Help (F1)</b>	
228	User manual and service manual are included in USB stick with each system. A printed manual is available upon request.	
229	<b>CINE Memory/Image Memory</b>	
230	1 GB of CINE memory	
231	Selectable CINE sequence for CINE review	
232	Prospective CINE mark	
233	Measurements/calculations and annotations on CINE playback	
234	Scrolling timeline memory	
235	Dual Image CINE display	
236	Quad Image CINE display	
237	CINE gauge and CINE image number display	
238	CINE review loop	
239	CINE review speed	
240	<b>Image Storage</b>	
241	On-board database of patient information from past exams	
242	Storage formats: DICOM	<ul style="list-style-type: none"> <li>• Compressed/uncompressed</li> <li>• Single/multi-frame</li> <li>• Enhanced (3D/4D)</li> <li>• With/without raw data</li> </ul>
243	Export JPEG, JPEG 2000, WMV (MPEG 4) formats	
244	Storage devices:	<ul style="list-style-type: none"> <li>• USB memory stick: 64 MB to 64 GB (for exporting individual images/clips)</li> <li>• CD-R storage: 700 MB</li> <li>• DVD storage: -R (4.7 GB)</li> <li>• Hard drive image storage: ~830GB</li> </ul>
245	Compare previous exam images with current exam	
246	Reload of archived date sets	
247	Network storage support for import, export, DICOM read, SaveAs, MPEGVue	
248	<b>Connectivity</b>	
249	Ethernet network connection	
250	Wireless LAN 802.11ac/a/b/g/n (Option)	
251	DICOM 3.0	<ul style="list-style-type: none"> <li>• Verify</li> <li>• Print</li> <li>• Store</li> <li>• Modality worklist</li> <li>• Storage commitment</li> <li>• Modality performed procedure step (MPPS)</li> <li>• Media exchange</li> <li>• Off network/mobile storage queue</li> <li>• Query/retrieve</li> </ul>
252	Public SR template	
253	Structured Reporting – compatible with vascular and OB, cardiac and breast standard	
254	InSite capability	
255	Advanced privacy and security (Option)	



256	<b>Physiological input panel (Option)</b>	
257	Physiological input	<ul style="list-style-type: none"> <li>• ECG, 1 channel</li> <li>• PCG, 1 channel</li> <li>• AUX, 1 channel</li> <li>• Dual R-Trigger</li> <li>• Pre-settable ECG R delay time</li> <li>• Pre-settable ECG position</li> <li>• Adjustable ECG gain control</li> <li>• Pre-settable PCG position</li> <li>• Adjustable PCG gain control</li> <li>• Pre-settable AUX position</li> <li>• Adjustable AUX gain control</li> </ul>
258	Automatic heart rate display	
259	Auto Ejection Fraction	
260	<b>Report writer (Option)</b>	
261	On-board reporting package automates report writing	
262	Formats various exam results into a report suitable for printing or reviewing on a standard PC	
263	Exam results include patient info, exam info, measurements, calculations, images, and comments Standard templates provided	
264	Customizable templates	
265	<b>Scanning Parameters</b>	
266	cSound™ Imageformer: Infinite number of effective channels	
267	Frame rate: 9,675 Hz maximum	
268	Displayed imaging depth: 0 – 100 cm	
269	Minimum depth of field: 0 – 2 cm (zoom) (probe dependent)	
270	Maximum depth of field: 0 – 100 cm (probe dependent)	
271	Continuous dynamic receive focus	
272	Continuous dynamic receive aperture	
273	Adjustable dynamic range, infinite upper level	
274	Adjustable field of view (FOV)	
275	System Frequency Range: 0.7-24 MHz	
276	Image reverse: right/left	
277	Image rotation of 0°, 90°, 180°, 270°	
278	8 bits stored per color	
279	256 shades of gray	
280	256 color tones	
281	<b>Digital B-Mode</b>	
282	Adjustable	<ul style="list-style-type: none"> <li>• Acoustic power</li> <li>• Gain</li> <li>• Dynamic range</li> <li>• Frame averaging</li> <li>• Gray scale map</li> <li>• Frequency</li> <li>• Speed of sound (application dependent)</li> <li>• Framerate</li> <li>• Scanning size (FOV or Angle) <ul style="list-style-type: none"> <li>– Depending on the probe, see probe specifications</li> </ul> </li> <li>• CrossXBeam</li> <li>• B colorization</li> <li>• Reject</li> <li>• Suppression</li> <li>• SRI</li> </ul>
283	<b>Digital M-Mode</b>	
284	Adjustable	<ul style="list-style-type: none"> <li>• Acoustic power</li> <li>• Gain</li> <li>• Dynamic range</li> <li>• Gray scale map</li> <li>• Frequency</li> <li>• Sweep speed</li> <li>• M colorization</li> <li>• M display format</li> <li>• Rejection</li> </ul>
285	<b>Anatomical M-Mode</b>	
286	M-mode cursor adjustable at any plane	



287	Can be activated from a CINE loop from a live or stored image	
288	M & A capability	
289	Available with Color Flow Mode	
290	<b>Digital Spectral Doppler Mode</b>	
291	Adjustable	<ul style="list-style-type: none"> <li>• Acoustic power</li> <li>• Gain</li> <li>• Dynamic range</li> <li>• Gray scale map</li> <li>• Transmit frequency</li> <li>• Wall filter</li> <li>• PW colorization</li> <li>• Velocity scale range</li> <li>• Sweep speed</li> <li>• Sample volume length</li> <li>• Angle correction</li> <li>• Steered linear</li> <li>• Spectrum inversion</li> <li>• Trace method</li> <li>• Baseline shift</li> <li>• Doppler auto trace</li> <li>• Time resolution</li> <li>• Compression</li> <li>• Trace direction</li> <li>• Trace sensitivity</li> </ul>
292	<b>Digital Color Flow Mode</b>	
293	Adjustable	<ul style="list-style-type: none"> <li>• Acoustic power</li> <li>• Color maps, including velocity-variance maps</li> <li>• Gain</li> <li>• Velocity scale range</li> <li>• Wall filter</li> <li>• Packet size</li> <li>• Line density</li> <li>• Spatial filter</li> <li>• Steering angle</li> <li>• Baseline shift</li> <li>• Frame average</li> <li>• Threshold</li> <li>• Auto ROI placement and steering on linear</li> <li>• Accumulation mode</li> <li>• Flash suppression</li> <li>• Shortcuts</li> </ul>
294	<b>Digital Power Doppler Imaging</b>	
295	Adjustable	<ul style="list-style-type: none"> <li>• Acoustic power</li> <li>• Color maps, velocity-variance maps</li> <li>• Gain including</li> <li>• Velocity scale range</li> <li>• Wall filter</li> <li>• Packet size</li> <li>• Line density</li> <li>• Spatial filter</li> <li>• Steering angle</li> <li>• Frame average</li> <li>• Threshold</li> <li>• Accumulation mode</li> <li>• Flash suppression</li> <li>• Shortcuts</li> </ul>
296	<b>Continuous Wave Doppler (Option)</b>	
297	Available on M5Sc-D, 6S-D, 6Tc-RS, P2D and P6D probes	
298	Steerable CW mode included	



299	Adjustable	<ul style="list-style-type: none"> <li>• Acoustic power</li> <li>• Gain</li> <li>• Dynamic range</li> <li>• Gray scale map</li> <li>• Transmit frequency</li> <li>• Wall filter</li> <li>• CW colorization</li> <li>• Velocity scale range</li> <li>• Sweep speed</li> <li>• Angle correction</li> <li>• Spectrum inversion</li> <li>• Trace method</li> <li>• Baseline shift</li> <li>• Doppler auto trace</li> <li>• Compression</li> <li>• Trace direction</li> <li>• Trace sensitivity</li> </ul>
300	<b>Automatic Optimization</b>	
301	Optimize B-Mode image to help improve contrast resolution with one button press	
302	Selectable amount of contrast resolution improvement (low, medium, high)	
303	CTO (Continuous Tissue Optimization) – continuously adjusts B-Mode axial and lateral gain uniformity and overall gain level suppressing the noise	
304	Auto-spectral optimize – adjusts baseline, invert, PRF (on live image), and angle correction with one button press	
305	Auto CF and PW positioning – adjusts ROI position, sample volume position and steering with one button press	
306	<b>Coded Harmonic Imaging</b>	
307	Available on all 2D and 4D probes	
308	<b>B-Flow (Option)</b>	
309	Available on the following probes: C1-6-D, C1-6VN-D, C2-7-D, C2-7VN-D, C2-9-D, C2-9VN-D, C3-10-D, L2-9-D, L2-9VN-D, L3-12-D, L6-24-D, ML6-15-D, M5Sc-D, L8-18i-D	
310	Background	
311	Sensitivity/PRf	
312	Acoustic power	
313	Frequency	
314	Line density	
315	Frame average	
316	Gray scale map	
317	Tint map	
318	Dynamic range	
319	Rejection	
320	Gain	
321	Suppression	
322	SRI	
323	Accumulation	
324	Visualization	
325	<b>Radiantflow™</b>	
326	Easy, fast visualization of tiny vessels, displaying as a 3D effect	
327	Available in Color Doppler, Power Doppler and MVI	
328	<b>B Steer+ (Option)</b>	
329	Available on the following probes: L2-9-D, ML6-15-D, L8-18i-D, L3-12-D, L2-9VN-D	
330	<b>Coded contrast imaging (Option)</b>	
331	Available on the following probes: C1-6-D, C1-6VN-D, C2-9-D, C2-9VN-D, C2-7-D, C2-7VN-D, C3-10-D, IC5-9-D, L2-9-D, L2-9VN-D, L3-12-D, M5Sc-D, ML6-15-D, RAB6-D, RIC5-9-D, L6-24-D	
332	2 contrast timers	
333	Timed updates: 0.05 – 10 seconds	
334	Accumulation mode, seven levels	
335	Maximum enhance mode	
336	Flash	
337	Time intensity curve (TIC) analysis	
338	Parametric imaging	
339	Ability to save still image during clip acquisition	



340	<p>The LOGIQ Fortis is designed for compatibility with most commercially available ultrasound contrast agents. Because the availability of these agents is subject to government regulation and approval, product features intended for use with these agents may not be commercially marketed nor made available before the contrast agent is cleared for use.</p> <p>Contrast related product features are enabled only on systems for delivery to an authorized country or region of use.</p>	
341	<b>LOGIQView</b>	
342	Extended field of view Imaging	
343	Up to 160 cm (63") scan length	
344	Available on all 2D imaging probes	
345	For use in B-Mode	
346	CrossXBeam is available on linear probes	
347	Auto detection of scan direction	
348	Pre-or post-process zoom	
349	Rotation	
350	Auto best fit on monitor	
351	Measurements in B-Mode	
352	<b>3D</b>	
353	Allows unlimited rotation and planar translation	
354	3D reconstruction from CINE sweep	
355	Easy 3D available on all probes	
356	<b>Advanced 3D</b>	
357	Acquisition of color data	
358	Automatic rendering	
359	3D landscape technology	
360	3D movie	
361	<b>Real-time 4D (Option)</b>	
362	Acquisition modes	<ul style="list-style-type: none"> <li>• Real Time 4D</li> <li>• Spatio-Temporal Image Correlation (Option)</li> <li>• Static 3D</li> </ul>
363	Visualization modes	<ul style="list-style-type: none"> <li>• 3D rendering (diverse surface and intensity projection modes)</li> <li>• Sectional planes (3 section planes perpendicular to each other)</li> <li>• Omniview (Option)</li> <li>• Volume contrast imaging – Static (Option)</li> <li>• Volume contrast imaging – Omniview (Option)</li> <li>• Tomographic ultrasound imaging (Option)</li> <li>• Volume Analyses <ul style="list-style-type: none"> <li>– VOCAL: semi-auto/manual segmentation tool (segmentation using touch screen) (Option)</li> <li>– 3D Static only</li> <li>– Threshold Volume: measure volume below and above a threshold</li> </ul> </li> </ul>
364	Render mode	<ul style="list-style-type: none"> <li>• Surface texture, surface smooth, max-, min- and X-ray (average intensity projection), mix mode of two render modes</li> <li>• HD<i>live</i>™</li> </ul>
365	SonoRender <i>live</i>	
366	Curved 3 point Render start	
367	3D Movie	
368	Scalpel: 3D cut tool	
369	Display format:	<ul style="list-style-type: none"> <li>• Quad: A-/B-/C-Plane/3D</li> <li>• Dual: A-Plane/3D</li> <li>• Single: 3D or A- or B- or C-Plane</li> </ul>
370	Automated Volume Calculation – VOCAL II	
371	Betaview	
372	<b>Volume navigation (Option)</b>	
373	Available on the following probes: C1-6VN-D, C2-9VN-D, C2-7VN-D, C3-10-D, L2-9VN-D, ML6-15-D, IC5-9-D, L8-18i-D, M5Sc-D	
374	Sensor-based acquisition	
375	Position markers	
376	Needle tip tracking	
377	Virtual tracking	
378	Auto image registration	
379	Tru3D feature includes	
380	Render modes: gray surface, texture, min-, max-, average-intensity	



381	Measurements: distance, angle, area, volume
382	3D Movie
383	<b>Scan assistant (Option)</b>
384	Factory programs
385	User-defined programs
386	Steps include image annotations, mode transitions, basic imaging controls and measurement initiation
387	<b>Compare Assistant (Option)</b>
388	Allows side-by-side comparison of previous ultrasound and other modality exams during live scanning
389	<b>Breast productivity package</b>
390	Auto measurement
391	Worksheet summary includes measurements and locations for lesions and lymph nodes
392	Feature assessment
393	BI-RADS™ assessment
394	User editable
395	<b>Thyroid productivity package (Option)</b>
396	Auto measurement
397	Worksheet summary includes measurements and locations for nodule, parathyroid and lymph nodes
398	Feature assessment
399	BI-RADS™ assessment
400	User editable
401	<b>Start Assistant</b>
402	Automatically select category, probe, preset, or scan assistant from worklist exam description
403	Learn the category, probe, preset, and scan assistant based on exam description
404	<b>Shear Wave Elastography (Option)</b>
405	Available on the following probes: C1-6-D, C1-6VN-D, L2-9-D, L2-9VN-D, IC5-9-D, L8-18i-D, ML6-15-D, L3-12-D
406	User programmable measurement display in kPa and meters per second
407	Single and dual view display
408	Applications: Abdominal, Breast, Musculoskeletal, Small Parts, Prostate
409	<b>Strain elastography (Option)</b>
410	Available on the following probes: ML6-15-D, L2-9-D, L2-9VN-D, L3-12-D, IC5-9-D, C2-9-D, C2-9VN-D, C1-6-D, C1-6VN-D, L8-18i-D, BE9CS-D
411	Relative analysis tool
412	Applications: Abdominal, Breast, Musculoskeletal, Small Parts, Prostate, Thyroid
413	<b>UGAP (Option)</b>
414	Available on the following probes: C1-6-D, C1-6VN-D, C2-9-D, C2-9VN-D
415	Measures liver attenuation* (attenuation coefficient [dB/cm/MHz]) by auto measure algorithm with reference B-mode
416	Simple and 2D color map (attenuation color map and Measurement Position Indicator Map)
417	<b>Quantitative flow analysis (Option)</b>
418	Available in color and power Doppler
419	<b>TVI (Option)</b>
420	Available on the following probes: M5Sc-D, 6Tc-RS, 6S-D probes
421	Myocardial Doppler imaging with color overlay on tissue image
422	Tissue color overlay can be removed to show just the 2D image, still retaining the tissue velocity information
423	Curved anatomical M-Mode: free (curved) drawing of M-Mode generated from the cursor independent from the axial plane
424	Q-Analysis: multiple time-motion trace display from selected points in the myocardium
425	<b>Stress echo (Option)</b>
426	Advanced and flexible stress echo examination capabilities
427	Provides exercise and pharmacological protocol templates
428	6 default templates
429	Template editor for user configuration of existing templates or creation of new templates
430	Reference scan display during acquisition for stress level comparison (dual screen)
431	Baseline level/previous level selectable
432	Raw data continuous capture
433	Over 100 sec. available
434	Wall motion scoring (bull's-eye and segmental)
435	Smart stress: Automatically set up various scanning parameters (e.g. geometry, frequency, gain) according to same projection on previous level
436	<b>Auto EF (Option)</b>
437	Allows semi-automatic measurement of the global EF (Ejection Fraction)
438	User editable
439	<b>Cardiac AFI (Option)</b>
440	Allows assessment of the complete left ventricle with all segments at a glance by combining three longitudinal views into one comprehensive bulls-eye view
441	2D strain based data moves into clinical practice



442	<b>Virtual Convex</b>	
443	Provides a convex field of view	
444	Compatible with CrossXBeam	
445	Available on all linear and sector probes	
446	<b>SRI-HD and Advanced SRI</b>	
447	Speckle reduction imaging	
448	Provides multiple levels of speckle reduction	
449	Compatible with side-by-side DualView display	
450	Advanced SRI: two types selectable	<ul style="list-style-type: none"> <li>• Type 1 <ul style="list-style-type: none"> <li>– Compatible with all linear, convex and sector probes</li> </ul> </li> <li>• Type 2 (Option) <ul style="list-style-type: none"> <li>– Compatible with OB/GYN application</li> </ul> </li> </ul>
451	<b>CrossXBeam</b>	
452	Provides variable angle spatial compounding	
453	Live side-by-side DualView display	
454	Compatible with	<ul style="list-style-type: none"> <li>• Color mode</li> <li>• PW</li> <li>• SRI</li> <li>• Coded harmonic imaging</li> <li>• Virtual convex</li> </ul>
455	Available on all curved and linear probes	
456	<b>Controls available while “live”</b>	
457	Magnification Zoom: Magnifies the entire image on the screen without zoom ROI, 20x maximum zoom factor	
458	Pan Zoom: Magnifies the display of the data within the ROI	
459	HD Zoom: Magnifies the image within the zoom ROI, with higher spatial resolution than original images	
460	B/M/CrossXBeam-Mode	<ul style="list-style-type: none"> <li>• Gain</li> <li>• TGC</li> <li>• Dynamic range</li> <li>• Acoustic output</li> <li>• Framerate control</li> <li>• Sweep speed for M-Mode</li> <li>• CrossXBeam angle</li> </ul>
461	PW-Mode	<ul style="list-style-type: none"> <li>• Gain</li> <li>• Dynamic range</li> <li>• Acoustic output</li> <li>• Transmission frequency</li> <li>• PRF</li> <li>• Wall filter</li> <li>• Spectral averaging</li> <li>• Sample volume gate: length, depth</li> <li>• Velocity scale</li> </ul>
462	Color Flow-Mode	<ul style="list-style-type: none"> <li>• CFM gain</li> <li>• CFM velocity range</li> <li>• Acoustic output</li> <li>• Wall echo filter</li> <li>• Packet size</li> <li>• Frame rate control</li> <li>• CFM spatial filter</li> <li>• CFM frame averaging</li> <li>• CFM line resolution</li> <li>• Frequency/velocity baseline shift</li> </ul>
463	<b>Controls available on “freeze” or recall</b>	
464	Automatic optimization	
465	SRI	
466	CrossXBeam – display non-compounded and compounded image simultaneously in split screen	
467	3D reconstruction from a stored CINE loop	
468	B/M/CrossXBeam-Mode	<ul style="list-style-type: none"> <li>• Gray map optimization</li> <li>• TGC</li> <li>• Colorized B and M</li> <li>• Frame average (loops only)</li> <li>• Dynamic range</li> </ul>
469	Anatomical M-Mode	
470	Magnification zoom	
471	Pan zoom	
472	Maximum read zoom to 8x	



473	Baseline shift	
474	Sweep speed	
475	PW mode	<ul style="list-style-type: none"> <li>• Gray map</li> <li>• Post gain</li> <li>• Baseline shift</li> <li>• Sweep speed</li> <li>• Invert spectral wave form</li> <li>• Compression</li> <li>• Rejection</li> <li>• Colorized spectrum</li> <li>• Display format</li> <li>• Doppler audio</li> <li>• Angle correct</li> <li>• Quick angle correct</li> <li>• Auto angle correct</li> </ul>
476	Color flow	<ul style="list-style-type: none"> <li>• Overall gain (loops and stills)</li> <li>• Color map</li> <li>• Transparency map</li> <li>• Frame averaging (loops only)</li> <li>• Flash suppression</li> <li>• CFM display threshold</li> <li>• Spectral invert for color/Doppler</li> </ul>
477	Anatomical M-Mode on cine loop	
478	4D	<ul style="list-style-type: none"> <li>• Gray map, colorize</li> <li>• Post gain</li> <li>• Change display – single, dual, quad sectional or rendered</li> </ul>
479	<b>Measurements/Calculations</b>	
480	<b>General B-Mode</b>	
481	Depth and distance	
482	Circumference (ellipse/trace)	
483	Area (ellipse/trace)	
484	Volume (ellipsoid)	
485	% Stenosis (area or diameter)	
486	Angle between two lines	
487	Dual B-mode capability	
488	<b>General M-Mode</b>	
489	M-Depth	
490	Distance	
491	Time	
492	Slope	
493	Heart rate	
494	<b>General Doppler measurements/calculations</b>	
495	Velocity	
496	Time	
497	A/B ratio (velocities/frequency ratio)	
498	PS (Peak Systole)	
499	ED (End Diastole)	
500	PS/ED (PS/ED Ratio)	
501	ED/PS (ED/PS Ratio)	
502	AT (Acceleration Time)	
503	ACCEL (Acceleration)	
504	TAMAX (Time Averaged Maximum Velocity)	
505	Volume flow (TAMEAN and vessel area)	
506	Heart rate	
507	PI (Pulsatility Index)	
508	RI (Resistivity Index)	
509	<b>Real-time Doppler Auto Measurements/Calculations</b>	
510	PS (Peak Systole)	
511	ED (End Diastole)	
512	MD (Minimum Diastole)	
513	PI (Pulsatility Index)	
514	RI (Resistivity Index)	
515	AT (Acceleration Time)	



516	ACC (Acceleration)	
517	PS/ED (PS/ED Ratio)	
518	ED/PS (ED/PS Ratio)	
519	HR (Heart Rate)	
520	TAMAX (Time Averaged Maximum velocity)	
521	PVAL (Peak Velocity value)	
522	Volume flow (TAMEAN and vessel area)	
523	<b>Abdominal measurements/calculations</b>	
524	Shear Elasto velocity	
525	Shear Elasto stiffness	
526	Attenuation rate	
527	Attenuation coefficient	
528	Summary reports	
529	<b>Small Parts measurements/calculations</b>	
530	Breast Lesion	
531	Thyroid	
532	Parathyroid	
533	Lymph Node	
534	Nodule	
535	Isthmus AP	
536	Shear Elasto velocity	
537	Shear Elasto stiffness	
538	Summary reports	
539	<b>OB measurements/calculations</b>	
540	Gestational age by	<ul style="list-style-type: none"> <li>• GS (Gestational Sac)</li> <li>• CRL (Crown Rump Length)</li> <li>• FL (Femur Length)</li> <li>• BPD (Biparietal Diameter)</li> <li>• AC (Abdominal Circumference)</li> <li>• HC (Head Circumference)</li> <li>• APTD x TTD (Anterior/Posterior Trunk Diameter by Transverse Trunk Diameter)</li> <li>• FTA (Fetal Trunk Cross-sectional Area)</li> <li>• HL (Humerus Length)</li> <li>• BD (Binocular Distance)</li> <li>• FT (Foot Length)</li> <li>• OFD (Occipital Frontal Diameter)</li> <li>• TAD (Transverse Abdominal Diameter)</li> <li>• TCD (Transverse Cerebellum Diameter)</li> <li>• THD (Thorax Transverse Diameter)</li> <li>• TIB (Tibia Length)</li> <li>• ULNA (Ulna Length)</li> <li>• OOD (Outer Orbital Diameter)</li> <li>• IOD (Inner Orbital Diameter)</li> <li>• FIB (Fibula length)</li> <li>• Radius (Radius length)</li> <li>• LV (Lateral Ventricle width) (= SL)</li> </ul>
541	Estimated Fetal Weight (EFW) by:	<ul style="list-style-type: none"> <li>• AC, BPD</li> <li>• AC, BPD, FL</li> <li>• AC, BPD, FL, HC</li> <li>• AC, FL</li> <li>• AC, FL, HC</li> <li>• AC, HC</li> <li>• BPD, APTD, TTD, FL</li> <li>• BPD, APTD, TTD, SL</li> </ul>
542	Fetal graphical trending	
543	Growth percentiles	
544	Multi-gestational calculations (4)	
545	Fetal qualitative description (anatomical survey)	
546	Fetal environmental description (biophysical profile)	
547	Programmable OB tables	
548	Over 20 selectable OB calculations	
549	Expanded worksheets	
550	Summary Reports	



551	<b>OB Calculations and ratios</b>
552	FL/BPD
553	FL/AC
554	FL/HC
555	HC/AC
556	CI (Cephalic Index)
557	AFI (Amniotic Fluid Index)
558	CTAR (Cardio-Thoracic Area Ratio)
559	Measurements/calculations by: Alexander, ASUM, ASUM 2001, Bahlmann, Baschat, Berkowitz, Bertagnoli, Brenner, Campbell, CFEF, Chervenak, Chitty, Doubilet, Ebinger, Eik-Nes Goldstein, Hadlock, Hansmann, Hellman, Hill, Hohler, Jeanty, JSUM, Kramer, Kurmanavicius, Kurtz, Mari, Mayden, Mercer, Merz, Moore, Nelson, Osaka University, Paris, Pexsters, Rempen, Robinson, Shepard, Shepard/Warsoff, Sonek, Tokyo University, Tokyo/Shinozuka, WHO, Williams, Yarkoni
560	<b>OB measure assistant</b>
561	Allows automatic measurement of BPD, HC, FL and AC
562	User editable
563	<b>SonoNT and SonoIT</b>
564	SonoNT measures the contour detection of the NT border
565	SonoIT is a system supported measurement for Intracranial Translucency
566	<b>GYN measurements/calculations</b>
567	Right ovary length, width, height
568	Left ovary length, width, height
569	Uterus length, width, height
570	Cervix length, trace
571	Ovarian volume
572	ENDO (Endometrial thickness)
573	Ovarian RI
574	Uterine RI
575	Follicular measurements
576	Fibroid measurements
577	Qualitative description (anatomical survey)
578	Mean Uterine Artery (Gomez) Doppler Measurement
579	Summary reports
580	<b>Vascular measurements/calculations</b>
581	SYS DCCA (Systolic Distal Common Carotid Artery)
582	DIAS DCCA (Diastolic Distal Common Carotid Artery)
583	SYS MCCA (Systolic Mid Common Carotid Artery)
584	DIAS MCCA (Diastolic Mid Common Carotid Artery)
585	SYS PCCA (Systolic Proximal Common Carotid Artery)
586	DIAS PCCA (Diastolic Proximal Common Carotid Artery)
587	SYS DICA (Systolic Distal Internal Carotid Artery)
588	DIAS DICA (Diastolic Distal Internal Carotid Artery)
589	SYS MICA (Systolic Mid Internal Carotid Artery)
590	DIAS MICA (Diastolic Mid Internal Carotid Artery)
591	SYS PICA (Systolic Proximal Internal Carotid Artery)
592	DIAS PICA (Diastolic Proximal Internal Carotid Artery)
593	SYS DECA (Systolic Distal External Carotid Artery)
594	DIAS DECA (Diastolic Distal External Carotid Artery)
595	SYS PECA (Systolic Proximal External Carotid Artery)
596	DIAS PECA (Diastolic Proximal External Carotid Artery)
597	VERT (Systolic Vertebral Velocity)
598	SUBCLAV (Systolic Subclavian Velocity)
599	Auto IMT (Option)
600	Summary reports
601	<b>Urological measurements/calculations</b>
602	Bladder volume
603	Prostate volume
604	Left/right renal volume
605	Generic volume
606	Post-void bladder volume
607	Pelvic floor measurements
608	Summary reports
609	<b>TCD measurements/calculations</b>
610	MCA, ACA, PCA, ICA
611	AComA, PComA
612	Vert



613	Basilar	
614	MCA/ICA Ratio	
615	Summary reports	
616	<b>Pediatric and Neonatal measurements/calculations</b>	
617	Hip angle	
618	Hip orientation	
619	Summary reports	
620	<b>Probes (All Optional)</b>	
621	<b>6S-D, sector probe</b>	
622	Applications	Pediatric cardiac, pediatric abdomen
623	Bandwidth	2.0 – 8.0 MHz
624	Number of elements	96
625	Field of view (max.)	115°
626	Physical foot print	15 x 9 mm
627	B-Mode frequency	4.0, 4.2, 5.0, 5.5, 6.5 MHz
628	Harmonic frequency	4.7, 4.9, 5.3, 5.7, 6.1, 6.3 MHz
629	PW Doppler frequency	2.8, 3.1, 3.6, 4.2 MHz
630	Color Doppler frequency	2.7, 3.1, 4.2, 5.0 MHz
631	<b>6Tc-RS, trans-esophageal probe</b>	
632	Applications	Adult cardiac
633	Bandwidth	2.0 – 8.0 MHz
634	Number of elements	64
635	Field of view (max.)	90°
636	Physical foot print	37 x 13 x 10 mm
637	B-Mode frequency	5.0, 6.0, 6.5 MHz
638	Harmonic frequency	6.0 MHz
639	PW Doppler frequency	3.1, 3.6, 4.2, 5.0, 6.3 MHz
640	Color Doppler frequency	3.3, 4.1, 4.7, 5.5 MHz
641	<b>BE9CS-D</b>	
642	Applications	Urology
643	Biopsy guide	Single angle, disposable (E8387M); Single angle, reusable (E8387MA)
644	Bandwidth	3.0 - 12.0 MHz
645	Number of elements	64
646	Field of view (max.)	133°
647	Physical foot print	19 x 19 mm
648	B-Mode frequency	6.0, 7.0, 8.0, 9.0 MHz
649	Harmonic frequency	7.0, 8.0, 9.0, 10.0 MHz
650	PW Doppler frequency	4.2, 5.0, 6.3 MHz
651	Color Doppler frequency	4.3, 6.3, 8.2 MHz
652	<b>C1-6-D, XDclear™ convex probe</b>	
653	Applications	Abdomen, OB/GYN, pediatric, peripheral vascular, general musculoskeletal
654	Biopsy guide	Multi-angle, disposable with a reusable bracket (H4917VB)
655	Bandwidth	1.0 – 6.0 MHz
656	Number of elements	192
657	Field of view (max.)	80°
658	Physical foot print	67 x 11 mm
659	B-Mode frequency	2.0, 2.5, 3.0, 4.0 MHz
660	Harmonic frequency	1.5, 2.5, 3.0, 4.5, 6.0, 6.5 MHz
661	PW Doppler frequency	1.7, 2.1, 2.5, 3.6 MHz
662	Color Doppler frequency	1.8, 2.1, 2.5, 2.8, 3.0 MHz
663	<b>C1-6VN-D, VNav inside XDclear convex probe</b>	
664	VNav sensor inside probe for Volume Navigation tracking without sensor cables	
665	Applications	Abdomen, OB/GYN, pediatric, peripheral vascular, general musculoskeletal
666	Biopsy guide	Multi-angle, disposable with a reusable bracket (H4917VB)
667	Bandwidth	1.0 – 6.0 MHz
668	Number of elements	192
669	Field of view (max.)	80°
670	Physical foot print	67 x 11 mm
671	B-Mode frequency	2.0, 2.5, 3.0, 4.0 MHz
672	Harmonic frequency	1.5, 2.5, 3.0, 4.5, 6.0, 6.5 MHz
673	PW Doppler frequency	1.7, 2.1, 2.5, 3.6 MHz
674	Color Doppler frequency	1.8, 2.1, 2.5, 2.8, 3.0 MHz



675	<b>C2-7-D, micro convex biopsy probe</b>	
676	Applications	Abdomen, pediatric
677	Biopsy guide	Multi-angle, disposable with a reusable bracket (H40482LK), Multi-Angle, reusable stainless bracket (H40482LL)
678	Bandwidth	1.0 – 6.0 MHz
679	Number of elements	144
680	Field of view (max.)	110°
681	Physical foot print	31 x 10 mm
682	B-Mode frequency	2.5, 4.0, 6.0 MHz
683	Harmonic frequency	3.0, 4.0, 5.0, 6.0 MHz
684	PW Doppler frequency	1.8, 2.1, 2.5, 3.1 MHz
685	Color Doppler frequency	2.1, 2.4, 3.1, 3.7 MHz
686	<b>C2-7-VN-D, VNav inside XDclear convex probe</b>	
687	VNav sensor inside probe for Volume Navigation tracking without sensor cables	
688	Applications	Abdomen, pediatric
689	Biopsy guide	Multi-angle, disposable with a reusable bracket (H40482LK), Multi-Angle, reusable stainless bracket (H40482LL)
690	Bandwidth	1.0 – 6.0 MHz
691	Number of elements	144
692	Field of view (max.)	110°
693	Physical foot print	31 x 10 mm
694	B-Mode frequency	2.5, 4.0, 6.0 MHz
695	Harmonic frequency	3.0, 4.0, 5.0, 6.0 MHz
696	PW Doppler frequency	1.8, 2.1, 2.5, 3.1 MHz
697	Color Doppler frequency	2.1, 2.4, 3.1, 3.7 MHz
698	<b>C2-9-D, XDclear convex probe</b>	
699	Applications	Abdomen, OB/GYN, pediatric, peripheral vascular, neonatal, neonatal transcranial, general musculoskeletal
700	Biopsy guide	Multi-angle, disposable with a reusable bracket (H4913BA)
701	Bandwidth	2.0 – 9.0 MHz
702	Number of elements	192
703	Field of view (max.)	80°
704	Physical foot print	52 x 9 mm
705	B-Mode frequency	3.0, 4.5, 6.0, 7.0 MHz
706	Harmonic frequency	2.5, 3.5, 5.0, 7.0, 9.0 MHz
707	PW Doppler frequency	2.5, 3.1, 3.6, 4.2, 5.0, 6.3 MHz
708	Color Doppler frequency	3.1, 4.2, 4.6, 5.4 MHz
709	<b>C2-9-VN-D, VNav inside XDclear convex probe</b>	
710	VNav sensor inside probe for Volume Navigation tracking without sensor cables	
711	Applications	Abdomen, OB/GYN, pediatric, peripheral vascular, neonatal, neonatal transcranial, general musculoskeletal
712	Biopsy guide	Multi-angle, disposable with a reusable bracket (H4913BA)
713	Bandwidth	2.0 – 9.0 MHz
714	Number of elements	192
715	Field of view (max.)	80°
716	Physical foot print	52 x 9 mm
717	B-Mode frequency	3.0, 4.5, 6.0, 7.0 MHz
718	Harmonic frequency	2.5, 3.5, 5.0, 7.0, 9.0 MHz
719	PW Doppler frequency	2.5, 3.1, 3.6, 4.2, 5.0, 6.3 MHz
720	Color Doppler frequency	3.1, 4.2, 4.6, 5.4 MHz
721	<b>C3-10-D, XDclear micro convex probe</b>	
722	Applications	Abdomen, neonatal, pediatric, peripheral vascular, neonatal transcranial, small part
723	Bandwidth	2.0 – 11.0 MHz
724	Number of elements	192
725	Field of view (max.)	95°
726	Physical foot print	26 x 5 mm
727	B-Mode frequency	4.0, 6.0, 8.0 MHz
728	Harmonic frequency	6.0, 8.0, 10.0 MHz
729	PW Doppler frequency	3.1, 4.2, 6.3, 7.1 MHz
730	Color Doppler frequency	3.9, 5.3, 6.6 MHz
731	<b>IC5-9-D, micro convex probe</b>	
732	Applications	OB/GYN, urology
733	Biopsy guide	Single angle, disposable with a disposable bracket (E8385MJ) or reusable bracket (H40412LN)



734	Bandwidth	3.0 – 10.0 MHz
735	Number of elements	192
736	Field of view (max.)	180°
737	Physical foot print	26 x 6 mm
738	B-Mode frequency	4.5, 5.0, 5.5, 6.0, 7.0, 8.0 MHz
739	Harmonic frequency	6.0, 6.5, 7.0, 9.0 MHz
740	PW Doppler frequency	3.6, 4.2, 5.0 MHz
741	Color Doppler frequency	4.6, 5.9, 6.7 MHz
742	<b>L2-9-D, XDclear linear probe</b>	
743	Applications	Peripheral vascular, pediatric, abdomen, OB/GYN, general musculoskeletal, superficial musculoskeletal, neonatal, neonatal transcranial and small parts including breast, thyroid and scrotal
744	Biopsy guide	Multi-angle, disposable with a reusable bracket (H44901AM)
745	Bandwidth	2.0 – 10.0 MHz
746	Number of elements	192
747	Field of view (max.)	44 mm
748	Physical foot print	53 x 14 mm
749	B-Mode frequency	4.0, 4.5, 5.0, 6.0, 7.0 MHz
750	Harmonic frequency	5.0, 6.0, 7.0, 8.0, 9.0, 9.4 MHz
751	PW Doppler frequency	2.5, 2.8, 3.1, 3.6, 4.2, 5.0 MHz
752	Color Doppler frequency	3.1, 4.0, 4.6, 5.3 MHz
753	<b>L2-9VN-D, VNav inside XDclear linear probe</b>	
754	VNav sensor inside probe for Volume Navigation tracking without sensor cables	
755	Applications	Peripheral vascular, pediatric, abdomen, OB/GYN, general musculoskeletal, superficial musculoskeletal, neonatal, neonatal transcranial and small parts including breast, thyroid and scrotal
756	Biopsy guide	Multi-angle, disposable with a reusable bracket (H44901AM)
757	Bandwidth	2.0 – 10.0 MHz
758	Number of elements	192
759	Field of view (max.)	44 mm
760	Physical foot print	53 x 14 mm
761	B-Mode frequency	4.0, 4.5, 5.0, 6.0, 7.0 MHz
762	Harmonic frequency	5.0, 6.0, 7.0, 8.0, 9.0, 9.4 MHz
763	PW Doppler frequency	2.5, 2.8, 3.1, 3.6, 4.2, 5.0 MHz
764	Color Doppler frequency	3.1, 4.0, 4.6, 5.3 MHz
765	<b>L3-12-D, linear probe</b>	
766	Applications	Abdomen, OB, general musculoskeletal, superficial musculoskeletal, neonatal, neonatal transcranial, small parts, vascular
767	Biopsy guide	Multi-angle, disposable with a reusable bracket (H78652PA)
768	Bandwidth	3.0 – 11.0 MHz
769	Number of elements	256
770	Field of view (max.)	51 mm
771	Physical foot print	51 x 4 mm
772	B-Mode frequency	6.0, 8.0, 10.0, 12.0 MHz
773	Harmonic frequency	4.0, 6.0, 8.0, 10.0, 12.0 MHz
774	PW Doppler frequency	4.2, 5.0, 6.3, 8.3 MHz
775	Color Doppler frequency	4.3, 4.9, 5.4, 6.1, 7.2, 8.0 MHz
776	<b>L6-24-D, linear probe</b>	
777	Applications	General musculoskeletal, superficial musculoskeletal, pediatrics, thyroid
778	Bandwidth	6.0 – 20.0 MHz
779	Number of elements	192
780	Field of view (max.)	26 mm
781	Physical foot print	26 x 2 mm
782	B-Mode frequency	12.0, 16.0, 21.0 MHz
783	Harmonic frequency	12.0, 18.0, 24.0 MHz
784	PW Doppler frequency	8.3, 10.0, 12.5 MHz
785	Color Doppler frequency	9.2, 11.2, 12.2 MHz
786	<b>L8-18i-D, linear probe</b>	
787	Applications	Small parts, peripheral vascular, neonatal, neonatal transcranial, general musculoskeletal, superficial musculoskeletal, intraoperative
788	Bandwidth	4.0 – 15.0 MHz
789	Number of elements	168



790	Field of view (max.)	25 mm
791	Physical foot print	35 x 10 mm
792	B-Mode frequency	7.0, 9.0, 13.0, 16.0 MHz
793	Harmonic frequency	14.0, 16.0, 18.0 MHz
794	PW Doppler frequency	5.0, 6.3, 7.1, 8.3 MHz
795	Color Doppler frequency	6.3, 6.7, 9.6, 10.5 MHz
796	<b>M5Sc-D, XDclear sector probe</b>	
797	Applications	Adult cardiac, pediatric cardiac, adult cephalic, abdominal
798	Biopsy guide	Multi-angle, disposable with a reusable bracket (H45561FC)
799	Bandwidth	1.0 – 5.0 MHz
800	Number of elements	288
801	Field of view (max.)	120°
802	Physical foot print	28 x 17 mm
803	B-Mode frequency	2.0, 2.5, 3.5, 4.5 MHz
804	Harmonic frequency	2.4, 3.0, 3.2, 3.3, 3.7, 4.0, 4.5 MHz
805	PW Doppler frequency	1.6, 1.7, 1.8, 1.9, 2.1, 2.5, 3.1, 3.6 MHz
806	Color Doppler frequency	1.7, 1.8, 1.9, 2.2, 2.4, 2.5, 3.0, 3.1, 3.7, 3.8 MHz
807	<b>ML6-15-D, matrix array linear probe</b>	
808	Applications	Abdomen, peripheral vascular, neonatal, pediatric, neonatal transcranial, general musculoskeletal, superficial musculoskeletal and small parts including breast, thyroid and scrotal
809	Biopsy guide	Multi-angle, disposable with a reusable bracket (H40432LJ)
810	Bandwidth	4.0 – 16.0 MHz
811	Number of elements	1008
812	Field of view (max.)	50 mm
813	Physical foot print	50 x 10 mm
814	B-Mode frequency	7.0, 9.0, 10.0, 11.0, 12.0, 15.0 MHz
815	Harmonic frequency	10.0, 12.0, 14.0, 15.0 MHz
816	PW Doppler frequency	5.0, 6.3, 8.3 MHz
817	Color Doppler frequency	5.1, 6.1, 7.3, 8.2, 9.2, 10.3, 11.4, 12.4 MHz
818	<b>P2D, CW split crystal probe</b>	
819	Applications	Adult cardiac, pediatric cardiac, peripheral vascular, adult cephalic
820	Frequency	2.1 MHz
821	<b>P6D, CW split crystal probe</b>	
822	Applications	Adult cardiac, pediatric cardiac, peripheral vascular, adult cephalic
823	Frequency	6.3 MHz
824	<b>RAB6-D, convex volume probe</b>	
825	Applications	Abdomen, OB/GYN, pediatric, neonatal
826	Biopsy guide	Single angle, reusable bracket (H46701AE)
827	Bandwidth	2.0 – 8.0 MHz
828	Number of elements	192
829	Field of view (max.)	80°
830	Physical foot print	62 x 34 mm
831	B-Mode frequency	3.5, 5.0, 8.0 MHz
832	Harmonic frequency	4.0, 5.0, 6.5, 8.0 MHz
833	PW Doppler frequency	3.1, 4.2, 5.0 MHz
834	Color Doppler frequency	2.8, 3.5, 3.8 MHz
835	<b>RIC5-9-D, convex volume probe</b>	
836	Applications	OB/GYN, urology
837	Biopsy guide	Single angle, reusable (H46721R)
838	Bandwidth	3.0 – 10.0 MHz
839	Number of elements	192
840	Field of view (max.)	180°
841	Physical foot print	32 x 27 mm
842	B-Mode frequency	5.0, 5.5, 6.0, 6.5, 7.0, 8.0 MHz
843	Harmonic frequency	6.0, 6.5, 7.0, 9.0 MHz
844	PW Doppler frequency	3.6, 4.2, 5.0 MHz
845	Color Doppler frequency	4.3, 6.1, 7.3 MHz
846	<b>External Inputs and outputs (not including on-board peripherals)</b>	
847	HDMI	
848	Ethernet	
849	Multiple USB 3.0 ports	
850	<b>Safety Conformance</b>	



851	<b>The LOGIQ Fortis is:</b>	
852	Classified to UL 60601-1 by a Nationally Recognized Test Lab	
853	Certified to CAN/CSA-C22.2 No. 60601.1-M90 by an SCC accredited test lab	
854	CE Marked to EU Medical Device Regulation MDR 2017/745	
855	Compliant to Council Directive 2011/65/EU for RoHS	
856	Conforms to the following standards for safety (including national deviations)	<ul style="list-style-type: none"> <li>• EMC Emissions group 1 class A device requirements as per sub clause 4.2 of CISPR 11</li> <li>• IEC 60601-1 Medical electrical equipment – Part 1: General requirements for safety</li> <li>• IEC 60601-1-2 Medical electrical equipment – Part 1-2: General requirements for basic safety and essential performance – Collateral standard: Electromagnetic disturbance – Requirements and tests</li> <li>• IEC 60601-1-6 Medical electrical equipment Part 1-6 general requirements for basic safety and essential performance – Collateral standard: usability</li> <li>• IEC 60601-2-37 Medical electrical equipment – Part 2-37: Particular requirements for the safety of ultrasonic medical diagnostic and monitoring equipment</li> <li>• IEC 62366 Medical devices – Application of usability engineering to medical devices</li> <li>• IEC62366-1 Medical device software – Software life-cycle processes</li> <li>• ISO 10993-1 Biological evaluation of medical devices – Part 1: Evaluation and testing within a risk management process</li> </ul>



857	<b>Supplement: cardiac measurements/calculations</b>	
858	<b>B-Mode measurements</b>	
859	Aorta	<ul style="list-style-type: none"> <li>• Aortic Root Diameter (Ao Root Diam)</li> <li>• Aortic Arch Diameter (Ao Arch Diam)</li> <li>• Ascending Aortic diameter (Ao Asc)</li> <li>• Descending Aortic Diameter (Ao Desc Diam)</li> <li>• Aorta Isthmus (Ao Isthmus)</li> <li>• Aorta (Ao st junct)</li> </ul>
860	Aortic valve	<ul style="list-style-type: none"> <li>• Aortic Valve Cusp Separation (AV Cusp)</li> <li>• Aortic Valve Area Planimetry (AVA Planimetry)</li> <li>• (Trans AVA)</li> </ul>
861	Left atrium	<ul style="list-style-type: none"> <li>• Left Atrium Diameter (LA Diam)</li> <li>• LA Length (LA Major)</li> <li>• LA Width (LA Minor)</li> <li>• Left Atrium Diameter to AoRoot Diameter Ratio (LA/Ao ratio)</li> <li>• Left Atrium Area (LAA(d), LAA(s))</li> <li>• Left Atrium Volume, Single Plane, Method of Disk (LAEDV A2C, LAESV A2C) (LAEDV A4C, LAESV A4C), (LAEDV A-L, LAEDV Index A-L, LAESV A-L, LAESV Index A-L)</li> </ul>
862	Left ventricle	<ul style="list-style-type: none"> <li>• Left Ventricle Mass (LVPWd, LVPWs)</li> <li>• Left Ventricle Volume, Teichholz/Cubic (LVIDd, LVI Ds)</li> <li>• Left Ventricle Internal Diameter (LVIDd, LVI Ds) Left Ventricle Length (LVLd, LVLs)</li> <li>• Left Ventricle Outflow Tract Diameter (LVOT Diam)</li> <li>• Left Ventricle Posterior Wall Thickness (LVPWd, LVPWs)</li> <li>• Left Ventricle Length (LV Major)</li> <li>• Left Ventricle Width (LV Minor)</li> <li>• Left Ventricle Outflow Tract Area (LVOT)</li> <li>• Left Ventricle Area, Two Chamber/Four Chamber/Short Axis (LVA (d), LVA (s))</li> <li>• Left Ventricle Endocardial Area, Width (LVA (d), LVA(s))</li> <li>• Left Ventricle Epicardial Area, Length (LVAepi (d), LVAepi (s))</li> <li>• Left Ventricle Mass Index (LVPWd, LVPWs)</li> <li>• Ejection Fraction, Teichholz/Cube (LVIDd, LVIDs)</li> </ul>
863	Left ventricle continued	<ul style="list-style-type: none"> <li>• Left Ventricle Posterior Wall Fractional Shortening (LVPWd, LVPWs)</li> <li>• Left Ventricle Stroke Index, Teichholz/Cube (LVIDd, LVIDs and Body Surface Area)</li> <li>• Left Ventricle Fractional Shortening (LVIDd, LVIDs)</li> <li>• Left Ventricle Stroke Volume, Teichholz/Cubic (LVIDd, LVIDs)</li> <li>• Left Ventricle Stroke Index, Single Plane, Two Chamber, Method of Disk (LVI Dd, LVIDs, LVSD, LVSS)</li> <li>• Left Ventricle Stroke Index, Single Plane, Four Chamber, Method of Disk (LVI Dd, LVIDs, LVSD, LVSS)</li> <li>• Left Ventricle Stroke Index, Bi-Plane, Bullet, Method of Disk (LVAd, LVAs)</li> <li>• Interventricular Septum (IVS)</li> <li>• Left Ventricle Internal Diameter (LVI D)</li> <li>• Left Ventricle Posterior Wall Thickness (LVPW)</li> </ul>
864	Mitral valve	<ul style="list-style-type: none"> <li>• Mitral Valve Annulus Diameter (MV Ann Diam)</li> <li>• E-Point-to-Septum Separation (EPSS)</li> <li>• Mitral Valve Area Planimetry (MVA Planimetry)</li> </ul>
865	Pulmonic valve	<ul style="list-style-type: none"> <li>• Pulmonic Valve Area (PV Planimetry)</li> <li>• Pulmonic Valve Annulus Diameter (PV Annulus Diam)</li> <li>• Pulmonic Diameter (Pulmonic Diam)</li> </ul>
866	Right atrium	<ul style="list-style-type: none"> <li>• Right Atrium Diameter, Length (RAD Ma)</li> <li>• Right Atrium Diameter, Width (RAD Mi)</li> <li>• Right Atrium Area (RAA)</li> <li>• Right Atrium Volume, Single Plane, Method of Disk (RAAd)</li> <li>• Right Atrium Volume, Systolic, Single Plane, Method of Disk (RAAs)</li> </ul>



867	Right ventricle	<ul style="list-style-type: none"> <li>• Right Ventricle Outflow Tract Area (RVOT Planimetry)</li> <li>• Left Pulmonary Artery Area (LPA Area)</li> <li>• Right Pulmonary Artery Area (RPA Area)</li> <li>• Right Ventricle Internal Diameter (RVIDd, RVIDs)</li> <li>• Right Ventricle Diameter, Length (RVD Ma)</li> <li>• Right Ventricle Diameter, Width (RVD Mi)</li> <li>• Right Ventricle Wall Thickness (RVAWd, RVAWs)</li> <li>• Right Ventricle Outflow Tract Diameter (RVOT Diam)</li> <li>• Left Pulmonary Artery (LPA)</li> <li>• Main Pulmonary Artery (MPA)</li> <li>• Right Pulmonary Artery (RPA)</li> </ul>
868	System inferior vena cava	<ul style="list-style-type: none"> <li>• Systemic Vein Diameter (Systemic Diam)</li> <li>• Patent Ductus Arteriosis Diameter (PDA Diam)</li> <li>• Pericard Effusion (PEs)</li> <li>• Patent Foramen Ovale Diameter (PFO Diam)</li> <li>• Ventricular Septal Defect Diameter (VSD Diam)</li> <li>• Interventricular Septum (IVS) Fractional Shortening (IVSd, IVSs)</li> </ul>
869	Tricuspid valve	<ul style="list-style-type: none"> <li>• Tricuspid Valve Area (TV Panimetry)</li> <li>• Tricuspid Valve Annulus Diameter (TV Annulus Diam)</li> </ul>
870	<b>M-Mode measurements</b>	
871	Aorta	<ul style="list-style-type: none"> <li>• Aortic Root Diameter (Ao Root Diam)</li> <li>• Aortic Valve</li> <li>• Aortic Valve Diameter (AV Diam)</li> <li>• Aortic Valve Cusp separation (AV Cusp)</li> <li>• Aortic Valve Ejection Time (LVET)</li> </ul>
872	Left atrium	<ul style="list-style-type: none"> <li>• Left Atrium Diameter to AoRoot Diameter Ratio (LA/Ao Ratio)</li> <li>• Left Atrium Diameter (LA Diam)</li> </ul>
873	Left ventricle	<ul style="list-style-type: none"> <li>• Left Ventricle Volume, Teichholz/Cubic (LVIDd, LVI Ds)</li> <li>• Left Ventricle Internal Diameter (LVIDd, LVI Ds)</li> <li>• Left Ventricle Posterior Wall Thickness (LVPWd, LVPWs)</li> <li>• Left Ventricle Ejection Time (LVET)</li> <li>• Left Ventricle Pre-Ejection Period (LVPEP)</li> <li>• Interventricular Septum (IVS)</li> <li>• Left Ventricle Internal Diameter (LVI D)</li> <li>• Left Ventricle Posterior Wall Thickness (LVPW)</li> </ul>
874	Mitral valve	<ul style="list-style-type: none"> <li>• E-Point-to-Septum Separation (EPSS)</li> <li>• Mitral Valve Leaflet Separation (D-E Excursion)</li> <li>• Mitral Valve Anterior Leaflet Excursion (D-E Excursion)</li> <li>• Mitral valve D-E Slope (D-E Slope)</li> <li>• Mitral Valve E-F Slope (E-F Slope)</li> <li>• Mitral Annular Plane Systolic Excursion (MAPSE)</li> </ul>
875	Pulmonic valve	<ul style="list-style-type: none"> <li>• QRS Complex to End of Envelope (Q-PV close)</li> </ul>
876	Right ventricle	<ul style="list-style-type: none"> <li>• Right Ventricle Internal Diameter (RVIDd, RVIDs)</li> <li>• Right Ventricle Wall Thickness (RVAWd, RVAWs)</li> <li>• Right Ventricle Outflow Tract Diameter (RVOT Diam)</li> <li>• Right Ventricle Ejection Time (RVET)</li> <li>• Right Ventricle Pre-Ejection Period (RVPEP)</li> </ul>
877	System	<ul style="list-style-type: none"> <li>• Pericard Effusion (PE (d))</li> </ul>
878	Tricuspid valve	<ul style="list-style-type: none"> <li>• QRS Complex to End of Envelope (Q-TV close)</li> <li>• Tricuspid Annular Plane Systolic Excursion (TAPSE)</li> </ul>



879	<b>Doppler Mode measurements</b>	
880	Aortic valve	<ul style="list-style-type: none"> <li>• Aortic Insufficiency Mean Pressure Gradient (AR Trace)</li> <li>• Aortic Insufficiency Peak Pressure Gradient (AR Vmax)</li> <li>• Aortic Insufficiency End Diastole Pressure Gradient (AR Trace)</li> <li>• Aortic Insufficiency Mean Velocity (AR Trace)</li> <li>• Aortic Insufficiency Velocity Time Integral (AR Trace)</li> <li>• Aortic Valve Mean Velocity (AV Trace)</li> <li>• Aortic Valve Velocity Time Integral (AV Trace)</li> <li>• Aortic Valve Mean Pressure Gradient (AV Trace)</li> <li>• Aortic Valve Peak Pressure Gradient (AR Vmax)</li> <li>• Aortic Insufficiency Peak Velocity (AR Vmax)</li> <li>• Aortic Insufficiency End-Diastolic Velocity (AR Trace)</li> <li>• Aortic Valve Peak Velocity (AV Vmax)</li> <li>• Aortic Valve Peak Velocity at Point E (AV Vmax)</li> </ul>
881	Aortic valve continued	<ul style="list-style-type: none"> <li>• Aorta Proximal Coarctation (Coarc Pre-Duct)</li> <li>• Aorta Distal Coarctation (Coarc Post-Duct)</li> <li>• Aortic Valve Insufficiency Pressure Half Time (AR PHT)</li> <li>• Aortic Valve Flow Acceleration (AV Trace)</li> <li>• Aortic Valve Pressure Half Time (AV Trace)</li> <li>• Aortic Valve Acceleration Time (AV Acc Time)</li> <li>• Aortic Valve Deceleration Time (AV Dec Time)</li> <li>• Aortic Valve Ejection Time (AVET)</li> <li>• Aortic Valve Acceleration to Ejection Time Ratio (AV Acc Time, AVET)</li> <li>• Aortic Valve Area(VTI): AVA (Vmax)</li> </ul>
882	Left ventricle	<ul style="list-style-type: none"> <li>• Left Ventricle Outflow Tract Peak Pressure Gradient (LVOT Vmax)</li> <li>• Left Ventricle Outflow Tract Peak Velocity (LVOT Vmax)</li> <li>• Left Ventricle Outflow Tract Mean Pressure Gradient (LVOT Trace)</li> <li>• Left Ventricle Outflow Tract Mean Velocity (LVOT Trace)</li> <li>• Left Ventricle Outflow Tract Velocity Time Integral (LVOT Trace)</li> <li>• Left Ventricle Ejection Time (LVET)</li> </ul>
883	Mitral valve	<ul style="list-style-type: none"> <li>• E' Early diastolic mitral valve annular velocity (E')</li> <li>• E' Avg Averaged early diastolic mitral valve annular velocity (E' Avg)</li> <li>• E' Lat Early diastolic mitral valve lateral annular velocity (E' Lat)</li> <li>• E' Medial Early diastolic mitral valve medial annular velocity (E' Medial)</li> <li>• E' Sept Early diastolic mitral</li> <li>• Mitral inflow E velocity to E' ratio (E/E')</li> <li>• Mitral inflow E velocity to E' Avg ratio (E/E' Avg)</li> <li>• Mitral inflow E velocity to E' Lat ratio (E/E' Lat)</li> <li>• Medial Mitral inflow E velocity to E' Medial ratio (E/E')</li> <li>• Mitral inflow E velocity to E' Sept ratio (E/E' Sept)</li> <li>• Mitral Valve Regurgitant Flow Acceleration (MR Trace)</li> <li>• Mitral Valve Regurgitant Mean Velocity (MR Trace)</li> </ul>
884	Mitral valve continued	<ul style="list-style-type: none"> <li>• Mitral Regurgitant Mean Pressure Gradient (MR Trace)</li> <li>• Mitral Regurgitant Velocity Time Integral (MR Trace)</li> <li>• Mitral Valve Mean Velocity (MV Trace)</li> <li>• Mitral Valve Velocity Time Integral (MV Trace)</li> <li>• Mitral Valve Mean Pressure Gradient (MV Trace)</li> <li>• Mitral Regurgitant Peak Pressure Gradient (MR Vmax)</li> <li>• Mitral Valve Peak Pressure Gradient (MV Vmax)</li> <li>• Mitral Regurgitant Peak Velocity (MR Vmax)</li> <li>• Mitral Valve Peak Velocity (MV Vmax)</li> <li>• Mitral Valve Velocity Peak A (MV A Velocity)</li> <li>• Mitral Valve Velocity Peak E (MV E Velocity)</li> </ul>



885	Mitral valve continued	<ul style="list-style-type: none"> <li>• Mitral Valve Area According to PHT (MV PHT)</li> <li>• Mitral Valve Flow Deceleration (MV DecT)</li> <li>• Mitral Valve Pressure Half Time (MV PHT)</li> <li>• Mitral Valve Flow Acceleration (MV AccT)</li> <li>• Mitral Valve E-Peak to A-Peak Ratio (A-C and D-E) (MV E/ARatio)</li> <li>• Mitral Valve Acceleration Time</li> <li>• (MV Acc Time)</li> <li>• Mitral Valve Deceleration Time (MV Dec Time)</li> <li>• Mitral Valve Ejection Time ((MVET)</li> <li>• Mitral Valve A-Wave Duration (MV A Dur)</li> <li>• Mitral Valve Time to Peak (MV TTP)</li> <li>• Mitral Valve Acceleration Time/Deceleration Time Ratio (MVAcc/Dec Time)</li> <li>• Stroke Volume Index by Mitral Flow (MVA Planimetry, MVTrace)</li> </ul>
886	Pulmonic Valve	<ul style="list-style-type: none"> <li>• Pulmonic Insufficiency Peak Pressure Gradient (PR Vmax)</li> <li>• Pulmonic Insufficiency End-Diastolic Pressure Gradient (PRTrace)</li> <li>• Pulmonic Valve Peak Pressure Gradient (PV Vmax)</li> <li>• Pulmonic Insufficiency Peak Velocity (PR Vmax)</li> <li>• Pulmonic Insufficiency End-Diastolic Velocity (Prend Vmax)</li> <li>• Pulmonic Valve Peak Velocity (PV Vmax)</li> <li>• Pulmonary Artery Diastolic Pressure (PV Trace)</li> <li>• Pulmonic Insufficiency Mean Pressure Gradient (PR Trace)</li> </ul>
887	Pulmonic valve continued	<ul style="list-style-type: none"> <li>• Pulmonic Valve Mean Pressure Gradient (PV Trace)</li> <li>• Pulmonic Insufficiency Mean Square Root Velocity (PR Trace)</li> <li>• Pulmonic Insufficiency Velocity Time Integral (PR Trace)</li> <li>• Pulmonic Valve Mean Velocity (PV Trace)</li> <li>• Pulmonic Valve Velocity Time Integral (PV Trace)</li> <li>• Pulmonic Insufficiency Pressure Half Time (PR PHT)</li> <li>• Pulmonic Valve Flow Acceleration (PV Acc Time)</li> <li>• Pulmonic Valve Acceleration Time (PV Acc Time)</li> <li>• Pulmonic Valve Ejection Time (PVET)</li> <li>• QRS Complex to End of Envelope (Q-to-PV Close)</li> <li>• Pulmonic Valve Acceleration to Ejection Time Ratio (PV Acc Time, PVET)</li> </ul>
888	Right ventricle	<ul style="list-style-type: none"> <li>• Right Ventricle Outflow Tract Peak Pressure Gradient (RVOT Vmax)</li> <li>• Right Ventricle Outflow Tract Peak Velocity (RVOT Vmax)</li> <li>• Right Ventricle Outflow Tract Velocity Time Integral (RVOTTrace)</li> <li>• Right Ventricle Ejection Time (RV Trace)</li> <li>• Stroke Volume by Pulmonic Flow (RVOT Planimetry, RVOTTrace)</li> <li>• Right Ventricle Stroke Volume Index by Pulmonic Flow (RVOT Planimetry, RVOT Trace)</li> </ul>
889	System	<ul style="list-style-type: none"> <li>• Pulmonary Artery Peak Velocity (PV Vmax)</li> <li>• Pulmonary Vein Velocity Peak A (Reverse) (P Vein A)</li> <li>• Pulmonary Vein Peak Velocity (P Vein D, P Vein S)</li> <li>• Systemic Vein Peak Velocity (PDA Diastolic, PDA Systolic)</li> <li>• Ventricular Septal Defect Peak Velocity (VSD Vmax)</li> <li>• Atrial Septal Defect (ASD Diastolic, ASD Systolic)</li> <li>• Pulmonary Vein A-Wave Duration (P Vein A Dur)</li> <li>• IsoVolumetric Relaxation Time (IVRT)</li> <li>• IsoVolumetric Contraction Time (IVCT)</li> <li>• Pulmonary Vein S/D Ratio (P Vein D, P Vein S)</li> <li>• Ventricular Septal Defect Peak Pressure Gradient (VSD Vmax)</li> <li>• Pulmonic-to-Systemic Flow Ratio (Qp/Qs)</li> </ul>
890	Tricuspid valve	<ul style="list-style-type: none"> <li>• Tricuspid Regurgitant Peak Pressure Gradient (TR Vmax)</li> <li>• Tricuspid Valve Peak Pressure Gradient (TV Vmax)</li> <li>• Tricuspid Regurgitant Peak Velocity (TR Vmax)</li> <li>• Tricuspid Valve Peak Velocity (TV Vmax)</li> <li>• Tricuspid Valve Velocity Peak A (TV A Velocity)</li> <li>• Tricuspid Valve Velocity Peak E (TV E Velocity)</li> <li>• Tricuspid Regurgitant Mean Pressure Gradient (TR Trace)</li> <li>• Tricuspid Valve Mean Pressure Gradient (TV Trace)</li> </ul>



891	Tricuspid valve continued	<ul style="list-style-type: none"><li>• Tricuspid Regurgitant Mean Velocity (TR Trace)</li><li>• Tricuspid Regurgitant Velocity Time Integral (TR Trace)</li><li>• Tricuspid Valve Mean Velocity (TV Trace)</li><li>• Tricuspid Valve Velocity Time Integral (TV Trace)</li><li>• Tricuspid Valve Time to Peak (TV TTP)</li><li>• Tricuspid Valve Ejection Time (TV Acc/Dec Time)</li><li>• Tricuspid Valve A-Wave Duration (TV A Dur)</li><li>• QRS Complex to End of Envelope (Q-TV Close)</li><li>• Tricuspid Valve Pressure Half Time (TV PHT)</li><li>• Stroke Volume by Tricuspid Flow (TV Planimetry, TV Trace)</li><li>• Tricuspid Valve E-Peak to A-Peak Ratio (TV E/A Velocity)</li></ul>
-----	---------------------------	---



892	<b>Color Flow Mode measurements</b>	
893	Aortic valve	<ul style="list-style-type: none"> <li>• Proximal Isovelocity Surface Area: Regurgitant Orifice Area (AR Radius)</li> <li>• Proximal Isovelocity Surface Area: Radius of Aliased Point (AR Radius)</li> <li>• Proximal Isovelocity Surface Area: Regurgitant Flow (AR Trace)</li> <li>• Proximal Isovelocity Surface Area: Regurgitant Volume Flow (AR Trace)</li> <li>• Proximal Isovelocity Surface Area: Aliased Velocity (AR Vmax)</li> </ul>
894	Mitral valve	<ul style="list-style-type: none"> <li>• Proximal Isovelocity Surface Area: Regurgitant Orifice Area (MR Radius)</li> <li>• Proximal Isovelocity Surface Area: Radius of Aliased Point (MR Radius)</li> <li>• Proximal Isovelocity Surface Area: Regurgitant Flow (MR Trace)</li> <li>• Proximal Isovelocity Surface Area: Regurgitant Volume Flow (MR Trace)</li> <li>• Proximal Isovelocity Surface Area: Aliased Velocity (MR Vmax)</li> </ul>
895	<b>Combination Mode measurements</b>	
896	Aortic valve	<ul style="list-style-type: none"> <li>• Aortic Valve Area (Ao Root Diam, LVOT Vmax, AV Vmax)</li> <li>• Aortic Valve Area by Continuity Equation by Peak Velocity (Ao Root Diam, LVOT Vmax, AV Vmax)</li> <li>• Stroke Volume by Aortic Flow (AVA Planimetry, AV Trace)</li> <li>• Cardiac Output by Aortic Flow (AVA Planimetry, AV Trace, HR)</li> <li>• Aortic Valve Area by Continuity Equation VTI (Ao Root Diam, LVOT Vmax, AV Trace)</li> </ul>
897	Left ventricle	<ul style="list-style-type: none"> <li>• Cardiac Output, Teichholz/Cubic (LVIDd, LVI Ds, HR)</li> <li>• Cardiac Output Two Chamber, Single Plane, Area-Length/Method of Disk (Simpson) (LVAd, LVAs, HR)</li> <li>• Cardiac Output Four Chamber, Single Plane, Area-Length/Method of Disk (Simpson) (LVAd, LVAs, HR)</li> <li>• Ejection Fraction Two Chamber, Single Plane, Area-Length/Method of Disk (Simpson) (LVAd, LVAs)</li> <li>• Ejection Fraction Four Chamber, Single Plane, Area-Length/Method of Disk (Simpson) (LVAd, LVAs)</li> <li>• Left Ventricle Stroke Volume, Single Plane, Two Chamber/Four Chamber, Area-Length (LVAd, LVAs)</li> </ul>
898	Left ventricle continued	<ul style="list-style-type: none"> <li>• Left Ventricle Stroke Volume, Single Plane, Two Chamber/Four Chamber, Method of Disk (Simpson) (LVIDd, LVIDs, LVAd, LVAs)</li> <li>• Left Ventricle Volume, Two Chamber/Four Chamber, Area-Length (LVAd, LVAs)</li> <li>• Ejection Fraction, Bi-Plane, Method of Disk (LVAd, LVAs, 2CH, 4CH)</li> <li>• Left Ventricle Stroke Volume, Bi-Plane, Method of Disk (LVAd, LVAs, 2CH, 4CH)</li> <li>• Left Ventricle Volume, Bi-Plane, Method of Disk (LVAd, LVAs, 2CH, 4CH)</li> <li>• Left Ventricle Stroke Index, Single Plane, Two Chamber/Four Chamber, Area-Length (LVSD, LVSS and BSA)</li> <li>• Left Ventricle Volume, Single Plane, Two Chamber/Four Chamber, Method of Disk (LVAd, LVAs)</li> <li>• Left Ventricle Volume, Apical View, Long Axis, Method of Disk (LVAd, LVAs)</li> </ul>
899	Mitral valve	<ul style="list-style-type: none"> <li>• Stroke Volume by Mitral Flow (MVA Planimetry, MV Trace)</li> <li>• Cardiac Output by Mitral Flow (MVA Planimetry, MV Trace, HR)</li> </ul>
900	Pulmonic valve	<ul style="list-style-type: none"> <li>• Stroke Volume by Pulmonic Flow (PV Planimetry, PV Trace)</li> <li>• Cardiac Output by Pulmonic Flow (PV Planimetry, PV Trace, HR)</li> </ul>
901	Tricuspid valve	<ul style="list-style-type: none"> <li>• Cardiac Output by Tricuspid Flow (TV Planimetry, TV Trace, HR)</li> </ul>
902	<b>Combination Mode measurements</b>	
903	Parameter: lists the mode, the measurement folder and the specific measurement	



904	Measured Value: Up to six measurement values for each item. Average, maximum, minimum or last
905	<b>Generic study in cardiology</b>
906	Stroke Volume (SV)
907	Cardiac Output (CO)



© GE, 2021

GE Healthcare reserves the right to make changes in specifications and features shown herein, or discontinue the product described at any time without notice or obligation. Contact your GE Healthcare representative for the most current information. GE, the GE Monogram, LOGIQ, cSound, XDclear, Radiantflow, InSite, CrossXBeam, and HDlive are trademarks of GE. Koios DS is a trademark of Koios Medical. BI-RADS is a registered trademark of the American College of Radiology. DICOM is a trademark of the National Electrical Manufacturers Association. Tricify is a trademark of Trice Imaging, Inc. GE Healthcare, a division of GE. GE Medical Systems, Inc., doing business as GE Healthcare.

DOC2671561





# cSound Architecture

Ultrasound for today, platform for tomorrow

The breadth of clinical scenarios in general imaging ultrasound places significant demands on the ultrasound device. A patient who cannot hold her breath while a renal Doppler is performed. A patient whose tendon tear requires sub millimeter resolution. An obese patient needing a liver biopsy. A brain scan of a neonate in an incubator. A liver fibrosis assessment that depends on detecting a shear wave signal thinner than a human hair. In today's demanding clinical environment, the ultrasound machine is a partner in helping the clinician meet every challenge.

GE Healthcare has designed its advanced cSound™ Architecture to put the latest ultrasound technology in the hands of clinicians. It combines the power of XDclear™ probes with a new cSound Imageformer to enable confident diagnoses, provide comprehensive tools, and support concise workflow.

## cSound Imageformer

The cSound Imageformer is the data acquisition and processing engine of the new architecture. At its core are cutting-edge NVIDIA® GPUs, the same graphics processing technology that is advancing the driverless car industry and the next generation of video gaming. This technology gives GE ultrasound engineers access to 48 times the data throughput and 10 times the processing power of our previous systems.\* This opens up new opportunities, allowing the cSound Imageformer to collect and use more data to create every ultrasound image.





## Traditional Beamforming

To understand cSound Imageforming, it helps to review how traditional beamforming works. As shown in Figure 1, traditional beamforming is performed in customized hardware and only the resulting beam or vector data is provided to the flexible, software-based processor that creates the ultrasound images.


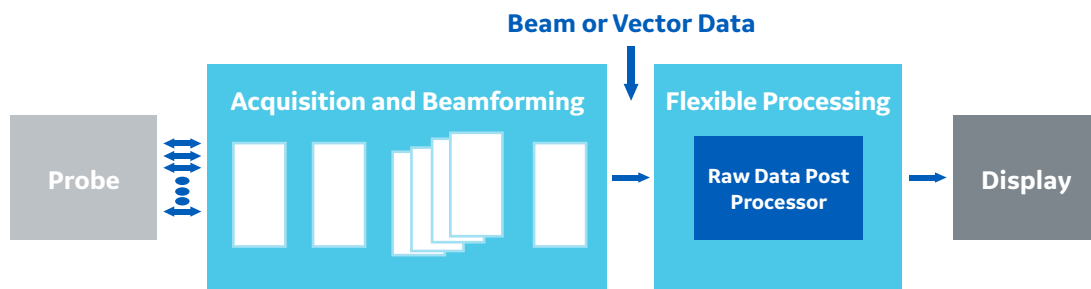


Figure 1. A traditional beamforming architecture.

### Traditional Beamforming Steps

1. A transmit event is performed. The return ultrasound data is dynamically received and collected in a single instance of channel memory.
2. The collected channel data is processed to create a particular portion of the image often referred to as one or more vectors or beams.  
*Note: If multiple focal depths are desired, steps 1 and 2 are also repeated with a transmit event focused at a different depth.*
3. Steps 1-2 are repeated for another portion of the image until the entire image has been created.

### Traditional Beamformer

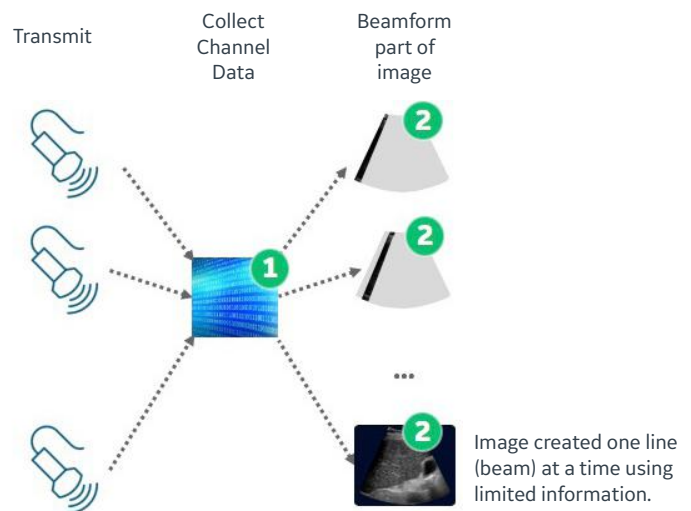

The channel data processed in step 2 and then overwritten still has useful information. However, a traditional beamformer has no means to extract this additional value before the channel data associated with the next transmit event overwrites it.



## cSound Imageforming – Methodology

As shown in Figure 2, cSound Imageforming is performed using flexible, GPU-based processing. In contrast to traditional beamforming, the cSound Architecture moves raw channel data at high speeds from the acquisition system to components that perform flexible, software-based processing, including the cSound Imageformer. This channel data can be retained in memory even as channel data from subsequent transmit events is acquired and transferred to the cSound Imageformer.


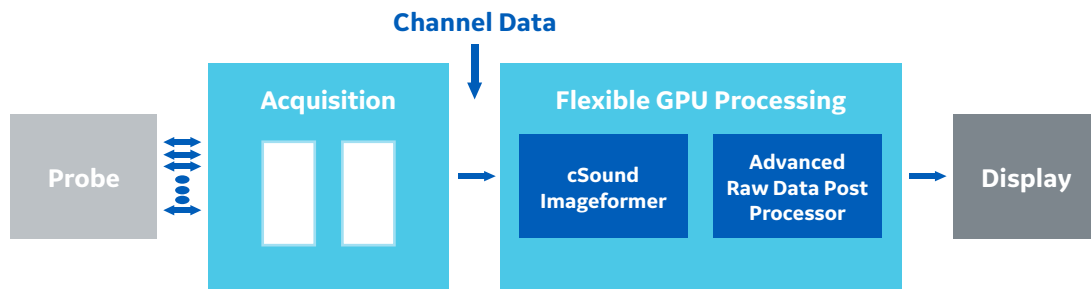


Figure 2. cSound Architecture.

### cSound Imageforming Phases

1. Acquisition – A series of transmit events are performed with the return ultrasound data being dynamically received and transferred to memory.
2. Reconstruction – The channel data from all of the transmits is combined to form the image.

### New cSound Imageformer

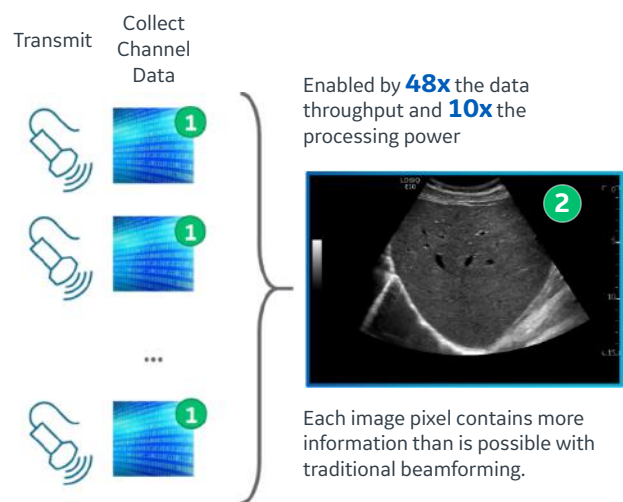

Similar to CT and MRI, cSound Imageforming has a distinct acquisition phase followed by a reconstruction phase. This requires the cSound Architecture to acquire, move and store large amounts of channel data and, once collected, the cSound Imageformer must be able to process the data at high speeds to enable real-time image reconstruction. The image formation process leverages channel data that would have been discarded in traditional beamforming. This additional data provides numerous samples for every point in the image. The image formation process combines these samples to achieve transmit focus for each point in the image, enhance contrast resolution and deliver fine spatial resolution.



## cSound Imageformer – Retrospective Transmit Focus

In traditional beamforming, each transmit event has a transmit focus that is created by adjusting the time delays of individual transducer elements. This generates a curved wave front that converges until reaching a particular depth (the focus depth) and then diverges as it continues to propagate beyond the focus depth. The focus is the location that is insonified from multiple directions.

For each transmit event, the cSound Imageformer collects and saves the receive ultrasound data for each element. This is referred to as channel data. *Even when a new transmit event occurs, the channel data associated with previous transmit events is retained and not overwritten.*

Individual transmit events are spatially and/or angularly offset from one another creating significant overlap. As a result, for any point in the image, there are multiple transmit events that have insonified the point, each from a different direction. Knowing the spatial locations of a particular point in the image relative to a given transmit event, the cSound Imageformer can retrospectively process the channel data of each intersecting transmit event, and then coherently

combine the results to achieve retrospective transmit focus at that point. It is worth noting that noise associated with each transmit beam is independent and therefore sums incoherently while the signal itself sums coherently. This increases the signal-to-noise ratio, further improving contrast resolution throughout the image.

This approach to focusing at each point in an image is possible for all types of transmit events providing there is overlap.

- **Converging waves** – Sound from multiple elements converges at a finite depth relative to the transducer face
- **Plane waves** – Sound from multiple elements is unfocused or essentially focused at an infinite depth
- **Diverging waves** – Sound from multiple elements diverges as if the focus was behind the transducer face

The cSound Imageformer is capable of all types of transmit events, giving engineers the flexibility to optimize the system uniquely depending on the needs of each clinical application.

## cSound Imageformer – Retrospective Transmit Focus, an Example

For illustrative purposes consider a simplified scenario, as shown in Figure 3.

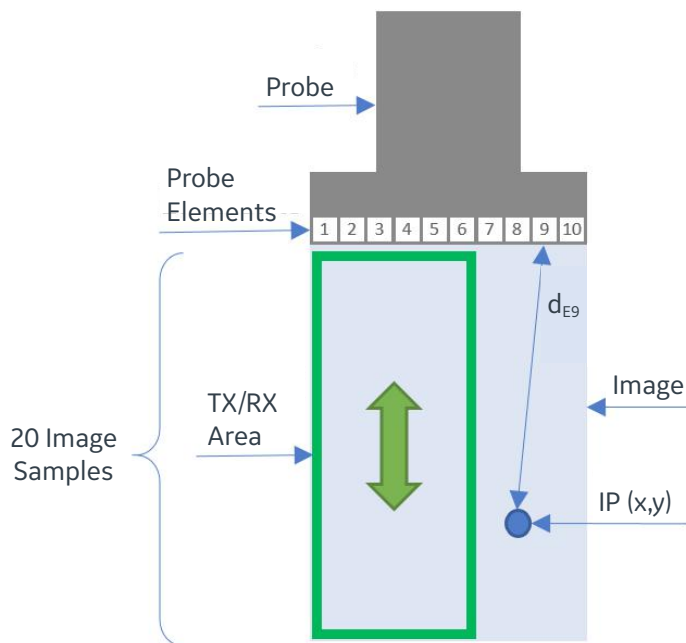


Figure 3. A simplified imaging scenario for illustrating retrospective transmit focus.

- Linear transducer with just 10 elements (E1 – E10)
- Each transmit event uses just six elements for transmitting and receiving. In this case, the first transmit event uses elements 1 through 6 (1-6) and then subsequent transmit events shift by a single element to use elements 2-7, 3-8, 4-9, and 5-10 for a total of 5 transmit events to create the image
- All transmit events are unfocused
- The receive signal is sampled so that 20 samples cover the depth of the image
- Each point in the image can be represented by IP (x,y) where x is the lateral direction and is restricted to the width of the image (which equals the width of the probe) and y is the axial direction and is restricted to the depth of the image
- The distance between IP (x,y) and a particular probe element is defined as  $d_{EN}$  where N is the element number 1-10



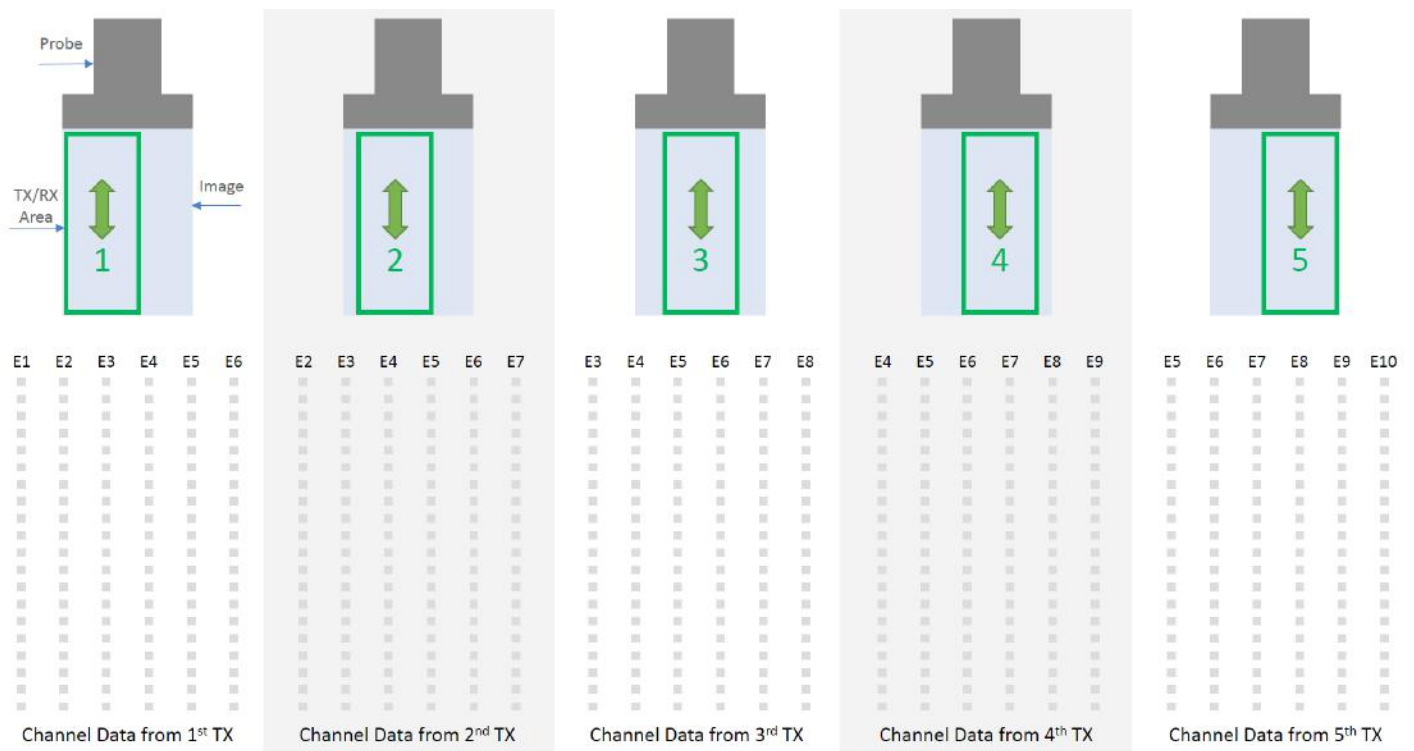


Figure 4. The first transmit (1) occurs and channel data is collected and stored. This is repeated for subsequent transmits (2 through 5) which are each offset from the previous.

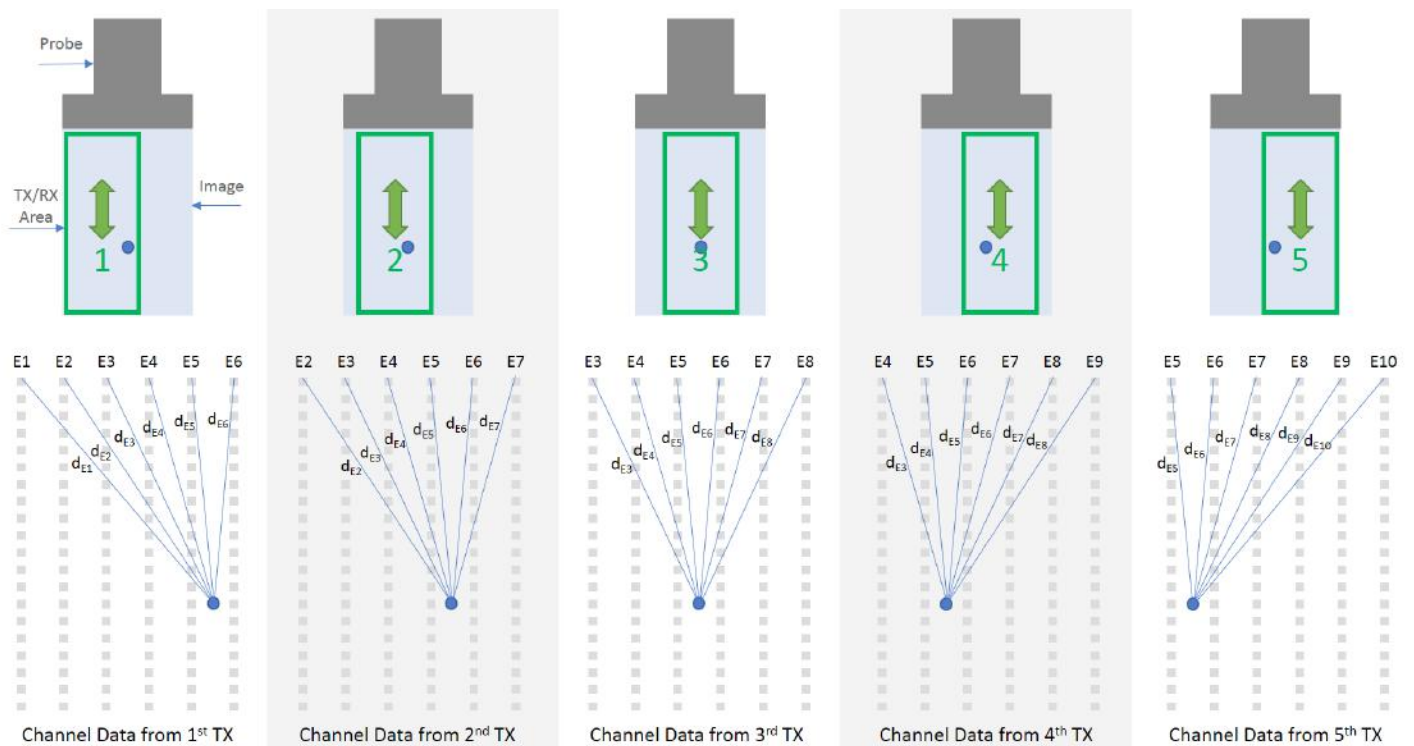


Figure 5. For each set of relevant channel data, the distance between the deep image point (represented by the circle) and each probe element is computed.



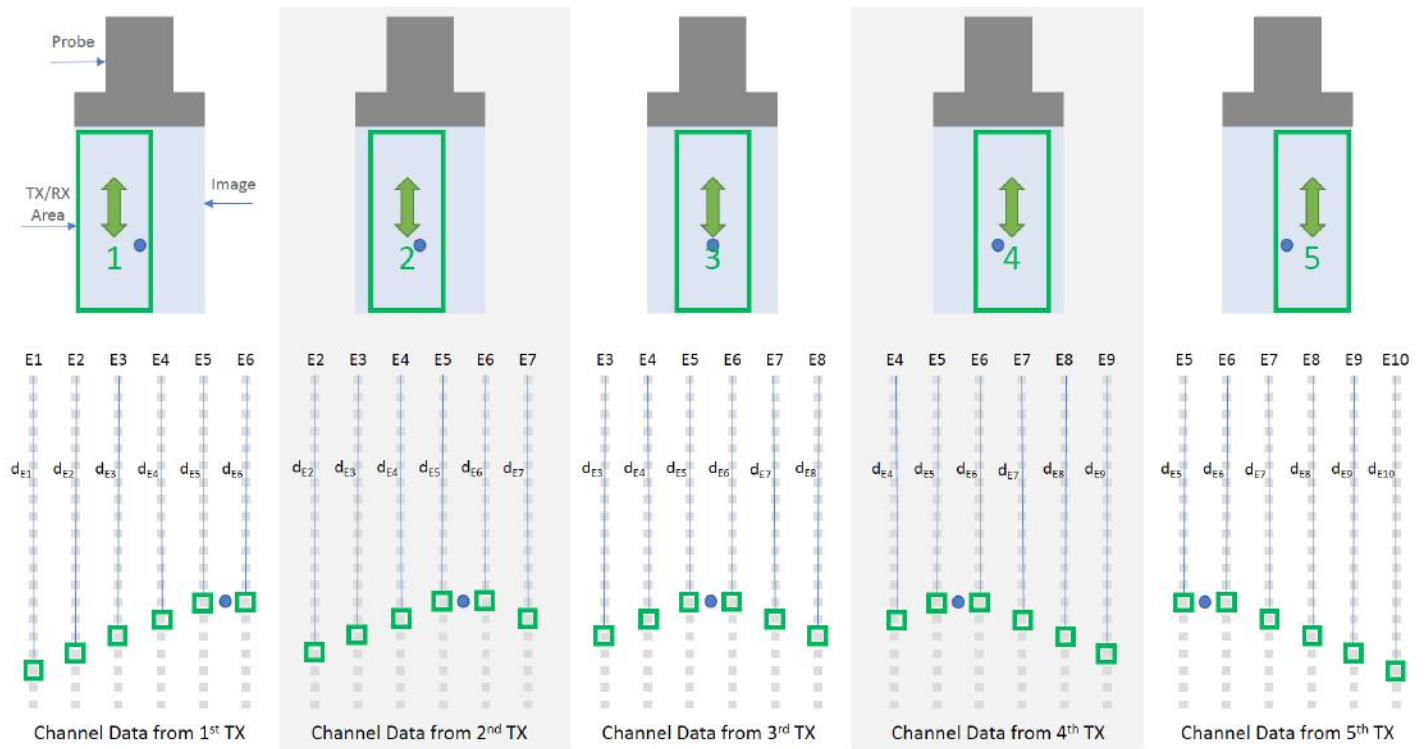


Figure 6. The computed distances between the image point and each element are used to access the channel data that focuses on the image point. The selected channel data from each transmit is coherently summed to determine the signal associated with the image point.

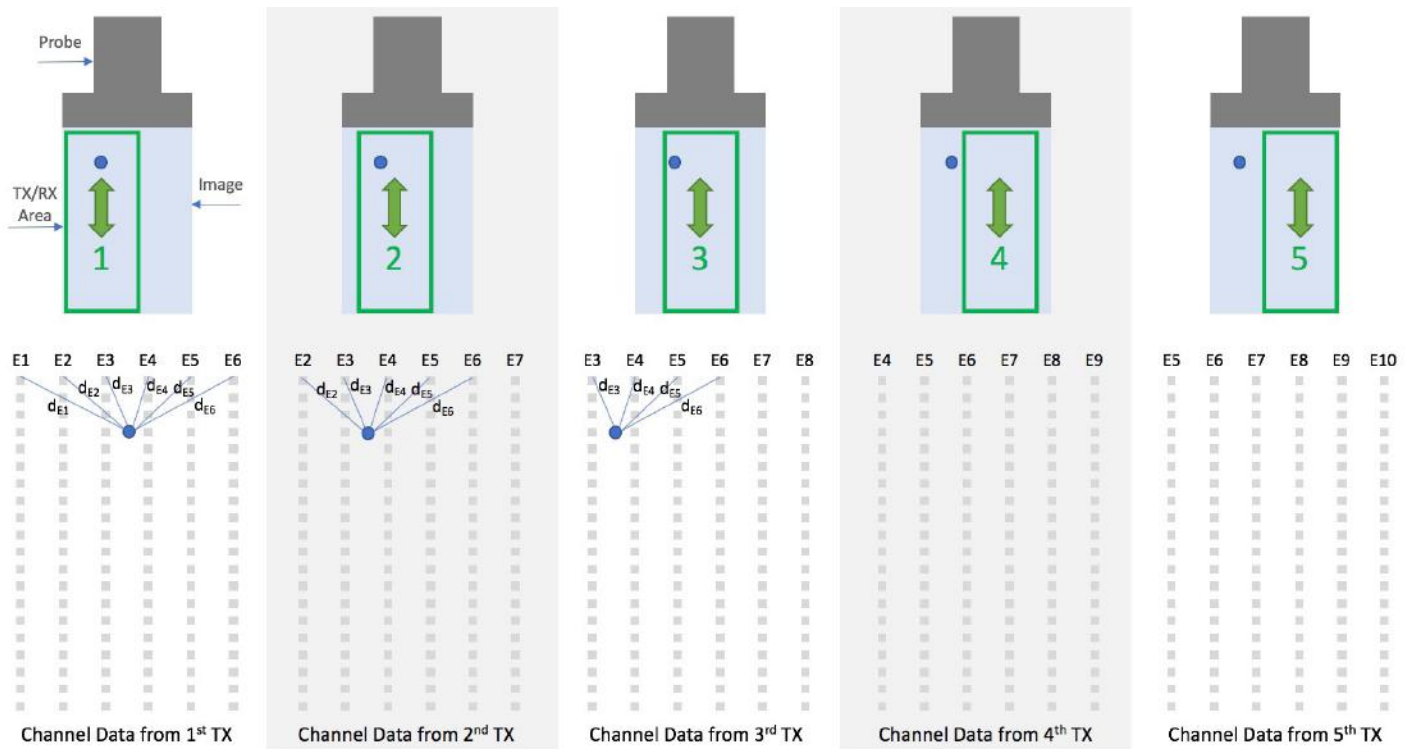


Figure 7. For each set of relevant channel data, the distance between the shallow image point (represented by the circle) and each probe element is computed. Note that transmits 4 and 5 do not overlap with the image point. Further note that some elements, such as E7 and E8 on transmit 3, are not included because of their steep angle relative to the image point.



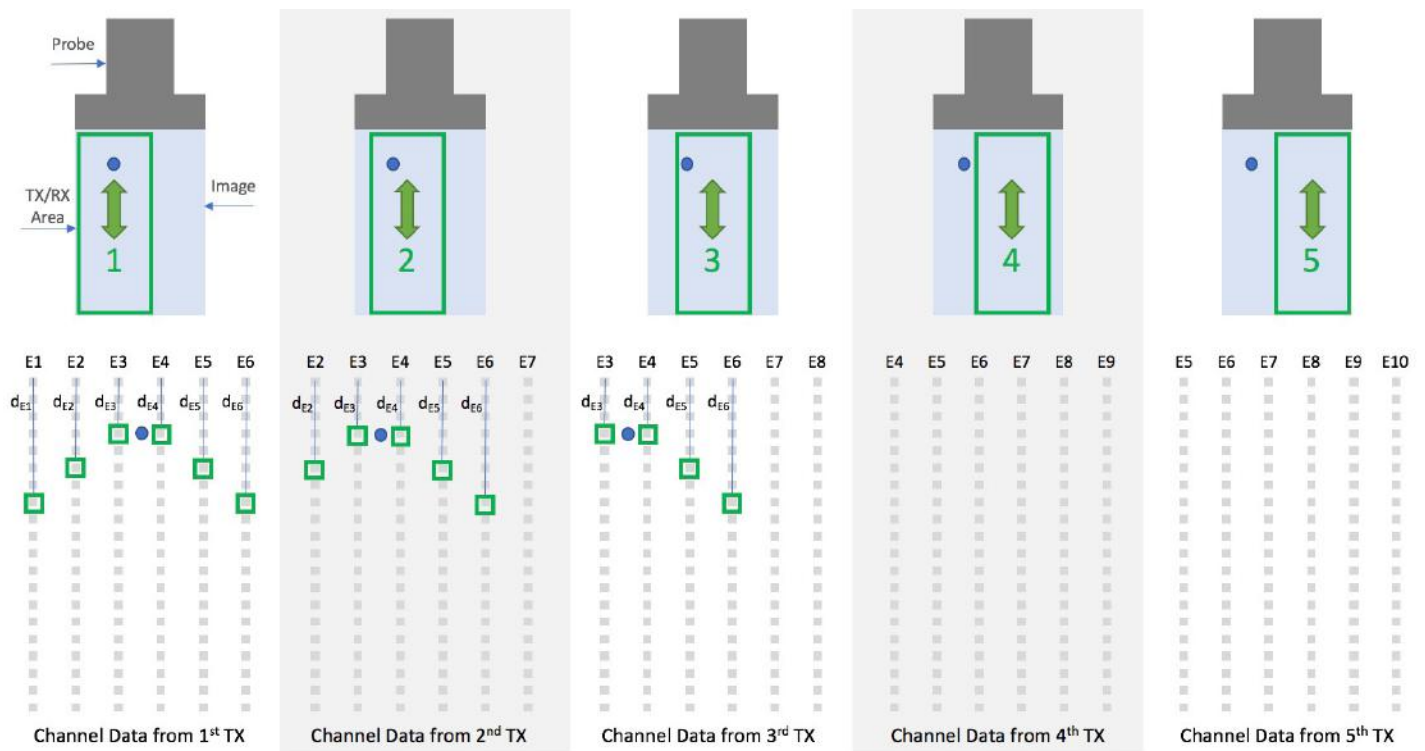


Figure 8. The computed distances between the image point and each element are used to access the channel data that focuses on the image point. The selected channel data from each transmit is coherently summed to determine the signal associated with the image point.

When extending this simplified scenario to the cSound Imageformer, there are additional complexities to consider. For example, the geometry of the transducer and the delay profile of the transmit event impact the computation of the image point to probe element distance and therefore the offset needed to reference the correct channel data. In another difference, the received elements are often larger than the number of transmit elements. Most notably, the sheer volume of data puts extensive demands on the system:

- The large quantity of collected channel data must be reliably and quickly streamed to the channel data memory before additional channel data is collected from the next transmit
- A massive amount of channel memory is required to store the channel data collected from many transmit events
- The retrospective processing of each relevant set of channel data for each point in the image requires intensive, ultra-high-speed, parallel computations to be performed to achieve real-time imaging at very high frame and volume rates

In a less powerful system, the real-time nature of imageforming could be achieved by restricting the amount of data collected by each transmit; speed would come at the expense of image quality. The cSound Architecture, in contrast, is able to keep up without restricting the data, even in radiology's most challenging applications. To put the cSound Architecture's performance in context, it can move the equivalent of multiple DVDs worth of data in one second.



## cSound Imageformer – Benefits

Imagine an ultrasound department where no image is acquired with the focal zone in the wrong position. With each point in the image in focus, the user doesn't need to select multiple focal zones or to move the focus position. Additionally, there are no trade-offs between near- and far-field image quality. Deep liver imaging provides detailed data from the capsule to the diaphragm. When biopsying a deep lesion, there is no compromise to needle visualization as it enters the image area. When surveying breast tissue, a clinician is able to see small lesions present from the skin line to the chest wall – all without the user having to make any adjustments.

While greater focal range in ultrasound has traditionally meant lower frame rates, cSound Imageforming actually increases frame rates. It requires a smaller collection of transmit events, a direct result of efficiently using the data collected from each individual transmit event. To understand this efficiency, consider that an ultrasound transmit event can be focused, but the sound energy still travels in many directions; it acts like a flashlight rather than a laser.

Though a flashlight generates maximum light energy in the center of its beam, there is still useful visual information in the light outside of the central beam. Similarly, there is much useful ultrasound image data in the sound that propagates outside the focused direction and the cSound Imageformer is designed to take full advantage of this data.

## cSound Imageformer – A Platform for Growth

cSound Imageforming runs on high performance NVIDIA GPUs, but the imageforming algorithms are software based. This affords significant flexibility; the algorithms can be adjusted for specific applications and evolve over time without impacting the underlying hardware architecture. In addition to forming the image, current algorithms can incorporate Adaptive Contrast Enhancement (ACE) and other GE proprietary techniques to boost the real image signal and suppress artifact. And with advances in GPU technology, there is potential to incorporate newer GPUs into the platform, enabling even more sophisticated algorithms.

## Advanced Raw Data Post Processor

The improved images resulting from the cSound Imageformer flow into the Advanced Raw Data Post Processor where additional enhancement is performed by spatial compounding, frame averaging, advanced speckle reduction imaging (Advanced SRI), and other functions. The post-processed image data is then mapped to gray scale levels and the scan is converted for display to the operator.

While speckle reduction imaging has been a feature of ultrasound systems for many years, Advanced SRI is GE's most sophisticated algorithm to date, and requires the expanded computational power of the cSound architecture to achieve real-time results. It employs proprietary processing steps at different resolutions of the raw image data to smooth speckle-based artifacts while simultaneously enhancing structures of all sizes within the image. The level of smoothing and enhancement is adjustable by the user.

The "Raw Data" aspect of the Advanced Raw Data Post Processor refers to the fact that image data is saved prior to the processing steps. This allows the user to continue to adjust the processing long after the images have been saved.


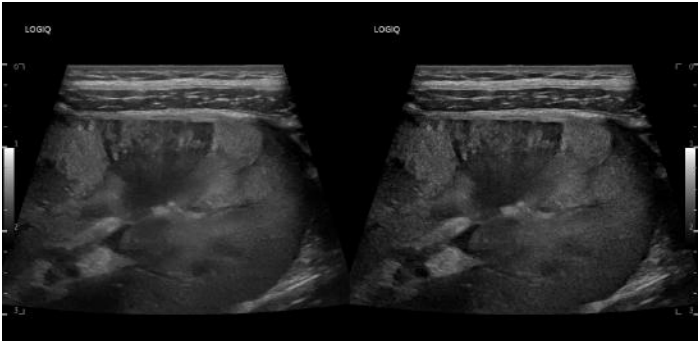


Figure 9. Advanced SRI (right) takes advantage of the increased computational power of the cSound Architecture to identify and enhance structures of all sizes while reducing speckle-based artifacts.



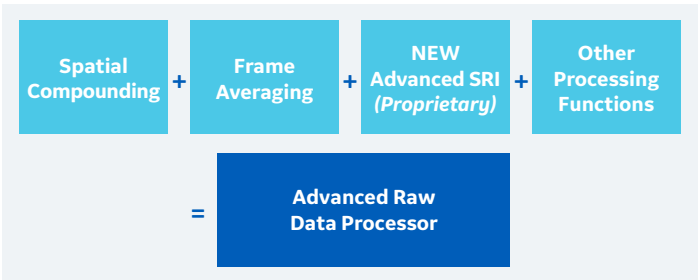

## XDclear Probes

While cSound Imageforming provides numerous benefits over traditional beamforming, the quality of the acoustic data coming into the system is still of utmost importance. In combination with the cSound Architecture's state-of-the-art transmit and receive electronics, XDclear transducers help deliver a more powerful, pure, and efficient sound wave with wider bandwidth than traditional GE transducer technology. This results in impressive deep penetration and high resolution, enabling ultrasound to be used effectively on a broad range of patients.



Figure 10. XDclear probes: Derive their superior performance from three key technologies: Single Crystal, Cool Stack, and Acoustic Amplifier.

XDclear transducers are a proprietary combination of advanced materials and innovative design. The XDclear design incorporates an enhanced piezoelectric material, Single Crystal, to generate a high quality acoustic signal. The quality of that signal is preserved through an innovative Acoustic Amplifier design coupled with GE's Cool Stack technology to help optimize energy management. The ability to effectively and efficiently combine these technologies is what makes XDclear extraordinary.

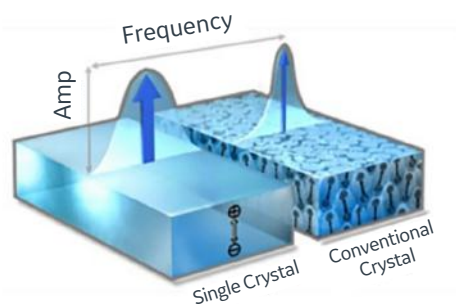


Figure 11. *Single Crystal*: Advanced piezoelectric material that delivers high quality acoustic signal with a wider bandwidth than conventional piezoelectric material.

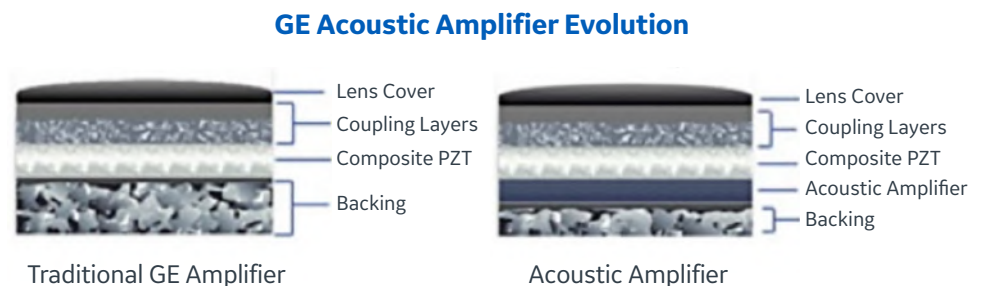


Figure 12. *Acoustic Amplifier*: Preserves the acoustic signal through an innovative design that captures and redirects the unused energy that passes through the crystal to enhance sensitivity, axial resolution, and penetration.



XDclear transducers enable deep penetration and resolution. One objective measure of transducer performance is bandwidth: the range of frequencies that the transducer can transmit and receive. Increased bandwidth allows a transducer to cover a broader frequency range, which makes it possible to achieve deep penetration and high resolution, as well as enhanced performance in harmonic imaging.

With sufficient bandwidth, one transducer can cover the range of acoustic frequencies that previously required separate transducers. XDclear transducers with Single Crystal materials have measurably enhanced bandwidth, achieving a -6 dB fractional bandwidth that can exceed 100 percent compared with 70 to 80 percent for traditional GE transducers. The result is a new level of penetration, resolution, and sensitivity in GE transducer performance.

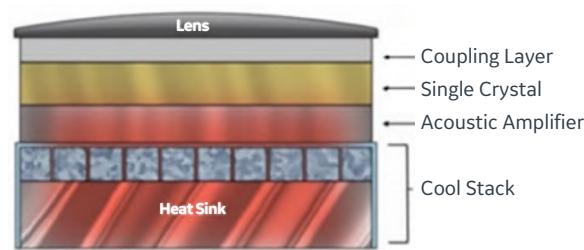


Figure 13. *Cool Stack*: Optimizes energy usage via patented technology integrated into the transducer’s internal architecture; it relieves inherent heat generation that can otherwise reduce sensitivity and penetration.

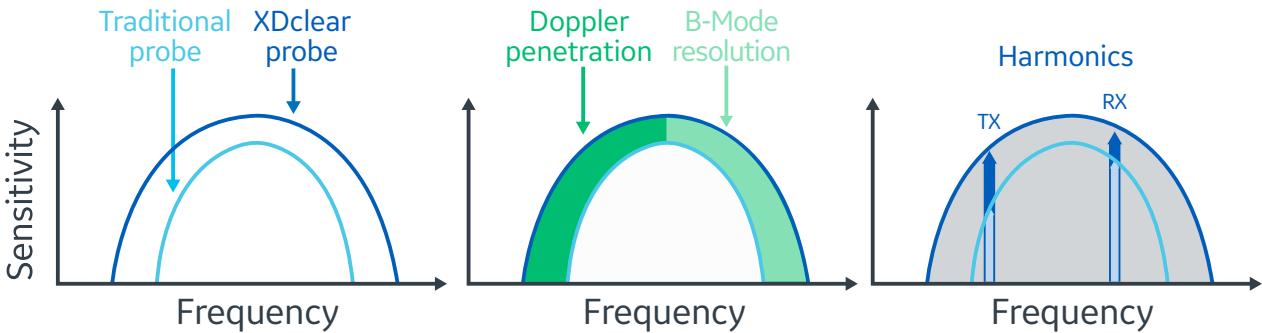


Figure 14. XDclear probe performance benefits are derived from improved sensitivity and wider bandwidth.

## cSound Architecture Summary

The cSound Architecture leverages next-generation data rates and processing power that were previously unavailable, allowing significantly more data to be collected and used to create every image. This additional data is used to achieve focus at every point and to increase contrast and spatial resolution—all while significantly improving frame rates. Combined with the performance advantages of XDclear probes and the Advanced Raw Data Post Processor, these advancements make the cSound Architecture an excellent imaging system for today and its flexible design makes it a powerful imaging platform for tomorrow.





\*As compared to the LOGIQ™ E9.

© GE, 2022

GE Healthcare reserves the right to make changes in specifications and features shown herein, or discontinue the product described at any time without notice or obligation. Contact your GE Healthcare representative for the most current information. GE, the GE Monogram, cSound, LOGIQ, and XDclear trademarks of GE. GE Healthcare, a division of GE. NVIDIA is a registered trademark of NVIDIA Corporation. GE Medical Systems, Inc., doing business as GE Healthcare.

March 2022  
JB19417XX





# Certificate of Approval

This is to certify that the Management System of:

## GE HEALTHCARE EUROPE SALES AND SERVICES

283 rue de la Minière, 78530 BUC, France

has been approved by Lloyd's Register to the following standards:

### ISO 14001:2015

Approval number(s): ISO 14001 – 0043295

This certificate is valid only in association with the certificate schedule bearing the same number on which the locations applicable to this approval are listed.

#### The scope of this approval is applicable to:

Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices.



**Daniel Oliva Marcilio de Souza**

Area Operations Manager - South Europe

Issued by: LRQA France SAS

for and on behalf of: Lloyd's Register Quality Assurance Limited



001



# Certificate Schedule

Location	Activities
<b>GE Medical Systems SCS</b> 283 rue de la Minière, 78530 BUC, France	<b>ISO 14001:2015</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices.
<b>GEMS SCS</b> 24 avenue de l'Europe, 78140 VELIZY VILLACOUBLAY, France	<b>ISO 14001:2015</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>GE Healthcare Austria GmbH &amp; Co OG</b> Technologiestr. 10, 1220 WIEN, Austria	<b>ISO 14001:2015</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>GE Healthcare BVBA</b> Kouterveldstraat 20, Eagle Building, 1831 DIEGEM, Belgium	<b>ISO 14001:2015</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>GE Healthcare Bulgaria LTD</b> Dragan Tzankov Blvd. 36, World Trade Centre, 1040 SOFIA, Bulgaria	<b>ISO 14001:2015</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>GE Medical Systems Česká republika, s.r.o.</b> Bucharova 2641/14, Explora Business Centre, Jupiter Building, 158 00 PRAHA 5, Czech Republic	<b>ISO 14001:2015</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.



001



# Certificate Schedule

Location	Activities
<b>GE Healthcare Danmark A/S</b> Park Allé 295, 2605 BRONDBY, Denmark	<b>ISO 14001:2015</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>GE Healthcare Finland Oy</b> Kuortaneenkatu 2, 00510 HELSINKI 18, Finland	<b>ISO 14001:2015</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>GE Medical Systems Information Technologies GmbH</b> Munzingerstr. 3a-5, 79111 FREIBURG, Germany	<b>ISO 14001:2015</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices.
<b>GE Healthcare GmbH</b> Beethovenstr. 239, 42655 SOLINGEN, Germany	<b>ISO 14001:2015</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>GE Healthcare S.A.</b> 8-10 Sorou, Maroussi, 151 25 ATHENS, Greece	<b>ISO 14001:2015</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>GE Healthcare Magyarország Kft.</b> Bence utca 3., 1138 BUDAPEST, Hungary	<b>ISO 14001:2015</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.



001



# Certificate Schedule

Location	Activities
<b>GE Medical Systems Ireland Ltd</b> Unit F5, Centre Point Business Park, Oak Drive DUBLIN 12, Ireland	<b>ISO 14001:2015</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>GE Medical Systems Italia SpA</b> Via Galeno 36, 20126 MILAN, Italy	<b>ISO 14001:2015</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>General Electric Kazakhstan LLP</b> 308 of. "Grand-Alatau" Business Center, "Grand-Alatau" Business Center, Almaty, 050040, Kazakhstan	<b>ISO 14001:2015</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>GE Medical Systems Nederland BV</b> De Wel 18, Building C, 3871 MV HOEVELAKEN, The Netherlands	<b>ISO 14001:2015</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>GE Healthcare Norge AS</b> Vitaminveien 1A, 0485 OSLO, Norway	<b>ISO 14001:2015</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>GE Medical Systems Polska Sp.z o.o.</b> ul. Woloska 9, 02-583 WARSAW, Poland	<b>ISO 14001:2015</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.



001



# Certificate Schedule

Location	Activities
<b>General Electric Healthcare Portugal, Sociedade Unipessoal, Lda.</b> Avenida do Forte 6 6-A, Ed. Ramazzotti, 2790-072 CARNAXIDE, Portugal	<b>ISO 14001:2015</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>GE Medical Systems SRL.</b> 301-311 Barbu Vacarescu St., District 2, Lakeview Building, 3rd floor, 020276 BUCHAREST, Romania	<b>ISO 14001:2015</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>GE Healthcare LLC</b> 10 Presnenskaya embankment, premise III, 12 floor, room 1, MOSCOW, 123112, Russian Federation	<b>ISO 14001:2015</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>GE Holdings d.o.o.</b> Bulevar Mihaila Pupina 6/17 PC,, Usce, Novi Beograd, BELGRADE, 11070, Republic of Serbia	<b>ISO 14001:2015</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>General Electric International (Slovensko), s.r.o.</b> Prievozská 4, 821 09 BRATISLAVA, Slovakia	<b>ISO 14001:2015</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>General Electric Healthcare España, S.A.U</b> Calle Gobelás 35-37, Urbanización La Florida, 28023 MADRID, Spain	<b>ISO 14001:2015</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.



001



# Certificate Schedule

Location	Activities
<b>GE Healthcare Sverige AB</b> Vendevägen 89, 182 32 DANDERYD, Sweden	<b>ISO 14001:2015</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>GE Medical Systems Schweiz AG</b> Europastrasse 31, 8152 GLATTBRUGG, Switzerland	<b>ISO 14001:2015</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>GE Healthcare</b> Pollards Wood, Nightingales Lane, Chalfont St Giles, HP8 4SP, Buckinghamshire, United Kingdom	<b>ISO 14001:2015</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.



001



# Certificate of Approval

This is to certify that the Management System of:

## GE HEALTHCARE EUROPE SALES AND SERVICES

283 rue de la Minière, 78530 BUC, France

has been approved by Lloyd's Register to the following standards:

### ISO 45001:2018

Approval number(s): ISO 45001 – 00027009

This certificate is valid only in association with the certificate schedule bearing the same number on which the locations applicable to this approval are listed.

#### The scope of this approval is applicable to:

Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.



**Daniel Oliva Marcilio de Souza**

Area Operations Manager - South Europe

Issued by: LRQA France SAS

for and on behalf of: Lloyd's Register Quality Assurance Limited



001



# Certificate Schedule

Location	Activities
<b>GE Medical Systems SCS</b> 283 rue de la Minière, 78530 BUC, France	<b>ISO 45001:2018</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>GEMS SCS</b> 24 avenue de l'Europe, 78140 VELIZY VILLACOUBLAY, France	<b>ISO 45001:2018</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>GE Healthcare BVBA</b> Kouterveldstraat 20, Eagle Building, 1831 DIEGEM, Belgium	<b>ISO 45001:2018</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>GE Healthcare Bulgaria LTD</b> Dragan Tzankov Blvd. 36, World Trade Centre, 1040 SOFIA, Bulgaria	<b>ISO 45001:2018</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>GE Medical Systems Česká republika, s.r.o.</b> Bucharova 2641/14, Explora Business Centre, Jupiter Building, 158 00 PRAHA 5, Czech Republic	<b>ISO 45001:2018</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>GE Healthcare Finland Oy</b> Kuortaneenkatu 2, 00510 HELSINKI 18, Finland	<b>ISO 45001:2018</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.



001



# Certificate Schedule

Location	Activities
<b>GE Medical Systems Information Technologies GmbH</b> Munzingerstr. 3a-5, 79111 FREIBURG, Germany	<b>ISO 45001:2018</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>GE Healthcare GmbH</b> Beethovenstr. 239, 42655 SOLINGEN, Germany	<b>ISO 45001:2018</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>GE Healthcare S.A.</b> 8-10 Sorou, Maroussi, 151 25 ATHENS, Greece	<b>ISO 45001:2018</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>GE Healthcare Magyarország Kft.</b> Bence utca 3., 1138 BUDAPEST, Hungary	<b>ISO 45001:2018</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>GE Medical Systems Ireland Ltd</b> Unit F5, Centre Point Business Park, Oak Drive DUBLIN 12, Ireland	<b>ISO 45001:2018</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>GE Medical Systems Italia SpA</b> Via Galeno 36, 20126 MILAN, Italy	<b>ISO 45001:2018</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.



001



# Certificate Schedule

Location	Activities
<b>GE Medical Systems Polska Sp.z o.o.</b> ul. Woloska 9, 02-583 WARSAW, Poland	<b>ISO 45001:2018</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management. repair and installation of medical devices
<b>General Electric Healthcare Portugal, Sociedade Unipessoal, Lda.</b> Avenida do Forte 6 6-A, Ed. Ramazzotti, 2790-072 CARNAXIDE, Portugal	<b>ISO 45001:2018</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>GE Medical Systems SRL.</b> 301-311 Barbu Vacarescu St., District 2, Lakeview Building, 3rd floor, 020276 BUCHAREST, Romania	<b>ISO 45001:2018</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>GE Healthcare LLC</b> 10 Presnenskaya embankment, premise III, 12 floor, room 1, MOSCOW, 123112, Russian Federation	<b>ISO 45001:2018</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>GE Holdings d.o.o.</b> Bulevar Mihaila Pupina 6/17 PC., Usce, Novi Beograd, BELGRADE, 11070, Republic of Serbia	<b>ISO 45001:2018</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management. associated with sales, marketing, services, repair and installation of medical devices



001



# Certificate Schedule

Location	Activities
<b>General Electric International (Slovensko), s.r.o.</b> Prievozská 4, 821 09 BRATISLAVA, Slovakia	<b>ISO 45001:2018</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>General Electric Healthcare España, S.A.U</b> Calle Gobelas 35-37, Urbanizacion La Florida, 28023 MADRID, Spain	<b>ISO 45001:2018</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>GE Healthcare Sverige AB</b> Vendevägen 89, 182 32 DANDERYD, Sweden	<b>ISO 45001:2018</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>GE Medical Systems Schweiz AG</b> Europastrasse 31, 8152 GLATTBRUGG, Switzerland	<b>ISO 45001:2018</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>GE Healthcare</b> Pollards Wood, Nightingales Lane, Chalfont St Giles, HP8 4SP, Buckinghamshire, United Kingdom	<b>ISO 45001:2018</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>GE Medical Systems Nederland BV</b> De Wel 18, Building C, 3871 MV HOEVELAKEN, The Netherlands	<b>ISO 45001:2018</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.



001



# Certificate Schedule

Location	Activities
<b>GE Healthcare Austria GmbH &amp; Co OG</b> Technologiestr. 10, 1220 WIEN, Austria	<b>ISO 45001:2018</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>General Electric Kazakhstan LLP</b> 308 of. "Grand-Alatau" Business Center, "Grand-Alatau" Business Center, Almaty, 050040, Kazakhstan	<b>ISO 45001:2018</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.



001



# Certificate of Approval

This is to certify that the Management System of:

## GE HEALTHCARE EUROPE SALES AND SERVICES

283 rue de la Minière, 78530 BUC, France

has been approved by Lloyd's Register to the following standards:

### ISO 50001:2018

Approval number(s): ISO 50001 – 0043293

This certificate is valid only in association with the certificate schedule bearing the same number on which the locations applicable to this approval are listed.

#### The scope of this approval is applicable to:

Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.



**Daniel Oliva Marcilio de Souza**

Area Operations Manager - South Europe

Issued by: LRQA France SAS

for and on behalf of: Lloyd's Register Quality Assurance Limited



001



# Certificate Schedule

Location	Activities
<b>GE Medical Systems SCS</b> 283 rue de la Minière, 78530 BUC, France	<b>ISO 50001:2018</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices.
<b>GEMS SCS</b> 24 avenue de l'Europe, 78140 VELIZY VILLACOUBLAY, France	<b>ISO 50001:2018</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>GE Healthcare BVBA</b> Kouterveldstraat 20, Eagle Building, 1831 DIEGEM, Belgium	<b>ISO 50001:2018</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>GE Healthcare Finland Oy</b> Kuortaneenkatu 2, 00510 HELSINKI 18, Finland	<b>ISO 50001:2018</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>GE Medical Systems Information Technologies GmbH</b> Munzingerstr. 3a-5, 79111 FREIBURG, Germany	<b>ISO 50001:2018</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices.
<b>GE Healthcare GmbH</b> Beethovenstr. 239, 42655 SOLINGEN, Germany	<b>ISO 50001:2018</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.



001



# Certificate Schedule

Location	Activities
<b>GE Medical Systems Ireland Ltd</b> Unit F5, Centre Point Business Park, Oak Drive DUBLIN 12, Ireland	<b>ISO 50001:2018</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>GE Medical Systems Italia SpA</b> Via Galeno 36, 20126 MILAN, Italy	<b>ISO 50001:2018</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>General Electric Healthcare Portugal, Sociedade Unipessoal, Lda.</b> Avenida do Forte 6 6-A, Ed. Ramazzotti, 2790-072 CARNAXIDE, Portugal	<b>ISO 50001:2018</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>GE Healthcare LLC</b> 10 Presnenskaya embankment, premise III, 12 floor, room 1, MOSCOW, 123112, Russian Federation	<b>ISO 50001:2018</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>General Electric Healthcare España, S.A.U</b> Calle Gobelas 35-37, Urbanizacion La Florida, 28023 MADRID, Spain	<b>ISO 50001:2018</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>GE Healthcare Sverige AB</b> Vendevägen 89, 182 32 DANDERYD, Sweden	<b>ISO 50001:2018</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.



001



# Certificate Schedule

Location	Activities
<b>GE Medical Systems Schweiz AG</b> Europastrasse 31, 8152 GLATTBRUGG, Switzerland	<b>ISO 50001:2018</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>GE Healthcare</b> Pollards Wood, Nightingales Lane, Chalfont St Giles, HP8 4SP, Buckinghamshire, United Kingdom	<b>ISO 50001:2018</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>GE Medical Systems Nederland BV</b> De Wel 18, Building C, 3871 MV HOEVELAKEN, The Netherlands	<b>ISO 50001:2018</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>General Electric Kazakhstan LLP</b> 308 of. "Grand-Alatau" Business Center, "Grand-Alatau" Business Center, Almaty, 050040, Kazakhstan	<b>ISO 50001:2018</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.
<b>GE Healthcare Austria GmbH &amp; Co OG</b> Technologiestr. 10, 1220 WIEN, Austria	<b>ISO 50001:2018</b> Sales, delivery, installation, repairing, servicing, commissioning, and decommissioning of GE Healthcare medical devices and multivendor medical devices. Excluding office facility management.



001





OVERVIEW

MULTI-PURPOSE/  
RADIOLOGY

CARDIOLOGY

MUSCULOSKELETAL

BREAST

PRODUCTIVITY

INVESTMENT

CONTACT



# LOGIQ Fortis™

Powerful | Streamlined | Multi-purpose  
*Always ready. Always by your side.*

[gehealthcare.com](https://www.gehealthcare.com)





[OVERVIEW](#)[MULTI-PURPOSE/  
RADIOLOGY](#)[CARDIOLOGY](#)[MUSCULOSKELETAL](#)[BREAST](#)[PRODUCTIVITY](#)[INVESTMENT](#)[CONTACT](#)

## Powerfully streamlined

### New GE LOGIQ Fortis

LOGIQ Fortis is the affordable, all-in-one solution for your ultrasound imaging needs. Powerfully streamlined and equipped with the most advanced technology, it helps users deliver on the promise of confident care in multiple clinical settings.

- **Exceeding your expectations** ... with next-generation imaging technologies for a wide range of patients and clinical applications—head to toe, obese to thin, neonate to geriatric
- **Optimizing your productivity** ... with user-friendly apps and AI-based productivity tools, and the ability to scan on battery
- **Maximizing your investment** ... with a future-focused digital platform, robust cybersecurity protection, and value-added lifecycle solutions

**LOGIQ Fortis.**  
Your trusted companion for every body.

**LOGIQ Fortis**



[OVERVIEW](#)[MULTI-PURPOSE/  
RADIOLOGY](#)[CARDIOLOGY](#)[MUSCULOSKELETAL](#)[BREAST](#)[PRODUCTIVITY](#)[INVESTMENT](#)[CONTACT](#)

# MULTI-PURPOSE/ RADIOLOGY

The high-performing LOGIQ Fortis enables a full spectrum of ultrasound exams and procedures on any body type.

- Exceptional image quality with cSound™ Architecture—now including advanced Speckle Reduction Imaging (SRI)
- Whole body imaging with versatile XDclear™ probes
- Advanced quantification and productivity tools, including 2D Shear Wave Elastography, Ultrasound-Guided Attenuation Parameter (UGAP), CEUS, and Volume Navigation

[+ CLINICAL IMAGES](#)[LOGIQ Fortis Overview](#)

**LOGIQ Fortis**





OVERVIEW

MULTI-PURPOSE/  
RADIOLOGY

CARDIOLOGY

MUSCULOSKELETAL

BREAST


PRODUCTIVITY

INVESTMENT

CONTACT

# CLINICAL IMAGES | Head & Neck

Exceeding your expectations: whole body imaging

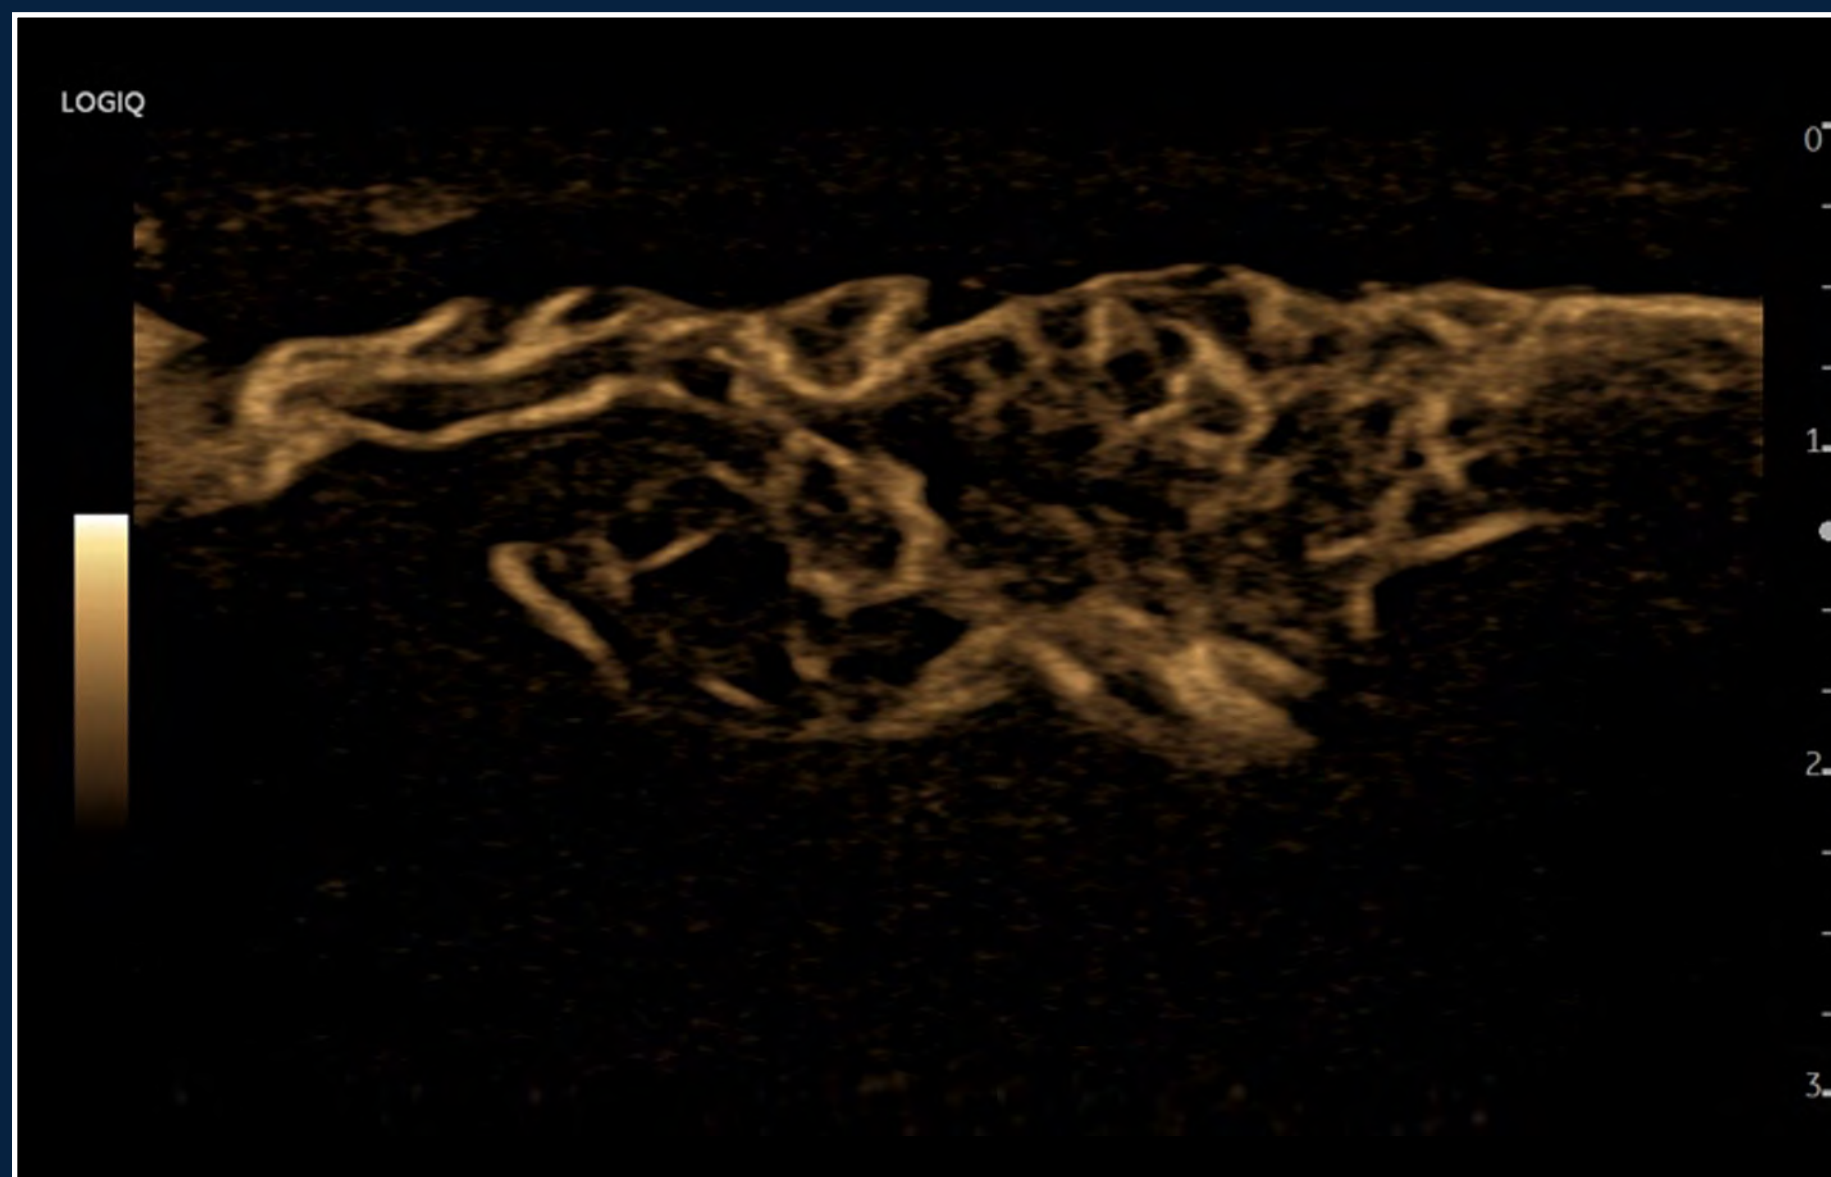

Flow Visualization, B-Flow in Thyroid, ML6-15-D







OVERVIEW

MULTI-PURPOSE/  
RADIOLOGY

CARDIOLOGY

MUSCULOSKELETAL

BREAST


PRODUCTIVITY

INVESTMENT

CONTACT

# CLINICAL IMAGES | Head & Neck

Exceeding your expectations: whole body imaging

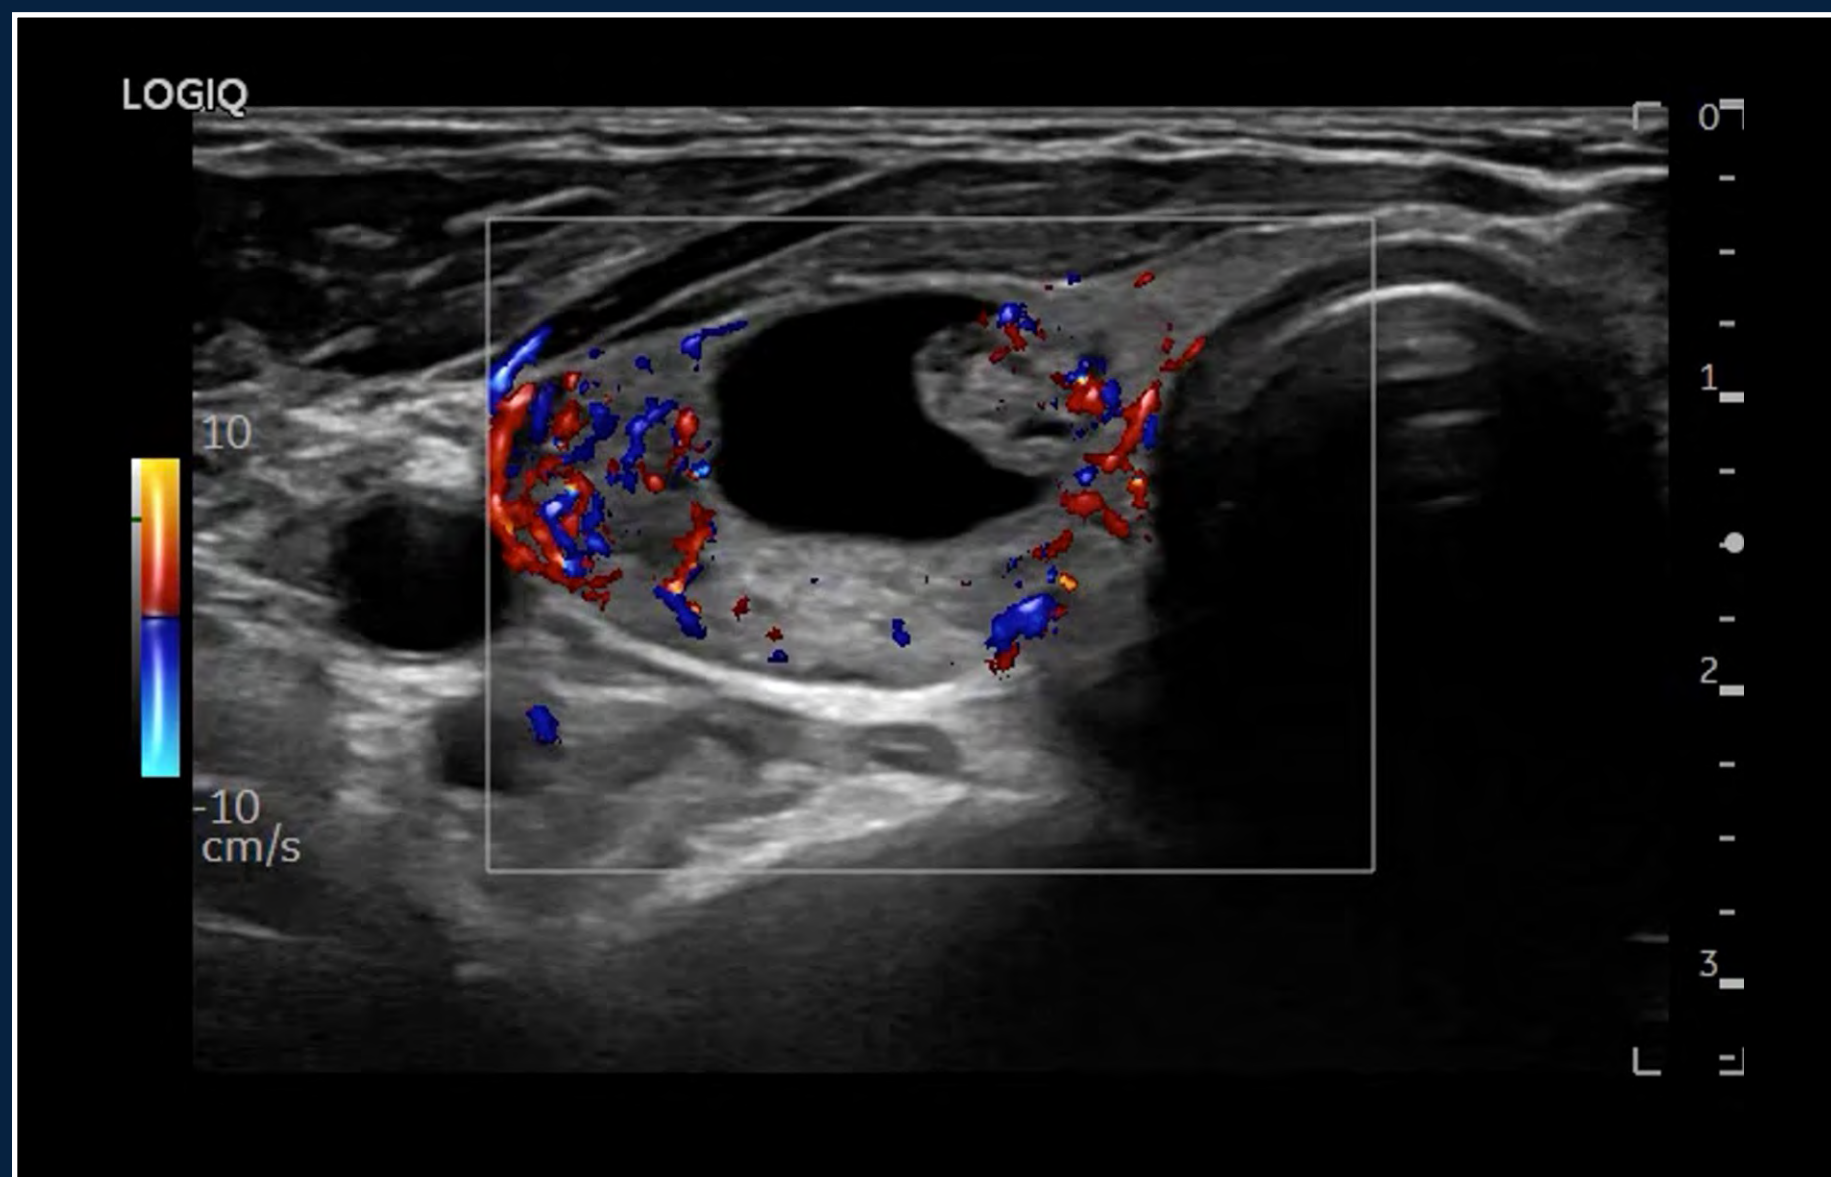

Radiantflow™ Color Flow in Thyroid, ML6-15-D







OVERVIEW

MULTI-PURPOSE/  
RADIOLOGY

CARDIOLOGY

MUSCULOSKELETAL

BREAST


PRODUCTIVITY

INVESTMENT

CONTACT

# CLINICAL IMAGES | Head & Neck

Exceeding your expectations: whole body imaging

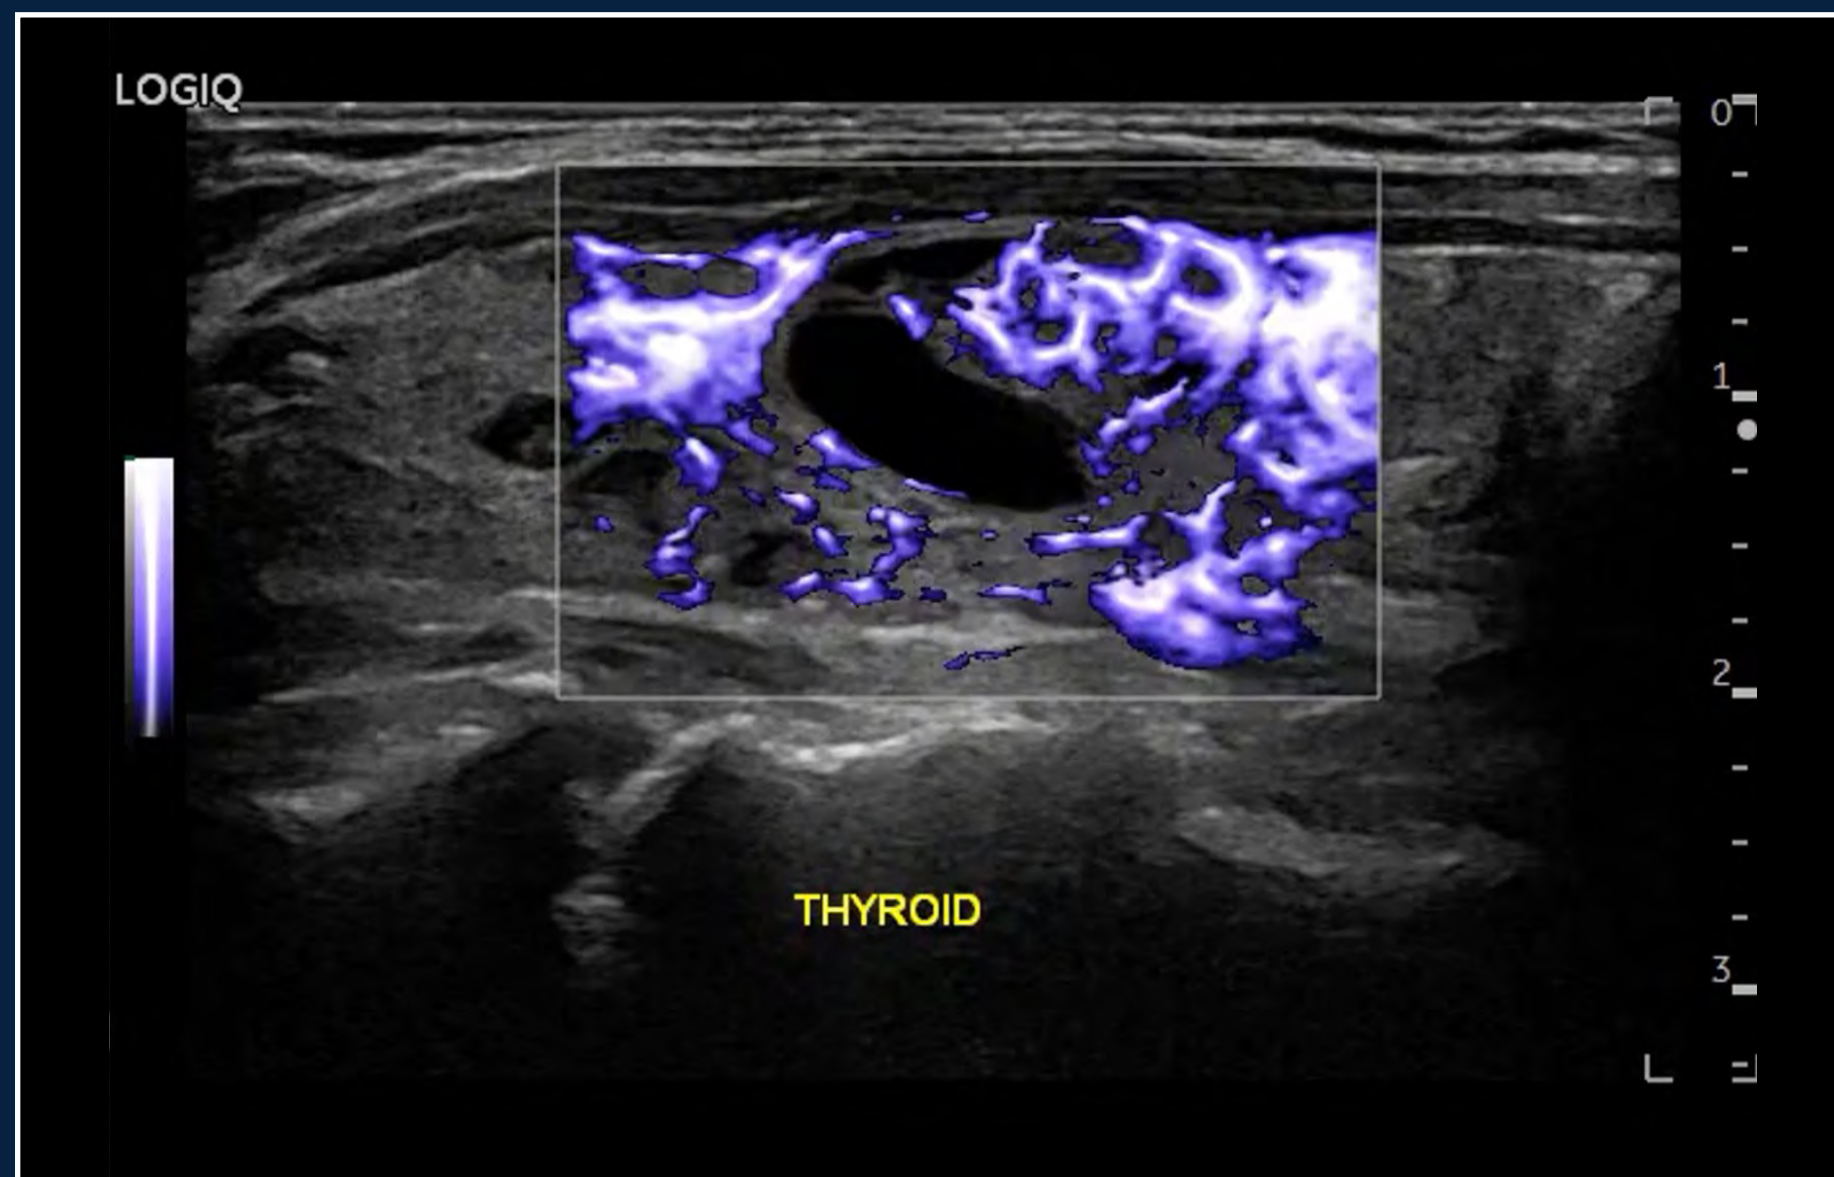

MVI with Radiantflow in Thyroid, ML6-15-D







OVERVIEW

MULTI-PURPOSE/  
RADIOLOGY

CARDIOLOGY

MUSCULOSKELETAL

BREAST


PRODUCTIVITY

INVESTMENT

CONTACT

# CLINICAL IMAGES | OB/GYN

Exceeding your expectations: whole body imaging

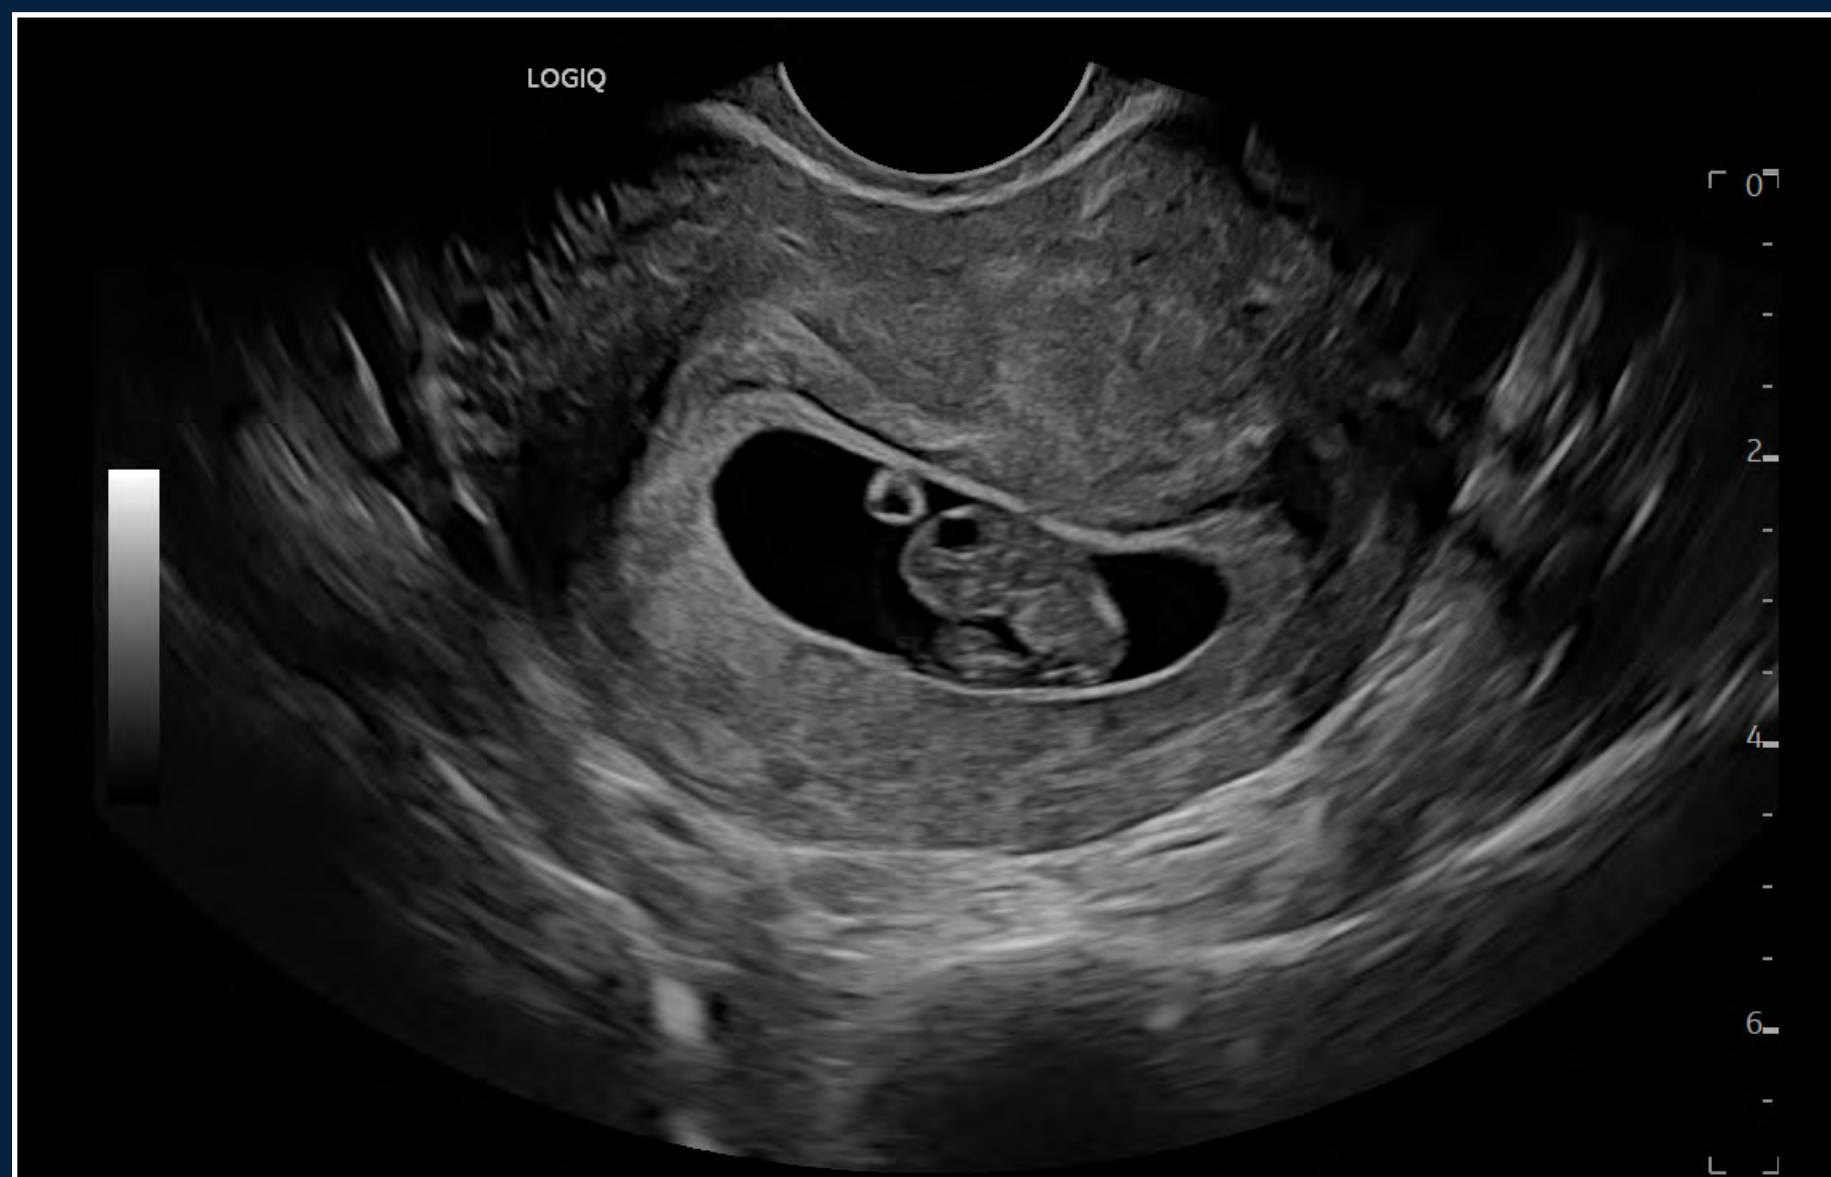

B-Mode with Advanced SRI Early Fetus and Yolk Sac, IC5-9-D







OVERVIEW

MULTI-PURPOSE/  
RADIOLOGY

CARDIOLOGY

MUSCULOSKELETAL

BREAST

PRODUCTIVITY

INVESTMENT

CONTACT

# CLINICAL IMAGES | OB/GYN

Exceeding your expectations: whole body imaging



PDI with Radiantflow in Umbilical Cord, C1-6-D







OVERVIEW

MULTI-PURPOSE/  
RADIOLOGY

CARDIOLOGY

MUSCULOSKELETAL

BREAST


PRODUCTIVITY

INVESTMENT

CONTACT

# CLINICAL IMAGES | OB/GYN

Exceeding your expectations: whole body imaging

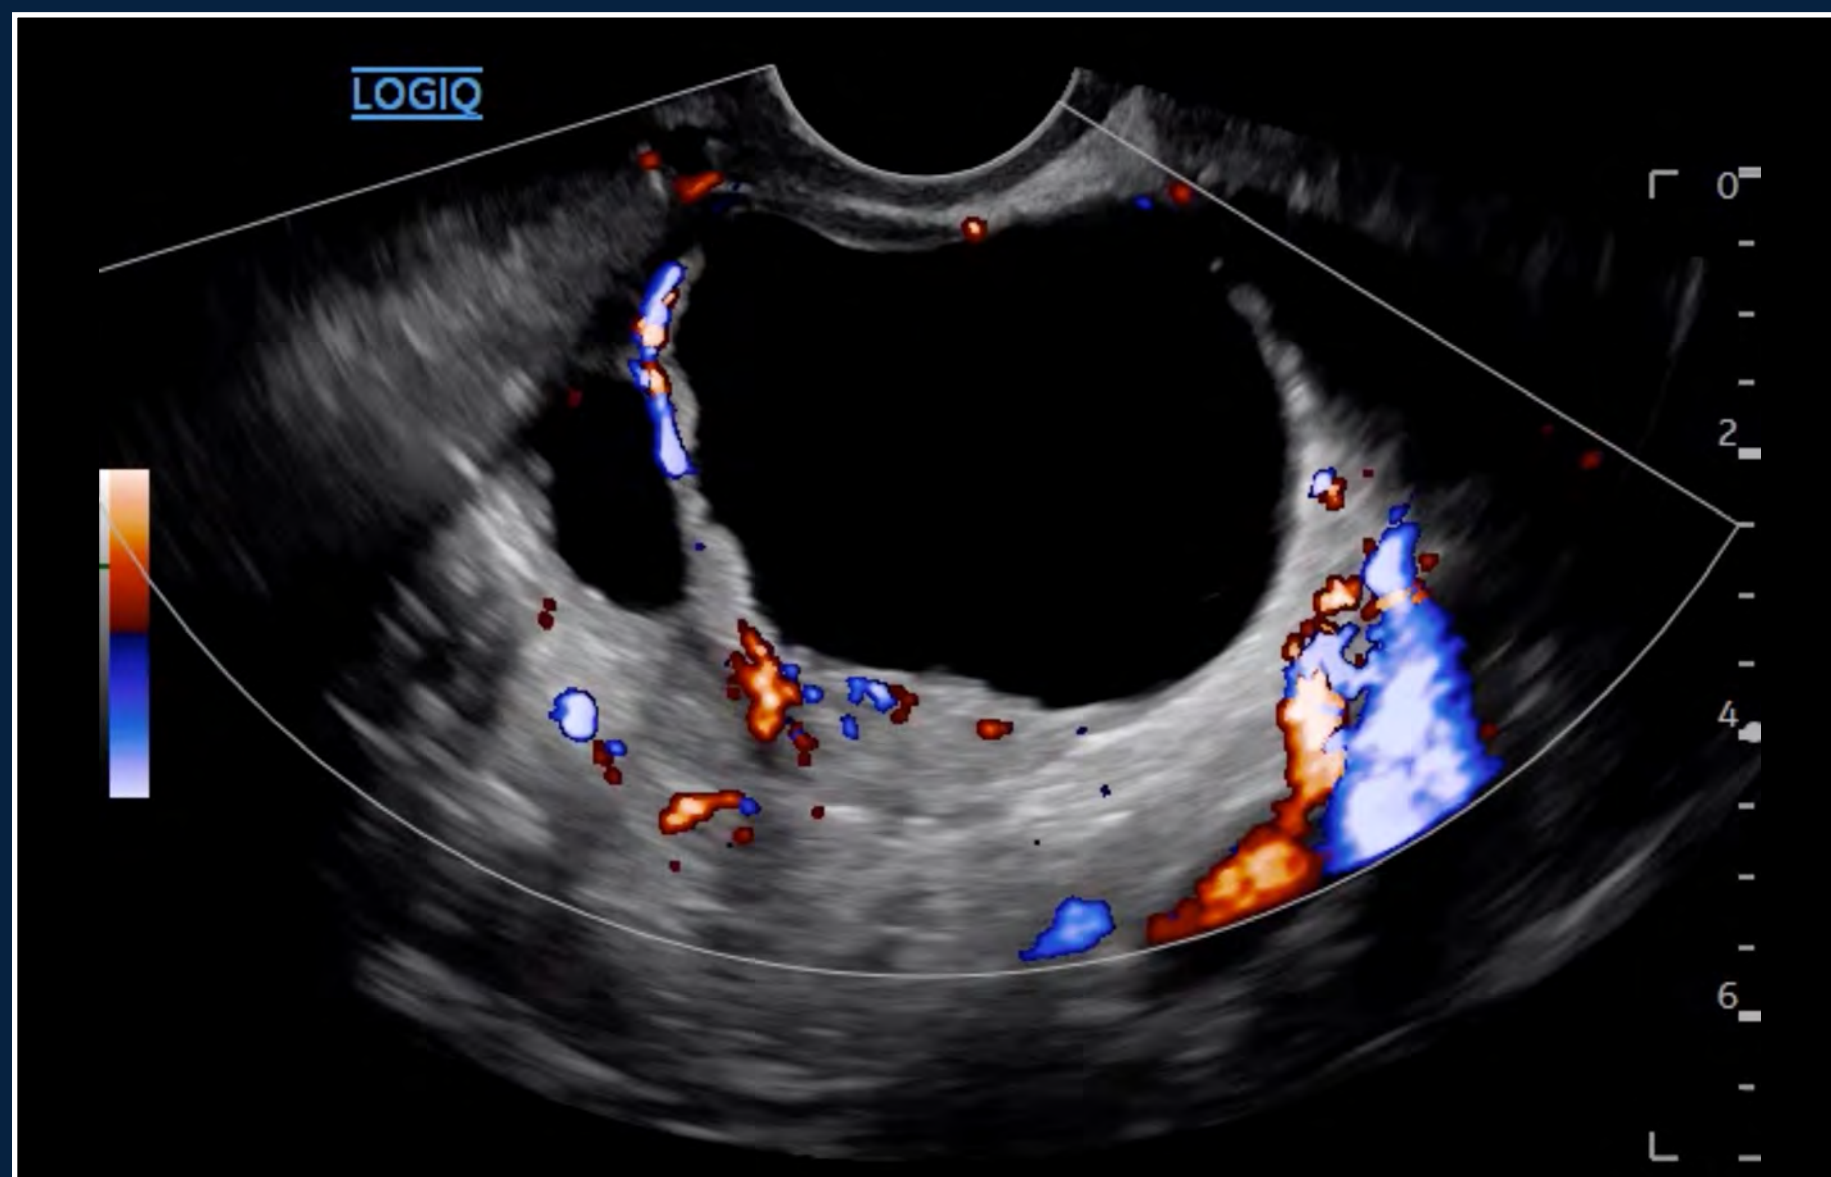

PDI of Ovary, IC5-9-D







OVERVIEW

MULTI-PURPOSE/  
RADIOLOGY

CARDIOLOGY

MUSCULOSKELETAL

BREAST


PRODUCTIVITY

INVESTMENT

CONTACT

# CLINICAL IMAGES | Vascular

Exceeding your expectations: whole body imaging

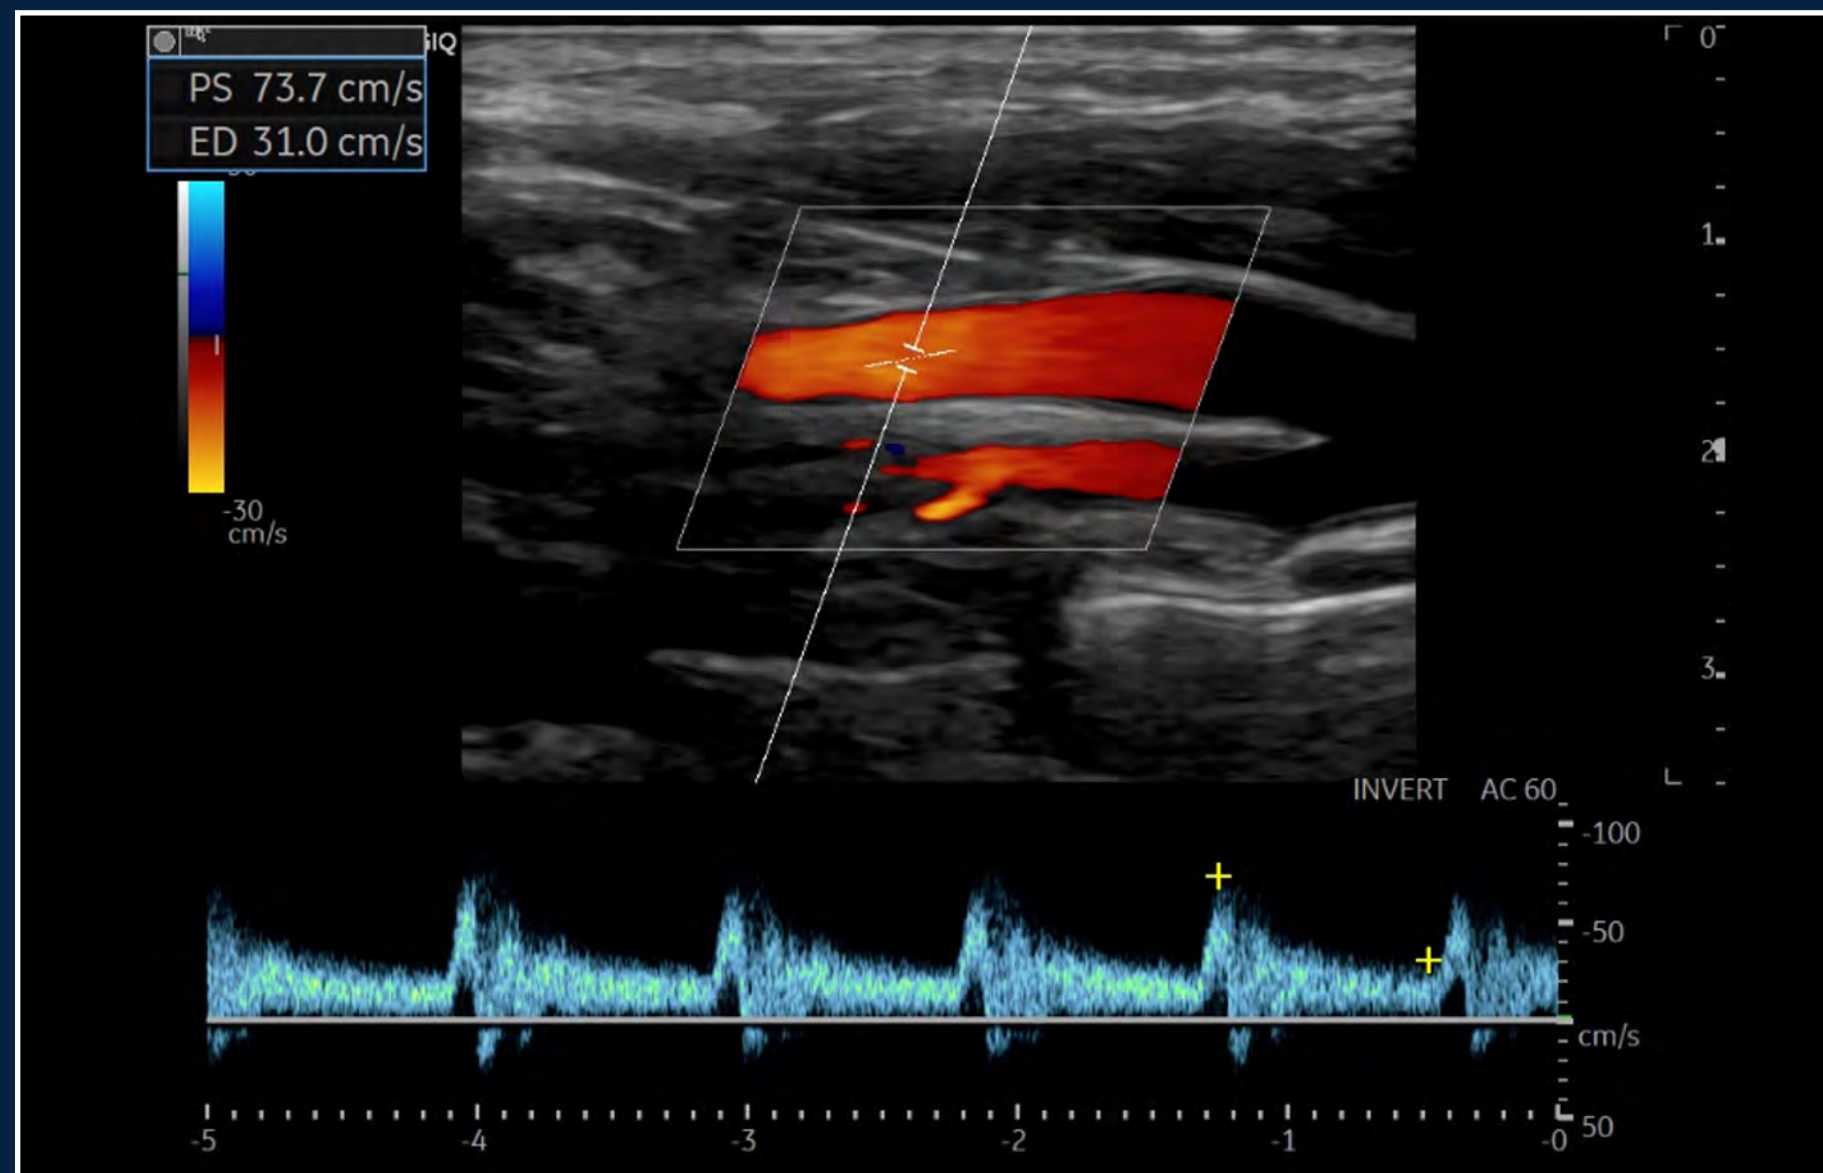

Color Flow and PW Doppler in Internal Carotid Artery, L2-9-D







OVERVIEW

MULTI-PURPOSE/  
RADIOLOGY

CARDIOLOGY

MUSCULOSKELETAL

BREAST


PRODUCTIVITY

INVESTMENT

CONTACT

# CLINICAL IMAGES | Vascular

Exceeding your expectations: whole body imaging

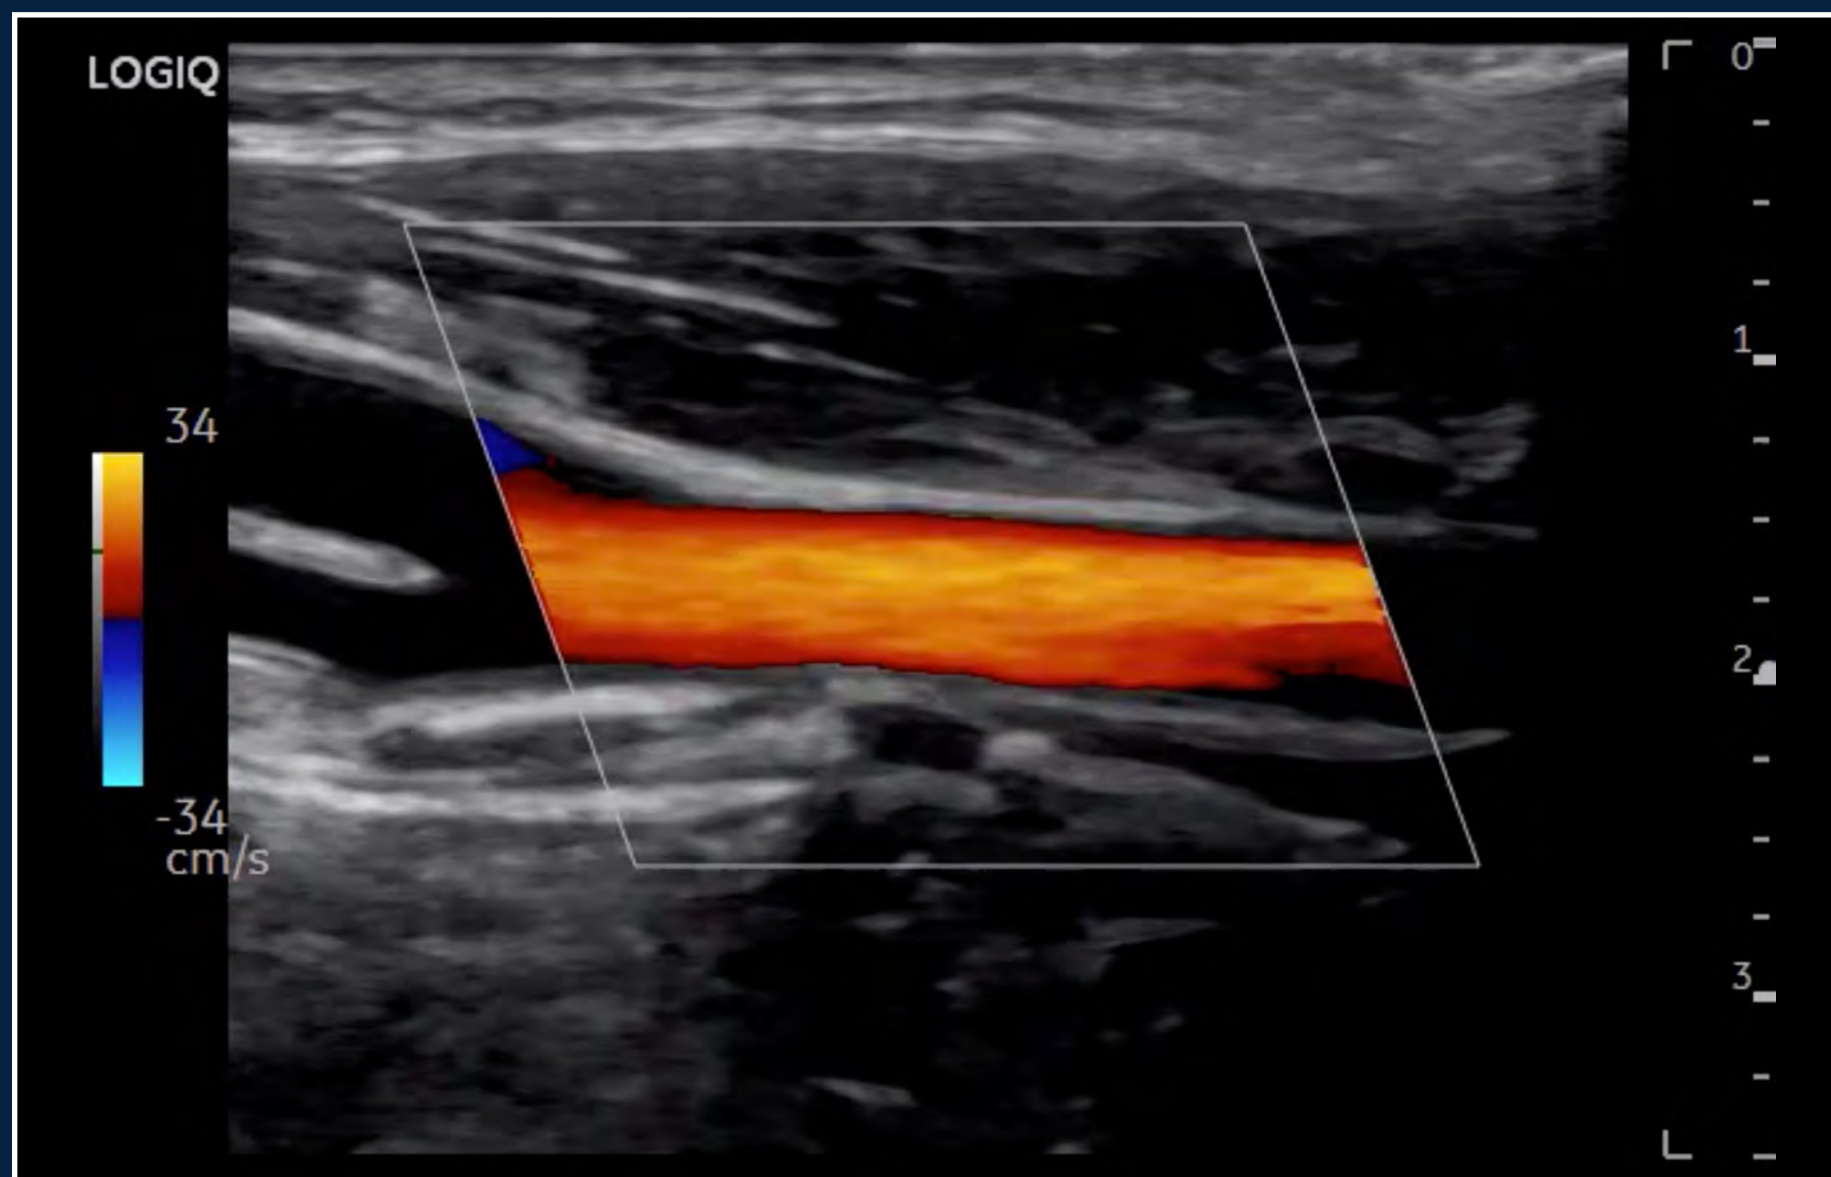

Color Flow Carotid, L2-9-D







OVERVIEW

MULTI-PURPOSE/  
RADIOLOGY

CARDIOLOGY

MUSCULOSKELETAL

BREAST


PRODUCTIVITY

INVESTMENT

CONTACT

# CLINICAL IMAGES | Vascular

Exceeding your expectations: whole body imaging

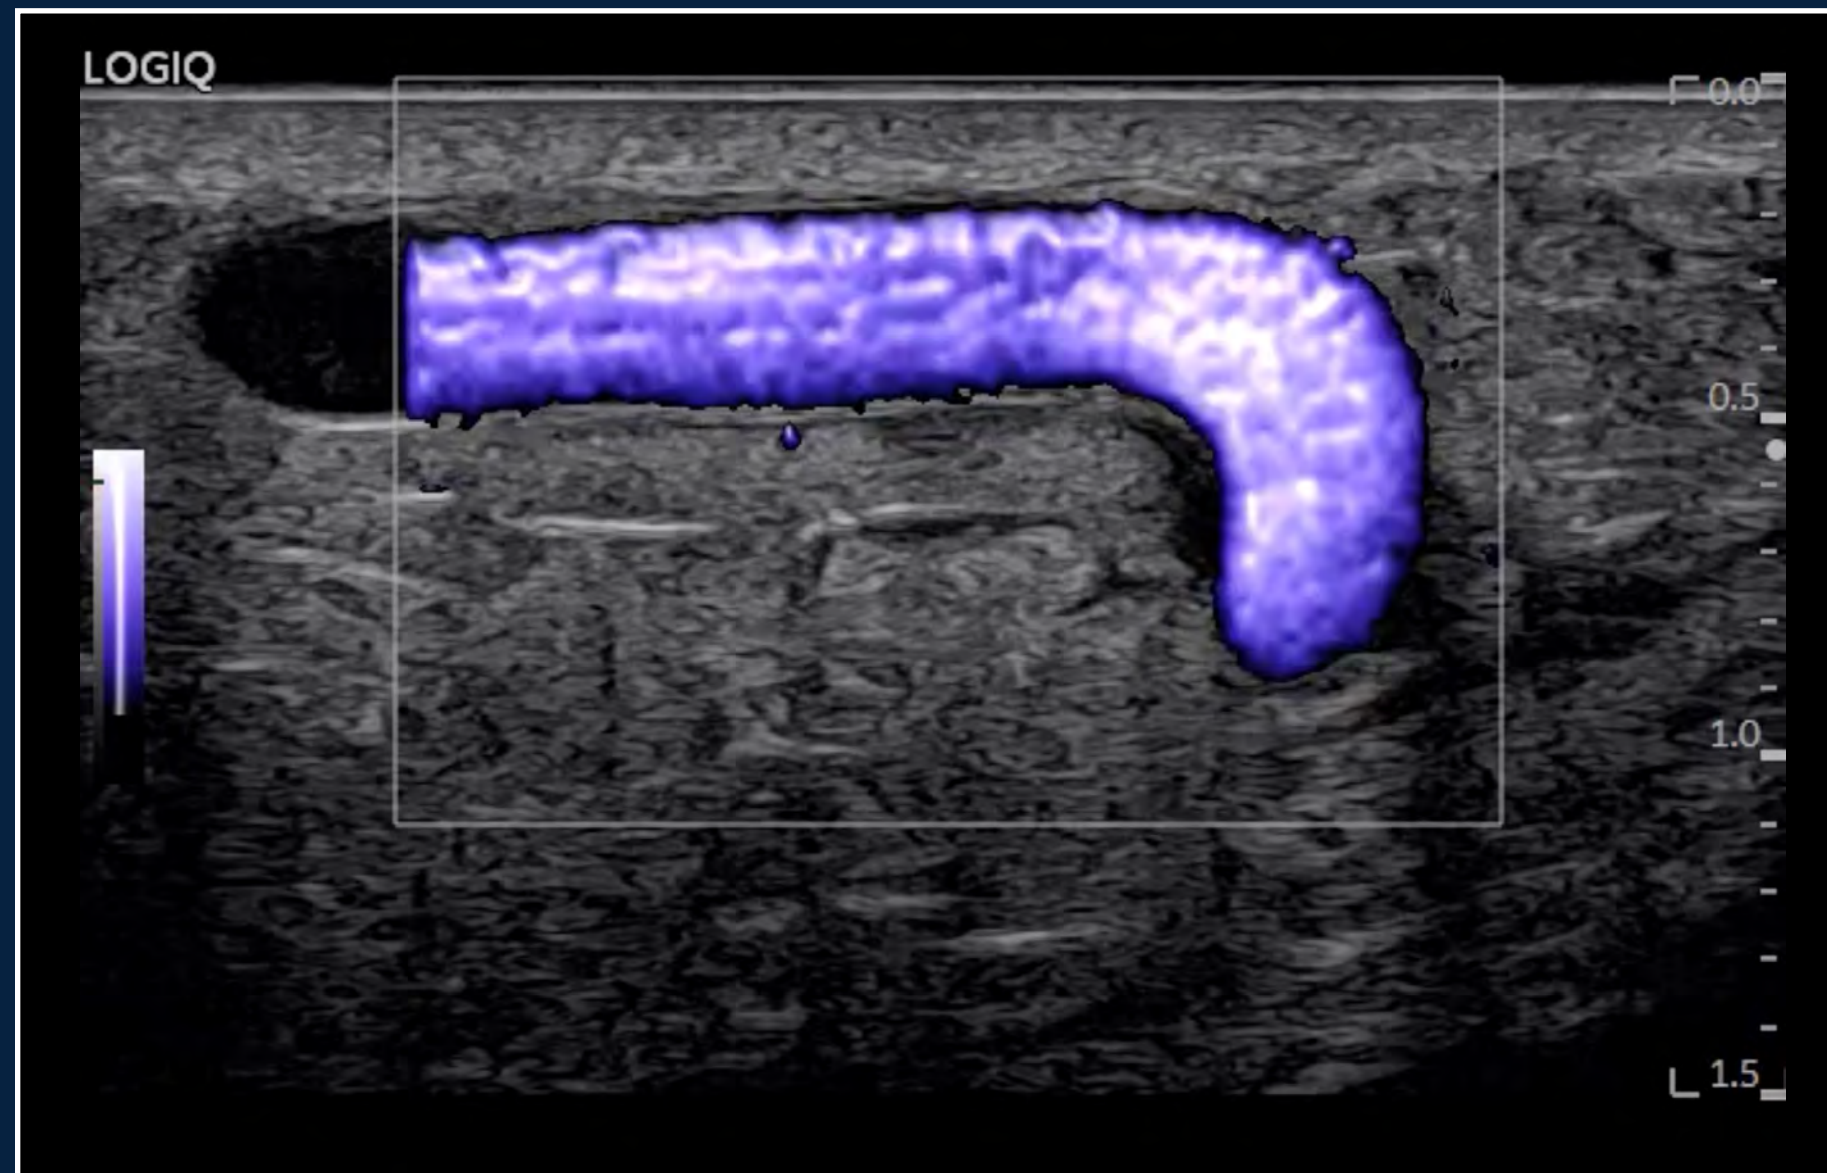

MVI Superficial Vein, L6-24-D







OVERVIEW

MULTI-PURPOSE/  
RADIOLOGY

CARDIOLOGY

MUSCULOSKELETAL

BREAST

PRODUCTIVITY

INVESTMENT

CONTACT

# CLINICAL IMAGES | Liver

Exceeding your expectations: whole body imaging



B-Mode with Advanced SRI Liver with TIPS, C1-6-D







OVERVIEW

MULTI-PURPOSE/  
RADIOLOGY

CARDIOLOGY

MUSCULOSKELETAL

BREAST

PRODUCTIVITY

INVESTMENT

CONTACT

# CLINICAL IMAGES | Liver

Exceeding your expectations: whole body imaging



Liver B-Flow Cine Capture, C2-9-D







OVERVIEW

MULTI-PURPOSE/  
RADIOLOGY

CARDIOLOGY

MUSCULOSKELETAL

BREAST


PRODUCTIVITY

INVESTMENT

CONTACT

# CLINICAL IMAGES | Liver

Exceeding your expectations: whole body imaging

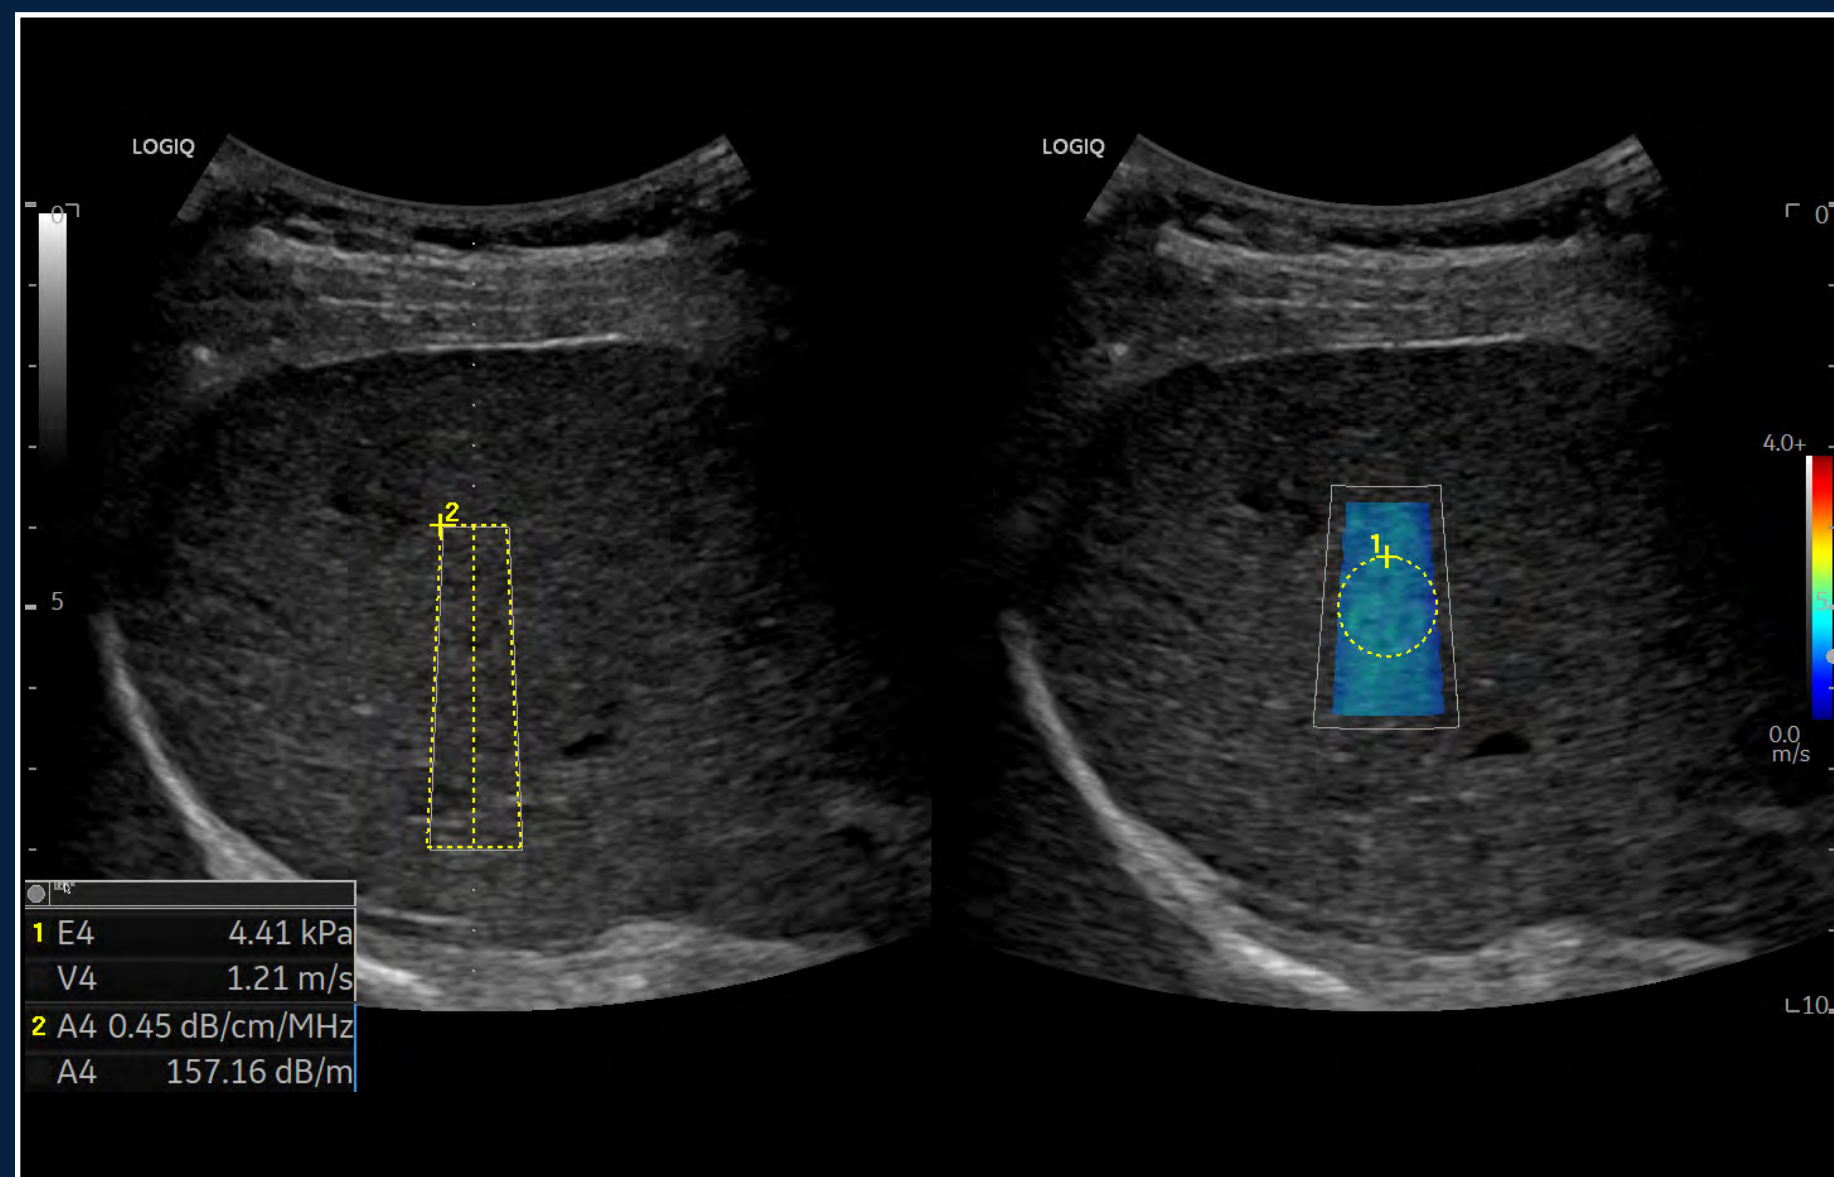

Hepatic Assistant UGAP and Shear Wave, C1-6-D







OVERVIEW

MULTI-PURPOSE/  
RADIOLOGY

CARDIOLOGY

MUSCULOSKELETAL

BREAST


PRODUCTIVITY

INVESTMENT

CONTACT

# CLINICAL IMAGES | Liver

Exceeding your expectations: whole body imaging

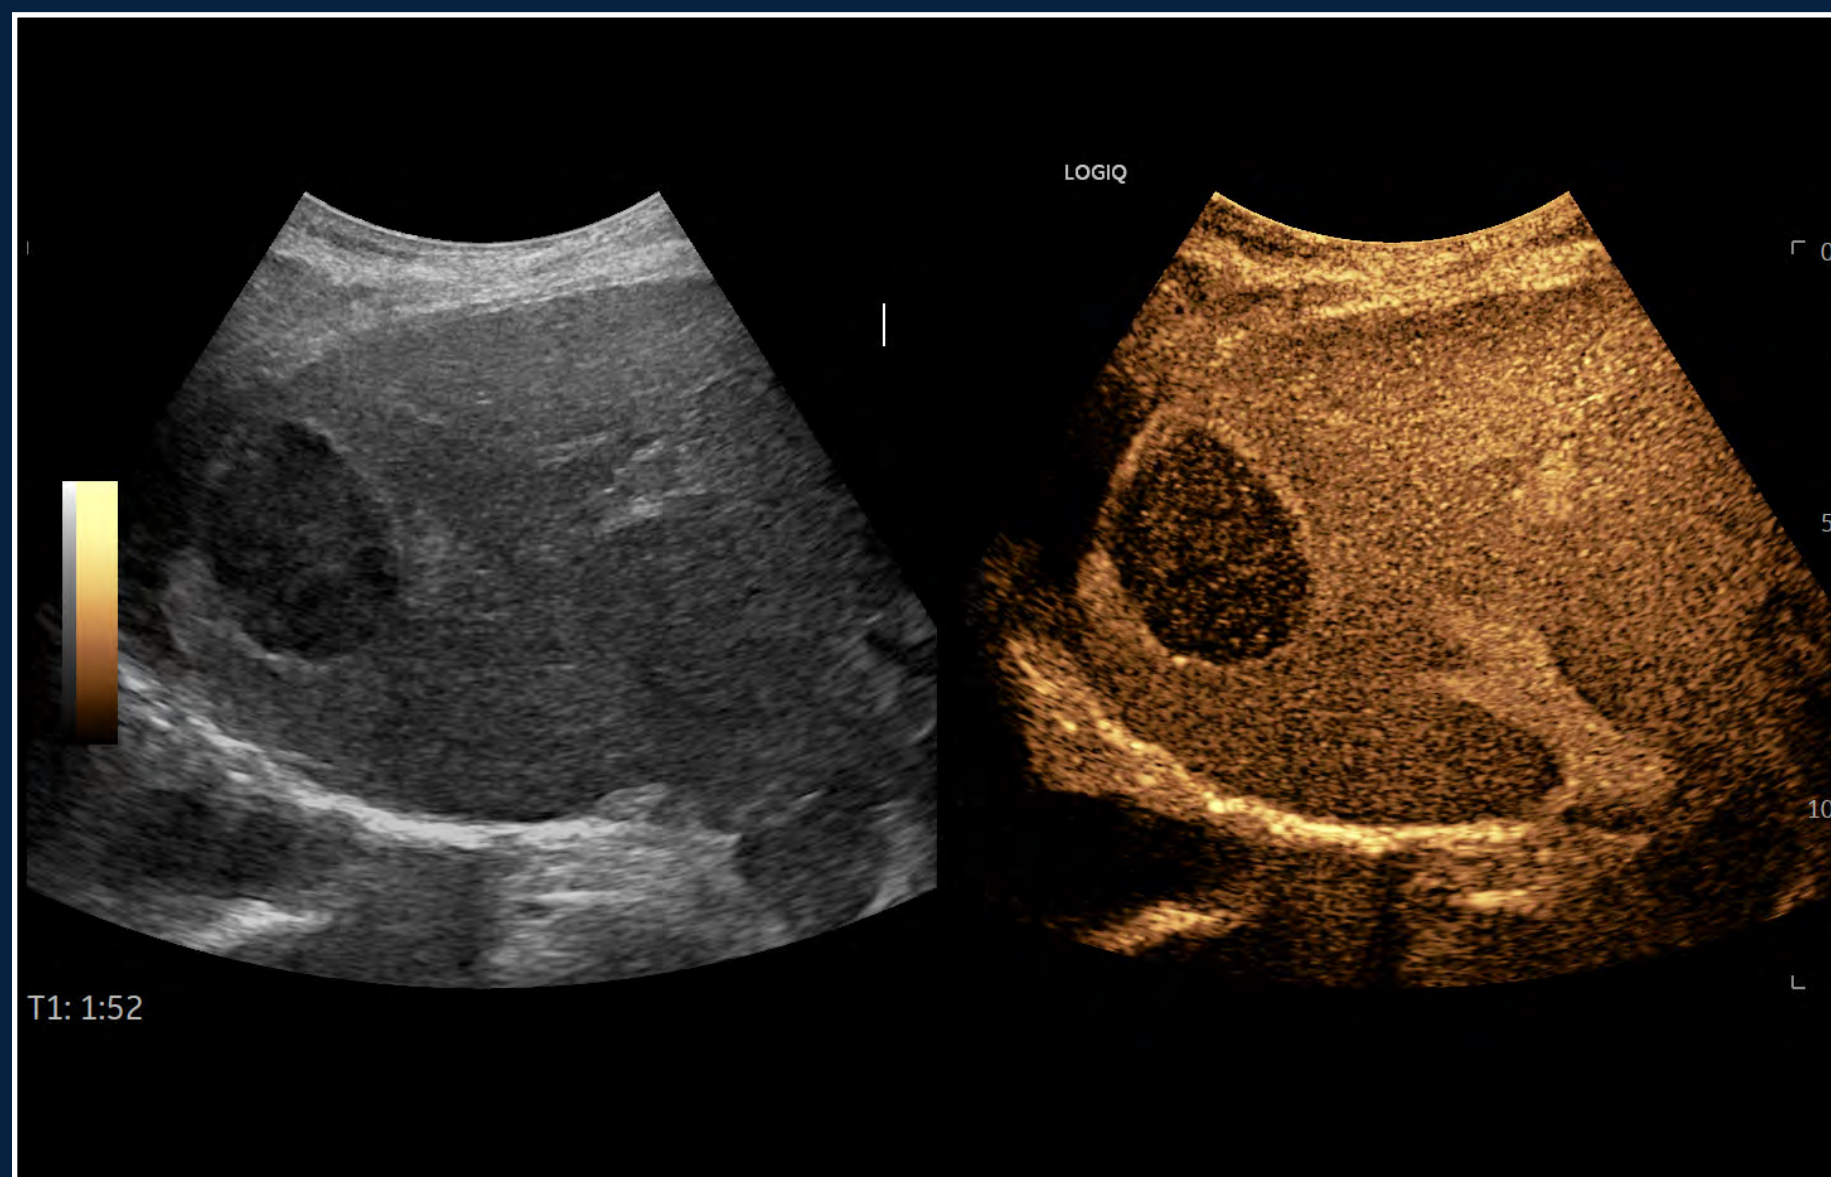

Liver Lesion CEUS, C1-6-D







OVERVIEW

MULTI-PURPOSE/  
RADIOLOGY

CARDIOLOGY

MUSCULOSKELETAL

BREAST


PRODUCTIVITY

INVESTMENT

CONTACT

# CLINICAL IMAGES | Spleen

Exceeding your expectations: whole body imaging

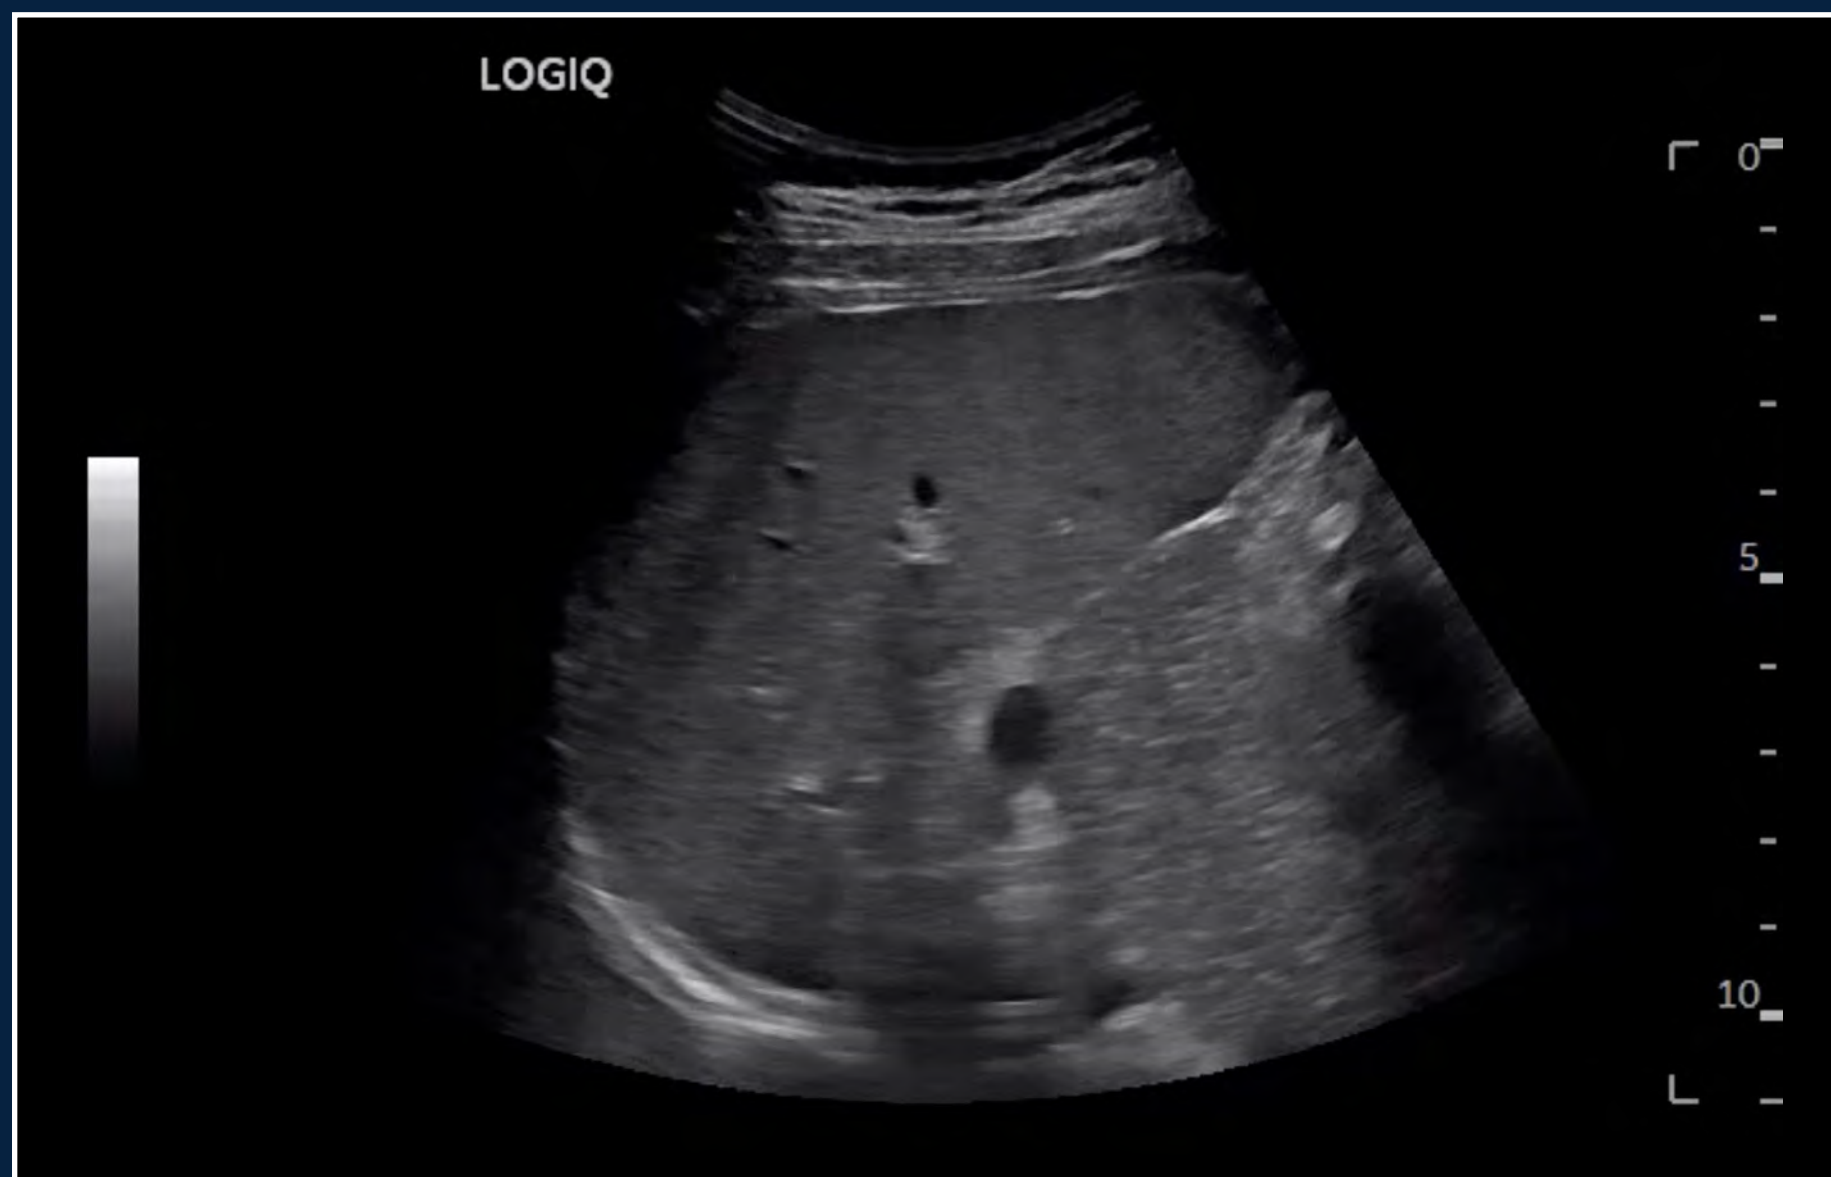

B-Mode with Advanced SRI Spleen, C2-9-D







OVERVIEW

MULTI-PURPOSE/  
RADIOLOGY

CARDIOLOGY

MUSCULOSKELETAL

BREAST

PRODUCTIVITY

INVESTMENT

CONTACT

# CLINICAL IMAGES | Kidney

Exceeding your expectations: whole body imaging



Color Flow with Radiantflow, C2-9-D







OVERVIEW

MULTI-PURPOSE/  
RADIOLOGY

CARDIOLOGY

MUSCULOSKELETAL

BREAST


PRODUCTIVITY

INVESTMENT

CONTACT

# CLINICAL IMAGES | Pediatrics

Exceeding your expectations: whole body imaging

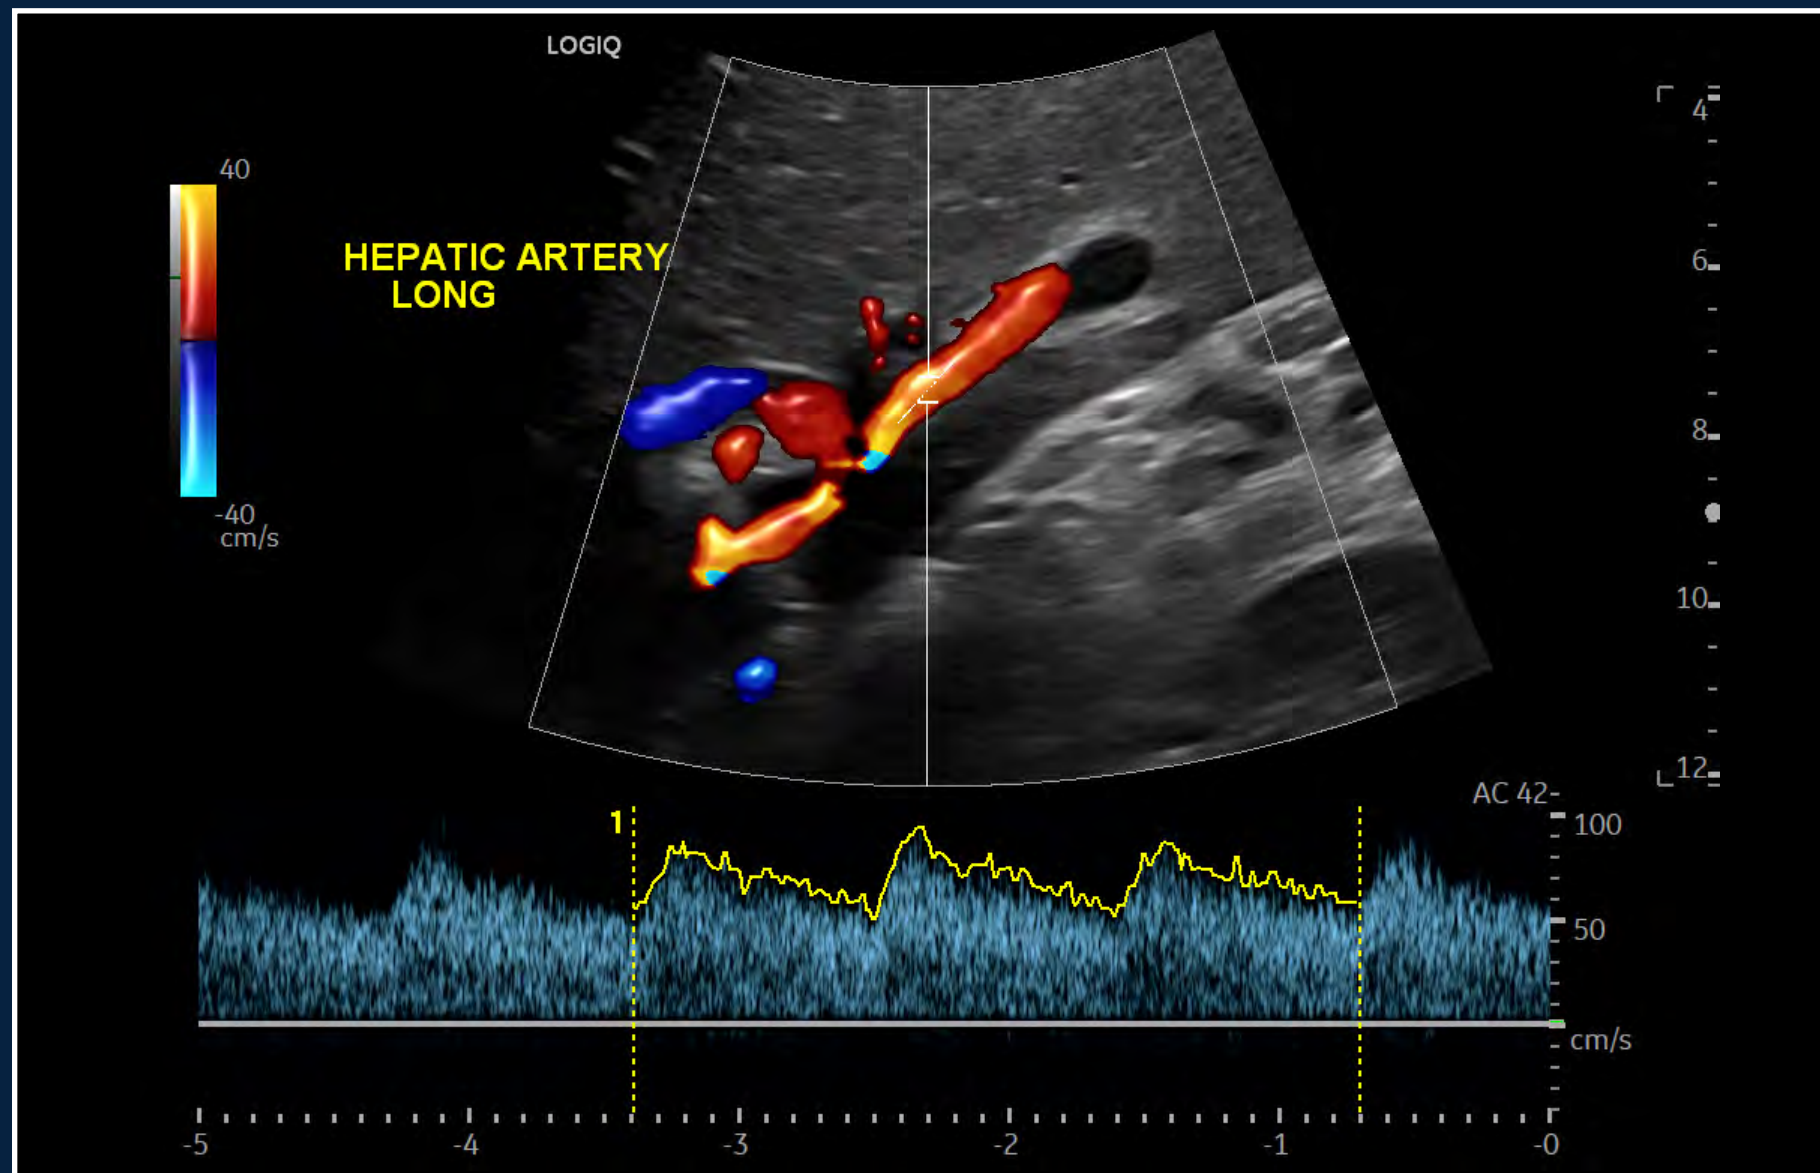

cSound B-Mode CF with Radiantflow and PW Doppler, C1-6-D







OVERVIEW

MULTI-PURPOSE/  
RADIOLOGY

CARDIOLOGY

MUSCULOSKELETAL

BREAST


PRODUCTIVITY

INVESTMENT

CONTACT

# CLINICAL IMAGES | Pediatrics

Exceeding your expectations: whole body imaging

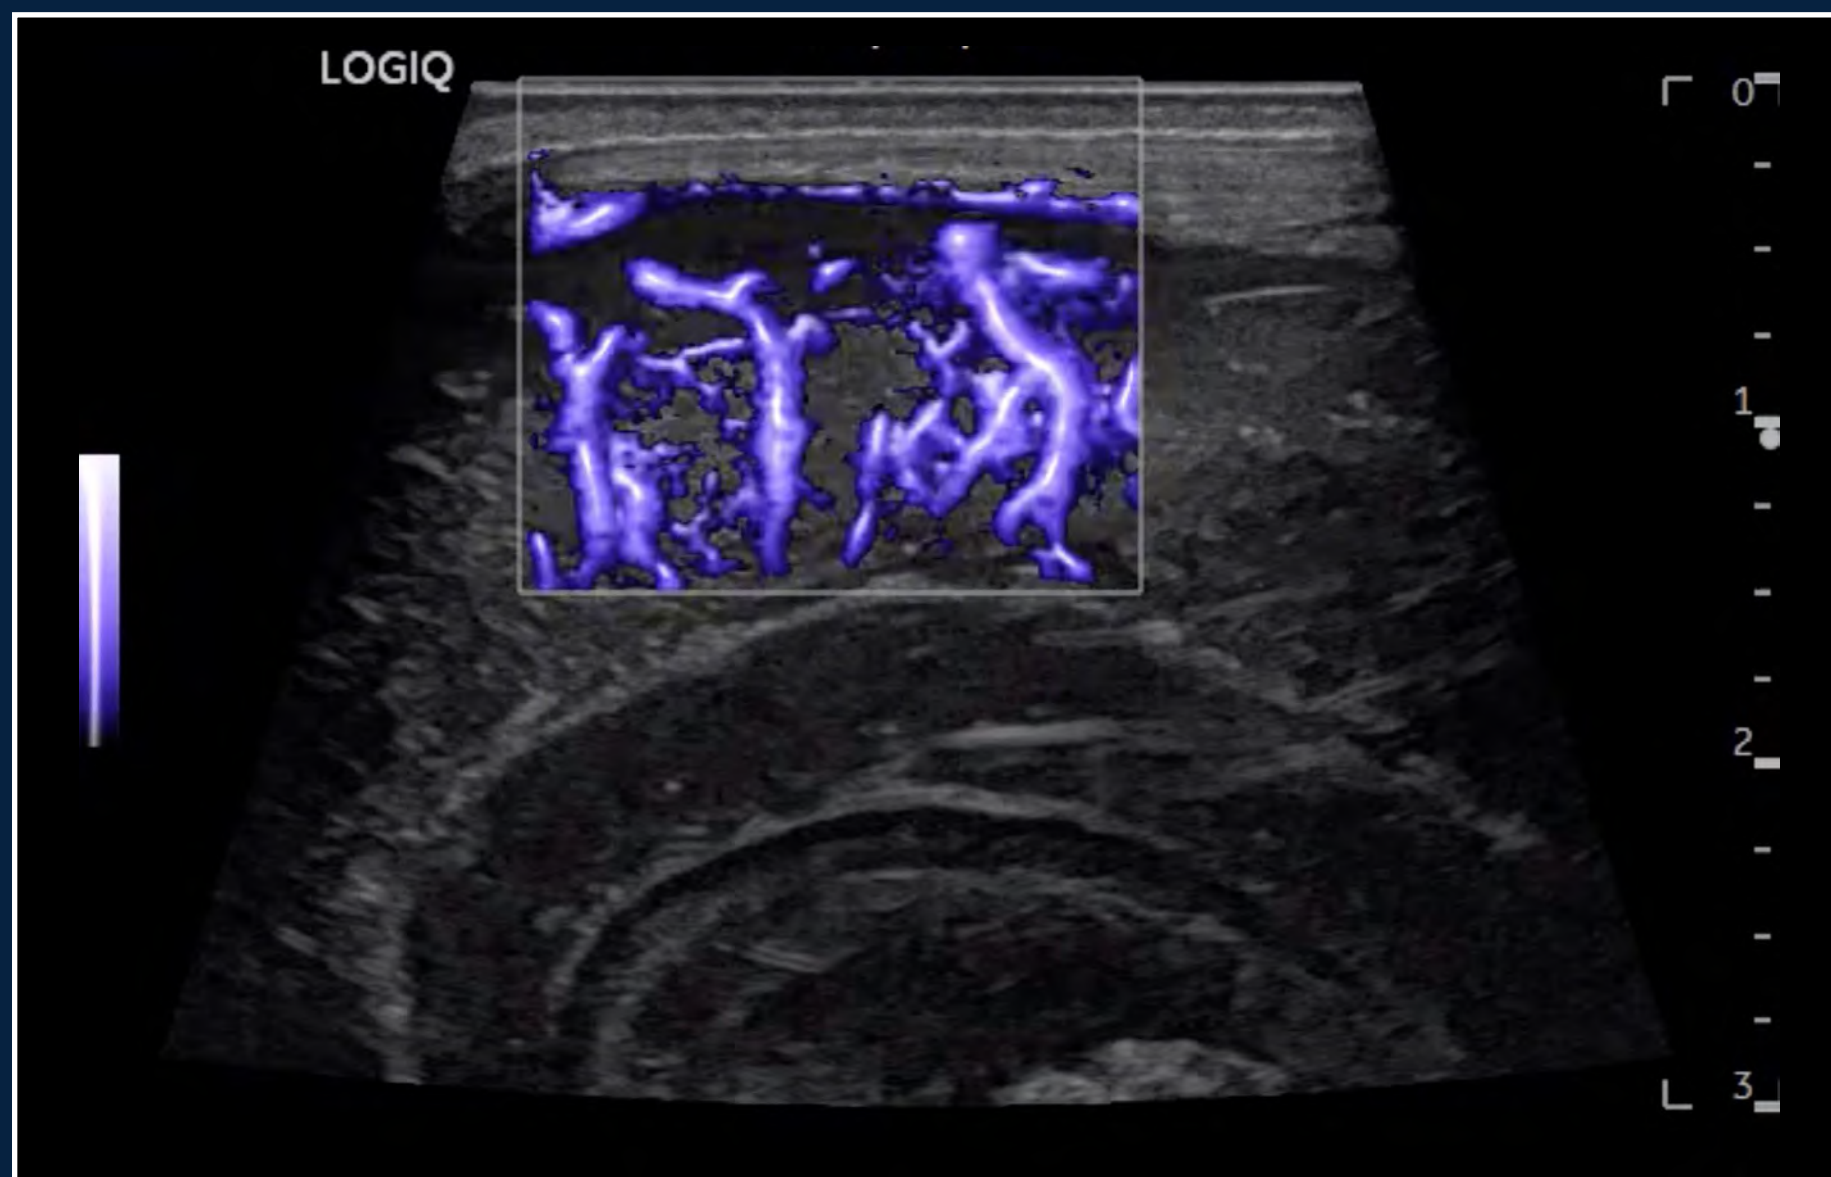

MVI with Radiantflow neonatal brain, L6-24-D







OVERVIEW

MULTI-PURPOSE/  
RADIOLOGY

CARDIOLOGY

MUSCULOSKELETAL

BREAST


PRODUCTIVITY

INVESTMENT

CONTACT

# CLINICAL IMAGES | Pediatrics

Exceeding your expectations: whole body imaging

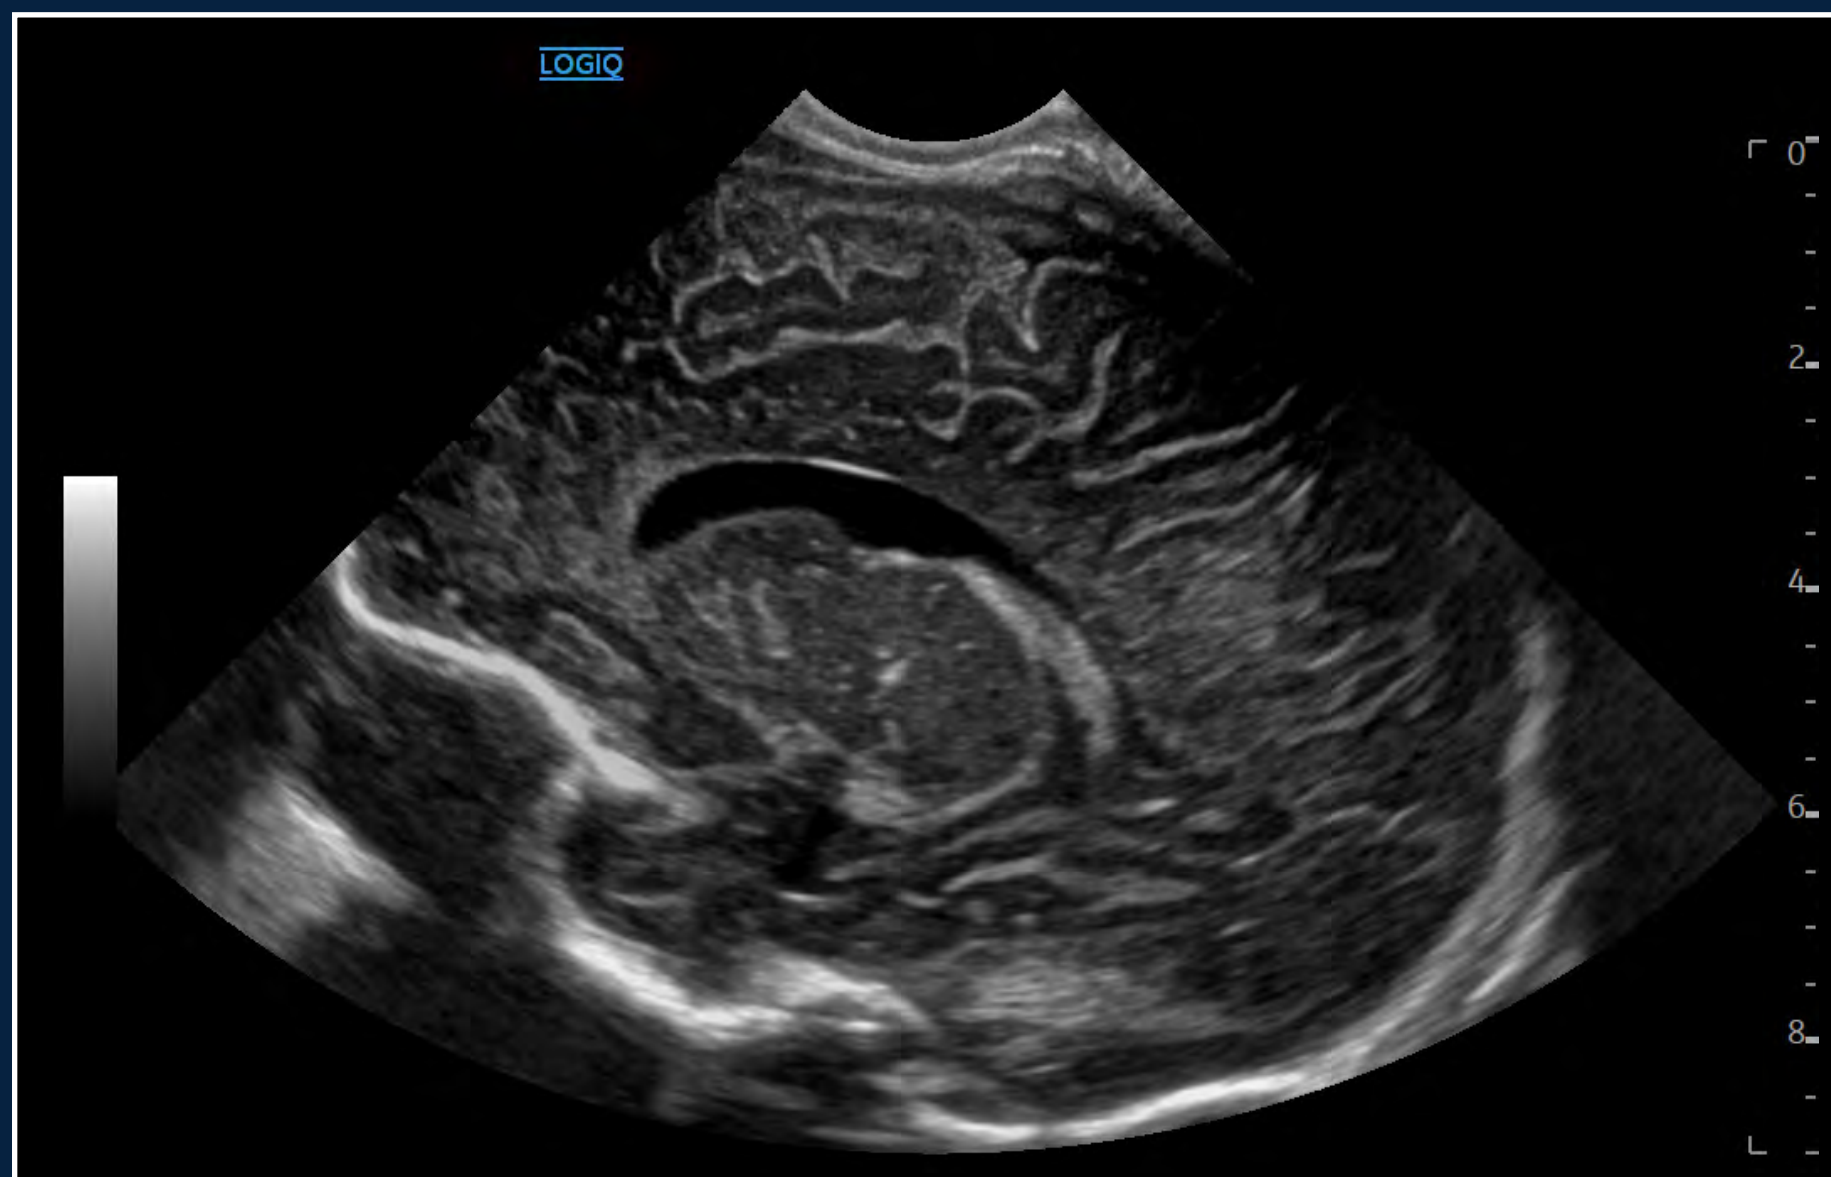

Neonatal head, C3-10-D







OVERVIEW

MULTI-PURPOSE/  
RADIOLOGY

CARDIOLOGY

MUSCULOSKELETAL

BREAST


PRODUCTIVITY

INVESTMENT

CONTACT

# CLINICAL IMAGES | Small Parts

Exceeding your expectations: whole body imaging

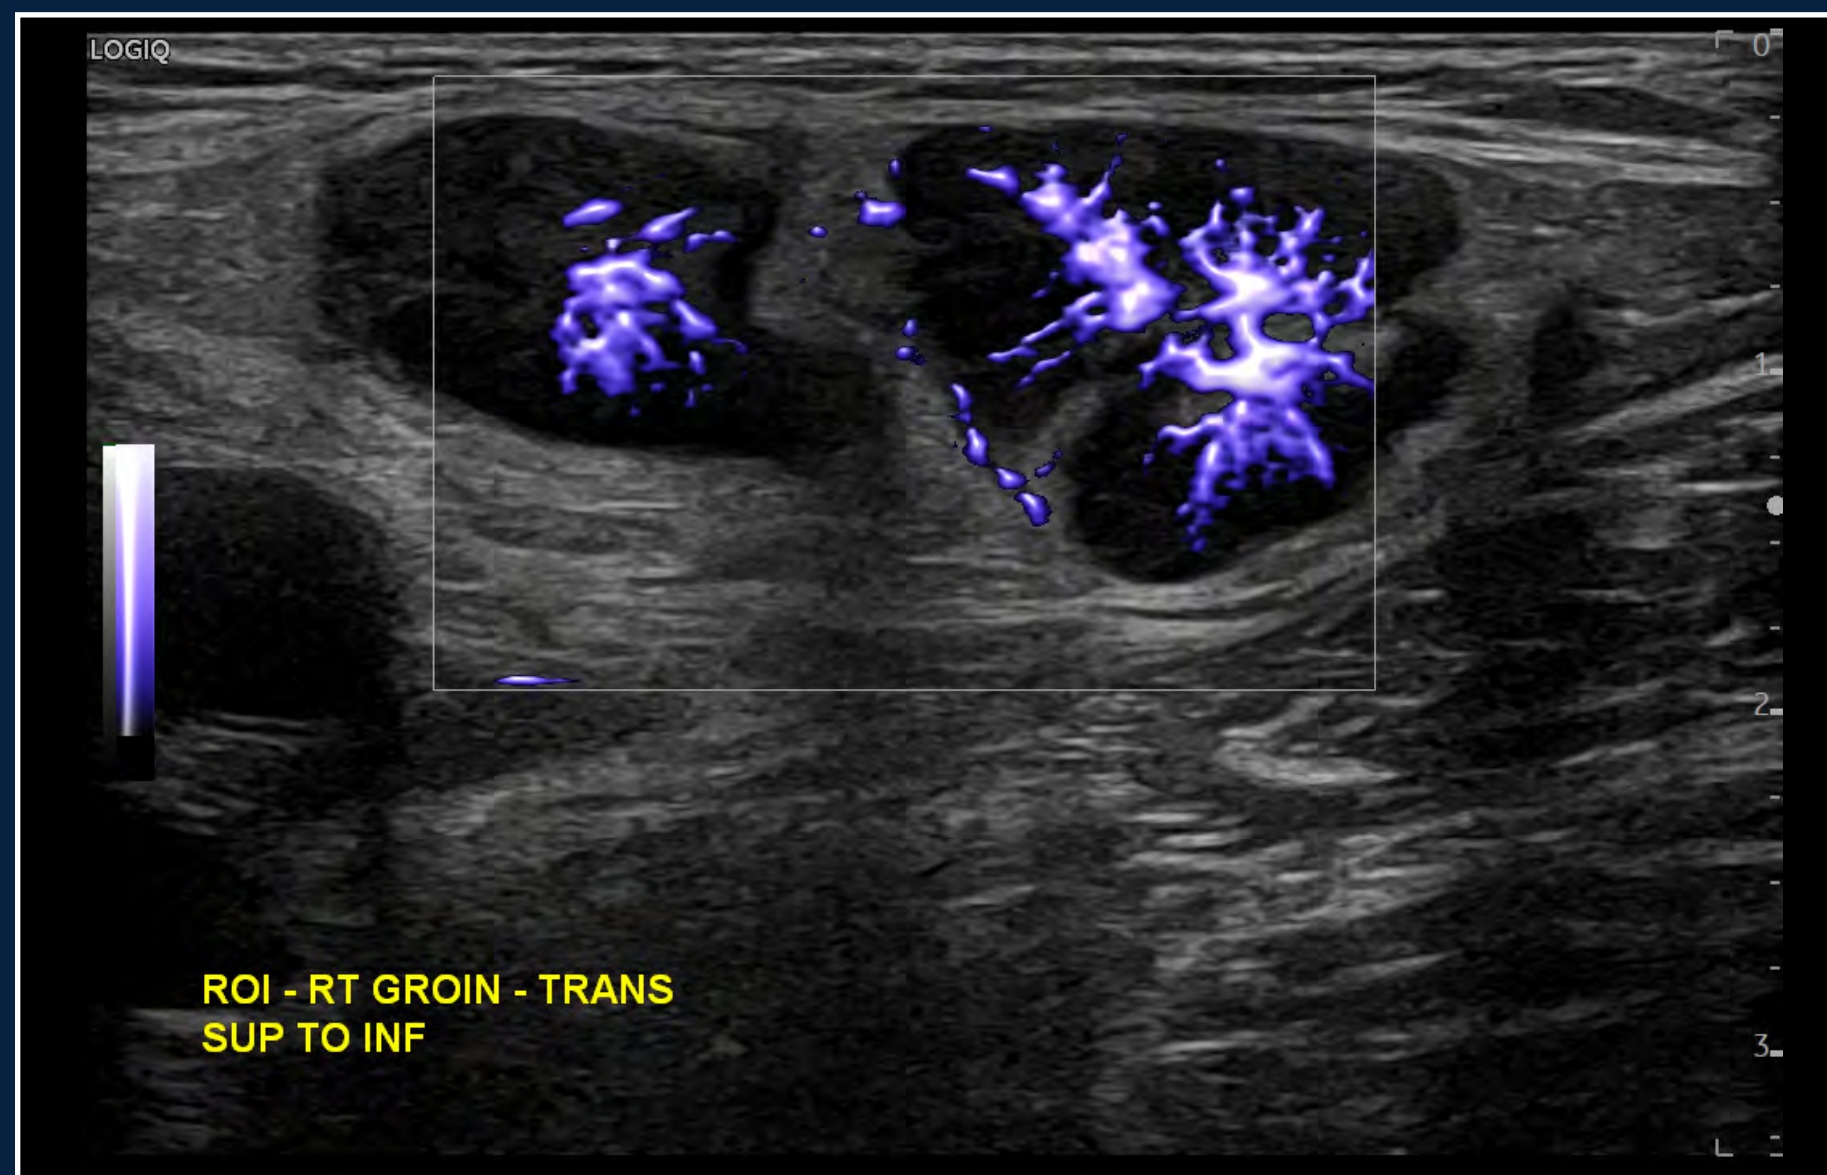

MVI with Radiantflow groin lymph node, ML6-15-D







OVERVIEW

MULTI-PURPOSE/  
RADIOLOGY

CARDIOLOGY

MUSCULOSKELETAL

BREAST


PRODUCTIVITY

INVESTMENT

CONTACT

# CLINICAL IMAGES | Small Parts

Exceeding your expectations: whole body imaging

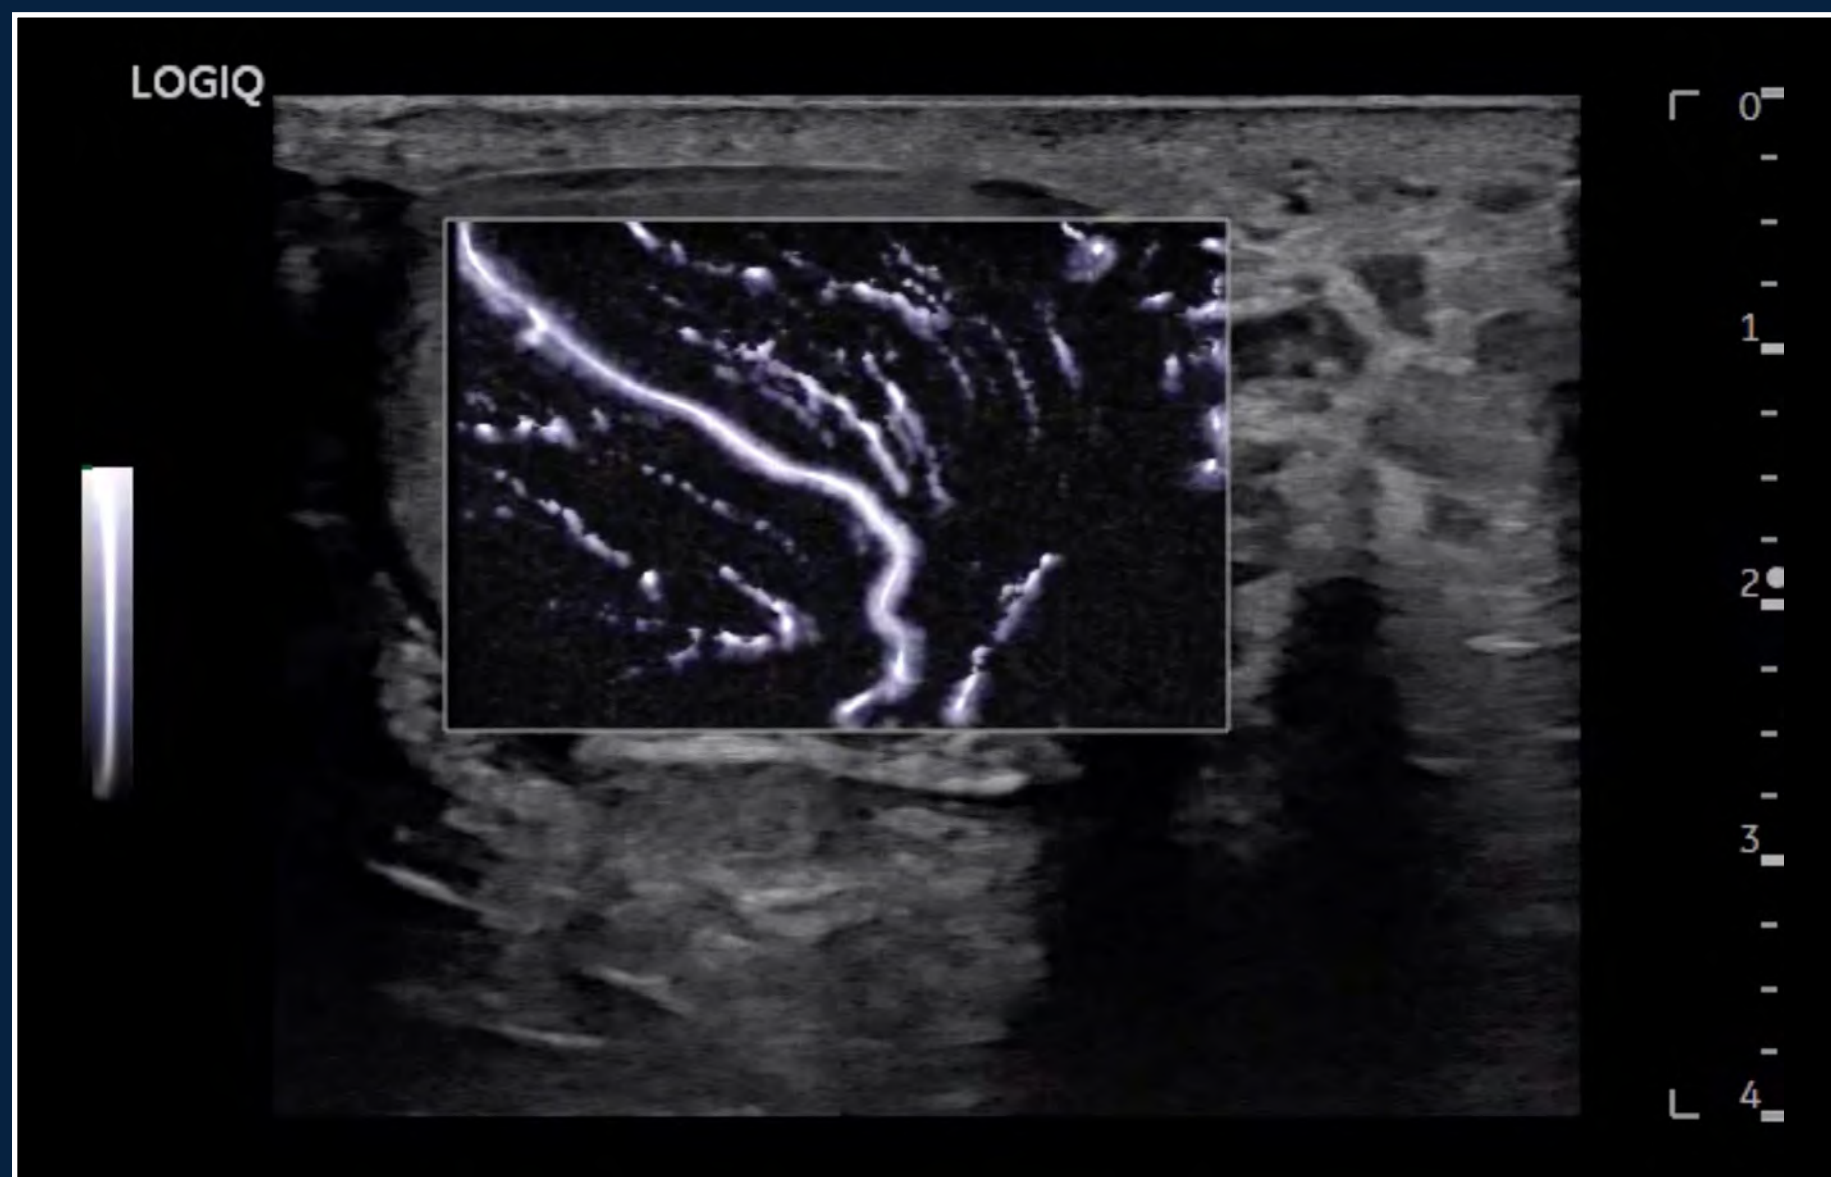

MVI with Radiantflow in scrotal, L3-12-D






[OVERVIEW](#)[MULTI-PURPOSE/  
RADIOLOGY](#)[CARDIOLOGY](#)[MUSCULOSKELETAL](#)[BREAST](#)[PRODUCTIVITY](#)[INVESTMENT](#)[CONTACT](#)

# CARDIOLOGY

LOGIQ Fortis delivers superb image quality within fast scan times across a wide range of cardiac exams.

- cSound Architecture with advanced SRI for precise details
- Cardiac Strain assists in early identification of underlying cardiac disease
- Contrast agent imaging with high contrast sensitivity
- TVI/TVD to help assess tissue velocities

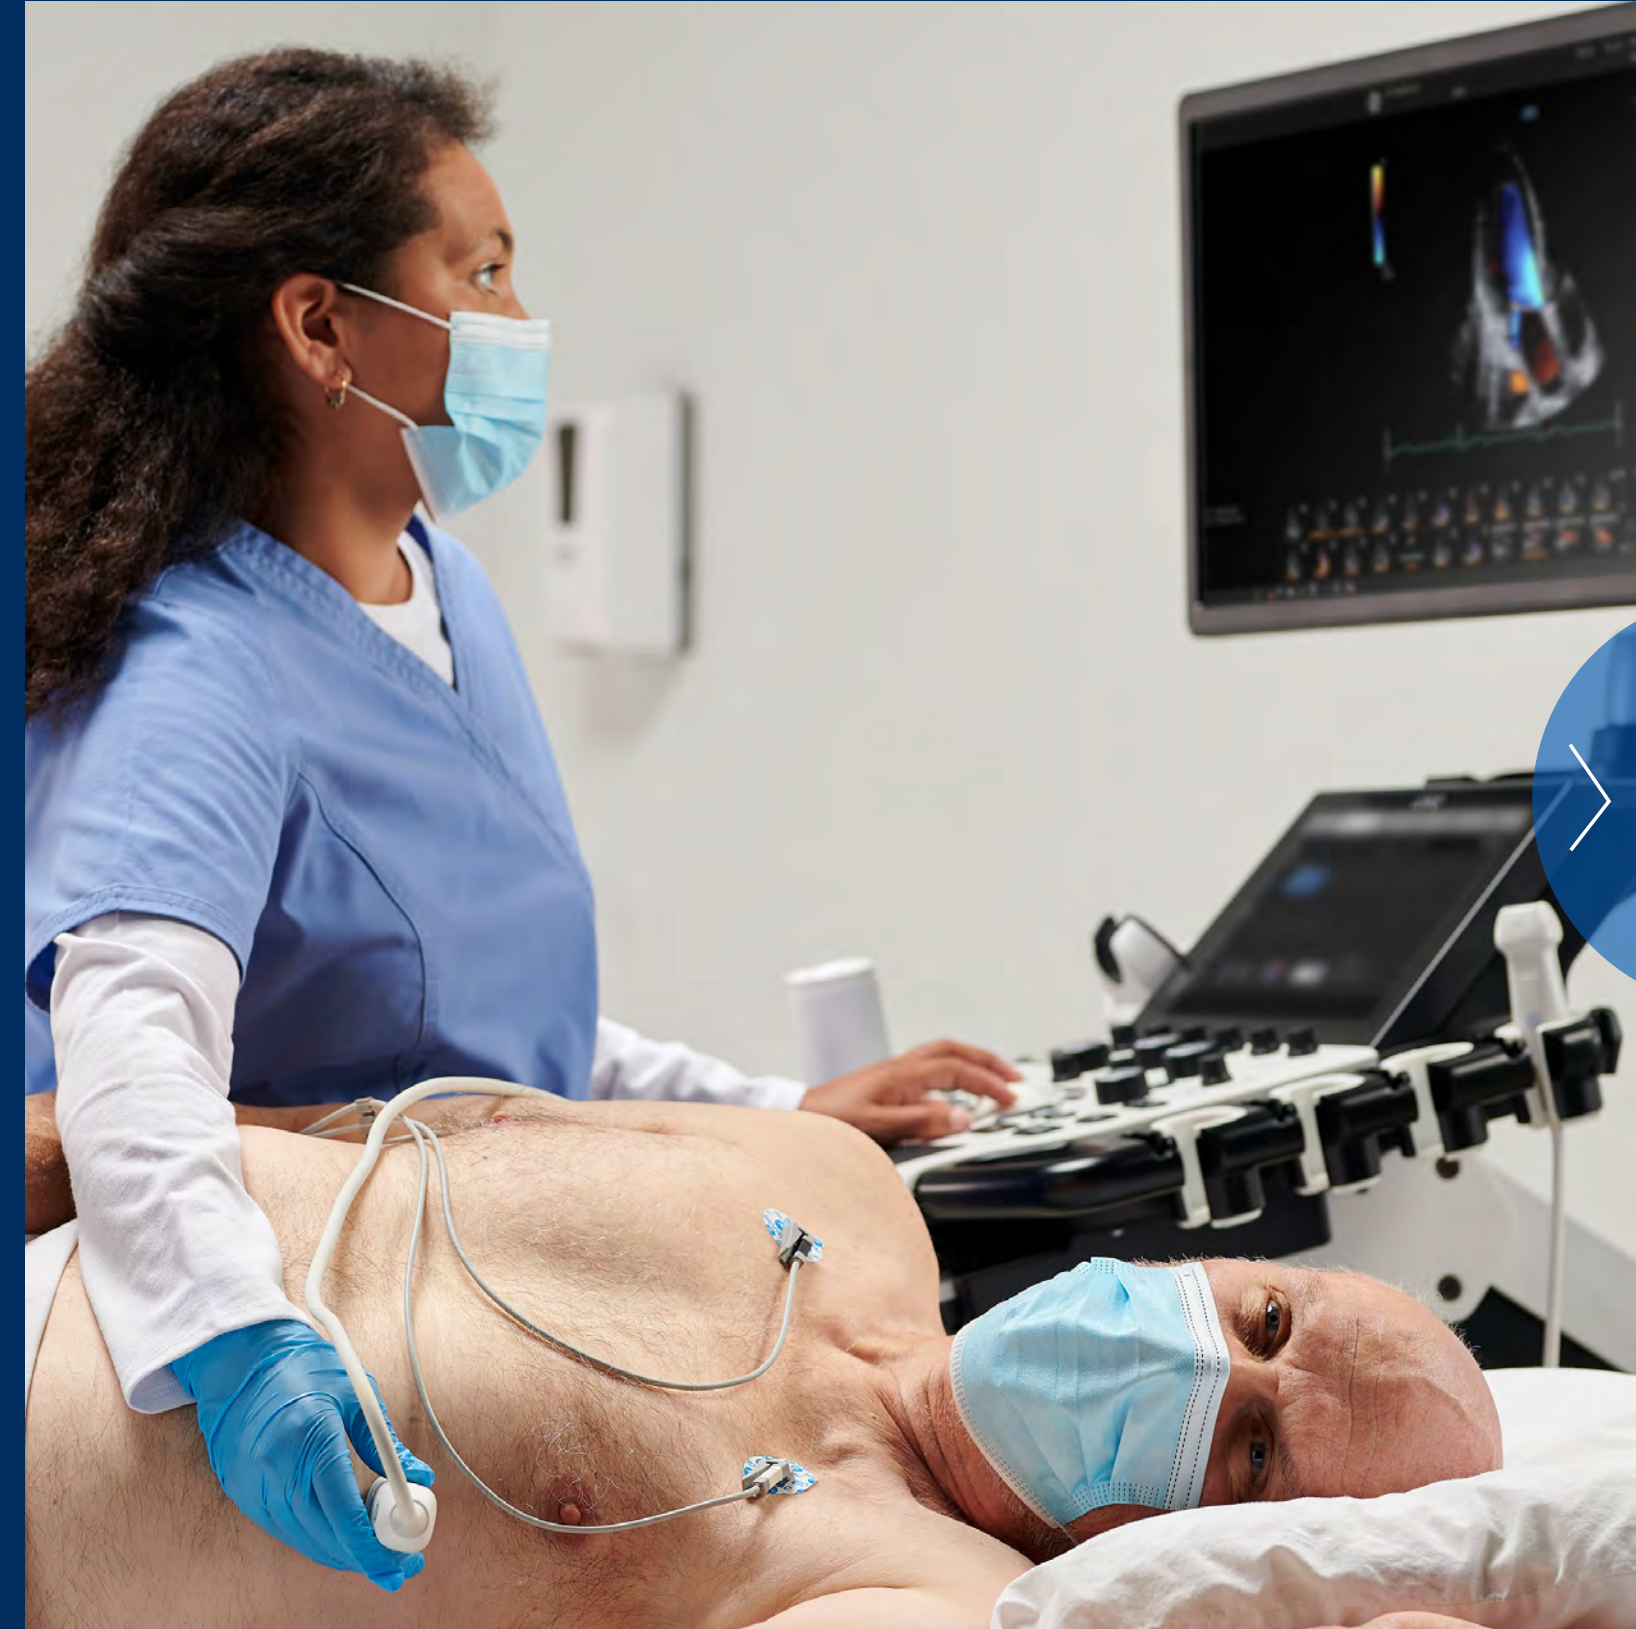[+ CLINICAL IMAGES](#)

LOGIQ Fortis





OVERVIEW

MULTI-PURPOSE/  
RADIOLOGY

**CARDIOLOGY**

MUSCULOSKELETAL

BREAST


PRODUCTIVITY

INVESTMENT


CONTACT

# CLINICAL IMAGES | Cardiology

Acquire highly detailed cardiac images within efficient exam times, even in challenging cases

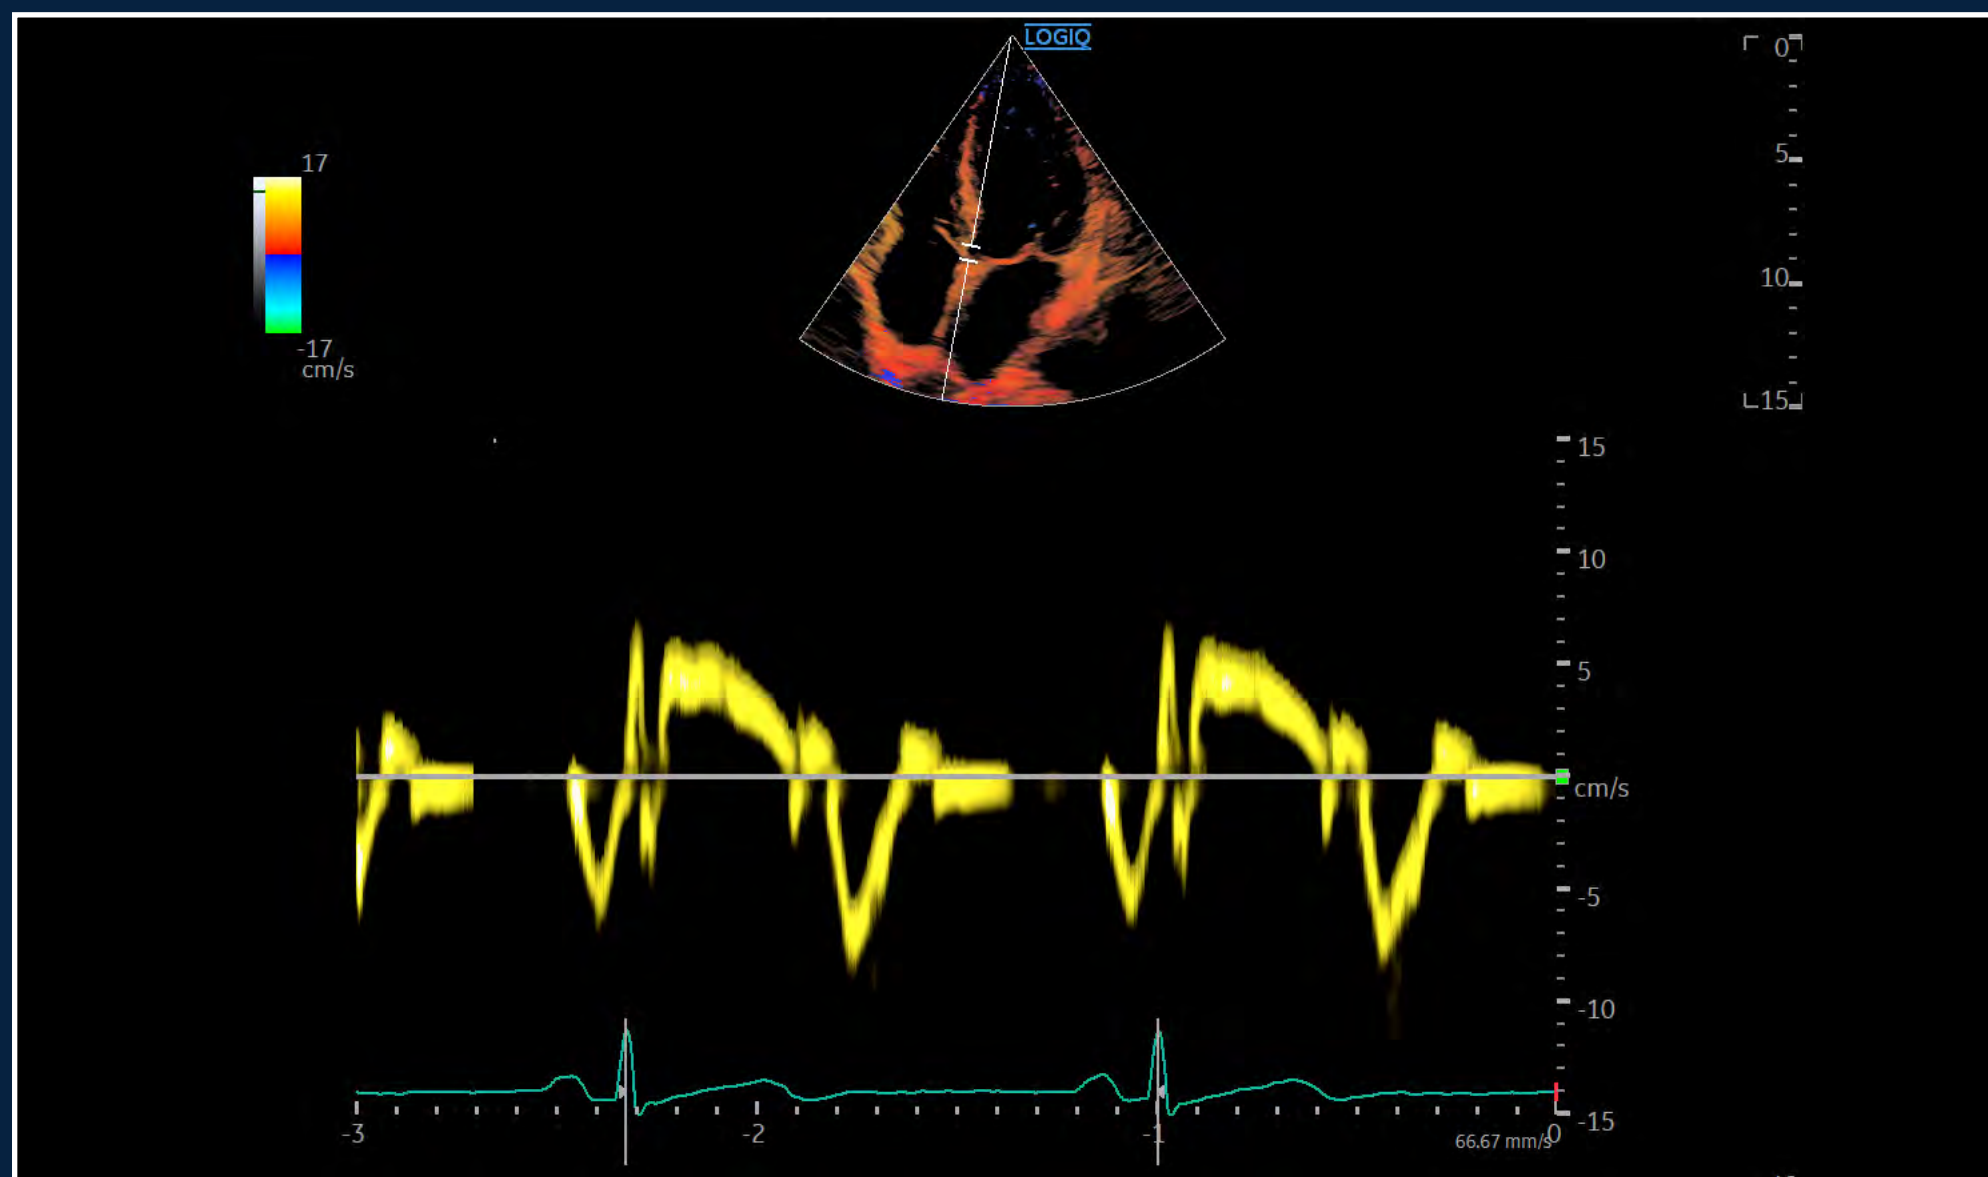

TVI and TVD Apical 4 Chamber View, M5Sc-D

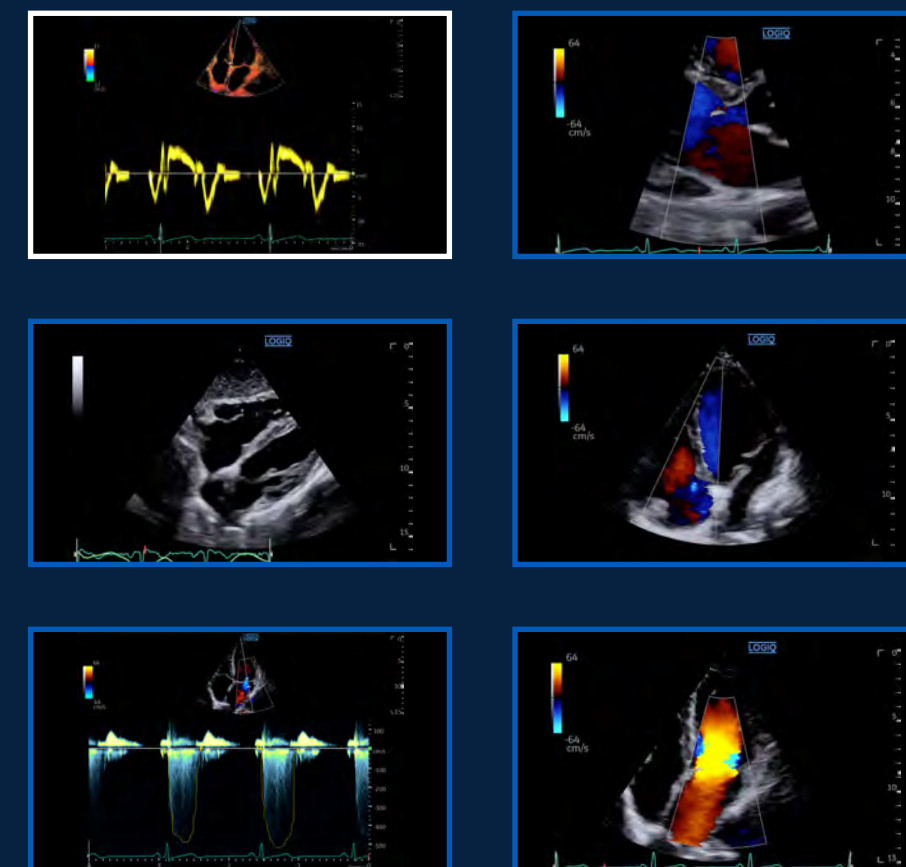





OVERVIEW

MULTI-PURPOSE/  
RADIOLOGY

**CARDIOLOGY**

MUSCULOSKELETAL

BREAST


PRODUCTIVITY

INVESTMENT


CONTACT

# CLINICAL IMAGES | Cardiology

Acquire highly detailed cardiac images within efficient exam times, even in challenging cases

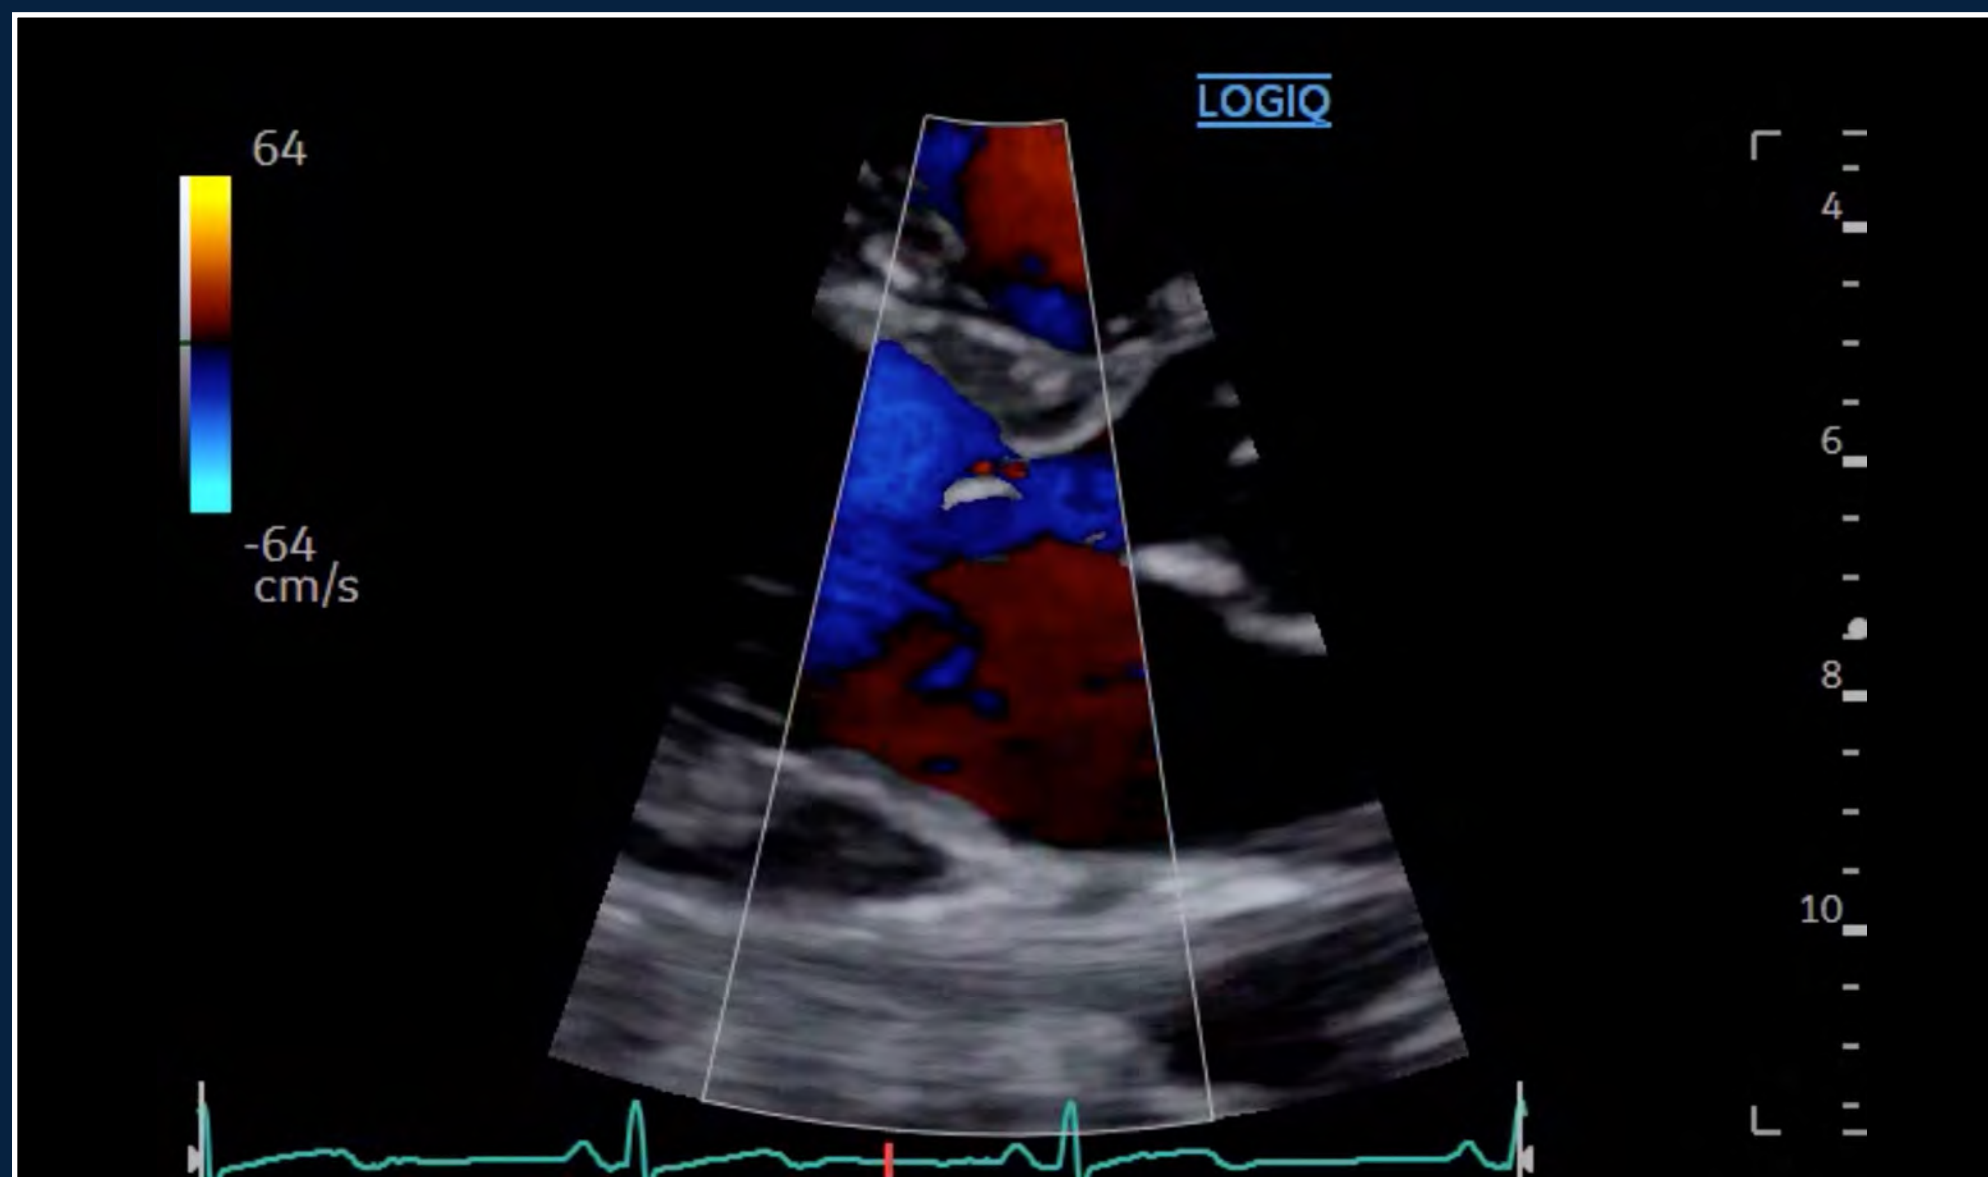

Color Flow in Cardiac Parasternal Long Axis View, M5Sc-D

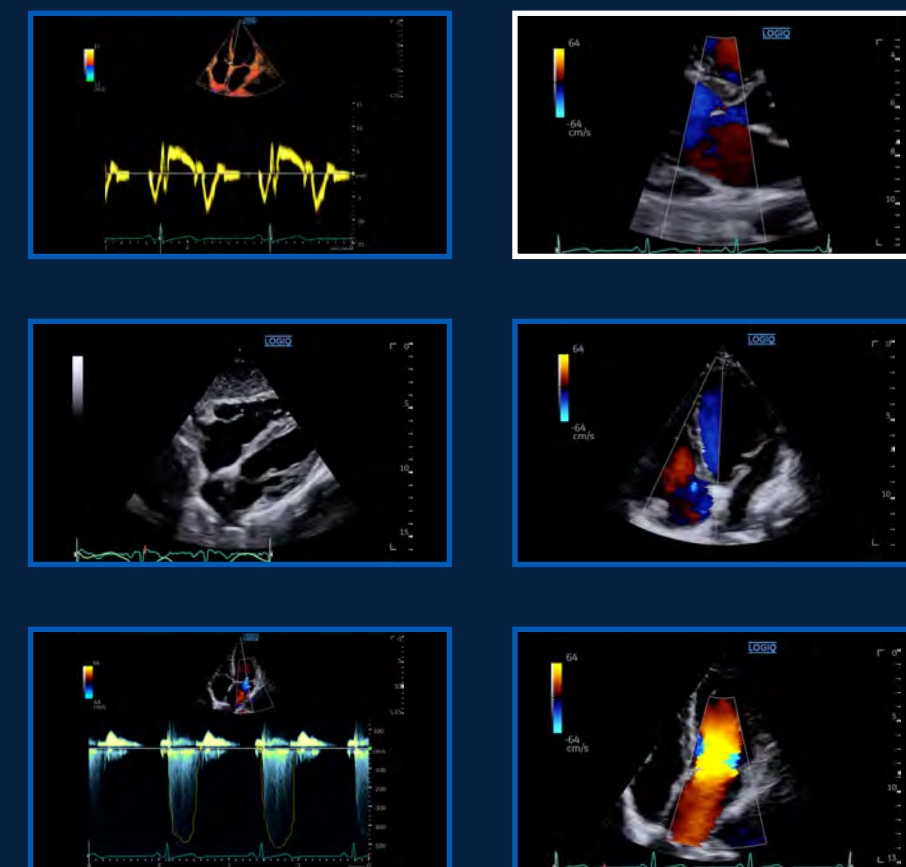





OVERVIEW

MULTI-PURPOSE/  
RADIOLOGY

**CARDIOLOGY**

MUSCULOSKELETAL

BREAST


PRODUCTIVITY

INVESTMENT







CONTACT

# CLINICAL IMAGES | Cardiology

Acquire highly detailed cardiac images within efficient exam times, even in challenging cases

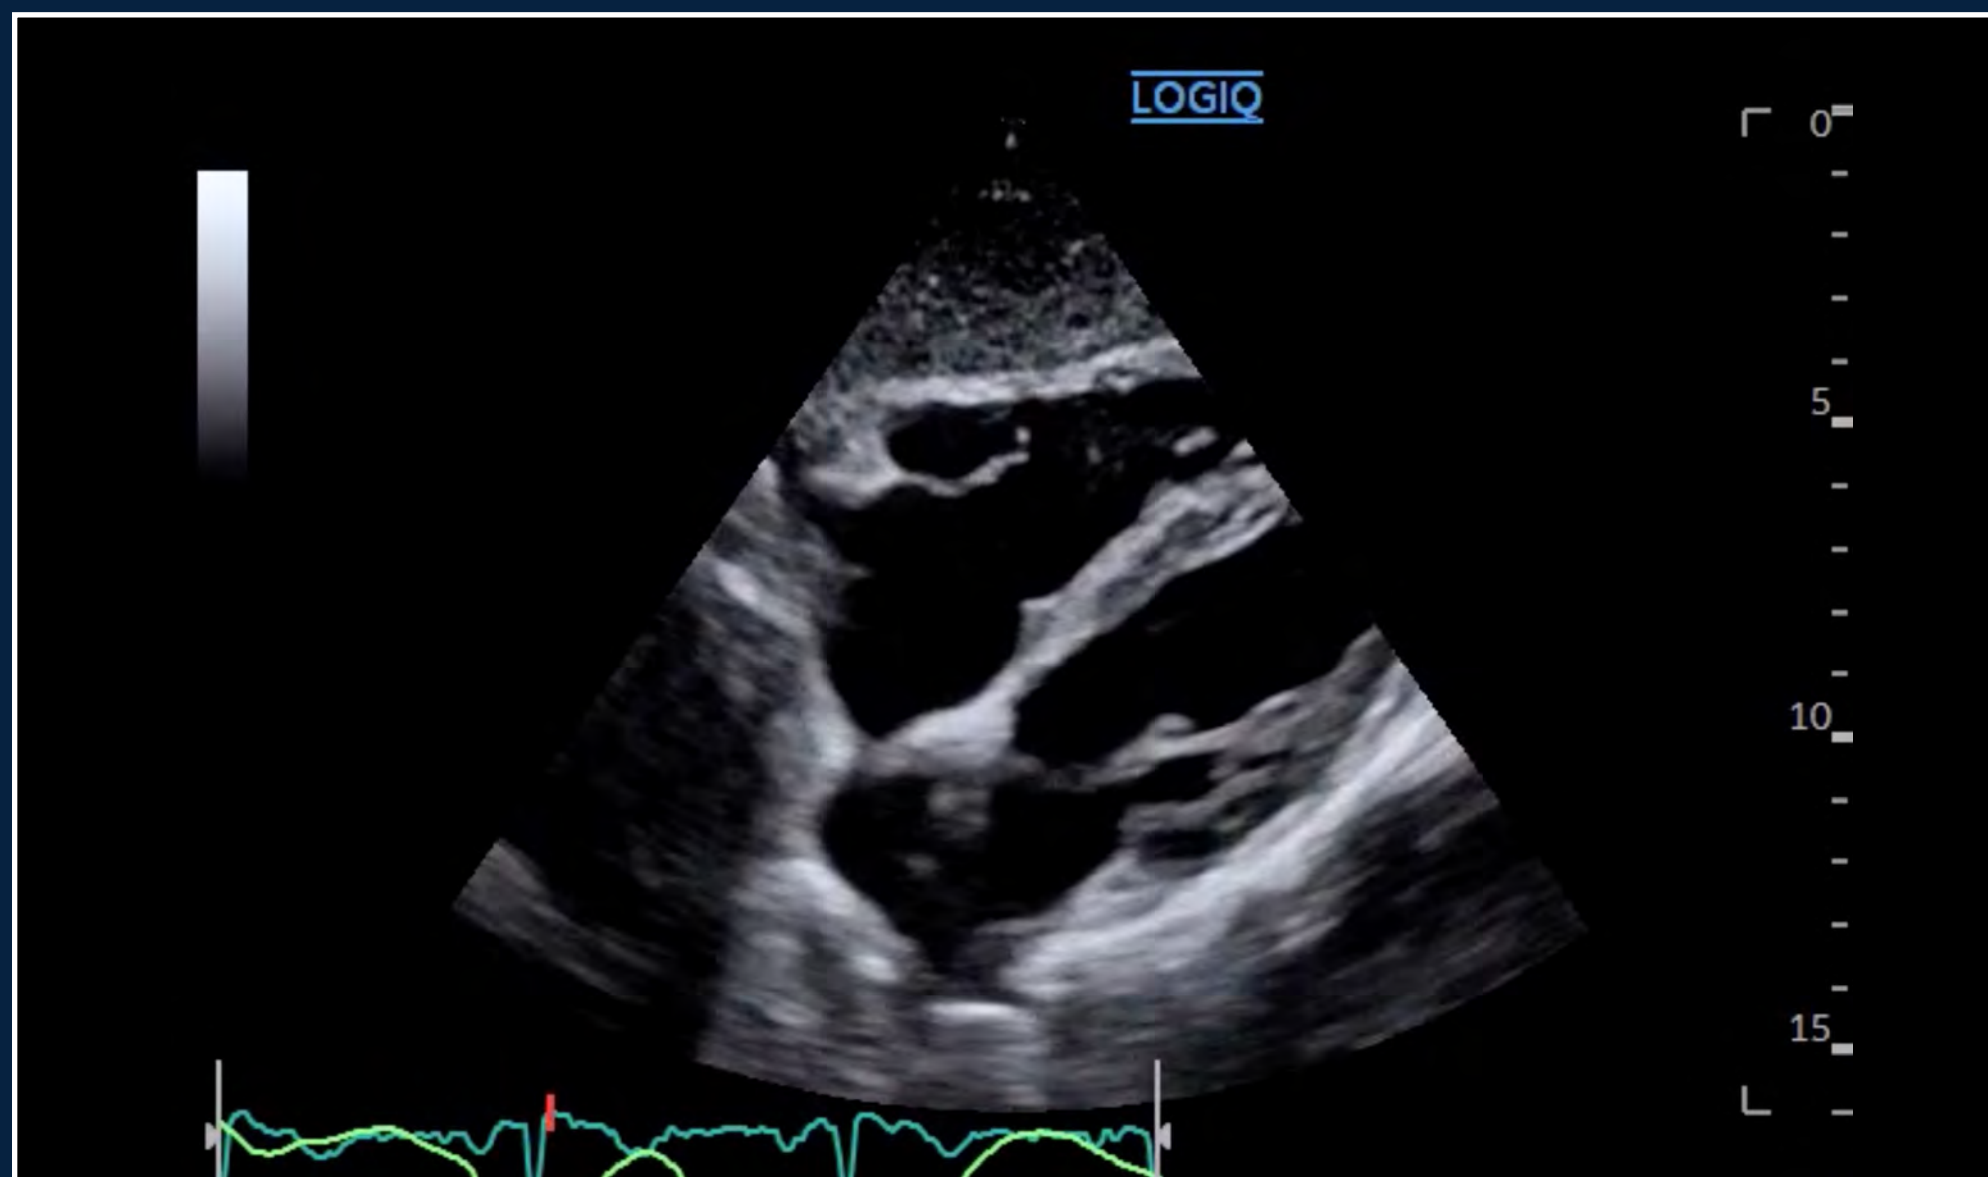

B-Mode with Advanced SRI ECG and Respirometer Display, M5Sc-D

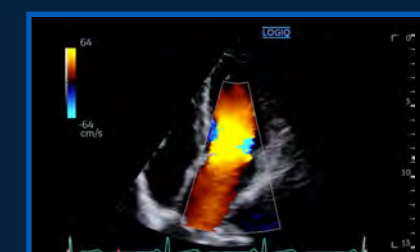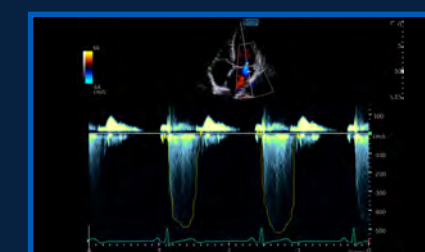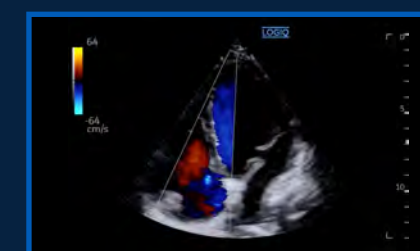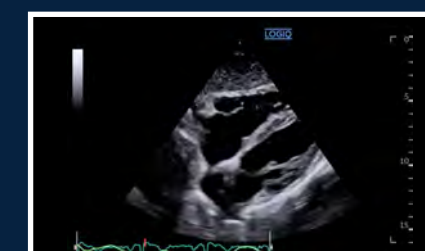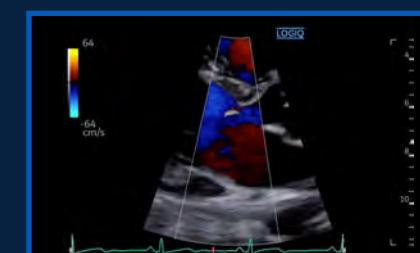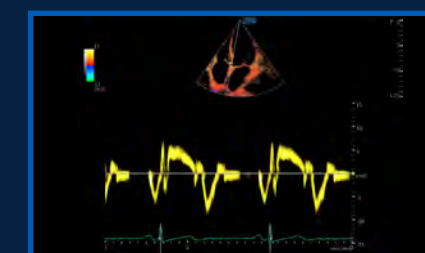





OVERVIEW

MULTI-PURPOSE/  
RADIOLOGY

**CARDIOLOGY**

MUSCULOSKELETAL

BREAST


PRODUCTIVITY

INVESTMENT


CONTACT

# CLINICAL IMAGES | Cardiology

Acquire highly detailed cardiac images within efficient exam times, even in challenging cases

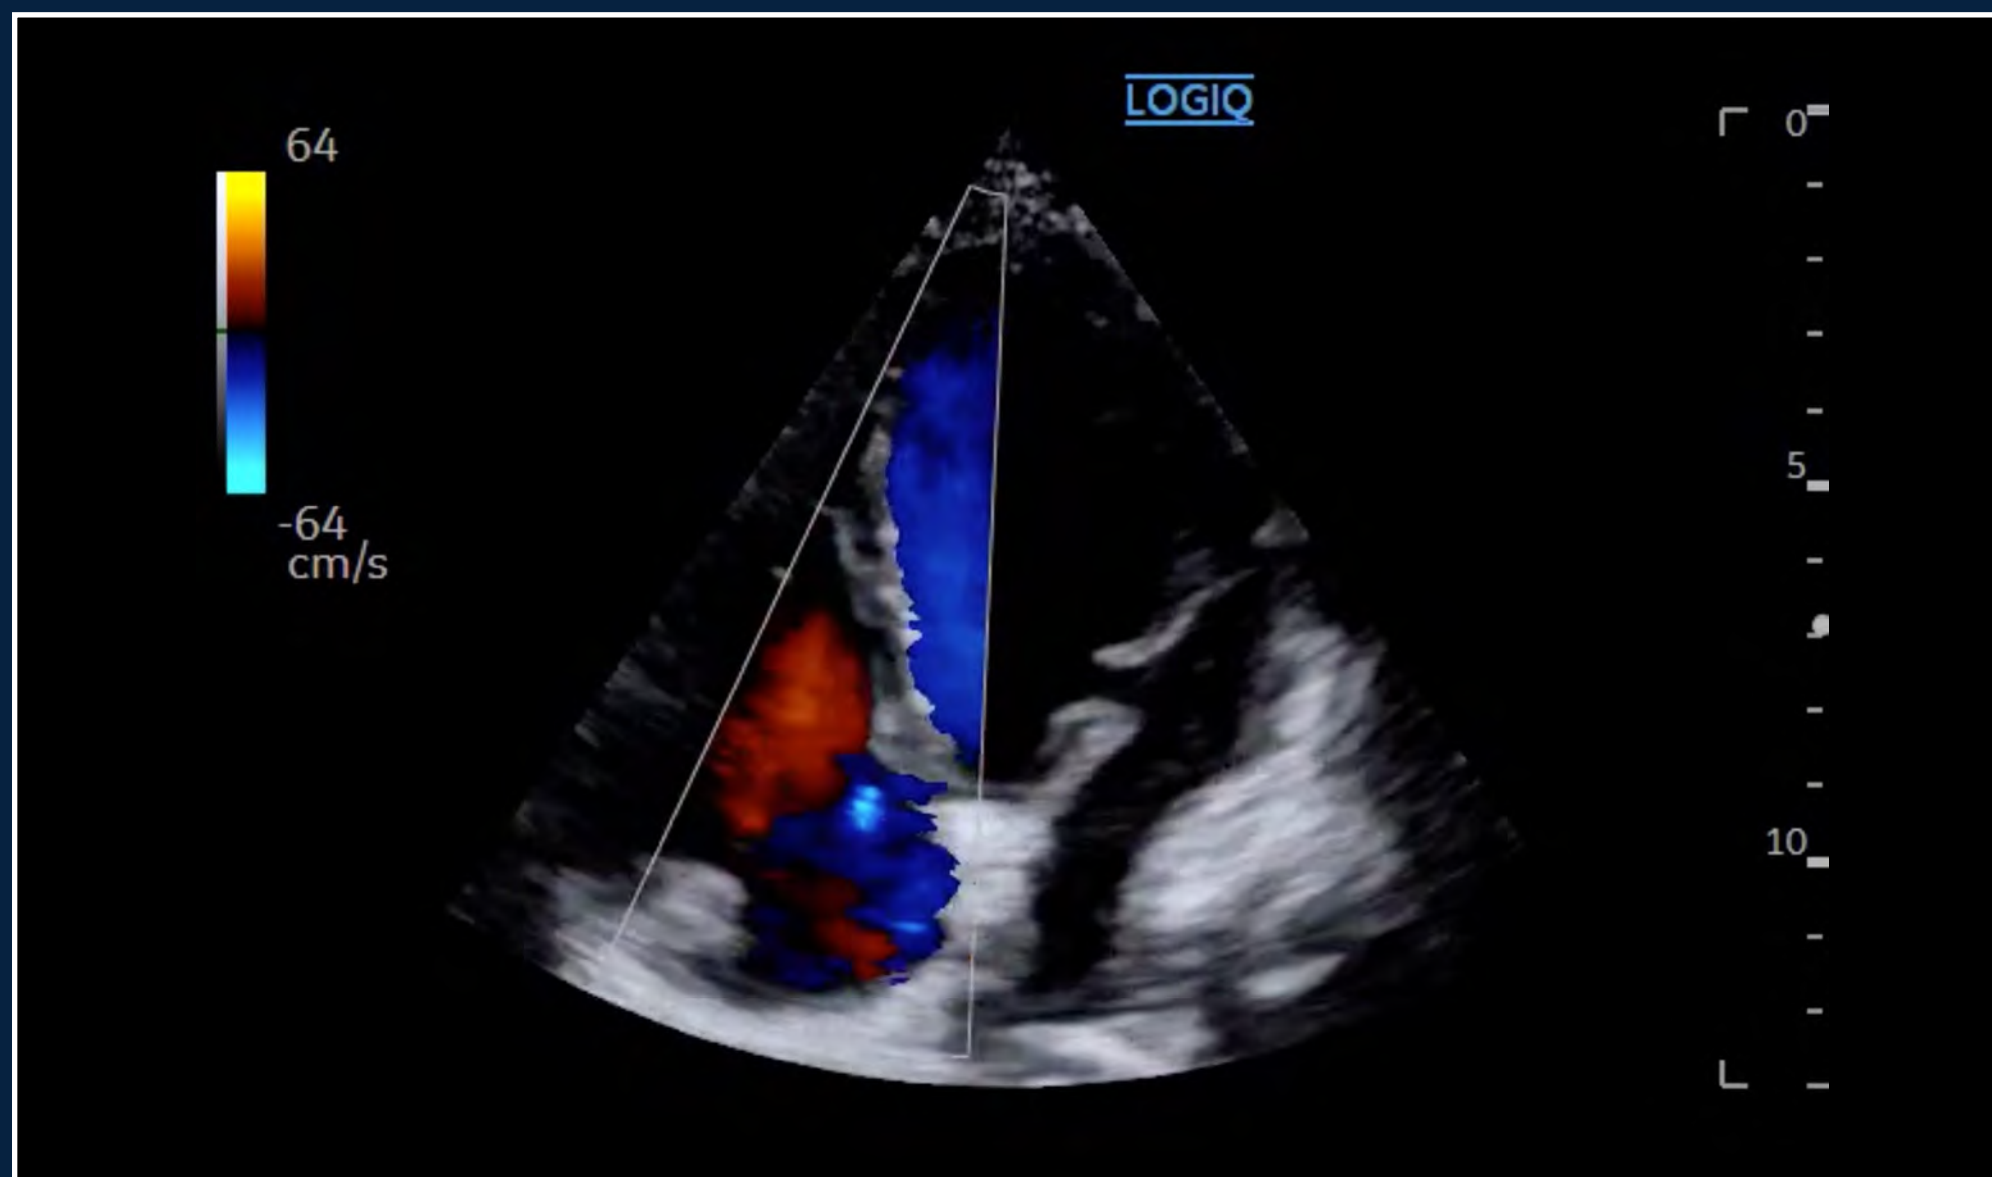

Color Flow Apical 4 Chamber View, M5Sc-D

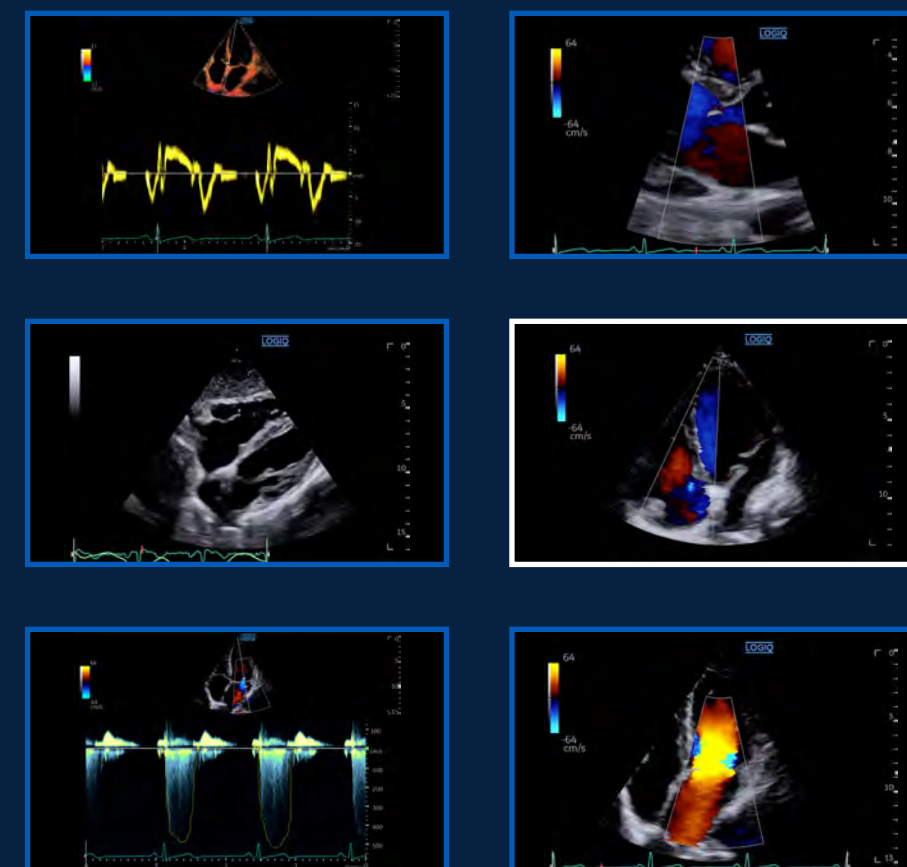





OVERVIEW

MULTI-PURPOSE/  
RADIOLOGY

**CARDIOLOGY**

MUSCULOSKELETAL

BREAST


PRODUCTIVITY

INVESTMENT


CONTACT

# CLINICAL IMAGES | Cardiology

Acquire highly detailed cardiac images within efficient exam times, even in challenging cases

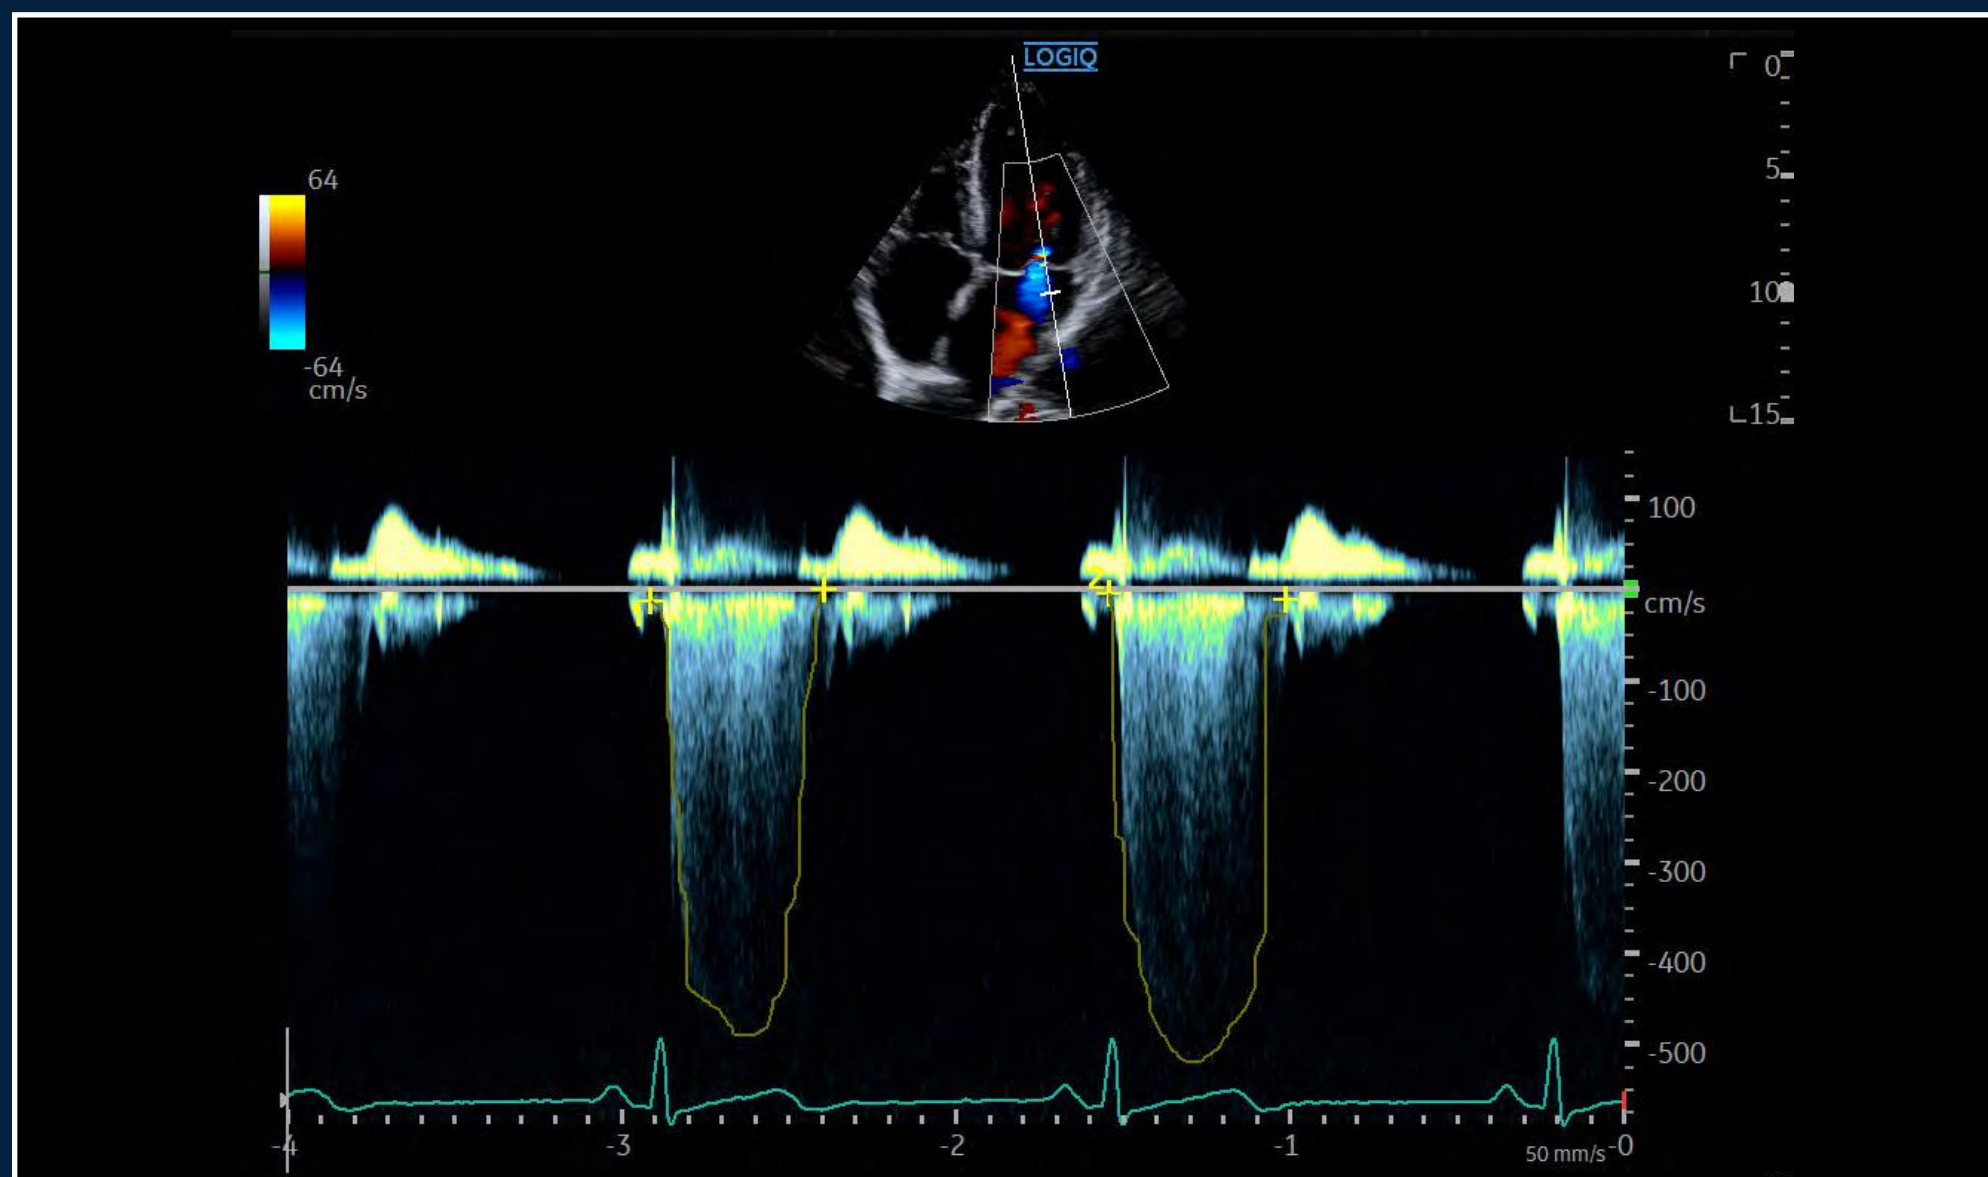

Color Flow and CW Doppler Mitral Valve, M5Sc-D

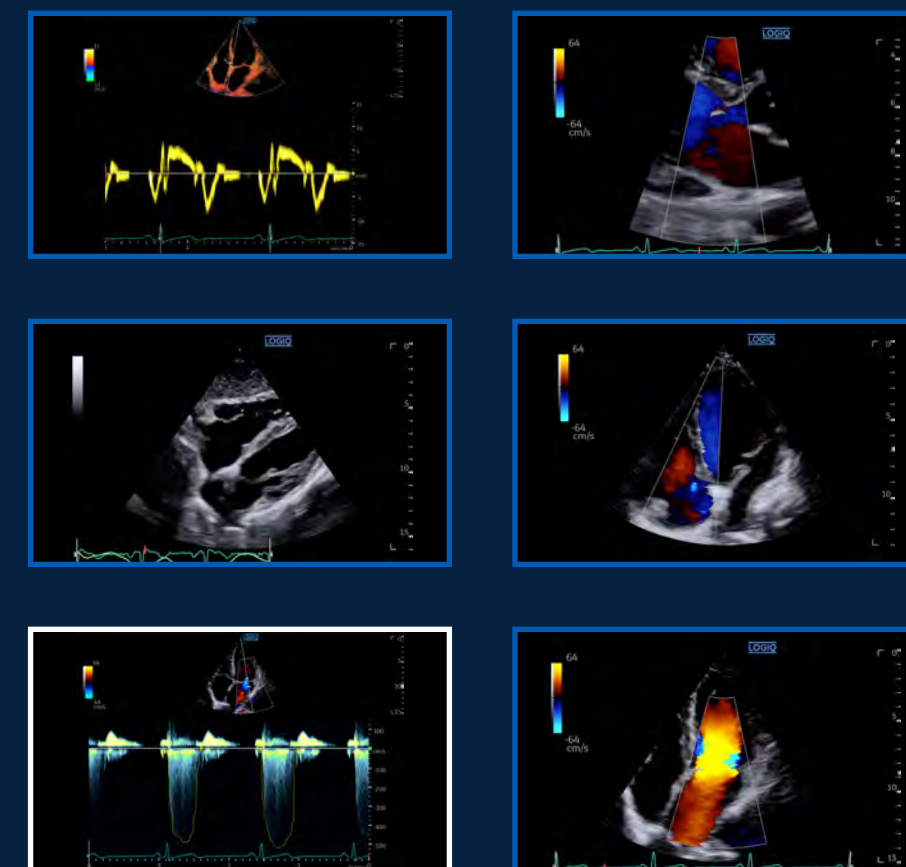





OVERVIEW

MULTI-PURPOSE/  
RADIOLOGY

**CARDIOLOGY**

MUSCULOSKELETAL

BREAST


PRODUCTIVITY

INVESTMENT


CONTACT

# CLINICAL IMAGES | Cardiology

Acquire highly detailed cardiac images within efficient exam times, even in challenging cases

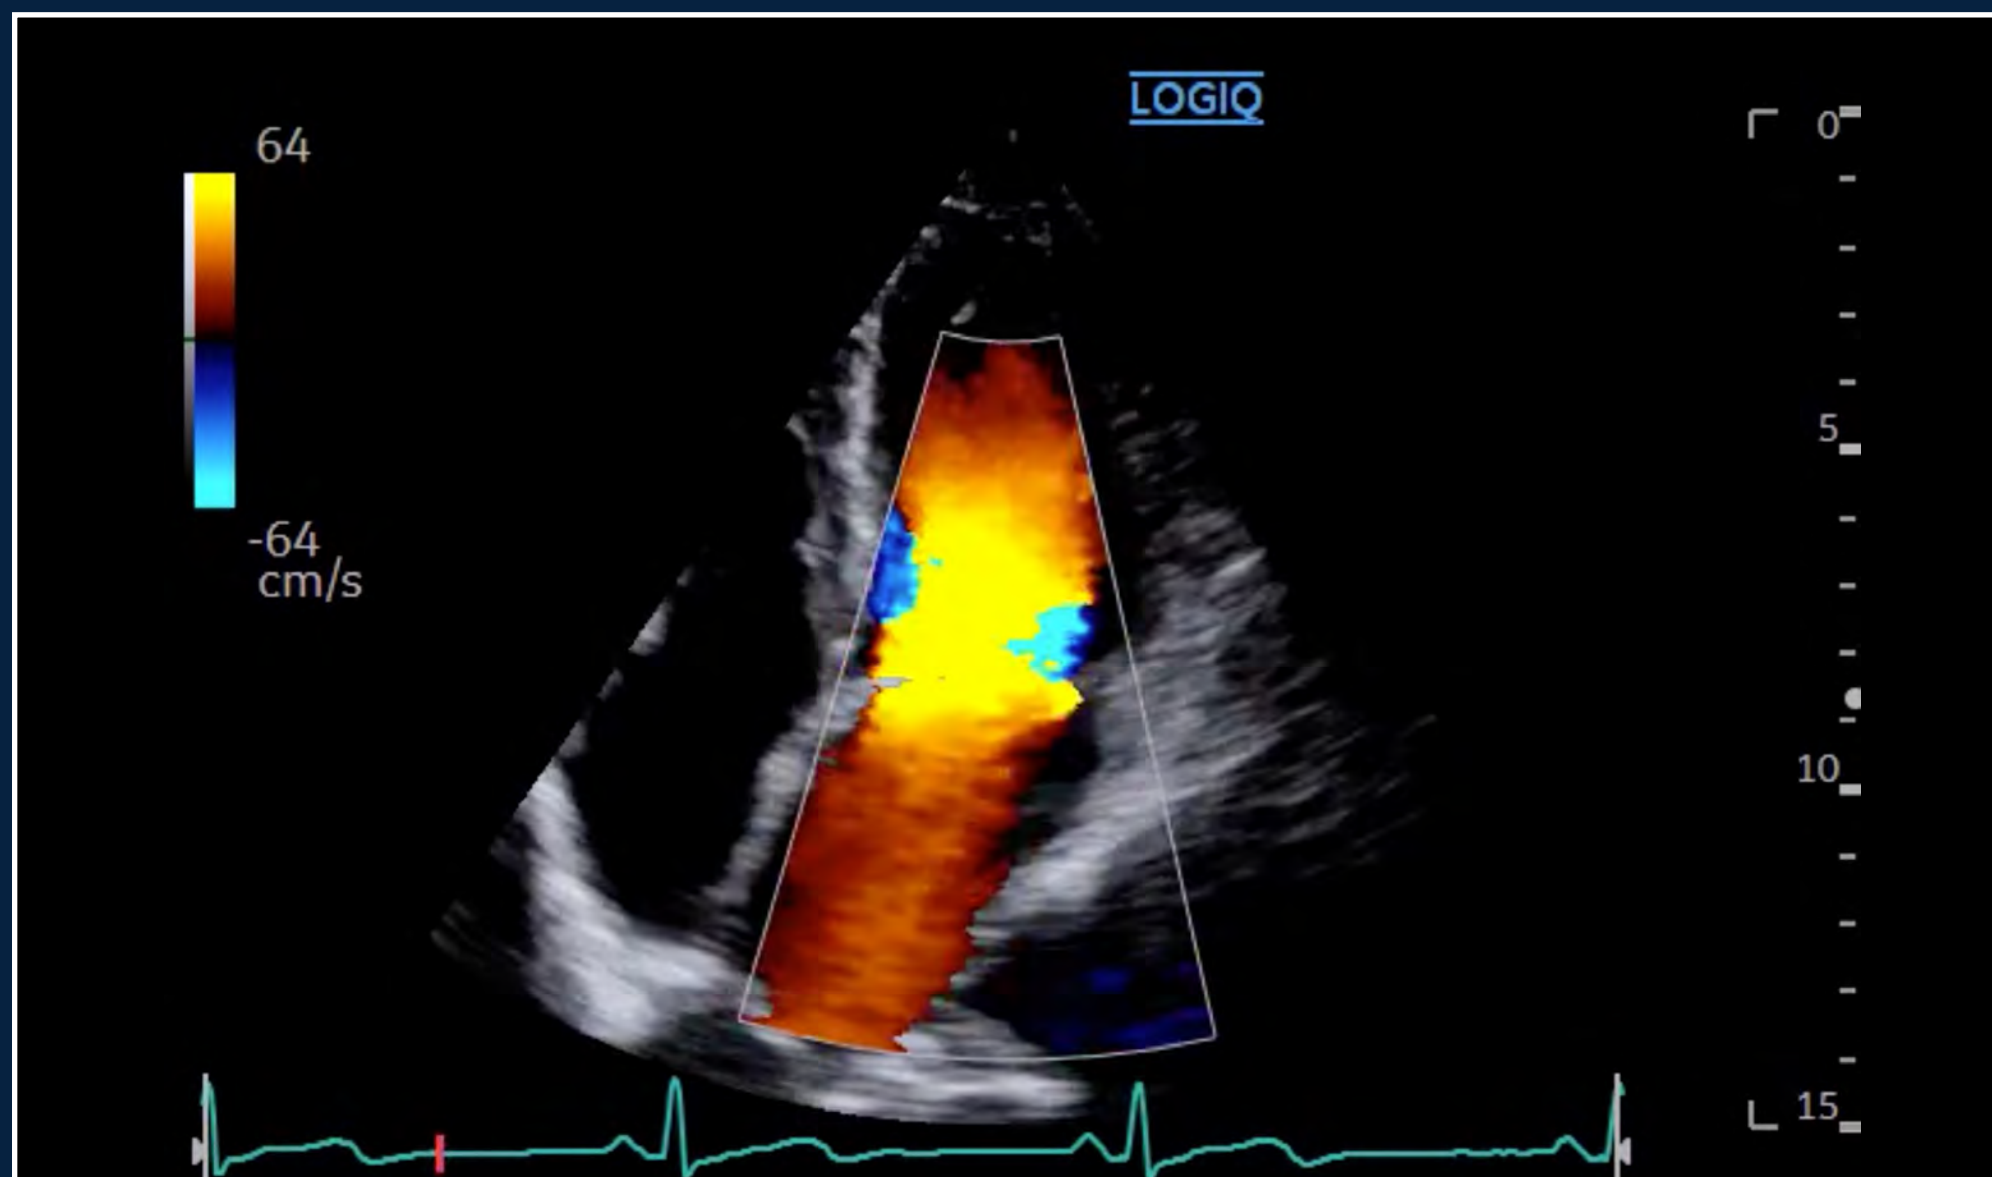

Color Flow Apical 4 Chamber View Mitral Valve, M5Sc-D

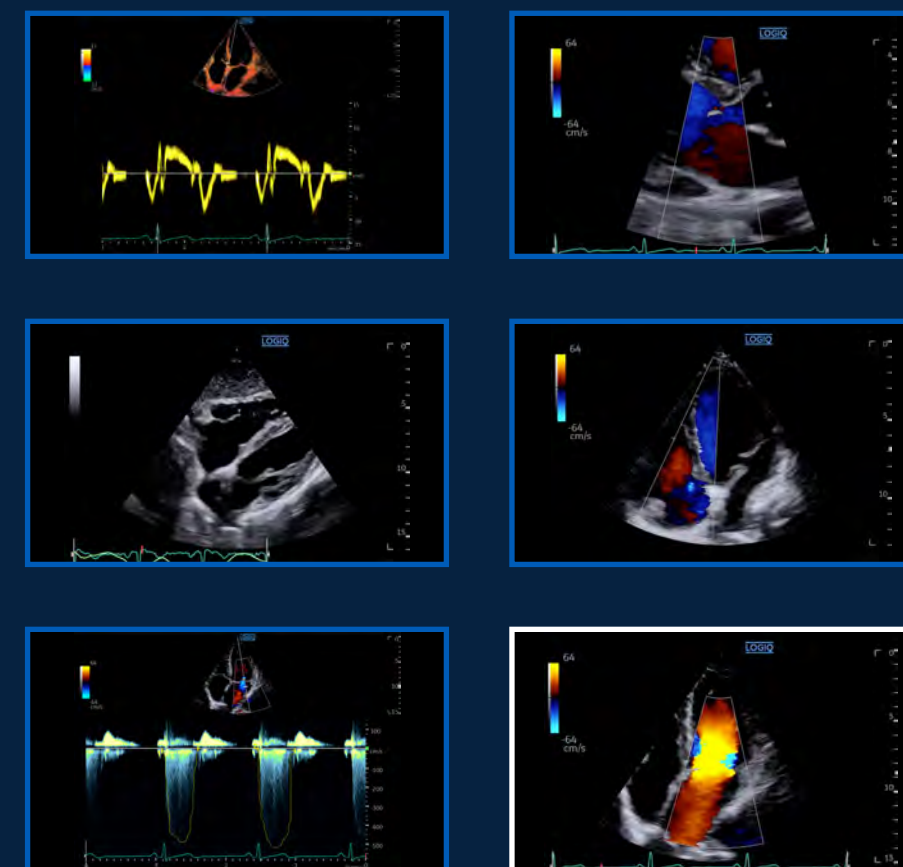



[OVERVIEW](#)[MULTI-PURPOSE/  
RADIOLOGY](#)[CARDIOLOGY](#)[MUSCULOSKELETAL](#)[BREAST](#)[PRODUCTIVITY](#)[INVESTMENT](#)[CONTACT](#)

# MUSCULOSKELETAL

With precise, efficient imaging, LOGIQ Fortis assists clinicians in managing a wide range of musculoskeletal conditions and a high volume of patients.

- Micro Vascular Imaging (MVI) and Radiant*flow* combine to enable near-3D visualization of tiny, slow-flow vessels
- 2D Shear Wave Elastography available on multiple probes
- Photo Assistant App lets you acquire and send photos of relevant anatomy from an Android™ device

[+ CLINICAL IMAGES](#)

LOGIQ Fortis





OVERVIEW

MULTI-PURPOSE/  
RADIOLOGY

CARDIOLOGY

**MUSCULOSKELETAL**

BREAST

PRODUCTIVITY




INVESTMENT

CONTACT

# CLINICAL IMAGES | Musculoskeletal



Excellent detail and contrast resolution to support in-depth understanding of tissue, pathology, blood flow, and inflammation

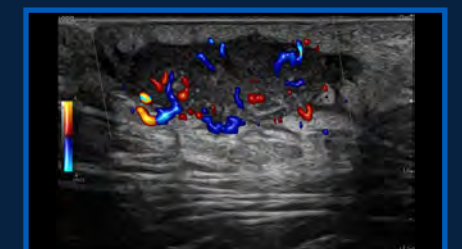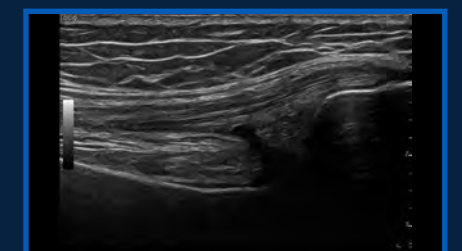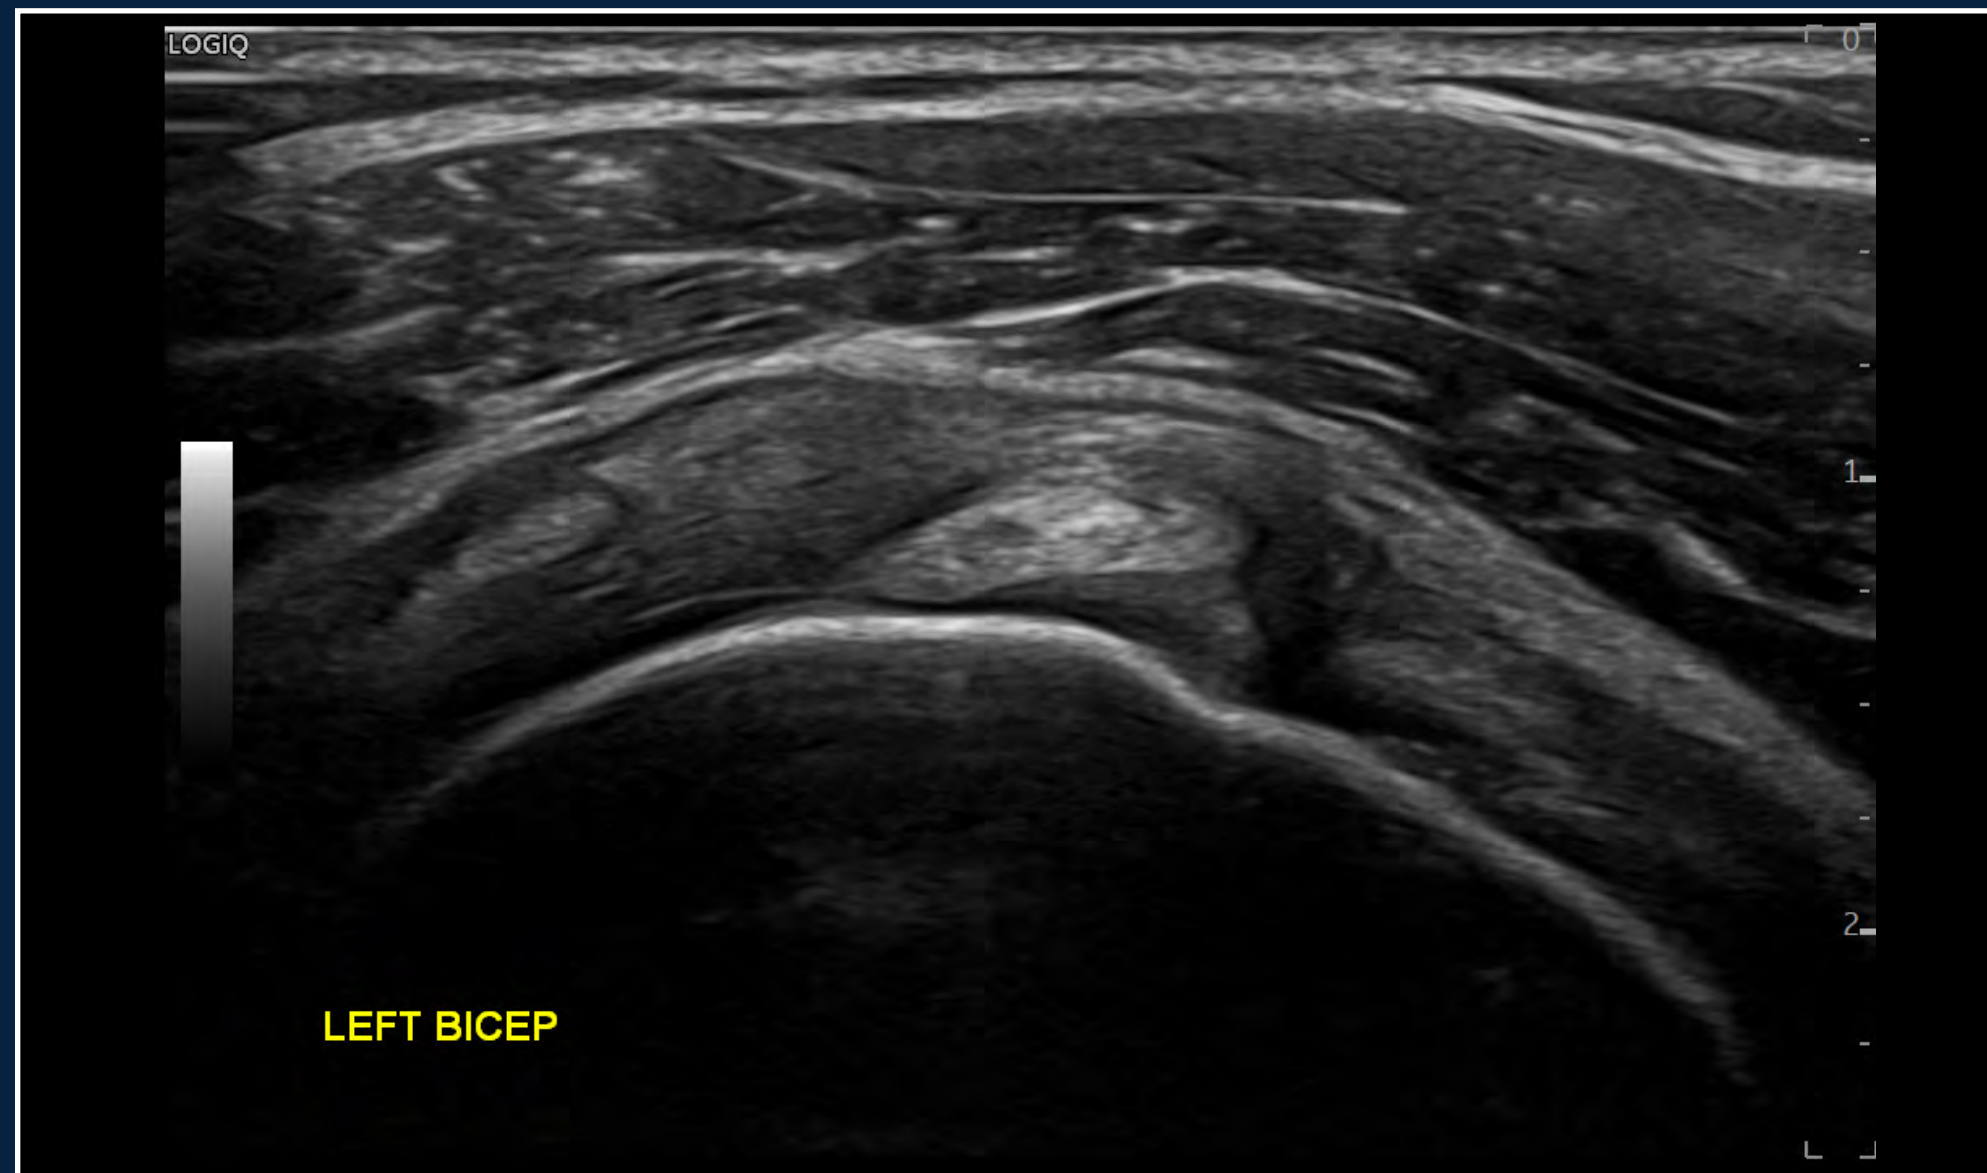

B-Mode with Advanced SRI Shoulder, ML6-15-D





OVERVIEW

MULTI-PURPOSE/  
RADIOLOGY

CARDIOLOGY

**MUSCULOSKELETAL**

BREAST

PRODUCTIVITY


INVESTMENT

CONTACT




# CLINICAL IMAGES | Musculoskeletal



Excellent detail and contrast resolution to support in-depth understanding of tissue, pathology, blood flow, and inflammation

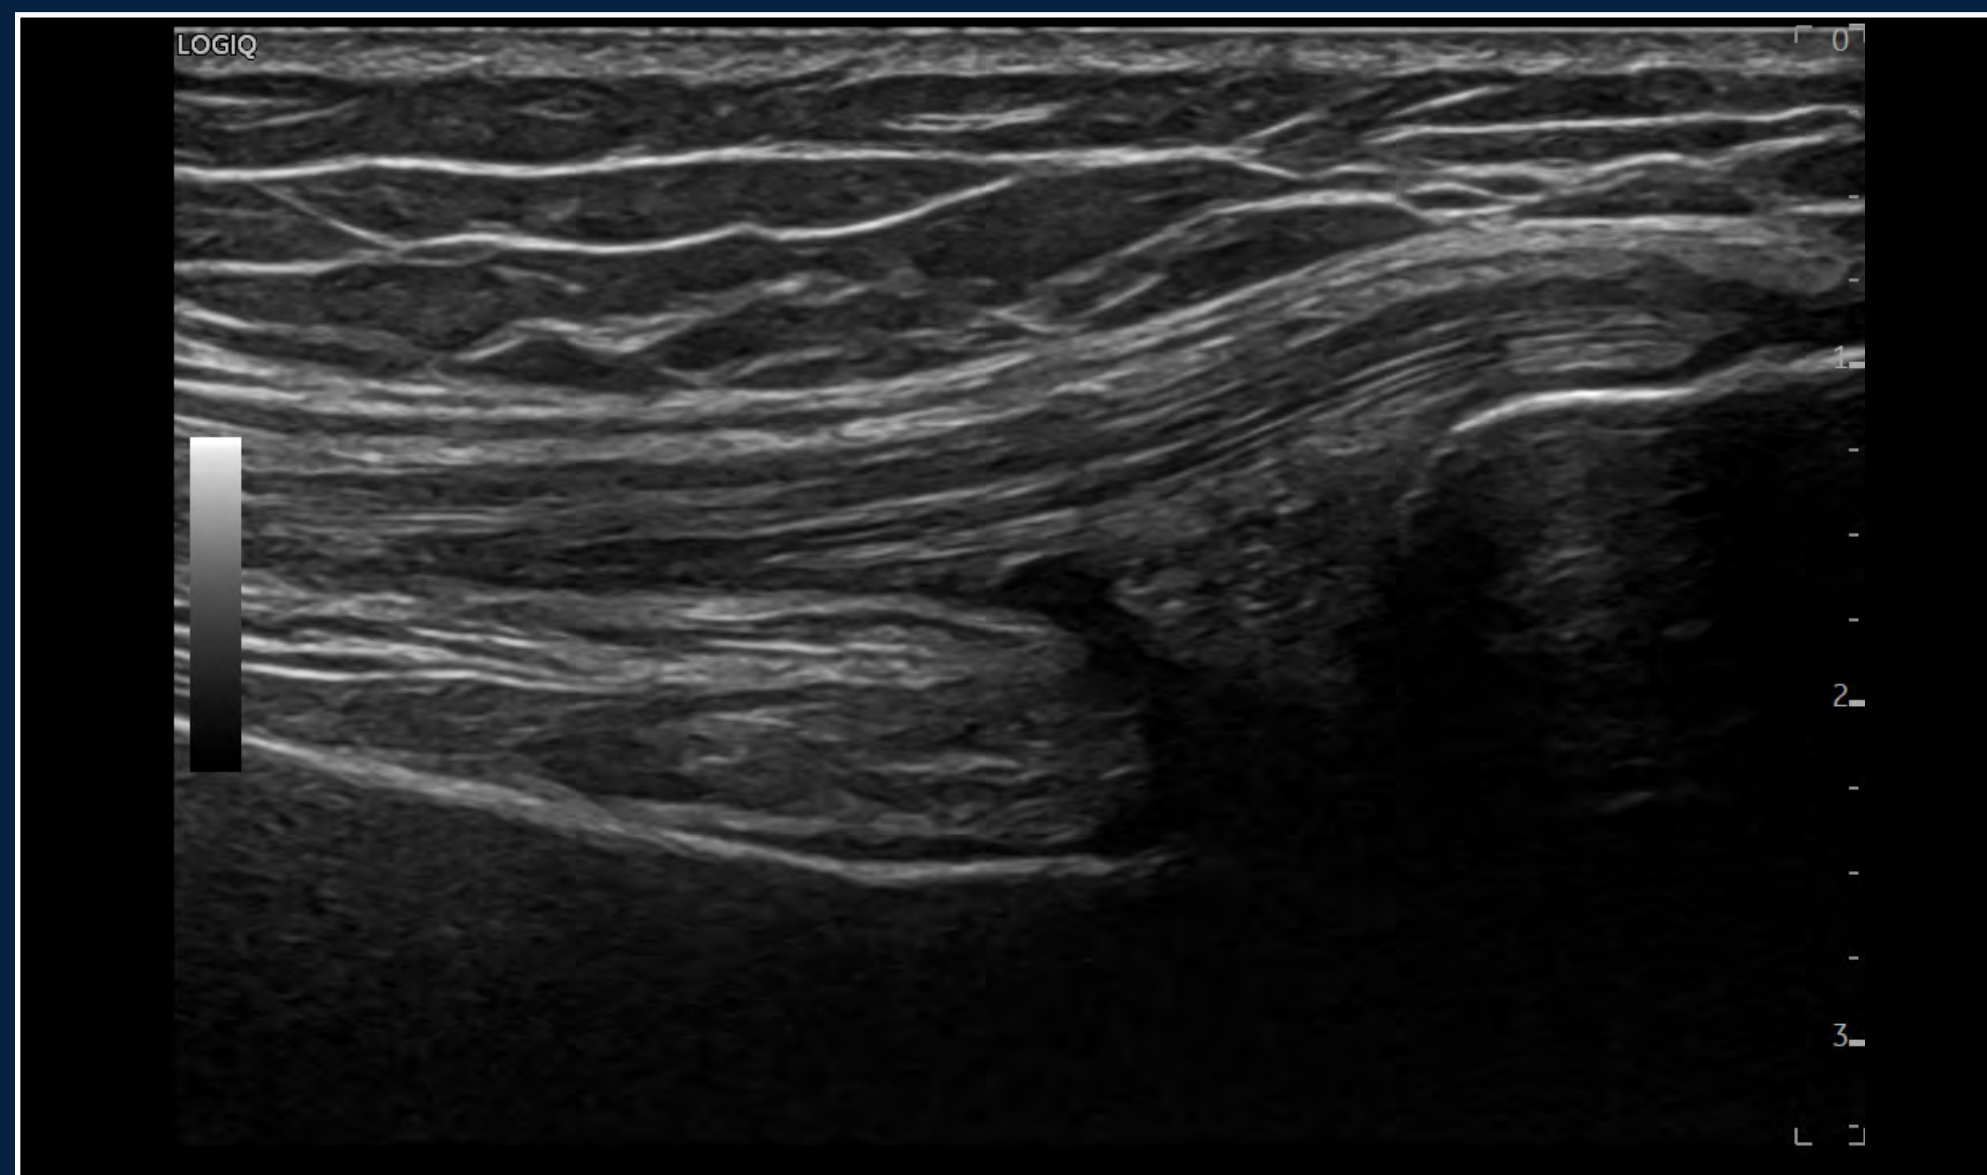

B-Mode with Advanced SRI Knee Tendon, ML6-15-D

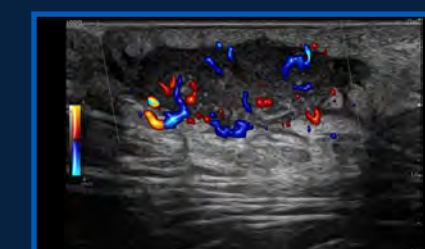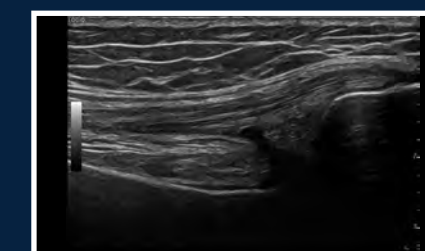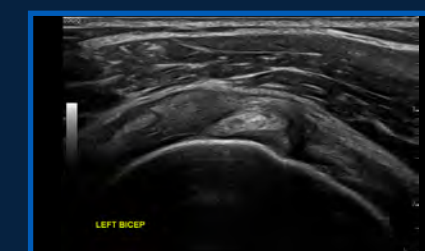





OVERVIEW

MULTI-PURPOSE/  
RADIOLOGY

CARDIOLOGY

MUSCULOSKELETAL

BREAST

PRODUCTIVITY


INVESTMENT

CONTACT





# CLINICAL IMAGES | Musculoskeletal



Excellent detail and contrast resolution to support in-depth understanding of tissue, pathology, blood flow, and inflammation

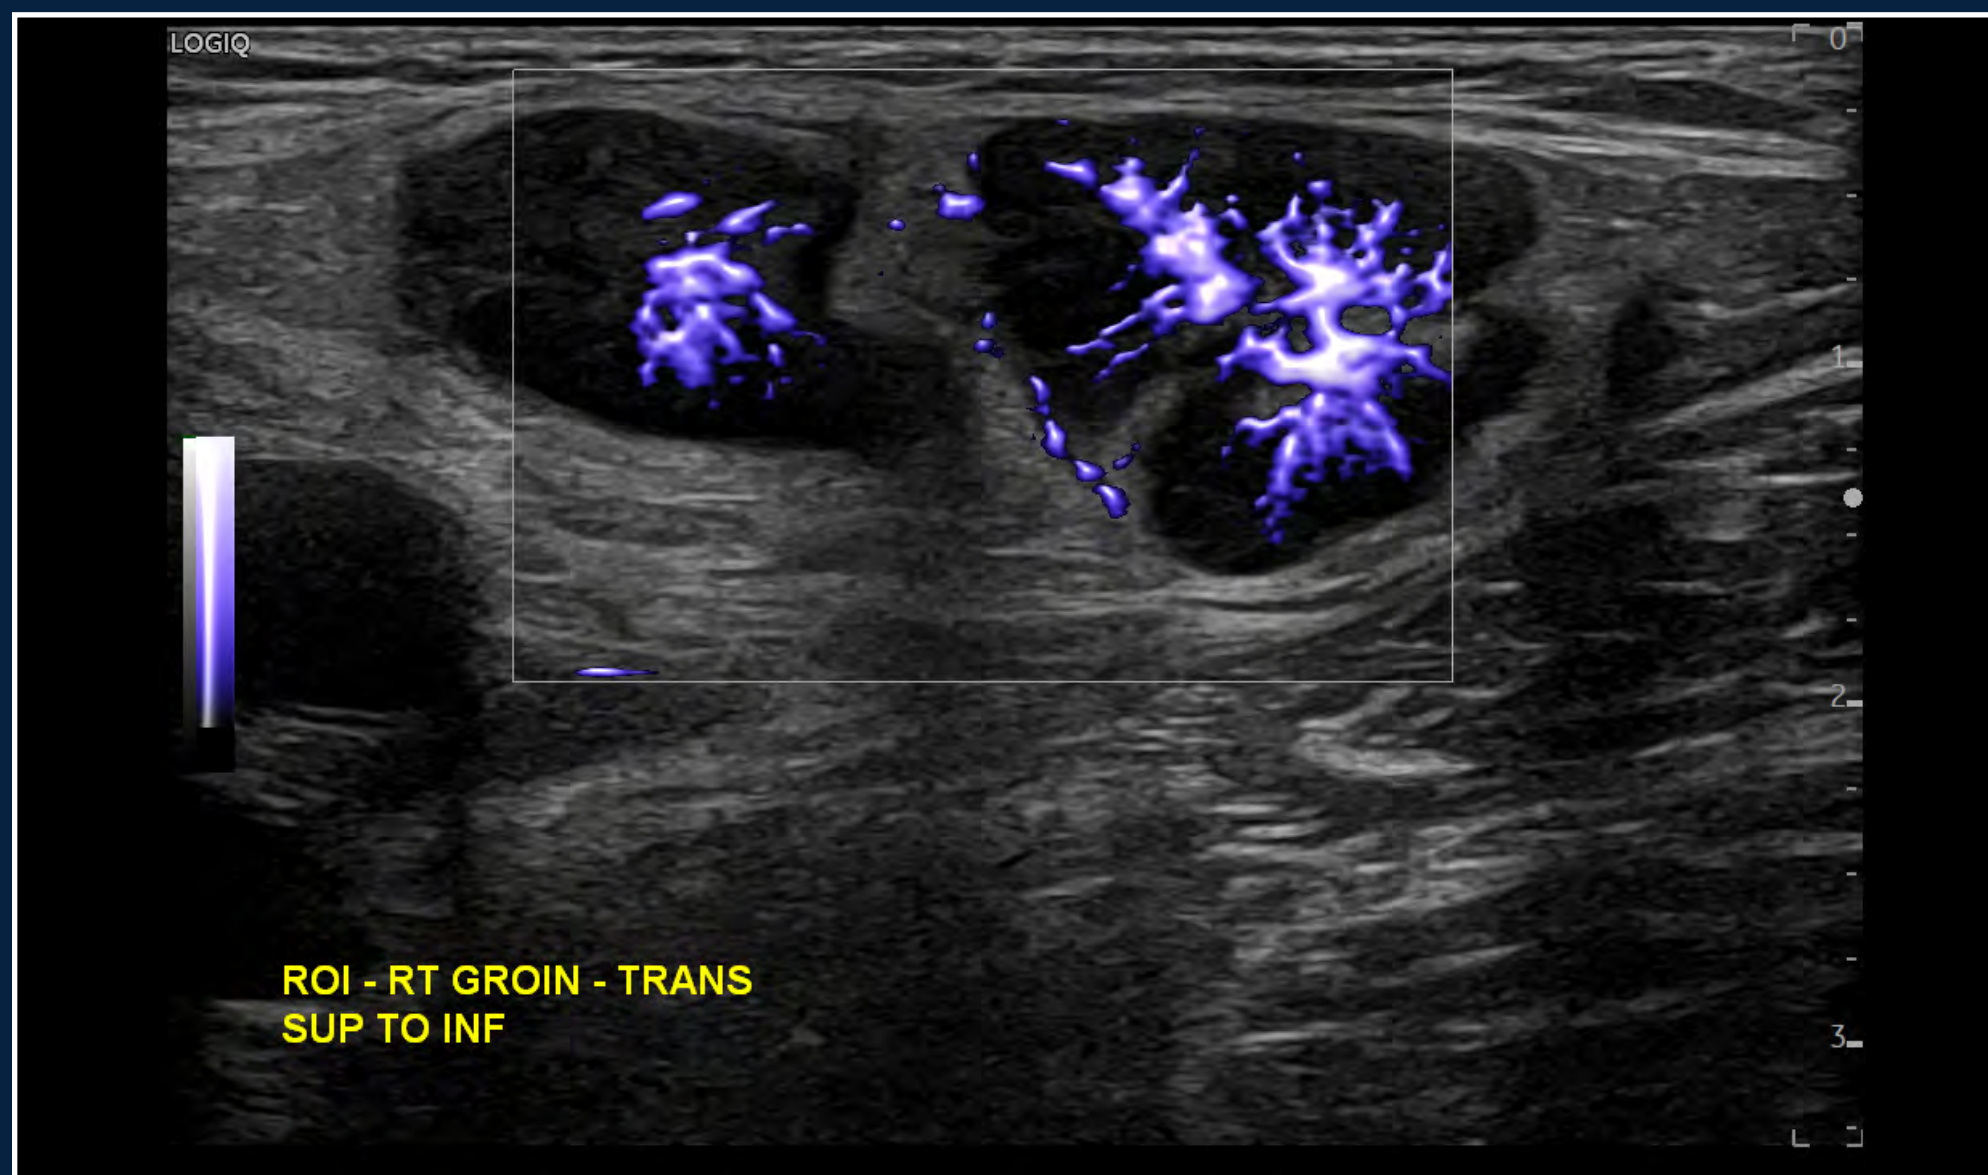

MVI with Radiantflow Groin Lymph Node, ML6-15-D

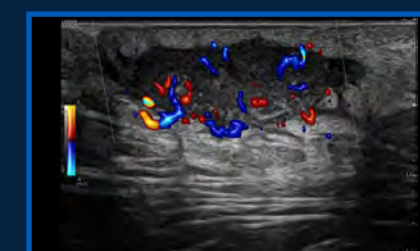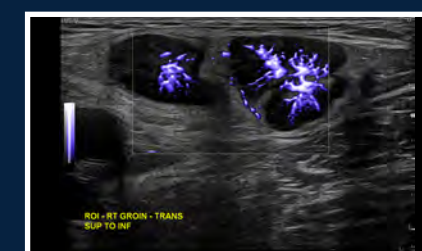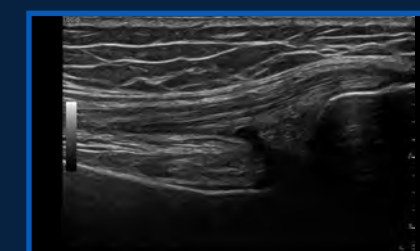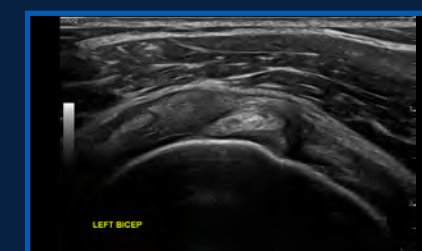





OVERVIEW

MULTI-PURPOSE/  
RADIOLOGY

CARDIOLOGY

MUSCULOSKELETAL

BREAST

PRODUCTIVITY


INVESTMENT

CONTACT




# CLINICAL IMAGES | Musculoskeletal



Excellent detail and contrast resolution to support in-depth understanding of tissue, pathology, blood flow, and inflammation

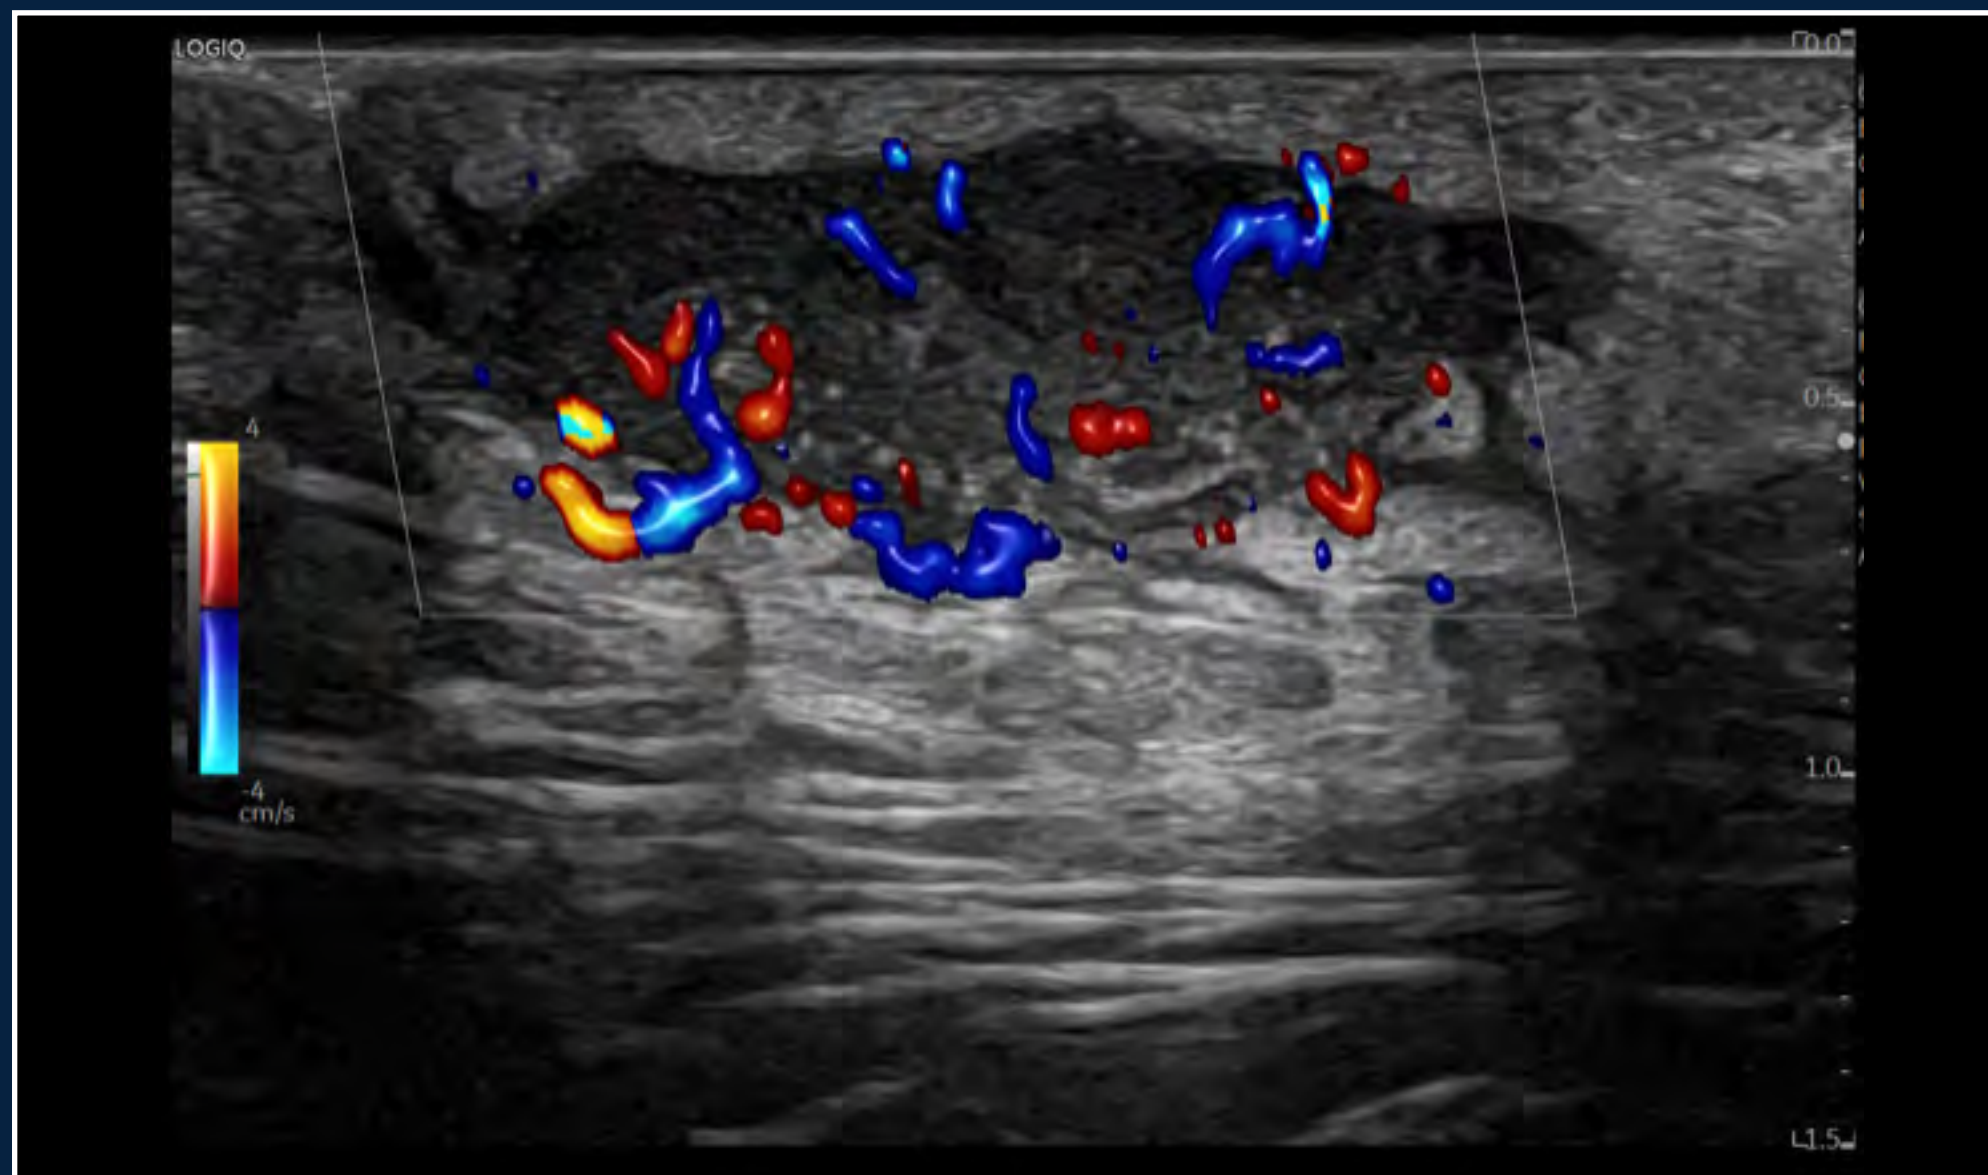

Leg Mass with Color Flow and Radiantflow, L6-24-D

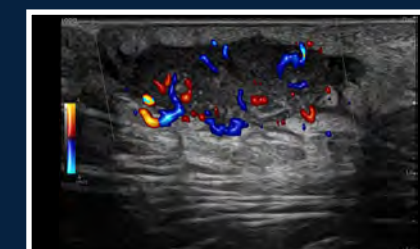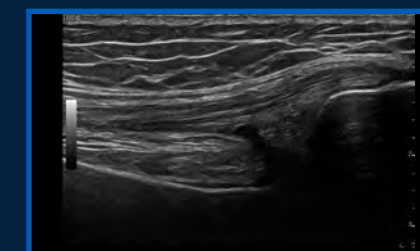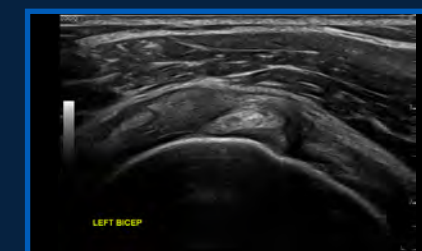



[OVERVIEW](#)[MULTI-PURPOSE/  
RADIOLOGY](#)[CARDIOLOGY](#)[MUSCULOSKELETAL](#)[BREAST](#)[PRODUCTIVITY](#)[INVESTMENT](#)[CONTACT](#)

# BREAST

LOGIQ Fortis provides high-quality images and robust tools to help clinicians detect and characterize breast disease as efficiently as possible.

- 2D Shear Wave Elastography with Quality Indicator
- Automated workflow tools, including Measure Assistant and Compare Assistant
- Breast Assistant, powered by Koios DS™, an AI-based decision support tool providing quantitative risk assessment aligned to a BI-RADS® category\*

[+ CLINICAL IMAGES](#)

LOGIQ Fortis





OVERVIEW

MULTI-PURPOSE/  
RADIOLOGY

CARDIOLOGY

MUSCULOSKELETAL

**BREAST**


PRODUCTIVITY

INVESTMENT



CONTACT

# CLINICAL IMAGES | Breast

Highly detailed images to detect and characterize breast disease efficiently

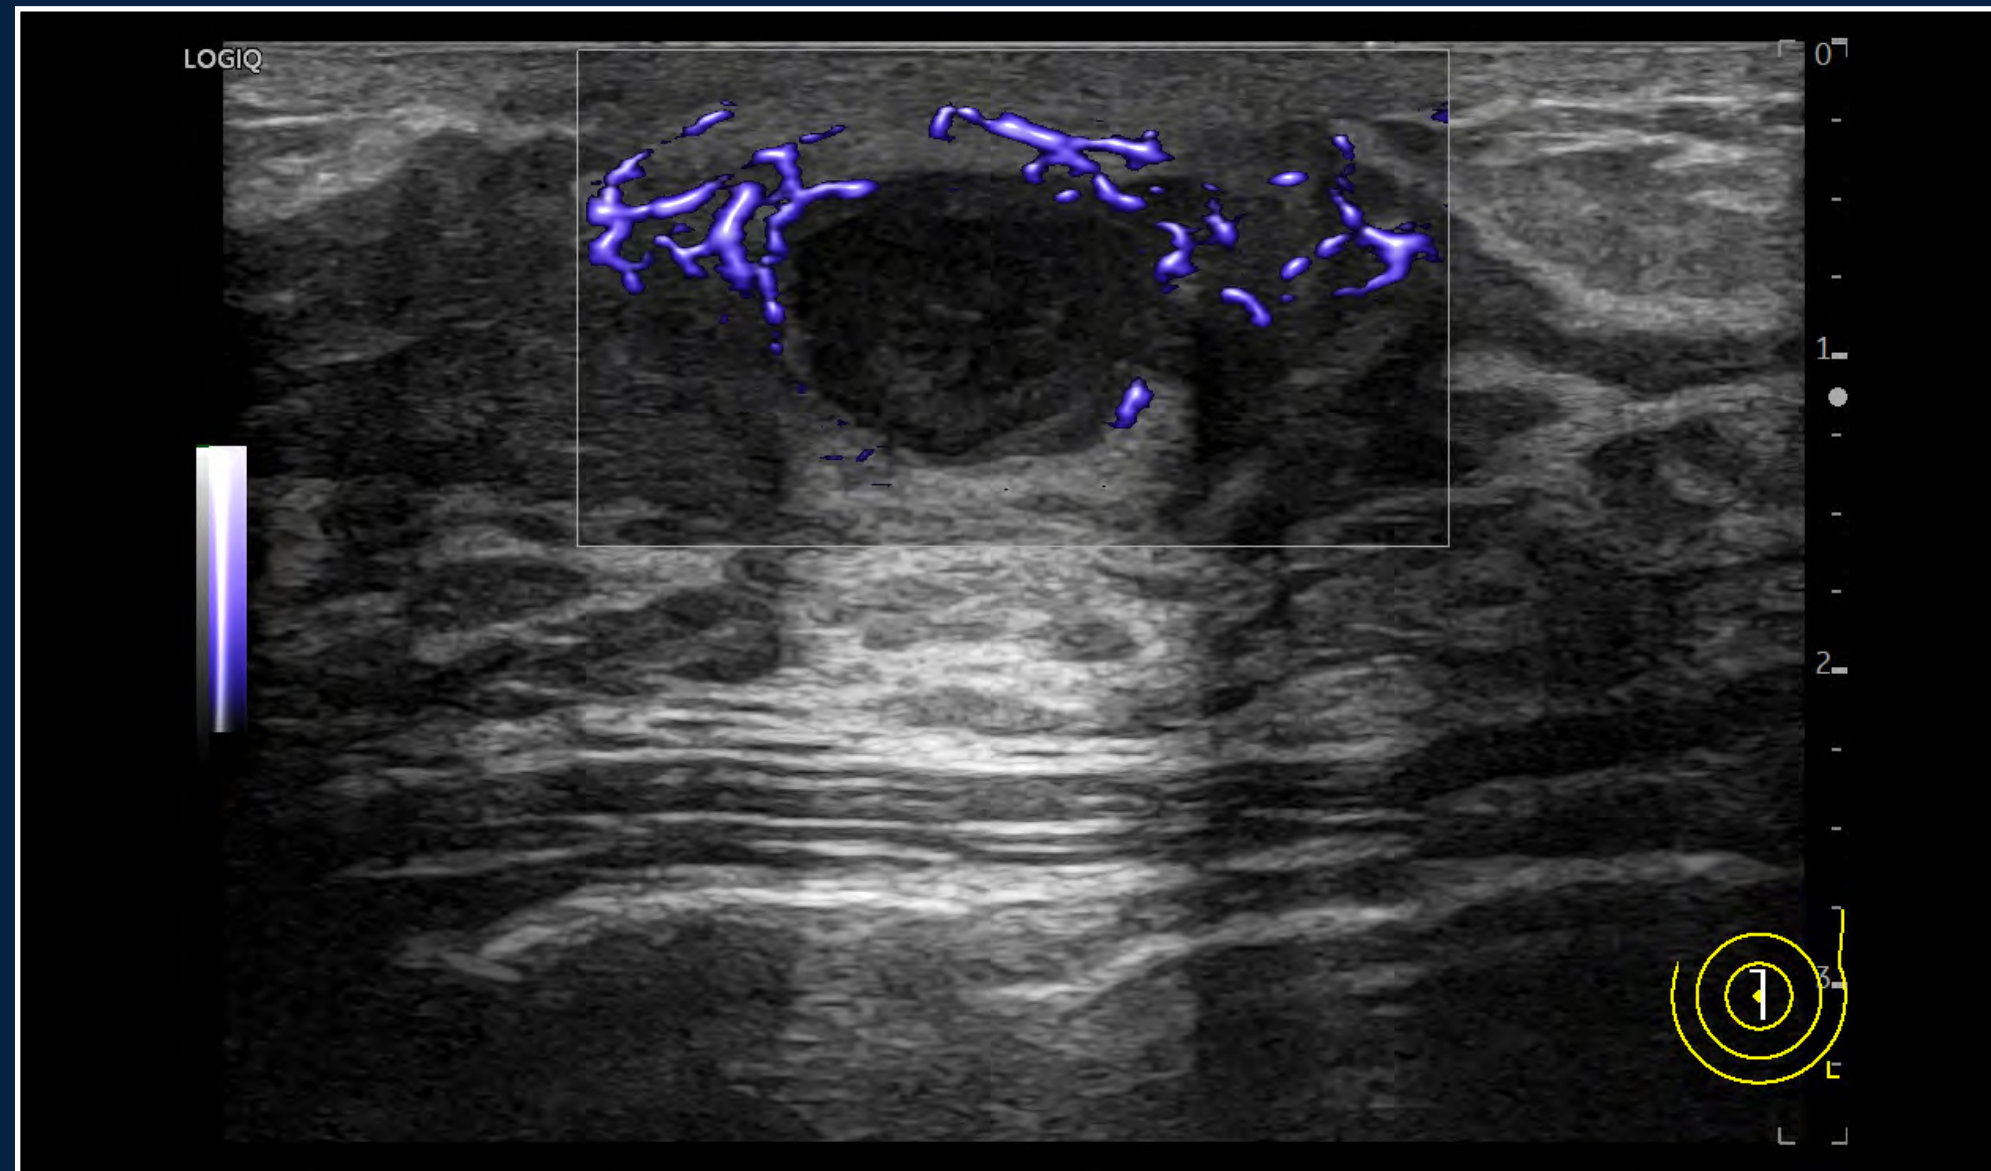

MVI Breast, ML6-15-D

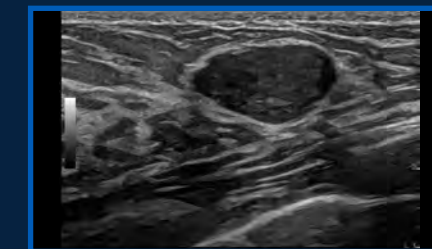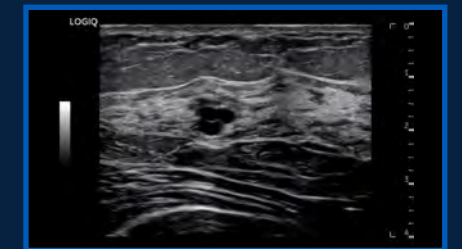





OVERVIEW

MULTI-PURPOSE/  
RADIOLOGY

CARDIOLOGY

MUSCULOSKELETAL

**BREAST**


PRODUCTIVITY

INVESTMENT




CONTACT

## CLINICAL IMAGES | Breast

Highly detailed images to detect and characterize breast disease efficiently

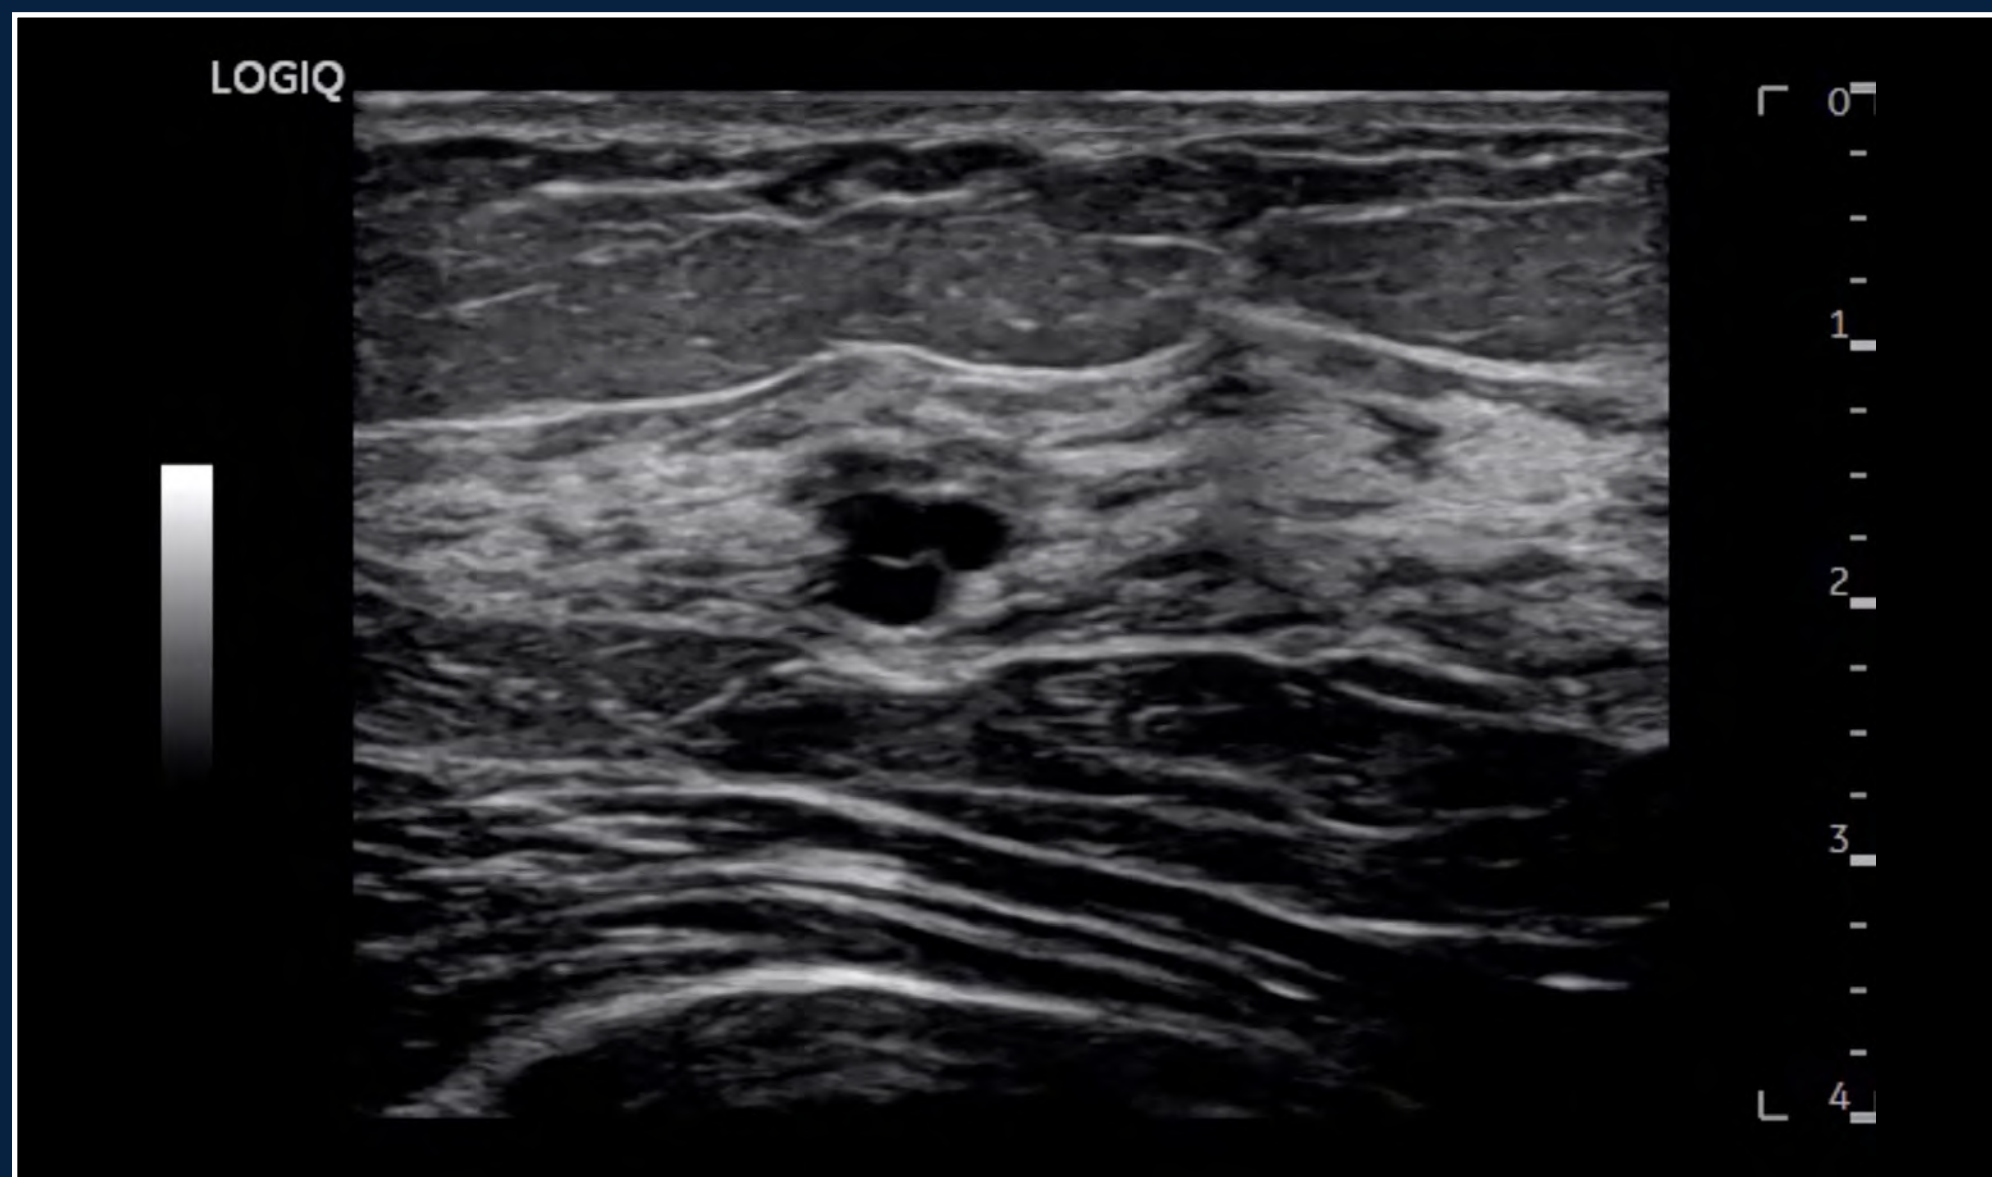

B-Mode with Advanced SRI in Breast, L3-12-D

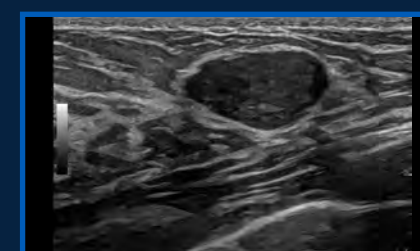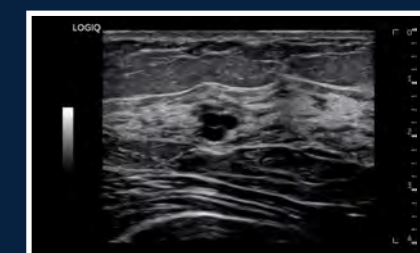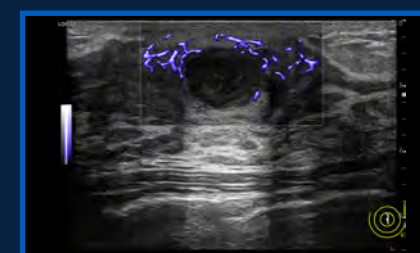





OVERVIEW

MULTI-PURPOSE/  
RADIOLOGY

CARDIOLOGY

MUSCULOSKELETAL

**BREAST**


PRODUCTIVITY

INVESTMENT



CONTACT

## CLINICAL IMAGES | Breast

Highly detailed images to detect and characterize breast disease efficiently

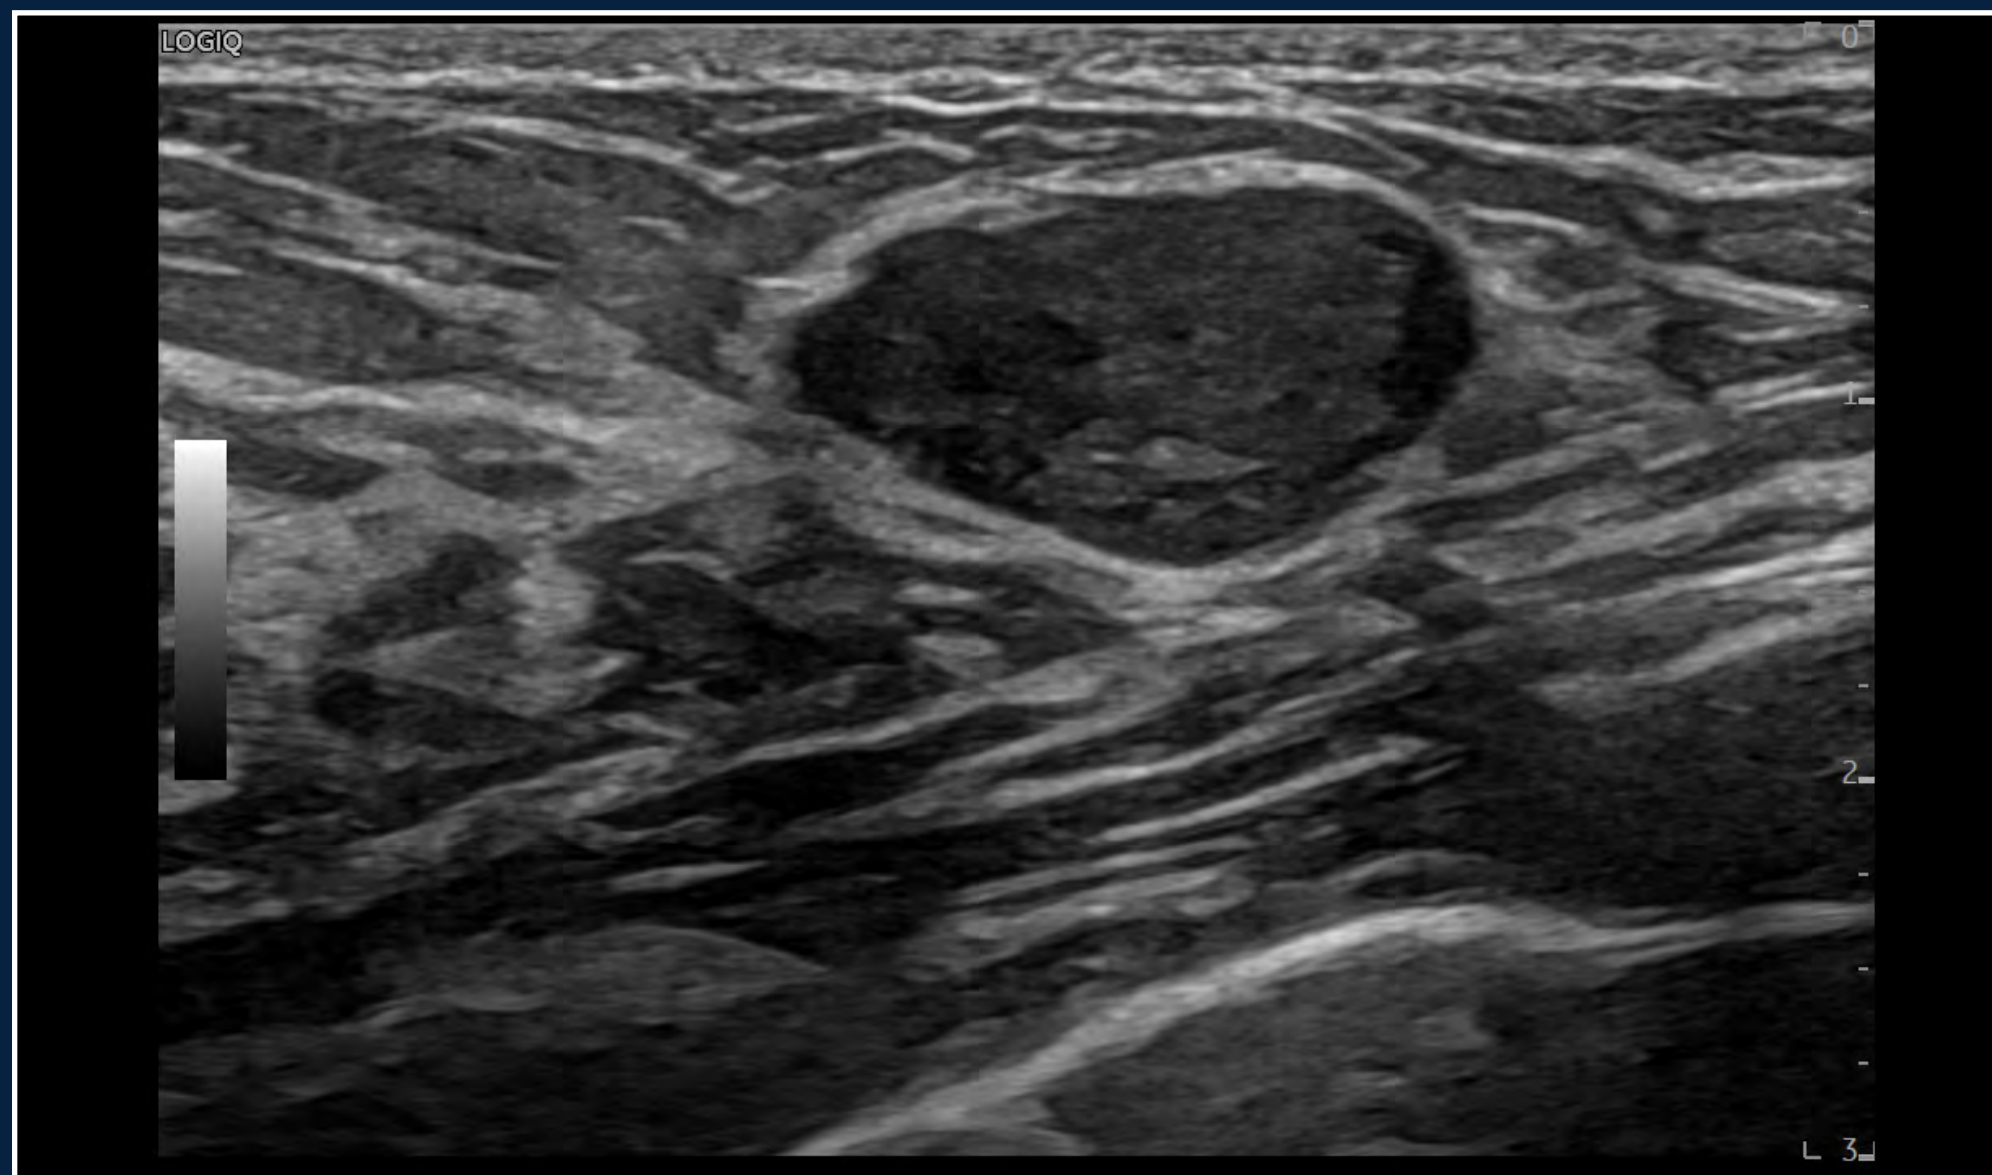

B-Mode with Advanced SRI in Breast, ML6-15-D

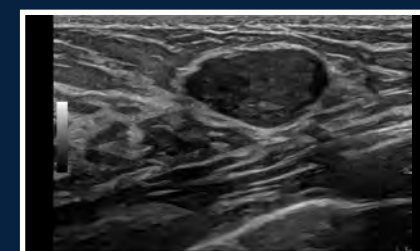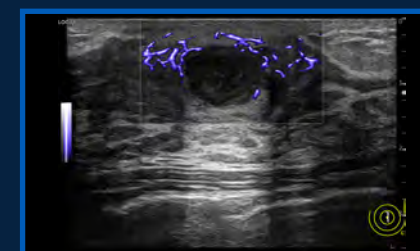



[OVERVIEW](#)[MULTI-PURPOSE/  
RADIOLOGY](#)[CARDIOLOGY](#)[MUSCULOSKELETAL](#)[BREAST](#)[PRODUCTIVITY](#)[INVESTMENT](#)[CONTACT](#)

# OPTIMIZING YOUR PRODUCTIVITY

LOGIQ Fortis is powerfully streamlined to help clinicians optimize workflow, ensure accurate results, and enhance clinical confidence.

- New EZ Imaging with customizable probe presets, simplified touch panel to reduce operator interactions, and quick patient set-up
- AI-based and automated tools to speed up workflow
- Easy system maneuverability with Scan on Battery

[COVID-19 Support](#)[Systems Cleaning Compatibility](#)[Transducers Cleaning Compatibility](#)[LOGIQ Club](#)

**LOGIQ Fortis**



[OVERVIEW](#)[MULTI-PURPOSE/  
RADIOLOGY](#)[CARDIOLOGY](#)[MUSCULOSKELETAL](#)[BREAST](#)[PRODUCTIVITY](#)[INVESTMENT](#)[CONTACT](#)

# MAXIMIZING YOUR INVESTMENT

From radiology to cardiology, the multi-purpose LOGIQ Fortis is easily scaled to your needs, so you can avoid acquiring multiple ultrasound systems for different requirements.

- A to A digital platform lets you add next-generation capabilities to stay at the forefront of ultrasound
- Lifecycle solutions—from InSite™ remote support to iCenter™ performance analytics—help optimize asset performance and utilization
- SonoDefense multi-layer cybersecurity and data privacy protection guards your investment 24/7



LOGIQ Fortis



[OVERVIEW](#)[MULTI-PURPOSE/  
RADIOLOGY](#)[CARDIOLOGY](#)[MUSCULOSKELETAL](#)[BREAST](#)[PRODUCTIVITY](#)[INVESTMENT](#)[CONTACT](#)

## LOGIQ Fortis

A powerful, streamlined ultrasound solution that's always ready, always by your side.

For more information, visit the [LOGIQ Digital Experience](#).

\* Not all products or features are available in all geographies.  
Check with your local GE Healthcare representative for availability in your country.

Product may not be available in all countries and regions. Full product technical specification is available upon request. Contact a GE Healthcare Representative for more information. Please visit [www.gehealthcare.com/promotional-locations](http://www.gehealthcare.com/promotional-locations).

Data subject to change.

© GE, 2022

GE, the GE Monogram, LOGIQ Fortis, cSound, XDclear, Radiantflow, InSite, and iCenter are trademarks of GE. Android is a trademark of Google, Inc. Koios DS is a trademark of Koios Medical. BI-RADS is a registered trademark of the American College of Radiology. All other third-party trademarks are the property of their respective owners.

Reproduction in any form is forbidden without prior written permission from GE. Nothing in this material should be used to diagnose or treat any disease or condition. Readers must consult a healthcare professional.

January 2022  
JB18811XX







# LOGIQ Fortis™

## Data sheet



The LOGIQ Fortis is GE's premium ultrasound imaging system designed for general imaging applications including abdominal, vascular, obstetric, gynecologic, neonatal, pediatric, urological, transcranial, cardiac, and small parts applications.



# General specifications

## Dimensions and weight

*(Dimensions given with floating keyboard stowed and display tilted for transport)*

Height	1250 – 1800 mm, 49 – 71"
Width	530 mm, 20.9" (Caster) 565 mm, 22.2" (Monitor)
Depth	885 mm, 34.8"
Weight	85 kg (187.4 lb)

## Electrical power

Voltage 100 – 240 VAC

Frequency 50/60 Hz

Power consumption maximum of 0.9 KVA with peripherals

## Console design

4 active probe ports

1 inactive probe storage port

Integrated SSD (1 TB)

Integrated DVD-R Multi Drive

On-board storage of thermal printer

Integrated speaker

Integrated locking mechanism that provides rolling lock and caster swivel lock

Integrated cable management

Front and rear handles

Easily removable air filters

# User interface

## Operator keyboard

Operating keyboard, adjustable in height and rotation

Ergonomic hard key layout

Interactive back-lighting

Integrated recording keys for remote control of up to 4 peripheral or DICOM® devices

Integrated gel warmer

## Touch screen

12.1" High-resolution, color, touch display screen

Interactive dynamic software menu

Brightness adjustment

User-configurable layout

## Display monitor

23.8" Widescreen high-resolution HDU Display

Display translation (independent of console)

350 mm (13.7") horizontal (both directions)

120 mm (4.7") vertical

90° swivel (both directions)

Fold-down and lock mechanism for transportation

Resolution: 1920 x 1080

Anti-glare

Viewing angle 89/89/89/89°

# System overview

## Applications

Abdominal

Obstetrical

Gynecological

Breast

Small Parts

Peripheral Vascular

Transcranial (adult and neonatal)

Pediatric and Neonatal

Musculoskeletal (general and superficial)

Urological

Cardiac (adult and pediatric)

Interventional

Pleural



# System overview *(cont.)*

## Operating modes

B-Mode

M-Mode

Color Flow Mode (CFM)

B-Flow™ (Option)

Extended Field of View (LOGIQ View)

Power Doppler Imaging (PDI)

PW Doppler

CW Doppler (Option)

Volume Modes (3D/4D) (Option)	<ul style="list-style-type: none"><li>• 3D Static</li><li>• 4D Real Time</li></ul>
----------------------------------	--

Anatomical M-Mode

Coded Contrast Imaging (Option)

Strain Elastography (Option)

B-Steer+ (Option)

Shearwave Elastography (Option)

UGAP (Option)

## Scanning methods

Electronic sector

Electronic convex

Electronic linear

Mechanical volume sweep

## Probe types

Sector phased array

Convex array

Micro convex array

Linear array

Matrix array

Volume probes (4D)

Split crystal

## System standard features

Advanced user interface with high-resolution 12.1" display touch panel

Automatic optimization

CrossXBeam™

Speckle Reduction Imaging (SRI-HD, Advanced SRI Type 1)

Fine angle steer

Coded harmonic imaging

Virtual convex

Patient information database

Image archive on integrated CD/DVD and hard drive

Advanced 3D

Real-time automatic Doppler calculations

OB calculations

Fetal trending

Multigestational calculations

Hip dysplasia calculations

Gynecological calculations

Vascular calculations

Urological calculations

Renal calculations

Cardiac calculations

InSite™ capability

On-board electronic documentation

Auto CF/PW positioning feature

Privacy and security, including user and rights management

LOGIQView

Breast productivity package (Option)

Thyroid productivity package (Option)

External USB printer connection

Network printer support

HDMI output (available for compatible devices)



# System overview *(cont.)*

## Options

Tricefy®

DICOM

B-Flow

Auto IMT

Compare assistant

Scan assistant

OB measure assistant

Color quantification

Strain Elastography

Elastography quantification

Advanced privacy and security (vulnerability scan)

Power assistant and scan on battery

Storage bins

Shear wave elastography

Volume navigation

UGAP

Hepatic assistant

Coded Contrast Imaging

Stress echo

Cardiac Strain (Automatic Function Imaging)

On-board reporting

TVI

Wireless LAN

CW

DVR

Tablet tools

Advanced probes

KOIOS

SonoNT SonoIT

Advanced SRI Type 2

## Peripheral options

Integrated options for

- Digital B&W thermal printer
- DVD video recorder

Digital color thermal printer

Digital A6 color thermal printer

Foot switch with programmable functionality

Console protective cover

LOGIQ smart device apps

- Photo Assistant
- Remote Control

CRF-200U card reader (for Japan)

## Display modes

Live and stored display format

- Full size and split screen – both w/ thumbnails. For still and CINE.

Review image format

- 4x4, and thumbnails. For still and CINE.

Timeline display

- Independent Dual B or CrossXBeam/PW Display
- CW
- Top/bottom selectable display format
- Side/side selectable format

Virtual convex

## Simultaneous capability

B or CrossXBeam/PW

B or CrossXBeam/CW (Option)

B or CrossXBeam/CFM or PDI

B/M

B/CrossXBeam

B-Flow/PW

Real-time Triplex Mode

B or CrossXBeam + CFM or PDI/PW

## Selectable alternating modes

B or CrossXBeam/PW

B or CrossXBeam + CFM (PDI)/PW

B/CW (Option)



# System overview *(cont.)*

## Multi-image (split/quad screen)

Live and/or frozen
B or CrossXBeam + B or CrossXBeam/CFM or PDI
PW/M
Independent CINE playback

## Display annotation

Patient name: first, last, and middle		
Patient ID		
Alternate patient ID		
Age, sex, and date of birth		
Hospital name		
Date format: three types selectable	<ul style="list-style-type: none"><li>• MM/DD/YY</li><li>• YY/MM/DD</li></ul>	<ul style="list-style-type: none"><li>• DD/MM/YY</li></ul>
Time format: two types selectable	<ul style="list-style-type: none"><li>• 24 hours</li></ul>	<ul style="list-style-type: none"><li>• 12 hours</li></ul>
Gestational age from	<ul style="list-style-type: none"><li>• LMP</li><li>• EDD</li></ul>	<ul style="list-style-type: none"><li>• GA</li><li>• BBT</li></ul>
Probe name		
Map names		
Probe orientation		
Depth scale marker		
Lateral scale marker		
Image depth		
Zoom depth		
B-Mode	<ul style="list-style-type: none"><li>• Gain</li><li>• Imaging frequency</li><li>• Gray map</li></ul>	<ul style="list-style-type: none"><li>• Dynamic range</li><li>• Frame averaging</li><li>• SRI-HD</li></ul>
M-Mode	<ul style="list-style-type: none"><li>• Gain</li><li>• Time scale</li></ul>	<ul style="list-style-type: none"><li>• Dynamic range</li></ul>
Doppler Mode	<ul style="list-style-type: none"><li>• Gain</li><li>• Sample volume depth and width</li><li>• Spectrum inversion</li><li>• Time scale</li><li>• Doppler frequency</li></ul>	<ul style="list-style-type: none"><li>• Angle</li><li>• Wall filter</li><li>• Velocity and/or frequency scale</li><li>• PRF</li></ul>

## Display annotation *(cont.)*

Color Flow Doppler Mode	<ul style="list-style-type: none"><li>• Line density</li><li>• Frame averaging</li><li>• Color Scale, 3 types: power, directional PDI, and symmetrical velocity imaging</li><li>• Color velocity range and baseline</li><li>• Color threshold marker</li><li>• Color gain</li><li>• PDI</li><li>• Spectrum inversion</li><li>• Doppler frequency</li></ul>
TGC curve	
Acoustic frame rate	
CINE gage, image number/frame number	
Body pattern: multiple human and animal types	
Application name	
Measurement results	
Operator message	
Displayed acoustic output	<ul style="list-style-type: none"><li>• TIS: Thermal Index Soft Tissue</li><li>• TIC: Thermal Index Cranial (Bone)</li><li>• TIB: Thermal Index Bone</li><li>• MI: Mechanical Index</li></ul>
% of maximum power output	
Biopsy guideline and zone	
Heart rate	

# General system parameters

## System setup

Pre-programmed categories
User programmable preset capability
Factory default preset data
Languages: English, French, German, Spanish, Italian, Brazilian Portuguese, Russian, Greek, Swedish, Danish, Dutch, Finnish, Norwegian
OB report formats including Tokyo Univ., Osaka Univ., USA, Europe, ASUM, and WHO
User defined annotations
Body patterns
Customized comment home position
EZ Imaging: Simplified user interface for high volume workflow



# General system parameters *(cont.)*

## Complete user manual available on-board through Help (F1)

User manual and service manual are included on USB with each system. A printed manual is available upon request.

## CINE memory/image memory

1 GB of CINE memory

Selectable CINE sequence for CINE review

Prospective CINE mark

Measurements/calculations and annotations on CINE playback

Scrolling timeline memory

Dual Image CINE display

Quad Image CINE display

CINE gauge and CINE image number display

CINE review loop

CINE review speed

## Image storage

On-board database of patient information from past exams

Storage formats: DICOM	<ul style="list-style-type: none"><li>• Compressed/uncompressed</li><li>• Single/multi-frame</li><li>• Enhanced (3D/4D)</li><li>• With/without raw data</li></ul>
---------------------------	---

Export JPEG, JPEG 2000, WMV (MPEG 4) formats

Storage devices	<ul style="list-style-type: none"><li>• USB memory stick: 64 MB to 64 GB (for exporting individual images/clips)</li><li>• CD-R storage: 700 MB</li><li>• DVD storage: -R (4.7 GB)</li><li>• Hard drive image storage: ~730GB</li></ul>
-----------------	---

Compare previous exam images with current exam

Reload of archived data sets

## Connectivity

Ethernet network connection

Wireless LAN 802.11ac/a/b/g/n (Option)

DICOM 3.0	<ul style="list-style-type: none"><li>• Verify</li><li>• Print</li><li>• Store</li><li>• Modality worklist</li><li>• Storage commitment</li><li>• Modality performed procedure step (MPPS)</li><li>• Media exchange</li><li>• Off network/mobile storage queue</li><li>• Query/retrieve</li></ul>
-----------	---

Public SR template

Structured Reporting – compatible with vascular, OB, cardiac, and breast standard

InSite capability

Advanced privacy and security (Option)

## Physiological input panel (Option)

Physiological input	<ul style="list-style-type: none"><li>• ECG, 1 channel</li><li>• PCG, 1 channel</li><li>• AUX, 1 channel</li><li>• Dual R-Trigger</li><li>• Pre-settable ECG R delay time</li><li>• Pre-settable ECG position</li><li>• Adjustable ECG gain control</li><li>• Pre-settable PCG position</li><li>• Adjustable PCG gain control</li><li>• Pre-settable AUX position</li><li>• Adjustable AUX gain control</li></ul>
---------------------	---

Automatic heart rate display

Auto Ejection Fraction

## Report writer (Option)

On-board reporting package automates report writing

Formats various exam results into a report suitable for printing or reviewing on a standard PC

Exam results include patient info, exam info, measurements, calculations, images, and comments with standard templates provided

Customizable templates



# General system parameters *(cont.)*

## Scanning parameters

Displayed imaging depth: 0 – 100 cm

Minimum depth of field: 0 – 2 cm (zoom) (probe dependent)

Maximum depth of field: 0 – 100 cm (probe dependent)

Continuous dynamic receive focus/continuous dynamic receive Aperture

Adjustable dynamic range      Adjustable field of view (FOV)

Image reverse: right/left

Image rotation of 0°, 90°, 180°, 270°

## Digital B-Mode

Adjustable	<ul style="list-style-type: none"><li>• Acoustic power</li><li>• Dynamic range</li><li>• Gray scale map</li><li>• Speed of sound (application dependent)</li><li>• Scanning size (FOV or Angle) – Probe type dependent; consult individual probe specifications</li></ul>	<ul style="list-style-type: none"><li>• Gain</li><li>• Frame averaging</li><li>• Frequency</li><li>• Frame rate</li><li>• CrossXBeam</li><li>• B colorization</li><li>• Reject</li><li>• Suppression</li><li>• SRI-HD</li></ul>
------------	---	---

## Digital M-Mode

Adjustable	<ul style="list-style-type: none"><li>• Acoustic power</li><li>• Dynamic range</li><li>• Frequency</li><li>• M colorization</li><li>• Rejection</li></ul>	<ul style="list-style-type: none"><li>• Gain</li><li>• Gray scale map</li><li>• Sweep speed</li><li>• M display format</li></ul>
------------	---	--

## Anatomical M-Mode

M-Mode cursor adjustable at any plane

Can be activated from a CINE loop from a live or stored image

M & A capability

Available with Color Flow Mode

## Digital Spectral Doppler Mode

Adjustable	<ul style="list-style-type: none"><li>• Acoustic power</li><li>• Dynamic range</li><li>• Transmit frequency</li><li>• PW colorization</li><li>• Sweep speed</li><li>• Sample volume length</li><li>• Spectrum inversion</li><li>• Baseline shift</li><li>• Time resolution</li><li>• Trace direction</li></ul>	<ul style="list-style-type: none"><li>• Gain</li><li>• Gray scale map</li><li>• Wall filter</li><li>• Velocity scale range</li><li>• Angle correction</li><li>• Steered linear</li><li>• Trace method</li><li>• Doppler auto trace</li><li>• Compression</li><li>• Trace sensitivity</li></ul>
------------	--	--

## Digital Color Flow Mode

Adjustable	<ul style="list-style-type: none"><li>• Acoustic power</li><li>• Gain</li><li>• Velocity scale range</li><li>• Wall filter</li><li>• Packet size</li><li>• Spatial filter</li><li>• Frame average</li><li>• Accumulation mode</li><li>• Flash suppression</li><li>• Shortcuts</li></ul>	<ul style="list-style-type: none"><li>• Color maps, including velocity-variance maps</li><li>• Line density</li><li>• Steering angle</li><li>• Threshold</li><li>• Auto ROI placement and steering on linear</li></ul>
------------	---	--

## Digital Power Doppler Imaging

Adjustable	<ul style="list-style-type: none"><li>• Acoustic power</li><li>• Gain</li><li>• Velocity scale range</li><li>• Wall filter</li><li>• Packet size</li><li>• Spatial filter</li><li>• Frame average</li><li>• Accumulation mode</li><li>• Shortcuts</li></ul>	<ul style="list-style-type: none"><li>• Color maps, including velocity-variance maps</li><li>• Line density</li><li>• Steering angle</li><li>• Threshold</li><li>• Flash suppression</li></ul>
------------	---	--

## Continuous Wave Doppler (Option)

Available on the following probes: M5Sc-D, P2D, P6D, 6S-D, 6Tc -RS

Steerable CW mode included

Adjustable	<ul style="list-style-type: none"><li>• Acoustic power</li><li>• Dynamic range</li><li>• Transmit frequency</li><li>• CW colorization</li><li>• Sweep speed</li><li>• Angle correction</li><li>• Trace method</li><li>• Baseline shift</li><li>• Compression</li><li>• Trace direction</li></ul>	<ul style="list-style-type: none"><li>• Gain</li><li>• Gray scale map</li><li>• Wall filter</li><li>• Velocity scale range</li><li>• Spectrum inversion</li><li>• Doppler auto trace</li><li>• Trace sensitivity</li></ul>
------------	--	--

## Automatic optimization

Optimize B-Mode image to help improve contrast resolution

Selectable amount of contrast resolution improvement (low, medium, high)

CTO (Continuous Tissue Optimization) – continuously adjusts B-Mode axial and lateral gain uniformity and overall gain level, suppressing the noise

Auto-spectral optimize – adjusts baseline, invert, PRF (on live image), and angle correction

Auto CF and PW positioning – adjusts ROI position, sample volume position, and steering



# General system parameters *(cont.)*

## Coded Harmonic Imaging

Available on all 2D and 4D probes

## B-Flow (Option)

Available on the following probes: C1-6-D, C1-6VN-D, C2-7-D, C2-7VN-D, C2-9-D, C2-9VN-D, C3-10-D, L2-9-D, L2-9VN-D, L3-12-D, ML6-15-D, M5Sc-D, L8-18i-D, L6-24D

Background

Sensitivity/PRI

Acoustic power

Frequency

Line density

Frame average

Gray scale map

Tint map

Dynamic range

Rejection

Gain

Flash suppression

SRI-HD

Accumulation

Visualization

## Radiantflow™

Easy, fast visualization of tiny vessels, displaying as a 3D effect

## B Steer+

Available on the following probes: L2-9-D, L3-12-D, ML6-15-D, L8-18i-D, L2-9VN-D, L6-24

## Coded contrast imaging (Option)

Available on the following probes: C1-6-D, C1-6VN-D, C2-9-D, C2-9VN-D, C2-7-D, C2-7VN-D, C3-10-D, IC5-9-D, L2-9-D, L2-9VN-D, L3-12-D, M5Sc-D, ML6-15-D, RAB6-D, RIC5-9-D

2 contrast timers

Timed updates: 0.05 – 10 seconds

Accumulation mode, seven levels

Maximum enhance mode

Flash

Time intensity curve (TIC) analysis

Parametric imaging

The LOGIQ Fortis is designed for compatibility with most commercially available ultrasound contrast agents. Because the availability of these agents is subject to government regulation and approval, product features intended for use with these agents may not be commercially marketed nor made available before the contrast agent is cleared for use. Contrast related product features are enabled only on systems for delivery to an authorized country or region of use.

## LOGIQView

Extended field of view Imaging

Up to 160 cm (63") scan length

Available on all 2D imaging probes

For use in B-Mode

CrossXBeam is available on linear probes

Auto detection of scan direction

Pre-or post-process zoom

Rotation

Auto best fit on monitor

Measurements in B-Mode

## 3D

Allows unlimited rotation and planar translations

3D reconstruction from CINE sweep

## Advanced 3D

Acquisition of color data

Automatic rendering

3D landscape technology

3D movie



# General system parameters *(cont.)*

## Real Time 4D (Option)

Acquisition modes	<ul style="list-style-type: none"><li>• Real Time 4D</li><li>• Static 3D</li><li>• Spatio-Temporal Image Correlation</li></ul>
Visualization modes	<ul style="list-style-type: none"><li>• 3D rendering (diverse surface and intensity projection modes)</li><li>• Sectional planes (3 section planes perpendicular to each other)</li><li>• Omniview</li><li>• Volume contrast imaging – static</li><li>• Volume contrast imaging – Omniview</li><li>• Tomographic ultrasound imaging</li><li>• Volume Analyses<ul style="list-style-type: none"><li>– VOCAL: semi-auto/manual segmentation tool (segmentation using touch screen)</li><li>– 3D static only</li><li>– Threshold Volume: measure volume above and below a threshold</li></ul></li></ul>
Render mode	<ul style="list-style-type: none"><li>• Surface texture, surface smooth, max-min- and X-ray (average intensity projection), mix mode of two render modes</li><li>• HDlive™</li></ul>

SonoRenderlive

Curved 3-point render start

3D movie

Scalpel: 3D cut tool

Display format	<ul style="list-style-type: none"><li>• Quad: A-/B-/C-Plane/3D</li><li>• Dual: A-Plane/3D</li><li>• Single: 3D or A- or B- or C-Plane</li></ul>
----------------	---

Automated volume calculation – VOCAL II

Betaview

## Volume navigation (Option)

Available on the following probes: C1-6VN-D, C2-9VN-D, C2-7VN-D, C3-10-D, L2-9VN-D, ML6-15-D, IC5-9-D, L8-18i-D, M5Sc-D

Sensor-based acquisition

Position markers

Needle tip tracking

Virtual tracking

Auto image registration

Tru3D feature includes:	Display of data in: main-, parallel-, angular-mode
-------------------------	--

Render modes: gray surface, texture, min-, max-, average-intensity

Measurements: distance, angle, area, volume

3D movie

## Scan assistant (Option)

Factory programs

User-defined programs

Steps include image annotations, mode transitions, basic imaging controls, and measurement initiation

## Compare assistant (Option)

Allows side-by-side comparison of previous ultrasound and other modality exams during live scanning

## Breast productivity package

Auto measurement

Worksheet summary includes measurements and locations for lesions and lymph nodes

Feature assessment

BI-RADS® assessment

User editable

## Thyroid productivity package

Auto measurement

Worksheet summary includes measurements and locations for nodule, parathyroid, and lymph node

Feature assessment

TI-RADS assessment

User editable

## Start Assistant

Automatically select category, probe, preset, or scan assistant from worklist exam description

Learn the category, probe, preset, and scan assistant based on exam description

## Shear Wave Elastography (Option)

Available on the following probes: C1-6-D, C1-6VN-D, IC5-9-D, L2-9-D, L2-9VN-D, L3-12D, ML6-15-D, L8-18D

User programmable measurement display in kPa and meters per second

Single and dual view display



# General system parameters *(cont.)*

## Strain Elastography (Option)

Available on the following probes: ML6-15-D, L2-9-D, L2-9VN-D, L3-12-D, IC5-9-D, C2-9-D, C2-9VN-D, C1-6-D, C1-6VN-D, L8-18i-D, BE9CS-D

Relative analysis tool

## UGAP (Option)

Available on the following probes: C1-6-D, C1-6VN-D, C2-9D, C2-9VN-D

Measures liver attenuation\* (attenuation coefficient [dB/cm/MHz]) by auto measure algorithm with reference B-mode

Simple and 2D color map (attenuation color map and Measurement Position Indicator Map)

## Quantitative flow analysis (Option)

Available in color and power Doppler

## TVI (Option)

Available on the following probes: M5Sc-D, 6S-D, 6TC-RS, 6Tc-RS

Myocardial Doppler imaging with color overlay on tissue image

Tissue color overlay can be removed to show just the 2D image, still retaining the tissue velocity information

Curved anatomical M-Mode: free (curved) drawing of M-Mode generated from the cursor independent of the axial plane

Q-Analysis: multiple time-motion trace display from selected points in the myocardium

## Stress echo (Option)

Advanced and flexible stress echo examination capabilities

Provides exercise and pharmacological protocol templates

6 default templates

Template editor for user configuration of existing templates or creation of new templates

Reference scan display during acquisition for stress level comparison (dual screen)

Baseline level/previous level selectable

Raw data continuous capture

Over 100 sec. available

Wall motion scoring (bulls-eye and segmental)

Smart stress: Automatically set up various scanning parameters (e.g. geometry, frequency, gain) according to same projection on previous level

## Auto EF (Option)

Allows semi-automatic measurement of the global EF (Ejection Fraction)

User editable

## Cardiac AFI (Option)

Allows assessment of the complete left ventricle with all segments at a glance by combining three longitudinal views into one comprehensive bulls-eye view

2D strain-based data moves into clinical practice

## Virtual convex

Provides a convex field of view

Compatible with CrossXBeam

Available on all linear and sector probes

## SRI-HD and Advanced SRI

Speckle reduction imaging

Provides multiple levels of speckle reduction

Compatible with side-by-side DualView display

Advanced SRI: two types selectable

- Type 1
  - Compatible with all linear, convex, and sector probes
- Type 2 (Option)
  - Compatible with OB/GYN application

## CrossXBeam

Provides variable angle spatial compounding

Live side-by-side DualView display

Compatible with

- Color mode
- SRI-HD
- Virtual convex
- PW
- Coded harmonic imaging

Available on all curved and linear probes

## Controls available while “live”

Magnification Zoom: Magnifies the entire image on the screen without zoom ROI

Pan Zoom: Magnifies the display of the data within the ROI

HD Zoom: Magnifies the image within the zoom ROI with higher spatial resolution than original images

B/M/CrossXBeam-Mode

- Gain
- Dynamic range
- Framerate control
- CrossXBeam angle
- TGC
- Acoustic output
- Sweep speed for M-Mode



# General system parameters *(cont.)*

## Controls available while “live” *(cont.)*

PW-Mode	<ul style="list-style-type: none"><li>• Gain</li><li>• Acoustic output</li><li>• PRF</li><li>• Wall filter</li><li>• Sample volume gate: length, depth</li></ul>	<ul style="list-style-type: none"><li>• Dynamic range</li><li>• Transmission frequency</li><li>• Spectral averaging</li><li>• Velocity scale</li></ul>
Color Flow Mode	<ul style="list-style-type: none"><li>• CFM gain</li><li>• Acoustic output</li><li>• Wall echo filter</li><li>• Frame rate control</li><li>• CFM frame averaging</li><li>• Frequency/velocity baseline shift</li></ul>	<ul style="list-style-type: none"><li>• CFM velocity range</li><li>• Packet size</li><li>• CFM spatial filter</li><li>• CFM line resolution</li></ul>

## Controls available on “freeze” or recall

Automatic optimization

SRI-HD

CrossXBeam – display non-compounded and compounded image simultaneously in split screen

3D reconstruction from a stored CINE loop

B/M/CrossXBeam mode	<ul style="list-style-type: none"><li>• Gray map optimization</li><li>• TGC</li><li>• Colorized B and M</li><li>• Frame average (loops only)</li><li>• Dynamic range</li></ul>
---------------------	--

Anatomical M-Mode

Magnification zoom

Pan zoom

Baseline shift

Sweep speed

PW mode	<ul style="list-style-type: none"><li>• Gray map</li><li>• Baseline shift</li><li>• Invert spectral wave form</li><li>• Colorized spectrum</li><li>• Quick angle correct</li></ul>	<ul style="list-style-type: none"><li>• Post gain</li><li>• Sweep speed</li><li>• Compression</li><li>• Display format</li><li>• Angle correct</li><li>• Auto angle correct</li></ul>
---------	--	---

Color flow	<ul style="list-style-type: none"><li>• Overall gain (loops and stills)</li><li>• Color map</li><li>• Transparency map</li><li>• Frame averaging (loops only)</li><li>• CFM display threshold</li><li>• Spectral invert for color/Doppler</li></ul>
------------	---

Anatomical M-Mode on CINE loop

4D	<ul style="list-style-type: none"><li>• Gray map, colorize</li><li>• Post gain</li><li>• Change display – single, dual, quad sectional or rendered</li></ul>
----	--

# Measurements/calculations

## General B-Mode

Depth and distance

Circumference (ellipse/trace)

Area (ellipse/trace)

Volume (ellipsoid)

% Stenosis (area or diameter)

Angle between two lines

Dual B-Mode capability

## General M-Mode

M-Depth

Distance

Time

Slope

Heart rate

## General Doppler measurements/calculations

Velocity

Time

A/B ratio (velocities/frequency ratio)

PS (Peak Systole)

ED (End Diastole)

PS/ED (PS/ED Ratio)

ED/PS (ED/PS Ratio)

AT (Acceleration Time)

ACCEL (Acceleration)

TAMAX (Time Averaged Maximum Velocity)

Volume flow (TAMEAN and vessel area)

Heart rate

PI (Pulsatility Index)

RI (Resistivity Index)

## Real-time Doppler auto measurements/calculations

PS (Peak Systole)

ED (End Diastole)

MD (Minimum Diastole)

PI (Pulsatility Index)

RI (Resistivity Index)



# Measurements/calculations *(cont.)*

## Real-time Doppler auto measurements/calculations *(cont.)*

AT (Acceleration Time)

ACC (Acceleration)

PS/ED (PS/ED Ratio)

ED/PS (ED/PS Ratio)

HR (Heart Rate)

TAMAX (Time Averaged Maximum Velocity)

PVAL (Peak Velocity Value)

Volume Flow (TAMEAN and Vessel Area)

## Abdominal measurements/calculations

Shear Elasto velocity

Shear Elasto stiffness

Attenuation rate

Attenuation coefficient

Summary reports

## Small Parts measurements/calculations

Breast Lesion

Thyroid

Parathyroid

Lymph Node

Nodule

Isthmus AP

Shear Elasto velocity

Shear Elasto stiffness

Summary reports

## OB measurements/calculations

Gestational age by

- GS (Gestational Sac)
- CRL (Crown Rump Length)
- FL (Femur Length)
- BPD (Biparietal Diameter)
- AC (Abdominal Circumference)
- HC (Head Circumference)
- APTD x TTD (Anterior/Posterior Trunk Diameter by Transverse Trunk Diameter)
- FTA (Fetal Trunk Cross-sectional Area)
- HL (Humerus Length)
- BD (Binocular Distance)
- FT (Foot Length)
- OFD (Occipital Frontal Diameter)
- TAD (Transverse Abdominal Diameter)
- TCD (Transverse Cerebellum Diameter)
- THD (Thorax Transverse Diameter)
- TIB (Tibia Length)
- ULNA (Ulna Length)
- OOD (Outer Orbital Diameter)
- IOD (Inner Orbital Diameter)
- FIB (Fibula length)
- Radius (Radius length)
- LV (Lateral Ventricle width) (= SL)

Fetal graphical trending

Growth percentiles

Multi-gestational calculations (4)

Fetal qualitative description (anatomical survey)

Fetal environmental description (biophysical profile)

Programmable OB tables

Over 20 selectable OB calculations

Expanded worksheets

## Estimated fetal weight (EFW) by:

AC, BPD

AC, BPD, FL

AC, BPD, FL, HC

AC, FL

AC, FL, HC

AC, HC

BPD, APTD, TTD, FL

BPD, APTD, TTD, SL



# Measurements/calculations *(cont.)*

## Calculations and ratios

FL/BPD

FL/AC

FL/HC

HC/AC

CI (Cephalic Index)

AFI (Amniotic Fluid Index)

CTAR (Cardio-Thoracic Area Ratio)

Measurements/calculations by: Alexander, ASUM, ASUM 2001, Bahlmann, Baschat, Berkowitz, Bertagnoli, Brenner, Campbell, CFEF, Chervenak, Chitty, Doubilet, Ebing, Eik-Nes Goldstein, Hadlock, Hansmann, Hellman, Hill, Hohler, Jeanty, JSUM, Kramer, Kurmanavicius, Kurtz, Mari, Mayden, Mercer, Merz, Moore, Nelson, Osaka University, Paris, Pexsters, Rempen, Robinson, Shepard, Shepard/Warsoff, Sonek, Tokyo University, Tokyo/Shinozuka, WHO, Williams, Yarkoni

## OB measure assistant

Allows automatic measurement of BPD, HC, FL, AC, and HL

User editable

## SonoNT and SonoIT

SonoNT measures the contour detection of the NT border

SonoIT is a system supported measurement for Intracranial Translucency

## GYN measurements/calculations

Right ovary length, width, height

Left ovary length, width, height

Uterus length, width, height

Cervix length, trace

Ovarian volume

ENDO (Endometrial thickness)

Ovarian RI

Uterine RI

Follicular measurements

Fibroid measurements

Summary reports

Mean Uterine Artery (Gomez) Doppler Measurement and graph

Qualitative description (anatomical survey)

## Vascular measurements/calculations

SYS DCCA (Systolic Distal Common Carotid Artery)

DIAS DCCA (Diastolic Distal Common Carotid Artery)

SYS MCCA (Systolic Mid Common Carotid Artery)

DIAS MCCA (Diastolic Mid Common Carotid Artery)

SYS PCCA (Systolic Proximal Common Carotid Artery)

DIAS PCCA (Diastolic Proximal Common Carotid Artery)

SYS DICA (Systolic Distal Internal Carotid Artery)

DIAS DICA (Systolic Distal Internal Carotid Artery)

SYS MICA (Systolic Mid Internal Carotid Artery)

DIAS MICA (Diastolic Mid Internal Carotid Artery)

SYS PICA (Systolic Proximal Internal Carotid Artery)

DIAS PICA (Diastolic Proximal Internal Carotid Artery)

SYS DECA (Systolic Distal External Carotid Artery)

DIAS DECA (Diastolic Distal External Carotid Artery)

SYS PECA (Systolic Proximal External Carotid Artery)

DIAS PECA (Diastolic Proximal External Carotid Artery)

VERT (Systolic Vertebral Velocity)

SUBCLAV (Systolic Subclavian Velocity)

Automatic IMT

Summary reports

## Urological calculations

Bladder volume

Prostate volume

Left/right renal volume

Generic volume

Post-void bladder volume

Pelvic floor measurements



# Probes *(All Optional)*

## BE9CS-D

Applications: urology

Biopsy guide: single angle, disposable (E8387M);  
single angle, reusable (E8387MA)

## 6S-D, sector probe

Applications: cardiac, pediatric cardiac

## 6Tc-RS, trans-esophageal probe

Applications: cardiac

TEE RS-DLP Adapter (H46352LK)

## C1-6-D, XDclear™ convex probe

Applications: abdomen, OB/GYN, pediatric, peripheral vascular, general musculoskeletal

Biopsy guide: multi-angle, disposable with a reusable bracket (H4917VB)

## C1-6VN-D, VNav inside XDclear convex probe

VNav sensor inside probe for Volume Navigation tracking without sensor cables

Applications: abdomen, OB/GYN, pediatric, peripheral vascular, general musculoskeletal

Biopsy guide: multi-angle, disposable with a reusable bracket (H4917VB)

## C2-7-D, micro convex biopsy probe

Applications: abdomen, pediatric

Biopsy guide: multi-angle, disposable with a reusable bracket (H40482LK); multi-angle, with a reusable stainless bracket (H40482LL)

## C2-7VN-D, VNav inside micro convex biopsy probe

VNav sensor inside probe for Volume Navigation tracking without sensor cables

Applications: abdomen, pediatric

Biopsy guide: multi-angle, disposable with a reusable bracket (H40482LK); multi-angle, with a reusable stainless bracket (H40482LL)

## C2-9-D, XDclear convex probe

Applications: abdomen, OB/GYN, pediatric, peripheral vascular, neonatal, neonatal transcranial, general musculoskeletal

Biopsy guide: multi-angle, disposable with a reusable bracket (H4913BA)

## C2-9VN-D, VNav inside XDclear convex probe

VNav sensor inside probe for Volume Navigation tracking without sensor cables

Applications: abdomen, OB/GYN, pediatric, peripheral vascular, neonatal, neonatal transcranial, general musculoskeletal

Biopsy guide: multi-angle, disposable with a reusable bracket (H4913BA)

## C3-10-D, XDclear micro convex probe

Applications: abdomen, neonatal, pediatric, peripheral vascular, neonatal transcranial, small parts

## IC5-9-D, micro convex probe

Applications: OB/GYN, urology

Biopsy guide: single angle, disposable with a disposable bracket (E8385MJ) or a reusable bracket (H40412LN)

## L2-9-D, XDclear linear probe

Applications: peripheral vascular, small parts, pediatric, abdomen, OB/GYN, general musculoskeletal, superficial musculoskeletal, neonatal, neonatal transcranial

Biopsy guide: multi-angle, disposable with a reusable bracket (H44901AM)

## L2-9VN-D, VNav inside XDclear linear probe

VNav sensor inside probe for Volume Navigation tracking without sensor cables

Applications: peripheral vascular, small parts, pediatric, abdomen, OB/GYN, general musculoskeletal, superficial musculoskeletal, neonatal, neonatal transcranial

Biopsy guide: multi-angle, disposable with a reusable bracket (H44901AM)

## L3-12-D, linear probe

Applications: abdomen, OB, general musculoskeletal, superficial musculoskeletal, neonatal, neonatal transcranial, small parts, vascular

Biopsy guide: multi-angle, disposable with a reusable bracket (H78652PA)

## L6-24-D, linear probe

Applications: general musculoskeletal, superficial musculoskeletal, pediatrics, thyroid



## Probes *(cont.)*

### L8-18i-D, linear probe

Applications: small parts, peripheral vascular, neonatal, neonatal transcranial, general musculoskeletal, superficial musculoskeletal, intraoperative

### M5Sc-D, XDclear sector probe

Applications: adult cardiac, pediatric cardiac, adult cephalic, abdominal

Biopsy guide: multi-angle, disposable with a reusable bracket (H45561FC)

### ML6-15-D, matrix array linear probe

Applications: abdomen, small parts, peripheral vascular, neonatal, pediatric, neonatal transcranial, general musculoskeletal, superficial musculoskeletal

Biopsy guide: multi-angle, disposable with a reusable bracket (H40432LJ)

### P2D, CW split crystal probe

Applications: adult cardiac, pediatric cardiac, peripheral vascular, adult cephalic

### P6D, CW split crystal probe

Applications: adult cardiac, pediatric cardiac, peripheral vascular, adult cephalic

### RAB6-D, convex volume probe

Applications: abdomen, OB/GYN, pediatric, neonatal

Biopsy guide: single angle, reusable bracket (H46701AE)

### RIC5-9-D, convex volume probe

Applications: OB/GYN, urology

Biopsy guide: single angle, reusable (H46721R)

### External Inputs and outputs (not including on-board peripherals)

HDMI

Ethernet

Multiple USB 3.0 ports

## Safety conformance

### The LOGIQ Fortis is:

Classified to ANSI/AAMI ES60601-1 2005 R1 2012 Medical Electrical Equipment, Part 1: General Requirements for Safety by a Nationally Recognized Test Lab

Certified to CSA CAN/CSA-C22.2 NO. 60601-1:14 General requirements for safety

CE Marked to EU Medical Device Regulation MDR 2017-745 and Council Directive 93/42/EEC on Medical Devices and conforms to the following standards for safety:

- IEC/EN 60601-1 Edition 3.1 Medical electrical equipment – Part 1: General requirements for basic safety and essential performance
- IEC/EN 60601-1-2 Medical electrical equipment – Parts 1-2: General requirements for safety – Collateral standard: Electromagnetic compatibility – requirements and tests
- IEC/EN 60601-1-6 Medical electrical equipment Parts 1 -6: General requirements for basic safety and essential performance – Collateral standard: usability
- IEC/EN 60601-2-37 Medical electrical equipment – Parts 2-37: Particular requirements for the safety of ultrasonic medical diagnostic and monitoring equipment
- IEC 61157 (Standard means for the reporting of the acoustic output of medical diagnostic ultrasonic equipment)
- IEC/EN 62366 Application of usability engineering to medical devices
- IEC/EN 62304 Software life cycle processes
- IEC/EN 62359 Ultrasonic – Field characterization – Test methods for the determination of thermal and mechanical indices related to medical diagnostic ultrasonic fields
- EN ISO 15223-1: Symbols to be used with medical device labels, labelling, and information to be supplied
- ISO 10993-1 Biological evaluation of medical devices – Part 1: Evaluation and testing
- ISO14971:2012 (Medical devices – Application of risk management to medical devices)
- EMC Emissions Group 1, Class A device requirements as per sub-clause 4.2 of CISPR 11
- WEEE (Waste Electrical and Electronic Equipment)
- ROHS according to 2011/65/EU including national deviations
- Wireless equipment shall be certified to FCC, RED, and Japan Radio Law.
- Medical Device Good Manufacturing Practice Manual issued by the FDA (Food and Drug Administration, Department of Health, USA)



# Supplement: cardiac measurements/calculations

## B-Mode measurements

Aorta	<ul style="list-style-type: none"> <li>• Aortic Root Diameter (Ao Root Diam)</li> <li>• Aortic Arch Diameter (Ao Arch Diam)</li> <li>• Ascending Aortic Diameter (Ao Asc Diam)</li> <li>• Descending Aortic Diameter (Ao Desc Diam)</li> <li>• Aorta Isthmus (Ao Isthmus)</li> <li>• Aorta (Ao st junct)</li> </ul>
Aortic valve	<ul style="list-style-type: none"> <li>• Aortic Valve Cusp Separation (AV Cusp)</li> <li>• Aortic Valve Area Planimetry (AVA Planimetry)</li> <li>• Trans AVA</li> </ul>
Left atrium	<ul style="list-style-type: none"> <li>• Left Atrium Diameter (LA Diam)</li> <li>• LA Length (LA Major)</li> <li>• LA Width (LA Minor)</li> <li>• Left Atrium Diameter to AoRoot Diameter Ratio (LA/Ao ratio)</li> <li>• Left Atrium Area (LAA(d), LAA(s))</li> <li>• Left Atrium Volume, Single Plane, Method of Disk (LAEDV A2C, LAESV A2C) (LAEDV A4C, LAESV A4C), (LAEDV A-L, LAEDV Index A-L, LAESV A-L, LAESV Index A-L)</li> </ul>

## B-Mode measurements (cont.)

Left ventricle	<ul style="list-style-type: none"> <li>• Left Ventricle Mass (LVPWd, LVPWs)</li> <li>• Left Ventricle Volume, Teichholz/Cubic (LVIDd, LVI Ds)</li> <li>• Left Ventricle Internal Diameter (LVIDd, LVI Ds) Left Ventricle Length (LVLd, LVLs)</li> <li>• Left Ventricle Outflow Tract Diameter (LVOT Diam)</li> <li>• Left Ventricle Posterior Wall Thickness (LVPWd, LVPWs)</li> <li>• Left Ventricle Length (LV Major)</li> <li>• Left Ventricle Width (LV Minor)</li> <li>• Left Ventricle Outflow Tract Area (LVOT)</li> <li>• Left Ventricle Area, Two Chamber/Four Chamber/Short Axis (LVA (d), LVA (s))</li> <li>• Left Ventricle Endocardial Area, Width (LVA (d), LVA(s))</li> <li>• Left Ventricle Epicardial Area, Length (LVAepi (d), LVAepi (s))</li> <li>• Left Ventricle Mass Index (LVPWd, LVPWs)</li> <li>• Ejection Fraction, Teichholz/Cube (LVIDd, LVIDs)</li> <li>• Left Ventricle Posterior Wall Fractional Shortening (LVPWd, LVPWs)</li> <li>• Left Ventricle Stroke Index, Teichholz/ Cube (LVIDd, LVIDs and Body Surface Area)</li> <li>• Left Ventricle Fractional Shortening (LVIDd, LVIDs)</li> <li>• Left Ventricle Stroke Volume, Teichholz/ Cubic (LVIDd, LVIDs)</li> <li>• Left Ventricle Stroke Index, Single Plane, Two Chamber, Method of Disk (LVI Dd, LVIDs, LVSD, LVSS)</li> <li>• Left Ventricle Stroke Index, Single Plane, Four Chamber, Method of Disk (LVI Dd, LVIDs, LVSD, LVSS)</li> <li>• Left Ventricle Stroke Index, Bi-Plane, Bullet, Method of Disk (LVAd, LVAs)</li> <li>• Interventricular Septum (IVS)</li> <li>• Left Ventricle Internal Diameter (LVI D)</li> <li>• Left Ventricle Posterior Wall Thickness (LVPW)</li> </ul>
----------------	--



# Supplement: cardiac measurements/calculations *(cont.)*

## B-Mode measurements *(cont.)*

Mitral valve	<ul style="list-style-type: none"> <li>Mitral Valve Annulus Diameter (MV Ann Diam)</li> <li>E-Point-to-Septum Separation (EPSS)</li> <li>Mitral Valve Area Planimetry (MVA Planimetry)</li> </ul>
Pulmonic valve	<ul style="list-style-type: none"> <li>Pulmonic Valve Area (PV Planimetry)</li> <li>Pulmonic Valve Annulus Diameter (PV Annulus Diam)</li> <li>Pulmonic Diameter (Pulmonic Diam)</li> </ul>
Right atrium	<ul style="list-style-type: none"> <li>Right Atrium Diameter, Length (RAD Ma)</li> <li>Right Atrium Diameter, Width (RAD Mi)</li> <li>Right Atrium Area (RAA)</li> <li>Right Atrium Volume, Single Plane, Method of Disk (RAAd)</li> <li>Right Atrium Volume, Systolic, Single Plane, Method of Disk (RAAs)</li> </ul>
Right ventricle	<ul style="list-style-type: none"> <li>Right Ventricle Outflow Tract Area (RVOT Planimetry)</li> <li>Left Pulmonary Artery Area (LPA Area)</li> <li>Right Pulmonary Artery Area (RPA Area)</li> <li>Right Ventricle Internal Diameter (RVIDd, RVIDs)</li> <li>Right Ventricle Diameter, Length (RVD Ma)</li> <li>Right Ventricle Diameter, Width (RVD Mi)</li> <li>Right Ventricle Wall Thickness (RVAWd, RVAWs)</li> <li>Right Ventricle Outflow Tract Diameter (RVOT Diam)</li> <li>Left Pulmonary Artery (LPA)</li> <li>Main Pulmonary Artery (MPA)</li> <li>Right Pulmonary Artery (RPA)</li> </ul>
System inferior vena cava	<ul style="list-style-type: none"> <li>Systemic Vein Diameter (Systemic Diam)</li> <li>Patent Ductus Arteriosis Diameter (PDA Diam)</li> <li>Pericard Effusion (PEs)</li> <li>Patent Foramen Ovale Diameter (PFO Diam)</li> <li>Ventricular Septal Defect Diameter (VSD Diam)</li> <li>Interventricular Septum (IVS) Fractional Shortening (IVSd, IVSs)</li> </ul>
Tricuspid valve	<ul style="list-style-type: none"> <li>Tricuspid Valve Area (TV Panimetry)</li> <li>Tricuspid Valve Annulus Diameter (TV Annulus Diam)</li> </ul>

## M-Mode measurements

Aorta	<ul style="list-style-type: none"> <li>Aortic Root Diameter (Ao Root Diam)</li> <li>Aortic Valve</li> <li>Aortic Valve Diameter (AV Diam)</li> <li>Aortic Valve Cusp separation (AV Cusp)</li> <li>Aortic Valve Ejection Time (LVET)</li> </ul>
Left atrium	<ul style="list-style-type: none"> <li>Left Atrium Diameter to AoRoot Diameter Ratio (LA/Ao Ratio)</li> <li>Left Atrium Diameter (LA Diam)</li> </ul>
Left ventricle	<ul style="list-style-type: none"> <li>Left Ventricle Volume, Teichholz/Cubic (LVIDd, LVI Ds)</li> <li>Left Ventricle Internal Diameter (LVIDd, LVI Ds)</li> <li>Left Ventricle Posterior Wall Thickness (LVPWd, LVPWs)</li> <li>Left Ventricle Ejection Time (LVET)</li> <li>Left Ventricle Pre-Ejection Period (LVPEP)</li> <li>Interventricular Septum (IVS)</li> <li>Left Ventricle Internal Diameter (LVI D)</li> <li>Left Ventricle Posterior Wall Thickness (LVPW)</li> </ul>
Mitral valve	<ul style="list-style-type: none"> <li>E-Point-to-Septum Separation (EPSS)</li> <li>Mitral Valve Leaflet Separation (D-E Excursion)</li> <li>Mitral Valve Anterior Leaflet Excursion (D-E Excursion)</li> <li>Mitral Valve D-E Slope (D-E Slope)</li> <li>Mitral Valve E-F Slope (E-F Slope)</li> <li>Mitral Annular Plane Systolic Excursion (MAPSE)</li> </ul>
Pulmonic valve	<ul style="list-style-type: none"> <li>QRS Complex to End of Envelope (Q-PV close)</li> </ul>
Right ventricle	<ul style="list-style-type: none"> <li>Right Ventricle Internal Diameter (RVIDd, RVIDs)</li> <li>Right Ventricle Wall Thickness (RVAWd, RVAWs)</li> <li>Right Ventricle Outflow Tract Diameter (RVOT Diam)</li> <li>Right Ventricle Ejection Time (RVET)</li> <li>Right Ventricle Pre-Ejection Period (RVPEP)</li> </ul>
System	<ul style="list-style-type: none"> <li>Pericard Effusion (PE (d))</li> </ul>
Tricuspid valve	<ul style="list-style-type: none"> <li>QRS Complex to End of Envelope (Q-TV close)</li> <li>Tricuspid Annular Plane Systolic Excursion (TAPSE)</li> </ul>



# Supplement: cardiac measurements/calculations *(cont.)*

## Doppler Mode measurements

Aortic valve	<ul style="list-style-type: none"> <li>• Aortic Insufficiency Mean Pressure Gradient (AR Trace)</li> <li>• Aortic Insufficiency Peak Pressure Gradient (AR Vmax)</li> <li>• Aortic Insufficiency End Diastole Pressure Gradient (AR Trace)</li> <li>• Aortic Insufficiency Mean Velocity (AR Trace)</li> <li>• Aortic Insufficiency Velocity Time Integral (AR Trace)</li> <li>• Aortic Valve Mean Velocity (AV Trace)</li> <li>• Aortic Valve Velocity Time Integral (AV Trace)</li> <li>• Aortic Valve Mean Pressure Gradient (AV Trace)</li> <li>• Aortic Valve Peak Pressure Gradient (AR Vmax)</li> <li>• Aortic Insufficiency Peak Velocity (AR Vmax)</li> <li>• Aortic Insufficiency End-Diastolic Velocity (AR Trace)</li> <li>• Aortic Valve Peak Velocity (AV Vmax)</li> <li>• Aortic Valve Peak Velocity at Point E (AV Vmax)</li> <li>• Aorta Proximal Coarctation (Coarc Pre-Duct)</li> <li>• Aorta Distal Coarctation (Coarc Post-Duct)</li> <li>• Aortic Valve Insufficiency Pressure Half Time (AR PHT)</li> <li>• Aortic Valve Flow Acceleration (AV Trace)</li> <li>• Aortic Valve Pressure Half Time (AV Trace)</li> <li>• Aortic Valve Acceleration Time (AV Acc Time)</li> <li>• Aortic Valve Deceleration Time (AV Dec Time)</li> <li>• Aortic Valve Ejection Time (AVET)</li> <li>• Aortic Valve Acceleration to Ejection Time Ratio (AV Acc Time, AVET)</li> <li>• Aortic Valve Area(VTI): AVA (Vmax)</li> </ul>
Left ventricle	<ul style="list-style-type: none"> <li>• Left Ventricle Outflow Tract Peak Pressure Gradient (LVOT Vmax)</li> <li>• Left Ventricle Outflow Tract Peak Velocity (LVOT Vmax)</li> <li>• Left Ventricle Outflow Tract Mean Pressure Gradient (LVOT Trace)</li> <li>• Left Ventricle Outflow Tract Mean Velocity (LVOT Trace)</li> <li>• Left Ventricle Outflow Tract Velocity Time Integral (LVOT Trace)</li> <li>• Left Ventricle Ejection Time (LVET)</li> </ul>
Mitral valve	<ul style="list-style-type: none"> <li>• E' Early diastolic mitral valve annular velocity (E')</li> <li>• E' Averaged Early diastolic mitral valve annular velocity (E' Avg)</li> <li>• E' Lat Early diastolic mitral valve lateral annular velocity (E' Lat)</li> <li>• E' Medial Early diastolic mitral valve medial annular velocity (E' Medial)</li> <li>• E' Sept Early diastolic mitral valve septal annular velocity (E' Sept)</li> </ul>

## Doppler Mode measurements *(cont.)*

Mitral valve <i>(cont.)</i>	<ul style="list-style-type: none"> <li>• Mitral inflow E velocity to E' ratio (E/E')</li> <li>• Mitral inflow E velocity to E' Avg ratio (E/E' Avg)</li> <li>• Mitral inflow E velocity to E' Lat ratio (E/E' Lat)</li> <li>• Medial Mitral inflow E velocity to E' Medial ratio (E/E')</li> <li>• Mitral inflow E velocity to E' Sept ratio (E/E' Sept)</li> <li>• Mitral Valve Regurgitant Flow Acceleration (MR Trace)</li> <li>• Mitral Valve Regurgitant Mean Velocity (MR Trace)</li> <li>• Mitral Regurgitant Mean Pressure Gradient (MR Trace)</li> <li>• Mitral Regurgitant Velocity Time Integral (MR Trace)</li> <li>• Mitral Valve Mean Velocity (MV Trace)</li> <li>• Mitral Valve Velocity Time Integral (MV Trace)</li> <li>• Mitral Valve Mean Pressure Gradient (MV Trace)</li> <li>• Mitral Regurgitant Peak Pressure Gradient (MR Vmax)</li> <li>• Mitral Valve Peak Pressure Gradient (MV Vmax)</li> <li>• Mitral Regurgitant Peak Velocity (MR Vmax)</li> <li>• Mitral Valve Peak Velocity (MV Vmax)</li> <li>• Mitral Valve Velocity Peak A (MV A Velocity)</li> <li>• Mitral Valve Velocity Peak E (MV E Velocity)</li> <li>• Mitral Valve Area According to PHT (MV PHT)</li> <li>• Mitral Valve Flow Deceleration (MV DecT)</li> <li>• Mitral Valve Pressure Half Time (MV PHT)</li> <li>• Mitral Valve Flow Acceleration (MV AccT)</li> <li>• Mitral Valve E-Peak to A-Peak Ratio (A-C and D-E) (MV E/ARatio)</li> <li>• Mitral Valve Acceleration Time (MV Acc Time)</li> <li>• Mitral Valve Deceleration Time (MV Dec Time)</li> <li>• Mitral Valve Ejection Time ((MVET)</li> <li>• Mitral Valve A-Wave Duration (MV A Dur)</li> <li>• Mitral Valve Time to Peak (MV TTP)</li> <li>• Mitral Valve Acceleration Time/Deceleration Time Ratio (MV Acc/Dec Time)</li> <li>• Stroke Volume Index by Mitral Flow (MVA Planimetry, MVTrace)</li> </ul>
Pulmonic valve	<ul style="list-style-type: none"> <li>• Pulmonic Insufficiency Peak Pressure Gradient (PR Vmax)</li> <li>• Pulmonic Insufficiency End-Diastolic Pressure Gradient (PR Trace)</li> <li>• Pulmonic Valve Peak Pressure Gradient (PV Vmax)</li> <li>• Pulmonic Insufficiency Peak Velocity (PR Vmax)</li> </ul>



# Supplement: cardiac measurements/calculations *(cont.)*

Doppler Mode measurements <i>(cont.)</i>	
Pulmonic valve <i>(cont.)</i>	<ul style="list-style-type: none"> <li>Pulmonic Insufficiency End-Diastolic Velocity (Prend Vmax)</li> <li>Pulmonic Valve Peak Velocity (PV Vmax)</li> <li>Pulmonary Artery Diastolic Pressure (PV Trace)</li> <li>Pulmonic Insufficiency Mean Pressure Gradient (PR Trace)</li> <li>Pulmonic Valve Mean Pressure Gradient (PV Trace)</li> <li>Pulmonic Insufficiency Mean Square Root Velocity (PR Trace)</li> <li>Pulmonic Insufficiency Velocity Time Integral (PR Trace)</li> <li>Pulmonic Valve Mean Velocity (PV Trace)</li> <li>Pulmonic Valve Velocity Time Integral (PV Trace)</li> <li>Pulmonic Insufficiency Pressure Half Time (PR PHT)</li> <li>Pulmonic Valve Flow Acceleration (PV Acc Time)</li> <li>Pulmonic Valve Acceleration Time (PV Acc Time)</li> <li>Pulmonic Valve Ejection Time (PVET)</li> <li>QRS Complex to End of Envelope (Q-to-PV Close)</li> <li>Pulmonic Valve Acceleration to Ejection Time Ratio (PV Acc Time, PVET)</li> </ul>
Right ventricle	<ul style="list-style-type: none"> <li>Right Ventricle Outflow Tract Peak Pressure Gradient (RVOT Vmax)</li> <li>Right Ventricle Outflow Tract Peak Velocity (RVOT Vmax)</li> <li>Right Ventricle Outflow Tract Velocity Time Integral (RVOT Trace)</li> <li>Right Ventricle Ejection Time (RV Trace)</li> <li>Stroke Volume by Pulmonic Flow (RVOT Planimetry, RVOT Trace)</li> <li>Right Ventricle Stroke Volume Index by Pulmonic Flow (RVOT Planimetry, RVOT Trace)</li> </ul>
System	<ul style="list-style-type: none"> <li>Pulmonary Artery Peak Velocity (PV Vmax)</li> <li>Pulmonary Vein Velocity Peak A (Reverse) (P Vein A)</li> <li>Pulmonary Vein Peak Velocity (P Vein D, P Vein S)</li> <li>Systemic Vein Peak Velocity (PDA Diastolic, PDA Systolic)</li> <li>Ventricular Septal Defect Peak Velocity (VSD Vmax)</li> <li>Atrial Septal Defect (ASD Diastolic, ASD Systolic)</li> <li>Pulmonary Vein A-Wave Duration (P Vein A Dur)</li> <li>IsoVolumetric Relaxation Time (IVRT)</li> <li>IsoVolumetric Contraction Time (IVCT)</li> </ul>

Doppler Mode measurements <i>(cont.)</i>	
System <i>(cont.)</i>	<ul style="list-style-type: none"> <li>Pulmonary Vein S/D Ratio (P Vein D, P Vein S)</li> <li>Ventricular Septal Defect Peak Pressure Gradient (VSD Vmax)</li> <li>Pulmonic-to-Systemic Flow Ratio (Qp/Qs)</li> </ul>
Tricuspid valve	<ul style="list-style-type: none"> <li>Tricuspid Regurgitant Peak Pressure Gradient (TR Vmax)</li> <li>Tricuspid Valve Peak Pressure Gradient (TV Vmax)</li> <li>Tricuspid Regurgitant Peak Velocity (TR Vmax)</li> <li>Tricuspid Valve Peak Velocity (TV Vmax)</li> <li>Tricuspid Valve Velocity Peak A (TV A Velocity)</li> <li>Tricuspid Valve Velocity Peak E (TV E Velocity)</li> <li>Tricuspid Regurgitant Mean Pressure Gradient (TR Trace)</li> <li>Tricuspid Valve Mean Pressure Gradient (TV Trace)</li> <li>Tricuspid Regurgitant Mean Velocity (TR Trace)</li> <li>Tricuspid Regurgitant Velocity Time Integral (TR Trace)</li> <li>Tricuspid Valve Mean Velocity (TV Trace)</li> <li>Tricuspid Valve Velocity Time Integral (TV Trace)</li> <li>Tricuspid Valve Time to Peak (TV TTP)</li> <li>Tricuspid Valve Ejection Time (TV Acc/Dec Time)</li> <li>Tricuspid Valve A-Wave Duration (TV A Dur)</li> <li>QRS Complex to End of Envelope (Q-TV Close)</li> <li>Tricuspid Valve Pressure Half Time (TV PHT)</li> <li>Stroke Volume by Tricuspid Flow (TV Planimetry, TV Trace)</li> <li>Tricuspid Valve E-Peak to A-Peak Ratio (TV E/A Velocity)</li> </ul>
Color Flow Mode measurements	
Aortic valve	<ul style="list-style-type: none"> <li>Proximal Isovelocity Surface Area: Regurgitant Orifice Area (AR Radius)</li> <li>Proximal Isovelocity Surface Area: Radius of Aliased Point (AR Radius)</li> <li>Proximal Isovelocity Surface Area: Regurgitant Flow (AR Trace)</li> <li>Proximal Isovelocity Surface Area: Regurgitant Volume Flow (AR Trace)</li> <li>Proximal Isovelocity Surface Area: Aliased Velocity (AR Vmax)</li> </ul>



# Supplement: cardiac measurements/calculations *(cont.)*

## Color Flow Mode measurements *(cont.)*

Mitral valve	<ul style="list-style-type: none"> <li>Proximal Isovelocity Surface Area: Regurgitant Orifice Area (MR Radius)</li> <li>Proximal Isovelocity Surface Area: Radius of Aliased Point (MR Radius)</li> <li>Proximal Isovelocity Surface Area: Regurgitant Flow (MR Trace)</li> <li>Proximal Isovelocity Surface Area: Regurgitant Volume Flow (MR Trace)</li> <li>Proximal Isovelocity Surface Area: Aliased Velocity (MR Vmax)</li> </ul>
--------------	---

## Combination Mode measurements

Aortic valve	<ul style="list-style-type: none"> <li>Aortic Valve Area (Ao Root Diam, LVOT Vmax, AV Vmax)</li> <li>Aortic Valve Area by Continuity Equation by Peak Velocity (Ao Root Diam, LVOT Vmax, AV Vmax)</li> <li>Stroke Volume by Aortic Flow (AVA Planimetry, AV Trace)</li> <li>Cardiac Output by Aortic Flow (AVA Planimetry, AV Trace, HR)</li> <li>Aortic Valve Area by Continuity Equation VTI (Ao Root Diam, LVOT Vmax, AV Trace)</li> </ul>
Left ventricle	<ul style="list-style-type: none"> <li>Cardiac Output, Teichholz/Cubic (LVIDd, LVIDs, HR)</li> <li>Cardiac Output Two-Chamber, Single Plane, Area-Length/Method of Disk (Simpson) (LVAd, LVAs, HR)</li> <li>Cardiac Output Four-Chamber, Single Plane, Area-Length/Method of Disk (Simpson) (LVAd, LVAs, HR)</li> <li>Ejection Fraction Two-Chamber, Single Plane, Area-Length/Method of Disk (Simpson) (LVAd, LVAs)</li> <li>Ejection Fraction Four-Chamber, Single Plane, Area-Length/Method of Disk (Simpson) (LVAd, LVAs)</li> <li>Left Ventricle Stroke Volume, Single Plane, Two-Chamber/Four-Chamber, Area-Length (LVAd, LVAs)</li> <li>Left Ventricle Stroke Volume, Single Plane, Two-Chamber/Four-Chamber, Method of Disk (Simpson) (LVIDd, LVIDs, LVAd, LVAs)</li> <li>Left Ventricle Volume, Two-Chamber/Four-Chamber, Area-Length (LVAd, LVAs)</li> </ul>

## Combination Mode measurements *(cont.)*

Left ventricle <i>(cont.)</i>	<ul style="list-style-type: none"> <li>Ejection Fraction, Bi-Plane, Method of Disk (LVAd, LVAs, 2CH, 4CH)</li> <li>Left Ventricle Stroke Volume, Bi-Plane, Method of Disk (LVAd, LVAs, 2CH, 4CH)</li> <li>Left Ventricle Volume, Bi-Plane, Method of Disk (LVAd, LVAs, 2CH, 4CH)</li> <li>Left Ventricle Stroke Index, Single Plane, Two-Chamber/Four-Chamber, Area-Length (LVSD, LVSS and BSA)</li> <li>Left Ventricle Volume, Single Plane, Two-Chamber/Four-Chamber, Method of Disk (LVAd, LVAs)</li> <li>Left Ventricle Volume, Apical View, Long Axis, Method of Disk (LVAd, LVAs)</li> </ul>
Mitral valve	<ul style="list-style-type: none"> <li>Stroke Volume by Mitral Flow (MVA Planimetry, MV Trace)</li> <li>Cardiac Output by Mitral Flow (MVA Planimetry, MV Trace, HR)</li> </ul>
Pulmonic valve	<ul style="list-style-type: none"> <li>Stroke Volume by Pulmonic Flow (PV Planimetry, PV Trace)</li> <li>Cardiac Output by Pulmonic Flow (PV Planimetry, PV Trace, HR)</li> </ul>
Tricuspid valve	<ul style="list-style-type: none"> <li>Cardiac Output by Tricuspid Flow (TV Planimetry, TV Trace, HR)</li> </ul>

## Cardiac worksheet

Parameter: lists the mode, the measurement folder, and the specific measurement

Measured Value: Up to six measurement values for each item. Average, maximum, minimum, or last

## Generic study in cardiology

Stroke Volume (SV)

Cardiac Output (CO)

© GE, 2021

GE Healthcare reserves the right to make changes in specifications and features shown herein, or discontinue the product described at any time without notice or obligation. Contact your GE Healthcare representative for the most current information. GE, the GE Monogram, LOGIQ Fortis, InSite, B-Flow, CrossXBeam, XDclear, Radiantflow and HDlive are trademarks of GE. DICOM is the registered trademark of the National Electrical Manufacturers Association for its standards publications relating to digital communications of medical information. Tricefy trademarks are trademarks of Trice Imaging Inc. BI-RADS is a trademark of the American College of Radiology. GE Healthcare, a division of GE. GE Medical Systems, Inc., doing business as GE Healthcare.

October 2021  
DOC2560319  
Global







# LOGIQ Fortis™

## Probe Guide



**Featuring XDclear™ Technology**

The LOGIQ Fortis is GE's premium ultrasound imaging system designed for abdominal, vascular, obstetric, gynecologic, neonatal, pediatric, urological, transcranial, cardiac, and small parts applications.





C1-6-D  
C1-6VN-D\*



C2-9-D  
C2-9VN-D\*



C3-10-D



IC5-9-D



C2-7-D  
C2-7VN-D\*



L2-9-D  
L2-9-VN-D\*



L3-12-D



L6-24-D



L8-18i-D



ML6-15-D

Description	Applications	FOV	Bandwidth	Biopsy Guide	Volume Navigation
<b>CONVEX</b>					
XDclear broad-spectrum convex probe	Abdominal, Obstetrics, Gynecology, Vascular, Musculoskeletal	80°	1 – 6 MHz	Multi-angle disposable with a reusable bracket	Yes * Internal VNav sensor, does not require an external bracket
XDclear broad-spectrum convex probe	Abdominal, Obstetrics, Gynecology, Pediatrics, Vascular, Musculoskeletal	80°	2 – 9 MHz	Multi-angle disposable with a reusable bracket	Yes * Internal VNav sensor, does not require an external bracket
XDclear broad-spectrum convex probe	Neonatal, Pediatrics, Vascular, Small Parts	95°	2 – 11 MHz	No	Yes
Broad-spectrum micro-convex intra-cavitary probe	Obstetrics, Gynecology, Urology	180°	3 – 10 MHz	Single-angle disposable or single-angle reusable	Yes
Broad spectrum convex probe	Abdominal	110°	1 – 6 MHz	Multi-angle disposable with reusable bracket options	Yes * Internal VNav sensor, does not require an external bracket
<b>LINEAR</b>					
XDclear broad-spectrum linear probe	Vascular, Small Parts, Musculoskeletal, Neonatal Cephalic, Pediatric, Abdominal, Obstetrical	44 mm	2 – 10 MHz	Multi-angle disposable with a reusable bracket	Yes * Internal VNav sensor, does not require an external bracket
Broad-spectrum linear probe	Abdominal, Obstetric, Vascular, Musculoskeletal, Small Parts, Pediatric, Neonatal	51 mm	2 – 11 MHz	Multi-angle disposable with a disposable bracket	Yes
Broad-spectrum linear probe	Musculoskeletal	26 mm	6 – 20 MHz	No	No
Broad-spectrum linear probe	Small Parts, Vascular, Intraoperative, Neonatal	25 mm	4 – 15 MHz	No	Yes
Broad-spectrum linear matrix array probe	Vascular, Small Parts, Neonatal, Pediatrics	50 mm	4 – 16 MHz	Multi-angle disposable with a reusable bracket	Yes





M5Sc-D



6S-D



RAB6-D



RIC5-9-D



P2D



P6D



6Tc-RS



BE9CS-D

Description	Applications	FOV	Bandwidth	Biopsy Guide	Volume Navigation
<b>SECTOR</b>					
XDclear broad-spectrum sector probe	Cardiac, Transcranial, Abdominal	120°	1 – 5 MHz	Multi-angle disposable with a reusable bracket	Yes
Broad-spectrum sector probe	Cardiac	115°	2 – 8 MHz	No	No
<b>REAL-TIME 4D</b>					
Broad-spectrum real-time 4D probe	Abdominal, Obstetrics, Gynecology, Pediatrics	80°	2 – 8 MHz	Single-angle disposable with a reusable bracket	No
Broad-spectrum real-time 4D micro-convex probe	Obstetrics, Gynecology, Urology	180°	3 – 10 MHz	Single-angle reusable	No
<b>SPECIALTY</b>					
CW split crystal pencil probe	Cardiac, Vascular	N/A	1 – 3 MHz	No	No
CW split crystal pencil probe	Cardiac, Vascular, Transcranial	N/A	5 – 7 MHz	No	No
TEE probe	Cardiac	90°	2 – 8 MHz	No	No
Wideband bi-plane micro-convex probe	Urology, Endocavity	133°	3 – 12 MHz	Single-angle disposable bracket or reusable bracket	No





Product may not be available in all countries and regions. Full product technical specifications is available upon request. Contact a GE Healthcare Representative for more information. Please visit [www.gehealthcare.com/promotional-locations](http://www.gehealthcare.com/promotional-locations).

Data subject to change.

© GE, 2021

GE, the GE Monogram, LOGIQ Fortis and XDclear are trademarks of GE.


Reproduction in any form is forbidden without prior written permission from GE. Nothing in this material should be used to diagnose or treat any disease or condition. Readers must consult a healthcare professional.

September 2021

DOC2621716

Global



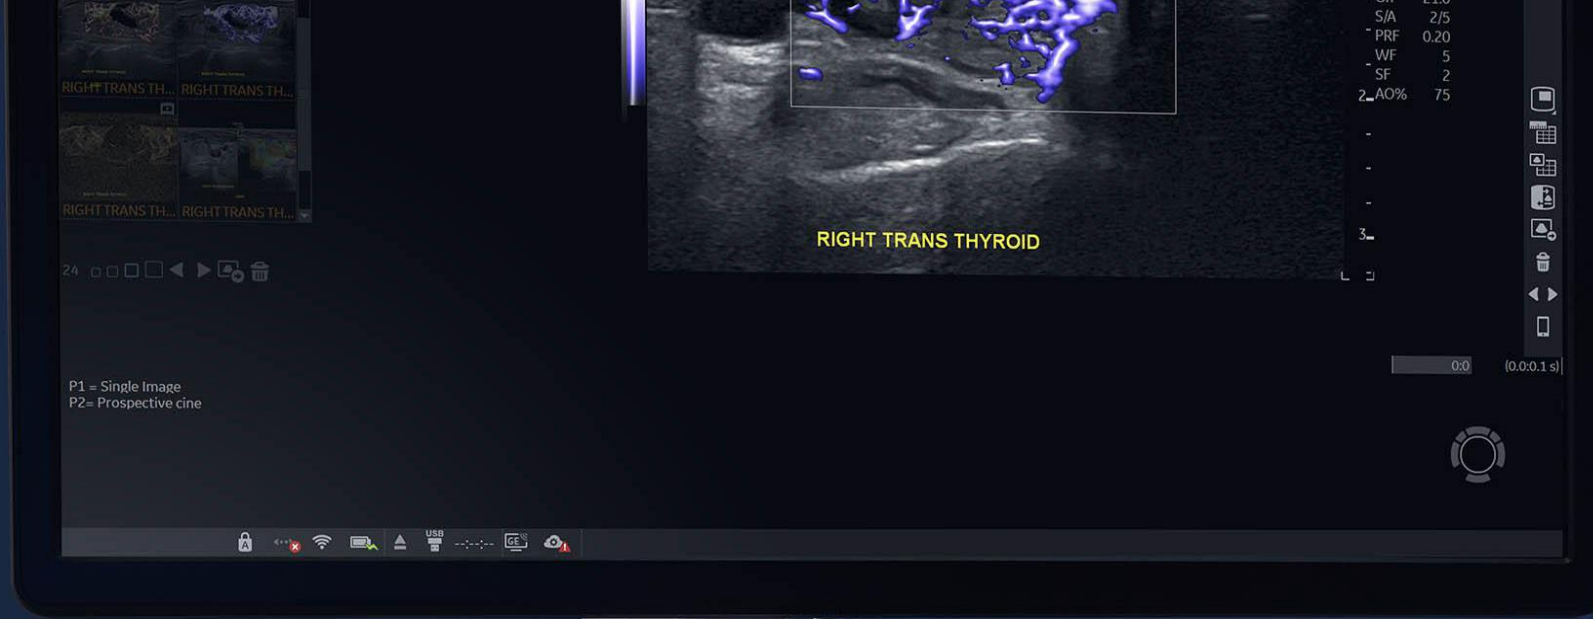

# LOGIQ Fortis

## Product Tree EMEA

Rev. 5

May 12th, 2022





# Content

- [Page 3](#) System overview
- [Page 4](#) Base System
- [Page 5](#) Power Cords, Power cords & Keyboards
- [Page 6](#) Manuals and Documentations
- [Page 7](#) XDclear Probes
- [Page 8](#) Probes
- [Page 9](#) TEE Probe
- [Page 10](#) Biopsy Guides
- [Page 11](#) Clinical Care Area Packages
- [Page 12 - 13](#) Software Options
- [Page 14](#) Software As A Service
- [Page 15](#) Hardware Options
- [Page 16](#) Volume Navigation Options
- [Page 17](#) Peripherals
- [Page 18](#) Education offering (EM only)
- [Page 19](#) Veterinary Use
- [Page 20](#) Revision History
- [Page 21](#) Appendix A – SonoDefense Information
- [Page 22](#) Appendix B – Cabinet Compatibility



[System Overview](#)

[Base System](#)

[Power Cords, Power cords & Keyboards](#)

[Manuals & Documentations](#)

[XDclear Probes](#)

[Probes](#)

[TEE probe](#)

[Biopsy Guides](#)

[Clinical Pckg.](#)

[Software Options](#)

[SaaS](#)

[Hardware Options](#)

[V Nav Options](#)

[Peripherals & Accessories](#)

[Education](#)

[Veterinary Use](#)

[Revision History](#)

[Appendix A – Sonodefense](#)



# System overview:

## LOGIQ Fortis

### Probes:

- C1-6(VN)-D
- C2-9(VN)-D
- C3-10-D
- C2-7(VN)-D
- L2-9(VN)-D
- L6-24-D
- L8-18i-D
- L3-12-D
- ML6-15-D
- M5Sc-D
- 6S-D
- 6TC-RS
- IC5-9-D
- RIC5-9-D
- RAB6-D
- BE9CS-D
- P2D
- P6D

### SW Options:

- Coded Contrast Imaging
- UGAP
- Shearwave Elastography
- Strain Elastography
- Cardiac AFI
- DVR
- Report Writer
- Stress Echo
- Tricefy
- LOGIQ Apps
- Scan Assistant
- Auto IMT
- B-Steer+
- Flow QA
- Measure Assist Breast
- Measure Assist OB
- SRI HD Type 2
- SonoNT/SonoIT

### HW Options:

- CW Doppler
- Pencil CW Kit
- Realtime 4D
- Power Assistant
- Scan on Battery
- Wireless LAN
- S-Video Kit

### ECG Options:

- ECG incl. Auto EF, TVI
- ECG cord – IEC & AHA

### Volume Navigation:

- Volume Navigation
- Dual Probe Sensors
- Navigation Stand
- eTrax Tracker
- Virtual Tracker
- OmniTrax (Active Tracker) Kit
- MR Active Tracker
- V Nav brackets

### Printers:

- BW printer UP-D898DC
- Color printer UP-D25MD
- Inkjet printer

### Accessories:

- Tray Box
- Probe Holder Inserts
- Footswitch – 3 buttons
- Protective cover
- UPS

### Veterinary Use:

- Veterinary Kit
- Probe Label Kit



Product Tree LOGIQ Fortis

Item Number	Description	Description / Comments
	Base System	
H43302LA	LOGIQ Fortis Console	

Standard Features (see datasheet for more information)

- 23.8” Wide-screen HDU monitor
- 12,1” High-resolution Touch Display
- Power Cord 220V for EU
- 4 Active Probe Ports, 1 Parking port
- Gel-Warmer
- Mid Cabinet
- LOGIQView
- Privacy & Security Package – SonoDefense Solution

EU offering only

EM / FSA offering only



Product Tree LOGIQ Fortis

Item Number	Description	Description / Comments
	Power Cords	
H46342LZ	Power Cord 220V for EU	Just as a replacement - one is included in the standard config
H46712LM	Power cord UK	Power cord for UK
H46712LR	Power cord ISRAEL	Power cord for Israel
H46712LS	Power cord SWISS	Power cord for Swiss
H46712LT	Power cord DENMARK	Power cord for Denmark
H46692LK	Power cord DENMARK Grey	Power cord DK STD C13 GRY
H46722LD	Power cord ITALY	Power cord for Italy - <b>only order if needed, standard EU power cord should be feasible for most Italian installations</b>
H46712LW	Power cord US	Power cord US
H46712LN	Power cord South Africa	Power cord South Africa
	Alphanumeric Keyboards	
H43342LR	AN Keyboard ENGLISH	AN Keyboard ENGLISH
H43342LS	AN Keyboard GERMAN	AN Keyboard GERMAN
H43342LT	AN Keyboard FRENCH	AN Keyboard FRENCH
H43342LW	AN Keyboard GREEK	AN Keyboard GREEK
H43342LY	AN Keyboard NORWEGIAN	AN Keyboard NORWEGIAN
H43342LZ	AN Keyboard RUSSIAN	AN Keyboard RUSSIAN
H43352LA	AN Keyboard SWEDISH	AN Keyboard SWEDISH

EU offering only

EM / FSA offering only



Product Tree LOGIQ Fortis

EU offering only

EM / FSA offering only

Item Number	Description	Item Number	Description
<b>Manuals and Documentation (Hard Copies)</b> <b>Contains: Basic User manual (translated), Advanced Reference Manual (English), Release Notes (translated), Service Manual (English)</b>			
H43312LA	LOGIQ Fortis Italian DOCs Kit	H43312LW	LOGIQ Fortis Latvian DOCs Kit
H43312LB	LOGIQ Fortis Bulgarian DOCs Kit	H43312LZ	LOGIQ Fortis Lithuanian DOCs Kt
H43312LC	LOGIQ Fortis Croatian DOCs Kit	H43322LA	LOGIQ Fortis Norwegian DOCs Kit
H43312LE	LOGIQ Fortis Czech DOCs Kit	H43322LC	LOGIQ Fortis Euro Port DOCs Kit
H43312LF	LOGIQ Fortis Danish DOCs Kit	H43322LD	LOGIQ Fortis Polish DOCs Kit
H43312LG	LOGIQ Fortis German DOCs Kit	H43322LE	LOGIQ Fortis Romanian DOCs Kit
H43312LH	LOGIQ Fortis Dutch DOCs Kit	H43322LF	LOGIQ Fortis Serbian DOCs Kit
H43312LJ	LOGIQ Fortis English DOCs Kit	H43322LG	LOGIQ Fortis Swedish DOCs Kit
H43312LK	LOGIQ Fortis Estonian DOCs Kit	H43322LH	LOGIQ Fortis Slovakian DOCs Kit
H43312LL	LOGIQ Fortis French DOCs Kit	H43322LJ	LOGIQ Fortis Slovenian DOCs Kit
H43312LM	LOGIQ Fortis Finnish DOCs Kit	H43322LK	LOGIQ Fortis Spanish DOCs Kit
H43312LN	LOGIQ Fortis Greek DOCs Kit	H43322LL	LOGIQ Fortis Turkish DOCs Kit
H43312LP	LOGIQ Fortis Hungarian DOCs Kit	H43322LM	LOGIQ Fortis Russian DOCs Kit
H43312LS	LOGIQ Fortis Ukrainian DOCs Kit	H43322LN	LOGIQ Fortis R3 Advanced Reference Manual - English
H43322LS	LOGIQ Fortis R3 Kazakhstan Docs Kit	H43322LT	LOGIQ Fortis R3 Advanced Reference Manual - French

**Note: Electronic Instructions for Use (eIFU) containing a leaflet with instructions translated into all languages and a USB Stick with all User Documentation are included with every system.**  
**Above DOCs Kits are only needed if a customer requires a printed copy of the documents listed below (electronic versions of those are included in the eIFU).**

[System Overview](#)

[Base System](#)

[Power Cords, Power cords & Keyboards](#)

[Manuals & Documentation](#)

[XDclear Probes](#)

[Probes](#)

[TEE probe](#)

[Biopsy Guides](#)

[Clinical Pckg.](#)

[Software Options](#)

[SaaS](#)

[Hardware Options](#)

[V Nav Options](#)

[Peripherals & Accessories](#)

[Education](#)

[Veterinary Use](#)

[Revision History](#)

[Appendix A – Sonodefense](#)



Product Tree LOGIQ Fortis

Item Number	Description	Description / Comments
	<b>XDclear Curved Array Probes</b>	
H40472LT	C1-6-D XDclear Convex Array Probe	<b>*Note:</b> <b>‘VN’ Probes also work on systems without V Nav Option</b>
H40472LW	C1-6VN-D ‘VNav Inside’ XDclear Convex Probe*	
H40462LN	C2-9-D XDclear Convex Array Probe	
H40472LY	C2-9VN-D ‘VNav Inside’ XDclear Convex Probe*	
H40482LB	C3-10-D XDclear Microconvex Probe	
		H4915P Probe Holder Insert 2 recommended
	<b>XDclear Linear Array Probes</b>	
H44901AI	L2-9-D XDclear Linear Array Probe	
H44901AJ	L2-9VN-D ‘VNav Inside’ XDclear Linear Array Probe*	
	<b>XDclear Sector Phased Array Probes</b>	
H44901AE	M5Sc-D XDclear Sector Phased Array Probe	CW Doppler requires H43342LA CW Doppler Kit
	<b>XDclear Pobe Enabler</b>	
H46612LS	Advanced Probes	SW option to enable XDclear probes; mandatory with following probes: H40472LT, H40472LW, H40462LN, H40472LY, H40482LB, H44901AI, H44901AJ, H44901AE

EU offering only

EM / FSA offering only



Product Tree LOGIQ Fortis

Item Number	Description	Description / Comments
	2D Curved Array Probes	
H46422LM	C2-7-D Probe	<b>*Note:</b> <b>‘VN’ Probes also work on systems without V Nav Option</b>
H46422LN	C2-7VN-D Probe*	
	2D Linear Array Probes	
H40452LG	ML6-15-D Active Matrix Linear Array Probe	
H40452LL	L8-18i-D Linear Array Hockeystick Probe	H43352LC Small Probe Holder recommended
H48062AA	L3-12-D Probe Linear Probe	
H4920HF	L6-24-D Linear Array Hockeystick Probe	H43352LC Small Probe Holder recommended
	2D Sector Phased Array Probes	
H45021RR	6S-D Sector Probe	CW Doppler requires H43342LA CW Doppler Kit
	2D Endocavitary Probes	
H40442LK	IC5-9-D Micro Convex Endocavitary Probe	
H40482LE	BE9CS-D Biplane Endocavitary Probe	
	4D Mechanical Probes	
H48681MG	RAB6-D Volume Convex Probe	Requires H43342LB Realtime 4D Option Kit
H48651MS	RIC5-9-D Volume Endocavitary Probe	
	Pencil Probes	
H4830JE	P2D - 2 MHz CWD Pencil Probe	Requires H43342LA CW Doppler Kit <u>and</u> H43342LJ Pencil CW Installation Kit
H4830JG	P6D - 6 MHz CW Pencil Probe	Requires H43342LA CW Doppler Kit and H43342LJ Pencil CW Installation Kit

EU offering only

EM / FSA offering only



Product Tree LOGIQ Fortis

Item Number	Description	Description / Comments
	TEE Adult Probe	
H45551ZE	6Tc-RS Multi-Plane TEE Probe	CW Doppler requires H43342LA CW Doppler Kit
H46352LK	TEE RS-DLP Adapter	MANDATORY!
	TEE Probe Accessories	
H45551NM	TEE Storage Rack	Strongly recommended to order with the TEE probe For storage of Adult and Pediatric TEE probes, wall mounted unit. Store (and dry) disinfected probes, ready for the next use.
H45521CK	TEE Scan-head protection cover	ADULT TEE SCANHEAD PROTECTION COVER
H45511EE	TEE Clip-on Bite Guard Adult	TEE clip-on bite guard for adults, keyhole type
H45521CB	TEE Clip-on Bite Guard Adult OR	TEE clip-on bite guard for adults, U-form type - Operating Room use
H45521JH	Conventional Bite Guard Adult	TEE clip-on bite guard for adults, U-form type
H45531HS	Bite Hole Indicator	Bite Hole Indicator for TEE Probes; Type: KZ200800

TEE Probe user manuals				
H45531RA	TEE Probes User Manual - English German French Chinese	H45541PP	TEE Probes User Manual - Czech	
H45531RD	TEE Probes User Manual - Italian	H45541PQ	TEE Probes User Manual - Latvian	
H45531RE	TEE Probes User Manual - Spanish	H45541PR	TEE Probes User Manual - Lithuanian	
H45531RJ	TEE Probes User Manual - Swedish	H45541PS	TEE Probes User Manual - Turkish	
H45531RK	TEE Probes User Manual - Norwegian	H45541PT	TEE Probes User Manual - Estonian	
H45531RL	TEE Probes User Manual - Danish	H45551ZQ	TEE Probes User Manual - Serbian	
H45531RM	TEE Probes User Manual - Polish	H45551ZR	TEE Probes User Manual - Bulgarian	
H45531RN	TEE Probes User Manual - Finnish	H45561RH	TEE probes User manual - Croatian	
H45531RP	TEE Probes User Manual - Greek	H45581AN	TEE Probes User Manual - Portuguese	
H45531RQ	TEE Probes User Manual - Russian	H45581PL	TEE Probes User Manual - Ukrainian	
H45531RR	TEE Probes User Manual - Dutch	H45581PT	TEE Probes User Manual - Slovenian	
H45541PL	TEE Probes User Manual - Hungarian	H45601HR	TEE Probes User Manual - Kazakh	
H45541PM	TEE Probes User Manual - Slovak			
H45541PN	TEE Probes User Manual - Romanian			

EU offering only

EM / FSA offering only





Product Tree LOGIQ Fortis

EU offering only

EM / FSA offering only

Item Number	Description	Description / Comments
	<b>Biopsy Guides (Biopsy Guides only, not for VNAV)</b>	
	<b>Biopsy Options 2D Curved Array</b>	
H4917VB	C1-6 Biopsy Starter Kit ( <i>Verza</i> )	
H40482LK	C2-7 Biopsy Kit	
H40482LL	C2-7 Stainless Biopsy Kit	
H4913BA	C2-9 Biopsy Starter Kit	
	<b>Biopsy Options 2D Linear Array</b>	
H44901AM	L2-9-D Biopsy Starter Kit ( <i>Verza</i> )	
H40432LJ	ML6-15-D Biopsy Starter Kit	
H48302AA	L3-12 Biopsy Kit	
	<b>Biopsy Options 2D Sector Phased Array</b>	
H45561FC	M5Sc-D Biopsy Bracket	
	<b>Biopsy Options 2D Endocavity</b>	
E8385MJ	E8C/IC5-9 Short Biopsy Kit (disposable)	This Kit Contains 24 Disposable Biopsy Needle Guides
H40412LN	E8C/IC5-9 Re-usable Biopsy Device	One stainless steel single angle, reusable biopsy kit for E8CS/E8C/E721/IC5-9 transducers.
E8387M	Sterile Disposable Biopsy Needle Guide Kit for BE9C Probe	This Kit Contains 24 Disposable Biopsy Needle Guides (Protek)
H42742LJ	BE9CS Biopsy Kit	This Kit Contains 24 Disposable Biopsy Needle Guides (Civco)
E8387MA	Reusable Biopsy Needle Guide for BE9C Probe	One stainless steel single angle, reusable biopsy kit
	<b>Biopsy Options 4D</b>	
H48681ML	RAB6-D Biopsy Starter Kit	None sterile multi angle bracket (Depth crossing w/ probe axis at 4, 6, 8 cm) & 5 needle guide kits
H46721R	RIC5-9-D Reusable Biopsy Guide	Reusable Stainless Steel: PEC 63 (<1.6 mm)
H48691Z	RIC Probe Disposable Biopsy Guide with Latex Cover	Civco - 24 Sterile endocavity needle guide kits with latex covers
H48681GF	RIC Probe Disposable Biopsy Guide without latex covers	Civco - 24 Sterile endocavity needle guide kits without covers





Product Tree LOGIQ Fortis

Item Number	Description	Description / Comments
	Software Options	
	<u>Care Area Packages</u>	
H43332CA	Cardiac Package	The Cardiac Package includes the following advanced tools: ECG Kit (incl. AutoEF & TVI) , IEC ECG cable, Cardiac AFI, Stress Echo, AutoIMT, Flow QA, Comapre Ass., Scan Ass.
H43332BR	Breast Package	The Breast Package includes the following advanced tools: B-Flow, Coded Contrast, Shearwave Elastography, Elastography, Elasto QSA, Breast Productivity, Measure Ass. Breast, B Steer+, Compare Ass., Scan Ass., LOGIQ Apps
H43332OB	OB Package	The OB Package includes the following advanced tools: Realtime 4D Kit, SRI HD type 2, OmniView, STIC, TUI; VCI-Static, VOCAL II, SonoNT/IT, Measure Ass. OB, Compare Ass., Scan Ass., LOGIQ Apps, Tricefy
H43332MS	MSK Package	The MSK Package includes the following advanced tools: B-Flow, Shearwave Elastography, B Steer+, Compare Ass., Scan Ass., LOGIQ Apps

EU offering only

EM / FSA offering only



Product Tree LOGIQ Fortis

EU offering only

EM / FSA offering only

Item Number	Description	Description / Comments
	Software Options 1/2	
	<u>Connectivity</u>	
H46622LA	DICOM	
H46622LL	Adv. Security	Vulnerability Scan Option for Nessus Server communication
H46622LT	Tricefy	Trice Imaging Ultrasound Cloud Solution
H46622LW	LOGIQ Apps	Requires H46612LH Wireless Option Kit for Bluetooth capability
H4918DR	DVR	Digital Video Recorder
	<u>Imaging</u>	
H46612LY	B-Flow	
H4920SR	SRI HD Type 2	For OB/Gyn application only
H46612LS	Advanced Probes	To enable XDclear probes
	<u>Comprehensive Tools</u>	
H43332LA	Coded Contrast	Incl. TIC Analysis
H43332LB	Parametric Imaging	
H46622LE	Shear Wave Elastography	
H46622LH	UGAP	Ultrasound Guided Attenuation Parameter
H43332LE	Hepatic Assistant	Both SWE (H46622LE) and UGAP (H46622LH) are required
H43332LC	Strain Elasto	
H43332LD	Elasto QA	Elastography quantification tool
H46622LS	Stress Echo	
H46622LN	Cardiac AFI	Cardiac Strain
H46622LB	FLOW QA	Quantification tool for Color Flow and Power Doppler imaging
H46612LW	B Steer+	B mode steering image to help improve needle visualization/reflectivity

[System Overview](#)

[Base System](#)

[Power Cords, Power cords & Keyboards](#)

[Manuals & Documentation](#)

[XDclear Probes](#)

[Probes](#)

[TEE probe](#)

[Biopsy Guides](#)

[Clinical Pckg.](#)

[Software Options](#)

[SaaS](#)

[Hardware Options](#)

[V Nav Options](#)

[Peripherals & Accessories](#)

[Education](#)

[Veterinary Use](#)

[Revision History](#)

[Appendix A – Sonodefense](#)



Product Tree LOGIQ Fortis

Item Number	Description	Description / Comments
	Software Options 2/2	
	<u>Concise Workflow</u>	
H46622LZ	Scan Assistant	
H46612LZ	Compare Assistant	
H46622LR	Report Writer	
H43332LL	Thyroid Productivity	Thyroid-specific measurement package allows user to enter TI-RADS criteria/assessment
H43332LM	Breast Productivity	Breast-specific measurement package allows user to enter BI-RADS criteria/assessment
H46622LC	Measure Assist Breast	
H46622LD	Measure Assist OB	
H46612LT	AUTO IMT	
H46622LJ	SonoNT/SonoIT	Sonography based Intracranial Translucency & Nuchal Translucency Measurement
	<u>3D/4D</u>	
H43332LF	Omni View	OmniView helps improve the contrast resolution and visualization of the rendered anatomy in any image plane
H43332LG	STIC	Advanced STIC (Spatio-Temporal Image Correlation)
H43332LH	TUI	Tomographic Ultrasound Imaging (TUI) enables volume data to be viewed in multiple slices
H43332LJ	VCI-Static	Static Volume Contrast Imaging is a volume acquisition technique which helps improve B-mode contrast resolution and speckle suppression
H43332LK	VOCAL_II	VOCAL provides both contour detection (manual, semi-automated or automated) and automated volume calculation

EU offering only

EM / FSA offering only



Product Tree LOGIQ Fortis

Item Number	Description	Description / Comments
	Software Options	
	Breast Assistant powered by Koios DS™	
H46622LY	KOIOS SW*	Breast Assistant SW option powered by Koios
	Software As A Service Option	
H4919KI	LOGIQ Koios Installation Service*	<b>Mandatory to be ordered for Koios Software Installation on Customer on-premises Server</b> (1st time only)
H4919SO	LOGIQ Breast Assistant Scanner only Subscription*	- One Year Subscription for 100 breast exams on Scanner Only - <b>Must order a minimum of 6 per customer</b> - 12 months plus 2 additional months at no charge (first year only)
H4919SP	LOGIQ Breast Scanner and PACS WS Subscription*	- One Year Subscription for 100 breast exams on PACS + Scanner - <b>Must order a minimum of 6 per customer</b> - 12 months plus 2 additional months at no charge (first year only)

EU offering only

EM / FSA offering only



**\*LOGIQ™ Breast Assistant powered by Koios DS™ commercial availability is subject to RA clearance in each country and upon regional go-to market strategy”**



Product Tree LOGIQ Fortis

EU offering only

EM / FSA offering only

Item Number	Description	Description / Comments
	Hardware Options	
H43342LA	CW Doppler Option kit	- includes SW Option Key in OAC
H43342LJ	Pencil CW Installation kit	- includes SW Option Key in OAC - Requires H43342LA CW Doppler Option
H43342LB	Realtime 4D Option kit	- includes SW Option Key in OAC
H43342LE	Power Assistant Option kit	Exclusive with "H43342LE Scan on Battery Option kit"
H43342LD	Scan on Battery Option kit	Exclusive with "H43342LD Power Assistant Option kit"
H43342LG	Wireless Option kit	- includes SW Option Key in OAC
H43342LH	S-Video Option Kit	
	ECG Option	
H43342LC	ECG Installation kit	- Requires H43342LP 5inch bay installation kit - includes SW Option Key in OAC Includes: - Auto Ejection Fraction Option - Tissue Velocity Imaging Option
H4911JC	ECG cords - IEC Style	
H4910EC	ECG cords – AHA styles	For USA/Emerging Market use
H45521AL	ECG Cable set ext.	Set of various cables and connectors to enable connection of ECG from stress treadmills and ECG monitors.
	Cabinet options	
H43342LL	High Cabinet	Refer to appendix B for cabinet compatibility
H43342LM	Low Cabinet	
H43342LN	Side Cabinet	
H43342LP	5inch bay Installation kit	Mandatory to be ordered with H43342LC and/or H43342LF (one kit)

Only one option can be selected:  
H43342LE OR H43342LD

Refer to appendix B for cabinet compatibility

[System Overview](#)

[Base System](#)

[Power Cords, Power cords & Keyboards](#)

[Manuals & Documentation](#)

[XDclear Probes](#)

[Probes](#)

[TEE probe](#)

[Biopsy Guides](#)

[Clinical Pckg.](#)

[Software Options](#)

[SaaS](#)

[Hardware Options](#)

[V Nav Options](#)

[Peripherals & Accessories](#)

[Education](#)

[Veterinary Use](#)

[Revision History](#)

[Appendix A – Sonodefense](#)



Product Tree LOGIQ Fortis

EU offering only

EM / FSA offering only

Item Number	Description	Description / Comments
	Volume Navigation	
	V Nav Hardware Options	
H43372LK	Volume Navigation Kit	- includes SW Option Key in OAC - Requires H43342LP 5inch bay installation kit
H4913PS	V Nav Dual Probe Sensors	For V Nav bracket probes: C3-10, IC5-9, ML6-15, L8-18i, M5Sc
H4908NS	Volume Navigation Stand	
	V Nav Brackets	
H40482LF	C3-10 V Nav Holder St Kit	<b>C1-6 and C2-9 V Nav brackets are not supported on LOGIQ Fortis. Only C1-6VN-D &amp; C2-9VN-D probes are supported in V Nav.</b>
H4908NF	IC5-9 Volume Navigation Bracket	
H40432LK	ML6-15 Volume Navigation Bracket	
H4908NH	L8-18i-D V Nav Bracket	
H4908NM	M5Sc-D V Nav Bracket	
	V Nav Needle Tracking Options	
H4910NT	V Nav eTRAX 16/18G Starter Kit	For use of 18G biopsy needles
H4913NT	V Nav eTRAX 18/20G Starter Kit	For use of 20G biopsy needles
H4913NU	V Nav eTRAX 12/14G Starter Kit	For use of 14G biopsy needles
H4913NV	V Nav eTRAX 14/16G Starter Kit	For use of 16G biopsy needles
H4910NY	V Nav Virtual Needle Tracker	VirtuTRAX Instrument Navigator (10FR-14GA)
H4911NG	Virtual Tracker Sensor	General Purpose Electromagnetic Sensor
H4913NS	V Nav Needle Tracking storage insert	
	V Nav Active Tracker	
H4913AT	omniTRAX Active Patient Tracker Kit	Non-sterile reusable general purpose electromagnetic sensor with omniTRAX Patient Tracker 10.4cm (4.1") (5)
H4915MT	omniTRAX MR Active Patient Tracker Kit	Non-sterile reusable general purpose electromagnetic sensor with omniTRAX MR Patient Tracker 10.4cm (4.1") (5)



[System Overview](#)

[Base System](#)

[Power Cords, Power cords & Keyboards](#)

[Manuals & Documentation](#)

[XDclear Probes](#)

[Probes](#)

[TEE probe](#)

[Biopsy Guides](#)

[Clinical Pckg.](#)

[Software Options](#)

[SaaS](#)

[Hardware Options](#)

[V Nav Options](#)

[Peripherals & Accessories](#)

[Education](#)

[Veterinary Use](#)

[Revision History](#)

[Appendix A – Sonodefense](#)




Product Tree LOGIQ Fortis

Item Number	Description	Description / Comments
	Peripherals	
H43342LK	Onboard Printer UP-D898DC	Onboard Installation
H4911JT	Sony UP-D25MD Color Printer	A6 Digital Color Printer for <u>off-board</u> installation, incl. EU 220V power cord; an appropriate power cord is required from the power cord list.
H4918RP	LOGIQ Inkjet Printer	For <u>off-board</u> installation, HP Officejet Pro 8210 Printer incl. USB-cable 2.0
	Accessories	
H46732LF	USB FOOTSWITCH 3 Button	
H43352LC	Small Probe Holder	
H43352LD	VERTICAL TV PROBE Holder	Position on L/H side of the OPIO
H43352LE	TVTR Probe Holder	
H44412LA	PROBE CABLE HANGER	
H43372LF	TRAY BOX	H43372LG is required for installation
H43372LG	TRAY Bracket	Brackets for tray box; H43372LF is required
H4918DC	LOGIQ Protective Cover	LOGIQ padded canvas cover to protect the ultrasound system for transport or storage
H43272LJ	Ethernet protection cable	
	UPS	
H4921UP	Powervar 1.44kVA 230V UPS medical grade	Must order H46672LM and specified power cord {H48502AW / H48512AF / H48512AJ / H48532AY} at same time
H46672LM	UPS Document Kit	Mandatory to be ordered if H4921UP is selected
H48502AW	AC Power Cord Europe/Korea	For use with H4921UP
H48512AF	AC Power Cord UK/Ireland	For use with H4921UP
H48512AJ	AC Power Cord Switzerland	For use with H4921UP
H48532AY	Power Cord for Denmark, Hospital Grade C13 RED	For use with H4921UP

EU offering only

EM / FSA offering only

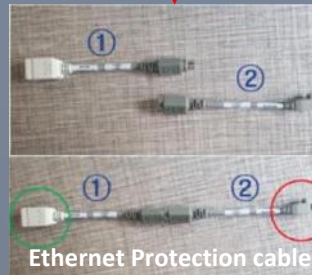

[System Overview](#)

[Base System](#)

[Power Cords, Power cords & Keyboards](#)

[Manuals & Documentation](#)

[XDclear Probes](#)

[Probes](#)

[TEE probe](#)

[Biopsy Guides](#)

[Clinical Pckg.](#)

[Software Options](#)

[SaaS](#)

[Hardware Options](#)

[V Nav Options](#)

[Peripherals & Accessories](#)

[Education](#)

[Veterinary Use](#)

[Revision History](#)

[Appendix A – Sonodefense](#)






GE Healthcare

# LEAD

LOGIQ Expert  
Academy Days

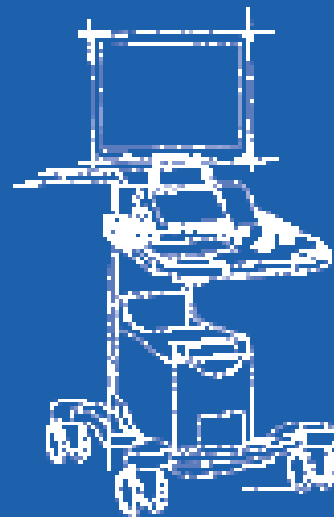

## LEAD Mission

Developing Skills and Improving  
Knowledge of Leadership Ultrasound

## LEAD Vision

Brining Experts together and Building  
a LOGIQ Super Users Network

GE Healthcare Ultrasound Middle East offers various educational experiences which aims to develop ultrasound skills, improve knowledge of advanced ultrasound and elevate diagnostic confidence.

H4917LC

LEAD Course - GIUS

For Emerging Markets offering only



Product Tree LOGIQ Fortis

Item Number	Description	Description / Comments
	Veterinary Use Items	
H43352LB	Console Veterinary Kit	Contains Vet console labels and multi-language Vet User Manual Addendum
H48492AW	Vet Probe Caution Labeling Kit	One Kit to be ordered for each probe

EU offering only

EM / FSA offering only

**Caution:**

For Veterinary use, dedicated VET Kits containing console and probe labels indicating that the system and probes are for veterinary use only must be ordered with the console and for each probe. A dedicated ‘VET Addendum’ to the Basic User Manual is also included.

Labels will be applied to the console and probes by either the Make Center or the LPC before shipping the system/probes.

**It is not allowed to ship/install any system and probe for Veterinary usage not being labeled “For Veterinary Use Only”**



# LOGIQ Fortis Product Tree

## Revision History

Rev	Date	Created by	Description of Changes
1	Dec 03, 2021	Jens Heimann	Initial Release
2	Feb 08, 2022	Jens Heimann	Corrected descriptions, typos, requirements Added UPS (page17)
3	Mar 01, 2022	Jens Heimann	Added Care Area Packages (page 11) Replaced Volume Navigation Kit H43342LF by H43372LK (page 16); dual probe sensor cable is no longer included Added Appendix B Cabinet Compatibility
4	Mar 08, 2022	Jens Heimann	Corrected Hcat for Strain Elastography to H43332LC (page 12)
5	May 12, 2022	Jens Heimann	Added H45521AL ECG Cable Set Kit ext. (page 15)





# Appendix A

SonoDefense is part of the main console and not an option.


## Defense-in-depth strategy

SonoDefense is designed for maximum security protection with a defense-in-depth strategy that incorporates security controls deployed in multiple layers. This approach enhances security by protecting the system against any particular attack using several independent methods.

Limits what can be run on the LOGIQ™ E10

- Customizable, role-based access
- Federated Identity Management
- Session management
- Auditing
- Secure remote access

- Customizable patient data encryption
- Enterprise wireless encryption
- IPv6 Internet Protocol address standard

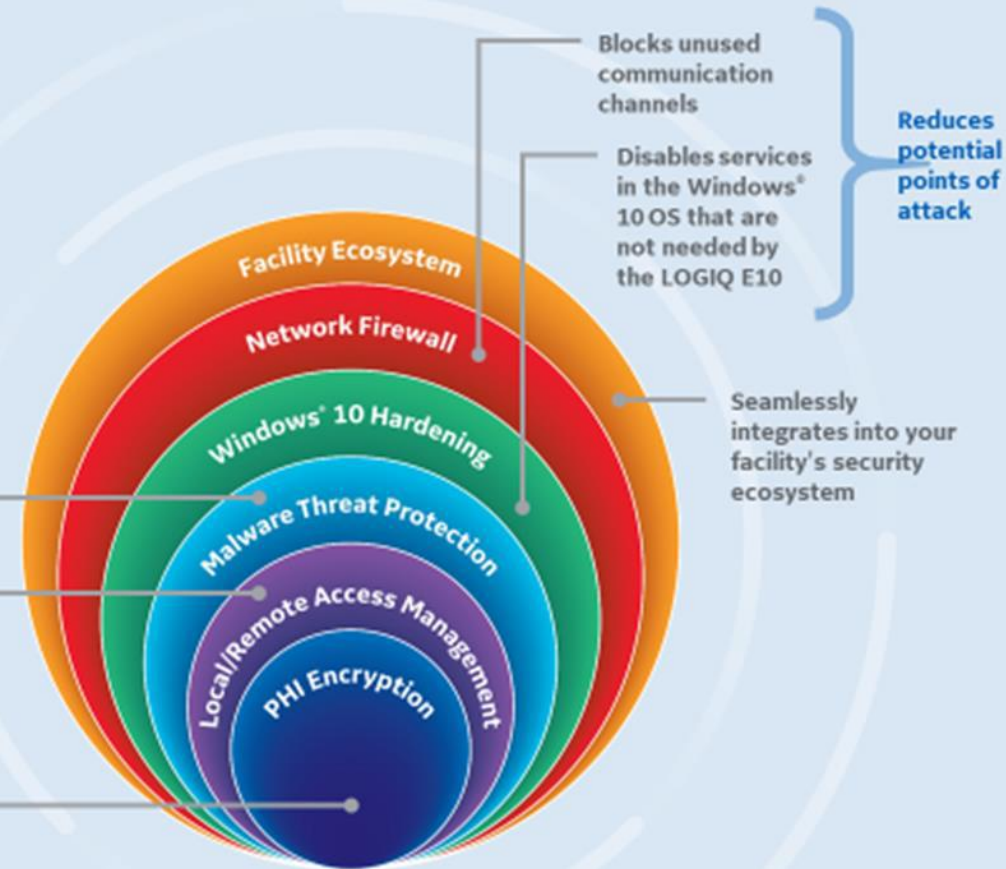

LOGIQ E10 R2 Customer Presentation | March 20, 2020

Windows is a registered trademark of Microsoft Corporation.  
LOGIQ is a trademark of General Electric Company.

188

[System Overview](#)

[Base System](#)

[Power Cords, Power cords & Keyboards](#)

[Manuals & Documentation](#)

[XDclear Probes](#)

[Probes](#)

[TEE probe](#)

[Biopsy Guides](#)

[Clinical Pckg.](#)

[Software Options](#)

[SaaS](#)

[Hardware Options](#)

[V Nav Options](#)

[Peripherals & Accessories](#)

[Education](#)

[Veterinary Use](#)

[Revision History](#)

[Appendix A – Sonodefense](#)



# Appendix B

## Cabinet Compatibility Overview

Cabinet Type	Side Cabinet?	Device Installation Location (Bay)								Note
		A	B-Upper	B-Lower	C-Upper	C-Lower	D	E	F	
Low	No	DVD	-		-		-	-		
	Yes	DVD	-		-		-	Open	BW	
		DVD	-		-		-	P-IO (ECG)	Open	
		DVD			-		-	V-Nav	Open	
		DVD					-	V-Nav	BW	
		DVD					-	P-IO (ECG)	BW	
Mid	No	DVD	Cover		-		-	-		Note 1
		DVD	BW		-		-	-		
		DVD	P-IO (ECG)	Cover	-		-	-		
		DVD	V-Nav	Cover	-		-	-		
		DVD	P-IO (ECG)	V-Nav	-		-	-		
	Yes	DVD	P-IO (ECG)	Cover	-		-	Open	BW	
		DVD	V-Nav	Cover	-		-	Open	BW	
		DVD	P-IO (ECG)	V-Nav			-	Open	BW	
High	No	DVD			P-IO (ECG)	Cover	BW	-		
		DVD			V-Nav	Cover	BW	-		
		DVD			P-IO (ECG)	V-Nav	BW			



*Note 1: Mid cabinet with DVD Drive and cover on device bay is standard LOGIQ Fortis configuration.*







# LOGIQ Fortis™

A powerfully streamlined,  
next-generation ultrasound solution

[gehealthcare.com](http://gehealthcare.com)





# Introducing GE LOGIQ Fortis—the next generation of LOGIQ ultrasound technology.

LOGIQ Fortis—the LOGIQ platform's newest member—provides a multi-purpose, all-in-one, ultra-secure ultrasound solution that can be easily scaled to fit your specific needs.



LOGIQ Fortis is characterized by both its **strength** and its **power**. It gives you the power to enhance your clinical capabilities and increase productivity exponentially.

## Everything you expect in a LOGIQ system—*powerfully streamlined*

With a sleek and compact design, LOGIQ Fortis can be used in almost any space. Its state-of-the-art features and technologies make it strong enough to conduct a full spectrum of ultrasound exams and procedures on any body type. It was specifically designed to optimize clinicians' productivity, exceed expectations regarding performance, and to maximize your investment.

## Clinical Expectations: **EXCEEDED**


With LOGIQ Fortis, you'll find that any expectations you might have regarding an all-in-one, high-performing ultrasound system aren't just met. They're exceeded. If your facility needs a powerful and scalable ultrasound solution, LOGIQ Fortis is the answer.

### **cSound™ Architecture facilitates next-generation imaging**

LOGIQ Fortis features cSound Architecture, which combines versatile XDclear™ probes, cSound Imageformer and new, advanced Speckled Reduction Imaging (SRI) technology. The result is increased processing power that delivers enhanced data throughput for exceptional image quality, clarity and confidence.


### **Advanced quantification simplifies patient management**

Robust tools, such as 2D Shear Wave Elastography and Ultrasound-Guided Attenuation Parameter (UGAP), help reduce the need for invasive procedures and help provide valuable information for patient management decisions.

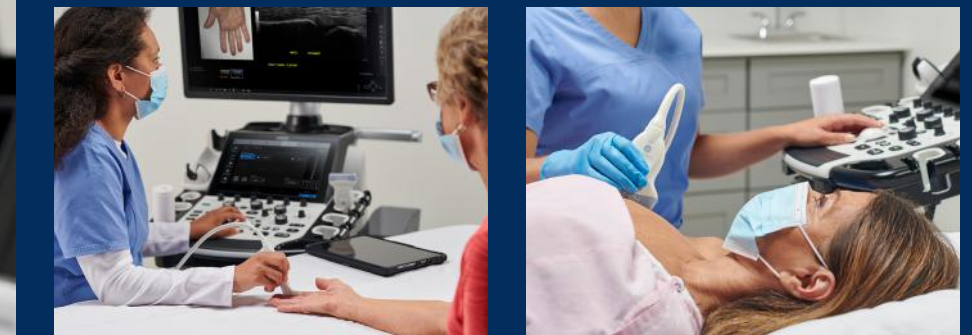





# LOGIQ Fortis at work

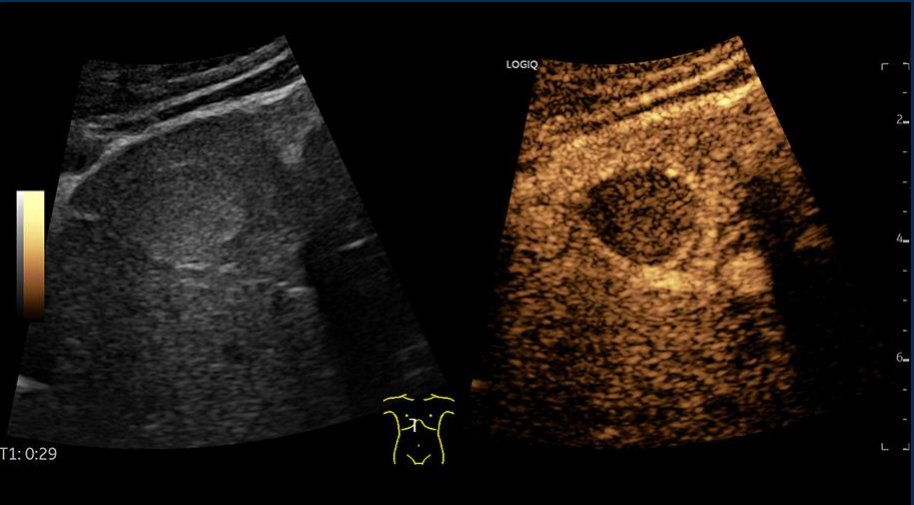


Contrast enhanced liver lesion, C2-9-D

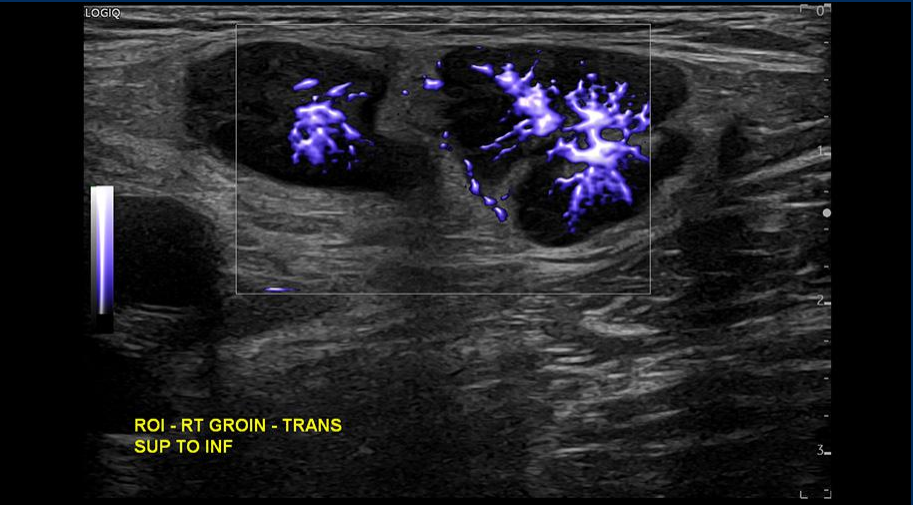


MVI with Radiantflow – groin lymph node, ML6-15-D

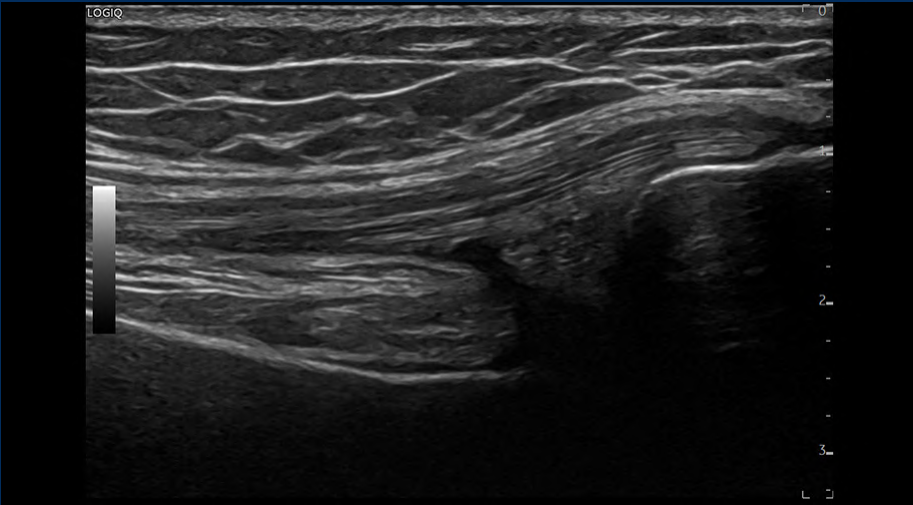


B-Mode with Advanced SRI – knee tendon, ML6-15-D

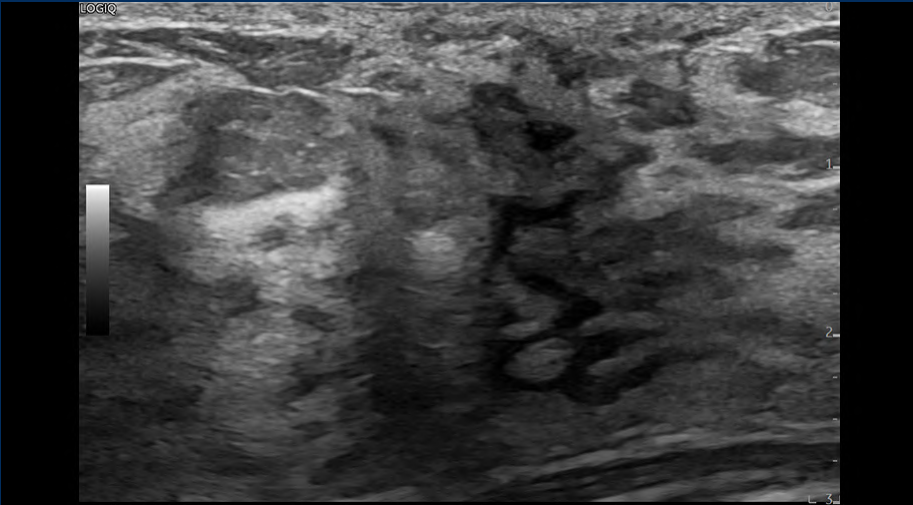


B-Mode with Advanced SRI in breast, ML6-15-D

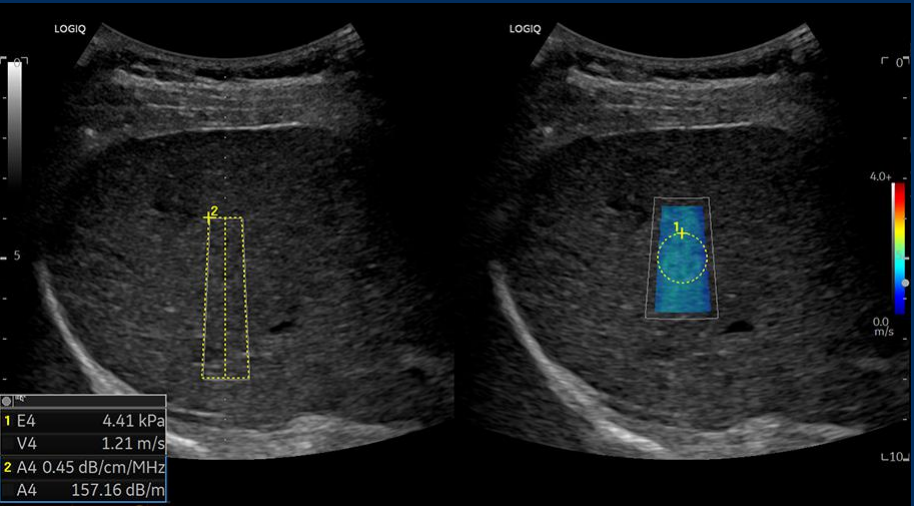

Hepatic Assistant – UGAP and Shear Wave Elastography, C1-6-D

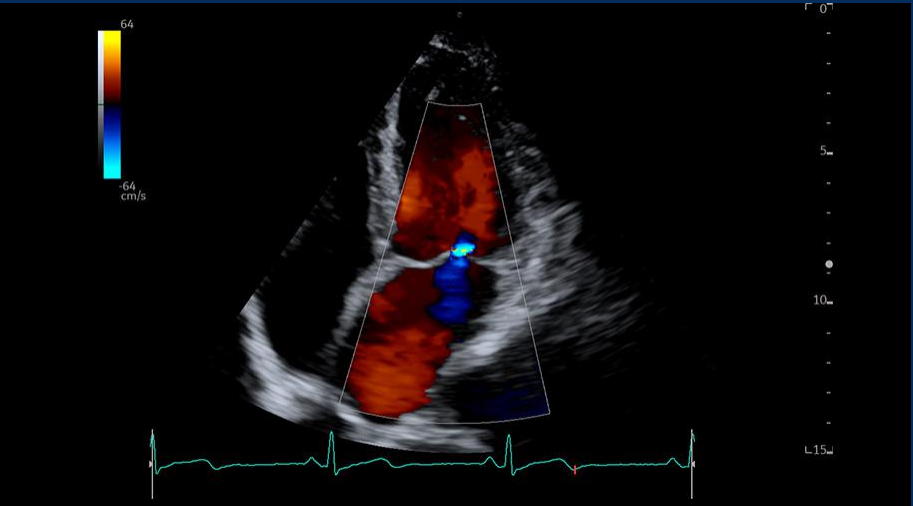

Color flow of mitral valve apical 4-chamber view, M5Sc-D

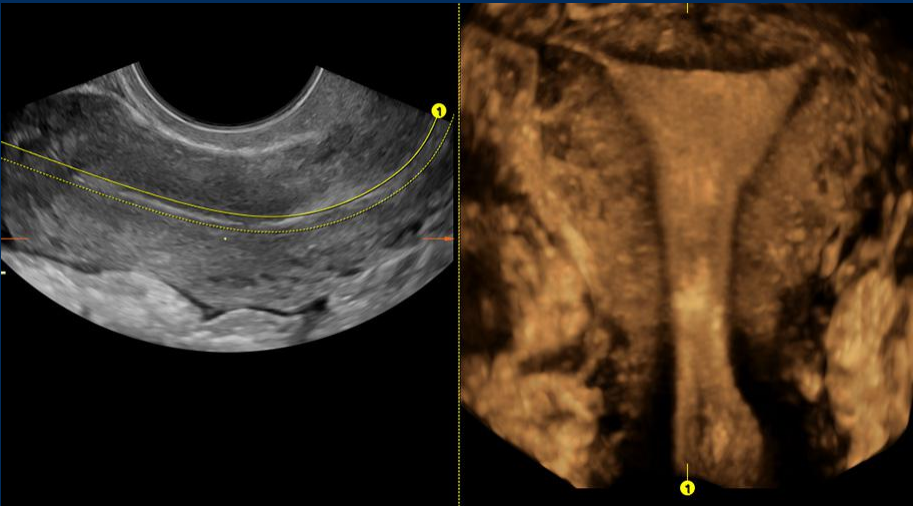

OmniView dual screen, RIC5-9-D

For your multi-purpose ultrasound needs, LOGIQ Fortis is always ready and always by your side.





LOGIQ Fortis helps clinicians streamline their workflow, ensure accurate results, and enhance patient comfort. Its productivity tools help facilitate diagnoses and its design makes it easy to clean and simple to operate.

**A system that’s easily moved to where it’s needed**  
Due to its sleek footprint, LOGIQ Fortis is simple to maneuver and can fit into almost any space—from patient rooms to exam rooms to operating rooms.

**AI-based tools streamline and optimize workflow**  
LOGIQ Fortis harnesses the power of artificial intelligence to improve the speed, ease and comfort of exams. With its AI-based tools, users can achieve exceptional images quickly.




**LOGIQ apps make remote usage possible—and simple**  
A variety of apps for mobile devices add next-level context with photos and enable users to control LOGIQ Fortis remotely. The result is an optimized ergonomic experience for you and your patients.

# Productivity & workflow: OPTIMIZED




# Your investment: MAXIMIZED

When you purchase an ultrasound system, it’s not just an investment for your facility—it’s also an investment in your clinicians and patients. With LOGIQ Fortis, you’ll be able to maximize that investment for everyone. Because it’s easily scaled to meet the evolving needs of today and tomorrow, you’ll be able to depend on LOGIQ Fortis for years to come. And, because it can be used for a wide variety of exams and procedures on any body type, the need to purchase multiple ultrasound systems for different requirements is eliminated. LOGIQ Fortis is the all-in-one ultrasound system that delivers a one-of-a-kind solution.

-  **The A to A digital platform enhances the intelligence of the LOGIQ Fortis**  
From Awareness to Assistance, our A to A digital platform allows your organization to stay at the forefront of clinical imaging. It’s specifically engineered so you can add next-generation capabilities to LOGIQ Fortis in the years ahead.
-  **Lifecycle solutions for where you are today—and where you will be tomorrow**  
The advanced digital support features of LOGIQ Fortis make it easy to optimize your ownership experience. From InSite™ remote support, to iCenter™ performance analytics, to AVURI remote device management, you’ll have access to the tools you’ll need to optimize your assets, streamline your operations, and to ensure you’re prepared to meet your facility’s evolving needs.
-  **SonoDefense Data Security Protection guards your investment 24/7**  
With its multi-layer approach to cybersecurity and data privacy protection, SonoDefense protects LOGIQ Fortis from cyberthreats and unauthorized access around the clock. Your investment is secured—and so is your confidence.



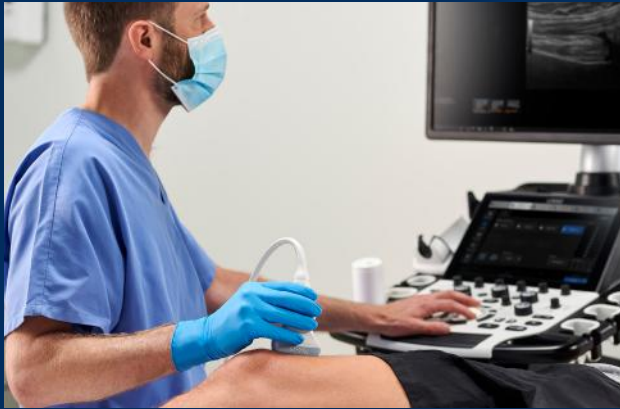

# LOGIQ Fortis

A powerful, streamlined ultrasound solution that's always ready, always by your side.



© GE, 2021

GE Healthcare reserves the right to make changes in specifications and features shown herein, or discontinue the product described at any time without notice or obligation. Contact your GE Healthcare representative for the most current information. GE, the GE Monogram, LOGIQ Fortis, cSound, XDclear and InSite are trademarks of GE. GE Healthcare, a division of GE. GE Medical Systems, Inc., doing business as GE Healthcare.

September 2021  
JB16976XX  
Global