

**Anexa 8 Lampa cu Fanta, Model: TSL-900H, SHANGHAI MEDIWORKS****PRECISION INSTRUMENTS CO., LTD./ Tomey****Nr. de înregistrare AMDM: DM000739306**

Specificarea tehnică deplină solicitată, Standarde de referință	Specificarea tehnică deplină oferita, Standarde de referință
<p>Lampă cu fantă</p> <ol style="list-style-type: none"> <li>1. Iluminare LED</li> <li>2. Tipul microscopului Galilean</li> <li>3. Microscop Binocular</li> <li>4. Schimbarea măririi rotativă în 5 pași</li> <li>5. Mărire totală 6.3X, 10X, 16X, 25X, 40X</li> <li>6. Ocular 12.5X</li> <li>7. Unghiul dintre oculare 10°</li> <li>8. Gama de reglare a dioptriei, dioptrii de la -8 la +8 minim</li> <li>9. Ajustarea pupilară 52mm-80mm</li> <li>10. Sistemul de iluminare: <ul style="list-style-type: none"> <li>- Lățimea fantei, mm 0-14 continuu, adjustabilă</li> <li>- Lungimea fantei, mm 1-14 continuu, adjustabilă</li> <li>- Diametrele aperturii Ø14mm, Ø10mm, Ø5mm, Ø3mm, Ø2mm, Ø1mm, Ø0.2mm</li> <li>- Unghiul fantei 0°~180°</li> <li>- Înclinarea fantei 5°, 10°, 15°, 20°</li> <li>- Filtre minim: filtru de absorbție a căldurii, filtru ND, filtru fără roșu, filtru albastru de cobalt, filtru galben încorporat</li> <li>- Iluminare <math>\geq</math>150KLX</li> </ul> </li> <li>11. Posibilitatea de a transforma lampa cu fantă într-o lampa digitală cu fantă</li> <li>12. Gama de mișcare: <ul style="list-style-type: none"> <li>- Deplasarea bazei manevrată de joystic</li> <li>- Deplasare laterală, mm 110</li> <li>- Deplasare în adâncime, mm <math>\geq</math>110</li> <li>- Deplasare în înălțime, mm 30</li> <li>- Reglarea înălțimii bărbiei, mm <math>\geq</math> 80</li> <li>- Alimentarea, 220 V, 50 Hz</li> </ul> </li> </ol>	<p>Lampă cu fantă</p> <ol style="list-style-type: none"> <li>1. Iluminare LED – manual, pag.2</li> <li>2. Tipul microscopului Galilean - manual, pag.2</li> <li>3. Microscop Binocular - manual, pag. 1 (poza), pag.19</li> <li>4. Schimbarea măririi rotativă în 5 pași - manual, pag.2,</li> <li>5. Mărire totală 6.3X, 10X, 16X, 25X, 40X - manual, pag.2</li> <li>6. Ocular 12.5X - manual, pag.2</li> <li>7. Unghiul dintre oculare 10° - manual, pag.2</li> <li>8. Gama de reglare a dioptriei, dioptrii de la -8 la +8 - manual, pag.2</li> <li>9. Ajustarea pupilară 52mm-80mm - manual, pag.2,</li> <li>10. Sistemul de iluminare: <ul style="list-style-type: none"> <li>- Lățimea fantei, mm 0-14 continuu, adjustabilă - manual, pag.2</li> <li>- Lungimea fantei, mm 1-14 continuu, djustabilă - manual, pag.2</li> <li>- Diametrele aperturii Ø14mm, Ø10mm, Ø5mm, Ø3mm, Ø2mm, Ø1mm, Ø0.2mm - manual, pag.2,</li> <li>- Unghiul fantei 0°~180° - manual, pag.2,</li> <li>- Înclinarea fantei 5°, 10°, 15°, 20°- manual, pag.2,</li> <li>- Filtre minim: filtru de absorbție a căldurii, filtru ND, filtru fără roșu, filtru albastru de cobalt, filtru galben încorporat - manual, pag.2,</li> <li>- Iluminare <math>\geq</math>150KLX - manual, pag.2,</li> </ul> </li> <li>11. Posibilitatea de a transforma lampa cu fantă într-o lampa digitală cu fantă - brosura, pag.3,</li> <li>12. Gama de mișcare: <ul style="list-style-type: none"> <li>- Deplasarea bazei manevrată de joystic - manual, pag.12</li> <li>- Deplasare laterală, mm 110 - manual, pag.2,</li> <li>- Deplasare în adâncime, mm 115 - manual, pag.2,</li> <li>- Deplasare în înălțime, mm 30 - manual, pag.3,</li> <li>- Reglarea înălțimii bărbiei, mm <math>\geq</math> 80 - manual, pag.3,</li> <li>- Alimentarea, 220 V, 50/60 Hz - manual, pag.3</li> </ul> </li> </ol>

# SLIT LAMPS TSL-900 SERIES

## LED Slit Lamps



TSL-900H

TSL-900Hdigital

TSL-900Z

With the TSL-900 series you'll get the ideal value for your money:  
**high-performance and affordable for everyone.**

The excellent quality of the HD optical system and the option to choose a digital imaging system will enable precise observation of the patient's eye. For reliable results and the added value of patient education.

 **TOMEY**

# SLIT LAMPS TSL-900 SERIES

Quality in detail

## MAIN FEATURES AT A GLANCE

### **Illumination system**

- Inclinable (HS-type only)
- Long-life economical LED lamp
- High illumination intensity
- Natural colour temperature
- Optimal observation and analysis of cornea and retina



TSL-900H(digital)



TSL-900Z



### **Metal Plate Table Kit**

- For fast and easy table mounting
- Perfect fit

### **HD optical system with**

#### **5-step magnification**

- Resolution up to 200 lp/mm (2,700 N lp/mm)
- Magnification 6×, 10×, 16×, 25×, 40×
- View every detail of all the various structures



### **All-encompassing filter range**

- Including built-in yellow filter
- Red-free, neutral density, blue, IR heat-absorbing filter
- Diffuser



## OPTIONAL EQUIPMENT

### **TAT-80R Applanation Tonometer**

- Gold standard in IOP measurement
- Best reproducibility and accuracy
- Reliable and durable



### **Measuring eyepiece**

- With a reticle inside
- Convenient measurement of pathologies
- For more accurate diagnosis



## **GET YOUR DIGITAL SLIT LAMP**

- TSL-900Hdigital as a complete solution
- Upgrade kit for TSL-900Z and TSL-900H

### **Digital imaging system includes**

- Digital camera system
- Beam-splitter
- USB cable
- Eyeview software
- Compatible with Windows OS
- IR Background illumination module for Meibomian glands observation (TSL-900H/TSL-900Hdigital)

### **Performance**

- Wide dynamic range
- Meibomian glands examination
- Auto exposure
- Auto gain
- Auto white balance
- Auto OD/OS indicator

### **Software features**

- Easy patient management
- Functional analysis of images and videos
- Comparison of several images at one time
- Customisation based on individual needs



### **CAMERA SYSTEM (TSL-900Z + digital upgrade kit/TSL-900Hdigital)**

Resolution	5 MP/2592 × 1944
Connectivity	USB 3.0
Photo format	JPEG
Video format	MP4 H.264
Chip size	1/1.8"
Frame rate	25 fps

---

# USER MANUAL

Slit Lamp Microscope

Model: TSL-900H



## Preface

Thank you for purchasing TSL-900H Slit Lamp Microscope. We totally provide its user manuals in 24 languages on Tomey GmbH official website, including Latvian, Dutch, French, German, Bulgarian, English, Greek, Czech, Danish, Estonian, Swedish, Finnish, Hungarian, Italian, Lithuanian, Polish, Portuguese, Romanian, Slovak, Slovenian, Spanish, Croatian, Turkish and Norwegian. To access, please visit Tomey GmbH website at [www.tomey.de](http://www.tomey.de).

The following is the description and specification of our product:

### General Description

- ❑ This operation instruction is an integral part of the Slit Lamp Microscope. Product-related operation instructions and technical instructions are given in this manual. The address for the user inquiry is recorded on the last page of this manual.
- ❑ This manual contains operation instruction and technical instruction. The equipment classification of the Slit Lamp Microscope according to the requirements of IEC 60601-1 is also given in this manual.
- ❑ The IEC 60601-1 standard stipulates that the applicable marks have been permanently attached to the instrument and are also described in the manual.
- ❑ Working principle: A beam of light attached to the slit lamp projects to the patients' eye, which forms an optical section of the living tissue of the eye, in this way the doctor can finish the observation and examination.
- ❑ Slit Lamp Microscopes are used to observe the disease of the anterior segments and tissue damage of eyes.

### Intended Use

- Intended Purpose

The device is intended for use in eye examination of the anterior eye segment. It is used to aid in the diagnosis of diseases or trauma which affect the structural properties of the anterior eye segment.

- Indications for Use

The use of the slit lamp is indicated for the following medical conditions:

- Local and systemic diseases affecting the eye
- Lesions and defects of the anterior segment
- Acute infections and inflammations
- Presence of intraocular foreign bodies
- Other traumata of the eye

- Intended Population

This device is intended for use on human patients with the physical ability to sit in front of a slit lamp with their head resting against the headrest in a steady position and the mental ability to follow instructions.

- Intended Users

The device is intended to be used by well-trained and authorized healthcare professionals.

- Contraindications

There are no known contraindications.

**Warning statement:**

The installation, operation and use of the device shall only be for the intended purpose, which is defined in this manual. Please pay attention to the warning information described in this manual, related to safety. Any unauthorized personnel shall not conduct the activities on the device.

**Instruments classification:**

According to the IEC 60601-1 classification standard of medical electrical equipment, the slit lamp microscope is a general equipment of Class I continuous operation instrument, which cannot be used under two circumstances: a flammable anesthetic gas and air mixture, oxygen or nitrous oxide gas and air mixture.

**The specification of this slit lamp microscope.**

Microscope: Type:	Galilean-Type
Magnification change:	5 Magnifications
Total magnification Ratio:	6.3X, 10X, 16X, 25X, 40X
Eyepieces	12.5X
Angle between eyepieces:	10°
Pupillary distance adjustment:	52mm~80mm
Diopter adjustment:	-8D—+8D
Field of view:	40X (Ø5.7mm), 25X (Ø8.9mm), 16X (Ø14mm), 10X (Ø22.3mm), 6X (Ø36.2mm)

**Slit Illumination:**

Slit width:	Continuously variable from 0 to 14mm (at 14mm, slit becomes a circle)
Slit length:	Continuously variable from 1mm to 14mm
Lamp:	3V/3W LED module
Slit angle:	0-180 (Adjustable both vertical and horizontal)
Slit inclination	4 step: 5°, 10°, 15°, 20°
Filters:	Heat-absorbing filter, ND filter, Red-free, Cobalt Blue, Build-in Yellow Filter
Aperture diameters:	Ø14mm, Ø10mm, Ø5mm, Ø3mm, Ø2mm, Ø1mm, Ø0.2mm
Luminance:	≥150klx
LED color-temperature:	3000-4000K

**Base**

Longitudinal movement:	115mm
Lateral movement:	110mm
Fine base movement:	15mm

Vertical movement:	30mm
Chin-Rest	
Vertical movement	80mm
Power Supply:	
Input:	100~240V, 50/60Hz
Rated current:	1.2A
Output:	3V (LED)
	Fixation: 15V
Size & Weight:	
Package size	770mm × 470mm × 570mm
Gross weight:	23Kg
Net weight:	17Kg
Working Environment	
Temperature:	+5°C~+40°C
Relative humidity:	≤90%
Air pressure:	860hpa~1060hpa
Storage Environment	
Temperature:	-40°C~+55°C
Relative humidity:	≤90%
Air pressure:	860hpa~1060hpa
Transportation Environment	
Temperature:	-40°C~+55°C
Relative humidity:	≤90%
Air pressure:	860hpa~1060hpa



### General Requirements for Safety

Dear customers, please read the instruction manual carefully before using our products to avoid accidental mechanical hazards and improper use of the user, resulting in unclear images and diagnostic errors. In particular, carefully read the following safety precautions to prevent the product is damaged, personal injury, and other hazards and accidents that may occur.

- 1 The product can only be used by qualified medical staff.
- 2 Do not disassemble or attempt to perform operations that are not described in this instruction manual. If the operation is not performed properly, excessive force may cause damage to the machine or personal injury. If the instrument fails, please read the troubleshooting guide carefully; follow the troubleshooting methods and steps to troubleshoot the problem; if the problems remain unsolved, please contact the authorized distributor or our after-sale service department, and our company will arrange professional maintenance personnel to help you troubleshoot.
- 3 Do not store and use in a flammable, explosive, high temperature, high humidity and dusty environment; use it in a clean room, keeping the product clean and dry.

- 4 Other medical instruments and equipment that installed at the same site must comply with the same electromagnetic compatibility principles. Equipment that cannot comply with or is known to have poor electromagnetic compatibility must be installed at least 3 meters away from the equipment and must be powered by a different power cord.
- 5 Please pay attention to the rating of all electrical connection ports.
- 6 Before using the instrument, please check all the wires are correctly connected; if the wires are inappropriately connected it may cause the instrument to be short-circuited, which may cause the product is damaged and personal injury.
- 7 Users should pay attention when using the instrument, and be careful when moving the parts to avoid damage due to the moving of the base and tilting of the projection tube
- 8 When replacing fuses and other electrical components, turn off the main power switch. Replace the fuse that meets the specifications specified in this manual.
- 9 If there is an need to replace power cord, please use the power cord specified in this manual.
- 10 Don't touch the surface of the lens and prism with hand or hard objects.
- 11 When the device is not operating, the power should be turned off, and cover the device with dust cover.
- 12 To prevent the instrument from falling down to floor, it should be placed on the floor where the inclination angle is less than 10°.
- 13 Please deal with the waste disposal produced by the machine following relevant laws and regulations.
- 14 Please read the safety signs and other illustrations used on this instrument carefully to use the device safely.
- 15 The chin rest has a load capacity of 10 kg.

### THE SAFETY MARKS, PICTURES USED IN THIS INSTRUMENT

According to the IEC 60601-1 standard, the following figures, symbols and marks are used on the products. For the specific meanings, see Table 1 below:

No.	Mark	Description
1		TYPE B
2		Date of Production
3		Consult instructions for use.

4		WEEE mark: Please deal with the waste disposal produced by the machine following relevant laws and regulations.
5		CE mark
6		Part Number
7		Serial Number
8	Output	Located on the base, indicate outlet of the power
9	Input	Located on the base, indicate input of the power
10		Located on the base, use with on and off
11		The mark of light dimmer
12		Caution: Possibly hazardous optical radiation emitted from this product.
13		Medical device
14		Manufacturer information
15		Authorized representative in the European Community
16		Authorized representative in Switzerland

### EMC precautions:

Below cables information are provided for EMC reference.

Cable	Max. cable length, Shielded/unshielded		Number	Cable classification
AC power cable	1.8m	Nonshielded	1 Set	AC Power
DC Power cable	1.36 m	Nonshielded	1 Set	DC Power
DC Power cable for the slit lamp microscope	0.7 m	Nonshielded	1 Set	DC Power
USB cable for the slit lamp microscope	0.3 m	shielded	1 Set	DC Power
USB cable for the slit lamp microscope	1.9 m	shielded	1 Set	DC Power

### Important information regarding Electronic Magnetic Compatibility (EMC)

The slit lamp microscope needs special precautions regarding EMC and put into service according to the EMC information provided in the user manual and other documents; The slit lamp microscope conforms to this EN 60601-1-2:2007+AC:2010/IEC 60601-1-2:2014 standard for both immunity and emissions.

Nevertheless, special precautions need to be observed:

- The use of accessories and cable other than those specified, with the exception of accessories and cables sold of the slit lamp microscope as replacement parts for internal components, may result in increased EMISSIONS or decreased IMMUNITY or decreased LIFESPAN of the Slit Lamp Microscope.
- The slit lamp microscope should not be used adjacent to or stacked with other equipment. In case adjacent or stacked use is necessary, The Slit Lamp Microscope should be observed to verify normal operation in the configuration in which it will be used.

## EMC Information

Guidance and manufacturer's declaration - electromagnetic emissions - for all ME EQUIPMENT and ME SYSTEM.

Table 1: Guidance and manufacturer's declaration – electromagnetic emissions

The slit lamp microscope is intended for use in the electromagnetic environment specified below. The customer or the user of the slit lamp microscope should assure that it is used in such an environment.		
Emissions test	Compliance	Electromagnetic environment - guidance
RF emissions CISPR 11	Group 1	The slit lamp microscope uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment
RF emissions CISPR 11	Class A	The slit lamp microscope is suitable for use in all establishments other than domestic and those directly connected to the public low-voltage power supply network that supplies buildings used for domestic purposes
Harmonic emissions IEC 61000-3-2	Class A	
Voltage fluctuations/ Flicker emissions IEC 61000-3-3	Complies	

Guidance and manufacturer's declaration - electromagnetic immunity - for all ME EQUIPMENT and ME SYSTEM.

Table 2: Guidance and manufacturer's declaration – electromagnetic immunity

The slit lamp microscope is intended for use in the electromagnetic environment specified below. The customer or the user of the slit lamp microscope should assure that it is used in such an environment.			
Immunity test	IEC 60601 Test level	Compliance level	Electromagnetic environment - guidance
Electrostatic Discharge(ESD) IEC 61000-4-2	±6 kV contact ±8 kV air	±6 kV contact ±8 kV air	Floors should be wood, concrete or ceramic tile. If floors are covered with synthetic material, the relative humidity should be at least 30%.
Electrical transient/burst IEC 61000-4-4	fast ±2 kV for power supply lines ±1 kV for input/output lines	±2 kV for power supply lines ±1 kV for input/output lines	Mains power quality should be that of a typical commercial or hospital environment
Surge IEC 61000-4-5	±1 kV lines to lines ±2 kV lines to earth	±1 kV lines to lines ±2 kV lines to earth	Mains power quality should be that of a typical commercial or hospital environment.
Voltage dips, short interruptions and voltage variations on power supply input lines IEC 61000-4-11	<5% $U_T$ (>95% dip in $U_T$ ) For 0,5 cycle 40% $U_T$ (60% dip in $U_T$ ) For 5 cycle	<5% $U_T$ (>95% dip in $U_T$ ) For 0,5 cycle 40% $U_T$ (60% dip in $U_T$ )	Mains power quality should be that of a typical commercial or hospital environment. If the user of slit lamp microscope requires continued operation during power mains interruptions, it is recommended that the slit lamp

	70% $U_T$ (30% dip in $U_T$ ) For 25 cycle <5% $U_T$ (>95% dip in $U_T$ ) For 5 cycle	$U_T$ ) For 5 cycle 70% $U_T$ (30% dip in $U_T$ ) For 25 cycle <5% $U_T$ (>95% dip in $U_T$ ) For 5 cycle	microscope be powered from an uninterruptible power supply or a battery.
Power frequency (50/60Hz) magnetic field IEC 61000-4-8	3A/m	3A/m	Power frequency magnetic fields should be at levels characteristic of a typical location in a typical commercial or hospital environment
Note: $U_T$ is the a.c. mains voltage prior to application of the test level.			

Guidance and manufacturer's declaration – electromagnetic immunity for ME EQUIPMENT and ME SYSTEM that are not LIFE-SUPPORTING.

Table 3: Guidance and manufacturer's declaration – electromagnetic immunity			
The slit lamp microscope is intended for use in the electromagnetic environment specified below. The customer or the user of the slit lamp microscope should assure that it is used in such an environment.			
Immunity test	IEC 60601 test level	Compliance level	Electromagnetic environment-guidance
Conducted RF IEC 61000-4-6	3 Vrms 150 kHz to 80MHz	$V_1=3V$	Portable and mobile RF communications equipment should be used no closer to any part of the SYSTEM, including cables, than the recommended separation distance calculated from the equation applicable to the frequency of the transmitter.  Recommended separation distance $d = \left[ \frac{3.5}{V_1} \right] \sqrt{P} \quad 150\text{KHz to 80MHz}$
Radiated RF IEC 61000-4-3	3 Vrms 80MHz to 2.5GHz	$E_1=3\text{V/m}$	$d = \left[ \frac{3.5}{E_1} \right] \sqrt{P} \quad 80\text{MHz to 800MHz}$ $d = \left[ \frac{7}{E_1} \right] \sqrt{P} \quad 800\text{MHz to 2.5GHz}$  Where $P$ is the maximum output power rating of the transmitter in watts(W) according to the transmitter manufacturer and $d$ is the recommended separation distance in metres (m).  Field strengths from fixed RF transmitters, as determined by an electromagnetic site survey, should be less than the compliance level in each frequency range.  Interference may occur in the vicinity of equipment marked with the following symbol: 

Recommended separation distances between portable and mobile RF communications equipment and the ME EQUIPMENT and ME SYSTEM – for ME EQUIPMENT and ME SYSTEM that are not LIFE-SUPPORTING.

Recommended separation distances between portable and mobile RF communications equipment and the slit lamp microscope			
Rated maximum output power of transmitter W	Separation distance according to frequency of transmitter m		
	150kHz to 80 MHz	80MHz to 800MHz	800MHz to 2.5GHz
0.01	$d = [\frac{3.5}{V_1}] \sqrt{P}$	$d = [\frac{3.5}{E_1}] \sqrt{P}$	$d = [\frac{7}{E_1}] \sqrt{P}$
0.1	0.12	0.12	0.23
1	0.37	0.37	0.73
10	1.2	1.2	2.3
100	3.7	3.7	7.3
	12	12	23



### WEEE precautions:

Please dispose the waste electrical and electronic equipment in accordance with relevant regulations and laws.

## 1 Technical specifications

### 1.1 Instrument Mark and Technical Specification

The slit lamp microscope is powered by network power supply. The following marks are required permanently affixed to the instruments according to IEC 60601-1 Standard. The following table lists the tips for your reference.

Table two:

No.	Content	Instructions
1	Manufacturer/ supplier	Shanghai MediWorks Precision Instruments Co., Ltd.
2	Figure /icon/ mark	Detail in table one
3	Connect to main power	Detail in power specification
4	Power frequency, Hz	Detail in power specification
5	Input power frequency	Detail in power specification
6	Network output power	N/A

7	Classification	Detail in table one item 1
8	Working time	No indication, work continuously
9	Output	Detail in table one item 8
10	Physiological reaction	No indication. N/A
11	AP/AGP type device	No indication. N/A
12	High pressure terminal device	No indication. N/A
13	Cooling condition	No indication. N/A
14	Mechanical stability	No indication. Detail in <b>General Requirements for Safety</b> item 12.
15	Protective packing	Transportation marks required by <EN ISO 780-1997 packing-handling icon marks> are affixed to the outer packing carton, which includes up, fragile, afraid of the rain, stacking Limit, stacking weight limit and so on.

## 1.2 Indicator Light

The power switch is designed with indicator light. When the light is blue, it means the power is on and the instrument is working.

## 1.3 Product Technical Specifications

Please refer to " General Description ".

## 2 Installation of the instrument and working condition

Slit lamps are network powered medical instrument. Please check according to the checking list after opening the carton and install the instrument according to this user manual. Test and ensure the instrument operating well before putting to use.

### 2.1 Replacements of consumables

**Detail in Chapter 5 of this manual.**

## 3 Component list

### 3.1 Component list

**The following electronic components are used in this instrument.**

Table three:

No.	Component name

1	15V/4A DC power adaptor
2	Control circuit board
3	Brightness adjustment potentiometer
4	Power switch with indicator
5	Photo shooting button
6	USB port
7	3 pin input aviation connector
8	4 pin output aviation connector
9	LED bulb as light source
10	Diode (for fixation light)


### **3.2 Transport and Storage Environmental Conditions**

**No special requirements besides the content about transportation and storage of IEC 60601-1 standard.**

## Catalog

Preface	1
EMC precautions:	5
1 Graphical description of each part of the slit lamp microscope	12
2 Installation	15
2.1 Check list	15
2.2 Installation procedure	16
2.3 Checking procedure	17
3 Operation procedure	18
3.1 Diopter compensation and Pupillary distance adjustment	18
3.2 Patient's head position and use of fixation target	19
3.3 How to use moving base	20
3.4 Operation of illumination system	20
3.5 Operation notes	21
4 Cleaning	22
4.1 Cleaning method	22
4.2 Cleaning cycle	23
5 Protection and Maintenance	23
5.1 Protection	23
5.2 Maintenance	24
5.2.1 Slit width control knob tightness adjustment	24
5.2.2 Illumination System tilt adjustment	24
5.2.3 Rail cover removal instructions	24
6 Trouble shooting	26

## 1 Graphical description of each part of the slit lamp microscope

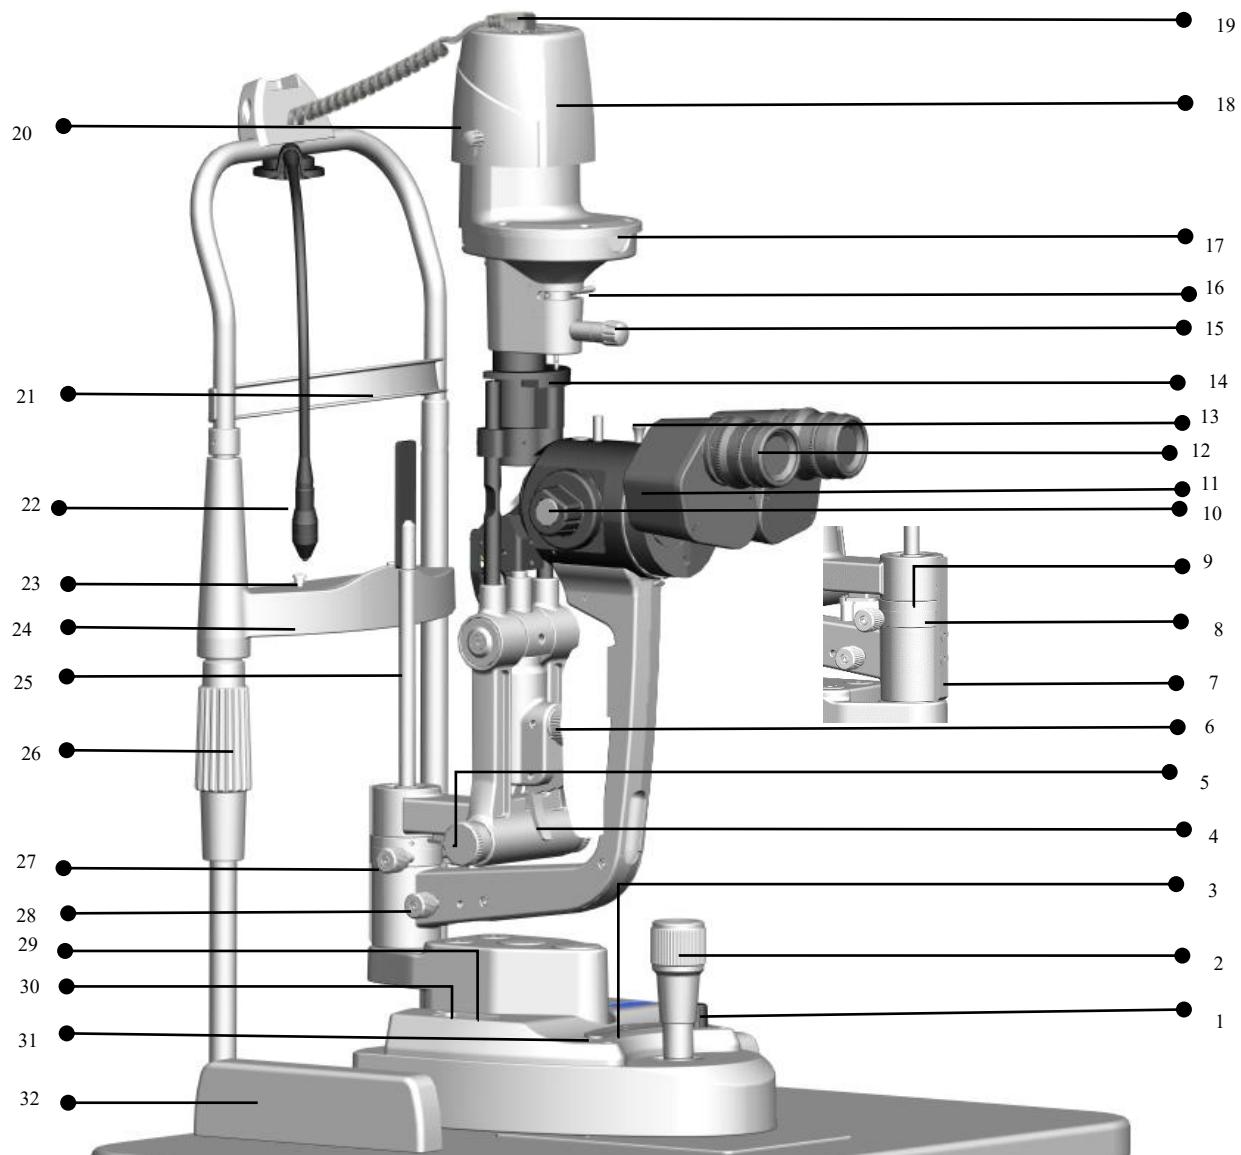

### 1 Brightness control knob

The brightness can be adjusted continuously. Avoid working continuously at high setting, as the service life of the bulb will be shortened.

### 2 Joystick

Incline joystick to move the instrument slightly on the horizontal surface and rotate it to

adjust the elevation of the microscope.

3 Shutter button  
Used for digital slit lamp photography.

4 Illumination Inclination Lever  
Four inclination stops are available from 5° up to 20°. The interval between each is 5°.

5 Slit Width control knob  
Turn the knob to adjust the slit width. The left knob is marked with a slit width indicator.

6 Illumination system reset knob  
By loosening the knob, the light can be offset from the center of the field of view of the microscope to provide indirect backlighting. When the knob is tightened, the light can be restored to the center of the microscope field of view.

7 Limit marker  
Limit viewing system and illumination system relative angle indicating and limiting illumination arm rotation angle.

8 The indication of relative angle between the microscope and illumination unit.

9 The mark of relative angle between the microscope and illumination unit.

10 Magnification changer  
Five different magnifications are provided.

11 Binocular tubes base  
Open it to both sides and adjust to the appropriate distance for easy observation.

12 12.5X Eyepieces

13 Yellow filter rod  
Pull up or press to switch the yellow filter.

14 Slit movement platform  
Moving up and down to makes the slit opening and closing, and the lower scale shows the angle between the slit and the vertical direction.

15 Slit height control knob  
Rotate this knob to adjust the spot and the slit height. Swing the knob horizontally to revolve the slit.

16 Filter selection lever and display mark  
The lever can choose different filters.

17 Aperture slit height and display window  
It will display the diameter of the slit and the aperture.

18 Lamp cap  
With the function of protecting and insulating, its normal working temperature is around 51°C.

19 Power plug  
Where the light source component power is connected.

20 The Fixation Knob of Lamp Cap

After fixing the knob, the lamp cap will not move.

21 Headrest belt

To fix the patient's head on an appropriate position.

22 Fixation target

Make the patient stare at it, it is convenient for checking.

23 Chin-rest paper fixing bolt

For fixing the pad paper.

24 Chin-rest

Supporting the patient's chin.

25 Focusing testing rod

26 Chin-rest elevation adjustment knob

Rotate the knob to adjust the elevation of the chin-rest.

27 Illumination arm locking knob

When the knob is tightened, the illumination system and the observation system are in a linked state and can rotate together. When the knob is loosened, the illumination system can be rotated separately.

28 Microscope arm locking knob

Lock the observation system so that it cannot rotate.

29 Power input

Used to supply power to the power module.

30 Power output

Used to power main lamp and fixation target.

31 Power switch

Press the power switch button once to turn it on, then press the button again shortly to enter standby mode, and press and hold for 3 seconds to turn off all power.

32 Rail cover

## 2 Installation

This section of the manual describes how to assemble the slit lamp microscope. All parts should be taken out with great care from the packing case before assembling.



Warning!

- Do not modify this equipment without the manufacturer's authorization.
- Installation and maintenance can only be carried out by trained specialists.
- Any third-party equipment connection must comply with EN 60601-1 standard.
- Only original parts may be used.
- Grounding reliability can only be achieved when the equipment is connected to a hospital-grade socket. (Not applicable to EU countries).
- The equipment should be set up in such a way that the plug is always accessible and the equipment can be easily disconnected from the mains.
- To avoid the risk of electric shock, this equipment must only be connected to a supply mains with protective earth.

### 2.1 Check list

No	Name	Qty.	Note
1	Microscope Part	1	Fig.2.1.1
2	Chin-rest	1	Fig.2.1.2
3	Binocular tubes Part	1	Fig.2.1.3
4	Rail Cover	2	Fig.2.1.4
5	Gas Shield	1	Fig.2.1.5
6	Power Cable	1	
7	Focusing Test Rod	1	Fig.2.1.6
8	Dust-proof Cover	1	
9	Chin-rest Paper	1	
10	5mm Wrench	1	
11	2mm Wrench	1	
12	User Manual	1	
13	Check list	1	

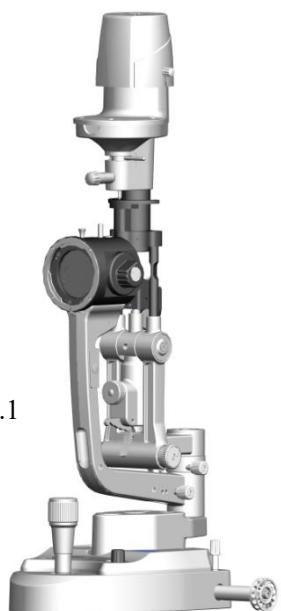


Fig.2.1.1




Fig. 2.1.4




Fig.2.1.5

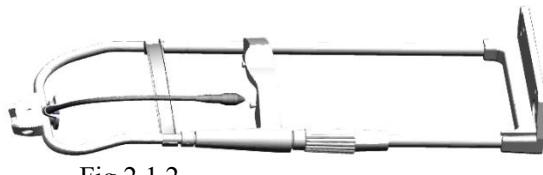


Fig.2.1.2




Fig.2.1.6




Fig.2.1.3

## 2.2 Installation procedure


1. Open the carton, take out the tools like screw driver and spanner.
2. Take out the slit lamp part (Fig.2.1.1), put it on the rails of the tabletop, check whether the wheels can move steadily on the rails, place the rail cover to the rail, remove four screws attached to the rail with the screw driver, and retighten the previously removed screws.

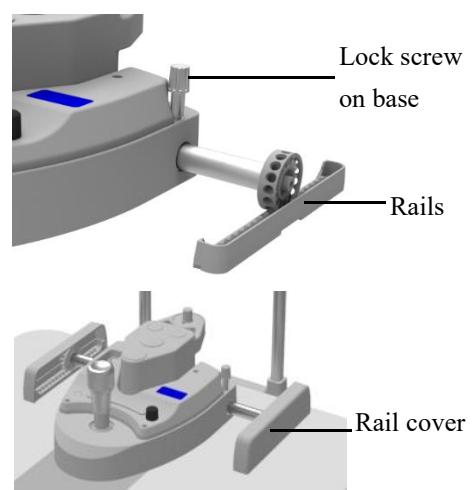

3. Take out the binocular tubes part, put the gas shield on the cylindrical surface of the binocular tubes, and then match the groove on the binocular tubes with the pin on the microscope body. Fasten the fixing screw on the body to the microscope. ATTENTION: Don't touch the objective lens and eyepiece when assembling.

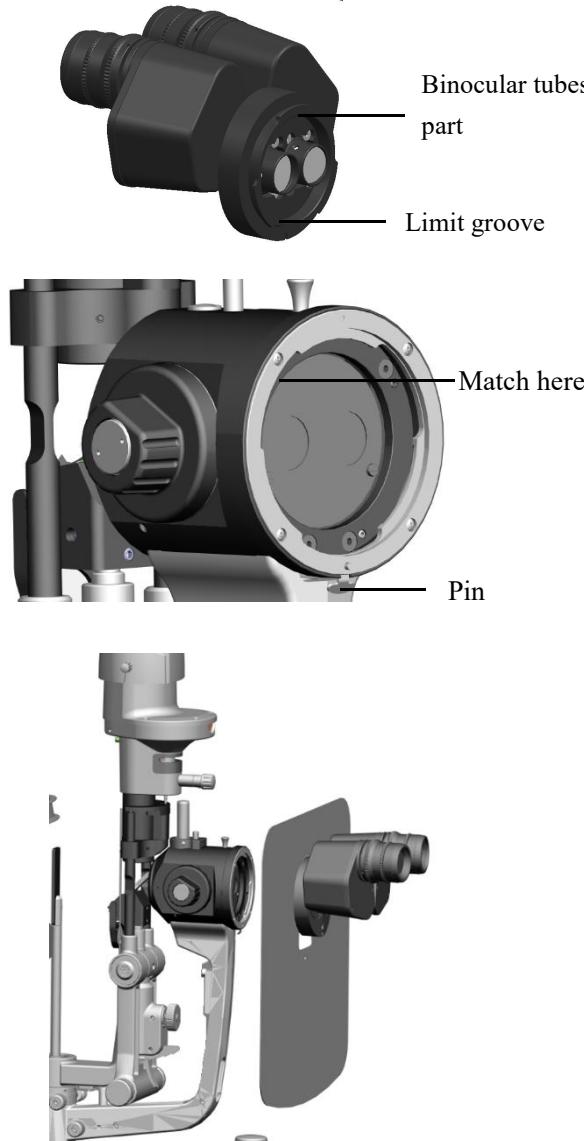


4. Refer to figure bellow, the 4-pin aviation plug of the chin-rest is connected to the “Output” on the base of the slit lamp microscope; the power adapter is connected to the “Input” on the base of the slit lamp microscope.

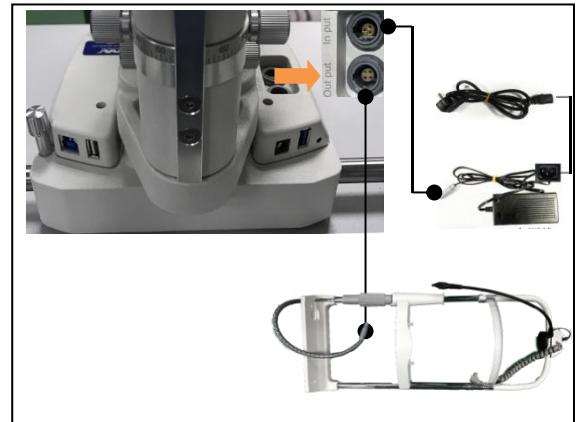


 Note: The limited slot on the air socket should be aligned corresponded slot when plugging and unplugging. Do not force the plug.

5. The power supply can work normally from 100V to 240V. The power switch can be turned on with one short-press, short-pressed again to hold, and long press for 3 seconds to turn off all power.



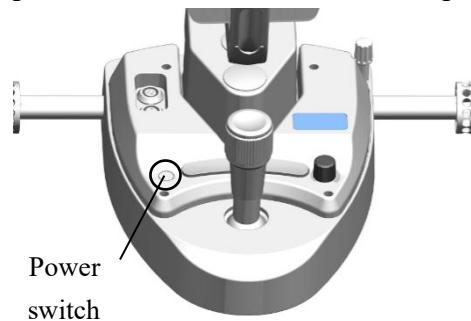


## 2.3 Checking procedure

1. The power cord of this instrument is a three-core power cord. Please select a suitable power socket to match it.
2. Insert the focusing test rod (Fig. 2.1.6) and turn the slit width control knob. The illumination spot should be observed on the black plane of the focusing test rod. The brightness change of the illumination should be observed when rotate the brightness adjustment knob (see Figure 3.1.2).

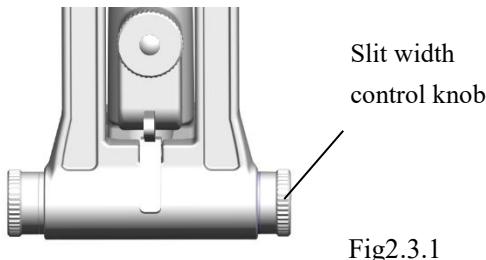

3. Check the fixation target (see Figure 3.2.1) to verify that it is properly illuminated.
4. Check whether the moving parts such as the slit and aperture width knob, the aperture adjustment knob, the filter selection lever (see Figure 2.3.2), the zoom knob (see Figure 2.3.3), and the joystick (see Figure 2.3.4) operate normally.

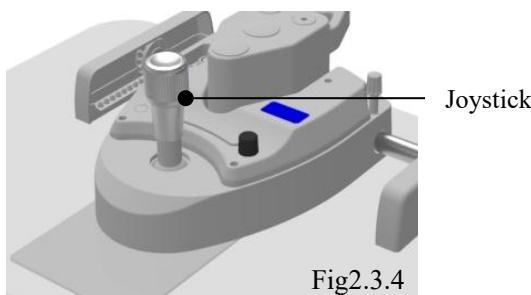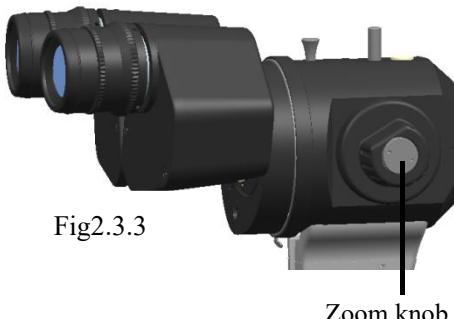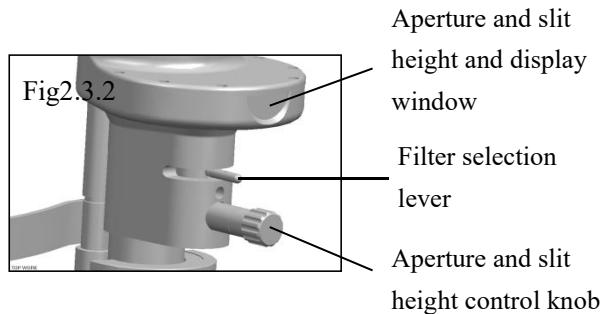

should be observed when rotate the brightness adjustment knob (see Figure 3.1.2)

6. After the checking is completed, press and hold the key for 3 seconds to turn off the power and cover the dust cover.


## 3 Operation procedure

### 3.1 Diopter compensation and Pupillary distance adjustment

#### 1. Use of focusing test rod

The focusing test rod is provided as a standard accessory to determine the correct adjustment of the microscope. Insert the focusing rod into the spindle hole with the black flat surface facing the objective lens of the microscope, ie the operator side (see Figure 3.1.1).

**Note: After adjustment, the focusing test rod should be removed.**

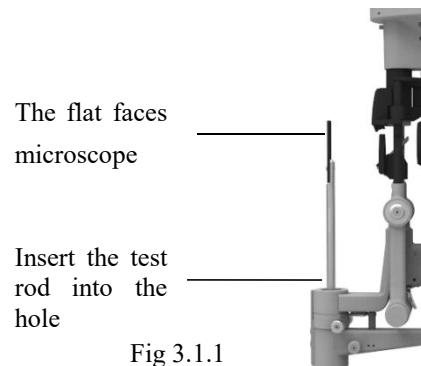

#### 2. Brightness adjustment

Turn on the main power switch and turn the brightness adjustment knob to the middle (see Figure 3.1.2). Adjust the slit width adjustment knob (see Figure 2.3.1) to make the slit width 2 to 3 mm.

5. The brightness change of the illumination


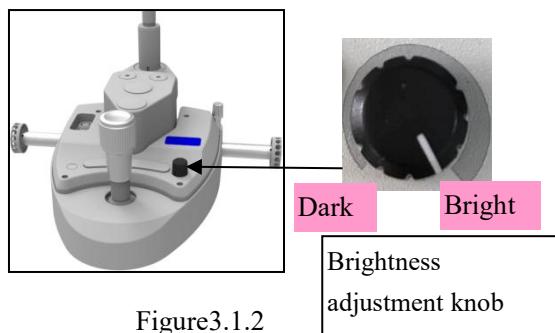


Figure 3.1.2

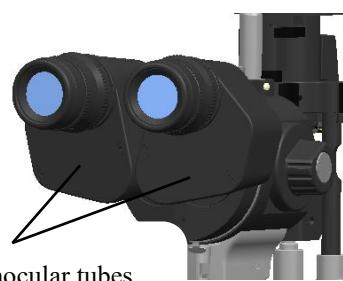

Tilt the binocular tubes base on both sides

### 3. Dipter adjustment

The focus of the microscope is adjusted in front of the emmetropia (ie, 0 diopter). If the operator has ametropia, gently rotate the eyepiece tube diopter adjustment ring to adjust the eyepiece diopter to the appropriate position (see Figure 3.1.3).

It is recommended to correct the diopter in the following order:

1. First, rotate the diopter adjustment ring counterclockwise to the end;
2. Then, turn the diopter adjustment ring clockwise until the clearest slit image appears on the focusing test bar
3. Adjust the other eyepiece in the same way;
4. Record the diopter value on each eyepiece for future reference.

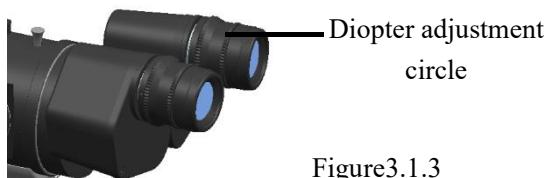


Figure 3.1.3

### 4. Pupillary distance adjustment

Use both hands to tilt the binocular tubes base on both sides, adjust the pupil distance to both eyes and observe the image on the focusing test rod through the eyepiece to obtain a stereoscopic image. When adjusting the pupil distance, ensure that the two eyepieces are at the same height.

## 3.2 Patient's head position and use of fixation target

1. Place the patient's chin on the chin-rest, with the forehead resting on the headrest belt and adjusting a handle below the chin-rest bracket until the patient's corner of the eye match with the level of the pole marked in line
2. The use of a fixation target is to fix the patient's vision, so that the patient's non-examined eye is gazing at the fixation target. When changing the fixation position, turn the fixation rod up and down or left and right to obtain the desired fixation target position (see Figure 3.2.1).


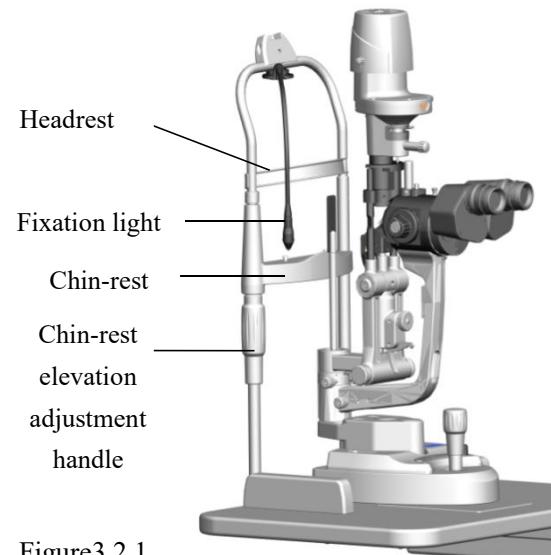



Figure 3.2.1

### 3.3 How to use moving base

1. Roughly adjustment in the horizontal direction. with the joystick in the upright position (see Figure 3.3.1), move the base back and forth to move the microscope in a horizontal direction to roughly align the target.
2. Adjustment in the vertical direction. Rotate the joystick to adjust the height of the microscope to align it with the target. Rotate clockwise to raise the microscope; counterclockwise to lower the microscope (see Figure 3.3.1).
3. Slightly adjustment in the horizontal direction. Tilt the joystick forward and backward to make the microscope move slightly in the horizontal direction. Observe through the eyepiece to accurately align the target to obtain a clear observation (see Figure 3.3.1).

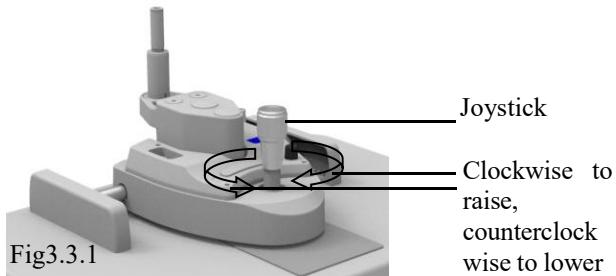

4. Lock the base. After the microscope is adjusted, tighten the base locking screw (see Figure 3.3.2) to fix the base so that it cannot move.

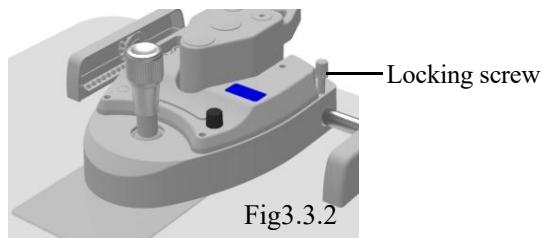

### 3.4 Operation of illumination system

1. Change the brightness of the slit image:

Rotate the slit width control knob (see Figure 2.3.1) to change the slit width from 0mm to 12mm (when the width is adjusted to 14mm, the slit becomes circular), the knob has a scale to indicate roughly the width value (see Figure 3.4.1).


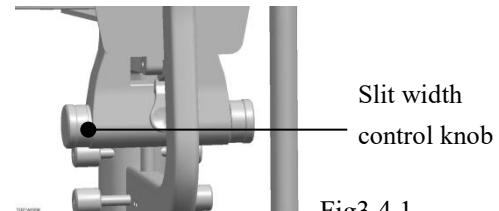


Fig3.4.1

2. Change the aperture diameter and slit height: Rotate the aperture selection knob to get 7 different sizes of circular spot and 1 continuous change aperture. The diameter of the circular spot is 14, 10, 5, 3, 2, 1, 0.2. Continuously changing the aperture can continuously change the length of the slit from 1 to 14 mm. The aperture data is displayed from the pupil reading window (see Figure 3.4.2).

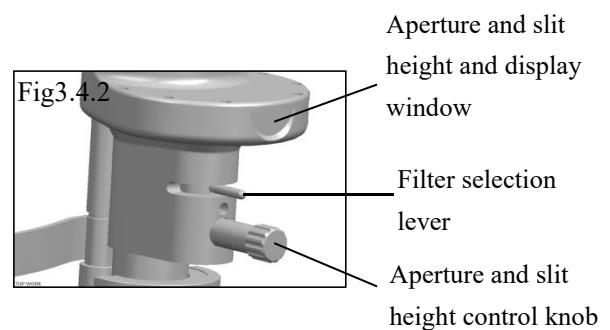

3. Rotating slit image: horizontally move aperture selection knob can rotate the slit image at any angle between vertical and horizontal. The angle of rotation can be displayed by the scale board. Each small grid is 5, and the larger grid is 10. (See Figure 3.4.3).

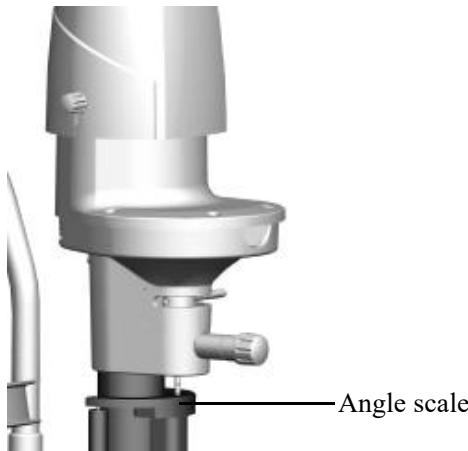


Figure 3.4.3

4. Offset illumination. Rotate the centering knob and rotate the slit width adjustment knob in the direction of the arrow to offset the illumination light from the center of the microscope field of view. This is mainly used for indirect inverse illumination methods to check the eyes. Rotate the centering knob and the slit light returns to the center of the field of view (see Figure 3.4.4).

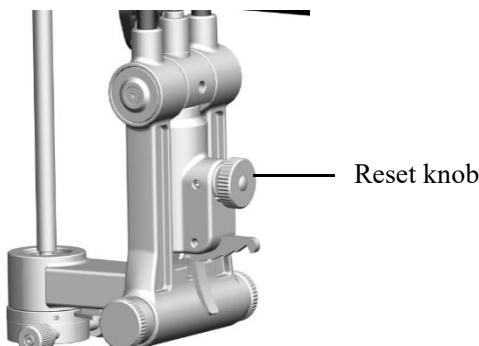


Figure 3.4.4

5. Tilt the illumination light. When using a contact lens and using a slit section view or fundus examination, oblique illumination is required. By pressing down on the tilting lever, the lighting components can be tilted from 5 to 20 (every 5th gear) (see Figure 3.4.5). **Since this method may touch the patient's head, be careful.**

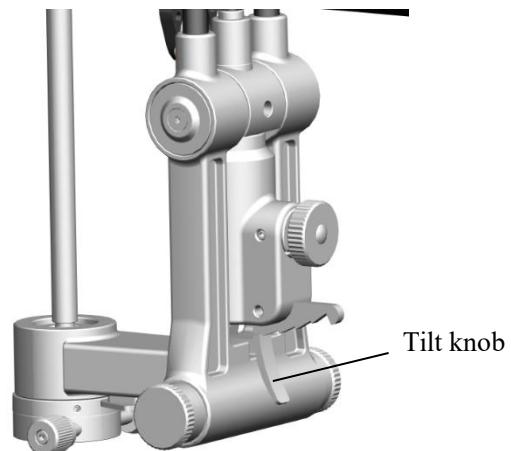


Figure 3.4.5

6. Select the color filter. Rotate the filter selector lever in the horizontal direction to switch four different color filters into the light path. Heat-absorbing filters are often used to make the patient feel more comfortable. Other filters should be placed in the position of the heat-absorbing filter after use. (See Figure 3.4.6).

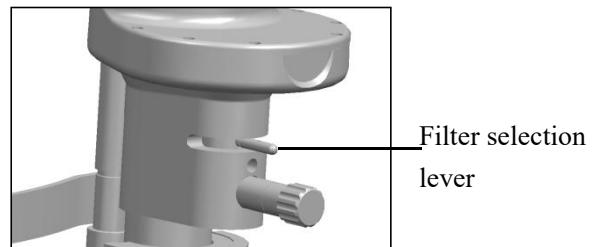


Figure 3.4.6

7. From left to right: white filter, heat absorbing filter, light reduction filter, red-free filter, cobalt blue filter. The white filter is only used when the factory is calibrated, and the operator does not have to use it.



### 3.5 Operation notes

1. During the operation, the operator should first understand the contents of the

instruction manual and master the structure and function of the slit lamp microscope. It is necessary for proper operation and diagnosis.

2. During the use of the operator, the different scales and different indication marks corresponding to the various knobs at different positions should be observed clearly, to prevent unnecessary misjudgments during observations.
3. The operator should adjust the pupil distance and the vision before observing the microscope during the operation. If the distance and vision are incorrect, there may be a feeling of dizziness.
4. The operator may have a feeling of dizziness if using microscope for a long time during the operation. Please adjust the observation time according to your personal situation.
5. When the patient is diagnosed with a slit lamp microscope, a beam of slit light is applied to the eye. If the slit light is too dark, it will affect the observation. If the slit light is too strong, and the observation last too long, it may affect the patient's vision. If the patient feels uncomfortable, please inform the operator or actively seek medical attention. Try to avoid illuminating the patient's eyes for a long time under strong light.

## 4 Cleaning

### 4.1 Cleaning method

1. Cleaning the lens and mirror: If dust adheres to the lens or mirror, gently wipe it off with soft cotton dampened with

absolute alcohol (see Figure 4.1.1).

**Attention: Don't wipe with hands or hard object or any corrosive detergent lest that the surface should be damaged.**

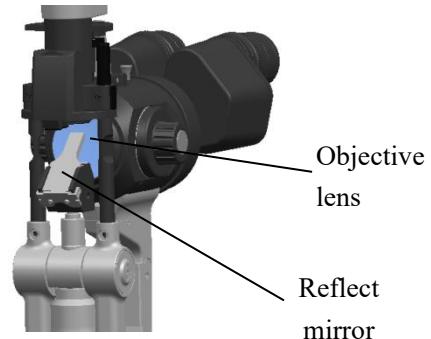


Fig. 4.1.1

2. Cleaning the pad, rails, and shaft: If the pad, rails, and shaft are not clean, the horizontal and vertical movements will not be smooth. Wipe clean with a clean soft cloth (see Figure 4.1.2).


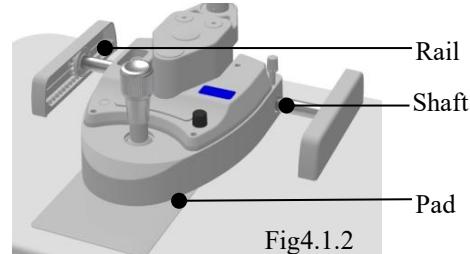


Fig4.1.2

3. Cleaning and disinfecting plastic parts: Clean plastic parts such as chin-rest, headrest belt, etc. Use a soft cloth dampened with a soluble detergent or water to clean the dirt, then wipe it with medical alcohol. **Note: Do not wipe with any abrasive cleaner to avoid damaging the surface.**
4. Replace the chin-rest paper: When the chin-rest paper is used up, pull out the two fixing bolts on the bracket and put on the new paper, then install the fixing bolt (see Figure 4.1.3).

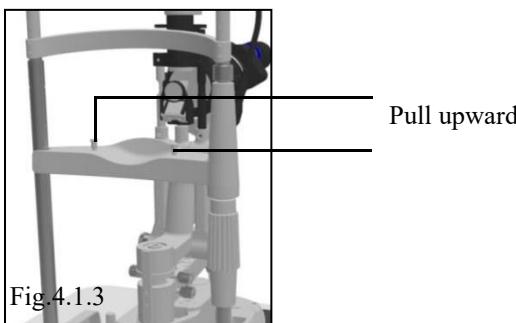

## 4.2 Cleaning cycle

The slit lamp microscope should be used in a relatively clean environment, and the main parts that need to be cleaned are as specified in the instruction manual 4.1. In order to ensure the normal use and observation of the slit lamp, the cleaning should be carried out regularly. The cleaning cycle is recommended as follows:

1. For the eyepiece area, lens and mirror parts:

**Cycle:** It is recommended to do it every 2 months.

Since the surface of the lens and the mirror is coated with an anti-reflection film and a reflective film, although the coating is sufficiently strong, frequent wiping tends to cause damage to the film, thereby affecting the optical effect of observation. This cycle is only a suggestion. If there is a lot of dust adhering to the lens that has affected the quality of the observation, it is recommended to clean it immediately according to the prescribed method.

2. For the rails, shaft and the pad:

**Cycle:** It is recommended to do it once every month.

The use of slit lamps in a relatively clean environment in a hospital does not cause the sliding pad, rails and shafts. They will not need to clean in a short period of time (within 1 year), nor does it affect

the horizontal and vertical movement of the moving base. However, we recommend that you clean the above parts with a clean soft cloth every 6 months for better positioning and positioning.

3. For chin-rest, plastic parts such as headrest straps:

**Cycle:** It is recommended to do it once a day.

These two parts are the parts that are in frequent contact with the inspected person. They should be cleaned and disinfected in time. The cleaning and disinfection cycle is only our recommendation. A new chin-rest paper should be replaced when inspecting each of the inspectors. The headrest strap area should also be cleaned. Both parts should be cleaned and disinfected daily before the first use.

4. For the whole device

**Cycle:** It is recommended to do it every 2 months.

5. Product Lifecycle

The slit lamp has a life cycle of 8 years.


## 5 Protection and Maintenance

Correct and regular protection and maintenance will help to extend the lifecycle of the slit lamp. The service period of the slit lamp is 2 months. Maintenance should be carried out every 2 months.

### 5.1 Protection

During the use of the slit lamp, dust and dirt are easily trapped in the spindle hole of the arm. To protect the instrument from damage, cover the spindle hole with a protective cover. When the focusing test bar needs to be installed, the protective cover can be removed

(see Figure 5.1.1).

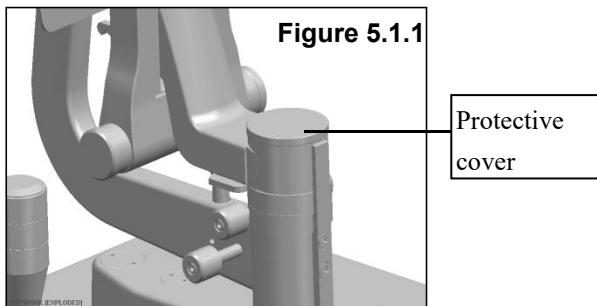

## 5.2 Maintenance

### 5.2.1 Slit width control knob tightness adjustment

**Slit width adjustment knob:** 1. If the slit width control knob is adjusted too loose, the slit width may be out of control. Use a hex driver to adjust the set screw on the right knob clockwise to achieve the proper tightness.


2. Adjust the tightness as follows:
  - a) Use a hex driver to tighten the set screw on the right knob



- b) If the width adjustment knob is too loose, the set screw will rotate clockwise (as shown in Figure 5.2.1). If the width adjustment knob is too tight, rotate it in the opposite direction. Attempt several times to reach the proper tightness.


### 5.2.2 Illumination System tilt adjustment

If the parts of illumination system are too loose, use a hex driver to tighten the screws on both sides (see 5.2.2).

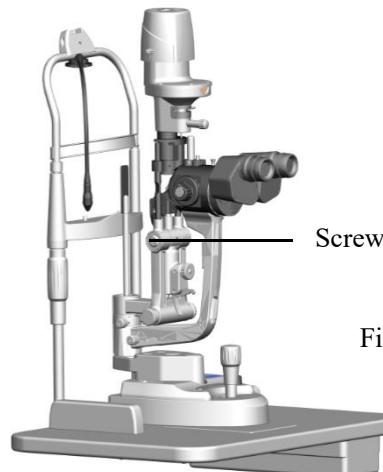


### 5.2.3 Rail cover removal instructions


1. Place your hand on the rail cover

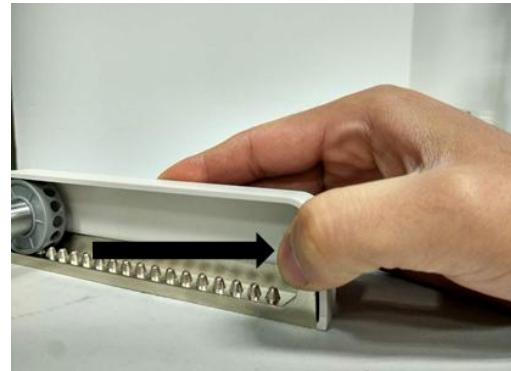

2. Pull the rail cover outwards to see an obvious gap.

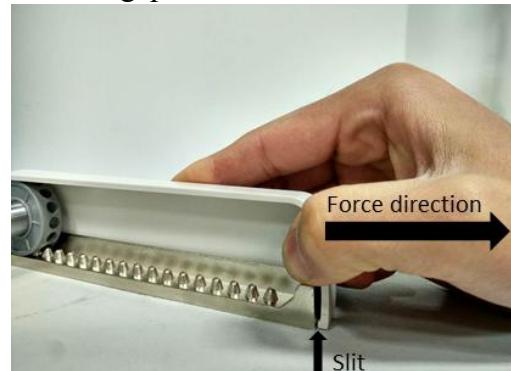


3. Move the rail cover in the direction of the arrow shown

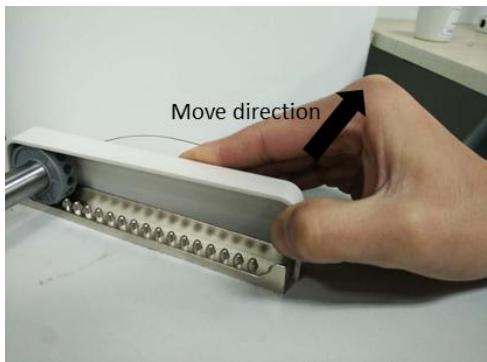


4. If the mid cover area is detached , the disassembly is successful.



6. The false example one

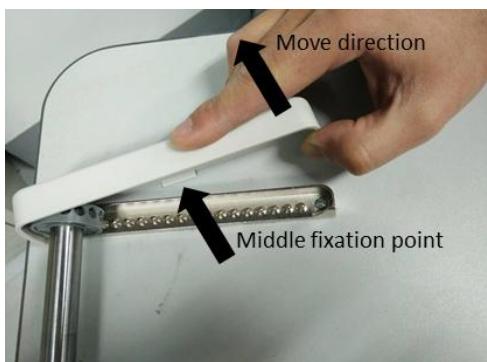

5. The false example one

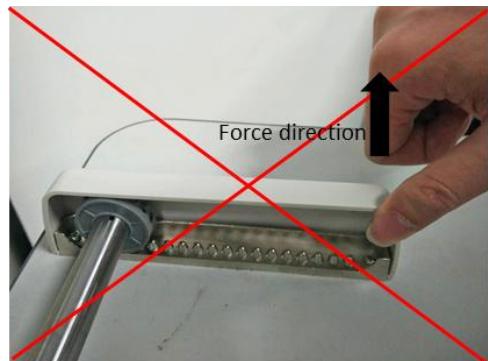

## 6. Trouble shooting

In case there is any trouble, please check according to the following table for reference. If it still cannot work, please contact the after-sales service department of an authorized distributor.

Error	Possible Cause	Solution
Illumination does not light	The power cord is not properly connected to the power outlet.	Connect the power cord correctly.
	The main power switch is not turned on.	Short press the switch key, the power indicator light is on.
	Loose plug on the power adapter	Tight plug on the power adapter
	The lamp cover is not aligned	Tighten the knob
	Burnt out the bulb	Switch the bulb
	Power adapter is damaged	Replace the power adapter
The slit is too dark	The brightness adjustment knob is in the Min	Adjustment brightness adjustment knob
	The reflect mirror coating is oxidized	Replace the reflect mirror
	Excessive dust on the mirror surface	Clean the surface with soft cotton
	The brightness adjustment knob position is not adjusted to the maximum.	Adjust the brightness adjustment knob.
The slit is automatically closed.	The filter rod is located in the first or middle position of the dimmer.	Correctly set the filter selector lever position.
	The slit width control button is too loose.	Adjust the tightness of the knob.
The fixation lamp does not work.	The fixation lamp plug is loose.	Tight fixed light plug.

**Subject to change in design or specifications without advance notice.**

Version: 6.0

20250425

---



CMC Medical Devices & Drugs SL  
C/ Horacio Lengo N18, Málaga, 29006, Spain



Tomey GmbH  
Wiesbadener Strasse 21, 90427 Nuernberg, Germany



Shanghai MediWorks Precision Instruments Co., Ltd.  
No.7, MingPu Phase II, No.3279 SanLu Road, MinHang District, 201100,  
Shanghai, China