



# KONFORMITÄTSERKLÄRUNG

## DECLARATION OF CONFORMITY

Doc#001/12-2020

Wir / We **TECO Medical Instruments Production and Trading GmbH**  
Name des Herstellers / Manufacturer's *name*  
**Dieselstrasse 1, 84088 Neufahrn, Germany**  
Anschrift / *Address*

erklären in alleiniger Verantwortung, dass die Produkte – IVD-Blutgerinnungsmessgeräte,  
*declare under our own responsibility, that the products – IVD Coagulation analyzers*

### Coatron X Eco, Pro, Top

Bezeichnung, Typ oder Modellname / *name, type or model*

Alle anwendbaren Anforderungen der folgenden Richtlinien entsprechen:

1. Richtlinie 98/79/EG über In-vitro Diagnostika  
klassifiziert gemäß Artikel 9 – "alle anderen Produkte"  
Anhang II – Liste A
2. Richtlinie 2014/30/EU über Elektromagnetische Verträglichkeit
3. Richtlinie 2011/65/EU RoHS II

Weitere angewandte Normen:

- |                           |                          |
|---------------------------|--------------------------|
| 4. Sicherheit:            | EN 61010-2-101:2015      |
| 5. Risikomanagement:      | DIN EN ISO 14971:2013-04 |
| 6. Informationen:         | EN ISO 18113-3:2011      |
| 7. Medizingeräte-Software |                          |
| - Lebenszyklus-Prozesse:  | DIN EN 62304:2016        |

*Standards and regulations applied:*

1. *Directive 98/79/EC on In-vitro diagnostic medical devices classified according to article 9 as: "all other products" Annex II – list A*
2. *Directive 2014/30/EU on electromagnetic Compatibility*
3. *Directive 2011/65/EU RoHS II*

*Further related standards:*

- |                                   |                                 |
|-----------------------------------|---------------------------------|
| 4. <i>Safety:</i>                 | <i>EN 61010-2-101:2015</i>      |
| 5. <i>Risikomanagement:</i>       | <i>DIN EN ISO 14971:2013-04</i> |
| 6. <i>Information:</i>            | <i>EN ISO 18113-3:2011</i>      |
| 7. <i>Medical device software</i> |                                 |
| - <i>life-cycle processes:</i>    | <i>DIN EN 62304:2016</i>        |

Das QM-System des Herstellers ist zertifiziert nach:

**EN ISO 13485:2016**

Konformitätsbewertungsverfahren:

Gemäß Anhang III der Richtlinie 98/79/EG

*The QM-system of the manufacturer is certified for:*

**EN ISO 13485:2016**

*Conformity assessment procedure:*

*According to Annex III of Directive 98/79/EC*

Ort und Datum der Unterzeichnung:  
Place and date of issue:

Neufahrn, 08.12.2020  
Neufahrn, December 8, 2020

Matthias Dieckmann  
General Manager





# KONFORMITÄTSERKLÄRUNG DECLARATION OF CONFORMITY

Doc#200/08-2022

Hersteller / Manufacturer: **TECO Medical Instruments  
Production + Trading GmbH**  
 Adresse / Address: **Dieselstrasse 1, 84088 Neufahrn, Germany**  
 Marktakteur / Actor ID SRN: **DE-MF-000022642 <https://ec.europa.eu>**

Wir erklären hier für die im Anhang A ( Seite 2 – 23 IVD Produkte) spezifizierten Produkte dass sie gemäß der Richtlinie für In-vitro-Diagnostika Medizinprodukte 98/79/EC klassifiziert sind als allgemeine IVD.

Diese Konformitätserklärung wird unter der alleinigen Verantwortung des Herstellers i.V.m. Artikel 110 Abs.3 und Abs.4 der Verordnung (EU) 2017/746 und des § 8 Abs.1 des Medizinprodukte-Durchführungsgesetzes, in der jeweils geltenden Fassung, ausgestellt.

Im Falle eigenmächtiger Veränderungen am Produkt oder der nicht bestimmungsgemäßen Verwendung verliert diese Erklärung ihre Gültigkeit.

We declare herewith for the products specified in Annex A ( page 2 - 23 IVD products) that they are classified as general IVD according to the In Vitro Diagnostic Medical Devices Directive 98/79/EC.

This declaration of conformity is issued under the sole responsibility of the manufacturer in according to article 110 para.3 and para.4 of Regulation (EU) 217/746 and section 8 para.1 of the Medical Device Law Implementing Act.

In case of unauthorised modifications to the products or un-intended use, this declaration loses its validity.

Sie entsprechen den anwendbaren Anforderungen der Richtlinie:	They meet applicable requirements of:
Richtlinie 98/79/EG über In-vitro-Diagnostika klassifiziert gemäß Artikel 9 als "alle anderen Produkte"	Directive 98/79/EC on in-vitro-diagnostic medical devices classified according to article 9 as „all other products“
Die Qualitätssicherung entspricht den Anforderungen der Richtlinie 98/79/EG über In-vitro-Diagnostika für diese Art von Produkten.	The Quality Assurance is in accordance with the requirements of Directive 98/79/EC on in-vitro-diagnostic medical devices for those kind of products.
Der implementierte QM-Prozess entspricht der EN ISO 13485:2021	The implemented QM Process complies with EN ISO 13485:2021
Die vorstehende Konformitätserklärung ist gültig für alle Chargen dieser Produkte, die nach dem Datum der Unterzeichnung in Verkehr gebracht wurden.	The above mentioned declaration of conformity is valid for all lots of this product, which are distributed after the date of signature.
Das Konformitätsbewertungsverfahren entspricht Anhang III der Richtlinie 98/79/EG über In-vitro-Diagnostika für diese Art von Produkten.	The conformity assessment procedure complies with Annex III of Directive 98/79/EC on in-vitro-diagnostic medical devices for those kind of products.

Ort und Datum der Unterzeichnung: **Neufahrn, 2022-08-31**  
Place and date of issue:



Christian Hötzl  
Verantwortliche Person / PRRC

Doc#200/08-2022

## KONFORMITÄTSERKLÄRUNG – DECLARATION OF CONFORMITY

Directive 98/79/EC Annex A

Übrige Produkte – Reagenzien für In-vitro-Diagnostika

Other products – Reagents for in vitro diagnostic – general IVD

Pos.	Article No	Tradename	Unit	Generic Device Term	EMDN / GMDN Code EUDAMED DI
1	A0230-040	TEClot PT-S (Quick)	10x4ml PT-S	Prothrombin time ( quick test )	W0103020101 / 30539 B-PTS-A0230-040X7
2	A0230-100	TEClot PT-S (Quick)	10x10ml PT-S	Prothrombin time ( quick test )	W0103020101 / 30539 B-PTS-A0230-100WY
3	A0260-050	TEClot PT-B (Owren)	5x10ml PT-B	Prothrombin time ( quick test )	W0103020199 / 55986 B-PTB-A0260-050G2
4	A0320-050	TEClot APTT-S	10x5ml APTT-S	Activated partial thromboplastin time	W0103020102 / 55982 B-APTT-A0320-050AM
5	A0401-020	TEClot TT	10x2ml TT	Thrombin time / reptilase / batroxbin time	W0103020103 / 55988 B-TT-A0401-0207P
6	A0511-020	TEClot FIB	10x2ml FIB	Fibrinogen assays (factor i)	W0103020201 / 55997 B-FIB-A0511-020N2
7	A0511-050	TEClot FIB	10x5ml FIB	Fibrinogen assays (factor i)	W0103020201 / 55997 B-FIB-A0511-050NB
8	C1010-020	TEChrom AT	6x6ml reagent FXa 3x3 ml substrate	Antithrombin	W0103020602 / 56156 B-AT-C1010-020HL
9	D2010-012	Red D-Dimer	3x4ml latex 3x7ml reaction buffer	D-Dimer	W0103020503 / 47349 B-DD-D2010-0126W
10	D2020-005	Blue D-Dimer LC	1x5ml latex LC 1x7ml reaction buffer	D-Dimer	W0103020503 / 47349 B-DD-D2020-0057E
11	P8001-010	TECal N	10x1ml	Calibration plasma for haemostasis	W0103020701 / 45786 B-CAL-P8001-005X8
12	P8200-005	TECal DD	5x1ml	Calibration plasma for haemostasis	W0103020701 / 47348 B-CAL-P8200-005XX
13	P6001-010	TEControl N	10x1ml	Control plasma for haemostasis	W0103020702 / 30590 B-CTRL-P6001-010H7
14	P6101-010	TEControl A	10x1ml	Control plasma for haemostasis	W0103020702 / 30590 B-CTRL-P6101-010HQ
15	P6201-010	TEControl A Plus	10x1ml	Control plasma for haemostasis	W0103020702 / 30590 B-CTRL-P6201-010J9
16	P5001-010	TEClot Factor II	10x1ml	Coagulation factor ii ( prothrombin )	W0103020202 / 30542 B-FAC-II-P5001-010ML
17	P5101-010	TEClot Factor V	10x1ml	Coagulation factor v	W0103020204 / 30544 B-FAC-V-P5101-010AN
18	P5201-010	TEClot Factor VII	10x1ml	Coagulation factor vii	W0103020205 / 30545 B-FAC-VII-P5201-0107B
19	P5301-010	TEClot Factor VIII	10x1ml	Coagulation factor viii	W0103020207 / 30547 B-FAC-VIII-P5301-01097
20	P5401-010	TEClot Factor IX	10x1ml	Coagulation factor ix	W0103020208 / 30548 B-FAC-IX-P5401-0106C
21	P5501-010	TEClot Factor X	10x1ml	Coagulation factor x	W0103020209 / 30549 B-FAC-X-P5501-010EQ
22	P5601-010	TEClot Factor XI	10x1ml	Coagulation factor xi	W0103020210 / 30551 B-FAC-XI-P5601-010A8
23	P5701-010	TEClot Factor XII	10x1ml	Coagulation factor xii	W0103020211 / 30552 B-FAC-XII-P5701-010CJ

(Recital 23 of Directive 98/79/EC on In Vitro Diagnostics Medical Devices) - Annex A - general IVD



# KONFORMITÄTSERKLÄRUNG

## DECLARATION OF CONFORMITY

Doc#100/07-2021

Wir / We

### **TECO Medical Instruments Production and Trading GmbH**

Name des Herstellers / Manufacturer's name

**Dieselstrasse 1, 84088 Neufahrn, Germany**

Anschrift / Address

erklären in alleiniger Verantwortung, dass die unten gelisteten IVD Zubehör Produkte:  
*declare under our own responsibility, that the IVD accessories products, listed below:*

Doppelküvette / <i>Double cuvette</i>	Ref. 19 000 02
Einzelküvette / <i>Single cuvette</i>	Ref. 20 000 02, 24 100 00
4-fach Küvette / <i>Cuvette 4 pos/ea</i>	Ref. 80 521 10
6-fach Küvette / <i>Cuvette 6 pos/ea</i>	Ref. 80 560 00
6-fach Küvette (micro) / <i>Cuvette 6 pos/ea (micro)</i>	Ref. 80 570 00

allen anwendbaren Anforderungen folgender Richtlinien entsprechen: *meet all applicable requirements of:*

1. Richtlinie 98/79/EG über In-vitro Diagnostika und ihrem Zubehör, klassifiziert gemäß Artikel 9 als: "alle anderen Produkte"- im Sinne von Zubehör zu In vitro Diagnostika gemäß Artikel 1.

*1. Directive 98/79/EC on In-vitro diagnostic medical devices and their accessories, classified according to article 9 as: "all other products" – and in term of accessories for in vitro diagnostics according to article 1.*

2. Richtlinie 2011/65/EU (RoHS III)

*2. Directive 2011/65/EU (RoHS III)*

Das QM-System des Herstellers ist zertifiziert nach:

*The QM-system of the manufacturer is certified for:*

**EN ISO 13485:2016**

***EN ISO 13485:2016***

Konformitätsbewertungsverfahren gemäß:

*Conformity assessment procedure according to:*

Gemäß Anhang III der Richtlinie 98/79/EG

*According to Annex III of Directive 98/79/EC*

Ort und Datum der Unterzeichnung:  
Place and date of issue:

Neufahrn, 27.07.2021  
Neufahrn, July 27, 2021

Matthias Dieckmann  
General Manager



# TECO

MEDICAL INSTRUMENTS  
PRODUCTION+TRADING GMBH

Dieselstraße 1  
D-84088 Neufahrn N.B.  
fon: +49-8773/707 80-0  
fax: +49-8773/707 80-29

Neufahrn, 26/04/2018

## TO WHOM IT MAY CONCERN

We confirm that the instruments Coatron X Eco, Coatron X Pro and Coatron X Top have a closed cuvette system. Cuvettes have to be purchased with voucher identification code from TECO GmbH.



Christian Hoetzl  
General Manager  
TECO Germany



Quality Management  
We are certified  
Voluntary participation in regular  
monitoring according to ISO 9001:2008



MEDICAL INSTRUMENTS  
PRODUCTION+TRADING GMBH  
Dieselstraße 1  
D-84088 Neufahrn N.B.  
fon: +49-8773/707 80-0  
fax: +49-8773/707 80-29

# CERTIFICATE

for: **Mr. Vitalie Goreacii**

---

Company: **Sanmedico SRL**  
Str. Petricani 88/1, oficiul 10  
Chisinau - Rep. Moldava MD-2059  
MOLDOVA

have participated with success at the intensive training session:

**Application and technical training for following instruments:**

- **Coatron X series**
  - **Installation**
  - **Application**
  - **General use, also in combination with TECAM Software**
  - **Technical and After Sales Service**

Supervisors: **Mr. Chr. Hoetzi and Mrs. Wendy Guo**

---

Place of Training: **TECO – Germany**

Date: **November 18<sup>th</sup>, 2019**



Christian Hoetzi  
General Manager

---

# Certificate of Approval

This is to certify that the Management System of:

## **TECO Medical Instruments, Production + Trading GmbH**

Dieselstr. 1, 84088 Neufahrn, Germany

has been approved by LRQA to the following standards:

**ISO 13485:2016**

Approval number(s): ISO 13485 – 00038268

**The scope of this approval is applicable to:**

Design, development, manufacturing, storage and sales of coagulation instruments and in-vitro-diagnostic reagents used in the hemostaseology and coagulation.



**Paul Graaf**

---

Area Operations Manager, Europe

Issued by: LRQA Limited



0001

## TO WHOM IT MAY CONCERN

To any governmental departments,  
registration and/or trade offices in MOLDOVA

### Distribution Authorisation Letter

This letter confirms that **Sanmedico**  
**Mun. Chisinau**  
**Str. Petricani 88/1 of. 10**  
**Republica MOLDOVA**

is the **legal, exclusive and sole** representative of **TECO Medical Instruments Production + Trading GmbH, Dieselstr. 1, 84088 Neufahrn NB, Germany**, for the territory of **MOLDOVA** only for all TECO products listed below. **Sanmedico** may participate in public and private tenders, providing sales to all TECO customers in the territory. We as manufacturer certify that our warranty is duly passed to the purchaser through **Sanmedico** for the price, delivery schedules and the specifications of the published literature, catalogues and fully covering the commodities offered.

**Sanmedico** will provide the following information to TECO GmbH when so required in relation to its market surveillance activities:

Reporting of incidents to TECO must take place within 3 working days  
Serial number of the device, exact location of the device and the user.

Validity: January 1<sup>st</sup>, 2023 to December 31<sup>st</sup>, 2024


Termination: Confirmation ends automatically on Dec. 31<sup>st</sup> of 2024  
and must be then renewed.

#### Products:

- Coatron M1 Semi-automated 1-channel Coagulometer (out of production)
  - Coatron M2 Semi-automated 2-channel Coagulometer (out of production)
  - Coatron X Eco Semi-automated 1-channel Coagulometer
  - Coatron X Pro Semi-automated 2-channel Coagulometer
  - Coatron X Top Semi-automated 4-channel Coagulometer
  - Coatron A4 Fully automated Coagulometer, 4 optic channels
  - Coatron A6 Fully automated Coagulometer, 6 optic channels
  - Coatron A6 plus Fully automated Coagulometer, 6 optic channels
  - Hemostasis Reagents Complete product line
- all instruments with complete accessory, consumables and spare parts

This document is signed in Neufahrn, Germany, on January 18<sup>th</sup>, 2023

TECO Medical Instruments Production+Trading GmbH

  
Christian Hoetzl







IVD

REF

A0230-010, A0230-040, A0230-100,

**Intended Use**

This product is used for the determination of prothrombin time (PT) in plasma according to Quick<sup>1,2</sup>. The test is sensitive to the extrinsic pathway coagulation factors II, V, VII, X and fibrinogen and therefore used for oral anticoagulant therapy with Vitamin-K inhibitors like Warfarin or Marcumar and also for the quantitative determination of extrinsic coagulation factors. The PT measures the extrinsic clotting time (factor VII activation) of test plasma after the addition PT reagent.

**Contents & Determinations**

Product	TECLOT PT-S	TECLOT PT-S	TECLOT PT-S
Cat.No.	A0230-010	A0230-040	A0230-100
PT-S Reagent*	5x2 mL	10x4 mL	10x10 mL

**Determinations**

Coatron M**	200 Det.	800 Det.	2000 Det.
Coatron A4	100 Det.	400 Det.	1000 Det.
Coatron A6	200 Det.	800 Det.	2000 Det.

\*contains an extract of Rabbit brain with buffer, stabilizers and Calcium chloride.

\*\*Micro method (75µL in total)

**Preparation**

Reconstitute with high purity water with the volume stated on the vial label.

A0230-010	A0230-040	A0230-100
2 mL	4 mL	10 mL

Let stand at room temperature with occasional swirling for at least 15 min. Then place reagent into instrument and let incubate for further 15 min. The reagent sediments and must be swirled before each testing. On Coatron instruments, you can use a mixing bar for this.

**Storage & Stability**

Unopened reagents are stable until the expiration date shown on the label stored at 2°-8°C. Opened reagent:

	2-8 °C	20-25 °C	37°C
PT Reagent	5 days	36 hours	8 hours

**Precautions**

Avoid contact with skin and eyes. Wear suitable protective clothing. Dispose components in compliance with local regulations for infectious material. All components are checked for HIV, HBV, HCV. However products from human blood should be considered as potentially infectious.

**Specimen collection and storage<sup>4</sup>**

- Obtain venous blood by clean vein puncture.
- Immediately mix 9 parts blood with 1 part 3.2% sodium citrate (0.105M) and mix well
- Centrifuge the specimen at 1500g for 10 min. (platelet < 10000/µL)
- Separate plasma after centrifugation and store in plastic or siliconised glass tube.
- Use plasma within 4 hours, otherwise store frozen and thaw just prior to use.

Stability of plasma: 4h at 18-26°C 8h at 2-8° 30d at -20°C 6m at -70°C

**Procedure****A. Automated Method: Coatron A**

Prothrombin Time		A4		A6				A4		A6	
PAT	Patient	50µl	CP1	25µl	CP1	Incubation	0s	SENS	2		
BUF	IBS Buffer	0µl	P39	0µl	P79	Maxtime	120s	POINTS	4		
CLR	-	0µl	-	0µl	-	Unit	251	MIX	No		
DP	-	0µl	P00	0µl	P00	Method	Coag	Clean	0	0	
R0	-	0µl	P00	0µl	P00	Math	log XY	Multi	1	3	
R1	-	0µl	P00	0µl	P00	CT-Mech	No	S-Corr	0%		
R2	PT Reagent	100µl	P25	50µl	P46	Deadtime	7s	T-Corr	30% - 4s		

**B. Manual Method: Coatron M system**

- Incubate PT reagent at 37°C for at least 10 minutes
- Pipette 25 µl of sample into a test cuvette. Incubate at 37°C for 1-2 minutes.
- Add 50 µl of PT reagent (37°C) and simultaneously start test.
- Record the clotting time in seconds.

For other instrument, please refer to your instrument manual for more detailed instrument specific instructions.

**Symbol keys**

	Expiry date		In Vitro Diagnostica		Biological hazard		Catalogue Number		Reconstitute with dest. water		Consult accompanying documents
	Store at 2-8°C		EU conformity		Manufacturer		Lot. Number		Ready to use		Authorized Representative

**Expected Results**

Typical seconds: 11 – 18 sec  
Normal range: 70 - 130% 0.85 – 1.15 INR

However results are influenced by instruments, technique, calibration etc. Each laboratory is recommended to establish its own range on the specific instrument used.

**Standardisation and Calibration**

The PT result is expressed as seconds or activity (% Quick) or INR (International Normalised Ratio).

**INR results:**

were calculated from normal time and ISI value (international sensitivity index). First is obtained by running fresh plasma from a pool of healthy individuals. The ISI value is stated in the LOT specific certificate of analysis.

$$INR = \left( \frac{Patient\ PT}{Normal\ PT} \right)^{ISI}$$

**Activity % (Quick) result:**

were calculated from a calibration curve, which is prepared from reference plasma (e.g. TECAL N) and dilutions in saline solution like 0.9% NaCl<sub>2</sub> or TECLOT IBS buffer. At least three or more calibration points are recommended. The calibration curve must be confirmed with control plasma in normal and abnormal range.

% of normal	100%*	50%	25%	12.5%**
diluted in saline	not dil.	1+1	1+3	1+7

\*The median of at least 21 healthy individuals is defined as 100%.<sup>5</sup>

\*\*12.5% dilution may cause "+++" results in some cases, because the level of fibrinogen is too high diluted for optical detection.

**Quality Control**

TEControl or other commercial control plasma should be used for reliable quality control of performance at a frequency in accordance with good laboratory practice (GLP). TEControl can be frozen one time after reconstitution. 120-150 µl stored in closed polypropylen tubes at -20°C is stable for 30 days

**Limitations**

Great care must be taken to minimize variations which may occur by seemingly insignificant factors.

**A. Specimen Collection. AVOID:**

- Use only plastic tubes or siliconised glass.
- Delayed mixing of blood with anticoagulant.
- Contamination with tissue thromboplastin.
- Improper ratio of anticoagulant with blood.
- Hemolyzed, icteric or lipemic samples may interfere optical systems

**B. Laboratory Techniques**

- Perform tests at 37°C.
- Use only high purity water.
- Optimum pH is 7.0-7.5.
- ISI value is not constant within the first 30 min after reconstitution.
- Reagent sediments and must be swirled before each testing.

**Performance Characteristics****Typical performance on instrument Coatron M4**

**Precision:** CV% (within run) CV% (inter-runs)  
Normal control < 3.0 < 5.0  
Abnormal control < 3.0 < 5.0

**Warranty**

This product is warranted to perform in accordance with its labelling and literature. TECO disclaims any implied warranty of merchantability or fitness for any other purpose, and in no event will TECO be liable for any consequential damages arising out of aforesaid express warranty.

**References**

- Quick, A.J., The Hemorrhagic Diseases and the Physiology of Hemostasis. Charles C. Thomas: Springfield, IL. 1942.
- Quick, A.J., Hemorrhagic Diseases. Lea and Febiger: Philadelphia. 1957.
- Miale, J.B., Laboratory Medicine-Hematology, 4th Edition. C.V. Mosby: St. Louis. 1972.
- National Committee for Clinical Laboratory Standards: Guidelines for the Standardized Collection, Transport and Preparation of Blood Specimens for Coagulation Testing and Performance of Coagulation Assays.
- Besselaar A M H P van den, Lewis SM, Mannucci P n Poller L. 1993. Status of present and candidate International Reference Preparations (IRP) of thromboplastin for prothrombin time. Thromb Hemostas 69; 85
- Besselaar A M H P van den. 1991. The significance of the International Normalized Ratio (INR) for oral anticoagulant therapy. H17CC 3; 146153.





IVD

REF

P6001-010

**Intended Use**

Use as a normal control for following coagulation tests:

**PT, APTT, Thrombin time, Fibrinogen,  
Anti-thrombin and D-Dimer**

**Contents**

10 x 1mL freeze dried citrate-anticoagulated human plasma

**Preparation**

Reconstitute individual vials with **1,0 ml** distilled water. Allow to stand at room temperature, with occasional swirling, for 15 min before use. Be certain all particulate matter is well dissolved.

PT whole blood (TEClot PT-B): Reconstitute individual vials with **1,7 ml** distilled water.

**Storage & Stability**

Unopened vials are stable until the expiration date shown on the label stored at 2°-8°C.

Dissolved plasma change analytic levels below 10% if stored as following:

-20 °C	2-8 °C	20-25 °C
1 month	8 hours	4 hours

Dissolved plasma can be refrozen only one time in aliquots (120-150µL). Stored at -20°C in closed polypropylene tubes, the aliquots must be used within 30 days.

**Precautions**

This product contains substance from human origin!  
Avoid contact with skin and eyes. Wear suitable protective clothing. Dispose components in compliance with local regulations for infectious material. All components are checked for HIV, HBV and HCV. However products from human blood should be considered as potentially infectious.

**Expected Results**

Refer to "Certificate of Analysis".

**Warranty**

This product is warranted to perform in accordance with its labelling and literature. TECO disclaims any implied warranty of merchantability or fitness for any other purpose, and in no event will TECO be liable for any consequential damages arising out of aforesaid express warranty.

Symbols key:

Expiry date	In Vitro Diagnostica	Biological hazard	Catalogue Number	Consult accompanying documents
Store at 2-8°C	EU conformity	Manufacturer	Lot. Number	Authorized Representative





### Verwendungszweck

Als normale Kontrolle für folgende Gerinnungstests verwenden:

**PT, APTT, Thrombinzeit, Fibrinogen,  
Antiithrombin und D-Dimer**

### Inhalt

10 x 1mL gefriergetrocknetes mit Zitrat versetztes gerinnungshemmendes Humanplasma

### Vorbereitung

Die einzelnen Fläschchen mit 1,0ml destilliertem Wasser anlösen. Fläschchen bei Raumtemperatur bis zur Anwendung unter gelegentlichen Verwirbeln 15 Minuten lang stehen lassen. Stellen Sie sicher, dass alle Partikel gut aufgelöst sind.

Vollblut PT (TEClot PT-B): einzelne Fläschchen mit 1,7ml destilliertem Wasser anlösen.

### Lagerung und Stabilität

Ungeöffnete Fläschchen sind bei Lagerung zwischen 2-8°C zum bis auf dem Etikett angegebenen Verfallsdatum haltbar.

Gelöstes Plasma verändern die analytischen Levels unter 10% wenn wie folgt gelagert:

-20 °C	2-8 °C	20-25 °C
1 Monat	8 Stunden	4 Stunden

Gelöstes Plasma kann einmalig wiedereingefroren werden. Die Aliquots (120-150µL) sind 30 Tage haltbar, wenn sie in polypropylen Gefäßen bei -20°C aufbewahrt werden.

### Vorsichtsmaßnahmen

Dieses Produkt enthält Substanzen humanen Ursprungs! Haut- und Augenkontakt vermeiden. Angemessene Schutzkleidung tragen. Abfälle laut lokaler Regelungen für infektiöse Materialien entsorgen. Alle Bestandteile wurden auf HIV, HBV und HCV getestet. Trotzdem müssen Produkte aus menschlichem Blut immer als potentiell infektiös angesehen werden.

### Erwartete Ergebnisse

Lesen Sie das Analysenzertifikat

### Garantie

Es wird garantiert, dass die Wirkungsweise dieses Produkts den Angaben auf der Packung und in der Produktliteratur entspricht. TECO haftet weder für die Verkäuflichkeit oder Eignung dieses Produktes für irgendwelche andere Zwecke noch für irgendwelche Folgeschäden, die sich aus der vorstehenden, expliziten Garantie ergeben.

Erklärung der Symbole:

Verfallsdatum	In-Vitro Diagnostik	Biologische Gefahr	Katalog-Nummer	Begleitpapiere beachten
Bei 2-8°C lagern	EU Konformität	Hersteller	Lot. - Nummer	Bevollmächtigter





IVD

REF

P6101-010

**Intended Use**

Use as an abnormal control for following coagulation tests:

**PT, APTT, Thrombin time, Fibrinogen,  
Antithrombin and D-Dimer**

**Contents**

10 x 1mL freeze dried citrate-anticoagulated human plasma

**Preparation**

Reconstitute individual vials with **1,0 ml** distilled water. Allow to stand at room temperature, with occasional swirling, for 15 min before use. Be certain all particulate matter is well dissolved.

PT whole blood (TEClot PT-B): Reconstitute individual vials with **1,7 ml** distilled water.

**Storage & Stability**

Unopened vials are stable until the expiration date shown on the label stored at 2°-8°C.

Dissolved plasma change analytic levels below 10% if stored as following:

-20 °C	2-8 °C	20-25 °C
1 month	8 hours	4 hours

Dissolved plasma can be refrozen only one time in aliquots (120-150µL). Stored at -20°C in closed polypropylene tubes, the aliquots must be used within 30 days.

**Precautions**

This product contains substance from human origin!  
Avoid contact with skin and eyes. Wear suitable protective clothing. Dispose components in compliance with local regulations for infectious material. All components are checked for HIV, HBV and HCV. However products from human blood should be considered as potentially infectious.

**Expected Results**

Refer to "Certificate of Analysis".

**Warranty**

This product is warranted to perform in accordance with its labelling and literature. TECO disclaims any implied warranty of merchantability or fitness for any other purpose, and in no event will TECO be liable for any consequential damages arising out of aforesaid express warranty.

Symbols key:

Expiry date	In Vitro Diagnostica	Biological hazard	Catalogue Number	Consult accompanying documents
Store at 2-8°C	EU conformity	Manufacturer	Lot. Number	Authorized Representative



**Verwendungszweck**

Als abnormale Kontrolle für folgende Gerinnungstests verwenden:

**PT, APTT, Thrombinzeit, Fibrinogen,  
Antithrombin und D-Dimer**

**Inhalt**

10 x 1mL gefriergetrocknetes mit Zitrat versetztes gerinnungshemmendes Humanplasma

**Vorbereitung**

Die einzelnen Fläschchen mit 1,0ml destilliertem Wasser anlösen. Fläschchen bei Raumtemperatur bis zur Anwendung unter gelegentlichen Verwirbeln 15 Minuten lang stehen lassen. Stellen Sie sicher, dass alle Partikel gut aufgelöst sind.

Vollblut PT (TEClot PT-B): einzelne Fläschchen mit 1,7ml destilliertem Wasser anlösen.

**Lagerung und Stabilität**

Ungeöffnete Fläschchen sind bei Lagerung zwischen 2-8°C zum bis auf dem Etikett angegebenen Verfallsdatum haltbar.

Gelöstes Plasma verändern die analytischen Levels unter 10% wenn wie folgt gelagert:

-20 °C	2-8 °C	20-25 °C
1 Monat	8 Stunden	4 Stunden

Gelöstes Plasma kann einmalig wiedereingefroren werden. Die Aliquots (120-150µL) sind 30 Tage haltbar, wenn sie in polypropylen Gefäßen bei -20°C aufbewahrt werden.

**Vorsichtsmaßnahmen**

Dieses Produkt enthält Substanzen humanen Ursprungs! Haut- und Augenkontakt vermeiden. Angemessene Schutzkleidung tragen. Abfälle laut lokaler Regelungen für infektiöse Materialien entsorgen. Alle Bestandteile wurden auf HIV, HBV und HCV getestet. Trotzdem müssen Produkte aus menschlichem Blut immer als potentiell infektiös angesehen werden.











**Erwartete Ergebnisse**

Lesen Sie das Analysenzertifikat

**Garantie**

Es wird garantiert, dass die Wirkungsweise dieses Produkts den Angaben auf der Packung und in der Produktliteratur entspricht. TECO haftet weder für die Verkäuflichkeit oder Eignung dieses Produktes für irgendwelche andere Zwecke noch für irgendwelche Folgeschäden, die sich aus der vorstehenden, expliziten Garantie ergeben.

Erklärung der Symbole:

 Verfallsdatum	 In-Vitro Diagnostik	 Biologische Gefahr	 Katalog-Nummer	 Begleitpapiere beachten
 Bei 2-8°C lagern	 EU Konformität	 Hersteller	 Lot. - Nummer	 Bevollmächtigter



TOP  
INNOVATION  
2017 - 2018

Clotting  
Chromogenic  
Immunturbidimetric

# Coatron

Semi-automated  
Coagulation Analyzer Series

With 1, 2 or 4 optical channels



# TECO

Innovation in Coagulation

# A new area of manual and semi-automated Coagulation Analyser rise up

The Coatron X instrument line is a consequent continuation in the development of the Coatron product line. Over 25 years in experience and innovation is the reference for our new Coatron X instrumentation line.

The unique detection principle in combination with the high-level analytical algorithm calculates exact, precise and reproducible results.

Easy in operation – self instructing user dialogue - reliable

## **Highest optical resolution, enlarged optic range, smallest sample and reagent volume**

0.1 mOD, 0 - 3800 mOD, just with 75 µL sample and reagent volume

## **Complete optical analysis**

No further parts required, like balls, stirrers etc.

## **Adaptation of the light level**

Automatic light level adjustment of the optic channels to each sample

## **Exclusion of disturbance**

Stray light reduction, exact temperature control, all parameter are preset

“Complete range of Coagulation Analysis with the highest standard and reliability. The new generation of Coagulation instruments with optical detection are here.”

Coatron X - product family



With 1, 2 or 4 optical channels.

[www.teco-medical.com](http://www.teco-medical.com)



## Prepared for the daily routine and the upcoming requirements


### One instrument – many possibilities

The Coatron X family is prepared to work with one, two or four channels. The built-up and functionality is specifically designed to each instrument version and requirements. The operation with the intuitive user dialogue and handling of the detection results are easy and effective. The possibility to connect the instrument to the **TECO Cloud** offers new perspective of instrument, reagent and consumables verification and handling. The precise and correct patient result is what we want to secure.




### Quality is our basic demand

TECO develop and produce with qualified and specialized companies, located in Germany. High reliability, nearly maintenance free instruments are our benefit. Our reference is 25 years, in worldwide laboratories, with satisfied users.

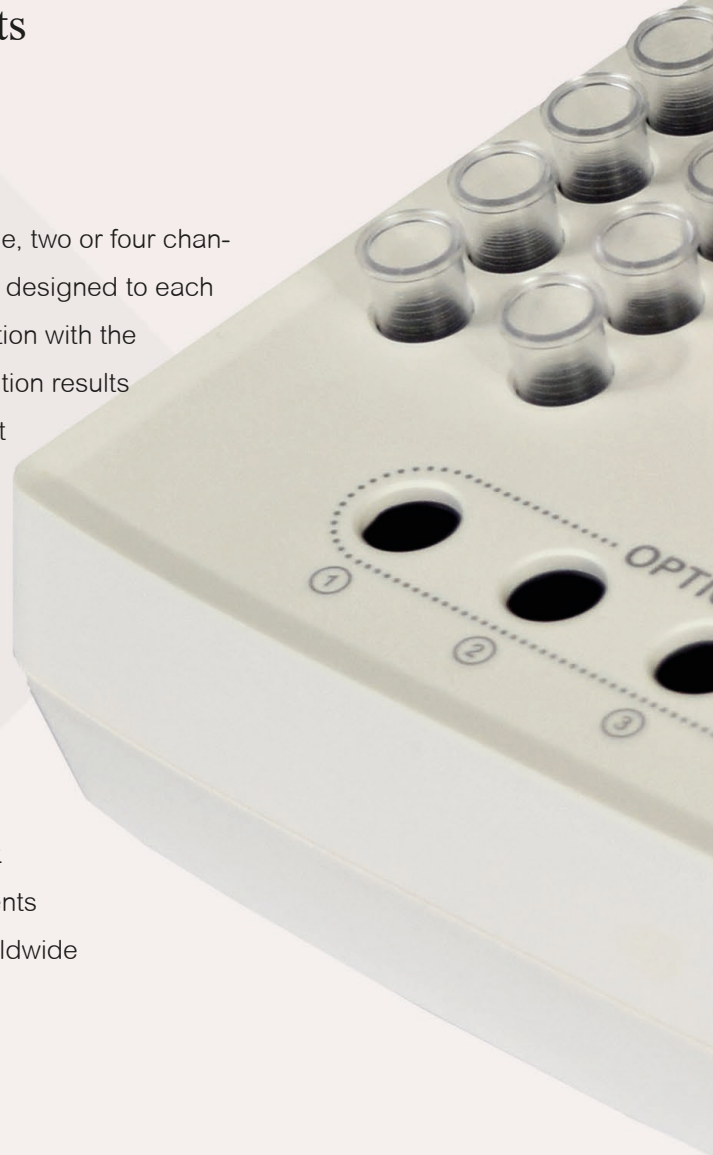

### TECO Cloud Services – A strong data bank and application service behind

All instrument versions of the Coatron X family are connectable via Bluetooth to Smart-devices, like mobile devices, tablets, etc. with a specific APP or direct access to the TECO Cloud Services.

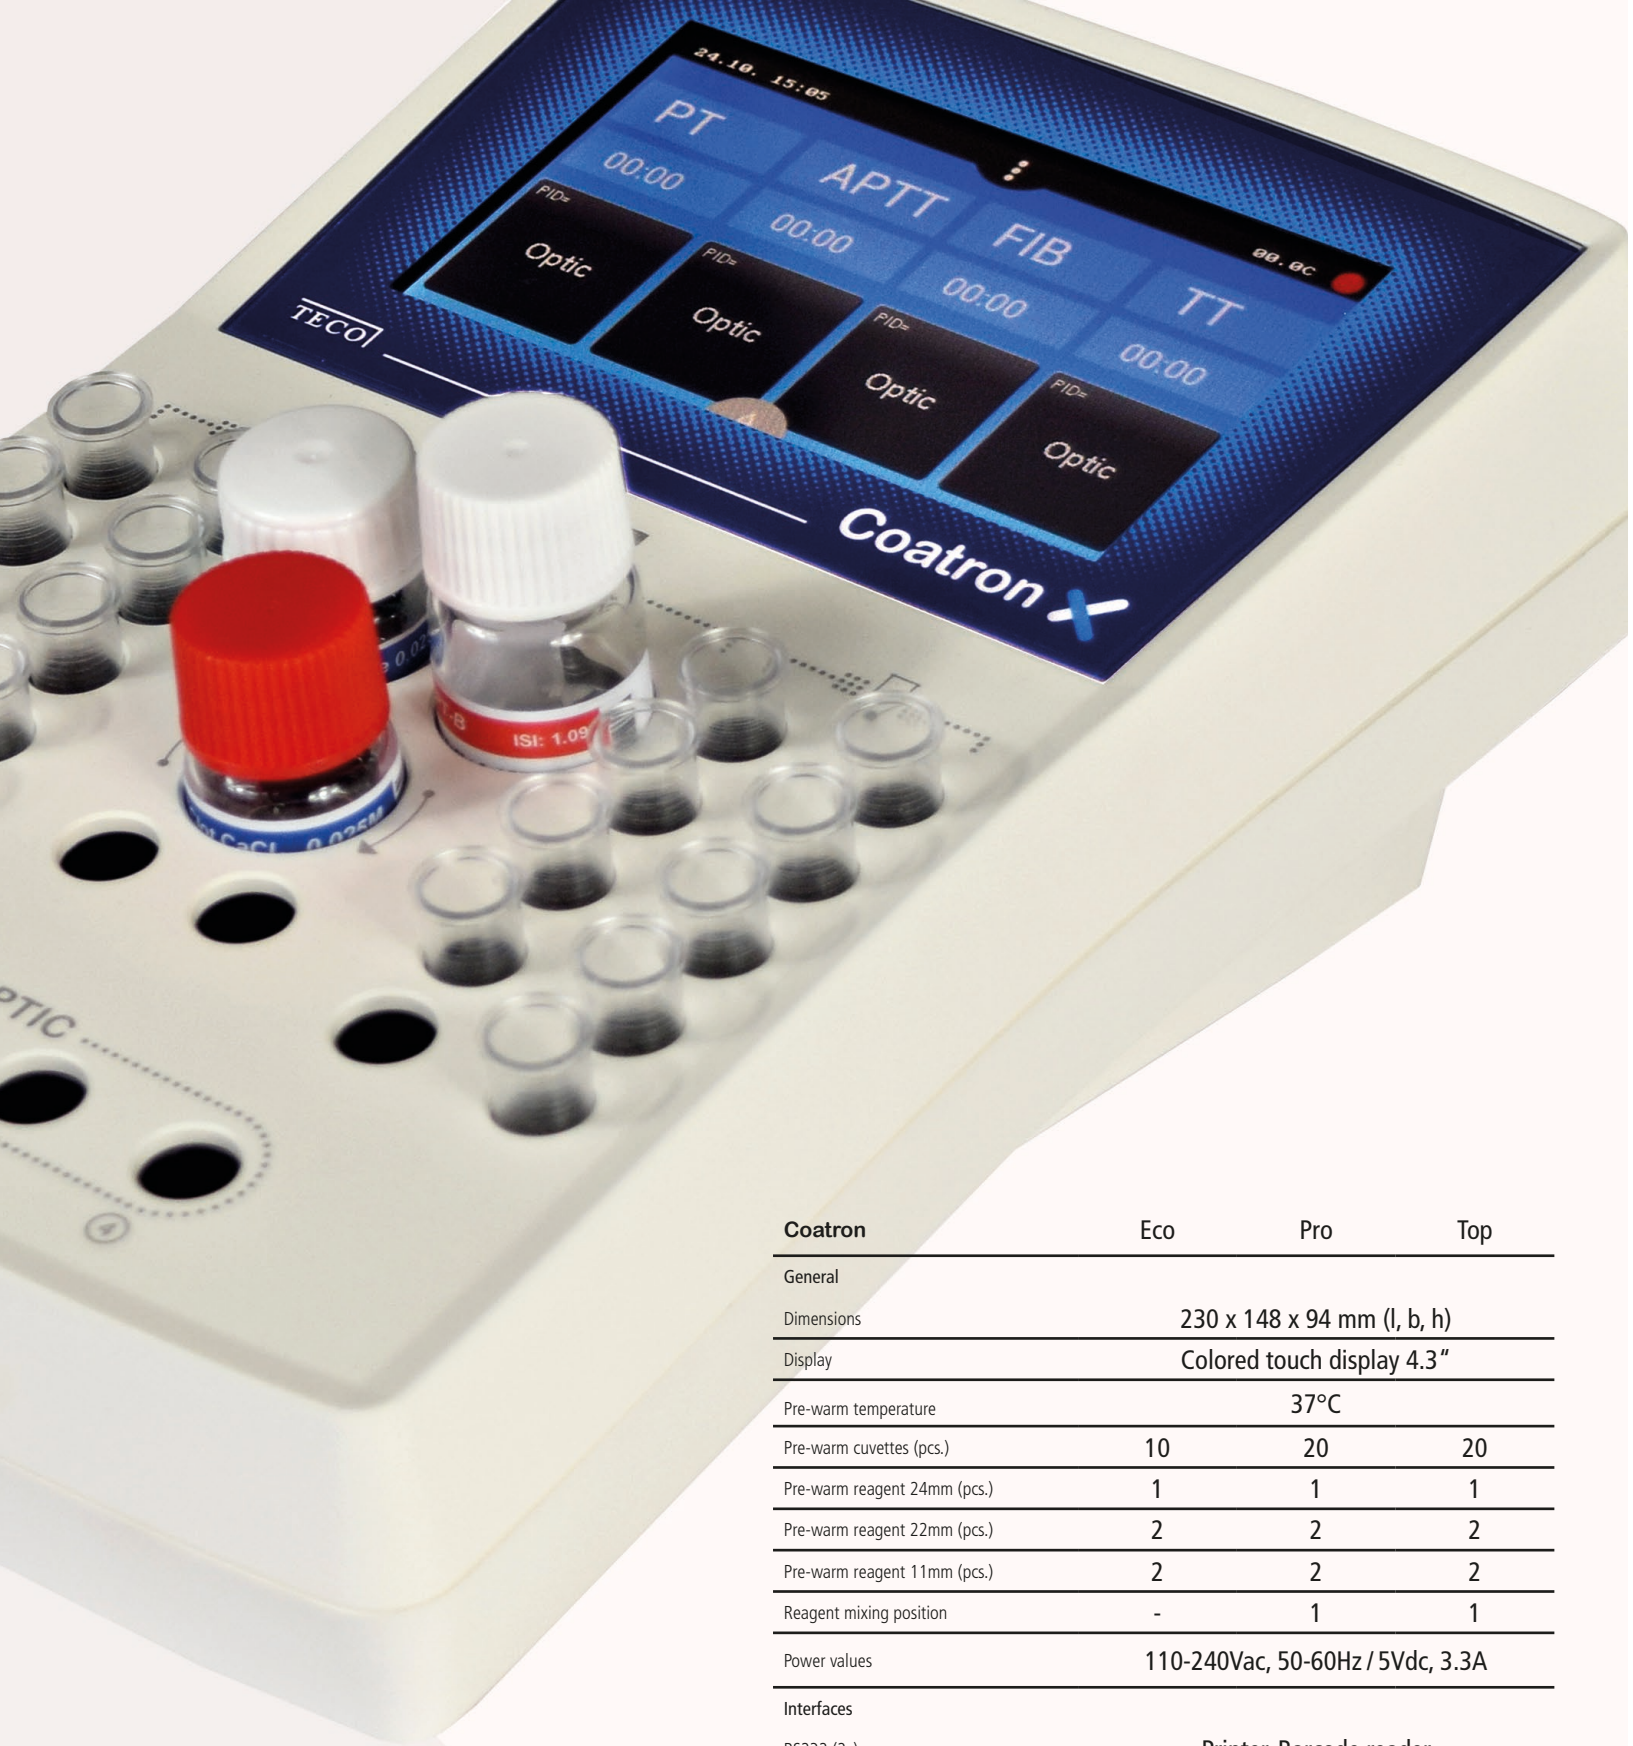

Coatron	Eco	Pro	Top
General			
Dimensions	230 x 148 x 94 mm (l, b, h)		
Display	Colored touch display 4.3"		
Pre-warm temperature	37°C		
Pre-warm cuvettes (pcs.)	10	20	20
Pre-warm reagent 24mm (pcs.)	1	1	1
Pre-warm reagent 22mm (pcs.)	2	2	2
Pre-warm reagent 11mm (pcs.)	2	2	2
Reagent mixing position	-	1	1
Power values	110-240Vac, 50-60Hz / 5Vdc, 3.3A		
Interfaces			
RS232 (2x)	Printer, Barcode reader		
USB (2x)	Network, Firmware update		
Bluetooth	TECO Cloud, App		
Optic / tests			
Optic channels	1	2	4
Wavelength (nm)	620 (red)	405 (UV)	405 (UV)
Global Coag. tests	PT, APTT, TT, FIB		
Specific Coag. tests	-	individual factors	
Chromogenic Coag. tests	-	AT, PC	
Latex based tests	D-Dimer		
Whole blood tests	PT-B		-



## The details make the difference

### Coatron X


The remarkable details in every single component is achieved by selecting of premium suppliers.

The performance of a high level instrument is strongly depending on the concept in general and the perfect usability to reach the requirements of a modern laboratory analyser.

Priority No. 1 was to get a daily routine reliability and easy-to-use operation.

### Software and connection possibilities

With the Coatron X product family starts a new time line in analysis management and service maintenance. Operation via intuitive, colored touchscreen, as well patient result management are perfectly optimized.

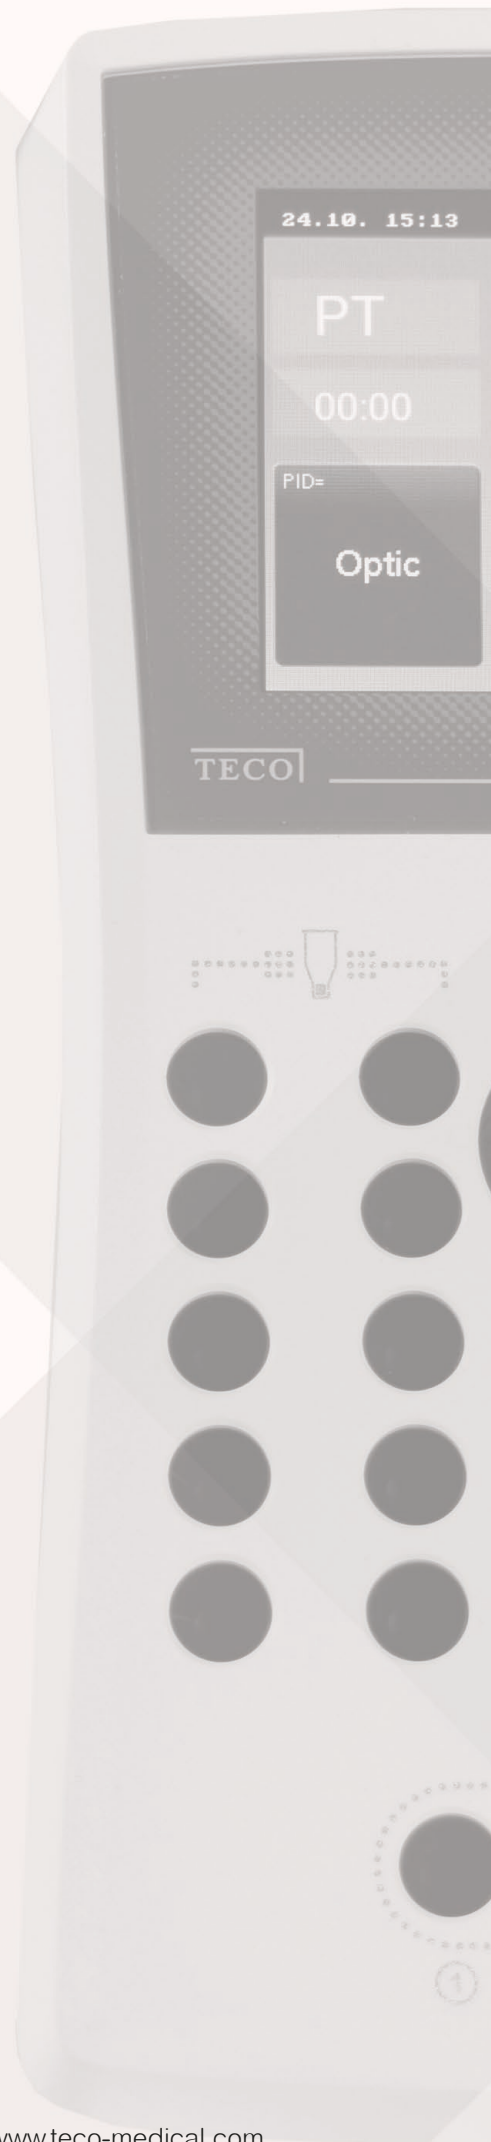

## Operation details

Coatron	Eco	Pro	Top
<b>Operation</b>			
Touchscreen 4.3"	✓	✓	✓
Real time clock	✓	✓	✓
Stopwatch	✓	✓	✓
Language selection	✓	✓	✓
<b>Interfaces</b>			
USB to LIS	✓	✓	✓
Network to LIS (TECAM software required)	✓	✓	✓
<b>Management</b>			
Test calibration	✓	✓	✓
Tracking to Pat.ID, Patient ID, Sample ID or Auto ID	✓	✓	✓
Automatic optic start (no Starterpipette required)	✓	✓	✓
Double determination	✗	✓	✓
Sample management (ID)	✗	✓	✓
Reagent management (ID) (lot und expiry)	✗	✓	✓
Internal result databank	✗	✓	✓
Patient identification with barcode		optional	



### Intuitive operation and control

Clear and easy to operate user dialogue with a high quality colored touchscreen

- Direct usable
- Short learning phase
- Logic, intuitive operation
- Reliable touchscreen surface
- Quick touch response



### For small and mediate laboratory requirements

Concept is suitable for daily routine work in Coagulation laboratories and hospitals

- Three different versions available, depending on number of samples per day
- In maximum up to 4 optic channels available

### Interfaces

#### RS232 (2x)

- For external serial printer and external barcodereader

#### LIS/USB

#### Bluetooth



Integrated barcode scan for reagents.





### **TECO Cloud Services**

#### **A strong data bank and application service behind**

All instrument versions of the Coatron X family are connectable via Bluetooth to Smart-devices, like mobile devices, tablets, etc. with a specific APP or direct access to the TECO Cloud Services.



For trading partners worldwide, please visit our web-page

**TECO Medical Instruments Production + Trading GmbH**  
Dieselstr. 1, 84088 Neufahrn, Germany  
Tel.: +49 (0) 8773 70780-0, Fax +49 (0) 8773 70780-29  
info@teco-gmbh.com, www.teco-medical.com

**TECO**  
Innovation in Coagulation