
# **IFU for Sterilant RENO-SA10**

\* For use in RENO-S130 and RENO-S130D

### **Product Specifications**


- Intended Use: It is a sterilant when medical products are sterilized in the low temperature plasma sterilizers made by Renosem. Co., Ltd.
- 2. Storage condition: The sterilants should be stored in a room temperature of 5°C~30°C.
- 3. Expiry date: 12 months
- 4. Capacity: 4 ml/capsule(50%)

## External Appearance and structure



No.	Part name	Fuction
1	Syringe rubber cap	As an inlet for sterilant
2	Syringe body	To store sterlant

#### How to insert the sterilant

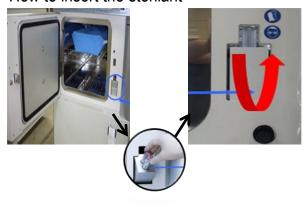

- 1. Take out the inlet of sterilant by pressing the button located on the right lower part of chamber.
- 2. Place the RENO-SA10 into the hole by holding the red rubber part.
- 3. Check if blue lamp turns on on the right upper part and push the inlet back to position.
- 4. Close the door.

### Outer box Package

- 1. 15 ea (per box)
- 2. Material: Carton
- 3. Size: 185W x 155L x 119H (mm)



#### Caution









- 1. Hazard statement
- 2. Precautionary statement
- 3. Please read the RENO sterilizer operator's manual for details on warnings.
- 4. Do not use this sterilant for any uses other than the original purpose.
- This sterilant is an accessory for the lowtemperature plasma sterilizers for medical instruments.

### **Pictograms**

1. Follow the instructions for use



To be used before YY/MM



3. Date of manufacture



4. EC representative



#### Renosem Co., Ltd.

Unit 103-806, 397, Seokcheon-ro Bucheon, Gyeonggi 14449 South Korea

T: +82 32 222 0143

F: +82 32 222 0110