

130325
OFFICE OF THE COMMISSIONER
FOOD & DRUGS CONTROL ADMINISTRATION
DR. JIVRAJ MEHTA BHAVAN, BLOCK NO. 8,
FIRST FLOOR, GANDHINAGAR-382 010
(GUJARAT) INDIA
DATE: -

- 4 DEC 2018

FREE SALE CERTIFICATE

This to certify that M/s. **HARDIK INTERNATIONAL**. Situated at. Plot no. G-2041/42A, Kishan Gate, Lodhika G.I.D.C. , Kalawad Road ,Metoda-360021, Rajkot (india) . Holding valid Drugs Manufacturing Licence in form 28-A bearing licence No: G/28/1356 is respectively issued on date .30/10/2010 & Valid up to 29/10/2020 is under consideration by the administration under the provisions of Drugs & cosmetics Act 1940 & Rules thereunder the said licence the firm is permitted to manufacture the following drugs(Orthopedic Implants-Non Sterile)to be freely sold in Indian market & Export.

Under the above licence the firm is permitted to manufacture & market the product listed below to Be exported freely.

Such type of similar products available in country of origin subject to laws of land in question

Sr. No.	Name Of Products
1.	Bone Screws (Non Sterile)
2.	Bone Plates (Non Sterile)
3.	Bone Nails (Non Sterile)
4.	Bone Wires, Pins & Staples
5.	Spine Implants (Non Sterile)
6.	Endoprosthesis (Non Sterile)
7.	Arthroscopy Implants (Non Sterile)
8.	Other Implants (Non Sterile)



This is also certified that manufacturing plant in which the product is manufactured is subjected to Regular inspection at suitable intervals.


This certificate is valid for two years from date of issue

Encl. Product List


For Commissioner,
Food & Drugs Control Administration,
Gujarat State, Gandhinagar.

Orthopedic Implants

S.no	Model Name	Generic name	Length in mm	Diameter in mm	Other Information Like Hole	Material of Construction	Intended Use	Sterile /Non Sterile	Self-life	Export/Domestic
1		BONE SCREW								
	HARDIK	Cortex Screw	10mm to 60mm	3.5mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Cortex Screw	12mm to 80mm	4.5mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Cancellous Screw	10mm to 70mm	4mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Cancellous Screw	25mm to 110mm	6.5mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Cannulated Cancellous Screw	25mm to 120mm	6.5mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Cannulated Cancellous Screw	25mm to 120mm	7mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Malleolar Screw	25mm to 100mm	4.5mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	DHS/DCS Lag Screw	50mm to 120mm	N.A.	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Interlocking Screw	20mm to 80mm	4.9mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Interlocking Screw	16mm to 60mm	3.9mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Interlocking Screw	16mm to 60mm	3.4mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Interlocking Screw	14mm to 50mm	2.9mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Locking Compression Screw	12mm to 70mm	3.5mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Locking Compression Screw	14mm to 80mm	5mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Hip Locking Screw Cannulated	50mm to 120mm	6.2mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Proximal Femoral Screw	50mm to 120mm	8mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Cortex Screw with Locking Head	10mm to 50mm	3.5mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Cortex Screw with Locking Head	14mm to 60mm	5mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH

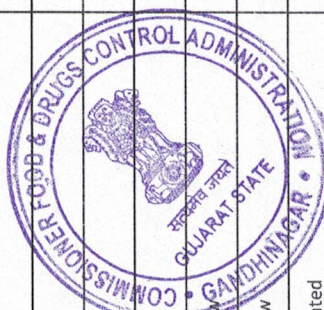


Orthopedic Implants

S.no	Model Name	Generic name	Length in mm	Diameter in mm	Other Information Like Hole	Material of Construction	Intended Use	Sterile /Non Sterile	Self-life	Export/Domestic
	HARDIK	Locking Cancellous Screw	25mm to 110mm	6.5mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Locking Cancellous Screw	14mm to 80mm	4mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Herbert Screw Cannulated	14mm to 34mm	3.5mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	ACL Screw	20mm to 40mm	6mm to 10mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Schanz Screw	100mm to 250mm	2mm to 6.5mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
2		BONE PLATES								
	HARDIK	One Third Tubular Plate 3.5mm	N.A.	N.A.	2hole to 14hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Small Dynamic Compression Plate 3.5mm	N.A.	N.A.	2hole to 14hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Small Limited Contact Dynamic Compression Plate 3.5mm (LC-DCP)	N.A.	N.A.	4hole to 14hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Small T-Plate 3.5 mm	N.A.	N.A.	3hole to 8hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Small Oblique T-Plate 3.5mm	N.A.	N.A.	3hole to 8hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Reconstruction Plate 3.5mm (DC Hole)	N.A.	N.A.	4hole to 28hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Reconstruction Plate 3.5mm (Round Hole) (LC-DCP)	N.A.	N.A.	4hole to 28hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Semi Tubular Plate 4.5mm	N.A.	N.A.	2hole to 18hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Narrow Dynamic Compression Plate 4.5mm	N.A.	N.A.	2hole to 18hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Broad Dynamic Compression Plate 4.5 mm	N.A.	N.A.	4hole to 18hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Narrow Limited Contact Dynamic Compression Plate 4.5mm (LC-DCP)	N.A.	N.A.	2hole to 16hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Broad Limited Contact Dynamic Compression Plate 4.5mm (LC-DCP)	N.A.	N.A.	4hole to 18hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	T-Plate 4.5 mm	N.A.	N.A.	3hole to 14hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	T-Butress Plate 4.5mm	N.A.	N.A.	3hole to 14hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH


Orthopedic Implants

S.no	Model Name	Generic name	Length in mm	Diameter in mm	Other Information Like Hole	Material of Construction	Intended Use	Sterile /Non Sterile	Self-life	Export/Domestic
	HARDIK	L-Butress Plate 4.5mm (Left & Right)	N.A.	N.A.	3hole to 14hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Condylar Butress Plate 4.5mm (Left & Right)	N.A.	N.A.	4hole to 16hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	DHS Plate (DC Hole) 125°/130°/135°/140° Barrel Length 25mm, 32mm & 38mm	N.A.	N.A.	2hole to 20hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	DHS Plate (Round Hole) 125°/130°/135°/140° Barrel Length 25mm, 32mm & 38mm	N.A.	N.A.	2hole to 20hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	95° DCS Plate (DC Hole)	N.A.	N.A.	4hole to 22hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	95° DCS Plate (Round Hole)	N.A.	N.A.	4hole to 22hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Small Locking Compression Plate 3.5mm	N.A.	N.A.	4hole to 14hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Narrow Locking Compression Plate 4.5mm/5.0mm	N.A.	N.A.	4hole to 18hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Broad Locking Compression Plate 4.5mm/5.0mm	N.A.	N.A.	4hole to 20hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Locking Small T Plate 3.5mm	N.A.	N.A.	3hole to 8hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Locking Small Oblique T Plate 3.5mm (Left & Right)	N.A.	N.A.	3hole to 8hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Locking Reconstruction Plate 3.5mm & 4.5mm/5.0mm	N.A.	N.A.	4hole to 28hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Locking T Butress Plate 4.5mm/5.0mm	N.A.	N.A.	4hole to 14hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Locking L-Butress Plate 4.5mm/5.0mm (Left & Right)	N.A.	N.A.	3hole to 14hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Locking Lateral Tibia Plate 4.5mm (Left & Right)	N.A.	N.A.	4hole to 16hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Locking Proximal Humeral Plate 3.5mm	N.A.	N.A.	3hole to 16hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Locking Distal Femoral Plate 4.5mm/5.0mm (Left & Right)	N.A.	N.A.	4hole to 16hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Locking Condylar Butress Plate 4.5mm (Left & Right)	N.A.	N.A.	4hole to 16hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Staffe Plate	1slot to 5slot	N.A.	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH

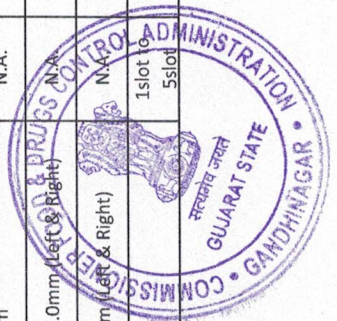

Orthopedic Implants

S.no	Model Name	Generic name	Length in mm	Diameter in mm	Other Information Like Hole	Material of Construction	Intended Use	Sterile /Non Sterile	Self-life	Export/Domestic
	HARDIK	Anterior Cervical Plate	21.5 mm to 110 mm	N.A.	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Bone Screw for Anterior Cervical Plate	10mm to 24mm	4mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Lock Screw for Anterior Cervical Plate	N.A.	N.A.	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
3		BONE WIRES, PINS AND STAPLES								
	HARDIK	Kirchner Wire (K-Wire)	100mm to 300mm	0.8mm to 3mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Staimann Pin	125mm to 300mm	3.5mm to 5mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	SS Wire Reel 16SWG to 34SWG	N.A.	N.A.	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Staple	N.A.	N.A.	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
4		ENDOPROSTHESIS								
	HARDIK	Bipolar Prosthesis (Non-Fen. & Fen.)	N.A.	37mm to 55mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Austin Moore Prosthesis	N.A.	37mm to 55mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Thompson Prosthesis	N.A.	37mm to 55mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
5		BONE NAILS								
	HARDIK	Humeral Interlocking Nail	180mm to 320mm	6mm to 8mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Universal Tibial Interlocking Nail	260mm to 380mm	8mm to 12mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Universal Femoral Interlocking Nail	360mm to 460mm	8mm to 14mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	XL Tibial Interlocking Nail	285mm to 320mm	8mm to 12mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	XL Femoral Interlocking Nail	285mm to 460mm	8mm to 12mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Proximal Femoral Nail (PFN)	220mm to 250mm	9mm to 12mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Antegrade Femoral Nail (AFN Nail)	340mm to 440mm	9mm to 14mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Sirustype Femur Nail	340mm to 440mm	9mm to 12mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH

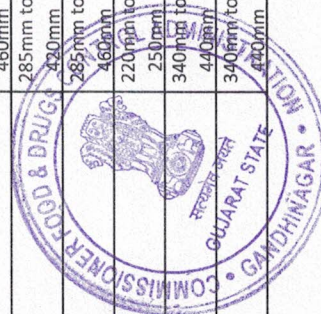

Orthopedic Implants

S.no	Model Name	Generic name	Length in mm	Diameter in mm	Other Information Like Hole	Material of Construction	Intended Use	Sterile /Non Sterile	Self-life	Export/Domestic
	HARDIK	Multifunctional Femoral Nail	340mm to 460mm	9mm to 14mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Enders Nail	150mm to 300mm	2.5mm to 4.5mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Reconstruction Femoral Nail (Recon Nail) (Left & Right)	340mm to 460mm	9mm to 12mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Elastic Nail	440mm	2mm to 4mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
6		SPINE IMPLANTS								
	HARDIK	Monoaxial Screw	30mm to 60mm	4mm to 7mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Polyaxial Screw	30mm to 60mm	4mm to 7mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Reduction Screw	30mm to 60mm	4mm to 7mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Monoaxial Screw Single Lock	30mm to 60mm	5mm to 7mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Polyaxial Screw Single Lock	30mm to 60mm	5mm to 7mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Staffe Screw	26mm to 42mm	4.5mm to 5.5mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Hooks	N.A.	N.A.	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Transversers Connector	N.A.	N.A.	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Rod	50mm to 150mm	3mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Rod	50mm to 140mm	5.5mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Cage Eco	20mm to 30mm	10mm to 24mm	N.A.	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH




Orthopedic Implants

S.no	Model Name	Generic name	Length in mm	Diameter in mm	Other Information Like Hole etc.	Material of Construction	Intended Use	Sterile /Non Sterile	Self-life	Export/Domestic
1	HARDIK	BONE SCREWS								
	HARDIK	Cortex Screw	4mm to 22mm	1.5mm to 2.5mm	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Cortex Screw (Cross Head)	4mm to 22mm	1.5mm to 2.5mm	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Cortex Screw (Hexagonal)	4mm to 22mm	1.5mm to 2.5mm	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Cortex Screw (Self Tapping)	8mm to 40mm	2.7 3.5mm & 4.5mm	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Cortex Screw (14 TPI)	10mm to 70mm	3.5mm	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Cancellous Screw (Short Th. & Full Thread)	12mm to 80mm	3.5mm & 4.0mm	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Locking Compression Screw	10mm to 60mm	2.4mm & 2.7mm	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Locking Cancellous Screw (Short Th. & Full Thread)	12mm to 80mm	3.5mm & 4.0mm	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Cancellous Screw (16mm, 32mm & Full Thread)	20mm to 130mm	6.5mm	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Locking Compression Screw	85mm to 100mm	5.0mm	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Locking Cancellous Screw (16mm, 32mm & Full Thread)	20mm to 130mm	5.5mm & 6.5mm	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Locking Canulated Cancellous Screw (16mm, 32mm & Full Thread)	20mm to 130mm	5.5, 6.5 & 7.0mm	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Compression Screw for DHS Lag Screw	20mm to 50mm	N.A	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Canulated Screw (Short & Full Thread)	16mm to 80mm	3.5mm & 4.0mm	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Canulated Screw (16mm, 32mm & Full Thread)	20mm to 130mm	6.5mm & 7.0mm	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Suture Anchor Screw	N.A	3mm & 5mm	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	BONE PLATES								




HARDIK	Mandible Plate With Center Space	N.A	1.5mm to 2.5mm	2hole to 10hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Mandible Plate	N.A	1.5mm to 2.5mm	2hole to 20hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Orbital Plate with Center Space	N.A	1.5mm to 2.5mm	2hole to 10hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Orbital Plate	N.A	1.5mm to 2.5mm	2hole to 10hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	L Plate Angle 2hole & 3hole (Left & Right)	N.A	1.5mm to 2.5mm	2hole to 6hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	T Plate Head 2hole & 3hole	N.A	1.5mm to 2.5mm	2hole to 6hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	X Plate	N.A	1.5mm to 2.5mm	5hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Y Plate	N.A	1.5mm to 2.5mm	3hole to 8hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Z Plate	N.A	1.5mm to 2.5mm	4hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Double End Y Plate	N.A	1.5mm to 2.5mm	6hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Curved Plate (Left & Right)	N.A	1.5mm to 2.5mm	2x2hole, 3x3hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	L Plate Angle 2hole & 3hole Without Bar (Left & Right)	N.A	1.5mm to 2.5mm	2hole to 6hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Angular Plate 150° (Left & Right)	N.A	1.5mm to 2.5mm	4hole & 6hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	L Plate 120° (Left & Right)	N.A	1.5mm to 2.5mm	4hole & 6hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Nose Y Shape Plate	N.A	1.5mm to 2.5mm	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Nose H Shape Plate	N.A	1.5mm to 2.5mm	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Chin Plate	N.A	1.5mm to 2.5mm	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	I Plate	N.A	1.5mm to 2.5mm	4hole & 6hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	TMJ Plate	N.A	1.5mm to 2.5mm	4hole to 22hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	3D Plate	N.A	1.5mm to 2.5mm	2+2, 2+3, 2+4hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Reconstruction Plate 2.4mm/2.7mm/3.5mm/4.5mm	N.A	N.A	2hole to 30hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Angled Reconstruction Plate 2.4mm (Left & Right)	N.A	N.A	4hole to 22hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Full Mandible Reconstruction Plate	N.A	N.A	22hole to 40hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Mesh		1.5mm to 2.5mm	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH

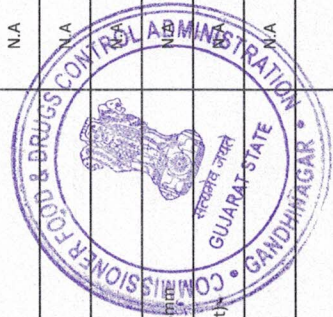

HARDIK	DCP 2.7mm	N.A	N.A	2hole to 10hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Small T-Ellis Plate 3.5mm	N.A	N.A	2hole to 8hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Small T Plate, Right Angle Head 4hole 3.5mm	N.A	N.A	2hole to 10hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Cloverleaf Plate 3.5mm	N.A	N.A	3hole to 14hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Locking Medial Distal Tibial Plate 3.5mm (Left & Right)	N.A	N.A	4hole to 16hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Locking Cloverleaf Plate 3.5mm	N.A	N.A	3hole to 12hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Locking Long Head Proximal Humeral Plate 3.5mm	N.A	N.A	3hole to 18hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Locking Distal Humeral Plate with Support 3.5mm (Left & Right)	N.A	N.A	3hole to 12hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Locking Distal Humeral Plate 3.5mm (Left & Right)	N.A	N.A	3hole to 12hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Locking Medial Distal Humeral Plate 3.5mm (Left & Right)	N.A	N.A	3hole to 10hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Locking Superior Anterior Clavicle Plate 3.5mm (Left & Right)	N.A	N.A	3hole to 10hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Locking Superior Anterior Clavicle Plate with Lateral Extension 3.5mm (Left & Right)	N.A	N.A	4hole to 18hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Locking Clavicle Hook Plate 3.5mm Hook Depth 12mm/15mm/18mm (Left & Right)	N.A	N.A	4hole to 8hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Locking Medial Distal Tibial Plate 3.5mm without tab (Left & Right)	N.A	N.A	3hole to 6hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Locking Hook Plate 3.5mm	N.A	N.A	2hole to 8hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Locking Volar Distal Radius Plate 2.7mm (Left & Right)	N.A	N.A	Small, Medium, Large, Extra Small	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Locking Calcaneal Plate 3.5mm (Left & Right)	N.A	N.A	2hole to 8hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Locking XVA Volar Distal Radius Plate 2.7mm (Left & Right)	N.A	N.A	2hole to 8hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Locking Ulna Osteotomy Plate 2.7mm	N.A	N.A	4hole to 8hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Locking Olecranon Plate 3.5mm (Left 7 Right)	N.A	N.A	3hole to 12hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Locking Proximal Radius Neck Plate 2.7mm	N.A	N.A	2hole to 6hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Locking Proximal Radius Rim Plate 2.7mm	N.A	N.A	2hole to 6hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Locking Anterolateral Distal Tibia Plate 3.5mm (Left & Right)	N.A	N.A	3hole to 14hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Locking Distal Femur Plate 3.5mm	N.A	N.A	3hole to 12hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH


HARDIK	Locking Proximal Tibia Plate 3.5mm & 4.5/5.0mm (Left & Right)	N.A	N.A	3hole to 16hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Locking Proximal Lateral Tibia Plate 3.5mm	N.A	N.A	4hole to 16hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Locking One Third Plate 3.5mm	N.A	N.A	4hole to 14hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Locking Posterior Medial Proximal Tibia Plate 3.5mm	N.A	N.A	1hole to 14hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Locking Reconstruction Plate (Thin) 3.5mm & 4.5/5.0mm	N.A	N.A	4hole to 22hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Locking Distal Radius Plate 2.7mm (Left & Right)	N.A	N.A	3hole to 6hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Locking Distal Radius Buttress Plate 2.7mm (Left & Right)	N.A	N.A	3hole to 6hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Locking Distal Radius Plate Extra Articular, Head 5 & 4 Hole 2.7mm (Left & Right)	N.A	N.A	3hole to 6hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Locking Distal Radius Plate Straight 2.7mm	N.A	N.A	5hole & 6hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Locking Distal Radius L Plate, Head 2 & 3hole 2.7mm (Left & Right)	N.A	N.A	3hole to 6hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Locking Distal Radius L Plate Oblique Angled, Head 2 & 3hole 2.7mm (Left & Right)	N.A	N.A	3hole to 6hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Locking Distal Radius T Plate 2.7mm	N.A	N.A	3hole to 6hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Lateral Tibia Head Buttress Plate 4.5mm (Left & Right)	N.A	N.A	3hole to 18hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Reconstruction Plate (DC Hole) 4.5mm	N.A	N.A	3hole to 30hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Locking L Buttress Plate 4.5/5.0mm (Left & Right)	N.A	N.A	3hole to 14hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Locking T Plate 4.5/5.0mm	N.A	N.A	3hole to 14hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Locking Proximal Femoral Plate (Left & Right)	N.A	N.A	3hole to 18hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Locking Metaphyseal Plate	N.A	N.A	3hole to 14hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Locking Tomofix Plate 4.5/5.0mm	N.A	N.A	Small, Medium	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Locking Medial Proximal Tibial Plate 4.5/5.0mm	N.A	N.A	4hole to 16hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	DHS Plate (DC Holes) 145° & 150° Barrel Length 25mm, 32mm & 38mm	N.A	N.A	2hole to 20hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	DHS Plate (Round Holes) 145° & 150° Barrel Length 25mm, 32mm & 38mm	N.A	N.A	2hole to 20hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Locking DHS Plate 125°, 130°, 135°, 140°, 145°, 150° Barrel Length 25mm, 32mm & 38mm	N.A	N.A	2hole to 20hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Locking 95° DCS Plate	N.A	N.A	4hole to 22hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH

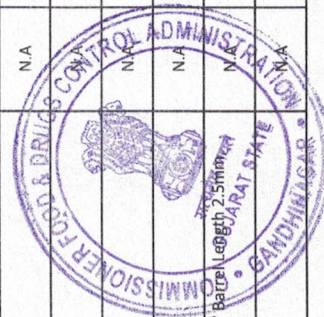

HARDIK	Pelvic Reconstruction Plate 3.5mm & 4.5mm	N.A	N.A	N.A	6hole to 20hole	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Trochanter Stabilization Plate For DHS	N.A	N.A	N.A	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	BONE NAILS									
HARDIK	XL Tibial Interlocking Nail (Distal Tip)	285mm to 420mm	8mm to 12mm	N.A	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Supra Condylar Nail	100mm to 300mm	9mm to 14mm	N.A	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Long Proximal Femoral Nail (Left & Right)	320mm to 460mm	9mm to 14mm	N.A	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	K Nail	260mm to 500mm	6mm to 16mm	N.A	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Rush Nail	16mm to 420mm	1.5mm to 7mm	N.A	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Square Nail (Radius & Ulna)	16mm to 420mm	1.5mm to 5.0mm	N.A	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Trochanteric Femoral Nail (TFN)	150mm to 170mm	9mm to 14mm	N.A	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Unreamed Tibial Interlocking Nail	285mm to 420mm	8mm to 14mm	N.A	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Unreamed Femoral Interlocking Nail	285mm to 420mm	9mm to 14mm	N.A	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Expert Tibial Interlocking Nail	280mm to 420mm	8mm to 14mm	N.A	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	End Cap for Nail	N.A	N.A	N.A	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	BONE WIRES,PINS & STAPLES									
HARDIK	Stairman Pin	100mm to 300mm	2mm to 6mm	N.A	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Spike Ligament Staple	N.A	N.A	Small, Medium, Large	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	K Wire (Single Side Trocar Tip)	100mm to 500mm	0.8mm to 3.0mm	N.A	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	K Wire (Single Side Threaded & Double Side Threaded)	100mm to 500mm	1.0mm to 3.0mm	N.A	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Coventry Staple	N.A	N.A	Small, Medium, Large	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	SPINE IMPLANTS									
HARDIK	Expendable Cage	10mm to 20mm	20mm to 100mm	N.A	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Tliff Cage 4°, 8°, 11°	N.A	6mm to 12mm	N.A	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
HARDIK	Plif Cage	15mm to 30mm	6mm to 12mm	N.A	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH

3

4

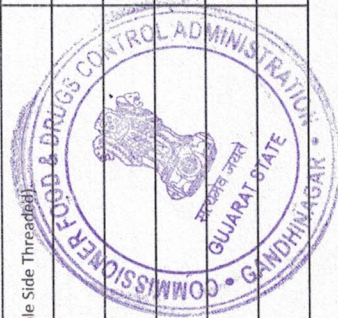

5	HARDIK	Banana Cage		20mm to 30mm	6mm to 12mm	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Pedical Hook		N.A	N.A	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Laminar Wide Blade Hook		N.A	N.A	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Laminar Reduce Distance Hook		N.A	N.A	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Laminar Angle Blade Hook		N.A	N.A	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
6	HARDIK	ENDOPROTHESIS									
	HARDIK	Austin Moore Prosthesis (Narrow Stem)		N.A	37mm to 55mm	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Femoral Stem Cemented		N.A	Small, Medium, Large	N.A	SS 316L /SS 316LVM /TITANIUM/	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Modular Bipolar Head (Short Neck/ Medium Neck/Long Neck)		N.A	37mm to 55mm	N.A	SS 316L /SS 316LVM /TITANIUM/UHMWPE	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	ARTHROSCOPY IMPLANTS									
7	HARDIK	Endo Buttons		N.A	N.A	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Endo Buttons with Loop		15mm to 50mm	N.A	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Suture Disc		N.A	N.A	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	Spike Washer		N.A	N.A	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH
	HARDIK	OTHER IMPLANTS									
8	HARDIK	Washer		N.A	4mm to 15mm	N.A	SS 316L /SS 316LVM /TITANIUM	BONE FRACTURE	NON STERILE	Not Applicable	BOTH

