



REAGEN

Certificate of Conformity

KIT :

Chlortetracycline ELISA Kit RND99050

Release Date

Oct.5th ,2019


Expiration Date:

Oct./2020

Temperature: 25°C

REAGEN LLC certifies that this lot has passed Quality control assays and conforms to product release specifications.

Standards	Rep. #1	Rep. #2	Rep.#3	Avg.	Std. Dev.	%RSD	%Bo
Negative Control	2.165	2.129	2.189	2.161	0.03	1.39	100%
0.2ppb Calibrator	1.898	1.954	1.925	1.926	0.028	1.45	89.1%
0.4ppb Calibrator	1.623	1.624	1.632	1.626	0.005	0.31	75.2%
0.8ppb Calibrator	1.019	1.043	1.026	1.029	0.012	1.17	47.6%
1.6 ppb Calibrator	0.519	0.534	0.528	0.527	0.008	1.52	24.4%
3.2 ppb Calibrator	0.239	0.23	0.241	0.237	0.006	2.53	11.0%

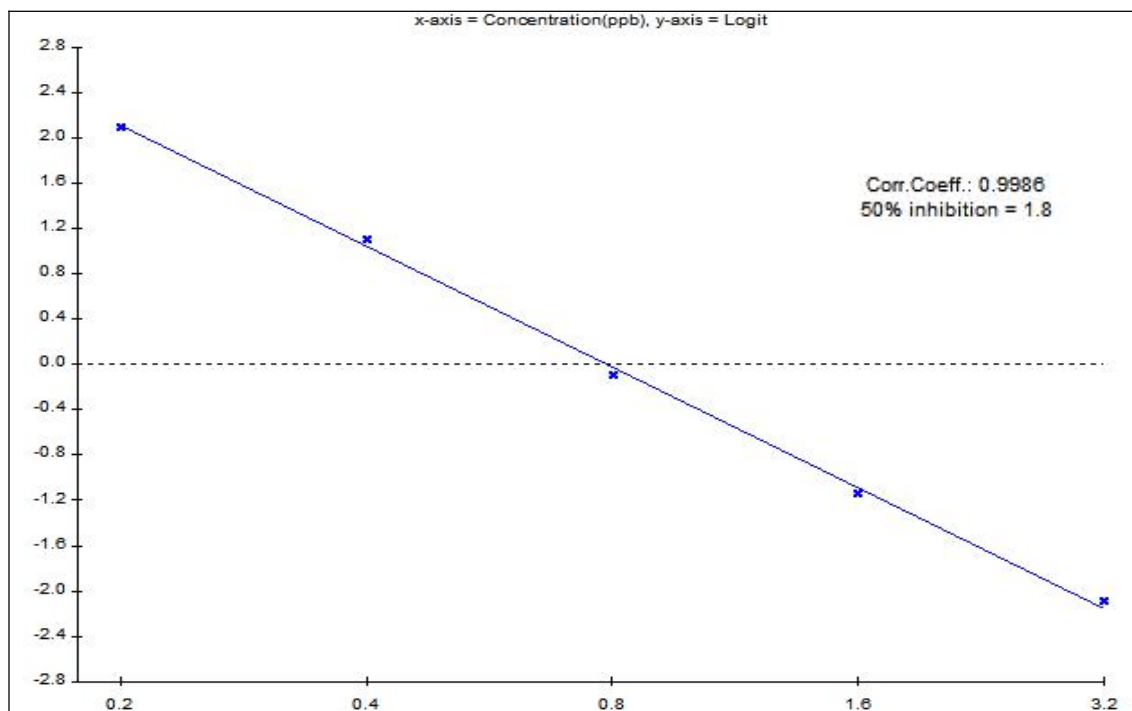

Note: The absorbance of the calibrators may Decrease during the shelf life of kit . Actual values may vary; this data is for example purposes only.

QA Manager Alexis Release Date Oct.5th ,2019

REAGEN