




■ Setting kV and mA or mAs and sec

You can specify values for kV (radiography tube voltage), mA (radiography tube current) or mAs (radiography tube current time product), and sec (radiography time).

- 1 Press the lower  icon on the touch panel.

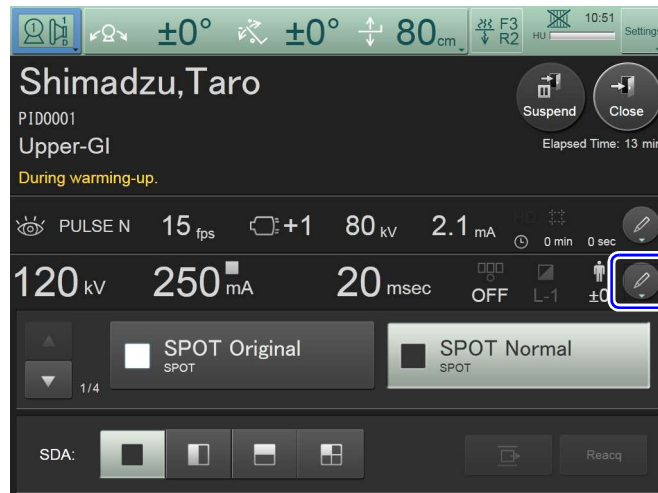

The [Radiography Condition Details] screen is displayed.

- 2 Use  or  under each item to specify a value.

