Digitally signed by Iurcu Nicolae
Date: 2026.05.05 10:36:55 EEST
Reason: MoldSign Signature
Location: Moldova
MOLDOVA EUROPEANĂ

OMSONS GERMANY

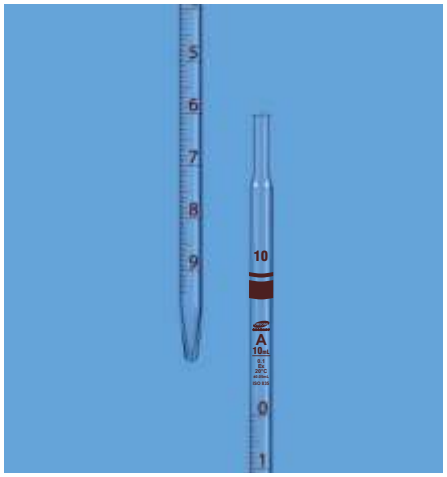

Chemical Resistant | Class A

5803.101

Pipettes, Graduated, Mohr,

Class 'A' with Batch Certificate

- Compliance with DIN ISO 835 standard with colour code.
- Class 'A' with Batch Certificate.
- Printed in Amber colour.
- These pipettes are graduated for delivery from zero mark to the last graduation mark.

BATCH CERTIFICATE

Cat. No.	Capacity (mL)	Graduation (mL)	Tolerance (±mL)	Pack of
5803.101.01	0.1	0.01	0.006	10
5803.101.02	0.2	0.01	0.006	10
5803.101.03	0.5	0.02	0.006	10
5803.101.04	1	0.01	0.007	10
5803.101.05	2	0.02	0.010	10
5803.101.06	5	0.05	0.030	10
5803.101.07	10	0.10	0.050	10
5803.101.08	25	0.20	0.100	10

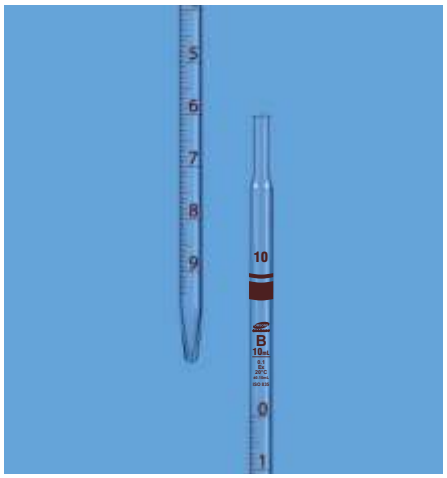

Chemical Resistant | Class A

5803.102

NEW ARRIVAL

Pipettes, Graduated, Mohr,

Class 'B'

- Compliance with DIN ISO 835 standard with colour code.
- Accuracy as per Class 'B'.
- Printed in Amber colour.
- These pipettes are graduated for delivery from zero mark to the last graduation mark.

BATCH CERTIFICATE

Cat. No.	Capacity (mL)	Graduation (mL)	Tolerance (±mL)	Pack of
5803.102.01	0.1	0.01	0.01	10
5803.102.02	0.2	0.01	0.01	10
5803.102.03	0.5	0.02	0.02	10
5803.102.04	1	0.01	0.01	10
5803.102.05	2	0.02	0.02	10
5803.102.06	5	0.05	0.05	10
5803.102.07	10	0.10	0.10	10
5803.102.08	25	0.20	0.20	10

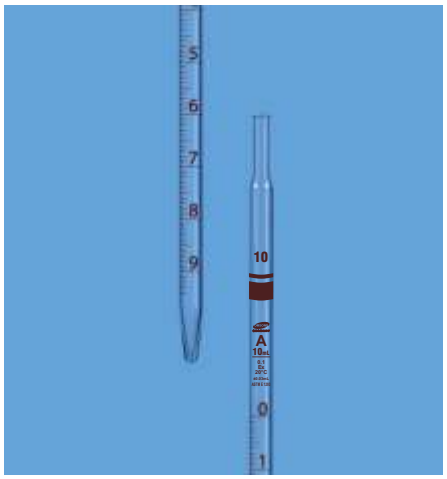

Chemical Resistant | Class A

5803.103

Pipettes, Graduated, Mohr,

ASTM Class 'A'

- Compliance with ASTM E 1293 standard.
- With individual Class 'A' Certificate.
- Printed in Amber colour.
- These pipettes are graduated for delivery from zero mark to the last graduation mark.

INDIVIDUAL CERTIFICATE

Cat. No.	Capacity (mL)	Graduation (mL)	Tolerance (±mL)	Pack of
5803.103.01	1	0.10	0.01	10
5803.103.02	1	0.01	0.01	10
5803.103.03	2	0.02	0.01	10
5803.103.04	5	0.05	0.02	10
5803.103.05	10	0.10	0.03	10
5803.103.06	25	0.20	0.05	10