



奥美医疗
ALLMED MEDICAL

GAUZE ROLL

TECHNICAL PROPERTIES


Content: 100% bleached cotton yarn;

Weft-Warp String number: 40Sx40S/30x30, $\geq 32\text{g/m}^2$;

Width: 90 cm;

Length: Standard length is 90 meters, Other length can be cut as required;

Shelf life: 5 years.



For and on behalf of
ALLMED MEDICAL PRODUCTS CO., LIMITED

Susan Liao

.....
Authorized Signature(s)

Document No.:	Revision No.:	Date of Revision:	Approved by:
WP-011100-AL-02	R-002	2022.10.12	Susan Liao



奥美医疗
ALLMED MEDICAL

Non-Sterile Hydrophilic Gauze Roll

REF Code	Specification	BOX in (Roll)	Box Size (cm)
AM-GR90-90-24A	Non-Sterile Gauze Roll, ≥32g/m ² , width: 90cm, length: 90m	4	49 x 48.5 x 24cm
AM-GR90-90-24A-1	Non-Sterile Gauze Roll, ≥32g/m ² , width: 90cm, length: 1m	195	41*35.5*24cm
AM-GR90-90-24A-2	Non-Sterile Gauze Roll, ≥32g/m ² , width: 90cm, length: 2m	120	44*36.5*24cm
AM-GR90-90-24A-5	Non-Sterile Gauze Roll, ≥32g/m ² , width: 90cm, length: 5m	56	46*40*24cm
AM-GR90-90-24A-10	Non-Sterile Gauze Roll, ≥32g/m ² , width: 90cm, length: 10m	30	48.5*40.5*24cm
AM-GR90-90-24A-20	Non-Sterile Gauze Roll, ≥32g/m ² , width: 90cm, length: 20m	12	46*34.5*24cm
AM-GR90-90-24A-50	Non-Sterile Gauze Roll, ≥32g/m ² , width: 90cm, length: 50m	6	54.5*36.5*24cm
AM-GR90-90-24A-100	Non-Sterile Gauze Roll, ≥32g/m ² , width: 90cm, length: 100m	4	52*51.5*24cm

For and on behalf of
ALLMED MEDICAL PRODUCTS CO., LIMITED

Susan Liao

Authorized Signature(s)

Document No.:	Revision No.:	Date of Revision:	Approved by:
WP-011100-AL-02	R-002	2022.10.12	Susan Liao



Intended use:

This device is intended to be widely used in medical circle and other area for preparing of dressings or tampon with their further fixation on the wound, with protection and barrier function (mechanical) of the injured skin. MD Class I according to Regulation (EU) 2017/745 of the European Parliament and Council.

Product standards: In compliance with EN 14079.

Certificates: CE, ISO13485.

Labeling: in accordance with Chapter III (23) of Annex I of Regulation 2017/745 of the European Commission.

Cautions:

- Read instructions before use.
- Before usage check the packing completeness, the LOT number and expiry date.
- Use only if package is undamaged and validity not expired;
- For single use.
- Destroy after use.

Properties:

- Non-toxic;
- Hypoallergenic;
- Non-inflammable;
- PHT and DEHP free;
- Latex free;
- Durable, hold the dressing securely in place;
- Easy to cut to any shapes and sizes;
- Super softness and patient comfort;
- Highly absorbent;
- Low linting;
- Free from loose wires;
- Non-Sterile unit packages.

For and on behalf of
ALLMED MEDICAL PRODUCTS CO., LIMITED

Susan Liao

Authorized Signature(s)

Document No.:	Revision No.:	Date of Revision:	Approved by:
WP-011100-AL-02	R-002	2022.10.12	Susan Liao



奥美医疗
ALLMED MEDICAL

Instructions for use:

1. Examine individual package of a roll for integrity of packaging prior to use. Do not use if packaging is broken.
2. Wash hands. (Wear gloves where necessary).
3. Before usage, open the roll package.
4. Cut the appropriate Gauze Material size for your procedure.
5. Apply the bandage in accordance with your facility's protocol.
6. Support the injured area while bandaging (if necessary).
7. Immediately dispose of after single use.

Packing:

- each gauze roll is individually packed
- then is packed in strong export carton

Storage:

Protect from sunlight, extreme humidity and heat sources. Not store with organic or chemical solvents. Not store with corrosive gases. Store in dry, cool, good ventilated and clean room, where temperatures between 10°C and 40°C and relative humidity between 30% and 60% are recommended. Once the package is opened, store the remaining roll isolated in clean environment in compliance with conditions mentioned above.



ALLMED MEDICAL PRODUCTS CO.,LTD.

Address: No.18 Qi Xing Road, Majiadian Town, 443200 Zhijiang City, Hubei Province, P.R.C

For and on behalf of
ALLMED MEDICAL PRODUCTS CO., LIMITED

Susan Liao

Authorized Signature(s)

Document No.:	Revision No.:	Date of Revision:	Approved by:
WP-011100-AL-02	R-002	2022.10.12	Susan Liao



奥美医疗
ALLMED MEDICAL

GAUZE BANDAGE

TECHNICAL PROPERTIES


Content: 100% bleached cotton yarn;
 Weft-Warp String number: 40Sx40S/30x30, ≥32g/m2;
 Width: 10cm, 14cm, other sizes available;
 Length: 5m, 7m, Other length can be cut as required;
 Shelf life: 5 years

For and on behalf of
 ALLMED MEDICAL PRODUCTS CO., LIMITED

Non-Sterile Hydrophilic Gauze Bandage

Susan Liao
 Authorized Signature(s)

REF Code	SIZE	BOX in (Roll)	Box Size (cm)
AM-GB10500	10cm x 5m	540	45 x 36.5 x 38 cm
AM-GB14700	14cm x 7m	360	51 x 48.5 x 31 cm



Document No.:	Revision No.:	Date of Revision:	Approved by:
WP-011100-AL-03	R-002	2022.10.12	Susan Liao



奥美医疗
ALLMED MEDICAL

Intended use:

This device is intended to be used for fixation of dressings or tampon on the wound, with protection and barrier function (mechanical) of the injured skin. It provides mild compression and support. MD Class I according to Regulation (EU) 2017/745 of the European Parliament and Council.

Product standards: In compliance with EN 14079.

Certificates: CE, ISO13485.

Labeling: in accordance with Chapter III (23) of Annex I of Regulation 2017/745 of the European Commission.

Cautions:

- Read instructions before use.
- Before usage check the packing completeness, the LOT number and expiry date.
- Use only if package is undamaged and validity not expired;
- For single use.
- Destroy after use.

Properties:

- Non-toxic;
- Hypoallergenic;
- Non-inflammable;
- PHT and DEHP free;
- Latex free;
- Soft and comfortable;
- Low linting;
- High absorbance capacity;
- Easy to cut;
- Free from loose wires;
- Non-Sterile unit packages.

For and on behalf of
ALLMED MEDICAL PRODUCTS CO., LIMITED

Susan Liao
Authorized Signature(s)

Document No.:	Revision No.:	Date of Revision:	Approved by:
WP-011100-AL-03	R-002	2022.10.12	Susan Liao



奥美医疗
ALLMED MEDICAL

Instructions for use:

1. Select the appropriate Gauze Bandage size for your procedure.
2. Examine individual package for integrity of packaging prior to use. Do not use if packaging is broken.
3. Wash hands. (Wear gloves where necessary).
4. Before usage, open the unit package.
5. Apply the bandage in accordance with your facility's protocol.
6. Support the injured area while bandaging (if necessary).
7. Immediately dispose of after single use.

Packing:

- each bandage is rolled and individually packed
- then is packed in strong export carton

Storage:

Protect from sunlight, extreme humidity and heat sources. Not store with organic or chemical solvents. Not store with corrosive gases. Store in dry, cool, good ventilated and clean room, where temperatures between 10°C and 40°C and relative humidity between 30% and 60% are recommended



ALLMED MEDICAL PRODUCTS CO.,LTD.

Address: No.18 Qi Xing Road, Majiadian Town, 443200 Zhijiang City, Hubei Province, P.R.C

For and on behalf of
ALLMED MEDICAL PRODUCTS CO., LIMITED

Susan Liao
.....
Authorized Signature(s)

Document No.:	Revision No.:	Date of Revision:	Approved by:
WP-011100-AL-03	R-002	2022.10.12	Susan Liao



STERILE GAUZE BANDAGE

TECHNICAL PROPERTIES

Content: 100% bleached cotton yarn;
 Weft-Warp String number: 40Sx40S/30x30, ≥32g/m²;
 Width: 10cm, 14cm, other sizes available;
 Length: 5m, 7m, Other length can be cut as required;
 Shelf life: 5 years


For and on behalf of
 ALLMED MEDICAL PRODUCTS CO., LIMITED

Sterile Hydrophilic Gauze Bandage

Susan Liao

Authorized Signature(s)

REF Code	SIZE	BOX in (Roll)	Box Size (cm)
AM-GB10500-S	10cm x 5m	540	45 x 36.5 x 38 cm
AM-GB14700-S	14cm x 7m	360	51 x 48.5 x 31 cm



Document No.:	Revision No.:	Date of Revision:	Approved by:
WP-011100-AL-01	R-002	2022.10.12	Susan Liao



奥美医疗
ALLMED MEDICAL

Intended use:

This device is intended to be used for fixation of dressings or tampon on the wound, with protection and barrier function (mechanical) of the injured skin. It provides mild compression and support. MD Class I-sterile according to Directive (EU) 93/42/ EEC (DL145/2009).

Product standards: In compliance with EN 14079; EN ISO 11737-2.

Certificates: CE, ISO13485.

Labeling: in accordance with according to Directive (EU) 93/42/ EEC (DL145/2009).

Cautions:

- Read instructions before use.
- Before usage check the sterility validity, packing completeness, the LOT number and expiry date.
- Use only if package is undamaged and validity not expired.
- For single use. The re-sterilization is prohibited.
- Destroy after use.

Properties:

- Non-toxic;
- Hypoallergenic;
- Non-inflammable;
- PHT and DEHP free;
- Latex free;
- Soft and comfortable;
- Low linting;
- High absorbance capacity;
- Easy to cut;
- Free from loose wires;
- Sterile unit packages.

For and on behalf of
ALLMED MEDICAL PRODUCTS CO., LIMITED

Susan Liao

.....
Authorized Signature(s)

Document No.:	Revision No.:	Date of Revision:	Approved by:
WP-011100-AL-01	R-002	2022.10.12	Susan Liao



奥美医疗
ALLMED MEDICAL

Instructions for use:

1. Select the appropriate Gauze Bandage size for your procedure.
2. Examine individual package for integrity of packaging prior to use. Do not use if packaging is broken.
3. Wash hands. (Wear gloves where necessary).
4. Before usage, open aseptically the unit package.
5. Apply the bandage aseptically in accordance with your facility's protocol.
6. Support the injured area while bandaging (if necessary).
7. Immediately dispose of after single use.

Packing:

- each bandage is rolled and individually packed
- then is packed in strong export carton

Storage:

Protect from sunlight, extreme humidity and heat sources. Not store with organic or chemical solvents. Not store with corrosive gases. Store in dry, cool, good ventilated and clean room, where temperatures between 10°C and 40°C and relative humidity between 30% and 60% are recommended



ALLMED MEDICAL PRODUCTS CO.,LTD.

Address: No.18 Qi Xing Road, Majiadian Town, 443200 Zhijiang City, Hubei Province, P.R.C


For and on behalf of
ALLMED MEDICAL PRODUCTS CO., LIMITED


Susan Liao

.....
Authorized Signature(s)

Document No.:	Revision No.:	Date of Revision:	Approved by:
WP-011100-AL-01	R-002	2022.10.12	Susan Liao

84x140mm Pantone green



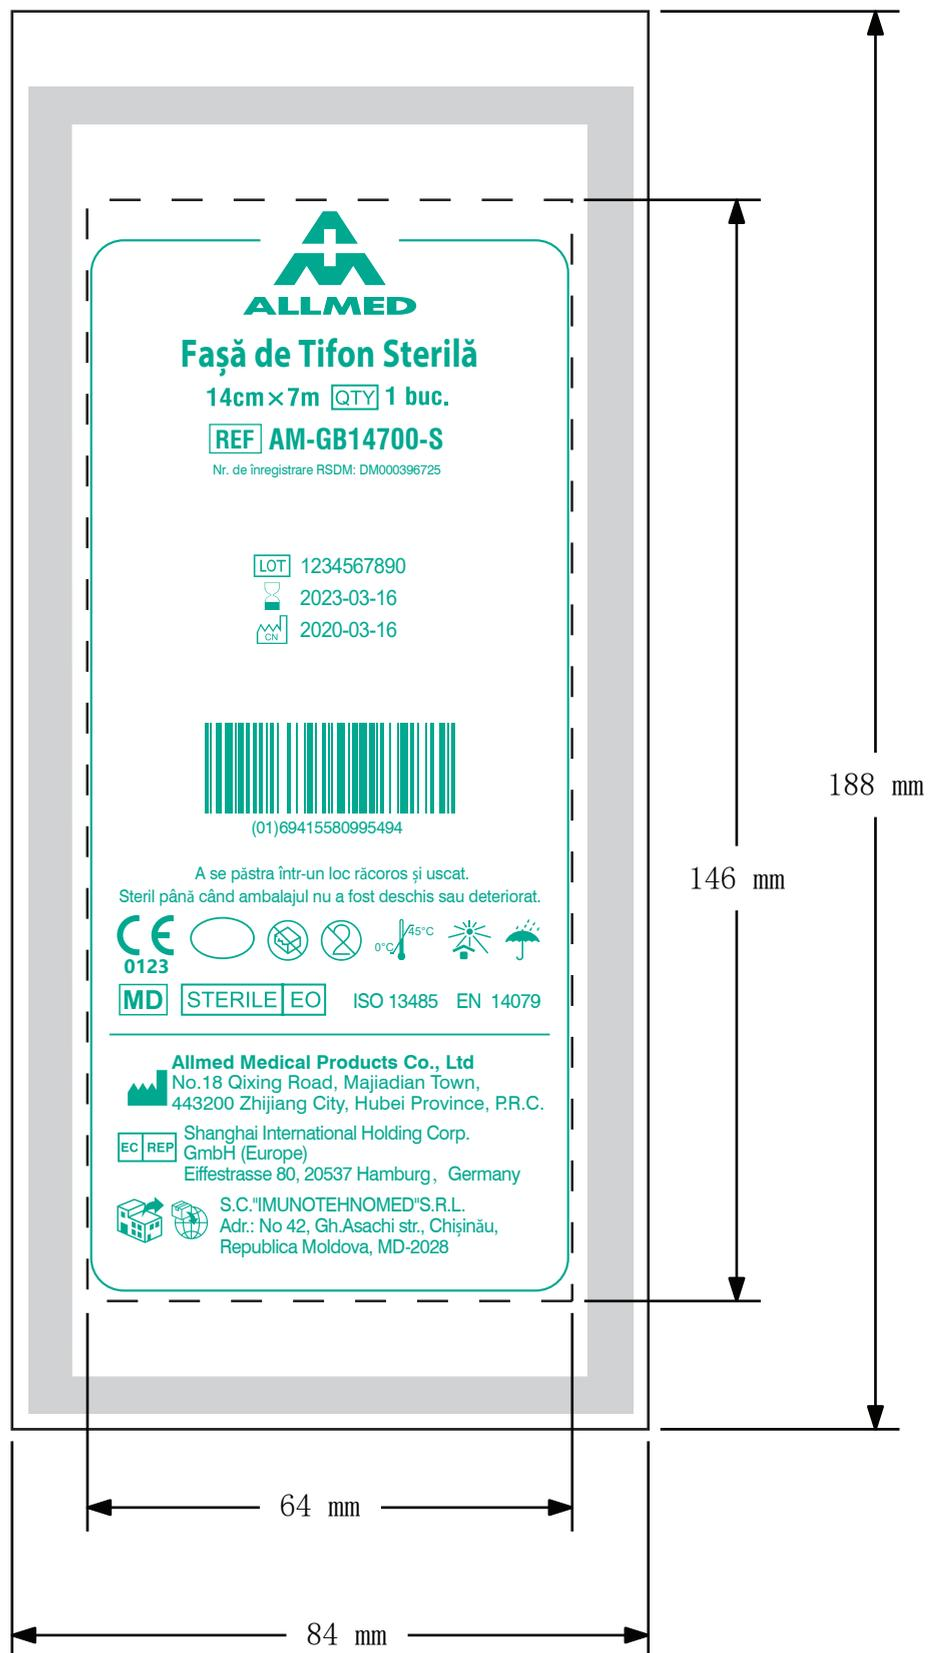

370x285x260mm
black



Fașă de Tifon Sterilă
10cm × 5m **QTY** 150 buc.

Allmed Medical Products Co., Ltd
No.18 Qixing Road, Majiadian Town,
443200 Zhijiang City, Hubei Province, P.R.C.

EC REP Shanghai International Holding Corp. GmbH (Europe)
Eiffelstrasse 80, 20537 Hamburg, Germany
S.C. "IMUNOTEHNOMED" S.R.L.
Adr.: No 42, Gh.Asachi str., Chișinău, Republica Moldova, MD-2028

REF AM-GB10500-S

LOT



(01)69415580995302

Nr. de înregistrare RSDM: DM000396724

A se păstra într-un loc răcoros și uscat.

ISO 13485 EN 14079



Fașă de Tifon Sterilă
10cm × 5m **QTY** 150 buc.

Allmed Medical Products Co., Ltd
No.18 Qixing Road, Majiadian Town,
443200 Zhijiang City, Hubei Province, P.R.C.

EC REP Shanghai International Holding Corp. GmbH (Europe)
Eiffelstrasse 80, 20537 Hamburg, Germany
S.C. "IMUNOTEHNOMED" S.R.L.
Adr.: No 42, Gh.Asachi str., Chișinău, Republica Moldova, MD-2028

REF AM-GB10500-S



(01)69415580995302

Nr. de înregistrare RSDM: DM000396724

A se păstra într-un loc răcoros și uscat.

ISO 13485 EN 14079



330x310x310mm
black



Fașă de Tifon Sterilă
14cm × 7m **QTY** 100 buc.

Allmed Medical Products Co., Ltd
No.18 Qixing Road, Majiadian Town,
443200 Zhijiang City, Hubei Province, P.R.C.

EC REP Shanghai International Holding Corp. GmbH (Europe)
Eiffelstrasse 80, 20537 Hamburg, Germany
S.C. "IMUNOTEHNOMED" S.R.L.
Adr.: No 42, Gh.Asachi str., Chișinău, Republica Moldova, MD-2028

REF AM-GB14700-S

LOT



(01)69415580995470

Nr. de înregistrare RSDM: DM000396725

A se păstra într-un loc răcoros și uscat.

ISO 13485 EN 14079



Fașă de Tifon Sterilă
14cm × 7m **QTY** 100 buc.

Allmed Medical Products Co., Ltd
No.18 Qixing Road, Majiadian Town,
443200 Zhijiang City, Hubei Province, P.R.C.

EC REP Shanghai International Holding Corp. GmbH (Europe)
Eiffelstrasse 80, 20537 Hamburg, Germany
S.C. "IMUNOTEHNOMED" S.R.L.
Adr.: No 42, Gh.Asachi str., Chișinău, Republica Moldova, MD-2028

REF AM-GB14700-S



(01)69415580995470

Nr. de înregistrare RSDM: DM000396725

A se păstra într-un loc răcoros și uscat.

ISO 13485 EN 14079



非消毒包装产品PE袋版面工艺

版面编号	客户号	产品号	PE袋尺寸	印刷颜色	修订日期	批准	审核	拟定	受控状态
11100-BPE-AM-GB14700-V01	11100	AM-GB14700	145x220mm	Pantone green	2023-04-07	廖淑霞	滕晓艳	滕晓艳	

100x100mm,pantone green



文件历史记录:

修改日期	修订内容
2023-2-3	新文件 (ZAM(1)-ECN-11100-2302033)
2023-04-07	改枕式包 (ZAM(1)-ECN-P-2304012)

注: 条形码需正确可读

非消毒包装产品PE袋版面工艺

版面编号	客户号	产品号	PE袋尺寸	印刷颜色	修订日期	批准	审核	拟定	受控状态
11100-BPE-AM-GB14700-V01	11100	AM-GB14700	145x220mm	Pantone green	2023-04-07	廖淑霞	滕晓艳	滕晓艳	

40x100mm,pantone green



文件历史记录:


- 修改日期 修订内容
- 2023-2-3 新文件 (ZAM(1)-ECN-11100-2302033)
- 2023-04-07 改枕式包 (ZAM(1)-ECN-P-2304012)

注: 条形码需正确可读

非消毒包装产品PE袋版面工艺

版面编号	客户号	产品号	PE袋尺寸	印刷颜色	修订日期	批准	审核	拟定	受控状态
11100-BPE-AM-GB14700-V01	11100	AM-GB14700	145x220mm	Pantone green	2023-04-07	廖淑霞	滕晓艳	滕晓艳	

100x100mm,pantone green



文件历史记录:

修改日期	修订内容
2023-2-3	新文件 (ZAM(1)-ECN-11100-2302033)
2023-04-07	改枕式包 (ZAM(1)-ECN-P-2304012)

注: 条形码需正确可读

非消毒包装产品PE袋版面工艺

版面编号	客户号	产品号	PE袋尺寸	印刷颜色	修订日期	批准	审核	拟定	受控状态
11100-BPE-AM-GB14700-V01	11100	AM-GB14700	145x220mm	Pantone green	2023-04-07	廖淑霞	滕晓艳	滕晓艳	

100x100mm,pantone green



文件历史记录:

修改日期	修订内容
2023-2-3	新文件 (ZAM(1)-ECN-11100-2302033)
2023-04-07	改枕式包 (ZAM(1)-ECN-P-2304012)

注: 条形码需正确可读

非消毒包装产品PE袋版面工艺

版面编号	客户号	产品号	PE袋尺寸	印刷颜色	修订日期	批准	审核	拟定	受控状态
11100-BPE-AM-GB14700-V01	11100	AM-GB14700	145x220mm	Pantone green	2023-04-07	廖淑霞	滕晓艳	滕晓艳	

50x100mm,pantone green



文件历史记录:

修改日期 修订内容
 2023-2-3 新文件 (ZAM(1)-ECN-11100-2302033)
 2023-04-07 改枕式包 (ZAM(1)-ECN-P-2304012)

注: 条形码需正确可读

非消毒包装产品PE袋版面工艺

版面编号	客户号	产品号	PE袋尺寸	印刷颜色	修订日期	批准	审核	拟定	受控状态
11100-BPE-AM-GB14700-V01	11100	AM-GB14700	145x220mm	Pantone green	2023-04-07	廖淑霞	滕晓艳	滕晓艳	

100x100mm,pantone green



ALLMED
Tifon Medical

90cm x 20m QTY 1 buc

REF AM-GR90-90-24A-20



(01)06941558083128
A se păstra într-un loc răcoros și uscat.

LOT 2023002

 2028-08

 2023-08











Allmed Medical Products Co., Ltd
No.18 Qixing Road, Majiadian Town,
443200 Zhijiang City, Hubei Province, P.R.C.

 Shanghai International Holding Corp.GmbH (Europe)
Eiffestrasse 80, 20537 Hamburg, Germany

S.C.'IMUNOTEHNOMED'S.R.L.
Adr: No 42, Gh.Asachi str., Chişinău,
Republica Moldova, MD-2028

文件历史记录:

修改日期	修订内容
2023-2-3	新文件 (ZAM(1)-ECN-11100-2302033)
2023-04-07	改枕式包 (ZAM(1)-ECN-P-2304012)

注: 条形码需正确可读

非消毒包装产品PE袋版面工艺

版面编号	客户号	产品号	PE袋尺寸	印刷颜色	修订日期	批准	审核	拟定	受控状态
11100-BPE-AM-GB14700-V01	11100	AM-GB14700	145x220mm	Pantone green	2023-04-07	廖淑霞	滕晓艳	滕晓艳	

80x100mm,pantone green



文件历史记录:


修改日期 修订内容
 2023-2-3 新文件 (ZAM(1)-ECN-11100-2302033)
 2023-04-07 改枕式包 (ZAM(1)-ECN-P-2304012)

注: 条形码需正确可读

非消毒包装产品PE袋版面工艺

版面编号	客户号	产品号	PE袋尺寸	印刷颜色	修订日期	批准	审核	拟定	受控状态
11100-BPE-AM-GB14700-V01	11100	AM-GB14700	145x220mm	Pantone green	2023-04-07	廖淑霞	滕晓艳	滕晓艳	

100x100mm,pantone green



文件历史记录:

修改日期	修订内容
2023-2-3	新文件 (ZAM(1)-ECN-11100-2302033)
2023-04-07	改枕式包 (ZAM(1)-ECN-P-2304012)

注: 条形码需正确可读

Pouch dimensions: 55x155mm
color: Pantone Green



ALLMED
Fasă de Tifon
10cm×5m QTY 1 buc.
REF AM-GB10500


(01)06941558099518
A se păstra într-un loc răcoros și uscat.

    ISO 13485
EN 14079

Allmed Medical Products Co., Ltd
No.18 Qixing Road, Majiadian Town,
443200 Zhijiang City, Hubei Province, P.R.C.

 Shanghai International Holding Corp.
GmbH (Europe)
Eiffelstrasse 90, 20537 Hamburg, Germany

 S.C. 1MUNOTEHNOMED S.R.L.
Adr.: No 42, Gh.Asachi str., Chişinău,
Republica Moldova, MD-2028





非消毒包装产品PE袋版面工艺

Pouch dimensions: 60x200mm
color: Pantone Green

版面编号	客户号	产品号	PE袋尺寸	印刷颜色	修订日期	批准	审核	拟定	受控状态
11100-BPE-AM-GB14700-V00	11100	AM-GB14700	60 X 200mm	Pantone green	2023/2/3	廖淑霞	滕晓艳	滕晓艳	



文件历史记录:

修改日期 修订内容
2023-2-3 新文件 (ZAM(1)-ECN-11100-2302033)
注: 条形码需正确可读

label dimensions: 80x80mm
color: Pantone Green



Fasă de Tifon

10cm×5m QTY 20 buc.

REF AM-GB10500

LOT



(01)16941558099515

A se păstra într-un loc răcoros și uscat.



ISO 13485
EN 14079



Allmed Medical Products Co., Ltd

No.18 Qixing Road, Majiadian Town,
443200 Zhijiang City, Hubei Province, P.R.C.

EC REP

Shanghai International Holding Corp. GmbH (Europe)
Eiffelstrasse 80, 20537 Hamburg , Germany



S.C."IMUNOTEHNOMED" S.R.L.

Adr.: No 42, Gh.Asachi str., Chișinău, Republica Moldova, MD-2028

label dimensions: 80x80mm
color: Pantone Green



Fasă de Tifon
14cm×7m QTY 20 buc.
REF AM-GB14700

LOT





(01)16941558099522

A se păstra într-un loc răcoros și uscat.

ISO 13485
EN 14079



Allmed Medical Products Co., Ltd
No.18 Qixing Road, Majiadian Town,
443200 Zhijiang City, Hubei Province, P.R.C.

EC REP Shanghai International Holding Corp. GmbH (Europe)
Eiffelstrasse 80, 20537 Hamburg, Germany



S.C."IMUNOTEHNOMED" S.R.L.
Adr.: No 42, Gh.Asachi str., Chişinău, Republica Moldova, MD-2028

500×350×320mm
black



Fasă de Tifon

10cm × 5m **QTY** 540 buc.

Allmed Medical Products Co., Ltd
No.18 Qixing Road, Majiadian Town,
443200 Zhijiang City, Hubei Province, P.R.C.




Shanghai International Holding Corp. GmbH (Europe)
Eiffestrasse 80, 20537 Hamburg, Germany



S.C. "IMUNOTEHNOMED" S.R.L.
Adr.: No 42, Gh.Asachi str., Chişinău, Republica Moldova, MD-2028

REF AM-GB10500

LOT



(01)36941558099519

A se păstra într-un loc răcoros și uscat.



ISO 13485 EN 14079



Fasă de Tifon

10cm × 5m **QTY** 540 buc.

Allmed Medical Products Co., Ltd
No.18 Qixing Road, Majiadian Town,
443200 Zhijiang City, Hubei Province, P.R.C.



Shanghai International Holding Corp. GmbH (Europe)
Eiffestrasse 80, 20537 Hamburg, Germany



S.C. "IMUNOTEHNOMED" S.R.L.
Adr.: No 42, Gh.Asachi str., Chişinău, Republica Moldova, MD-2028

REF AM-GB10500



(01)36941558099519

A se păstra într-un loc răcoros și uscat.



ISO 13485 EN 14079

575×320×380mm

black



Fasă de Tifon

14cm × 7m **QTY** 360 buc.

Allmed Medical Products Co., Ltd
No.18 Qixing Road, Majiadian Town,
443200 Zhijiang City, Hubei Province, P.R.C.



Shanghai International Holding Corp. GmbH (Europe)
Eiffestrasse 80, 20537 Hamburg, Germany



S.C."IMUNOTEHNOMED"S.R.L.
Adr.: No 42, Gh.Asachi str., Chişinău, Republica Moldova, MD-2028

REF AM-GB14700

LOT



(01)36941558099526

A se păstra într-un loc răcoros și uscat.

ISO 13485 EN 14079



Fasă de Tifon

14cm × 7m **QTY** 360 buc.

Allmed Medical Products Co., Ltd
No.18 Qixing Road, Majiadian Town,
443200 Zhijiang City, Hubei Province, P.R.C.



Shanghai International Holding Corp. GmbH (Europe)
Eiffestrasse 80, 20537 Hamburg, Germany



S.C."IMUNOTEHNOMED"S.R.L.
Adr.: No 42, Gh.Asachi str., Chişinău, Republica Moldova, MD-2028

REF AM-GB14700



(01)36941558099526

A se păstra într-un loc răcoros și uscat.

ISO 13485 EN 14079





ALLMED MEDICAL PRODUCTS CO.,LTD

No.18 Qixing Road, Majiadian Town,443200

Zhijiang City, Hubei province, (China)

Quality Report (Absorbent Cotton Gauze)

Report No: 2306001

Report Date: 2023.06.02

制 造 商 Manufacturer	ALLMED MEDICAL PRODUCTS CO.,LTD	产 品 号 Reference No.	AM-GB10500-S/AM-GB14700-S
规 格 Specification	40s×40s/30×30 Gauze	订 单 号 PO#	2023002
检 验 数 量 Inspection Quantity	5m	检 测 时 间 Inspection Date	2023.04.11
特 征 Characteristic	EN14079 要求 REQUIREMENT OF EN14079	结 果 RESULT	判 定 Complies (Yes or No)
纤维鉴别 Fibre Identification	符合 IDENT 试验 A、B、C 项 Shall conform to the IDENT tests A, B and C	A、纤维呈扁平带状。端部增粗且有内腔。 Fibre consists of single cell, in the form of flattened tube with thick and rounded walls and often twisted. B、纤维显紫色。 Fibre becomes violet with iodinated zinc chloride solution. C、纤维未溶解。 Fibre does not dissolve	Yes
酸碱度 Acidity and alkalinity	两种溶液均不得显粉红色 No pink colour develops in either portion	未显粉红色 No pink colour develops in either portion	Yes
外来纤维 Foreign fibres	只允许出现少量孤立的外来纤维 Only occasionally a few isolated foreign fibres allowed	未见外来纤维 No isolated foreign fibres	Yes
荧光 Fluorescence	不允许显示深蓝色纤维 No intense blue fluorescence shall be displayed	未见深蓝色纤维 No intense blue fluorescence displayed	Yes
经密 Warp	120±6th/100mm	116 th/100mm	Yes
纬密 Weft	120±6th/100mm	115 th/100mm	Yes
平方米克重 Mass per square metre	≥ 32.0 g/m ²	32.25 g/m ²	Yes
最小断裂强度 Minimum breaking load	MD: ≥60N CD: ≥50N	MD:109.0N; CD:89.5N	Yes
吸水时间 Sinking time	≤10 s	1.21s	Yes
醚中可溶物 Ether-soluble substances	≤0.5%	0.29%	Yes
表面活性物 Surface active substances	≤2mm	1.0mm	Yes
水中可溶物 Water-soluble substances	≤0.5%	0.20%	Yes
淀粉和糊精 Starch and dextrin	不得显示蓝、紫、微红或褐色 Shall not show any blue, violet, reddish or brownish colour	未显蓝、紫、微红或褐色 No blue, violet, reddish or brownish colour develops	Yes
可浸提的着色物质 Extractable colouring matter	不超过参考溶液 Y5 或 GY6 Shall not be more intensely coloured than reference solution Y5, GY6	颜色未超过溶液 Y5 Colour is less intense than reference solution Y5	Yes
干燥失重 Loss on drying	≤ 8.0%	4.02%	Yes
硫酸盐灰份 Sulphated ash	≤ 0.40%	0.13%	Yes
结 论 Conclusion	Complies with EN14079		

审核 (Reviewed): You Dequan

准备 (Prepared By): Zheng Qiong



ALLMED MEDICAL PRODUCTS CO.,LTD

No.18 Qixing Road, Majiadian Town,443200

Zhijiang City, Hubei province, (China)

Absorbent Gauze Quality Report 纱布质量报告

报告编号 Report No: 2401001

报告日期:Report Date: 2024.02.03

制造商 Manufacturer	ALLMED MEDICAL PRODUCTS CO.,LTD	产品号 Reference No.	AM-GR90-90-24A/AM-GR90-90-24A-50 AM-GR90-90-24A-5/AM-GR90-90-24A-10 AM-GR90-90-24A-20
规格 Specification	40*×40*/30×30	订单号 PO#	20231201
检验数量 Inspection Quantity	5m	灭菌状态 Sterilization Status	<input type="checkbox"/> Sterile 已灭菌 <input checked="" type="checkbox"/> Non-Sterile 未灭菌
检测日期 Inspection Date	2024.01.30	灭菌方式 Sterilization Methods	<input type="checkbox"/> ETO <input type="checkbox"/> Steam <input type="checkbox"/> Gamma
特征 Characteristic	EN14079 要求 REQUIREMENT OF EN14079	结果 RESULT	判定 Complies (Yes or No)
纤维鉴别 Fibre Identification	符合 IDENT 试验 A、B、C 项 Shall conform to the IDENT tests A, B and C	Complies	Yes
酸碱度 Acidity and alkalinity	中性 (两者均不得显粉红色) Neutral(no pink color develops in either portion)	Neutral	Yes
外来纤维 Foreign fibres	只允许出现少量孤立的外来纤维 Only occasionally a few isolated foreign fibres allowed	未见外来纤维 No isolated foreign fibres	Yes
荧光 Fluorescence	只应显微棕紫色荧光和少量黄色颗粒。除少量 孤立的纤维外, 不应显强蓝色荧光。 It shall only display a slight brownish-violet fluorescence and a few yellow particles. With the exception of that shown by a few isolated fibres, no intense blue fluorescence shall be displayed	未见强蓝色荧光 No strong blue fluorescence was observed	Yes
经密 Warp	120±6th/100mm	117 th/100mm	Yes
纬密 Weft	120±6th/100mm	116 th/100mm	Yes
平方米克重 Mass per square metre	≥ 32.0 g/m ²	32.61g/m ²	Yes
最小断裂强度 Minimum breaking load	MD: ≥60N CD: ≥50N	MD:93.8N; CD:79.9N	Yes
吸水时间 Sinking time	≤10 s	1.47S	Yes
醚中可溶物 Ether-soluble substances	≤0.5%	0.31%	Yes
表面活性物 Surface active substances	≤2mm	0mm	Yes
水中可溶物 Water-soluble substances	≤0.5%	0.3%	Yes
淀粉和糊精 Starch and dextrin	不得显示蓝、紫、微红或褐色 Shall not show any blue, violet, reddish or brownish colour	未显蓝、紫、微红或褐色 No blue, violet, reddish or brownish colour develops	Yes
可浸提的着色物质 Extractable colouring matter	滤液的颜色应不深于对照液 Y5 或 GY6 或蓝 色对照溶液 Liquid obtained shall not be more intensely coloured than reference solution Y5,GY6 or blue reference solution	Complies	Yes
干燥失重 Loss on drying	≤ 8.0%	3.03%	Yes
硫酸盐灰份 Sulphated ash	≤ 0.40%	0.16%	Yes
结论 Conclusion	Complies with EN14079		

表格编号 Form#: AMQR-005-007

1 OF 2

执行日期 Effective Date: 2023-01-01

表格批准人 Approved By: 刘宜娇

相关文件号 Relevant documen#: SIP-I-004



ALLMED MEDICAL PRODUCTS CO.,LTD

**No.18 Qixing Road, Majiadian Town,443200
Zhijiang City, Hubei province, (China)**

* Inspection sampling procedure in accordance with ISO 2859.

审核人 (Reviewed): YouDequan

准备人 (Prepared By): ZhengXiaoting