

HEV IgG

**Third generation Enzyme Immunoassay
for the determination of IgG antibodies
to Hepatitis E Virus
in human serum and plasma**

- for “in vitro” diagnostic use only -



DIA.PRO

**Diagnostic Bioprobes Srl
Via G. Carducci n° 27
20099 Sesto San Giovanni
(Milano) - Italy**

Phone +39 02 27007161

Fax +39 02 44386771

e-mail: info@diapro.it

REF EVG.CE
96 Tests

HEV IgG

A. INTENDED USE

Third generation Enzyme ImmunoAssay (ELISA) for the qualitative determination of IgG antibodies to Hepatitis E Virus in human plasma and sera.

The kit is intended for the follow-up of HEV-infected patients. For "in vitro" diagnostic use only.

B. INTRODUCTION

Hepatitis E Virus or HEV is a recently discovered agent of enterically transmitted viral hepatitis. HEV is an un-enveloped single-strand RNA virus, after being provisionally assigned to the Caliciviridae family, HEV was re-classified as the sole member of the genus Hepevirus, family Hepeviridae, in 2004. HEV is found in the stool of infected patients and present in 4 strains (1, 2, 3 and 4) differently spread geographically and virulent.

HEV is a serious problem in many developing countries since its first outbreak was reported in 1955 in New Delhi, India.

A high case-fatality rate has been found among pregnant women and chronic hepatitis carriers.

The cloning and sequencing of HEV genome have led to the development of serological tests for the detection of anti HEV antibodies based on recombinant immunodominant antigens derived from conservative regions of the four virus strains.

C. PRINCIPLE OF THE TEST

Microplates are coated with HEV-specific recombinant antigens encoding for conservative and immunodominant determinants of all the 4 subtypes.

The solid phase is first treated with the diluted sample and anti HEV IgG are captured, if present, by the antigens.

After washing out all the other components of the sample, in the 2nd incubation bound anti-HEV IgG are detected by the addition of polyclonal specific anti hlgG antibodies, labelled with peroxidase (HRP).

The enzyme captured on the solid phase, acting on the substrate/chromogen mixture, generates an optical signal that is proportional to the amount of anti HEV IgG present in the sample. A cut-off value let optical densities be interpreted into anti-HEV IgG negative and positive results.

D. COMPONENTS

Code EVG.CE contains reagents for 96 tests.

1. Microplate **MICROPLATE**

n° 1 microplate. 12 strips of 8 microwells coated with HEV specific recombinant antigens. Plates are sealed into a bag with desiccant.

2. Negative Control **CONTROL -**

1x4.0ml/vial. Ready to use control. It contains 1% goat serum proteins, 10 mM Na-citrate buffer pH 6.0 +/-0.1, 0.5% Tween 20, 0.09% Na-azide and 0.045% ProClin 300 as preservatives. The negative control is olive green colour coded.

3. Positive Control **CONTROL +**

1x4.0ml/vial. Ready to use control. It contains 1% goat serum proteins, human antibodies positive to HEV, 10 mM Na-citrate buffer pH 6.0 +/-0.1, 0.5% Tween 20, 0.09% Na-azide and 0.045% ProClin 300 as preservatives. The Positive Control is blue colour coded.

4. Calibrator **CAL ...**

n° 1 vial. Lyophilized calibrator. To be dissolved with the volume of EIA grade water reported on the label.

It contains foetal bovine serum proteins, human antibodies to HEV whose content is calibrated on 1st WHO reference reagent for HEV antibody, NIBSC code 95/584 at 1 IU/ml +/-20%, 10 mM Na-citrate buffer pH 6.0 +/-0.1, 0.3 mg/ml gentamicine sulphate and 0.045% ProClin 300 as preservatives.

Note: The volume necessary to dissolve the content of the vial may vary from lot to lot. Please use the right volume reported on the label.

5. Wash buffer concentrate **WASHBUF 20X**

1x60ml/bottle. 20x concentrated solution. Once diluted, the wash solution contains 10 mM phosphate buffer pH 7.0 +/-0.2, 0.05% Tween 20 and 0.045% ProClin 300.

6. Enzyme Conjugate **CONJ**

1x16ml/vial. Ready to use and red colour coded reagent. It contains Horseradish Peroxidase conjugated goat polyclonal antibodies to human IgG, 5% BSA, 10 mM Tris buffer pH 6.8 +/-0.1, 0.045% ProClin 300 and 0.02% gentamicine sulphate as preservatives.

7. Chromogen/Substrate **SUBS TMB**

1x16ml/vial. Ready-to-use component. It contains 50 mM citrate-phosphate buffer pH 3.5-3.8, 4% dimethylsulphoxide, 0.03% tetra-methyl-benzidine or TMB and 0.02% hydrogen peroxide or H₂O₂.

Note: To be stored protected from light as sensitive to strong illumination.

8. Assay Diluent **DILAS**

1x8ml/vial. 10 mM tris buffered solution pH 8.0 +/-0.1 containing 0.045% ProClin 300 for the pre-treatment of samples and controls in the plate, blocking interference.

9. Sulphuric Acid **H₂SO₄ 0.3 M**

1x15ml/vial. It contains 0.3 M H₂SO₄ solution. Attention: Irritant (H315, H319; P280, P302+P352, P332+P313, P305+P351+P338, P337+P313, P362+P363).

10. Sample Diluent: **DILSPE**

1x50ml/vial. It contains 10 mM Na-citrate buffer pH 6.0 +/-0.1, 0.5% Tween 20, 0.09% Na-azide and 0.045% ProClin 300 as preservatives. To be used to dilute the sample.

Note: The diluent changes colour from olive green to dark bluish green in the presence of sample.

11. Plate sealing foils n° 2

12. Package insert n° 1

E. MATERIALS REQUIRED BUT NOT PROVIDED

1. Calibrated Micropipettes (200ul and 10ul) and disposable plastic tips.
2. EIA grade water (bidistilled or deionised, charcoal treated to remove oxidizing chemicals used as disinfectants).
3. Timer with 60 minute range or higher.
4. Absorbent paper tissues.
5. Calibrated ELISA microplate thermostatic incubator capable to provide a temperature of +37°C.
6. Calibrated ELISA microwell reader with 450nm (reading) and with 620-630nm (blanking) filters.
7. Calibrated ELISA microplate washer.
8. Vortex or similar mixing tools.

F. WARNINGS AND PRECAUTIONS

1. The kit has to be used by skilled and properly trained technical personnel only, under the supervision of a medical doctor responsible of the laboratory.
2. When the kit is used for the screening of blood units and blood components, it has to be used in a laboratory certified and

qualified by the national authority in that field (Ministry of Health or similar entity) to carry out this type of analysis.

3. All the personnel involved in performing the assay have to wear protective laboratory clothes, talc-free gloves and glasses. The use of any sharp (needles) or cutting (blades) devices should be avoided. All the personnel involved should be trained in biosafety procedures, as recommended by the Center for Disease Control, Atlanta, U.S. and reported in the National Institute of Health's publication: "Biosafety in Microbiological and Biomedical Laboratories", ed. 1984.

4. All the personnel involved in sample handling should be vaccinated for HBV and HAV, for which vaccines are available, safe and effective.

5. The laboratory environment should be controlled so as to avoid contaminants such as dust or air-borne microbial agents, when opening kit vials and microplates and when performing the test. Protect the Chromogen/Substrate from strong light and avoid vibration of the bench surface where the test is undertaken.

6. Upon receipt, store the kit at +2..8°C into a temperature controlled refrigerator or cold room.

7. Do not interchange components between different lots of the kits. It is recommended that components between two kits of the same lot should not be interchanged.

8. Check that the reagents are clear and do not contain visible heavy particles or aggregates. If not, advise the laboratory supervisor to initiate the necessary procedures for kit replacement.

9. Avoid cross-contamination between serum/plasma samples by using disposable tips and changing them after each sample. Do not reuse disposable tips.

10. Avoid cross-contamination between kit reagents by using disposable tips and changing them between the use of each one. Do not reuse disposable tips.

11. Do not use the kit after the expiration date stated on the external container and internal (vials) labels.

12. Treat all specimens as potentially infective. All human serum specimens should be handled at Biosafety Level 2, as recommended by the Center for Disease Control, Atlanta, U.S. in compliance with what reported in the Institutes of Health's publication: "Biosafety in Microbiological and Biomedical Laboratories", ed. 1984.

13. The use of disposable plastic-ware is recommended in the preparation of the liquid components or in transferring components into automated workstations, in order to avoid cross contamination.

14. Waste produced during the use of the kit has to be discarded in compliance with national directives and laws concerning laboratory waste of chemical and biological substances. In particular, liquid waste generated from the washing procedure, from residuals of controls and from samples has to be treated as potentially infective material and inactivated before waste. Suggested procedures of inactivation are treatment with a 10% final concentration of household bleach for 16-18 hrs or heat inactivation by autoclave at 121°C for 20 min..

15. Accidental spills from samples and operations have to be adsorbed with paper tissues soaked with household bleach and then with water. Tissues should then be discarded in proper containers designated for laboratory/hospital waste.

16. The Sulphuric Acid is an irritant. In case of spills, wash the surface with plenty of water

17. Other waste materials generated from the use of the kit (example: tips used for samples and controls, used microplates) should be handled as potentially infective and disposed according to national directives and laws concerning laboratory wastes.

G. SPECIMEN: PREPARATION AND RECOMMANDATIONS

1. Blood is drawn aseptically by venepuncture and plasma or serum is prepared using standard techniques of preparation of samples for clinical laboratory analysis. No influence has been

observed in the preparation of the sample with citrate, EDTA and heparin.

2. Avoid any addition of preservatives to samples; especially sodium azide as this chemical would affect the enzymatic activity of the conjugate, generating false negative results.

3. Samples have to be clearly identified with codes or names in order to avoid misinterpretation of results. When the kit is used for the screening of blood units, bar code labeling and electronic reading is strongly recommended.

4. Haemolysed (red) and visibly hyperlipemic ("milky") samples have to be discarded as they could generate false results. Samples containing residues of fibrin or heavy particles or microbial filaments and bodies should be discarded as they could give rise to false results.

5. Sera and plasma can be stored at +2°...+8°C in primary collection tubes for up to five days after collection.

Do not freeze primary tubes of collection. For longer storage periods, sera and plasma samples, carefully removed from the primary collection tube, can be stored frozen at -20°C for at least 12 months. Any frozen samples should not be frozen/thawed more than once as this may generate particles that could affect the test result.

6. If particles are present, centrifuge at 2.000 rpm for 20 min or filter using 0.2-0.8u filters to clean up the sample for testing.

H. PREPARATION OF COMPONENTS AND WARNINGS

A study conducted on an opened kit has not pointed out any relevant loss of activity up to 6 re-use of the device and up to 6 months.

1. Microplates:

Allow the microplate to reach room temperature (about 1 hr) before opening the container. Check that the desiccant is not turned to dark green, indicating a defect of storing.

In this case call Dia.Pro's customer service.

Unused strips have to be placed back into the aluminium pouch, in presence of desiccant supplied, firmly zipped and stored at +2°..8°C.

When opened the first time, residual strips are stable till the indicator of humidity inside the desiccant bag turns from yellow to green.

2. Negative Control:

Ready to use. Mix well on vortex before use.

3. Positive Control:

Ready to use. Mix well on vortex before use. Handle this component as potentially infective, even if HCV, eventually present in the control, has been chemically inactivated.

4. Calibrator:

Dissolve carefully the content of the lyophilized vial with the volume of EIA grade water reported on its label.

Mix well on vortex before use.

Handle this component as potentially infective, even if HEV, eventually present in the control, has been chemically inactivated.

Note: When dissolved the Calibrator is not stable. Store in aliquots at -20°C.

5. Wash buffer concentrate:

The whole content of the 20x concentrated solution has to be diluted with bidistilled water up to 1200 ml and mixed gently end-over-end before use.

Once diluted, the wash solution is stable for 1 week at +2..8° C.

In the preparation avoid foaming as the presence of bubbles could give origin to a bad washing efficiency.

Note: Once diluted, the wash solution is stable for 1 week at +2..8° C.

6. Enzyme conjugate:

Ready to use. Mix well on vortex before use.

Be careful not to contaminate the liquid with oxidizing chemicals, air-driven dust or microbes.
If this component has to be transferred use only plastic, possibly sterile disposable containers.

7. Chromogen/Substrate:

Ready to use. Mix well on vortex before use.

Be careful not to contaminate the liquid with oxidizing chemicals, air-driven dust or microbes.

Do not expose to strong illumination, oxidizing agents and metallic surfaces.

If this component has to be transferred use only plastic, possible sterile disposable container.

8. Assay Diluent:

Ready to use. Mix well on vortex before use.

9. Sulphuric Acid:

Ready to use. Mix well on vortex before use.

Attention: Irritant (H315, H319; P280, P302+P352, P332+P313, P305+P351+P338, P337+P313, P362+P363).

Legenda:

Warning H statements:

H315 – Causes skin irritation.

H319 – Causes serious eye irritation.

Precautionary P statements:

P280 – Wear protective gloves/protective clothing/eye protection/face protection.

P302 + P352 – IF ON SKIN: Wash with plenty of soap and water.

P332 + P313 – If skin irritation occurs: Get medical advice/attention.

P305 + P351 + P338 – IF IN EYES: Rinse cautiously with water for several minutes. Remove contact lenses, if present and easy to do. Continue rinsing.

P337 + P313 – If eye irritation persists: Get medical advice/attention.

P362 + P363 – Take off contaminated clothing and wash it before reuse.

10. Sample Diluent:

Ready to use. Mix well on vortex before use.

I. INSTRUMENTS AND TOOLS USED IN COMBINATION WITH THE KIT

- 1. Micropipettes** have to be calibrated to deliver the correct volume required by the assay and must be submitted to regular decontamination (household alcohol, 10% solution of bleach, hospital grade disinfectants) of those parts that could accidentally come in contact with the sample. They should also be regularly maintained in order to show a precision of 1% and a trueness of +/-2%. Decontamination of spills or residues of kit components should also be carried out regularly.
- The **ELISA incubator** has to be set at +37°C (tolerance of +/-0.5°C) and regularly checked to ensure the correct temperature is maintained. Both dry incubators and water baths are suitable for the incubations, provided that the instrument is validated for the incubation of ELISA tests.
- The **ELISA washer** is extremely important to the overall performances of the assay. The washer must be carefully validated in advance, checked for the delivery of the right dispensation volume and regularly submitted to maintenance according to the manufacturer's instructions for use. In particular the washer, at the end of the daily workload, has to be extensively cleaned out of salts with deionized water. Before use, the washer has to be extensively primed with the diluted Washing Solution.

The instrument weekly has to be submitted to decontamination according to its manual (NaOH 0.1 M decontamination suggested).

5 washing cycles (aspiration + dispensation of 350ul/well of washing solution + 20 sec soaking = 1 cycle) are sufficient to ensure the assay with the declared performances. If soaking is not possible add one more cycle of washing.

An incorrect washing cycle or salt-blocked needles are the major cause of false positive reactions.

- 4. Incubation times** have a tolerance of $\pm 5\%$.
- The **ELISA reader** has to be equipped with a reading filter of 450nm and with a second filter (620-630nm, mandatory) for blanking purposes. Its standard performances should be (a) bandwidth ≤ 10 nm; (b) absorbance range from 0 to ≥ 2.0 ; (c) linearity to ≥ 2.0 ; repeatability $\geq 1\%$. Blanking is carried out on the well identified in the section "Assay Procedure". The optical system of the reader has to be calibrated regularly to ensure that the correct optical density is measured. It should be regularly maintained according to the manufacturer's instructions.
- When using an **ELISA automated work station**, all critical steps (dispensation, incubation, washing, reading, data handling) have to be carefully set, calibrated, controlled and regularly serviced in order to match the values reported in the sections "Validation of Test" and "Assay Performances". The assay protocol has to be installed in the operating system of the unit and validated as for the washer and the reader. In addition, the liquid handling part of the station (dispensation and washing) has to be validated and correctly set. Particular attention must be paid to avoid carry over by the needles used for dispensing and for washing. This must be studied and controlled to minimize the possibility of contamination of adjacent wells. The use of ELISA automated work stations is recommended for blood screening when the number of samples to be tested exceed 20-30 units per run.
- Dia.Pro's customer service offers support to the user in the setting and checking of instruments used in combination with the kit, in order to assure compliance with the requirements described. Support is also provided for the installation of new instruments to be used with the kit.

L. PRE ASSAY CONTROLS AND OPERATIONS

- Check the expiration date of the kit printed on the external label of the kit box. Do not use if expired.
- Check that the liquid components are not contaminated by naked-eye visible particles or aggregates. Check that the Chromogen/Substrate is colorless or pale blue by aspirating a small volume of it with a sterile transparent plastic pipette. Check that no breakage occurred in transportation and no spillage of liquid is present inside the box. Check that the aluminum pouch, containing the microplate, is not punctured or damaged.
- Dilute all the content of the 20x concentrated Wash Solution as described above.
- Dissolve the Calibrator as described above.
- Allow all the other components to reach room temperature (about 1 hr) and then mix as described.
- Set the ELISA incubator at +37°C and prepare the ELISA washer by priming with the diluted washing solution, according to the manufacturers instructions. Set the right number of washing cycles as reported in the specific section.
- Check that the ELISA reader has been turned on at least 20 minutes before reading.
- If using an automated workstation, turn it on, check settings and be sure to use the right assay protocol.
- Check that the micropipettes are set to the required volume.
- Check that all the other equipment is available and ready to use.
- In case of problems, do not proceed further with the test and advise the supervisor.

M. ASSAY PROCEDURE

The assay has to be carried out according to what reported below, taking care to maintain the same incubation time for all the samples in testing.

Automated assay:

In case the test is carried out automatically with an ELISA workstation, we suggest to make the instrument aspirate 200 ul Sample Diluent and then 10 ul sample.
All the mixture is then carefully dispensed directly into the appropriate sample well of the microplate. Before the next sample is aspirated, needles have to be duly washed to avoid any cross-contamination among samples.
Do not dilute controls/calibrator as they are ready to use.
Dispense 200 ul controls/calibrator in the appropriate control/calibration wells.

Important Note: Visually monitor that samples have been diluted and dispensed into appropriate wells. This is simply achieved by checking that the color of dispensed samples has turned to dark bluish-green while the color of the negative control has remained olive green.

For the next operations follow the operative instructions reported below for the Manual Assay.

It is strongly recommended to check that the time lap between the dispensation of the first and the last sample will be calculated by the instrument and taken into consideration by delaying the first washing operation accordingly.

Manual assay:

- Place the required number of Microwells in the microwell holder. Leave the 1st well empty for the operation of blanking.
- Dispense 200 ul of Negative Control in triplicate, 200 ul Calibrator in duplicate and 200 ul Positive Control in single in proper wells. Do not dilute Controls and Calibrator as they are pre-diluted, ready to use !
- Add 200 ul of Sample Diluent (DILSPE) to all the sample wells; then dispense 10 ul sample in each properly identified well. Mix gently the plate, avoiding overflowing and contaminating adjacent wells, in order to fully disperse the sample into its diluent.

Important note: Check that the color of the Sample Diluent, upon addition of the sample, changes from light green to dark bluish green, monitoring that the sample has been really added.

- Dispense 50 ul Assay Diluent (DILAS) into all the controls/calibrator and sample wells. Check that the color of samples has turned to dark blue.
- Incubate the microplate for **45 min at +37°C**.

Important note: Strips have to be sealed with the adhesive sealing foil, supplied, only when the test is carried out manually. Do not cover strips when using ELISA automatic instruments.

- Wash the microplate with an automatic washer by delivering and aspirating 300ul/well of diluted washing solution as reported previously (section I.3).
- Pipette 100µl Enzyme Conjugate into each well, except the 1st blanking well, and cover with the sealer. Check that this red colored component has been dispensed in all the wells, except A1.

Important note: Be careful not to touch the plastic inner surface of the well with the tip filled with the Enzyme Conjugate. Contamination might occur.

- Incubate the microplate for **45 min at +37°C**.
- Wash microwells as in step 6.

- Pipette 100µl Chromogen/Substrate mixture into each well, the blank well included. Then incubate the microplate at **room temperature (18-24°C) for 15 minutes**.

Important note: Do not expose to strong direct illumination. High background might be generated.

- Pipette 100µl Sulphuric Acid into all the wells using the same pipetting sequence as in step 10 to stop the enzymatic reaction. Addition of acid will turn the positive control and positive samples from blue to yellow.
- Measure the color intensity of the solution in each well, as described in section I.5, at 450nm filter (reading) and at 620-630nm (background subtraction, mandatory), blanking the instrument on A1.

Important notes:

- Ensure that no finger prints are present on the bottom of the microwell before reading. Finger prints could generate false positive results on reading.
- Reading has to be carried out just after the addition of the Stop Solution and anyway not any longer than 20 minutes after its addition. Some self oxidation of the chromogen can occur leading to high background.

N. ASSAY SCHEME

Method	Operations
Controls & Calibrator(*)	200 ul
Samples	200ul dil.+10ul
Assay Diluent (DILAS)	50 ul
1st incubation	45 min
Temperature	+37°C
Wash step	n° 5 cycles with 20" of soaking OR n° 6 cycles without soaking
Enzyme conjugate	100 ul
2nd incubation	45 min
Temperature	+37°C
Wash step	n° 5 cycles with 20" of soaking OR n° 6 cycles without soaking
TMB/H2O2	100 ul
3rd incubation	15 min
Temperature	r.t.
Sulphuric Acid	100 ul
Reading OD	450nm/620-630nm

(*) Important Notes:

- The Calibrator (CAL) does not affect the Cut Off calculation, therefore it does not affect the test's results calculation.
- The Calibrator (CAL) used only if a laboratory internal quality control is required by the Management.

An example of dispensation scheme is reported below:

Microplate												
	1	2	3	4	5	6	7	8	9	10	11	12
A	BLK	S2										
B	NC	S3										
C	NC	S4										
D	NC	S5										
E	CAL(*)	S6										
F	CAL(*)	S7										
G	PC	S8										
H	S1	S9										

Legenda: BLK = Blank NC = Negative Control
CAL(*) = Calibrator - Not mandatory PC = Positive Control
S = Sample

O. INTERNAL QUALITY CONTROL

A check is carried out on the controls any time the kit is used in order to verify whether their OD450nm/620-630nm values are as expected and reported in the table below.

Check	Requirements
Blank well	< 0.100 OD450nm value
Negative Control (NC)	< 0.050 mean OD450nm value after blanking
Positive Control	> 1.000 OD450nm value

If the results of the test match the requirements stated above, proceed to the next section.

If they do not, do not proceed any further and operate as follows:

Problem	Check
Blank well > 0.100 OD450nm	1. that the Chromogen/Substrate solution has not got contaminated during the assay
Negative Control (NC) > 0.050 OD450nm after blanking	1. that the washing procedure and the washer settings are as validated in the pre qualification study; 2. that the proper washing solution has been used and the washer has been primed with it before use; 3. that no mistake has been done in the assay procedure (dispensation of positive control instead of negative control); 4. that no contamination of the negative control or of their wells has occurred due to positive samples, to spills or to the enzyme conjugate; 5. that micropipettes haven't got contaminated with positive samples or with the enzyme conjugate 6. that the washer needles are not blocked or partially obstructed.
Positive Control < 1.000 OD450nm	1. that the procedure has been correctly executed; 2. that no mistake has been done in the distribution of controls (dispensation of negative control instead of positive control. In this case, the negative control will have an OD450nm value > 0.150, too. 3. that the washing procedure and the washer settings are as validated in the pre qualification study; 4. that no external contamination of the positive control has occurred.

Should these problems happen, after checking, report any residual problem to the supervisor for further actions.

** Note:

If Calibrator has used, verify the following data:

Check	Requirements
Calibrator	S/Co > 1.1

If the results of the test doesn't match the requirements stated above, operate as follows:

Problem	Check
Calibrator S/Co < 1.1	1. that the procedure has been correctly executed; 2. that no mistake has been done in its distribution (e.g.: dispensation of negative control instead of Calibrator) 3. that the washing procedure and the washer settings are as validated in the pre qualification study; 4. that no external contamination of the calibrator has occurred.

Anyway, if all other parameters (Blank, Negative Control, Positive Control), match the established requirements, the test may be considered valid.

Important note:

The analysis must be done proceeding as the reading step described in the section M, point 12.

P. CALCULATION OF THE CUT-OFF

The tests results are calculated by means of a cut-off value determined with the following formula:

$$\text{Cut-Off} = \text{NC mean OD450nm/620-630nm} + 0.350$$

The value found for the test is used for the interpretation of results as described in the next paragraph.

Important note: *When the calculation of results is done by the operative system of an ELISA automated work station be sure that the proper formulation is used to calculate the cut-off value and generate the right interpretations of results.*

Q. INTERPRETATION OF RESULTS

Test results are interpreted as ratio of the sample OD450nm/620-630nm and the Cut-Off value (or S/Co) according to the following table:

S/Co	Interpretation
< 0.9	Negative
0.9 - 1.1	Equivocal
> 1.1	Positive

A negative result indicates that the patient has not been infected by HEV or that the blood unit may be transfused.

Any patient showing an equivocal result should be tested again on a second sample taken 1-2 weeks later from the patient and examined. The blood unit should not be transfused.

A positive result is indicative of HEV infection and therefore the patient should be treated accordingly or the blood unit should be discarded.

Important notes:

1. *Interpretation of results should be done under the supervision of the responsible of the laboratory to reduce the risk of judgment errors and misinterpretations.*
2. *By definition, any positive result should be confirmed by an alternative method before a diagnosis of viral hepatitis is formulated.*
3. *When test results are transmitted from the laboratory to an informatics center, attention has to be done to avoid erroneous data transfer.*
4. *Diagnosis of viral hepatitis infection has to be done and released to the patient only by a qualified medical doctor.*

An example of calculation is reported below (data obtained proceeding as the reading step described in the section M, point 12):

The following data must not be used instead of real figures obtained by the user.

Negative Control: 0.019 – 0.020 – 0.021 OD450nm

Mean Value: 0.020 OD450nm

Lower than 0.050 – Accepted

Positive Control: 2.189 OD450nm

Higher than 1.000 – Accepted

Cut-Off = 0.020 + 0.350 = 0.370

Calibrator: 0.600 - 0.640 OD450nm

Mean value: 0.620 OD450nm

S/Co = 1.7

S/Co higher than 1.1 – Accepted

Sample 1: 0.070 OD450nm
Sample 2: 1.690 OD450nm
Sample 1 S/Co < 0.9 = negative
Sample 2 S/Co > 1.1 = positive

R. PERFORMANCES

Evaluation of Performances has been conducted on negative and positive samples in an external clinical center with reference to a FDA approved kit.

1. LIMIT OF DETECTION

The limit of detection of the assay has been calculated by means of 1st WHO reference reagent for HEV antibody, NIBSC code 95/584. The assay shows an analytical sensitivity of about 0.1 WHO IU/ml.

2. DIAGNOSTIC SPECIFICITY AND SENSITIVITY

They were checked with a sensitivity set at 0.25 WHO IU/ml on more than total 700 samples.

2.1 Diagnostic Specificity:

It is defined as the probability of the assay of scoring negative in the absence of specific analyte.

A total number of more than one hundred 1-5 years old children, by definition negative for HEV antibodies as they never chanced to eat uncooked swine meat and get therefore infected, were tested; a value of 100% specificity (negativity) was assured at a sensitivity set at a cut-off of 0.25 WHO IU/ml.

In addition, a total of more 500 unselected donors, including 1st time donors, and HEV negative hospitalized patients, coming from Italy, were examined maintaining the sensitivity of 0.25 WHO IU/ml. About 5% of such population turned out to be repeatedly positive; confirmation was not carried out in absence of a commercial Confirmation kit. However, these samples were detected positive with a commercial CE-marked ELISA. From this study a diagnostic specificity of 100% was observed.

Moreover, the Diagnostic Specificity was also assessed by testing more than 100 potentially interfering specimens (other infectious diseases, patients affected by non viral hepatic diseases, dialysis patients, pregnant women, haemolized, lipemic, etc.). A value of specificity of 100% was assessed.

No false reactivity due to the method of specimen preparation has been observed. Both plasma, derived with different standard techniques of preparation (citrate, EDTA and heparin), and sera have been used to determine the value of specificity.

Frozen specimens have been tested, as well, to check for interferences due to collection and storage.

No interference was observed.

2.2 Diagnostic Sensitivity

It is defined as the probability of the assay of scoring positive in the presence of specific analyte.

The diagnostic sensitivity has been assessed externally (Institute of Virology, University of Milan) and internally on a total number of 200 positive specimens (maintaining a sensitivity set at a cut-off of 0.25 WHO IU/ml); a diagnostic sensitivity (or correlation with a commercial reference kit manufactured in Europe and CE marked) of 100% was found.

3. PRECISION:

It has been calculated on two samples, one negative and one low positive, examined in 16 replicates in three separate runs.

CV values ranging between 5-10%, depending on OD450nm/620-630nm values, were found. The variability seen did not result in sample misclassification.

S. LIMITATIONS

Frozen samples containing fibrin particles or aggregates after thawing have been observed to generate some false results.

REFERENCES

1. Ellner PD, Neu HC. Viral agents of gastroenteritis. In "Understanding infectious disease. St.Louis: Mosby-Year Book, 1992, pp183-186.
2. Hollinger FB, Dreesman GR. Hepatitis virus. In "Rose NR, de Macario EC, Fahey JL, et al. (eds), Manual of clinical laboratory immunology, 4th ed. Washington, DC: ASM, 1992, pp634-650.
3. Fody EP, Johnson DF. J Med Technol 1987, 4:54-59.
4. Bradley D.W. et al.. Br.Med.Bull. 46: 442-461, 1990
5. Dawson G.J. et al.. J.Virol.Methods 38: 175-186, 1992
6. Favorov M.O. et al.. J.Med.Virol.. 36: 246-250, 1992
7. Purdy M. et al.. J.Arch.Virol. 123: 335-349, 1992
8. Tam A.W. et al.. Virology 185: 120-131, 1991

All the IVD Products manufactured by the company are under the control of a certified Quality Management System in compliance with ISO 13485 rule. Each lot is submitted to a quality control and released into the market only if conforming with the EC technical specifications and acceptance criteria.

Manufacturer:
Dia.Pro Diagnostic Bioprobes Srl
Via G. Carducci n° 27 – Sesto San Giovanni (MI) – Italy





Dia.Pro
Diagnostic
Bio**Probes**

EC DECLARATION OF CONFORMITY

MANUFACTURER	DIA.PRO DIAGNOSTIC BIOPROBES S.R.L. VIA G. CARDUCCI N° 27 – 20099 SESTO SAN GIOVANNI (MILANO) – ITALY
PRODUCT	HEV IgG CODE: EVG.CE (96 tests)
CLASSIFICATION	GENERAL IVD
CONFORMITY ASSESSMENT ROUTE	SELF CERTIFICATION

**WE HEREBY DECLARE THAT THE ABOVE MENTIONED PRODUCT MEETS
THE PROVISIONS OF THE COUNCIL DIRECTIVE 98/79/EC
FOR IN VITRO DIAGNOSTIC DEVICES.**

ISO CERTIFICATE	UNE EN ISO 13485 N° 2013 11 0039 EN, RELEASED BY AEMPS (AGENCIA ESPAÑOLA DE MEDICAMENTOS Y PRODUCTOS SANITARIOS)
------------------------	---

PLACE & DATE OF FIRST ISSUE	MILANO – JULY 2004
PLACE & DATE OF CURRENT ISSUE	SESTO SAN GIOVANNI (MI) – MARCH 2019
SIGNATURE Legal Representative Dr.ssa Fiorenza Scozzesi	

Rev: 05/2018



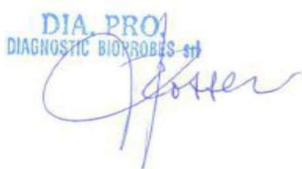
Dia.Pro
Dia**g**nostic
Bio**P**robes

EC DECLARATION OF CONFORMITY

MANUFACTURER	DIA.PRO DIAGNOSTIC BIOPROBES S.R.L. VIA G. CARDUCCI N° 27 – 20099 SESTO SAN GIOVANNI (MILANO) – ITALY
PRODUCT	HEV IgM CODE: EVM.CE (96 tests)
CLASSIFICATION	GENERAL IVD
CONFORMITY ASSESSMENT ROUTE	SELF CERTIFICATION

**WE HEREBY DECLARE THAT THE ABOVE MENTIONED PRODUCT MEETS
THE PROVISIONS OF THE COUNCIL DIRECTIVE 98/79/EC
FOR IN VITRO DIAGNOSTIC DEVICES.**

ISO CERTIFICATE	UNE EN ISO 13485 N° 2013 11 0039 EN, RELEASED BY AEMPS (AGENCIA ESPAÑOLA DE MEDICAMENTOS Y PRODUCTOS SANITARIOS)
------------------------	---

PLACE & DATE OF FIRST ISSUE	MILANO – MARCH 2004
PLACE & DATE OF CURRENT ISSUE	SESTO SAN GIOVANNI (MI) – MARCH 2019
SIGNATURE Legal Representative Dr.ssa Fiorenza Scozzesi	

Rev: 05/2018

HEV IgM

**Enzyme Immunoassay (ELISA)
for the determination of IgM antibodies
to Hepatitis E Virus
in human serum and plasma**

- for “in vitro” diagnostic use only -



DIA.PRO

**Diagnostic Bioprobes Srl
Via G. Carducci n° 27
20099 Sesto San Giovanni
(Milano) - Italy**

Phone +39 02 27007161

Fax +39 02 44386771

e-mail: info@diapro.it

HEV IgM

A. INTENDED USE

Enzyme ImmunoAssay (ELISA) for the determination of IgM antibodies to Hepatitis E Virus in human plasma and sera. The kit may be used for the determination of the acute phase of infection where IgM antibodies are generated before the other immunoglobulins and for the follow-up of HEV-infected patients. For "in vitro" diagnostic use only.

B. INTRODUCTION

Hepatitis E Virus or HEV is a recently discovered agent of enterically transmitted viral hepatitis. HEV is an un-enveloped single-strand RNA virus, after being provisionally assigned to the Caliciviridae family, HEV was re-classified as the sole member of the genus Hepevirus, family Hepeviridae, in 2004. HEV is found in the stool of infected patients and present in 4 strains (1, 2, 3 and 4) differently spread geographically and virulent.

HEV is a serious problem in many developing countries since its first outbreak was reported in 1955 in New Delhi, India.

A high case-fatality rate has been found among pregnant women and chronic hepatitis carriers.

The cloning and sequencing of HEV genome have led to the development of serological tests for the detection of anti HEV antibodies based on recombinant immunodominant antigens derived from conservative regions of the four virus strains.

C. PRINCIPLE OF THE TEST

Microplates are coated with HEV-specific recombinant antigens encoding for conservative and immunodominant determinants of all the 4 subtypes.

The solid phase is first treated with the diluted sample and anti HEV IgM are captured, if present, by the antigens.

After washing out all the other components of the sample, in the 2nd incubation bound anti-HEV IgM are detected by the addition of polyclonal specific anti hIgM antibodies, labelled with peroxidase (HRP).

The enzyme captured on the solid phase, acting on the substrate/chromogen mixture, generates an optical signal that is proportional to the amount of anti HEV IgM present in the sample. A cut-off value let optical densities be interpreted into anti-HEV IgM negative and positive results.

Neutralization of IgG anti-HEV and Rheumatoid Factor, carried out directly in the well, is performed in the assay in order to block such kind of interferences.

D. COMPONENTS

Code EVM.CE contains reagents for 96 tests.

1. Microplate MICROPLATE

n° 1 microplate. 12 strips of 8 microwells coated with HEV specific recombinant antigens. Plates are sealed into a bag with desiccant.

2. Negative Control CONTROL -

1x4.0ml/vial. Ready to use control. It contains 1% goat serum proteins, 10 mM Na-citrate buffer pH 6.0 +/-0.1, 0.5% Tween 20, 0.09% Na-azide and 0.045% ProClin 300 as preservatives. The negative control is yellow colour coded.

3. Positive Control CONTROL +

1x4.0ml/vial. Ready to use control. It contains 1% goat serum proteins, human anti HEV IgM, 10 mM Na-citrate buffer pH 6.0 +/-0.1, 0.5% Tween 20, 0.09% Na-azide and 0.045% ProClin 300 as preservatives.

The Positive Control is dark green colour coded.

4. Wash buffer concentrate WASHBUF 20X

1x60ml/bottle. 20x concentrated solution. Once diluted, the wash solution contains 10 mM phosphate buffer pH 7.0+/-0.2, 0.05% Tween 20 and 0.045% ProClin 300.

5. Enzyme Conjugate CONJ

1x16ml/vial. Ready to use and red colour coded reagent. It contains Horseradish Peroxidase conjugated goat polyclonal antibodies to human IgM, 5% BSA, 10 mM Tris buffer pH 6.8+/-0.1, 0.045% ProClin 300 and 0.02% gentamicine sulphate as preservatives.

6. Chromogen/Substrate SUBS TMB

1x16ml/vial. Ready-to-use component. It contains 50 mM citrate-phosphate buffer pH 3.5-3.8, 4% dimethylsulphoxide, 0.03% tetra-methyl-benzidine or TMB and 0.02% hydrogen peroxide or H₂O₂.

Note: To be stored protected from light as sensitive to strong illumination.

7. Sulphuric Acid H₂SO₄ 0.3 M

1x15ml/vial. It contains 0.3 M H₂SO₄ solution.

Attention: Irritant (H315, H319; P280, P302+P352, P332+P313, P305+P351+P338, P337+P313, P362+P363).

8. Specimen Diluent: DILSPE

2x60ml/vial. It contains 2% casein, 10 mM Na-citrate buffer pH 6.0 +/-0.1, 0.1% Tween 20, 0.09% Na-azide and 0.045% ProClin 300 as preservatives. To be used to dilute the sample.

9. Neutralizing Reagent: SOLN NTR

1x8ml/vial. Ready-to-use Reagent. It contains goat anti hIgG, 2% casein, 10 mM Na-citrate buffer pH 6.0 +/-0.1, 0.1% Tween 20, 0.09% Na-azide and 0.045% ProClin 300 as preservatives.

10. Plate sealing foils n° 2

11. Package insert n° 1

E. MATERIALS REQUIRED BUT NOT PROVIDED

1. Calibrated Micropipettes (100ul and 10ul) and disposable plastic tips.
2. EIA grade water (bidistilled or deionised, charcoal treated to remove oxidizing chemicals used as disinfectants).
3. Timer with 60 minute range or higher.
4. Absorbent paper tissues.
5. Calibrated ELISA microplate thermostatic incubator capable to provide a temperature of +37°C.
6. Calibrated ELISA microwell reader with 450nm (reading) and with 620-630nm (blanking) filters.
7. Calibrated ELISA microplate washer.
8. Vortex or similar mixing tools.

F. WARNINGS AND PRECAUTIONS

1. The kit has to be used by skilled and properly trained technical personnel only, under the supervision of a medical doctor responsible of the laboratory.
2. All the personnel involved in performing the assay have to wear protective laboratory clothes, talc-free gloves and glasses. The use of any sharp (needles) or cutting (blades) devices should be avoided. All the personnel involved should be trained in biosafety procedures, as recommended by the Center for Disease Control, Atlanta, U.S. and reported in the National Institute of Health's publication: "Biosafety in Microbiological and Biomedical Laboratories", ed. 1984.
3. All the personnel involved in sample handling should be vaccinated for HBV and HAV, for which vaccines are available, safe and effective.
4. The laboratory environment should be controlled so as to avoid contaminants such as dust or air-born microbial agents, when opening kit vials and microplates and when performing the

test. Protect the Chromogen/Substrate from strong light and avoid vibration of the bench surface where the test is undertaken.

5. Upon receipt, store the kit at 2..8°C into a temperature controlled refrigerator or cold room.

6. Do not interchange components between different lots of the kits. It is recommended that components between two kits of the same lot should not be interchanged.

7. Check that the reagents are clear and do not contain visible heavy particles or aggregates. If not, advise the laboratory supervisor to initiate the necessary procedures for kit replacement.

8. Avoid cross-contamination between serum/plasma samples by using disposable tips and changing them after each sample. Do not reuse disposable tips.

9. Avoid cross-contamination between kit reagents by using disposable tips and changing them between the use of each one. Do not reuse disposable tips.

10. Do not use the kit after the expiration date stated on the external container and internal (vials) labels.

11. Treat all specimens as potentially infective. All human serum specimens should be handled at Biosafety Level 2, as recommended by the Center for Disease Control, Atlanta, U.S. in compliance with what reported in the Institutes of Health's publication: "Biosafety in Microbiological and Biomedical Laboratories", ed. 1984.

12. The use of disposable plastic-ware is recommended in the preparation of the liquid components or in transferring components into automated workstations, in order to avoid cross contamination.

13. Waste produced during the use of the kit has to be discarded in compliance with national directives and laws concerning laboratory waste of chemical and biological substances. In particular, liquid waste generated from the washing procedure, from residuals of controls and from samples has to be treated as potentially infective material and inactivated before waste. Suggested procedures of inactivation are treatment with a 10% final concentration of household bleach for 16-18 hrs or heat inactivation by autoclave at 121°C for 20 min..

14. Accidental spills from samples and operations have to be adsorbed with paper tissues soaked with household bleach and then with water. Tissues should then be discarded in proper containers designated for laboratory/hospital waste.

15. The Sulphuric Acid is an irritant. In case of spills, wash the surface with plenty of water

16. Other waste materials generated from the use of the kit (example: tips used for samples and controls, used microplates) should be handled as potentially infective and disposed according to national directives and laws concerning laboratory wastes.

G. SPECIMEN: PREPARATION AND RECOMMANDATIONS

1. Blood is drawn aseptically by venepuncture and plasma or serum is prepared using standard techniques of preparation of samples for clinical laboratory analysis. No influence has been observed in the preparation of the sample with citrate, EDTA and heparin.

2. Samples have to be clearly identified with codes or names in order to avoid misinterpretation of results. When the kit is used for the screening of blood units, bar code labeling and electronic reading is strongly recommended.

3. Haemolysed (red) and visibly hyperlipemic ("milky") samples have to be discarded as they could generate false results. Samples containing residues of fibrin or heavy particles or microbial filaments and bodies should be discarded as they could give rise to false results.

4. Sera and plasma can be stored at +2°...+8°C in primary collection tubes for up to five days after collection.

Do not freeze primary tubes of collection. For longer storage periods, sera and plasma samples, carefully removed from the primary collection tube, can be stored frozen at -20°C for at least 12 months. Any frozen samples should not be

frozen/thawed more than once as this may generate particles that could affect the test result.

5. If particles are present, centrifuge at 2.000 rpm for 20 min or filter using 0.2-0.8u filters to clean up the sample for testing.

H. PREPARATION OF COMPONENTS AND WARNINGS

A study conducted on an opened kit has not pointed out any relevant loss of activity up to 6 re-use of the device and up to 6 months.

Microplates:

Allow the microplate to reach room temperature (about 1 hr) before opening the container. Check that the desiccant is not turned to dark green, indicating a defect of conservation.

In this case call Dia.Pro's customer service.

Unused strips have to be placed back into the aluminium pouch, in presence of desiccant supplied, firmly zipped and stored at +2°..8°C.

When opened the first time, residual strips are stable till the indicator of humidity inside the desiccant bag turns from yellow to green.

Negative Control:

Ready to use. Mix well on vortex before use.

Positive Control:

Ready to use. Mix well on vortex before use. Handle this component as potentially infective, even if HCV, eventually present in the control, has been chemically inactivated.

Wash buffer concentrate:

The whole content of the 20x concentrated solution has to be diluted with bidistilled water up to 1200 ml and mixed gently end-over-end before use.

Once diluted, the wash solution is stable for 1 week at +2..8° C.

In the preparation avoid foaming as the presence of bubbles could give origin to a bad washing efficiency.

Note: Once diluted, the wash solution is stable for 1 week at +2..8° C.

Enzyme conjugate:

Ready to use. Mix well on vortex before use.

Be careful not to contaminate the liquid with oxidizing chemicals, air-driven dust or microbes.

If this component has to be transferred use only plastic, possibly sterile disposable containers.

Chromogen/Substrate:

Ready to use. Mix well on vortex before use.

Be careful not to contaminate the liquid with oxidizing chemicals, air-driven dust or microbes.

Do not expose to strong illumination, oxidizing agents and metallic surfaces.

If this component has to be transferred use only plastic, possible sterile disposable container.

Neutralizing Reagent

Ready to use component. Mix carefully on vortex before use.

Sample Diluent:

Ready to use. Mix well on vortex before use.

Sulphuric Acid:

Ready to use. Mix well on vortex before use.

Attention: Irritant (H315, H319; P280, P302+P352, P332+P313, P305+P351+P338, P337+P313, P362+P363).

Legenda:

Warning H statements:

H315 – Causes skin irritation.

H319 – Causes serious eye irritation.

Precautionary P statements:

P280 – Wear protective gloves/protective clothing/eye protection/face protection.

P302 + P352 – IF ON SKIN: Wash with plenty of soap and water.

P332 + P313 – If skin irritation occurs: Get medical advice/attention.

P305 + P351 + P338 – IF IN EYES: Rinse cautiously with water for several minutes. Remove contact lenses, if present and easy to do. Continue rinsing.

P337 + P313 – If eye irritation persists: Get medical advice/attention.

P362 + P363 – Take off contaminated clothing and wash it before reuse.

I. INSTRUMENTS AND TOOLS USED IN COMBINATION WITH THE KIT

1. **Micropipettes** have to be calibrated to deliver the correct volume required by the assay and must be submitted to regular decontamination (household alcohol, 10% solution of bleach, hospital grade disinfectants) of those parts that could accidentally come in contact with the sample. They should also be regularly maintained in order to show a precision of 1% and a trueness of +/-2%. Decontamination of spills or residues of kit components should also be carried out regularly.
2. The **ELISA incubator** has to be set at +37°C (tolerance of +/-0.5°C) and regularly checked to ensure the correct temperature is maintained. Both dry incubators and water baths are suitable for the incubations, provided that the instrument is validated for the incubation of ELISA tests.
3. The **ELISA washer** is extremely important to the overall performances of the assay. The washer must be carefully validated in advance, checked for the delivery of the right dispensation volume and regularly submitted to maintenance according to the manufacturer's instructions for use. In particular the washer, at the end of the daily workload, has to be extensively cleaned out of salts with deionized water. Before use, the washer has to be extensively primed with the diluted Washing Solution. The instrument weekly has to be submitted to decontamination according to its manual (NaOH 0.1 M decontamination suggested).
5 washing cycles (aspiration + dispensation of 350ul/well of washing solution + 20 sec soaking = 1 cycle) are sufficient to ensure the assay with the declared performances. If soaking is not possible add one more cycle of washing.
An incorrect washing cycle or salt-blocked needles are the major cause of false positive reactions.
4. Incubation times have a tolerance of ±5%.
5. The **ELISA reader** has to be equipped with a reading filter of 450nm and with a second filter of 620-630nm, mandatory for blanking purposes. Its standard performances should be (a) bandwidth ≤ 10 nm; (b) absorbance range from 0 to ≥ 2.0; (c) linearity to ≥ 2.0; repeatability ≥ 1%. Blanking is carried out on the well identified in the section "Assay Procedure". The optical system of the reader has to be calibrated regularly to ensure that the correct optical density is measured. It should be regularly maintained according to the manufacturer's instructions.
6. When using an **ELISA automated work station**, all critical steps (dispensation, incubation, washing, reading, data handling) have to be carefully set, calibrated, controlled and regularly serviced in order to match the values reported in the sections "Validation of Test" and "Assay Performances". The assay protocol has to be installed in the operating system of the unit and validated as for the washer and the reader. In addition, the liquid handling part of the station (dispensation and washing) has to be validated and correctly set. Particular attention must be paid to avoid carry over by the needles used for dispensing and for washing. This must be studied and controlled to minimize the

possibility of contamination of adjacent wells. The use of ELISA automated work stations is recommended when the number of samples to be tested exceed 20-30 units per run.

7. Dia.Pro's customer service offers support to the user in the setting and checking of instruments used in combination with the kit, in order to assure compliance with the requirements described. Support is also provided for the installation of new instruments to be used with the kit.

L. PRE ASSAY CONTROLS AND OPERATIONS

1. Check the expiration date of the kit printed on the external label (primary container). Do not use if expired.
2. Check that the liquid components are not contaminated by visible particles or aggregates.
3. Check that the Chromogen (TMB) is colourless or pale blue by aspirating a small volume of it with a sterile plastic pipette.
4. Check that no breakage occurred in transportation and no spillage of liquid is present inside the box (primary container). Check that the aluminium pouch, containing the microplate, is not punctured or damaged.
5. Dissolve the content of the Control Serum as reported.
6. Dilute all the content of the 20x concentrated Wash Solution as described above.
7. Allow all the other components to reach room temperature (about 1 hr) and then mix gently on vortex all liquid reagents.
8. Set the ELISA incubator at +37°C and prepare the ELISA washer by priming with the diluted washing solution, according to the manufacturers instructions. Set the right number of washing cycles as as reported in the specific section.
9. Check that the ELISA reader is turned on or ensure it will be turned on at least 20 minutes before reading.
10. If using an automated work station, turn on, check settings and be sure to use the right assay protocol.
11. Check that the micropipettes are set to the required volume.
12. Check that all the other equipment is available and ready to use.
13. In case of problems, do not proceed further with the test and advise the supervisor.

M. ASSAY PROCEDURE

The assay has to be carried out according to what reported below, taking care to maintain the same incubation time for all the samples in testing.

1. Dilute samples 1:101 into a properly defined dilution tube (example: 1000 µl Sample Diluent + 10 µl sample). Do not dilute the negative Control and the Positive Control as they are ready to use. Mix carefully all the liquid components on vortex and then proceed as described below.
2. Place the required number of Microwells in the microwell holder. Leave A1 well empty for the operation of blanking.
3. Dispense 50 µl of the Neutralizing Reagent (SOLN NTR) in all the wells of the samples. Do not add it in the wells used for Controls and in A1!

Important note: The Neutralizing Reagent is able to block false positive reactions due to RF. Positive samples in internal QC panels might be detected negative if such samples were tested positive with an IVD that does not carry out any RF blocking reaction.

4. Dispense 100 µl of Negative Control in triplicate and 100 µl of Positive control in single. Then dispense 100 µl of diluted samples in each properly identified well.
5. Incubate the microplate for **60 min at +37°C**.

Important note: Strips have to be sealed with the adhesive sealing foil, supplied, only when the test is carried out manually. Do not cover strips when using ELISA automatic instruments.

- Wash the microplate with an automatic washer by delivering and aspirating 300 µl/well of diluted washing solution as reported previously (section I.3).
- Pipette 100 µl Enzyme Conjugate into each well, except the A1 well, and cover with the sealer. Check that this red coloured component has been dispensed in all the wells, except A1.

Important note: Be careful not to touch the plastic inner surface of the well with the tip filled with the Enzyme Conjugate. Contamination might occur.

- Incubate the microplate for **60 min at +37°C**.
- Wash microwells as in step 6.
- Pipette 100 µl Chromogen/Substrate mixture into each well, the blank well included. Then incubate the microplate at **room temperature (18-24°C) for 20 minutes**.

Important note: Do not expose to strong direct illumination. High background might be generated.

- Pipette 100 µl Sulphuric Acid into all the wells using the same pipetting sequence as in step 10. Addition of acid will turn the positive calibrators, the control serum and the positive samples from blue to yellow.
- Measure the colour intensity of the solution in each well, as described in section I.5, at 450nm filter (reading) and at 620-630nm (background subtraction, mandatory), blanking the instrument on A1.

General Important notes:

- Ensure that no finger prints are present on the bottom of the microwell before reading. Finger prints could generate false positive results on reading.
- Reading has to be carried out just after the addition of the Stop Solution and anyway not any longer than 20 minutes after its addition. Some self oxidation of the chromogen can occur leading to high background.

N. ASSAY SCHEME

Method	Operations
Neutralizing Reagent (in sample wells only !)	50 µl
Negative and Positive Controls	100 µl
Samples diluted 1:101	100 µl
1st incubation	60 min
Temperature	+37°C
Wash step	n° 5 cycles with 20" of soaking OR n° 6 cycles without soaking
Enzyme conjugate	100 µl
2nd incubation	60 min
Temperature	+37°C
Wash step	n° 5 cycles with 20" of soaking OR n° 6 cycles without soaking
TMB/H2O2	100 µl
3rd incubation	20 min
Temperature	r.t.
Sulphuric Acid	100 µl
Reading OD	450nm/620-630nm

An example of dispensation scheme is reported below:

Microplate												
	1	2	3	4	5	6	7	8	9	10	11	12
A	BLK	S4										
B	NC	S5										
C	NC	S6										
D	NC	S7										
E	PC	S8										
F	S1	S9										
G	S2	S10										
H	S3	S11										

Legenda: BLK = Blank NC = Negative Control
PC = Positive Control S = Sample

O. INTERNAL QUALITY CONTROL

A check is carried out on the controls any time the kit is used in order to verify whether their OD450nm/620-630nm values are as expected and reported in the table below.

Check	Requirements
Blank well	< 0.100 OD450nm value
Negative Control (NC)	< 0.100 mean OD450nm value after blanking
Positive Control	> 0.500 OD450nm value

If the results of the test match the requirements stated above, proceed to the next section.

If they do not, do not proceed any further and operate as follows:

Problem	Check
Blank well > 0.100 OD450nm	1. that the Chromogen/Substrate solution has not got contaminated during the assay
Negative Control (NC) > 0.100 OD450nm after blanking	1. that the washing procedure and the washer settings are as validated in the pre qualification study; 2. that the proper washing solution has been used and the washer has been primed with it before use; 3. that no mistake has been done in the assay procedure (dispensation of positive control instead of negative control); 4. that no contamination of the negative control or of their wells has occurred due to positive samples, to spills or to the enzyme conjugate; 5. that micropipettes haven't got contaminated with positive samples or with the enzyme conjugate 6. that the washer needles are not blocked or partially obstructed.
Positive Control < 0.500 OD450nm	1. that the procedure has been correctly executed; 2. that no mistake has been done in the distribution of controls (dispensation of negative control instead of positive control. In this case, the negative control will have an OD450nm value > 0.150, too. 3. that the washing procedure and the washer settings are as validated in the pre qualification study; 4. that no external contamination of the positive control has occurred.

Should these problems happen, after checking, report any residual problem to the supervisor for further actions.

Important note:

The analysis must be done proceeding as the reading step described in the section M, point 12.

P. CALCULATION OF THE CUT-OFF

The tests results are calculated by means of a cut-off value determined with the following formula:

$$\text{Cut-Off} = \text{NC mean OD}_{450\text{nm}/620-630\text{nm}} + 0.250$$

The value found for the test is used for the interpretation of results as described in the next paragraph.

Important note: When the calculation of results is done by the operative system of an ELISA automated work station be sure that the proper formulation is used to calculate the cut-off value and generate the right interpretations of results.

Q. INTERPRETATION OF RESULTS

Test results are interpreted as ratio of the sample $\text{OD}_{450\text{nm}/620-630\text{nm}}$ and the Cut-Off value (or S/Co) according to the following table:

S/Co	Interpretation
< 1.0	Negative
1.0 – 1.2	Equivocal
> 1.2	Positive

A negative result indicates that the patient has no detectable anti HEV IgM reactivity.

Any patient showing an equivocal result should be tested again on a second sample taken 1-2 weeks later from the patient and examined.

A positive result is indicative of HEV infection and therefore the patient should be treated accordingly.

Important notes:

1. Interpretation of results should be done under the supervision of the responsible of the laboratory to reduce the risk of judgment errors and misinterpretations.
2. Any positive result should be confirmed by an alternative method before a diagnosis of viral hepatitis is formulated.
3. When test results are transmitted from the laboratory to an informatics center, attention has to be done to avoid erroneous data transfer.
4. Diagnosis of viral hepatitis E infection has to be done and released to the patient only by a qualified medical doctor.

An example of calculation is reported below (data obtained proceeding as the the reading step described in the section M, point 12):

The following data must not be used instead of real figures obtained by the user.

Negative Control: 0.060 – 0.080 – 0.070 DO 450nm

Mean Value: 0.070 OD450nm

Lower than 0.100 – Accepted

Positive Control: 1.589 OD450nm

Higher than 0.500 – Accepted

Cut-Off = 0.070+0.250 = 0.320

Sample 1: 0.070 OD450nm

Sample 2: 1.690 OD450nm

Sample 1 S/Co < 1.0 = negative

Sample 2 S/Co > 1.2 = positive

R. PERFORMANCES

Evaluation of Performances has been conducted on negative and positive samples in an external clinical center with reference to a FDA approved kit.

1. LIMIT OF DETECTION

The limit of detection of the product has been checked on the international reference reagent for HEV antibody supplied by NIBSC/WHO with code n° 95/584. This material was assessed to be positive also for anti HEV IgM, low titer. The observed value is about 1 IU/ml.

2. DIAGNOSTIC SPECIFICITY AND SENSITIVITY

They were checked on about 700 sample derived from acute infections, HEV Ab positive patients, random individuals under diagnostic examination and healthy individuals with a sensitivity set at about 5 IU/ml in order to assure the highest sensitivity and be able to detect primary infection at the earliest phase.

2.1 Diagnostic specificity:

It is defined as the probability of the assay of scoring negative in the absence of specific analyte.

A total of more 500 unselected donors and HEV negative hospitalized patients, including 1st time donors, were examined. The diagnostic specificity was assessed against a kit US FDA approved. A diagnostic specificity of $\geq 95\%$ was observed.

Moreover, diagnostic specificity was assessed by testing more than 100 potentially interfering specimens (other infectious diseases, patients affected by non viral hepatic diseases, dialysis patients, pregnant women, haemolized, lipemic, etc.).

A value of specificity of 100% was assessed.

No false reactivity due to the method of specimen preparation has been observed. Both plasma, derived with different standard techniques of preparation (citrate, EDTA and heparin), and sera have been used to determine the value of specificity.

Frozen specimens have been tested, as well, to check for interferences due to collection and storage.

No interference was observed.

High reactive RF positive samples were observed to give origin to false positive results in not more than 5% of HEV Ab negative individuals.

2.2 Diagnostic Sensitivity

It defined as the probability of the assay of scoring positive in the presence of specific analyte.

The diagnostic sensitivity has been assessed externally and internally on a total number of 100 positive specimens coming from Germany, Mexico and from Burma.

A diagnostic sensitivity of 100% was found.

3. PRECISION:

It has been calculated on two samples, one negative and one positive, examined in 16 replicates in three separate runs.

CV values ranging between 5-15%, depending on OD450nm values, were found. The variability seen did not result in sample misclassification.

S. LIMITATIONS

Repeatable false positive results were assessed for high titer RF positive samples, escaping the effect of the Neutralizing Reagent.

Frozen samples containing fibrin particles or aggregates after thawing have been observed to generate some false results.

REFERENCES

1. Ellner PD, Neu HC. Viral agents of gastroenteritis. In "Understanding infectious disease. St.Louis: Mosby-Year Book, 1992, pp183-186.
2. Hollinger FB, Dreesman GR. Hepatitis virus. In "Rose NR, de Macario EC, Fahey JL, et al. (eds), Manual of clinical laboratory immunology, 4th ed. Washington, DC: ASM, 1992, pp634-650.
3. Fody EP, Johnson DF. J Med Technol 1987, 4:54-59.
4. Bradley D.W. et al.. Br.Med.Bull. 46: 442-461, 1990
5. Dawson G.J. et al.. J.Virol.Methods 38: 175-186, 1992
6. Favorov M.O. et al.. J.Med.Virol.. 36: 246-250, 1992
7. Purdy M. et al.. J.Arch.Virol. 123: 335-349, 1992
8. Tam A.W. et al.. Virology 185: 120-131, 1991

All the IVD Products manufactured by the company are under the control of a certified Quality Management System in compliance with ISO 13485 rule. Each lot is submitted to a quality control and released into the market only if conforming with the EC technical specifications and acceptance criteria.

Manufacturer:
Dia.Pro. Diagnostic Bioprobes Srl.
Via G. Carducci n° 27 – Sesto San Giovanni (MI) – Italy

