



PRODUCT DESCRIPTION

UR .53

Revision

1

Date

1.09.2021

DESCRIPTION

GENERAL INFORMATION

Product :	CAESAREAN SET	Standard :	DIR 93/42/CE
Art. N° :	INT-8010-XX	Sterile :	Yes
Class :	1S	All items	LATEX-FREE

Inaccordance with EN 13795 ISO 811:2018

Products

Table Cover x 1

RAW MATEREAL

Weight	Color	Material	Use
40g/m2 (+/-2)	Blue	SMMS	Drape

FEATURES


Designation	Value	Tolerance
A Total width	200cm	+/-10cm
B Total width	150cm	+/-10cm



Caesarean Drape x 1

RAW MATEREAL			
Weight	Color	Material	Use
56g/m2 (+/-2)	Blue	Biflex	Drape
30mic (+/-2)	Transparent	PE	Pouch


FEATURES		
Designation	Value	Tolerance
A Total width	200cm	+/-10cm
B Total width	300cm	+/-10cm
C Total width	75cm	+/-10cm

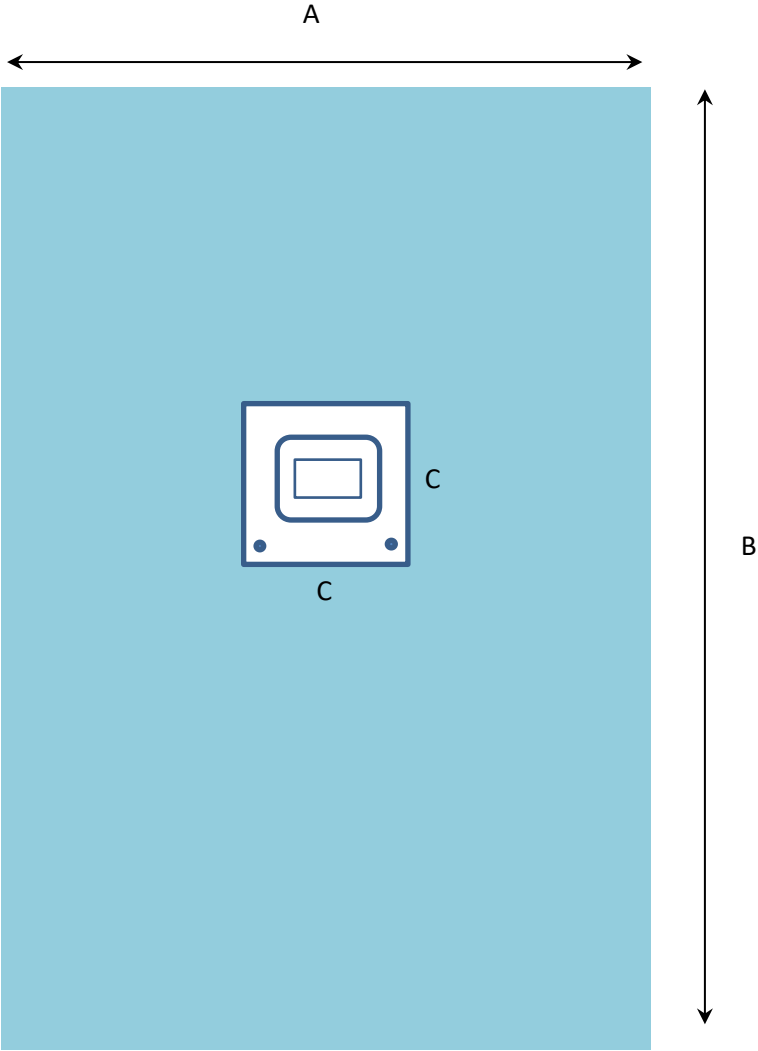

Baby Wrapping Towel x1

RAW MATEREAL			
Weight	Color	Material	Use
52g/m2 (+/-2)	White	Absrb. Nonwoven	Towel

FEATURES		
Designation	Value	Tolerance
A Total width	75cm	+/-10cm
B Total width	90cm	+/-10cm

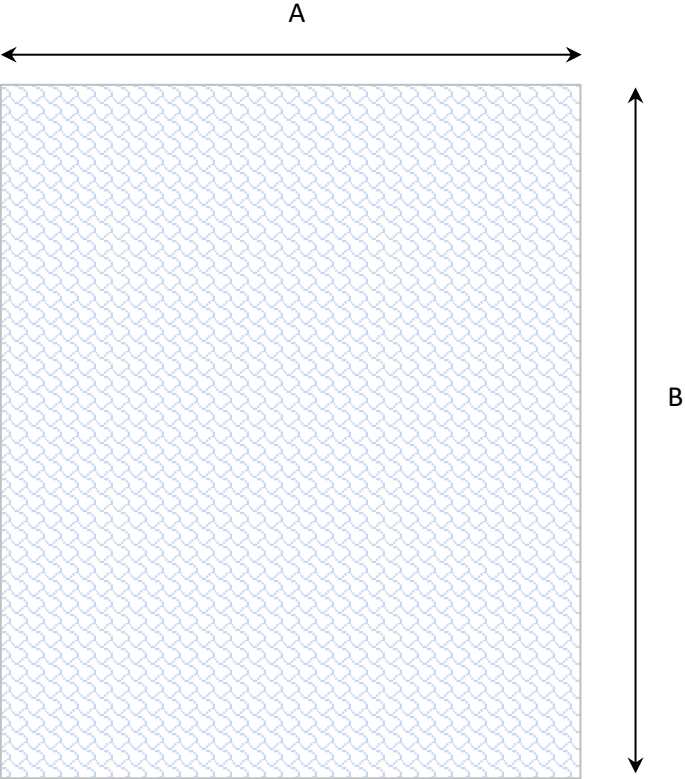


Umbilical Clamp x1

RAW MATEREAL			
Weight	Color	Material	Use
	White / Blue	PP	Clamp



Reinforced Surgical Gown L x2

RAW MATEREAL			
Weight	Color	Material	Use
37g/m2 (+/-2)	Blue	SMS	Gown
28g/m2(+/-2)	White	Laminated Spunbonded	Barier
Letter	Designation	Value (cm)	Tolerance (cm)
A	Total height	125	+/-2
B	Total width	150	+/-2
C	Chest width	80	+/-2
D	Collar width	23	+/-2
E	Shoulder width	21	+/-2
F	Armhole height	26	+/-2
G	Cuffs width	15	+/-2
H	Sleeves length	58	+/-2
I	Collar tie length	120	+/-10
J	Collar tie width	0.8	+/-0,2
K	Belt length	180	+/-10
L	Belt width	0,8	+/-0,2
M	Reinforced width	100	+/-0,5
N	Reinforced height	50	+/-0,5
O	Sleeve reinforcement length	35	+/-0,5

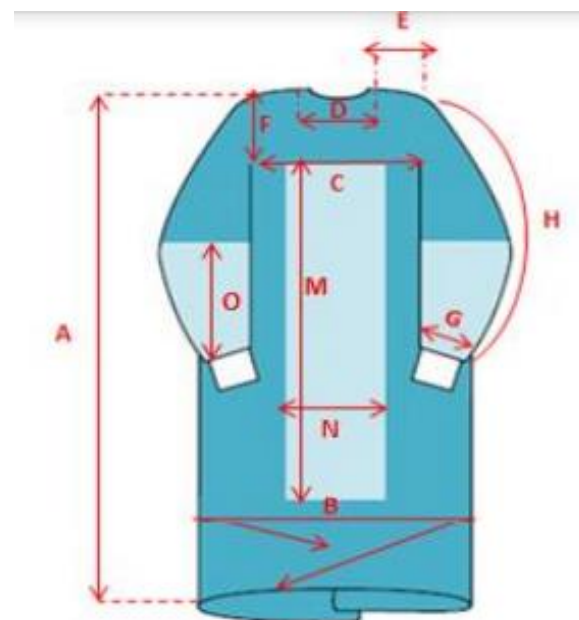


x2

Hand Towel x2

RAW MATEREAL			
Weight	Color	Material	Use
50g/m2 (+/-2)	White	Viscon	Towel

FEATURES		
Designation	Value	Tolerance
A Total width	40cm	+/-3cm
B Total width	40cm	+/-3cm

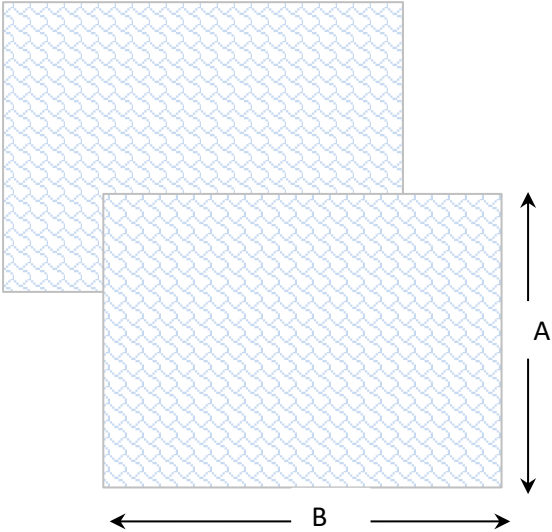


Laminated Bed Sheet x 1

RAW MATEREAL

Weight	Color	Material	Use
56g/m2 (+/-2)	Blue	Laminated NW	Bed Sheet

FEATURES

Designation	Value	Tolerance
A Total width	100	+/-10cm
B Total width	100	+/-10cm



- All the dimensions of the plain drape can be customized according to the desir of the customer. Available - custom dimensions, Reinforcement area, wrap.
- Intersect set is manufactured in accordance with the EN ISO 13485 standard. This ensures that we deliver products and services that consistently meet customer requirements, guaranteeing full customer satisfaction.
- All our products have a CE label and comply with the requirements of the Medical Device Directive 93/42/EEC

Manufacturer: TOTAL İth. İhr. ve Paz. Ltd. Şti