# SPINE PORTFOLIO

A COMPLETE RANGE OF SOLUTIONS



Brochure

Joint

Spine Sp

ports Med



## **SPINE PORTFOLIO**

## A COMPLETE RAN

#### CERVICAL

## Adecta-C SYSTEM

A **comprehensive system** of cervical interbody fusion **cages** and anterior **plates** for cases of degenerative disease, trauma, tumours and deformity.

Large range of implant sizes and lordosis to accommodate different patient anatomies.

## **Mecta-C** STAND ALONE

The **MODULAR design** incorporates the benefits of an anterior plate and a separate radiolucent titanium coated interbody spacer.

The surgeon has the ability to choose intraoperatively from **four different plate designs** and the option of fixing the construct with **lag** or **locking screws**, according to the patient's individual anatomy.





#### LUMBAR

## **AdectaLIF** ANTERIOR

**Modular cage and plate design** provides the surgeon with intra-operative freedom of choice.

Multiple configurations to cover different patient anatomy and surgical needs.



#### SACRO-ILIAC

## ▲.U.S.T. SACRO ILIAC

The M.U.S.T. Sacro Iliac System is designed for the **sacroiliac joint fusion** for patients suffering from degenerative sacroiliitis and sacroiliac joint disruptions.







## GE OF SOLUTIONS

#### CERVICAL



## **44.U.S.T.** MINI

A **simple and flexible** solution for **posterior cervical spine fixation** that allows the surgeon to assemble the desired construct according to the anatomy of the patient.

#### THORACOLUMBAR







## **44**.U.S.T.

**Versatile** and **comprehensive** pedicle screw system designed to provide **flexibility** to the surgeon.

Harmonious, single-system approach for most spine stabilisation applications.

## **AdectaLIF** SYSTEM

A **complete system** of **cages** for solid initial fixation, and long term spine stabilisation.

Versatile interbody fusion devices platform with various anatomic shaping to **address your unique patients**.

## ▲.U.S.T. MIS SYSTEM

M.U.S.T. MIS Platform: an **effective and harmonic** concept in terms of minimally invasive solutions.

The **Mini Open Retractor** together with the **Percutaneous System** can assist the surgeon to achieve efficient spine surgery results.



## **SPINE PORTFOLIO**

#### **TECHNOLOGIES**

y Spine

MySpine is a **patient specific** pedicle screw placement guide that, thanks to the 3D **pre-operative planning**, supports the surgeon during the critical steps of pedicle screw placement in order to:

- improve accuracy
- reduce the surgical time
- reduce X-ray radiation to the patient and OR Staff

This innovative concept combines several different features to offer potential benefits to both the surgeon and the patient.





MySpine MC is a **3D printed** patient matched solution in the **midline cortical** approach. Posterior lumbar fusion is driven in a **minimally invasive**<sup>[1]</sup>, muscle sparing way, potentially allowing for shorter operating times<sup>[2,3]</sup> and a reduction of both radiation exposure<sup>[2]</sup> and costs<sup>[3]</sup>.

## **AdectaLIF** TIPEEK

Medacta's TiPEEK cages represent the next generation plasma sprayed Ti-Coated interbody fusion device designed to:

- promote bony on-growth
- provide optimal diagnostic assessment
- deliver improved stability

**Titanium coated** PEEK cervical and lumbar cages offer **superior properties** with regard to biocompatibility and biomechanical behaviour.

## **Cement & Biologics**

A dedicated **cement system** that can provide pedicle screw augmentation and strong fixation. Fully synthetic **moldable bone graft** that easily fits into different size and shaping of Medacata' cages. The microporous resorbable granules of calcium phosphate promotes a **faster bone growth**.

#### REFERENCES

[1] Matsukawa -2nd MORE Japan MySpine cortical Bone Trajectory 2017. [2] Farshad et. al. Accuracy of patient-specific template-guided vs. free-hand fluoroscopically controlled pedicle screw placement in the thoracic and lumbar spine: a randomized cadaveric study. Eur Spine J. 2016 [3] Landi et al. Spinal Neuronavigation and 3D-Printed Tubular Guide for Pedicle Screw Placement: A Really New Tool to Improve Safety and Accuracy of the Surgical Technique? J Spine 2015, 4:5

All trademarks and registered trademarks are the property of their respective owners. This document is not intended for the US market. Please verify approval of the devices described in this document with your local Medacta representative.



Medacta International Strada Regina - 6874 Castel San Pietro - Switzerland Phone +41 91 696 60 60 - Fax + 41 91 696 60 66 Info@medacta.ch - www.medacta.com

99.99.1spine-c rev. 01 Last update: October 2018

Spine Portfolio

# **Aecta-C**° STAND ALONE

ANTERIOR CERVICAL INTERBODY FUSION DEVICE

MODULAR DESIGN OFFERS FREEDOM OF CHOICE



International

# **Mecta-C**<sup>®</sup> STAND ALONE

## ACDF STAND

#### **MECTA-C STAND ALONE**

Mecta-C Stand Alone is indicated for use in patients suffering from Degenerative Disc Disease at multiple contiguous levels from C2 to T1.

#### ANGULAR STABILITY

- Divergent & Convergent screws combination
  - Increased pull-out strength
    - Enhanced in-situ primary stability

#### SIMPLICITY

Designed to simplify the surgical steps through an **easy and controlled implantation**.

Four plate configurations and angled instruments to cover different needs and **challenging anatomies**.

#### **BONE GRAFT VOLUME**

Wide central bone **graft area** may help to accelerate the occurrence of fusion through the implant.

#### **CLEAR FUSION ASSESSMENT**

- Radiolucent TiPEEK cage
- Titanium marker with limited image artifact
- Accurate reference for diagnostic assessment

#### TIPEEK TECHNOLOGY

The modular Mecta-C Stand Alone system in conjunction with the TiPEEK bioactive<sup>[1]</sup> plasma-sprayed titanium coated cages, provides value to improved stability and enhanced **fusion** rate.





# ALONE SOLUTION

## **VERSATILE SYSTEM**

Two diffferent options allow the surgeons to select the one that will best suit their patient's needs.






#### **RIGID FIXATION**

- Locking Screw & Threaded Plate for a secure rigid fixation of the construct
- One step screw lock system
- Intrinsic Antibackout system

#### **"VARIABLE" FIXATION**

- Lag Screw & Unthreaded Plate to allow micromotion and proper load distribution according to the Wolff's law<sup>[2]</sup>
- **Physiological-like support** that may lead to a stable configuration
- Easy insertion of the central **Antibackout screw** to safely fix the Lag screw

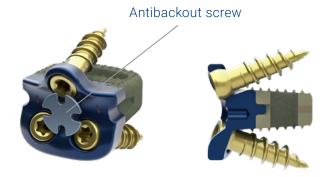


### **COMPREHENSIVE SYSTEM TO COVER DIFFERENT PATIENTS' NEEDS**

#### Footprint [WxD]



16x14 mm 18x15 mm

#### Height [mm]




5mm - 12 mm (+1mm increments)


#### Lordosis



#### SCREWS

Self-Tapping & Self-Drilling screws are avaiable both for Locking and Lag screws.








## **Mecta-C**<sup>®</sup> STAND ALONE

#### MODULAR DESIGN OFFERS FREEDOM OF CHOICE

Universal cage to plate «snap-in» concept allows 1-click construct assembly:

- Easy **intraoperative assembly** through the dedicated instrumentation
- Create an **indication-specific** interbody fusion device
- One cage fits in four plate configurations

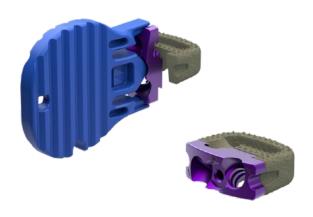

#### **MULTIPLE CONFIGURATIONS**

Reduces the risk of impingement with

surronding anatomical structures.

Best fit design for C7-T1 or C2-C3.





**TRIO** 

QUATTRO



Offers improved **Stability and Torsional Resistance**. The convergent/divergent screw trajectory minimize the adjecent level interference in multilevel fixation.

#### REFERENCES

[1] B Walsh et el. Effect of titanium coating on PEEK osteoconductivity in an ovine model, 8° M.O.R.E. International Symposium [2] H.M. Frost, Wolff's Law and bone's structural adaptations to mechanical usage: an overview for clinicians, Angled Ortho 1994

All trademarks are property of their respective owners and are registered at least in Switzerland. This document is not intended for the US market. Please verify approval of the devices described in this document with your local Medacta representative.



Medacta International Strada Regina, 34 - 6874 Castel San Pietro - Switzerland Phone +41 91 696 60 60 - Fax + 41 91 696 60 66 Info@medacta.ch - www.medacta.com

ref: 99.44CSA.11 rev.01 Last update: February 2021

Mecta-C<sup>®</sup> Leaflet



# **Mecta-C**

CERVICAL INTERVERTEBRAL BODY FUSION DEVICE









## Adecta-C

## UNIQUE PATIENTS - SPECIFIC INDICATIONS - ONE SYSTEM

Medacta Spine has developed a portfolio of spine implants that have been designed to complement one another.

The M.U.S.T. Pedicle Screw System, the MectaLIF Family of Interbody Fusion Devices and the Mecta C Plate-Cage system for cervical spine along with our suite of specialised surgical instruments, create a harmonised, single-system approach for most spine stabilisation applications.

Traditional and MIS surgical approaches are supported.

### MECTA-C CERVICAL SYSTEM

The Mecta-C family of Cervical Interbody Fusion Cages and Anterior Plates represent a complete System to fuse and mechanically support the cervical spine in case of degenerative disease, trauma, tumors and deformity.

#### **MECTA-C INTERBODY FUSION CAGES**

 Made of PEEK and Titanium coated PEEK to offer effective load sharing and optimal biocompatibility. The Ti-Peek implant is entirely coated with Titanium plasma spray coating.


- Maintain modulus of PEEK, while addressing premium acute fixation and potential for long-term osseointegration of the entire implant.
- Options for selecting footprint, lordosis and profile parameters to address patients' unique anatomical needs.
- 12x14, 12x16, 14x14, 14x16 and 15x18 footprints (Depth mm x Width mm) to provide structural support at cortical bone foundations
- Flat profile 7° lordosis for last stage of degeneration and Dome profile 5° lordosis to restore the anatomical alignment and mechanical stability for younger patients.
- Pyramidal shaped spikes to improve the primary stability and multi-dimensional pull-out resistance.
- Large central window to maximize the bone graft volume.

#### **MECTA-C ANTERIOR PLATES**

- Pre-lordosed plates to match the natural curvature of the spine and deliver secure fixation and stabilization for one, two, three and four level configurations
- Bone screw options include self-tapping or self-drilling designs, with variable and fixed angle locking to secure primary and revision surgeries (up to 20° cephalad/ caudal screw angulation)
- Advantages of a polyaxial screw with the capability to convert it into a locking screw
- Preserve the option to build Fixed, Variable and Hybrid constructs to allow optimal load sharing and stability to match the specific needs of your patient
- Low 2mm profile design to reduce soft tissue irritation
- Large window to facilitate final bone graft placement, graft visibility and to assess bone growth via post-operative imaging.







Mecta-C Leaflet 99.44C.11 rev.00 Last update: April 2014



ONE SYSTEM, MULTIPLE OPTIONS



Ô





## **44.U.S.T.** MINI


## ONE SYSTEM,

The **M.U.S.T. MINI** posterior cervical screw system is a **comprehensive solution** for fixation of the occipito-cervico-thoracic spine. The variety of screws, hooks, rods and connectors allows the surgeon to tailor the construct to the specific patient anatomy and pathology to be treated.

#### **HIGH POLY-AXIALITY**

The broad range of motion, up to 96° for the overall cone angle, eases the surgical practice in challenging anatomies.



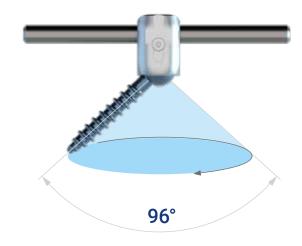

#### **UNIQUE FRICTION HEAD**

All the M.U.S.T. MINI screws have the **friction head** feature to facilitate **rod placement** and **ease** of **maneuvers** during surgery.







## MULTIPLE OPTIONS


## **COMPREHENSIVE SOLUTION**

Screws:

- Solid & Cannulated Ø3.5, 4, 4.5mm
- Full and partial threaded





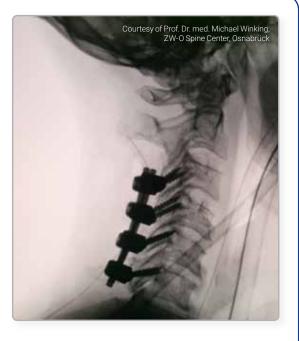

Rods:

- CoCr for superior construct stability
- Transition rods for cervico-thoracic fixation




## **ARTIFICIAL SPINOUS PROCESS**

Seating between the neck muscles allows to:

- Fix and adapt the neck muscles in the midline
- Safely secure the bone graft with soft wires
- Protect in case of spinous process removal
- Naturally reshape the posterior aspect



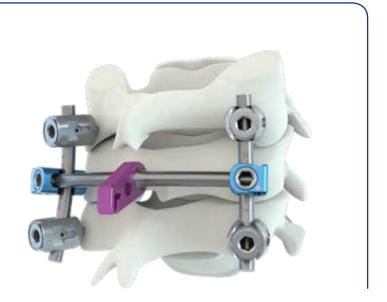




## **⊿⊿.U.S.T.** MINI

## **OCCIPITO-CERVICAL FUSION**

The Occipital Plate offers **flexibility** to extend and further **stabilise** the posterior cervical construct.

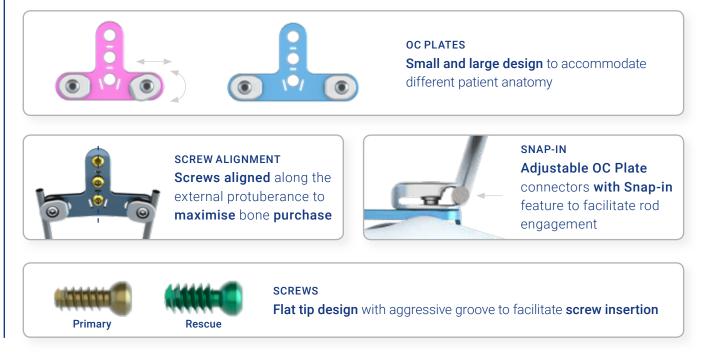

### UNIQUE SYNERGY WITH MYSPINE CERVICAL

Guided insertion of the **M.U.S.T. MINI screws** thanks to the **MySpine Cervical**, a 3D patient matched technology based on pre-operative planning designed for **pedicle screw** positioning.

- Steered pedicle screw insertion
- Increased stability vs lateral masses screws trajectory
- **Drastic reduction** in radiation exposure for patients and OR Staff





All trademarks and registered trademarks are the property of their respective owners. This document is not intended for the US market. Please verify approval of the devices described in this document with your local Medacta representative.



Medacta International Strada Regina - 6874 Castel San Pietro - Switzerland Phone +41 91 696 60 60 - Fax + 41 91 696 60 66 Info@medacta.ch - www.medacta.com M.U.S.T. Mini Leaflet ref: 99.46c.11 rev. 01 Last update: October 2018

# **JectaLIF** ANTERIOR

ANTERIOR LUMBAR INTERBODY FUSION DEVICE



Spine

## Brochure

Navigatior





## **A**dectaLIF

## MECTALIF ANTERIOR HYBRID

The MectaLIF **Hybrid** Interbody Fusion Device merges the mechanical features of the **Flush** zero anterior profile plate with the **Long** enhanced stability construct, thus providing added value in Anterior lumbar fixation.



## MECTALIF ANTERIOR HYBRID RATIONALE

The MectaLIF **Hybrid** Interbody Fusion Device provides an aided solution for L5-S1 implantation where additional stability is required and low profile construct is necessary to deal with difficult tilted anatomies.



The **Flush** caudal profile avoids impingement and irritation of the soft tissues.



The low-angle 10° screws offer easier insertion in challenging anatomies avoiding interference with the pubic symphysis. Low angle trajectory allows for screw insertion with straight instruments and a simple surgical technique.



The **Long** cranial profile provides high level stability in extension and torsion.



Diverging screws provide enhanced stability and increased pull-out strength.

REFERENCES		
Hybrid Plate Height	Ref. code	
H.12 mm	03.30.232	
H.14 mm	03.30.233	
H.16 mm	03.30.234	
H.18 mm	03.30.235	





# **JectaLIF** ANTERIOR

ANTERIOR LUMBAR INTERBODY FUSION DEVICE

00

00



## Brochure

Knee

Nav

Spine



# **AdectaLIF** ANTERIOR

## ANTERIOR LUMBAR

#### MECTALIF ANTERIOR SYSTEM, A COMPREHENSIVE SOLUTION FOR LUMBAR SPINE FUSION

#### SECURE LOCKING SYSTEM

- Controlled torque means securely locked screws with no need for a separate anti-migration system
- Threaded Titanium helps avoid cross threading
- Horizontal screw angle reduces the bending moments, preventing screw back out

#### **ANGULAR STABILITY**

- Exclusive divergent & convergent screws
- Enhanced in-situ system stability
- Increased pull-out strength



#### ENHANCED BONE GRAFT VOLUME

Large central bone graft area may help to accelerate the occurrence of fusion through the implant.

#### **TIPEEK TECHNOLOGY**

The MectaLIF Anterior system exploits Medacta's uniquely **bioactive** and **osteoconductive** Titanium coating technology.




# INTERBODY FUSION DEVICE

## EASE OF IMPLANTATION

Dedicated instruments simplify surgical steps:

- in challenging anatomies
- in cases of **extreme** spine **curvature**
- in angled L5-S1 anatomy



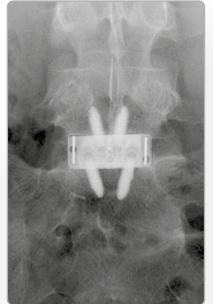




## VERSATILE OFFERING


MectaLIF Anterior cages are offered with numerous implant heights, footprints and lordoses:


- ensuring an optimal anterior / posterior support
- providing patients with the best anatomical fit
- accommodating surgeon's practice

#### FOOTPRINT [D X W]

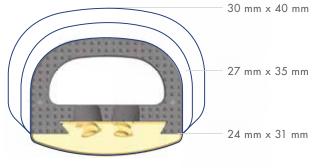

#### SCREWS LENGTHS



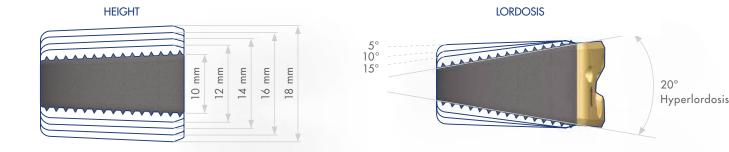



# **MectaLIF** ANTERIOR

### UNIQUE MODULARITY

Universal cage to plate "snap in" concept allows the assembly of the construct in 1-click to:

- Perform intraoperative assembly
- Create an indication-specific interbody fusion device



### MULTIPLE CONFIGURATIONS - FREEDOM OF CHOICE

ANTERIOR STAND-ALONE SOLUTIONS to cover diverse patient anatomies and surgical needs.



No anterior profile, **minimal impact**, reduced irritation



Stable solution for L5-S1 **challenging anatomy** 



**Superior stability** in extension and torsion



Flexible design for the iliac artery bifurcation



Offset profile, minimize vessels manipulation



All trademarks and registered trademarks are the property of their respective owners







# **A**ectaLIF

INTERVERTEBRAL BODY FUSION DEVICE



## Brochure

nee

Spine

Navigat





## **A**dectaLIF

### MEDACTA INTERNATIONAL

The foundation of Medacta International is built upon world-class hip and knee arthroplasty technology and leadership by the family Siccardi and a dedicated team of talented professionals based in Lugano, Switzerland.

The company began in the year 2000, and has proceeded on an accelerated growth curve that reflects our Customer's appreciation for Quality, Innovation and Service.

Bringing Swiss precision and engineering to the Spine Specialists, Medacta Spine, founded in 2009, is moving forward globally to deliver surgical technology solutions for degenerative, deformity and trauma/oncology indications through traditional open and MIS surgical approaches.


Medacta International has achieved FDA approval of a number of unique and effective spine implants. An active pipeline of technology development is being validated in worldwide markets and utlimately planned for eventual availability in the United States. Until then, we are proud to represent posterior and anterior fixation options designed with an important Philosophy: Unique Patients - Specific Indications - One System.

#### MECTALIF OLIF, TLIF AND PLIF FUSION DEVICES

The MectaLIF Family of Interbody Fusion Devices are shaped for solid initial fixation, and long term spine stabilization. Made of PEEK and Titanium coated PEEK material, the MectaLIF Fusion Devices offer biocompatibility and anatomic shaping to address your unique patients.

- Each implant features a chamfered leading edge for effective interbody distraction and less effort upon insertion.
- A variety of interbody heights, lordotic angles and footprints allow significant options when selecting the correct implant for your unique patients with bi-cortical bridging.
- Large autograft windows allow the delivery of significant volumes of bone to support bone growth through the cages.

\* The MectaLIF implants in combination with supplemental fixation are indicated for use with autogenous bone graft in patients with degenerative disc disease at one or two contiguous spinal levels from L2 – S1 whose condition requires the use of interbody fusion.

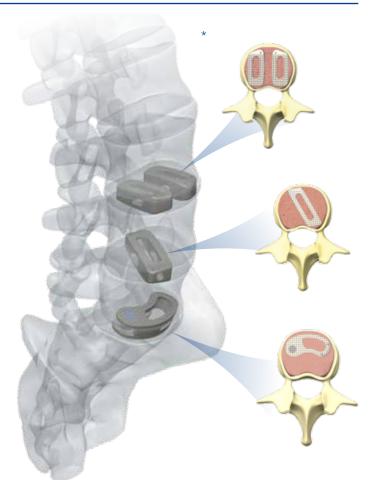



MectaLIF Leaflet 99.44pot.11 rev.00 Last update: September 2013

# **11.U.S.T.**

MEDACTA UNCONSTRAINED SCREW TECHNOLOGY



## Brochure

Spine

Navigation





## **⊿**⊿.U.S.T.

## UNIQUE PATIENTS - SPECIFIC INDICATIONS - ONE SYSTEM

Medacta Spine has developed a portfolio of spine implants designed to complement one another.

The M.U.S.T. Pedicle Screw System, the MectaLIF Family of Interbody Fusion Devices and our Suite of Specialized Surgical Instruments create a harmonized, single-system approach for most spine stabilization applications.

Traditional and MIS surgical approaches are supported.



#### M.U.S.T. PEDICLE SCREW SYSTEM

The M.U.S.T. Pedicle Screw System is an unconstrained polyaxial screw, rod & connector design applicable to degenerative, deformity and trauma indications using traditional open or MIS (mini-open) surgical approaches.

- Ultimate Versatility in One System.
- Ability to lock polyaxial head without in-situ rod to create monaxial rigidity for parallel compression/distraction.
- Pre-sterilized implants increase logistic efficiencies and reduce hospital preparation.
- Dual-thread lead advances screw with control and speed.
- Specialized enabling instruments for rod reduction and set-screw threading.
- Polyaxial and monoaxial in solid and cannulated versions.
- Range of diameters available to cover the thoracic, lumbar, sacral and sacro-iliac fixation needs.
- M.U.S.T. Link Cross Connectors provide an easy-to-use option to improve the stabilisation of the treated spine.





# **AUUST.** SI SACRO-ILIAC JOINT SCREW SYSTEM

A COMPLETE SYSTEM WITH DIFFERENT OPTIONS



Brochure


Spine



## **4.U.S.T.** SI

The M.U.S.T. SI, Medacta Universal Screw Technology Sacro Iliac System, is intended for sacroiliac joint fusion of skeletally mature patients suffering from sacroiliac **joint disruptions**, degenerative **sacroiliitis** and degenerative sacroiliac **arthritis**, secondary to pelvic disruption.

#### **IMPLANT FEATURES**

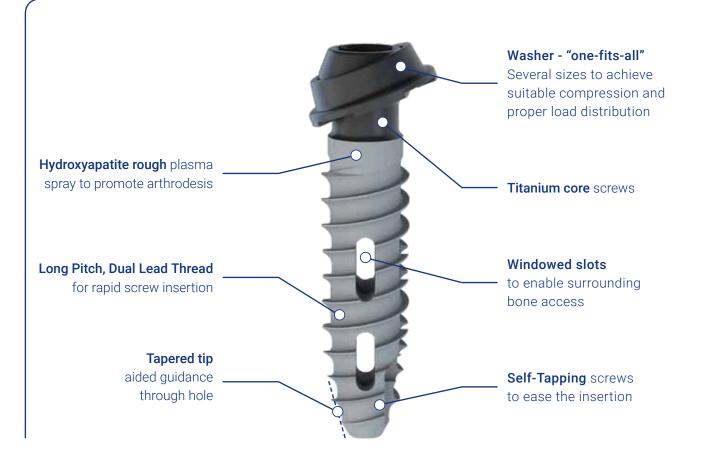

#### **PRODUCT RANGE**









UNIQUE ANATOMIES PATIENT-MATCHED SOLUTIONS

10 a

0

3



		Brochure
Joint	Spine	Sports Med
	S2-AL	AR/ALAR-ILIAC






#### S2-ALAR-ILIAC TECHNIQUE

**MySpine S2AI** is the Medacta Patient-Specific Solution for **S2-Alar-Iliac fixation**: a **minimally invasive** solution at surgeon's hand for long constructs, designed to overcome the limits of a potentially insufficient lower spine fixation.

The S2-Alar-Iliac technique represents a valid solution since the trajectory crosses 5 cortical bone structures, resulting in a **strong bone fixation**, while the medial entry points **reduce** the need of **muscle dissection** leading to<sup>[5]</sup>:

- Reduced screw loosening rate<sup>[5]</sup>\*
- Lower incidence of Sacro-Iliac Joint pain<sup>[5]</sup>\*
- Small incision<sup>[5]</sup>
- Less dissection<sup>[5]</sup>\*

\*compared with alternative lumbosacral instrumentations (S2-Alar and Iliac screws)

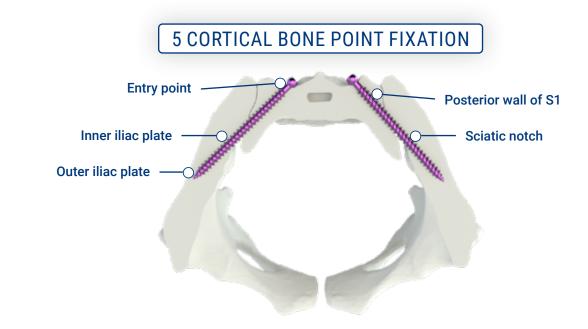



Prominent conventional **lliac screws** may lead to **irritation** and **pain** with **high revision rate.**<sup>[2,5]</sup>

#### **MYSPINE IS DIFFERENT!**

MySpine guided S2-Alar-Iliac trajectory may allow for a small incision and less lateral retraction, and the medial entry point allows for a **quick** rod connection, thus eliminating the need for additional connectors.<sup>[5]</sup>



## PATIENT-MATCHED SOLUTIONS

## **MYSPINE S2AI VALUE PROPOSITION**

**MySpine** is a **personalized surgical platform** that is **cost effective, efficient** and **intuitive**. MySpine provides pre-op planning, single-use patient-specific drill guides and intra-operative surgical plan.

MySpine S2AI Pre-Op Plan



MySpine S2AI 3D Planning

MySpine S2AI can be used in those treatments where strong bone fixation is required, as it may provide<sup>[1]</sup>:

- Robust bone anchor and improved pelvic tilt correction in Adult Spine Deformity
- Spine balance recovery in rigid neuromuscular Adolescent Idiopathic Scoliosis
- Added value in fixing fractured segments


The guided technique leads to **precise screw placement**, comparable to that offered by gold standard navigation tools, while **reducing the radiation exposure and the surgical time.**<sup>[3,4]</sup>







#### THE MYSPINE JOURNEY

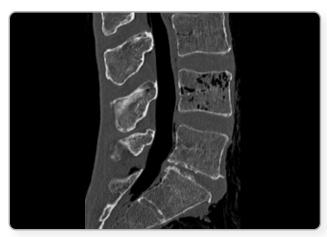

**1. IMAGE ACQUISITION** Low Dose CT scan to deliver 3D reconstructed vertebrae and the pelvic region



2. 3D PRE-OP PLAN MANAGEMENT The surgeon defines optimal implant parameters



**3. 3D PRINTING** Patient-matched Jigs are sent to the hospital



**4. PROCTORED SURGERY** An experienced surgeon will support you during your first cases

#### REFERENCES

Sponseller P. et al., "Low Profile Pelvic Fixation With the Sacral Alar Iliac Technique in the Pediatric Population Improves Results at Two-Year Minimum Follow-up", Spine, September 15, 2010
 Emami A. et al., "Outcome and Complications of Long Fusions to the Sacrum in Adult Spine Deformity: Luque-Galveston, Combined Iliac and Sacral Screws, and Sacral Fixation", Spine, April 1, 2002
 Matsukawa K. et al., Accuracy of cortical bone trajectory screw placement using gatient-specific template guide system, Neurosurgical Review, July 2019
 Matsukawa K. et al., Cortical pedicle screw trajectory technique using 3D printed patient-specific-guide, M.O.R.E. Journal, September 2018
 Kreig S. et al., "Revision by S2-alar-liac instrumentation reduces caudal screw lossening while improving sacroliac joint pain – a group comparison", Neurosurgical Review, September 2020 study

All trademarks are property of their respective owners and are registered at least in Switzerland. This document is not intended for the US market. Please verify approval of the devices described in this document with your local Medacta representative.



Medacta International Strada Regina, 34 - 6874 Castel San Pietro - Switzerland Phone +41 91 696 60 60 - Fax + 41 91 696 60 66 Info@medacta.ch - www.medacta.com MySpine<sup>®</sup> S2AI Leaflet ref: 99.MY46S2AI.11 rev.00 Last update: November 2020



# **1.U.S.T.** MIS SYSTEM

ç • Ç ;

MINIMALLY INVASIVE SOLUTIONS

M.I.S. MAKE IT SMART IN ONE SYSTEM



Spine

1




# M.I.S. MAKE IT

# **44.U.S.T.** MIS SYSTEM

The **MUST MIS System** represents an effective and harmonic concept in terms of minimally invasive solutions. The MIS system is composed of:

- an innovative mini open retractor
- a percutaneous system
- TLIF and PLIF cages with dedicated MIS Instruments

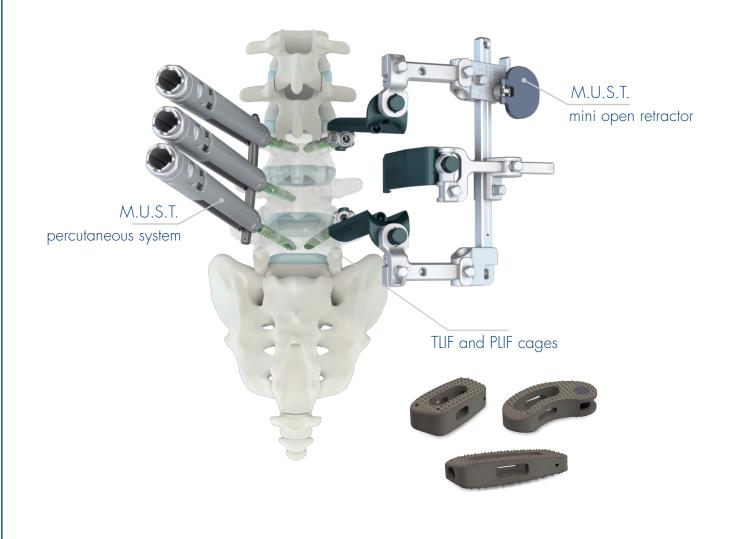

A small incision, a gentle interface with soft tissues and an atraumatic technique may offer **valuable benefits to the patient**:

- Small incisions
- Reduced blood loss <sup>[1]</sup>
- Reduced site infection risks <sup>[3]</sup>
- Potential reduced vascular disruption
- Minimised soft tissue and muscle damages <sup>[2]</sup>
- Reduced post-op analgesic therapy [1]
- Minimum scar
- Improved recovery <sup>[1]</sup>
- Rapid hospital discharge <sup>[2]</sup>



# SMART IN ONE SYSTEM

# **4.U.S.T.** MINI OPEN

#### Specifically designed retractor for:

- decompression
- fusion and fixation
- optimal TLIF and PLIF cage placement with a comprehensive system of dedicated MIS instruments



**On the patient's side** Small incision, Large visualization

Low profile frame with ergonomic and radiolucent blade design to provide better visual exposure with dedicated light cables for optimal site illumination.

# **4.U.S.T.** PERCUTANEOUS


A further step in the development of the well-established MIS approach. The Medacta MIS system relies on a dedicated **MUST screw-based platform** assuring **superior stability**. Slim Percutaneous tubes provide **atraumatic access**.



An **effective** tool in MIS treatments



#### **ROBUST CONNECTION**



A dedicated blade-to-screw connector gives the polyaxial screw monoaxial function, allowing for **direct and effective distraction of the vertebral bodies**.

Optimal application for minimally invasive PLIF Insertion and Wiltse TLIF approach with **TiPEEK** interbody fusion technology.

### ENHANCED BONE CONTACT IN MIS SURGERIES

Optimal application for minimally invasive PLIF Insertion and Wiltse TLIF approach with **TiPEEK** interbody fusion technology.

#### **High fusion rate, low subsidence** for accelerated fusion<sup>[1]</sup> & fast bone remodelling<sup>[4]</sup>

**Disc height preservation** for a substantial restoration of interbody height and lordosis<sup>[1]</sup>

Improved stability With an effective rough surface

Easy and clear fusion assessment TiPEEK cages are compatible with diagnostic bio-imaging techniques



#### REFERENCES

[1] S. Chusheng et al. Five-Year Outcomes of Minimally Invasive Versus Open Transforaminal Lumbar Interbody Fusion: A Matched-Pair Comparison Study. Spine. 38(23):2049-2055, November 01, 2013, [2] Lee KH et al. Clinical and radiological outcomes of open versus minimally invasive transforaminal lumbar interbody fusion. Eur Spine J. 2012 Nov;21(11):2265-70. [3] McGirt et al. J Neurosurg Spine. 2011 Jun;14(b):771-8 Comparative analysis of perioperative surgical site infection after minimally invasive versus open posterior/transforaminal lumbar interbody fusion: analysis of hospital billing and discharge data from 5170 patients.[3] M.Rickert et al. Transforaminal lumbar interbody fusion in PEEK oblique cages with and without titanium coating: results from a randomized clinical trial [4] B.Walsh et al.

All trademarks and registered trademarks are the property of their respective owners.

swiss made

Medacta International Strada Regina - 6874 Castel San Pietro - Switzerland Phone +41 91 696 60 60 - Fax + 41 91 696 60 66 Info@medacta.ch - www.medacta.com M.U.S.T. MIS System 99.46MIS.11 rev. 00 Last update: April 2017





# **MYSPINE**:

# A new technology to reduce radiation exposure while maintaining high accuracy





The tools and instruments used in spine surgery are continuously changing and improving. It has been shown and is accepted that the use of a navigation system is an extremely valuable tool in determining the **appropriate placement of pedicle screws**.

Everyone is exposed to natural radiation from food, water, radon gas, cosmic rays, and other naturally occurring radioactive materials resulting in an annual effective dose of approximately 3 mSv <sup>[e]</sup>. With the use of any ionizing radiation, such as x-ray, there are risks to the patient and to the staff in the operating room. Additional radiation from medical imaging augments the already present **risks of radiation-induced adverse consequences**, such as cancer, birth defects, and other deleterious occurrences.

## PATIENT WISE

- +91% of breast cancer reported in women exposed to multiple diagnostic x rays <sup>[h]</sup> vs. normal population
- +8% risk of mortality among patients frequently exposed to radiographic exams <sup>[]</sup> vs. normal population

## SURGEON WISE

- +190% risk of breast cancer reported in orthopedic surgeons vs. normal population <sup>[k]</sup>
- +100% risk of all cancer reported in orthopedic surgeons vs. normal population <sup>[k]</sup>

There are measures that are taken to reduce the risk of radiation exposure, lead shields to cover the torso and neck, protective gloves and eye shields, and maintaining a safe distance from the radiation source. Even with appropriate measures taken, **the surgeon and the staff are still at risk of exposure from scatter radiation**. The newest imaging modalities such as the O-Arm<sup>™</sup>, have provided benefits, by utilizing intraoperative acquisition of 2D and 3D images of the spine and potentially allowing better placement of pedicle screws. However, these technologies are not without additional risks to the patient and operating room staff.

The effective dose limit for a non-occupationally exposed individual is 1 mSv per year above the background radiation dose of 3 mSv <sup>[e]</sup>. During a single O-Arm<sup>™</sup> image acquisition, **the patient is exposed to an effective dose up to 81 mSv, a value over the documented annual dose limit** <sup>[b]</sup>. This can be over 50 times the regulated dose limit for a non-radiation worker.

Though the risks of intraoperative radiation exposure to surgeons and staff are well documented within the peer reviewed literature, the perceived benefit in the accuracy of screw placement has made the use of intraoperative fluoroscopy and other sources of ionizing radiation in the operating room a fundamental requirement. The development of technologies to increase **surgical accuracy**, **reducing operative times**, and **improving outcomes** are the collaborative goals with industry and healthcare professionals. New instruments to aid in screw placement, imaging tools, and robotics have all been introduced in the last years with the goal of improving screw placement. Some of the most valuable tools, new imaging modalities and robotics, require a large capital investment for the facilities and therefore these options may not be available to all users.




# MySpine Patient-Matched Technology by Medacta

**MySpine technology** utilizes a **low dose CT scan** of the patient's spine to create **patient specific instruments** designed and manufactured with the express intent of increasing accuracy when placing pedicle screws, thus reducing the need for the use of intra-operative fluoroscopy to confirm the appropriate placement of screws. The risks of exposure to high doses of radiation to both the patient and the surgical team can potentially be reduced through the utilization of this technology.

A patient who has been identified as needing a posterior, thoracolumbar fusion, is sent to a scanning facility and a low dose CT scan of their spine is performed. The data from this scan is transmitted securely to the manufacturer. The patient's anatomy is reconstructed and a **surgical plan is reviewed and approved by the surgeon**, determining the appropriate screw diameter, length and trajectory within the pedicle. 3D printed surgical guides are then created and provided for intraoperative use during the posterior fusion.

The figure below shows a comparison of radiation doses to the patient from different modalities in comparison to the MySpine technology.

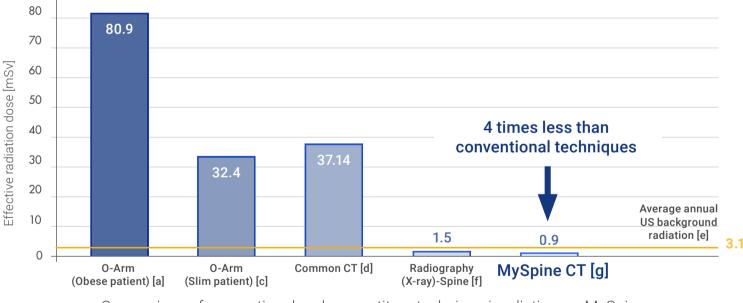

## MySpine is Safe for both OR Staff and Patients!

Comparison of conventional and competitors technique irradiation vs. MySpine

The accuracy of MySpine technology is proven in a clinical study of pedicle screw placement utilizing post implantation CT scans. [1]

A total of **198 screws** were implanted, out of these **99.5%** were inserted in the safe zone. This result is comparable (or even better) to the values of robotic (97.8%) and navigated assisted techniques (95.6%) and greater than the traditional freehand approach (80%).



# Conclusions



The pedicle screw is one of the spine surgeon's most commonly used tools, but its widespread prevalence doesn't make its proper placement any less challenging. The practice remains technically demanding, with a very small margin for error.

In order to assist the surgeons to accurately position the pedicle screws, intraoperative-based utilization of X-ray imaging tools and technologies have been successfully introduced. However these technologies expose the patient and the Operating Room team to the health risks associated with increased radiation exposure.

Recently introduced MySpine technology supports spine surgeons during the critical steps of pedicle screw placement by offering the potential for improved accuracy, as well as reduced radiation exposure.



# Bibliography

<sup>[ac]</sup> Lange et.al. "Estimating the effective radiation dose imparted to patients by intraoperative cone-beam computed tomography in thoracolumbar spinal surgery" Spine 2013 <sup>[b]</sup> US Nuclear Regulatory Commission's (USNRC) <sup>[d]</sup> Biswas et.al. "Radiation Exposure from Musculoskeletal Computerized Tomographic Scans" JBJS Am. 2009 <sup>[e]</sup> Health Physics Society Specialists in Radiation Safety, Lawrence Berkeley National Laboratory; Fact Sheet 2010 <sup>[f]</sup> Radiation Dose in X-Ray and CT Exams; 2013 Radiological Society of North America, Inc <sup>[g]</sup> MySpine, Charité University Hospital, Berlin, Germany. Data on internal file - Medacta <sup>[h]</sup> Hoffman DA et al. "Breast cancer in women with scoliosis exposed to multiple diagnostic x rays" J Natl Cancer Inst. 1989 Sep 6; 81(17):1307-12 <sup>[I]</sup> Cécile M. Ronckers et al. « Cancer mortality among women frequently exposed to radiographic exams for spinal disorders" Radiat Res. 2010 Jul; 174(1): 83–90. <sup>[k]</sup> Chou et al. "Prevalence of Cancer in Female Orthopaedic Surgeons in the United States" Journal of Bone & Joint Surgery, American Volume; Jan2010, Vol. 92-A Issue 1, p240 <sup>[I]</sup> Matsukawa K. et al., Accuracy of cortical bone trajectory screw placement using patient-specific template guide system, Neurosurgical Review, July 2019



PATIENT MATCHED TECHNOLOGY IN SPINE SURGERY

UNIQUE ANATOMIES PATIENT-MATCHED SOLUTIONS







# UNIQUE ANATOMIES PATIENT-MATCHED SOLUTIONS

MySpine is a tailor made patient specific spine vertebrae guide, created to lead the surgeon through the critical steps of accurate pedicle screw placement whilst reducing the surgical time and intra-operative X-ray radiation.

### **REAL PATIENT MATCHED INSTRUMENTATION**

MySpine Pedicle Screw Placement guides are developed specifically for each patient.

#### COMPREHENSIVE

- Standard MySpine guides are suitable for challenging deformities and long constructs.
- Low Profile MySpine guides are ideal for degenerative cases.

### AT THE SURGEON'S HAND

The surgeon determines the entry points for the pedicle screws, and sets their trajectory along with the main geometrical parameters.



STANDARD VERSION



#### LOW PROFILE VERSION K-WIRE BASED

## MYSPINE CASE MANAGEMENT

Online interactive 3D planning tool for reliable pedicle targeting and screw trajectory identification.

#### ONLINE CASE MANAGEMENT

MySpine cases are managed entirely online with no need to install additional software. The case database is available to the surgeon anytime and anywhere. The information on the website is always kept up-to-date.

#### COMPLETE IN-HOUSE TECHNOLOGY


The MySpine process is kept entirely in-house from the 3D anatomical reconstruction to the manufacturing of the guides, allowing a direct contact between the surgeon and the MySpine team.

### ONLY 3 WEEKS LEAD TIME

The shortest delivery time in today's market for this technology.


### A PERSONAL MYSPINE TECHNICIAN JUST FOR YOU

Each surgeon is assigned a personal MySpine technician to assist with any questions or concerns.

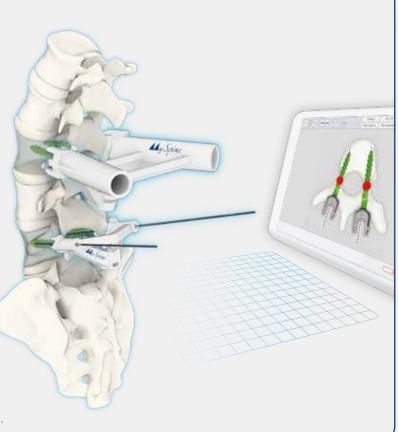


# UNIQUE ANATOMIES PATIENT-MATCHED

# ACCURATE SCREW POSITIONING

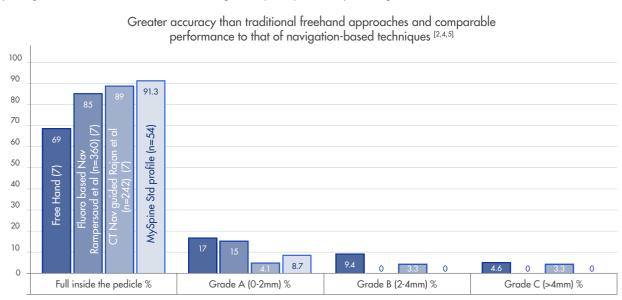

The MySpine guides are made to match the surgeon's pre-operative planning.

Up to 100% of pedicle screws correctly placed within the 2mm breach zone within the pedicle [1,2, 3] as per the pre-operative planning instructions.

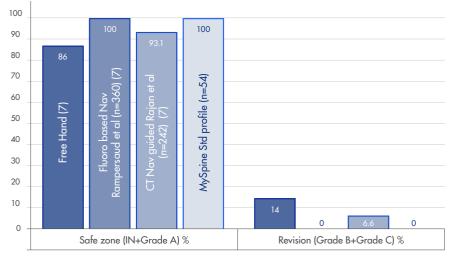

## OUTSTANDING PERFORMANCE

#### **REPRODUCIBLE SURGICAL TECHNIQUE**

The MySpine technology, along with the M.U.S.T. Pedicle Screw System, leads to a more accurate screw positioning for both junior and expert surgeons<sup>[6]</sup>.

#### SIGNIFICANT REDUCTION IN THE SURGERY TIME

Substantial results in terms of screw positioning mean time have been achieved with the MySpine technique; the overall time is reduced about 30% vs free hand technique<sup>[6]</sup>.

#### SIGNIFICANT REDUCTION IN THE HOSPITAL STAY

From the patient side, potential reduction in the post-operative morbidity and shortened length of hospital stay<sup>[4]</sup> is a direct advantage of the MySpine technology.



# SOLUTIONS

## **COST SAVING**

Reducing treatment costs is crucial for all Hospitals. To this end, the MySpine system is a good tool to act on the following:

- Improving screw positioning may result in reducing the number of revision surgeries.
   Literature data show that misplaced screws range from 1 to 5% of the total number<sup>[8]</sup>. A revision surgery has been calculated to cost between \$18,000 and \$28,000<sup>[8]</sup>.
- Reducing surgery time.


In a cadaver experiment, template-guided pedicle screw placement was measured to be faster<sup>[6]</sup>. According to the above-mentioned study, the cost of an active Operative Room was measured to be worth \$93 per minute. Higher accuracy can therefore be coupled with lower expenditure.

 No capital investment. Unlike navigation systems, MySpine technology does not require any capital investment.

## **REDUCED X-RAY DOSE**

A dedicated MySpine Low Dose CT protocol has been developed in order to minimize the X-ray exposure for the patient, moreover MySpine pedicle screw placement potentially allows a reduction of intraoperative fluoroscopy without sacrificing accuracy<sup>[6]</sup>.

- Low dose radiation protocol allows for dramatic dose reduction to patients than using C-Arm or O-Arm technologies: more than 30 times less irradiation! (c).
- Overall radiation dose per surgery is up to 50 full spine X-rays less than the free-hand technique (data on internal files)

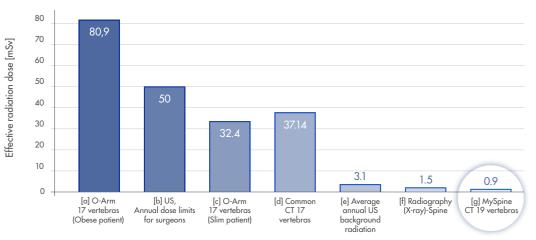

#### MySpine is Safe for both OR Staff and Patients!

[a] Lange et.al. Estimating the effective radiation dose imparted to patients by intraoperative cone-beam computed tomography in toracolumbar spinal surgery, Spine 2013 [b] US Nuclear Regulatory Commission's (USNRC) [c] Lange et.al. Estimating the effective radiation dose imparted to patients by intraoperative cone-beam computed tomography in toracolumbar spinal surgery, Spine 2013 [d] Biswas et.al. Radiation Exposure from Musculoskeletal Computerized Tomographic Scans, JBJS Am. 2009 [e] Health Physics Society Specialists in Radiation Scatery, Lawrence Berkeley National Laboratory; Fact Sheet 2010 [f] Radiation Dose in XRay and CT Exams; 2013 Radiological Society of North America, Inc [g] MySpine, Charité University Hospital, Berlin, Germany

Comparison of conventional and competitors technique irradiation vs. MySpine





## **TECHNICAL FEATURES**

The MySpine Pedicle Screw Placement guides are made to match the individual patient's anatomy.


#### **MAXIMIZED STABILITY**

MySpine guides are positioned on the vertebra using distinct references, such as the spinous and transverse processes, in order to achieve the maximum stability.





The MySpine guides are designed to preserve the patient's anatomy.

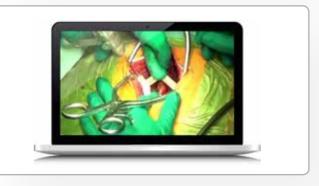



#### **MAXIMIZED VISIBILITY**

Distal windows enhance the field of view during all surgical steps.

## REFERENCES

[1] Lamartina et al. Adolescent idiopathic scoliosis surgery with patient-specific screw placement-guide Eur Spine J. 2014 Dec;23(12). MySPINE VIDEO CASE / REDUCED DOSE RADIATION
 [2] Lamartina et al. Pedicle screw placement accuracy in thoracic and lumbar spinal surgery with a patient-matched targeting guide: a cadaveric study. Eur Spine J. 2015 Nov;24(7).
 MySPINE ACCURACY VS FREE HAND

MySPINE ACCURACY VS FREE HAND [3] Putzier et al. A New Navigational Tool for Pedicle Screw Placement in Patients with Severe scoliosis: A Pilot Study to Prove Feasibility, Accuracy, and Identify Operative Challenges. J Spinal Disord Tech. 2014 MySPINE PILOT STUDY [4] Landi et al. Spinal Neuronavigation and 3D-Printed Tubular Guide for Pedicle Screw Placement: A Really New Tool to Improve Safety and Accuracy of the Surgical Technique? J Spine 2015, 4:5 MySPINE ACCURACY VS GUIDED TECHNIQUE

[5] Landi et al. 3D Printed Tubular Guides for Pedicle Screw Placement: The Answer for the Need of a Greater Accuracy in Spinal Stabilization. Orthop Muscular Syst 2015, 4:3 MySPINE ACCURACY / EASE OF USE [6] Farshoel v Libe of out [6] Farshoel et. al. Accuracy of patient-specific template-guided vs. free-hand fluoroscopically controlled pedicle screw placement in the thoracic and lumbar spine: a randomized cadaveric study. Eur Spine J. 2016


[7] Gelalis et.al. Accuracy of pedicle screw placement: a systematic review of prospective in vivo studies comparing free hand, fluoroscopy guidance and navigation technique. Euro Spine nal 2012

181 Landi et al. Pedicle screw placement accuracy with patient-matched targeting guides: a cadaveric study and first clinical experiences. 8th M.O.R.E. International Symposium, LUGANO APRIL 22-23 2016





## THE MYSPINE JOURNEY



**1.** Medacta receives the CT scan of the patient's spine.



**2.** MySpine pre-operative planning commences with the 3D reconstruction of the spine.



 Following the surgeon's preferences, virtual positioning of the implants is proposed. This planning can be modified if required.



**4.** Once the planning has been validated by the surgeon, the in-house manufacturing process starts.

## MYSPINE EDUCATION PROGRAM

The M.O.R.E. Institute has created a comprehensive Education Program which supports the surgeon in the application of the MySpine system through:

#### Reference Center

You will have the opportunity to visit a Reference Center and attend live MySpine surgeries.

#### Learning Center

The Learning Center offers the opportunity to attend a MySpine workshop, meet experienced surgeons and discuss the clinical and economic benefits of the MySpine technology.

#### Support

Upon request, you will receive the assistance of an experienced Reference Surgeon to attend your first surgery in your own hospital.

#### Continuous Education

You can continue your education through MySpine user meetings, M.O.R.E. International events, Reference Center visits and other educational tools.

# Designed for you by you!

Simply contact Medacta and we will create an Education Program for you!

All trademarks and registered trademarks are the property of their respective owners.









MINIMALLY INVASIVE PATIENT-MATCHED SOLUTIONS







# MINIMALLY INVASIVE PATIENT-MATCHED SOLUTIONS

MySpine MC is a **3D printed** patient-matched solution in the **midline cortical** approach. Posterior lumbar fusion is performed in a **minimally invasive**, muscle sparing way, allowing for shorter operating times and a substantial reduction of both radiation exposure and costs.

- MINIMALLY INVASIVE
- EXCELLENT CLINICAL OUTCOMES
- HIGH EFFICIENCY

*y Spine* MC

• LOW RADIATION DOSE

The goal of MySpine MC is to combine an **excellent fusion rate** with **greater predictability** of the clinical outcomes.




MySpine MC - Midline Cortical

## **EXCELLENT CLINICAL OUTCOMES**

MySpine MC provides **highly precise implant positioning** which:

- allow accurate positioning of entry points in the the pars interarticularis with favourable cortical bone purchase<sup>[4]</sup>
- may enable the use of **longer screws** and **larger diameters** than CBT free hand <sup>[5]</sup>
- may lead to uncompromised fusion rate [6]

Moreover, the pre-operative trajectory management may **reduce the risk of nerve root injury**<sup>[7]</sup>

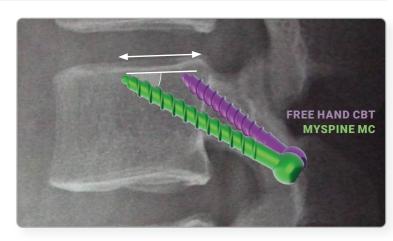




# PERSONALIZED MIS SOLUTION

# WHY A MYSPINE MC MINIMALLY INVASIVE SURGERY?

Thanks to its muscle sparing technique, the erector spinae muscles are gently manipulated and a **small skin incision** of 4-5cm is performed.

For this reason, MySpine MC delivers a **minimally disruptive surgery**, which is fundamental to drive a **fast patient recovery**. MySpine MC will **improve the patients' quality of life** and **hasten their recovery** after a spinal fusion surgery.

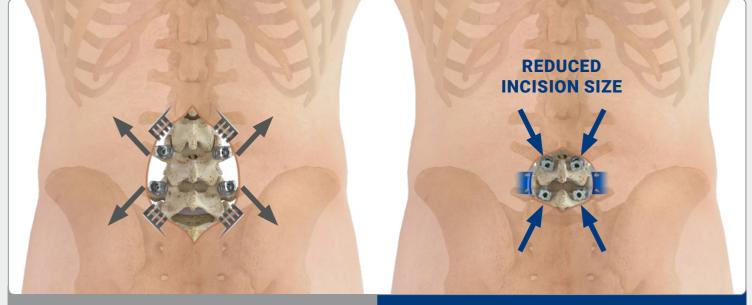

CONVENTIONAL APPROACH

**MIS MYSPINE MC APPROACH** 

# From Minimally Invasive Surgery to Personalized Medicine

and beyond

## **HIGH EFFICIENCY**

## **ECONOMIC EFFICIENCY**

- No expensive capital investment is required
- No recurrent service cost
- Rapid Learning Curve for effective accuracy
- Outpatient Surgery: hospital can potentially capitalize on resources and increase volumes as patients return home the same day of the surgery<sup>[12]</sup>



### DECREASED POST-OPERATIVE PAIN

In comparison with "conventional" open surgical techniques, the MySpine MC approach may reduce the postoperative pain thanks to a less invasive technique. [16,17] ODI index at 12 months is reduced by 18% more than conventional technique, leading to a better patient clinical score.

#### SHORTER REHABILITATION

While not violating the neuro-muscular structures, the MySpine MC technique may decrease the muscular atrophy leading to a **shorter rehabilitation**. <sup>[16,17]</sup>

"My patients can walk autonomously the day after the surgery." MD N. Marengo, Italy

#### SHORTER HOSPITAL STAY

The MySpine MC technique usually significantly reduces the duration of the hospital stay by 37%. [13] "MySpine MC is a **Minimally Invasive** technique proven to be successful in **Outpatient Setting**." MD I. LaMotta, USA

### SMALL SKIN INCISION

With MySpine MC, the skin incision is often shorter than with "conventional" open surgery and therefore scar tissue is reduced, guaranteeing an easier soft tissue handling and a more "cosmetic" procedure. [16,17]

## FASTER RETURN TO DAILY ACTIVITIES

The MySpine MC 3D Printed Patient-Specific Solution may provide better biomechanical performance, allowing for an improved long-term outcome. [15,16,17]

"At 6-month follow-up, our patients show important clinical improvements, without new neurologic deficits or radiologic pathologic findings." MD K. Matsukawa, Japan

### LESS BLOOD LOSS

Preservation of muscles and vessels may reduce blood loss, -16% compared to conventional open access surgery, for more conservative treatments. [16,17]

## **REDUCED COMPLICATIONS**

The MySpine MC technique significantly reduces the incidence of complications, when compared to free-hand techniques, because of the highly accurate implant positioning. [13,14]

"In our specific setting, the same surgical team reduced complications from 16% using the free-hand technique to 0% with MySpine MC." MD S. Petrone, MD N. Marengo et al., Italy

### TIME EFFICIENCY

- No peri-operative image acquisition, thanks to the accurate pre-op planning<sup>[11]</sup>
- Compared to free-hand CBT, the MIS MySpine MC technique leads to a significant 34% reduction of procedural time<sup>[13]</sup>






















# LOW RADIATION DOSE

- Patients are exposed to a low dose pre-op CT scan, resulting in a lower radiation exposure than a single full spine x-ray
- Pre-operative planning potentially **eliminates the need of intra-operative checks**, with a dramatic reduction of irradiation **-33%** compared to the free-hand technique <sup>[11,13]</sup>
- The cumulative dose is potentially reduced with respect to navigation-assisted technique

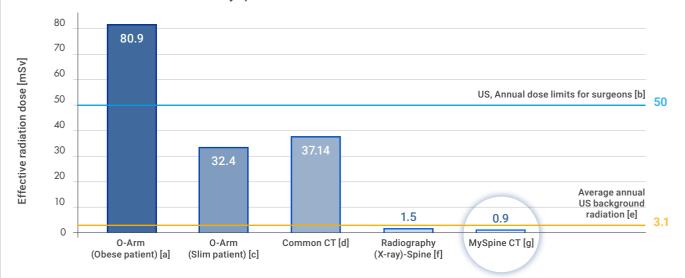


#### MySpine is Safe for both OR Staff and Patients!

#### Comparison of irradiation between conventional and competitors' techniques and MySpine

[a] Lange et.al. Estimating the effective radiation dose imparted to patients by intraoperative cone-beam computed tomography in toracolumbar spinal surgery, Spine 2013 [b] US Nuclear Regulatory Commission's (USNRC) [c] Lange et.al. Estimating the effective radiation dose imparted to patients by intraoperative cone-beam computed tomography in toracolumbar spinal surgery, Spine 2013 [b] US Nuclear Regulatory Commission's (USNRC) [c] Lange et.al. Estimating the effective radiation dose imparted to patients by intraoperative cone-beam computed tomography in toracolumbar spinal surgery, Spine 2013 [d] Biswas et.al. Radiation Exposure from Musculoskeletal Computerized Tomographic Scans, JBJS Am. 2009 [e] Health Physics Society Specialists in Radiation Safety, Lawrence Berkeley National Laboratory, Fact Sheet 2010 [f] Radiation Dose in X-Ray and CT Exams; 2013 Radiological Society of North America, Inc [g] MySpine, Charté University Hospital, Berlin, Germany

## ACCURATE PRE-OP PLANNING

The MySpine Web Platform allows for a **simple** and **accurate 3D pre-operative planning**. The surgeon can simulate the final screw position in the patient's medical images and **preview any potential surgical critical aspects**.

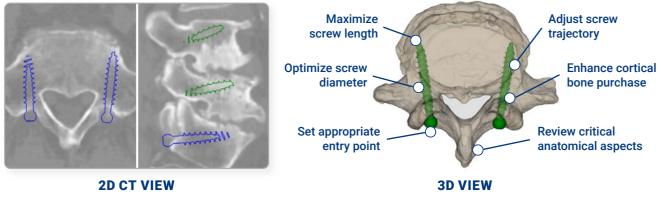



An effective tool for a personalized surgical planning.





## **MYSPINE CASE MANAGEMENT**





CT BASED SEGMENTATION

**3D ANATOMY** 

#### **1. IMAGE ACOUISITION**

Low Dose CT scan to deliver 3D reconstruction of each patient's vertebral anatomy



**3. 3D PRINTING MYSPINE MC** 3D patient-matched Jigs are sent to the hospital



2. 3D PRE-OP PLAN MANAGEMENT The surgeon defines optimal implant parameters: screw diameter, length and trajectory



4. MYSPINE MC MIS SURGERY Surgery with dedicated MySpine MC system

## REFERENCES

- Matsukawa K. et al., Incidence and Risk Factors of Adjacent Cranial Facet Joint Violation Following Pedicle Screw Insertion Using Cortical Bone Trajectory Technique, Spine, 2016
   Sakaura H. et al., Posterior lumbar interbody fusion with cortical bone trajectory screw fixation versus posterior lumbar interbody fusion using traditional pedicle screw fixation for degenerative
- lumbar spondylolisthesis: a comparative study, JNS, 2016 [3] Khanna N. et al, Spine (Phila Pa 1976). 2016 Apr;41 Suppl 8:S90-6. doi: 10.1097/BRS.00000000001475. Medialized, Muscle-Splitting Approach for Posterior Lumbar Interbody Fusion:
- Technique and Multicenter Perioperative Results
  [4] Gautschi O. et al., Maximal access surgery for posterior lumbar inter body fusion (PLIF) with divergent, cortical bone trajectory (CBT) pedicle-screws: a good option for minimize spine access and maximize the field for nerve decompression, Journal of neurosurgical sciences, 2015 [5] Matsukawa -2nd MORE Japan MySpine cortical Bone Trajectory 2017. https://mysurgeon.medacta.com/uploads/presentation/attachments/d33a45ed-c550-438b-96b8-5e3fb1696725.mp4

[6] Matsukawa - Biomechanics of CBT (internal file)

[7] Regev G etal., Nerve injury to the posterior rami medial branch during the insertion of pedicle screws: comparison of mini-open versus percutaneous pedicle screw insertion techniques. Spine. 20093411239-42
 [8] Lamartina C. et al., Pedicle screw placement accuracy in thoracic and lumbar spinal surgery with a patient-matched targeting guide: a cadaveric study, European Spine Journal, 2015

 [9] Santoni B.G. et al., Cortical bone trajectory for lumbar pedicle screws, The Spine Journal, 2009
 [10] Mori K. et al., Short-Term Clinical Result of Cortical Bone Trajectory Technique for the Treatment of Degenerative Lumbar Spondylolisthesis with More than 1-Year Follow-Up, Asian Spine Journal, 2016 [11] Farshad M. et al., Accuracy of patient-specific template-guided vs. free-hand fluoroscopically controlled pedicle screw placement in the thoracic and lumbar spine: a randomized cadaveric study, European Spine Journal, 2017

[12] Chin K.R., Clinical Outcomes With Midline Cortical Bone Trajectory Pedicle Screws Versus Traditional Pedicle Screws in Moving Lumbar Fusions From Hospitals to Outpatient Surgery Centers,

Clinical Spine Surgery, 2017 [13] Petrone S. et al., Cortical bone trajectory technique's outcomes and procedures for posterior lumbar fusion: A retrospective study, Journal of Clinical Neuroscience, 2020

[14] Matsukawa K. et al., Accuracy of cortical bone trajectory screw placement using patient-specific template guide system, Neurosurgical Review, 2019 [15] Matsukawa K. et al., Cortical pedicle screw trajectory technique using 3D printed patient-specific-guide, M.O.R.E. Journal, 2018

[16] Marengo N. et al., Cortical Bone Trajectory Screw Placement Accuracy with a Patient-Matched 3-Dimensional Printed Guide in Lumbar Spinal Surgery: A Clinical Study, WORLD NEUROSURGERY, 2019 [17] Marengo N. et al., Cortical Bone Trajectory Screws in Posterior Lumbar Interbody Fusion: Minimally Invasive Surgery for Maximal Muscle Sparing—A Prospective Comparative Study with the Traditional Open Technique, Clinical Study, 2018

All trademarks are property of their respective owners and are registered at least in Switzerland. This document is not intended for the US market.



Strada Regina, 34 - 6874 Castel San Pietro - Switzerland Phone +41 91 696 60 60 - Fax + 41 91 696 60 66 Info@medacta.ch -www.medacta.com

MySpine<sup>®</sup> MC Leaflet 99.mv46MC.11 rev.01

