

VINNO^{IO}



Data sheet

V1.14.40





Contents


Ultrasound system Specifications	1
1. System Overview	1
1.1. Architecture	1
1.2. Applications	1
1.3. Imaging features	2
1.4. Standard features	3
1.5. Language support	3
2. Ergonomics	3
2.1. Keyboard	3
2.2. Image display screen	4
2.3. Comments	4
2.4. Bodymark	4
2.5. Peripherals (optional)*	4
2.6. Dimensions and Weight	4
2.7. Power	4
2.8. Operating Environment	4
3. Transducers.....	4
3.1. Transducer types.....	4
3.2. Transducer selection.....	5
S1-8CM.....	5
X2-6C.....	5
F2-5C.....	5
D2-6C	5
X4-9E.....	5
B2-6C.....	5
X3-10L.....	5
X4-12L.....	6
F4-12L.....	6
X6-16L.....	6
U5-15LE.....	6
X9-22L.....	6
G1-4P	6
S1-6P	6
G3-10PX	6
G4-12P	6
I7-18L	7
BP4-9.....	7
4. Advanced Imaging controls.....	7
4.1. VFusion.....	7
4.2. VSpeckle.....	7
4.3. VTissue	7
4.4. 3D/4D.....	7
4.4.1. HQ.....	7
4.4.2. Magic Cut	7
4.4.3. 3D Smart Face	7
4.4.4. Free view.....	8



4.4.5.	Inversion mode	8
4.5.	Tissue Doppler (TD).....	8
4.6.	Tissue Velocity Imaging (TVI)	8
4.7.	Tissue Velocity M mode (TVM) (optional)*	8
4.8.	Stress Echo	8
4.9.	Elastography imaging (EI).....	8
4.10.	Strain Imaging	9
4.11.	Multi-angle M mode	9
4.12.	Contrast imaging (CBI)	9
5.	Imaging modes.....	9
5.1.	2D Imaging	9
5.2.	Harmonic Imaging.....	10
5.3.	M mode.....	10
5.4.	Color Doppler mode.....	10
5.5.	Power Doppler mode.....	10
5.6.	Pulsed Wave (PW) Doppler	11
5.7.	Continuous Wave Doppler (CW).....	11
5.8.	TView	11
5.9.	PView(optional)*	11
5.10.	Tissue Doppler Imaging (TD)	12
5.11.	Tissue Velocity Imaging (TVI)	12
5.12.	Tissue Velocity M mode (TVM) (optional)*	12
5.13.	Elastography imaging (EI).....	12
5.13.1.	Elastic imaging (EI)	12
5.13.2.	VShear (ShearWave Elastography)	13
5.14.	3D/4D.....	13
5.14.1.	MCUT	13
5.14.2.	Free view.....	13
5.14.3.	VOCAL (optional) *	13
5.14.4.	Niche view.....	14
6.	System Feature	14
6.1.	Display modes.....	14
6.2.	Display annotation	14
6.3.	Cineloop	14
6.4.	Quick save feature	15
6.5.	Archive	15
6.6.	Report	15
6.7.	Connectivity	15
6.8.	Probes/application.....	15
6.9.	Safety Conformance.....	16
7.	Measurement and Analysis.....	16
7.1.	Measurement in different modes.....	16
7.1.1.	Generic Measurement in 2D mode.....	16
7.1.2.	Generic Measurement in M mode.....	16
7.1.3.	Generic Measurement in PW mode.....	17
7.2.	Measurement in different applications	17
7.2.1.	Abdominal Measurement	17



7.2.2.	Small Part Measurement	17
7.2.3.	Vessel Measurement	17
7.2.4.	Gynecology Measurement.....	17
7.2.5.	Obstetrics Measurement	17
7.2.6.	Pediatric Measurement	17
7.2.7.	Urology Measurement	17
7.2.8.	Cardiac Measurement.....	18
7.3.	Auto Measurement.....	18
7.3.1.	VAim OB measurement.....	18
7.3.2.	VAim Follicle(2D) measurement	18
7.3.3.	3D Auto Follicle (optional) *.....	18
7.3.4.	Auto IMT (Intima-Media Thickness).....	18
7.3.5.	Live IMT measurement (optional) *	18
7.3.6.	Auto NT (Nuchal Translucency) (optional)*	18
8.	POC	18
8.1.	POC workflow(optional) *	18
8.2.	POC Auto Function.....	19
8.2.1.	Auto Pleura (optional) *	19
8.2.2.	Auto DPF (optional) *	19
8.2.3.	Auto B-Line (optional) *	19

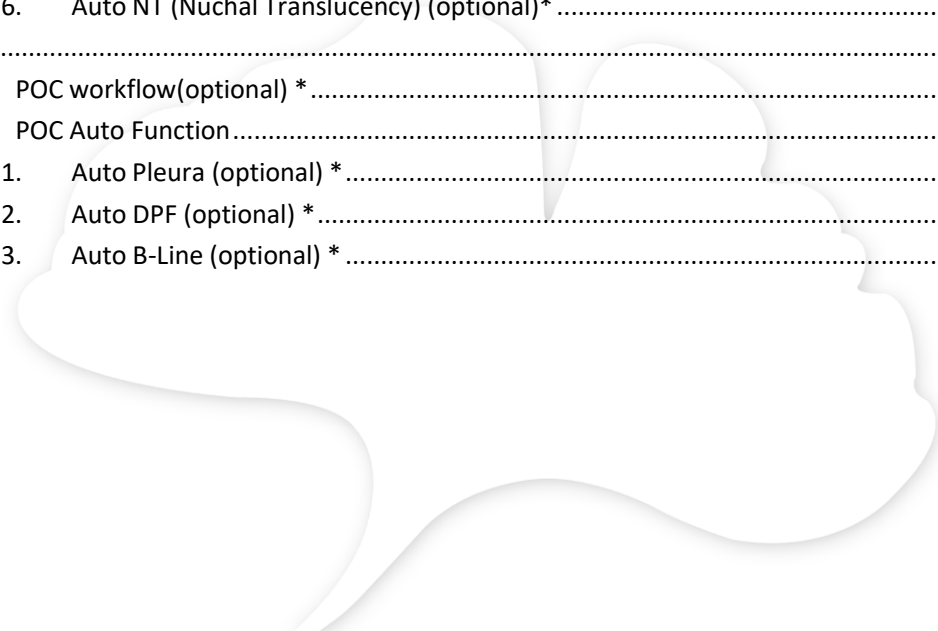



VINNO¹⁰

Ultrasound system Specifications

The premium performance of the full functional Portable VINNO 10 provides a fast and easy diagnosis by:

- New multistage pulse emission platforms (Vlucid) deliver improved image contrast and resolution
- All ranges of features, functions and probes
- Ease of use and ergonomic design

1. System Overview

1.1. Architecture

- New multistage pulse emission platform (Vlucid): single focused emission, forming multiple receiving lines, through phase correction, eliminate artifacts. Through the coherent combination of receiving lines at the same position of different transmissions, the contrast and signal-to-noise ratio of the image are improved obviously, while the time resolution of the image remains the same, and the penetration of the image is improved.
- Thanks to the Vlucid platform, it allows the development of many raw data-based processing algorithms, which have ultra-premium contrast and resolution imaging
- World-class Up to 25MHz imaging



performance

- Directional-enhanced information compiling for more tissue detail and reduction of angle-generated artifacts
- Next generation adaptive image processing for noise and artifact reduction that improves tissue presentation and edge definition
- Fully independent, triplex multiple mode operation for easy in doppler procedures
- Multi-processor, allow simultaneous mode changes, and supports advanced system functionality
- Boot-up in about 30sec

1.2. Applications

- Abdomen
- Gynecology
- Obstetric



- Small Parts
- Cardiology
- Vascular
- TCD
- Urology
- POC

1.3. Imaging features

- 2D grayscale imaging
- Harmonic imaging both in tissue harmonic and pulse inversion harmonic technologies
- VFusion, directional-enhanced information compounding
- VSpeckle, specialized and adaptive imaging processing to remove speckle noise artifacts and enhance tissue edge for clarity and accuracy
- Auto imaging optimization
- VTissue, the advanced adaptive image processing to compensate for sound and speed variation in different tissue
- Easy Comparative Function to compare previous exam
- Color Doppler imaging
- VFlow, adaptive color flow filter to increase the sensitivity of blood flow
- VLuminous flow, a feature which shows the blood flow in a 3-D view with excellent sensitivity
- Power Doppler imaging
- Pulse wave Doppler imaging
- Tissue Doppler (TD) mode
- Multi Doppler mode
- Duplex 2D/PW Doppler
- Triplex 2D/Color/PW Doppler

- Continuous wave Doppler
- Multi-angle M mode, up to 4 sample lines
- Curved M mode, user can draw any curved sample line freely and get corresponding results
- Stress echo
- Elastic Imaging (EI)
- HD Zoom
- FULL screen imaging to enlarge imaging size
- Dual real time imaging without compromising imaging size
- PView for panoramic imaging (optional)*
- TView for trapezoidal imaging
- Auto needle enhancement
- Auto IMT
- Live IMT, display intima-media thickness in real time (optional)*
- 2D/3D auto follicle (optional)*
- Free 3D
- 3D/4D Imaging
- 3D Smart Face, for fetal face optimization
- Tomographic display (MCUT)
- HQ (optional)*
- Magic cut
- Free view
- Niche view (optional)*
- Inversion mode
- Auto NT (Nuchal translucency) (optional)*
- VAim (Vinnno Artificial Intelligent Measurement) for OB, Follicle, Hip, pelvic
- PWV, a real-time, multi-point, RF tracking at single imaging site of the carotid artery intima media complex with high precision and generates arterial distension/tracking waveform. Calculates PWV to assess the

arterial stiffness and risk stratification of arteriosclerosis (optional) *

1.4. Standard features

- Up to 25Mhz high frequency in system platform
- Up to 9 000 000 system processing channels
- Up to 40 cm scanning depth
- Up to 23MHz probes are supported
- Up to 1500 seconds cine storage
- 512GB SSD quick boot up and storage
- Patient information database
- Image archive on hard drive
- Quick store to USB memory stick
- Quick store to hard drive
- Quick print to B/W and color thermal video printer
- Full measurement and analysis package
- Real time/Freez auto wave Doppler track and calculations
- Vascular calculations
- Cardiac calculations
- OB calculations and tables
- Gynecological calculations
- Urological calculations
- Renal calculations
- Volume calculations
- Network storage and printing
- 4 USB 3.0 ports
- 6 TGC slides
- 1 DP port
- 1 type-C port

1.5. Language support

- Software: Chinese, English, German,

Greek, Malay, Portuguese, Romanian, Spanish, Swedish, Norwegian, Danish, Finnish, French, Polish, Russian, Uighur, Italian, Czech, Hungarian, Cambodia

- Keyboard input: Chinese, English, German, Greek, Malay, Portuguese, Romanian, Spanish, Swedish, Polish, Norwegian, Danish, Finnish, French, Russian, Italian, Czech, Cambodia, Polish
- Control panel overlay: English

2. Ergonomics

- Unique human oriented design for comfort and convenience
- 15.6-inch high resolution display
- panel display with up to 178 ° positioning adjustments
- Easy to carry by integrated handle
- Full integrated probe to reduce overall space
- Integrated touchable alphabetic keyboard
- Integrated capacity touch panel to easy and simplify workflow
- 1 probe interface, can be expanded to 3 (optional)*

2.1. Keyboard

- Highly sensitive 8 inch capacity touch panel
- Intuitive, configurable and touchable interactive operation interface
- Ergonomic hard keys for general ultrasound operations
- Backlight keys

2.2. Image display screen

- 15.6 inch high resolution IPS, LCD technology, pixel resolution
- Backlight adjustment
- Resolution: 1920*1080 pixels

2.3. Comments

- Supports text input and arrow
- Adjustable text size and arrow size
- User customizable

2.4. Bodymark

- More than 215 bodymarks for versatile application
- User customizable

2.5. Peripherals (optional)*

- USB DVDRW
- B&W thermal video printer: Sony UP-D898MD
- Color thermal video printer: Sony UP-D25MD
- HDMI port, VGA port, S-Video port
- Keyboard dust film
- Wireless adapter
- Bluetooth adapter
- USB double button foot switch
- ECG
- Travelling case
- Battery 1.5 h
- External Gel Warmer
- Cart L
- Cart-S INT

- Cart-F with battery and 3 probe ports
- Physical keyboard (Cart required)
- 3 extended probe ports (For Cart S/ Cart L)
- 2 extended probe ports (For Cart L)
- CART battery pack assembly 3 h

2.6. Dimensions and Weight

- Length: 387mm
- Width: 340mm
- Thickness: 67.5mm
- Weight: without accessories approx 3.5 kg

2.7. Power

- Voltage: 100-240V
- Frequency: 50/60Hz
- Power: Max 200VA

2.8. Operating Environment

- Ambient temperature: 10-40°C
- Relative humidity: 30-75%
- Atmospheric pressure: 700hPa-1060hPa

3. Transducers

3.1. Transducer types

- Convex & Micro-convex array
- Linear array
- Phase array
- 4D probe
- Endocavity probe
- Intra operative
- TEE prone
- CW probe



3.2. Transducer selection

- Electronic switching of transducers
- User customizable imaging presets for each transducer and application
- Automatic dynamic receiving focus in all transducers
- Multiple adjustable transmit focal zone, up to 4 focal zoom

S1-8CM Single Crystal Curved Array

- Single Crystal technology
- Field of view: 60 °
- Convex radius: 60mm
- Transducer elements: 192
- Frequency range: 1- 8MHz
- Center frequency: 4MHz
- Physical Footprint: 78mm×27.2mm
- Application: Abdomen、OB/Gyn 、Urology

X2-6C Single Crystal Curved Array

- Field of view: 75 °
- Convex radius: 59.16mm mm
- Transducer elements: 192
- Frequency range: 1.5 - 8MHz
- Center frequency: 4MHz
- Physical Footprint: 76mm×27mm
- Application: Abdomen、OB/Gyn 、Urology

F2-5C

- Field of view: 59 °
- Convex radius: 59mm
- Transducer elements: 128
- Frequency range: 2.0 -6.5MHz
- Center frequency: 4MHz
- Physical Footprint: 72mm×27mm

- Application: Abdomen OB/Gyn Urology, Pediatr

D2-6C

- Field of view: 78 °
- Convex radius: 40mm
- Transducer elements: 128
- Frequency range: 2-8.0MHz
- Center frequency: 4MHz
- Physical Footprint: 75.5mm×49.2mm
- Application: Abdomen、OB/Gyn 、Urology

X4-9E Single Crystal Curved Array

- Single Crystal technology
- Field of view: 180 °
- Convex radius: 8.8mm
- Transducer elements: 192
- Frequency range: 3-10MHz
- Center frequency: 6.5MHz
- Physical Footprint: 32.4mm×40mm
- Application: OB/Gyn、 Urology

B2-6C

- Field of view: 80 °
- Convex radius: 20.2mm
- Transducer elements: 128
- Frequency range: 2.0 - 9MHz
- Center frequency: 4.0MHz
- Physical Footprint: 36.8mm×22.7mm
- Application: Abdomen、OB/Gyn 、Urology

X3-10L

- Field of view: 44.16mm
- Transducer elements: 192
- Frequency range: 3-15MHz
- Center frequency: 6MHz
- Physical Footprint: 61mm x 26mm
- Application: Vascular、 MSK、 Nerve



X4-12L

- Field of view: 38.4mm
- Transducer elements: 192
- Frequency range: 3-17MHz
- Center frequency: 7.3MHz
- Physical Footprint: 53.2mm x 23.4mm
- Application: Vascular, Small parts, MSK, Nerve

F4-12L

- Field of view: 38.4mm
- Transducer elements: 128
- Frequency range: 6-18MHz
- Center frequency: 7.3MHz
- Physical Footprint: 52.5mm x 25mm
- Application: Vascular, Small parts, MSK, Nerve

X6-16L

- Field of view: 38.4mm
- Transducer elements: 192
- Frequency range: 3.0-19MHz
- Center frequency: 10MHz
- Physical Footprint: 52.8mm x 26mm
- Application: Vascular, Small parts, MSK, Nerve

U5-15LE

- Field of view: 51.2mm
- Transducer elements: 256
- Frequency range: 5-15MHz
- Center frequency: 7.3MHz
- Physical Footprint: 99mm x 26mm
- Application: Vascular, Small parts, Specially for Breast, MSK, Nerve

X9-22L

- Field of view: 28.8mm
- Transducer elements: 192
- Frequency range: 9-23MHz
- Center frequency: 15MHz
- Physical Footprint: 45mm x 25.4mm
- Application: Vascular, Small parts, MSK, Nerve

G1-4P

- Field of view: 90 °
- Transducer elements: 64
- Frequency range: 1-6MHz
- Center frequency: 2.8MHz
- Physical Footprint: 34.2mm x 28.7mm
- Application: Application, Abdomen

S1-6P

- Single Crystal technology
- Field of view: 90 °
- Transducer elements: 96
- Frequency range: 1-8MHz
- Center frequency: 3.5MHz
- Physical Footprint: 36mm x 29mm
- Application: Application, Abdomen

G3-10PX

- Field of view: 90 °
- Transducer elements: 96
- Frequency range: 3-10MHz
- Center frequency: 6.5MHz
- Physical Footprint: 33mm x 33mm
- Application: Application, Abdomen

G4-12P

- Field of view: 90 °
- Transducer elements: 96
- Frequency range: 4-15MHz



- Center frequency: 7.5MHz
- Physical Footprint: 22mm x 22mm
- Application: Application、 Abdomen

I7-18L

- Field of view: 25.6mm
- Transducer elements: 128
- Frequency range: 6-20MHz
- Center frequency: 8.5MHz
- Physical Footprint: 31.8mm x 10mm
- Application: Vascular、 Small parts、 MSK、 Nerve

BP4-9

- Field of view (convex): 150 °
- Convex radius: 10mm
- Transducer elements (Convex): 128
- Transducer elements (Line): 128
- Frequency range (Convex): 4-10MHz
- Frequency range (Line): 4-12MHz
- Center frequency (Convex): 6.5MHz/
- Center frequency (Line): 7.3MHz
- Physical Footprint: 26mm×21.4mm
- Application: Urology

4. Advanced Imaging controls

4.1. VFusion

- Available on all transducers and for 2D, 3D/4D
- Operate in conjunction with VSpeckle, harmonic imaging

4.2. VSpeckle

- Available on all transducers and for 2D,

3D/4D

- Virtually eliminate speckle noise artifact and dynamically enhances tissue margins
- Selectable multiple levels of speckle noise reduction and smoothing
- Operates in conjunction with VFusion and harmonic imaging

4.3. VTissue

- Special imaging processing to adapt to the speed of the ultrasound variation in different tissue
- Improved conspicuity of lesions, such as stone and tendon

4.4. 3D/4D

4.4.1. HQ

- Amazing high image quality
- Extreme realistic rendering images
- Similar operation as normal rendering

4.4.2. Magic Cut

- Ability to edit images, make possible to cut away structure obstructing the view in the ROI
- Several cutting methods available

4.4.3. 3D Smart Face

- An intelligent tool for fetal face optimization. This tool detects the fluid/tissue interface and smartly removes noise in front of the baby inside the ROI, to obtain an optimal baby face.
- Use Auto key on the keyboard to remove the obstacle in front of the baby
- Only works on 3D Render



- Can not use this feature together with Magic Cut

4.4.4. Free view

- Provide any plan view to visualize the internal organization information
- Increasing the contrast resolution facilitates the detection of diffuse lesions in organs

4.4.5. Inversion mode

- This render mode is used to display anechoic structures such as vessels
- It invert the gray values of the rendered image, such as black image information become white and vice versa

4.5. Tissue Doppler (TD)

- Present wall motion spectrum by using Doppler principle
- Provide wall motion direction and velocity information

4.6. Tissue Velocity Imaging (TVI)

- Color codes the velocities in tissue
- Present tissue color imaging by using Doppler principle
- This color image is overlaid onto the 2D image
- Captures low flow but high amplitude signals associated with wall motion

4.7. Tissue Velocity M mode (TVM)

(optional)*

- Color codes the velocities in tissue

- Present wall motion spectrum based on tissue moving

- This color image is overlaid onto the 2D image

- Captures low flow but high amplitude signals associated with wall motion

4.8. Stress Echo

- Stress echo is a non-invasive, dynamic evaluation of myocardial structure and its function under an external stress (exercise or pharmacology)

- 12 Ready to use templates (max 8 stages * 6 views) Editable

- User definable template

- Re-arrange & Select default template

- 10 View names available

- 14 Stage names are available (can add user defined stage name)

- One Touch Shuffle (Stage / View)

- Touch & Compare any view of stage

- Systole only review

4.9. Elastography imaging (EI)

- Available on linear transducers and convex probe

- Shows the spatial distribution of tissue elasticity properties in a region of interest to estimate the strain before and after tissue distortion caused by external force

- The strain estimation is scaled by color to have smooth distribution display

- Have quality index to indicate if there is proper external force



4.10. Strain Imaging

- Auto-ROI (after selecting Mitral Valve Plane)
- Adjust Segment-wise (Longitudinal strain)
- Adjust Segment-wise and Rotate whole ROI (Radial & Circumf. Strain)
- ECG to select heart cycle
- View based Bulls Eye view
- Result type (Peak Strain or Peak Time)
- Parameter type (L Strain, C Strain)

4.11. Multi-angle M mode

- Sample on moving tissue from multi-angle
- Present wall motion spectrum based on tissue moving

4.12. Contrast imaging (CBI)

- Available on linear transducers and convex probe
- Support contrast imaging in both 2D and 3D volume
- By contrast agent, imaging is enhanced within vessel which agent flow
- Have one button push to destroy the agent. Useful in the bubble wash-in characteristics of anatomy being scanned

5. Imaging modes

5.1. 2D Imaging

- Pre-defined ATGC (adaptive temporal gain

compensation) curves optimized for consistently excellent imaging

- Display format: Single, Dual, Quad
- B/M acoustic output: 10%-100
- Up to 4 focus zone adjustable for whole depth
- Reverse function: on/off
- 2D optimization: on/off
- Centerline: on/off
- L/R flip and U/D flip: on/off
- VFusion: ≥ 7 steps
- VSpeckle: ≥ 6 steps
- Harmonic imaging both tissue harmonic and phase inversion
- Cine loop image review
- Selectable 2D line density
- Dual imaging with independent Cine loop
- 256(8 bit) gray level
- Multiple color maps with chroma imaging: 10 steps
- FULL screen imaging to larger image size
- Selectable Multi frequency: probe dependent
- Gray filter: ≥ 7 steps
- Persistence: ≥ 8 steps
- Selectable image angles, probe Dependent
- Gain: 0-100%
- Selectable Dynamic range: 30-350 db
- VSharpen to enhance edge contrast: ≥ 8 steps
- Smooth to improve spatial resolution: ≥ 11 steps
- Gray Map: ≥ 32 types
- Tint Map: ≥ 24 types
- TGC: 8 slides on control panel
- TI heat index: TIB, TIS, TIC
- Rotation: 0°, 90°, 180°, 270°
- Pan/Zoom HD (up to 10x) Real/Freez mode



5.2. Harmonic Imaging

- Supports both tissue harmonic and phase inversion imaging (transducer and frequency dependence)
- Second harmonic processing to reduce artifacts and improve image clarity
- Maximize detail resolution and enhance contrast
- Available on all imaging transducers
- Extends high performance imaging capabilities to all patient body types

5.3. M mode

- Selectable sweeping rates: ≥ 10 steps
- Selectable display format prospective or retrospective (V1/3, V1/2, V2/3, H1/2, H3/4, full screen)
- 256 gray levels
- Acoustic output: 10%-100%
- Gray filter: ≥ 7 steps
- Dynamic range: 108db-128db, 2db/step
- Vsharpen: ≥ 6 steps
- Gray Map: ≥ 32 types
- Tint Map: ≥ 24 types
- Gain: 0-100%
- Color M mode: available
- MultiAngle: available

5.4. Color Doppler mode

- Available on all imaging transducers
- Selectable in baseline, line density, flash reduction, persistence, maps, frequency, PRF, wall filter, packet size, color level,

sensitivity, focus position, acoustic power, and smooth

- Automatically adapts transmit and receive bandwidth processing based on the color box position
- Cineloop review with full playback control
- Steering on linear array transducers
- FULL screen imaging to larger image size
- L/R flip and U/D flip: on/off
- Frequency: ≥ 4 steps, depend on probes
- Line density: ≥ 7 steps
- Smooth: ≥ 7 steps
- Color Map: ≥ 33 types
- Persistence: ≥ 20 steps
- Invert: on/off
- Baseline: 0-100%
- Color level: ≥ 16 steps
- Acoustic power: 5-100%
- Color gain: 0-100%
- Adjustable region of interest

5.5. Power Doppler mode

- High sensitive mode for small vessel visualization
- Available on all transducers
- Selectable line density, flash reduction, persistence, maps, frequency, PRF, wall filter, packet size, color level, sensitivity, focus position, acoustic power, and smooth
- Cineloop review Display format: Single, Dual, Quad
- Color maps: ≥ 24 types
- Smooth: ≥ 7 steps
- Color levels: ≥ 11 steps
- Persistence: ≥ 20 steps



- Adjustable region of interest

5.6. Pulsed Wave (PW) Doppler

- Available on all imaging transducers
- Selectable gray filter, dynamic range, frequency, PRF, wall filter, baseline, angle correct, sample volume
- Ultra high resolution spectral FFT rate
- Normal, invert display around horizontal zero line
- Dynamic range: 108db-128db
- Angle correct: -80°~ 80°
- Invert: on/off
- Baseline: 5%-95%
- Sample volume: 0.5mm-10mm
- Selectable display format prospective or retrospective (V1/3, V1/2, V2/3, H1/2, H3/4, full screen)
- Gray map: ≥13types
- Tint map: ≥11types
- Spectrum Optimize: ≥28steps
- Gray filter: ≥6steps
- PW acoustic output: 5%-100%
- Audio Volume: 0~20
- Trace direction: above, below, both
- Trace type: max, mean, both
- Cardiac cycle: 1-5
- Selectable grayscale curve for optimal display
- Selectable low frequency signal filtering with adjustable wall filter settings
- Selectable chroma colorization maps
- Auto function to optimize spectral Doppler displ
- Digitally enhanced stereo Output
- Post-processing in frozen mode includes

map, baseline, invert and chroma

- Simultaneous or duplex mode of operation

5.7. Continuous Wave Doppler (CW)

- Cardiac sector array transducer only
- Selectable gray filter, dynamic range, frequency, PRF, wall filter, baseline, angle correct
- Dynamic range: 108db-128db
- Angle correct: -80°~ 80°
- Invert: on/off
- Baseline: 5%-95%
- Selectable display format prospective or retrospective (V1/3, V1/2, V2/3, H1/2, H3/4, full screen)
- Gray map: ≥13types
- Tint map: ≥11types
- Spectrum Optimize: ≥28steps
- Gray filter: ≥6steps
- PW acoustic output: 5%-100%
- Audio Volume: 0~20

5.8. TView

- Expand view of scanning
- Available on all transducers

5.9. PView(optional)*

- Real time extended field of view composite imaging
- Ability to back up and realign the image during acquisition
- Full zoom, cinelooop review and image rotation capabilities

- Available on all transducers

5.10. Tissue Doppler Imaging (TD)

- Cardiac sector array transducer only
- Selectable frequency, PRF, wall filter, Gain
- Baseline: 5%-95%
- Angle correct: -80°~ 80°
- Sample volume: 0.5mm-10mm, 0.5mm/step
- Spectrum optimize: ≥20steps
- Acoustic power:5%-100%
- Dynamic range: 92db-128db
- Audio volume:0-20
- Gray filter: ≥6steps
- Heart cycle: 1-5
- Gray map: ≥13 types
- Tint map: ≥11 types

5.11. Tissue Velocity Imaging (TVI)

- Color codes the velocities in tissue
- Present tissue color imaging by using Doppler principle
- This color image is overlaid onto the 2D image
- Captures low flow but high amplitude signals associated with wall motion
- Available on all sector transducer for cardiac imaging
- Tissue velocity M mode display for wall motion(optional)
- Gain
- Velocity
- Color level: ≥ 11steps
- Transparency: ≥ 13 steps
- Smooth: ≥ 7steps

- Line density: ≥ 3steps
- Persistence: ≥ 7steps
- Color map: ≥ 10types

5.12. Tissue Velocity M mode (TVM)

(optional)*

- Color codes the velocities in tissue
- Present wall motion spectrum based on tissue moving
- This color image is overlaid onto the 2D image
- Captures low flow but high amplitude signals associated with wall motion
- Selectable frequency, PRF, Focus position
- Baseline: 0%-100%
- Color level: ≥ 11steps
- Transparency: ≥ 13steps
- Packet size: 3,4,5,6
- Acoustic power: 5%-100%
- Display format: Single, Dual, Quad

5.13. Elastography imaging (EI)

5.13.1. Elastic imaging (EI)

- Available on linear transducers and convex probe
- Shows the spatial distribution of tissue elasticity properties in a region of interest to estimate the strain before and after tissue distortion caused by external force
- The strain estimation is scaled by color to have smooth distribution display
- Have quality index to indicate if there is proper external force
- Winsize: 0, 1, 2, 3, 4



- Overlap: 0, 1, 2, 3, 4
- Transparency: 0-12
- Smooth: 0-6
- Line density: 0-4
- Map: E10
- Display format: Single, Dual, Quad

5.13.2. VShear (ShearWave Elastography)

- Available on linear transducers and convex probe
- A non-invasive method which can detect tissue hardness by calculating the shear wave propagation velocity and elastic modulus
- Persistence: 0-6, 1/step
- Smooth: 0-6, 1/step
- Transparency: 0-5, 1/step
- Scale: 0-14, 1/step
- Sync Display, simultaneously display 2D and shear wave elastography imaging in left and right respectively
- Reliable Display, display the reliable area in shear wave elastography imaging
- Measurement type (Kind): G, Cs, E
- Map: VShear0, VShear1
- Display format: Single, Dual, Quad

5.14. 3D/4D

- Category: Face, Spine, Brain, Heart, Hi speed, Lip & Plate, Limbs, Custom
- Display format: Single, Double, MPR, Quad
- Flip: 0°, 90°, 180°, 270°
- View: Front/Back, Back/Front; Left/Right, Right/Left; Up/Down, Down/Up
- Selectable rendering approaches: HQ

Surface, HQ Grad, HQ Silhouette, Surf Texture, Surf Smooth, Grad Light, Surf HDR, Trans Max, X-ray, Trans Min, Light

- Render Type: Gray, GrayInv
- Threshold: 0-255
- Transparency: 0.1-2, 0.1steps
- Rotation Direction: X, Y, Z
- Tint maps: ≥ 24 Types
- Gray maps: ≥ 32 Types
- 3D Map: ≥ 10 types
- 2D VSpeckle: ≥ 3 types
- 3D VSpeckle: ≥ 3 types

5.14.1. MCUT

- Slice Number: 2x2, 3x3, 4x4, 5x5
- Max Slice Number: 25
- Gray Map: ≥ 32 types
- Tint Map: ≥ 24 types
- Cut plane: A, B, C
- Volume Angle: 15°~ 85°
- Quality: Low, Mid, Good, High
- Interval: 1mm-20mm, 0.5mm/step

5.14.2. Free view

- Direction: Left, Right, Up, Down
- Rotation Direction: X, Y, Z
- Active line: 1, 2, 3
- Slice thickness: 0mm-20mm, 1mm/step
- Route: Curve, Straight line
- Display format: Single, Double, MPR, Quad
- Reference image: A, B, C
- Mix: 10-90,5/step
- Threshold: 255 steps,1/step
- Transparency: 0.1-2.0,0.1/step

5.14.3. VOCAL (optional) *

- Vocal layers: 8, 12,16,20,24,28,32

- Display format: single, Quad
- Image reference: A, B, C

5.14.4. Niche view

- Model type: upper, lower
- Display format: single, quad
- Rotation direction: X, Y, Z
- Image reference: A, B, C, N

6. System Feature

6.1. Display modes

- Simultaneous capability
 - 2D/PW/CW
 - 2D/CF or PDI
 - 2D/M
 - Dual, 2D/2D
 - Dual, 2D/2D+CF or PDI
 - Dual, duplex and triplex
- Time line display
- Independent dual 2D/PW

6.2. Display annotation

- Institution/hospital name
- Date: 3 types selectable, Year-Month-Day, Day-Month-Year, Month-Day-Year
- Time: 2 types selectable, 24hours or 12 hours
- Operator identification
- Patient name, first, last
- Patient identification: 30 characters
- Gestational age from LMP/ BBT/ DOC/ IVF
- Power output index
 - MI: mechanical index
 - TIS: thermal index soft tissue

-TIC: thermal index cranial(Bone)

-TIB: thermal index bone

- Probe orientation marker: coincide with a probe orientation marking on the probe
- Gray/color bar
- Measurement result window
- Probe type
- Application name
- Image depth
- Imaging parameters by mode
 - 2D/M mode:
 - acoustic power output, gain, frequency, frame rate, dynamic range
 - Color mode:
 - color acoustic power output, color gain, color flow frequency, PRF, wall filter
 - PW/CW mode:
 - Doppler acoustic power output, Doppler gain, Doppler frequency, PRF, wall filter, sample depth
- Focus zone marker
- Body pattern
- PW and CW scale markers: time/speed
- M scale markers: time/depth, time
- System measurement display
- System message display
- Biopsy guide line
- Heart rate
- Battery status

6.3. Cineloop

- Acquisition, storage in memory and display of up to 1500 seconds long of 2D, color and PW/CW images for review
- Supports custom start and end frames
- Support manual playback frame by frame, or automatic playback, and the playback

speed is adjustable

- Compare live imaging with stored imaging

6.4. Quick save feature

- The system provides quick save function through USB stick during or after exam
- Configurable saving file format, VRD (VINNO Raw Data), DICOM, JPEG, BMP, PNG, MP4 and AVI

6.5. Archive

- Patient data input which include patient ID, name, birth date, sex, Perf. Physician, Ref. Physician, Operator
- Physical data such as weight, height
- Patient exam management
- Patient exam images storage and management
- Import VRD format data into the system from outside media, such as USB stick
- Export patient data into outside medias

6.6. Report

- Automatically pull patient data into the report
- Automatically load measurement worksheet into the report
- Pull related images into the report
- Write comments in the report
- Print report through network or local printer

6.7. Connectivity

- Standard connectivity features

-Connect to the local printer through the USB port or to the network printer via ethernet port or wireless for image printing

-Page report print

-Image export to removable media (USB stick)

- Network Transmission

-Email

-FTP service

-Cloud service

-DICOM 3.0 export and storage, printer,worklist (optional)*

- Data storage format Includes VRD, DICOM, PNG, AVI

-VRD and DICOM images stored in disc can be recalled on the VINNO system

-JPEG, BMP, PNG and AVI images can be played on normal computers

- Mobile data transfer solution by

-Blue tooth, need bluetooth adapter (optional)*

-Email

-VCloud (VINNO Cloud service)

-Support for standard DVD media (optional)*

6.8. Probes/application

- Selectable multiple applications and probe
- Edit exist application preset
- Edit user defined preset
- Rename preset
- Return to factory preset
- Quick save user defined parameters in related application



6.9. Safety Conformance

- This device is tested to meet all applicable requirements in relevant
- Conformity to Standards:
- ✧ IEC 60601-1: 2005/A1: 2012+A2: 2020 Medical electrical equipment - Part 1: General requirements for basic safety and essential performance
- ✧ IEC 60601-1-2: 2014/A1: 2020 Medical electrical equipment - Part 1-2: General requirements for basic safety and essential performance – Collateral Standard: Electromagnetic disturbances - Requirements and tests
- ✧ IEC 60601-1-6: 2010/A1: 2013+A2: 2020 Medical electrical equipment - Part 1-6: General requirements for basic safety and essential performance - Collateral standard: Usability
- ✧ IEC 60601-2-37: 2007/A1: 2015 Medical electrical equipment - Part 2-37: Particular requirements for the basic safety and essential performance of ultrasonic medical diagnostic and monitoring equipment
- ✧ -IEC 61157: 2007/A1: 2013 Standard means for the reporting of the acoustic output of medical diagnostic ultrasonic equipment
- ✧ ISO 10993-1: 2018 Biological evaluation of medical devices - Part 1: Evaluation and testing within a risk management process
- ✧ IEC 62304: 2006/A1: 2015 Medical device software - Software life-cycle processes

- ✧ IEC 62366-1: 2015/A1: 2020 Medical devices - Application of usability engineering to medical devices
- ✧ WEEE according to 2012/19/EU
- ✧ RoHS according to 2011/65/EU

7. Measurement and Analysis

7.1. Measurement in different modes

7.1.1. Generic Measurement in 2D mode

- Depth
- Distance
- Perimeter
 - Length and width method
 - Ellipse method
 - Polygon method
 - Spline method
 - Tracing method
- Area
 - Length and width method
 - Ellipse method
 - Polygon method
 - Spline method
 - Tracing method
- Angle
- Stenosis
 - Diameter method
 - Square meter method
- A and B ratio
 - Diameter ratio
 - Square meter ratio

7.1.2. Generic Measurement in M mode

- Depth
- Distance



- Time
- Slope
- Heart rate
- Stenosis
- A and B ratio
 - Diameter ratio
 - Time ratio
 - Velocity ratio

7.1.3. Generic Measurement in PW mode

- Methods: Manual, Semi-Automatic, Automatic, Real-Time Automatic
- Speed (include PV (Peak Velocity))
- Time (include AT (Accelerate Time))
- Acceleration
- PS (Peak Speed in systole period)
- ED (The speed in the end of diastole period)
- MD (Minimum speed in diastole period)
- Mean Vel (Max Mode)
- Mean Vel (Mean Mode)
- PI (Pulsation Index)
- RI (Resistance Index)
- PS and ED ratio
- ED and PS ratio
- A and B ratio (A/B ratio)
 - Speed ratio
 - Time ratio
 - Acceleration ratio
- SV (Stroke Volume)
- Heart rate

7.2. Measurement in different applications

7.2.1. Abdominal Measurement

- General abdomen

- Difficult abdomen
- Kidney
- Renal vessel
- Abdominal trauma

7.2.2. Small Part Measurement

- Thyroid
- Breast
- Testis
- Musculoskeletal
- Upper and lower extremity joint
- Nerve block

7.2.3. Vessel Measurement

- Carotid artery
- Upper artery
- Upper vein
- Lower artery
- Lower vein
- Vessel puncture
- Transcranial Doppler

7.2.4. Gynecology Measurement

- Uterus and Pelvis
- Follicle

7.2.5. Obstetrics Measurement

- OB Early
- OB Mid
- OB Late
- Fetal Heart

7.2.6. Pediatric Measurement

- Neonatal Head
- Neonatal Abdomen
- Pediatric Abdomen
- Pediatric Hip

7.2.7. Urology Measurement

- Bladder

- Prostate
- Renal
- Kidney and ureter
- Pelvic Floor dysfunction

7.2.8. Cardiac Measurement

- General
- LV
- MV
- AO
- AV
- LA
- RV
- TV
- PV
- RA
- Auto EF
- System

7.3. Auto Measurement

7.3.1. VAim OB measurement

- VAim OB is a tool for fetal growth calculation, just one touch to activate the measurement items (BPD, OFD, HC, AC, FL, HL) and get the results, helps to make clinical decisions quickly and confidently, improving the speed and ease of exams
- The results will be added into the worksheet and report automatically

7.3.2. VAim Follicle(2D) measurement

- A tool for follicle calculation, one touch to get the follicle status, dedicated for women's reproductive health
- Choose left or right follicle
- Automatically identify all the follicles with different colors and calculate follicle

volume and diameter

7.3.3. 3D Auto Follicle (optional) *

- Click the "Start" button on the touch screen, the follicles will be automatically identified and marked with different colors
- Report the area of different follicle in the volume data automatically

7.3.4. Auto IMT (Intima-Media Thickness)

- Automatically detect intima media thickness in interest box
- Automatically report the result of IMT
- Available in linear probe

7.3.5. Live IMT measurement (optional) *

- Real-time automatically display IMT items with the different ROI positions
- The IMT items include: max, min, average, SD, points (how many points are used for the result), size of ROI
- Available in carotid application

7.3.6. Auto NT (Nuchal Translucency) (optional)*

- Automatically detect Nuchal Translucency in interest box
- Automatically report thickness result of NT

8. POC

8.1. POC workflow(optional) *

- Includes lung, hemodynamics, FAST and other assessment modules
- Provide custom process mechanisms,



which can be personalized workflow customization based on different scenarios and parts

8.2. POC Auto Function

8.2.1. Auto Pleura (optional) *

- Diagnostic diagnosis of lung status assessment by imaging the patient
- Automatic positioning of the pleural line
- Automatic pleural line thickness measurement
- Automatic pleural slip detection


8.2.2. Auto DPF (optional) *

- Various indices of diaphragm evaluation are measured in M mode as a basis for judging diaphragm function

- Measure the right diaphragm alone or both diaphragms as an average of thickness
- Calculate changes in diaphragm thickness during the respiratory cycle
- Measures the distance that the diaphragm is able to move during the respiratory cycle

8.2.3. Auto B-Line (optional) *

- Automatically identifies the position and type of the B-Line in real time
- Automatic score calculation
- Image recognition quality is indicated by different colors

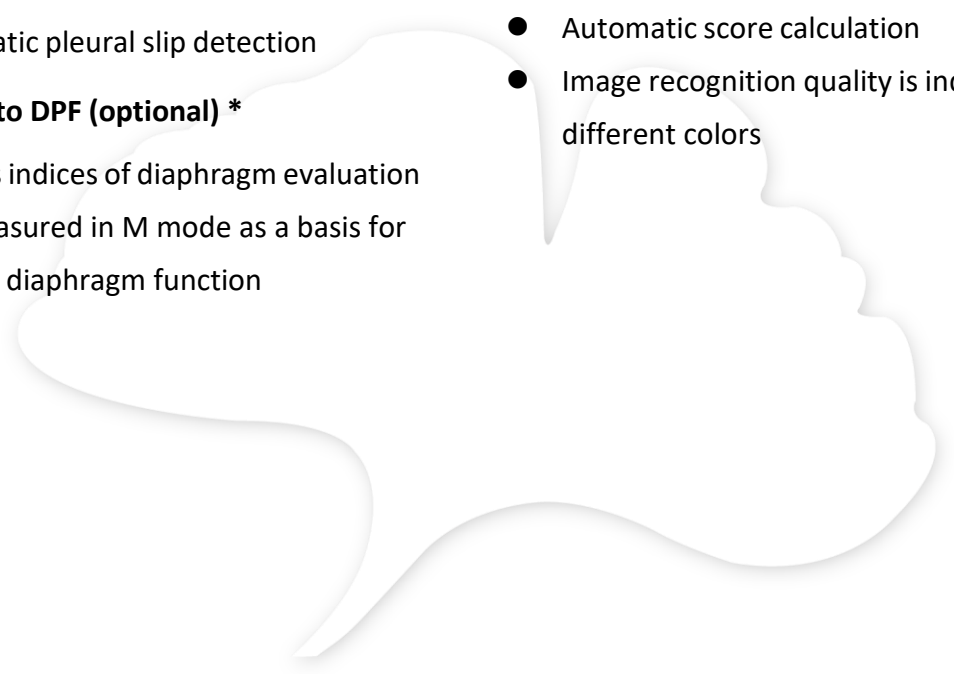



VINNO Technology (Suzhou) Co., Ltd

VINNO is focusing on producing premium diagnostic ultrasound development to provide customer clinical value through Continuous Innovation, Excellent Performance and Accessible Solutions.



Thanks you for your interest in VINNO.

You can contact us by phone and email (below) or contact our local representatives.

📍 5F, A Building, NO.27 Xinfra Rd, Suzhou Industrial Park, 215123, China(215.6123)

☎ Tel: +86 512 62873806

📠 Fax: +86 512 62873801

✉ email address: vinno@vinno.com

🌐 website: www.vinno.com

Internal Revision: Rev5