

Formularul ofertei (F3.1)

Data depunerii ofertei: **25 iunie 2020**

Procedura de achiziție Nr.: **21024104**

Anunț de participare Nr.: _____

Către: **IP USMF "Nicolae Testemițanu"**

GBG-MLD SRL declară că:

- a) Au fost examinate și nu există rezervări față de documentele de atribuire.
- b) **GBG-MLD SRL** se angajează să furnizeze în conformitate cu documentele de atribuire și condițiile stipulate în specificațiile tehnice și preț, următoarele bunuri Utilaj medical pentru activitatea științifică.
- c) Suma totală a ofertei fără TVA constituie: 84 410,00 (optzeci și patru mii patru sute zece) lei.
- d) Suma totală a ofertei cu TVA constituie: 101 292,00 (una suta mii două sute nouăzeci și doi) lei.
- e) Prezența ofertă va rămâne valabilă pentru perioada de timp specificată în **FDA3.8.**, începînd cu data-limită pentru depunerea ofertei, în conformitate cu **FDA4.2.**, va rămîne obligatorie și va putea fi acceptată în orice moment pînă la expirarea acestei perioade;
- f) În cazul acceptării prezentei oferte, **GBG-MLD SRL** se angajează să obțină o Garanție de bună execuție în conformitate cu **FDA6**, pentru executarea corespunzătoare a contractului de achiziție publică.
- g) Nu sîntem în nici un conflict de interese, în conformitate cu art. 74 din Legea nr. 131 din 03.07.2015 privind achizițiile publice.
- h) Compania semnatară, afiliații sau sucursalele sale, inclusiv fiecare partener sau subcontractor ce fac parte din contract, nu au fost declarate neeligibile în baza prevederilor legislației în vigoare sau a regulamentelor cu incidență în domeniul achizițiilor publice.

Semnat: _____

Nume: Tudor Cealcoyschi

În calitate de: director

Ofertantul: "GBG-MLD" SRL

Adresa: mun. Chisinau, str. Tighina 65 of. 607

Data: **25.06.2020**



SPECIFICAȚII DE PREȚ (F4.2)

Numărul procedurii de achiziție:21024104	Data:25.06.20	Alternativa nr.nu
Denumirea procedurii de achiziție:utilaj medical pentru activitatea științifică	Lot _____	Pagina1 din 1

Cod CPV	Denumirea bunurilor	Unitatea de măsură	Cantitatea	Preț unitar (fără TVA)	Preț unitar (cu TVA)	Suma fără TVA	Suma cu TVA	Termenul de livrare
	10. Tavijă cu capac	buc.	2	990,00	1188,00	1980,00	2376,00	45 zile din momentul solicitării la locul indicat de autoritatea contractantă
	12. Caliper (cutimetru) mecanic	buc.	6	70,00	84,00	420,00	504,00	45 zile din momentul solicitării la locul indicat de autoritatea contractantă
	14. Dinamometru de mână mecanic	buc.	4	520,00	624,00	2080,00	2496,00	45 zile din momentul solicitării la locul indicat de autoritatea contractantă
	22. Spălător pentru microplăci	buc.	1	64255,00	77106,00	64255,00	77106,00	45 zile din momentul solicitării la locul indicat de autoritatea contractantă
	26. Centrifuga	buc.	1	15675,00	18810,00	15675,00	18810,00	45 zile din momentul solicitării la locul indicat de autoritatea contractantă
	Suma totala					84410,00	101292,000	

Semnati: _____ Numele, prenumele: Ceaicovschi Tudor În calitate de: Director General



Ofertantul: "GBG-MLD" SRL Adresa: mun. Chișinău, str. Tighina, 65, of. 607

SPECIFICAȚII TEHNICE (F4.1)

Numărul procedurii de achiziție: 21024104				Data: 25.06.2020		Alternativa nr. NU	
Denumirea procedurii de achiziție: utilaj medical pentru activitatea științifică				Lot		Pagina 1 din 1	
Nr. d/o	Denumirea bunurilor	Modelul articolului	Tara de origine	Producătorul	Specificarea tehnică deplină solicitată	Specificarea tehnică deplină propusă de către ofertant	Stăndarde de referință
10	10. Taviță cu capac	26608	Italia	Gima	Material – inox, Dimensiuni: 355 x254 x 50 mm	Material – inox, Dimensiuni: 355 x254 x 50 mm	
12	12. Caliper (cutimetru) mecanic	27318	Italia	Gima	Tip: mecanic, tip arc Material: plastic sau metal Diapazon măsurare: 0-70 mm	Tip: mecanic, tip arc Material: plastic Diapazon măsurare: 0-70 mm	
14	14. Dinamometru de mână mecanic	28790	Italia	Gima	Tip: mecanic, tip arc Unitatea calibrată: kilograme Diapazon măsurări: minim 0 – 75 kg Caracteristici speciale: Indicatorul ramane la maxim pana la resetare	Tip: mecanic, tip arc Unitatea calibrată: kilograme Diapazon măsurări: minim 0 – 75 kg Caracteristici speciale: Indicatorul ramane la maxim pana la resetare	
22	22. Spălător pentru microplăci	3D-IW8 Inteliwas her	Letonia	Biosan	de tipul BioTek 405 sau analogic Garanție minim 24 luni - Permite centrifugarea:	de tipul BioTek 405 sau analogic Garanție minim 24 luni - Permite centrifugarea:	
26	26. Centrifuga		Turcia	Nuve	Tuburi standard (5-10 ml) Tuburi de testare conice Falcon (15 ml) Sisteme de colectare a sângelui (4-10 ml) - Viteza maximă - 6000 rpm - Reglarea vitezei în pași de 100 rpm - Viteza minima - 500 rpm - Accelerația maximă este de 3461xg. - Introducerea timpului în minute - de la 1 la 99 de minute - Dimensiuni +/- 228 x 262 x 352 mm - Greutate max 8 kg Garanție minim 12 luni	Tuburi standard (5-10 ml) Tuburi de testare conice Falcon (15 ml) Sisteme de colectare a sângelui (4-10 ml) - Viteza maximă - 5000 rpm - Reglarea vitezei în pași de 100 rpm - Viteza minima - 500 rpm - Accelerația maximă este de 2822xg. - Introducerea timpului în minute - de la 1 la 99 de minute - Dimensiuni 280x360x260 mm - Greutate max 12 kg Garanție minim 12 luni	

Semnăt: _____ Numele, prenumele: Ceaicovschi Tudor In calitate de: Director General


Ofertantul: "GBC-MED" SRL Adresa: mun. Chișinău, str. Tighina, 65, of. 607





NF200

Bench Top Centrifuge

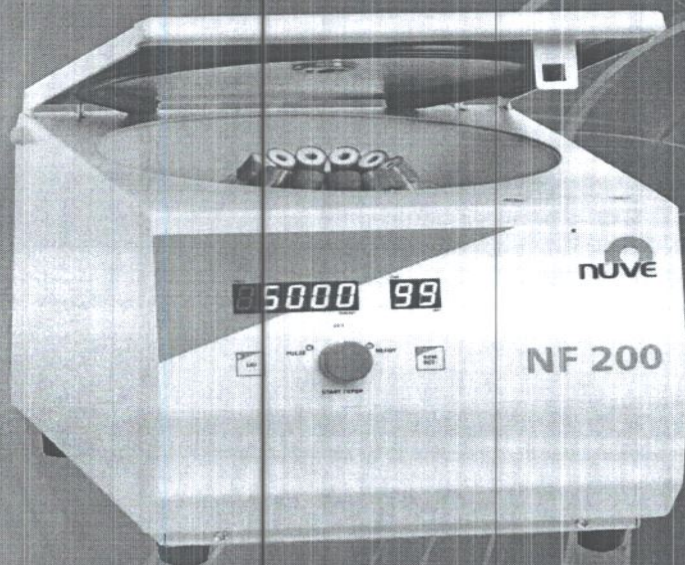

- Compact design for separation of blood samples, urine particle sedimentation and other routine applications in emergency and small laboratories
- N-Prime™ programmable microprocessor control system for accurate and reliable operations
- Easy programming with one button, just turn and push
- Two large LED displays for speed/RCF and time
- Possibility of programming RCF
- Pulse key for short centrifugation requirements
- Reduced temperature increase in the chamber by means of continuous air cooling through air channel in the lid
- Quiet brushless induction drive
- Safety ensured by steel body, lid and chamber, lid locking system and motor over temperature protection
- Delivered with 12x15 ml. angle rotor

N-prime

TECHNICAL SPECIFICATIONS


Maximum Speed	5.000 rpm
Maximum RCF	2.822xg
Tube Capacity	12x15 ml.
Control System	N-Prime™ Programmable Microprocessor Control
Speed Set Range	1.000-5.000 rpm
Speed Set Step	10 rpm
Timer Set Range	1-99 Minutes and Hold Position
Timer Set Step	1 minute
Motor	Induction Motor
Body, Lid and Chamber	Epoxy-Polyester Powder Coated Steel
Power Supply	230 V / 50-60 Hz (115 V / 60 Hz)
Power Consumption	150 W
External Dimensions (WxDxH) mm.	280x360x260
Packing Dimensions (WxDxH) mm.	350x420x480
Net / Packed Weight, kg.	12 / 16

ROTOR

Rotor Type	Capacity	Max. Tube Dia. (mm)	Radius (mm)	Max. Speed	Max. RCF
Angle	12x15 ml.	17	101	5.000 rpm	2.822xg

ADAPTORS

Code	Tube Type	Max. Tube Dia. (mm)
G 03 057	1.5/2 ml tubes	11
G 03 014	7 ml vacuumed/ non vacuumed tubes	13
G 03 015	5 ml vacuumed/ non vacuumed tubes	13

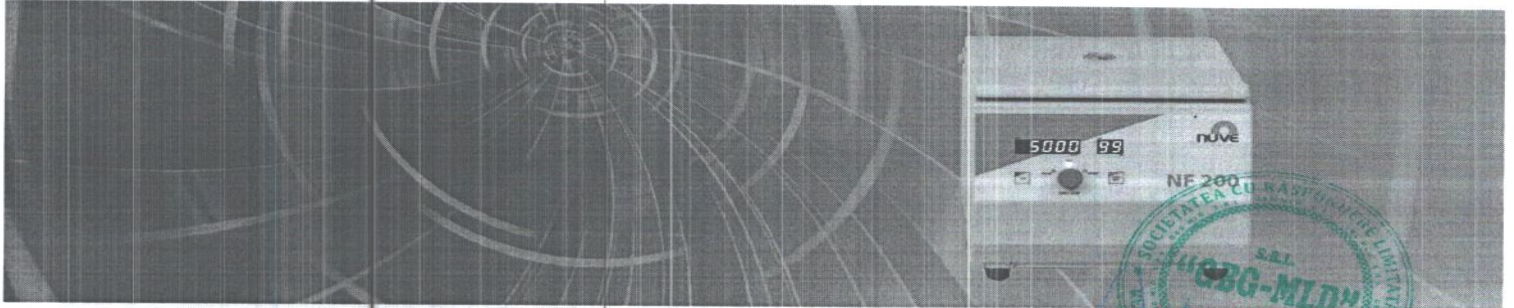

NÜVE SANAYİ MALZEMELERİ İMALAT VE TİCARET A.Ş.

Saracalar Mah. Saracalar Kümevleri No: 4/2 Akyurt 06750 ANKARA / TURKEY t. +90 312 399 28 30 f. --90 312 399 21 97
nuve.com.tr sales@nuve.com.tr

ISO 9001: 2008
ISO 13485: 2003



EC DECLARATION OF CONFORMITY

We, NÜVE Sanayi Malzemeleri İmalat ve Ticaret A.Ş.
Saracalar Mah. Saracalar Kümeevleri No: 4/2
Akyurt 06750 Ankara / TURKEY

Herewith declare that the following described product meets the provisions of the following directives. All supporting documentation is retained under the premises of the manufacturer.

PRODUCT:

CENTRIFUGE

MODEL:

NF 200

APPLICABLE EC DIRECTIVES

LVD : 93/68/EEC & 2006/95/EC

EMC :92/31/EEC & 2004/108/EC

APPLICABLE HARMONISED STANDARDS:

EN 61010-1
EN 61010-2-020
EN 61000-6-2
EN 55011

DATE OF ISSUE:

March 01, 2014

SIGNATURE:


GBG-MLD
N:6
Beril İZGİN
General Manager

CE

3D-IW8, Inteliwasher

DESCRIPTION

Inteliwasher 3D-IW8 series microplate washer is designed for washing various types of standard 96-well microtitre plates, microstrips as well as microarrays on FastFRAME (rectangular well shape). It is suitable for washing wells with different bottom shapes: flat, U-shape and V-shape. The unit is fully programmable ensuring multi-step solution ripening, aspiration (aspiration, combination of aspiration/liquid dispensing and soaking, as well as soaking cycle during a particular period of time). Dispense system of liquid dosage for each channel separately.

The unit provides:

- Washing mode
- Rinsing mode
- Mixing mode
- Single point, two point, circular (circle or rectangular path) aspiration
- Possibility of additional solution mixing during time gap between two work cycles
- Possibility to use microtest plates by different manufacturers, ensured by automated plate set up (adjusting to different depths of plate wells)
- Round-bottom plate and strip washing mode
- Possibility of user-defined programs with adjustable parameters


The unit has 50 programs divided into 5 following aspiration categories (see figure leftward):

- Type 1 (1.0–1.9) IPF96 U/V is intended for round and V-shape immunoplates, 1 point aspiration.
- Type 2 (2.0–2.9) IPF96 FLAT-2 is intended for flat-bottom shape immunoplates, 2 point aspiration.
- Type 3 (3.0–3.9) IPF96 FLAT-C is intended for rectangular shape immunoplates, full-circle aspiration direction.
- Type 4 (4.0–4.9) FastFRAME-2 is intended for multi-slide plate* with rectangular wells.
- Type 5 (5.0–5.9) FastFRAME-C is intended for multi-slide* plate with rectangular wells.

* - The FastFRAME (GVS Life Sciences) multi-slide plate or analog plate of another manufacturer, that is compatible with standard 25 x 76 mm (1 x 3 inch) glass slides.

The unit is designed for use in closed laboratory rooms at temperatures from +10°C to +35°C and relative humidity up to 80% at +25°C decreasing linearly to 50% relative humidity at 35°C.

4-channel washing solution weight logger, **4 CHW Logger** provides automatic control of rinsing solution and waste volumes. The washer shows remaining volume for each bottle as percentage and gives a warning message in case of low solution volume or full waste bottle when **4 CHW Logger** is connected.

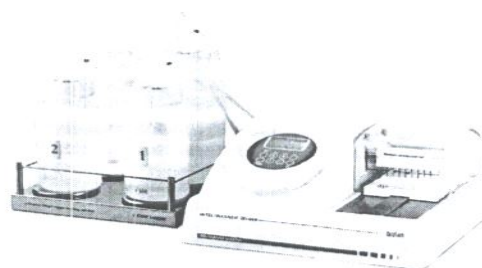

CAT. NUMBER


BS-060102-AA1	230VAC 50/60Hz Euro plug
BS-060102-AAB	230VAC 50/60Hz UK plug
BS-060102-AA4	230VAC 50/60Hz AU plug
BS-060102-AAJ	100VAC 50/60Hz US plug / 120VAC 60Hz US plug
IVD certified	IVD certified
BS-060102-IVD1	230VAC 50/60Hz Euro plug
BS-060102-IVD2	230VAC 50/60Hz UK plug
BS-060102-IVD3	100VAC 50/60Hz US plug
BS-060102-BK	IQ/OQ document
BS-060102-CK	PQ document



SPECIFICATIONS

Minimum dispense volume	25 µl
Maximum dispense volume	1600 µl
Dispense increment	25 µl
Dispensing accuracy	±2.5%
Allowed residual liquid volume in plate well	not more than 2 µl
Number of wells washed simultaneously	8
Number of washing cycles	1–15
Aspiration time	1–3 s
Final aspiration time	1–3 s
Aspiration/dispensing speed	3 levels
Max. number of channels in a program	2
Choice of 3 washing liquid bottles	+
Soaking time	0–300 s (increment 10 s)
Shaking time	0–150 s (increment 5 s)
Number of washed rows	1 – 12
Time of one plate wash (300 µl), not more	45 s
Number of programs	50
Plate platform and washing head movement	automated
Indication of operation modes	LCD, 8-line
Overall dimensions (W×D×H)	375 x 345 x 180 mm
Weight	9.9 kg
Input current/power consumption	12 V DC, 1.8 A / 22 W
External power supply	Input AC 100–240 V; 50/60 Hz; Output DC 12 V



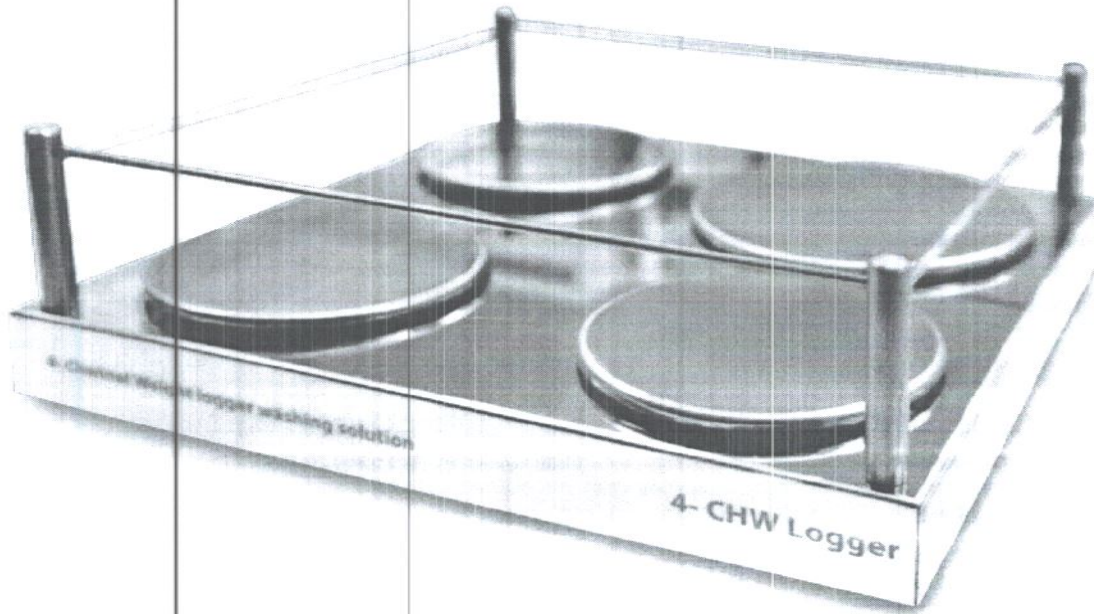

4-CHW Logger
BS-060102-AK

4-channel washing solution weight logger, 4 CHW Logger provides automatic control of rinsing solution and waste volumes. The washer shows remaining volume for each bottle as percentage and gives a ...

[read more](#)



EU Declaration of Conformity

Unit type Microplate washers
Models IW-8, 3D-IW8
Serial number 14 digits styled XXXXXYYMMZZZZ, where XXXXXX is model code, YY and MM – year and month of production, ZZZZ – unit number.
Manufacturer SIA BIOSAN
 Latvia, LV-1067, Riga, Ratsupites str. 7/2

The objects of the declaration described above is in conformity with the following relevant Union harmonization legislations:

LVD 2014/35/EU	LVS EN 61010-1:2011 Safety requirements for electrical equipment for measurement, control, and laboratory use. General requirements.
EMC 2014/30/EU	LVS EN 61326-1:2013 Electrical equipment for measurement, control and laboratory use. EMC requirements. General requirements.
RoHS3 2015/863/EU	Directive on the restriction of the use of certain hazardous substances in electrical and electronic equipment.
WEEE 2012/19/EU	Directive on waste electrical and electronic equipment.

I declare that the Declaration of Conformity is issued under sole responsibility of the manufacturer and belongs to the above-mentioned objects of the declaration.

Svetlana Bankovska
Managing director

Signature

Date

07.02.2020.

