

AVAILABLE ITEMS

Group	Catalog No.	Item	Specimen	Reaction time	Measurement range	
Cardiac markers	VID09-03-011	cTnI	WB/S/P	15 min	0.1-50 ng/mL	
	VID10-03-011	CK-MB	WB/S/P	15 min	0.3-100 ng/mL	
	VID11-03-011	D-Dimer	WB/P	10 min	0.05-10 µg/mL	
	VID12-03-011	MYO	WB/S/P	8 min	2-400 ng/mL	
	VID13-03-011	H-FABP	WB/S/P	5 min	1-120 ng/mL	
	VID14-03-011	NT-proBNP	WB/S/P	15 min	18-35000 pg/mL	
	VID15-03-011	cTnI/CK-MB/MYO	WB/S/P	15 min	Same as single item	
	VID45-03-011	cTnI/CK-MB	WB/S/P	15 min	Same as single item	
	VID60-03-011	cTnT	WB/S/P	15 min	0.1-10ng/mL	
Inflammation	VID01-01-011	hsCRP/CRP ▲	WB/S/P	3 min	0.5-200 mg/L	
	VID02-01-011	PCT	WB/S/P	10 min	0.1-50 ng/mL	
	VID04-01-011	SAA	WB/S/P	10 min	5-100 mg/L	
	VID05-01-011	IL-6	WB/S/P	15 min	3-2000 pg/mL	
	VID119-01-011	Anti-CCP	S/P	15 min	3.5-300 U/mL	
Renal function	VID03-02-011	Cys C	WB/S/P	3 min	0.5-10 mg/L	
	VID06-02-011	MAU	U	3 min	10-200 mg/L	
	VID07-02-011	β2-MG	WB/S/P	3 min	0.5-20 mg/L	
	VID08-02-011	NGAL	WB/S/P	3 min	25-1600 ng/mL	
Diabetes	VID16-04-011	HbA1c ▲	WB	5 min	4-16%	
Hormone	VID19-05-011	β-hCG	WB/S/P	15 min	2-4000 mIU/mL	
	VID20-05-011	TSH	WB/S/P	15 min	0.1-100 mIU/L	
	VID21-05-011	T3	S/P	15 min	0.61-10 nmol/L	
	VID22-05-011	T4	S/P	15 min	20-310 nmol/L	
	VID23-05-011	LH	WB/S/P	10 min	1-200 mIU/mL	
	VID30-05-011	AMH	S/P	15 min	0.08-20 ng/mL	
	VID31-05-011	FSH	WB/S/P	15 min	0.1-200 mIU/mL	
	VID32-05-011	PRL NEW	WB/S/P	15 min	20-4000 mIU/L	
	VID55-05-011	Progesterone	S/P	10 min	0.8-50 ng/mL	
	VID56-05-011	Testosterone	S/P	15 min	0.2-15 ng/mL	
Drug of abuse	VID37-09-011	MOP	H	5 min	0.1-5 ng/mg	
	VID38-09-011	MET	H	5 min	0.1-5 ng/mg	
	VID39-09-011	KET	H	5 min	0.1-5 ng/mg	
	VID46-09-011	MOP/MET/KET	H	5 min	Same as single item	
	VID24-06-011	PSA ▲	WB/S/P	15 min	0.5-100 ng/mL	
	VID25-06-011	AFP	WB/S/P	15 min	2-400 ng/mL	
Tumor markers	VID26-06-011	CEA	WB/S/P	15 min	1-400 ng/mL	
	VID27-06-011	FOB	F	5 min	25-2000 ng/mL	
	VID61-10-011	IgE	WB/S/P	15 min	1-1000 IU/mL	
	VID36-08-011	Flu A+B Ag	Swab	15 min	Negative/Positive	
Infectious diseases	VID44-08-011	SARS-CoV-2 Ag	Swab	15 min	Negative/Positive	
	VID49-08-011	Anti-SARS-CoV-2 S ▲	WB/S/P	15 min	0.4-250 BAU/mL	
	VID87-01-011	Dengue IgM/IgG ▲ NEW	WB/S/P	15 min	Negative/Positive	
	VID88-01-011	Dengue NS1 Ag ▲ NEW	WB/S/P	15 min	Negative/Positive	
	VID104-01-011	HBsAg	WB/S/P	15 min	Negative/Positive	
	VID107-01-011	Strep A	Swab	5 min	Negative/Positive	
	VID122-01-011	RSV NEW	Swab	10min	Negative/Positive	
	VID166-01-011	Adeno NEW	Swab	10min	Negative/Positive	
	Others	VID29-07-011	25-OH-D3 ▲	WB/S/P	15 min	4-100 ng/mL
		VID28-07-011	FER	WB/S/P	10 min	5-1500 ng/mL
VID106-07-011		CAL	F	10 min	10-1000 mg/kg	

WB=Whole blood; S=Serum; P=Plasma; U=Urine; F=Feeces; H=Hair; min=minutes; fingerstick=▲



VivaChek Biotech (Hangzhou) Co., Ltd.
Level 2, Block 2, 146 East Chaofeng Rd.,
Yuhang Economy Development Zone,
Hangzhou, 311100, Zhejiang, P.R. China
www.vivachek.com

Not Available for Sales in the US

Number: 1606012506
Effective Date: 2025-01-15
©2025 VivaChek Biotech (Hangzhou) Co., Ltd.

VivaChek



VIM3000

VIVACHEK

VivaDiag POCT Analyzer

VivaDiag VIM3000

Test Procedures

— Nasal swab, oropharyngeal swab or nasopharyngeal swab



— Blood or urine



— Hair



Advanced Features



User-friendly interface



Touch screen



Batch test





Unit Conversions

Specification

Analyzer	Specification
Model	VIM3000
Size	192 x 209 x 169 mm
Weight	1.8 kg
Screen	7" color touch screen
Sample type	Whole blood, serum, plasma, urine, hair, etc.
Coding	ID Card
Operation temperature	5 ~ 40°C
Storage temperature	-10 ~ 55°C
Connectivity	Ethernet port RJ-45, USB
Power	AC/DC adapter
Printer	Built-in thermal printer
Memory	10000 results

Clinical Performance

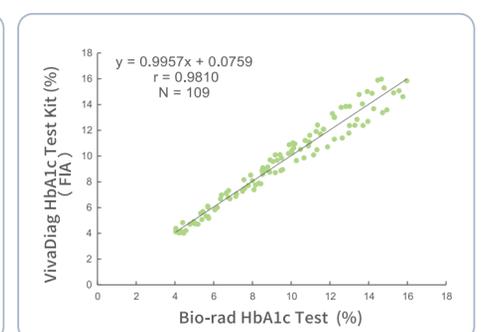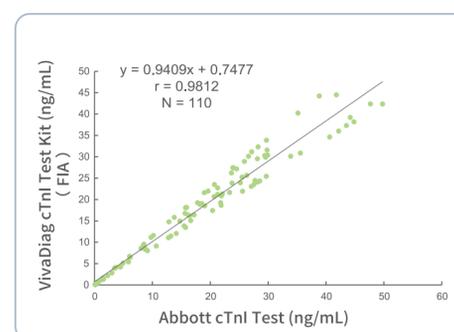

VIM3000

VivaChek



VIM3000

VIVACHEK

VivaDiag POCT Analyzer



VivaDiag VIM3000

Test Procedures

— Nasal swab, oropharyngeal swab or nasopharyngeal swab



— Blood or urine



— Hair



Advanced Features



User-friendly interface



Touch screen



Batch test





Unit Conversions

VIM3000

Specification

Analyzer	Specification
Model	VIM3000
Size	192 x 209 x 169 mm
Weight	1.8 kg
Screen	7" color touch screen
Sample type	Whole blood, serum, plasma, urine, hair, etc.
Coding	ID Card
Operation temperature	5 ~ 40°C
Storage temperature	-10 ~ 55°C
Connectivity	Ethernet port RJ-45, USB
Power	AC/DC adapter
Printer	Built-in thermal printer
Memory	10000 results

Clinical Performance

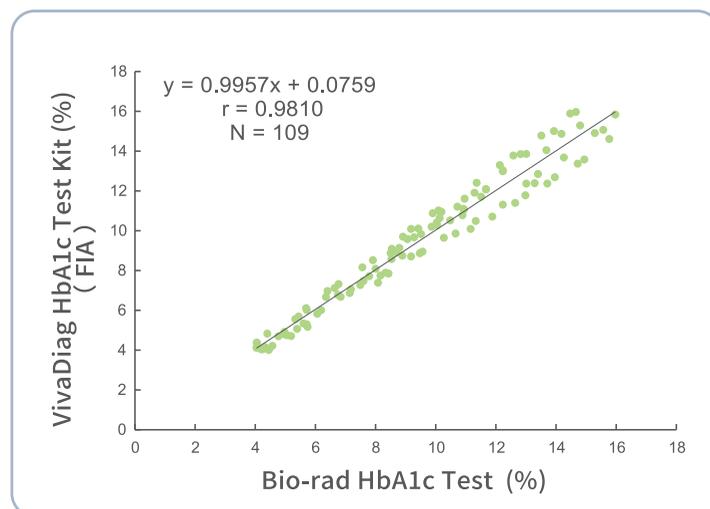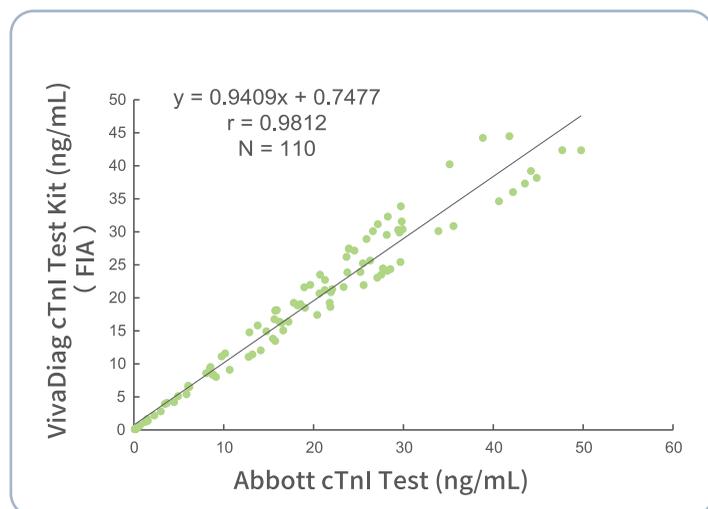

AVAILABLE ITEMS

Group	Catalog No.	Item	Specimen	Reaction time	Measurement range
Cardiac markers	VID09-03-011	cTnI	WB/S/P	15 min	0.1-50 ng/mL
	VID10-03-011	CK-MB	WB/S/P	15 min	0.3-100 ng/mL
	VID11-03-011	D-Dimer	WB/P	10 min	0.05-10 µg/mL
	VID12-03-011	MYO	WB/S/P	8 min	2-400 ng/mL
	VID13-03-011	H-FABP	WB/S/P	5 min	1-120 ng/mL
	VID14-03-011	NT-proBNP	WB/S/P	15 min	18-35000 pg/mL
	VID15-03-011	cTnI/CK-MB/MYO	WB/S/P	15 min	Same as single item
	VID45-03-011	cTnI/CK-MB	WB/S/P	15 min	Same as single item
	VID60-03-011	cTnT	WB/S/P	15 min	0.1-10ng/mL
Inflammation	VID01-01-011	hsCRP/CRP ▲	WB/S/P	3 min	0.5-200 mg/L
	VID02-01-011	PCT	WB/S/P	10 min	0.1-50 ng/mL
	VID04-01-011	SAA	WB/S/P	10 min	5-100 mg/L
	VID05-01-011	IL-6	WB/S/P	15 min	3-2000 pg/mL
	VID119-01-011	Anti-CCP	S/P	15 min	3.5-300 U/mL
Renal function	VID03-02-011	Cys C	WB/S/P	3 min	0.5-10 mg/L
	VID06-02-011	MAU	U	3 min	10-200 mg/L
	VID07-02-011	β2-MG	WB/S/P	3 min	0.5-20 mg/L
	VID08-02-011	NGAL	WB/S/P	3 min	25-1600 ng/mL
Diabetes	VID16-04-011	HbA1c ▲	WB	5 min	4-16%
Hormone	VID19-05-011	β-hCG	WB/S/P	15 min	2-4000 mIU/mL
	VID20-05-011	TSH	WB/S/P	15 min	0.1-100 mIU/L
	VID21-05-011	T3	S/P	15 min	0.61-10 nmol/L
	VID22-05-011	T4	S/P	15 min	20-310 nmol/L
	VID23-05-011	LH	WB/S/P	10 min	1-200 mIU/mL
	VID30-05-011	AMH	S/P	15 min	0.08-20 ng/mL
	VID31-05-011	FSH	WB/S/P	15 min	0.1-200 mIU/mL
	VID32-05-011	PRL NEW	WB/S/P	15 min	20-4000 mIU/L
	VID55-05-011	Progesterone	S/P	10 min	0.8-50 ng/mL
	VID56-05-011	Testosterone	S/P	15 min	0.2-15 ng/mL
	VID63-05-011	ft4	S/P	15 min	5-100 pmol/L
	VID64-05-011	ft3	S/P	15 min	2-50 pmol/L
	Drug of abuse	VID37-09-011	MOP	H	5 min
VID38-09-011		MET	H	5 min	0.1-5 ng/mg
VID39-09-011		KET	H	5 min	0.1-5 ng/mg
VID46-09-011		MOP/MET/KET	H	5 min	Same as single item
Tumor markers	VID24-06-011	PSA ▲	WB/S/P	15 min	0.5-100 ng/mL
	VID25-06-011	AFP	WB/S/P	15 min	2-400 ng/mL
	VID26-06-011	CEA	WB/S/P	15 min	1-400 ng/mL
	VID27-06-011	FOB	F	5 min	25-2000 ng/mL
Autoimmune	VID61-10-011	IgE	WB/S/P	15 min	1-1000 IU/mL
Infectious diseases	VID36-08-011	Flu A+B Ag	Swab	15 min	Negative/Positive
	VID44-08-011	SARS-CoV-2 Ag	Swab	15 min	Negative/Positive
	VID49-08-011	Anti-SARS-CoV-2 S ▲	WB/S/P	15 min	0.4-250 BAU/mL
	VID87-01-011	Dengue IgM/IgG NEW	WB/S/P	15 min	Negative/Positive
	VID88-01-011	Dengue NS1 Ag NEW	WB/S/P	15 min	Negative/Positive
	VID104-01-011	HBsAg	WB/S/P	15 min	Negative/Positive
	VID107-01-011	Strep A	Swab	5 min	Negative/Positive
	VID122-01-011	RSV NEW	Swab	10min	Negative/Positive
	VID166-01-011	Adeno NEW	Swab	10min	Negative/Positive
Others	VID29-07-011	25-OH-D3 ▲	WB/S/P	15 min	4-100 ng/mL
	VID28-07-011	FER	WB/S/P	10 min	5-1500 ng/mL
	VID106-07-011	CAL	F	10 min	10-1000 mg/kg

WB=Whole blood; S=Serum; P=Plasma; U=Urine; F=Feces; H=Hair; min=minutes; fingerstick= ▲



VivaChek Biotech (Hangzhou) Co., Ltd.
Level 2, Block 2, 146 East Chaofeng Rd.,
Yuhang Economy Development Zone,
Hangzhou, 311100, Zhejiang, P.R. China
www.vivachek.com

Not Available for Sales in the US

Number: 1606012506
Effective Date: 2025-01-15
©2025 VivaChek Biotech (Hangzhou) Co., Ltd.