


AL-1303-060.V009

Adult Anesthesia Circuit Extendible PP Tube 200cm, 150cm limb, 2lt neoprene brathing bag

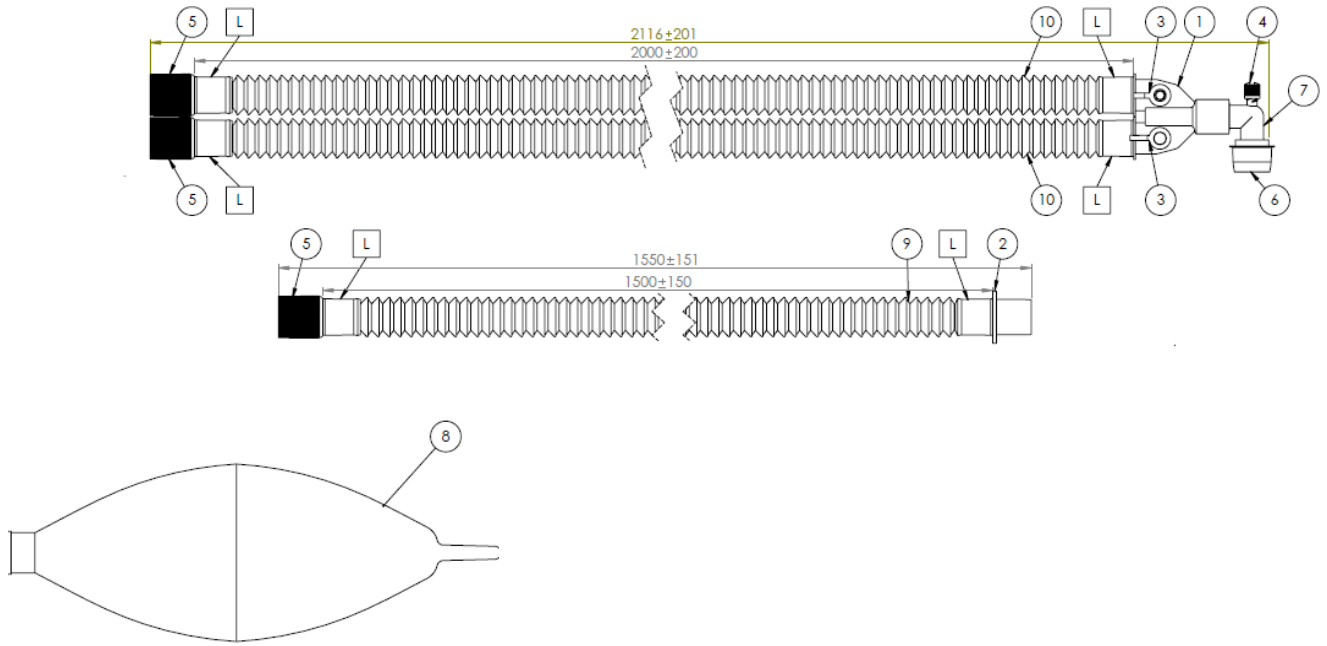

1. Manufacturer:

Meditera Tibbi Malzeme Sanayi ve Ticaret A.Ş.

2. Sterilization Method :

Ethylene oxide sterilization. This product line is provided both as sterile and nonsterile.

3. Packaging:

Nylon packaging.

4. Intended Use and Functional Description :

Disposable circuits used to conduct medical gases from the anaesthesia system to the patient. Anaesthetic gas exits the anaesthesia machine (via the common gas outlet) and then enters a breathing circuit. The function of the circuit is to deliver oxygen and anaesthetic gases to the patient and to eliminate CO₂. The CO₂ may be eliminated by gas inflow or by soda lime absorption.

5. Shelf life :

5 years from the date of production .

6. Product Description:

6.1. Classification: Class IIa Rule 2

6.2. This product does not contain any metallic parts

6.3. **Spesification of the product :**

Item	Description	Quantity
150.07.040	2 LT NEOPRENE SINGLE FOLDED BREATHING BAG WITH STICKER(RIGID PP CONNECTOR)	1
150.11.036	ELBOW CONNECTOR LUER CAP	1
151.03.001.01	22 MM STRAIGHT CONNECTOR	3
151.03.021.01	LONG CONNECTOR CAP RED	1
151.03.074	Y CONNECTOR CAP	2
151.03.110	22-22MM STRAIGHT CONNECTOR	1
151.03.150	22 MM PARALLEL Y CONNECTOR PP	1
151.03.178.01	ELBOW CONNECTOR WITH CO2 PORT PP	1
151.05.02.203	22 MM EXTENDIBLE TUBING 150 CM CUT	1
151.05.02.218	22 MM EXTENDIBLE TUBING PP 200 CM CUT	2

7. Standarts:

EN ISO 13485:2016, 93/42/EEC Medical Device Directive, EN 556-1:2001, EN ISO 11607-1:2020, EN ISO 11607-2:2020, EN ISO 23328-1, EN ISO 23328-2

8. Waste Method:

After use product will be “contaminated medical waste” and package will be “packaging waste” so they should be handled according to relevant national and international standards and regulations.