Declaration of Conformity

According to annex III of the Council Directive 98/79/EC on in vitro diagnostic medical device We,

EKVITESTLAB LLC

Velyka Vasylkivska St. 114, Kyiv, Ukraine, 03150, tel. 0(800)31-89-87; +38 (044)334-89-87
e-mail: info@equitest.com.ua, web-site: www.equitest.com.ua

Declare under our sole responsibility that the following in vitro diagnostic medical devices other than those covered by annex II and devices for performance evaluation

EQUI anti-Lamblia - ELISA kit for the qualitative detection of antibodies to *Giardia lamblia (intestinalis)*, REF EI-606

Meet the provisions of the Council Directive 98/79/EC concerning medical devices which apply to them.

Undersigned declares to fulfill the obligations imposed by Annex III section 2 to 5:
- availability of the technical documentation set in Annex III (section 3), allowing the assessment of conformity of the product with the requirements of the Directive.
- the manufacturer shall take necessary measures to ensure that the manufacturing process follows the principles of quality assurance as appropriate for the products manufactured (Annex III section 4).
- the manufacturer shall institute and keep up to date a systematic procedure to review experience gained from devices in the post-production phase and to implement appropriate means to apply any necessary corrective actions (Annex III section 5).

Conformity assessment was performed according to Article 9 (7) and Annex III, section 3.

Our current Quality System is formatted to international standards:

- **ISO 13485:2016 «Medical devices — Quality management systems — Requirements for regulatory purposes»**

Digitally signed by Monastîrschii Viorica
Date: 2023.01.06 12:36:40 EET
Reason: MoldSign Signature
Location: Moldova

Corporate Contact Information

EKVITESTLAB LLC
Velyka Vasylkivska St. 114, Kyiv, Ukraine, 03150
tel. 0(800)31-89-87; +38 (044)334-89-87
e-mail: info@equitest.com.ua
RESPONSIBLE PERSON'S name: Anna Yurchuk
Position: Director

SIGNATURE :

Date : October 25, 2021
Stamp

European Authorized Representative:
Registered Address:
Obelis s.a.
Bd. Général Wahis 53
B-1030 Brussels, Belgium
Phone: 32.2.732.59.54
Fax: 32.2.732.60.03
E-mail: mail@obelis.net
Representative: Mr. Gideon ELKAYAM (CEO)

Declaration of Conformity

According to annex III of the Council Directive 98/79/EC on in vitro diagnostic medical device
We,

EKVITESTLAB LLC

Velyka Vasylkivska St. 114, Kyiv, Ukraine, 03150, tel. 0(800)31-89-87; +38 (044)334-89-87
e-mail: info@equitest.com.ua, web-site: www.equitest.com.ua

Declare under our sole responsibility that the following in vitro diagnostic medical devices other than those covered by annex II and devices for performance evaluation

EQUI Ascaris lumbricoides IgG - ELISA kit for the qualitative detection of IgG antibodies to *Ascaris lumbricoides*, REF EI-601

Meet the provisions of the Council Directive 98/79/EC concerning medical devices which apply to them.

Undersigned declares to fulfill the obligations imposed by Annex III section 2 to 5:
- availability of the technical documentation set in Annex III (section 3), allowing the assessment of conformity of the product with the requirements of the Directive.
- the manufacturer shall take necessary measures to ensure that the manufacturing process follows the principles of quality assurance as appropriate for the products manufactured (Annex III section 4).
- the manufacturer shall institute and keep up to date a systematic procedure to review experience gained from devices in the post-production phase and to implement appropriate means to apply any necessary corrective actions (Annex III section 5).

Conformity assessment was performed according to Article 9 (7) and Annex III, section 3.

Our current Quality System is formatted to international standards:

- **ISO 13485:2016 «Medical devices — Quality management systems — Requirements for regulatory purposes»**

Corporate Contact Information

EKVITESTLAB LLC
Velyka Vasylkivska St. 114, Kyiv, Ukraine, 03150
tel. 0(800)31-89-87; +38 (044)334-89-87
e-mail: info@equitest.com.ua
RESPONSIBLE PERSON'S name: Anna Yurchuk
Position: Director

SIGNATURE :

Date : October 25, 2021
Stamp

European Authorized Representative:
Registered Address:
Obelis s.a.
Bd. Général Wahis 53
B-1030 Brussels, Belgium
Phone: 32.2.732.59.54
Fax: 32.2.732.60.03
E-mail: mail@obelis.net
Representative: Mr. Gideon ELKAYAM (CEO)

Declaration of Conformity

According to annex III of the Council Directive 98/79/EC on in vitro diagnostic medical device
We,

EKVITESTLAB LLC

Velyka Vasylkivska St. 114, Kyiv, Ukraine, 03150, tel. 0(800)31-89-87; +38 (044)334-89-87

e-mail: info@equitest.com.ua, web-site: www.equitest.com.ua

Declare under our sole responsibility that the following in vitro diagnostic medical devices other than those covered by annex II and devices for performance evaluation

EQUI Toxocara canis IgG - ELISA kit for the qualitative detection of IgG antibodies to *Toxocara canis*, REF EI-603

Meet the provisions of the Council Directive 98/79/EC concerning medical devices which apply to them.

Undersigned declares to fulfill the obligations imposed by Annex III section 2 to 5:
- availability of the technical documentation set in Annex III (section 3), allowing the assessment of conformity of the product with the requirements of the Directive.
- the manufacturer shall take necessary measures to ensure that the manufacturing process follows the principles of quality assurance as appropriate for the products manufactured (Annex III section 4).
- the manufacturer shall institute and keep up to date a systematic procedure to review experience gained from devices in the post-production phase and to implement appropriate means to apply any necessary corrective actions (Annex III section 5).

Conformity assessment was performed according to Article 9 (7) and Annex III, section 3.

Our current Quality System is formatted to international standards:

- **ISO 13485:2016 «Medical devices — Quality management systems — Requirements for regulatory purposes»**

Corporate Contact Information

EKVITESTLAB LLC
Velyka Vasylkivska St. 114, Kyiv, Ukraine, 03150
tel. 0(800)31-89-87; +38 (044)334-89-87
e-mail: info@equitest.com.ua
RESPONSIBLE PERSON’S name: Anna Yurchuk
Position: Director

SIGNATURE :

Date : October 25, 2021
Stamp

European Authorized Representative:
Registered Address:
Obelis s.a.
Bd. Général Wahis 53
B-1030 Brussels, Belgium
Phone: 32.2.732.59.54
Fax: 32.2.732.60.03
E-mail: mail@obelis.net
Representative: Mr. Gideon ELKAYAM (CEO)

Obelis SA
EUROPEAN AUTHORIZED
REPRESENTATIVE CENTER

EUROPEAN RESPONSIBLE PERSON CENTER
Obelis SA
SINCE 1988

E.A.R.-CERTIFICATE

(ART 10.3 of the Directive 98/79/EC on In Vitro Diagnostic)

REF. NO. : RP 2901-2021
ORDER NO. : DK 2491-2021

DATE: 11/01/2022

MANUFACTURER:
EKVITESTLAB LLC
Velyka Vasylkivska street, 114
03150, Kyiv, Ukraine

FACILITIES:
EKVITESTLAB LLC
Peremohy Avenue, 60/2
03057, Kyiv, Ukraine

PRODUCT CATEGORIES: Please See Annex A - List of Devices (13 Devices, 2 Pages)

MODELS: Please See Annex A - List of Devices (13 Devices, 2 Pages)

The European Authorized Representative Center Obelis s.a. declares that the aforementioned manufacturer has fulfilled the essential requirement of appointing a European Authorized Representative in accordance with article 10.3 of the Directive 98/79/EC and to the terms and conditions set out in the agreement entered into force on 1st May 2021.*

G. ELKAYAM
C.E.O.

Obelis s.a. - O.E.A.R.C.
Registered Address :
Bld Général Wahis 53
1030 Bruxelles
Tél. +32 2 732 59 54 - Fax +32 2 732 60 03

Mr. G. Elkayam CEO
Obelis sa

EA AR

Obelis European Authorized Representative Center is a member of the European Association of Authorized Representatives (E.A.R.), ISO 9001 : 2015 and ISO 13485 : 2016 certified in accordance to the profession of a European Authorized Representative.

* This is not a CE mark and is only provided as a template for informational purposes.

*This certificate is not a confirmation of product notification nor an approval to place products on the market.
**This certificate will become void automatically upon termination of the EAR agreement.

Order No.: DK 2491-2021
Reference No.: RP 2901-2021

ANNEX to IVDD EAR Certificate

Manufacturer: Ekvitestlab LLC

Country: Ukraine

#	EMDN	Generic device name (including BASIC UDI)	Commercial Name of device	Intended use	Class
1	52133	EQUI Ascaris lumbricoides IgG	EI-601	ELISA kit for the qualitative detection of IgG antibodies to Ascaris lumbricoides	Class I (Others)
2	63005	EQUI Opisthorchis felineus IgG	EI-602	ELISA kit for the qualitative detection of IgG antibodies to Opisthorchis felineus	Class I (Others)
3	52418	EQUI Toxocara canis IgG	EI-603	ELISA kit for the qualitative detection of IgG antibodies to Toxocara canis	Class I (Others)
4	52464	EQUI anti-Trichinella spiralis	EI-605	ELISA kit for the qualitative detection of antibodies to Trichinella spiralis	Class I (Others)
5	52464	EQUI anti-Trichinella spiralis	EI-605	ELISA kit for the qualitative detection of antibodies to Trichinella spiralis	Class I (Others)
6	62915	EQUI anti-Lamblia	EI-606	ELISA kit for the qualitative detection of antibodies to Giardia lamblia (intestinalis)	Class I (Others)
7	48281	EQUI HAV IgM	EI-031	ELISA kit for the qualitative detection of IgM antibodies to hepatitis A virus	Class I (Others)
8	51021	EQUI anti-Helicobacter	EI-501	ELISA kit for the qualitative detection of total antibodies to Helicobacter pylori	Class I (Others)
9	51008	EQUI Helicobacter IgG	EI-502	ELISA kit for the qualitative and semiquantitative detection of IgG antibodies to CagA protein of Helicobacter pylori	Class I (Others)
10	51012	EQUI Helicobacter	EI-504	ELISA kit for the qualitative detection of IgM	Class I (Others)

		IgM		antibodies to CagA protein of Helicobacter pylori	
11	64800	EQUI SARS-CoV-2 IgM swift	EI-165	ELISA kit for the qualitative detection of IgM antibodies to nucleoprotein and spike antigens of SARS-CoV-2 virus	Class I (Others)
12	64830	EQUI SARS-CoV-2 IgA swift	EI-166	ELISA kit for the qualitative detection of IgA antibodies to nucleoprotein and spike antigens of SARS-CoV-2 virus	Class I (Others)
13	64824	EQUI SARS-CoV-2 IgG swift	EI-167	ELISA kit for the qualitative detection of IgG antibodies to nucleoprotein and spike antigens of SARS-CoV-2 virus	Class I (Others)

Date: 11 January 2022

CEO Of Obelis

Gideon Elkayam

G. ELKAYAM
C.E.O.
Obelis s.a. - O.E.A.R.C.
Registered Address :
Bld Général Wahis 53
1030 Bruxelles
Tél. +32 2 732 59 54 - Fax +32 2 732 60 03

CERTIFICATE

MANAGEMENT SYSTEM CERTIFICATION BODY
«CONFORMITY ASSESSMENT BODY «PROMSTANDART», LLC
certifies that the enterprise

EKVITESTLAB
Limited Liability Company
registration code 38745936

legal address:
Ukraine, 03150, Kyiv, 114 Velyka Vasylkivska street,

manufacturer's address:
Ukraine, 04212, Kyiv, 60/2 Peremohy Avenue

has established and applies quality management system for
development, production, storage and sale of ELISA kits for in vitro diagnostic

Audit, № report 2020/015-20.2.1
confirmed that the requirements

ISO 13485:2016
«Medical devices — Quality management systems — Requirements for regulatory purposes»

are performed.

The control of conformity of the certified quality management system to the requirements of the specified standard is carried out by means of supervisory audit, the periodicity and procedures of which are regulated by the program.

Certificate registration number	№ UA.QMS.00014-21
Registered	06 April 2021
Valid until	05 April 2024

80156
DSTU EN ISO/IEC 17021-1

Director of Certification Body
«CAB «PROMSTANDART», LLC

stamp (signature) Sergiy Dubrovskyi

210107

The validity of certificate can be verified by telephone: (056) 742-82-39
or on website of «CAB «PROMSTANDART», LLC: prom-standart.com.ua

ПРОМСТАНДАРТ PROMSTANDART ПРОМСТАНДАРТ PROMSTANDART ПРОМСТАНДАРТ

EKVITESTLAB LLC

Velyka Vasylkivska St. 114
03150 Kyiv, Ukraine
Tel. 0-800-31-89-87
e-mail: info@equitest.com.ua
www.equitest.com.ua

STATEMENT

We, EKVITESTLAB LLC, having a registered office at Velyka Vasylkivska street 114, Kyiv, 03150, Ukraine assign SRL SANMEDICO having a registered office at A. Corobceanu street 7A, apt. 9, Chişinău MD-2012, Moldova, as authorized representative in correspondence with the conditions of directive 98/79/EEC.

We declare that the company mentioned above is authorized to register, notify, renew or modify the registration of medical devices on the territory of the Republic of Moldova.

Date: 03 January 2023

Signature: ____________________

Director, Anna Yurchuk

anti-HBs Calibrators

Комплект калибраторов для количественного определения суммарних антител к поверхносному антигену віруса гепатиту В

Инструкция поприменению

IVD

REF EI-018

Σ 20 анализов

UA.TR.061

EQUI anti-HBs Calibrators

Комплект калибраторов для количественного определения суммарных антител к поверхностному антигену вируса гепатита В

1. НАЗНАЧЕНИЕ

Комплект калибраторов «EQUI anti-HBs Calibrators» предназначен для количественного определения антител к поверхностному антигену вируса гепатита В (HBsAg) в сыворотке или плазме крови человека методом иммуноферментного анализа (ИФА) с целью оценки протективного иммунитета. Комплект используется только с ИФА-наборами «EQUI anti-HBs» и рассчитан как для ручной постановки с автоматическими пипетками и стандартным оборудованием, так и для автоматического иммуноферментного анализатора «открытого» типа.

Целевая группа: доноры; лица-потребители инъекционных наркотиков; реципиенты крови или органов; беременные женщины; дети, рожденные от инфицированных матерей; лица, инфицированные ВИЧ; пациенты с симптомами заболеваний печени.

Применение: ИФА-набор применяется в клинических диагностических лабораториях, в станциях переливания крови, а также в других учреждениях, работающих в области *in vitro* диагностики.

2. КЛИНИЧЕСКОЕ ЗНАЧЕНИЕ

Одним из самых распространенных заболеваний печени является гепатит В. Его этиологический агент - вирус гепатита В (ВГВ). ВГВ относится к семейству *Hepadnaviridae* и содержит двухцепочечную ДНК. Инфекционной формой вируса являются так называемые «частицы Дейна» диаметром 42-49 nm, в белковом составе которых основными являются поверхностный антиген (HBsAg) и коревой антиген (HBcAg).

Клиническая картина гепатита В не позволяет диагностировать его длительное время и отличить от других вирусных гепатитов. Поэтому для скрининговых исследований и подтверждения диагноза важную роль играет лабораторная диагностика, особенно выявления антигенов ВГВ и антител к ним методом ИФА. Первым и основным маркером гепатита В является HBsAg, который обнаруживается в крови через 3-5 недель после инфицирования. Примерно в то же время в крови можно обнаружить ДНК ВГВ и HBeAg, который считается маркером активной репликации вируса и «заразности» крови. ВОЗ рекомендует проводить проверку всей донорской крови на HBsAg, чтобы предотвратить трансмиссивнуй передачу ВГВ. Через 2-3 недели после появления HBsAg появляются антитела IgM к коровому антигену HBcAg, а вскоре после них – анти HBcore IgG, которые быстро достигают высоких уровней. ВВыздоровление от острого гепатита В сопровождается выводом вируса из организма, перестают проявляться HBsAg и анти HBc IgM, появляются антитела к HBeAg. Антитела IgG к коровому антигену персистируют в течение всей жизни и является маркером имеющегося или перенесенного гепатита В, их уровень в крови снижается медленно. Через несколько месяцев после исчезновения из крови HBsAg начинают В и проявляться анти-HBs антитела, которые являются свидетельством перенесенного гепатита наличии иммунитета. В период «серологического окна» между выводом HBsAg и появлением анти-HBs антител маркером инфекции ВГВ является суммарные антитела к коровому антигену, также могут проявляться анти-HBe антитела.

Если после острой фазы не происходит элиминация вируса и не являются анти-HBs антитела, развивается хронический гепатит В. HBsAg продолжает определяться более 6 месяцев, его количество в крови может значительно колебаться. На репликативной стадии хронического гепатита В оказывается ДНК вируса и HBeAg, антител к HBeAg нет.

ВОЗ рекомендует диагностировать острый гепатит В с наличием HBsAg и антител IgM к HBcAg, а хронический - за стойким присутствием HBsAg в течение не менее шести месяцев.

Главным средством профилактики гепатита В является вакцинация, которая рекомендована в первую очередь новорожденным.

После вакцинации организмом вырабатываются анти-HBs антитела и формируется иммунитет у лиц, которые не сталкивались с вирусом гепатита В. Наличие анти-HBs антител на уровне более 10 IU / l (МЕ / л) принято считать нижней границей протективного иммунитета вследствие вакцинации или перенесенного гепатита В.

3. ПРИНЦИП АНАЛИЗА

Количественное определение специфических к HBsAg антител с использованием ИФА-набора «EQUI anti-HBs» и набора калибраторов «EQUI anti-HBs Calibrators» базируется на принципе «сэндвич»-варианта твердофазного ИФА в одноэтапной инкубации. В лунках планшета засорбирован рекомбинантный HBsAg субтипов ad та ay. В каждую лунку добавляются образцы сыворотки или плазмы пациента и конъюгат рекомбинантных белков – аналогов HBsAg, с пероксидазой хрена. Во время инкубации, в случае наличия антител к HBsAg в образце, на твердой фазе формируется комплекс антиген-антитело-антиген («сэндвич»). Несвязанные компоненты удаляются во время отмывания. Иммунные комплексы оказываются путем добавления раствора хромогена 3,3 ‘, 5,5’-тетраметилбензидина (ТМБ) с перекисью водорода. После 30-ти минутной инкубации реакция останавливается добавлением стоп-раствора. Оптическая плотность (ОП) в лунках определяется на спектрофотометре при длине волны 450 / 620-695nm. Интенсивность желтой окраски пропорциональна количеству антител в образце.

4. 4. МАТЕРИАЛЫ И ОБОРУДОВАНИЕ

4.1. Состав набора

CAL 0	1 x 11 ml	**Калибратор 0** Отрицательная сыворотка крови с консервантом (желтый). Хранить при температуре 2-8 °С
CAL 10	1 x 1,5 ml	**Калибратор 10** Раствор с содержанием специфичных к HBsAg иммуноглобулинов в концентрации 10 mIU / ml (мМЕ / мл) с консервантом (сине-зеленый). Хранить при температуре 2-8°С
CAL 50	1 x 1,5 ml	**Калибратор 50** Раствор с содержанием специфичных к HBsAg иммуноглобулинов в концентрации 50 mIU / ml (мМЕ / мл) с консервантом (оранжевый). Хранить при температуре 2-8°С
CAL 100	1 x 1,5 ml	**Калибратор 100** Раствор с содержанием специфичных к HBsAg иммуноглобулинов в концентрации 100 mIU/ml (мМЕ/мл) с консервантом (красный). Хранить при температуре 2-8°С
CAL 200	1 x 1,5 ml	**Калибратор 200** Раствор с содержанием специфичных к HBsAg иммуноглобулинов в концентрации 200 mIU/ml (мМЕ/мл) с консервантом (фмолетовый). ранить при температуре 2-8°С

В состав набора также входят: схема внесения образцов (1 шт.), бланк для построения калибровочной кривой (1 шт.), лист контрольных испытаний и инструкция по применению.

4.2. Дополнительные реактивы, материалы и оборудование

ИФА-набор «EQUI anti-HBs», автоматические пипетки переменного объема на 10–1000 µl и наконечники для них, мерная лабораторная посуда (10–1000 ml), деионизированная или дистиллированная вода, термостат на 37°С, автоматический или полуавтоматический промыватель планшетов (вошер), спектрофотометр (ридер) для микропланшетов на 450/620-695 nm, соответствующие контейнеры для отходов потенциально зараженного материала, таймер, фильтровальная бумага, одноразовые неопудренные перчатки, дезинфицирующие средства.

5. 5. ПРЕДОСТЕРЕЖЕНИЯ И ТЕХНИКА БЕЗОПАСНОСТИ

5.1. Предостережения

Перед проведением анализа внимательно ознакомьтесь с инструкцией по использованию. Достоверность результата зависит от четкого следования процедуре анализа.

- не используйте компоненты ИФА-набора после окончания срока годности;
- не используйте во время анализа и не смешивайте компоненты разных серий, компоненты из наборов разных нозологий или реагенты других производителей в сочетании с набором «EQUI anti-HBs» и «EQUI anti-HBs Calibrators»;
- не замораживайте ИФА-набор или его компоненты;
- после использования реагента закрывайте каждый флакон своей крышкой;
- каждый раз используйте новый наконечник пипетки для внесения образцов или реагентов;
- избегайте попадания прямых солнечных лучей на реагенты ИФА-наборов;
- не используйте реагенты, цвет которых не соответствует указанному в пункте 4.1;
- нне проводите визуальный учет результатов анализа (без использования ридера);
- дополнительное оборудование, находящееся в непосредственном контакте с биологическим материалом или компонентами набора, считается загрязненным и нуждается в очищении и обеззараживании;
- ккомплект калибраторов предназначен для 20 анализов. Компоненты после использования и остатки неиспользованных компонентов должны быть утилизированы.

5.2. Техника безопасности

- все реагенты набора предназначены только для лабораторного профессионального применения в *in vitro* диагностике и могут использоваться только квалифицированным персоналом;
- постановку анализа проводить только в одноразовых неопудренных перчатках и защитных очках;
- не допускается принимать пищу, пить, курить или пользоваться косметикой в комнате проведения теста;
- не пипетировать растворы ртом;
- калибраторы комплекта «EQUI anti-HBs Calibrators» протестированы и признаны отрицательными на HBsAg и антитела к ВИЧ 1/2, ВГС, Treponema pallidum, однако обращаться с калибраторами и исследуемыми образцами следует как с потенциально опасным инфекционным материалом;
- в случае разбрызгивания растворов, не содержащих кислоту, например, сывороток, обработать поверхность дезинфицирующим средством, а затем насухо вытереть фильтровальной бумагой. В ином случае кислоту необходимо сначала нейтрализовать раствором бикарбоната натрия, а затем вытереть поверхность, как описано выше.

5.3. Инактивация и утилиация отходов

- жидкие отходы необходимо инактивировать, например, раствором перекиси водорода в конечной концентрации 6% в течение 3 часов при комнатной температуре или гипохлоритом натрия в конечной концентрации 5% в течение 30 минут или другими разрешенными дезинфицирующими средствами;

– твердые отходы следует инактивировать путем автоклавирования при температуре стерилизации не меньше 132°С;
– не автоклавируйте растворы, содержащие азид натрия или гипохлорит натрия;
– утилизацию инактивированных отходов проводить в соответствии с действующим национальным законодательством.

6. ХРАНЕНИЕ И ТРАНСПОРТИРОВКА

Комплект калибраторов стабилен в течение срока годности, указанного на этикетке, если его хранить при температуре 2-8°С. Транспортировать набор при температуре 2-8°С. Допускается одноразовая транспортировка при температуре не выше 23°С в течение двух суток.

7. РЕКОМЕНДАЦИИ ПО ОТБОРУ, ТРАНСПОРТИРОВКЕ И ХРАНЕНИЮ ОБРАЗЦОВ

Кровь необходимо отбирать из вены в стерильную пробирку. Пробирка должна быть промаркирована с указанием идентификационных данных пациента и даты отбора образца. Цельную кровь до отделения сыворотки можно хранить до 24 часов при температуре 2-8°С, не допуская замораживания.

Сыворотку или плазму крови можно хранить при температуре 2-8°С не более 3 суток. Допускается более продолжительное хранение замороженной сыворотки при температуре -20°С или -70°С. Замороженные образцы перед использованием следует разморозить и выдержать при комнатной температуре в течение 30 минут. После размораживания образцы следует перемешать для достижения однородности. Избегать повторного замораживания-оттаивания исследуемых образцов. В случае помутнения сыворотки (или плазмы) освобождаются от нерастворенных включений центрифугированием при 3000 об/мин в течение 10-15 минут. Не следует использовать образцы сывороток с выраженной липидемией, гемолизом, а также бактериальным проростом.

Образцы сывороток транспортировать в термоизоляционных контейнерах. Для этого закрытые промаркированные пробирки необходимо поместить в полиэтиленовый пакет, плотно запечатать и положить в центре термоконтейнера. Замороженные хладагенты положить на дно вдоль боковых стенок термоконтейнера и накрыть ими образцы сывороток.

8. ПОДГОТОВКА РЕАГЕНТОВ

Примечание: Перед использованием выдержите все компоненты ИФА-набора при комнатной температуре 18-25°С в течение 30 минут!

Комплект калибраторов используется вместе с ИФА-набором «EQUI anti-HBs», поэтому следует подготовить STRIPS, TWEEN WASH 20x и раствор коньюгата в соответствии с пунктами инструкции к ИФА-набору «EQUI anti-HBs».

9. ПРОЦЕДУРА АНАЛИЗА

9.1. Подготовьте необходимое количество лунок для анализа (пять лунок для калибраторов и необходимое количество для исследуемых образцов), вставьте их в рамку планшета ИФА. Лунки с калибраторами обязательно включайте в каждую постановку анализа.

9.2. Заполните схему внесения образцов.

9.3. Приготовьте раствор для промывания в соответствии с инструкцией к ИФА-набору «EQUI anti-HBs».

9.4. Приготовьте раствор коньюгата согласно инструкции к ИФА-набору «EQUI anti-HBs».

9.5. Внесите в лунки по 70 µl калибраторов и исследуемых образцов:
CAL 0 – в лунку A1, CAL 10 – в лунку B1, CAL 50 – в лунку C1,

CAL 100 – в лунку D1, CAL 200 – в лунку E1,
в остальные лунки – исследуемые образцы.

Образцы с ожидаемой концентрацией специфических антител выше CAL 200 (200 mIU/ml (мМЕ/мл)) рекомендуем исследовать в разведении 1:5 (1+4), разведение следует приготовить на CAL 0, что входит в состав набора «EQUI anti-HBs Calibrators». Например, в отдельной пробирке смешать 80 µl CAL 0 и 20 µl исследуемого образца и перенести в лунку планшета 70 µl разведенного образца.

9.6. Внесите в лунки по 35 µl раствора конъюгата поверх контролей и исследуемых образцов. Для предотвращения кросконтаминации образцов внесите раствор конъюгата, не касаясь содержания лунок. Осторожно постукивая по планшету, перемешайте смесь в лунках.

9.7. Заклейте стрипы клейкой пленкой и инкубируйте в течение 120 минут при температуре 37°С.

9.8. По окончании инкубации аккуратно снимите клейкую пленку и промойте лунки пять раз с использованием автоматического промывателя или 8-канальной пипетки следующим образом:
– удалите содержимое лунок в контейнер для жидких отходов;
– наполните лунки стрипов не менее чем по 300 µl раствором для промывания, оставьте не менее, чем на 30 секунд;
– аспирируйте раствор из лунок. Остаточный объем раствора после каждого этапа аспирации должен составлять не больше 5 µl;
– повторите процедуру промывания еще пять раз;
– после последней аспирации избавьтесь от лишней влаги, постукивая планшетом по фильтровальной бумаге.

9.9. Внесите в лунки по 100 µl SOLN TMB, не касаясь дна и стенок лунок планшета.

9.10. Инкубируйте стрипы в течение 30 минут в темном месте при комнатной температуре 18-25°С. Не используйте клейкую пленку на данном этапе.

9.11. Внесите в лунки стрипов по 100 µl SOLN STOP для остановки ферментативной реакции, придерживаясь той же последовательности, что и при внесении SOLN TMB Во время внесения происходит изменение цвета раствора с голубого на желтый, в лунках с прозрачным раствором незначительно меняется оттенок.

9.12. Измерьте на ридере ОП в каждой лунке при длине волны 450/620-695 nm в течение 5 минут после остановки реакции. До проведения измерения убедитесь в чистоте внешней поверхности дна лунок и отсутствии пузырьков.

Учет результатов анализа можно проводить в одноволновом режиме при длине волны 450 nm, в этом случае оставьте лунку для установления бланка (в такую лунку внесите только SOLN TMB *и* SOLN STOP*).*

10. УЧЁТ РЕЗУЛЬТАТОВ И ИХ ИНТЕРПРЕТАЦИЯ

10.1. Контроль достоверности результатов анализа

Данные теста считаются достоверными, если они соответствуют следующим требованиям:

CAL 0	ОП < 0,100
CAL 10	ОП ≥ 0,150
CAL 50	ОП ≥ ОП CAL 10 x 2,5
CAL 100	ОП ≥ ОП CAL 50 x 1,3
CAL 200	ОП ≥ 1,8

10.2. Учет результатов анализа

Для получения количественных результатов определения концентрации специфических к HBsAg антител в mIU/ml (мМЕ/мл) постройте калибровочную кривую: на оси OY отложите полученные значение ОП пяти калибраторов CAL 0, CAL 10, CAL 50, CAL 100 и CAL 200, а на оси OX – соответствующие им концентрации – 0, 10, 50, 100, 200 mIU/ml (мМЕ/мл). При помощи калибровочного графика определите концентрацию (mIU/ml (мМЕ/мл)) специфических антител в исследуемых образцах, которая соответствует значению полученной ОП.

Для образцов, которые исследовались в разведении 1:5, определенную по графику концентрацию специфических антител следует умножить на степень разведения, то есть

конечная концентрация = концентрация по графику × 5

Если содержание специфических к HBsAg антител в исследуемых образцах, взятых в разведении 1:5, больше 200 mIU/ml (мМЕ/мл), следует приготовить другие разведения этих образцов 1:10 (1+9), 1:20 (1+19) или 1:40 (1+39). Конечную концентрацию рассчитывать только для разведения, концентрация которых попадает в диапазон работы калибраторов (10–200 mIU). Для этого определённую по графику концентрацию специфических антител в разведенном образце следует умножить на степень разведения.

Пример калибровочного графика приведен на рисунке

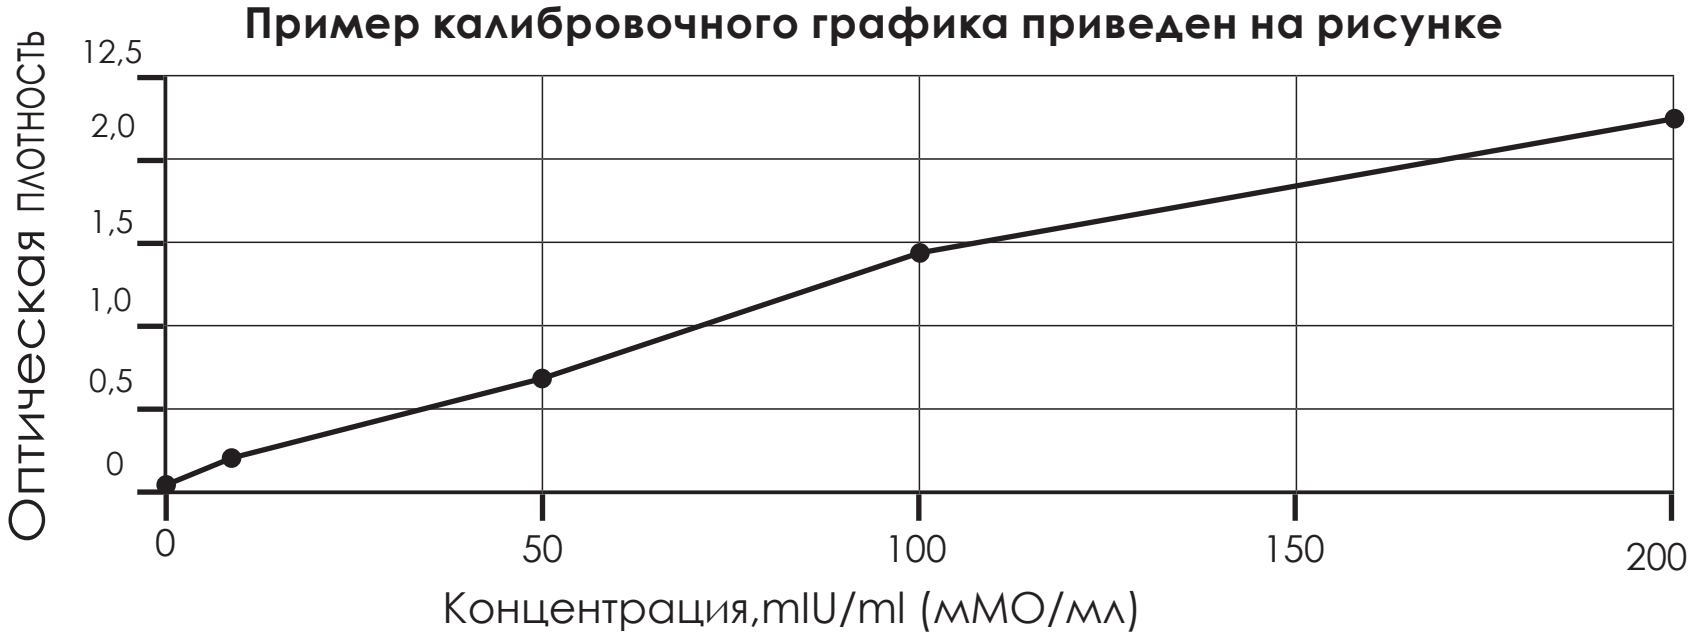

Примечание: Не используйте этот график для определения концентрации специфических антител в Вашем анализе. Для каждой постановки анализа необходимо строить отдельную калибровочную кривую!

Для удобства учета результатов реакции можно использовать компьютерные программы считывания и расчета результатов исследований.

10.3. Интерпретация результатов

Концентрация анти-HBs в образце	Интерпретация
> 12 mIU/ml (мМЕ/мл)	ПОЛОЖИТЕЛЬНЫЙ
10–12 mIU/ml (мМЕ/мл)	НЕОПРЕДЕЛЕННЫЙ
< 8 10 IU/ml (МЕ/мл)	ОТРИЦАТЕЛЬНЫЙ

Концентрация специфических антител к HBsAg выше 12 mIU/ml (мМЕ/мл) является показателем перенесенного гепатита B или проведенной вакцинации. Концентрация антител ниже 10 mIU/ml (мМЕ/мл) свидетельствует об отсутствии протективного иммунитета.

10.4. Метрологическая прослеживаемость калибраторов

Концентрация калибраторов «EQUI anti-HBs Calibrators» в ИФА-наборе «EQUI anti-HBs» отвечают Второму Международному Стандарту anti-hepatitis B surface antigen (anti-HBs) immunoglobulin, Human, 07/164 (NIBSC, WHO) в диапазоне 10-200

IU/ml (МЕ/мл) (slope = 0,9801; R2 = 0,9992). Это свидетельствует о метрологической прослеживаемости комплекта калибраторов «EQUI anti-HBs Calibrators» в ИФА-наборе «EQUI anti-HBs» к международно согласованному калибровочному материалу (Второго Международного Стандарта anti-HBs 07/164).

11. ХАРАКТЕРИСТИКИ ТЕСТА

11.1. Аналитические характеристики

Прецизионность

Воспроизводимость результатов в пределах одной постановки анализа (Intra assay repeatability)

Коэффициент вариации (CV) для двух сывороток с разным уровнем специфических антител оценивали в 32 повторах на одной серии ИФА-наборов «EQUI anti-HBs».

№ сыворотки	mIU/ml (мМЕ/мл)	CV, %
103/10	95,9	3,4
104/24	16,7	5,1

Воспроизводимость результатов между разными постановками анализа (Inter assay reproducibility)

Коэффициент вариации (CV) для двух сывороток с разным уровнем специфических антител оценивали на протяжении 3 дней в 3 постановках анализа, по 8 повторов в каждом анализе.

№ сыворотки	mIU/ml (мМЕ/мл)	CV, %
103/10	102,9	9,9
104/24	16,8	9,1

Аналитическая чувствительность

«Граница обнаружения» (LoD) – наименьшая концентрация анализируемого вещества в образце, выявляемом с заявленной вероятностью, для ИФА-набора «EQUI anti-HBs» с комплектом калибраторов «anti-HBs Calibrators» составляет 1 mIU/ml (мМЕ/мл).

«Предел количественного определения» (LoQ) – наименьшая концентрация аналита в образце, определяемая количественно с заявленной приемлемой точностью и правильностью, для ИФА-наборов «EQUI anti-HBs» с комплектом калибраторов «EQUI anti-HBs Calibrators» составляет 7 mIU/ml (мМЕ/мл).

«Предел отрицательного значения» (LoB) составляет 0,1 mIU/ml (мМЕ/мл).

Диапазон линейности

Диапазон линейности ИФА-наборов «EQUI anti-HBs» з комплектом калібраторів «anti-HBs Calibrators» знаходиться в межах 10–160 mIU/ml (мМЕ/мл).

12. ОГРАНИЧЕНИЕ АНАЛИЗА

Положительный результат в ИФА-наборе «EQUI anti-HBs» с комплектом калибраторов «EQUI anti-HBs Calibrators» является свидетельством наличия у пациента антител к поверхностному антигену вируса гепатита В. Антитела к HBsAg являются показателем протективного иммунитета.

Негативный результат в ИФА-наборе «EQUI anti-HBs» показывает, что тестируемый образец не содержит анти-HBs антител или их концентрация ниже уровня чувствительности анализа.

Выявление анти-HBs антител у пациента не является доказательством наличия вируса гепатита В в организме, эти антитела обнаруживаются при хроническом и перенесенном в анамнезе гепатите В, а также у вакцинированных против гепатита В лиц. Чтобы отличить эти состояния, рекомендуется протестировать пациента на другие маркеры гепатита В и исследовать образец на наличие HBsAg и специфических антител классов IgM и IgG к HBcore антигену (например, в ИФА-наборах «EQUI HBsAg», «EQUI HBcore IgM» и «EQUI HBcore IgG», соответственно).

13. Трудности, которые могут возникнуть при проведении ИФА

Высокий фон в лунках всего планшета может возникнуть из-за:

– загрязненный промыватель;
– низкое качество или загрязнение воды;
– использование плохо помытой посуды;
– использование дезинфицирующих средств, содержащих хлор;
– использование загрязненных наконечников;
– увеличение времени инкубации или изменение температурного режима.

Высокий фон в отдельных рядах может быть связан с:

– повторным внесением раствора ТМБ;
– загрязнением конуса автоматической пипетки раствором конъюгата;
– загрязнением одного из каналов промывателя.

Полученные значения ОП калибраторов (кроме Калибратора 0) ниже установленного предела, если:

– неправильно приготовленный или не внесенный один из реагентов (раствор конъюгата или раствор ТМБ);
– сокращено время инкубации на одном из этапов.

Интенсивность окраски лунок не соответствует полученной оптической плотности. Это может свидетельствовать о смещенном оптическом луче.

ЛИТЕРАТУРА

1. Mahoney F.J. Update on Diagnosis, Management, and Prevention of Hepatitis B Virus Infection // Clinical Microbiology Review – 1999. – Vol.12, N 2 - P.351–366.
2. Maddrey W.C. Hepatitis B - an important public health issue // Clin. Lab. - 2001. - Vol. 47, N 1-2. - P.51-55.
3. Spradling P.R., Xing J., Williams R. et al. Immunity to Hepatitis B Virus (HBV) Infection Two Decades after Implementation of Universal Infant HBV Vaccination: Association of Detectable Residual Antibodies and Response to a Single HBV Challenge Dose // Clinical and Vaccine Immunology. - 2013. - Vol.20, N 4. - P.559–561.
4. Walsh K., Alexander G.J.M. Update on chronic viral hepatitis // Postgraduate Medical Journal - 2001. - V. 77. - P. 498-505.
5. Возіанова Ж.І. Вірусний гепатит В // Інфекційні та паразитарні хвороби: В 3 т. – К.:»Здоров'я», 2001. т.1. – С.601-614.
6. European Centre for Disease Prevention and Control (ECDC). Systematic review on hepatitis B and C prevalence in the EU/EEA. Stockholm: 2016.
7. CDC Hepatitis B Information // https://www.cdc.gov/hepatitis/hbv/index.htm.
8. World Health Organization (WHO). WHO guidelines on hepatitis B and C testing. Geneva: World Health Organization; 2017 // http://www.who.int/hepatitis/publications/guidelines-hepatitis-c-b-testing/en/.
9. Regulation (EU) 2017/746 of the European Parliament and of the Council of 5 April 2017 on in vitro diagnostic medical devices and repealing Directive 98/79/EC and Commission Decision 2010/227/EU.
10. Закон України «Про відходи» // Відомості Верховної Ради України. - 1998. - №36-37.
11. Наказ МОЗ України №325 від 08.06.2015 «Про затвердження Державних санітарно-протиепідемічних правил і норм щодо поводження з медичними відходами».
12. Постанова КМУ від 02 жовтня 2013р. №754 «Про затвердження технічного регламенту щодо медичних виробів для діагностики in vitro».
13. ДСТУ EN ISO 17511:2015 - Медичні вироби для діагностики in vitro Вимірювання величин у біологічних пробах. Метрологічна простежуваність значень, приписаних калібраторам і контрольним матеріалам (EN ISO 17511:2003, IDT)
14. Hanna Tolonen, Kari Kuulasmaa, Tiina Laatikainen, Hermann Wolf and the European Health Risk Monitoring Project. Recommendation for indicators, international collaboration, protocol and manual of operations for chronic disease risk factor surveys Part 4.Storage and transfer of serum/plasma samples// Finnish National Public Health Institute 2002// https://thl.fi/publications/ehrm/product2/part_iii4.htm
15. Surveillance Guidelines for Measles, Rubella and Congenital Rubella Syndrome in the WHO European Region. Annex 3.Collection, storage and shipment of specimens for laboratory diagnosis and interpretation of results//Geneva: World Health Organization; 2012 Dec.

	Производитель
IVD	Медицинское изделие для диагностики *in vitro*
REF	Номер по каталогу
	Дата изготовления
	Использовать до
LOT	Код партии
	Температурное ограничение
Σ	Содержит достаточно для (n-) испытаний
!	Предостережение, ознакомиться с сопроводительными документами
i	Ознакомление с инструкцией по применению
	Беречь от прямых солнечных лучей
	Знак соответствия техническим регламентам

Редакция 7 от 30.12.2021г.

С вопросами и пожеланиями по работе набора обращайтесь к производителю:

ООО «Эквитестлаб»
ул. Большая Васильковская 114, г. Киев, Украина, 03150

проспект Победы 60/2, г. Киев, Украина, 03057 (адрес производства)

тел.: 0 (800)31-89-87, +38 (044)334-89-87,
e-mail: info@equitest.com.ua, www.equitest.com.ua

СХЕМА ПРОВЕДЕНИЯ АНАЛИЗА

Выдержать реагенты 30 min при температуре 18-25°С
Внести по 70 µl калибраторов и исследуемых образцов в лунки: A1 – CAL 0, B1 – CAL 10, C1 – CAL 50, D1 – CAL 100, E1 – CAL 200, в остальные лунки - исследуемые образцы
Внести по 35 µl приготовленного 1:11 (1+10) раствора коньюгата
Заклеить стрипы пленкой, инкубировать **120 min при температуре 37°С**
Промыть лунки 6 раз приготовленным 1:20 (1+19) раствором для промывания TWEEN (300 µl в лунку)
В лунки стрипов внести по 100 µl SOLN TMB
Инкубировать в течение **30 min в темноте при температуре 18-25°С**
В лунки стрипов внести по 100 µl SOLN STOP (происходит изменение цвета с голубого на желтый)
Измерить оптическую плотность (ОП) на спектрофотометре при 450/620-695 nm

УЧЕТ РЕЗУЛЬТАТОВ АНАЛИЗА

Построить калибровочную кривую, определить концентрацию mIU/ml (мМЕ/мл)

ИНТЕРПРЕТАЦИЯ РЕЗУЛЬТАТОВ

> 12 mIU/ml (мМЕ/мл)	ПОЛОЖИТЕЛЬНЫЙ
10–12 mIU/ml (мМЕ/мл)	НЕОПРЕДЕЛЕННЫЙ
< 10 IU/ml (МЕ/мл)	ОТРИЦАТЕЛЬНЫЙ

anti-Lamblia

ELISA kit for the qualitative detection of antibodies to *Giardia lamblia (intestinalis)*

Instructions for use

IVD

REF EI-606

96 tests

CE

EQUI anti-Lamblia

ELISA kit for the qualitative detection of antibodies to
до *Giardia lamblia (intestinalis)*

1. INTENDED USE

The «EQUI anti-Lamblia» is ELISA kit intended to qualitatively detect antibodies to *Giardia lamblia (intestinalis)* in human serum or plasma by enzyme-linked immunosorbent assay (ELISA) to diagnose giardiasis. The testing procedure is designed for both manual arrangement with automatic pipettes and standard equipment, and for automated «open» immunoassay analysers.

Target group: children, pet owners, citizens of rural areas, summer house owners.

Usage: ELISA kit is used in clinical diagnostic laboratories and other institutions engaged in *in vitro* diagnostics.

2. CLINICAL SIGNIFICANCE

Giardiasis is considered one of the most common parasitic diseases of the small intestine in the world. This infection is a major cause of acute and chronic diarrhea, especially in children. The etiological agent of giardiasis is *Giardia lamblia*, which is also called *Giardia intestinalis* or *Giardia duodenalis*.

Giardia lamblia are unicellular flagellate protozoa that parasitize in the intestines of humans and some other mammals. During the life cycle of these parasites, two stages alternate: cysts, resistant to external conditions, and a vegetative form - trophozoites. Infection occurs when cysts enter the human gastrointestinal tract. After experiencing the effects of gastric acid, cysts in the duodenum turn into trophozoites, which parasitize in the upper parts of the small intestine. They absorb nutrients from the intestinal lumen, block parietal digestion and disrupt the motility of the intestine.

Humans get infected via fecal-oral routes through cyst-contaminated food, water, unwashed hands, and so on. Giardia can also be transmitted to humans from infected cats, dogs, and livestock. Giardiasis is especially common in regions with poor sanitation. In addition, human-to-human transmission is common in preschools.

In many cases, the invasion of Giardia occurs without clinical manifestations. In other cases, the first symptoms of giardiasis appear in 1-3 weeks after infection. They are most often manifested by spasms, bloating, nausea and diarrhea, which leads to dehydration and weight loss. The acute form of the disease can last up to two weeks and end in recovery without additional treatment or become chronic. Chronic giardiasis develops when the duration of the invasion is longer than 2 month and the exacerbation of clinical manifestations (diarrhea) is cyclical. *Giardia lamblia* parasitism can lead to malabsorption syndrome, which disrupts the absorption of carbohydrates and fats, as well as the metabolism of vitamins B12, A and C.

Immune response to invasion and non-immune factors are important to control the development of the disease and the severity of clinical manifestations. Both humoral and cellular immunity play the part in the eradication of the pathogen, the role of which is still subjected to scientific research. In addition, partial resistance to re-infection is formed due to protective mechanisms of the body.

Typically, to diagnose giardiasis, the duodenal contents and feces are examined for trophozoites and cysts of giardiasis. In case of the chronic course of the disease, cysts get excreted periodically, and, considering this, the additional tests should be performed regularly for several weeks. Another method of diagnosing giardiasis is to detect *Giardia lamblia* antigens in the feces. However, serodiagnosis with the detection of specific antibodies to Giardia antigens is an important step in assessing the immune response of patients. Detection of specific IgM antibodies suggests an acute stage of giardiasis. However, the detection of specific IgG and IgA antibodies should be interpreted with caution: in some regions they persist for a long time after infection, while in others their level decreases after eradication of the pathogen.

3. ANALYSIS PRINCIPLE

The procedure of testing for *Giardia lamblia* specific antibodies in «EQUI anti-Lamblia» ELISA kit is based on «indirect» solid-phase ELISA with a two-stage incubation. Recombinant *Giardia lamblia* antigens are entrapped in the wells. During the first step of incubation of the test samples in the wells of the ELISA plate, *Giardia lamblia*-specific antibodies, if present in the samples, bind to the solid phase antigens. The wells are washed to remove unbound antibodies and have only specific antigen-antibody complexes left. Then, a conjugate of anti-species (anti-IgG and anti-IgA) monoclonal antibodies with horseradish peroxidase is added, which binds to solid-phase immune complexes. Unbound components are removed by washing. Antigen-antibody complexes are detected by adding a solution of chromogen 3,3',5,5'-tetramethylbenzidine (TMB) with hydrogen peroxide. After 30-minute incubation, the reaction is stopped by adding the stop solution. The optical density (OD) in the wells is determined using a spectrophotometer at 450/620-695 nm. The intensity of the yellow colour is proportional to the level of antibodies in the sample.

4. MATERIALS AND EQUIPMENT

4.1. Contents of the ELISA kit

STRIPS	1 x 96 wells	**Microplate** Each plate well is coated with *Giardia lamblia* purified antigens. The wells are detachable. After the first opening, store unused strips in the package at 2-8 °C for a maximum of 6 months
CONTROL +	1 x 0,35 ml	**Positive control** Conjugated specific monoclonal antibody solution with preservative (pink). Store at 2-8 °C
CONTROL -	1 x 1,2 ml	**Negative control** Negative human serum with a preservative (yellow). Store at 2-8 °C

DIL SAMPLE	1 x 11 ml	**Serum dilution solution** Buffer solution with a milk extract, a detergent and a preservative (purple). Store at 2-8 °C
SOLN CONJ	1 x 13 ml	**Conjugate solution (ready to use)** Buffer solution of monoclonal antibodies to human IgG and IgA, conjugated with horseradish peroxidase, with stabilizers and preservative (green). Store at 2-8 °C
SOLN TMB	1 x 13 ml	**TMB solution (ready to use)** TMB solution, H_2O_2, a stabilizer, a preservative (colourless). Store at 2-8 °C
TWEEN WASH 20x	1 x 50 ml	**Washing solution TWEEN (20x concentrated)** 20-fold phosphate buffer concentrate with Tween-20 (colourless). Dilute TWEEN detergent (20x) at 1:20 with distilled or deionized water (e. g., 5 mL of concentrate + 95 mL of water for 8 wells) before use. Store the diluted solution at 2-8 °C for a maximum of 7 days
SOLN STOP	1 x 13 ml	**Stop Solution (ready to use)** 0.5 mol H_2SO_4 solution (colourless). Store at 2-8 °C

The ELISA kit also includes adhesive films (2 items), sample application plan (1 item), checklist, and instruction for use.

4.2. Optional reagents, materials and equipment

Automatic single and multichannel pipettes 10–1000 µL, tips, volumetric laboratory glassware (10–1,000 mL), deionized or distilled water, thermostat at 37 °C, automatic or semi-automatic plate washer, spectrophotometer (reader) for microplates at 450/620-695 nm, appropriate containers for potentially contaminated waste, timer, filter paper, disposable powder-free gloves, disinfectants.

5. PRECAUTIONS AND SAFETY

5.1. Precautions

Be sure to read the instructions for use carefully before the test. The validity of the test results depends on strict following of the test procedure.

– do not use the ELISA kit components after the expiry date;
– do not use for analysis or mix components of different batches, components of kits for different nosologies, or reagents from other manufacturers with the «EQUI anti-Lamblia» ELISA kit;
– do not freeze the ELISA kit or its contents;
– after using a reagent, close each vial with its cap;
– when washing, control filling and complete aspiration of solution from the wells;
– use a new pipette tip each time you add samples or reagents;
– prevent direct sunlight from reaching the reagents from the ELISA kit;
– SOLN TMB solution must be colourless before use. Do not use the solution if its colour is blue or yellow. Avoid contact of SOLN TMB with metals or metal ions. Use only clean glassware thoroughly rinsed with distilled water;

– do not use reagents with colour not in line with para. 4.1;
– under no circumstances should the same glassware be used for SOLN CONJ and SOLN TMB;
– do not evaluate the test results visually (without a reader);
– any optional equipment that is in direct contact with biological material or kit components should be considered contaminated and requires cleaning and decontamination;
– the ELISA kit includes materials for 96 tests. Dispose of the used components as well as any remaining unused components.

5.2. Safety requirements

– all reagents in the ELISA kit are for laboratory professional use for *in vitro* diagnosis only and may only be used by qualified personnel;
– conduct the tests in disposable powder-free gloves and goggles only;
– do not eat, drink, smoke, or apply make-up in the test room;
– do not mouth-pipette the solutions;
– controls from the «EQUI anti-Lamblia» ELISA kit have been tested and found to be for anti-HIV1/2, anti-HCV and anti-*Treponema pallidum* antibodies and HBsAg negative; however, controls and test samples should be handled as potentially hazardous infectious materials;
– some of the kit components contain low concentrations of harmful substances and can damage skin or mucoga. In case of contact of SOLN TMB, SOLN STOP and SOLN CONJ with mucous membranes or skin, immediately wash the affected area with plenty of water;
– in case of spillage of acid-free solutions, e. g. sera, treat the surface with a disinfectant solution and then wipe dry with filter paper. Otherwise first neutralize acid with sodium bicarbonate solution and then wipe the surface dry as described above.

5.3. Waste inactivation and disposal

– the liquid waste must be inactivated, for example, with hydrogen peroxide solution at the final concentration of 6% for 3 hours at room temperature, or with sodium hypochlorite at the final concentration of 5% for 30 minutes, or with other approved disinfectants;
– the solid waste must be inactivated by autoclaving at a temperature not less than 132°C;
– do not autoclave the solutions that contain sodium azide or sodium hypochlorite;
– disposal of inactivated waste must be conducted due to national laws and regulations.

6. STORAGE AND STABILITY

ELISA kit is stable up to the expiry date stated on the label when stored at 2-8°C. The kit should be transported at 2-8°C. Single transportation at a temperature up to 23°C for two days is possible.

7. SAMPLE COLLECTION, TRANSPORTATION AND STORAGE GUIDELINES

Collect blood from the vein into the sterile test tube. Test tube must be marked with patient ID and date of sample collecting. Blood before serum separation can be stored at 2-8 ºC for 24 hours, avoiding freezing.

Serum or plasma can be stored at 2-8 °C for maximum 3 days. Frozen serum can be stored for longer periods of time at -20 °C or -70 °C. Thaw frozen samples and keep them at room temperature for 30 minutes before use. After thawing, the stir samples to achieve homogeneity. Avoid repeated freezing-thawing cycles for test samples. If serum (or plasma) is turbid, remove insoluble inclusions by centrifugation at 3000 rpm for 10-15 minutes. Do not use serum samples with hyperlipidemia, hemolysis, and bacterial growth.

Transport serum samples in insulated containers. To do that, put closed labelled tubes in a plastic bag, tightly seal it and place in the centre of an insulated container.Put the frozen cold packs on the bottom, along the side walls of the insulated container and on top of the serum samples.

8. REAGENT PREPARATION

NOTE! It is very important to keep all ELISA kit components for at least 30 min at room temperature 18-25 ºC before the assay!

8.1. Microplate preparation

To prevent water condensation in the wells, keep the STRIPS for 30 minutes at a room temperature before opening. Open the vacuum pack, detach the appropriate number of wells, and carefully pack the remaining wells with a desiccant and store tightly zip-locked at 2-8 °C. Storing the packed plate this way ensures its stability for 6 months.

8.2. Washing solution preparation

To prepare detergent, dilute TWEEN WASH 20x at 1:20 (1+19) with distilled or deionized water and stir. E. g., 5 mL of concentrate + 95 mL of water, which is enough for 8 wells. If there are crystals present in the detergent concentrate, heat the vial at 37 °C until the crystals dissolve completely (15–20 minutes). Store the diluted solution at 2-8 °C for a maximum of 7 days.

9. ASSAY PROCEDURE

9.1. Prepare the necessary number of wells (four wells for controls and a necessary number of wells for test samples) and insert them into the ELISA plate frame. Be sure to add control wells in every test run.

9.2. Fill in the sample application plan.

9.3. Prepare the detergent as per para. 8.2.

9.4. Add 80 µL of DIL SAMPLE into each plate well.

9.5. Add 20 µL of controls and test samples into the wells:

CONTROL + – into well A1,

CONTROL - – into wells B1, C1 and D1,

and test samples into the remaining wells.

At the time of adding, the solution changes its colour from brown to blue. Pipette the mix in the wells carefully to avoid foaming.

9.6. Cover the strips up with adhesive film and incubate for **30 minutes at 37 °C**.

9.7. Remove and discard the adhesive film and wash all wells 5 times with automatic washer or 8-channel pipette as follows:
– aspirate the content of all wells into a liquid waste container;
– add a minimum of 300 μl of diluted washing solution to each well, soak each well for 30 seconds;
– aspirate the content of all wells again. The residual volume after every aspiration should be less than 5 μl;
– repeat the washing step 4 more times;
– after the final aspiration, eliminate extra moisture by tapping the plate against a piece of filter paper.

9.8. Add 100 μL of SOLN CONJ into each well. Cover the strips with a new piece of adhesive film and incubate for **30 minutes at 37 °C**.

9.9. Following incubation, remove the film carefully and wash the wells five times as described in para. 9.7.

9.10. Add 100 μL of SOLN TMB into the wells; do not touch the bottom and the walls of the plate wells.

9.11. Incubate the strips for **30 minutes** in a dark place at a room temperature of 18-25 °C. Do not use adhesive film at this stage.

9.12. Add 100 μL of SOLN STOP into each strip well to stop the enzymatic reaction; adhere to the same sequence of actions as when adding SOLN TMB. At the time of adding, the solution colour changes from blue to yellow, and clear solution slightly changes its shade.

9.13. Measure the optical density (OD) of the wells at 450/620-695 nm wavelength using an ELISA microplate reader within 5 minutes after stopping the reaction. Pay attention to the cleanness of the plate bottom and the absence of bubbles in the wells before reading.

Measurement at the single wavelength of 450 nm is possible, in that case, it is needed to leave one well for blank (only SOLN TMB and SOLN STOP must be added in blank well).

10. CALCULATION AND INTERPRETATION OF RESULTS

10.1. Calculation of results

Calculate the average OD for the negative control ($\overline{Nc}$), Cut off (CO) and a sample positivity index (IP_{sample}).

$$\overline{Nc} = (Nc1 + Nc2 + Nc3)/3; \quad CO = \overline{Nc} + 0{,}25$$

$$IP_{sample} = OD_{sample}/CO, \text{ where } OD_{sample} \text{ is the OD sample.}$$

10.2. Quality control (assay validation)

The test results are considered valid if they meet the following requirements:

CONTROL +	OD ≥ 1,0	
CONTROL -	OD ≤ 0,150	
CONTROL -	$\overline{Nc} \times 0,5 \leq Ncn \leq \overline{Nc} \times 2,0$	where Ncn is the OD for each Nc run

If any of the OD values for the negative control is beyond the above interval, it should be discarded, and $\overline{Nc}$ is calculated based on the remaining OD values for the negative control. If several OD values for the negative control fail to meet the above requirements, the test is considered invalid and requires a new run.

10.3. Interpretation of results

$IP_{sample} > 1,1$	POSITIVE
$0,9 \leq IP_{sample} \leq 1,1$	BORDERLINE*
$IP_{sample} < 0,9$	NEGATIVE

* Uncertain samples are recommended to be re-examined in two wells of the ELISA kit. If the results are again uncertain, a new sample should be selected and analyzed in 2-4 weeks. In case of repeated indeterminate results, such samples shall be considered negative.

11. PERFORMANCE CHARACTERISTICS

11.1. Analytical performance characteristic

Precision of measurement

Intra assay repeatability

The coefficient of variation (CV) for two sera with different levels of specific antibodies was evaluated in 32 replicates on one series of ELISA kits.

Sample No.	OD_{av}	IP_{av}	CV, %
14L	0,679	2,47	6,5
16L	0,490	1,79	6,6

Inter assay reproducibility

The coefficient of variation (CV) for three sera with different levels of specific antibodies was evaluated for 3 days in 3 sets of analysis, 8 replicates in each analysis.

Sample No.	OD_{av}	IP_{av}	CV, %
14L	0,670	2,39	5,55
16L	0,463	1,65	7,06

Analytical specificity

The test results are not affected by bilirubin at up to 0.21 mg/mL (361.8 µmol/L), haemoglobin at up to 10 mg/mL and triglycerides at up to 10 mg/mL (11.3 mmol/l) present in the sample.

11.2. Diagnostic characteristics

Studies of the characteristics of the method in comparison with a similar commercial ELISA kit were performed on a sample of characterized sera, the target group of children and a group of donors. The relative sensitivity of «EQUI anti-Lamblia» ELISA kits was determined from a group of 23 serum samples that were tested for antibodies to *Giardia lamblia* and characterized as positive in a commercial ELISA kit. All sera were also determined to be positive in «EQUI anti-Lamblia» kits, so the relative sensitivity equals 100%. For 148 serum samples of children that were tested and characterized in commercial analogues, the relative specificity of «EQUI anti-Lamblia» ELISA kits was 92.86%, the percentage of coincidence - 93.24%. According to a similar principle, for 238 serum samples of donor blood, the relative specificity was 97% and the percentage of coincidence was 96.64%.

12. LIMITATIONS OF ASSAY

The final diagnosis cannot be made solely on the basis of serological test results, sunce clinical manifestations of the disease and laboratory data (such as the detection of cysts in faecal samples or trophozoites in duodenal contents; the results of detection of *Giardia lamblia* antigen in faeces) should be taken into account as well.

Addionally, cross-reactions with antibodies to antigens of other parasites cannot be completely ruled out.

Giardia lamblia-specific antibodies may not be detected in case of children with persistent and prolonged giardiasis.

It should be noted that IgG antibodies to *Giardia lamblia* can be detected via ELISA for a long time, even after successful treatment.

13. DIFFICULTIES THAT CAN OCCUR DURING THE ASSAY PROCEDURE

Possible reasons	Solution
High background in all wells	
Contaminated washer	Clean the washer head and rinse according to the instructions for use
Poor quality or contaminated water	Use purified water with specific resistance ≥ 10 MΩ · cm
Use of poorly washed glassware	Use chemically clean utensils
Use of chlorinated disinfectants	Do not use chlorine disinfectants
Use of contaminated tips	Use new tips
Increased incubation times or change in the temperature conditions	Adhere to the incubation regime according to the instructions for use
High background in a row of wells	

Repeat application of TMB solution	TMB solution should be applied once
Contamination of the automatic pipette nozzle with conjugate solution	Clean the pipette and dial carefully liquid
Contamination of one of the washer's channel	Clean the flush channel, rinse washer
Received OD of the positive control is below the border value	
One of the reagents (conjugate solution or TMB solution) was not prepared in a correct way or was not added	Re-conduct ELISA, pay attention to the correctness of the introduction of these reagents
Reduced incubation times at any stage	Incubate according to instructions for use
The colour density of the wells fails to meet the obtained optical density value	
This may suggest that the optical beam has been displaced	Check the correct operation of the reader

14. TECHNICAL ASSISTANCE AND CUSTOMER SERVICE

In case of technical problems, you can obtain assistance by contacting the manufacturer.

REFERENCES

1. Adam R. D. Biology of Giardia lamblia // Clinical Microbiology Reviews. - 2001. - Vol. 14(3). - P. 447–475.
2. CDC - Giardia // https://www.cdc.gov/parasites/giardia/index.html.
3. Choy S. H., Al-Mekhlafi H. M. et al. Prevalence and Associated Risk Factors of Giardia Infection among Indigenous Communities in Rural Malaysia // Scientific Reports. - 2014. - Vol. 4, Article number: 6909.
4. DuPont H. L. Giardia: both a harmless commensal and a devastating pathogen // Journal of Clinical Investigation. - 2013. - Vol. 123(6). - P. 2352–2354.
5. Faubert G. Immune Response to Giardia duodenalis // Clinical Microbiology Reviews. - 2000. - Vol. 13(1). - P. 35–54.
6. Lopez-Romero G., Quintero J. et al. Host defences against Giardia lamblia // Parasite Immunology. - 2015. -Vol. 37(8). - P. 394-406.
7. Saghaug C. S., Sørnes S. et al. Human Memory CD4+ T Cell Immune Responses against Giardia lamblia // Clinical and Vaccine Immunology. - 2016. - Vol. 23, No. 1. - P. 11-18.
8. Solaymani-Mohammadi S. and Singer S. M. Giardia duodenalis: The Double-edged Sword of Immune Responses in Giardiasis // Experimental Parasitology. - 2010. - Vol. 126 (3). - P. 292–297.
9. Regulation (EU) 2017/746 of the European Parliament and of the Council of 5 April 2017 on in vitro diagnostic medical devices and repealing Directive 98/79/EC and Commission Decision 2010/227/EU.
10. Закон України «Про відходи» // Відомості Верховної Ради України. - 1998. - №36-37.
11. Наказ МОЗ України №325 від 08.06.2015 «Про затвердження Державних санітарно-протиепідемічних правил і норм щодо поводження з медичними відходами».
12. Постанова КМУ від 02 жовтня 2013р. №754 «Про затвердження технічного регламенту щодо медичних виробів для діагностики in vitro».
13. Hanna Tolonen, Kari Kuulasmaa, Tiina Laatikainen, Hermann Wolf and the European Health Risk Monitoring Project. Recommendation for indicators, international collaboration, protocol and manual of operations for chronic disease risk factor surveys Part 4.Storage and transfer of serum/plasma samples// Finnish National Public Health Institute 2002// https://thl.fi/publications/ehrm/product2/part_iii4.htm
14. Surveillance Guidelines for Measles, Rubella and Congenital Rubella Syndrome in the WHO European Region. Annex 3.Collection, storage and shipment of specimens for laboratory diagnosis and interpretation of results// Geneva: World Health Organization; 2012 Dec.

Manufacturer

EC REP Authorized Representative in the European Community

IVD In vitro diagnostic medical device

REF Catalogue number

Date of manufacture

Use by date

LOT Batch code

Temperature limit

Contains sufficient for <n> tests

Caution

NON STERILE Non-Sterile

Consult instructions for use

Keep away from sunlight

Keep dry

CE Compliance with EU safety requirements

Edition 7, 18.02.2022

For questions and suggestions regarding the ELISA kit contact:

EC REP

Obelis s.a.
Bd Général Wahis 53
1030 Brussels
Belgium
Tel: +(32)2 732-59-54
Fax: +(32)2 732-60-03
mail@obelis.net

Ekvitestlab LLC
Velyka Vasylkivska St. 114, Kyiv, Ukraine, 03150
Tel: 0(800)31-89-87, +38 (044)334-89-87,
e-mail: info@equitest.com.ua, www.equitest.com.ua

ASSAY PROCEDURE SCHEME

Keep all reagents for 30 min at temperature18-25°C before use
Dispense 80 µl DIL SAMPLE into the wells (purple)
Add to 20 µl of controls and samples into the wells: A1 – CONTROL + , B1, C1, D1 – CONTROL – , other wells – examined samples (change of colour from purple to blue)
Cover strips with an adhesive film, incubate for **30 min at 37°C**
Rinse the wells 5 times with prepared 1:20 (1+19) washing solution TWEEN (300 µl per well)
Add 100 µl of SOLN CONJ into all wells (green)
Cover strips with an adhesive film, incubate for **30 min at 37°C**
Rinse the wells 5 times with prepared 1:20 (1+19) washing solution TWEEN (300 µl per well)
Add 100 µl of SOLN TMB into all wells
Incubate for **30 min** in the dark at **18-25°C**
Add 100 µl of SOLN STOP into all wells (change of colour from blue to yellow)
Measure the optical density (OD) with an ELISA microplate reader at 450/620-695 nm

CALCULATION OF RESULTS

$\overline{Nc}$ = (Nc1 + Nc2 + Nc3)/3;

CO = $\overline{Nc}$ + 0,25;

$IP_{sample} = OD_{sample}/CO$

$\overline{Nc}$ - the average value of OD 3-x CONTROL –

CO - Cut off

IP_{sample} - sample positivity index

INTERPRETATION OF RESULTS

$IP_{sample} > 1,1$	POSITIVE
$0,9 \le IP_{sample} \le 1,1$	BORDERLINE
$IP_{sample} < 0,9$	NEGATIVE

Ascaris lumbricoides IgG

ELISA kit for the qualitative detection of IgG antibodies to *Ascaris lumbricoides*

Instructions for use

IVD

REF EI-601

Σ 96 tests

CE

EQUI Ascaris lumbricoides IgG

ELISA kit for the qualitative detection of
IgG antibodies to *Ascaris lumbricoides*

1. INTENDED USE

The «EQUI Ascaris lumbricoides IgG» is ELISA kit intended to qualitatively detect anti-*Ascaris lumbricoides* IgG in human serum or plasma by enzyme-linked immunosorbent assay (ELISA) in order to diagnose lumbricosis. The testing procedure is designed for both manual arrangement with automatic pipettes and standard equipment, and for automated «open» immunoassay analysers.

Target group: children, rural people, summer visitors.

Usage: ELISA kit is used in clinical diagnostic laboratories and other institutions engaged in *in vitro* diagnostics.

2. CLINICAL SIGNIFICANCE

Ascaris lumbricoides is a human parasite resulting in lumbricosis — one of the most common helminthiases in the world. By some estimates, over a milliard of people infested with acaricides are on earth.

Human ascaris belongs to *Nematoda* roundworms infesting the small intestine of a man who is its exclusive host. *Ascaris lumbricoides* eggs are excreted in the environment with faeces of the infested man. In a warm, wet soil, ascaris larvae develops in the eggs, therefore eggs become invasive only after a maturation period (2 to 3 weeks at 25–30 °C, lower temperatures require longer term). After infestation, larvae leave eggs in the human intestine, penetrates blood circulation and migrate to the liver and lungs with blood flow. The larvae move to the pharynx from the lungs, and here they are re-ingested and further enter the small intestine. In 2 to 3 months, adult ascaris able to propagate develops from larvae in the small intestine.

The helminths are transferred by faecal-oral route upon injection of mature eggs of *Ascaris lumbricoides* with soil-contaminated vegetables, fruits, water, as well as through dirty hands after contact with soil. Lumbricosis is conditionally divided into the early stage (migration of larvae) and late stage (parasitism of adults in the intestine). Invasion is asymptomatic in most cases. Primary feeling of being unwell occurs as early as several days after infestation and is accompanied by weakness, abdominal pain, nausea. Migration of larvae to the lungs may manifest as rales and cough. In some cases, intense invasion may result in pneumonia and liver damage. However, the most common symptom of early lumbricosis are allergic reactions due to hypersensitivity to metabolic products of larvae.

Late stage manifests as decreases appetite, abdominal pain, vomiting, diarrhoea, constipation. Massive ascaris invasion may result in the intestinal obstruction with a lump of helminths or rupture of the walls with peritonitis. When ascarides penetrate other organs, complications may develop such as hepatitis, cholangitis, pancreatitis and even asphyxia. Cases of neurological disorders sometimes develop in lumbricosis, namely: headache, irritability, sleep impairment, inattention, etc. If no timely treatment is started for intense invasion, it may lead to death, especially in younger children.

Strong immune response to *Ascaris lumbricoides* invasion develops as early as at the early stage. It includes cellular and humoral immunity. Antigens of ascaris larvae stimulate secretion of all-class specific immunoglobulins, however, the level of specific and total IgE antibodies is the highest. The intensity of the immune response (including increased IgG titres) correlates with the massiveness of the invasion.

For diagnosis of lumbricosis, parasitologic stool test for presence of ascaris larvae and eggs is the most common. X-ray imaging of the lungs is additionally applied at the early stage of invasion. Complete blood count (eosinophilia develops in lumbricosis) and detection of serum anti-*Ascaris lumbricoides* antibodies also is included in the set of exams. The presence of specific anti-ascaris antibodies may suggest asymptomatic invasion, and allows initiation of treatment before complications develop in conjunction with other diagnostic instruments.

3. ANALYSIS PRINCIPLE

The procedure of testing for anti-*Ascaris lumbricoides* IgG in «EQUI Ascaris lumbricoides IgG» ELISA kit is based on «indirect» solid-phase ELISA with a two-stage incubation. Antigens of *Ascaris lumbricoides* larvae are entrapped in the wells. During the first step of incubation of ELISA plate wells with test samples, specific anti-*Ascaris lumbricoides* antibodies (if present in the samples) bind to the solid-phase antigens. The wells are washed to remove unbound antibodies and have only specific antigen-antibody complexes left. Then, a conjugate of anti-species IgG monoclonal antibodies with horseradish peroxidase is added, which binds to solid-phase immune complexes. Unbound components are removed by washing. Antigen-antibody complexes are detected by adding a solution of chromogen 3,3’,5,5’-tetramethylbenzidine (TMB) with hydrogen peroxide. After 30-minute incubation, the reaction is stopped by adding the stop solution. The optical density (OD) in the wells is determined using a spectrophotometer at 450/620-695 nm. The intensity of the yellow colour is proportional to the level of antibodies in the sample.

4. MATERIALS AND EQUIPMENT

4.1. Contents of the ELISA kit

STRIPS	1 x 96 wells	**Microplate** Each plate well is coated with *Ascaris lumbricoides* antigen. The wells are detachable. After the first opening, store unused strips in the package at 2-8 °C for a maximum of 6 months

CONTROL +	1 x 0,25 ml	**Positive control** Conjugated specific monoclonal antibody solution with preservative (pink). Store at 2-8 °C
CONTROL -	1 x 0,6 ml	**Negative control** Negative human serum with a preservative (yellow). Store at 2-8 °C
DIL SAMPLE	1 x 13 ml	**Serum dilution solution** Buffer solution with a milk extract, a detergent and a preservative (brown). Store at 2-8 °C
SOLN CONJ	1 x 13 ml	**Conjugate solution (ready to use)** Buffer solution of monoclonal antibodies to human IgG, conjugated with horseradish peroxidase, with stabilizers and preservative (green). Store at 2-8 °C
SOLN TMB	1 x 13 ml	**TMB solution (ready to use)** TMB solution, H_2O_2, a stabilizer, a preservative (colourless). Store at 2-8 °C
TWEEN WASH 20x	1 x 50 ml	**Washing solution TWEEN (20x concentrated)** 20-fold phosphate buffer concentrate with Tween-20 (colourless). Dilute TWEEN detergent (20x) at 1:20 with distilled or deionized water (e. g., 5 mL of concentrate + 95 mL of water for 8 wells) before use. Store the diluted solution at 2-8 °C for a maximum of 7 days
SOLN STOP	1 x 13 ml	**Stop Solution (ready to use)** 0.5 mol H_2SO_4 solution (colourless). Store at 2-8 °C

The ELISA kit also includes adhesive films (2 items), sample application plan (1 item), checklist, and instruction for use.

4.2. Optional reagents, materials and equipment

Automatic single and multichannel pipettes 10–1000 µL, tips, volumetric laboratory glassware (10–1,000 mL), deionized or distilled water, thermostat at 37 °C, automatic or semi-automatic plate washer, spectrophotometer (reader) for microplates at 450/620-695 nm, appropriate containers for potentially contaminated waste, timer, filter paper, disposable powder-free gloves, disinfectants.

5. PRECAUTIONS AND SAFETY

5.1. Precautions

Be sure to read the instructions for use carefully before the test. The validity of the test results depends on strict following of the test procedure.

– do not use the ELISA kit components after the expiry date;
– do not use for analysis or mix components of different batches, components of kits for different nosologies, or reagents from other manufacturers with the «EQUI Ascaris lumbricoides IgG» ELISA kit;
– do not freeze the ELISA kit or its contents;
– after using a reagent, close each vial with its cap;

– when washing, control filling and complete aspiration of solution from the wells;
– use a new pipette tip each time you add samples or reagents;
– prevent direct sunlight from reaching the reagents from the ELISA kit;
– SOLN TMB solution must be colourless before use. Do not use the solution if its colour is blue or yellow. Avoid contact of SOLN TMB with metals or metal ions. Use only clean glassware thoroughly rinsed with distilled water;
– do not use reagents with colour not in line with para. 4.1;
– under no circumstances should the same glassware be used for SOLN CONJ and SOLN TMB;
– do not evaluate the test results visually (without a reader);
– any optional equipment that is in direct contact with biological material or kit components should be considered contaminated and requires cleaning and decontamination;
– the ELISA kit includes materials for 96 tests. Dispose of the used components as well as any remaining unused components.

5.2. Safety requirements

– all reagents in the ELISA kit are for laboratory professional use for *in vitro* diagnosis only and may only be used by qualified personnel;

– conduct the tests in disposable powder-free gloves and goggles only;

– do not eat, drink, smoke, or apply make-up in the test room;

– do not mouth-pipette the solutions;

– controls from the «EQUI Ascaris lumbricoides IgG» ELISA kit have been tested and found to be for anti-HIV1/2, anti-HCV and anti-*Treponema pallidum* antibodies and HBsAg negative; however, controls and test samples should be handled as potentially hazardous infectious materials;

– some of the kit components contain low concentrations of harmful substances and can damage skin or mucoga. In case of contact of SOLN TMB, SOLN STOP and SOLN CONJ with mucous membranes or skin, immediately wash the affected area with plenty of water;

– in case of spillage of acid-free solutions, e. g. sera, treat the surface with a disinfectant solution and then wipe dry with filter paper. Otherwise first neutralize acid with sodium bicarbonate solution and then wipe the surface dry as described above.

5.3. Waste inactivation and disposal

– the liquid waste must be inactivated, for example, with hydrogen peroxide solution at the final concentration of 6% for 3 hours at room temperature, or with sodium hypochlorite at the final concentration of 5% for 30 minutes, or with other approved disinfectants;

– the solid waste must be inactivated by autoclaving at a temperature not less than 132°C;

– do not autoclave the solutions that contain sodium azide or sodium hypochlorite;
– disposal of inactivated waste must be conducted due to national laws and regulations.

6. STORAGE AND STABILITY

ELISA kit is stable up to the expiry date stated on the label when stored at 2-8°C. The kit should be transported at 2-8°C. Single transportation at a temperature up to 23°C for two days is possible.

7. SAMPLE COLLECTION, TRANSPORTATION AND STORAGE GUIDELINES

Collect blood from the vein into the sterile test tube. Test tube must be marked with patient ID and date of sample collecting. Blood before serum separation can be stored at 2-8 ºC for 24 hours, avoiding freezing.

Serum or plasma can be stored at 2-8 °C for maximum 3 days. Frozen serum can be stored for longer periods of time at -20 °C or -70 °C. Thaw frozen samples and keep them at room temperature for 30 minutes before use. After thawing, the stir samples to achieve homogeneity. Avoid repeated freezing-thawing cycles for test samples. If serum (or plasma) is turbid, remove insoluble inclusions by centrifugation at 3000 rpm for 10-15 minutes. Do not use serum samples with hyperlipidemia, hemolysis, and bacterial growth.

Transport serum samples in insulated containers. To do that, put closed labelled tubes in a plastic bag, tightly seal it and place in the centre of an insulated container.Put the frozen cold packs on the bottom, along the side walls of the insulated container and on top of the serum samples.

8. REAGENT PREPARATION

NOTE! It is very important to keep all ELISA kit components for at least 30 min at room temperature 18-25 ºC before the assay!

8.1. Microplate preparation

To prevent water condensation in the wells, keep the STRIPS for 30 minutes at a room temperature before opening. Open the vacuum pack, detach the appropriate number of wells, and carefully pack the remaining wells with a desiccant and store tightly zip-locked at 2-8 °C. Storing the packed plate this way ensures its stability for 6 months.

8.2. Washing solution preparation

To prepare detergent, dilute TWEEN WASH 20x at 1:20 (1+19) with distilled or deionized water and stir. E. g., 5 mL of concentrate + 95 mL of water, which is enough for 8 wells. If there are crystals present in the detergent concentrate, heat the vial at 37 °C until the crystals dissolve completely (15–20 minutes). Store the diluted solution at 2-8 °C for a maximum of 7 days.

9. ASSAY PROCEDURE

9.1. Prepare the necessary number of wells (four wells for controls and a necessary number of wells for test samples) and insert them into the ELISA plate frame. Be sure to add control wells in every test run.

9.2. Fill in the sample application plan.

9.3. Prepare the detergent as per para. 8.2.

9.4. Add 90 µL of DIL SAMPLE into each plate well.

9.5. Add 10 µL of controls and test samples into the wells:
CONTROL + – into well A1,
CONTROL - – into wells B1, C1 and D1,
and test samples into the remaining wells.
At the time of adding, the solution changes its colour from brown to blue. Pipette the mix in the wells carefully to avoid foaming.

9.6. Cover the strips up with adhesive film and incubate for **30 minutes at 37 °C**.

9.7. Remove and discard the adhesive film and wash all wells 5 times with automatic washer or 8-channel pipette as follows:
– aspirate the content of all wells into a liquid waste container;
– add a minimum of 300 µl of diluted washing solution to each well, soak each well for 30 seconds;
– aspirate the content of all wells again. The residual volume after every aspiration should be less than 5 µl;
– repeat the washing step 4 more times;
– after the final aspiration, eliminate extra moisture by tapping the plate against a piece of filter paper.

9.8. Add 100 µL of SOLN CONJ into each well. Cover the strips with a new piece of adhesive film and incubate for **30 minutes at 37 °C**.

9.9. Following incubation, remove the film carefully and wash the wells five times as described in para. 9.7.

9.10. Add 100 µL of SOLN TMB into the wells; do not touch the bottom and the walls of the plate wells.

9.11. Incubate the strips for **30 minutes** in a dark place at a room temperature of 18-25 °C. Do not use adhesive film at this stage.

9.12. Add 100 µL of SOLN STOP into each strip well to stop the enzymatic reaction; adhere to the same sequence of actions as when adding SOLN TMB. At the time of adding, the solution colour changes from blue to yellow, and clear solution slightly changes its shade.

9.13. Measure the optical density (OD) of the wells at 450/620-695 nm wavelength using an ELISA microplate reader within 5 minutes after stopping the reaction. Pay attention to the cleanness of the plate bottom and the absence of bubbles in the wells before reading.

Measurement at the single wavelength of 450 nm is possible, in that case, it is needed to leave one well for blank (only SOLN TMB and SOLN STOP must be added *in blank well).*

10. CALCULATION AND INTERPRETATION OF RESULTS

10.1. Calculation of results

Calculate the average OD for the negative control ($\overline{Nc}$), Cut off (CO) and a sample positivity index (IP_{sample}).

$$\overline{Nc} = (Nc1 + Nc2 + Nc3)/3; \quad CO = \overline{Nc} + 0{,}3$$

$$IP_{sample} = OD_{sample}/CO, \text{ where } OD_{sample} \text{ is the OD sample.}$$

10.2. Quality control (assay validation)

The test results are considered valid if they meet the following requirements:

CONTROL +	OD ≥ 1,0	
CONTROL -	OD ≤ 0,150	
CONTROL -	$\overline{Nc} \times 0{,}5 \le Ncn \le \overline{Nc} \times 2{,}0$	where Ncn is the OD for each Nc run

If any of the OD values for the negative control is beyond the above interval, it should be discarded, and $\overline{Nc}$ is calculated based on the remaining OD values for the negative control. If several OD values for the negative control fail to meet the above requirements, the test is considered invalid and requires a new run.

10.3. Interpretation of results

$IP_{sample} > 1{,}1$	POSITIVE
$0{,}9 \le IP_{sample} \le 1{,}1$	BORDERLINE*
$IP_{sample} < 0{,}9$	NEGATIVE

* Uncertain samples are recommended to be re-examined in two wells of the ELISA kit. If the results are again uncertain, a new sample should be selected and analyzed in 2-4 weeks. In case of repeated indeterminate results, such samples shall be considered negative.

11. PERFORMANCE CHARACTERISTICS

11.1. Analytical performance characteristics

Precision of measurement

Intra assay repeatability

The coefficient of variation (CV) for three sera with different levels of specific antibodies was evaluated in 24 replicates on one series of ELISA kits.

Sample No.	OD_{av}	IP_{av}	CV, %
547	0,504	1,43	2,9
671	0,753	2,13	3,6
413	1,165	3,30	3,1

Inter assay reproducibility

The coefficient of variation (CV) for three sera with different levels of specific antibodies was evaluated for 4 days in 4 sets of analysis, 8 replicates in each analysis.

Sample No.	OD_{av}	IP_{av}	CV, %
547	0,534	1,55	5,0
671	0,750	2,17	4,6
413	1,159	3,36	3,6

Analytical specificity

The test results are not affected by bilirubin at up to 0.21 mg/mL (361.8 μmol/L), haemoglobin at up to 10 mg/mL and triglycerides at up to 10 mg/mL (11.3 mmol/l) present in the sample.

11.2. Diagnostic characteristics

To evaluate clinical sensitivity and specificity of «EQUI Ascaris lumbricoides IgG» ELISA kits, 55 serum samples from patients with clinical symptoms typical for lumbricosis and 60 serum samples from patients without clinical manifestations (seronegative in terms of *Ascaris lumbricoides*) were used. Clinical sensitivity of «EQUI Ascaris lumbricoides IgG» ELISA kits was 94.55 % and clinical specificity — 93.3 %.

Method characteristics in comparison with equal commercial ELISA kit was studied in target paediatric population (160 samples) and population of donors (346 samples). For paediatric population serum, relative specificity of «EQUI Ascaris lumbricoides IgG» ELISA kits was established at the level of 97.92 % and percent agreement was 95.51 %. For donor population serum, relative specificity of was 89.74 %, relative specificity — 96.30 % and percent agreement was 95.47 %.

12. LIMITATIONS OF ASSAY

Positive result in «EQUI Ascaris lumbricoides IgG» ELISA kit supports presence of anti-*Ascaris lumbricoides* specific IgG antibodies. Presence of this class antibodies in newborns is not an evidence of *Ascaris lumbricoides* invasion.

Inconclusive results may suggest a history of *Ascaris lumbricoides* invasion.

Negative result of «EQUI Ascaris lumbricoides IgG» ELISA kit supports the absence of anti- *Ascaris lumbricoides* IgG specific antibodies in the test sample or concentration of specific antibodies is below the sensitivity limit of the assay.

The results of serological test only are not the basis for final diagnosis. When establishing the diagnosis, the results of complex laboratory and instrumental tests, as well as clinical manifestations should be considered. Cross-reactions with antibodies to antigens of other helminths cannot be fully ruled out.

13. DIFFICULTIES THAT CAN OCCUR DURING THE ASSAY PROCEDURE

Possible reasons	Solution
High background in all wells	
Contaminated washer	Clean the washer head and rinse according to the instructions for use
Poor quality or contaminated water	Use purified water with specific resistance ≥ 10 MΩ · cm
Use of poorly washed glassware	Use chemically clean utensils
Use of chlorinated disinfectants	Do not use chlorine disinfectants
Use of contaminated tips	Use new tips
Increased incubation times or change in the temperature conditions	Adhere to the incubation regime according to the instructions for use
High background in a row of wells	
Repeat application of TMB solution	TMB solution should be applied once
Contamination of the automatic pipette nozzle with conjugate solution	Clean the pipette and dial carefully liquid
Contamination of one of the washer's channel	Clean the flush channel, rinse washer
Received OD of the positive control is below the border value	
One of the reagents (conjugate solution or TMB solution) was not prepared in a correct way or was not added	Re-conduct ELISA, pay attention to the correctness of the introduction of these reagents
Reduced incubation times at any stage	Incubate according to instructions for use
The colour density of the wells fails to meet the obtained optical density value	
This may suggest that the optical beam has been displaced	Check the correct operation of the reader

14. TECHNICAL ASSISTANCE AND CUSTOMER SERVICE

In case of technical problems, you can obtain assistance by contacting the manufacturer.

REFERENCES

1. CDC - Ascariasis // https://www.cdc.gov/parasites/ascariasis/index.html.
2. Cooper P. J., Chico M. E. et al. Human Infection with Ascaris lumbricoides Is Associated with a Polarized Cytokine Response // The Journal of Infectious Diseases. - 2003. - Vol. 182 (4). - P. 1207–1213.
3. Gupta S., Kumar S. et al. Ascaris lumbricoides: an unusual aetiology of gastric perforation // Journal of Surgical Case Reports. - 2012. - Vol. 2012. - rjs008.
4. Li Q., Zhao D. et al. Life-threatening complications of ascariasis in trauma patients: a review of the literature // World Journal of Emergency Medicine. - 2014. - Vol. 5 (3). - P. 165–170.
5. McSharry C., Xia Y. et al. Natural Immunity to Ascaris lumbricoides Associated with Immunoglobulin E Antibody to ABA-1 Allergen and Inflammation Indicators in Children // Infection and Immunity. - 1999. - Vol. 67(2). - P. 484–489.
6. Palmer L. J., Celedón J. C. et al. Ascaris lumbricoides Infection Is Associated with Increased Risk of Childhood Asthma and Atopy in Rural China // American Journal of Respiratory and Critical Care Medicine. - 2002. - Vol. 165, No. 11. - P. 1489–1493.
7. Shalaby N. Effect of Ascaris lumbricoides infection on T helper cell type 2 in rural Egyptian children // Therapeutics and Clinical Risk Management. - 2016. - Vol. 12. - P. 379–385.
8. WHO. Water related diseases: ascariasis. 2013 // http://www.who.int/water_sanitation_health/ diseases/ascariasis/en/.
9. Regulation (EU) 2017/746 of the European Parliament and of the Council of 5 April 2017 on in vitro diagnostic medical devices and repealing Directive 98/79/EC and Commission Decision 2010/227/EU.
10. Закон України «Про відходи» // Відомості Верховної Ради України. - 1998. - №36-37.
11. Наказ МОЗ України №325 від 08.06.2015 «Про затвердження Державних санітарно-протиепідемічних правил і норм щодо поводження з медичними відходами».
12. Постанова КМУ від 02 жовтня 2013р. №754 «Про затвердження технічного регламенту щодо медичних виробів для діагностики in vitro».
13. Hanna Tolonen, Kari Kuulasmaa, Tiina Laatikainen, Hermann Wolf and the European Health Risk Monitoring Project. Recommendation for indicators, international collaboration, protocol and manual of operations for chronic disease risk factor surveys Part 4.Storage and transfer of serum/plasma samples// Finnish National Public Health Institute 2002// https://thl.fi/publications/ehrm/product2/part_iii4.htm
14. Surveillance Guidelines for Measles, Rubella and Congenital Rubella Syndrome in the WHO European Region. Annex 3.Collection, storage and shipment of specimens for laboratory diagnosis and interpretation of results// Geneva: World Health Organization; 2012 Dec.

	Manufacturer
EC REP	Authorized Representative in the European Community
IVD	In vitro diagnostic medical device
REF	Catalogue number
	Date of manufacture
	Use by date
LOT	Batch code
	Temperature limit
Σ	Contains sufficient for <n> tests
!	Caution
NON STERILE	Non-Sterile
i	Consult instructions for use
	Keep away from sunlight
	Keep dry
CE	Compliance with EU safety requirements

Edition 8, 10.02.2022

For questions and suggestions regarding the ELISA kit contact:

EC REP

Obelis s.a.
Bd Général Wahis 53
1030 Brussels
Belgium
Tel: +(32)2 732-59-54
Fax: +(32)2 732-60-03
mail@obelis.net

Ekvitestlab LLC
Velyka Vasylkivska St. 114, Kyiv, Ukraine, 03150
Tel: 0(800)31-89-87, +38 (044)334-89-87,
e-mail: info@equitest.com.ua, www.equitest.com.ua

ASSAY PROCEDURE SCHEME

Keep all reagents for 30 min at temperature18-25°C before use
Dispense 90 μl $\boxed{\text{DIL}\,\vert\,\text{SAMPLE}}$ into the wells (brown)
Add to 10 μl of controls and samples into the wells: A1 – $\boxed{\text{CONTROL}\,\vert\,+}$, B1, C1, D1 – $\boxed{\text{CONTROL}\,\vert\,-}$, other wells – examined samples (change of colour from brown to blue)
Cover strips with an adhesive film, incubate for **30 min at 37°C**
Rinse the wells 5 times with prepared 1:20 (1+19) washing solution TWEEN (300 μl per well)
Add 100 μl of $\boxed{\text{SOLN}\,\vert\,\text{CONJ}}$ into all wells (green)
Cover strips with an adhesive film, incubate for **30 min at 37°C**
Rinse the wells 5 times with prepared 1:20 (1+19) washing solution TWEEN (300 μl per well)
Add 100 μl of $\boxed{\text{SOLN}\,\vert\,\text{TMB}}$ into all wells
Incubate for **30 min** in the dark at **18-25°C**
Add 100 μl of $\boxed{\text{SOLN}\,\vert\,\text{STOP}}$ into all wells (change of colour from blue to yellow)
Measure the optical density (OD) with an ELISA microplate reader at 450/620-695 nm

CALCULATION OF RESULTS

$\overline{Nc}$ = (Nc1 + Nc2 + Nc3)/3;

CO = $\overline{Nc}$ + 0,3;

$IP_{sample} = OD_{sample}/CO$

$\overline{Nc}$ - the average value of OD 3-x $\boxed{\text{CONTROL}\,\vert\,-}$

CO - Cut off

IP_{sample} - sample positivity index

INTERPRETATION OF RESULTS

$IP_{sample} > 1,1$	POSITIVE
$0,9 \leq IP_{sample} \leq 1,1$	BORDERLINE
$IP_{sample} < 0,9$	NEGATIVE

Toxocara canis IgG

ELISA kit for the qualitative detection of IgG antibodies to *Toxocara canis*

Instructions for use

IVD

REF EI-603

Σ 96 tests

CE

EQUI Toxocara canis IgG

ELISA kit for the qualitative detection of
IgG antibodies to *Toxocara canis*

1. INTENDED USE

The «EQUI Toxocara canis IgG» is ELISA kit intended to qualitatively detect anti-*Toxocara canis* IgG in human serum or plasma by enzyme-linked immunosorbent assay (ELISA) in order to diagnose toxocariasis. The testing procedure is designed for both manual arrangement with automatic pipettes and standard equipment, and for automated «open» immunoassay analysers.

Target group: children, pet owners, rural people, summer visitors, forest guards, veterinarians.

Usage: ELISA kit is used in clinical diagnostic laboratories and other institutions engaged in *in vitro* diagnostics.

2. CLINICAL SIGNIFICANCE

Toxocariasis is a common disease induced by *Toxocara* helminth which is transmitted from animals to human. Toxocariasis is spread throughout the world, however, it is more common in depressed areas with poor hygienic conditions. In some regions, up to 90 % of puppies and up to 10 % of adult domesticated dogs are infested with toxocara. The risk of infestation is higher for owners of cats and dogs and for children due to playing in the sandpits and on the playgrounds contaminated with animal faeces.

Toxocara are threadworms belonging to *Nematoda*. Human conditions are mostly caused by *Toxocara canis*, which infested canids, rare - *Toxocara cati*, which is more common in felids. Adult toxocara in the body of infested animals reaches 5–15 cm in length; their propagation takes place here. Female helminths lay about 200 thous eggs daily, which are excreted in the environment with faeces. If conditions are favourable, following several weeks of maturation in the soil they become invasive — a larva is developed in the eggs. In the paratenic host (mice, poultry, cows, pigs, etc.). larva develops without propagation. If the conditions are unfavourable, larvae are encapsulated and may maintain viability for a long time (up to 10 years). They may also be the source of invasion.

People are infested through faecal-oral route when ingesting *Toxocara canis* mature eggs with soil-contaminated vegetables, fruits, berries, via dirty hands or when consuming meat of paratenic hosts. In the small intestine, larvae leave their cover and penetrates blood circulation through the intestinal walls. The larvae migrate to other organs and tissues with blood, namely: liver, lungs, muscles, eyes, CNS, etc. In the most of the infested, toxocariasis is asymptomatic. Clinical manifestations of this disease are associated with the site of larvae migration and depend on the intensity of invasion and age of the host. Visceral syndrome larva migrans is typical after infestation of the internal organs with *Toxocara canis* and occular toxocariasis, when eye and optic nerve are involved. Symptoms of visceral toxocariasis: fever, fatigue, abdominal pain, anorexia, hepatomegaly, cough and others. Heart and respiratory failure may develop in severe cases. Due to a strong immune response to larvae antigens, immediate and delayed hypersensitivity reactions develop. Granulomatosis in occular toxocariasis may result in retinal detachment and loss of vision.

Diagnosis of toxocariasis is complicated due to the lack of specific manifestations of the disease, even upon intense invasion. Furthermore, a man is an intermediate host of *Toxocara canis* and does not excrete parasites in the environment, whereas it is difficult to localise larvae in certain organs via non-invasive methods. Eosinophilia may appear in blood tests, however, serological tests are more common to detect toxocariasis (immunofluorescence reaction, ELISA and immunoblotting). Detection of specific anti-*Toxocara canis* IgG to larvae antigens may suggest current or previous invasion. High titter of IgE antibodies is also typical for active invasion. However, the combination of clinical manifestations and laboratory findings are necessary for diagnosis.

3. ANALYSIS PRINCIPLE

The procedure of testing for anti-*Toxocara canis* IgG in «EQUI Toxocara canis IgG» ELISA kit is based on «indirect» solid-phase ELISA with a two-stage incubation. Antigens of *Toxocara canis* larvae are entrapped in the wells. During the first step of incubation of ELISA plate wells with test samples, specific anti-*Toxocara canis* antibodies (if present in the samples) bind to the solid-phase antigens. The wells are washed to remove unbound antibodies and have only specific antigen-antibody complexes left. Then, a conjugate of anti-species IgG monoclonal antibodies with horseradish peroxidase is added, which binds to solid-phase immune complexes. Unbound components are removed by washing. Antigen-antibody complexes are detected by adding a solution of chromogen 3,3’,5,5’-tetramethylbenzidine (TMB) with hydrogen peroxide. After 30-minute incubation, the reaction is stopped by adding the stop solution. The optical density (OD) in the wells is determined using a spectrophotometer at 450/620-695 nm. The intensity of the yellow colour is proportional to the level of antibodies in the sample.

4. MATERIALS AND EQUIPMENT

4.1. Contents of the ELISA kit

STRIPS	1 x 96 wells	**Microplate** Each plate well is coated with *Toxocara canis* larval antigens. The wells are detachable. After the first opening, store unused strips in the package at 2-8 °C for a maximum of 6 months

CONTROL +	1 x 0,25 ml	**Positive control** Conjugated specific monoclonal antibody solution with preservative (pink). Store at 2-8 °C
CONTROL -	1 x 0,6 ml	**Negative control** Negative human serum with a preservative (yellow). Store at 2-8 °C
DIL SAMPLE	1 x 13 ml	**Serum dilution solution** Buffer solution with a milk extract, a detergent and a preservative (brown). Store at 2-8 °C
SOLN CONJ	1 x 13 ml	**Conjugate solution (ready to use)** Buffer solution of monoclonal antibodies to human IgG, conjugated with horseradish peroxidase, with stabilizers and preservative (green). Store at 2-8 °C
SOLN TMB	1 x 13 ml	**TMB solution (ready to use)** TMB solution, H_2O_2, a stabilizer, a preservative (colourless). Store at 2-8 °C
TWEEN WASH 20x	1 x 50 ml	**Washing solution TWEEN (20x concentrated)** 20-fold phosphate buffer concentrate with Tween-20 (colourless). Dilute TWEEN detergent (20x) at 1:20 with distilled or deionized water (e. g., 5 mL of concentrate + 95 mL of water for 8 wells) before use. Store the diluted solution at 2-8 °C for a maximum of 7 days
SOLN STOP	1 x 13 ml	**Stop Solution (ready to use)** 0.5 mol H_2SO_4 solution (colourless). Store at 2-8 °C

The ELISA kit also includes adhesive films (2 items), sample application plan (1 item), checklist, and instruction for use.

4.2. Optional reagents, materials and equipment

Automatic single and multichannel pipettes 10–1000 μL, tips, volumetric laboratory glassware (10–1,000 mL), deionized or distilled water, thermostat at 37 °C, automatic or semi-automatic plate washer, spectrophotometer (reader) for microplates at 450/620-695 nm, appropriate containers for potentially contaminated waste, timer, filter paper, disposable powder-free gloves, disinfectants.

5. PRECAUTIONS AND SAFETY

5.1. Precautions

Be sure to read the instructions for use carefully before the test. The validity of the test results depends on strict following of the test procedure.

– do not use the ELISA kit components after the expiry date;
– do not use for analysis or mix components of different batches, components of kits for different nosologies, or reagents from other manufacturers with the «EQUI Toxocara canis IgG» ELISA kit;

– do not freeze the ELISA kit or its contents;
– after using a reagent, close each vial with its cap;
– when washing, control filling and complete aspiration of solution from the wells;
– use a new pipette tip each time you add samples or reagents;
– prevent direct sunlight from reaching the reagents from the ELISA kit;
– SOLN TMB solution must be colourless before use. Do not use the solution if its colour is blue or yellow. Avoid contact of SOLN TMB with metals or metal ions. Use only clean glassware thoroughly rinsed with distilled water;
– do not use reagents with colour not in line with para. 4.1;
– under no circumstances should the same glassware be used for SOLN CONJ and SOLN TMB;
– do not evaluate the test results visually (without a reader);
– any optional equipment that is in direct contact with biological material or kit components should be considered contaminated and requires cleaning and decontamination;
– the ELISA kit includes materials for 96 tests. Dispose of the used components as well as any remaining unused components.

5.2. Safety requirements

– all reagents in the ELISA kit are for laboratory professional use for *in vitro* diagnosis only and may only be used by qualified personnel;
– conduct the tests in disposable powder-free gloves and goggles only;
– do not eat, drink, smoke, or apply make-up in the test room;
– do not mouth-pipette the solutions;
– controls from the «EQUI Toxocara canis IgG» ELISA kit have been tested and found to be for anti-HIV1/2, anti-HCV and anti-*Treponema pallidum* antibodies and HBsAg negative; however, controls and test samples should be handled as potentially hazardous infectious materials;
– some of the kit components contain low concentrations of harmful substances and can damage skin or mucoga. In case of contact of SOLN TMB, SOLN STOP and SOLN CONJ with mucous membranes or skin, immediately wash the affected area with plenty of water;
– in case of spillage of acid-free solutions, e. g. sera, treat the surface with a disinfectant solution and then wipe dry with filter paper. Otherwise first neutralize acid with sodium bicarbonate solution and then wipe the surface dry as described above.

5.3. Waste inactivation and disposal

– the liquid waste must be inactivated, for example, with hydrogen peroxide solution at the final concentration of 6% for 3 hours at room temperature, or with sodium hypochlorite at the final concentration of 5% for 30 minutes, or with other approved disinfectants;

– the solid waste must be inactivated by autoclaving at a temperature not less than 132°C;
– do not autoclave the solutions that contain sodium azide or sodium hypochlorite;
– disposal of inactivated waste must be conducted due to national laws and regulations.

6. STORAGE AND STABILITY

ELISA kit is stable up to the expiry date stated on the label when stored at 2-8°C. The kit should be transported at 2-8°C. Single transportation at a temperature up to 23°C for two days is possible.

7. SAMPLE COLLECTION, TRANSPORTATION AND STORAGE GUIDELINES

Collect blood from the vein into the sterile test tube. Test tube must be marked with patient ID and date of sample collecting. Blood before serum separation can be stored at 2-8 ºC for 24 hours, avoiding freezing.

Serum or plasma can be stored at 2-8 °C for maximum 3 days. Frozen serum can be stored for longer periods of time at -20 °C or -70 °C. Thaw frozen samples and keep them at room temperature for 30 minutes before use. After thawing, the stir samples to achieve homogeneity. Avoid repeated freezing-thawing cycles for test samples. If serum (or plasma) is turbid, remove insoluble inclusions by centrifugation at 3000 rpm for 10-15 minutes. Do not use serum samples with hyperlipidemia, hemolysis, and bacterial growth.

Transport serum samples in insulated containers. To do that, put closed labelled tubes in a plastic bag, tightly seal it and place in the centre of an insulated container.Put the frozen cold packs on the bottom, along the side walls of the insulated container and on top of the serum samples.

8. REAGENT PREPARATION

NOTE! It is very important to keep all ELISA kit components for at least 30 min at room temperature 18-25 ºC before the assay!

8.1. Microplate preparation

To prevent water condensation in the wells, keep the STRIPS for 30 minutes at a room temperature before opening. Open the vacuum pack, detach the appropriate number of wells, and carefully pack the remaining wells with a desiccant and store tightly zip-locked at 2-8 °C. Storing the packed plate this way ensures its stability for 6 months.

8.2. Washing solution preparation

To prepare detergent, dilute TWEEN WASH 20x at 1:20 (1+19) with distilled or deionized water and stir. E. g., 5 mL of concentrate + 95 mL of water, which is enough for 8 wells. If there are crystals present in the detergent concentrate, heat the vial at 37 °C until the crystals dissolve completely (15–20 minutes). Store the diluted solution at 2-8 °C for a maximum of 7 days.

9. ASSAY PROCEDURE

9.1. Prepare the necessary number of wells (four wells for controls and a necessary number of wells for test samples) and insert them into the ELISA plate frame. Be sure to add control wells in every test run.

9.2. Fill in the sample application plan.

9.3. Prepare the detergent as per para. 8.2.

9.4. Add 90 µL of DIL SAMPLE into each plate well.

9.5. Add 10 µL of controls and test samples into the wells:

CONTROL + – into well A1,

CONTROL - – into wells B1, C1 and D1,

and test samples into the remaining wells.

At the time of adding, the solution changes its colour from brown to blue. Pipette the mix in the wells carefully to avoid foaming.

9.6. Cover the strips up with adhesive film and incubate for **30 minutes at 37 °C**.

9.7. Remove and discard the adhesive film and wash all wells 5 times with automatic washer or 8-channel pipette as follows:

– aspirate the content of all wells into a liquid waste container;

– add a minimum of 300 µl of diluted washing solution to each well, soak each well for 30 seconds;

– aspirate the content of all wells again. The residual volume after every aspiration should be less than 5 µl;

– repeat the washing step 4 more times;

– after the final aspiration, eliminate extra moisture by tapping the plate against a piece of filter paper.

9.8. Add 100 µL of SOLN CONJ into each well. Cover the strips with a new piece of adhesive film and incubate for **30 minutes at 37 °C**.

9.9. Following incubation, remove the film carefully and wash the wells five times as described in para. 9.7.

9.10. Add 100 µL of SOLN TMB into the wells; do not touch the bottom and the walls of the plate wells.

9.11. Incubate the strips for **30 minutes** in a dark place at a room temperature of 18-25 °C. Do not use adhesive film at this stage.

9.12. Add 100 µL of SOLN STOP into each strip well to stop the enzymatic reaction; adhere to the same sequence of actions as when adding SOLN TMB. At the time of adding, the solution colour changes from blue to yellow, and clear solution slightly changes its shade.

9.13. Measure the optical density (OD) of the wells at 450/620-695 nm wavelength using an ELISA microplate reader within 5 minutes after stopping the reaction. Pay attention to the cleanness of the plate bottom and the absence of bubbles in the wells before reading.

Measurement at the single wavelength of 450 nm is possible, in that case, it is needed to leave one well for blank (only SOLN TMB and SOLN STOP must be added *in blank well).*

10. CALCULATION AND INTERPRETATION OF RESULTS

10.1. Calculation of results

Calculate the average OD for the negative control ($\overline{Nc}$), Cut off (CO) and a sample positivity index (IP_{sample}).

$$\overline{Nc} = (Nc1 + Nc2 + Nc3)/3; \quad CO = \overline{Nc} + 0{,}3$$

$$IP_{sample} = OD_{sample}/CO, \text{ where: } OD_{sample} \text{ is the OD sample.}$$

10.2. Quality control (assay validation)

The test results are considered valid if they meet the following requirements:

CONTROL +	$OD \geq 1{,}0$	
CONTROL -	$OD \leq 0{,}150$	
CONTROL -	$\overline{Nc} \times 0{,}5 \leq Ncn \leq \overline{Nc} \times 2{,}0$	where Ncn is the OD for each Nc run

If any of the OD values for the negative control is beyond the above interval, it should be discarded, and $\overline{Nc}$ is calculated based on the remaining OD values for the negative control. If several OD values for the negative control fail to meet the above requirements, the test is considered invalid and requires a new run.

10.3. Interpretation of results

$IP_{sample} > 1{,}1$	POSITIVE
$0{,}9 \leq IP_{sample} \leq 1{,}1$	BORDERLINE*
$IP_{sample} < 0{,}9$	NEGATIVE

* Uncertain samples are recommended to be re-examined in two wells of the ELISA kit. If the results are again uncertain, a new sample should be selected and analyzed in 2-4 weeks. In case of repeated indeterminate results, such samples shall be considered negative.

11. PERFORMANCE CHARACTERISTICS

11.1. Analytical performance characteristics

Precision of measurement

Intra assay repeatability

The coefficient of variation (CV) for three sera with different levels of specific antibodies was evaluated in 24 replicates on one series of ELISA kits.

Sample No.	OD_{av}	IP_{av}	CV, %
669	0,927	2,81	4,8
544	1,503	4,56	1,4
666	1,694	5,14	4,5

Inter assay reproducibility

The coefficient of variation (CV) for three sera with different levels of specific antibodies was evaluated for 4 days in 4 sets of analysis, 8 replicates in each analysis.

Sample No.	OD_{av}	IP_{av}	CV, %
669	1,016	3,04	4,7
544	1,516	4,54	1,9
666	1,683	5,04	4,1

Analytical specificity

The test results are not affected by bilirubin at up to 0.21 mg/mL (361.8 μmol/L), haemoglobin at up to 10 mg/mL and triglycerides at up to 10 mg/mL (11.3 mmol/l) present in the sample.

11.2. Diagnostic characteristics

To evaluate diagnostic characteristics of «EQUI Toxocara canis IgG» ELISA kits, 78 serum samples from patients with clinical symptoms typical for toxocariasis and 60 serum samples from patients without clinical manifestations (seronegative in terms of *Toxocara canis*) were used. Clinical sensitivity of «EQUI Toxocara canis IgG» ELISA kits was 98.7 %, clinical specificity — 96.7 %.

Method characteristics in comparison with equal commercial ELISA kit was studied in target paediatric population (160 samples) and population of donors (298 samples). For paediatric population serum, relative specificity of «EQUI Toxocara canis IgG» ELISA kits was established at the level of 99.28 % and percent agreement was 97.45 %. For donor population serum, relative specificity of was 89.19 %, relative specificity — 93.55 % and percent agreement was 91.73 %.

12. LIMITATIONS OF ASSAY

Positive result in «EQUI Toxocara canis IgG» ELISA kit supports presence of anti-*Toxocara canis* specific IgG antibodies. Presence of this class antibodies in newborns is not an evidence of *Toxocara canis* invasion.

Inconclusive results may suggest a history of *Toxocara canis* invasion.

Negative result of «EQUI Toxocara canis IgG» ELISA kit supports the absence of anti-*Toxocara canis* specific IgG antibodies in the test sample or concentration of specific antibodies is below the sensitivity limit of the assay.

The results of serological test only are not the basis for final diagnosis. When establishing the diagnosis, the results of complex laboratory and instrumental tests, as well as clinical manifestations should be considered. Cross-reactions with antibodies to antigens of other helminths cannot be fully ruled out.

13. DIFFICULTIES THAT CAN OCCUR DURING THE ASSAY PROCEDURE

Possible reasons	Solution
High background in all wells	
Contaminated washer	Clean the washer head and rinse according to the instructions for use
Poor quality or contaminated water	Use purified water with specific resistance ≥ 10 MΩ · cm
Use of poorly washed glassware	Use chemically clean utensils
Use of chlorinated disinfectants	Do not use chlorine disinfectants
Use of contaminated tips	Use new tips
Increased incubation times or change in the temperature conditions	Adhere to the incubation regime according to the instructions for use
High background in a row of wells	
Repeat application of TMB solution	TMB solution should be applied once
Contamination of the automatic pipette nozzle with conjugate solution	Clean the pipette and dial carefully liquid
Contamination of one of the washer's channel	Clean the flush channel, rinse washer
Received OD of the positive control is below the border value	
One of the reagents (conjugate solution or TMB solution) was not prepared in a correct way or was not added	Re-conduct ELISA, pay attention to the correctness of the introduction of these reagents
Reduced incubation times at any stage	Incubate according to instructions for use
The colour density of the wells fails to meet the obtained optical density value	
This may suggest that the optical beam has been displaced	Check the correct operation of the reader

14. TECHNICAL ASSISTANCE AND CUSTOMER SERVICE

In case of technical problems, you can obtain assistance by contacting the manufacturer.

REFERENCES

1. Cobzaru R. G., Rîpă C. et al. Correlation between asthma and Toxocara canis infection // Rev Med Chir Soc Med Nat Iasi. - 2012. - Vol. 116(3). - P. 727–730.
2. Despommier D. Toxocariasis: Clinical Aspects, Epidemiology, Medical Ecology, and Molecular Aspects // Clinical Microbiology Reviews. - 2003. - Vol. 16, No. 2. - P. 265–272.
3. Havasiová-Reiterová K., Tomašovicová O. and Dubinský P. Effect of various doses of infective Toxocara canis and Toxocara cati eggs on the humoral response and distribution of larvae in mice // Parasitology Research. - 1995. - Vol. 81. - P. 13–17.
4. Iddawela D., Ehambaram K., and Bandara P. Prevalence of Toxocara antibodies among patients clinically suspected to have ocular toxocariasis: A retrospective descriptive study in Sri Lanka // BMC Ophthalmology. - 2017. - Vol. 17. - 6 p.
5. Maizels R. M. Toxocara canis: Molecular basis of immune recognition and evasion // Veterinary Parasitology. - 2013. - Vol. 193 (4). - P. 365–374.
6. Magnaval J.-F., Glickman L. T. et al. Highlights of human toxocariasis // Korean Journal of Parasitology. - 2001. - Vol. 39 (1). - P. 1–11.
7. McGuinness S. L., Leder K. Global Burden of Toxocariasis: A Common Neglected Infection of Poverty // Current Tropical Medicine Reports. - 2014. - Vol. 1 (1). - P. 52–61.
8. Núñez C. R., Mendoza Martínez G. D. et al. Prevalence and Risk Factors Associated with Toxocara canis Infection in Children // The Scientific World Journal. - Volume 2013. - Article ID 572089. - 4 p.
9. Okulewicz A., Perec-Matysiak A. et al. Toxocara canis, Toxocara cati and Toxascaris leonina in wild and domestic carnivores // Helminthologia. - 2012. - Vol. 49. - P. 3–10.
10. Regulation (EU) 2017/746 of the European Parliament and of the Council of 5 April 2017 on in vitro diagnostic medical devices and repealing Directive 98/79/EC and Commission Decision 2010/227/EU.
11. Закон України «Про відходи» // Відомості Верховної Ради України. - 1998. - №36-37.
12. Наказ МОЗ України №325 від 08.06.2015 «Про затвердження Державних санітарно-протиепідемічних правил і норм щодо поводження з медичними відходами».
13. Постанова КМУ від 02 жовтня 2013р. №754 «Про затвердження технічного регламенту щодо медичних виробів для діагностики in vitro».
14. Hanna Tolonen, Kari Kuulasmaa, Tiina Laatikainen, Hermann Wolf and the European Health Risk Monitoring Project. Recommendation for indicators, international collaboration, protocol and manual of operations for chronic disease risk factor surveys Part 4.Storage and transfer of serum/plasma samples// Finnish National Public Health Institute 2002// https://thl.fi/publications/ehrm/product2/part_iii4.htm
15. Surveillance Guidelines for Measles, Rubella and Congenital Rubella Syndrome in the WHO European Region. Annex 3.Collection, storage and shipment of specimens for laboratory diagnosis and interpretation of results//Geneva: World Health Organization; 2012 Dec.

	Manufacturer
EC REP	Authorized Representative in the European Community
IVD	In vitro diagnostic medical device
REF	Catalogue number
	Date of manufacture
	Use by date
LOT	Batch code
	Temperature limit
Σ	Contains sufficient for <n> tests
	Caution
NON STERILE	Non-Sterile
	Consult instructions for use
	Keep away from sunlight
	Keep dry
CE	Compliance with EU safety requirements

Edition 8, 04.04.2022

For questions and suggestions regarding the ELISA kit contact:

EC REP

Obelis s.a.
Bd Général Wahis 53
1030 Brussels
Belgium
Tel: +(32)2 732-59-54
Fax: +(32)2 732-60-03
mail@obelis.net

Ekvitestlab LLC
Velyka Vasylkivska St. 114, Kyiv, Ukraine, 03150
Tel: 0(800)31-89-87, +38 (044)334-89-87,
e-mail: info@equitest.com.ua, www.equitest.com.ua

ASSAY PROCEDURE SCHEME

Keep all reagents for 30 min at temperature18-25°C before use
Dispense 90 µl DIL SAMPLE into the wells (brown)
Add to 10 µl of controls and samples into the wells: A1 – CONTROL + , B1, C1, D1 – CONTROL − , other wells – examined samples (change of colour from brown to blue)
Cover strips with an adhesive film, incubate for **30 min at 37°C**
Rinse the wells 5 times with prepared 1:20 (1+19) washing solution TWEEN (300 µl per well)
Add 100 µl of SOLN CONJ into all wells (green)
Cover strips with an adhesive film, incubate for **30 min at 37°C**
Rinse the wells 5 times with prepared 1:20 (1+19) washing solution TWEEN (300 µl per well)
Add 100 µl of SOLN TMB into all wells
Incubate for **30 min** in the dark at **18-25°C**
Add 100 µl of SOLN STOP into all wells (change of colour from blue to yellow)
Measure the optical density (OD) with an ELISA microplate reader at 450/620-695 nm

CALCULATION OF RESULTS

$\overline{Nc}$ = (Nc1 + Nc2 + Nc3)/3;

CO = $\overline{Nc}$ + 0,3;

$IP_{sample} = OD_{sample}/CO$

$\overline{Nc}$ - the average value of OD 3-x CONTROL −

CO - Cut off

IP_{sample} - sample positivity index

INTERPRETATION OF RESULTS

IP_{sample} > 1,1	POSITIVE
0,9 ≤ IP_{sample} ≤ 1,1	BORDERLINE
IP_{sample} < 0,9	NEGATIVE

HBsAg

ИФА-набор для качественного обнаружения поверхностного антигена вируса гепатита В

Инструкция по применению

IVD

REF EI-011

Σ 96 анализов

UA.TR.061

EQUI HBsAg

ИФА-набор для качественного обнаружения поверхностного антигена вируса гепатита В

1. НАЗНАЧЕНИЕ

Набор «EQUI HBsAg» предназначен для качественного обнаружения поверхностного антигена вируса гепатита В (HBsAg) в сыворотке или плазме крови человека методом иммуноферментного анализа (ИФА) с целью диагностики гепатита В и скрининга донорской крови. Процедура анализа рассчитана как для ручной постановки с автоматическими пипетками и стандартным оборудованием, так и для автоматического иммуноферментного анализатора «открытого» типа.

Целевая группа: доноры; лица-потребители инъекционных наркотиков; реципиенты крови или органов; беременные женщины; дети, рожденные от инфицированных матерей; лица, инфицированные ВИЧ; пациенты с симптомами заболеваний печени; пациенты гемодиализа.

Применение: ИФА-набор применяется в клинических диагностических лабораториях, станциях переливания крови, а также в других учреждениях, работающих в области *in vitro* диагностики.

2. КЛИНИЧЕСКОЕ ЗНАЧЕНИЕ

Одним из распространенных заболеваний печени является гепатит В. Его этиологический агент – вирус гепатита В (ВГВ). ВГВ относится к семейству Hepadnaviridae и содержит двухцепочечную ДНК. Инфекционной формой вируса являются так называемые частицы Дейна диаметром 42-49 nm, в белковом составе которых основными являются поверхностный антиген (HBsAg) и коровой антиген (HBcAg).

Клиническая картина гепатита В не позволяет диагностировать его длительное время и отличить от других вирусных гепатитов. Поэтому для скрининговых исследований и подтверждения диагноза важную роль играет лабораторная диагностика, особенно выявление антигенов ВГВ и антител к ним методом ИФА. Первым и основным маркером гепатита В является HBsAg, проявляющийся в крови через 3-5 недель после инфицирования. Приблизительно в то же время в крови можно обнаружить ДНК ВГВ и HBeAg, который считается маркером активной репликации вируса и «заразности» крови. ВОЗ рекомендует проводить проверку всей донорской крови на HBsAg, чтобы предотвратить трансмиссивную передачу ВГВ. Через 2-3 недели после появления HBsAg появляются антитела IgM к коровому антигену HBcAg, а вскоре после них – анти-HBcore IgG, быстро достигающие высоких уровней. Выздоровление от острого гепатита В сопровождается выведением вируса из организма, перестают выявляться HBsAg и анти-HBc IgM, появляются антитела к HBeAg. Антитела IgG к коровому антигену персистируют в течение всей жизни и являются маркером имеющегося или перенесенного гепатита В, их уровень в крови снижается медленно. Через несколько месяцев после исчезновения из крови HBsAg начинают выявляться анти-HBs антитела, свидетельствующие о перенесенном гепатите В и наличии иммунитета. В период «серологического окна» между выводом HBsAg и появлением анти-HBs антител маркером инфекции ВГВ являются суммарные антитела к коровому антигену, также могут проявляться анти-НВе антитела.

Если после острой фазы не происходит элиминация вируса и не появляются анти-HBs антитела, развивается хронический гепатит В. HBsAg продолжает определяться более 6 месяцев, его количество в крови может значительно колебаться. На репликативной стадии хронического гепатита В находится ДНК вируса и HBeAg, антител к HBeAg нет.

ВОЗ рекомендует диагностировать острый гепатит В при наличии HBsAg и антител IgM к HBcAg, а хронический – при устойчивом присутствии HBsAg в течение не менее шести месяцев.

Главным средством профилактики гепатита В является вакцинация, рекомендованная в первую очередь новорожденным. После вакцинации организмом продуцируются анти-HBs антитела и формируется иммунитет у лиц, не соприкасавшихся с вирусом гепатита В. Наличие анти-HBs антител на уровне более 10 IU/l (МЕ/л) принято считать нижним пределом протективного иммунитета вследствие вакцинации или перенесенного гепатита В.

3. ПРИНЦИП АНАЛИЗА

Обнаружение HBsAg в ИФА-наборе «EQUI HBsAg» базируется на принципе «сэндвич»-варианта твердофазного ИФА в одноэтапной инкубации. В лунках планшета засорбированы моноклональные антитела, специфические к HBsAg. В каждую лунку добавляются образцы сыворотки или плазмы пациента и конъюгат специфических к HBsAg антител с пероксидазой хрена. Во время инкубации исследуемых образцов и пероксидазного конъюгата в лунках планшета HBsAg, при наличии в образцах, связывается как с первыми антителами на твердой фазе, так и со вторыми антителами, конъюгированными с пероксидазой хрена, образуя «сэндвич» антитело -антиген-антитело. Несвязанные компоненты удаляются при отмывании. Иммунные комплексы обнаруживаются путем добавления раствора хромогена 3,3',5,5'-тетраметилбензидина (ТМБ) с перекисью водорода. После 30-минутной инкубации реакция останавливается добавлением стоп-раствора. Оптическая плотность (ОП) в лунках определяется на спектрофотометре при длине волны 450/620-695 nm. Интенсивность желтой окраски пропорциональна количеству HBsAg в образце.

4. МАТЕРИАЛЫ И ОБОРУДОВАНИЕ

4.1. Состав набора

STRIPS	1 x 96 лунок	**Планшет ИФА** В каждой лунке планшета засорбированы моноклональные антитела к HBsAg. Лунки можно отделять. После первого открытия храните неиспользованные стрипы в упаковке при температуре 2-8°C не более 6 месяцев
CONTROL +	1 x 1,6 ml	**Позитивный контроль** Раствор поверхностного антигена вируса гепатита B в буфере с альбумином и консервантом (розовый). Хранить при температуре 2-8°C
CONTROL -	2 x 1,6 ml	**Негативный контроль** Негативная сыворотка крови человека с консервантом (желтый). Хранить при температуре 2-8°C
CONJ 11x	1 x 0,8 ml	**Конъюгат (11x концентрат)** 11-кратный концентрат конъюгата моноклональных антител к HBsAg с пероксидазой хрена в буферном растворе со стабилизаторами и консервантом (фиолетовый). Развести конъюгат (11x) 1:11 раствором для разведения конъюгата перед использованием (например, 50 µl концентрата + 500 µl раствора для разведения конъюгата, достаточно для 8 лунок). Разбавленный раствор хранить при температуре 2-8°C не более 1 суток
DIL CONJ	1 x 8 ml	**Раствор для разведения конъюгата** Буферный раствор с белками сыворотки крови крупного рогатого скота и иммуноглобулинами мыши с консервантом (розовый). Хранить при температуре 2-8°C
SOLN TMB	1 x 13 ml	**Раствор ТМБ (готов к использованию)** Раствор ТМБ, H_2O_2, стабилизатор, консервант (бесцветный). Хранить при температуре 2-8°C
TWEEN WASH 20x	1 x 50 ml	**Раствор для промывки TWEEN (20x концентрат)** 20-кратный концентрат фосфатного буфера с Твином-20 (бесцветный). Развести раствор для промывки TWEEN (20x) 1:20 дистиллированной или деионизированной водой (например, 5 ml концентрата + 95 ml воды для 8 лунок) перед использованием. Разбавленный раствор хранить при температуре 2-8°C не более 7 суток
SOLN STOP	1 x 13 ml	**Стоп-раствор (готов к использованию)** Раствор 0,5 mol H_2SO_4 (бесцветный). Хранить при температуре 2-8°C

В состав набора входят: клейкая пленка (1 шт.), схема внесения образцов (1 шт.), лист контрольных испытаний и инструкция по применению.

4.2.Дополнительные реактивы, материалы и оборудование

Автоматические пипетки переменного объема на 10–1000 µl и наконечники к ним, мерная лабораторная посуда (10–1000 ml), деионизированная или дистиллированная вода, термошейкер на 37°С или термостат на 42°С, автоматический или полуавтоматический промыватель планшетов (вошер), спектрофотометр (ридер) для микропланшетов на 450/620-695 nm, соответствующие контейнеры для отходов потенциально зараженного материала, таймер, фильтровальная бумага, одноразовые неопудренные перчатки, дезинфицирующие средства.

5. ПРЕДОСТЕРЕЖЕНИЕ И ТЕХНИКА БЕЗОПАСНОСТИ

5.1. Предостережение

Перед проведением анализа внимательно ознакомьтесь с инструкцией по применению. Достоверность результата зависит от четкого следования процедуре анализа.

- не используйте компоненты ИФА-набора после окончания срока годности;
- не используйте во время анализа и не смешивайте компоненты разных серий, компоненты из наборов разных нозологий или реагенты других производителей в сочетании с набором «EQUI HBsAg»;
- не замораживайте ИФА-набор или его компоненты;
- после использования реагента закрывайте каждый флакон своей крышкой;
- во время промывания контролируйте наполнение и полную аспирацию раствора из лунок;
- каждый раз используйте новый наконечник пипетки для внесения образцов или реагентов;
- избегайте попадания прямых солнечных лучей на реагенты ИФА-набора;
- SOLN TMB должен быть бесцветным перед использованием. Если раствор окрашен в синий или желтый цвет, его нельзя использовать. Избегайте контакта SOLN TMB с металлами или ионами металлов. Для работы используйте только чистую, тщательно выполосканную дистиллированной водой посуду;
- не используйте реагенты, цвет которых не соответствует указанному в пункте 4.1;
- ни в коем случае не используйте одну и ту же посуду для рствора коньюгата и SOLN TMB;
- не проводите визуальный учет результатов анализа (без использования ридера);
- дополнительное оборудование, находящееся в непосредственном контакте с биологическим материалом или компонентами набора, считается загрязненным и нуждается в очищении и обеззараживании;

– ИФА-набор предназначен для 96 анализов. Компоненты после использования и остатки неиспользованных компонентов должны быть утилизированы.

5.2. Техника безопасности

– все реагенты набора предназначены только для лабораторного профессионального применения в *in vitro* диагностике и могут использоваться только квалифицированным персоналом;
– постановку анализа проводить только в одноразовых неопудреных перчатках и защитных очках;
– не допускается принимать пищу, пить, курить или пользоваться косметикой в комнате проведения теста;
– не пипетировать растворы ртом;
– CONTROL + ИФА-набора «EQUI HBsAg» содержит очищенный поверхностный антиген вируса гепатита В, выделенный с инактивированным прогреванием сыворотки крови человека, в которой не было обнаружено антител к ВИЧ1/2, ВГС и *Treponema pallidum*, однако работать с контролем следует как с потенциально инфекционным материалом;
– CONTROL - ИФА-набора «EQUI HBsAg» протестирован и признан отрицательным на HBsAg и антитела к ВИЧ1/2, ВГС, *Treponema pallidum*, однако обращаться с контролем и исследуемыми образцами следует как с потенциально опасным инфекционным материалом;
– некоторые компоненты набора содержат низкие концентрации вредных веществ и могут вызвать раздражение кожи и слизистых. При попадании SOLN TMB , SOLN STOP и раствора конъюгата на слизистые или кожу, необходимо немедленно промыть пораженное место большим количеством воды;
– в случае разбрызгивания растворов, не содержащих кислоту, например, сывороток, обработать поверхность дезинфицирующим средством, а затем насухо вытереть фильтровальной бумагой. В ином случае кислоту необходимо сначала нейтрализовать раствором бикарбоната натрия, а затем вытереть поверхность, как описано выше.

5.3. Инактивация и утилизация отходов

– жидкие отходы необходимо инактивировать, например, раствором перекиси водорода в конечной концентрации 6% в течение 3 часов при комнатной температуре или гипохлоритом натрия в конечной концентрации 5% в течение 30 минут или другими разрешенными дезинфицирующими средствами;
– твердые отходы следует инактивировать путем автоклавирования при температуре стерилизации не меньше 132°С;
– не автоклавируйте растворы, содержащие азид натрия или гипохлорит натрия;
– утилизацию инактивированных отходов проводить в соответствии с действующим национальным законодательством.

6. ХРАНЕНИЕ И ТРАНСПОРТИРОВКА

ИФА-набор стабилен в течение срока годности, указанного на этикетке, если его хранить при температуре 2-8°С. Транспортировать набор при температуре 2-8°С. Допускается одноразовая транспортировка при температуре не выше 23°С в течение двух суток.

7. РЕКОМЕНДАЦИИ ПО ОТБОРУ, ТРАНСПОРТИРОВКЕ И ХРАНЕНИЮ ОБРАЗЦОВ

Кровь необходимо отбирать из вены в стерильную пробирку. Пробирка должна быть промаркирована с указанием идентификационных данных пациента и даты отбора образца. Цельную кровь до отделения сыворотки можно хранить до 24 часов при температуре 2-8°С, не допуская замораживания.

Сыворотку или плазму крови можно хранить при температуре 2-8°С не более 3 суток. Допускается более продолжительное хранение замороженной сыворотки при температуре -20°С или -70°С. ЗЗамороженные образцы перед использованием следует разморозить и выдержать при комнатной температуре в течение 30 минут. После размораживания образцы следует перемешать для достижения однородности. Избегать повторного замораживания-оттаивания исследуемых образцов. В случае помутнения сыворотки (или плазмы) освобождаются от нерастворенных включений центрифугированием при 3000 об/мин в течение 10-15 минут. Не следует использовать образцы сывороток с выраженной липидемией, гемолизом, а также бактериальным проростом.

Образцы сывороток транспортировать в термоизоляционных контейнерах. Для этого закрытые промаркированные пробирки необходимо поместить в полиэтиленовый пакет, плотно запечатать и положить в центре термоконтейнера. Замороженные хладагенты положить на дно вдоль боковых стенок термоконтейнера и накрыть ими образцы сывороток.

8. ПОДГОТОВКА РЕАГЕНТОВ

Примечание: Перед использованием выдержите все компоненты ИФА-набора при комнатной температуре 18-25°С в течение 30 минут!

8.1. Подготовка планшета ИФА

Для предупреждения конденсации воды в лунках открывайте STRIPS только после выдерживания 30 минут при комнатной температуре. Раскройте вакуумную упаковку, отделите необходимое количество лунок, а остальное сразу же тщательно упакуйте с влагопоглотителем и храните плотно закрытыми на замок zip-lock при температуре 2-8°С. Хранение упакованного таким образом планшета обеспечивает его стабильность в течение 6 месяцев·

8.2. Приготовление промывочного раствора

Для приготовления раствора для промывания разведите TWEEN WASH 20x 1:20 (1+19) дистиллированной или деионизированной водой, потом перемешайте. Например, 5 ml концентрата + 95 ml воды, чего достаточно для 8 лунок. При наличии кристаллов в концентрате раствора для промывания прогрейте флакон при температуре 37°С до полного растворения кристаллов (15–20 минут). Разведенный раствор можно хранить при температуре 2-8°С не более 7 суток.

8.3. Приготовление раствора конъюгата

Рабочее разведение конъюгата готовится следующим образом: разведите CONJ 11x (фиолетовый) в чистом флаконе раствором DIL CONJ (розовый) в соотношении 1:11 (то есть, 1+10), раствор окрашивается в фиолетовый цвет. Например, для 8 лунок анализа добавить до 500 µl DIL CONJ 50 µl CONJ 11x. Раствор конъюгата в рабочем разведении стабильный в течение суток при условии хранения при температуре 2-8°С.

9. ПРОЦЕДУРА АНАЛИЗА

9.1. Подготовьте необходимое количество лунок для анализа (четыре лунки для контролей и необходимое количество для исследуемых образцов), вставьте их в рамку планшета ИФА. Лунки с контролями обязательно включайте в каждую постановку анализа.

9.2. Заполните схему внесения образцов.

9.3. Приготовьте раствор для промывания в соответствии с пунктом 8.2.

9.4. Приготовьте раствор конъюгата согласно пункту 8.3.

9.5. Внесите в лунки по 100 µl контролей и исследуемых образцов:
CONTROL + – в лунку А1,
CONTROL - – в лунки В1, С1, D1,
в остальные лунки – исследуемые образцы.

9.6. Внесите в лунки по 50 µl раствора конъюгата поверх контролей и исследуемых образцов. Для предотвращения кросконтаминации образцов внесите раствор конъюгата, не касаясь содержания лунок. Осторожно постукивая по планшету, перемешайте смесь в лунках.

9.7. Заклейте стрипы клейкой пленкой и инкубируйте в течение 120 минут при 37°С и постоянном орбитальном перемешивании содержимого лунок со скоростью 300 об/мин. *Инкубацию образцов с конъюгатом в лунках ИФА-планшета можно проводить в течение 120 минут при температуре 42°С в статическом режиме. Однако при этом может наблюдаться снижение специфичности анализа.*

9.8. По окончании инкубации аккуратно снимите клейкую пленку и промойте лунки пять раз с использованием автоматического промывателя или 8-канальной пипетки следующим образом:
– удалите содержимое лунок в контейнер для жидких отходов;
– наполните лунки стрипов не менее чем по 300 µl раствором для промывания, оставьте не менее, чем на 30 секунд;
– аспирируйте раствор из лунок. Остаточный объем раствора после каждого этапа аспирации должен составлять не больше 5 µl;

– повторите процедуру промывания еще пять раз;
– после последней аспирации избавьтесь от лишней влаги, постукивая планшетом по фильтровальной бумаге.

9.9. Внесите в лунки по 100 µl SOLN|TMB, не касаясь дна и стенок лунок планшета.

9.10. Инкубируйте стрипы в течение 30 минут в темном месте при комнатной температуре 18-25°С. Не используйте клейкую пленку на данном этапе.

9.11. Внесите в лунки стрипов по 100 µl SOLN|STOP для остановки ферментативной реакции, придерживаясь той же последовательности, что и при внесении SOLN|TMB. Во время внесения происходит изменение цвета раствора с голубого на желтый, в лунках с прозрачным раствором незначительно меняется оттенок.

9.12. Измерьте на ридере ОП в каждой лунке при длине волны 450/620-695 nm в течение 5 минут после остановки реакции. До проведения измерения убедитесь в чистоте внешней поверхности дна лунок и отсутствии пузырьков.

Учет результатов анализа можно проводить в одноволновом режиме при длине волны 450 nm, в этом случае оставьте лунку для установления бланка (в такую лунку внесите только SOLN|TMB и SOLN|STOP).

10. УЧЁТ РЕЗУЛЬТАТОВ И ИХ ИНТЕРПРЕТАЦИЯ

10.1. Учет результатов анализа

Рассчитать среднее значение ОП негативного контроля ($\overline{Nc}$) уровень граничного значения (Cut off - CO).

$$\overline{Nc} = (Nc1 + Nc2 + Nc3)/3; \quad CO = \overline{Nc} + 0{,}07$$

10.2. Контроль достоверности результатов анализа

Данные теста считаются достоверными, если они соответствуют следующим требованиям:

CONTROL|+ ОП ≥ 1,5

CONTROL|- ОП ≤ 0,100

CONTROL|- $\overline{Nc} \times 0{,}5 \leq Ncn \leq \overline{Nc} \times 2{,}0$ где Ncn – ОП каждого повтора Nc

Если одно из значений ОП негативного контроля выходит за пределы указанного выше интервала, его отбрасывают и рассчитываю $\overline{Nc}$ по остальным значениям ОП негативного контроля. Если более одного значения ОП негативного контроля не отвечает указанным требованиям, то тест считается некорректным и требует повторного проведения.

10.3. Интерпретация результатов

$OD_{sample} \geq CO$	ПОЛОЖИТЕЛЬНЫЙ	, где OD_{sample} – ОП образца
$OD_{sample} < CO$	ОТРИЦАТЕЛЬНЫЙ**	

* Первоначально положительные образцы должны быть исследованы повторно в двух лунках ИФА-набора «EQUI HBsAg». После повторного тестирования положительными считаются образцы, оптическая плотность которых хотя бы в одном из повторов превышает граничное значение. Если при повторном тестировании оптическая плотность образца в обоих повторах ниже граничного значения, такой образец считать отрицательным.

Результаты для образцов, ОП которых равно граничному значению или находится в пределах ±10%, следует интерпретировать осторожно. Такие образцы должны быть исследованы повторно в двух лунках набора «EQUI HBsAg». Если при повторном тестировании OD_{sample} снова находится в пределах ±10% граничного значения, следует провести отбор и анализ нового образца.

** Образцы со значением оптической плотности ниже граничного значения считаются отрицательными в ИФА-наборе «EQUI HBsAg». Однако результаты в пределах 10% ниже граничного значения следует интерпретировать с осторожностью (рекомендуется повторно исследовать такие образцы в двух лунках набора ИФА).

11. ХАРАКТЕРИСТИКИ ТЕСТА

11.1. Аналитические характеристики

Прецизионность

Воспроизводимость результатов в пределах одной постановки анализа (Intra assay repeatability)

Коэффициент вариации (CV) для двух сывороток с разной концентрацией поверхностного антигена оценивали в 32 повторах на одной серии ИФА-наборов.

№ сыровотки	$ОП_{ср}$	CV, %
2	1,809	3,3
45/15	0,922	3,7

Воспроизводимость результатов между разными постановками анализа (Inter assay reproducibility)

Коэффициент вариации (CV) для двух сывороток с разным уровнем специфических антител оценивали в течение 4 дней в 4 постановках анализа по 8 повторов в каждом анализе.

№ сыровотки	$ОП_{ср}$	CV, %
2	1,827	5,6
45/15	0,936	5,8

Аналитическая чувствительность

Предел чувствительности анализа по обнаружению поверхностного антигена вируса гепатита В определяли на Британском стандартном образце 07/288-010 для HBsAg (Национальный институт биологических стандартов Соединенного королевства, NIBSC) и подтверждали с использованием Третьего Международного Стандарта для HBsAg 12/226 (Third International Standard for HBsAg, производства NIBSC). Предел чувствительности ИФА-набора «EQUI HBsAg» составил 0,05 IU/ml (МЕ/мл).

Аналитическая специфичность

На результат анализа не влияет присутствие в образце билирубина в концентрации до 0,1 mg/ml (172,3 μmol/l), гемоглобина в концентрации до 5 mg/ml и триглицеридов в концентрации до 10 mg/ml (11,3 mmol/ l).

11.2. Диагностические характеристики

Для определения клинической чувствительности и специфичности наборов «EQUI HBsAg» использовали 57 образцов сывороток, полученных от пациентов с диагнозом гепатит В, и 294 образца сывороток клинически здоровых доноров (сероотрицательных по отношению к вирусу гепатита В). Кроме того, были использованы образцы из коммерческих панелей производства «SeraCare Life Sciences» (США). По результатам анализа клиническая чувствительность ИФА-набора составляет 100%, клиническая специфичность – 100%.

Исследование характеристик метода по сравнению с аналогичной коммерческой тест-системой проводилось на целевой группе беременных женщин (171 образец). Для выборки беременных женщин относительная специфичность составляла 100%, процент совпадения – 100%.

Положительная прогностическая ценность (PPV) ИФА-набора «EQUI HBsAg» составляет 100%, отрицательная прогностическая ценность (NPV) – 100%.

12. ОГРАНИЧЕНИЕ АНАЛИЗА

Отрицательный результат в ИФА-наборе «EQUI HBsAg» показывает, что тестируемый образец не содержит HBsAg или его концентрация ниже 0,05 IU/ml (МЕ/мл). Поскольку образец может содержать HBsAg в очень низкой концентрации, отрицательный результат в ИФА-наборе «EQUI HBsAg» не позволяет полностью исключить инфицирование вирусом гепатита В.

Кроме того, в литературных источниках описаны некоторые примеры вирусного гепатита В (острого или хронического), когда в образце обнаруживалась вирусная ДНК при отсутствии HBsAg. В таких случаях полезным будет исследование образца на другие маркеры вирусного гепатита В, выявление ДНК и оценка биохимических показателей сыворотки крови пациента.

Для верификации специфичности реакции каждый положительный результат (согласно критериям интерпретации ИФА-набора «EQUI HBsAg») необходимо подтвердить в нейтрализационном ИФА с использованием комплекта реагентов «EQUI HBsAg Confirmation». Для корректной диагностики гепатита В рекомендуется провести исследование образца на наличие специфических антител классов IgM и IgG к HBcore антигену и антител к HBsAg (например, в ИФА-наборах «EQUI HBcore IgM», «EQUI HBcore IgG» и «EQUI anti-HBs», соответственно).

В целях нивелирования ложноположительных результатов, вызванных наличием в образцах сывороток крови человека антител, специфических к иммуноглобулинам мыши, в ИФА-наборе используется специальный блок-компонент, препятствующий формированию иммунных комплексов с антимышиными антителами (англ. НАМА) на твердой фазе.

13. ТРУДНОСТИ, КОТОРЫЕ МОГУТ ВОЗНИКНУТЬ ПРИ ПРОВЕДЕНИИ ИФА

Высокий фон в лунках всего планшета может возникнуть из-за:

- загрязненного промывателя;
- низкого качества или загрязнения воды;
- использования плохо помытой посуды;
- использования дезинфицирующих средств, содержащих хлор;
- использования загрязненных наконечников;
- увеличения времени инкубации или изменения температурного режима.

Высокий фон в отдельных рядах может быть связан с:

- повторным внесением раствора ТМБ;
- загрязнением конуса автоматической пипетки раствором конъюгата;
- загрязнением одного из каналов промывателя.

Полученное значение ОП положительного контроля ниже установленной границы, если:

- неправильно приготовлен или не внесен один из реагентов (раствор конъюгата или раствор ТМБ);
- сокращено время инкубации на одном из этапов.

Интенсивность окрашивания лунок не соответствует полученной оптической плотности. Это может свидетельствовать о смещенном оптическом луче.

ЛИТЕРАТУРА

1. Mahoney F.J. Update on Diagnosis, Management, and Prevention of Hepatitis B Virus Infection // Clinical Microbiology Review – 1999. – Vol.12, N 2 - P.351–366.
2. Maddrey W.C. Hepatitis B - an important public health issue // Clin. Lab. - 2001. - Vol. 47, N 1-2. - P.51-55.
3. Spradling P.R., Xing J., Williams R. et al. Immunity to Hepatitis B Virus (HBV) Infection Two Decades after Implementation of Universal Infant HBV Vaccination: Association of Detectable Residual Antibodies and Response to a Single HBV Challenge Dose // Clinical and Vaccine Immunology. - 2013. - Vol.20, N 4. - P.559–561.
4. Walsh K., Alexander G.J.M. Update on chronic viral hepatitis // Postgraduate Medical Journal - 2001. - V. 77. - P. 498-505.
5. Возіанова Ж.І. Вірусний гепатит B // Інфекційні та паразитарні хвороби: В 3 т. – К.:»Здоров'я», 2001. т.1. – С.601-614.
6. European Centre for Disease Prevention and Control (ECDC). Systematic review on hepatitis B and C prevalence in the EU/EEA. Stockholm: 2016.
7. CDC Hepatitis B Information // https://www.cdc.gov/hepatitis/hbv/index.htm.
8. World Health Organization (WHO). WHO guidelines on hepatitis B and C testing. Geneva: World Health Organization; 2017 // http://www.who.int/hepatitis/publications/guidelines-hepatitis-c-b-testing/en/
9. Regulation (EU) 2017/746 of the European Parliament and of the Council of 5 April 2017 on *in vitro* diagnostic medical devices and repealing Directive 98/79/EC and Commission Decision 2010/227/EU
10. Закон України «Про відходи» // Відомості Верховної Ради України. - 1998. - №36-37.
11. Наказ МОЗ України №325 від 08.06.2015 «Про затвердження Державних санітарно-протиепідемічних правил і норм щодо поводження з медичними відходами».
12. Постанова КМУ від 02 жовтня 2013р. №754 «Про затвердження технічного регламенту щодо медичних виробів для діагностики in vitro».
13. Hanna Tolonen, Kari Kuulasmaa, Tiina Laatikainen, Hermann Wolf and the European Health Risk Monitoring Project. Recommendation for indicators, international collaboration, protocol and manual of operations for chronic disease risk factor surveys Part 4.Storage and transfer of serum/plasma samples// Finnish National Public Health Institute 2002// https://thl.fi/publications/ehrm/product2/part_iii4.htm
14. Surveillance Guidelines for Measles, Rubella and Congenital Rubella Syndrome in the WHO European Region. Annex 3.Collection, storage and shipment of specimens for laboratory diagnosis and interpretation of results//Geneva: World Health Organization; 2012 Dec.

Производитель

Медицинское изделие для диагностики *in vitro*

Номер по каталогу

Дата изготовления

Использовать до

Код партии

Температурное ограничение

Содержит достаточно для (n-) испытаний

Предостережение, ознакомиться с сопроводительными документами

Ознакомление с инструкцией по применению

Беречь от прямых солнечных лучей

Знак соответствия техническим регламентам

Редакция 8 от 21.09.2021г.

С вопросами и пожеланиями по работе набора обращайтесь к производителю:

ООО «Эквитестлаб»
ул. Большая Васильковская 114, г. Киев, Украина, 03150

проспект Победы 60/2, г. Киев, Украина, 03057
(адрес производства)

тел.: 0 (800)31-89-87, +38 (044)334-89-87,
e-mail: info@equitest.com.ua, www.equitest.com.ua

СХЕМА ПРОВЕДЕНИЯ АНАЛИЗА

Выдержать реагенты 30 min при температуре 18-25°С

Внести по 100 μl контролей и исследуемых образцов в лунки:
A1 – CONTROL | + , B1, C1, D1 – CONTROL | − ,
E1 и в остальные лунки - исследуемые образцы

В лунки стрипов внести по 50 μl приготовленного 1:11 (1+10) раствора конъюгата.
(фиолетовый цвет)

Заклеить стрипы пленкой, инкубировать **120 мин при температуре 37°С** и постоянном орбитальном перемешивании содержимого лунок со скоростью 300 об/мин

Промыть лунки 6 раз приготовленным 1:20 (1+19) промывным раствором TWEEN (300 μl в лунку)

В лунки стрипов внести по 100 μl SOLN | TMB

Инкубировать на протяжении **30 min в темноте при температуре 18-25°С**

В лунки стрипов внести по 100 μl SOLN | STOP
(происходит изменение цвета с голубого на желтый)

УЧЕТ РЕЗУЛЬТАТОВ АНАЛИЗА

$\overline{Nc}$ = (Nc1 + Nc2 + Nc3)/3;

CO = $\overline{Nc}$ + 0,07;

$\overline{Nc}$ - Среднее значение ОП 3-х CONTROL | −

CO - Уровень граничного значения (Cut off)

ИНТЕРПРЕТАЦИЯ РЕЗУЛЬТАТОВ

$OD_{sample} \geq CO$	ПОЛОЖИТЕЛЬНЫЙ
$OD_{sample} < CO$	ОТРИЦАТЕЛЬНЫЙ