
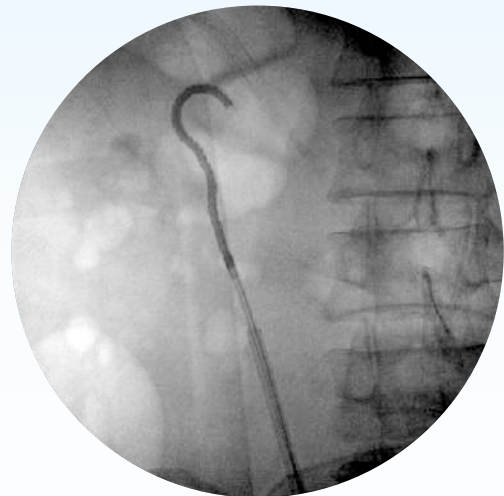


PUSEN[®]

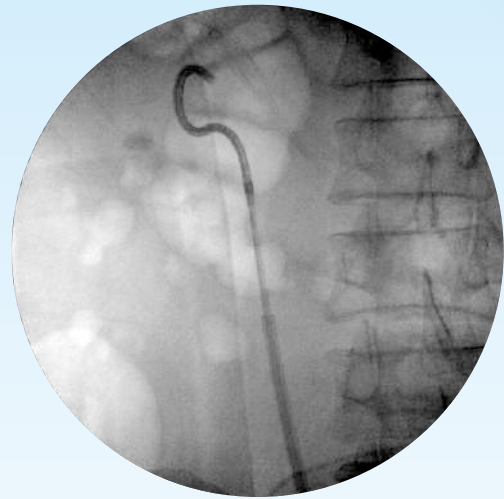

-  No Cross Infection
-  No Sterilization
-  No Maintenance

Uscope PU3022A Specifications

Optical System	
Field of view	90°
Line of vision	0°
Depth of field	3-50 mm
Illumination	Optical fiber
Insertion Portion	
Deflection of distal tip	270° up, 270° down
Nominal width of insertion cord	9.2 Fr
Maximum width of distal tip	9 Fr
Maximum width of insertion portion	9.6 Fr
Working length	650 mm
Channel	
Working channel	3.6 Fr

Eview Specifications

Image Processor PV210	
Max. Resolution	1920 x 1080
Connections	DVI, VGA, SDI, VIDEO
Dimensions	311 mm x 188 mm x 65 mm
Weight	2.3 kg
Image Processor UTV100	
Max. Resolution	1024 x 768
Orientation	Landscape
Display type	12.1" color TFT LCD
Storage capacity	8 GB
Connections	USB, RCA, HDMI
Dimensions	315 mm x 308 mm x 187 mm
Weight	4.3 kg


PUSEN®

Zhuhai Pusen Medical Technology Co., Ltd.
Address: 5/F, Building 1, No 33, Keji San Road, High-tech Zone,
Tangjiawan Town, Zhuhai, Guangdong, PRC.
Tel:0086 400 6882023 Fax:0086 756 6880401
http://www.pusenmedical.com Email:Pusen@pusenmedical.com



Version: A/2 201803
Note: Specifications indicated in the above table
are subject to change without any notice.

PUSEN®

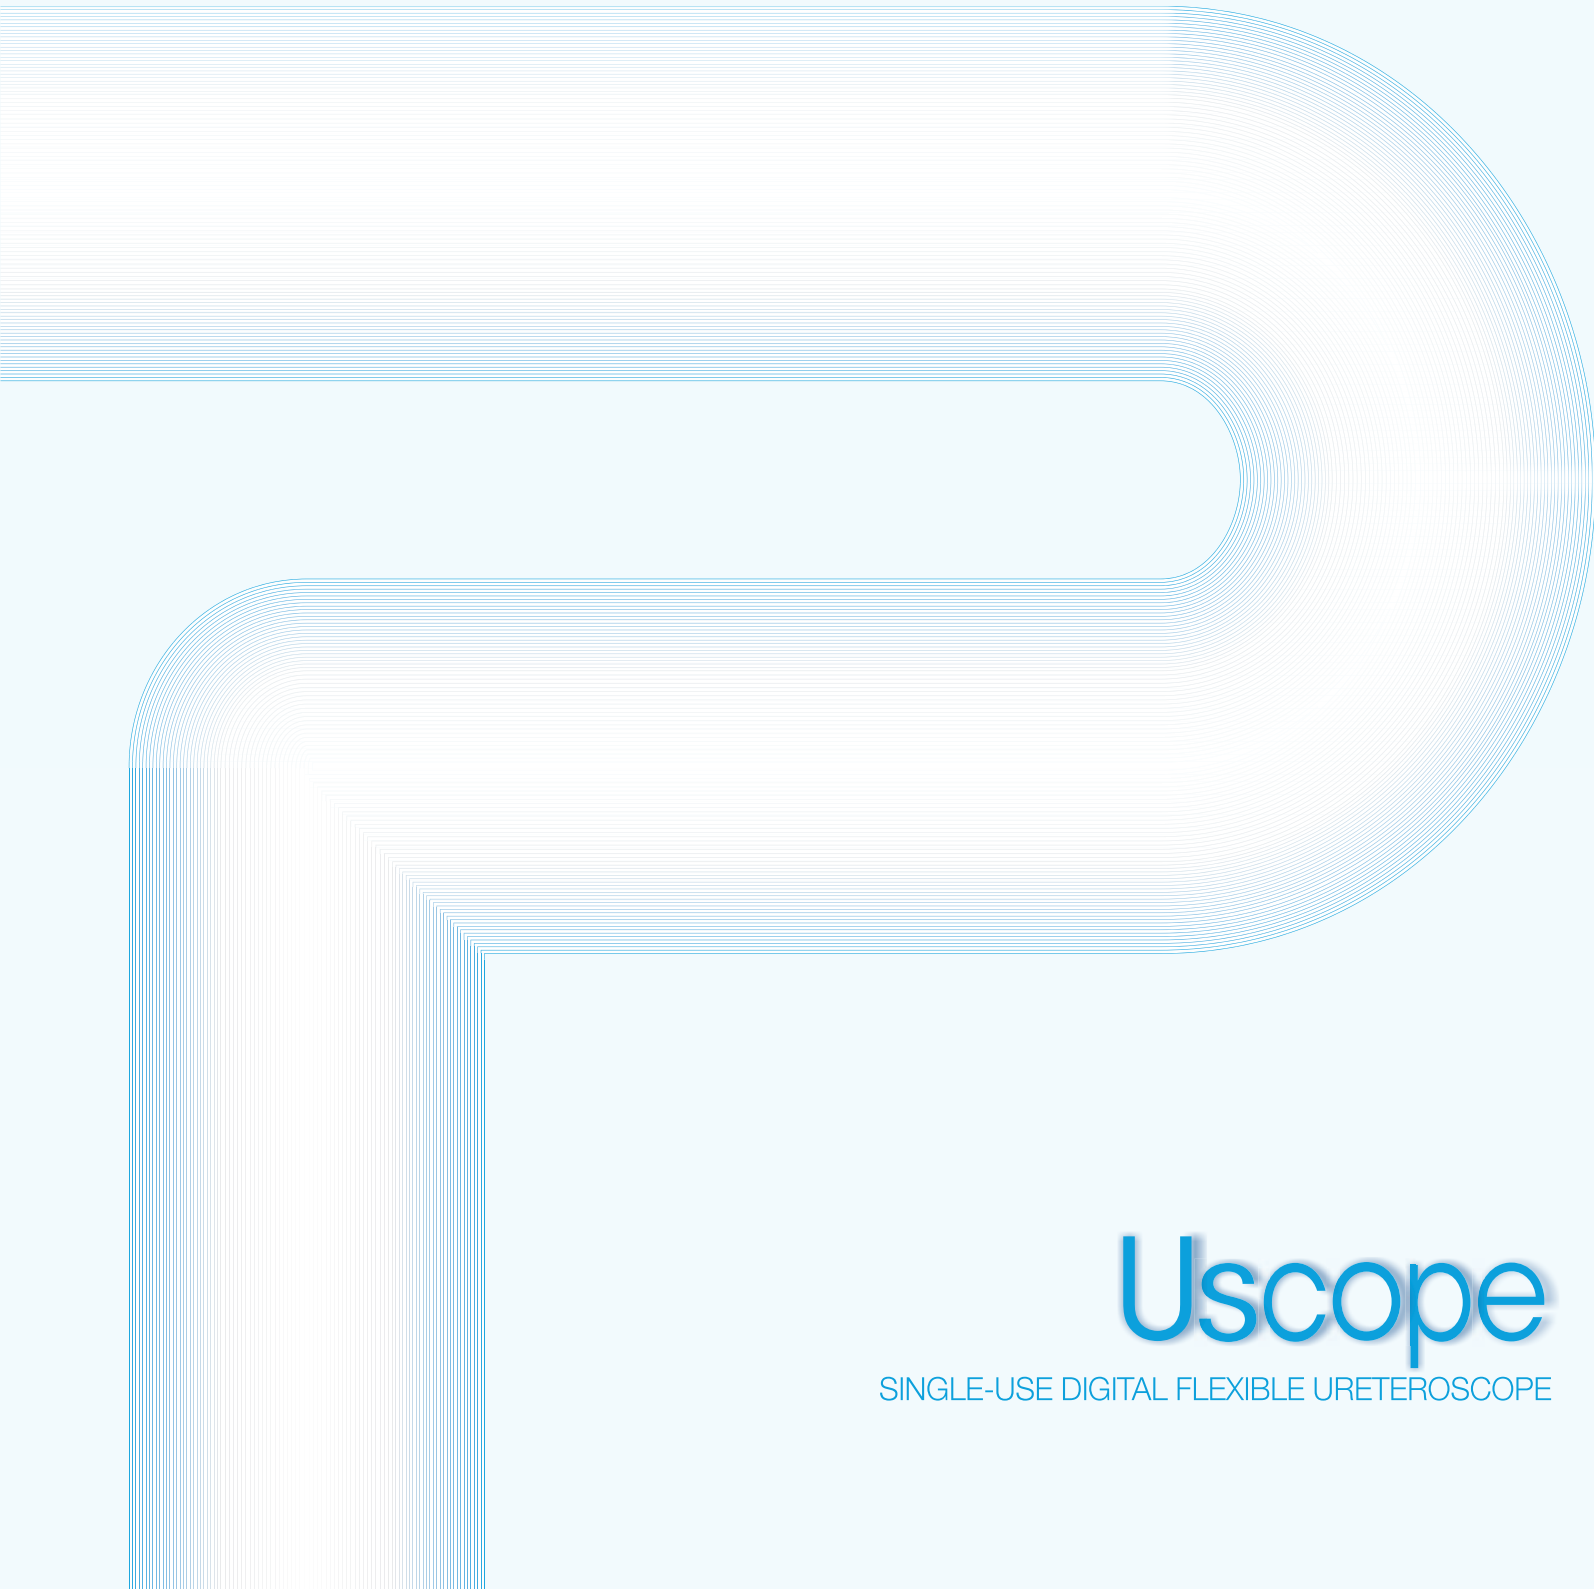

Uscope

SINGLE-USE DIGITAL FLEXIBLE URETEROSCOPE



REGISTRUL DE STAT AL DISPOZITIVELOR MEDICALE

Nr	Denumire	Den.comerc.	Model	Nr. catalog	Tara	Producatorul	Reprezentant	Ordin	Data
						pusen			
DM000236459	PROCESOR PENTRU VIDEOENDOSCOPI		UTV100		China	ZHUHAI PUSEN MEDICAL TECHNOLOGY CO., LTD.	ERICON S.R.L.	Rg04-000210	04-09-2019
DM000236456	VIDEO ENDOSCOPI		PU3021		China	ZHUHAI PUSEN MEDICAL TECHNOLOGY CO., LTD.	ERICON S.R.L.	Rg04-000210	04-09-2019
DM000236460	PROCESOR PENTRU VIDEOENDOSCOPI		PV210		China	ZHUHAI PUSEN MEDICAL TECHNOLOGY CO., LTD.	ERICON S.R.L.	Rg04-000210	04-09-2019
DM000236454	VIDEO ENDOSCOPI		UE3011		China	ZHUHAI PUSEN MEDICAL TECHNOLOGY CO., LTD.	ERICON S.R.L.	Rg04-000210	04-09-2019
DM000236458	VIDEO ENDOSCOPI		PU3022		China	ZHUHAI PUSEN MEDICAL TECHNOLOGY CO., LTD.	ERICON S.R.L.	Rg04-000210	04-09-2019
DM000236457	VIDEO ENDOSCOPI		PU3022A		China	ZHUHAI PUSEN MEDICAL TECHNOLOGY CO., LTD.	ERICON S.R.L.	Rg04-000210	04-09-2019
DM000236455	VIDEO ENDOSCOPI		PU3021A		China	ZHUHAI PUSEN MEDICAL TECHNOLOGY CO., LTD.	ERICON S.R.L.	Rg04-000210	04-09-2019

☒ Содержит ([Producatorul]), 'pusen'.



Benannt durch/Designated by
Zentralstelle der Länder
für Gesundheitsschutz
bei Arzneimitteln und
Medizinprodukten
www.zlg.de
ZLG-BS-244.10.08



Product Service

EC Certificate

Full Quality Assurance System

Directive 93/42/EEC on Medical Devices (MDD), Annex II excluding (4)
(Devices in Class IIa, IIb or III)

No. G1 092464 0013 Rev. 00

Manufacturer:

Zhuhai Pusen Medical Technology Co, Ltd.

5/F, Building 1, No 33, Keji San Road
High-tech Zone, Tangjiawan Town
519085 Zhuhai, Guangdong
PEOPLE'S REPUBLIC OF CHINA

Facility(ies):

Zhuhai Pusen Medical Technology Co., Ltd.

4/F, Building 4, No.20, Jinfengxi Road, High-tech Zone,
Tangjiawan, 519080 Zhuhai, PEOPLE'S REPUBLIC OF CHINA

Zhuhai Pusen Medical Technology Co, Ltd.

5/F, Building 1, No 33, Keji San Road, High-tech Zone,
Tangjiawan Town, 519085 Zhuhai, Guangdong, PEOPLE'S
REPUBLIC OF CHINA

Zhuhai Pusen Medical Technology Co., Ltd.

Changshapu, Cuiheng Village, Nanlang, 528454 Zhongshan,
Guangdong, PEOPLE'S REPUBLIC OF CHINA

Product Category(ies): Medical Video Endoscope

The Certification Body of TÜV SÜD Product Service GmbH declares that the aforementioned manufacturer has implemented a quality assurance system for design, manufacture and final inspection of the respective devices / device categories in accordance with MDD Annex II. This quality assurance system conforms to the requirements of this Directive and is subject to periodical surveillance. For marketing of class III devices an additional Annex II (4) certificate is mandatory. See also notes overleaf.

Report No.:

SH1994301

Valid from:

2019-10-29

Valid until:

2024-05-26

Date,

2019-10-29

Christoph Dicks

Head of Certification/Notified Body



Benannt durch/Designated by
Zentralstelle der Länder
für Gesundheitsschutz
bei Arzneimitteln und
Medizinprodukten
www.zlg.de
ZLG-BS-244.10.08



Product Service

EC Certificate

Full Quality Assurance System

Directive 93/42/EEC on Medical Devices (MDD), Annex II excluding (4)
(Devices in Class IIa, IIb or III)

No. G1 092464 0013 Rev. 00

Manufacturer:

Zhuhai Pusen Medical Technology Co, Ltd.

5/F, Building 1, No 33, Keji San Road
High-tech Zone, Tangjiawan Town
519085 Zhuhai, Guangdong
PEOPLE'S REPUBLIC OF CHINA

Facility(ies):

Zhuhai Pusen Medical Technology Co., Ltd.

4/F, Building 4, No.20, Jinfengxi Road, High-tech Zone,
Tangjiawan, 519080 Zhuhai, PEOPLE'S REPUBLIC OF CHINA

Zhuhai Pusen Medical Technology Co, Ltd.

5/F, Building 1, No 33, Keji San Road, High-tech Zone,
Tangjiawan Town, 519085 Zhuhai, Guangdong, PEOPLE'S
REPUBLIC OF CHINA

Zhuhai Pusen Medical Technology Co., Ltd.

Changshapu, Cuiheng Village, Nanlang, 528454 Zhongshan,
Guangdong, PEOPLE'S REPUBLIC OF CHINA

Product Category(ies): Medical Video Endoscope

The Certification Body of TÜV SÜD Product Service GmbH declares that the aforementioned manufacturer has implemented a quality assurance system for design, manufacture and final inspection of the respective devices / device categories in accordance with MDD Annex II. This quality assurance system conforms to the requirements of this Directive and is subject to periodical surveillance. For marketing of class III devices an additional Annex II (4) certificate is mandatory. See also notes overleaf.

Report No.:

SH1994301

Valid from:

2019-10-29

Valid until:

2024-05-26

Date,

2019-10-29

Christoph Dicks

Head of Certification/Notified Body