

Bodystik

Serial numbers: xx|8|301|yyy and 2301xxxxx



Instructions for Use

Version: 20

Revision: 2

Release date: December 30, 2024

Please read carefully and store in a place which is always accessible for future consultation!

Version: 20
Revision: 2
Release date: December 30, 2024
Filename: BOD_II-2_P22-01_R14
Language: English
Affected serial numbers: xx|8|301|yyy and 2301xxxxx
Software version: valid from 1.2.0
Release:

Managing Director
Geratherm Respiratory GmbH



Geratherm® Respiratory GmbH
Kasernenstraße 4
97688 Bad Kissingen, GERMANY
Tel.: +49 971 7857043-0
Fax: +49 971 7857043-30
info@geratherm-respiratory.com
www.geratherm-respiratory.com

Table of Contents

1	General Information.....	7
1.1	Abbreviations.....	8
1.2	Explanations.....	8
1.3	Symbols	10
1.4	Copyright.....	14
1.5	Limitation of Liability	14
2	Conditions of Use	15
2.1	Intended Purpose.....	15
2.1.1	Indication.....	16
2.1.2	Contraindications and Side Effects.....	17
2.1.2.1	Contraindications.....	17
2.1.2.2	Side Effects	18
2.1.3	Definition of the Groups of People	19
2.2	Intended Use.....	20
2.2.1	Original Spare Parts / Accessories / Optional Expansions	22
2.2.1.1	Original Spare Parts / Accessories.....	23
2.2.1.2	Optional Expansions.....	30
2.2.2	Consumable Items / Auxiliary Materials	32
3	Safety in Handling	34
3.1	General Safety at Work and Personnel Qualification	35
3.2	The Technical State of Bodystik and System Construction.....	36
3.3	Operation / Servicing and Maintenance	38
3.4	Electromagnetic Compatibility (EMC).....	40
3.5	Cleaning and Disinfection	41
4	Structure and General Function of Bodystik	42
4.1	Hardware	42
4.1.1	Overview	42
4.1.2	Operating Elements	43
4.1.2.1	User Panel.....	43
4.1.2.2	Patient Panel	44
4.1.3	Connections / Interfaces of the Bodystik	45
4.1.3.1	Connection Panel.....	45
4.1.3.2	Connectors on the Height-Adjustable Arm	46
4.1.3.3	Sensors.....	46
4.1.3.4	Pressure Reducer (optional with Extension „Diffusion Measurement“) 48	
4.1.4	System Construction and Electrical Safety	49
4.1.4.1	Equipment Cart with Isolating Transformer	51

4.1.4.2	Data Connection	52
4.1.4.3	Power Supply	54
4.2	Technical Protection Measures	55
4.2.1	Emergency Stop	56
4.2.2	Door-Opener Patient Panel	57
4.3	Software	58
5	Transport, Storage and Assembly	59
5.1	Transport to the Location of Use	59
5.2	Storage	59
5.3	Assembly	60
6	Operation	61
6.1	Initial Operating	61
6.2	Recommissioning after Servicing / Cleaning Work	61
6.2.1	Recommissioning after Termination by Patient	63
6.2.2	Recommissioning after Maintenance / Cleaning Work by the Operator	63
6.2.3	Assembly Flow Measuring System	64
6.2.3.1	Assembly Shutter System	68
6.2.3.2	Inserting the Flow Sensor	70
6.2.3.3	Connection Power Supply and PC	71
7	Operating Instructions	73
7.1	Checking for Worn Parts	73
7.2	Switching Bodystik on	74
7.3	Calibrating Bodystik	74
7.4	Setting up the Cabin	75
7.4.1	Height-Adjustable Arm	75
7.4.2	Patient Chair	76
7.5	Using Bodystik / Performing Measurements	77
7.6	Exchange of Disposable Products / Disinfection	80
7.6.1	Bacteria- and Virus Filter / Noseclip	80
7.6.2	Bodystik / Cabin	80
7.7	Switching off Bodystik	81
8	Servicing / Maintenance	82
8.1	Duties of the Responsible Organisation	82
8.2	Servicing / Maintenance by the User / Operator	83
8.2.1	Checking / Exchange of Tubes and Cables	84
8.2.2	Checking / Replacing O-Rings and Sealing Rubbers	85
8.2.3	Care of Door Rubbers	86

9	Cleaning and Disinfection	87
9.1	Single Use	88
9.2	Disinfection.....	88
9.2.1	Flow Unit	91
9.2.2	Ergoflow / Flow Sensor.....	91
9.2.3	Shutter System.....	92
9.2.3.1	Shutter Cage or Shutter Block.....	92
9.2.3.2	Shutter Drive	93
9.2.4	Bodystik / Cabin.....	93
10	Fault Indication and Repair	94
11	Decommissioning / Disposal.....	97
11.1	Expected Service Life	97
11.2	Decommissioning.....	97
11.3	Disposal	97
11.3.1	Transport Packaging	97
11.3.2	Bodystik	97
11.3.3	Patient Chair.....	98
11.3.4	Infectious / Contaminated Single Use Items	98
12	Technical Specifications	99
12.1	Technical Data.....	99
12.2	Installation and Operating Conditions	102
12.3	Electrical Safety Concept.....	103
12.3.1	Bodystik without USB isolator with Medical Device Cart and Isolation Transformer.....	103
12.3.2	Bodystik with USB isolator with Medical Device Cart and Isolation Transformer.....	104
12.3.3	Bodystik with USB isolator, without Medical Device Cart and Isolation Transformer.....	105
12.4	Electromagnetic Compatibility / EMC Guidelines	106
12.4.1	Emitted Interference Guideline and Manufacturer Declaration.....	106
12.4.2	Interference Resistance for all ME Systems Guideline and Manufacturer Declaration	107
12.4.3	Interference Resistance for Non-Life-Supporting ME Systems Guideline and Manufacturer Declaration	108
12.4.4	Recommended Safety Distances for Non-Life-Supporting ME Systems	111
13	Safety of Product and Material.....	112
14	Product Labeling / Type Label	113

15	Warranty and Service	114
15.1	General Conditions.....	114
15.2	Warranty Exemption	114
15.3	Packaging and Shipping.....	115
16	Authorised Specialist Retail Partner	116
Attachment – Declaration of Conformity		117

Foreword

Thank you for purchasing a medical device from Geratherm® Respiratory GmbH. Bodystik is part of our product family with solutions for cardiopulmonary function diagnostics which are operated using the common software platform BLUE CHERRY®. This means that you have the option of optimizing the working processes in your practice using the networked application of further products from Geratherm® Respiratory GmbH, and to benefit from the simple use of our products.

1 General Information

All our medical devices are manufactured and tested in accordance with certified quality standards. This means that Bodystik fulfills the regulatory requirements for medical devices (class IIa).

This IFU is a component of the product in accordance with DIN EN ISO 60601-1. It should make it easier to familiarize yourself with Bodystik, as well as give you instructions about its intended use and safe operation.

This IFU has been written for healthcare professionals who are qualified to perform spirometric examinations.

The basic prerequisite for safe working with the Bodystik is to follow all the safety instructions given.

In addition to the notes in this IFU, the local accident prevention regulations and the national industrial safety regulations apply.

Read this IFU carefully and in its entirety before using Bodystik. For future reference, keep them in the immediate vicinity of the medical device, ready at hand for the user / operator and accessible at all times!

Please refer to the separate IFU of the BLUE CHERRY® software platform for pulmonary function diagnostics.

If, in spite of careful reading of this IFU, you require more information, please contact your specialist retail partner on site. You can obtain the contact details via a form provided by the manufacturer at www.geratherm-respiratory.com/login/.

1.1 Abbreviations

The following simplified style of writing and abbreviations are used hereinafter to make this IFU easier to read.

Instructions for Use	→ IFU
Geratherm® Respiratory GmbH	→ Manufacturer
Medical specialist personnel	→ User(s)
Personnel instructed in cleaning / maintenance work	→ Operator(s)

1.2 Explanations

For the safety of your patients, for your personal safety and to avoid damage to property, observe the meaning of the following explanations of symbols. These are divided into hazard levels. If several severity levels occur at the same time, the warning note for the highest level is always used.

The safety instructions are presented in accordance with DIN ISO 3864 following ANSI Z535.4 (American National Standards Institute).



Indicates a directly hazardous situation.
Not observing and not avoiding the situation will lead to death or severe injuries. The signal word DANGER is only used for extreme situations.



Indicates a possibly hazardous situation.
Not observing and not avoiding the situation may lead to death or severe injuries.



Indicates a possibly hazardous situation.
Not observing and not avoiding the situation may lead to minor or moderate injuries.



Attention

Not observing this warning information may lead to faults or malfunctions of the Bodystik or may indicate that something in its environment may be damaged.



Indicates places in the IFU which are relevant to the current topic but do not present any danger, or which simplify your handling of the Bodystik.

1.3 Symbols

Symbols displayed in this IFU, on the medical device itself and / or on its packaging are standardised symbols.

Symbol	Explanation
	Follow the instructions for use!
	Electronic instructions for use To indicate on product or product packaging that relevant information for use of the product is available in electronic form rather than, or in addition to, printed paper form.
	Applied part from type BF corresponding to DIN EN 60601-1 The applied part is in direct contact with the patient (BF: Body Floating). In order to comply with the limit value for the patient leakage current, the applied part is insulated from earth.
	Device of protection class II (Protective measure against contact) Protection by double or reinforced insulation. To prevent electric shock.
	Only use indoors!
IP20	Protection type (safe environmental conditions) IP2x: Protection of enclosure against ingress of solid foreign objects with a diameter greater than or equal to 12.5 mm and access to hazardous parts with finger. IPx0: No protection of enclosure against harmful ingress of water.

Symbol	Explanation
	Do not dispose of the device along with general household waste! It must be disposed of in a proper and correct manner via the specialist retail partner. By marking a device with this symbol, the manufacturer also declares that he fulfills all the requirements of the law on the distribution, return and environmentally friendly disposal of electrical and electronic devices. (Rechargeable) batteries must be taken to a central collection point for used batteries or to the manufacturer.
	For single use only! This symbol does not refer to the Bodystik itself, but to the consumable items used in connection with it. This is applied to the respective packaging and must be observed.
	Batch number This symbol identifies the batch or lot code given by the manufacturer. The code is placed adjacent to the symbol.
	Serial number This symbol identifies the serial number given by the manufacturer.
	Catalog number This symbol identifies the catalog number given by the manufacturer.
	Medical Device
	Unique Device Identifier (UDI) Unique identifier of the product.

Symbol	Explanation
	GTIN identification Machine-readable number for the type of product assigned by the manufacturer.
	Manufacturer This symbol identifies the manufacturer of a product.
	Date of manufacture This symbol indicates the date on which a product is manufactured.
	Conformity mark This symbol indicates conformity with health, safety and environmental protection standards for products sold within the European Economic Area (EEA). The additional four-digit number identifies the Notified Body involved in the conformity evaluation procedure of this product. In this case 0494 identifies SLG Prüf- und Zertifizierungs GmbH as Notified Body.
	Caution, non-ionizing electromagnetic radiation Precautions must be taken to avoid an unexpected effect of non-ionizing radiation.
	General warning sign Warning of a hazardous location.
	Fragile, handle with care The package contains a product that must be handled with appropriate care to prevent damage during transport and storage.

Symbol	Explanation
	Keep away from rain The package contains a product that must be protected from moisture during transport and storage.
	Temperature limitation The product can be safely transported, stored or operated within the specified temperature range.
	Humidity limitation The product can be safely transported, stored or operated within the specified humidity range.
	Atmospheric pressure limitation The product can be safely transported, stored or operated within the permissible atmospheric pressure.
	Package The symbol indicates the identifier of the package and the total number of packages.

1.4 Copyright

The manufacturer reserves all rights to this document and the information contained therein. No part of this document or the information contained herein may be reproduced or transmitted without the written consent of the manufacturer. All information or brand names of a third party contained in this document are subject to the copyright of that third party.

1.5 Limitation of Liability

The manufacturer emphasises the creation of accompanying documents for his products. Despite careful checking, errors or inaccuracies in this document version cannot be completely ruled out. The liability of the manufacturer for direct or indirect damages arising in connection with the present documentation is excluded to the extent permitted by law. Technical or content information in this document is subject to change at any time and without notice. Should any questions arise, please contact your authorised specialist retailer or the manufacturer directly.

2 Conditions of Use

Any other use of Bodystik which is not described in this IFU is deemed improper use. The responsible organisation of Bodystik alone is liable for any direct or indirect damage resulting from not adhering to these conditions. They are then solely responsible for the fulfillment of the basic requirements of the medical device and assumes complete product liability for the whole system.

2.1 Intended Purpose

The Bodystik is a medical electrical device. As a PC connected bodyplethysmograph, it is mainly intended to determine lung volumes and airway resistance in lung function diagnostics in the clinical sector and by general practitioners.

Bodystik is designed for use in the mouth, nose, upper throat area, trachea and lungs of the patient (definition see chap 2.1.3 “Definition of the Groups of People”).

The standard version of the software allows the measurements spirometry, flow / volume, TGV, airway resistance and pre / post examinations and trend analysis.

Using Bodystik, you can also carry out the examination stated below.

Examination	Required option
CO Diffusion	Add-on CO Diffusion (REF 259149)
MIP / MEP	MIP / MEP (REF 250798)
P0.1	MIP / MEP (REF 250798)
Breathing Pattern Analysis	MIP / MEP (REF 250798)
Rint	Rint (REF 868750)



You can find more information in:

- IFU Spirometry and Bodyplethysmography for carrying out the examination.
- IFU BLUE CHERRY® for the general operation of the software and carrying out the examination.

2.1.1 Indication

With the Bodystik bodyplethysmographic examinations can be performed for diagnosis, follow-up, screening and severity assessment of pulmonary diseases. In particular, this includes:

Obstructive diseases

- Complaints such as dyspnea (shortness of breath) or coughing when at rest as well as under stress
- Bronchial asthma
- Chronic obstructive pulmonary disease (COPD)
- Pulmonary emphysema

Restrictive diseases

- Interstitial lung diseases
- Pulmonary fibrosis
- Impairments of the chest
- Neuromuscular diseases

Allergy diagnosis

2.1.2 Contraindications and Side Effects

2.1.2.1 Contraindications

The following contraindications apply for body-plethysmographic examinations:

Contraindications

Due to increases in myocardial demand or changes in blood pressure

- Acute myocardial infarction within 1 week
- Systemic hypotension or severe hypertension
- Significant atrial / ventricular arrhythmia
- Noncompensated heart failure
- Uncontrolled pulmonary hypertension
- Acute cor pulmonale
- Clinically unstable pulmonary embolism
- History of syncope related to forced expiration / cough

Due to increases in intracranial / intraocular pressure

- Cerebral aneurysm
- Brain surgery within 4 weeks
- Recent concussion with continuing symptoms
- Eye surgery within 1 week

Due to increases in sinus and middle ear pressures

- Sinus surgery or middle ear surgery or infection within 1 week

Due to increases in intrathoracic and intraabdominal pressure

- Presence of pneumothorax
- Thoracic surgery within 4 weeks
- Abdominal surgery within 4 weeks
- Late-term pregnancy

Infection control issues

- Active or suspected transmissible respiratory or systemic infection, including tuberculosis
- Physical conditions predisposing to transmission of infections, such as hemoptysis,
- significant secretions, or oral lesions or oral bleeding



Spirometry should be discontinued if the patient experiences pain during the maneuver. Relative contraindications do not preclude spirometry but should be considered when ordering spirometry. The decision to conduct spirometry is determined by the ordering healthcare professional on the basis of their evaluation of the risks and benefits of spirometry for the particular patient. Potential contraindications should be included in the request form for spirometry.

(Source: Graham, B. L. et al. 2019. Standardization of Spirometry 2019 Update. Am J Respir Crit Care Med Vol 200, Iss 8, pp e70–e88.)

2.1.2.2 Side Effects

If there are no contraindications and the examination is carried out in accordance with the descriptions in this IFU, side effects rarely occur in pulmonary function examinations. These can be described as follows:

Side effect / Frequency	Rules of conduct
Dizziness, syncope / on a case-by-case basis	Examinations should preferably be performed in a sitting position and the patient should be permanently observed during the examination
Spontaneous pneumomediastinum, pneumopericardium and subcutaneous emphysema in spirometry / in extremely rare cases	Investigate any persistent dyspnea that occurs after the examination

2.1.3 Definition of the Groups of People

Groups of people named in this IFU are defined as follows:

Manufacturer

specifies all measures to ensure the safe and proper handling and application of Bodystik. They are responsible for instructing the users in relation to this via the corresponding specialist retail partner.

Responsible Organisation

is any natural or legal person who is responsible for the operation of the health institution where Bodystik is used by their employees (users / operators).

User

is a medically trained specialist who is familiar with spirometry examinations, who uses Bodystik on the patient after verifiable instruction by the responsible organisation and / or is responsible for rectifying faults to the Bodystik, as well as its calibration.

Users must be aware of the clinical meaning and, for example, be a physician, physician's assistant, assistant or trained maintenance personnel with basic electrical or mechanical training. The user is able to identify, assess and, in the best case, to avoid possible hazards when using Bodystik. Trainee medical specialists must also be supervised in addition to receiving training in how to use Bodystik.

Operator

is a person who has received instruction on cleaning Bodystik by a medically trained specialist.

Patient

is a person undergoing medical treatment (check-up, initial diagnosis as well as progress / treatment monitoring) to assess their pulmonary function. The persons can be adults without an age limitation as well as children from 4 years of age. A requirement for carrying out the examination is the ability to follow the instructions of the user.

2.2 Intended Use

Bodystik can be operated independently as a non-stationary device or in combination with all other Geratherm® Respiratory GmbH products via the universal software BLUE CHERRY®. (See chap. 4.1.4 "System Construction and Electrical Safety")



Attention

The following applies to Bodystik systems before February 2023 (up to serial number 230100528): The Bodystik must only be operated with the Geratherm Respiratory approved equipment cart (REF 509409). The equipment cart provides galvanic isolation from the power supply network. All necessary peripheral devices such as computer, printer and monitor may only be connected to the power supply network via the equipment cart (see also chap. 4.1.4 "System Construction and Electrical Safety"). If you have any questions, please contact your local specialist retail partner.

In all cases, the Bodystik is only intended for use in closed, pleasantly temperature-controlled (19 °C – 25 °C) rooms in a clinical area.

In the respective room, there must be neither flammable or explosive gases, nor magnetic fields (e.g. MRI).

In combination with the "Add-on CO Diffusion" extension, the room must always be well ventilated, to protect users / operators and third parties from continuous exposure to harmful carbon monoxide (CO).

The following applies in general: The installation of Bodystik is only deemed safe and in line with intended use when this is carried out in accordance with the details in chap. 12.2 "Installation and Operating Conditions".

The responsible organisation must ensure that only medically trained specialist personnel (see chap. 2.1.3 "Definition of the Groups of People") operates Bodystik. Personnel must demonstrably have been given training in the function of Bodystik. This also includes a complete study of this IFU.

The manufacturer has determined the expected service life (see chap. 11.1 "Expected Service Life") and the maintenance work required for this (see chap. 8 "Servicing / Maintenance").

The Bodystik may only be used for the duration of its service life if the specifications are observed.

Any changes to Bodystik, in particular unauthorised modifications, are prohibited.

The Bodystik is not intended for the control of vital physiological parameters where the nature of the change could lead to immediate danger to the patient, e.g. changes in heart function, respiration or central nervous system activity.

Any other than the described use is deemed improper use.

The responsible organisation of Bodystik alone is liable for any damage resulting from not adhering to these conditions.

Intended use also includes complying with all further information and instructions in this IFU, without exception.



Attention

Electromagnetic compatibility (EMC) in accordance with DIN EN 60601-1-2:2016-05; VDE 0750-1-2:2016-05; IEC 60601-1-2:2014. See chap.12.4 “Electromagnetic Compatibility / EMC Guidelines”. Bodystik is suitable for use in all institutions including those in residential areas and those which are directly connected to the public supply network which also supplies buildings used for residential purposes.

2.2.1 Original Spare Parts / Accessories / Optional Expansions

Intended use also includes using prescribed original spare parts, accessories and expansions in constructing the system.

Only the components stated in the following are deemed tested and approved, as products by the manufacturer of Bodystik.

The installation or use of other products can, under certain circumstances, negatively change constructive prescribed properties of Bodystik and, in the worst case, impair the safety of the patient, user / operator and / or third parties.

The manufacturer assumes no liability for such consequences. All warranty claims shall expire.

See also chap. 15.2 “Warranty Exemption”



Possible danger to life.

Reason: **Cross contamination.** Therefore:

- Do not use consumable articles with a limited life span after their use-by date has expired!



Possible physical injury.

Reason: **Device damage as well as impurities / contamination due to improper handling of components.** Therefore:

- Protect separately stored components, accessories and consumable materials from unauthorised access!
- Observe the storage conditions stipulated by the manufacturer!

2.2.1.1 Original Spare Parts / Accessories

The following components can be purchased via specialist retail partners.



You will find:

- A list of specialist retail partners as an insert in this IFU or in your medical device book, as well as the most updated version at www.geratherm-respiratory.com/login/
- Instructions on safe system construction in chap. 4.1.3 of this IFU

Component	Description / name	Supply scope in units	REF
	Bodystik ➤ Comfortable USB 2.0 Bodyplethysmograph with 5 glass sides, electro-magnetic door-lock, electronic height-adjustment for arm, communication system, low doorstep and swing-out-chair. Includes flow unit, Shutter System and ambient module for continuous BTPS compensation. ➤ Measures SVC, FVC, MVV, Resistance and TGV. Comes together with intuitive Windows based diagnostic software platform BLUE CHERRY®.	01	785155 [old:40.600]
	BLUE CHERRY® Media Pack ➤ Modular and intuitive Windows based diagnostic software platform for pulmonary function	01	598197 [old:10.500]

Component	Description / name	Supply scope in units	REF
	Ergoflow ➤ Re-useable lightweight flow sensor for use with Ergostik, PFTstik, Bodystik and Diffustik device.	01	139094 [old:10.600]
	Flow Unit ➤ Flow unit for PFTstik, Bodystik and Diffustik. ➤ Including flow electronic and rubber seal plates.	01	983244 [old:40.630]
	Shutter Drive ➤ Electromagnetic shutter drive for shutter system.	01	122919 [old:40.610]
	Shutter Block ➤ Shutter block for shutter system for fast occlusion of breathing path. ➤ For connection of shutter system with flow unit (see also shutter plug) or demand valve with flow unit. <i>Replaces shutter head (40.612) or shutter head CO (40.613) and shutter cage (40.611). Can be retrofitted for all systems.</i>	01* from 11 / 2018	198961 [old:40.620]
	Shutter Plug ➤ Plug to close opening for demand valve in shutter block if device is used without Add-on CO Diffusion. <i>Can be retrofitted for all systems</i>	01* from 11 / 2018	347975 [old:40.622]

Component	Description / name	Supply scope in units	REF
	Shutter Cage ➤ For fast occlusion of breathing path. <i>Replaced by shutter block (40.620).</i>	01* until 11 / 2018	40.611
	Shutter Head ➤ For connection of shutter system with flow unit without Add-on CO Diffusion (demand valve). <i>Replaced by shutter block (40.620).</i>	01* until 11 / 2018 without Add-on CO Diffusion	40.612
	Shutter Head CO ➤ For connecting shutter system with flow unit with Add-on CO Diffusion (demand valve). <i>Replaced by shutter block (40.620).</i>	01* until 11 / 2018 with Add-on CO Diffusion	40.613
	Mounting Plate ➤ Mounting plate to fix the shutter system on the Height Adjustable Arm.	01	700178 [old:40.702-07]
	Softclip ➤ Disposable noseclip for lung function tests ➤ Made of soft, skin-friendly foam for best wearing comfort ➤ One size 	03	787158 [old:10.200]

Component	Description / name	Supply scope in units	REF
	Neumofilt ➤ Single use disposable bacterial and viral filter for use in pulmonary function testing 	03	199479 [old:10.003]
	Medical Power Supply, 24 V ➤ Medical grade 24 V power supply. ➤ Recognisable by the manufacturer "Bicker" and the model name "BET-1024M"). ➤ 1.8 m connection cable. <i>Replaces power supply unit, 24 V. Can be retrofitted to all systems.</i>	01*from 08 / 2015	290495 [old:10.842]
	Power Supply, 24 V ➤ 24 V power supply ➤ Recognisable by the manufacturer „Deutronic“ and the model name „ETC70G-24“). <i>Replaced by medical power supply, 24 V (290495).</i>	01*until 08 / 2015	---

Component	Description / name	Supply scope in units	REF
	Power Cord, CEE 7 / 16, C7 (IEC 60320, EU) ➤ Power Cord with European plug for use with Power Supply (12 V) and Power Supply (24 V) ➤ For connecting the Power Supply unit (10.842) to a socket. <i>Replaces power cables (10.838-1). Can be retrofitted to all systems.</i>	01* <i>from</i> 08 / 2015	142297 [old:10.838]
	Power Cord, CEE 7 / 7, C13 (IEC 60320, EU) ➤ Power cable (2 m) with European plug (earth contact). ➤ For connecting the power supply unit to a three-pole socket. <i>Replaced by power supply cable (40.620).</i>	01*until 08 / 2015	719626 [old:10.838-1]
	USB Isolator ➤ USB connection cable (male A and male B) for connecting USB-based devices to the PC (galvanic 4 KV AC isolation between Bodystik and PC). ➤ Length: 3 m ➤ Replaces USB connection cable (10.820-1). Retrofittable for all systems.	01* / --- * <i>from</i> 02/2023	565942 [old:10.820-01]

Component	Description / name	Supply scope in units	REF
	USB connection cable ➤ USB connection cable (male A and male B) for connecting USB-based devices to the PC. ➤ Length: 1.8 m	--- / 01* <i>*until 02/2023</i>	362803 [old:10.820]
	Silicon Adapter, Small ➤ Silicon adapter size small used for Ergoflow to connect to calibration syringe.	10	919774 [old:10.831]
	O-Ring Set, Shutter Head ➤ 2 x 23 x 2 mm for shutter head (outside).	01* <i>from 11 / 2018</i>	40.623
	O-Ring, Demand Valve ➤ O-Ring 1 x 26 x 3 mm for demand valve.	01* <i>from 11 / 2018</i>	457033 [old:40.617]
	O-Ring Set, Shutter Head ➤ O-Ring Set 2 x 23 x 2 mm and 2 x 30 x 2 mm for Shutter Head and Shutter Head CO.	01* <i>until 11 / 2018</i>	952017 [old:40.616]
	Rubber Seal, Flow Unit ➤ 2 Rubber seal plates for flow unit.	01	885146 [old: 40.630-05]
	Pressure Regulator GM, Diffusion Gas ➤ For bottle with connector DIN 477-1, 1990 Nr. 14 (External thread, Left-hand thread, M 19 x 1.5)	normally not included but recommended!	392281 [old: 659623]

Component	Description / name	Supply scope in units	REF
	Pressure Regulator GM, Diffusion Gas ➤ For bottle with connector DIN477-1, 1990 No. 1 (External thread, Left-hand thread, W 21.80 x 1/14")	normally not included but recommended!	224718 [old: 781429]
	PFT Cart Consisting of ➤ Cart for PFT systems consisting of base frame, ➤ Drawer block, ➤ 1 Storage shelf, ➤ 1 Monitor holder, ➤ 10 liter gas bottle holder and 1 Universal bottom storage shelf. ➤ Includes safety transformer and multiple sockets. Mandatory (See also chap. 4.1.4 "System Construction and Electrical Safety").	---	509409 [old:10.905]

2.2.1.2 Optional Expansions

The following add-ons can be purchased via specialist retail partners.



You will find:

List of specialist retail partners as an insert in this IFU or in your medical device book, as well as the most updated version at www.geratherm-respiratory.com/login/
Instructions on safe system construction in chap. 4.1.4 of this IFU

Component	Description / name	REF
	Add-on CO Diffusion ➤ Single breath CO Diffusion option adds TLco measurement to Bodystik or PFTstik. Includes: ➤ Fast NDIR CO / CH₄ Analyzer (CO: 0 – 3000 ppm, CH₄: 0 – 3000 ppm), ➤ Demand Valve ➤ Connection Tubes / Cable.	259149 [old:40.702]
	Pressure Regulator GM, Diffusion Gas ➤ For bottle with connector DIN 477-1, 1990 Nr. 14 (External thread, Left-hand thread, M 19 x 1.5)	392281 [old: 659623]
	Pressure Regulator GM, Diffusion Gas ➤ For bottle with connector DIN477-1, 1990 No. 1 (External thread, Left-hand thread, W 21.80 x 1/14")	224718 [old: 781429]

Component	Description / name	REF
	Pressure Regulator, Diffusion No longer available ➤ Pressure Regulator for CO Diffusion measurement gas mixture (Providing a fixed pressure of 5 bar, connector DIN 477-1:1990 No. 14.) ➤ According to ISO 10524-1 (See also chap. 4.1.3 "Connections / Interfaces of the Bodystik" \ 4.1.3.4)	659623 [old:10.822]
	Calibration Syringe ➤ Precision calibration instrument for calibration of flow or volume-based systems. ➤ 3 liter volume (nonadjustable). ➤ Comes together with adapter for Spiraflow and Ergoflow.	608220 [old:10.801]
	MIP / MEP ➤ Software option for BLUE CHERRY® to add measurement of ○ max. inspiratory pressure (MIP), ○ max. expiratory pressure (MEP) ○ and P0.1.	250798 [old:10.525]
	Rint ➤ Software option for BLUE CHERRY® to add measurement of airway resistance by occlusion (Rint or Rocc).	868750 [old:10.526]

2.2.2 Consumable Items / Auxiliary Materials

The following items were tested by the manufacturer for Bodystik.
The use of other consumable items as well as auxiliary materials with different properties is deemed improper use.



You will find a list of specialist retail partners as an insert in this IFU or in your medical device book, as well as the most updated version at www.geratherm-respiratory.com/login/

Component	Description / name	REF
	Softclip ➤ Disposable noseclip for lung function tests ➤ Made of soft, skin-friendly foam for best wearing comfort ➤ One size	 787158 [old:10.200]
	Neumofilt ➤ Single use disposable Bacterial and Viral Filter for use in pulmonary function testing.	 199479 [old:10.003]

Component	Description / name	REF
Disinfectant	For wipe disinfection , alcoholic quick-acting ➤ Bacillol Tissues (BODE Chemie GmbH) ➤ SprayIn (Dr. Deppe GmbH)	depend- ing on provider
	For disinfection bath with low chloride concentration ➤ InstruPlus (Dr. Deppe GmbH) ➤ Bomix Plus (BODE Chemie GmbH) ➤ Gigasept Pearls (Schülke & Mayr GmbH)	
Technical vaseline	For rubber care of the door seal ➤ Free from fragrances and dyes. ➤ Suitable for lubrication of components.	

3 Safety in Handling

Bodystik has been designed and built in accordance with the state of technology and its recognised safety and technical regulations.

In spite of this, dangers of injury to users / operators, patients and third parties as well as damage to Bodystik or other materials may occur if this is:

- Not used in accordance with the conditions of intended use.
- Not operated in a technically flawless state.
- Operated by untrained or uninstructed personnel.
- Maintained or serviced improperly.



DANGER

In order for Bodystik or the complete system to be operated in accordance with its intended use, the safety information and procedures in this IFU must be understood.

Ensure that these are followed!

Otherwise, in the worst case, death or severe injuries are the consequence resulting from the risks described in more detail in the respective chapters!
Therefore:

- Read this IFU carefully and in its entirety before using the Bodystik. Keep it in close proximity to the medical device for later reference and make it accessible to the user / operator at all times!
- Also observe the safety information of all other accompanying documents of the complete system!
- If you have any questions, ask your authorised specialist retail partner!

3.1 General Safety at Work and Personnel Qualification



Possible danger to life.

Reason: Not complying with health and safety regulations. Ignoring essential preventive measures.

Therefore:

- Always comply with general national regulations on accident prevention! Instruct users / operators accordingly!
- Safety and warning information on Bodystik may not be altered or removed! Have missing or not readable information replaced immediately!
- When working with auxiliary materials, always observe the safety information from the respective manufacturer! Wear suitable protective clothing!

Reason: Electric shock. False diagnosis. Ignoring contraindications. Triggering malfunctions of Bodystik. Unqualified user / operator can detect sources of failures too late or even cause them. Therefore:

- Only use officially trained users!
- Users must be familiar with the test methods and their clinical significance!
- All maintenance and servicing work may only be performed by specialised personnel who have been authorised by the manufacturer!

3.2 The Technical State of Bodystik and System Construction



Possible danger to life.

Reason: Electrical shock. Cross-contamination or misdiagnosis. For this: **Only use Bodystik within its performance limits!** Therefore:

- Do not overstress Bodystik Use with care!
- Do not modify or use product Bodystik or complete system contrary to the respective manufacturer's specification!
- Only use Bodystik within its expected service life, determined by the manufacturer!
- Under no circumstances use or connect any devices, systems, equipment and other products that are not part of the complete system!
- Never obstruct the access to the mains plug or On / Off switch of the equipment cart!
Disconnection of the power supply must be easily accessible!
- Only use accessories and consumables which are authorised by the manufacturer as well as authorised replacement components, add-ons and auxiliary materials.
Check that the components are in a functional and safe condition!
- Ensure that in the patient environment – a distance of 1.5 meters to the patient – there are no accessible electrical parts (interfaces, plugs, etc.) that are not isolated from the mains with an isolation voltage of 4 kV!

- Ensure that the users or third party persons do not touch the patient and any conductive connections or parts of the device that are located outside the patient environment at the same time!

Reason: Electric shock and / or misdiagnosis due to loss of electrical safety caused by exceeding the recommended maintenance schedule Therefore:

- Regularly check the specified maintenance schedule!
- If a maintenance schedule is exceeded, do not continue to use the complete system!
- Request maintenance work from your authorised specialist retail partner!
- The device may only be operated in conjunction with the equipment cart (ergoline ergocar PC) offered by manufacturer!

Reason: Electric shock. Lack of galvanic isolation when assembling non-approved components. Therefore:

The followings applies to systems without integrated galvanic isolation (24 V Power Supply or USB Extension Cable, see chap. 4.1.4.2 "Data Connection" and chap. 4.1.4.3 "Power Supply"):

- These devices may only be operated in conjunction with the equipment cart (ergoline ergocar PC) offered by manufacturer!

3.3 Operation / Servicing and Maintenance



DANGER

Danger to life.

Reason: Electric shock. Carbon monoxide (CO) intoxication. Explosion. Device damage. Unpredictable movement of metal parts.

For this: **Comply with the required installation and operating conditions!** Therefore:

- In principle, observe chap. 12 "Technical Specifications"!
- When using the optional diffusion measurement, note the separate IFU "Add-on CO Diffusion"!
- Do not operate Boystik if there are flammable or explosive gases in the room!
- Do not operate Bodystik near the magnetic field of an MRT system!



WARNING

Possible danger to life.

Reason: Electric shock. Cross-contamination.

Misdiagnosis caused by measurement error. Device damage. For this: **Ensure that the used components are undamaged and that you are working in a careful way!** Therefore:

- Do not use consumable items with a limited expected service life after their use-by date has been reached!
- Do not use single use products more than once!
- Prior to each use, visually inspect the complete system (housing, cables, connectors, tubings, pneumatic connections, etc.) for any damages!
- If there are any damages, do not operate the system. The damaged parts must be replaced or repaired properly!
- Calibrate Bodystik at the intervals stated!

Reason: Disregard of a contraindication. Misdiagnosis caused by measurement error. Cross-contamination.
For this: Observe the general medical principles!
Therefore:

- Inform yourself and observe the respective contraindications before each test!
- When carrying out tests, observe the content of the applicable guidelines and recommendations (e.g. ATS / ERS Guidelines)!

Reason: Collapse of the patient due to claustrophobia.
For this: Observe general medical principles! Therefore:

- Before examination, inform the patient about the emergency opening of the door!
- Do not leave the patient unattended in the cabin!

Possible severe physical injury.

Reason: Bodystik can tilt over. Therefore:

- Observe the maximum weight of the person on the chair when chair is swivelled outwards. It is 125 kg!



CAUTION

Possible physical injury

Reason: Skin burn caused by short-circuit inside the device. Therefore:

- Do not touch shutter drive in case of excessive heat!

3.4 Electromagnetic Compatibility (EMC)



WARNING

Possible danger to life.

Reason: Misdiagnosis due to measurement error caused by a system failure due to uncontrollable electromagnetic fields of inadmissible transmitting devices. Therefore:

- While using Bodystik, do not use any transmitting devices (e.g. mobile phones, portable phones, power lines ...) within close proximity (< 30 cm) that exceed the immunity levels as specified in the EMC guidelines!
- Ask your authorised specialist retail partner about this!

Reason: Misdiagnosis caused by uncontrollable electromagnetic fields. Triggering malfunctions. Device damage due to improper handling of components. Therefore:

- No stacking of devices on top of each other and no close arrangement. Observe the installation and operating conditions from the manufacturer!
- Check the correct function of the Bodystik!

3.5 Cleaning and Disinfection



WARNING

Possible danger to life.

Reason: **Cross-contamination.** For this: **Observe the general medical principles!** Therefore:

- Clean and disinfect the Bodystik and its reusable components as instructed by the manufacturer at regular intervals as specified!

Possible severe physical injury.

Reason: **Contamination with transferable germs during improper disposal.** Therefore:

- Dispose single use items (disposable flow sensors, mouthpieces and noseclips) after each use. For this observe the applicable regulatory requirements for biologically hazardous materials!
- Observe regulations on wearing personal protective equipment (PPE)!



CAUTION

Possible physical injury.

Reason: **misinterpretation of obvious measuring errors (drift) caused by liquid in the tubes.** Therefore:

- Clean tubes only externally!
- Replace dirty tubes!



Attention

Bodystik could be damaged.

Reason: **Penetrating liquids into electronic components.** Therefore:

- Disconnect the Bodystik from the power supply before cleaning and disinfecting! (When switching off via the On / Off switch of the equipment cart), shut down the PC completely before doing so!
- Wipe off remaining moisture with a dry cloth!

4 Structure and General Function of Bodystik

4.1 Hardware

4.1.1 Overview




- [1] Pressure-stable aluminium cabin with all-sided glass and integrated electronics
- [2] Door with electromagnetic lock (see also chap. 4.2.2)
- [3] Height-adjustable and pivoting patient chair (see also chap. 7.4.2)
- [4] Adjustable feet for a secure stand
- [5] Magnets (top and bottom) for secure door locking (see also [2])
- [6] User Panel incl. **EMERGENCY STOP** (see also chap. 4.1.2.1 and 4.2.1)
- [7] Electrically height-adjustable stand for mounting the flow system (see also chap. 7.4.1)
- [8] Patient panel on the inside of the cabin with loudspeaker and door opener (see also chap. 4.1.2.2 and chap. 4.2.2)
- [9] Type label (see also chap. 14)
- [10] Connection panel for Bodystik (see also chap. 4.1.3.1)

4.1.2 Operating Elements

4.1.2.1 User Panel



User panel on the front right-hand side of the cabin

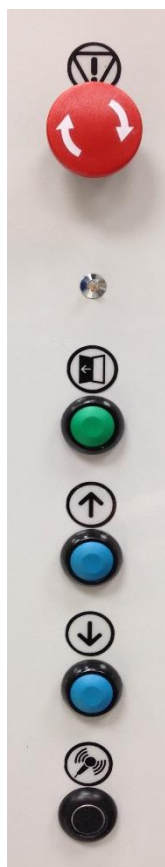

1

EMERGENCY OFF button

To disconnect the cabin from the power Supply in case of emergency (see also chap. 4.2.1)

2

LED for door status

To indicate the door status
Door open = LED OFF
Door closed = LED GREEN

3

Door opener

To open the cabin door

4

Button stand up

For electrical height adjustment

5

Button stand down

6

Microphone

For communication with the patient during the examination

4.1.2.2 Patient Panel



Patient panel on the inside of the cabin to the right of the door.



1

Speaker

To reproduce the commands to the patient during the measurement by the user

2

Door opener


for opening the cabin door from inside possible at all times (see also chap. 4.2.2)

4.1.3 Connections / Interfaces of the Bodystik

4.1.3.1 Connection Panel




Connection panel to the right of the door
on the lower right-hand side of the cabin.

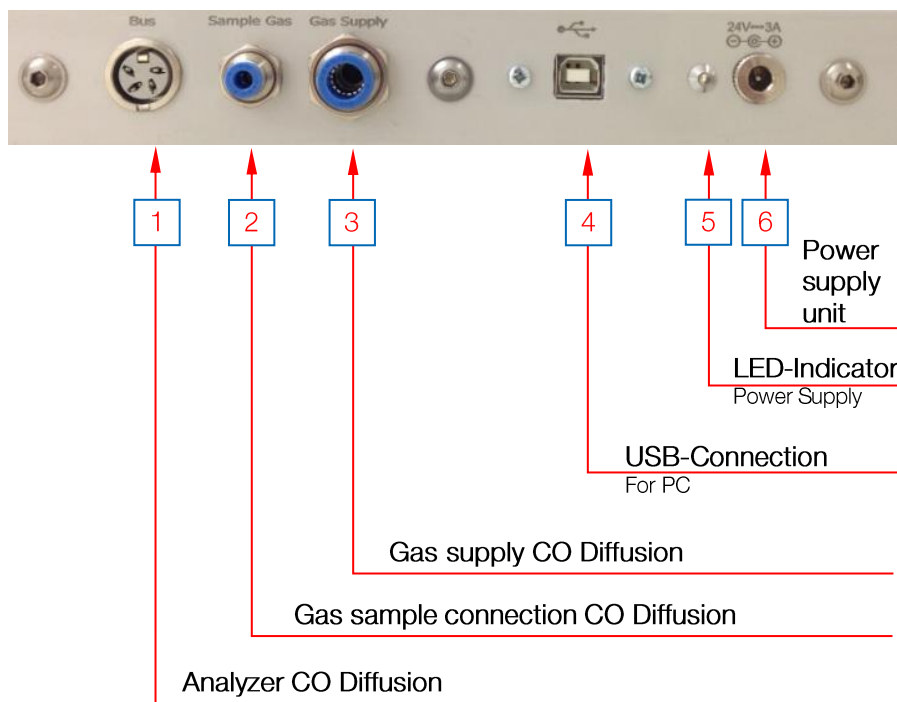

4.1.3.2 Connectors on the Height-Adjustable Arm



Connection sockets on the Height Adjustable Arm.



Flow unit

1

Gas sample
(CO Diffusion connection)

2

Gas supply CO Diffusion

3



The connection of the components for extending the Bodystik with the CO Diffusion option is described in the separate IFU:

- Add-on Co-Diffusion

4.1.3.3 Sensors



Attention

Bodystik could be damaged.

Reason: **Sensors of Bodystik are precise and high-resolution components.**

For this: **Ensure the respective functions are preserved!**

Therefore:

- Exactly follow instructions for cleaning, disinfection and calibration!



You will find a detailed description in:

- Chap. 9 "Cleaning and Disinfection"
- The separate IFU
Calibration Flow Sensor and
Calibration Bodyplethysmograph

Pressure Sensor

The Bodystik has a highly sensitive pressure sensor which is able to precisely resolve even the slightest pressure changes in the cabin. It must be calibrated before the first examination of the day.

Flow Sensor

The heart of the Bodystik for precise flow measurement is the Ergoflow flow sensor. It must be calibrated after every cleaning and before the first examination of a day.

As the flow sensor ensures the precise flow measurements, the cleaning and calibration requirements must absolutely be adhered to, regardless of the version selected.

Mouth Pressure Sensor

A precise and long-term stable pressure sensor for measuring the mouth pressure is integrated in the flow unit.

This can be calibrated with the help of an external manometer.

Temperature / Humidity / Air pressure Sensor

In the height-adjustable stand of the Bodystik are sensors for determining the current temperature and humidity as well as a sensor for the air pressure at the rear of the cabin. These continuously measure the current environmental conditions and enable exact measurement results through online tracking of the BTPS compensation. The installed sensors are extremely stable over the long-term and are regularly checked by the specialist dealer.

4.1.3.4 Pressure Reducer (optional with Extension „Diffusion Measurement“)

The Bodystik provides the option of extension for CO Diffusion measurement. A suitable pressure reducer for the Diffusion gas bottle is required for safe application. If you are planning the extension with Diffusion measurement, please note:



Danger to life.

Reason: Poisoning by carbon monoxide (CO) during prolonged exposure. Therefore:

- Arrange the pressure reducer so that it is easily accessible to enable the gas supply to be quickly interrupted in the event of leakage!

Reason: damage to the CO Analyzer because of excessive working pressure on the demand valve. Therefore:

- Only use a pressure reducer that complies with the specifications defined by the manufacturer and provides a fixed outlet pressure of 5 bar!



A suitable pressure reducer has been approved by the manufacturer and is recommended for use. You can receive this from your authorised specialist retail partner.

- See also chap. 2.2.1 "Original Spare Parts / Accessories / Optional Expansions". \ 2.2.1.2

Depending on the regulations in the country of use, similar pressure reducers may be considered. The inspection and maintenance intervals specified in the operating instructions of the pressure reducer used must be observed.

For a complete explanation of the optional diffusion measurement with the "Add-On CO Diffusion", please refer to the separate IFU Add-on CO Diffusion

4.1.4 System Construction and Electrical Safety

The following instructions are intended for safe handling of the entire system, taking into account the electrical safety concept of the Bodystik.

The system may be set up only by an authorised specialist retail partner.

It is essential to note: Anyone who combines additional devices or medical devices or unauthorised or non-original components / spare parts / consumables with existing medical, electrical equipment or systems, and this combination is used by third parties or this combination is placed on the market, will legally become a producer of a system or a procedure pack. In any case the assembler of a system is therefore responsible for compliance with the requirements placed on the system by the relevant, harmonised standards and the additional national and international standards and guidelines in the currently valid versions!



You will find a detailed description of the correct system formation in:



- The technical manual "Formation of Systems".



WARNING

Possible danger to life.

Reason: Electric shock due to lack of galvanic separation with composition of non-approved components. Therefore:

- Only use the power supply and USB connection cable supplied by the manufacturer as spare parts, which are always part of the medical device!

The followings applies to systems without integrated galvanic isolation (24 V Power Supply or USB Extension Cable, see chap. 4.1.4.2 “Data Connection” and chap. 4.1.4.3 “Power Supply”):

- The device may only be operated in conjunction with the equipment cart (ergoline ergocar PC) offered by manufacturer!

Reason: Electrical shock and / or misdiagnosis due to loss of electrical safety caused by exceeding the recommended maintenance schedule. Therefore:

- Regularly check the specified maintenance schedules!
- If a maintenance schedule is exceeded, do not continue to use the complete system! Request maintenance work from your authorised specialist retail partner!

Reason: **Misdiagnosis caused by measurement error.**
Therefore:

- Do not connect any additional USB devices! (except mouse, keyboard and printer)!
- Do not install any further software!
- Ask your authorised specialist retail partner which devices are approved by the manufacturer!



Attention

Bodystik could be damaged.

Reason: **Electrostatic discharges.** Therefore:

- Preferably no floor made of synthetic material!
- Otherwise a relative air humidity of at least 30 % is required!

4.1.4.1 Equipment Cart with Isolating Transformer



The cart, approved by the manufacturer, meets the requirements of the IEC 60601 series of standards and is mandatory to use.

You will find more detailed information in:

- Chap. 2.2.1 "Original Spare Parts / Accessories / Optional Expansions". \ 2.2.1.2
- Chap. 4.1.4.2 "Data Connection"
- Chap. 4.1.4.3 "Power Supply"
- Respectively consult with your authorised specialist retail partner.

4.1.4.2 Data Connection



The hardware connection between the cabin and the computer is established via an integrated USB interface and USB cable. This is considered a spare part approved by the manufacturer and must be obtained from an authorised specialist retail partner. (See also chap. 2.2.1.1 "Original Spare Parts / Accessories").

Depending on the date of manufacture, the USB connection cable contains an integrated galvanic isolation, see the following table. This can also be retrofitted.



WARNING

Possible danger to life

Reason: Electric shock due to lack of galvanic separation with composition of non-approved components. Therefore:

- Only use the USB connection cable supplied by the manufacturer as spare parts, which are always part of the medical device. (See chap. 2.2.1.1 "Original Spare Parts / Accessories").

The followings applies to systems without integrated galvanic isolation (USB Extension Cable, see chap. 2.2.1.1 "Original Spare Parts / Accessories":

These devices may only be operated in conjunction with the equipment cart (ergoline ergocar PC) offered by manufacturer!

From 02/2023 (Serial number 230100528)	Until 02/2023 (Serial number 230100528)
With galvanic isolation	Without galvanic isolation
	
Recognisable by the housing along the cable	Recognisable by the missing housing along the cable

All measurement results and graphical data can be displayed on the screen as well as printed out via the Windows printer interface. Any printer compatible with Windows can be used for this.

4.1.4.3 Power Supply



The power supply is provided by an external desktop power supply Unit. Only this is considered a spare part approved by the manufacturer and can be obtained from an authorised specialist retail partner (see also chap. 2.2.1.1 "Original Spare Parts / Accessories").

Depending on the time of manufacture, the power supply contains an integrated 4 KV isolation, see the following table.

This can also be retrofitted.

from 08 / 2015	to 08 / 2015
With 4 KV Isolation	Without 4 KV Isolation
	
Recognisable by the manufacturers information on the type label "Bicker", Model "BET-1024M"	Recognisable bei the manufacturers information on the type label "Deutronic", Model "ETC70G-24"

4.2 Technical Protection Measures

Bodystik has been designed and built in accordance with the recognised state of technology and the requirements of the applicable, safety-relevant regulations.

This chapter of the IFU only describes the operation of protective and safety equipment or safety systems that can be triggered by patients and operators themselves in an emergency to protect themselves.

The technical safety condition is checked by the authorised specialist retail partner of the manufacturers within the framework of technical monitoring (see also chap. 8 “Servicing / Maintenance”).

4.2.1 Emergency Stop

When the **EMERGENCY OFF button** is actuated, the power and data lines are immediately disconnected.



EMERGENCY OFF button on the user panel of the cabin



Release

By applying strong pressure to the **EMERGENCY OFF button**

- Push button engages.
- Cabin door lock is deactivated (door opens).
- Height-Adjustable Arm is no more height adjustable.
- Communication with the PC no longer functions.
- LED "Power Supply" on the connection panel turns off.



Reset / Unlock

- By turning the **EMERGENCY OFF button** counterclockwise until the overcoming of a resistance can be felt

EMERGENCY OFF button is unlocked and ready for operation again.



The Bodystik can only be operated again after unlocking the **EMERGENCY STOP**. For more detailed information, please see:

- Chap. 6.2 "Recommissioning after Servicing / Cleaning Work".

4.2.2 Door-Opener Patient Panel

With the door opener, the cabin door can be opened any time by the patient sitting in the cabin in case of emergency.



Danger to life possible.

Reason: Collapse of the patient due to claustrophobia.

For this: Observe general medical principles!

Therefore:

- Before examination, inform the patient about the emergency opening of the door!
- Do not leave the patient unattended in the cabin!



Door opener on the patient panel in the cabin



Press button

- Cabin door opens.
- GREEN LED turns off.
- Depending on the currently running examination, measurement may be aborted.
- For further operation follow the instructions of the software.



Expected consequences in case of abort during:

- **Resistance-Measurement**
The recorded data are saved and the measurement finished.



Expected consequences in case of abort during:

TGV-Measurement



- TGV curves recorded up to this point and switched to the IC/ERV manoeuvre. If no TGV curve is available yet, the examination is aborted.

Other investigations continue without interruption.

- For a more detailed description see IFU BLUE CHERRY®

4.3 Software

The measurement device (Bodystik) is supplied with BLUE CHERRY® software. This serves to manage patient and examination data as well as carry out, depict, process and record measurements with the devices of the manufacturer.

The communication between the BLUE CHERRY® software and a practice computer system or hospital information system is supported by standardised software interfaces (e.g. HL7, GDT). Paid software options are necessary for this, if applicable.

A modular and flexible hardware and software concept makes it possible to combine this with additional measurement options and consequently allows the overall system to be configured separately for individual customers.

For the identification of the current firmware version, this can be read by the BLUE CHERRY® device management system.



For further information see the separate IFU of

BLUE CHERRY® – information on the configuration and use of the Software BLUE CHERRY®.



5 Transport, Storage and Assembly

5.1 Transport to the Location of Use

The Bodystik is transported secured against damage, where necessary in special wooden packaging, which is mounted on pallets. Standard components, additionally wrapped in bubble wrap, are in a cardboard box.



The packaging must be kept by the user / operator in case the device must be returned to the authorised specialist retail partner or manufacturer.

For further information see:

- Chap. 11 "Decommissioning / Disposal" / 11.3.1
- Chap. 15 "Warranty and Service" / 15.3

The specialist retail partners authorised by the manufacturer are responsible for delivering the Bodystik to the responsible organisation and for unpacking and transporting it to the actual installation site.

5.2 Storage

Requirements regarding space requirements, media connections and operating conditions can be found in chap. 12 "Technical Specifications".

The responsible organisation of the Bodystik is solely in charge of compliance with these requirements.

For storage and transport conditions, see chap. 12 "Technical Specifications".

5.3 Assembly

Installation or assembly for the first commissioning of the Bodystik may only be carried out by qualified personnel of the manufacturer's specialist retail partners.



Possible danger to life.

Reason: Electric shock. Misdiagnosis caused by measurement error. Therefore:

- Prevent improper assembly / installation!
- Bodystik should only be assembled and installed by officially trained personnel authorised by the manufacturer!



For further information see:

- Chap. 4.1.4 "System Construction and Electrical Safety".



Information on assembly work in connection with the Recommissioning in:

- Chap. 6.2 "Recommissioning after Servicing / Cleaning Work".

6 Operation

6.1 Initial Operating

The first commissioning of the Bodystik and its recommissioning after maintenance work in accordance with the responsible organisation's obligations (see chap. 8 "Servicing / Maintenance"), which is carried out by qualified personnel of the specialist retail partner, is also only carried out by these qualified personnel.

Bodystik is only completely ready to function after calibration and once the initial operation is complete.

6.2 Recommissioning after Servicing / Cleaning Work

The responsible organisation is responsible for returning the device to operation after servicing / cleaning work for which the user / operator is authorised.



Attention

Bodystik could be damaged.

Reason: **Careless operation.** Therefore:

- Assure that all cables and tubes are connected carefully!
- Generally, do not expose cables, tubes and their connections to mechanical stress such as tension, pressure, bending or similar!



WARNING

Possible danger to life

Reason: **Electric shock.** Therefore:

Never obstruct the access to the mains plug or On / Off switch of the equipment cart!
Disconnection of the power supply must be easily accessible!

Recommissioning after an EMERGENCY STOP Signal
With successful unlocking of the EMERGENCY OFF button:

- The communication to the BLUE CHERRY[®] Software is automatically initialised and a zero-point adjustment is performed.
- The Cabin is restarted (audible by the "click").
- The Bodystik is ready for operation and function again.



WARNING

Possible severe physical injury.

Reason: **Crushing by unintentional height-adjustable stand movements. Patient collapses because the cabin door is firmly closed.** Therefore:

- Do not restore the EMERGENCY OFF button to a functional state until the cause of the release has been eliminated!



If the last calibration was carried out within the valid time frame according to chap. 7.3 "Calibrating Bodystik", the Bodystik is ready for operation after an EMERGENCY STOP without a new calibration.

Further descriptions can be found in:

- Chap. 4.2.1 "Emergency Stop"
(to unlock EMERGENCY STOP)
- Separate IFU
 - Calibration Flow Sensor and
 - Calibration Bodyplethysmograph

6.2.1 Recommissioning after Termination by Patient

If the door is opened by the patient from the inside of the cabin, the Bodystik still remains functional.

Only the current measurement is aborted.

You can now decide if the interrupted measurement should be resumed or continued with the next measurement.

Follow the Software instructions.



To continue the "Resistance" and "TGV" measurements, the door must be closed again. If this is not done, the BLUE CHERRY® Software will inform you with the message **"Please close the door"**

You can find more information on:

- Resistance and TGV
in chap. 4.2.2 "Door-Opener Patient Panel"
- Software operation generally
in the separate IFU BLUE CHERRY®

6.2.2 Recommissioning after Maintenance / Cleaning Work by the Operator

Before the Bodystik can be used to perform measurements again, all components must be properly reconnected, the USB connection to the computer must be established, and the Bodystik must be connected to the power supply and calibrated. Calibration also fulfils the regulatory requirements for functional testing after maintenance work.

Please proceed as described in the respective chapters.

6.2.3 Assembly Flow Measuring System



CAUTION

Possible physical injury.

Reason: **Measurement error due to leakage caused by incorrect assembly of components.** Therefore:

- Carefully observe the assembly instructions!



Attention

Functional disorders possible.


Reason: **Components and e.g. plug connections can be damaged.** Therefore:

- All connections must be made carefully and without too much force!




For connecting the cables please read:

- Chap. 4.1.3.2 "Connectors on the Height-Adjustable Arm".



Height-adjustable arm with flow measuring system and shutter system incl. connection sockets

From Prod. 11 / 2018

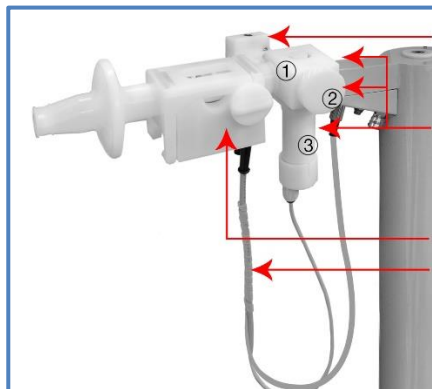


Mounting plate

Shutter block [1] with
 Shutter plug [2] and
 Shutter drive [3]

Flow unit

Connection cable

Until Prod. 11 / 2018

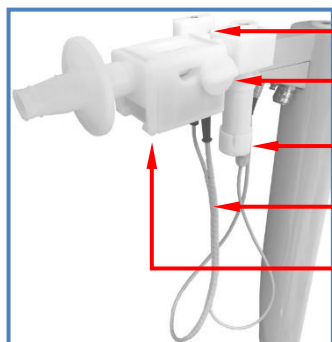


Mounting plate

Shutter head

Shutter drive with shutter cage

Connection cable

Flow unit

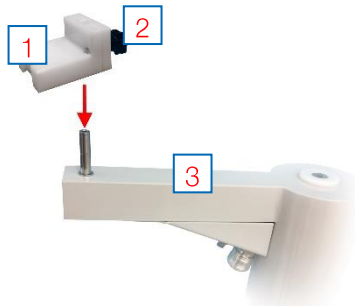

1. **Attach the mounting plate [1] to the height-adjustable arm [3].**

For this:


Insert the stand holding plate on the bolt of the height-adjustable arm and

tighten the knob [2] until the mounting plate remains movable.




2. **Connect the shutter block [4a] to the mounting plate [1] from production 11 / 2018**
By

pressing the dovetail of the shutter block into the appropriate groove [5] of the mounting plate [1].

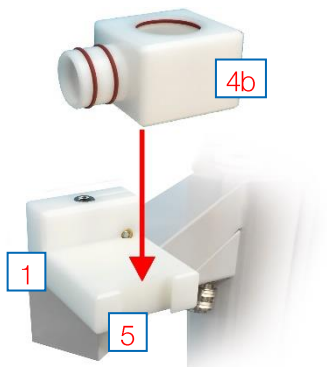

3. **Connect the shutter head [4b] with the mounting plate [1] before production 11 / 2018**
By

pressing the dovetail of the shutter head into the appropriate groove [5] of the mounting plate [1].

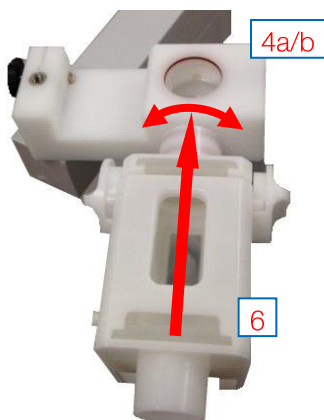


4. Insert the flow unit [6] into the connection socket of the shutter block or shutter head [4a / b]

For this:

Push the flow unit with the fixed side slightly to the stop and simultaneously turn it back and forth.



Turning in both directions has no functional task but serves only to protect the O-Rings.

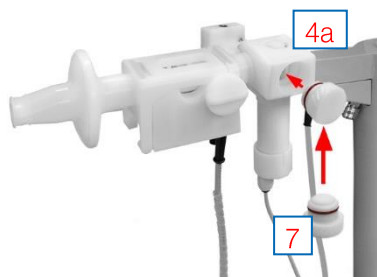


5. Connect the connector cable at the bottom of the height-adjustable arm.
6. For installation from 11 / 2018 without CO Diffusion Add-on: Connect shutter plug [7] to shutter block [4a].


6.2.3.1 Assembly Shutter System



Height-adjustable arm with shutter system including connection sockets.
(detailed overview see chap. 4.1.3.2)

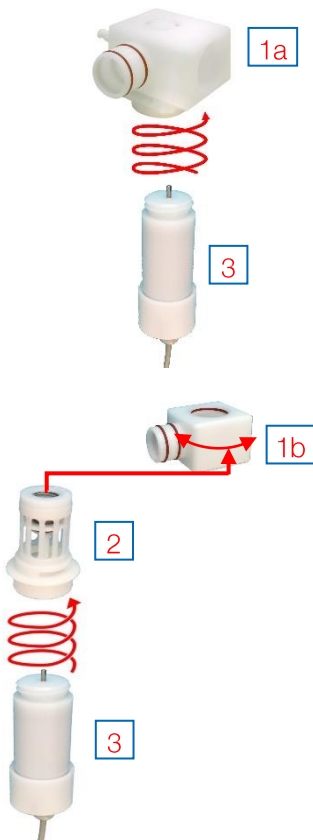

1. **From prod. 11 / 2018:**
Screw shutter drive [3] to shutter block [1a] until stop
2. **Until prod. 11 / 2018:**
Screw shutter drive [3] on the shutter cage [2] until stop
3. Slide the shutter cage into the shutter head [1b]
By
Slight rotation (to protect the O-Rings) until stop.

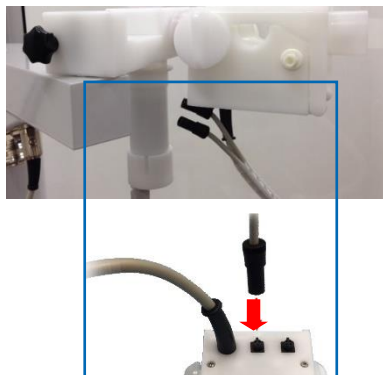


4. Connect the connector cable of the shutter drive [3] with three-pole socket on the flow unit – central.



If possible, observe the sequence of the work steps, because otherwise it is more difficult to assemble!

6.2.3.2 Inserting the Flow Sensor

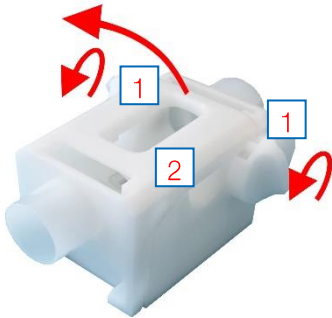


1. Open the closing cap [2] on the flow unit

For this:

Turn the screw lock [1] on the left and right side and

open the closure cap [2] upwards.

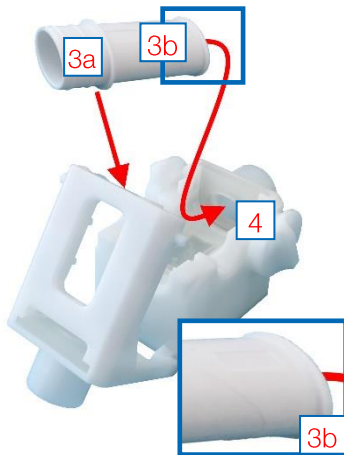

2. Insert the flow sensor [3]

For this:


Carefully press the patient-far side with connection piece [3b] into the holder with silicone seal [4].

Press the patient-close side [3a] into the receptacle.

3. Close and lock the cover cap

For this:

Proceed in reverse order as described in point 1.



Attention

Measurement function could be impaired.

Therefore: Make sure that the sensor pins [3a] inserted in the silicone seal [4]!

6.2.3.3 Connection Power Supply and PC



WARNING

Possible danger to life.


Reason: Electric shock due to lack of galvanic separation with composition of non-approved components. Therefore:

- Only use the power supply and USB-connection cable supplied by the manufacturer as spare parts, which are always part of the medical device!

The followings applies to systems without integrated galvanic isolation (24 V Power Supply or USB Extension Cable, see chap. 4.1.4.2 "Data Connection" and chap. 4.1.4.3 "Power Supply"):

- The device may only be operated in conjunction with the equipment cart (ergoline ergocar PC) offered by the manufacturer!

The Bodystik is activated by establishing the power supply.
To do this, connect the power supply:

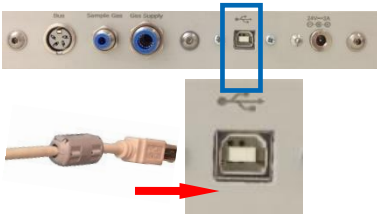

1. USB-connection cable

- To USB socket of the Bodystik
- To free USB port of the PC



2. Medical power supply unit

- To socket of the connection panel on the Bodystik
- With power supply cable to a socket

3. Insert the power supply of the equipment cart into the power socket.
4. Turn on the equipment cart with the On / Off switch
Display "**Power Supply**" of the equipment cart lights up



If the corresponding power supply unit is connected:

- The LED Display "Power Supply" on the connection panel lights up.
- Bodystik is ready for operation.



Only after a new calibration is the Bodystik ready to operate again. see also:

- Chap. 7.3 "Calibrating Bodystik".
- Separate IFU
 - Flow Sensor Calibration
 - Calibration Bodyplethysmograph

7 Operating Instructions

7.1 Checking for Worn Parts



The Bodystik should be checked for defective wearing parts each day before beginning treatments.

You can get a description in:

- Chap. 8 "Servicing / Maintenance"

And:



WARNING

Possible danger to life.

Reason: **Misdiagnosis caused by measurement error due to incorrect components or improper use.**

Therefore:

- Replace the flow sensor and the mouthpiece in case of a functional error!
- Replace the flow sensor immediately in case of saliva or moisture inside the flow sensor!
- Always follow instructions (see chap. 8 "Servicing / Maintenance" and chap. 9 "Cleaning and Disinfection")!

7.2 Switching Bodystik on

The Bodystik is designed for permanent operation and doesn't need to be switched on and off daily.

But there are different ways to finish the work with the Bodystik. Therefore the Bodystik is "switched on" again in different ways.



For descriptions of "Recommissioning after Servicing / Cleaning Work" see:

- Chap. 4.2.1 "Emergency Stop"
- Chap. 6.2.1 "Recommissioning after Termination by Patient"
- Chap. 6.2.2 "Recommissioning after Maintenance / Cleaning Work by the Operator"

7.3 Calibrating Bodystik

There are various processes to be carried out for Bodystik in order to calibrate or validate the volume measurement.

The required intervals can be found in the tables below.

Interval	Calibration
Once per day	Box calibration
Once per day, and after changing the Flow Sensor	Volume calibration
Once per week	Flow linearity test
Once per year	Mouth pressure calibration



For details of individual calibrations, please read the separate IFU:

- Flow Sensor Calibration
- Calibration Bodyplethysmograph

7.4 Setting up the Cabin

The correct sitting position of the patient is decisive for the success of the examination. This must always be individually adjusted.



- Make sure that the patient is sitting upright, and the back of the chair doesn't touch the back wall of the cabin.
- Adjust the seat height so that the patient's feet are horizontal on the floor and the thighs rest completely on the chair surface.
- The height of the height-adjustable arm should be adjusted so that the patient can easily reach the Mouthpiece from this sitting position.
- For adjustment use the push buttons on the outside of the cabin. (see chap. 4.1.2.1 Operating Elements [4] + [5])

7.4.1 Height-Adjustable Arm




Height adjustment

By

pressing the corresponding button on the user panel [1].


7.4.2 Patient Chair

In addition to height adjustment, the chair can also be swivelled in the direction of the door. This can make it easier to sit down or stand up and leave the cabin if necessary.

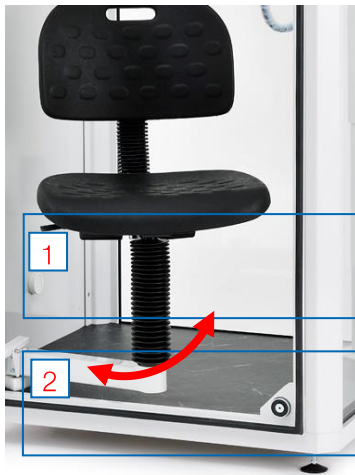

Height adjustment

Swivel



To unlock the swivel mechanism, step on the footrest [2]

→ Re-engages automatically in the end positions of the swivel mechanism.



Possible physical injury.

Reason: Pressure unloading through damaged gas pressure spring of the patient chair. Therefore:

- Observe the maximum weight of the person on the chair. It is 150 kg!



Possible severe physical injury.

Reason: Bodystik can tilt over. Therefore:

- Observe the maximum weight of the person on the chair when chair is swivelled outwards. It is 125 kg!

7.5 Using Bodystik / Performing Measurements



Descriptions of the applications can be found in the separate IFU:



- Spirometry
- Bodyplethysmography
- Rint
- Respiratory Drive (MIP / MEP, P0.1)
- CO Diffusion

And for general use of the software:

- BLUE CHERRY[®]



Possible danger to life.

Reason: Disregard of a contraindication.

Misdiagnosis due to measurement errors. For this:
Observe the general medical principles! Therefore:

- Inform yourself and observe the respective contraindications before each test!
- When carrying out tests, observe the content of the applicable guidelines and recommendations (e.g. ATS / ERS Guidelines)!
- Before examination, inform the patient about the emergency opening of the door!
- Do not leave the patient unattended in the cabin!

Reason: **Misdiagnosis due to measurement error caused by a system failure due to uncontrollable electromagnetic fields of inadmissible transmitting devices.** Therefore:

- While using Bodystik, do not use any transmitting devices (e.g. mobile phones, portable phones, power lines ...) within close proximity (< 30 cm) that exceed the immunity levels as specified in the EMC guidelines! Ask your authorised specialist retail partner about this!

Reason: **Electrical shock.** Therefore

- Ensure that the users or third party persons do not touch the patient and any conductive connections or parts of the device that are located outside the patient environment at the same time!



CAUTION

Possible physical injury

Reason: **Skin burn caused by short-circuit inside the device.** Therefore:

- Do not touch shutter drive in case of excessive heat!



Attention

Bodystik could be damaged.

Reason: **Penetrating liquid. Uncleanliness. External exposure**

Therefore:

- Do not use liquids near the Bodystik!
- Do not expose the Bodystik to excessive temperature fluctuations during operation!
- Do not drop any objects on the device!
- Do not lay any objects on it!
- Never push foreign objects into the housing!

Reason: **Condensation.** Therefore:

- Do not expose the device to excessive temperature fluctuations during operation!

7.6 Exchange of Disposable Products / Disinfection

7.6.1 Bacteria- and Virus Filter / Noseclip



Possible danger to life.

Reason: **Cross-contamination.** For this: **Observe the general medical principles!** Therefore:

- Do not use single use products more than once!
- Dispose of bacteria / virus filter and noseclip after each use!

The bacteria and virus filters provided by the manufacturer are optimally adapted to the measuring systems and, due to the very high filtration rate, offer maximum patient safety while protecting against cross-contamination. The filters must also be disposed after each examination or patient. The same applies to the noseclip.

7.6.2 Bodystik / Cabin

Parts of the cabin which have come into contact with the patient during the treatment must be treated with surface disinfection.



For further weekly cleaning and disinfection tasks, please see:

- Chap. 9 "Cleaning and Disinfection"

Information about disposal of the disposable products can be found in:

- Chap. 11.3 "Disposal" / 11.3.3

7.7 Switching off Bodystik

Switching off the Bodystik can be done by disconnecting the power supply. If an equipment cart is used, it can be switched on by using the On / Off switch on the equipment cart (see chap. 7.2 “Switching off Bodystik”).

Disconnection from the mains can only be effected by removing the power cable connector of the power supply unit from the socket. The Bodystik is intended for continuous operation and therefore doesn't need be switched on and off daily. **But:**



Attention

Bodystik could be damaged.

Reason: **Penetrating liquids into electronic components.**

Therefore:

- Disconnect the Bodystik from the power supply before cleaning and disinfecting!
(When switching off via the On / Off switch of the Equipment Cart), shut down the PC completely before doing!
- Wipe off remaining moisture with a dry cloth!



For more reasons why the Bodystik must be „Switched Off“ please see:

- Chap. 4.2 “Technical Protection Measures“

8 Servicing / Maintenance

8.1 Duties of the Responsible Organisation

Responsible organisations of medical devices are obligated, in accordance with the corresponding, applicable regulations, to preserve the properties of this medical device assured by the manufacturer over its whole service life. This also includes carrying out regular and proper servicing as well as safety checks at intervals recommended by the manufacturer carried out by specialist personnel who have been authorised by the manufacturer for the respective tasks.

The expected service life of Bodystik is 8 years.

In its development, a great deal of value was placed on making the servicing of all device components as simple as possible. Only a little work is necessary to guarantee a fault-free operation of the device.

However, to maintain a high quality of measurement results and the safe operation, the manufacturer recommends having the device safety and measurement precision checked by an authorised specialist retail partner every 24 months.

These checks include:

- Visual check
- Electrical measurement
- Functional Check



WARNING

Possible danger to life.

Reason: Electric shock and / or misdiagnosis due to loss of electrical safety caused by exceeding the recommended maintenance schedule. Therefore:

- Regularly check the specified maintenance schedule!
- If a maintenance schedule is exceeded, do not continue to use the complete system!
Request maintenance work from your authorised specialist retail partner!



Attention

Independent of this, the user / operator must carry out regular checks during day-to-day operation, see also the following chap. 8.2 “Servicing / Maintenance by the User / Operator”!

8.2 Servicing / Maintenance by the User / Operator

In order to ensure a flawless operation of Bodystik over its whole service life, regular servicing and repairs, if applicable, are required.

Interval	Servicing work
Once per day	Visual checks of the device and its components for damage and replacing them if necessary (see chap. 8.2.1 “Checking / Exchange of Tubes and Cables”)
Once per day	Checking the O-Rings and Sealing Rubbers for tears / wear and replace if necessary (see chap. 8.2.2 “Checking / Replacing O-Rings and Sealing Rubbers”)
Once per week	Brush the door rubber with Vaseline (see chap. 8.2.3 “Care of Door Rubbers”)
Once per year	Replacing the O-Rings and Sealing Rubbers (see chap. 8.2.2 “Checking / Replacing O-Rings and Sealing Rubbers”)



WARNING

Possible danger to life

Reason: **electric shock. Misdiagnosis caused by damaged components of the Bodystik.**

Therefore

- Always make controls before starting the Bodystik examination!

Reason: Electric shock. Triggering malfunctions of Bodystik. Unqualified user / operator can detect sources of failures too late or even cause them. Therefore:

- All maintenance and servicing work may only be performed by specialised personnel who have been authorised by the manufacturer!

8.2.1 Checking / Exchange of Tubes and Cables

All parts of Bodystik should be checked for visible mechanical damage (cracks, tears) each day. If damage is ascertained, the corresponding component must be replaced.



For replacing components see:

- Chap. 4.1.3 “Connections / Interfaces of the Bodystik”
- Chap. 4.1.4 “System Construction and Electrical Safety”
- Chap. 6.2.2 “Recommissioning after Maintenance / Cleaning Work by the Operator”

8.2.2 Checking / Replacing O-Rings and Sealing Rubbers




During the daily inspection of the O-Rings and sealing rubbers, attention must be paid to mechanical damage or signs of abrasion. If necessary, any affected parts must be replaced. Once a year it must generally be replaced. Proceed as described below:

O-Rings Shutter Block



- [1a] Insert with a slight rotation
 - [1b] Press firmly
- Identical steps [1a und 1b], see below.

O-Rings Shutter Head



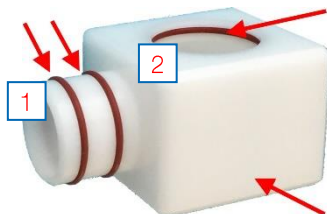


- [1a] Insert with a slight rotation
 - [1b] Press firmly
 - [2a] Insert one side into the groove
 - [2b] Slightly screw in
 - [2c] Press the second side into the groove
 - [2d] Press all around
- To remove the rings, proceed in reverse order.




Attention

The unit may be damaged.
Therefore: Do not use any pointed / sharp objects for removal!



Sealing Rubber Flow Unit

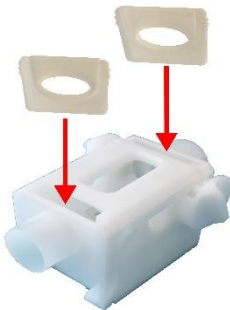

When ordering new O-rings and sealing rubbers, please note

- Chap 0 "System Construction and Electrical Safety"
- Chap 6.2.2 "Recommissioning after Maintenance / Cleaning Work by the Operator"

8.2.3 Care of Door Rubbers

To care for the door rubber, a film of vaseline is applied with a soft brush.



For the selection of suitable Vaseline please see:

- Kap. 2.2.2 "Consumable Items / Auxiliary Materials"

9 Cleaning and Disinfection

The devices of the manufacturer were designed in such a way that minimal effort is required for cleaning and disinfection. This is why just a few tasks are necessary to keep Bodystik functional and clean.

Cleaning and disinfection may cause discolouration of the components, but without impairing their function.

The following intervals apply:

Component	Interval	Method
Bacteria and virus filter	After each patient	Dispose of!
Noseclip	After each patient	Dispose of!
Flow unit (chap. 9.2.1)	Weekly	Wipe disinfection
Ergoflow (chap. 9.2.2)	Weekly	Cleaning and disinfection bath
Shutter block (chap. 9.2.3.1)	Weekly	Cleaning and disinfection bath
Shutter plug (chap. 9.2.3.1)	Weekly	Cleaning and disinfection bath
Shutter cage (chap. 9.2.3.1)	Weekly	Cleaning and disinfection bath
Shutter head (chap. 9.2.3)	Weekly	Cleaning and disinfection bath
Shutter drive (chap. 9.2.3)	Weekly	Surface / Wipe disinfection
All other touchable parts	Weekly	Surface / Wipe disinfection



Personal injury possible.

Reason: **misinterpretation of obvious measuring errors (drift) caused by liquid in the tubes.** Therefore:

- Clean tubes only externally!
- Replace dirty tubes!



Attention

Bodystik could fail.

Reason: **Damaged connections.** Therefore:

- To disconnect electrical connections, always pull the plug and never the cable!

9.1 Single Use



For instructions on handling bacteria and virus filters and noseclips, read:



- Chap. 7.6 “Exchange of Disposable Products / Disinfection”

9.2 Disinfection

In spite of the high filtration rate and single use of the bacteria and virus filters, it is necessary to clean and disinfect at least once a week all components which come into contact with the patient respiratory flow. This applies to the flow unit, Ergoflow, shutter cage and shutter head or shutter block.

All parts of the Bodystik can be cleaned from dirt with a soft cloth using a cleaning solution / weak soap suds.

All parts of Bodystik which come into contact, or could come into contact, with the patient must be treated with a surface disinfection. Otherwise, these can be wiped with a soft cloth using a weak soap solution.

When using a disinfectant that has not been tested and approved by the manufacturer, the following steps must be observed:

- Preferably use agents that correspond in composition to the approved agents. The composition is available on data sheets, which we can provide on request.
- Check bactericidal and virucidal effect suitable for the intended use.
- Use only disinfectants listed in public databases (e.g. RKI)
- Check data sheet for material compatibility with plastics (especially polyoxymethylene, polystyrene, acrylonitrile butadiene styrene, Makrolon®) as well as metal
- First test the disinfectant for material compatibility in an inconspicuous place.
- During the regular visual inspection for damage, also pay attention to material changes (discoloration, cracks, embrittlement...)
- Observe long-term trend of calibrations for changes in measuring function

The manufacturer accepts no liability for any resulting equipment damage or any consequential damage caused by the use of disinfectants that have not been tested and approved by the manufacturer.



Attention

Bodystik could be damaged.

Reason: **Improperly treated components.** Therefore:

- For cleaning and disinfection only use those active substances that are approved by the manufacturer (see chap. 2.2.2 "Consumable Items / Auxiliary Materials")!
- Follow the instructions on the concentration and dwell time stated by the cleanser and disinfectant manufacturer!
- Do not put the flow unit and the shutter drive in cleaning or disinfection fluid! (Both are containing electronic components)
- Do not disassemble the demand valve or put it into disinfection fluid! Only surface disinfection!

Reason: **Higher temperatures can lead to deformation and damage.** Therefore:


- Observe the maximum permissible temperature of 75 °C for cleaning and disinfection!
- Do not dry with heat!

Possible impairment of the measuring function.

Reason: **Moisture in the connection port.** Therefore:

- Ensure that there is no moisture in the connection piece before recommissioning!

9.2.1 Flow Unit

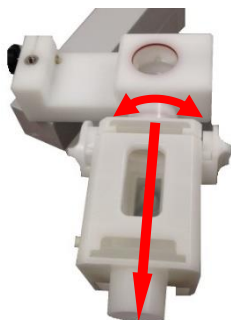

1. Remove the Ergoflow

For this:

Proceed in reverse order as described in chap. 6.2.3 "Assembly Flow Measuring System".

2. Perform a wipe disinfection

For this:

Wipe all accessible surfaces with a wet disinfecting cloth.

9.2.2 Ergoflow / Flow Sensor



Attention

Bodystik could be damaged.

Reason: **destruction of the orifice.** Therefore:

- Do not clean the interior of the sensor, mechanical or with hard water jet!
- Do not use any disinfectants which contain high chloride concentrations!



1. Remove the flow sensor

(in reverse order as in chap. 6.2.3.2. "Inserting the Flow Sensor" described)

2. Visible contamination wipe off with a soft cloth


3. Put the sensor in disinfectant fluid

4. Wash the sensor in distilled water thoroughly so that no residual dirt and disinfectants remain

5. Air-dry sensor until no moisture is visible

9.2.3 Shutter System

9.2.3.1 Shutter Cage or Shutter Block

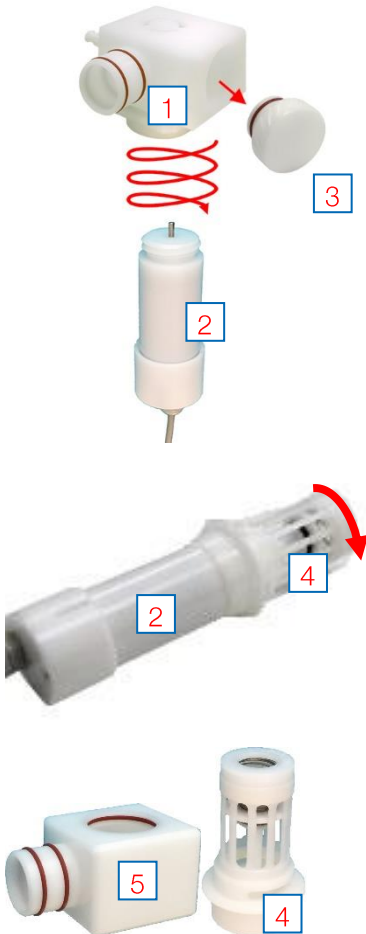

1. Disassemble the shutter system

For this:

Proceed in reverse order as described in chap. 6.2.3.1 "Assembly Shutter System".

2. a) Until product. 11 / 2018:
disconnect the shutter block [1] from the shutter drive [2]
by turning it counterclockwise.
Also separate the shutter block [1] from the shutter plug [3] by screwing and pulling it out.

b) Until product. 11 / 2018:
disconnect the shutter cage [4] from the shutter drive [2]
by turning it counterclockwise.

3. Remove visible dirt
with a soft cloth.
4. Put the components [1] + [3] or [4] + [5] in disinfectant fluid.
5. Wash the components [1] + [3] or [4] + [5] thoroughly in distilled water
so that no residues of contamination and disinfectants remain.
6. Components [1] + [3] or [4] + [5]
air dry
until no more moisture is visible.

9.2.3.2 Shutter Drive



Perform a wipe disinfection
For this:

Wipe the surface with a wet
disinfecting cloth.

9.2.4 Bodystik / Cabin



Attention

Bodystik could be damaged.

Reason: **Penetrating liquid into electrical components.**

Therefore:

- Disconnect the Bodystik from the power supply before cleaning and disinfecting! (When switching off via the On / Off switch of the equipment cart), shut down the PC completely before doing so!
- Wipe off remaining moisture with a dry cloth!

10 Fault Indication and Repair

Simple errors which occur when using Bodystik can be recognised quickly and rectified using the following table. If you cannot find the error in the table or the problem cannot be rectified using the method described, please contact your specialist retail partner.



You will reach your authorised specialist retail partner via contact form on the manufacturer's website
www.geratherm-respiratory.com/login/



DANGER

Danger to life.

Reason: **Unauthorised work carried out by the user to troubleshoot and rectify an error.** Therefore:

- Users may only carry out work which is described and permitted by the manufacturer!

In case of not complying with this restriction, the responsible operator alone is liable for any resulting injuries to persons and / or damages to Bodystik!

Error	Rectification
The device is not recognised by the PC	Check the power supply - Cable OK and connected?
	Check the USB connection - Cable OK and connected?
Height adjustment of the height-adjustable arm not possible	Check the power supply - Cable OK and connected?
	Unlocking the EMERGENCY OFF button (see chap. 4.2.1)

Error	Rectification
A closed door is not detected by the device	Check the contact of both holding plates with the respective magnet (see chap. 4.1.1[5]) Cleaning the magnets and the holding plates with a soft damp cloth
The speaker does not work	Checking the closed-door detection - is the door LED lighting up? (see chap. 4.1.2.1[2]) Check the volume setting in the software
Error message BLUE CHERRY® "Emergency stop pressed" (also in connection with a signal, e.g. "Flow: Emergency stop pressed")	Unlocking the EMERGENCY OFF button (see chap. 4.2.1) Checking the power supply - Cable OK and connected?
Error message: "Flow: No flow electronics detected".	Checking the connection between flow unit and Height-Adjustable Arm (see chap. 6.2.3.2)
Error message: "Pm: No mouth pressure sensor detected".	Checking the connection between flow unit and Height-Adjustable Arm (see chap. 6.2.3.2)
Error message: "Flow out of the valid range" or "PM out of the valid range".	Checking the position of the Ergoflow in the Flow Unit (see chap. 6.2.3) Checking the connection of the flow unit and the Height-Adjustable Arm (see chap. 6.2.3.2) System restart – Computer and Bodystik (see chap. 6.2)
Error message: "Temperature out of valid range" or "Air pressure out of valid range" or "Air humidity out of valid range"	Checking the ambient conditions System reboot - PC and Bodystik (see chap. 6.2 "Recommissioning after Servicing / Cleaning Work" and separate IFU BLUE CHERRY®)

Error	Rectification
Resistance" and "TGV" measurements cannot be performed	Closing the cabin door
Obvious measuring error	Checking the last calibration date and recalibrate if necessary (see chap. 7.3)

11 Decommissioning / Disposal

11.1 Expected Service Life

The expected service life of Bodystik has been stated by the manufacturer as 8 years.

This applies provided the operating conditions, the prescribed servicing intervals, taking into account and complying with all safety information such as is described in this IFU as well as other technical standard regulations are adhered to.

11.2 Decommissioning

For decommissioning, the Bodystik must be freed from any contaminated material.

11.3 Disposal

In general, the applicable national laws and regulations stipulated by the local authority should be complied with for disposal.

11.3.1 Transport Packaging

The transport packaging should be reused or sent for material recycling. Before doing so, you should check whether it is possible to reuse the packaging.

11.3.2 Bodystik

Bodystik is an active medical device and is thus subject to the WEEE directive 2012 / 19 / EU and the German law on electrical and electronic devices (ElektroG) for the disposal for old electrical items. Neither Bodystik itself, nor any of its components may be disposed of via household or practice waste.



In order to ensure environmentally friendly disposal, please contact the authorised specialist retail partner where you purchased Bodystik and / or the accessories.

11.3.3 Patient Chair

The patient chair in the cabin is equipped with a gas pressure spring. This is filled with oil.



WARNING

Possible severe physical injury.

Reason: **Pressure unloading through damage of the gas pressure spring on the patient chair.** Therefore:

- Do not open the gas pressure spring!
- Do not heat above 80 °C!



Attention

Environmental damage possible.

Reason: **Oil leaks into the soil or water.** Therefore:

- Do not dispose the gas spring in household waste!
- Disposal only through raw material dealers or hazardous waste collection points!

11.3.4 Infectious / Contaminated Single Use Items

All contaminated items such as filters, mouthpieces and noseclips must be disposed of through the hospital or medical practice waste.



WARNING

Possible severe physical injury.

Reason: **Contamination with transferable germs during improper disposal.** Therefore:

- Dispose single use items (disposable flow sensors, mouthpieces and noseclips) after each use. For this observe the applicable regulatory requirements for biologically hazardous materials!
- Observe regulations on wearing personal protective equipment (PPE)!

12 Technical Specifications

12.1 Technical Data

Medical device:	Class IIa (in accordance with Annex VIII of Regulation (EU) 2017/745 (MDR))
Cabin outer dimensions:	(L) 950 mm x (W) 850 mm x (H) 1730 mm
Cabin weight: (completely equipped):	164 kg
Chair- max: load capacity:	150 kg, respectively 125 kg with chair swivelled out

Electrical data:

Protection type:	IP20 (IEC 529)
Protection class:	II
Applied part:	BF (according to DIN EN 60601-1)
PC interface:	USB 2.0
Power supply:	Primary site : 100 – 240 V/50 – 60 Hz Secondary site : 24 V max. 4.2 A
Power consumption:	< 100 VA

EMC:	Group 1 / Class B
-------------	-------------------

Noise emission:	< 80 dB(A)
------------------------	------------

Surface temperature:

Normal operation:	< 48 °C
First error:	< 65 °C



In climatically controlled measurements, it has been proven that the housing temperatures of the flow unit and shutter drive do not exceed **44 °C**. Safe contact is therefore possible if this:

- the contact duration does not exceed a maximum of one minute,
- is made exclusively with healthy and uninjured skin,
- takes place within the intended use.

The temperatures of the Neumofilt, Softclip and chair application parts never exceeded **41 °C**.

Gas connection

(Add-on CO Diffusion):

Max. Pressure:	6 bar / 87 psi
Min. Flow:	6 l/s
CO max.:	0.3 %
CH ₄ max.:	0.3 %

Flow measurement:

Flow sensor:	Ergoflow
Measuring principle:	Differential pressure
Measuring range:	±16 l/s
Ventilation measuring range:	0 – 300 l/min
Flow resistance:	< 0.12 kPa/(l/s) < 14 l/s
Dead space:	< 32 ml
Flow resolution:	15 Bit
Sample rate:	125 Hz
Accuracy:	±3 % or 50 ml/s

Volume:

Measuring range:	0 –20 l
Accuracy:	±3 % or 50 ml

Cabin pressure:

Measuring principle:	Differential pressure / Thermal Microflow-measurement
Measuring range:	±0.25 kPa
Accuracy:	±(1.5 % of measured value +1.5 %FSS)
Flow resolution:	16 Bit

Mouth pressure:

Measuring principle:	Differential pressure
Measuring range:	±25 kPa
Accuracy:	±0.25 %FSS

Flow resolution: 15 Bit

Temperature measurement:

Measuring range: 0 °C to +50 °C
Resolution: 0,01 °C
Sample rate: 0,488 Hz
Accuracy: $\pm 1,25$ °C

Humidity measurement:

Measuring range: 0 – 100%
Resolution: 0,1 %
Sample rate: 0,488 Hz
Accuracy: $\pm 7\%$

Ambient pressure measurement

Measuring range: 300 – 1100 hPa
Resolution: 1 hPa
Sample rate: 0,488 Hz
Accuracy: ± 10 hPa bei 1000 hPa

Minimum PC system requirements:

Standard: at least EN 62368-1 / EN 60950
recommended EN 60601

Processor: X86 / amd64 compatible,
1 GHz or higher

RAM storage: 1 GB or higher

Hard drive storage: 5 GB or higher

Monitor: XGA (1024 x 768) or higher

PC interface: USB 2.0 recommended

Operating system: Windows 8.1 or higher

12.2 Installation and Operating Conditions


The following conditions supplement chap. 2.2 "Intended Use" and must be observed to maintain the properties of the Bodystik guaranteed by the manufacturer and for the safety of the patient and user / operator.

Storage / Transport:	min.	max.	
Temperature:	-10 °C	+50 °C	
Relative air humidity:	10 %	95 %	non-condensing
Atmospheric pressure:	700 hPa	1100 hPa	
Operation:	min.	max.	
Environmental temperature:	+10 °C	+35 °C	Avoid extreme temperature fluctuations!
Relative air humidity:	20 % (at least 30 % for synthetic flooring)	95 %	non-condensing
Atmospheric pressure:	700 hPa	1100 hPa	
Setup:	fixed		
Space requirement cabin: (door completely open)	(L) 1600 mm x (W) 950 mm x (H) 1730 mm		
Necessary ceiling load: (cabin + patient)	300 kg/m ²		
Flooring:	Wood, concrete or ceramic tiles stable; even; conductive		
Environment / room:	Closed, clinical area air-conditioned not an explosive or flammable environment! not near an MRI! not in direct sunlight not draught / flow to air conditioning system well ventilated		
Operating Mode:	Continuous operation		


12.3 Electrical Safety Concept

12.3.1 Bodystik without USB isolator with Medical Device Cart and Isolation Transformer

- External Medical Power Supply for Bodystik (Protection Class 2)
- Internal Medical Power Supply in Analysator (Protection Class 1)
- Communication with PC via USB Interface
- With Isolation Transformer via Medical Device Cart



Green Blocks = Geratherm Respiratory Medical Devices
Blue Blocks = 3rd Party Medical Devices
Grey Blocks = Non-Medical Devices
Hatched Blocks = Optional Devices/respectively Medical Devices
Blue Lines = Mains Power 100/240 VAC N/L/PE
Pink Lines = Mains Power 100/240 VAC N/L
Purple Lines = 24 VDC permanent
Purple dotted Lines = 24 VDC switched
Orange Lines = BUS with 24 VDC
Red Lines = Non-Electrical Connections
Green Lines = USB Connectivity
Yellow Lines = Unknown, External Data Connections
Double Framework = Galvanic Isolation from Electrical Connections
Arrows = Plug Connections
Rectangles = Screwed/Fixed Connections

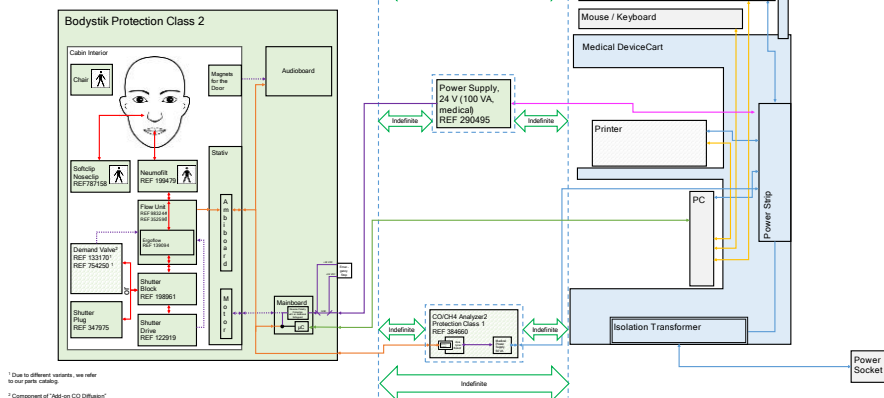


¹ Due to different variants, we refer to our parts catalog.
² Component of "Add-on CO2 Diffuser" REF 239149

The following safety concept applies to devices up to SN 230100528 for which a USB isolator has not yet been retrofitted (see chap. 4.1.4.2).

12.3.2 Bodystik with USB isolator with Medical Device Cart and Isolation Transformer

- External Medical Power Supply for Bodystik (Protection Class 2)
- Internal Medical Power Supply in Analysator (Protection Class 1)
- Communication with PC via USB Interface
- USB/PC Galvanic Isolation
- With Isolation Transformer via Medical Device Cart

Green Blocks = Geratherem Respiratory Medical Devices
Blue Blocks = 3rd Party Medical Devices
Grey Blocks = Non-Medical Devices
Hatched Blocks = Optional Devices/respectively Medical Devices
Blue Lines = Mains Power 100240 VAC N/L/PE
Pink Lines = Mains Power 100240 VAC N/L
Purple Lines = 24 VDC permanent
Purple dotted Lines = 24 VDC switched
Orange Lines = BUS with 24 VDC
Red Lines = Non-Electrical Connections
Green Lines = USB Connections
Yellow Lines = Unknown, External Data Connections
Double Framework = Galvanic Isolation from Electrical Connections
Arrows = Plug Connections
Rectangles = Screwed/Fixed Connections

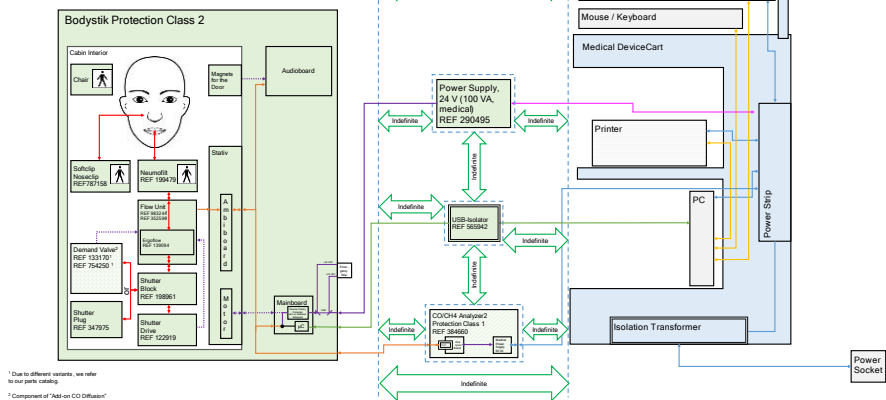


The following safety concept applies to devices from SN 230100528, and to older devices where the USB isolator has been retrofitted (see chap. 4.1.4.2).

12.3.3 Bodystik with USB isolator, without Medical Device Cart and Isolation Transformer



- External Medical Power Supply for Bodystik (Protection Class 2)
- Internal Medical Power Supply in Analysator (Protection Class 1)
- Communication with PC via USB Interface
- USB/PC Galvanic Isolation
- Without Medical Device Cart, without Isolation Transformer

Green Blocks = Geratherm Respiratory Medical Devices
Grey Blocks = Non-Medical Devices
Hatched Blocks = Optional Devices/respectively Medical Devices
Blue Lines = Mains Power 100/240 VAC N/L/PE
Pink Lines = Mains Power 100/240 VAC N/L
Purple Lines = 24 VDC permanent
Purple dotted Lines = 24 VDC switched
Orange Lines = BUS with 24 VDC
Red Lines = Non-Electrical Connections
Green Lines = USB Connectivity
Yellow Lines = Unknown, External Data Connections
Double Framework = Galvanic Isolation from Electrical Connections
Arrows = Plug Connections
Rectangles = Screwed/Fixed Connections

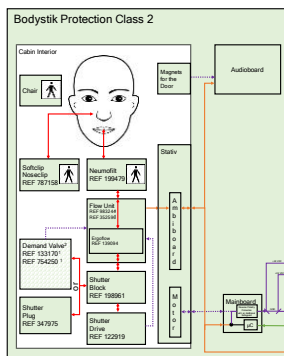

¹ Due to different variants, we refer to our parts catalog.

² Component of 'Add-on CO2 Dilution' REF 230149.

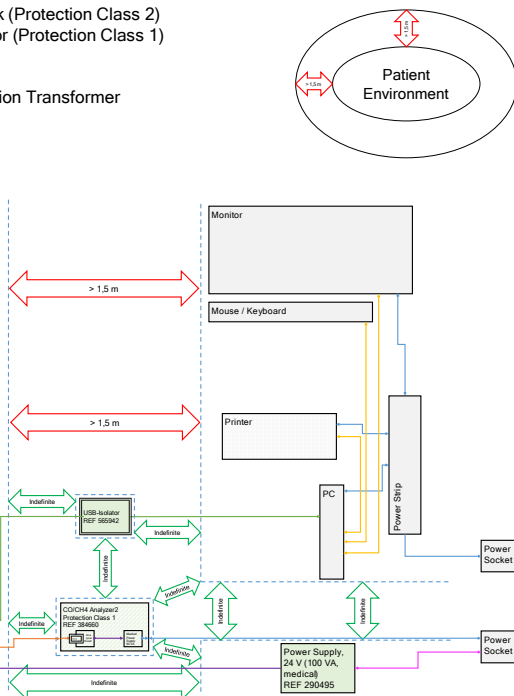

The following safety concept applies to devices from SN 230100528, and to older devices where the USB isolator has been retrofitted (see chap. 4.1.4.2).

12.4 Electromagnetic Compatibility / EMC Guidelines

The manufacturer tests his products for emitted interference and interference resistance. Compliance with the relevant standards and directives is certified in the Declaration of Conformity that accompanies this device. The results of the EMC test can be found in the following chapter.

12.4.1 Emitted Interference Guideline and Manufacturer Declaration

Guidelines and manufacturer's declaration – electromagnetic emissions		
The Bodystik is determined for operation in an electromagnetic environment as specified below. The user / operator of the Bodystik should ensure that it is operated in this environment.		
Measurement of electromagnetic emissions	Compliance	Electromagnetic environment – Guideline
RF emissions CISPR 11	Group 1	The Bodystik uses RF energy exclusively for its internal function. Therefore, its RF emission is very low and is improbable to interfere with adjacent electronic equipment.
RF emissions CISPR 11	Class B	The Bodystik is suitable for use in all establishments, including living areas and those directly connected to the public supply network, which also supplies buildings used for residential purposes.
Emissions of harmonic oscillations according to IEC 61000-3-2	Class A	
Emissions of voltage fluctuations / flicker according to IEC 61000-3-3	Compliance	

12.4.2 Interference Resistance for all ME Systems Guideline and Manufacturer Declaration

Guidelines and manufacturer's declaration – electromagnetic interference immunity			
The Bodystik is determined for operation in an electromagnetic environment as specified below. The user / operator of the Bodystik should ensure that it is operated in this environment.			
Measurement of interference immunity	IEC 60601 – test level	Compliance level	Electromagnetic environment – Guideline
Electrostatic discharge (ESD) according to IEC 61000-4-2	±8 kV contact ±15 kV air	±8 kV contact ±15 kV air	Floors should be made of wood, concrete or ceramic tiles. If the floor is covered with synthetic material, the relative humidity must be at least 30 %.
Fast transient electrical disturbances, bursts according to IEC 61000-4-4	±2 kV for power cables ±1 kV for input and output lines	±2 kV for power cables ±1 kV for input and output lines	The quality of the supply voltage should be appropriate for a typical business- or hospital environment
Surges according to IEC 61000-4-5	±1 kV Voltage outer conductor - outer conductor ±2 kV Voltage outer conductor end	±1 kV Voltage outer conductor - outer conductor ±2 kV Voltage outer conductor end	The quality of the supply voltage should be appropriate for a typical business or hospital environment
Voltage dips, short interruptions and supply voltage fluctuations according to IEC 61000-4-11	0% U_T , ½ Period at 0, 45, 90, 135, 180, 225, 270, 315 Degree	0% U_T , ½ Period at 0, 45, 90, 135, 180, 225, 270, 315 Degree	The quality of the supply voltage should be appropriate for a typical business or hospital environment. If the user of the Bodystik -system requires continued operation even during power interruptions, it is recommended that the Bodystik be powered from an uninterruptible power supply or a battery.
Magnetic field at the supply frequency (50/60 Hz) to IEC 61000-4-8	30 A/m	30 A/m	Magnetic fields at the mains frequency should correspond to the typical values as found in the business and hospital environment.

12.4.3 Interference Resistance for Non-Life-Supporting ME Systems Guideline and Manufacturer Declaration

Guidelines and manufacturer's declaration – electromagnetic interference immunity			
The Bodystik is recommended for operation in an electromagnetic environment as specified below. The user / operator of the Bodystik should ensure that it is operated in this environment.			
Measurement of interference immunity	IEC 60601 -level	Compliance level	Electromagnetic environment - Guideline
			Portable and mobile RF communication devices should not be used at a shorter distance from the Bodystik as the recommended safety distance calculated according to the equation applicable to the transmission frequency.
Recommended safety distance:			
Conducted HF-disturbance variable IEC 61000-4-6	3 V Effective value 150 kHz to 80 MHz	$U_1 = 3 \text{ V}$	$d = \left[\frac{3.5}{U_1} \right] \sqrt{P}$
	6 V Effective value ISM-frequency bands: 6.765 MHz to 6.795 MHz 13.553 MHz to 13.567 MHz 26.957 MHz to 27.283 MHz 40.66 MHz to 40.70 MHz Amateur Radio frequency bands: 1.8 MHz to 2.0 MHz 3.5 MHz to 4.0 MHz 5.3 MHz to 5.4 MHz	$U_2 = 6 \text{ V}$	$d = \left[\frac{6}{U_2} \right] \sqrt{P}$

	7 MHz to 3 MHz 10.1 MHz to 10.15 MHz 14 MHz to 14.2 MHz 18.07 MHz to 18.17 MHz 21.0 MHz to 21.4 MHz 24.89 MHz to 24.99 MHz 28.0 MHz to 29.7 MHz 50 MHz to 54.0 MHz		
Radiated HF- disturbance according to IEC 61000-4-3	3 V/m 80 MHz to 2.7 GHz	$E_1 = 3 \text{ V/m}$	$d = \left\lceil \frac{3.5}{E_1} \right\rceil \sqrt{P}$ from 80 MHz up to 800 MHz
			$d = \left\lceil \frac{7}{E_1} \right\rceil \sqrt{P}$ from 800 MHz up to 2.7 GHz
	27 V/m, PM 18 Hz, 385 MHz	$E_2 = 27 \text{ V/m}$ PM 18 Hz	$d = \left\lceil \frac{6}{E_2} \right\rceil \sqrt{P}$
	28 V/m FM± 5 kHz Hub 1 kHz Sinus, 450 MHz	$E_3 = 28 \text{ V/m}$ FM± 5 kHz Hub 1 kHz Sinus	$d = \left\lceil \frac{6}{E_3} \right\rceil \sqrt{P}$
	9 V/m PM 217 Hz, 710 MHz, 745 MHz, 780 MHz	$E_4 = 9 \text{ V/m}$ PM 217 Hz	$d = \left\lceil \frac{6}{E_4} \right\rceil \sqrt{P}$
	28 V/m PM 18 Hz, 810 MHz, 870 MHz, 930 MHz	$E_3 = 28 \text{ V/m}$ PM 18 Hz	$d = \left\lceil \frac{6}{E_3} \right\rceil \sqrt{P}$
	28 V/m PM 217 Hz, 1720 MHz, 1845 MHz, 1970 MHz, 2450 MHz	$E_3 = 28 \text{ V/m}$ PM 217 Hz	$d = \left\lceil \frac{6}{E_3} \right\rceil \sqrt{P}$

9 V/m PM 217 Hz, 5240 MHz, 5500 MHz, 5785 MHz		$E_4 = 9 \text{ V/m}$ PM 217 Hz	$d = \left[\frac{6}{E_4} \right] \sqrt{P}$
			P is the maximum rated power of the transmitter in watts (W) according to the manufacturer's specifications and d is the recommended safety distance in meters (m) Field strengths from fixed RF transmitters should be less than the compliance level at all frequencies according to on-site investigations. Interference may occur in the environment of equipment marked with the following symbol: 
Note 1: The higher frequency range shall be used at 80 MHz and 800 MHz. Note 2: These guidelines may not be applicable in all cases. The propagation of electromagnetic parameters is influenced by absorptions and reflections from buildings, objects and people.			
a) The field strengths of stationary transmitters, such as base stations and mobile land-based radios, amateur radio stations, AM and FM radio and television transmitters, can theoretically not be predicted exactly. In order to determine the electromagnetic environment with regard to the stationary transmitters, a study of the electromagnetic phenomena of the site should be considered. If the measured field strength at the site where the Bodystik is used exceeds the abovementioned compliance levels, the Bodystik should be observed to demonstrate its intended function. If unusual performance characteristics are observed, additional measures may be required, such as a change in orientation or in location of the Bodystik. b) Over the frequency range from 150 kHz to 80 MHz, the field strengths should be less than 3 V/m.			

12.4.4 Recommended Safety Distances for Non-Life-Supporting ME Systems

Recommended safety distance between portable and mobile RF communication devices and the Bodystik

The **Bodystik** is determined for operation in an electromagnetic environment in which the RF disturbances are controlled. The user / operator of the **Bodystik** may help to avoid electromagnetic interference by keeping the minimum distance between portable and mobile RF telecommunication devices (transmitters) and the **Bodystik**, depending on the emitted power of the communication device as indicated below:

Power rating of the transmitter [W]	Safety distance, depending on the transmitter frequency [m]		
	150 kHz to 80 MHz	80 MHz to 800 MHz	800 MHz to 2.7 GHz
	$d = 1.17\sqrt{P}$	$d = 1.17\sqrt{P}$	$d = 2.33\sqrt{P}$
0.01	0.12	0.12	0.23
0.1	0.37	0.37	0.74
1	1.2	1.2	2.3
10	3.7	3.7	7.4
100	12	12	23

For transmitters whose maximum power rating is not given in the table above, the recommended safety distance d in meters (m) can be determined using the equations given with each column, where P is the maximum power rating of the transmitter in watts (W) as specified by the manufacturer.

Note 1: The higher frequency range shall be used at 80 MHz and 800 MHz.

Note 2: These guidelines may not be applicable in all cases. The propagation of electromagnetic parameters is influenced by absorptions and reflections from buildings, objects and people.

13 Safety of Product and Material

The manufacturer develops, produces and tests its products according to the essential requirements of Regulation (EU) 2017/745 (MDR)) and the safety standards of DIN EN 60601-1.

All materials which are used are carefully selected and correspond to the biocompatibility requirements (in accordance with ISO 10993-1 ff) and those of the RoHS directive 2011 / 65 / EU (RoHS II). All materials in contact with the patient were evaluated and tested according to DIN EN ISO 10993-1:2017-04 "Biological evaluation of medical devices" (biocompatibility).


Bodystik is a class IIa active medical device. Conformity with the underlying standards and directives is certified in the declaration of conformity which is included in the documentation accompanying the device.

14 Product Labeling / Type Label



The type label can be found on the outside of the cabin at the height of the Height-Adjustable Arm. See:

- Chap. 4.1.1 "Overview" point [9]

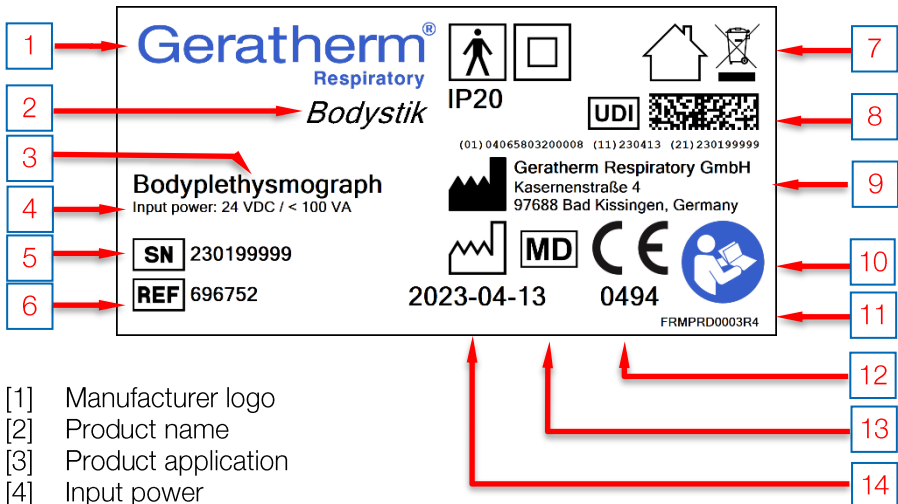

- [1] Manufacturer logo
- [2] Product name
- [3] Product application
- [4] Input power
- [5] Serial number
- [6] Catalog number
- [7] For symbol descriptions see chap 1.3 "Symbols".
- [8] Unique Device Identifier (UDI)
- [9] Manufacturer details
- [10] Follow the IFU
- [11] Type label revision indication
- [12] Conformity mark in accordance with the the Medical Device Regulation MDR 2017 / 745 with identification of the involved notified body
- [13] Medical Device
- [14] Date of manufacture

Safety symbols have been applied to the Bodystik type label. It may not be changed or removed. If information should become unreadable, the type label should be replaced immediately. Contact the manufacturer to do this.

15 Warranty and Service

15.1 General Conditions

The manufacturer guarantees that the products you have purchased fulfill the listed technical data and that the medical devices are free from technical material and production defects. This limited warranty is valid for 12 months from the date of purchase. During this time, the manufacturer declares that it will replace or repair defective products. The date of purchase corresponds to the delivery date if the product was purchased directly from us, or the date of installation if you purchased the device via a specialist retail partner.

All repairs to products which are covered by the warranty must be carried out by the manufacturer or by a specialist retail partner. All warranty claims expire if the repairs were unauthorised.

15.2 Warranty Exemption

The warranty does not cover damage which was caused by the following:

- Not complying with the storage or transportation conditions.
- Improper use, servicing or repair.
- Use of spare parts other than the original spare parts or spare parts approved by the manufacturer.
- Any technical changes to the device.
- Overvoltage or undervoltage.
- Installing and operating third-party software which has not been approved by the manufacturer.
- Connecting third-party devices which has not been approved by the manufacturer.
- Operating the device outside of the valid environmental conditions.

15.3 Packaging and Shipping

To avoid damage during transport, devices must be sent along with the warranty claim in the original packaging. This also applies for defective devices being repaired.

Transport damage arising from improper packing is the responsibility of the customer. In addition, insurance during transport is recommended. Claims due to loss or damage must be made by the shipper.

16 Authorised Specialist Retail Partner

You can reach your responsible specialist retail partner via a contact form of the manufacturer
www.geratherm-respiratory.com/login/

Attachment – Declaration of Conformity

The Bodystik declaration of conformity is enclosed with each device by the manufacturer.