

AB Tip İnceleme Sertifikası EU Type-Examination Certificate

Belge No / Certificate No

Belgelendirme Tarihi - Bir Sonraki Belge Tarihi /

Certification Date / Certificate Validity Date

Belge Geçerlilik Tarihi / Document Validity Period

Firma Unvanı ve Adresi /

Company Name and Address

: 92-20-03

: 25.12.2020-25.12.2025

: 5 yıl / 5 years

: FAGO MEDİKAL SAN. VE TİC. LTD. ŞTİ.

15 Temmuz Mah. Cami Yolu Cad. No:106 / Z1 Bağcılar/

İSTANBUL

Ürün Adı /Modeller / Product Name / Models

Direktifi / Directive

Modülü/Kategori / Module / Category

: FAGO S 101

: 2016/425 REGULATION

: B MODÜLÜ/ KATEGORİ III

MODULE B / CATEGORY III

Test Rapor No/ları / Test Report No : MNA M-2020-00576

Urün Tipi / Product Type:

 EN 149:2001+ A1:2009 Solunumla ilgili koruyucu cihazlar - Parçacıklara karşı koruma amaçlı filtreli yarım maskeler/ Respiratory protective devices - Filtering half masks to protect against particles

Ürünün Malzeme Bilgisi / Product Material Information: FAGO S 101 model ürünleri kumaş, kulak kayışı, burun klipsi ve filtre katmanı kullanılarak imal edilmiştir./ FAGO S 101 model products are manufactured using fabric, earloop, nose clip and filter layer.

Volkan AKIN 25.12.2020

Karar Verici / Approver

Okan AKEL 25.12.2020

Şirket Müdürü / General manager







MNA Laboratuvarları San. Tic.Ltd .Şti

Adres: Küçükbakkalköy Mahallesi Yenidoğan Cad.No:21 Ataşehir/İstanbul

Tel: 0216 574 07 08 Faks: 0216 575 13 31 www.mnalab.com




ATTACHMENTS (92-20-03)

To certify the PPE product at Category III level, C2 or D module is accompanied by applying one of the conformity assessment methods along with the EU Type Examination (Module B).

Model: FAGO S 101

PPE SPECIFICATION	PERFORMANCE LEVELS
Classification	FFP2
Reusable / Single Shift Use	NR

PPE produced as a single unit to fit an individual user, all the necessary instructions for manufacturing such PPE on the basis of the approved basic model:

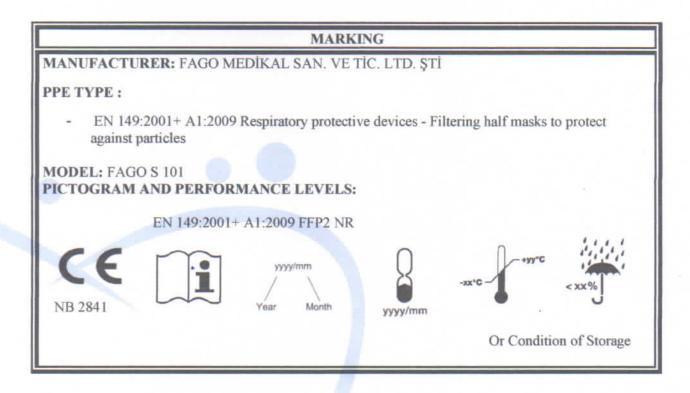


MNA LABORATORIES SAN. TIC. LTD. \$TI declares that the above-mentioned product meets the requirements of the directive according to the EU Directive 2016/425, the safety of the product is covered by the conditions and use specified in this certificate and in the technical file.

MNA Laboratuvarları San. Tic.Ltd .Şti
Adres: Küçükbakkalköy Mahallesi Yenidoğan Cad.No:21 Ataşehir/İstanbul
Tel: 0216 574 07 08 Faks: 0216 575 13 31 www.mnalab.com



ATTACHMENTS (92-20-03)

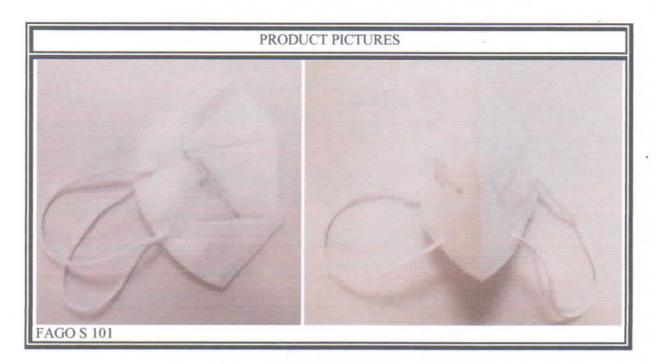

DOCUMENTS IN THE TECHNICAL

- Basic Health Safety Requirements
- Risk Assessment
- Test Reports
- Technical Report

MNA LABORATUVARLARI SAN. TIC. LTD. STI.

MNA LABORATUVARLARI

TECHNICAL EVALUATION REPORT (92-20-03)

Report No

: 92-20-03

Report Date

: 25.12.2020

Application No

: 92-20-03

1. COMPANY INFORMATION:

FAGO MEDIKAL SAN. VE TIC. LTD. ŞTİ.

15 Temmuz Mah. Cami Yolu Cad. No:106 / Z1 Bağcılar/ İSTANBUL

Tel: +90 532 388 44 44

E-mail: burak@unionmedikal.com


2. PPE INFORMATION:


Disposable and non-sterile half mask made of particulate protection filter material.

3. PPE TYPE IDENTIFICATION

EN 149:2001 +A1:2009 Respiratory protective devices - Filtering half masks to protect against particles - Requirements, testing, marking

4. PPE PICTURES



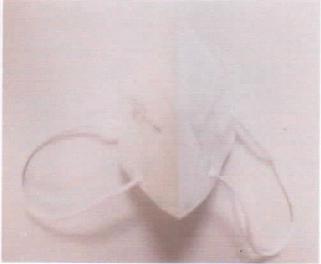

FAGO S 101

5. PPE DIMENSIONS:

FAGO S 101 model has been found to be produced using standard sizes.

6. PPE PRODUCT MATERIAL INFORMATION:

The product is made of elastic strap, nonwoven fabric on the outer and inner layers, filter material on the middle layer.

MNA LABORATUVARLARI



TECHNICAL EVALUATION REPORT (92-20-03)

7. ESSENTIAL HEALTH AND SAFETY REQUIREMENTS

- A visual inspection was made according to EN 149:2001 +A1:2009 for ergonomics.
- · Protection levels and degrees are defined by the manufacturer.
- Suitable construction materials were determined by visual inspection according to EN 149:2001 +A1:2009.
- Respiratory protective dimensions are evaluated according to EN 149:2001 +A1:2009.
- Conditioning EN 149:2001 +A1:2009 part 8.3, Penetration EN 149:2001 +A1:2009 part 8.11 (EN 13274-7), Application performance EN 149:2001 +A1:2009 part 8.4, Inward leakage EN 149:2001 +A1:2009 part 8.5, Flammability EN 149:2001 +A1:2009 part 8.6, The carbon dioxide content of the inhaled air EN 149:2001 +A1:2009 part 8.7, Inhalation resistance EN 149:2001 +A1:2009 part 8.9, Exhalation resistance EN 149:2001 +A1:2009 part 8.9 has been tested and evaluated.

8. ANALYSIS AND EVALUATIONS:

EN 149:2001 +A1:2009

TESTS PARAMETER	PARAMETER	PERFORMANCE LEVELS			RESULTS	PERFORMANCE LEVELS	EVALUATION
		FFP1	FFP2	FFP3			
Visual inspection	Shall also the markin supplied by the manu			mation	Appropriate	-	PASS
Total inward	At least 46 out of the 50 individual exercise result	<25	<11	<5	See the table below	FFP2	PASS
leakage	At least 8 out of the 10 individual wearer arithmetic means	<22	<8	<2	See the table below	FFP2	PASS

Total Inward Leakage (%)								
	Exercise 1	Exercise 2	Exercise 3	Exercise 4	Exercise 5	Average		
Subject 1 (As recieved)	4.6	4.9	4.8	5.4	4.7	4.9		
Subject 2 (As recieved)	5.4	5.3	4.7	4.8	5.5	5.1		
Subject 3 (As recieved)	4.9	5.3	4.9	4.9	4.9	5.0		
Subject 4 (As recieved)	4.8	4.9	4.8	5.4	5.5	5.1		
Subject 5 (As recieved)	5.4	4.7	4.9	5.0	4.9	5.0		
Subject 6 (After temperature conditioning)	4.9	4.9	4.8	5.4	4.8	5.0		
Subject 7 (After temperature conditioning)	5.5	5.0	5.1	6.0	6.2	5.6		
Subject 8 (After temperature conditioning)	5.5	5.2	5.5	4.7	4.7	5.1		
Subject 9 (After temperature conditioning)	4.9	4.8	4.9	4.6	4.9	4.8		
Subject 10 (After temperature conditioning)	5.0	4.9	4.7	4.8	4.8	4.8		

MNA LABORATUVARLARI SAN. TIC, LTD, STI.

MNA LABORATUVARLARI

TECHNICAL EVALUATION REPORT (92-20-03)

TESTS PARAMETER	PARAMETER	PERFORMANCE LEVELS			RESULTS	PERFORMANCE LEVELS	EVALUATION
	FFP1	FFP2	FFP3				
Flammibility	Mask shall not burn burn for more than 5	n or not to continue to			Flame not seen	-	PASS
Carbondioxide content of the inhalation air	Shall not exceed an av	erage o	f % 1		0,70 0,75 0,71	-	PASS
Penetration of filter material	Sodium chloride, 95 L/min %, max	% 20	% 6	%1	See the table below	FFP2	PASS .
	Paraffin oil, 95 L/min % 20 % 6 % 1 %, max				See the table below	FFP2	PASS

Penetration of filter material	Sodium Chloride (%)	Paraffin Oil (%)	
As recieved	3.6	2.8	
As recieved	3.3	3.2	
As recieved	3.5	3.0	
After the simulated wearing treatment	3.2	2.9	
After the simulated wearing treatment	3.6	2.6	
After the simulated wearing treatment	3.6	3.1	
Mechanical strength and temperature conditioning	3.4	3.1	
Mechanical strength and temperature conditioning	3.0	3.0	
Mechanical strength and temperature conditioning	3.5	3.2	

TESTS PARAMETER		PERFORMANCE LEVELS			RESULTS	PERFORMANCE LEVELS	EVALUATION
	FFP1	FFP2	FFP3				
Compatibility with skin	Materials shall not be cause irritation or an to health			100	Appropriate	-	PASS
Head harness	It can be donned and	removed easily			Appropriate	*	PASS
Breathing Resistance	Inhalation 30L/min	0,6 mbar	0,7 mbar	1 mbar	See the table below	FFP2	PASS
	Inhalation 95L/min	2,1 mbar	2,4 mbar	3 mbar	See the table below	FFP2	PASS
	Exhalation 160L/min 3 3 3 mbar mbar mbar				See the table below	FFP2	PASS

Breathing Resistance (mbar)	Inhalation 30L/min (mbar)	Inhalation 95L/min (mbar	
As recieved	0.5	1.9	
As recieved	0.5	1.9	
As recieved	0.4	1.8	



MNA LABORATUVARLARI

TECHNICAL EVALUATION REPORT (92-20-03)

After temperature conditioning	0.4	1.8
After temperature conditioning	0.4	1.9
After temperature conditioning	0.5	1.9
After the simulated wearing treatment	0.4	1.8
After the simulated wearing treatment	0.4	1.9
After the simulated wearing treatment	0.5	1.9
After the flow conditioning	0.9	2.3
After the flow conditioning	0.9	2.4
After the flow conditioning	0.9	2.4

Breathing Resistance 160L/min (mbar)	Facing directly ahead	Facing vertically upwards	Facing vertically downwards	Lying on the left side	Lying on the right side
As recieved	2,0	2,0	2,0	2,0	2,0
As recieved	1,9	2,0	2,0	2,0	2,0
As recieved	2,0	2,0	2,0	2,0	2,0
After temperature conditioning	1,9	2,0	1,9	2,0	2,0
After temperature conditioning	1,9	2,0	2,0	1,9	2,0
After temperature conditioning	1,9	2,0	2,0	2,0	2,0
After the simulated wearing treatment	1,9	1,9	1,9	2,0	2,0
After the simulated wearing treatment	2,0	2,0	1,9	1,9	1,9
After the simulated wearing treatment	2,0	2,0	2,0	2,0	2,0

9. DECISION PROPOSAL

Analysis and examinations FAGO S 101 model coded personal protective equipment; Respiratory Protective Devices EN 149:2001 +A1:2009- Filtered Half Masks for Protection Against Particles - Properties, Experiments and Marking standards are evaluated. It is recommended to be certified at the performance levels specified as a result of technical evaluations.

10. ATTACHMENTS

- Basic Health Safety Requirements
- Risk Assessment
- Test Reports
- User Instruction

CONTROLLER

VOLKAN AKIN

SING

DATE

: 25.12.2020