




Certificate of Conformity

KIT : **Oxytetracycline ELISA Kit RND99049**

Release Date: Oct.9th ,2019
 Expiration Date: Oct/2020 Temperature: 25°C

REAGEN LLC certifies that this lot has passed Quality control assays and conforms to product release specifications.

Standards	Rep. #1	Rep. #2	Rep.#3	Avg.	Std. Dev.	%RSD	%Bo
Negative Control	2.063	2.083	2.048	2.065		0.9	100%
0.5 ppb Calibrator	1.883	1.887	1.865	1.878	0.0	0.6	90.9%
1 ppb Calibrator	1.528	1.536	1.549	1.538	0.0	0.7	74.5%
2 ppb Calibrator	1.010	1.053	0.999	1.021	0.0	2.8	49.4%
4 ppb Calibrator	0.536	0.558	0.542	0.545	0.0	2.1	26.4%
8 ppb Calibrator	0.258	0.239	0.261	0.253	0.1	4.7	12.3%

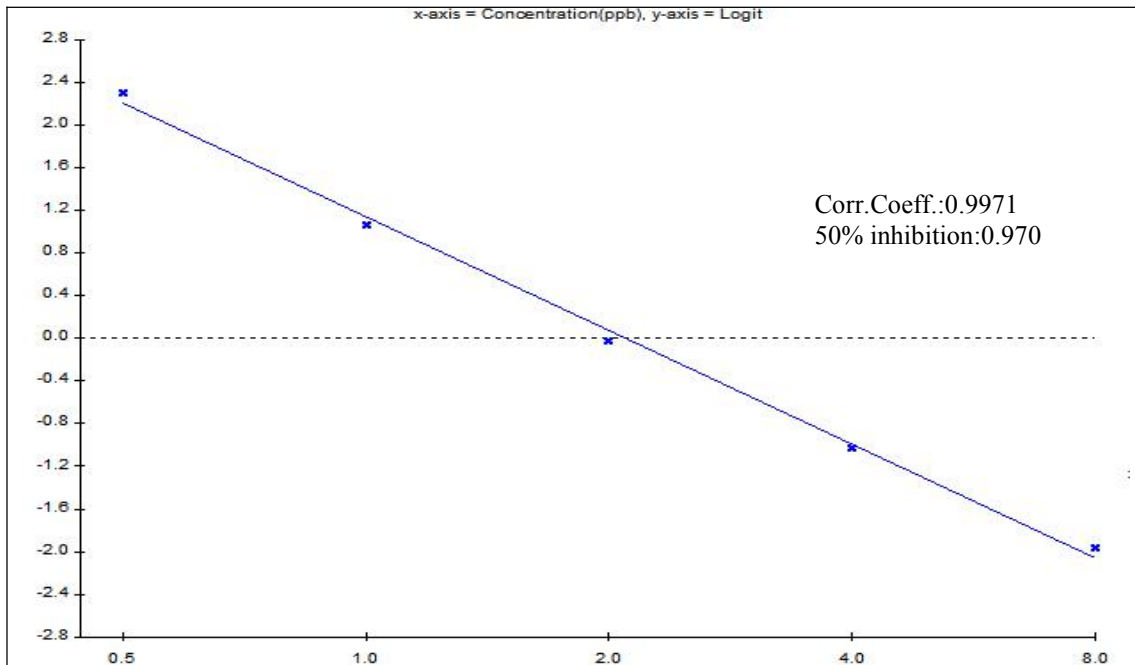

Note: The absorbance of the calibrators may Decrease during the shelf life of kit . Actual values may vary; this data is for example purposes only.

QA Manager Alexis Release Date Oct.9th ,2019

