



**Clinical • Food&Feed Safety**

## **Oxytetracycline ELISA Test Kit Manual**



**REAGEN LLC**

Add.: 102CommerceDr.Unit8, Moorestown, NJ08057  
Tel.: 856-727-0250 Fax.: 856-727-0251  
E-mail: reagenkits@gmail.com reagenllc@gmail.com  
Web.: www.reagen.us

REAGEN FOOD AND FEED SAFETY • [WWW.REAGEN.US](http://WWW.REAGEN.US)

**REAGEN**



## TABLE OF CONTENTS

<b>GENERAL INFORMATION.....</b>	<b>2</b>
Product Description.....	2
The unique features of the kit are:.....	2
Procedure Overview.....	2
Kit Contents, Storage and Shelf Life.....	2
Detection Limit Of Quantitation.....	3
Specificity (Cross-Reactivity).....	3
Required Materials Not Provided With the Kit.....	3
Warnings and Precautions.....	4
<b>SAMPLE PREPARATION.....</b>	<b>5</b>
Feed.....	5
Cheese/Egg/Sour Cream.....	5
Honey.....	5
Meat/Meat ProductsFish/Shrimp/Butter.....	6
Milk/Yogurt/Curd.....	6
Milk Powder.....	6
<b>OXYTETRACYCLINE ELISA TEST KIT PROTOCOL.....</b>	<b>7</b>
Reagent Preparation.....	7
ELISA Testing Protocol.....	7
Concentration Calculations.....	8
<b>TROUBLESHOOTING.....</b>	<b>10</b>
No Color Development or No Signals with Standards.....	10
Low Optical Density (OD) Readings.....	10
High Background or High Optical Density (OD) Readings.....	10
High Intra-Plate Variance.....	11
High Inter-Plate Variance.....	11
One or More of the Standard Curve Points Are Out of Range.....	11



## Oxytetracycline ELISA Test Kit- RND99049

### ➤ GENERAL INFORMATION

#### Product Description

**REAGEN™** Oxytetracycline ELISA Test Kit is a competitive enzyme immunoassay for the quantitative analysis of Oxytetracycline in honey, butter, whey, egg, cheese, milk, meat, meat products such as sausage, fish and shrimp.

#### The unique features of the kit are:

- High recovery (75-120%), rapid , and cost-effective extraction methods.
- High reproducibility.
- A quick ELISA assay (less than 2 hours regardless of number of samples).

#### Procedure Overview

**REAGEN™** Oxytetracycline ELISA Test Kit is based on a competitive colorimetric ELISA assay. The drug of interest has been coated in the plate wells. During the analysis, sample is added along with the primary antibody specific for the target drug. If the target is present in the sample, it will compete for the antibody, thereby preventing the antibody from binding to the drug attached to the well. The secondary antibody, tagged with a peroxidase enzyme, targets the primary antibody that is complexed to the drug coated on the plate wells. The resulting color intensity, after addition of substrate, has an inverse relationship with the target concentration in the sample.

#### Kit Contents, Storage and Shelf Life

**REAGEN™** Oxytetracycline ELISA Test Kit has the capacity for 96 determinations or testing of 42 samples in duplicate (assuming 12 wells for standards). Return any unused microwells to the foil bag and reseal them with the desiccant provided in the original package. Store the kit at 2-8°C . The shelf life is 12 months when the kit is properly stored

Kit Contents	Amount	Storage
Oxytetracycline-Coated Plate	1 x 96-well plate (8 wells x 12 strips)	2-8°C
Oxytetracycline Standards: Negative control (white Cap tube)	0.2 mL	2-8°C
2ng/mL (yellow Cap tube)	0.2 mL	

### Oxytetracycline ELISA Test Kit- RND99049

4 ng/mL (orange Cap tube)	0.2 mL	
8 ng/mL (pink Cap tube)	0.2 mL	
16 ng/mL (purple Cap tube)	0.2 mL	
64 ng/mL (blue Cap tube)	0.2 mL	
200ng/mL (Spiking red Cap tube)	1 mL	
Oxytetracycline Antibody #1	6mL	2-8°C
HRP-Conjugated Antibody #2	12mL	
20X Wash Solution	30mL	
Stop Buffer	12mL	
30X Sample Dilution	30mL	
TMB Substrate	12mL	

\* If you are not planning to use the kit for over 1 month, storing Oxytetracycline Standard Stock, Oxytetracycline Antibody #1 and HRP-Conjugated Antibody #2 at  $-20^{\circ}\text{C}$  or in a freezer is recommended.

### Detection Limit Of Quantitation

Sample Type	Limit Of Quantitation (ng/g)
Egg/Cheese/Sour Cream	0.8
Honey	0.8
Meat/Meat Products Fish/Shrimp/Butter	1.6
Reconstituted Milk Powder	0.8
Milk/Yogurt/Curd/Feed	2

### Specificity (Cross-Reactivity)

Analytes	Cross-Reactivity (%)
Oxytetracycline	100
Chlortetracycline	180
Tetracycline	180
Doxycycline	110

### Required Materials Not Provided With the Kit

1. Microtiter plate reader (450 nm)

2. Vortex mixer, (e.g. Gneie Vortex mixer from VWR)
3. 10, 20, 100 and 1000  $\mu$ L pipettes
4. Multi-channel pipette: 50-300  $\mu$ L (Optional)

### **Warnings and Precautions**

1. The standards contain Oxytetracycline. Handle with particular care.
2. Do not use the kit past the expiration date.
3. Do not intermix reagents from different kits or lots except for components with the same part No's within their expiration dates. ANTIBODIES AND PLATES ARE KIT-AND LOT-SPECIFIC.
4. Try to maintain a laboratory temperature of 20–25°C (68°–77°F). Avoid running assays under or near air vents, as this may cause excessive cooling, heating and/or evaporation. Also, do not run assays in direct sunlight, as this may cause excessive heat and evaporation. Cold bench tops should be avoided by placing several layers of paper towel or some other insulation material under the assay plates during incubation.
5. Make sure you are using only distilled or deionized water since water quality is very important.
6. When pipetting samples or reagents into an empty microtiter plate, place the pipette tips in the lower corner of the well, making contact with the plastic.
7. Incubations of assay plates should be timed as precisely as possible. Be consistent when adding standards to the assay plate. Add your standards first and then your samples.
8. Add standards to plate only in the order from low concentration to high concentration as this will minimize the risk of compromising the standard curve.
9. Always refrigerate plates in sealed bags with a desiccant to maintain stability. Prevent condensation from forming on plates by allowing them equilibrate to room temperature (20 – 25°C / 68 – 77°F) while in the packaging.

## ➤ SAMPLE PREPARATION

Be sure samples are properly stored. In general, samples should be refrigerated at 2-4°C for no more than 1-2 days. Freeze samples to a minimum of -20°C if they need to be stored for a longer period. Frozen samples can be thawed at room temps (20 – 25°C / 68 – 77°F) or in a refrigerator before use.

### 1 . Preparation of 1X Sample Dilution

Mix 1 volume of 30X Sample Dilution with 29 volumes of distilled water.

### 2 . Preparation of 2X Sample Dilution

Mix 1 volume of 30X Sample Dilution with 14volumes of distilled water

### Feed

1. Take 1 g of feed sample, add 5mL of 1X Sample Dilution.
2. Vortex samples for 5 minutes using a multi-vortexer.
3. Centrifuge for 10 minutes at 4,000 x g.
4. Transfer 500µL of clear supernatant to a new tube containing 500µL of 1X Sample Dilution.
5. Vortex samples for 1 minute.
6. Use 100 µ L of the sample for the assay.

**Note:** Dilution factor: 10

### Cheese/Egg/Sour Cream

1. Add 3mL of 2X Sample Dilution to 1 g of sample, vortex for 5 minutes in a multi-tube vortexer or shake 30 minutes on a shaker.
2. Centrifuge for 5 min at 4000 rpm.
3. Use 100 µL per well in the assay.

**Note:** Dilution factor: 4

### Honey

1. Weigh out 1 g of honey in a centrifuge vial.
2. Add 3mL 2X Sample Dilution .
3. Vortex for 5 minutes in a multi-tube vortexer or shake 15 minutes on a shaker.
4. Centrifuge for 5 min at 4000 rpm
5. Use 100 µL of the sample for the assay.

**Note:** Dilution factor: 4.

**Meat/Meat Products/Fish/Shrimp/Butter**

1. To 1 g of homogenized sample, add 3 mL of 1X Sample Dilution.
2. Vortex for 5 minutes in a multi-tube vortexer or shake 15 minutes on a shaker.
3. Centrifuge for 5 minute at 4,000 x g.
4. Transfer 500  $\mu$  L of the supernatant to a new tube containing 500  $\mu$  L of distilled water.
5. Vortex for 1 minute.
6. Use 100  $\mu$  L per well in the assay.

**Note:** Dilution factor: 8

**Milk/Yogurt/Curd**

1. To 1 g of sample (or 1mL of liquid sample), Vortex for 5 minutes in a multi-tube vortexer or shake 15 minutes on a shaker. To 0.1 g of sample (or 0.1mL of liquid sample) add 0.9mL of distilled water.
2. Vortex for 5 minutes in a multi-tube vortexer or shake 15 minutes on a shaker.
3. Use 100  $\mu$  L per well in the assay.

**Note:** Dilution factor: 10

**Milk Powder**

1. Reconstitute 1 g of dry milk powder with 10mL of deionized or distilled water. Mix well.
2. Use this solution as the starting sample.
3. To 1mL of sample, add 3mL of 2X Sample Dilution.
4. Vortex for 5 minutes in a multi-tube vortexer or shake 15 minutes on a shaker.
5. Use 100  $\mu$  L per well in the assay.

**Note:** Dilution factor: 4

**➤ OXYTETRACYCLINE ELISA TEST KIT PROTOCOL****Reagent Preparation**

IMPORTANT: All reagents should be brought up to room temperature before use (1 – 2 hours at 20 – 25°C / 68 – 77°F); Make sure you read “Warnings and Precautions” section. Solutions should be prepared just prior to ELISA test. All reagents should be mixed by gently inverting or swirling prior to use. Prepare volumes that are needed for the number of wells being run. Do not return the reagents to the original stock tubes/bottles. Using disposable reservoirs when handling reagents can minimize the risk of contamination and is recommended.

**Preparation of 1X Wash Solution**

Mix 1 volume of the 20X Wash Solution with 19 volumes of distilled water.

**Preparation of 1X Standards**

Mix 50 µL of the Standards with 450 µL of 1X Sample Dilution.

**Special Notes for Optimal ELISA Performance**

- 1) Allow the entire kit to equilibrate at room temperature for at least two hours before starting any ELISA assay.
- 2) Avoid light as much as possible during sample preparation and ELISA assay.
- 3) For plate washing steps: after addition of 250 µL wash buffer to the wells, incubate the plate for 20 – 30 seconds; shake the plate gently before pouring out the wash buffer. Repeat this procedure for each of the 4 washes.
- 4) Pipette all reagents and samples very accurately, especially the samples, even if you must slow down while pipetting.

**ELISA Testing Protocol**

Label the individual strips that will be used and aliquot reagents as the following example:

Component	Volume per Reaction	24 Reactions
Oxytetracycline Antibody #1	50µL	1.2 mL
HRP-Conjugated Antibody #2	100µL	2.4 mL
1X Wash Solution	2.5 mL	60 mL
Stop Buffer	100 µL	2.4 mL
TMB Substrate	100 µL	2.4 mL



---

**Oxytetracycline ELISA Test Kit- RND99049**

---

1. Add 100  $\mu$ L of each Tetracycline Standards (0, 0.2, 0.4, 0.8, 1.6, 6.4ppb) in duplicate into different wells ( Add standards to plate only in the order from low concentration to high concentration).
2. Add 100 $\mu$ L of each sample in duplicate into different sample wells.
3. Add 50  $\mu$ L of Antibody #1 and mix well by gently rocking the plate manually for 1 minute.
4. Incubate the plate for 30minutes at room temperature (20 – 25°C / 68 – 77°F).
5. Wash the plate 4 times with 250  $\mu$ L of 1X Wash Solution. After the last wash, invert the plate and gently tap the plate dry on paper towels ( Perform the next step immediately after plate washings. Do not allow the plate to air dry between working steps).
6. Add 100 $\mu$ L of 1X Antibody #2 solution. Incubate the plate for 30 minutes at room temperature (20 – 25°C / 68 – 77°F) ( Avoid direct sunlight and cold bench tops during the incubation. Covering the microtiter plate while incubating is recommended).
7. Wash the plate 4 times with 250 of  $\mu$ L 1X Wash Solution. After the last wash, invert the plate and gently tap the plate dry on paper towels ( Perform the next step immediately after plate washings. Do not allow the plate to air dry between working steps).
8. Add 100  $\mu$ L of TMB Substrate to each well. Time the reaction immediately after adding the substrate. Mix the solution by gently rocking the plate manually for 1 minute while incubating , Incubate the plate for 15 minutes at room temperature (20 – 25°C / 68 – 77°F). ( Do not put any substrate back to the original container to avoid any potential contamination. Covering the microtiter plate while incubating is recommended).
9. After incubating,add 100  $\mu$ L of Stop Buffer to stop the enzyme reaction.
10. Read the plate as soon as possible following the addition of Stop Buffer on a plate reader with 450 nm wavelength ( Before reading, use a lint-free wipe on the bottom of the plate to ensure no moisture or fingerprints interfere with the readings).

**Concentration Calculations**


A standard curve can be constructed by plotting the mean relative absorbance (%) obtained from each reference standard against its concentration in ng/mL on a Logarithm curve.

## Oxytetracycline ELISA Test Kit- RND99049

$$\text{Relative absorbance (\%)} = \frac{\text{absorbance standard (or sample)} \times 100}{\text{absorbance zero standard}}$$

When use computing software, recommends Log/Log standard curves.

The following figure is a typical Oxytetracycline standard curve.

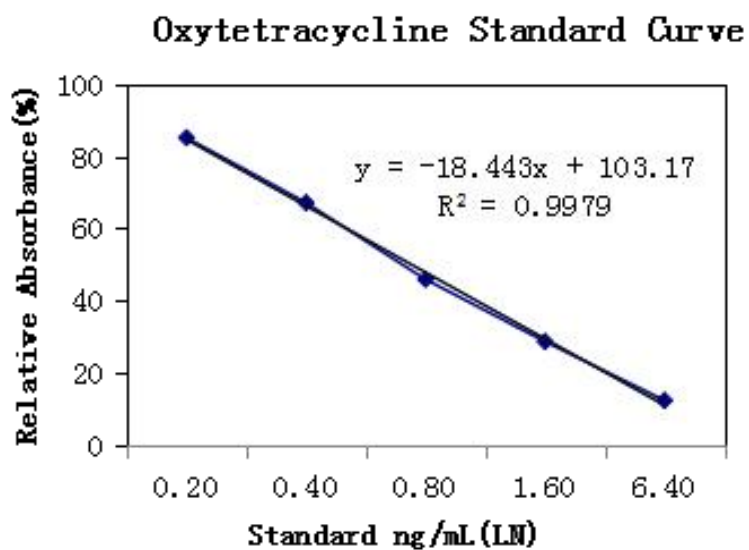

## ➤ TROUBLESHOOTING

### *No Color Development or No Signals with Standards*

Possible Causes	Recommended Action
<i>Reagents were used in the wrong order or a step was skipped.</i>	Follow the protocol carefully and repeat the assay.
<i>Wrong antibodies were used or antibodies have deteriorated.</i>	Make sure that the antibodies used are the ones that came with the kit. All antibodies are kit- and lot-specific.
<i>TMB substrate has deteriorated.</i>	Use a new set of REAGEN TMB substrate.

### *Low Optical Density (OD) Readings*

Possible Causes	Recommended Action
<i>Reagents were expired or mixed with a different lot number.</i>	Verify the expiration dates and lot numbers.
<i>Wash solution was prepared incorrectly.</i>	Use the wash solution for the kit and that make sure it is prepared correctly.
<i>Too many wash cycles were used.</i>	Make sure to use the number of washes per the protocol instruction.
<i>Incubation times were too short.</i>	Time each plate separately to ensure accurate incubation times, follow protocol.
<i>Lab temperature was too low.</i>	Maintain the lab room temperature within 20°–25°C (68°–77°F). Do not run assays under air conditioning vents or near cold windows.
<i>Reagents and plates were too cold.</i>	Make sure plates and reagents are brought up to room temperature. Keep the kit components out of the kit box for at least 1 hour before starting the assay.
<i>Reader was at wrong wavelength, or reader was malfunctioning.</i>	Make sure the wavelength is 450 nm for the assay and read the plate again. Verify reader calibration and lamp alignment.
<i>Excessive kit stress has occurred.</i>	Check records to see how many times the kit has cycled from the refrigerator. Check to see if the kit was left at extreme temperatures for too long.
<i>Assay plates were compromised.</i>	Always refrigerate plates in sealed bags with a desiccant to maintain stability. Prevent condensation from forming on plates by allowing them equilibrate to room temperature (20 – 25°C / 68 – 77°F) while in the packaging.

### *High Background or High Optical Density (OD) Readings*

Possible Causes	Recommended Action
<i>Poor quality water was used in wash solution.</i>	If water quality is questionable, try substituting an alternate distilled water source to prepare the wash solution.
<i>Substrate solution has deteriorated.</i>	Make sure the substrate is colorless prior to addition to the plate.
<i>There was insufficient washing or poor washer performance.</i>	Use the number of washes per the protocol instruction. Make sure that at least 250 µL of wash solution is dispensed per well per wash. Verify the performance of the washer system; have the system repaired if any ports drip, dispense or aspirate poorly.

## Oxytetracycline ELISA Test Kit- RND99049

<i>Reader was malfunctioning or not blanked properly. This is a high possibility if the OD readings were high and the color was light.</i>	Verify the reader's performance using a calibration plate and check the lamp alignment. Verify the blanking procedure, if applicable, and reblank.
<i>Lab temperature was too high.</i>	Maintain the room temperature within 20°–25°C (68°–77°F). Avoid running assays near heat sources or in direct sunlight.
<i>Reagents were intermixed, contaminated or prepared incorrectly.</i>	Ensure that the correct reagents were used, that working solutions were prepared correctly and that contamination has not occurred.

### ***High Intra-Plate Variance***

<b>Possible Causes</b>	<b>Recommended Action</b>
<i>Inconsistent time was taken when adding standards, reagents or samples to the assay plate.</i>	Make sure all materials are set up and ready to use. Use a multichannel pipette to add reagents to multiple wells whenever possible. Do not interrupt while adding standards, reagents and samples.
<i>Multichannel pipette was not functioning properly.</i>	Verify pipette calibration and check that tips are on tight. Be sure all channels of the pipette draw and dispense equal volumes.
<i>There was inconsistent washing or washer system malfunctioning.</i>	Check performance of the wash system. Have the system repaired if any ports drip or dispense/aspirate poorly.

### ***High Inter-Plate Variance***

<b>Possible Causes</b>	<b>Recommended Action</b>
<i>Inconsistent incubation times occurred from plate to plate.</i>	Time each plate separately to ensure consistent incubation times.
<i>Inconsistent washing occurred from plate to plate.</i>	Make sure to use the number of washes per the protocol instruction. Verify performance of the wash system and have the system repaired if any ports drip or dispense/ aspirate poorly.
<i>Pipette was working improperly.</i>	Check the pipette calibration. Verify that pipette tips are on tight before use and that all channels draw and dispense equal volumes.
<i>Kit plates, reagents, standards and samples were at different temperatures.</i>	Make sure to allow sufficient time for kit plates, reagents, standards and samples come to room temperature (20 – 25°C / 68 – 77°F). Larger volumes will require longer equilibration time. If using a water bath to hasten equilibration, make sure it is maintained at room temperature; do not use a warm water bath to warm reagents, samples and kit standards.
<i>Reagents used were intermixed from different kit lots, or the kits were of different expiration dates.</i>	Carefully label each reagent to make sure the reagents are not intermixed. Kits with different expiration dates might generate different range of OD readings, however, the relative absorbance values may very well be comparable. In general, a value of less than 0.6 in zero standard reading may indicate certain degrees of deterioration of reagents.

### ***One or More of the Standard Curve Points Are Out of Range***

<b>Possible Causes</b>	<b>Recommended Action</b>
<i>Standards were added in wrong order or recorded in wrong position.</i>	Follow the protocol and re-run the assay. Make sure the standards are applied and recorded correctly.
<i>Standards were</i>	<i>Use a new set of standards. Add standards to plate only in the</i>

### Oxytetracycline ELISA Test Kit- RND99049

<i>contaminated or intermixed with other standards.</i>	order from low concentration to high concentration.
<i>There was inconsistent washing or washer system malfunctioning.</i>	Perform washing consistently. Check performance of the wash system. Have the system repaired if any ports drip or dispense/aspirate poorly.
<i>Inconsistent time was taken to add standards and reagents to plate.</i>	Make sure all materials are set up and ready to use. Add standards to plate only in the order from low concentration to high concentration at uninterrupted pace. Use a multichannel pipette to add reagents to multiple wells simultaneously.
<i>Multichannel pipette was not functioning properly.</i>	Verify pipette calibration and check that tips are on tight. Be sure all channels of the pipette draw and dispense equal volumes.