



Home » Products » Interventional Product » Introducer Sets



## Introducer Sets

· The introducer set is intended for percutaneous introduction of guide wire or catheter into the vascular system through introducer needle. The introducer set should be used only by physicians trained in percutaneous, intravascular techniques and procedures.


INQUIRY

## FEATURES

• Comparing with other manufacturers, the special cutting method design of the valve ensures less blood leak in the case of continuous pumping;



- Hydrophilic coating sheath entering skin tissues greatly reduces the possibility of transradial muscle tension in the patient, thereby avoiding prolonged surgery;
- Smooth transition between the dilator and sheath;
- Small OD and large ID minimizes the size ( compromising ease of device passage );
- Seamless guide wire to dilator and dilator to reduce the risks of gaps and arterial damage;
- \* We can supply kink resistance nitinol guide wire to increase clinician confidence.

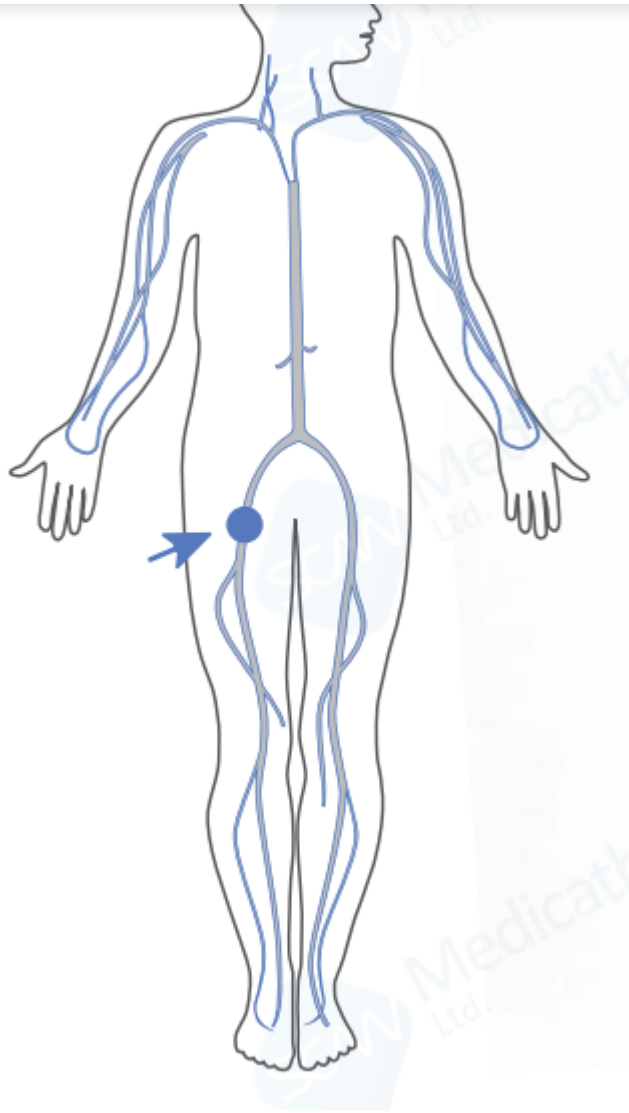



# CONTENTS

Femoral Introducer Sheath+ dilator

Syringe

Guide Wire

Introducer Needle

Scapel

## PRODUCT QUICK LOOK

Product at a glance -



# PARAMETER



Product No.	Size(Fr.)	Length(cm)	Guidewire	Introducer Needle
42.09.10000	4	9	0.021"*45cm J	20G*3.8cm
42.09.10001	5	11	0.038"*45cm J	18G*6.5cm
42.09.10002	6	11	0.038"*45cm J	18G*6.5cm
42.09.10003	7	11	0.038"*45cm J	18G*6.5cm
42.09.10004	8	11	0.038"*45cm J	18G*6.5cm
42.09.10005	9	11	0.038"*45cm J	18G*6.5cm
42.09.10006	10	11	0.038"*45cm J	18G*6.5cm
42.09.10007	4	19	0.021"*60cm J	20G*3.8cm
42.09.10008	5	23	0.038"*60cm J	18G*6.5cm
42.09.10009	6	23	0.038"*60cm J	18G*6.5cm
42.09.10010	7	23	0.038"*60cm J	18G*6.5cm
42.09.10011	8	23	0.038"*60cm J	18G*6.5cm



CLICK TYPE-Ter				
Product No.	Size(Fr.)	Length(cm)	Guidewire	Introducer Needle
42.09.20000	4	9	0.021"*45cm J	20G X 3.8 cm
42.09.20001	5	11	0.038"*45cm J	18G*6.5cm
42.09.20002	6	11	0.038"*45cm J	18G*6.5cm
42.09.20003	7	11	0.038"*45cm J	18G*6.5cm
42.09.20004	8	11	0.038"*45cm J	18G*6.5cm
42.09.20005	4	19	0.021"*60cm J	20G*3.8cm
42.09.20006	5	23	0.038"*60cm J	18G*6.5cm
42.09.20007	6	23	0.038"*60cm J	18G*6.5cm
42.09.20008	7	23	0.038"*60cm J	18G*6.5cm
42.09.20009	8	23	0.038"*60cm J	18G*6.5cm



Product No.	Size(Fr.)	Length(cm)	Guidewire	Introducer Needle
42.09.30000	4	9	0.021"*45cm J	20G X 3.8 cm
42.09.30001	5	11	0.038"*45cm J	18G*6.5cm
42.09.30002	6	11	0.038"*45cm J	18G*6.5cm
42.09.30003	7	11	0.038"*45cm J	18G*6.5cm
42.09.30004	4	19	0.021"*60cm J	20G*3.8cm
42.09.30005	5	23	0.038"*60cm J	18G*6.5cm
42.09.30006	6	23	0.038"*60cm J	18G*6.5cm
42.09.30007	7	23	0.038"*60cm J	18G*6.5cm

## CE CERTIFICATION





**Manufacturer:**

**SCW MEDICATH LTD.**

NO.4, Baolong 6th Road, Baolong Industrial  
Town, Longgang District, Shenzhen,  
518116, Guangdong, P.R. China

We, the manufacturer, herewith declare that the products

**whose single Authorized Representative:**

**OBELIS S.A.**

Bd. Général Wahis 53  
1030 Brussels, Belgium

**Introducer Sets**

Models: Standard introducer set, Peelable introducer set

meet the provisions of Directive 93/42/EEC which apply to them.

The medical device has been assigned to class IIa according to Annex IX Rule 6 of the  
Directive 93/42/EEC. It bears the mark

CE 0197

The product concerned has been manufactured under a quality management system  
according to Annex II of Directive 93/42/EEC.

Compliance of the designated product with the Directive 93/42/EEC has been assured via  
assessment of the quality management system by the Notified Body

**TÜV Rheinland LGA Products GmbH**

Tillystraße 2  
90431 Nürnberg  
Deutschland

Certificate No.: HD 60144232 0001

Issue date: 26.05.2020

Expiry date: 26.05.2024

following the procedure relating to the EC Declaration of Conformity set out in Annex II of  
Directive 93/42/EEC.

This Declaration of conformity is valid in connection with the release document for the  
respective batch of produced devices.

The above mentioned declaration of conformity is exclusively under the responsibility of

**SCW MEDICATH LTD.**

NO.4, Baolong 6<sup>th</sup> Road, Baolong Industrial Town,  
Longgang District, Shenzhen, 518116, Guangdong, P.R. China



Shenzhen, 2020/07/16

Place, date

Miriam Xie, RA

Legally binding signature, Function