

NO.2 SWING ROTOR

 Capacity:6x2X1000ml Max speed:4200rpm Max RCF:5900xg	Adapter:6x72x0.2ml		Adapter:6x72x0.5ml		Adapter:6x50x1.5/2.2ml	
	Adapter:6x30x5ml		Adapter:6x26x10ml		Adapter:6x26x15ml	
	Adapter:6x18x20ml		Adapter:6x16x30ml		Adapter:6x10x50ml	
	Adapter:6x6x100ml		Adapter:6x2x250ml		Adapter:6x2x300ml	
	Adapter:6x2x500ml		Adapter:6x48x2ml(75mm) (vacuum blood collection tube)		Adapter:6x48x5ml(100mm) (vacuum blood collection tube)	

NO.3 SWING ROTOR

 Capacity:6x2400ml Max speed:4600rpm Max RCF:7060xg	Adapter:6x71x0.2ml		Adapter:6x71x0.5ml		Adapter:6x47x1.5/2.2ml	
	Adapter:6x33x5ml		Adapter:6x27x10ml		Adapter:6x27x15ml	
	Adapter:6x20x20ml		Adapter:6x14x30ml		Adapter:6x11x50ml	
	Adapter:6x4x100ml		Adapter:6x2x250ml		Adapter:6x2x300ml	
	Adapter:6x500ml		Adapter:6x46x2ml(75mm) (vacuum blood collection tube)		Adapter:6x46x5ml(100mm) (vacuum blood collection tube)	


NO.4 SWING ROTOR

 Capacity:6x2000ml Max speed:4200rpm Max RCF:6045xg	Adapter:6x68x0.2ml		Adapter:6x68x0.5ml		Adapter:6x45x1.5/2.2ml	
	Adapter:6x28x5ml		Adapter:6x22x10ml		Adapter:6x22x15ml	
	Adapter:6x19x20ml		Adapter:6x14x30ml		Adapter:6x9x50ml	
	Adapter:6x5x100ml		Adapter:6x250ml		Adapter:6x300ml	
	Adapter:6x500ml		Adapter:6x42x2ml(75mm) (vacuum blood collection tube)		Adapter:6x42x5ml(100mm) (vacuum blood collection tube)	



BW12R

湖南柏威科学仪器有限公司

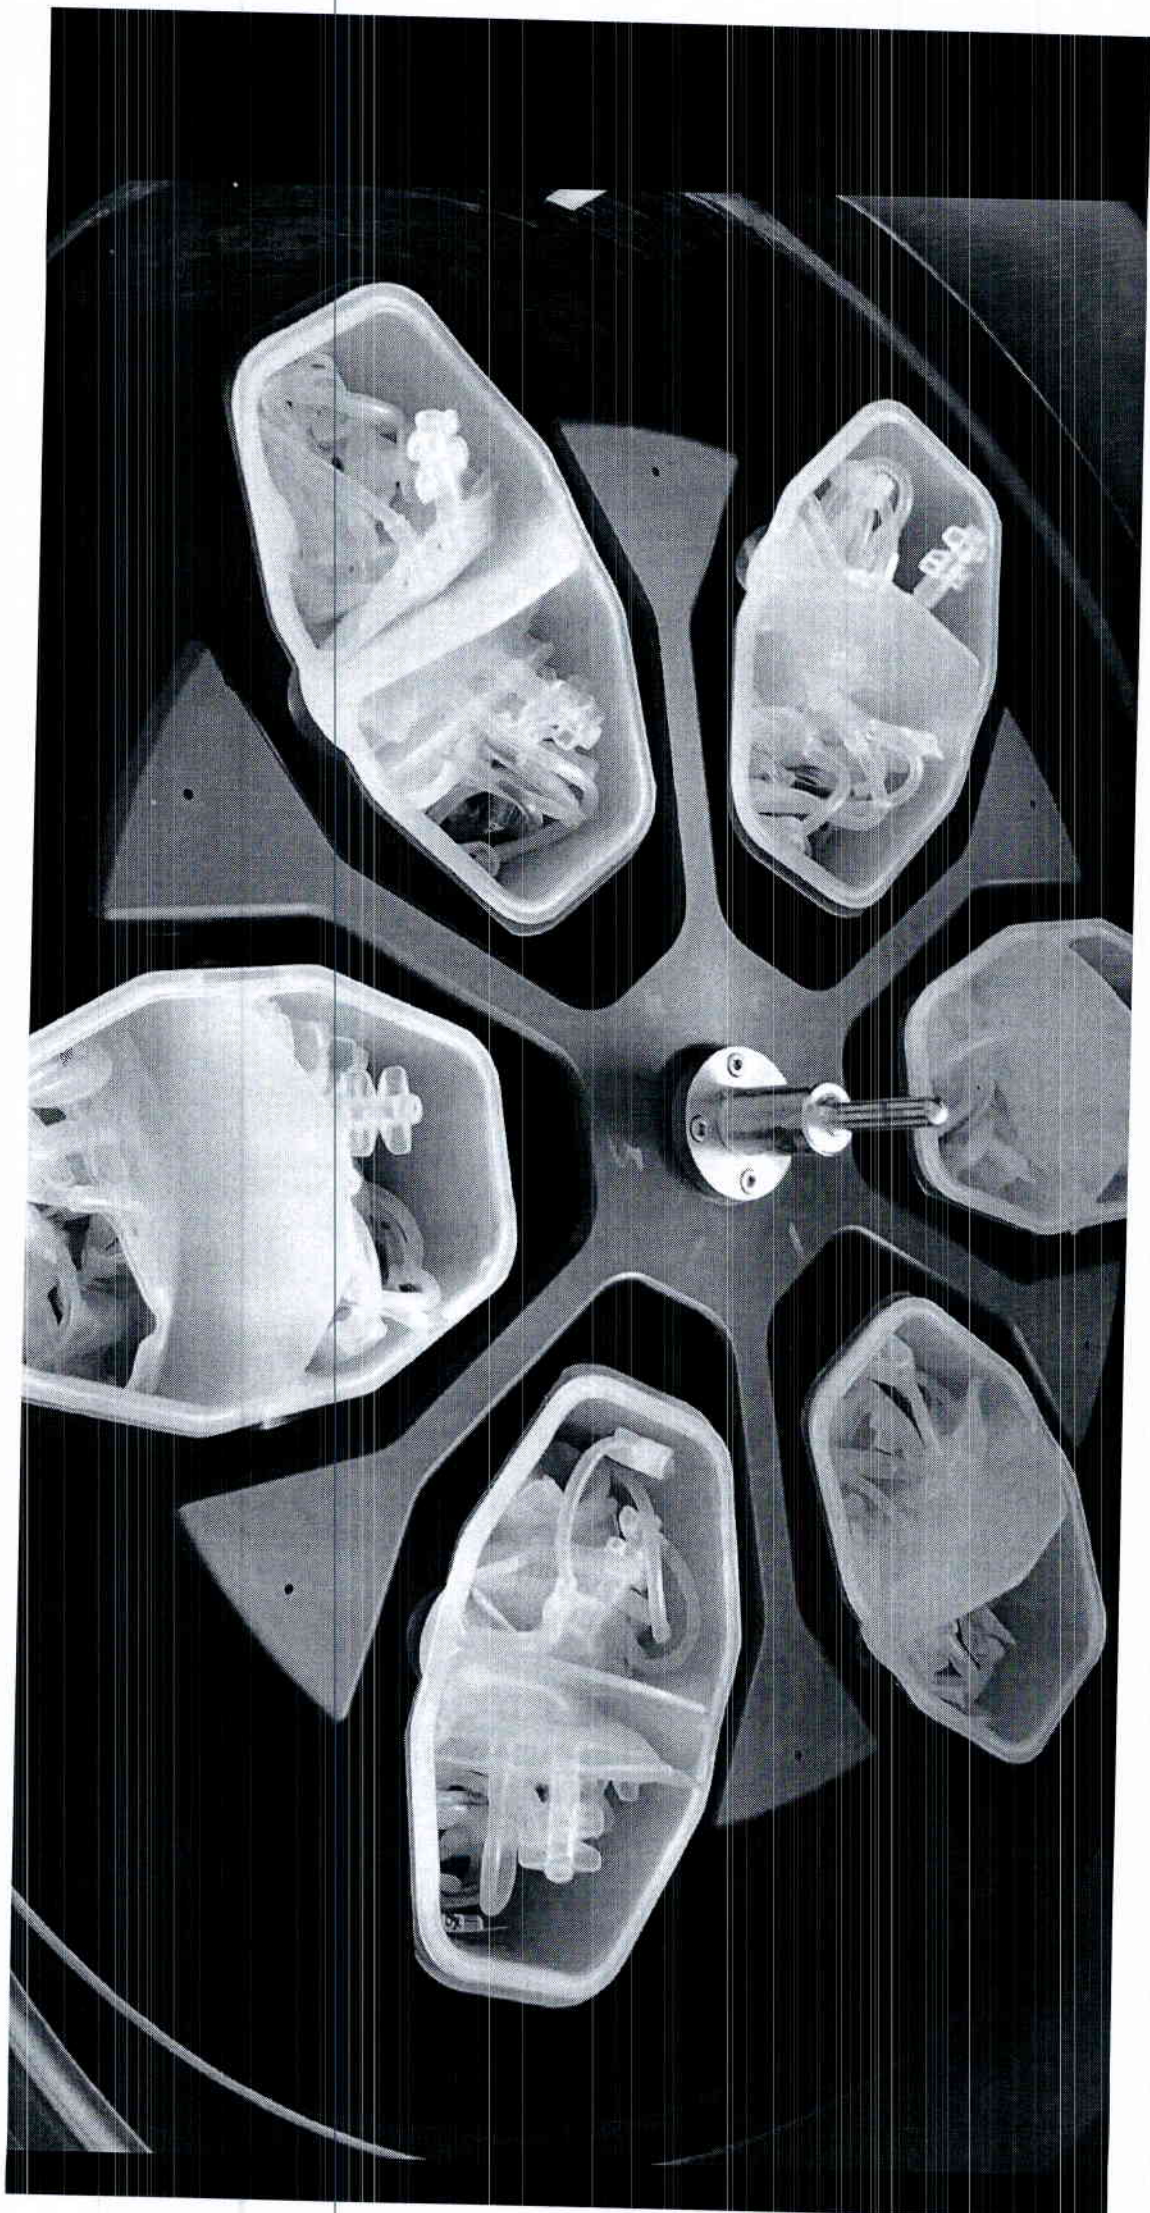



MANAGEMENT SYSTEM CERTIFICATE

Certificate No.: 117 19 QOM 0018 ROS

This is to certify the quality management systems of

**Hunan Labwe Scientific Instruments
Co., Ltd**

Unified Social Credit Code 91430100MA4L34H17T

Registered Address 504#, Building F10, Lugulinyu Community, 408#,
Tongzipo West Road, Changsha High-Tech Industrial
Development Zone, Hunan, China

Auditing Address 505#, Building 13, Xinggong Technology Park, 100#,
Luyun Road, Yuelu District, Changsha, Hunan, China

has been assessed and registered as meeting the requirements of
ISO13485: 2016 <Medical device-Quality management
systems - Requirements for regulatory purposes>

Produce and Sale of Medical Centrifuges

Signed by:



First Certification: 26 Feb. 2019

Expiry Date: 25 Feb. 2022

Shanghai Ingeer Certification Assessment Co., Ltd.

Certification and Accreditation Administration of PRC CNCA-R-2003-117

Tel: 400-182-8001/86 21-51114700

Web: www.icas.org.cn

Add: Room 801, HuaDing Mansion, 2388 West Zhongshan Rd.,
Xuhui District, Shanghai, China, 200235



Focus on the WeChat platform



--	--	--

First Surveillance Audit

Second Surveillance Audit

Third Surveillance Audit

The ownership of the certificate belongs to Shanghai Ingeer Certification Assessment Co., Ltd. The information & validation of this certificate can be checked on the CNCA website: WWW.CNCA.GOV.CN and ICAS website, or by calling ICAS's clients services Dept. The certificate is only valid when used together with related permits when appropriate. If the organization can't effectively maintain the above management system, ICAS has the right to withdraw the qualification certificate.



Hunan labwe scientific instruments co.ltd

Add:504#,F10 building,408#,Tong-zi-po west road,Changsha High-Tech industrial development zone,Hunan,China Mobile:86-137 8725 3412 www.lab-we.com

Declaration of conformity

WE Hunan Labwe Scientific Instruments co.,ltd are the professional centrifuges manufacturer having refrigerated office in 504#,F10 building,408#,Tong-zi-po west road,Changsha High-Tech industrial development zone,Hunan,China .

Do hereby declares that our centrifuge:

Model :BW12R

Applicable standards:

EN61010-1:2010 EN61010-2-020:2006 EN61326-1:2013 EN61000-3-2:2014
EN61000-3-3:2013

LVD(Low voltage directive) 2014/35/EU

Electromagnetic Compatibility 2014/30/EU

DPA

General Manager





Hunan labwe scientific instruments co.,ltd
www.lab-we.com



BW12R

Super capacity refrigerated centrifuge

FEATURES

- Microprocessor control with AC Brushless Motor .
- CFC free cooling system with pre-cooling function.
- LCD Display the parameters of speed ,timer,RCF, Temperature, rotors information, Program(Memory) information, Acceleration & Deceleration information and Error code information.
- Steel centrifuge body and 304# stainless steel chamber are autoclaveable and resistant detergents and disinfection liquids.
- Gas hinge for lid drop protection.
- Safety Electrical lid interlock, door can not open when rotor is running and machine won't run when lid open and error code appears.
- Emergency lid lock release when power failure.
- Window on lid for speed calibration and noise measurement.
- Continuous operation, working continuous according the set time.
- 10 kinds of Program(Memory) and 10 kinds of Acceleration&Deceleration for choice. If ask for more Programs please specially mentioned when place the order.
- Automatic troubleshooting with indication of error code and alarm on the screen.
- Wide choice of rotors are autoclaveable.
- With CE and ISO9001:2008, ISO13485 certificate



SPECIFICATION

Speed range(rpm)	0-8000rpm adjustable
Max Capacity(ml)	6x2400ml/ 18 pcs 400ml bags
RCF range (xg)	0-14336xg adjustable
Noise(dBA)	58dB(A)
Time range	1-99minutes adjustable
Temperature range(°C)	-20°C ~+40°C adjustable
Speed accuracy	±20r/min
Temperature accuracy	±1°C
Dimension(mm)	960*860*1220mm
Net weight(without rotor)	500KGS
Power supply	AC220~240V,50/60HZ,30A,5.5KW

NO.1 FIXED ROTOR

 Capacity: 6x1000ml Max speed: 8000rpm Max RCF: 14336xg	Adapter: 6x35x0.2ml 	Adapter: 6x35x0.5ml 	Adapter: 6x24x1.5/2.2ml 
	Adapter: 6x15x5ml 	Adapter: 6x13x10ml 	Adapter: 6x13x15ml 
	Adapter: 6x10x20ml 	Adapter: 6x8x30ml 	Adapter: 6x7x50ml 
	Adapter: 6x3x100ml 	Adapter: 6x250ml 	Adapter: 6x300ml 
	Adapter: 6x500ml 	All can be custom made	

