

SERATEC® HemDirect

REF: HBF07, HBF07/8, HBF07/30


Application

SERATEC® HemDirect is a chromatographic immunoassay for rapid detection of human hemoglobin (Hb) to identify blood in forensic samples. The product contains two monoclonal anti-human Hb antibodies as active components.

Materials

- 8 or 30 (HBF07/8, HBF07/30) individually packaged HemDirect in cassette format with one plastic pipette each
 - 8 or 30 (HBF07/8, HBF07/30) vials with 1.5 ml extraction buffer
 - Instructions for use
- Additionally required: stopwatch or timer

Test performance

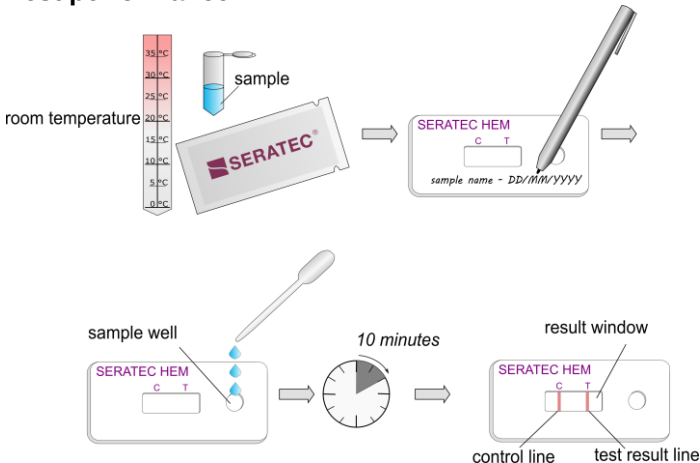

- Bring all test components to room temperature before performing the test. Low temperatures can lead to a decrease in sensitivity.
- Remove the test cassette from the pouch and label it for identification.
- Add 3 drops of the sample (approx. 120 µl) to the sample well with the enclosed plastic pipette and start the time measurement.
- Read the test result after 10 minutes at room temperature. The liquid in the sample well should have been completely absorbed.
- Keep the remaining sample material to perform further testing if necessary.


Interpretation of results

After 10 minutes, up to two lines may be visible in the result window:

Test result line (T): only visible when the sample is Hb-positive; the colour intensity of the line may vary and depends on the Hb concentration of the sample.

Control line (C): Control for potential application errors and for the integrity of the test components. This line is always visible after successful performance of the test.

Negative result (Hb is not detectable; no Hb in the sample or concentration below the limit of detection):



Positive result (Hb detectable):



Two lines visible in the result window: the test result line (T) and the control line (C). Any visible T-line (with strong or weak intensity) is to be considered a positive result.

Invalid result (no usable result):



No control line (C) visible. In this case, the test is invalid and should be repeated with a new test cassette.

Sample preparation

In order to obtain optimal test results, follow these instructions:

- It is not recommended to use unknown samples undiluted. Liquid samples should be diluted at least 1:500 prior to testing. The colouration of the sample can be a visual indicator of a suitable dilution factor: the visible colouration of blood samples will disappear at a dilution between approx. 1:10³ and 1:10⁴.
- Viscous samples should be diluted until the sample flows smoothly on the test membrane.
- Use the buffer solution included in the scope of supply, as it has been developed specifically for the HemDirect. Other buffer solutions or the use of water may result in reduced sensitivity or fluctuating line intensities.
- Do not use liquids with a pH below 3 or above 12, as this may cause incorrect or invalid results.
- Adding detergents such as SDS, sarcosyl or bleach to the sample material may cause incorrect or invalid results. This is probably caused by the denaturation of Hb.
- Tissue particles do not affect the test result.
- Cotton swabs, cloth or condom pieces should be extracted in a sufficient amount of buffer. The cut piece should be between 0.25 and 1 cm² in size and can be given directly into the buffer vial. Alternatively the samples can be collected with the applicator attached to the lid of the buffer tube.
- An extraction time of approx. 10 minutes is recommended. You should however follow the rule that the older or smaller the stain, the longer the recommended extraction time.[1,2]
- Extracted samples are stable at room temperature for about 2 days. Samples kept for longer periods should be stored dry and cold (2 – 8 °C). Liquid samples may be frozen.

Extraction buffer

The supplied extraction buffer contains the following constituents (in 1 l distilled H₂O):

12,1 g Tris; 8,8 g Na₃Citrat; 0,2 g NaN₃; 0,5 g Tween 20; 5 g BSA; pH 6,8.


Further analyses

For the further differentiation of blood traces, we recommend using the **SERATEC® PMB Test** for detection of Hb and D-dimer to identify and differentiate peripheral blood and menstrual blood.

DNA profiling

The extracted samples can be stored for further analyses (e.g. DNA profiling; see Sample preparation).

The extracted sample is compatible with DNA analyses. It is also possible to extract DNA from the sample pad for further analysis.[3,4]

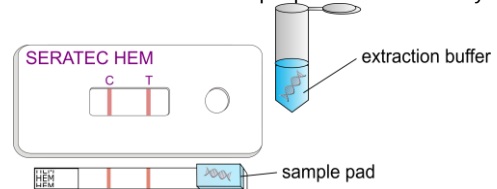

Safety information

Forensic samples are potentially infectious material which should be examined with the appropriate care and only when suitable protective measures (e.g. gloves, laboratory clothing) are applied. Materials used to perform the test should be autoclaved before disposal, as they contain potentially infectious material. Observe the following instructions:

- Do not use the product if damaged.
- Only remove the test cassette from the pouch immediately before use.
- Do not use the product after the expiration date.

- The materials used in the test (e.g. antibodies) are potentially infectious materials. When used and disposed of properly, however, there is no danger to the user or others.
- Do not freeze the test cassette.

Background

The red blood pigment hemoglobin (Hb) is a protein complex which occurs in red blood cells and primarily serves to transport gas in the body. It has a molecular weight of 64.5 kDa and consists of 4 subunits (amino acid chains), two of which are identical. Each subunit is associated with a haem group, an iron complex responsible for oxygen binding. At concentrations of 120-160 mg/ml (women) and 140-180 mg/ml (men), Hb is one of the most common proteins in blood.

There are several methods for the detection of blood in forensic sample material by means of detecting Hb. However, many detection methods are unspecific regarding the origin (human or animal) of the sample. This means that further examinations are necessary, which usually cannot be performed directly at the crime scene. SERATEC® HemDirect features **high sensitivity and specificity** and the **detection of human hemoglobin as a marker of blood** offers the following benefits in forensic applications:

- Easy handling without additional equipment – directly at the crime scene or in the laboratory.
- A quick and reliable result after 10 minutes.
- Very high specificity through direct detection of human Hb (see Specificity).
- High stability of Hb; positive detection could be obtained with 31-year-old samples.[1]

Sensitivity

SERATEC® HemDirect can be used to detect quantities of min. 20 ng/ml human Hb. In very high Hb concentrations, the **high dose hook effect** can cause reduced line intensity; therefore, it is recommended to always dilute fresh liquid samples (see Sample preparation). Human blood diluted in the range between 1:50 and 1:10⁷ is positively detected in the recommended extraction buffer.

Specificity

SERATEC® HemDirect does not show any cross-reactivity with other proteins in blood. No cross-reactivity has been observed with the blood of various animal species (dog, rabbit, cat, cattle, pig, wild boar, horse, chicken, sheep, mule, goat, red deer and others).[1] Primate and ferret blood can cause positive results.

Storage and shelf life

- Store test cassettes and buffer solution at +2 to +30 °C (38 to 86 °F).
- Keep test cassettes in the pouch until use.
- Do not use after the specified expiration date.

Quality features

Our products are manufactured according to the quality standards of European standard ISO 9001. The performance characteristics are confirmed during final quality control in application of the following standard: *human hemoglobin* (Sigma Aldrich, H7379).

Please contact us if you have any questions or require more information.

Literature

- [1] A. Misencik, D.L. Laux, Validation Study of the Seratec HemDirect Hemoglobin Assay for the Forensic Identification of Human Blood, in: 2007.
- [2] M.N. Hochmeister, B. Budowle, R. Sparkes, O. Rudin, C. Gehrig, M. Thali, L. Schmidt, A. Cordier, R. Dirnhofer, Validation studies of an immunochromatographic 1-step test for the forensic identification of human blood, J. Forensic Sci. 44 (1999) 597–602.
- [3] A. Barbaro, P. Cormaci, S. Votano, A.L. Marca, Evaluation study about the SERATEC® rapid tests, Forensic Sci. Int. Genet. Suppl. Ser. 5 (2015) e63–e64. doi:10.1016/j.fsigss.2015.09.025.
- [4] H. Holtkötter, C.R. Dias Filho, K. Schwender, C. Stadler, M. Vennemann, A.C. Pacheco, G. Roca, Forensic differentiation between peripheral and menstrual blood in cases of alleged sexual assault—validating an immunochromatographic multiplex assay for simultaneous detection of human hemoglobin and D-dimer, Int. J. Legal Med. 132 (2018) 683–690. doi:10.1007/s00414-017-1719-y.

Symbols



Expiry date



Storage temperature



Lot number