

Hohenstein Laboratories - Schloss Hohenstein - 74357 Bönnigheim

medi GmbH & Co. KG

Medicusstraße 1
95448 Bayreuth

**Hohenstein Laboratories
GmbH & Co. KG**

Schloss Hohenstein
74357 Bönnigheim · Germany

Consumer Tests
Phone +49 7143 271 201
Fax +49 7143 271 94 201
c.doege@hohenstein.de

Client no.

—

Contact person

C.Doege

Our ref.

CD

Date

03. February 2017

Report No. 16.2.20.13414/I

Client: See address

Test sample: 2 pairs of anti-embolism stockings with adhesive welt,
article "mediven thrombexin 18", AG,
size M

Aim of test: Examination into compressive properties following RAL-GZ 387/1:2008-01^A,
section 3.6.2 to 3.6.5

Date of order: 19.12.2016

Receipt of order: 20.12.2016

Receipt of test samples: 20.12.2016

Period of testing: 20.01.2017

Preliminary results: 25.01.2017

Sampling: The test sample has been delivered to us by the client.

The Report comprises 3 pages and a set of tables of 2 pages.

Es gelten unsere Allgemeinen
Geschäftsbedingungen:
Our terms of business shall apply:
www.hohenstein.de/pdf/agb.pdf

Telefon / Phone
+49 7143 271 0
Fax +49 7143 271 51
info@hohenstein.de
www.hohenstein.de

USt-IdNr.
VAT REG No.
DE815128169

Hohenstein Laboratories GmbH & Co. KG · Registergericht Amtsgericht Stuttgart HRA 724658
Persönlich haftender Gesellschafter: Hohenstein Verwaltungs GmbH HRB 752904
Sitz der Gesellschaft ist Bönnigheim · Geschäftsführer: Dr. Stefan Droste, Florian Girmond,
Prof. Dr. Dirk Höfer, Dr. Andreas Schmidt
Hohenstein Laboratories GmbH & Co. KG · Court of Registration County Stuttgart HRA 724658
personally liable associate: Hohenstein Verwaltungs GmbH HRB 752904 ·
company headquarter is Boennigheim · CEOs: Dr. Stefan Droste, Florian Girmond,
Prof. Dr. Dirk Höfer, Dr. Andreas Schmidt

METHODS

COMPRESSION TEST

■ Pre-Treatment

The samples are washed once in accordance with DIN EN ISO 6330/4G:2013-02 and dried flat at room temperature (procedure C of this standard). Then the samples are laid out for 24 hours in normal conditions in accordance with DIN EN ISO 139:2011-10, Section 3.1.

■ Elongation, Pressure and Residual Pressure

Number of tested samples : 2

The test is carried out at $(20\pm 2)^{\circ}\text{C}$ and $(65\pm 5)\%$ relative humidity, using the Compression Measurement System Hohenstein (HOSY).

The 6th load curve is evaluated. The results are shown in table and diagram form. Each table also contains the specified length and circumference measurements.

Note:

For the test with HOSY, the joint between the knitted fabric and the top edge of the stocking is located at the nearest joint between two clamps.

In the tables, the values shown for the uppermost measuring point are those from the clamp which is holding only the knitted fabric. On the pressure profile sheet, this measuring point is shown at the height that was actually specified (end of the stocking).

SIZE INFORMATION

The following values for length and circumference were defined by the customer:

Measurements in cm

(L = lengths, C = circumferences)


	B	B ₁	C	D	E	F	G
L	12	23	33	41	49	64	77
C	24	31,5	40	39	43,5	54,5	63

Compression Measurement System Hohenstein	
Orderer:	medi GmbH & Co. KG
Item:	mediven thrombexin 18
Manuf. size:	M
Special details:	with adhesive welt

Pos.	Measurement		Wear stretch (%)	Tension (N/cm)	Pressure (kPa)	Residual pressure (%)
	Circ. (cm)	Height (cm)				
B	24.0	12.0	58.4	.89	2.34	100.0
B1	31.5	23.0	75.0	1.02	2.05	87.6
C	40.0	33.0	82.6	1.07	1.68	71.9
D	39.0	41.0	68.3	.82	1.32	56.7
E	43.5	49.0	68.6	.81	1.18	50.4
F	54.5	64.0	75.6	.94	1.09	46.5
G	59.8	72.0	72.9	.98	1.03	43.9
1	24.6	7.0	36.3	.51	1.30	55.8
2	24.0	12.0	58.4	.89	2.34	100.0
3	26.1	17.0	64.7	.89	2.13	91.3
4	30.4	22.0	73.7	1.02	2.10	89.7
5	35.8	27.0	78.4	1.00	1.75	75.0
6	39.7	32.0	83.3	1.07	1.70	72.8
7	39.6	37.0	75.0	.95	1.51	64.5
8	39.2	42.0	67.5	.80	1.29	55.2
9	41.9	47.0	67.9	.80	1.21	51.6
10	45.8	52.0	68.9	.82	1.13	48.3
11	49.6	57.0	68.5	.83	1.05	44.9
12	53.1	62.0	73.8	.89	1.05	44.9
13	56.5	67.0	76.8	1.00	1.11	47.6
14	59.8	72.0	72.9	.98	1.03	43.9
15	63.0	77.0	56.6	1.33	1.33	56.8

The results show the average of 2 measurements.

Compression Measurement System Hohenstein	
Orderer:	medi GmbH & Co. KG
Item:	mediven thrombexin 18
Manuf. size:	M
Special details:	with adhesive welt

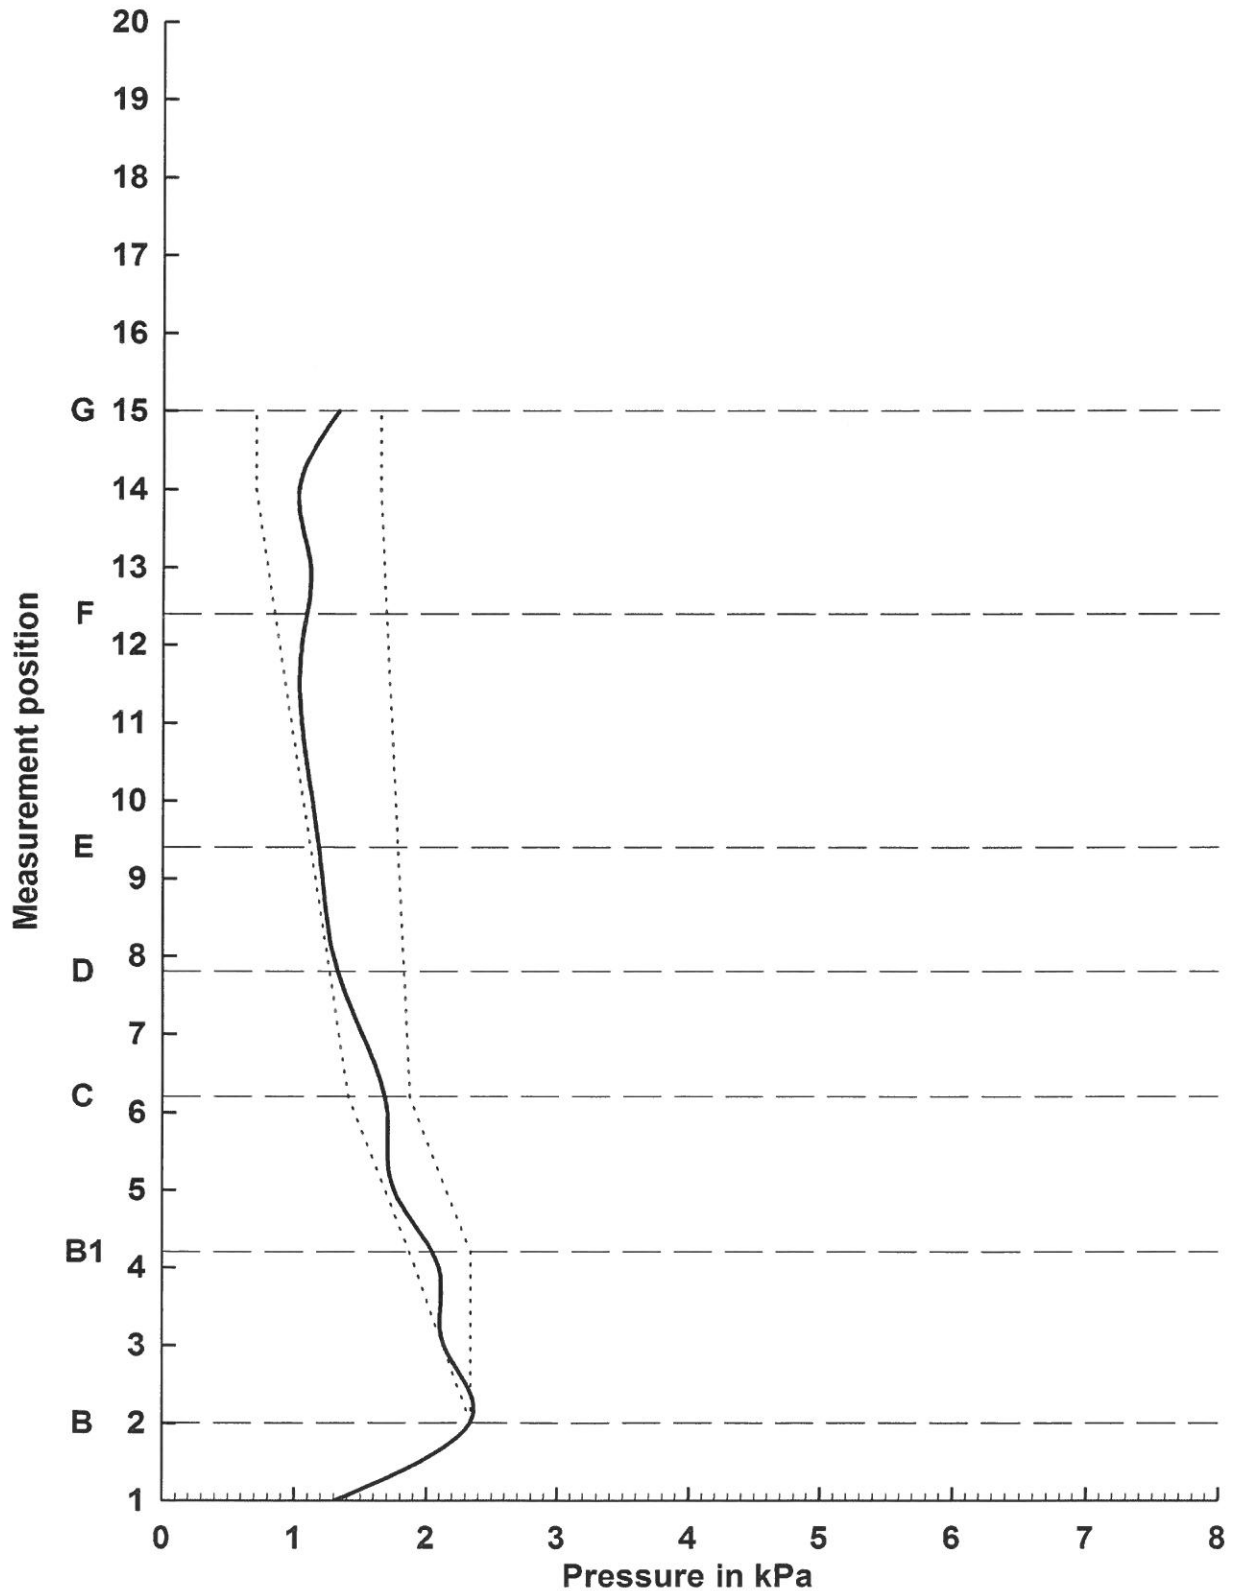

RESULT

The article reaches a pressure value of 2,34 kPa resp. 17,5 mm Hg at measuring point B.

The residual pressure ratio is not higher at any measuring point than the one below.

The increase in residual pressure at the adhesive welt amounts to 12,9 percent points.

Remark:

The specifications concerning pressure and pressure characteristic in RAL-GZ 387/1:2008-01^A apply to medical compression hosiery only. But nevertheless even with anti-embolism stockings it makes sense, if the residual pressure decreases continuously from the ankle to the edge respectively if the increase of the residual pressure at the edge is in a similar range (15 percent points).

Schloss Hohenstein, 03. February 2017

Chief Executive Officer



Dipl.-Ing. (FH) Florian Girmond



Division medical compression textiles
Consumer Tests



Dipl.-Ing. (FH) Christine Doege

Das Ergebnis bezieht sich nur auf die eingereichten Gegenstände. Der Bericht darf nicht auszugsweise, sondern nur in seinem vollen Umfang weitergegeben werden. Eine Benutzung des Berichts zu Werbezwecken oder die Veröffentlichung freier Interpretationen der Ergebnisse ist nur mit ausdrücklicher Genehmigung der Hohenstein Institute zulässig. Rechtsverbindlich ist nur der autorisierte Bericht. Die vom Kunden übergebenen Unterlagen bzw. Materialien werden, soweit die Beschaffenheit dies zulässt, 3 Monate aufbewahrt. Für den gesetzlich geregelten Bereich gilt eine Aufbewahrungsfrist von 10 Jahren.
Die Akkreditierung gilt für die in der Urkundenanlage aufgeführten Verfahren (Akkreditierungen siehe http://www.hohenstein.de/de/about_hohenstein/akkreditation/akkreditation.html) - im Bericht mit ^A gekennzeichnet.
The results relate only to the samples submitted. This report must only be reproduced in full and not in extract form. Use of the report in advertising or the publication of free interpretations of the results is only allowed with the express permission of the Hohenstein Institute. Only the authorized report is legally binding. Documents and materials delivered by the client will be retained for 3 months, provided their condition allows it. A storage period of 10 years applies to the legally regulated area.
The accreditation applies for the methods listed in the annex to the certificate (accreditations see http://www.hohenstein.de/de/about_hohenstein/akkreditation/akkreditation.html) - marked ^A in the report.