

Specificații de preț (F 4.2)

Numărul licitației: ocds-b3wdp1-MD-1597127433513					Data: 15.08.2020				
Denumirea licitației: Piese de schimb pentru dispozitive medicale (Printer)					Lot: 1.		Pagina: _1_ din _1_.		
Nr. d/o	Cod CPV	Denumirea bunurilor și/sau a serviciilor	Unitate a de măsură	Can ti-tate	Preț (fără TVA)	Preț (cu TVA)	Suma fără TVA	Suma cu TVA	Termenul de livrare/ prestare
	1	2	3	4	5	6	7	8	9
Lotul 1: Piese de schimb pentru dispozitive medicale (Printer)									
1.1	331000 00-1	Piese de schimb pentru dispozitive medicale (Printer)	Buc.	1,00	14 700,00	17 640,00	14 700,00	17 640,00	La solicitarea autorității contractate.
Total Lotul 1:							14 700,00	17 640,00	
TOTAL pe ofertă:							14 700,00	17 640,00	

Semnat electronic
Numele, Prenumele: Loghinov Rodion
În calitate de: Director
Ofertantul: Moldan-Service SRL
Adresa: Mun. Chişinău, str. Sciusev 16, of.2





Specificații tehnice (F4.1)

Numărul licitației: ocds-b3wdp1-MD-1597127433513					Data: 15.08.2020			
Denumirea licitației: Piese de schimb pentru dispozitive medicale (Printer)					Lot: 1		Pagina: 1 din 1.	
Nr. d/o	Cod CPV	Denumirea bunurilor și/sau a serviciilor	Modelul articolului	Țara de origine	Produsul	Specificarea tehnică deplină solicitată de către autoritatea contractantă	Specificarea tehnică deplină propusă de către ofertant	Standar de de referință
1	2	3	4	5	6	7	8	9
Lotul 1: Piese de schimb pentru dispozitive medicale (Printer)								
1.1	33100 000-1	Piese de schimb pentru dispozitive medicale (Printer)	P93W-Z	Japonia	Mitsubishi Electric	Printer compatibil pentru Ultrasonograf PHILIPS	Printer compatibil cu Ultrasonograf PHILIPS	CE,ISO

Semnata electronică
Numele, Prenumele: Loghinov Rodion
În calitate de: Director
Ofertantul: Moldan-Service SRL
Adresa: mun. Chisinau, str. Seicusev 16,of.2





- ① Power switch
- ② COPY button
- ③ SIZE switch
- ④ PRINT button
- ⑤ MODE switch
- ⑥ Printout/Cutler
- ⑦ LED indicator
- ⑧ (BRT/CONT/EXP) indicator
- ⑨ Open lever
- ⑩ ADJUST control
- ⑪ DIP switch
- ⑫ VIDEO IN connector (BNC)
- ⑬ BRT button
- ⑭ VIDEO OUT connector (BNC)
- ⑮ CONT button
- ⑯ Remote control terminal
- ⑰ FUNC button
- ⑱ Power terminal (AC LINE)
- ⑲ FEED button
- ⑳ Potential equalization terminal

Model	P93E
Print method	Thermal sensitive
Resolution	Printhead 325 dpi (12.8 dots/mm), max. resolution: 1280x600 dots (P&L, normal)
Color depth	256 greyscale
Print speed (Picture (without data transfer))	Normal: 3.5 seconds (P&L, UnderScan) Normal 2 split: 3.9 seconds (P&L, UnderScan) Side 8.4 seconds (P&L, UnderScan) Side 2 split: 4.2 seconds (P&L, UnderScan) 1-1: 5.0 seconds (P&L, UnderScan) 1-7: 10.6 seconds (P&L, UnderScan) 2-times: 11.5 seconds (P&L, UnderScan)
Paper size	Thermal paper roll, 110mm wide
Print Area	Normal: 100x75mm (P&L, UnderScan) Normal 2 split: 50x37mm (P&L, UnderScan) Side: 99x133mm (P&L, UnderScan) Side 2 split: 47x53mm (P&L, UnderScan) 1-1: 100x100mm (P&L, UnderScan) 1-7: 100x227mm (P&L, UnderScan) 2-times: 100x266mm (P&L, UnderScan)
Picture enlargement	0.5 to 2.0
Picture memory	10 frames
Interface	BAS/FBAS (Composite), BNC connector for input and output
Special features	36 steps for contrast and brightness, paper-saving function, 5 different gamma curves, selectable print area by expansion, negative print, reversed print direction, multiple copies
Power supply	220-240V, 50/60Hz; 100-120V, 50/60Hz
Power consumption	approx. 115W during printing, approx. 10W in stand-by
Dimensions (WxHxD)	approx. 154 x 90 x 256 mm
Weight	approx. 2.8kg
Approvals	TUV-GS/GM, CE (LVD, EMC, MDD)
Accessories (incl. in delivery)	Power cable, wire remote control, cleaning paper, thermal paper KP66HM-CE, BNC-signal cable, operation manual
Consumables	KP66B-CE, KP66HM-CE, KP9THG-CE



for a greener tomorrow

ECO Changes is the Mitsubishi Electric Group's environmental statement, and expresses the Group stance on environmental management. Through a wide range of businesses, we are helping contribute to the realization of a sustainable society.




MITSUBISHI ELECTRIC CORPORATION

www.mitsubishielectric-printing.com

P93E

HIGHLIGHTS

- User-friendly settings with control switches and LED indicator
- High-resolution thermal head with 325 dpi
- Extremely compact dimensions and lightweight design
- Fast print speed
- 7 different picture formats
- Picture memory for 10 individually selectable frames

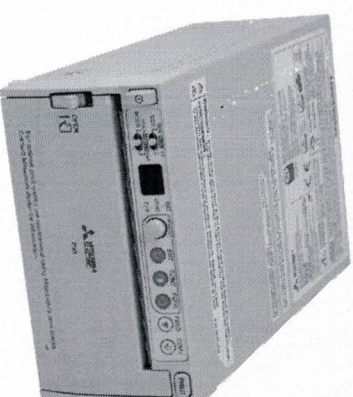

Let's go into more detail on picture quality

Meeting the high demands of medical documentation. Fast, precise and at the same time very efficient. This is the standard the new analogue b/w video printer has set itself. 256 greyscales and a 352 dpi resolution guaranty the truly detailed, contrast rich printing of patient pictures. And this in speedy 3.9 seconds. At the same time the picture memory of the P93E delivers up to 10 frames, which can be individually selected. Free choice is also available over the adjustments. The P93E can print specific parts of the image. You can print in increments of 0.1 and set the picture enlargement scale from 0.5 to 2.0. To control the brightness and contrast, there are 39 steps available to you (from -19 to +19). Convenient top: All picture corrections are adjustable using the control switches on the front panel, and are also shown by a LED indicator.



VIDEO COPY PROCESSOR

This video copy processor complies with the requirements of the EC Directive 89/336/EEC, 73/23/EEC, 93/42/EEC and 93/68/EEC.

The electro-magnetic susceptibility has been chosen at a level that gains proper operation in residential areas, on business and light industrial premises and on small-scale enterprises, inside as well as outside of the buildings. All places of operation are characterised by their connection to the public low voltage power supply system.



THIS OPERATION MANUAL IS IMPORTANT
TO YOU.
PLEASE READ IT BEFORE USING YOUR
VIDEO COPY PROCESSOR.



MITSUBISHI ELECTRIC
VIDEO COPY PROCESSOR
MODEL
P93W
P93E
OPERATION MANUAL



CE

WARNING:

In the USA or Canada, use the AC power cord according to the recommendations as below, in order to comply with UL2601-1 and CAN/CSA C22.2 No. 601.1.



Case 1. Connect to the 120V receptacle of the room or the host equipment.

The AC power cord should be UL or CSA approved and consist of type SJT, size 16 or 18AWG, length 2.5m or shorter cord with IEC320/C13 type, 125V 10A or higher rating connector and NEMA 5-15 type, 125V 10A or higher rating, Hospital Grade plug.

Case 2. Connect to the 230V receptacle of the room or the host equipment.

The AC power cord should be UL or CSA approved and consist of type SJT, size 16 or 18AWG, length 2.5m or shorter cord with IEC320/C13 type, 250V 10A or higher rating connector and NEMA 6-15 type, 250V 10A or higher rating, Hospital Grade plug.

Case 3. Connect to the 120V receptacle of the host equipment.

The AC power cord should be UL or CSA approved and consist of type SJT, size 16 or 18AWG, length 2.5m or shorter cord with IEC320/C13 type, 125V 10A or higher rating connector and IEC320-2.2/E type, 125V 10A or higher rating plug.

Case 4. Connect to the 230V receptacle of the host equipment.

The AC power cord should be UL or CSA approved and consist of type SJT, size 16 or 18AWG, length 2.5m or shorter cord with IEC320/C13 type, 250V 10A or higher rating connector and IEC320-2.2/E type, 250V 10A or higher rating plug.

CAUTION:

Changes or modifications not expressly approved by the party responsible for compliance could void the user's authority to operate the equipment.

NOTE:

This equipment has been tested and found to comply with the limits for a Class A digital device, pursuant to Part 15 of the FCC Rules.

These limits are designed to provide reasonable protection against harmful interference when the equipment is operated in a commercial environment. This equipment generates, uses, and can radiate radio frequency energy and, if not installed and used in accordance with the instruction manual, may cause harmful interference to radio communications.

Operation of this equipment in a residential area is likely to cause harmful interference in which case the user will be required to correct the interference at his or her own expense.

Information:

This class A digital apparatus complies with Canadian ICES-003.

"CLASSIFIED BY UNDERWRITERS LABORATORIES INC.®

WITH RESPECT TO ELECTRIC SHOCK, FIRE AND MECHANICAL HAZARDS ONLY IN ACCORDANCE WITH UL2601-1 AND CAN/CSA C22.2 No. 601.1"

CAUTION:



RISK OF ELECTRIC SHOCK DO NOT OPEN.



TO REDUCE THE RISK OF ELECTRIC SHOCK, DO NOT REMOVE COVER (OR BACK)

NO USER-SERVICEABLE PARTS INSIDE. REFER SERVICING TO QUALIFIED SERVICE PERSONNEL.



The lightning flash with arrowhead symbol, within an equilateral triangle, is intended to alert the user to the presence of uninsulated "dangerous voltage" within the product's enclosure that may be of sufficient magnitude to constitute a risk of electric shock.



The exclamation point within an equilateral triangle is intended to alert the user to the presence of important operating and maintenance (servicing) instructions in the literature accompanying the appliance.



The "Caution, hot surface" symbol indicates that the marked item may be hot and should not be touched.



The "ON/OFF" symbol indicates connection to or disconnection from the mains, at least for mains switches.



The "Equipotentiality" symbol identifies the terminals connected each other. The potential of various parts of equipment or of a system is equalized.



The "Alternating current" symbol indicates that the equipment is suitable for alternating current only.

When you dispose of the unit or accessories, you must obey the law in the relative area or country and/or regulation in the relative hospital.

WARNING:

Install and use this appliance in accordance with the operation manual for safety and EMC (Electromagnetic Compatibility). If it is not installed and used in accordance with the operation manual, it may cause interference to other equipment and/or other risk.



To prevent fire or shock hazard, do not expose this appliance to rain or moisture.

This appliance must be earthed.

In Europe, use the AC power cord according to the recommendations as below, in order to comply with EN60601-1 and EN60950.

Connect to the 230V receptacle of the room or the host equipment.

The AC power cord should be VDE approved and consist of core size 1mm² or bigger, length 2.5m or shorter cord with IEC320/C13 type, 250V 10A or higher rating connector and CEE(7)VII type or IEC 320-2.2/E type, 250V 10A or higher rating plug.

Use the video cable and/or the wired remote control according to the recommendations as below, in order to comply with safety and EMC standards.

The video cable shall be 2m long or shorter, 75Ω coaxial, 3C-2VT or equivalent, with BNC plug at each end.

The wired remote control shall be Mitsubishi Electric parts No. 939P951010. (2m long or shorter, shielded wire, with 3.5mm diameter stereo mini-plug and switch box.)

This product is to be employed with medical equipment, just for reference purpose, not for medical diagnostic purpose.



Note: This symbol mark is for EU countries only.

This symbol mark is according to the directive 2002/96/EC Article 10 Information for users and Annex IV.

Your MITSUBISHI ELECTRIC product is designed and manufactured with high quality materials and components which can be recycled and reused.

This symbol means that electrical and electronic equipment, at their end-of-life, should be disposed of separately from your household waste.

Please, dispose of this equipment at your local community waste collection/recycling centre.

In the European Union there are separate collection systems for used electrical and electronic product.

Please, help us to conserve the environment we live in!