


Appendix B - Fitting the Vent Kit


An optional vent kit is available to allow any fumes to be extracted from Gemini AS into a fume cupboard or vented to the outside atmosphere. The maximum air-flow rate is 58 m³ per hour.



The vent kit should not be used to extract fumes via the building Heating, Ventilating, and Air Conditioning (HVAC) system or through a common site extraction system.

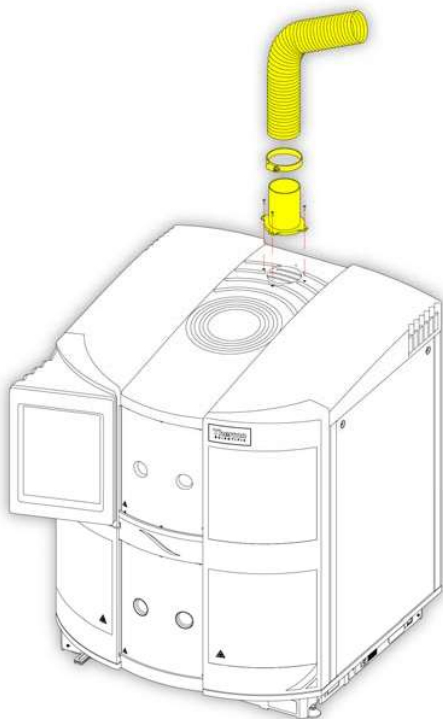

Step 1: Fit the flexible ducting over the mounting bracket and secure using the clip provided. Fix the mounting bracket to the Gemini AS top cover over the fan outlet grille using the four screws and gasket provided.

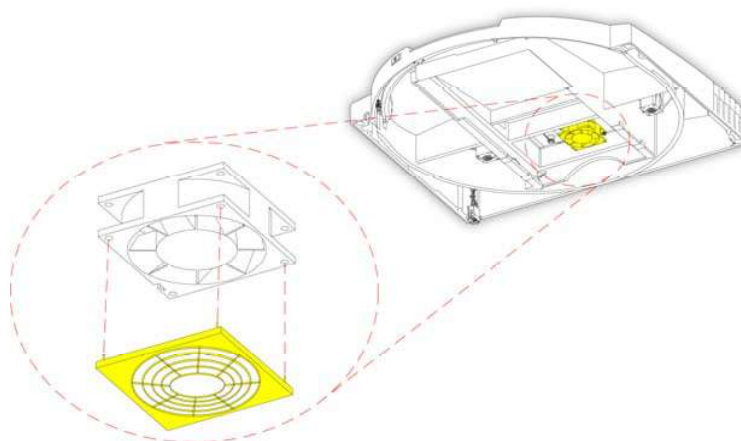

Step 2: Remove the filter (if fitted) from inside the Gemini AS top cover. Attach the fan guard to inlet side of the extractor fan by firmly inserting the plastic lugs into the holes at the corners of the fan.