

# Certificate of Registration

## QUALITY MANAGEMENT SYSTEM - ISO 13485:2016

This is to certify that:

Terumo Medical Corporation  
265 Davidson Avenue, Suite 320  
Somerset  
New Jersey  
08873  
USA


DUNS Number: 96-252-0628

Holds Certificate No:

**MDSAP 695791**

**Statement of Conformity:** The company listed on this certificate has been audited to and found to conform with the following criteria: ISO 13485:2016 and Australia - Therapeutic Goods (Medical Devices) Regulations, 2002, Schedule 3 Part 1 (excluding Part 1.6) - Full Quality Assurance Procedure; Brasil - RDC ANVISA n. 16/2013, RDC ANVISA n. 23/2012, RDC ANVISA n. 67/2009; Canada - Medical Devices Regulations - Part 1 - SOR 98/282; Japan - MHLW Ministerial Ordinance 169, Article 4 to Article 68, PMD Act; USA - 21 CFR 820, 21 CFR 803, 21 CFR 806, 21 CFR 807 - Subparts A to D

Design and Development, Manufacture and Distribution of Sterile Vascular Closure Devices

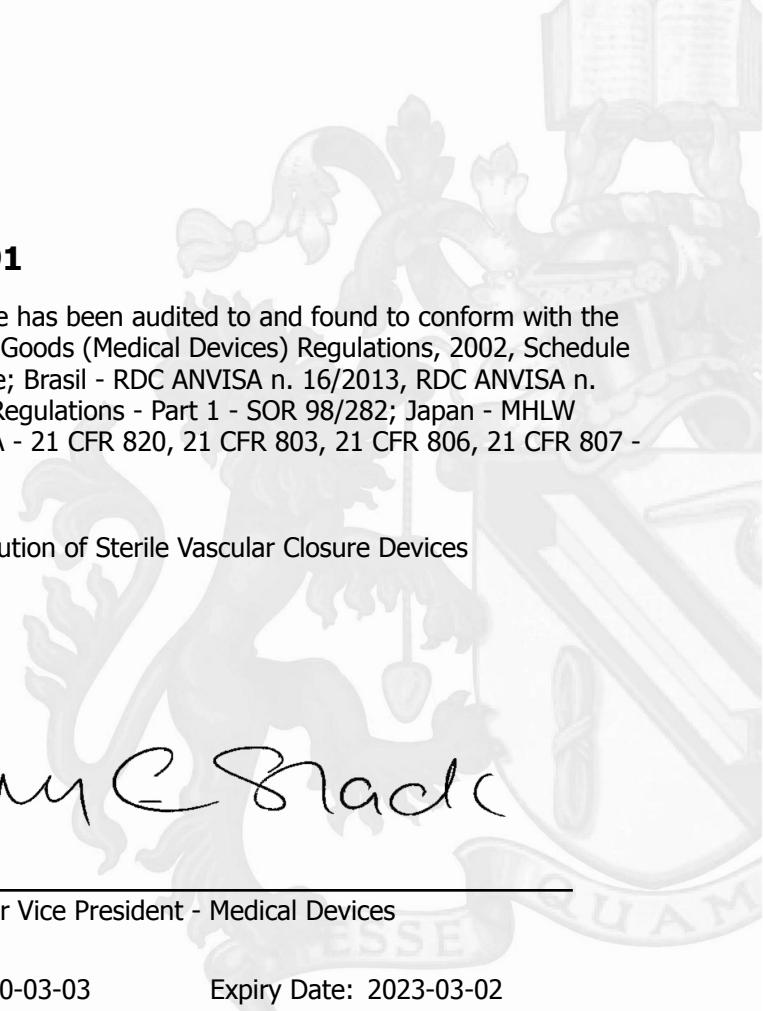

*Gary E Slack*

For and on behalf of BSI:

---

Gary E Slack, Senior Vice President - Medical Devices

Original Registration Date: 2020-03-03

Effective Date: 2020-03-03

Expiry Date: 2023-03-02



**MDSAP**  
MEDICAL DEVICE SINGLE AUDIT PROGRAM

BSI Group America Inc. is an MDSAP authorized auditing organization

Page: 1 of 1

...making excellence a habit.™

This certificate remains the property of BSI and shall be returned immediately upon request.  
An electronic certificate can be authenticated [online](#). Printed copies can be validated at [www.bsigroup.com/ClientDirectory](http://www.bsigroup.com/ClientDirectory)  
To be read in conjunction with the scope above or the attached appendix.

Americas Headquarters: BSI Group America Inc., 12950 Worldgate Drive, Suite 800, Herndon, VA 20170-6007 USA  
A Member of the BSI Group of Companies.