

Lot 20, centrifuga pentru pungi de sange

Rotixa 500 RS, rotor 4294, 4x buckets 4298-A, 4x adaptor 4237-A

Parametri solicitati	Parametri oferiti
"Centrifugă pentru centrifugarea pungilor de sânge Parametri: Viteza de rotație: Minimală, rpm reglabilă Maximală, rpm ≥ 6000 Setări setarea vitezei Rotor: Tipul rotor pentru pungi de sange volum 750-1000ml Numărul de locuri 4 Timer: Gama de timp 0 - ≥ 60 min Incrementarea ≤ 1 min Interval de temperatura $-20\text{ }^{\circ}\text{C} \dots +40\text{ }^{\circ}\text{C}$ reglabil Precizia temperaturii $\pm 1\text{ }^{\circ}\text{C}$ Securitatea Blocarea capacului în timpul lucrului da Indicatori: Indicari vizual și acustic da Debalansare da Pornire/oprire da Capac deschis da Display Digital da Nivelul de zgomot ≤ 70 dB Fereastra, orificiu sau alt acces, necesar pentru efectuarea procedurii de verificare periodica, conform normelor si standartelor in vigoare da Cerințe: Anul producerii minim 2023-24 Garanție minim 24 luni Servicii de mentenanță preventivă pe perioada de garanție Manuale de utilizare limba romana sau rusa Manual de service limba engleza, rusa sau romana Training pentru utilizatori Da, pregătire de lucru, mod de utilizare a dispozitivului, întreținerea zilnică. Training pentru personal tehnic Ajustarea, calibrarea, înlăturarea defecțiunilor minore, parole de acces după caz. "	Centrifugă pentru centrifugarea pungilor de sânge Parametri: Viteza de rotație: Minimală, rpm reglabilă Maximală, rpm 11500 Setări setarea vitezei Rotor, 4294, max. RPM max. RCF 2) 4,500 min-1 5,071: Tipul rotor pentru pungi de sange volum 750 si 1000ml, buckets 4298-A, 4x adaptor 4237-A Numărul de locuri 4 Timer: Gama de timp 1 - 999 min Incrementarea 1 min Interval de temperatura $-20\text{ }^{\circ}\text{C} \dots +40\text{ }^{\circ}\text{C}$ reglabil Precizia temperaturii $\pm 1\text{ }^{\circ}\text{C}$ Securitatea Blocarea capacului în timpul lucrului da Indicatori: Indicari vizual și acustic da Debalansare da Pornire/oprire da Capac deschis da Display Digital da Nivelul de zgomot 58 dB Fereastra, orificiu sau alt acces, necesar pentru efectuarea procedurii de verificare periodica, conform normelor si standartelor in vigoare da Cerințe: Anul producerii 2023-24 Garanție 24 luni Servicii de mentenanță preventivă pe perioada de garanție Manuale de utilizare limba romana sau rusa Manual de service limba engleza, rusa sau romana Training pentru utilizatori Da, pregătire de lucru, mod de utilizare a dispozitivului, întreținerea zilnică. Training pentru personal tehnic Ajustarea, calibrarea, înlăturarea defecțiunilor minore, parole de acces după caz. "

FLOORSTANDING CENTRIFUGES

— ROTIXA 500 RS

SMALL FOOTPRINT - HIGH VOLUMES

Its durable components make the ROTIXA 500 RS a reliable unit with a long service life. High sample capacity and maximum RCF of 5,252 make it suitable for 4 x 450-750 ml blood bags. Specially designed buckets keep blood bags upright during centrifugation for improved separation of blood components. In industrial research labs, it accommodates 4 bottles up to 1,000 ml, specialty racks, as well as containers and vessels for various applications.

This unit includes refrigeration with a temperature range from -20°C to +40°C.



— HIGHLIGHTS

- RPM: 50 - 11,500 min⁻¹
Adjustable in increments of 10
- RCF: 50 - 18,038
Adjustable in increments of 1
- max. capacity: 4 x 1,000 ml
- Choice of 5 rotors
- Medical Device according to directive 93/42/EC
- easy operation with keypad and control knob
- 89 program memories for more individuality
- 19 individual acceleration and deceleration stages

— FEATURES

- metal housing and lid
- viewing port in the lid
- powered one hand lid lock
- lid dropping protection
- emergency lid lock release
- stainless steel chamber
- automatic rotor recognition
- brushless drive
- error display
- display in °C and °F possible
- imbalance monitoring and switch-off

TECHNICAL DATA

ROTIXA 500 RS ^{>)} refrigerated




voltage ^{*)}	230 – 240 V 1 ~	220 V 1 ~
frequency	50 Hz	60 Hz
consumption	3,800 VA	
emission, immunity	EN/IEC 61326-1, class B	
max. capacity	4 x 1,000 ml	
max. RPM	11,500 min ⁻¹	
max. RCF	18,038	
running time	1 – 999 min: 59 s, ∞ continuous run	
dimensions (WxDxH)	650x814x973 mm	
weight	approx. 219 kg	
noise level	58 dB (A) with rotor 4282	
temperature control, infinitely variable	from -20 to +40 °C	
Cat. No.	4950	

^{*)} Other voltages on request.



^{>)} Other models on request.

AVAILABLE ROTORS


SWING-OUT ROTORS

		angle	max. RPM	max. capacity	Cat. No.	page
	swing-out rotor, 4-place	90°	4,500 min ⁻¹	4 x 1,000 ml	4294	3
	swing-out rotor, 6-place	90°	4,000 min ⁻¹	6 x 250 ml	4296	9
	swing-out rotor, 2-place	90°	3,600 min ⁻¹	20 plates	4282	11

ANGLE ROTORS

	angle rotor, 6-place	25°	9,500 min ⁻¹	6 x 250 ml	4266	12
	angle rotor, 6-place	45°	11,500 min ⁻¹	6 x 94 ml	4246	13

SWING-OUT ROTOR, 4-PLACE | 4294



Rotor	
max. RPM max. RCF ²⁾	4,500 min ⁻¹ 4,958
max. capacity	4 x 750 ml
run-up run-down, braked in sec	115 116
angle temperature in °C ¹⁾	90° +6
Cat. No.	4294

Bucket	
lid	4229-B
Cat. No.	4295-A

Tubes														
capacity in ml	0.8	1.5	2.0	4	5	6	7	9	12	15	25	50	94	100
Ø x L in mm	8x45	11x38	11x38	10x88	12x75	12x82	12x100	14x100	16x101	17x100	24x100	34x100	38x102	40x115
max. RCF ²⁾	4,777	3,690	4,867	4,777	4,777	4,777	4,777	4,777	4,777	4,777	4,777	4,777	4,777	4,777
radius in mm	211	163	215	211	211	211	211	211	211	211	211	211	211	211
Cat. No.	microliter tubes						tubes²⁾							

Adapter														
boring Ø x L in mm	8.2x32	11.2x40	11.2x40	11x70	12.5x32	12.5x70	12.5x70	16 x 70	16 x 70	17.5x74	26x70	35x70	41.5x70	41.5x70
tubes per rotor	312	336	336	252	192	192	192	100	100	120	44	24	16	16
Cat. No.	4226	4225	4225	4224	4213-93	4213	4213	4223	4223	4214	4215	4216	4218	4218

Tubes														
capacity in ml	2.6-3.4	2.7-3	4-5.5	4.5-5	7.5-8.2	9-10	10	1.6-5	4-7	4-7	8	8.5-10	15	50
Ø x L in mm	13 x 65	11x66	15x75	11x92	15x92	16x92	15x102	13 x 75	13 x 100	16x75	16x125	16x100	17x120	29x115
max. RCF ²⁾	4,777	4,777	4,777	4,777	4,777	4,777	4,777	4,777	4,777	4,777	4,777	4,777	4,958	4,958
radius in mm	211	211	211	211	211	211	211	211	211	211	211	211	219	219
Cat. No.	blood collection / urine tubes												tubes with screw cap	

Adapter														
boring Ø x L in mm	13.2x32	12.5x32	17.5x32	12.5x70	17.5x74	17.5x70	17.5x74	13.2x32	13.2x70	17.5x32	16x70	17.5x74	17x70	30x70
tubes per rotor	120	192	120	192	120	64	120	120	120	120	100	120	92	32
Cat. No.	4222-93	4213-93	4214-93	4213	4214	4220	4214	4222-93	4222	4214-93	4223	4214	4232	4245-A

Tubes												
capacity in ml	12	30	50	100	100	250	650	750	750	250	500	
Ø x L in mm	17x100	25x110	29x115	40x115	40x115	62 x 122	97 x 139	97 x 152	96 x 135	60 x 162	96 x 147	
max. RCF ²⁾	4,777	4,777	4,867	4,777	4,777	4,777	4,958	4,958	4,958	4,777	4,958	
radius in mm	211	211	215	211	211	211	219	219	219	211	219	
Cat. No.	tubes with screw cap					5127²⁴⁾	0554²⁴⁾	0512²⁴⁾	4234-A	Corning[®]	Corning[®]	+4449

Adapter											
boring Ø x L in mm	17.5x70	26 x 70	30 x 96	41.5 x 70	41.5 x 70	62 x 90	97.5x105	97.5x105	97.5x105	62 x 125	97.5x105
tubes per rotor	64	44	24	16	16	4	4	4	4	4	4
Cat. No.	4220	4215	4249	4218	4218	4238	4258	4258	4258	6322	4258


1) For cooled versions: Lowest temperature achievable with precooling and max. speed.
 2) Please note that the RCF values indicated refer only to rotor performance. The max. permissible RCF of tubes used should be verified with the individual manufacturers. The max. RCF for glass tubes annotated with footnote 2) is 4,000.
 3.12) When using these tubes, bucket 4290 cannot be closed with lid 4291.
 3.13) When using these tubes, bucket 4295-A cannot be closed with lid 4229-B.
 24) At temperatures of over +40 °C and / or when not filled to capacity, bottles may warp during centrifugation.

SWING-OUT ROTOR, 4-PLACE | 4294




Rotor

max. RPM max. RCF ²⁾	4.500 min ⁻¹ 4.618
max. capacity	40 x 50 ml
run-up run-down, braked in sec	115 116
angle	90°
temperature in °C ¹⁾	+2
Cat. No.	4294



Bucket

lid bioseal ⁵⁾	4291
Cat. No.	4290

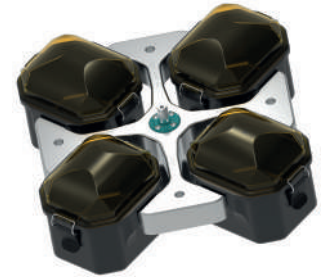

Tubes

capacity in ml	5	6	7	9	14	2.6-3.4	4.9	4-5.5	7.5-8.2	9-10	10	1.6-5	4-7	4-7	8.5-10
Ø x L in mm	12x75	12x82	12x100	14x100	16x101	13 x 65	13x90	15x75	15x92	16x92	15x102	13 x 75	13 x 100	16x75	16x100
max. RCF ²⁾	4,551	4,551	4,551	4,551	4,551	4,551	4,551	4,551	4,551	4,573	4,573	4,551	4,551	4,551	4,551
radius in mm	201	201	201	201	201	201	201	201	201	202	202	201	201	201	201
Cat. No.	tubes²⁾					blood collection / urine tubes									



Adapter

boring Ø x L in mm	13.2x57	13.2x57	13.2x57	17.5 x 62	17.5 x 62	13.2x57	13.2x57	17.5 x 62	17.5 x 62	17.5 x 63	17.5 x 63	13.2 x 57	13.2 x 57	17.5 x 62	17.5 x 62
tubes per rotor	200	200	200	168	168	200	200	168	168	132	132	200	200	168	168
Cat. No.	4273	4273	4273	4338	4338	4273	4273	4338	4338	4311	4311	4273	4273	4338	4338

Tubes

capacity in ml	15	10	12	15	15	50	50	50	50
Ø x L in mm	17x100	16x80	17x100	17x120	17x120	29x115	29x115	29x115	29x115
max. RCF ²⁾	4,551	4,551	4,437	4,607	4,607	4,607	4,607	4,517	4,517
radius in mm	201	201	196	204	204	204	204	200	200
Cat. No.	- 2)	tubes with screw cap							




Adapter

boring Ø x L in mm	17.5 x 62	17.5 x 62	17.2 x 57	17 x 60	17 x 60	30 x 60	30 x 60	30 x 56	30 x 56
tubes per rotor	168	168	112	68	112	32	40	32	40
Cat. No.	4338	4338	4310	4314	4320^{3,12)}	4321	4323^{3,12)}	4313	4339^{3,12)}


1) For cooled versions: Lowest temperature achievable with precooling and max. speed.
 2) Please note that the RCF values indicated refer only to rotor performance. The max. permissible RCF of tubes used should be verified with the individual manufacturers.
 The max. RCF for glass tubes annotated with footnote 2) is 4,000.
 3.12) When using these tubes, bucket 4290 cannot be closed with lid 4291.
 3.13) When using these tubes, bucket 4295-A cannot be closed with lid 4229-B.
 24) At temperatures of over +40 °C and / or when not filled to capacity, bottles may warp during centrifugation.












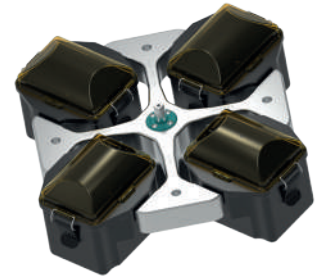




— SWING-OUT ROTOR, 4-PLACE | 4294

	
Rotor	
max. RPM max. RCF ²⁾	4,500 min ⁻¹ 4,573
max. capacity	24 plates
run-up run-down, braked in sec	115 116
angle temperature in °C ¹⁾	90° +5
Cat. No.	4294




	
Bucket	
lid bioseal [®]	5629
Cat. No.	4280



Plates								
W x D x H in mm	128x86x15	128x86x17.5	128x86x22	128x86x44.5	128x86x46	128x86x83	124x82x20	-
capacity in ml	-	-	-	-	-	-	-	0.2
max. RCF ²⁾	4,625	4,625	4,625	4,625	4,625	4,625	4,625	4,625
radius in mm	204	204	204	204	204	204	204	204
Cat. No.	MTP	MTP	CP	DWP	MS	QP	PCR plates 96-places	PCR strips
+								
Removal aid								
boring Ø x L in mm	-	-	-	-	-	-	-	-
plates / strips per rotor	24	24	20	8	4	4	4	48 x 8
Cat. No.	4279	4279	4279	4279	4279	4279	4279 + 1485	4279 + 1485






— SWING-OUT ROTOR, 4-PLACE | 4294

	
Rotor	
max. RPM max. RCF ²⁾	4,500 min ⁻¹ 4,867
max. capacity	20 Racks
run-up run-down, braked in sec	115 116
angle temperature in °C ¹⁾	90° +7
Cat. No.	4294




	
Bucket	
Cat. No.	4257

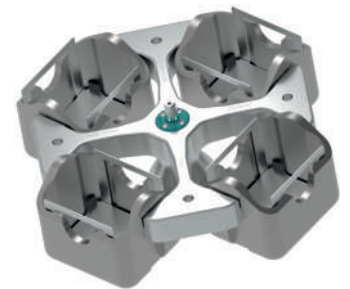

	
Rack	
W x D x H in mm	118 x 20 x 70
capacity in ml	-
max. RCF ²⁾	4,867
radius in mm	215
Cat. No.	Hitachi Rack
+	
Removal aid	
boring Ø x L in mm	-
tubes per rotor	20
Cat. No.	4259-A²³⁾

- 1) For cooled versions: Lowest temperature achievable with precooling and max. speed.
- 2) Please note that the RCF values indicated refer only to rotor performance. The max. permissible RCF of tubes used should be verified with the individual manufacturers. The max. RCF for glass tubes annotated with footnote 2) is 4,000.
- 23) When using removal frame 4259-A, please take the spacer out of carrier 4257.


SWING-OUT ROTOR, 4-PLACE | 4294



Rotor	
max. RPM max. RCF ²⁾	4,500 min ⁻¹ 5,184
max. capacity	4 x 1,000 ml
run-up run-down, braked in sec	115 116
angle temperature in °C ¹⁾	90° +5
Cat. No.	4294



Bucket	
adapter including lid	4255
Cat. No.	4254



Tubes

capacity in ml	5	7	9	15	25	50	100	2.6-3.4	2.7-3	4-5.5	4.5-5	4.9	7.5-8.2	9-10	10
Ø x L in mm	12x75	12x100	14x100	17x100	24x100	34x100	44x100	13 x 65	11x66	15x75	11x92	13x90	15x92	16x92	15x102
max. RCF ²⁾	4,618	4,618	4,777	4,777	4,505	4,573	4,551	4,618	4,618	4,777	4,618	4,618	4,777	4,777	4,777
radius in mm	204	204	211	211	199	202	201	204	204	211	204	204	211	211	211
Cat. No.	tubes²⁾							blood collection / urine tubes							



Adapter

boring Ø x L in mm	13 x 58	13 x 58	17,5 x 60	17,5 x 60	26 x 72	36 x 79	45 x 78	13,5 x 58	13 x 58	17,5 x 60	13 x 58	13,5 x 58	17,5 x 60	17,5 x 60	17,5 x 60
tubes per rotor	120	120	76	76	28	16	8	84	120	76	120	84	76	76	76
Cat. No.	4433	4433	4434	4434	4438	4439	4442	4435	4433	4434	4433	4435	4434	4434	4434

Tubes

capacity in ml	1.6-5	4-7	4-7	8	8.5-10	15	30	50	25	30	10	250	290	650	750
Ø x L in mm	13x75	13x100	16x75	16x81	16x100	17x120	25 x 110	29x115	25x90	25 x 110	16 x 80	61 x 122	62 x 137	97 x 139	97 x 152
max. RCF ²⁾	4,618	4,618	4,777	4,777	4,777	4,890	4,709	4,890	4,709	4,709	4,777	5,003	5,003	5,184	5,184
radius in mm	204	204	211	211	211	216	208	216	208	208	211	221	221	229	229
Cat. No.	blood collection / urine tubes							tubes with screw cap				5127²⁴⁾	-²⁴⁾	0554²⁴⁾	0512²⁴⁾



Adapter

boring Ø x L in mm	13,5 x 58	13,5 x 58	17,5 x 60	17,5 x 60	17,5 x 60	17 x 86	26 x 72	30 x 87	26 x 72	26 x 72	17,5 x 60	62 x 92	62 x 92	98 x 138	98 x 138
tubes per rotor	84	84	76	76	76	48	28	20	28	28	76	4	4	4	4
Cat. No.	4435	4435	4434	4434	4434	4437	4438	4441	4438	4438	4434	4443	4443	-	-

Tubes

capacity in ml	1,000	1,000	175	175	200	225	250	500
Ø x L in mm	96 x 176	98 x 138	61 x 118	61,5x144,3	60 x 130	61 x 137	60 x 162	96 x 147
max. RCF ²⁾	5,184	5,184	5,184	5,184	5,184	5,184	5,184	5,184
radius in mm	229	229	229	229	229	229	229	229
Cat. No.	4239²⁴⁾	4255	Falcon	Nalgene	Nunc®	Falcon	Corning®	Corning®




Adapter

boring Ø x L in mm	98 x 138	-	-	-	-	-	-	-
tubes per rotor	4	4	4	4	4	4	4	4
Cat. No.	-	-	4440	4430	4430	4440	4430	4449

- 1) For cooled versions: Lowest temperature achievable with precooling and max. speed.
- 2) Please note that the RCF values indicated refer only to rotor performance. The max. permissible RCF of tubes used should be verified with the individual manufacturers. The max. RCF for glass tubes annotated with footnote 2) is 4,000.
- 3.15) When using these tubes, bucket 4255 cannot be closed with its lid.
- 24) At temperatures of over +40 °C and / or when not filled to capacity, bottles may warp during centrifugation.

SWING-OUT ROTOR, 4-PLACE | 4294




Rotor

max. RPM max. RCF ²⁾	4,500 min ⁻¹ 5,252
max. capacity	4 blood bags
run-up run-down, braked in sec	115 116
angle temperature in °C ¹⁾	90° +2
Cat. No.	4294



Bucket

Cat. No.	4293
-----------------	-------------



Blood bags

capacity in ml	450	500
blood bags	3-place	3-place
max. RCF ²⁾	5,252	5,252
radius in mm	232	232

Cat. No.	blood bags	
-----------------	-------------------	--



Insert

boring Ø x L in mm	-	-
blood bags per rotor	4	4
Cat. No.	4244-A	4244-A



Additional blood bank accessories can be found on [page 185](#)

SWING-OUT ROTOR, 4-PLACE | 4294




Rotor

max. RPM max. RCF ²⁾	4,500 min ⁻¹ 5,071
max. capacity	4 blood bags
run-up run-down, braked in sec	115 116
angle temperature in °C ¹⁾	90° +3
Cat. No.	4294



Bucket


Cat. No.	4298-A
-----------------	---------------



Blood bags

capacity in ml	450	500	750	1,000
blood bags	4-place	4-place	1-place	1-place
max. RCF ²⁾	5,003	5,003	5,003	5,071
radius in mm	221	221	221	224

Cat. No.	blood bags			
-----------------	-------------------	--	--	--



Insert

boring Ø x L in mm	-	-	-	-
blood bags per rotor	4	4	4	4
Cat. No.	4237-A	4237-A	4237-A	-




Additional blood bank accessories can be found on [page 185](#)

- 1) Lowest attainable temperature in precooled refrigerated centrifuges at max. speed. Lower temperatures can be attained by reducing the speed.
- 2) Please note that the RCF values indicated refer only to rotor performance. The max. permissible RCF of tubes used should be verified with the individual manufacturers. The max. RCF for glass tubes annotated with footnote 2) is 4,000.

SWING-OUT ROTOR, 6-PLACE | 4296



Rotor	
max. RPM max. RCF ²⁾	4,000 min ⁻¹ 3,363
max. capacity	6 x 100 ml
run-up run-down, braked in sec	33 50
angle max. noise level	90° 52 dB (A)
temperature in °C ¹⁾	0
Cat. No.	4296



Bucket	
lid	5053
Cat. No.	5051



Vessels															
capacity in ml		1.5	2	1.5	2	5	6	7	9	15	25	50	100	100	1-8
Ø x L in mm		11 x 38	11 x 38	11 x 38	11 x 38	12 x 75	12 x 82	12 x 100	14 x 100	17 x 100	24 x 100	34 x 100	44 x 100	40 x 115	simple / multiple
max. RCF ²⁾	top / bottom	2,486 / 3,363	2,486 / 3,363	3,363	3,363	3,309	3,309	3,291	3,309	3,291	3,291	3,291	3,291	3,291	2,290 / 3,274
radius in mm	top / bottom	139 / 188	139 / 188	188	188	185	185	184	185	184	184	184	184	184	128 / 183
Cat. No.		microliter tubes				tubes²⁾									cyto chambers

Adapter															
boring Ø x L in mm		12.5x42	12.5x42	11.5x50	11.5x50	12.5x42	12.5x42	12.5x86	16x50	17.5x86	26x86	36x86	45.5x86	42x86	-
vessels per rotor		240	240	96	96	120	120	120	72	72	30	12	6	6	12
Cat. No.		5257	5257	5281	5281	5227	5227	5247¹⁵⁾	5264	5248¹⁵⁾	5242	5243	5262	5249	5280

Vessels																
capacity in ml		1.1-1.4	2.6-2.9	2.7-3	4-5.5	4.5-5	4.9	7.5-8.2	9-10	1.6-5	4-7	8.5-10	15	50	15	30
Ø x L in mm		8x66	13x65	11 x 66	15 x 75	11 x 92	13x90	15x92	16x92	13x75	16x75	16x100	17x120	29x115	17x100	25x110
max. RCF ²⁾		3,274	3,345	3,309	3,309	3,309	3,345	3,309	3,291	3,345	3,309	3,291	3,434	3,363	3,434	3,291
radius in mm		183	187	185	185	185	187	185	184	187	185	184	192	188	192	184
Cat. No.		blood collection / urine tubes										tubes with screw cap				

Adapter																
boring Ø x L in mm		11 x 44	13.5x52	12.5x42	16x50	12.5x42	13.5x52	16x50	17,6x82,5	13.5x52	16x50	17,5x82,5	17x90	30x82,5	17x90	26 x 82,5
vessels per rotor		120	72	120	72	120	72	72	66	72	72	72	42	12	42	30
Cat. No.		5267	5268	5227	5264	5227	5268	5264	5258	5268	5264	5248	6306	5259	6306	5266

Vessels		
capacity in ml		50
Ø x L in mm		29x115
max. RCF ²⁾		3,291
radius in mm		184
Cat. No.		tubes with screw cap

Adapter		
boring Ø x L in mm		26 x 82,5
vessels per rotor		12
Cat. No.		5243

1) Lowest attainable temperature in precooled refrigerated centrifuges at max. speed. Lower temperatures can be attained by reducing the speed.
 2) Please note that the RCF values indicated refer only to rotor performance. The max. permissible RCF of tubes used should be verified with the individual manufacturers. The max. RCF for glass tubes annotated with footnote 2) is 4,000.
 3.11) When using these tubes, bucket 5051 cannot be closed with lid 5053.


SWING-OUT ROTOR, 6-PLACE | 4296



Rotor	
max. RPM max. RCF	4,000 min ⁻¹ 3,631
max. capacity	6 x 250 ml
run-up run-down, braked in sec	33 50
angle max. noise level	90° 59 dB (A)
temperature in °C ¹⁾	-2
Cat. No.	4296



Bucket	
lid bioseal ⁵⁾	5093
Cat. No.	5092

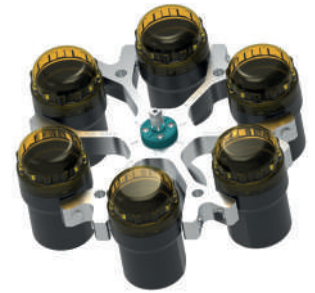

Vessels															
capacity in ml	5	6	7	15	25	50	100	100	250	1.1-1.4	1.1-1.4	2.6-2.9	2.7-3	2.7-3	4.9
Ø x L in mm	12x75	12x82	12x100	17x100	24x100	34x100	44x100	40x115	65x115	8 x 66	8 x 66	13 x 65	11x66	11x66	13x90
max. RCF ²⁾	3,542	3,542	3,542	3,488	3,434	3,488	3,488	3,488	3,641	3,488	3,077	3,077	3,488	3,077	3,488
radius in mm	198	198	198	195	192	195	195	195	203	195	172	172	195	172	195
Cat. No.	tubes²⁾									blood collection / urine tubes					

Adapter															
boring Ø x L in mm	12.8x42	12.8x42	12.8x79.5	17.5x56.7	25.5x74	35.5x77.5	45.5x85	42x86.5	66x103	13.5x56.7	12.8x54.5	12.8x54.5	13.5x56.7	12.8x54.5	13.5x56.7
vessels per rotor	72	72	72	48	24	6	6	6	6	48	72	72	48	72	48
Cat. No.	5128	5128	5120	5136	5122	5124	5125	5126	1791	5137	5138	5138	5137	5138	5137

Vessels															
capacity in ml	4-4.5	4.5-5	7.5-8.2	9-10	10	1.6-5	4-7	4-7	8	8.5-10	15	50	25	30	50
Ø x L in mm	15x75	11x92	15x92	16x92	15x102	13x75	16x75	13x100	16x125	16x100	17x120	29x115	25x90	25 x 110	29x115
max. RCF ²⁾	3,488	3,542	3,488	3,488	3,488	3,077	3,488	3,542	3,542	3,488	3,631	3,631	3,363	3,434	3,560
radius in mm	195	198	195	195	195	172	195	198	198	195	203	203	188	192	199
Cat. No.	blood collection / urine tubes										tubes with screw cap				


Adapter															
boring Ø x L in mm	17.5x56.7	12.8x79.5	17.5x56.7	17.5x56.7	17.5x56.7	12.8x54.5	17.5x56.7	12.8x79.5	17.5x79.5	17.5x56.7	17x85	30x85	26x73	25.5x87	30x99
vessels per rotor	48	72	48	48	48	72	48	72	42	48	42	12	18	24	12
Cat. No.	5136	5120	5136	5136	5136	5138	5136	5120	5121⁴⁾	5136	5129	5123	5134	5122	5135

Vessels			
capacity in ml	10	250	290
Ø x L in mm	16 x 80	61 x 122	62 x 137
max. RCF ²⁾	3,488	3,631	3,631
radius in mm	195	203	203
Cat. No.	-	5127²⁴⁾	-²⁴⁾

Adapter			
boring Ø x L in mm	17.5x56.7	62x90	62x90
vessels per rotor	48	6	6
Cat. No.	5136	6319	6319

- 1) Lowest attainable temperature in precooled refrigerated centrifuges at max. speed. Lower temperatures can be attained by reducing the speed.
- 2) Please note that the RCF values indicated refer only to rotor performance. The max. permissible RCF of tubes used should be verified with the individual manufacturers. The max. RCF for glass tubes annotated with footnote 2) is 4,000.
- 3,4) When using these tubes, bucket 5051 or 5092 cannot be closed with lid 5053 or 5093.
- 4) Please remove the spacer.
- 5) Tested by the TÜV in conformity with DIN EN 61010, section 2 - 020.
- 24) At temperatures of over +40 °C and / or when not filled to capacity, bottles may warp during centrifugation.


SWING-OUT ROTOR, 2-PLACE | 4282


	
Rotor	
max. RPM max. RCF	3,600 min ⁻¹ 2,652
max. capacity	20 plates
run-up run-down, braked in sec	87 94
angle max. noise level	90° 58 dB (A)
temperature in °C ¹⁾	-2
Cat. No.	4282





	
Bucket	
Cat. No.	4285-A



							
Plates							
W x D x H in mm	128x86x15	128x86x17.5	128x86x22	128x86x44.5	84x59x46	124x82x20	-
max. RCF ²⁾	2,434	2,434	2,434	2,434	2,434	2,434	2,434
radius in mm	168	168	168	168	168	168	168
Cat. No.	MTP	MTP	CP	DWP	MS	PCR plates	PCR strips


							
Removal aid							
boring Ø x L in mm	-	-	-	-	-	-	-
plates / strips per rotor	16	12	12	4	4	4	48 x 8
Cat. No.	4281	4281	4281	4281	4281	4281+1485	4281+1485

			
Racks			
W x D x H in mm	176x20x41	118x20x70	193x25x60
max. RCF ²⁾	2,652	2,652	2,652
radius in mm	183	183	183
Cat. No.	Olympus Racks	Hitachi Racks	Behring Racks

			
Adapter			
boring Ø x L in mm	-	-	-
plates / racks per rotor	12	20	10
Cat. No.	4283-B	4287-B	4288-A

1) Lowest attainable temperature in precooled refrigerated centrifuges at max. speed. Lower temperatures can be attained by reducing the speed.
 2) Please note that the RCF values indicated refer only to rotor performance. The max. permissible RCF of tubes used should be verified with the individual manufacturers. The max. RCF for glass tubes annotated with footnote 2) is 4,000.

— ANGLE ROTOR, 6-PLACE | 4266



Rotor

max. RPM max. RCF	9,500 min ⁻¹ 14,025
max. capacity	6 x 250 ml
run-up run-down, braked in sec	82 96
angle	25°
temperature in °C ¹⁾	+2
Cat. No.	4266



Lid bioseal⁵⁾ and phenol-resistant

Cat. No.

INCLUSIVE



Vessels

capacity in ml	15	25	94	10	30	50	85	94	250
Ø x L in mm	17 x 100	24 x 100	38 x 102	16 x 80	26 x 95	29 x 107	38 x 106	38 x 102	61.5 x 122
max. RCF ²⁾	13,319	12,915	12,310	13,420	12,915	12,108	12,310	12,310	14,025
radius in mm	132	128	122	133	128	120	122	122	139
Cat. No.	tubes²⁾			tubes with screw cap					5127²⁴⁾




Adapter

boring Ø x L in mm	17.6 x 83	26 x 80	38.6 x 88	16.6 x 70	26 x 80	29 x 90	38.6 x 88	38.6 x 88	61.5 x 109
vessels per rotor	42	18	6	48	18	6	6	6	6
Cat. No.	5646	5642	5644	5641	5642	5643	5644	5644	-

1) Lowest attainable temperature in precooled refrigerated centrifuges at max. speed. Lower temperatures can be attained by reducing the speed.
 2) Please note that the RCF values indicated refer only to rotor performance. The max. permissible RCF of tubes used should be verified with the individual manufacturers. The max. RCF for glass tubes annotated with footnote 2) is 4,000.
 5) Tested by the TÜV in conformity with DIN EN 61010, section 2 - 020.
 24) At temperatures of over +40 °C and / or when not filled to capacity, bottles may warp during centrifugation.

— ANGLE ROTOR, 6-PLACE | 4246



Rotor	
max. RPM max. RCF	11,500 min ⁻¹ 18,038
max. capacity	6 x 94 ml
run-up run-down, braked in sec	64 64
angle	45°
temperature in °C ¹⁾	+4
Cat. No.	4246

Lid bioseal[®] and phenol-resistant

Cat. No.

INCLUSIVE



Vessels															
capacity in ml	0.5	1.5	2.0	3	15	25	50	94	7.5 – 8.2	9 – 10	10	8.5 – 10	5	15	50
Ø x L in mm	10.7x46	11x38	11x38	10x60	17x100	24x100	34x100	38x102	15x92	16x92	15x102	16x100	17x51	17x120	29x115
max. RCF ²⁾	17,299	17,299	17,299	17,299	17,003	16,560	17,743	18,038	17,003	17,003	17,003	17,003	16,856	17,299	17,595
radius in mm	117	117	117	117	115	112	120	122	115	115	115	115	114	117	119
Cat. No.	pediatric	microliter tubes			tubes²⁾				blood collection / urine tubes				-	tubes with screw cap	

Adapter															
boring Ø x L in mm	11.4x39	11.4x39	11.4x39	11.4x39	17.5x91.5	26x85	35x89.3	38.2x89.6	17.5x91.5	17.5x91.5	17.5x91.5	17.5x91.5	17x51	17x106	29.8x96.7
vessels per rotor	24	24	24	24	6	6	6	6	6	6	6	6	6	6	6
Cat. No.	1449	1449	1449	1449	1451	1447	1463	-	1451	1451	1451	1451	1476	1466	1454

Vessels				
capacity in ml	10	30	50	85
Ø x L in mm	16x80	26x95	29x107	38 x 106
max. RCF ²⁾	17,003	16,560	17,299	18,038
radius in mm	115	112	117	122
Cat. No.	tubes with screw cap			

Adapter				
boring Ø x L in mm	16.5x74	26x85	29x92	38.2x89.6
vessels per rotor	12	6	6	6
Cat. No.	1448	1447	1446	-

1) Lowest attainable temperature in precooled refrigerated centrifuges at max. speed. Lower temperatures can be attained by reducing the speed.
 2) Please note that the RCF values indicated refer only to rotor performance. The max. permissible RCF of tubes used should be verified with the individual manufacturers. The max. RCF for glass tubes annotated with footnote 2) is 4,000.
 5) Tested by the TÜV in conformity with DIN EN 61010, section 2 - 020.

— ACCESSORIES FOR CENTRIFUGING BLOOD BAG SYSTEMS



Hettliner

Blood bags can be secured in adapters using HettLiners. After centrifuging, they can be removed by their loops without disturbing the sediment.

Cat. No. 4564



Set of compensatory weights

If blood bag carriers are not filled to the same weight, then compensatory weights can be used to make up the difference.

One set includes:
 40 balancing weights, 2 g each; 20 balancing weights, 5 g each; 10 balancing weights, 10 g each; 5 balancing weights, 20 g each; 5 balancing weights, 40 g each

Cat. No. 4566



Loading station

Secure your samples and avoid accidental spillage with the convenient Loading Station for centrifuge inserts. The Hettich Loading Station allows users to confidently hold and manage their samples without the risk of the inserts toppling over.

Cat. No. 4509

— CERTIFICATIONS / REGISTRATIONS

Product certification:



www.tuev-sued.de/ps-zert



Product registration:



Company certifications:



— DIMENSIONS

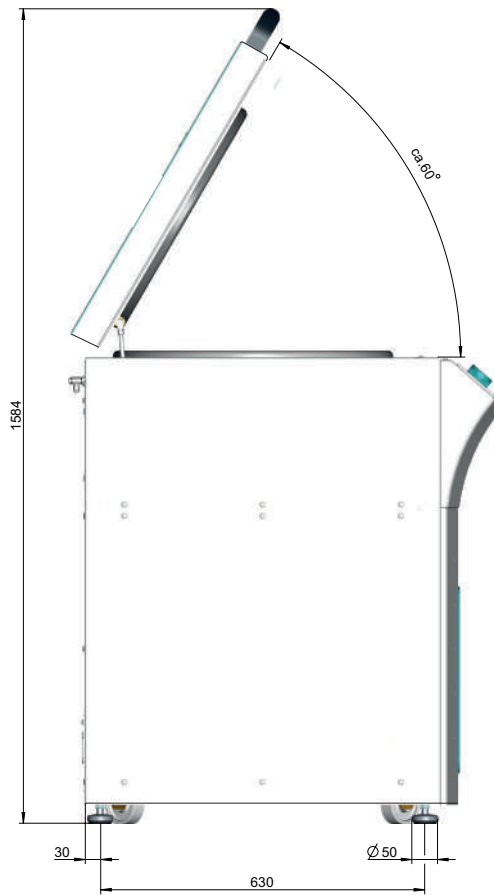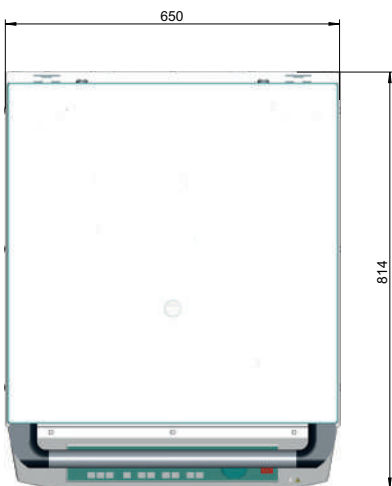

EU-Konformitätserklärung

EU Declaration of conformity

des Herstellers

of the manufacturer

Andreas Hettich GmbH & Co. KG • Föhrenstrasse 12 • D-78532 Tuttlingen • Germany
SRN: DE-MF-000010680

Hiermit erklären wir in unserer Verantwortung,
dass das bezeichnete Gerät:

We hereby declare under our responsibility
that the designated device:

Geräteart	Zentrifuge
Name	ROTIXA 500 RS
Basic UDI-DI	040506740100029L
GMDN	15115
Klassifizierung	Medizinprodukt, Klasse IIa (Anhang VIII, Kapitel III, Regel 3)
Gemäß	Verordnung (EU) 2017/745 Anhang IX
Mitwirkende Benannte Stelle	mdc medical device certification GmbH; CE 0483 Kriegerstraße 6; 70191 Stuttgart; Germany

Type of device	Centrifuge
Name	ROTIXA 500 RS
Basic UDI-DI	040506740100029L
GMDN	15115
Classification	Medical Device, class IIa (Annex VIII, Chapter III, Rule 3)
according to	Regulation (EU) 2017/745 Annex IX
Involved Notified Body	mdc medical device certification GmbH; CE 0483 Kriegerstraße 6; 70191 Stuttgart; Germany

inklusive des mit dem Gerät
konformitätsbewerteten Zubehörs laut Zubehörliste
der zugehörigen technischen Dokumentation, den
einschlägigen Bestimmungen der Verordnung
(EU) 2017/745 über Medizinprodukte entspricht.

and its accessories, which are listed in the rela-
ted technical documentation and whose conform-
ity has been assessed together with the device,
complies with the relevant provisions of the
Regulation (EU) 2017/745 on medical devices.

Zweckbestimmung

Bei dem vorliegenden Gerät handelt es sich um
eine Laborzentrifuge, die für medizinische
Anwendungen geeignet ist. Ihre ausschließliche
therapeutische Zweckbestimmung besteht darin,
Blut in Blutbeutelssystemen zu zentrifugieren. Die
separierten Blutkomponenten werden von einem
anderen Gerät (Separator) in entsprechende
Satellitenbeutel überführt. Die so gewonnenen
Einzelkomponenten werden dann für die
Transfusion oder Autotransfusion eingesetzt.
Die Zentrifuge darf nur von Fachpersonal in
Blutspendediensten oder Krankenhäusern
betrieben werden.
Die Zentrifuge ist nur für die oben genannten
Verwendungszwecke bestimmt. Eine andere oder
darüberhinausgehende Benutzung gilt als nicht
bestimmungsgemäß. Für hieraus entstehende
Schäden haftet die Firma Andreas Hettich GmbH &
Co. KG nicht. Zur bestimmungsgemäßen
Verwendung gehört auch die Beachtung aller
Hinweise aus der Bedienungsanleitung und die

Intended use

This device is a laboratory centrifuge suitable for
medical applications. Their exclusive therapeutic
purpose is to centrifuge blood in blood bag
systems. The separated blood components are
transferred by another device (separator) into
corresponding satellite bags. The individual
components obtained in this way are then used
for transfusion or autotransfusion.

The centrifuge is only to be operated by qualified
personnel working for blood donation services or
hospitals.

The centrifuge is only intended for the uses
referred to above. Any other use or use beyond
this is considered improper. Andreas Hettich
GmbH & Co. KG shall not be liable for any
damage arising from this. Intended use also
includes the observation of all instructions in the
Operating Manual and compliance with the
required inspection and maintenance intervals.

Einhaltung der Inspektions- und Wartungsintervalle.

Das Gerät entspricht auch den anwendbaren Bestimmungen der folgenden europäischen Richtlinien und Verordnungen

- 2006/42/EG „Maschinenrichtlinie“
- 2014/30/EU „EMV-Richtlinie“
- 2014/35/EU „Niederspannungsrichtlinie“
- 2011/65/EG „RoHS-Richtlinie“
(ohne Beteiligung einer benannten Stelle)
- (EG) 1907/2006 „REACH Verordnung“
(ohne Beteiligung einer benannten Stelle)

Angewandte Normen:

Siehe Liste der angewandten Normen, die Teil der technischen Dokumentation ist.

The device also complies to the applicable provisions of the following European directives, ordinances and standards

- 2006/42/EC "Directive on machinery"
- 2014/30/EU "EMC Directive"
- 2014/35/EU „Low Voltage Directive“
- 2011/65/EC "RoHS Directive"
(without involvement of a notified body)
- (EC) 1907/2006 „Regulation on REACH“
(without involvement of a notified body)

Standards applied:

See the list of applied standards that forms part of the technical documentation.

Tuttlingen, 30.10.2023



Klaus-Günter Eberle
Geschäftsführer, Chief Executive Officer



Diese Konformitätserklärung ist gültig von 30.10.2023 bis 25.08.2027

This declaration of conformity is valid from 30.10.2023 until 25.08.2027