

Медицинский кислородный датчик O2 cell Maquet Siemens для  
Servo-I Servo-S артикул 66 40 044 6640044



упаковка 1 штука

метод регистрации - ультразвуковой

обслуживание датчика - необслуживаемый

Номинальный срок службы - не нормируется


Рабочая температура: от 0 до 45°C

Вентиляторы Servo-I должны иметь версию не ниже 1.02.04 Вентиляторы

Servo-S могут иметь любую версию

P/N	Original Part no.	Brand
U938-01A	M-11	International Technologies
U938-01B	M-15	International Technologies
U938-01C	M-03	International Technologies
U938-01D	M-04	International Technologies
U938-01E	M-02	ITG
U938-02A	PSR-11-917M	Analytical Industries Inc
U938-02B	PSR-11-75-KE8	Analytical Industries Inc
U938-02C	PSR-11-75-KE4	Analytical Industries Inc
U938-02D	PSR-11-915-4	Analytical Industries Inc
U938-02E	PSR-11-75-KE250A	Analytical Industries Inc
U938-02F	PSR-11-75-KE7	Analytical Industries Inc
U938-02H	PSR-11-75-KE8	Analytical Industries Inc
U938-02J	PSR-11-917-M2	Analytical Industries Inc
U938-02G	PSR-11-60-08	Analytical Industries Inc
U938-02K	GPR-11-60-RTS	Analytical Industries Inc
U938-03A	MOX-20	City Technology
U938-03B	MOX-2	City Technology
U938-03C	MOX-3	City Technology
U938-03D	MOX-4	City Technology
U938-04A	MAX 10	Maxtec
U938-04B	MAX 12	Maxtec
U938-04C	MAX 250A	Maxtec
U938-04D	MAX 250E	Maxtec
U938-04E	MAX 250B	Maxtec
U938-05A	MX01049	Siemens Drager / OXY Trace / VE

P/N	Original Part no.	Brand
U938-17A	MX01050	Drager
U938-05B	6850645	Siemens Drager
U938-06A	66 40 044	Maquet
U938-07A	OOM201	EnviteC
U938-07B	OOM202	EnviteC
U938-07C	OOM204	EnviteC
U938-07D	OOM102-1	EnviteC
U938-07E	OOM105	EnviteC
U938-07F	OOM102	EnviteC
U938-07G	OOM101	EnviteC
U938-07H	OOM103	EnviteC
U938-07J	OOM103-1	EnviteC
U938-07K	OOM103-1M	EnviteC
U938-07L	OOM104	EnviteC
U938-07M	OOM105	EnviteC
U938-07N	OOM106	EnviteC
U938-07P	OOM107	EnviteC
U938-07Q	OOM107-2	EnviteC
U938-07R	OOM110	EnviteC
U938-07S	OOM202-1	EnviteC
U938-07T	OOM202-2	EnviteC
U938-07U	OOM202-2S	EnviteC
U938-08A	T-7	Teledyne
U938-09A	R-17MED	Teledyne
U938-10A	396200/01	Hamilton
U938-12A	7700	Aeon

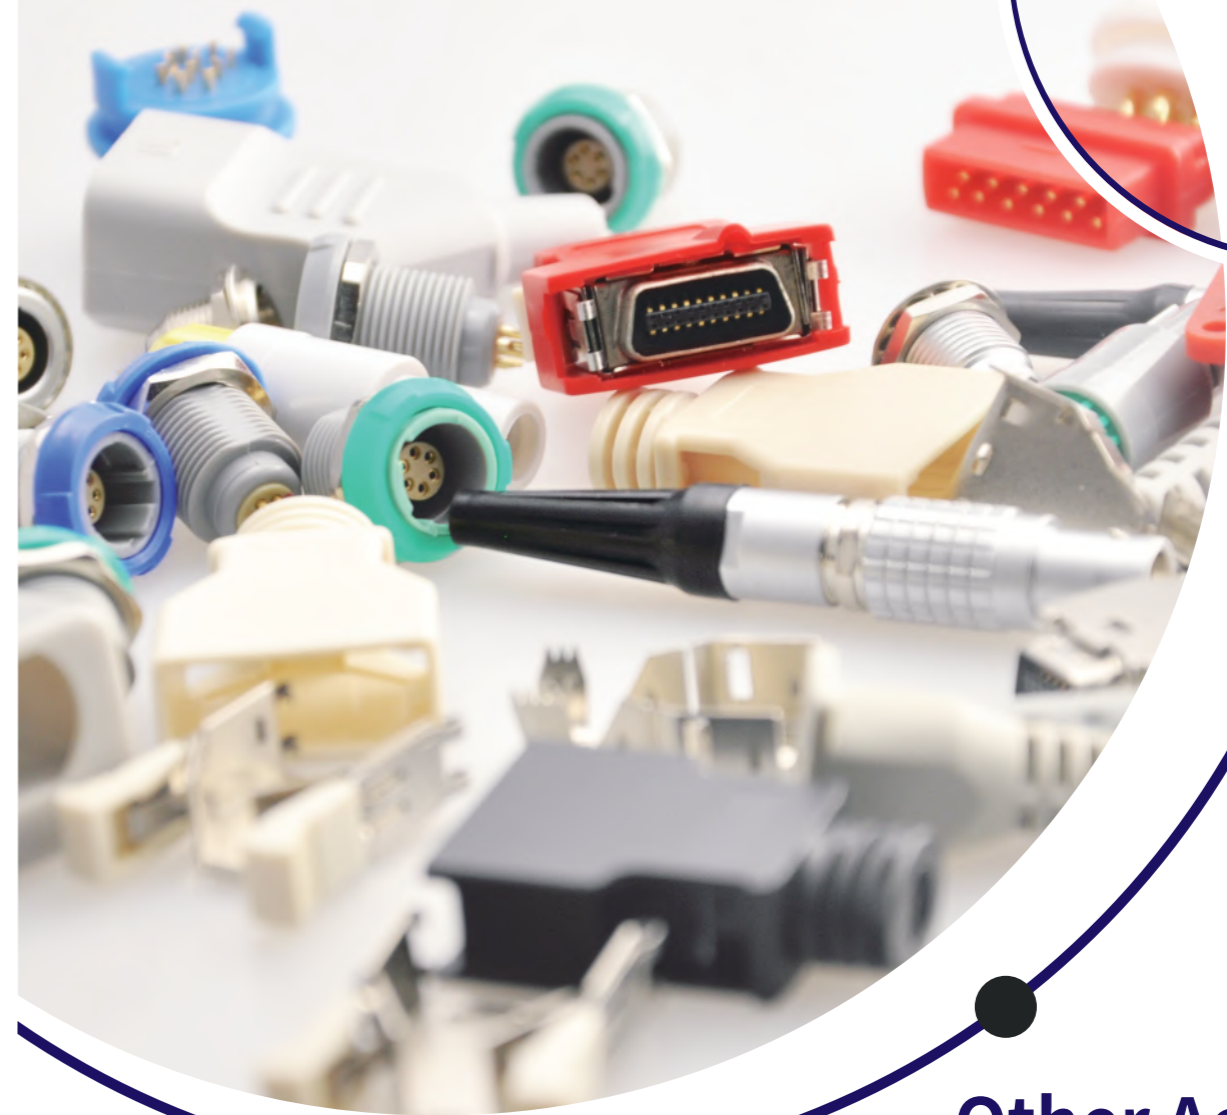

## Other Accessories



# EC Declaration of Conformity

**Name of Manufacturer:** Shenzhen Upnmed Equipment Co.,Ltd  
**Address of Manufacturer:** 301,Building #41st ,The 3rd Industrial Zone, Xitian Community, Gongming Street, Guangming District, Shenzhen,China,zip:518106  
**Declares that product:** Oxygen Sensor  
**Type/Model of product:** U938 series  
**Product Classification** Class I  
**CONFORMITY ASSESSMENT ROUTE:** EU Directive 2017/745 Annex I &VII

Conformed to 93/42/EEC (including Directive 2007/47/EC) as attested by conformity with the following harmonized standards:

EN980:2008 EN1041:2008 EN ISO 14971:2012 EN ISO 10993-1:2010 EN ISO10993-5:2009  
EN ISO 10993-10:2010

We,Shenzhen Upnmed Equipment Co.,Ltd,hereby declare that the equipment bearing the trade name and model number specified above was tested conforming to the applicable Rules under the most accurate measurement standards possible, and that all the necessary steps have been taken and are in force to assure that production units of the same equipment will continue to comply with the requirements.

Name and address of the person authorized

Company Name: **SUNGO Europe B.V.**

Company Address: Fascinatio Boulevard 522,Unit 1.7,2909VA Capelle aan den IJssel, The Netherlands

Signature



Position/title Director for Europe and the CIS regions