

# Qubit™ 1X dsDNA HS Assay Kits

**Catalog No.** Q33230, Q33231

**Pub. No.** MAN0017455

**Rev.** C.0

## Product information

Qubit™ 1X dsDNA HS (High Sensitivity) Assay Kits make DNA quantitation easy and accurate. The kits include a ready-to-use assay buffer and DNA standards. To perform the assay, simply dilute your sample (any volume from 1–20 µL is acceptable) into the 1X working solution provided, then read the concentration using a Qubit™ Fluorometer. The assay is recommended for initial sample concentrations ranging from 10 pg/µL to 100 ng/µL providing a core detection range of 0.2 ng to 100 ng of DNA. Additionally, the assay is selective for double-stranded DNA (dsDNA) over RNA (Figure 2, page 6) and tolerant of common contaminants such as salts, free nucleotides, solvents, detergents, or protein (Table 2, page 7). The assay is performed at room temperature, and the signal is stable for 3 hours when the samples are protected from light. In addition to the Qubit™ 1X dsDNA HS Assay Kits described here, we also offer other kits for assaying RNA, protein, and dsDNA at a higher concentration range (Table 3, page 8) as well as the Qubit™ dsDNA HS Assay - Lambda Standard (Cat. No. Q33233).

**Note:** To use the assay with the Qubit™ 2 and 3 models, you will need to download and install the appropriate program file from [thermofisher.com/qubit](http://thermofisher.com/qubit).

**Table 1.** Contents and storage

| Material                                                                                       | Amount                 |                        | Concentration         | Storage*                                                                             |
|------------------------------------------------------------------------------------------------|------------------------|------------------------|-----------------------|--------------------------------------------------------------------------------------|
|                                                                                                | Q33230<br>(100 assays) | Q33231<br>(500 assays) |                       |                                                                                      |
| Qubit™ 1X dsDNA HS Working Solution<br>(Component A)                                           | 50 mL                  | 250 mL                 | 1X                    | <ul style="list-style-type: none"><li>• 2–8°C</li><li>• Protect from light</li></ul> |
| Qubit™ 1X dsDNA HS Standard #1<br>(Component B)                                                | 1 mL                   | 5 mL                   | 0 ng/μL in TE buffer  | <ul style="list-style-type: none"><li>• 2–8°C</li></ul>                              |
| Qubit™ 1X dsDNA HS Standard #2<br>(Component C)                                                | 1 mL                   | 5 mL                   | 10 ng/μL in TE buffer |                                                                                      |
| * When stored as directed, the kits are stable for at least 6 months from the date of receipt. |                        |                        |                       |                                                                                      |

**Materials required but not provided**

- Nuclease-free pipettors and tips
- Qubit™ Assay Tubes (Cat. No. Q32856)
- Qubit™ Flex Tube Strips (Cat. No. Q33252)

## Critical assay parameters

---

|                                          |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                              |
|------------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Assay temperature</b>                 | <p>The Qubit™ 1X dsDNA HS Assay delivers optimal performance when all solutions are at room temperature (18–28°C). Temperature fluctuations can influence the accuracy of the assay.</p> <p>To minimize temperature fluctuations, insert all assay tubes into the Qubit™ Fluorometer only for as much time as it takes for the instrument to measure the fluorescence; the Qubit™ Fluorometers can raise the temperature of the assay solution significantly, even over a period of a few minutes. Do not hold the assay tubes in your hand before reading because this warms the solution and results in a different reading.</p>                                                                                           |
| <b>Incubation time</b>                   | <p>To allow the Qubit™ 1X dsDNA HS Assay to reach optimal fluorescence, incubate the tubes for 2 minutes after mixing the sample or the standard with the working solution. After this incubation period, the fluorescence signal is stable for 3 hours at room temperature when samples are protected from light.</p>                                                                                                                                                                                                                                                                                                                                                                                                       |
| <b>Photostability of Qubit™ reagents</b> | <p>The Qubit™ reagents exhibit high photostability in the Qubit™ Fluorometer, showing &lt;0.3% drop in fluorescence after 9 readings and &lt;2.5% drop in fluorescence after 40 readings. However, if the assay tube remains in the Qubit™ Fluorometer for multiple readings, a temporary reduction in fluorescence will be observed as the solution increases in temperature. Note that the temperature inside the Qubit™ Fluorometer may be as much as 3°C above room temperature after 1 hour. For this reason, if you want to perform multiple readings of a single tube, remove the tube from the instrument and let it equilibrate to room temperature for 30 seconds before taking another reading.</p>               |
| <b>Qubit™ Fluorometer calibration</b>    | <p>For each assay, you have the choice to run a new calibration or use the values from the previous calibration. When you first use the instrument, perform a new calibration each time. As you become familiar with the assays, the instrument, your pipetting accuracy, and significant temperature fluctuations within your laboratory, you can decide how comfortable you are using the calibration data stored from the last time the instrument was calibrated. Additionally, remember that the fluorescence signal in the tubes containing standards and samples is stable for no longer than 3 hours. See Figure 3 (page 6) for an example of the calibration curve used to generate the quantification results.</p> |
| <b>Handling and disposal</b>             | <p>No data are currently available that address the mutagenicity or toxicity of the Qubit™ 1X dsDNA HS Reagent (the dye in Component A). This reagent is known to bind nucleic acids. Treat the Qubit™ 1X dsDNA HS buffer with the same safety precautions as all other potential mutagens and dispose of the dye in accordance with local regulations.</p>                                                                                                                                                                                                                                                                                                                                                                  |

## Prepare standards and samples

---

This protocol assumes that you are preparing standards for calibrating the Qubit™ Fluorometer. If you plan to use the last calibration performed on the instrument (see “Qubit™ Fluorometer calibration”, page 2), you need fewer tubes (step 1.1) and less working solution (step 1.3).

- 1.1 Set up the required number of assay tubes (or tube strips) for standards and samples. The Qubit™ 1X dsDNA HS Assay requires 2 standards.

**Note:** Use thin-wall, clear, 0.5-mL PCR tubes (Cat. No. Q32856) for the Qubit™ 4 Fluorometer and 8 × 200 µL tube strips (Cat. No. Q33252) for the Qubit™ Flex Fluorometer.

- 1.2 Label the tube lids.

**Note:** Do not label the side of the tube as this could interfere with the sample read. Label the lid of each standard tube correctly. Calibration of the Qubit™ Fluorometer requires the standards to be inserted into the instrument in the right order.

- 1.3 Add 10 µL of each Qubit™ standard to the appropriate tube.

- 1.4 Add 1–20 µL of each user sample to the appropriate tube.

**Note:** If you are adding 1–2 µL of sample, use a P-2 pipette for best results.

- 1.5 Add the Qubit™ 1X dsDNA working solution to each tube such that the final volume is 200 µL.

**Note:** The final volume in each tube must be 200 µL. Each standard tube requires 190 µL of Qubit™ working solution, and each sample tube requires anywhere from 180–199 µL. Ensure that you have sufficient Qubit™ working solution to accommodate all standards and samples.

**Note:** To avoid any cross-contamination, we recommend that you remove the total amount of working solution required for your samples and standards from the working solution bottle and then add the required volume to the appropriate tubes instead of pipetting directly from the bottle to each tube.

- 1.6 Mix each sample vigorously by vortexing for 3–5 seconds.

- 1.7 Allow all tubes to incubate at room temperature for 2 minutes, then proceed to “Read standards and samples”. Follow the procedure appropriate for your instrument:

## Read standards and samples

---

### Qubit™ Flex Fluorometer

- 2.1 On the **Home** screen of the Qubit™ Flex Fluorometer, press the **1X dsDNA High Sensitivity (HS)** assay icon. The “Read standards” screen is displayed. Press **Read Standards & run samples** to proceed.

**Note:** If you have already performed a calibration for the selected assay, the instrument prompts you to choose between reading new standards and running samples using the previous calibration. If you want to use the previous calibration, press **Run samples** and skip to step 2.4. Otherwise, continue with step 2.2.

- 2.2 Insert the tube strip containing Standard #1 into the sample chamber, close the lid, then press **Run standards**. When the reading is complete (~3 seconds), remove Standard #1.
- 2.3 Insert the tube strip containing Standard #2 into the sample chamber, close the lid, then press **Read standards**. When the reading is complete, remove Standard #2.

The instrument displays the graphical results on the **Standards complete** screen. For information on interpreting the calibration results, refer to the *Qubit™ Flex Fluorometer User Guide*, available for download at [thermofisher.com/qubit](http://thermofisher.com/qubit).

- 2.4 Press **Next** from the **Standards complete** screen. When prompted, load the tubes as shown in the **Insert samples** screen. If you have fewer than 8 samples, press to deselect the tube positions that do not contain a sample. Select the units for the output sample concentration, then select **Next**.

**Note:** (Optional) Select **More Options** to add the assay kit lot number, Tags, or sample IDs. For information on using these options, refer to the *Qubit™ Flex Fluorometer User Guide*.

- 2.5 In the **Sample volume** screen, enter the sample volume added to the assay tube (from 1-20 µL). Enter the volume directly in the sample volume text box, use the + or – buttons or adjust the sample volume wheel to select the sample volume added to the assay tube.

**Note:** The sample volume used (1-20 µL) changes the assay accuracy range. A different sample volume or assay may be required if the sample concentration is outside of what the assay can accurately quantify.

- 2.6 Insert a sample tube strip into the sample chamber, close the lid, then press **Run samples**. When the reading is complete (~3 seconds), remove the sample tube.


Standards and samples are displayed on a graph with the results in a list below. Select the graph icon only to view the results list. The value listed is the concentration of the original sample. For more information on interpreting the sample results, refer to the *Qubit™ Flex Fluorometer User Guide*.

- 2.7 Select **Add samples** to read more samples and repeat step 2.6.

**Note:** (Optional) Select **Calculators** to access the Molarity and Normalization calculators. For information on the calculators, refer to the *Qubit™ Flex Fluorometer User Guide*.

## Read standards and samples

Figure 1. Workflow using Qubit™ Flex Fluorometer

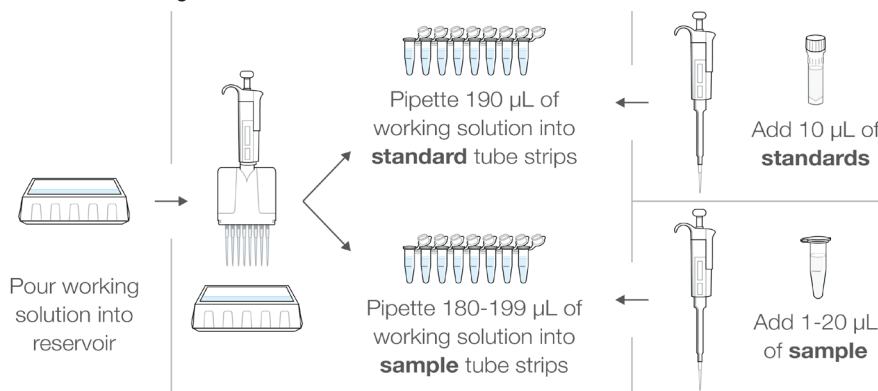

### Qubit™ 4 Fluorometer

- 3.1 On the **Home** screen of the Qubit™ 3 or the Qubit™ 4 Fluorometer, press **DNA**, then select **1X dsDNA HS** as the assay type. The “Read standards” screen is displayed. Press **Read Standards** to proceed.

**Note:** If you have already performed a calibration for the selected assay, the instrument prompts you to choose between reading new standards and running samples using the previous calibration. If you want to use the previous calibration, skip to step 3.4. Otherwise, continue with step 3.2.

- 3.2 Insert the tube containing Standard #1 into the sample chamber, close the lid, then press **Read standard**. When the reading is complete (~3 seconds), remove Standard #1.
- 3.3 Insert the tube containing Standard #2 into the sample chamber, close the lid, then press **Read standard**. When the reading is complete, remove Standard #2.

The instrument displays the results on the Read standard screen. For information on interpreting the calibration results, refer to the *Qubit™ Fluorometer User Guide*, available for download at [thermofisher.com/qubit](https://www.thermofisher.com/qubit).

- 3.4 Press **Run samples**.

- 3.5 On the assay screen, select the sample volume and units:

- a. Press the **+** or **–** buttons on the wheel, or anywhere on the wheel itself, to select the **sample volume** added to the assay tube (from 1–20 µL).
- b. From the **unit** dropdown menu, select the units for the output sample concentration.

- 3.6 Insert a sample tube into the sample chamber, close the lid, then press **Read tube**. When the reading is complete (~3 seconds), remove the sample tube.

The top value (in large font) is the concentration of the original sample and the bottom value is the dilution concentration. For information on interpreting the sample results, refer to the *Qubit™ Fluorometer User Guide*.

- 3.7 Repeat step 3.6 until all samples have been read.

Selectivity of the  
Qubit™ 1X dsDNA HS Assay

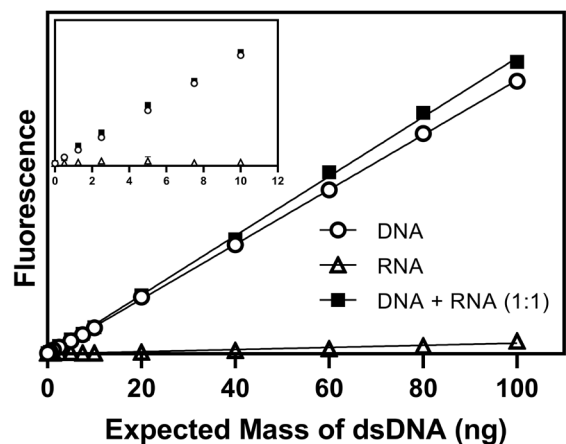


Figure 2. DNA selectivity and sensitivity of the Qubit™ 1X dsDNA HS Assay (Cat. Nos. Q33230, Q33231). Triplicate 10-μL samples of λ DNA (Cat. No. Q33233), *E. coli* rRNA, or a 1:1 Mixture of DNA and RNA were assayed with the Qubit™ dsDNA HS Assay. Fluorescence was measured and plotted versus the concentration of the RNA or DNA sample alone, or versus the mass of the DNA component in the 1:1 Mixture. The variation (CV) of replicate DNA determinations was ≤2%. The inset is an expanded view of the low range of the assay showing the extreme sensitivity of the assay for DNA. Background fluorescence has not been subtracted.

How the Qubit™ Fluorometer  
calculates concentration

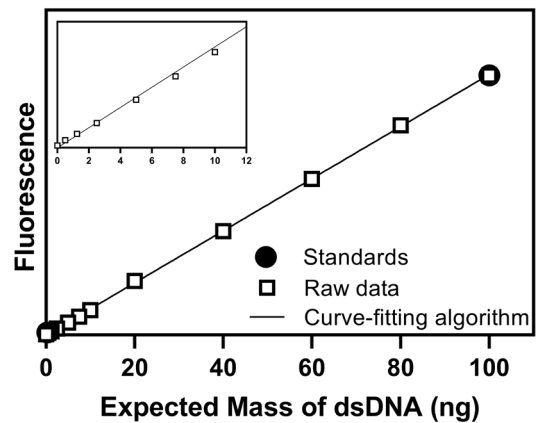


Figure 3. The curve-fitting algorithm used to determine concentration in the Qubit™ 1X dsDNA HS Assay. The Qubit™ Fluorometer generates concentration data based on the relationship between the two standards used in the calibration. This plot shows the line corresponding to the curve-fitting algorithm (a modified Hill plot) used in the calculation of concentration data for the Qubit™ 1X dsDNA HS Assay. For reference, the positions of the standards and a set of data points from an actual experiment are shown superimposed onto the line, demonstrating that the curve-fitting algorithm gives accurate values for quantitation. The application note "Comparison of Quant-iT™ and Qubit™ quantitation assays for accuracy and precision" (available at [thermofisher.com/qubit](http://thermofisher.com/qubit)) describes in greater detail how the optimized Qubit™ algorithm provides improved accuracy and precision at the low end of the concentration range (<10 ng/mL) over traditional 8-point standard curve and linear regression.

Qubit™ assay kits compatible  
with the Qubit™ Fluorometer

Contaminants tolerated by the  
Qubit™ 1X dsDNA HS Assay

**Note:** While the contaminant tolerances of Qubit™ 1X dsDNA HS assay and the Qubit™ dsDNA HS assay are largely similar, they are not identical.

**Table 2.** Effect of contaminants in the Qubit™ 1X dsDNA HS Assay\*

| Contaminant             | Final concentration in the assay | Concentration in 10-µL sample | Concentration in 1-µL sample | Result |
|-------------------------|----------------------------------|-------------------------------|------------------------------|--------|
| Sodium chloride         | 50 mM                            | 1 M                           | 10 M                         | OK     |
| Magnesium chloride      | 1 mM                             | 20 mM                         | 200 mM                       | OK     |
| Sodium acetate          | 30 mM                            | 600 mM                        | 6 M                          | OK     |
| Ammonium acetate        | 25 mM                            | 500 mM                        | NA                           | OK     |
| Sodium azide            | 1 mM                             | 20 mM                         | 200 mM                       | OK     |
| Ethanol                 | 1%                               | 20 %                          | NA**                         | OK     |
| Phenol                  | 0.1%                             | 2%                            | 20%                          | OK     |
| Chloroform <sup>†</sup> | 1%                               | 20 %                          | NA**                         | OK     |
| SDS                     | 0.002%                           | 0.04%                         | 0.4%                         | OK     |
| BSA                     | 1X <sup>‡</sup>                  | 1X <sup>‡</sup>               | 1X <sup>‡</sup>              | OK     |
| IgG                     | 1X <sup>‡</sup>                  | 1X <sup>‡</sup>               | 1X <sup>‡</sup>              | OK     |
| ssDNA                   | 1X <sup>‡</sup>                  | 1X <sup>‡</sup>               | 1X <sup>‡</sup>              | OK     |
| RNA                     | 1X <sup>‡</sup>                  | 1X <sup>‡</sup>               | 1X <sup>‡</sup>              | OK     |
| dNTPs <sup>§</sup>      | 1X <sup>‡</sup>                  | 1X <sup>‡</sup>               | 1X <sup>‡</sup>              | OK     |

\* DNA standards were assayed in the presence or absence of contaminants at the indicated final concentrations. Equivalent concentrations (approximate) in 10 µL or 1 µL sample volumes are also listed. In all cases, results are given as OK, usually less than 10% perturbation. For best results, add the same amount of contaminant to the standard samples.

\*\* User sample would require greater than 100% of listed contaminant.

† Immiscible.

‡ 1X indicates a concentration equal to the concentration of dsDNA.

§ A mixture of dATP, dCTP, dGTP, and dTTP.

NA: Not available.

**Qubit assay kits compatible  
with the Qubit™ Fluorometer**

A number of fluorescence-based quantification kits are available for use with the Qubit™ Fluorometer. Use Table 3 to choose a kit based on the target molecule being measured and the number of assays you require.

**Table 3.** Qubit™ assay kits for use with the Qubit™ Fluorometer

| Product                      | Cat. No.         | No. of assays* | Target                    | Notes                                                                                                                                                                                                                                                                                                                                                                                                                                                |
|------------------------------|------------------|----------------|---------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Qubit™ 1X dsDNA BR Assay Kit | Q33265           | 100            | dsDNA                     | <ul style="list-style-type: none"> <li>Core range (high confidence): 0.01 µg/mL to 5 µg/mL<sup>†</sup></li> <li>Extended range (moderate confidence): 5 µg/mL to 10 µg/mL<sup>†</sup></li> <li>Useful for quantitation of genomic and miniprep DNA samples</li> <li>Accurate in the presence of RNA, salts, solvents, proteins, and free nucleotides</li> </ul>                                                                                      |
|                              | Q33266           | 500            |                           |                                                                                                                                                                                                                                                                                                                                                                                                                                                      |
| Qubit™ dsDNA HS Assay Kit    | Q32851<br>Q33230 | 100            | dsDNA                     | <ul style="list-style-type: none"> <li>Core range (high confidence): 1 ng/mL to 500 ng/mL<sup>†</sup></li> <li>Extended ranges (moderate confidence): 0.5 ng/mL to 1 ng/mL and 500 ng/mL to 600 ng/mL<sup>†</sup></li> <li>Useful for quantitation of PCR products, viral DNA, and samples for subcloning</li> <li>Accurate in the presence of RNA, salts, solvents, proteins, and free nucleotides</li> </ul>                                       |
|                              | Q32854<br>Q33231 | 500            |                           |                                                                                                                                                                                                                                                                                                                                                                                                                                                      |
| Qubit™ ssDNA Assay Kit       | Q10212           | 100            | ssDNA                     | <ul style="list-style-type: none"> <li>Core range (high confidence): 5 ng/mL to 1000 ng/mL<sup>†</sup></li> <li>Extended ranges (moderate confidence): 1 ng/mL to 5 ng/mL and 1000 ng/mL to 1200 ng/mL<sup>†</sup></li> <li>Useful for quantitation of oligos, primers, denatured DNA, PCR products</li> <li>Accurate in the presence of salts, urea, solvents, proteins, ATP, and agarose</li> </ul>                                                |
| Qubit™ RNA HS Assay Kit      | Q32852           | 100            | RNA                       | <ul style="list-style-type: none"> <li>Core range (high confidence): 25 ng/mL to 500 ng/mL<sup>†</sup></li> <li>Extended ranges (moderate confidence): 20 ng/mL to 25 ng/mL and 500 ng/mL to 1000 ng/mL<sup>†</sup></li> <li>Useful for quantitation of samples for microarray, RT-PCR, and Northern blot procedures</li> <li>Accurate in the presence of DNA, salts, solvents, proteins, and free nucleotides</li> </ul>                            |
|                              | Q32855           | 500            |                           |                                                                                                                                                                                                                                                                                                                                                                                                                                                      |
| Qubit™ RNA BR Assay Kit      | Q10210           | 100            | RNA                       | <ul style="list-style-type: none"> <li>Core range (high confidence): 0.1 µg/mL to 5 µg/mL<sup>†</sup></li> <li>Extended ranges (moderate confidence): 0.05 µg/mL to 0.1 µg/mL and 5 µg/mL to 6 µg/mL<sup>†</sup></li> <li>Useful for quantitation of samples for microarray, RT-PCR, and Northern blot procedures</li> <li>Accurate in the presence of DNA, salts, solvents, proteins, and free nucleotides</li> </ul>                               |
|                              | Q10211           | 500            |                           |                                                                                                                                                                                                                                                                                                                                                                                                                                                      |
| Qubit™ microRNA Assay Kit    | Q32880           | 100            | RNA                       | <ul style="list-style-type: none"> <li>Core range (high confidence): 5 ng/mL to 500 ng/mL<sup>†</sup></li> <li>Extended ranges (moderate confidence): 2.5 ng/mL to 5 ng/mL and 500 ng/mL to 750 ng/mL<sup>†</sup></li> <li>Useful for quantification of samples for qRT-PCR and sequencing applications</li> <li>Accurate in the presence of rRNA, large mRNA (&gt;1000 bp), salts, solvents, proteins, and free nucleotides</li> </ul>              |
|                              | Q32881           | 500            |                           |                                                                                                                                                                                                                                                                                                                                                                                                                                                      |
| Qubit™ Protein Assay Kit     | Q33211           | 100            | Protein                   | <ul style="list-style-type: none"> <li>Core range (high confidence): 1.25 µg/mL to 25 µg/mL<sup>†</sup></li> <li>Extended ranges (moderate confidence): 1 µg/mL to 1.25 µg/mL and 25 µg/mL to 26 µg/mL<sup>†</sup></li> <li>Little protein-to-protein difference in signal</li> <li>Accurate in the presence of DTT, β-mercaptoethanol, amino acids, and DNA</li> <li>Signal is stable for 3 hours</li> </ul>                                        |
|                              | Q33212           | 500            |                           |                                                                                                                                                                                                                                                                                                                                                                                                                                                      |
| Qubit™ RNA IQ Assay Kit      | Q33221           | 75             | RNA integrity and quality | <ul style="list-style-type: none"> <li>Although small in size, the tertiary structure of 5s and tRNA will bind the large RNA dye</li> <li>Accurate in the presence of salts, protein, solvents and RNA stabilization reagents</li> <li>Signal is stable for 1 hour</li> <li>The Qubit™ RNA IQ Assay will only work on the Qubit™ 4 or Flex Fluorometer. The assay is not designed for use with Qubit™, Qubit™ 2, or Qubit™ 3 Fluorometers</li> </ul> |
|                              | Q33222           | 275            |                           |                                                                                                                                                                                                                                                                                                                                                                                                                                                      |

\*Based on an assay volume of 200 µL.

<sup>†</sup>Concentration ranges refer to the concentration of sample after dilution in the assay tube.

## Ordering information

| Cat. No.                | Product name                                                                                       | Unit size |
|-------------------------|----------------------------------------------------------------------------------------------------|-----------|
| Q33230                  | Qubit™ 1X dsDNA HS Assay Kit, 100 assays . . . . .                                                 | 1 kit     |
| Q33231                  | Qubit™ 1X dsDNA HS Assay Kit, 500 assays . . . . .                                                 | 1 kit     |
| <b>Related products</b> |                                                                                                    |           |
| Q32850                  | Qubit™ dsDNA BR Assay Kit, 100 assays *2–1000 ng* *for use with the Qubit™ Fluorometer* . . . . .  | 1 kit     |
| Q32853                  | Qubit™ dsDNA BR Assay Kit 500 assays *2–1000 ng* *for use with the Qubit™ Fluorometer* . . . . .   | 1 kit     |
| Q32851                  | Qubit™ dsDNA HS Assay Kit, 100 assays *0.2–100 ng* *for use with the Qubit™ Fluorometer* . . . . . | 1 kit     |
| Q32854                  | Qubit™ dsDNA HS Assay Kit, 500 assays *0.2–100 ng* *for use with the Qubit™ Fluorometer* . . . . . | 1 kit     |
| Q10212                  | Qubit™ ssDNA Assay Kit, 100 assays *1–200 ng* *for use with the Qubit™ Fluorometer* . . . . .      | 1 kit     |
| Q10210                  | Qubit™ RNA BR Assay Kit, 100 assays *20–1000 ng* *for use with the Qubit™ Fluorometer* . . . . .   | 1 kit     |
| Q10211                  | Qubit™ RNA BR Assay Kit, 500 assays *20–1000 ng* *for use with the Qubit™ Fluorometer* . . . . .   | 1 kit     |
| Q32852                  | Qubit™ RNA HS Assay Kit, 100 assays *5–100 ng* *for use with the Qubit™ Fluorometer* . . . . .     | 1 kit     |
| Q32855                  | Qubit™ RNA HS Assay Kit, 500 assays *5–100 ng* *for use with the Qubit™ Fluorometer* . . . . .     | 1 kit     |
| Q33221                  | Qubit™ RNA IQ Assay Kit, 75 assays *for use with the Qubit™ 4 Fluorometer* . . . . .               | 1 kit     |
| Q33222                  | Qubit™ RNA IQ Assay Kit, 275 assays *for use with the Qubit™ 4 Fluorometer* . . . . .              | 1 kit     |
| Q32880                  | Qubit™ microRNA Assay Kit, 100 assays *1–100 ng* *for use with the Qubit™ Fluorometer* . . . . .   | 1 kit     |
| Q32881                  | Qubit™ microRNA Assay Kit, 500 assays *1–100 ng* *for use with the Qubit™ Fluorometer* . . . . .   | 1 kit     |
| Q33211                  | Qubit™ Protein Assay Kit, 100 assays *0.25–5 µg* *for use with the Qubit™ Fluorometer* . . . . .   | 1 kit     |
| Q33212                  | Qubit™ Protein Assay Kit, 500 assays *0.25–5 µg* *for use with the Qubit™ Fluorometer* . . . . .   | 1 kit     |
| Q33233                  | Qubit™ 1X dsDNA HS Assay - Lambda Standard . . . . .                                               | 5 mL      |
| Q32856                  | Qubit™ assay tubes *set of 500* . . . . .                                                          | 1 set     |

# Documentation and support

---

## Customer and Technical Support

Visit [thermofisher.com/support](https://www.thermofisher.com/support) for the latest in services and support, including:

- Worldwide contact telephone numbers
- Product support, including:
  - Product FAQs
  - Software, patches, and updates
  - Training for many applications and instruments
- Order and web support
- Product documentation, including:
  - User guides, manuals, and protocols
  - Certificates of Analysis
  - Safety Data Sheets (SDSs; also known as MSDSs)

**Note:** For SDSs for reagents and chemicals from other manufacturers, contact the manufacturer.

## Limited Product Warranty

Life Technologies Corporation and/or its affiliate(s) warrant their products as set forth in the Life Technologies' General Terms and Conditions of Sale found on Life Technologies' website at [www.thermofisher.com/us/en/home/global/terms-and-conditions.html](https://www.thermofisher.com/us/en/home/global/terms-and-conditions.html). If you have any questions, please contact Life Technologies at [thermofisher.com/support](https://www.thermofisher.com/support).

The information in this guide is subject to change without notice.

**For Research Use Only. Not for use in diagnostic procedures.**

**DISCLAIMER:** TO THE EXTENT ALLOWED BY LAW, THERMO FISHER SCIENTIFIC INC. AND/OR ITS AFFILIATE(S) WILL NOT BE LIABLE FOR SPECIAL, INCIDENTAL, INDIRECT, PUNITIVE, MULTIPLE OR CONSEQUENTIAL DAMAGES IN CONNECTION WITH OR ARISING FROM THIS DOCUMENT, INCLUDING YOUR USE OF IT.

**Important Licensing Information:** These products may be covered by one or more Limited Use Label Licenses. By use of these products, you accept the terms and conditions of all applicable Limited Use Label Licenses.

**Revision history:** Pub. No. MAN0017455

| Revision | Date             | Description                                                                             |
|----------|------------------|-----------------------------------------------------------------------------------------|
| C.0      | 08 December 2020 | Adding Qubit™ Flex Fluorometer protocol and correcting assay range to 0.2 ng to 100 ng. |
| B.0      | 02 April 2019    | Correct assay range from 0.1 ng to 100 ng to 0.2 ng to 200 ng                           |
| A.0      | 08 November 2017 | New user guide                                                                          |



**Manufacturer:** Life Technologies Corporation | 29851 Willow Creek Road | Eugene, OR 97402

**Trademarks:** All trademarks are the property of Thermo Fisher Scientific and its subsidiaries unless otherwise specified.

©2020 Thermo Fisher Scientific Inc. All rights reserved.