

# VENUS

## Specifications

### Physical Specifications

Display  
15.6" TFT Touch screen  
Resolution: 1366 x 768  
Number of traces: up to 12 ECG waveforms  
Dimension: 398×302×183mm(W×H×D)  
Weight: < 7 kg under standard configuration  
LAN: 1 standard RJ45 port  
WLAN: IEEE 802.11b/g/n  
USB: 2 USB connectors  
HDMI: 1 HDMI monitor connector  
Output: 1 connector for Nurse call, Defib Sync Analog Output

### ECG

Lead type: 3-lead, 5-lead, 12-lead(optional)  
ECG waveform: 2 channels, 7 channels, 12 channels  
Display sensitivity (wave gain):  
1.25mm/mV (×0.125), 2.5mm/mV (×0.25), 5mm/mV (×0.5),  
10mm/mV (×1.0), 20mm/mV (×2.0), 40mm/mV (×4.0),  
Auto  
Wave sweep speed:  
3.125mm/s, 6.25mm/s, 12.5 mm/s, 25 mm/s, 50 mm/s  
Bandwidth  
Diagnostic mode: 0.05Hz~150Hz  
Monitor mode: 0.5Hz~40Hz  
Surgery mode: 0.5Hz~25Hz  
Strong filter mode: 5Hz~25Hz  
CMRR > 100dB  
Notch: 50/60Hz notch filter can be set to on or off  
Differential input impedance > 5MΩ  
Electrode polarization voltage range: ±400mV  
HR range: 15 ~ 350 bpm  
Baseline recovery time < 3s after defibrillation (in monitor and surgery mode)  
Calibration signal: 1mV (peak - peak), accuracy ±3%

### RESP

Measurement method: Thoracic electrical bioimpedance  
Measuring lead: Lead I, II  
Wave gain: ×0.25, ×0.5, ×1, ×2  
Respiratory impedance range: 0.5~5Ω  
Respiration range: 0 ~ 150bpm  
Baseline impedance: 500~4000Ω  
Gain: 10 grades  
Scan speed: 3.125mm/s, 6.25mm/s, 12.5 mm/s, 25mm/s

### TEMP

Accuracy: ±0.1°C or ±0.2°F (without probe)  
Measurement range: 5~50°C (41~122°F)  
Channel: Two channels  
Resolution: 0.1°C

### SpO2

Measurement range: 0~100%  
Parameter monitoring: Perfusion Index (PI)  
Pleth Variability Index (PVI)

Resolution: 1%  
Accuracy: ±2% or ±2bpm  
Refreshing Rate: 1s  
Pleth wave speed: 3.125mm/s, 6.25mm/s, 12.5 mm/s, 25mm/s

### Masimo SET® SpO2(Optional)

Measurement range: 0~100%  
Resolution: 1%  
Accuracy: ±2% (70~100%, Adult/Pediatric, non-motion, low perfusion);  
±3% (70~100%, Neonate, non-motion);  
±3% (70~100%, motion);  
0~69%, unspecified

Refreshing Rate: 1s

### Pulse Rate

Range: 20~300 bpm  
Resolution: 1bpm  
Accuracy: ±2bpm (non-motion)  
±5bpm (motion)  
Refreshing rate: 1s

### NIBP

Measurement method: Automatic oscillometric method  
Operating mode: Manual, automatic, continuous  
Measurement unit: mmHg/kPa selectable  
Typical measurement time: 20~40s  
Measurement type: Systolic, Diastolic, Mean  
Measurement range (mmHg)  
Range of Systolic pressure: Adult 40~280  
Pediatric 40~200  
Neonatal 40~135  
Range of Diastolic pressure: Adult 10~210  
Pediatric 10~150  
Neonatal 10~95  
Range of Mean pressure: Adult 20~230  
Pediatric 20~165  
Neonatal 20~105

Measurement accuracy  
Maximum average error: ±5mmHg  
Maximum standard deviation: 8mmHg  
Resolution: 1mmHg  
Interval: 1, 2, 3, 4, 5, 10, 15, 30, 60, 90, 120, 180, 240, 480 minutes  
Overpressure protection: Software and hardware, double safety protection  
Cuff pressure range: 0~300mmHg

### IBP(Optional)

Channel: 2-channel or 4-channel  
ART: 0 to 300 mmHg  
PA: -6 to 120 mmHg  
CVP/RAP/LAP/ICP: -10 to 40 mmHg  
Measurement range: P1/P2 -50 to 300 mmHg  
Resolution: 1mmHg  
Accuracy:  
±2% or ±1mmHg, whichever is greater (without sensor)  
Sensitivity: 5μV/mmHg/V  
Impedance range: 300 to 3000Ω

### C.O.(Optional)

Method: Thermodilution  
Range: C.O.: 0.2 to 20 L/min  
TB: 23 to 45°C  
T1: -1 to 27°C  
Accuracy: C.O.: ±5% or ±0.1L/min, whichever is greater  
TB, T1: ±0.5°C (without sensor)

### Northern Mainstream CO2(Optional)

Measurement range: 0~19.7%, 150mmHg, or 0~20kPa  
Resolution: 0.1mmHg  
Measurement accuracy  
0 ~ 40 mmHg: ± 2 mmHg  
41 ~ 70 mmHg: ± 5% of reading  
71 ~ 100 mmHg: ± 8% of reading  
101 ~ 150 mmHg: ± 10% of reading  
Respiration rate: 3~150 bpm  
Respiration rate accuracy: 1% ±1bpm  
Warm-up time: 97% within 8s, full accuracy within 20s

### Northern Sidestream CO2(Optional)

Measurement range: 0~20% (0 ~ 150mmHg)  
Accuracy: < 5.0% CO2 ± 2 mmHg  
> 5.0% CO2: < 6% of reading  
Respiration rate: 0 ~ 150 BPM  
Respiration rate accuracy: 1% ±1BPM  
Warm-up time: 97% within 45s, full accuracy within 10 min  
Rise times (t10~90%): About 100ms, when flow is 100 ml/min, adult water trap, 1.5m sampling tube  
Delay time: < 3sec when flow is 100 ml/min, adult water trap, 1.5m sampling tube

### Recorder (Optional)

Built-in, Thermal dot array  
Horizontal resolution: 16 dots/mm (25 mm/s paper speed)  
Vertical resolution: 8 dots/mm  
Paper speed: 12.5mm/s, 25 mm/s, 50 mm/s  
Number of waveform channels: 3

### Masimo ISA™ Sidestream CO2 (Optional)

Warm-up time: Full accuracy within 10 seconds  
Sampling flow rate: 50ml/min (+/-10/min)  
Measurement Range: 0 ~ 25%  
Accuracy: 0~15% (±0.2% of the reading)  
15~25%, unspecified  
Rise time: 200ms, typical at 50ml/min flow rate  
Total response time:  
within 3 seconds (with 2 m Nomoline sampling line)  
AWRR Range: 0~150bpm  
AWRR Accuracy: ±1 breath

### Masimo IRMA™ Mainstream CO2 (Optional)

Measurement Range: 0 ~ 25%  
Accuracy: 0~15% (±0.2% of the reading)  
15~25%, unspecified  
Warm-up time: Full accuracy within 10 seconds  
AWRR Range: 0~150bpm  
AWRR Accuracy: ±1 breath

### Masimo Multi-gas ISA AX+Mainstream CO2 (Optional)

Gas: CO2, N2O, HAL, ISO, ENF, SEV, DES with automatic identification  
Warm-up time: Full accuracy within 20 seconds for IRMA AX+ CO2 Accuracy: 0~10%±(0.2%+2% of the reading)  
0~15%±(0.3%+2% of the reading)  
N2O Accuracy: 0~100%±(2%+2% of the reading)  
HAL, ISO, ENF: 0~8%±(0.15%+5% of the reading)  
SEV: 0~10%±(0.15%+5% of the reading)  
DES: 0~22%±(0.15%+5% of the reading)  
Agent identification time: < 20s (typical < 10s)  
AWRR range: 0~150bpm  
AWRR accuracy: ±1bpm  
Apnea time: 20~60s

### Aspect BISx module(Optional)

Parameter Measurement:  
BIS: 0~30 (Only limited to the combined use of an external sensor with a BIS module)  
EMG: 30~55dB (bar chart) with intensity between 30dB and 80dB (tendency chart)  
BIS: 0~100  
SQI: 0%~100%  
SR: 0%~100%  
SEF: 0.5Hz~30Hz  
TP: 40~100Db  
EEG Measurement:  
Input impedance > 5MΩ  
Noise (RTI) < 2μV (0.25~50Hz)  
Input signal range: ±1mV  
EEG bandwidth between: 0.25Hz~110Hz

### NMT (Optional)

Microprocessor-controlled  
Stimulation Mode: TOF, TOFS, PTC, 1Hz Twitch, 0.1Hz Twitch, DBS DBS3.3 and 3.2 (Double Burst), Tetanic Stimulation (Burst), 5s ~ 50Hz or 100Hz  
Output (accuracy ±5% of full scale value)  
Surface electrodes:  
Constant current, 0~60mA (0~12/18μC) up to 5KOhm.  
Monophasic, 200μs or 300μs pulse width  
Needle electrodes:  
Constant current, 0~6mA (0~0.24μC) up to 5KOhm.  
Monophasic, 40μs pulse width  
Acceleration transducer: Accuracy ±5% of full scale value  
Temperature sensor: Range 20.0~41.5°C (accuracy ±5°C)

### Operation Environment

Power: AC 100~250V, 50/60Hz  
Temperature: 5~40°C  
Humidity: < 80%  
Patient Range: Adult, Pediatric, Neonate



Committed to Excellence



Venus

Critical Care Patient Monitor

## Northern Meditec Limited

Add: 4th Floor, Building C, Jinwei Yuan Industrial Park, Julongshan Area, Longtian Street, Pingshan District, Shenzhen, P.R.China

Tel: +86 755 29970566 Fax: +86 755 86528647

Email: info@northernmeditec.com

Website: http://www.northernmeditec.com







## Features

- 15.6" High resolution TFT LCD Touch screen
- 10 waveform display, up to 12-lead ECG analysis
- Powerful calculation (Hemodynamic, Dose, Oxygenation, Ventilation)
- MEWS (Modified Early Warning Score)
- Pacemaker detection
- ST & arrhythmia analysis (26 types)
- SpO2 support PVI and PI, low perfusion 0.2%
- Night mode, standby mode, venipuncture mode
- Trolley/wall mount bracket solutions
- Support BIS module, NMT module
- Wired/Wireless/4G connection, support HL7 protocol to HIS
- SpO2 pulse-tone modulation (Pitch Tone)
- VGA/HDMI support external display
- Graphical & tabular trend review
- Rechargeable Lithium-ion Battery
- 72 hours full disclosure wave review for each patient

## Easy access to view the historical data

480	Hours long trend
120	Min short trend
10000	NIBP measurement
200	alarm event

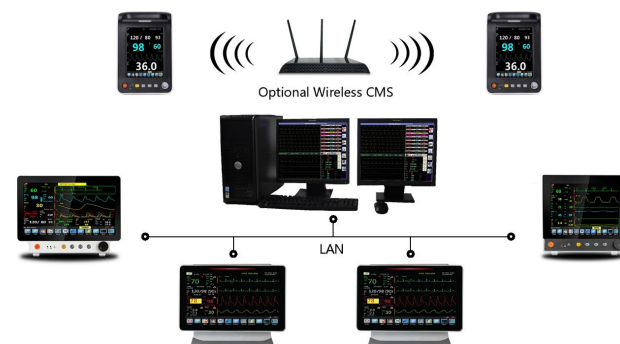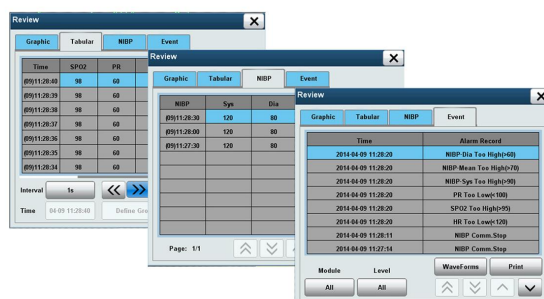

## Central Monitoring System

Up to 64 beds  
Net work is compatible to wired or wireless CMS  
Auto adaptable to different screen resolution

## Configuration

5-lead ECG, SpO2, NIBP, TEMP, Resp, PR; Touchscreen, HDMI, Li-ion battery

## Optional

12-Lead ECG, Masimo/Nellcor SpO2, IBP, C.O., EtCO2, Multi-gas, BIS, NMT; Thermal Recorder, Wired/Wireless CMS, 4G module



### Masimo SET® SpO2

Measure-through Motion and Low Perfusion pulse oximetry delivers accurate and reliable oxygenation



### Bispectral Index™ by Aspect

Monitor the level of consciousness of the patient under general anesthesia or sedation. provides BIS, SQI, EMG, SR, SEF, TP, PC value and EEG wave.



### Masimo Gas Technology

IRMA™ Mainstream & ISA™ Sidestream Analyzers  
Allows selection of the modality best suited to the application



### NMT

Neuromuscular monitoring




### IBP

2-4 Channel, support IBP waveform overlapping display




### C.O.


Cardiac Output

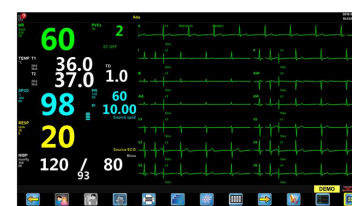


12-Lead ECG

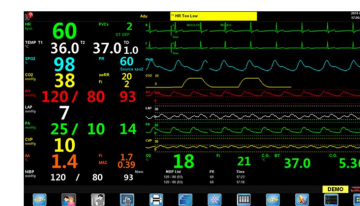

4 channel IBP

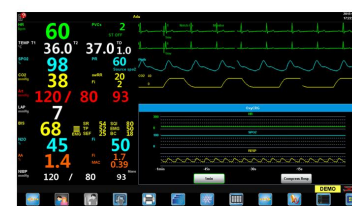

OxyCRG screen

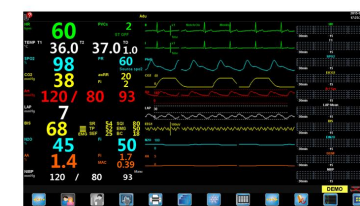

Dynamic trends