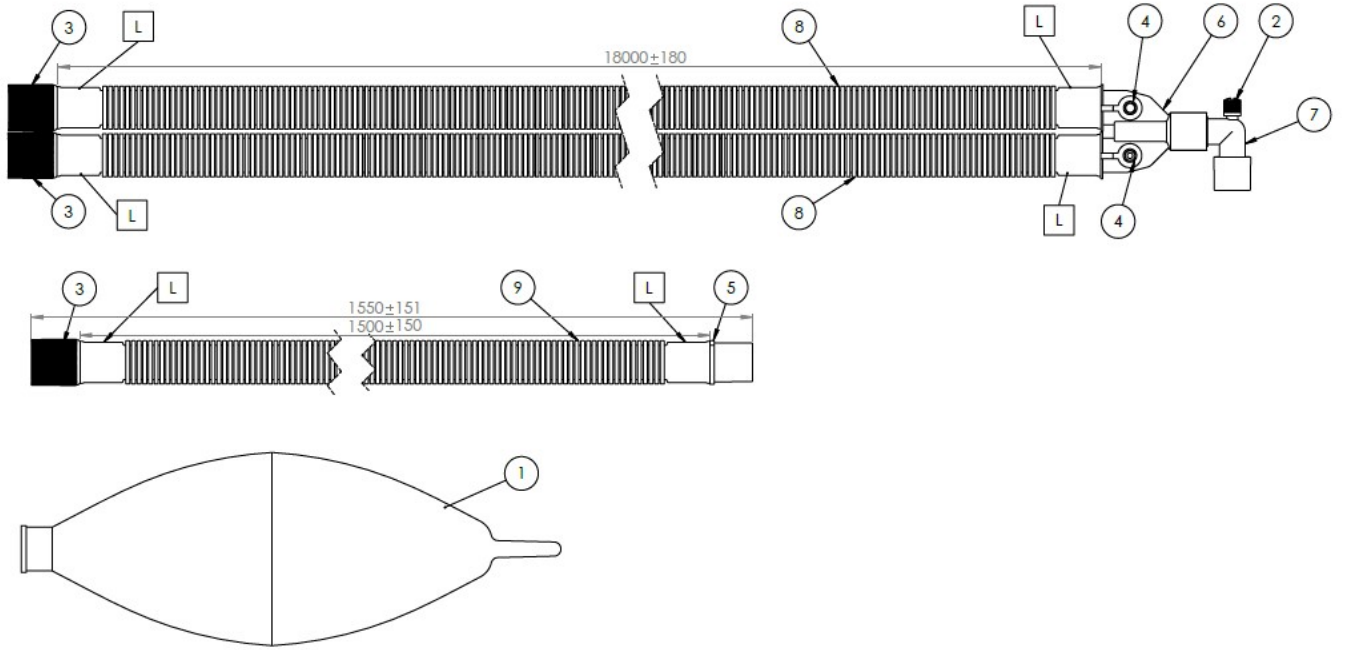


**1. Product Name and Product Code:**

AL-1101-060.V003- Adult Anesthesia Circuit Corrugated PE Tube

**2. Manufacturer:**

Meditera Tibbi Malzeme Sanayi ve Ticaret A.Ş.

**3. Sterilization Method :**

Ethylene oxide sterilization. This product line is provided both as sterile and nonsterile.

**4. Packaging:**

Nylon packaging.

**5. Intended Use and Functional Description :**

Disposable circuits used to conduct medical gases from the anaesthesia system to the patient.

Anaesthetic gas exits the anaesthesia machine (via the common gas outlet) and then enters a breathing circuit. The function of the circuit is to deliver oxygen and anaesthetic gases to the patient and to eliminate CO<sub>2</sub>. The CO<sub>2</sub> may be eliminated by gas inflow or by soda lime absorption.

**6. Shelf life :**

5 years from the date of production .

**7. Product Description:**

**7.1.** Classification: Class IIa Rule 2

**7.2.** This product does not contain any metallic parts

**7.3. Spesification of the product :**

Item	Description	Quantity
150.07.040	2 LT NEOPRENE SINGLE FOLDED BREATHING BAG WITH STICKER(RIGID PP CONNECTOR)	1
150.11.036	ELBOW CONNECTOR LUER CAP	1
151.03.074	Y CONNECTOR CAP	2
151.03.110	22-22MM STRAIGHT CONNECTOR	1
151.03.001.01	22MM STRAIGHT CONNECTOR	3
151.03.150	22 MM PARALLEL Y CONNECTOR PP	1
151.05.01.074	22 MM CORRUGATED TUBING PE 150 CM CUT	1
151.03.178.01	ELBOW CONNECTOR WITH CO2 PORT PP	1
151.05.01.062	22 MM CORRUGATED TUBING PE 180 CM CUT	2

**8. Standarts:**

EN ISO 13485:2016, 93/42/EEC Medical Device Directive, EN 556-1:2001, EN ISO 11607-1:2020, EN ISO 11607-2:2020, EN ISO 23328-1, EN ISO 23328-2

**9. Waste Method:**

After use product will be “contaminated medical waste” and package will be “packaging waste” so they should be handled according to relevant national and international standards and regulations.