




## Certificate of Conformity

KIT : **Ochratoxin A ELISA Kit RNM98008**

Release Date Dec.17<sup>th</sup>, 2024  
Expiration Date: Dec.16<sup>th</sup>, 2025 Temperature: 25°C

REAGEN INC certifies that this lot has passed Quality control assays and conforms to product release specifications.

Standards	Rep. #1	Rep. #2	Rep.#3	Avg.	Std. Dev.	%RSD	%Bo
Negative Control	2.258	2.235	2.251	2.248	0.0118	0.524	100%
0.1 ppb Calibrator	2.037	2.042	2.025	2.035	0.0087	0.429	90.5%
0.3 ppb Calibrator	1.833	1.845	1.854	1.844	0.0105	0.571	82.0%
0.9 ppb Calibrator	1.192	1.192	1.158	1.181	0.0196	1.663	52.5%
2.7 ppb Calibrator	0.509	0.510	0.508	0.509	0.0010	0.196	22.6%
8.1 ppb Calibrator	0.218	0.204	0.213	0.212	0.0071	3.352	9.4%

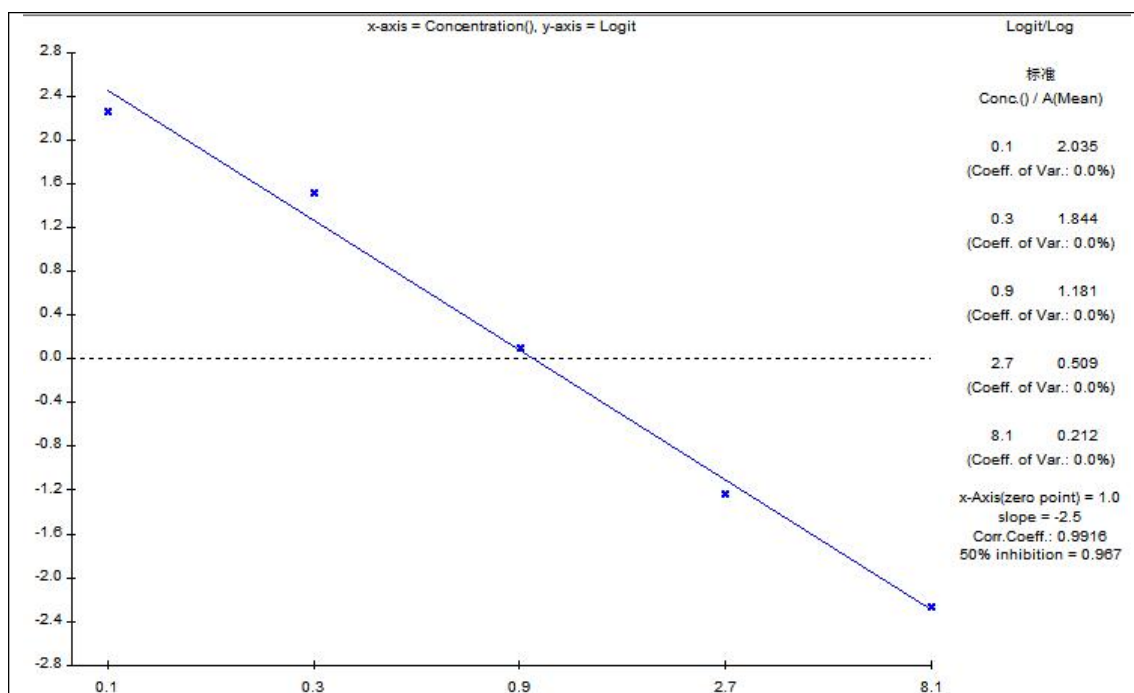

Note: The absorbance of the calibrators may Decrease during the shelf life of kit . Actual values may vary; this data is for example purposes only.

QA Manager Alexis

Release Date Dec.17<sup>th</sup> 2024

**REAGEN**